



Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details




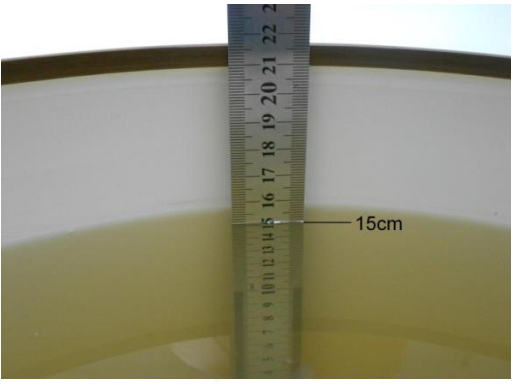



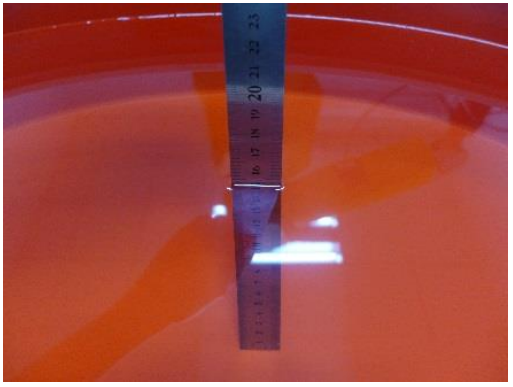


1. SAR measurement System



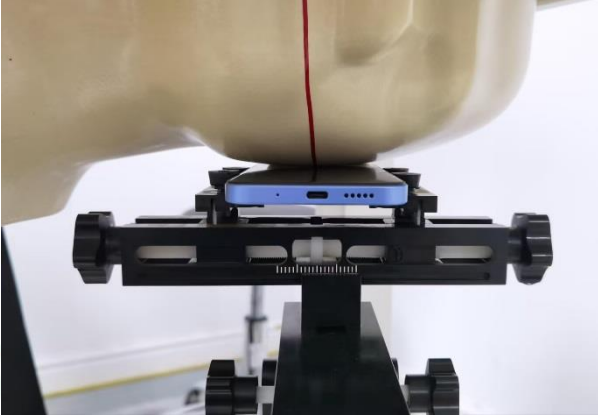
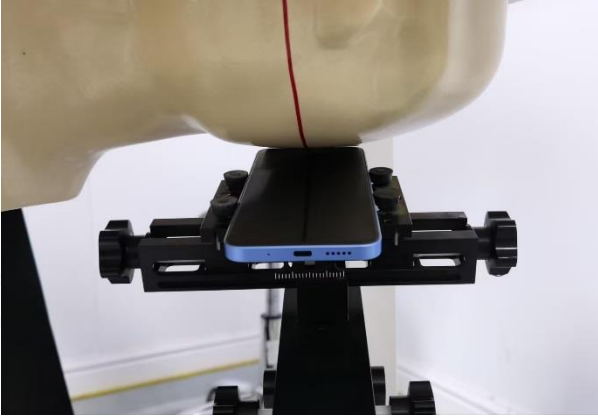
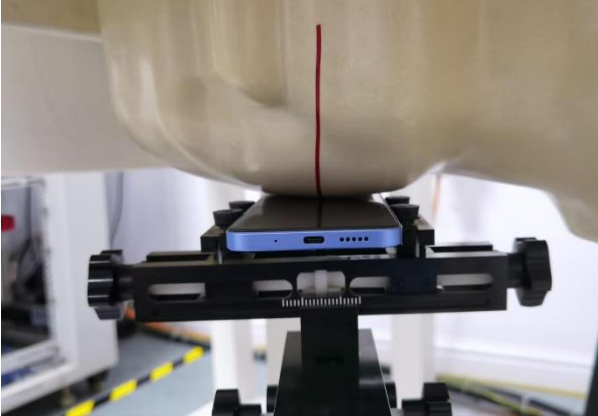
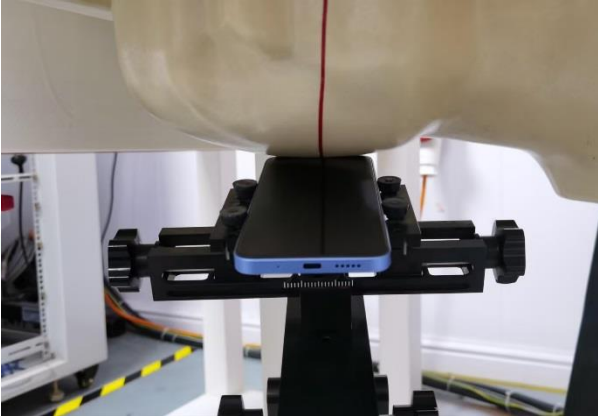




2. Photographs of Tissue Simulate Liquid

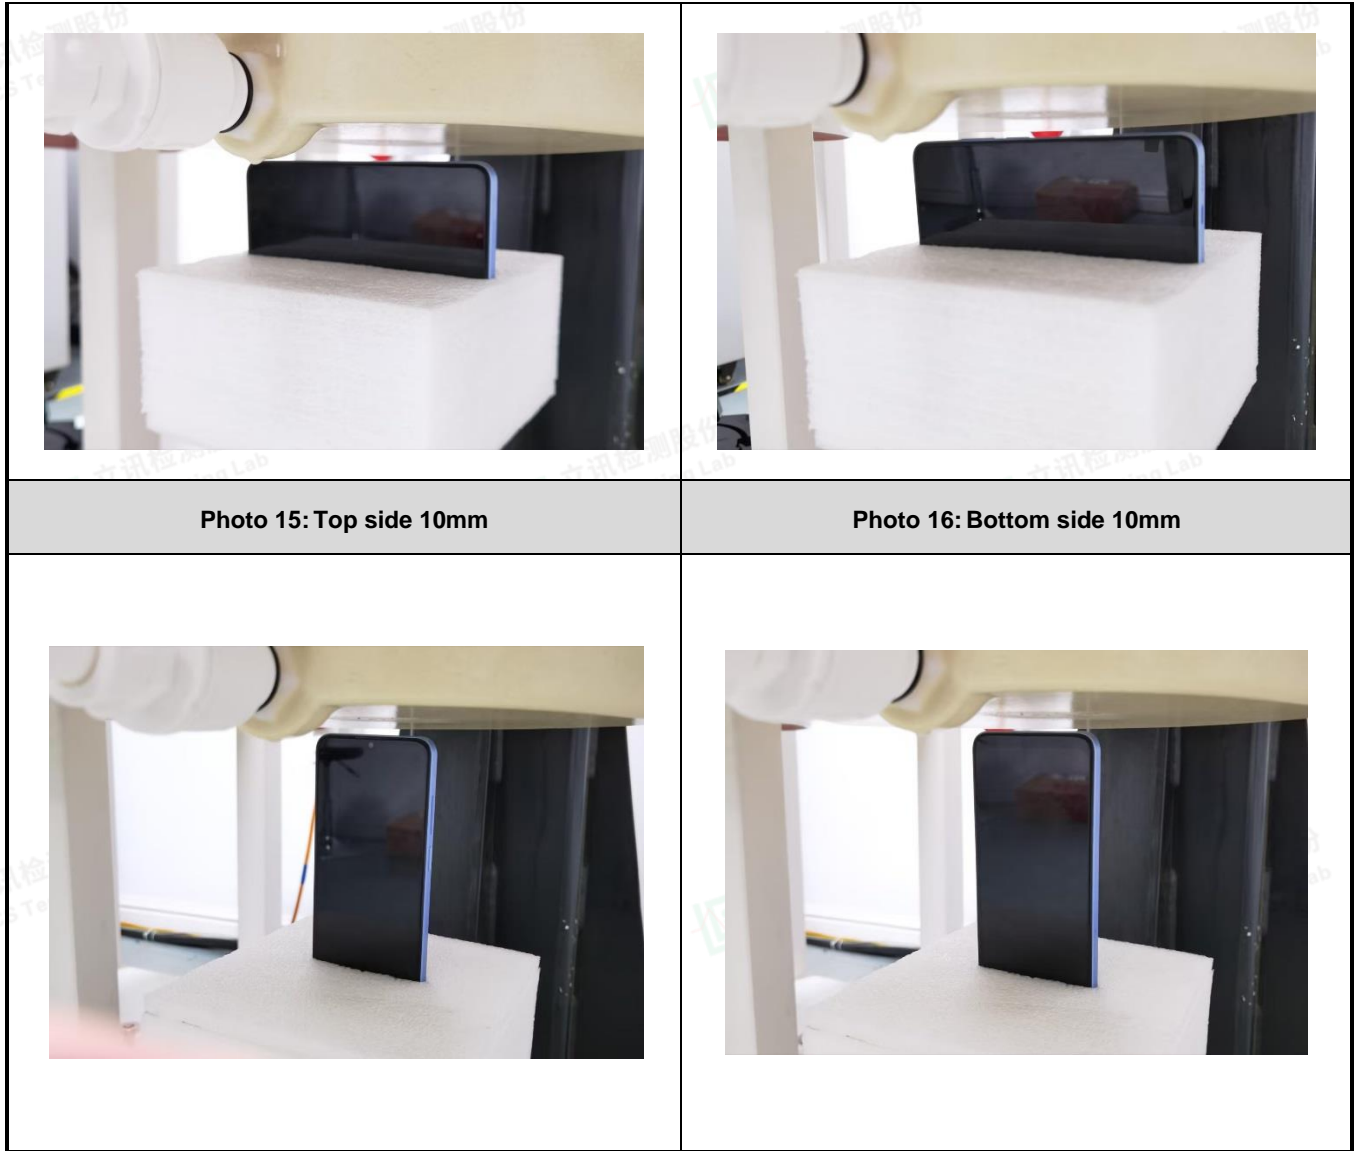
Photo 1: Tissue Simulant Liquid for Head 750	Photo 2: Tissue Simulant Liquid for Head 835
	
Photo 3: Tissue Simulant Liquid for Head 1750	Photo 4: Tissue Simulant Liquid for Head 1900
	
Photo 5: Tissue Simulant Liquid for Head 2450	Photo 6: Tissue Simulant Liquid for Head 5000
	



3. Photographs of EUT test position

Photo 7: Left Cheek	Photo 8: Left Tilt
	
Photo 9: Right Cheek	Photo 10: Right Tilt
	
Photo 11: Front side 10mm	Photo 12: Rear side 10mm
	
Photo 13: Left side 10mm	Photo 14: Right side 10mm







4. EUT Constructional Details

Photo 17: Front View	Photo 18: Back View
