



Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details




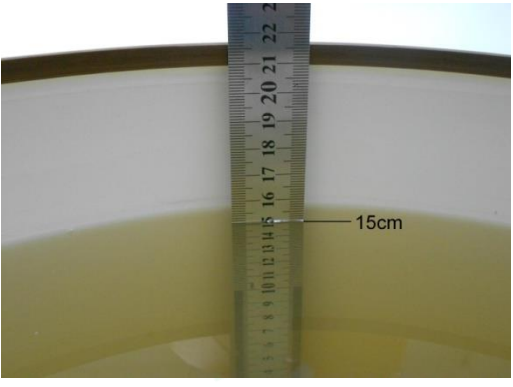






1. SAR measurement System






2. Photographs of Tissue Simulate Liquid

<p>Photo 1: Tissue Simulant Liquid for Head 750</p>	<p>Photo 2: Tissue Simulant Liquid for Head 835</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 1750</p>	<p>Photo 4: Tissue Simulant Liquid for Head 1900</p>
	
<p>Photo 5: Tissue Simulant Liquid for Head 2450</p>	<p>Photo 6: Tissue Simulant Liquid for Head 2600</p>
	
<p>Photo 7: Tissue Simulant Liquid for Head 5000</p>	<p>NA</p>



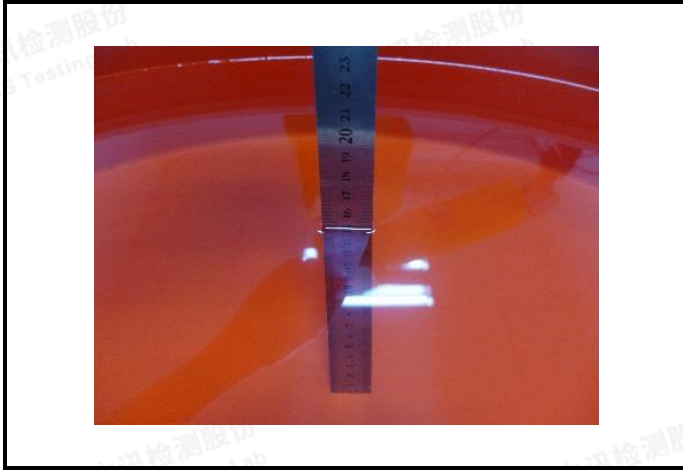

NA



3. Photographs of EUT test position

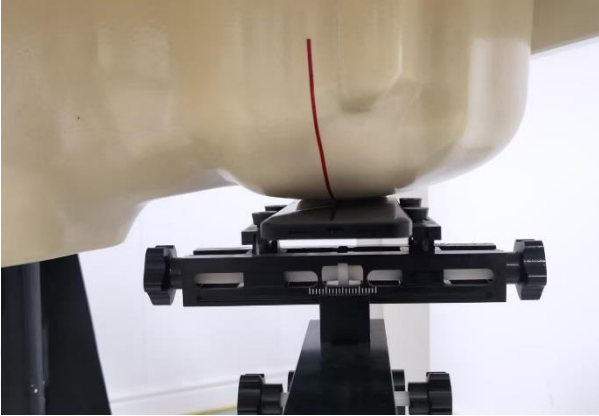

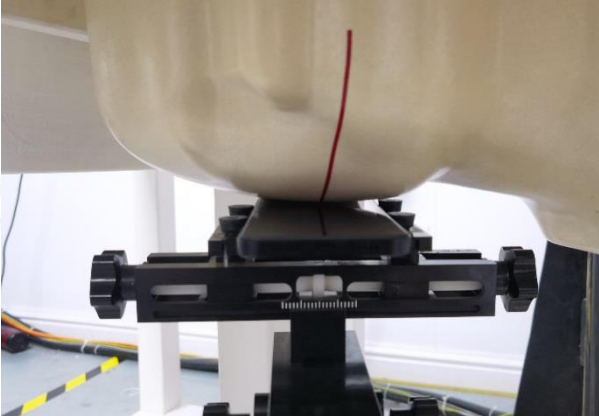
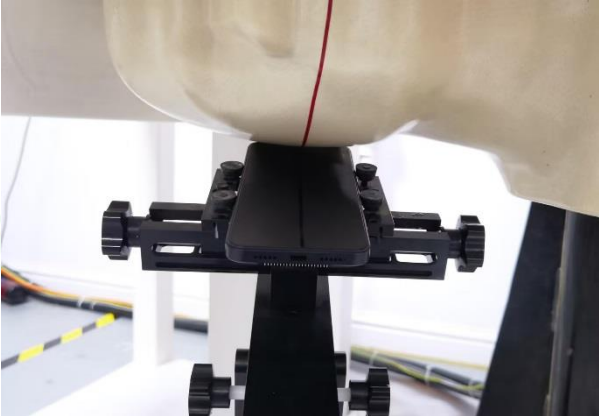






Photo 8: Left touch cheek	Photo 9: Left tilted 15 degree
	
Photo 10: Right touch cheek	Photo 11: Right tilted 15 degree
	
Photo 12: Front side 10mm	Photo 13: Back side 10mm
	





Photo 14: Left side 10mm	Photo 15: Right side 10mm
	
Photo 16: Top side 10mm	Photo 17: Bottom side 10mm
	



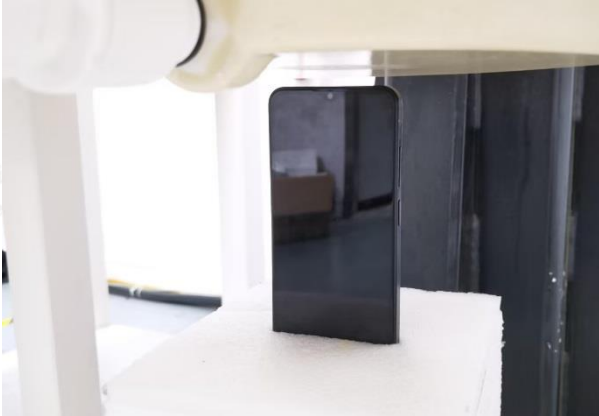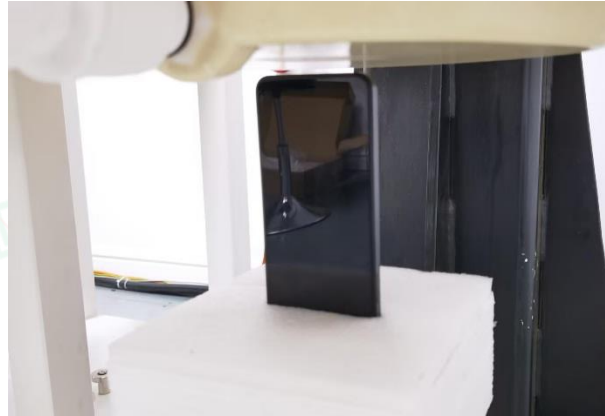

4. EUT Constructional Details

