



Appendix D

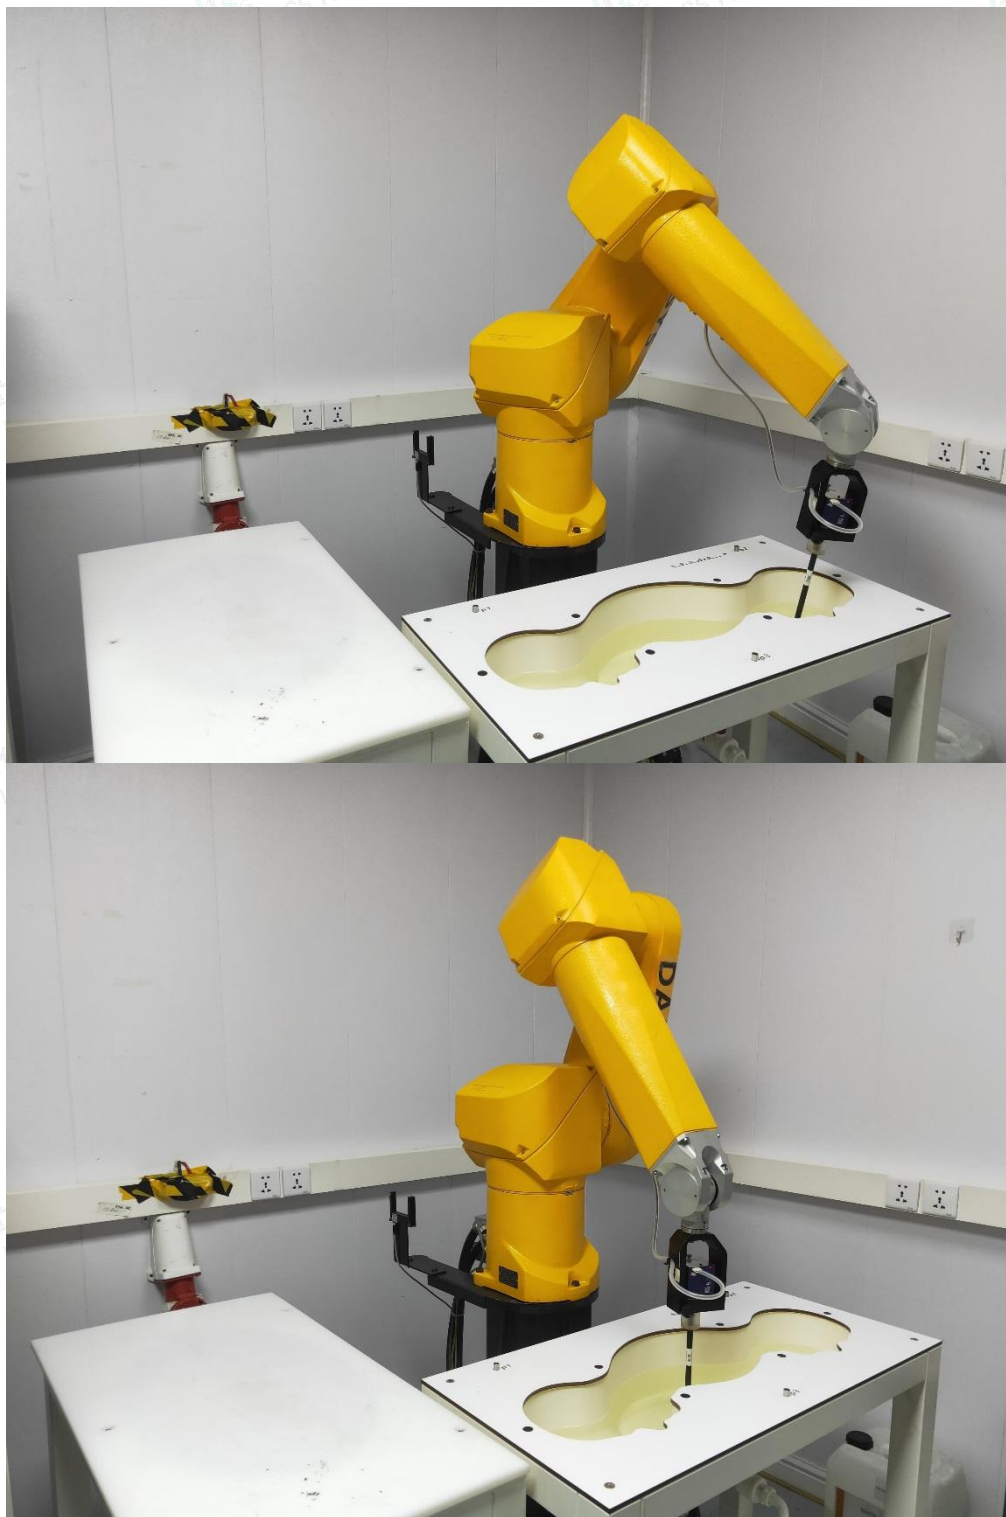
Photographs

- | |
|--|
| 1. SAR measurement System |
| 2. Photographs of Tissue Simulate Liquid |
| 3. Photographs of EUT test position |
| 4. EUT Constructional Details |



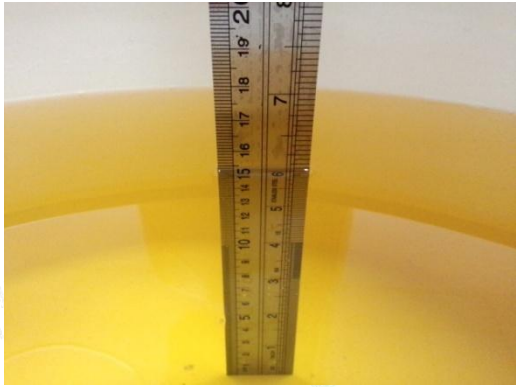
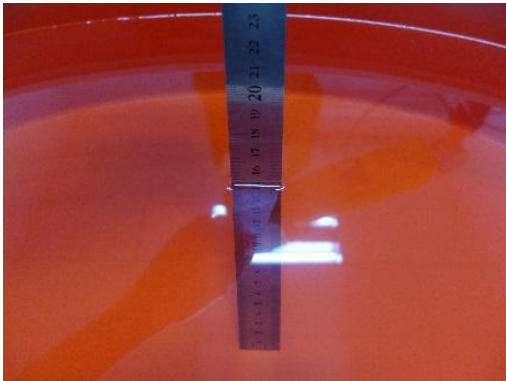


1. SAR measurement System





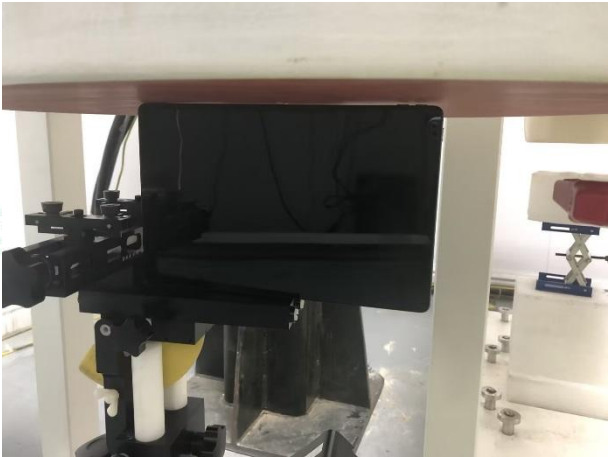
2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 650-900	Photo 2: Tissue Simulant Liquid for Head 1700-2000
	
Photo 3: Tissue Simulant Liquid for Head 2300-2500	Photo 4: Tissue Simulant Liquid for Head 2500-2700
	
Photo 5: Tissue Simulant Liquid for Head 5000-6000	N/A
	





3. Photographs of EUT test position

Photo 6: Back side 0mm	Photo 7: Left side 0mm
	
Photo 8: Top side 0mm	
	





4. EUT Constructional Details

