



## **FCC/ISED Test Setup Photos**

**For:**  
Smith & Nephew Medical, Ltd.

**Model Number:**  
66803060

**Product Description:**  
LEAF Patient sensor is a wireless, disposable patient monitoring sensor that continuously monitors the patient's orientation and movements.

**FCC ID:** 2AWH9-LEAFS

**Addition to Report #:** EMC\_SMITH-013-20001\_FCC\_15.247\_Rev1

**DATE:** 2021-09-28


***CETECOM Inc.***

411 Dixon Landing Road ♦ Milpitas, CA 95035 ♦ U.S.A.

Phone: + 1 (408) 586 6200 ♦ Fax: + 1 (408) 586 6299 ♦ E-mail: [info@cetecom.com](mailto:info@cetecom.com) ♦ <http://www.cetecom.com>  
*CETECOM Inc.* is a Delaware Corporation with Corporation number: 2905571

**Radiated Measurements**

9 KHz to 30 MHz

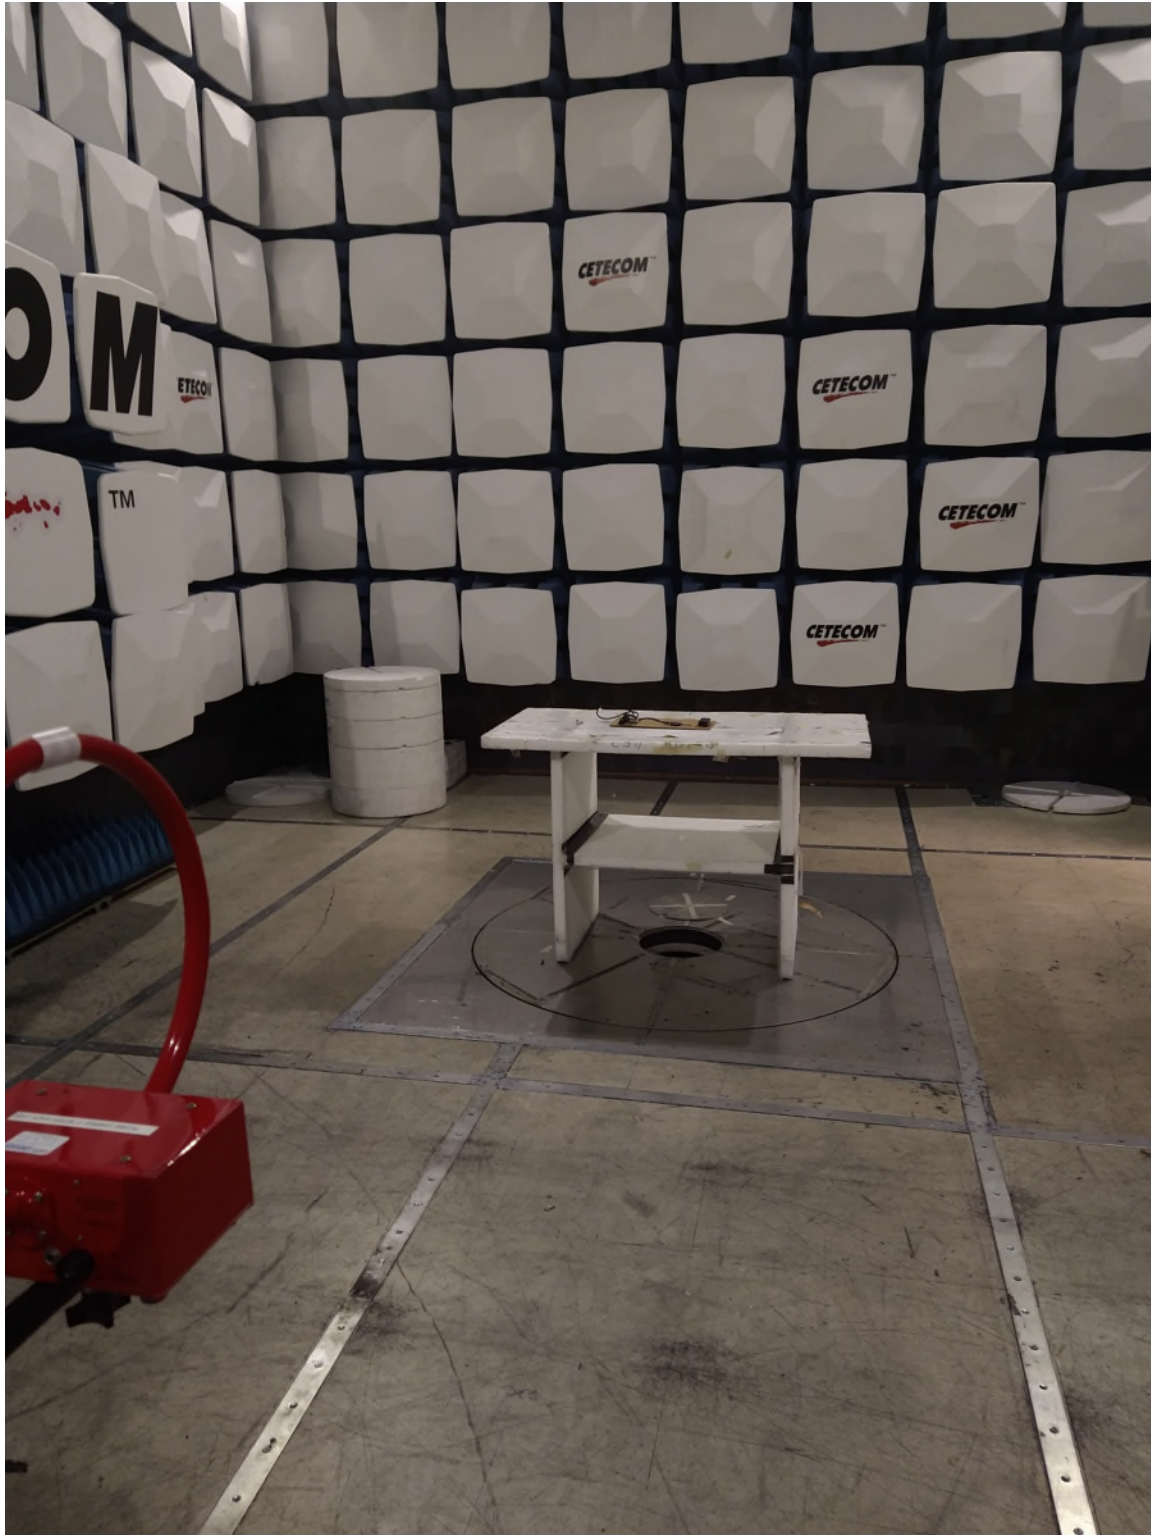

30 MHz to 1 GHz






1 GHz to 3 GHz



3 GHz to 18 GHz

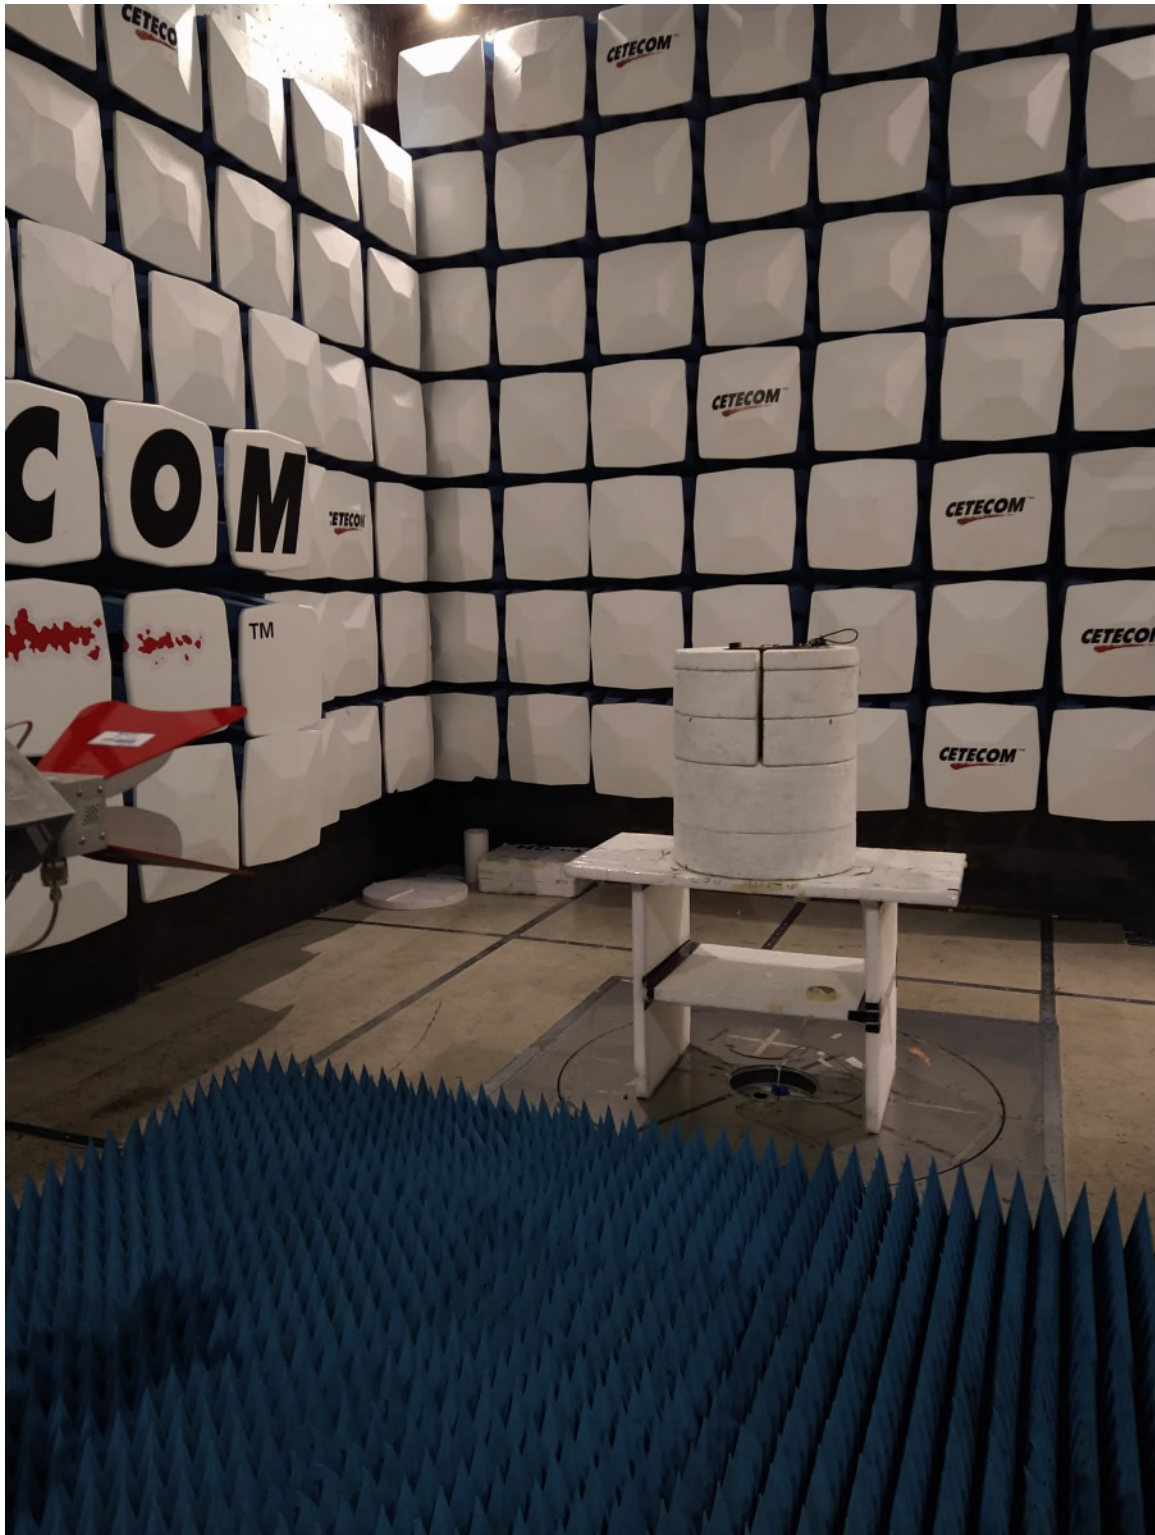




18 GHz to 26 GHz




Conducted RF

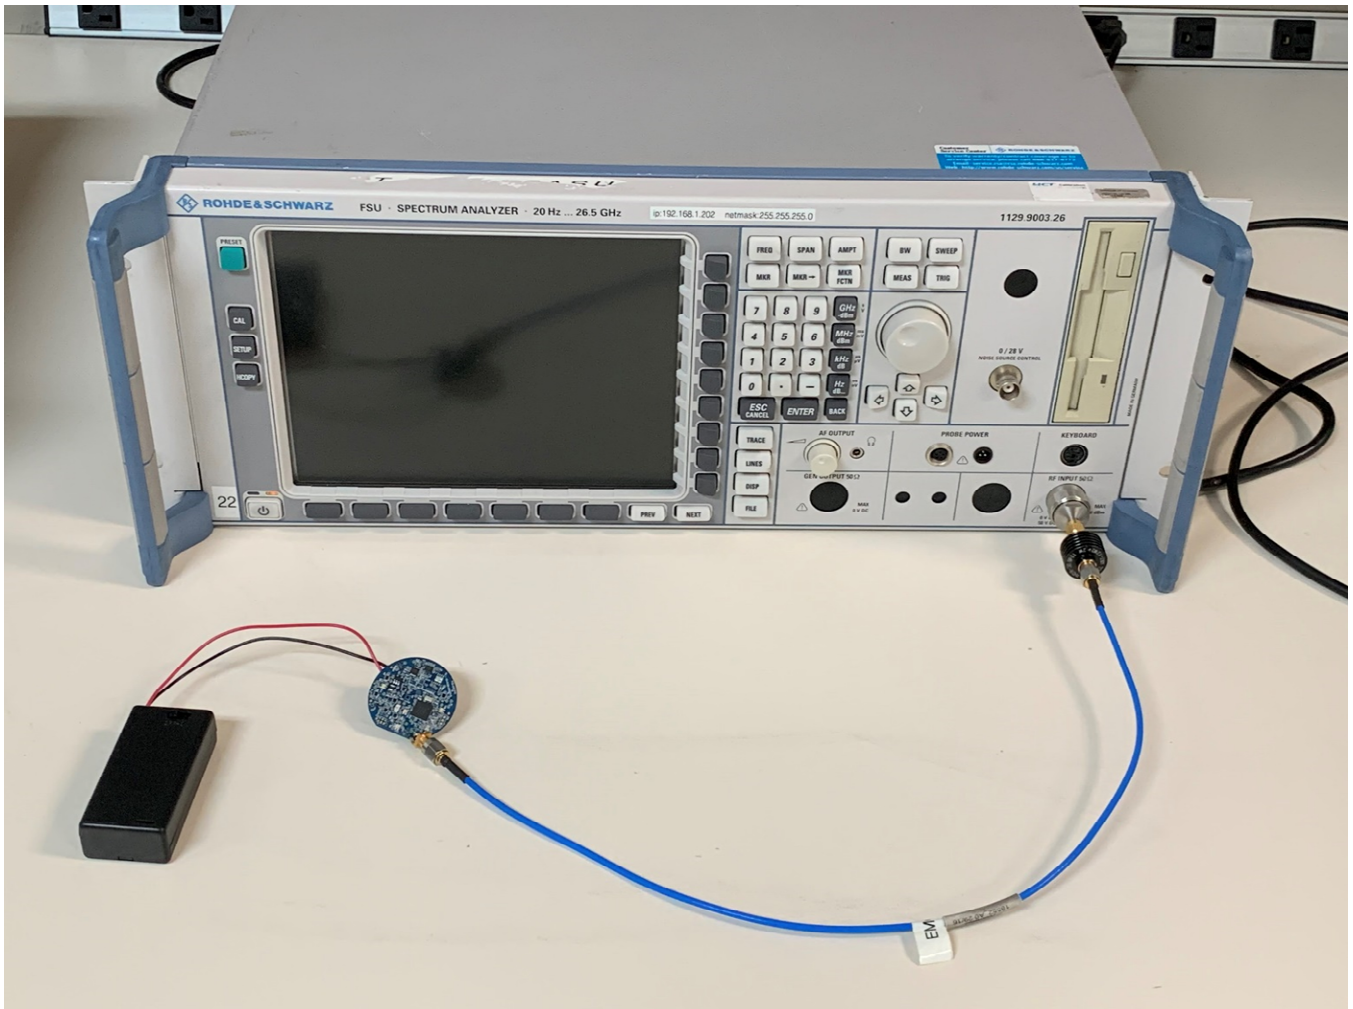

**EUT Photos**

---

EUT Top View

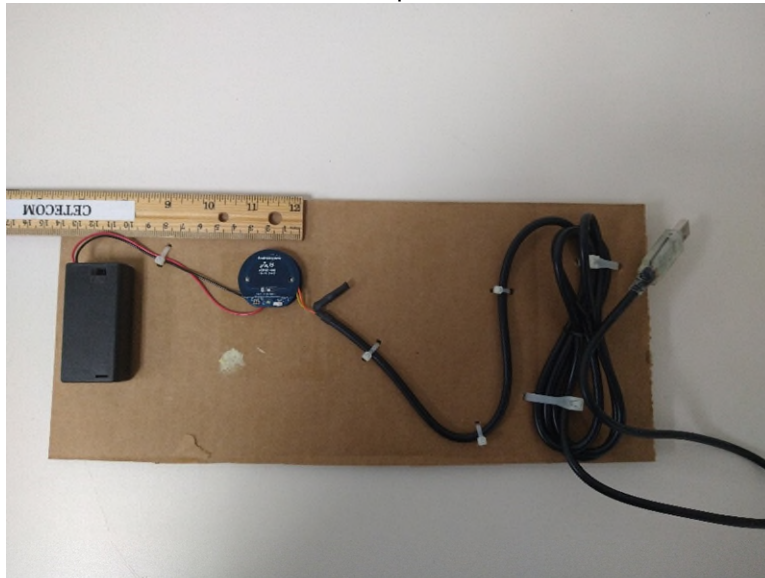

EUT Side View





<b>Date</b>	<b>Report Name</b>	<b>Changes to report</b>	<b>Prepared by</b>
2021-09-27	EMC_SMITH-013-20001_FCC_15.247_Setup_Photos	Initial Version	Cheng Song

<<< The End >>>