

TEST REPORT

Part 15.209



Equipment under test ANESTHESIA INJECTION
SYSTEM(CRADLE)
Model name AN100-C
FCC ID 2AXRNAN100-C
Applicant DENTIS CO., LTD
Manufacturer DENTIS MEDICAL DIVISIONTD
Date of test(s) 2023.04.20 ~ 2023.05.18
Date of issue 2023.05.22

Issued to**DENTIS CO., LTD**

99, Seongseoseo-ro, Dalseo-gu, Daegu, Republic of Korea
Tel: +82-53-589-3667

Issued by**KES Co., Ltd.**

3701, 40, Simin-daero 365beon-gil, Dongan-gu, Anyang-si,
Gyeonggi-do, 14057, Korea
473-21, Gayeo-ro, Yeosu-si, Gyeonggi-do, Korea
Tel: +82-31-425-6200 / Fax: +82-31-424-0450

Test and report completed by :	Report approval by :
	
Gu-Bong, Kang Test engineer	Yeong-Jun Cho Technical manager

This test report is not related to KS Q ISO/IEC 17025 and KOLAS



KES Co., Ltd.

3701, 40, Simin-daero 365beon-gil,
Dongan-gu, Anyang-si, Gyeonggi-do, 14057, Korea
Tel: +82-31-425-6200 / Fax: +82-31-424-0450
www.kes.co.kr

Report No.:
KES-RF-23T0066
Page (2) of (21)

Revision history

Revision	Date of issue	Test report No.	Description
-	2023.05.22	KES-RF-23T0066	Initial

This report shall not be reproduced except in full, without the written approval of KES Co., Ltd.
The results shown in this test report refer only to the sample(s) tested unless otherwise stated.
The authenticity of the test report, contact kes@kes.co.kr



TABLE OF CONTENTS

1.	General information	4
1.1.	EUT description	4
1.2.	Test configuration.....	4
1.3.	Test frequency	4
1.4.	Test mode	5
1.5.	Information about derivative model	5
1.6.	Accessory information.....	5
1.7.	Measurement Uncertainty	5
2.	Summary of tests	6
3.	Test results.....	7
3.1.	Radiated spurious emission	7
3.2.	20 dB Bandwidth	16
3.3.	AC conducted emissions	18
	Appendix A. Measurement equipment	20
	Appendix B. Test setup photo.....	21

This report shall not be reproduced except in full, without the written approval of KES Co., Ltd.

The results shown in this test report refer only to the sample(s) tested unless otherwise stated.

The authenticity of the test report, contact kes@kes.co.kr



KES Co., Ltd.

3701, 40, Simin-daero 365beon-gil,
Dongan-gu, Anyang-si, Gyeonggi-do, 14057, Korea
Tel: +82-31-425-6200 / Fax: +82-31-424-0450
www.kes.co.kr

Report No.:
KES-RF-23T0066
Page (4) of (21)

1. General information

Applicant DENTIS CO., LTD
Applicant address 99, Seongseoseo-ro, Dalseo-gu, Daegu, Republic of Korea
Test site KES Co., Ltd.
Test site address 3701, 40, Simin-daero 365beon-gil, Dongan-gu, Anyang-si, Gyeonggi-do, 14057, Korea
 473-29, Gayeo-ro, Yeosu-si, Gyeonggi-do, Korea
Test Facility FCC Accreditation Designation No.: KR0100, Registration No.: 444148
FCC rule part(s): Part 15.209
FCC ID: 2AXRNAN100-C
Test device serial No. Production Pre-production Engineering

1.1. EUT description

Equipment under test ANESTHESIA INJECTION SYSTEM(CRADLE)
Frequency 0.110 ~ 0.130 MHz
Inductive charging technique Magnetic Induction
Model: AN100-C
Antenna specification Internal type(Coil antenna)
Power source AC 120 V(Adapter DC output 5 V)
H/W version 1.0.0
S/W version 1.0.0

1.2. Test configuration

The **DENTIS CO., LTD / AN100-C / ANESTHESIA INJECTION SYSTEM(CRADLE) / FCC ID: 2AXRNAN100-C** was tested according to the specification of EUT, the EUT must comply with following standards.

FCC Part 15C
ANSI C63.10-2013

1.3. Test frequency

		Frequency Range
Power source	AC 120 V (Adapter DC output 5 V)	0.110 ~ 0.130 MHz

This report shall not be reproduced except in full, without the written approval of KES Co., Ltd.
The results shown in this test report refer only to the sample(s) tested unless otherwise stated.
The authenticity of the test report, contact kes@kes.co.kr

1.4. Test mode

Mode	Charging current	Description
Charging mode With load	90%	Using Max load
	50%	Using Mid load
	10%	Using Min load

1.5. Information about derivative model

N/A

1.6. Accessory information

Equipment	Manufacturer	Model	Serial No.	Power source
AC/DC Adapter	Adapter Technology Co., Ltd.	ATM012T-W050V	-	DC 5 V
ANESTHESIA INJECTION SYSTEM	DENTIS CO., LTD.	AN100	-	DC 3.7 V(Battery)

1.7. Measurement Uncertainty

Test Item	Uncertainty
Uncertainty for Conduction emission test	2.38 dB (SHIELD ROOM #6)
Uncertainty for Radiation emission test (include Fundamental emission)	Below 1GHz
	Above 1GHz
Note. This uncertainty represents an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of k=2.	

This report shall not be reproduced except in full, without the written approval of KES Co., Ltd.

The results shown in this test report refer only to the sample(s) tested unless otherwise stated.

The authenticity of the test report, contact kes@kes.co.kr



KES Co., Ltd.

3701, 40, Simin-daero 365beon-gil,
Dongan-gu, Anyang-si, Gyeonggi-do, 14057, Korea
Tel: +82-31-425-6200 / Fax: +82-31-424-0450
www.kes.co.kr

Report No.:
KES-RF-23T0066
Page (6) of (21)

2. Summary of tests

FCC Part Sections	Parameter	Test results
15.209	Radiated spurious emission	Pass
2.1049	20 dB Bandwidth	Pass
15.207	AC conducted emissions	Pass

NOTE.

1. This report is based on testing with the product to add an optional mainboard as a C2PC.


This report shall not be reproduced except in full, without the written approval of KES Co., Ltd.
The results shown in this test report refer only to the sample(s) tested unless otherwise stated.
The authenticity of the test report, contact kes@kes.co.kr

3. Test results


3.1. Radiated spurious emission

Test setup

The diagram below shows the test setup that is utilized to make the measurements for emission from 9 kHz to 30 MHz Emissions.

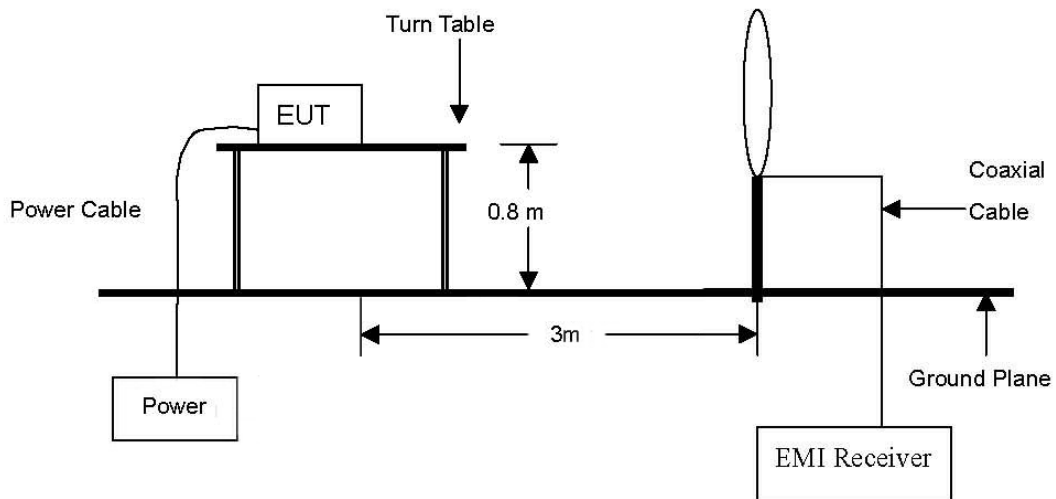

The diagram below shows the test setup that is utilized to make the measurements for emission from 30 MHz to 1 GHz emissions.

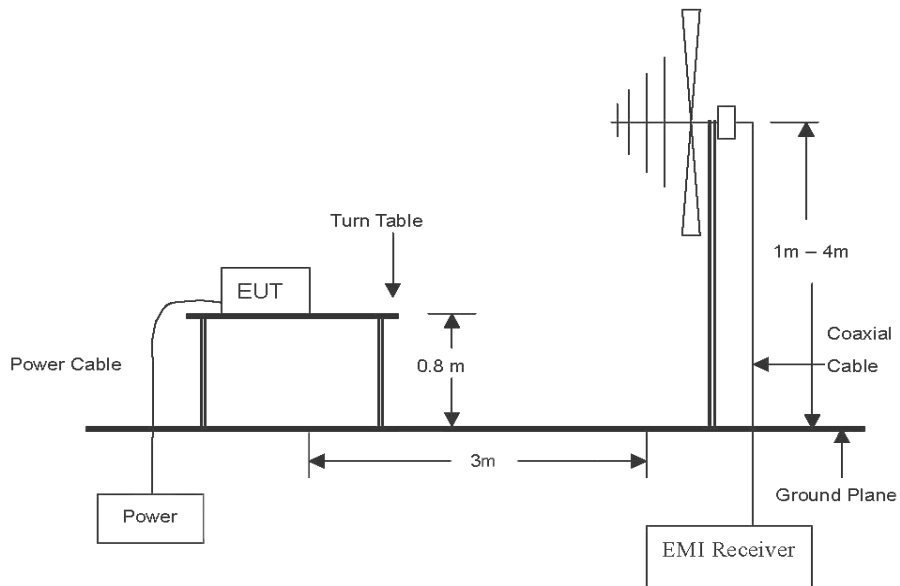

Test procedure

[9 kHz to 30 MHz]

The EUT was placed on the top of a rotating table 0.8 meter above the ground at a 3 meter anechoic chamber test site. The table was rotated 360 degrees to determine the position of the highest radiation. Then antenna is a loop antenna is fixed at one meter above the ground to determine the maximum value of the field strength. Both parallel and perpendicular and ground parallel of the antenna are set to make the measurement. For each suspected emission, the EUT was arranged to its worst case and then the table was turned from 0 degrees to 360 degrees to find the maximum reading. The test-receiver system was set to Quasi-peak function and specified bandwidth with maximum hold mode.

[30 MHz to 1 GHz]

The height of the measuring antenna was varied between 1 to 4 m and the table was rotated a full revolution in order to obtain maximum values of the electric field intensity.

The measurement was made in both the vertical and horizontal polarization, and the maximum value is presented in the report.

Note:

1. According to exploratory test no any obvious emission were detected from 9 kHz to 30 MHz. Although these tests were performed other than open area test site, adequate comparison measurements were confirmed against 30 m open area test site. Therefore sufficient tests were made to demonstrate that the alternative site produces results that correlate with the ones of tests made in an open field based on KDB 414788.
2. Measurement distance : 3 m.
3. Field strength = Level + Correction factor + F_d
4. $F_d = 40\log(D_m / D_s)$

Where:

 F_d = Distance factor in dB D_m = Measurement distance in meters D_s = Specification distance in metersFor 300m: $40\log(300/3) = 80$ dB for frequency band 0.009 MHz to 0.490 MHzFor 30m: $40\log(30/3) = 40$ dB for frequency band 0.490 MHz to 30 MHz

5. No significant emissions were found in the 90 - 110kHz restricted band.



KES Co., Ltd.

3701, 40, Simin-daero 365beon-gil,
Dongan-gu, Anyang-si, Gyeonggi-do, 14057, Korea
Tel: +82-31-425-6200 / Fax: +82-31-424-0450
www.kes.co.kr

Report No.:
KES-RF-23T0066
Page (9) of (21)

Limit

According to 15.209(a), for an intentional radiator devices, the general required of field strength of radiated emissions from unintentional radiators at a distance of 3 meters shall not exceed the following values :


Frequency (MHz)	Distance (Meters)	Radiated ($\mu\text{V}/\text{m}$)
0.009 ~ 0.490	300	2400 / F(kHz)
0.490 ~ 1.705	30	24000 / F(kHz)
1.705 ~ 30.0	30	30
30 ~ 88	3	100**
88 ~ 216	3	150**
216 ~ 960	3	200**
Above 960	3	500

**Except as provided in paragraph (g), fundamental emissions from intentional radiators operating under this Section shall not be located in the frequency bands 54 ~ 72 MHz, 76 ~ 88 MHz, 174 ~ 216 MHz or 470 ~ 806 MHz. However, operation within these frequency bands is permitted under other sections of this Part, e.g., Sections 15.231 and 15.241.

Test results (Below 30 MHz)

Mode: 5W // 10 % charger

Distance of measurement: 3 meter

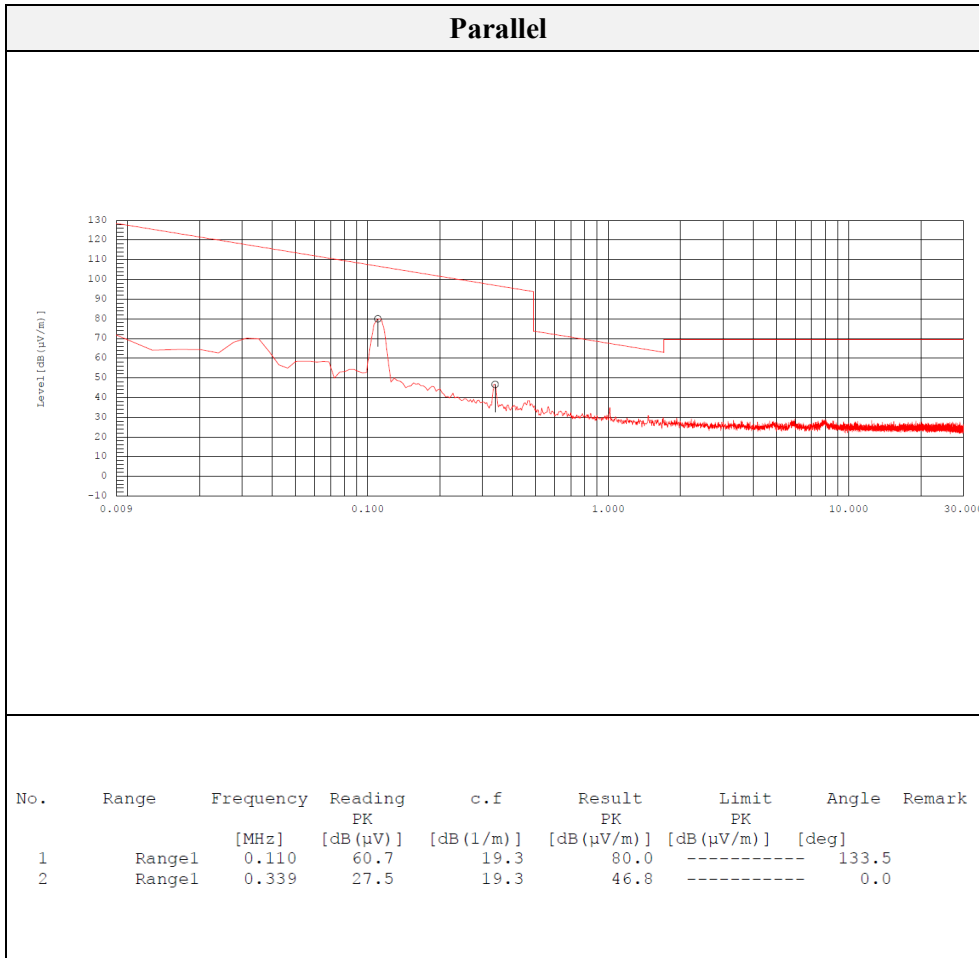


NOTE.

- Signal at 0.110 MHz is fundamental signal and the above test results are peak results.

Mode: 5W // 50 % charger

Distance of measurement: 3 meter

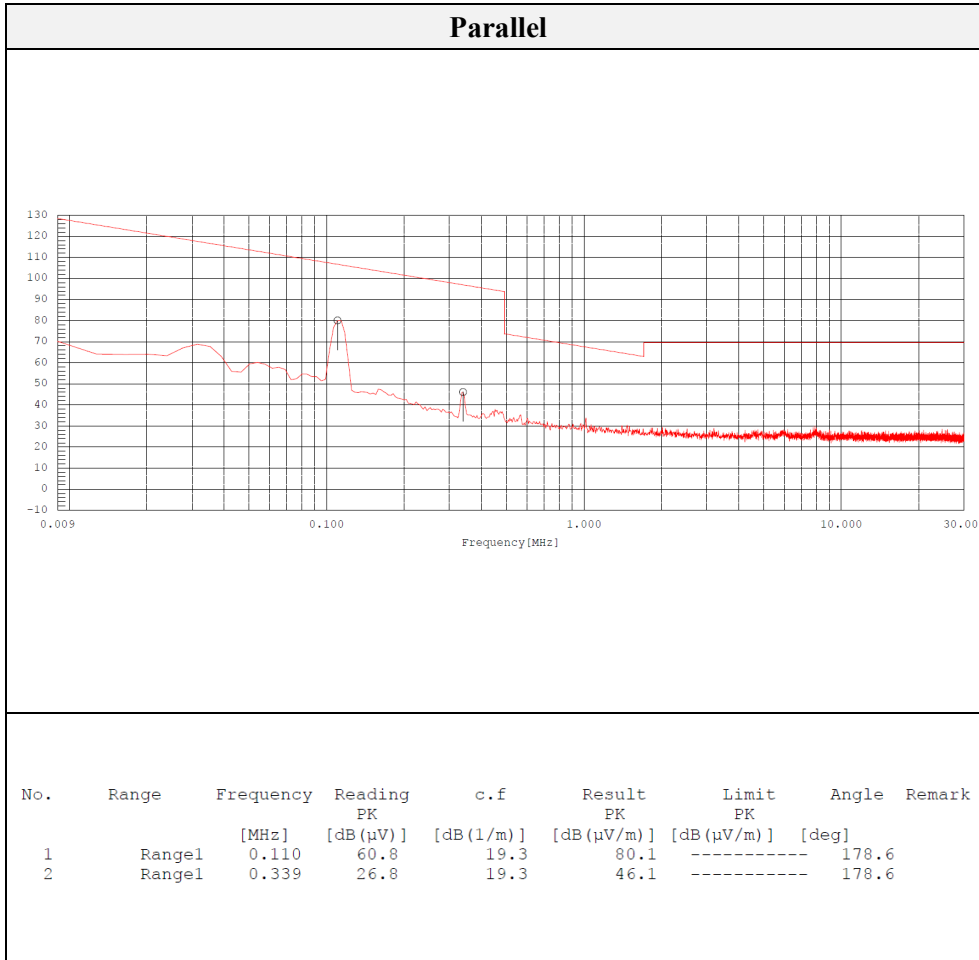


NOTE.

- Signal at 0.110 MHz is fundamental signal and the above test results are peak results.

Mode: 5W // 90 % charge

Distance of measurement: 3 meter

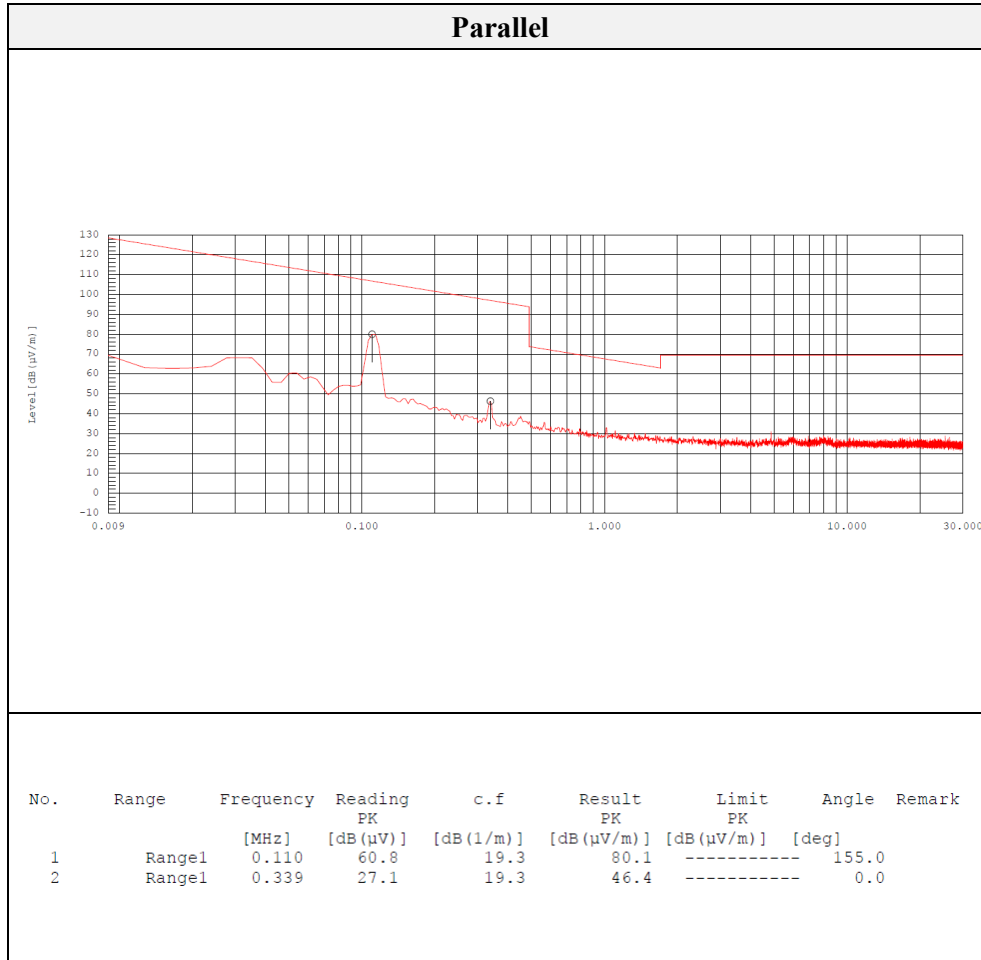

NOTE.

- Signal at 0.110 MHz is fundamental signal and the above test results are peak results.



KES Co., Ltd.

3701, 40, Simin-daero 365beon-gil,
 Dongan-gu, Anyang-si, Gyeonggi-do, 14057, Korea
 Tel: +82-31-425-6200 / Fax: +82-31-424-0450
 www.kes.co.kr


Report No.:
 KES-RF-23T0066
 Page (13) of (21)

Test results (Below 1 000 MHz)

Mode: 5W // 10 % charge

Distance of measurement: 3 meter

Horizontal // Vertical

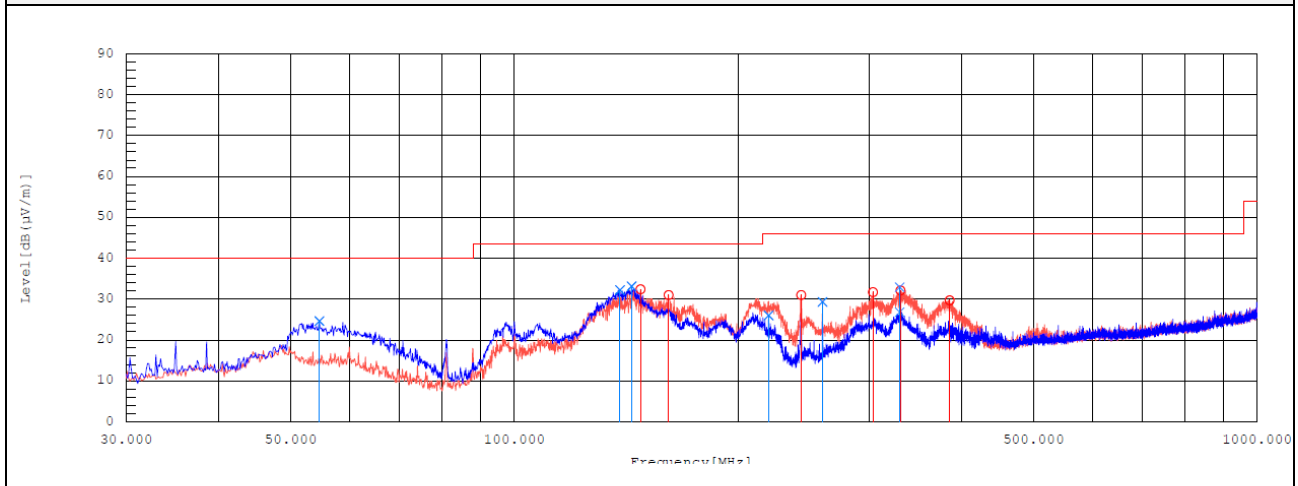

Final Result

No.	Frequency [MHz]	Pol	Reading QP [dB (µV)]	c.f [dB (1/m)]	Result QP [dB (µV/m)]	Limit QP [dB (µV/m)]	Margin QP [dB]	Height [cm]	Angle [deg]	Remark
1	54.614	V	36.8	-12.2	24.6	40.0	15.4	100.0	114.6	
2	138.761	V	48.3	-16.1	32.2	43.5	11.3	100.0	337.0	
3	143.854	V	49.4	-16.3	33.1	43.5	10.4	114.0	92.7	
4	147.855	H	48.8	-16.4	32.4	43.5	11.1	187.0	95.7	
5	161.314	H	46.5	-15.5	31.0	43.5	12.5	243.0	332.4	
6	219.999	V	38.1	-12.1	26.0	46.0	20.0	105.0	225.6	
7	243.279	H	42.3	-11.3	31.0	46.0	15.0	143.0	112.6	
8	260.011	V	40.2	-10.9	29.3	46.0	16.7	381.0	0.1	
9	303.904	H	41.6	-9.9	31.7	46.0	14.3	127.0	222.1	
10	330.215	V	41.6	-8.7	32.9	46.0	13.1	150.1	67.8	
11	331.064	H	40.8	-8.7	32.1	46.0	13.9	107.0	157.4	
12	385.626	H	37.1	-7.4	29.7	46.0	16.3	113.0	69.0	


This report shall not be reproduced except in full, without the written approval of KES Co., Ltd.

The results shown in this test report refer only to the sample(s) tested unless otherwise stated.

The authenticity of the test report, contact kes@kes.co.kr

Mode: 5W // 50 % charge

Distance of measurement: 3 meter

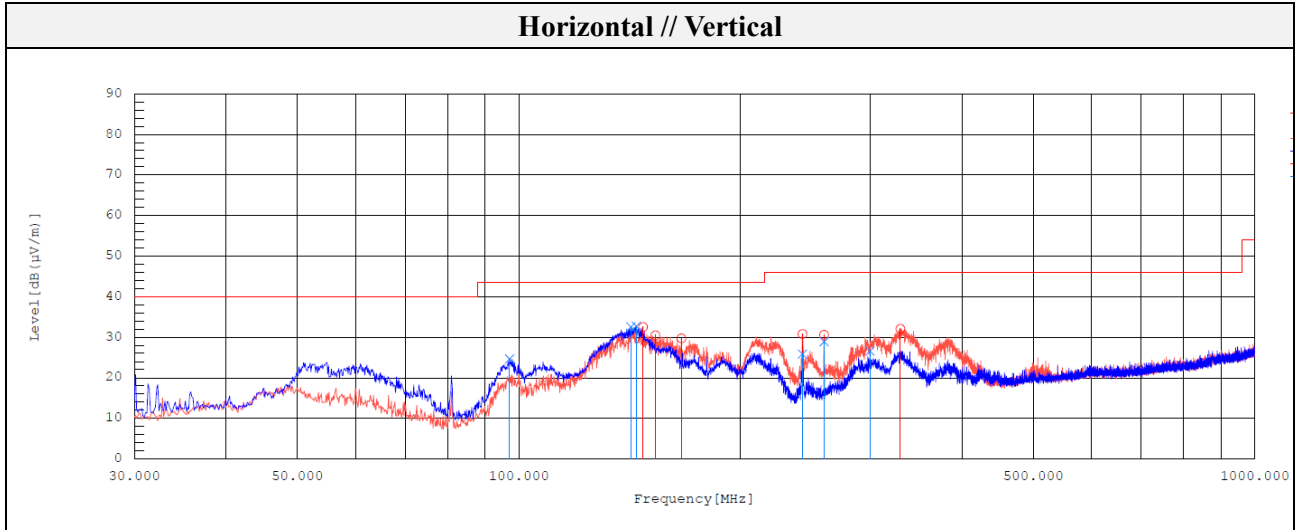

Final Result

No.	Frequency [MHz]	Pol	Reading QP [dB (µV)]	c.f [dB (1/m)]	Result QP [dB (µV/m)]	Limit QP [dB (µV/m)]	Margin QP [dB]	Height [cm]	Angle [deg]	Remark
1	97.173	V	38.6	-14.0	24.6	43.5	18.9	114.0	45.3	
2	142.035	V	48.8	-16.3	32.5	43.5	11.0	147.0	135.9	
3	144.460	V	49.0	-16.3	32.7	43.5	10.8	100.0	0.0	
4	147.491	H	48.9	-16.4	32.5	43.5	11.0	186.0	27.5	
5	153.311	H	46.7	-16.2	30.5	43.5	13.0	241.0	268.3	
6	166.285	H	44.8	-15.1	29.7	43.5	13.8	214.0	68.2	
7	242.915	H	42.1	-11.3	30.8	46.0	15.2	105.0	141.5	
8	242.915	V	37.1	-11.3	25.8	46.0	20.2	157.0	337.3	
9	260.011	H	41.5	-10.9	30.6	46.0	15.4	104.0	55.3	
10	260.011	V	39.8	-10.9	28.9	46.0	17.1	357.0	89.9	
11	300.024	V	36.6	-10.0	26.6	46.0	19.4	142.0	314.7	
12	329.851	H	40.8	-8.7	32.1	46.0	13.9	104.0	0.8	


This report shall not be reproduced except in full, without the written approval of KES Co., Ltd.

The results shown in this test report refer only to the sample(s) tested unless otherwise stated.

The authenticity of the test report, contact kes@kes.co.kr

Mode: 5W // 90 % charge

Distance of measurement: 3 meter

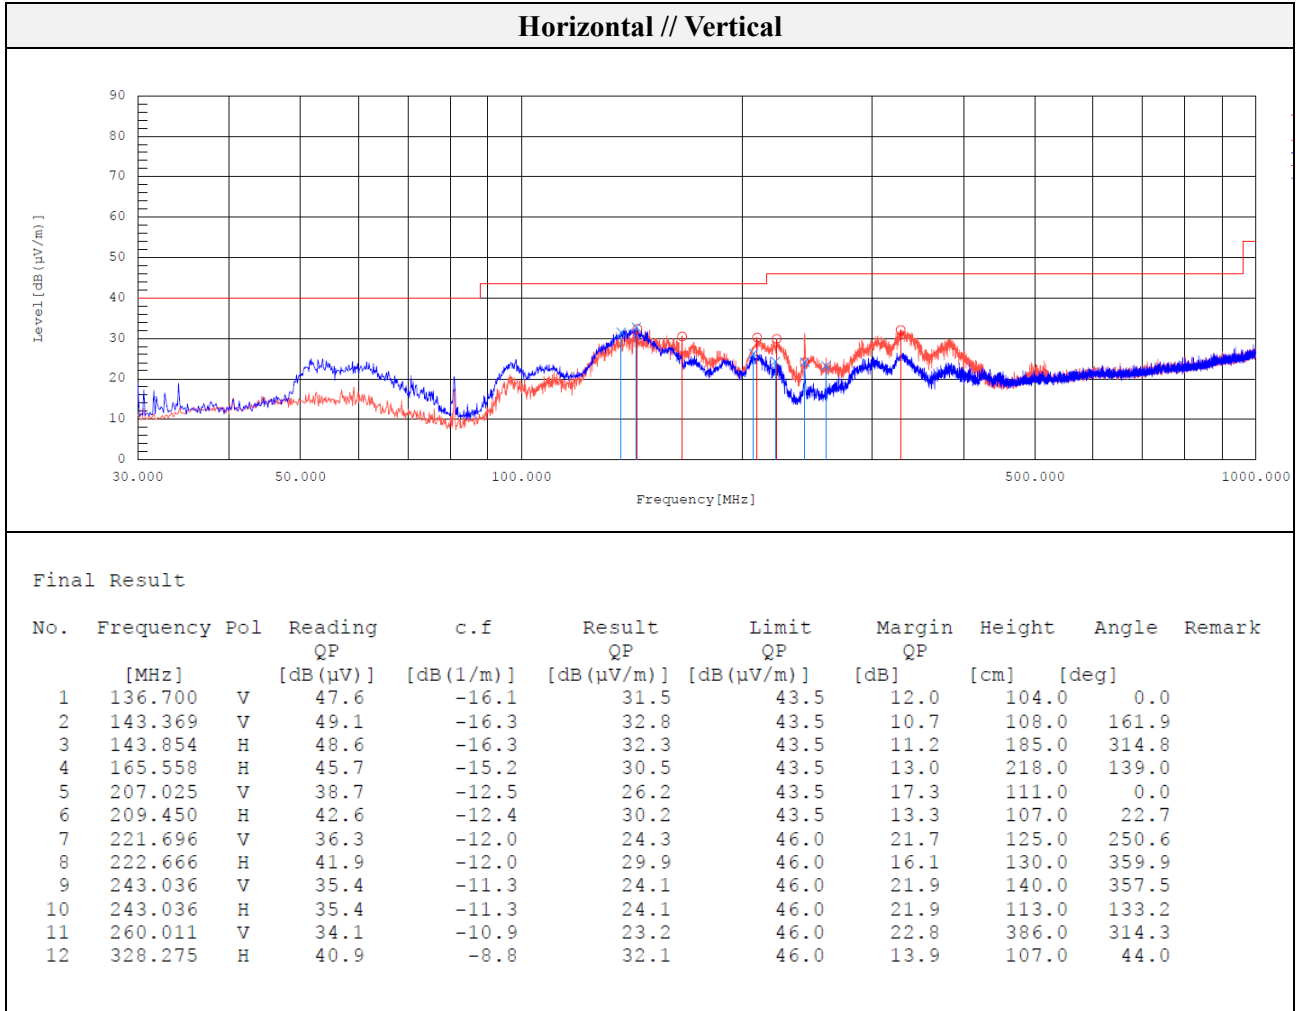


This report shall not be reproduced except in full, without the written approval of KES Co., Ltd.

The results shown in this test report refer only to the sample(s) tested unless otherwise stated.

The authenticity of the test report, contact kes@kes.co.kr

3.2. 20 dB Bandwidth

Test setup



Test procedures


The transmitter output is connected to a spectrum analyzer. The RBW is set to $\geq 1\%$ of the emission bandwidth. The VBW is set to \geq RBW. The sweep time is coupled.

Limit

None; for reporting purposes only.

Test results

Test Mode	Frequency(MHz)	Measured bandwidth(kHz)
5W	0.110	0.500

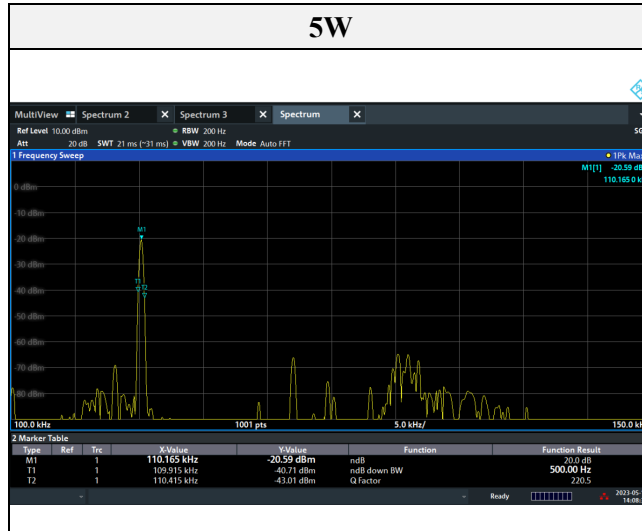

Note.

Because the measured signal is CW/CW-like, adjusting the RBW per C63.10 would not be practical since measured bandwidth will always follow the RBW and the result will be approximately twice the RBW.

3.3. AC conducted emissions


Limit

According to 15.207(a), for an intentional radiator that is designed to be connected to the public utility (AC) power line, the radio frequency voltage that is conducted back onto the AC power line on any frequency or frequencies, within the band 150 kHz to 30 MHz, shall not exceed the limits in the following table, as measured using a 50uH/50 ohm line impedance stabilization network (LISN). Compliance with the provision of this paragraph shall on the measurement of the radio frequency voltage between each power line and ground at the power terminal. The lower applies at the boundary between the frequencies ranges.

Frequency of Emission (MHz)	Conducted limit (dB μ V)	
	Quasi-peak	Average
0.15 – 0.50	66 - 56*	56 - 46*
0.50 – 5.00	56	46
5.00 – 30.0	60	50

Test results

Mode: 5W // 10 % charge
(Worst Case)

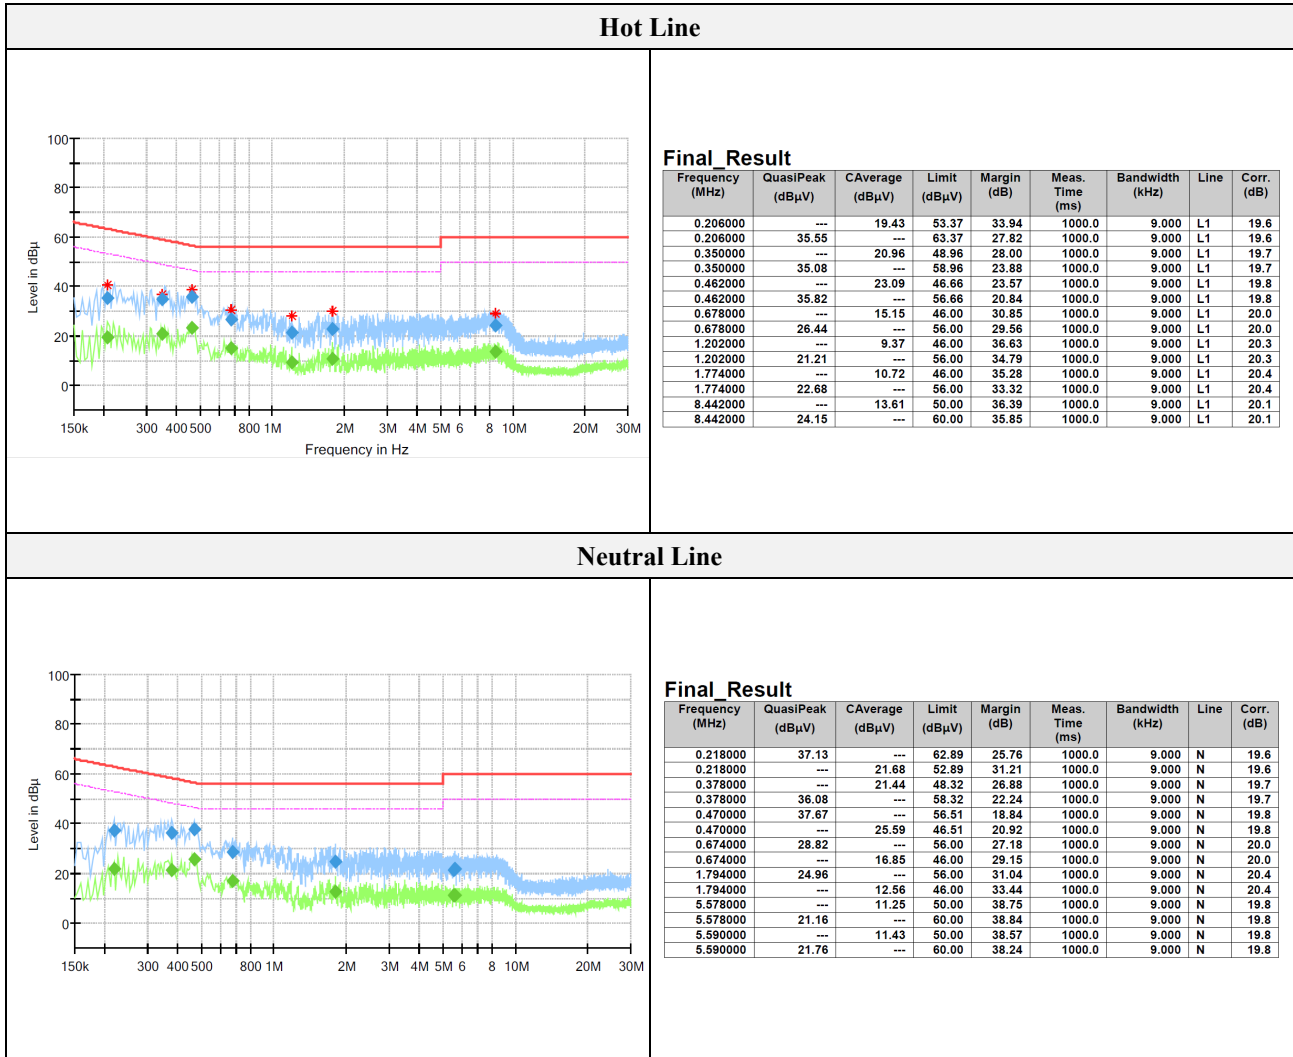

This report shall not be reproduced except in full, without the written approval of KES Co., Ltd.
The results shown in this test report refer only to the sample(s) tested unless otherwise stated.

The authenticity of the test report, contact kes@kes.co.kr



KES Co., Ltd.

3701, 40, Simin-daero 365beon-gil,
Dongan-gu, Anyang-si, Gyeonggi-do, 14057, Korea
Tel: +82-31-425-6200 / Fax: +82-31-424-0450
www.kes.co.kr

Report No.:
KES-RF-23T0066
Page (20) of (21)

Appendix A. Measurement equipment

Equipment	Manufacturer	Model	Serial No.	Calibration interval	Calibration due.
Spectrum Analyzer	R&S	FSV40-N	102194	1 year	2023.08.11
Spectrum Analyzer	R&S	FSV3044	101272	1 year	2024.03.16
AC POWER SOURCE/ ANALYZER	HP	6813A	3729A00754	1 year	2024.01.12
8360B Series Swept Signal Generator	HP	83630B	3844A00786	1 year	2024.01.12
Loop Antenna	Schwarzbeck	FMZB1513	1513-257	2 years	2025.01.16
TRILOG- BROADBAND ANTENNA	Schwarzbeck	VULB 9163	714	2 years	2024.04.19
Attenuator	HUBER+SHHNER	6806.17.A	NONE	1 year	2024.03.21
Amplifier	SONOMA INSTRUMENT	310N	186549	1 year	2024.03.21
EMI Test Receiver	R&S	ESU26	100517	1 year	2023.08.01
EMI Test Receiver	R&S	ESR3	101783	1 year	2023.11.11
PULSE LIMITER	R&S	ESH2-Z2	101915	1 year	2023.11.10
LISN	R&S	ENV216	101787	1 year	2023.11.10

Peripheral device

Device	Manufacturer	Model No.	S/N	Note
ANESTHESIA INJECTION SYSTEM	DENTIS CO., LTD.	AN100	-	DC 3.7 V(Battery)

This report shall not be reproduced except in full, without the written approval of KES Co., Ltd.
The results shown in this test report refer only to the sample(s) tested unless otherwise stated.
The authenticity of the test report, contact kes@kes.co.kr