



## Moisture analyzer MA X2 - external photographs

### 1. Device equipped with internal calibration

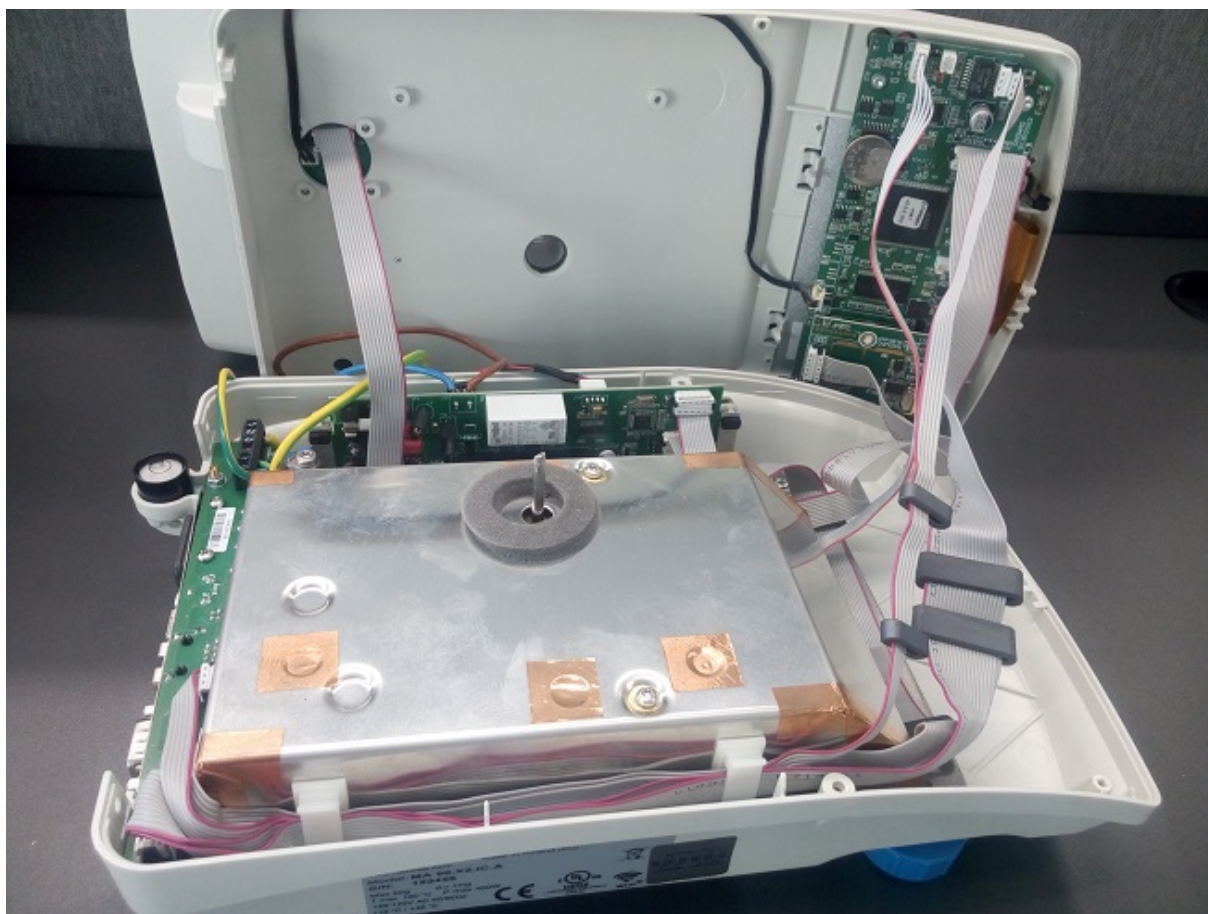


Both parts of housing

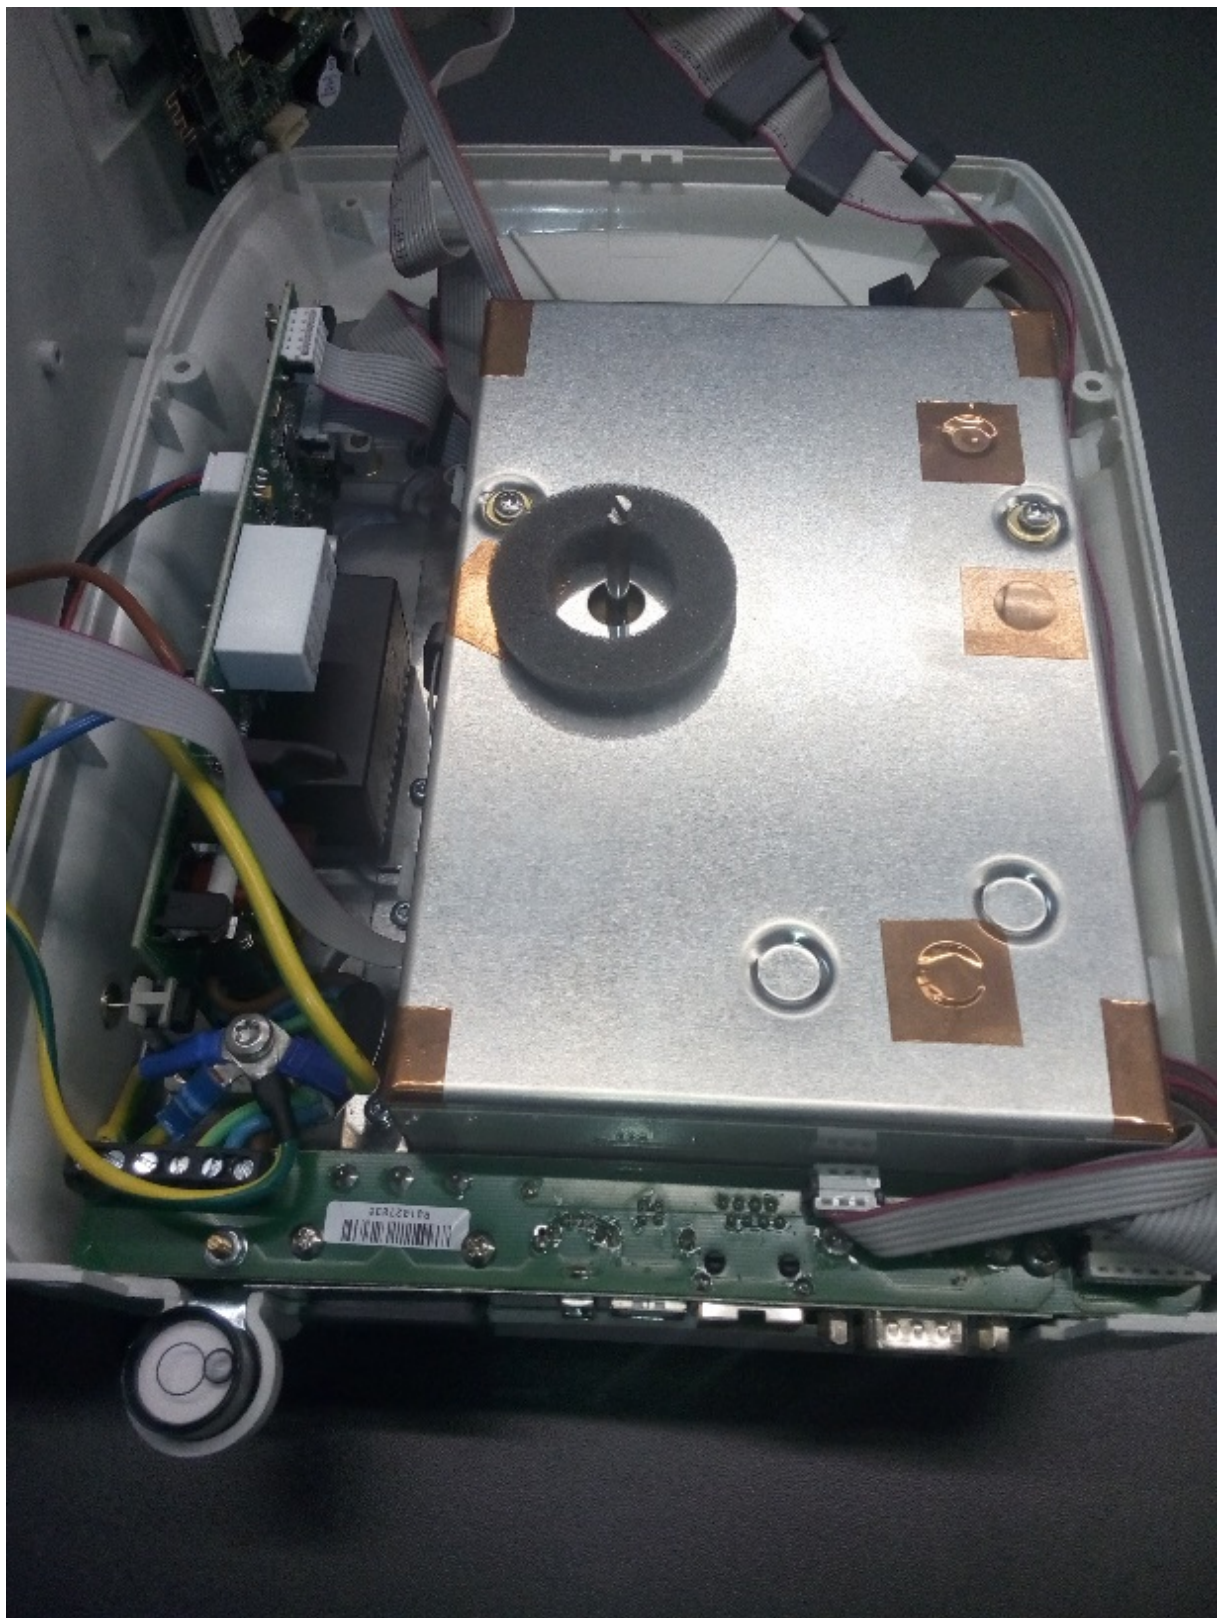


Bottom part



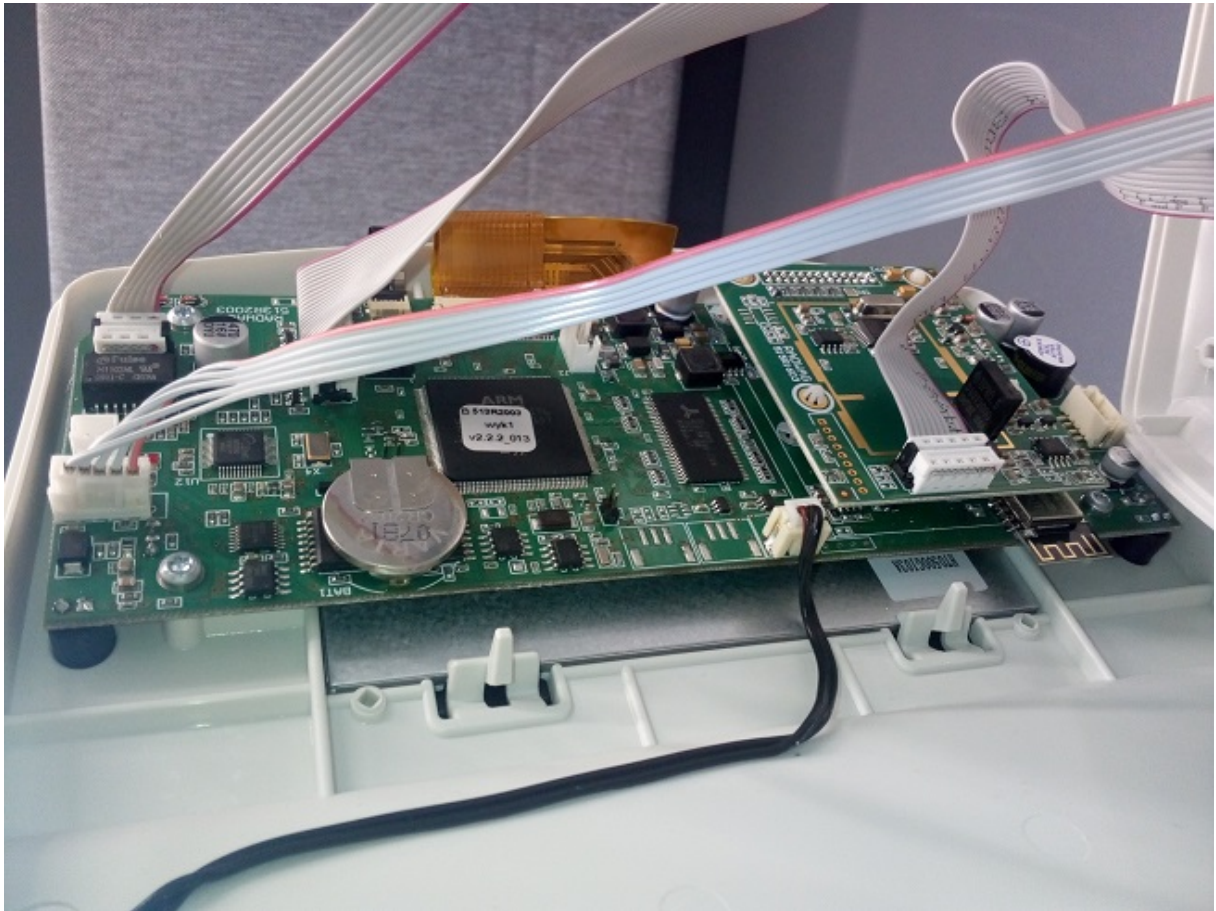


Top part

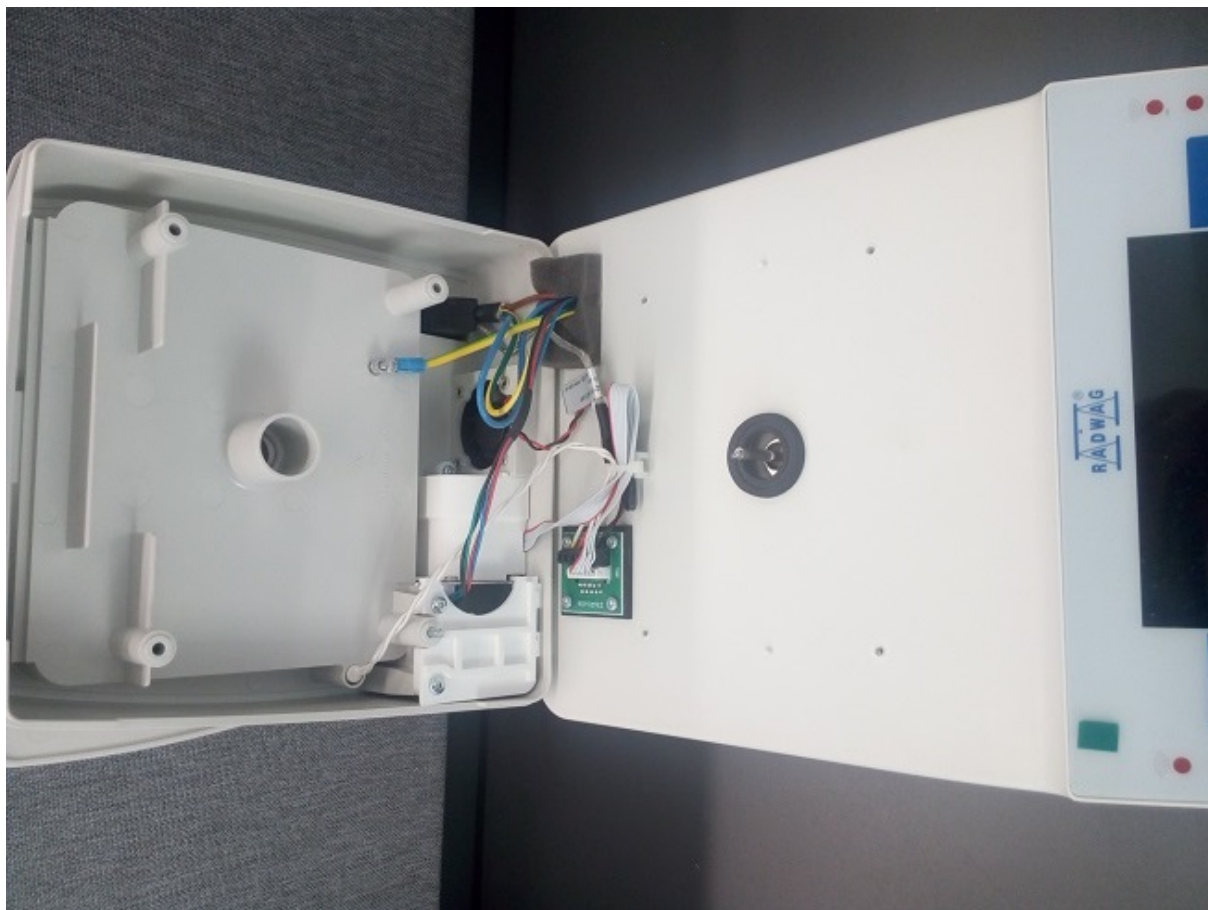


A cooling chamber under the weighing pan

2. Device not equipped with internal calibration

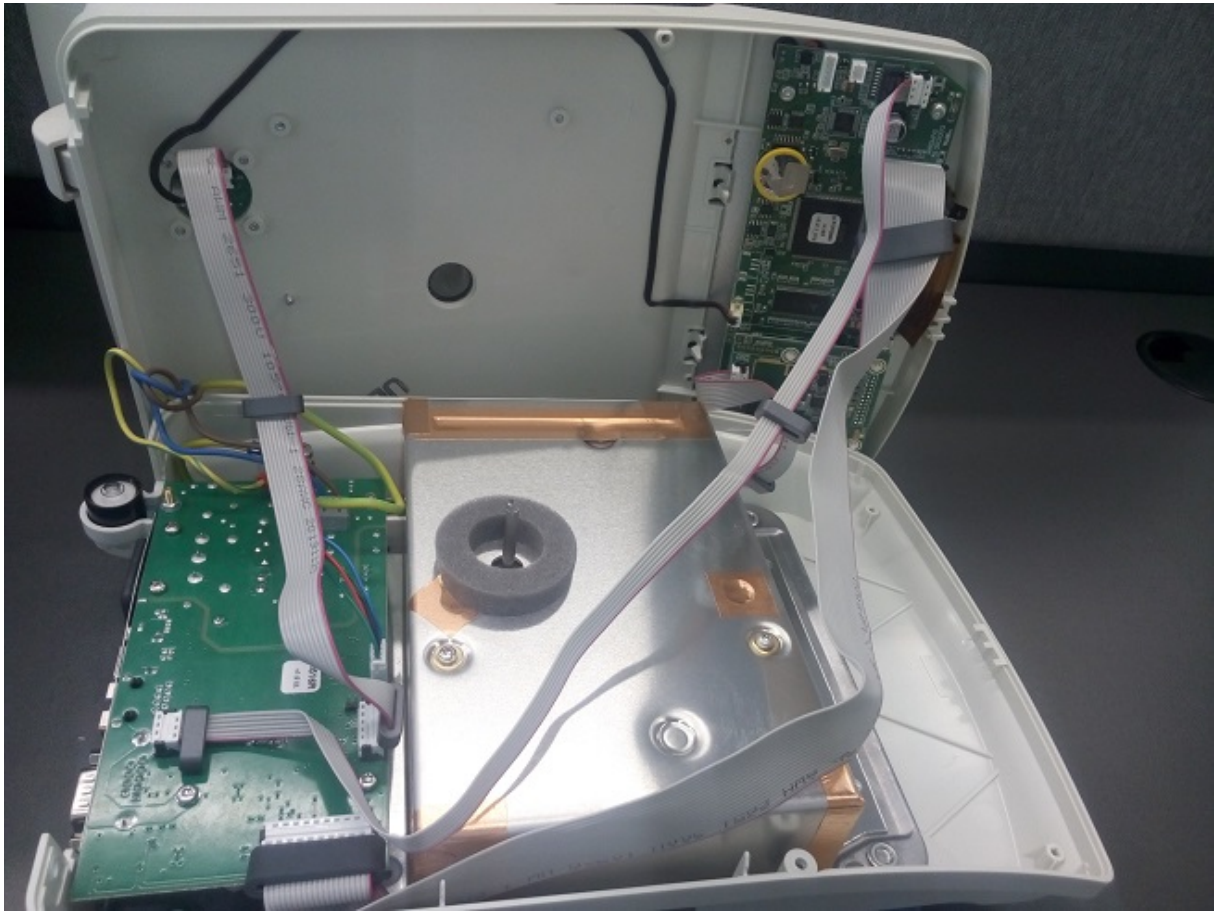

Both parts of housing

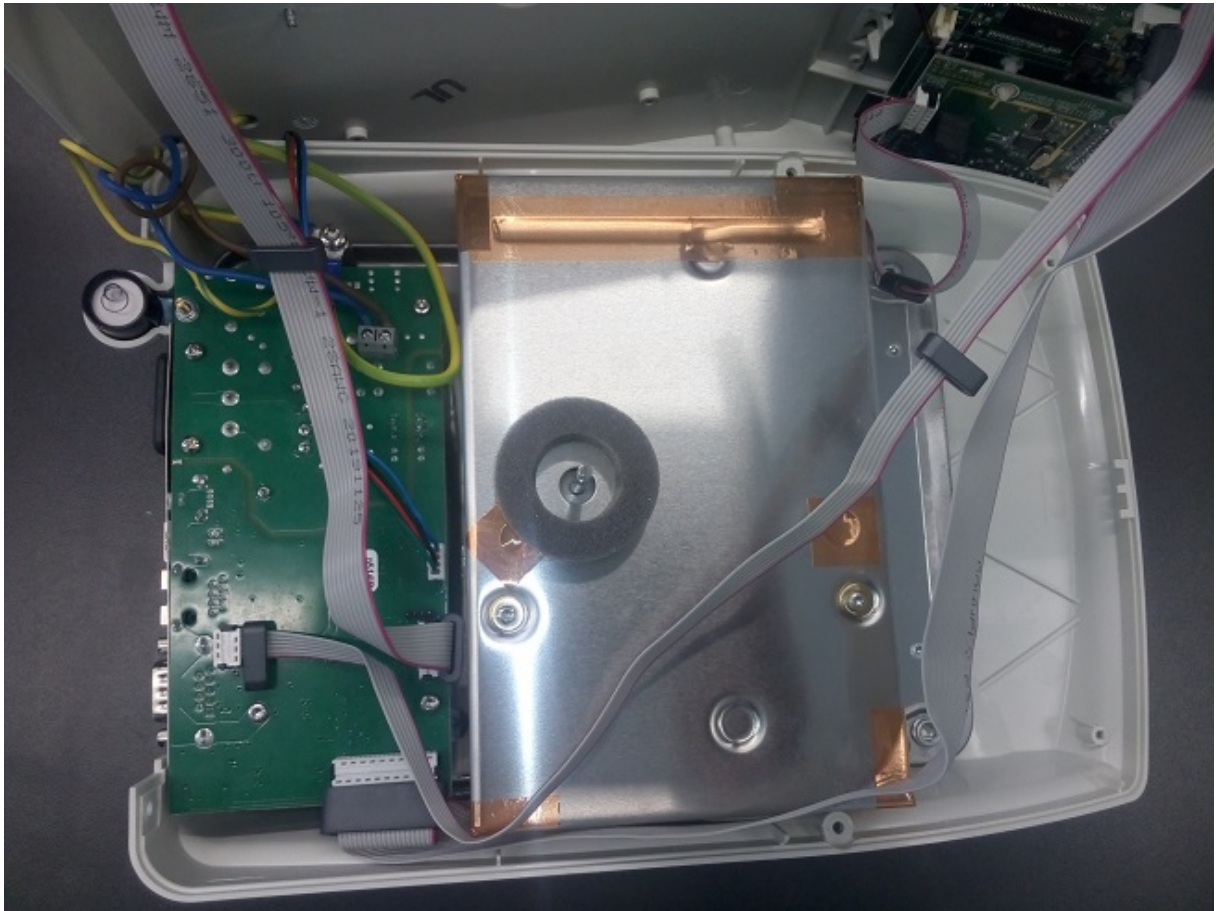


Bottom part





Top part

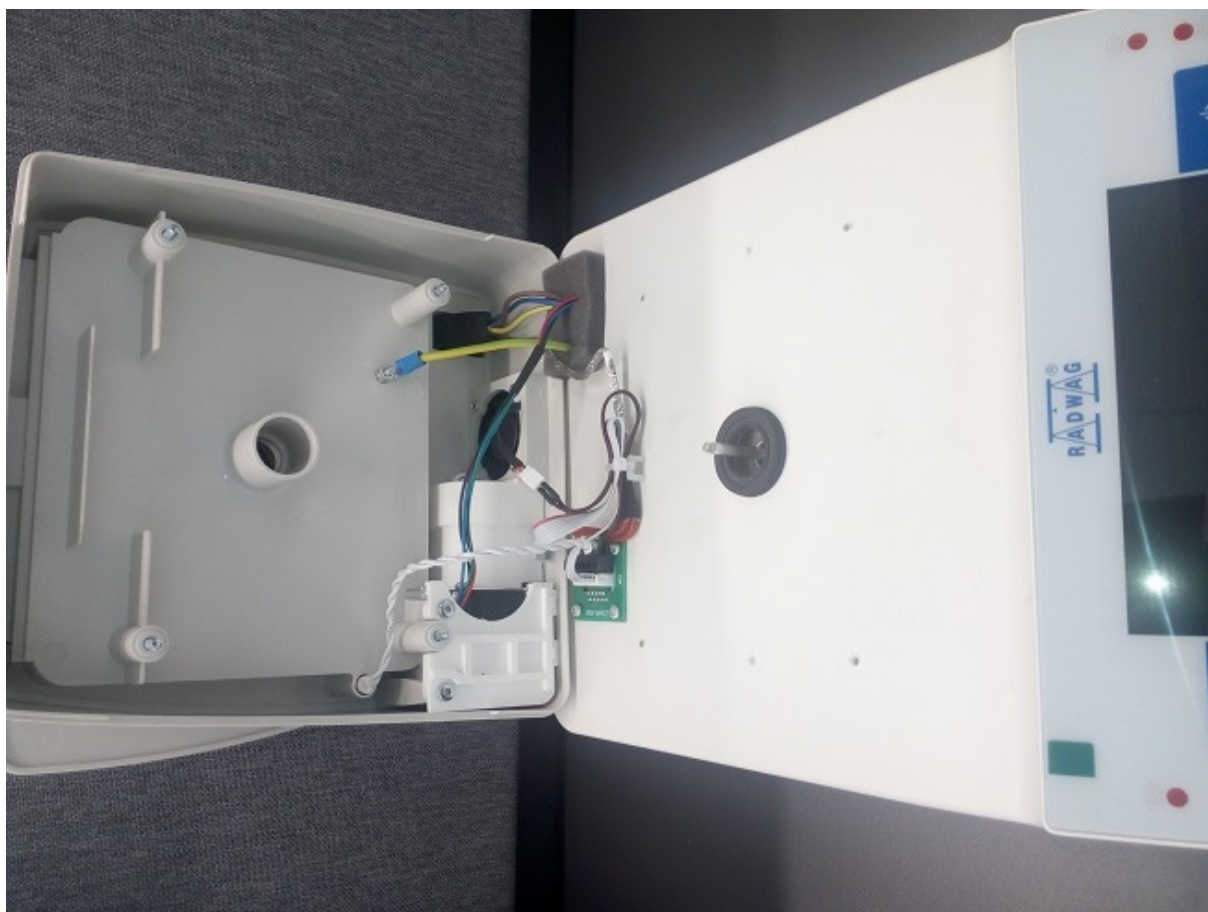

A cooling chamber under the weighing pan