



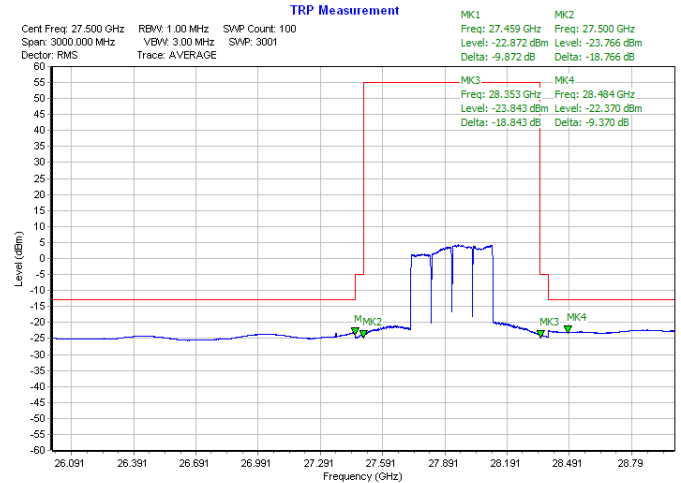


NR Band n261 / 400MHz / QPSK

Lowest Band Edge

Middle Band Edge

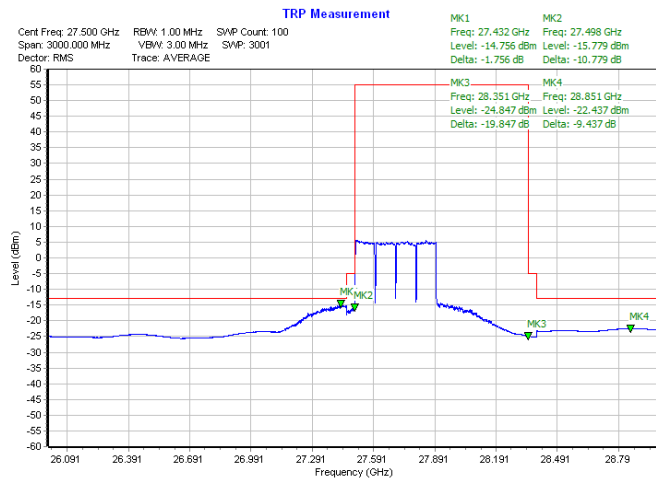

Highest Band Edge

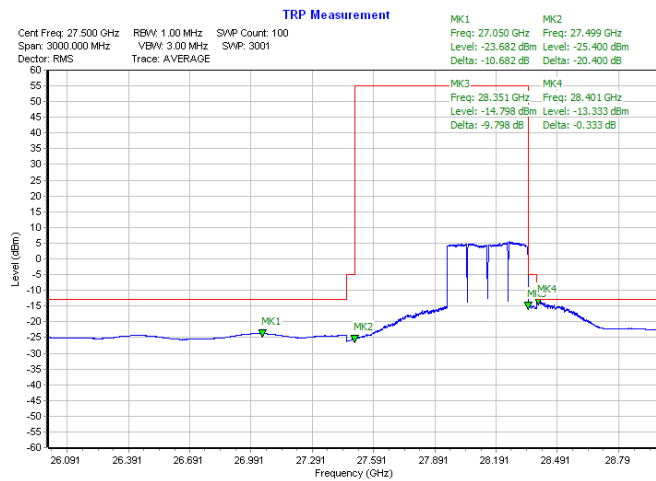


Spurious Emission

There is no significant spurious emission signal found for frequency started from 30MHz up to 18GHz.
Only the noise floor is reported.

NR Band n261 (30MHz-1GHz)

Horizontal

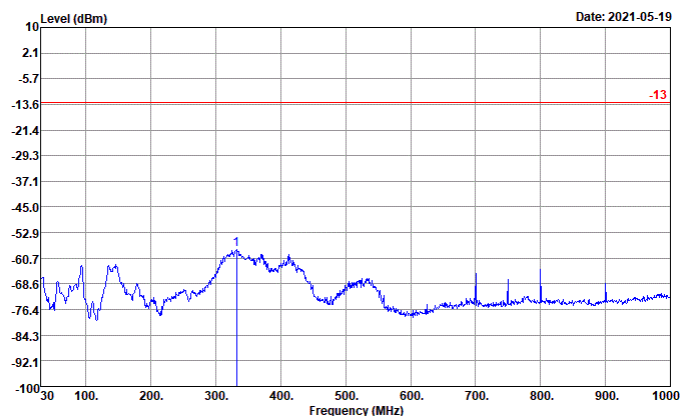

Site : 03CH19-HY
Condition : -13 ERP EIRP_20210305 HORIZONTAL
Project : 142801


Freq	Level	Over	Limit
MHz	dBm	Limit	Line
1	331.67	-57.97	-44.97 -13.00

Vertical




Site : 03CH19-HY
Condition : -13 ERP EIRP_20210305 VERTICAL
Project : 142801

Freq	Level	Over	Limit
MHz	dBm	Limit	Line
1	90.14	-57.07	-44.07 -13.00

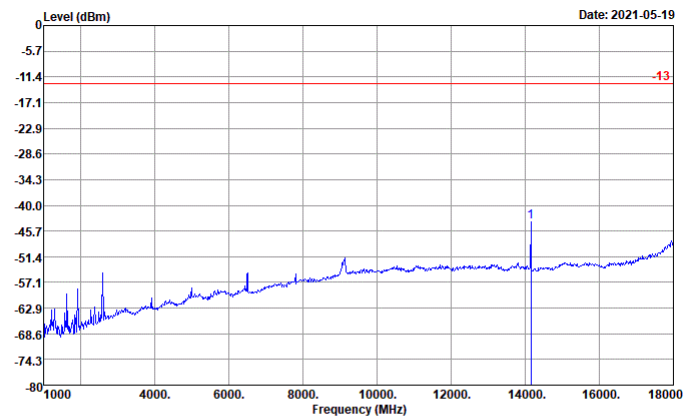**NR Band n261 (1GHz-18GHz)****Horizontal**

Site : 03CH19-HY
Condition : -13 ERP EIRP_20210305 HORIZONTAL
Project : 142801

Freq	Level	Over	Limit
		Limit	Line
MHz	dBm	dB	dBm
1 14158.00	-43.67	-30.67	-13.00

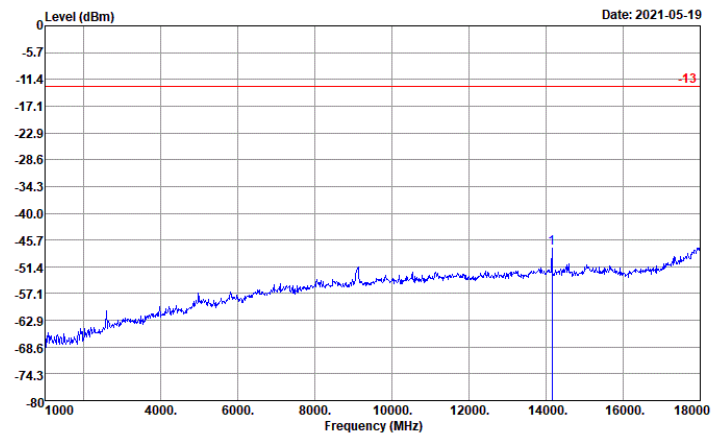
Vertical

Site : 03CH19-HY
Condition : -13 ERP EIRP_20210305 VERTICAL
Project : 142801


Freq	Level	Over	Limit
		Limit	Line
MHz	dBm	dB	dBm
1 14158.00	-47.36	-34.36	-13.00



Spurious emission between 18GHz to 40GHz worst case plot is reported as following.

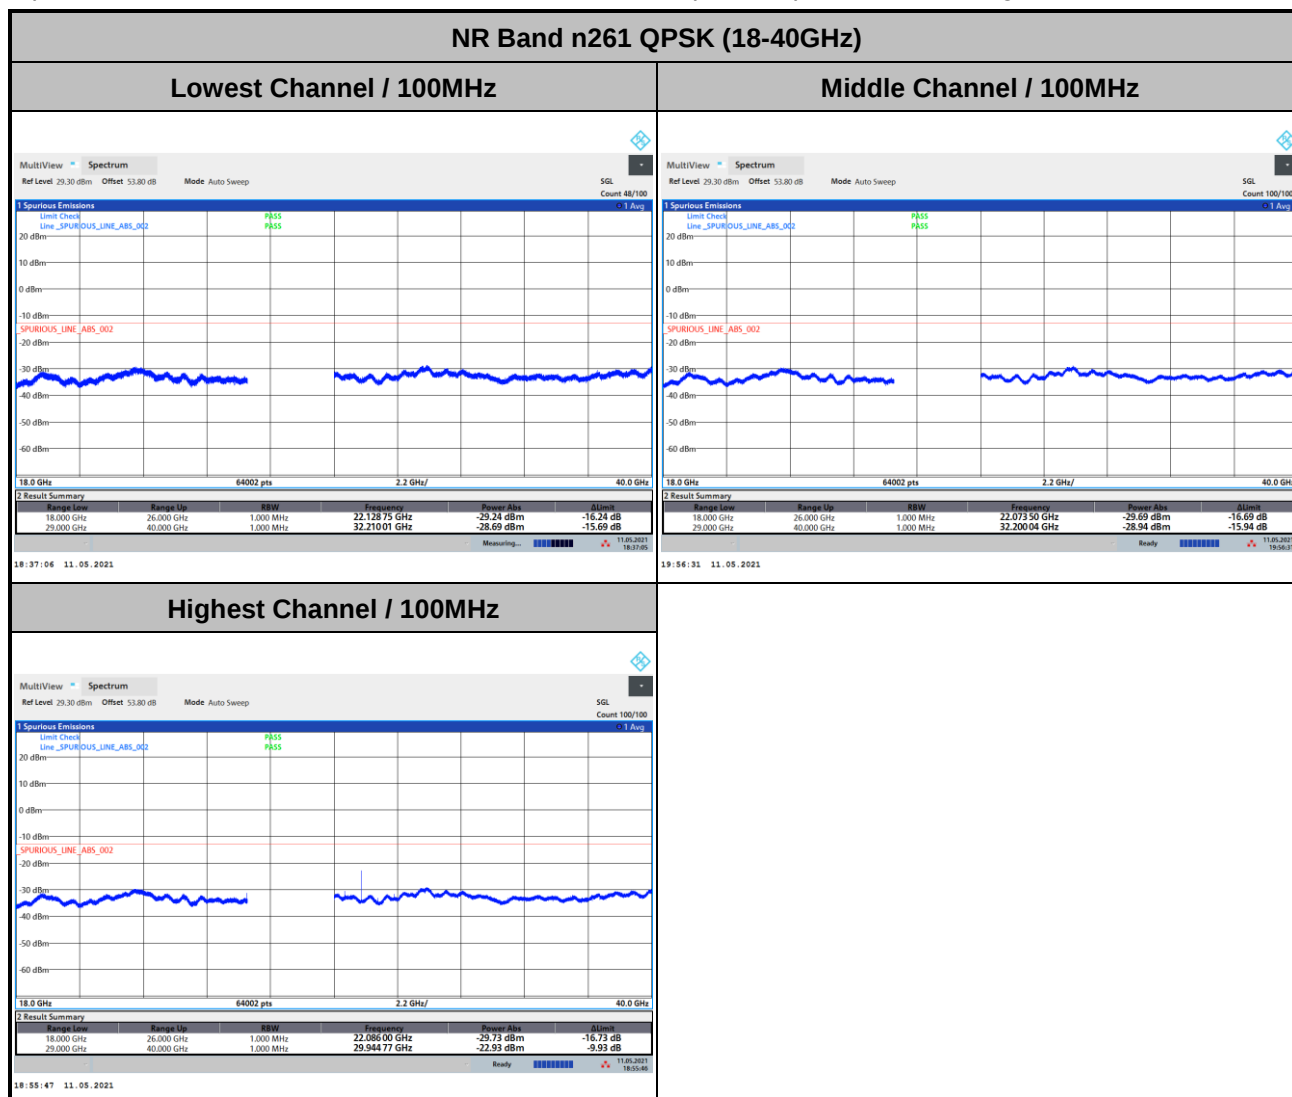

Remark: Above plots, the spurious emissions were measured from 18GHz to 26GHz and 29GHz to 40GHz. The test results within the omitted frequency 26GHz to 29GHz were measured and reported in the section of Radiated Out of Band Emission with frequency range, 26GHz to 29GHz, and all spurious comply with limits.

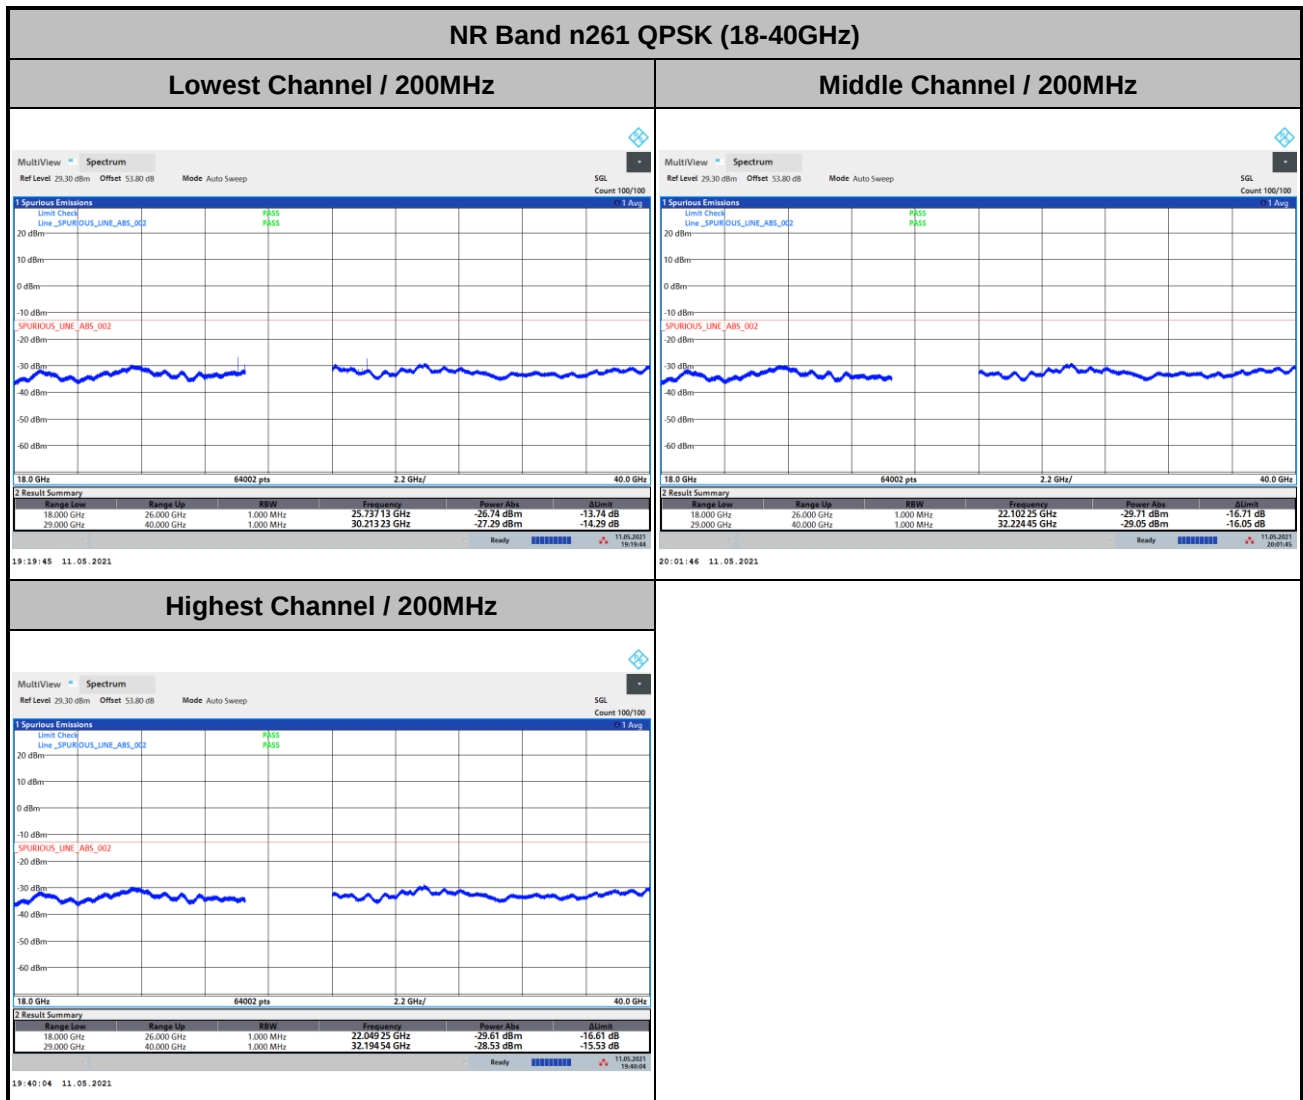


Remark: Above plots, the spurious emissions were measured from 18GHz to 26GHz and 29GHz to 40GHz. The test results within the omitted frequency 26GHz to 29GHz were measured and reported in the section of Radiated Out of Band Emission with frequency range, 26GHz to 29GHz, and all spurious comply with limits.




NR Band n261 QPSK (18-40GHz)


Lowest Channel / 400MHz

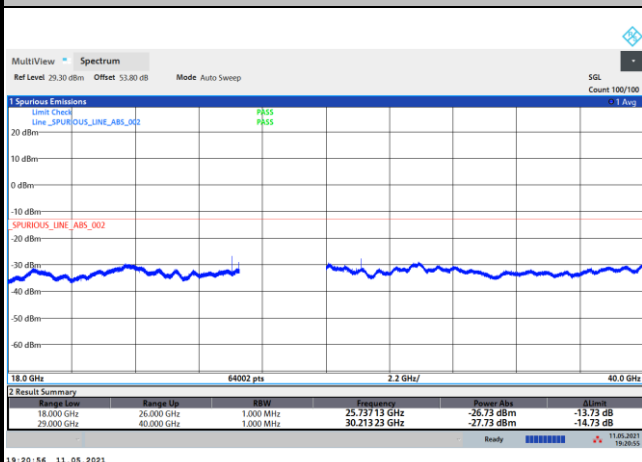

Middle Channel / 400MHz

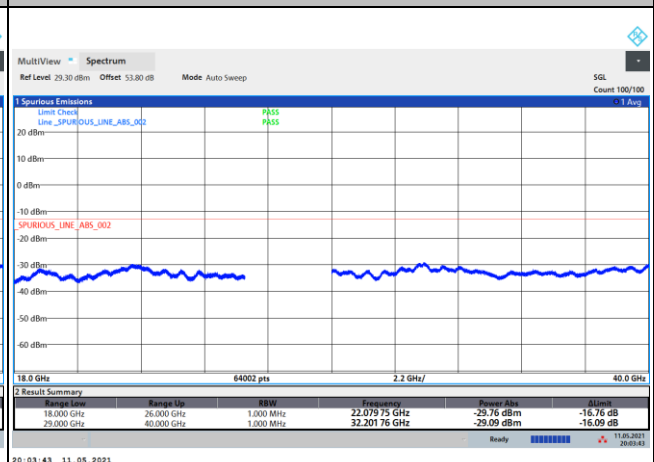

Highest Channel / 400MHz

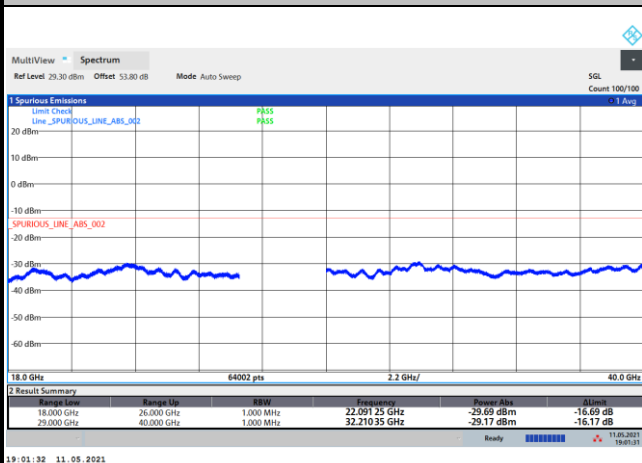


Remark: Above plots, the spurious emissions were measured from 18GHz to 26GHz and 29GHz to 40GHz. The test results within the omitted frequency 26GHz to 29GHz were measured and reported in the section of Radiated Out of Band Emission with frequency range, 26GHz to 29GHz, and all spurious comply with limits.




NR Band n261

(40GHz-60GHz)

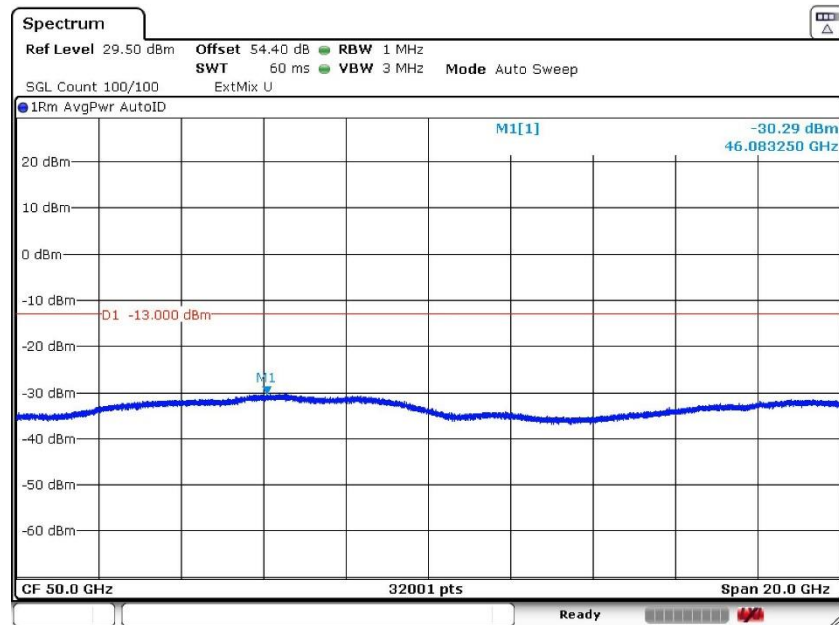


Date: 11.MAY.2021 22:27:28

$$\begin{aligned} \text{Offset} &= \text{Antenna Factor (dB/m)} + \text{Cable Loss (dB)} + 107 + 20\log(D) - 104.8 \\ &= 42.3 + 0.34 + 107 + 20\log(3) - 104.8 = 54.4 \text{ (dB)} \end{aligned}$$

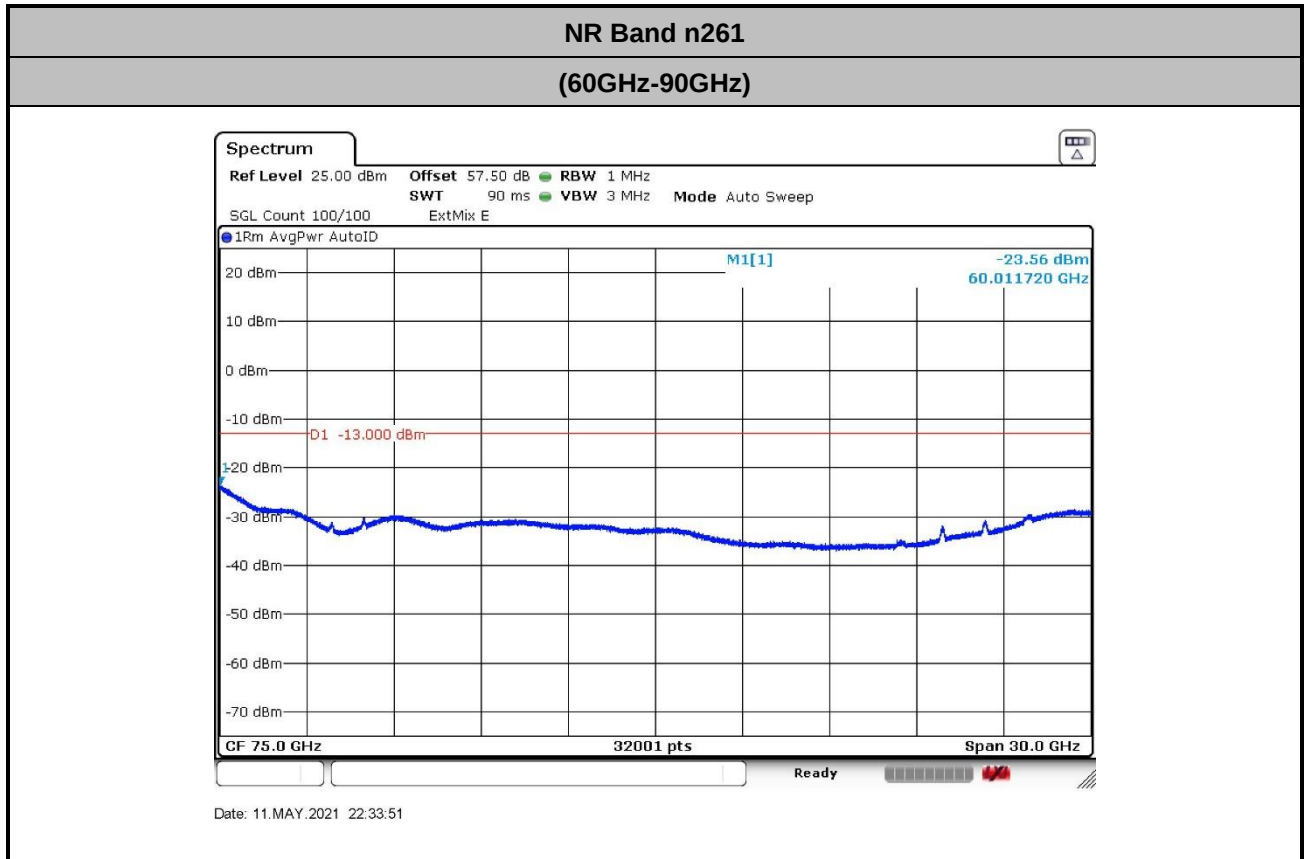

$$\text{Offset} = \text{Antenna Factor (dB/m)} + \text{Cable Loss (dB)} + 107 + 20\log(D) - 104.8$$

$$= 45.4 + 0.34 + 107 + 20\log(3) - 104.8 = 57.5 \text{ (dB)}$$

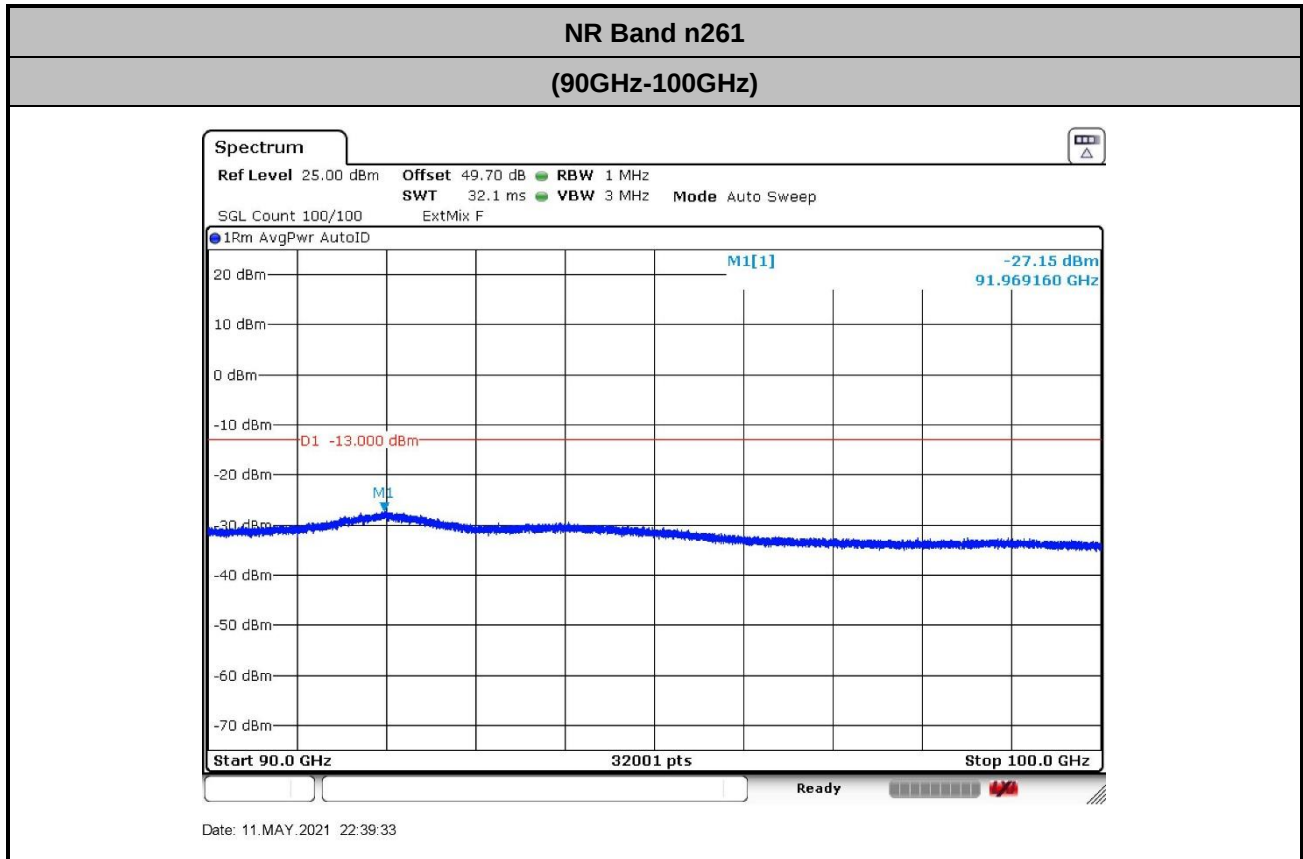

$$\begin{aligned} \text{Offset} &= \text{Antenna Factor (dB/m)} + \text{Cable Loss (dB)} + 107 + 20\log(D) - 104.8 \\ &= 47.2 + 0.34 + 107 + 20\log(1) - 104.8 = 49.7 \text{ (dB)} \end{aligned}$$

**Frequency Stability**

Test Conditions		NR Band n261 / Middle Channel			Limit
Temperature (°C)	Voltage (Volt)	CW tone			Note.
		Frequency (GHz)	Deviation (kHz)	Deviation (ppm)	Result
50	120	27.9248492	-4.000	0.143	PASS
40	120	27.9248462	-1.000	0.036	
30	120	27.9248452	0.000	0.000	
20(Ref.)	120	27.9248452	0.000	0.000	
10	120	27.9248462	-1.000	0.036	
0	120	27.9248482	-3.000	0.107	
-10	120	27.9248472	-2.000	0.072	
-20	120	27.9248442	1.000	0.036	
-30	120	27.9248442	1.000	0.036	
20	102	27.9248462	-1.000	0.036	
20	120	27.9248462	-1.000	0.036	
20	138	27.9248472	-2.000	0.072	

Note: The frequency fundamental emissions stay within the operation band.



Appendix C. R&S Mixer Certificate



Calibration Certificate

Kalibrierschein

Certificate Number 24-0060-101033-01

Zertifikatsnummer

Unit Data

Item Harmonic Mixer, 40 GHz to 60 GHz
Gegenstand

Manufacturer RPG
Hersteller

Type RPG FS-Z60
Typ

Material Number 1048.0171.02 **Serial Number** 101033
Materialnummer **Seriennummer**

Asset Number
Inventarnummer

This calibration certificate documents, that the named item is tested and measured against defined specifications. Measurement results are located usually in the corresponding interval with a probability of approx. 95% (coverage factor $k = 2$). Calibration is performed with test equipment and standards directly or indirectly traceable by means of approved calibration techniques to the PTB/DKD or other national/international standards, which realize the physical units of measurement according to the International System of Units (SI). In all cases where no standards are available, measurements are referenced to standards of the R&S laboratories. Principles and methods of calibration correspond with EN ISO/IEC 17025. This calibration certificate may not be reproduced other than in full. Calibration certificates without signatures are not valid. The user is obliged to have the object recalibrated at appropriate intervals.

Order Data

Customer
Auftraggeber

Order Number
Bestellnummer

Date of Receipt
Eingangsdatum

Dieser Kalibrierschein dokumentiert, dass der genannte Gegenstand nach festgelegten Vorgaben geprüft und gemessen wurde. Die Messwerte lagen im Regelfall mit einer Wahrscheinlichkeit von annähernd 95% im zugeordneten Werteintervall (Erweiterte Messunsicherheit mit $k = 2$). Die Kalibrierung erfolgte mit Messmitteln und Normalen, die direkt oder indirekt durch Ableitung mittels anerkannter Kalibriertechniken rückgeführt sind auf Normale der PTB/DKD oder anderer nationaler/internationaler Standards zur Darstellung der physikalischen Einheiten in Übereinstimmung mit dem Internationalen Einheitensystem (SI). Wenn keine Normale existieren, erfolgt die Rückführung auf Bezugsnormale der R&S-Laboratorien. Grundsätze und Verfahren der Kalibrierung beziehen sich auf EN ISO/IEC 17025. Dieser Kalibrierschein darf nur vollständig und unverändert weiterverbreitet werden. Kalibrierscheine ohne Unterschriften sind ungültig. Für die Einhaltung einer angemessenen Frist zur Wiederholung der Kalibrierung ist der Benutzer verantwortlich.

Performance

Place and Date of Calibration
Ort und Datum der Kalibrierung

Meckenheim, 2020-03-17

Scope of Calibration
Umfang der Kalibrierung

Standard Calibration

Statement of Compliance (Incoming)
Konformitätsaussage (Anlieferung)

New device

Statement of Compliance (Outgoing)
Konformitätsaussage (Auslieferung)

All measured values are within the data sheet specifications.

Extend of Calibration Documents
Umfang des Kalibrierdokuments

2 pages Calibration Certificate
4 pages Outgoing Results

Radiometer Physics GmbH; Meckenheim

Date of Issue
Ausstellungsdatum

2020-03-20

Head of Laboratory
Laborleitung

Schulze

Person Responsible
Bearbeiter

Heinze

Page (Seite) 1/2
Vers2010-05-05/
RPG2014-02-28

Calibration Method
Kalibrieranweisung

RPG-PAQA-TN-2014-002

Relative Humidity **20 % - 80 %**
Relative Luftfeuchte

Ambient Temperature
Umgebungstemperatur

(23 ⁺⁷₋₃) °C

Working standards used (having a significant effect on the accuracy)
Verwendete Gebrauchsnormale (mit signifikantem Einfluss auf die Genauigkeit)

Item Gegenstand	Type Typ	Serial Number Seriennummer	Calibration Certificate Number Kalibrierscheinnummer	Cal. Due Kalibr. bis
Vector Network Analyzer	R&S® ZVA40	100103	0001-300467129	2021-06-13
Powersensor	R&S® NRP-Z55	140091	509915_D-K-15195-01-01_2019-05	2020-05-22
Powersensor	R&S® NRP-Z57	101423	508173_D-K-15195-01-01_2019-05	2020-05-07

UGB1 A compliance statement may be possible where a confidence level of less than 95 % is acceptable.
Die Bestätigung der Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

UGB2 A non-compliance statement may be possible where a confidence level of less than 95 % is acceptable.
Die Bestätigung der Nicht-Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

Ref.: ILAC-G8:03/2009 'Guidelines on the Reporting of Compliance with Specification'.

Notes

Anmerkungen


If the new product is stored under the climate conditions as specified in the data sheet upon delivery, the product's accuracy is not significantly affected within 12 month after its calibration in our factory. In this case, the recommended calibration interval starts on the date when the product is actually put into operation.

Outgoing Results

The following abbreviations may be used in this document

{a}	No measurement uncertainty stated because the errors always add together. So it is sure that a measurement result evaluated as "PASS" is pass.
{b}	The measurement uncertainty depends on the measurement result. The stated measurement uncertainty is valid for the close area around the specification. Measurement results outside the close area have a higher measurement uncertainty but are within the specification.
{c}	Functional test, therefore no measurement uncertainty is stated.
{d}	Typical value, refer to performance test.
{e}	The measurement uncertainty is taken into account when setting the measuring system.
DL or DT	Data Limit for symmetrical tolerance limits
DLL	Datasheet Lower Limit
DUL	Datasheet Upper Limit
MU	Measurement Uncertainty
MLL or MLV	Measurement Uncertainty Lower Value
MUL or MUV	Measurement Uncertainty Upper Value
Nom.	Nominal Value
Dev.	Deviation
MErr.	Measurement Error
Act.	Actual Value
UGB	Uncertainty Guard Band: Measuring uncertainty violates the data (spec.) limit.
UGB1	Measurement results marked as UGB1 show conformity with a probability of >50 % and <95 %.
UGB2	Measurement results marked as UGB2 show non-conformity with a probability of >50 % and <95 %.
DU	Datasheet Uncertainty

Explanation of charts

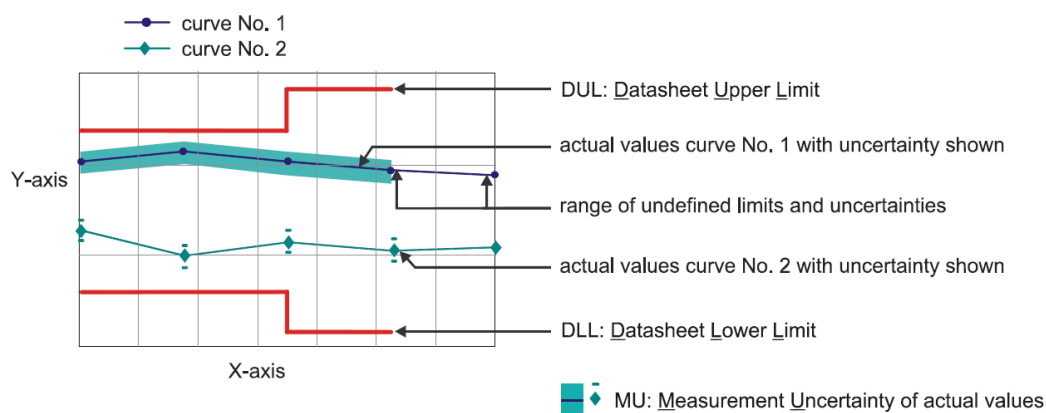

Software used for measurement**Item Type**

Measurement Studio Professional Edition
MixerCertification

Version


2013
7_13

Remark

1.1 Conversion loss

LO level +13 dBm nominal
Bias 0 A

Measurement uncertainty: 1.5 dB

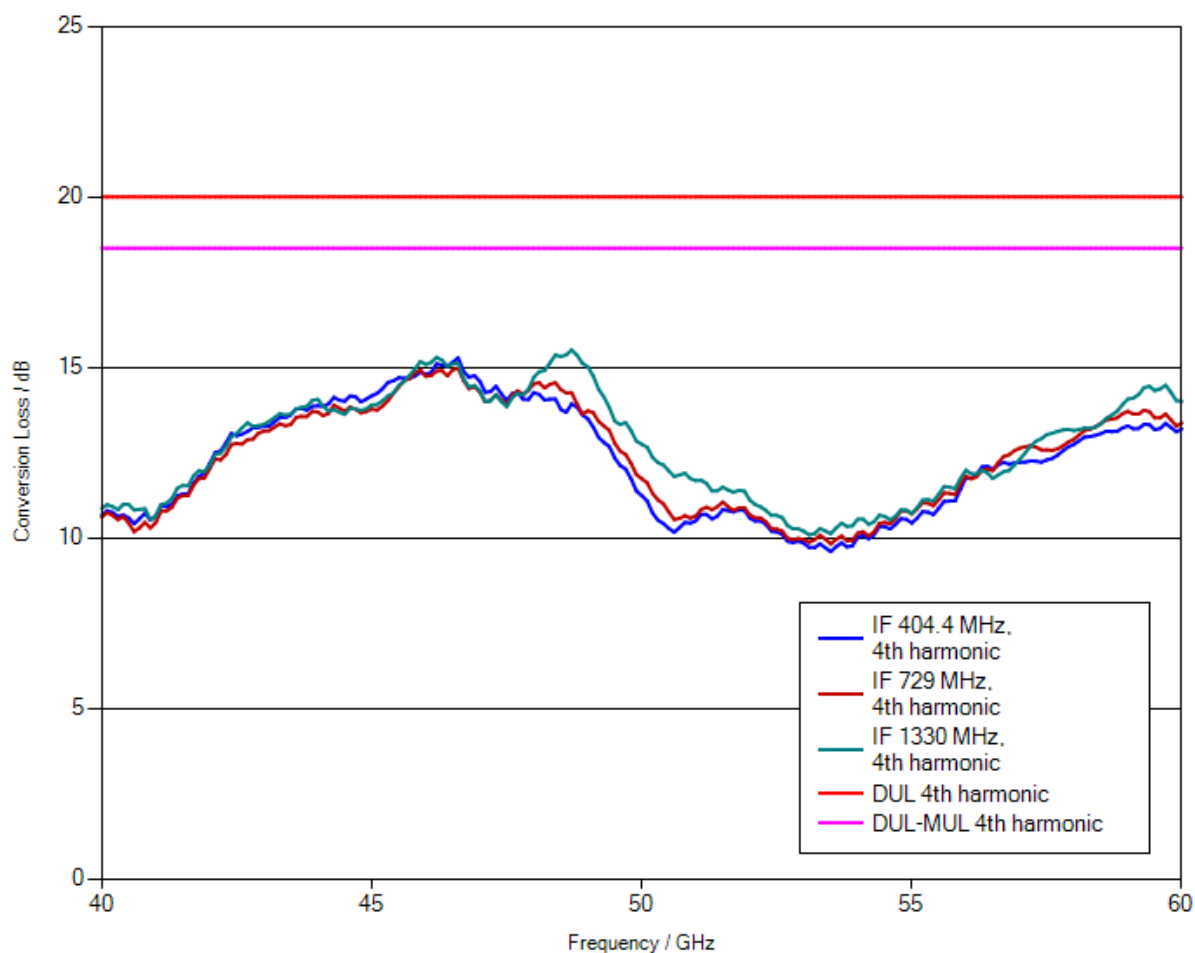

Note: Numeric calibration data can be found attached to the PDF file of the calibration certificate. Click the “paper clip” symbol to display the file.

The file has been renamed for safety reasons.

When downloading the file onto your PC, please delete the “.file” extension and unzip the data.

1.2 Frequency response within 1 GHz

	DUL	Actual (worst case)	Evaluation
IF = 404.4 MHz, 4th harmonic	4 dB	2.16 dB	PASS
IF = 729 MHz, 4th harmonic	4 dB	2.04 dB	PASS
IF = 1330 MHz, 4th harmonic	4 dB	2.19 dB	PASS

Calibration Certificate

Kalibrierschein

Certificate Number **24-0090-101811-01**

Zertifikatsnummer

Unit Data

Item
Gegenstand **Harmonic Mixer, 60 GHz to 90 GHz**

Manufacturer
Hersteller **ROHDE & SCHWARZ**

Type
Typ **R&S® FS-Z90**

Material Number
Materialnummer **1048.0371.02** Serial Number
Seriennummer **101811**

Asset Number
Inventarnummer

This calibration certificate documents, that the named item is tested and measured against defined specifications. Measurement results are located usually in the corresponding interval with a probability of approx. 95% (coverage factor $k = 2$). Calibration is performed with test equipment and standards directly or indirectly traceable by means of approved calibration techniques to the PTB/DKD or other national/international standards, which realize the physical units of measurement according to the International System of Units (SI). In all cases where no standards are available, measurements are referenced to standards of the R&S laboratories. Principles and methods of calibration correspond with EN ISO/IEC 17025. This calibration certificate may not be reproduced other than in full. Calibration certificates without signatures are not valid. The user is obliged to have the object recalibrated at appropriate intervals.

Order Data

Customer
Auftraggeber

Order Number
Bestellnummer

Date of Receipt
Eingangsdatum

Performance

Place and Date of Calibration
Ort und Datum der Kalibrierung

Scope of Calibration
Umfang der Kalibrierung

Statement of Compliance
(Incoming)
Konformitätsaussage
(Anlieferung)

Statement of Compliance
(Outgoing)
Konformitätsaussage
(Auslieferung)

Extend of Calibration Documents
Umfang des Kalibrierdokuments

Meckenheim, 2018-07-16

Standard Calibration

New device

All measured values are within the data sheet specifications.

**2 pages Calibration Certificate
5 pages Outgoing Results**

Dieser Kalibrierschein dokumentiert, dass der genannte Gegenstand nach festgelegten Vorgaben geprüft und gemessen wurde. Die Messwerte lagen im Regelfall mit einer Wahrscheinlichkeit von annähernd 95% im zugeordneten Werteintervall (Erweiterte Messunsicherheit mit $k = 2$). Die Kalibrierung erfolgte mit Messmitteln und Normalen, die direkt oder indirekt durch Ableitung mittels anerkannter Kalibriertechniken rückgeführt sind auf Normale der PTB/DKD oder anderer nationaler/internationaler Standards zur Darstellung der physikalischen Einheiten in Übereinstimmung mit dem Internationalen Einheitensystem (SI). Wenn keine Normale existieren, erfolgt die Rückführung auf Bezugsnormale der R&S-Laboratorien. Grundsätze und Verfahren der Kalibrierung beziehen sich auf EN ISO/IEC 17025. Dieser Kalibrierschein darf nur vollständig und unverändert weiterverbreitet werden. Kalibrierscheine ohne Unterschriften sind ungültig. Für die Einhaltung einer angemessenen Frist zur Wiederholung der Kalibrierung ist der Benutzer verantwortlich.

Radiometer Physics GmbH; Meckenheim

Date of Issue
Ausstellungsdatum

2018-07-19

Head of Laboratory
Laborleitung

Ceru

Person Responsible
Bearbeiter

Grossmindorf

Page (Seite) 1/2
Vers2010-05-05/
RPG2014-02-28

Calibration Method
KalibrieranweisungAmbient Temperature
Umgebungstemperatur

RPG-PAQA-TN-2014-002

(23 ⁺⁷/₋₃) °CRelative Humidity 20 % - 80 %
Relative LuftfeuchteWorking standards used (having a significant effect on the accuracy)
Verwendete Gebrauchsnormale (mit signifikantem Einfluss auf die Genauigkeit)

Item Gegenstand	Type Typ	Serial Number Seriennummer	Calibration Certificate Number Kalibrierscheinnummer	Cal. Due Kalibr. bis
Vector Network Analyzer	R&S® ZVA67	101097	20-300432406	2020-07-21
Powersensor	R&S® NRP-Z55	140093	20-300426315	2019-05-17
Powersensor	R&S® NRP-Z58	101063	20-611462	2018-07-21
Calibration kit	WR12	E10001	RPG-PAQA-TN-2014-005	2019-02-01

UGB1 A compliance statement may be possible where a confidence level of less than 95 % is acceptable.
Die Bestätigung der Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

UGB2 A non-compliance statement may be possible where a confidence level of less than 95 % is acceptable.
Die Bestätigung der Nicht-Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

Ref.: ILAC-G8:03/2009 'Guidelines on the Reporting of Compliance with Specification'.

Notes

Anmerkungen


If the new product is stored under the climate conditions as specified in the data sheet upon delivery, the product's accuracy is not significantly affected within 12 month after its calibration in our factory. In this case, the recommended calibration interval starts on the date when the product is actually put into operation.

Outgoing Results

The following abbreviations may be used in this document

{a}	No measurement uncertainty stated because the errors always add together. So it is sure that a measurement result evaluated as "PASS" is pass.
{b}	The measurement uncertainty depends on the measurement result. The stated measurement uncertainty is valid for the close area around the specification. Measurement results outside the close area have a higher measurement uncertainty but are within the specification.
{c}	Functional test, therefore no measurement uncertainty is stated.
{d}	Typical value, refer to performance test.
{e}	The measurement uncertainty is taken into account when setting the measuring system.
DL or DT	Data Limit for symmetrical tolerance limits
DLL	Datasheet Lower Limit
DUL	Datasheet Upper Limit
MU	Measurement Uncertainty
MLL or MLV	Measurement Uncertainty Lower Value
MUL or MUV	Measurement Uncertainty Upper Value
Nom.	Nominal Value
Dev.	Deviation
MErr.	Measurement Error
Act.	Actual Value
UGB	Uncertainty Guard Band: Measuring uncertainty violates the data (spec.) limit.
UGB1	Measurement results marked as UGB1 show conformity with a probability of >50 % and <95 %.
UGB2	Measurement results marked as UGB2 show non-conformity with a probability of >50 % and <95 %.
DU	Datasheet Uncertainty

Explanation of charts

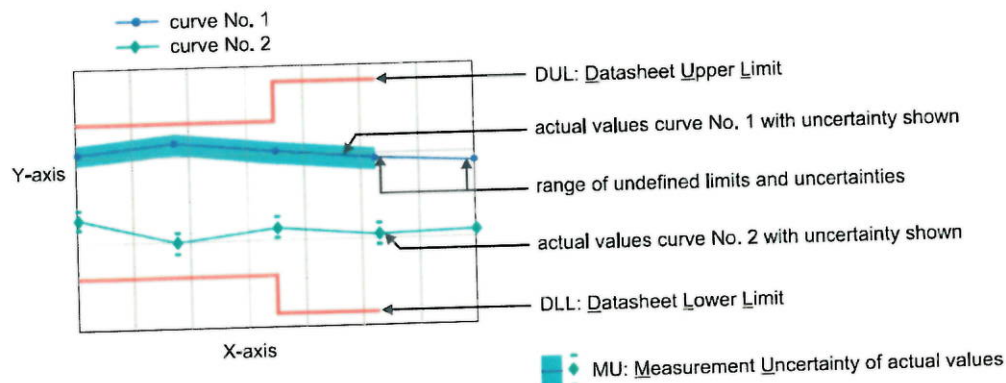


Software used for measurement
Item Type
Measurement Studio Professional Edition
MixerCertification

Version
2013
7_08

Remark

1.1 RF Input – VSWR


Measurement uncertainty: 0.05 (VSWR)

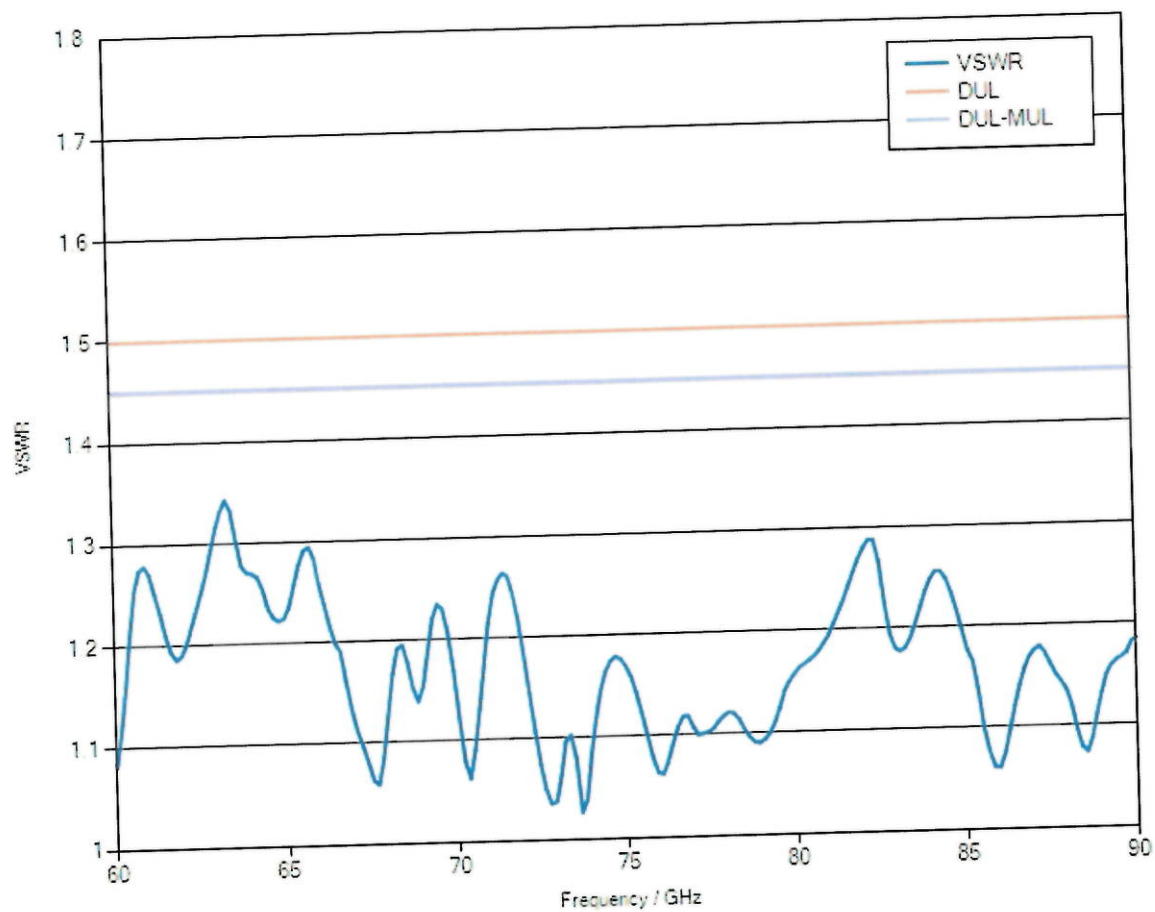

1.2 Conversion loss

LO level +14 dBm nominal
Bias 0 A

Measurement uncertainty: 1.5 dB

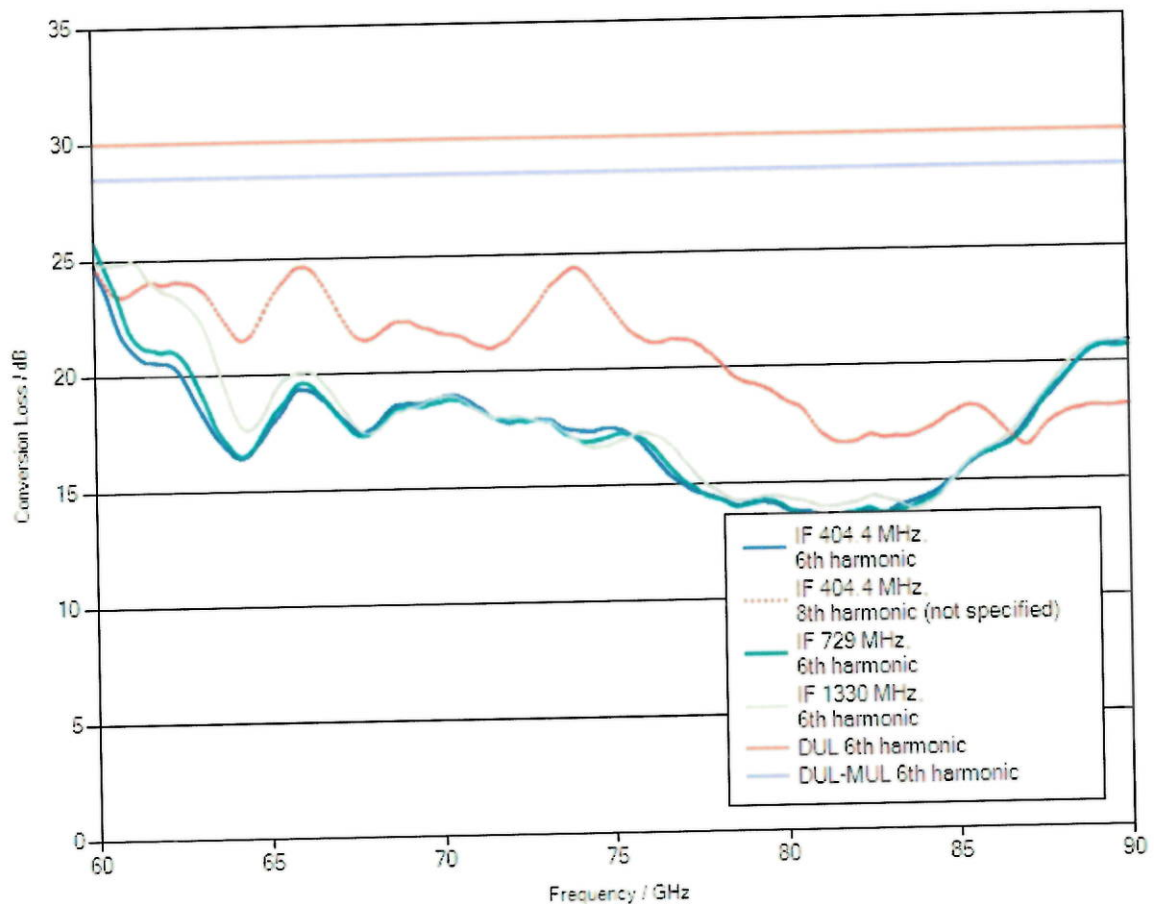

Note: Numeric calibration data can be found attached to the PDF file of the calibration certificate.
Click the "paper clip" symbol to display the file.

The file has been renamed for safety reasons.
When downloading the file onto your PC, please delete the ".file" extension and unzip the data.

1.3 Frequency response within 1 GHz

	DUL	Actual (worst case)	Evaluation
IF = 404.4 MHz, 6th harmonic	6 dB	3.29 dB	PASS
IF = 404.4 MHz, 8th harmonic	not specified	2.25 dB	not specified
IF = 729 MHz, 6th harmonic	6 dB	3.47 dB	PASS
IF = 1330 MHz, 6th harmonic	6 dB	3.84 dB	PASS



Calibration Certificate

Kalibrierschein

Certificate Number **24-0140-101128-02**

Zertifikatsnummer

Unit Data

Item Harmonic Mixer, 90 GHz to 140 GHz
Gegenstand

Manufacturer RPG Radiometer-Physics GmbH
Hersteller

Type RPG FS-Z140
Typ

Material Number 3622.0708.02 **Serial Number** 101128
Materialnummer **Seriennummer**

Asset Number
Inventarnummer

This calibration certificate documents, that the named item is tested and measured against defined specifications. Measurement results are located usually in the corresponding interval with a probability of approx. 95% (coverage factor $k = 2$). Calibration is performed with test equipment and standards directly or indirectly traceable by means of approved calibration techniques to the PTB/DKD or other national/international standards, which realize the physical units of measurement according to the International System of Units (SI). In all cases where no standards are available, measurements are referenced to standards of the R&S laboratories. Principles and methods of calibration correspond with EN ISO/IEC 17025. This calibration certificate may not be reproduced other than in full. Calibration certificates without signatures are not valid. The user is obliged to have the object recalibrated at appropriate intervals.

Order Data

Customer Sporton International Inc.
Auftraggeber No. 106 6F., Sec. 1, Hsin Tai Wu Rd., Xizhi Dist., 000000 NEW TAIPEI CITY-000000 221- TAIWAN

Order Number 8800003072
Bestellnummer

Date of Receipt 2020-10-06
Eingangsdatum

Dieser Kalibrierschein dokumentiert, dass der genannte Gegenstand nach festgelegten Vorgaben geprüft und gemessen wurde. Die Messwerte lagen im Regelfall mit einer Wahrscheinlichkeit von annähernd 95% im zugeordneten Werteintervall (Erweiterte Messunsicherheit mit $k = 2$). Die Kalibrierung erfolgte mit Messmitteln und Normalen, die direkt oder indirekt durch Ableitung mittels anerkannter Kalibriertechniken rückgeführt sind auf Normale der PTB/DKD oder anderer nationaler/internationaler Standards zur Darstellung der physikalischen Einheiten in Übereinstimmung mit dem Internationalen Einheitensystem (SI). Wenn keine Normale existieren, erfolgt die Rückführung auf Bezugsnormale der R&S-Laboratorien. Grundsätze und Verfahren der Kalibrierung beziehen sich auf EN ISO/IEC 17025. Dieser Kalibrierschein darf nur vollständig und unverändert weiterverbreitet werden. Kalibrierscheine ohne Unterschriften sind ungültig. Für die Einhaltung einer angemessenen Frist zur Wiederholung der Kalibrierung ist der Benutzer verantwortlich.

Performance

Place and Date of Calibration
Ort und Datum der Kalibrierung

Meckenheim, 2020-10-26

Scope of Calibration
Umfang der Kalibrierung

Standard Calibration

Statement of Compliance (Incoming)
Konformitätsaussage (Anlieferung)

Defective.

Statement of Compliance (Outgoing)
Konformitätsaussage (Auslieferung)

All measured values are within the data sheet specifications.

Extend of Calibration Documents
Umfang des Kalibrierdokuments

2 pages Calibration Certificate
4 pages Outgoing Results

RPG Radiometer-Physics GmbH; Meckenheim

Date of Issue
Ausstellungsdatum

2020-10-27

Head of Laboratory
Laborleitung

Schulze

Person Responsible
Bearbeiter

Gottbehüt

Calibration Method
Kalibrieranweisung

RPG-PAQA-TN-2014-002

Relative Humidity **20 % - 80 %**
Relative Luftfeuchte

Ambient Temperature
Umgebungstemperatur

(23 ⁺⁷₋₃) °C

Working standards used (having a significant effect on the accuracy)
Verwendete Gebrauchsnormale (mit signifikantem Einfluss auf die Genauigkeit)

Item Gegenstand	Type Typ	Serial Number Seriennummer	Calibration Certificate Number Kalibrierscheinnummer	Cal. Due Kalibr. bis
Vector Network Analyzer	R&S® ZVA40	100103	0001-300467129	2021-06-13
Powersensor	R&S® NRP-Z55	140093	509916_D-K-15195-01-01_2019-05	2021-05-22

UGB1 A compliance statement may be possible where a confidence level of less than 95 % is acceptable.
Die Bestätigung der Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

UGB2 A non-compliance statement may be possible where a confidence level of less than 95 % is acceptable.
Die Bestätigung der Nicht-Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

Ref.: ILAC-G8:03/2009 'Guidelines on the Reporting of Compliance with Specification'.

Notes

Anmerkungen


If the new product is stored under the climate conditions as specified in the data sheet upon delivery, the product's accuracy is not significantly affected within 12 month after its calibration in our factory. In this case, the recommended calibration interval starts on the date when the product is actually put into operation.

Outgoing Results

The following abbreviations may be used in this document

{a}	No measurement uncertainty stated because the errors always add together. So it is sure that a measurement result evaluated as "PASS" is pass.
{b}	The measurement uncertainty depends on the measurement result. The stated measurement uncertainty is valid for the close area around the specification. Measurement results outside the close area have a higher measurement uncertainty but are within the specification.
{c}	Functional test, therefore no measurement uncertainty is stated.
{d}	Typical value, refer to performance test.
{e}	The measurement uncertainty is taken into account when setting the measuring system.
DL or DT	Data Limit for symmetrical tolerance limits
DLL	Datasheet Lower Limit
DUL	Datasheet Upper Limit
MU	Measurement Uncertainty
MLL or MLV	Measurement Uncertainty Lower Value
MUL or MUV	Measurement Uncertainty Upper Value
Nom.	Nominal Value
Dev.	Deviation
MErr.	Measurement Error
Act.	Actual Value
UGB	Uncertainty Guard Band: Measuring uncertainty violates the data (spec.) limit.
UGB1	Measurement results marked as UGB1 show conformity with a probability of >50 % and <95 %.
UGB2	Measurement results marked as UGB2 show non-conformity with a probability of >50 % and <95 %.
DU	Datasheet Uncertainty

Explanation of charts

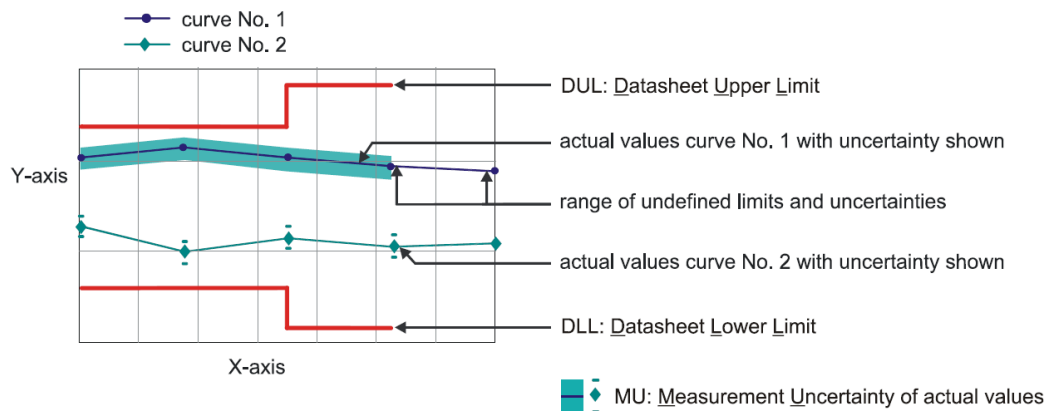


Software used for measurement**Item Type**Measurement Studio Professional Edition
MixerCertification**Version**2013
7_14**Remark**

1.1 Conversion loss

LO level +14 dBm nominal
Bias 0 A

Measurement uncertainty: 3.5 dB

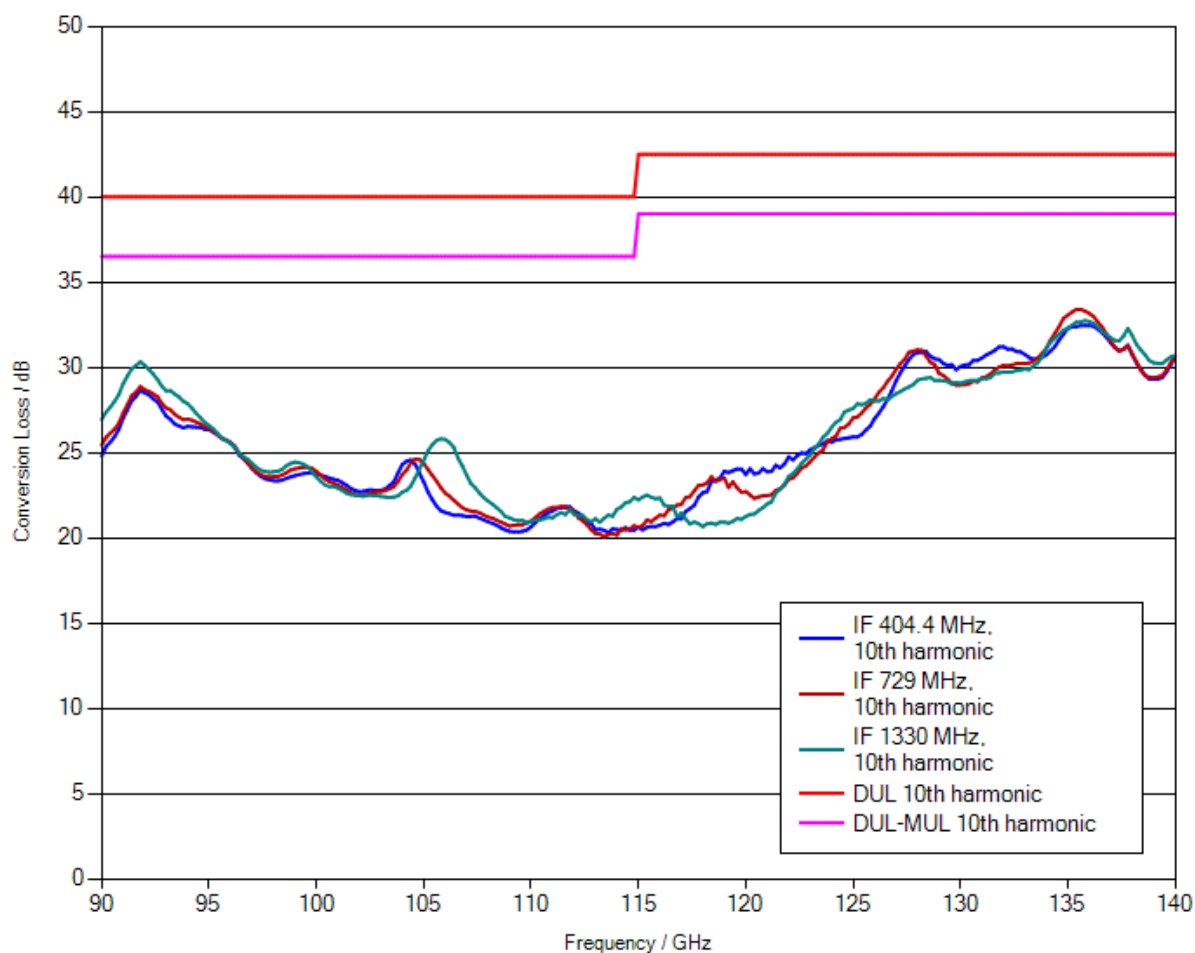

Note: Numeric calibration data can be found attached to the PDF file of the calibration certificate. Click the “paper clip” symbol to display the file.

The file has been renamed for safety reasons.


When downloading the file onto your PC, please delete the “.file” extension and unzip the data.

1.2 Frequency response within 1 GHz

	DUL	Actual (worst case)	Evaluation
IF = 404.4 MHz, 10th harmonic	6 dB	2.1 dB	PASS
IF = 729 MHz, 10th harmonic	6 dB	1.96 dB	PASS
IF = 1330 MHz, 10th harmonic	6 dB	2.13 dB	PASS



Appendix D. Calibration Certificate of Standard Gain Horn Antennas





Calibration certificate



Accreditation certificate No. **№ BY/112 02.5.0.0065** of **09.01.2015**

Certificate number **25-18** Date when calibrated **08/17/2018** Page **1** of **2**

**Item
calibrated**

Antenna QWH-UPRR00 # 923600007

Description of measurement standard / measuring instrument / identification

Customer

Sporton International Inc.

No. 52, HwaYa 1st Road, HwaYa Technology Park, Kwei-Shan District,
TaoYuan City 333, Taiwan, R.O.C.

Name of the customer, address

**Method of
calibration**

GOST 20271.1, MK KL 8.2-16

Name of the method / identification

All measurements are traceable to the SI units which are realized by national measurement standards of NMI and state standards of RF. This certificate shall not be reproduced, except in full. Any publication extracts from the calibration certificate requires written permission of the issuing calibration laboratory of microwave measuring equipment.

**Authorising
signature**



M. Svirid/ Technical manager

Name and position

Date of issue 08/17/2018

Calibration Certificate

Certificate number **25-18**

Page 2 of 2

Calibration is performed by using

#	Measuring equipment	Serial number
1	Wattmeter M 568	164
2	Wattmeter M 546	163
3	Signal generator G4-186	5
4	Signal generator G4-161	3
5	Voltmeter V7-34	0067787
6	Frequency meter RCH3-72	931200
7	Horn antenna P6-133	15005

Calibration conditions

Temperature: 22.5 °C.


Humidity: 44.0 %.

Pressure: 99.9 kPa.

Calibration results are given in the Measuring report # 25-18.

#	Parameter	Specifications required	Specifications tested and measured
1	Frequency range	40 – 60 GHz	Corresponds (Table 1)
2	Waveguide Interface	WR-19	Corresponds
3	Antenna Gain	24 dB	Corresponds (Table 1)
4	Antenna Factor	42 dB/m	Corresponds (Table 1)

Signature of the person who has performed calibration


M. Kasperovich/ Engineer
Name and function

**Calibration Laboratory of
Microwave Measuring Equipment**

Accreditation certificate

No. BY/112 02.5.0.0065

Address: 6, P. Brovki str., Minsk
220027, Belarus

Phone/Fax: +375 17 2938496



Technical Manager

M. Svirid

August 17, 2018

MEASURING REPORT # 25-18

August 17, 2018

Customer:	Sporton International Inc. No. 52, HwaYa 1st Road, HwaYa Technology Park, Kwei-Shan District, TaoYuan City 333, Taiwan, R.O.C.
Item calibrated:	Antenna QWH-UPRR00 # 923600007
Method of calibration:	GOST 20271.1, MK KL 8.2-16
Number of samples:	One
Delivery date of the sample:	07/20/2018
Date of calibration:	From 07/23/2018 to 08/17/2018

MEASURING CONDITIONS

Temperature: 22.5 °C	Humidity: 44 %	Pressure: 99.9 kPa
----------------------	----------------	--------------------

MEASURING EQUIPMENT

#	Measuring equipment	Serial number
1	Wattmeter M 568	164
2	Wattmeter M 546	163
3	Signal generator G4-186	5
4	Signal generator G4-161	3
5	Voltmeter V7-34	0067787
6	Frequency meter RCH3-72	931200
7	Horn antenna P6-133	15005

MEASURING RESULTS

Distance between the testing and generating antennas was 2 m.

Table 1

Frequency, GHz	40	50	60
Input power, mW	10.0	10.0	10.0
Power density of electromagnetic field, W/m ²	0.049	0.067	0.072
Maximum level of measured power, μ W	36.56	37.07	31.98
Gain, dB	22.2	22.8	23.5
Antenna factor, dB/m	40.0	41.4	42.3
Expanded uncertainty, dB	2.1	2.1	2.1

Engineer



M. Kasperovich

Quality Manager



A. Kostrikin

This Measuring report issued in duplicate and sent to:

1. Sporton International INC.

Address: No. 52, HwaYa 1st Road, HwaYa Technology Park, Kwei-Shan District, TaoYuan City 333, Taiwan, R.O.C.

2. Calibration Laboratory of Microwave Measuring Equipment

Duplication of Measuring report (complete or partial) must be authorized by the laboratory.



Calibration certificate

ISO 17025
ACCREDITED LABORATORY



Accreditation certificate No. **№ BY/112 02.5.0.0065** of **09.01.2015**

Certificate number **28-18** Date when calibrated **08/17/2018** Page **1** of **2**

Item

calibrated

Antenna QWH-EPRR00 # 784600034

Description of measurement standard / measuring instrument / identification

Customer

Sporton International Inc.

No. 52, HwaYa 1st Road, HwaYa Technology Park, Kwei-Shan District,
TaoYuan City 333, Taiwan, R.O.C.

Name of the customer, address

**Method of
calibration**

GOST 20271.1, MK KL 8.2-16

Name of the method / identification

All measurements are traceable to the SI units which are realized by national measurement standards of NMI and state standards of RF. This certificate shall not be reproduced, except in full. Any publication extracts from the calibration certificate requires written permission of the issuing calibration laboratory of microwave measuring equipment.

**Authorising
signature**



M. Svirid/ Technical manager
Name and position

Date of issue 08/17/2018

Calibration Certificate

Certificate number **28-18**

Page 2 of 2

Calibration is performed by using

#	Measuring equipment	Serial number
1	Wattmeter M 534	161
2	Wattmeter M 546	163
3	Signal generator G4-186	5
4	Signal generator RG4-14	22
5	Voltmeter V7-34	0067787
6	Frequency meter RCH3-72	931200
7	Horn antenna P6-134	14002
8	Horn antenna P6-31A	35864

Calibration conditions

Temperature: 22.5 °C.

Humidity: 44.0 %.

Pressure: 99.9 kPa.

Calibration results are given in the Measuring report # 28-18.

#	Parameter	Specifications required	Specifications tested and measured
1	Frequency range	60 – 90 GHz	Corresponds (Table 1)
2	Waveguide Interface	WR-12	Corresponds
3	Antenna Gain	24 dB	Corresponds (Table 1)
4	Antenna Factor	45 dB/m	Corresponds (Table 1)

Signature of the person who has performed calibration


M. Kasperovich/ Engineer
Name and function

**Calibration Laboratory of
Microwave Measuring Equipment**

Accreditation certificate

No. BY/112 02.5.0.0065

Address: 6, P. Brovki str., Minsk
220027, Belarus

Phone/Fax: +375 17 2938496



Technical Manager

M. Svirid

August 17, 2018

MEASURING REPORT # 28-18

August 17, 2018

Customer:	Sporton International Inc. No. 52, HwaYa 1st Road, HwaYa Technology Park, Kwei-Shan District, TaoYuan City 333, Taiwan, R.O.C.
Item calibrated:	Antenna QWH-EPRR00 # 784600034
Method of calibration:	GOST 20271.1, MK KL 8.2-16
Number of samples:	One
Delivery date of the sample:	07/20/2018
Date of calibration:	From 07/23/2018 to 08/17/2018

MEASURING CONDITIONS

Temperature: 22.5 °C	Humidity: 44 %	Pressure: 99.9 kPa
----------------------	----------------	--------------------

MEASURING EQUIPMENT

#	Measuring equipment	Serial number
1	Wattmeter M 534	161
2	Wattmeter M 546	163
3	Signal generator G4-186	5
4	Signal generator RG4-14	22
5	Voltmeter V7-34	0067787
6	Frequency meter RCH3-72	931200
7	Horn antenna P6-134	14002
8	Horn antenna P6-31A	35864

MEASURING RESULTS

Distance between the testing and generating antennas was 1.8 m at 60-75 GHz and 1.5 m at 90 GHz.

Table 1

Frequency, GHz	60	75	90
Input Power, mW	10.0	10.0	8.0
Power density of electromagnetic field, W/m ²	0.063	0.081	0.121
Maximum level of measured power, μ W	21.44	21.84	26.14
Gain, dB	22.3	23.3	23.9
Antenna Factor, dB/m	43.5	44.5	45.4
Expanded uncertainty, dB	2.1	2.1	2.1

Engineer



M. Kasperovich

Quality Manager



A. Kostrikin

This Measuring report issued in duplicate and sent to:

1. Sporton International INC.

Address: No. 52, HwaYa 1st Road, HwaYa Technology Park, Kwei-Shan District, TaoYuan City 333, Taiwan, R.O.C.

2. Calibration Laboratory of Microwave Measuring Equipment

Duplication of Measuring report (complete or partial) must be authorized by the laboratory.



Calibration certificate

ISO 17025
ACCREDITED LABORATORY



Accreditation certificate No. № BY/112 02.5.0.0065 of 09.01.2015

Certificate number 30-18 Date when calibrated 08/17/2018 Page 1 of 2

Item

calibrated

Antenna QWH-FPRR00 # 923800008

Description of measurement standard / measuring instrument / identification

Customer

Sporton International Inc.

No. 52, HwaYa 1st Road, HwaYa Technology Park, Kwei-Shan District,
TaoYuan City 333, Taiwan, R.O.C.

Name of the customer, address

**Method of
calibration**

GOST 20271.1, MK KL 8.2-16

Name of the method / identification

All measurements are traceable to the SI units which are realized by national measurement standards of NMI and state standards of RF. This certificate shall not be reproduced, except in full. Any publication extracts from the calibration certificate requires written permission of the issuing calibration laboratory of microwave measuring equipment.

**Authorising
signature**



M. Svirid/ Technical manager
Name and position

Date of issue 08/17/2018

Calibration Certificate

Certificate number **30-18**

Page 2 of 2

Calibration is performed by using

#	Measuring equipment	Serial number
1	Wattmeter M 523	162
2	Wattmeter M 534	161
3	Voltmeter V7-34	0067787
4	Frequency meter RCH3-72	931200
5	Signal generator RG4-14	22
6	Signal generator G4-161	282
7	Antenna P6-31A	35864
8	Antenna P6-32	115671

Calibration conditions

Temperature: 22.5 °C.

Humidity: 44.0 %.

Pressure: 99.9 kPa.

Calibration results are given in the Measuring report # 30-18.

#	Parameter	Specifications required	Specifications tested and measured
1	Frequency range	90 – 140 GHz	Corresponds (Table 1)
2	Waveguide Interface	WR-8	Corresponds
3	Antenna Gain	24 dB	Corresponds (Table 1)
4	Antenna Factor	48 dB/m	Corresponds (Table 1)

Signature of the person who has performed calibration

M. Kasperovich/ Engineer

Name and function

**Calibration Laboratory of
Microwave Measuring Equipment**

Accreditation certificate

No. BY/112 02.5.0.0065

Address: 6, P. Brovki str., Minsk
220027, Belarus

Phone/Fax: +375 17 2938496

Technical Manager



M. Svirid

August 17, 2018

MEASURING REPORT # 30-18

August 17, 2018

Customer:	Sporton International Inc. No. 52, HwaYa 1st Road, HwaYa Technology Park, Kwei-Shan District, TaoYuan City 333, Taiwan, R.O.C.
Item calibrated:	Antenna QWH-FPRR00 # 923800008
Method of calibration:	GOST 20271.1, MK KL 8.2-16
Number of samples:	One
Delivery date of the sample:	07/20/2018
Date of calibration:	From 07/23/2018 to 08/17/2018

MEASURING CONDITIONS

Temperature: 22.5 °C	Humidity: 44 %	Pressure: 99.9 kPa
----------------------	----------------	--------------------

MEASURING EQUIPMENT

#	Measuring equipment	Serial number
1	Wattmeter M 523	162
2	Wattmeter M 534	161
3	Voltmeter V7-34	0067787
4	Frequency meter RCH3-72	931200
5	Signal generator RG4-14	22
6	Signal generator G4-161	282
7	Antenna P6-31A	35864
8	Antenna P6-32	115671

MEASURING RESULTS

Distance between the testing and generating antennas was 1.5 m at 90-115 GHz and 1.2 m at 140 GHz.

Table 1


Frequency, GHz	90	115	140
Input Power, mW	8.0	8.0	5.0
Power density of electromagnetic field, W/m ²	0.125	0.174	0.212
Maximum level of measured power, μW	18.03	20.22	21.08
Gain, dB	22.1	23.3	24.4
Antenna Factor, dB/m	47.2	48.1	48.8
Expanded uncertainty, dB	2.1	2.2	2.2

Engineer



M. Kasperovich

Quality Manager



A. Kostrikin

This Measuring report issued in duplicate and sent to:

1. Sporton International INC.

Address: No. 52, HwaYa 1st Road, HwaYa Technology Park, Kwei-Shan District, TaoYuan City 333, Taiwan, R.O.C.

2. Calibration Laboratory of Microwave Measuring Equipment

Duplication of Measuring report (complete or partial) must be authorized by the laboratory.