

Appendix C for KSCR220700126406

Calibration Certificate

Object	Apply	No	Model	SN	Calibration Date
Dipole	<input type="checkbox"/>	1	CLA150	4025	2021/04/26
	<input type="checkbox"/>	2	D450V3	1103	2021/04/21
	<input type="checkbox"/>	3	D750V3	1188	2022/03/29
	<input type="checkbox"/>	4	D835V2	4d114	2022/03/31
	<input type="checkbox"/>	5	D900V2	1d079	2022/06/07
	<input type="checkbox"/>	6	D1800V2	2d170	2022/03/31
	<input type="checkbox"/>	7	D1900V2	5d1136	2022/06/07
	<input type="checkbox"/>	8	D2000V2	1041	2022/06/06
	<input type="checkbox"/>	9	D2300V2	1096	2022/03/31
	<input checked="" type="checkbox"/>	10	D2450V2	817	2022/04/01
	<input type="checkbox"/>	11	D2600V2	1158	2022/03/31
	<input checked="" type="checkbox"/>	12	D5GHzV2	1095	2022/06/01
DAE	<input checked="" type="checkbox"/>	13	DAE4	1245	2022/05/30
Probe	<input checked="" type="checkbox"/>	14	EX3DV4	7346	2022/03/30



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN_Doccheck@sgs.com
 No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300 t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
 中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300 t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

1 Dipole

1.1 CLA150 - SN 4025

Calibration Laboratory of Schmid & Partner Engineering AG
Zürcherstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client: **SGS-CN (Auden)** Certificate No.: **CLA150-4025_Apr21**

Accreditation No.: **SCS 0108**

CALIBRATION CERTIFICATE

Object: **CLA150 - SN: 4025**

Calibration procedure(s): **QA CAL-15.v9
Calibration Procedure for SAR Validation Sources below 700 MHz**

Calibration date: **April 26, 2021**

The calibration certificate documents the traceability to national standards, which reflect the physical units of measurement (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the enclosed laboratory facility; environment temperature (22 ± 3°C and humidity < 70%).

Calibration Equipment Used (M&TE: critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Schedule / Calibration
Power meter NRP	SN: 10476	09-Apr-21 (No. 217-03091.03292)	Apr-22
Power sensor NRP Z01	SN: 103345	09-Apr-21 (No. 217-03051)	Apr-22
Power sensor NRP Z01	SN: 103345	09-Apr-21 (No. 217-03052)	Apr-22
Reference 20 dB Attenuator	SN: C22662 (20d)	09-Apr-21 (No. 217-03343)	Apr-22
Type-N mismatch combination	SN: 310957 / 00397	09-Apr-21 (No. 217-03344)	Apr-22
Reference Probe EX3004 (DIE4)	SN: 3877	30-Dec-20 (No. 13X3877_Dec20)	Dec-21
	SN: 663	15-Jan-20 (No. 13X654-652_Jan20)	Jan-21

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter S44195	SN: G34139322	05-Apr-19 (in house check Jun-20)	In house check Jun-22
Power sensor E4413A	SN: M41498087	06-Apr-16 (in house check Jun-20)	In house check Jun-22
Power sensor E4413A	SN: 00010210	06-Apr-19 (in house check Jun-20)	In house check Jun-22
RF generator HP 85940C	SN: U5040201700	06-Apr-19 (in house check Jun-20)	In house check Jun-22
Network Analyzer Agilent 83686A	SN: U541005477	31-Mar-14 (in house check Oct-20)	In house check Dec-21

Calibrated by: **Jarhey Katsman** (Name) / **Laboratory Technician** (Function) / *[Signature]* (Signature)

Approved by: **Kajko Polovic** (Name) / **Technical Manager** (Function) / *[Signature]* (Signature)

This calibration certificate shall not be reproduced except in full without written approval of the laboratory. Issued: April 26, 2021

Certificate No: CLA150-4025_Apr21 Page 1 of 6

Calibration Laboratory of Schmid & Partner Engineering AG
Zürcherstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL: Issue simulating liquid sensitivity in TSL; NORM x,y,z

ConvF: not applicable or not measured

N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in this certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The source is mounted in a touch configuration below the center marking of the flat phantom.
- Return Loss:** This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR for nominal TSL parameters:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: CLA150-4025_Apr21 Page 2 of 6

Measurement Conditions
DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	ELN Flat Phantom	Shell thickness: 2 ± 0.2 mm
EUT Positioning	Touch Position	
Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	150 MHz ± 1 MHz	

Head TSL parameters
The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	52.3	0.75 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	51.1 ± 6 %	0.75 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	1 W input power	3.90 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	3.88 W/kg ± 18.4 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	1 W input power	2.60 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	2.59 W/kg ± 18.0 % (k=2)

Certificate No: CLA150-4025_Apr21 Page 3 of 6

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	47.9 Ω ± 1.5 Ω
Return Loss	-31.4 dB

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Certificate No: CLA150-4025_Apr21 Page 4 of 6



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN_Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgsgroup.com.cn
(86-512)57355888 (86-512)57370818 sgs.china@sgs.com

DASY5 Validation Report for Head TSL

Date: 26.04.2021

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: CLA150; Type: CLA150; Serial: CLA150 - SN: 4025

Communication System: UTD 0, CW, Frequency: 150 MHz
Medium parameters used: $f = 150 \text{ MHz}$; $\sigma = 0.76 \text{ S/m}$; $\epsilon = 51.1$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(12.51, 12.51, 12.51) @ 150 MHz; Calibrated: 30.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DA54 Snt54; Calibrated: 26.06.2020
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP.1003
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

CLA Calibration for HSL-LF Tissue/CLA150, touch configuration, Pin=1W/Zoom Scan, dist=1.4mm (8x10x8)/Tube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
Reference Value = 85.93 W/m; Power Drift = -0.02 dB
Peak SAR (extrapolated) = 7.36 W/kg
SAR(1 g) = 3.90 W/kg; SAR(10 g) = 2.60 W/kg
Smallest distance from peaks to all points 3 dB below: Larger than measurement grid (> 30mm)
Ratio of SAR at M2 to SAR at M1 = 80.4%
Maximum value of SAR (measured) = 5.48 W/kg

0 dB = 5.48 W/kg = 7.39 dBW/kg

Certificate No: CLA150-4025_Apr21 Page 6 of 6

Certificate No: CLA150-4025_Apr21 Page 6 of 6

1.2 D450V3 - SN 1103

Calibration Laboratory of Schmid & Partner Engineering AG
Ziegelhausstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client: **SGS-CN (Aiden)** Certificate No: **D450V3-1103_Apr21**

CALIBRATION CERTIFICATE

Object: **D450V3 - SN: 1103**

Calibration procedure(s): **QA CAL-15_V9**
Calibration Procedure for SAR Validation Sources below 700 MHz

Calibration date: **April 21, 2021**

This calibration certificate documents the traceability in national statements, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environmental temperature (22 ± 2) °C and humidity < 75%.

Calibration Equipment used (MPE critical for calibration)

Primary Standards	ID #	Exp. Date (Certificate No.)	Scheduled Calibration
Power Meter NRP1	SN: 104779	09-Apr-21 (No. 217-030710320)	Apr-22
Power sensor NRP1-Z91	SN: 103244	09-Apr-21 (No. 217-03251)	Apr-22
Power sensor NRP1-Z91	SN: 103245	09-Apr-21 (No. 217-03259)	Apr-22
Reference 20 dB Attenuator	SN: C2352 (20)	09-Apr-21 (No. 217-03343)	Apr-22
Type-A impedance combination	SN: 310827/06327	09-Apr-21 (No. 217-03344)	Apr-22
Reference Probe EPC05A	SN: 3077	30-Dec-20 (No. E23-2077_De20)	Dec-21
DAEA	SN: 604	05-Jun-20 (No. DAE4-604_Jun20)	Jun-21

Secondary Standards	ID #	Check Date (in House)	Scheduled Check
Power meter E4418B	SN: GB41200274	09-Apr-19 (In house check Jun-20)	In house check Jun-22
Power sensor E4412A	SN: MY41496047	09-Apr-19 (In house check Jun-20)	In house check Jun-22
Power sensor E4412A	SN: 00010210	09-Apr-19 (In house check Jun-20)	In house check Jun-22
HP generator HP 8448C	SN: US3406011700	06-Aug-19 (In house check Jun-20)	In house check Jun-22
Network Analyzer Agilent E8358A	SN: US41980477	31-Mar-14 (In house check Oct-20)	In house check Oct-21

Calibrated by: **Christoph Linder** (Function: Laboratory Technician)

Approved by: **Katja Fritsch** (Function: Technical Manager)

This calibration certificate shall not be reproduced except in full without approval of the laboratory.

Certificate No: D450V3-1103_Apr21 Page 1 of 6

Calibration Laboratory of Schmid & Partner Engineering AG
Ziegelhausstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client: **SGS-CN (Aiden)** Certificate No: **D450V3-1103_Apr21**

Glossary:

TSL: Issue simulating liquid sensitivity in TSL / NORM x,y,z

ConvF: not applicable or not measured

N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2015
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 605664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D450V3-1103_Apr21 Page 2 of 6



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgs.com.cn
(86-512)57355888 (86-512)57370818 sgs.china@sgs.com

Measurement Conditions
DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V82.10.4
Extrapolation	Advanced Extrapolation	
Phantom	ELJ Flat Phantom	Shell thickness: 2 ± 0.2 mm
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	450 MHz ± 1 MHz	

Head TSL parameters
The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	43.5	0.57 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	43.1 ± 0.6 %	0.57 mho/m ± 0 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	1.14 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	4.55 W/kg ± 18.1 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	0.757 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	3.06 W/kg ± 17.6 % (k=2)

Certificate No: D450V3-1103_Apr21 Page 3 of 6

Appendix (Additional assessments outside the scope of SCS 0106)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	57.1 Ω - 2.6 jΩ
Return Loss	-23.0 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.346 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard straight coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole design is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Certificate No: D450V3-1103_Apr21 Page 4 of 6

DASY5 Validation Report for Head TSL

Test Laboratory: SPEAG, Zurich, Switzerland Date: 21.04.2021

DUT: Dipole 450 MHz; Type: D450V3; Serial: D450V3 - SN:1103

Communication System: UTD 0 - CW; Frequency: 450 MHz
Medium parameters used: $f = 450 \text{ MHz}$, $n = 0.87 \text{ Sin}$, $\epsilon_r = 43.1$, $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section
Measurement Standard: DASY5 (IEE/IEC/ANSI C63.19-2011)


DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF [10.64, 10.64, 10.64] @ 450 MHz; Calibrated: 30.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 26.06.2020
- Phantom: ELJ v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52: 10.4 (1527); SEMCAD X (4.6.14/7483)

Dipole Calibration for Head Tissue/d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0:
Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 39.18 W/m; Power Diff = -0.08 dB
Peak SAR (extrapolated) = 1.76 W/kg
SAR(1g) = 1.14 W/kg; SAR(10g) = 0.767 W/kg
Smallest distance from peaks to all points: 3 dB below: Larger than measurement grid
Ratio of SAR at M2 to SAR at M1 = 64.9%
Maximum value of SAR (measured) = 1.53 W/kg

0 dB = 1.53 W/kg = 1.85 dBW/kg

Certificate No: D450V3-1103_Apr21 Page 5 of 6

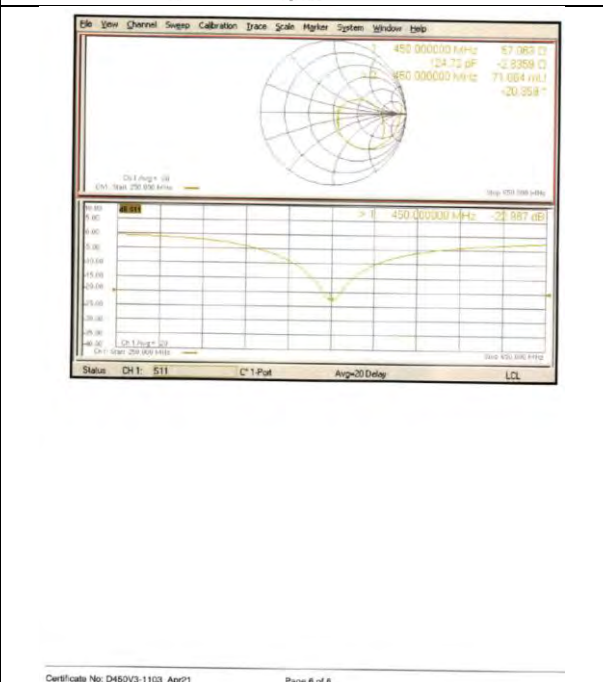

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.
Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgsgroup.com.cn
(86-512)57355888 (86-512)57370818 sgs.china@sgs.com

1.3 D750V3 - SN 1188

<p>In Collaboration with TTL Speag CALIBRATION LABORATORY</p> <p>Address: No. 52 HuaYuanle Road, Haidian District, Beijing, 100191, China Tel: +86-10-42296633-2152 Fax: +86-10-42296633-2594 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn</p> <p>Client: SGS-CN Certificate No: Z22-40103</p> <p>CALIBRATION CERTIFICATE</p> <p>Object: D750V3 - SN: 1188</p> <p>Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits</p> <p>Calibration date: March 29, 2022</p> <p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility; environment temperature (23±3)°C and humidity <70%.</p> <p>Calibration Equipment used (M&TE critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter NRP2</td> <td>104277</td> <td>24-Sep-21 (CITL No. J21X08328)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP8S</td> <td>104291</td> <td>24-Sep-21 (CITL No. J21X08328)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX30V4</td> <td>SN 7307</td> <td>26-May-21 (SPEAG No. EX3-7307_May21)</td> <td>May-22</td> </tr> <tr> <td>DAE4</td> <td>SN 1556</td> <td>12-Jan-22 (CITL-SPEAG No. Z22-60007)</td> <td>Jan-23</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Signal Generator S4436C</td> <td>MY48071430</td> <td>13-Jan-22 (CITL No. J22X00409)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MY46110673</td> <td>14-Jan-22 (CITL No. J22X00409)</td> <td>Jan-23</td> </tr> </tbody> </table> <p>Calibrated by: Zhao Jing SAR Test Engineer</p> <p>Reviewed by: Lin Hao SAR Test Engineer</p> <p>Approved by: Qi Diayuan SAR Project Leader</p> <p>Issued: April 3, 2022</p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> <p>Certificate No: Z22-40103 Page 1 of 6</p>	Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Power Meter NRP2	104277	24-Sep-21 (CITL No. J21X08328)	Sep-22	Power sensor NRP8S	104291	24-Sep-21 (CITL No. J21X08328)	Sep-22	Reference Probe EX30V4	SN 7307	26-May-21 (SPEAG No. EX3-7307_May21)	May-22	DAE4	SN 1556	12-Jan-22 (CITL-SPEAG No. Z22-60007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Signal Generator S4436C	MY48071430	13-Jan-22 (CITL No. J22X00409)	Jan-23	Network Analyzer E5071C	MY46110673	14-Jan-22 (CITL No. J22X00409)	Jan-23	<p>In Collaboration with TTL Speag CALIBRATION LABORATORY</p> <p>Address: No. 52 HuaYuanle Road, Haidian District, Beijing, 100191, China Tel: +86-10-42296633-2079 Fax: +86-10-42296633-2594 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn</p> <p>Glossary:</p> <p>TSL Issue simulating liquid CorvF sensitivity in TSL / NORMx,y,z N/A not applicable or not measured</p> <p>Calibration is Performed According to the Following Standards:</p> <p>a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices-Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDB 855654, "SAR Measurement Requirements for 100 MHz to 6 GHz"</p> <p>Additional Documentation:</p> <p>c) DASY4/5 System Handbook</p> <p>Methods Applied and Interpretation of Parameters:</p> <ul style="list-style-type: none"> Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. SAR measured: SAR measured at the stated antenna input power. SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. <p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p> <p>Certificate No: Z22-40103 Page 2 of 6</p>																												
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																																																										
Power Meter NRP2	104277	24-Sep-21 (CITL No. J21X08328)	Sep-22																																																										
Power sensor NRP8S	104291	24-Sep-21 (CITL No. J21X08328)	Sep-22																																																										
Reference Probe EX30V4	SN 7307	26-May-21 (SPEAG No. EX3-7307_May21)	May-22																																																										
DAE4	SN 1556	12-Jan-22 (CITL-SPEAG No. Z22-60007)	Jan-23																																																										
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																																																										
Signal Generator S4436C	MY48071430	13-Jan-22 (CITL No. J22X00409)	Jan-23																																																										
Network Analyzer E5071C	MY46110673	14-Jan-22 (CITL No. J22X00409)	Jan-23																																																										
<p>In Collaboration with TTL Speag CALIBRATION LABORATORY</p> <p>Address: No. 52 HuaYuanle Road, Haidian District, Beijing, 100191, China Tel: +86-10-42296633-2079 Fax: +86-10-42296633-2594 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn</p> <p>Measurement Conditions</p> <p>DASY system configuration, as far as not given on page 1</p> <table border="1"> <thead> <tr> <th>DASY Version</th> <th>DASY52</th> <th>V52.10.4</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>15 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>750 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table> <p>Head TSL parameters</p> <p>The following parameters and calculations were applied:</p> <table border="1"> <thead> <tr> <th></th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>42.0</td> <td>0.90 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>41.4 ± 0.5 %</td> <td>0.89 mho/m ± 0 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><1.0 °C</td> <td></td> <td></td> </tr> </tbody> </table> <p>SAR result with Head TSL</p> <table border="1"> <thead> <tr> <th>SAR averaged over 1 cm² (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>2.07 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>8.27 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm² (10 g) of Head TSL</td> <th>Condition</th> <th></th> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>1.37 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>5.48 W/kg ± 18.7 % (k=2)</td> </tr> </tbody> </table> <p>Certificate No: Z22-40103 Page 3 of 6</p>	DASY Version	DASY52	V52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	15 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	750 MHz ± 1 MHz			Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	42.0	0.90 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	41.4 ± 0.5 %	0.89 mho/m ± 0 %	Head TSL temperature change during test	<1.0 °C			SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		SAR measured	250 mW input power	2.07 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	8.27 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		SAR measured	250 mW input power	1.37 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	5.48 W/kg ± 18.7 % (k=2)	<p>In Collaboration with TTL Speag CALIBRATION LABORATORY</p> <p>Address: No. 52 HuaYuanle Road, Haidian District, Beijing, 100191, China Tel: +86-10-42296633-2079 Fax: +86-10-42296633-2594 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn</p> <p>Appendix (Additional assessments outside the scope of CNAS L0570)</p> <p>Antenna Parameters with Head TSL</p> <table border="1"> <thead> <tr> <th>Impedance, transformed to feed point</th> <th>53.6Ω - 1.1jΩ</th> </tr> </thead> <tbody> <tr> <td>Return Loss</td> <td>-28.7dB</td> </tr> </tbody> </table> <p>General Antenna Parameters and Design</p> <table border="1"> <tbody> <tr> <td>Electrical Delay (one direction)</td> <td>0.947 ns</td> </tr> </tbody> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when placed according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p>Additional EUT Data</p> <table border="1"> <tbody> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </tbody> </table> <p>Certificate No: Z22-40103 Page 4 of 6</p>	Impedance, transformed to feed point	53.6Ω - 1.1jΩ	Return Loss	-28.7dB	Electrical Delay (one direction)	0.947 ns	Manufactured by	SPEAG
DASY Version	DASY52	V52.10.4																																																											
Extrapolation	Advanced Extrapolation																																																												
Phantom	Triple Flat Phantom 5.1C																																																												
Distance Dipole Center - TSL	15 mm	with Spacer																																																											
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																												
Frequency	750 MHz ± 1 MHz																																																												
	Temperature	Permittivity	Conductivity																																																										
Nominal Head TSL parameters	22.0 °C	42.0	0.90 mho/m																																																										
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.4 ± 0.5 %	0.89 mho/m ± 0 %																																																										
Head TSL temperature change during test	<1.0 °C																																																												
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition																																																												
SAR measured	250 mW input power	2.07 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	8.27 W/kg ± 18.8 % (k=2)																																																											
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition																																																												
SAR measured	250 mW input power	1.37 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	5.48 W/kg ± 18.7 % (k=2)																																																											
Impedance, transformed to feed point	53.6Ω - 1.1jΩ																																																												
Return Loss	-28.7dB																																																												
Electrical Delay (one direction)	0.947 ns																																																												
Manufactured by	SPEAG																																																												



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgs.com.cn
(86-512)57355888 (86-512)57370818 sgs.china@sgs.com

TTL Speaq Calibration Laboratory
 In Collaboration with **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304631-2079 Fax: +86-10-42304631-2504
 E-mail: cti@chinaul.com http://www.chinaul.com

DASY5 Validation Report for Head TSL Date: 2022-03-29
 Test Laboratory: CTTL, Beijing, China
DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN: 1188
 Communication System: UID 0, CW; Frequency: 750 MHz; Duty Cycle: 1:1
 Medium parameters used: $f = 750 \text{ MHz}$; $\sigma = 0.888 \text{ S/m}$; $\epsilon_r = 41.36$; $\rho = 1000 \text{ kg/m}^3$
 Phantom section: Right Section
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
 DASY5 Configuration:

- Probe: EX3DV4 - SN7307; ConvF(10.31, 10.31, 10.31) @ 750 MHz; Calibrated: 2021-05-26
- Sense-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2022-01-12
- Phantom: MFP-V5.1C (20kg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52.52.10.4(1535); SEMCAD-X (4.6.14(7501))

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 55.06 V/m; Power Drift = 0.00 dB
 Peak SAR (extrapolated) = 2.07 W/kg
 SAR(1 g) = 2.07 W/kg; SAR(10 g) = 1.37 W/kg
 Smallest distance from peaks to all points 3 dB below = 18.9 mm
 Ratio of SAR at M2 to SAR at M1 = 67.1%
 Maximum value of SAR (measured) = 2.74 W/kg

Certificate No: Z22-60103 Page 5 of 6

TTL Speaq Calibration Laboratory
 In Collaboration with **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304631-2079 Fax: +86-10-42304631-2504
 E-mail: cti@chinaul.com http://www.chinaul.com

Impedance Measurement Plot for Head TSL

Certificate No: Z22-60103 Page 6 of 6

1.4 D835V2 - SN 4d114

TTL Speaq Calibration Laboratory
 In Collaboration with **CAICT** and **CNAS**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304631-2079 Fax: +86-10-42304631-2504
 E-mail: cti@chinaul.com http://www.chinaul.com

Client: **SGS-CN** Certificate No: **Z22-60104**

CALIBRATION CERTIFICATE

Object: D835V2 - SN: 4d114
 Calibration Procedure(s): FF-Z11-003-01
 Calibration Procedures for dipole validation kits
 Calibration date: March 31, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL, No.J21X08326)	Sep-22
Power sensor NRPBS	104281	24-Sep-21 (CTTL, No.J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7307	28-May-21(SPEAG No.EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG No.Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL, No.J22X00409)	Jan-23
Network Analyzer E5071C	MY48110873	14-Jan-22 (CTTL, No.J22X00406)	Jan-23

Calibrated by: Zhao Jing, SAR Test Engineer
 Reviewed by: Lin Hao, SAR Test Engineer
 Approved by: Qi Dianyuan, SAR Project Leader

Signature: [Signatures]
 Issued: April 6, 2022
 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60104 Page 1 of 6

TTL Speaq Calibration Laboratory
 In Collaboration with **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304631-2079 Fax: +86-10-42304631-2504
 E-mail: cti@chinaul.com http://www.chinaul.com

Glossary:
 TSL: tissue simulating liquid
 ConvF: sensitivity in TSL / NORMx.y.z
 N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:
 a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
 b) KDB 685664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:
 c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60104 Page 2 of 6



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
 中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgsgroup.com.cn
 (86-512)57355888 (86-512)57370818 sgs.china@sgs.com

In Collaboration with
TTL Speag
 CALIBRATION LABORATORY

CAICT

Address: No. 52 HuaYuanHu Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504
 E-mail: cti@china.ttl.com http://www.china.ttl.com

Measurement Conditions
 DASY system configuration, as far as not given on page 1

DASY Version	DASY52	VS2 10.4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz ± 1 MHz	

Head TSL parameters
 The following parameters and calculations were applied:

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.0 ± 0.6 %	0.91 mho/m ± 0.6 %
Head TSL temperature change during last	<+1.0 °C	—	—

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.37 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	6.40 W/kg ± 18.6 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	1.54 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	6.12 W/kg ± 18.7 % (k=2)

Certificate No: Z22-60104 Page 1 of 6

In Collaboration with
TTL Speag
 CALIBRATION LABORATORY

CAICT

Address: No. 52 HuaYuanHu Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504
 E-mail: cti@china.ttl.com http://www.china.ttl.com

Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	48.7Ω - j22Ω
Return Loss	-25.5dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.307 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is set according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Certificate No: Z22-60104 Page 1 of 6

In Collaboration with
TTL Speag
 CALIBRATION LABORATORY

CAICT

Address: No. 52 HuaYuanHu Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504
 E-mail: cti@china.ttl.com http://www.china.ttl.com

DASY5 Validation Report for Head TSL
 Test Laboratory: CTTL, Beijing, China
 DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 40114
 Communication System: UFD 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1
 Medium parameters used: F = 835 MHz; σ = 0.907 S/m; ε_r = 40.98; ρ = 1000 kg/m³
 Phantom section: Right Section
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
 DASY5 Configuration:

- Probe: EX3DV4 - SN7307; ConvF(10,13, 10,13) @ 835 MHz; Calibrated: 2021-05-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DA-E4 Sn1556; Calibrated: 2022-01-12
- Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52.52.10.4(153); SEMCAD X 14.6.14(7501)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 57.88 V/m; Power Drift = 0.04 dB
 Peak SAR (extrapolated) = 3.56 W/kg
 SAR(1 g) = 2.37 W/kg; SAR(10 g) = 1.54 W/kg
 Smallest distance from peaks to all points 3 dB below = 15.8 mm
 Ratio of SAR at M2 to SAR at M1 = 66.2%
 Maximum value of SAR (measured) = 3.17 W/kg

0 dB = 3.17 W/kg = 5.01 dBW/kg

Certificate No: Z22-60104 Page 1 of 6

In Collaboration with
TTL Speag
 CALIBRATION LABORATORY

CAICT

Address: No. 52 HuaYuanHu Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504
 E-mail: cti@china.ttl.com http://www.china.ttl.com

Impedance Measurement Plot for Head TSL

Certificate No: Z22-60104 Page 6 of 6



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN_Doccheck@sgs.com

No.10, Weiyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
 中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgs.com.cn
 (86-512)57355888 (86-512)57370818 sgs.china@sgs.com

1.5 D900V2 - SN 1d079

<div style="display: flex; justify-content: space-between;"> </div> <p>Client: SGS-CN Certificate No: Z22-60184</p> <h3>CALIBRATION CERTIFICATE</h3> <p>Object: D900V2 - SN: 1d079</p> <p>Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits</p> <p>Calibration date: June 7, 2022</p> <p>The calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility, environment temperature: (22±)°C and humidity:70%.</p> <p>Calibration Equipment used (M&TE critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter NRP2</td> <td>106277</td> <td>24-Sep-21 (CTTL No. J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP8S</td> <td>104291</td> <td>24-Sep-21 (CTTL No. J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN 7464</td> <td>26-Jan-22 (SPEAG No. EX3-7464_Jan22)</td> <td>Jan-23</td> </tr> <tr> <td>DAEA</td> <td>SN 1566</td> <td>12-Jan-22 (CTTL-SPEAG No. Z22-60007)</td> <td>Jan-23</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Signal Generator E4438C</td> <td>MV48071430</td> <td>13-Jan-22 (CTTL No. J22X00409)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MV48110473</td> <td>14-Jan-22 (CTTL No. J22X00409)</td> <td>Jan-23</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Calibrated by:</th> <th>Name</th> <th>Function</th> <th>Signature</th> </tr> </thead> <tbody> <tr> <td>Reviewed by:</td> <td>Lin Hao</td> <td>SAR Test Engineer</td> <td></td> </tr> <tr> <td>Approved by:</td> <td>Qi Dianyuan</td> <td>SAR Project Leader</td> <td></td> </tr> </tbody> </table> <p>Issued: June 13, 2022</p> <p>The calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> <p>Certificate No: Z22-60184 Page 1 of 4</p>	Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Power Meter NRP2	106277	24-Sep-21 (CTTL No. J21X08326)	Sep-22	Power sensor NRP8S	104291	24-Sep-21 (CTTL No. J21X08326)	Sep-22	Reference Probe EX3DV4	SN 7464	26-Jan-22 (SPEAG No. EX3-7464_Jan22)	Jan-23	DAEA	SN 1566	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MV48071430	13-Jan-22 (CTTL No. J22X00409)	Jan-23	Network Analyzer E5071C	MV48110473	14-Jan-22 (CTTL No. J22X00409)	Jan-23	Calibrated by:	Name	Function	Signature	Reviewed by:	Lin Hao	SAR Test Engineer		Approved by:	Qi Dianyuan	SAR Project Leader		<div style="display: flex; justify-content: space-between;"> </div> <p>Address: Add: No.52 HuaYuanRoad, Haidian District, Beijing, 100191, P.R.China</p> <p>Client: SGS-CN Certificate No: Z22-60184</p> <h3>Glossary:</h3> <p>TSL: liquid simulating liquid ConvF: sensitivity in TSL / NORM.y.z NVA: not applicable or not measured</p> <p>Calibration is Performed According to the Following Standards:</p> <p>a) IEC/IEEE 62209-1529, "Measurement Procedures for the Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices-Part 1529: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDB 865684, "SAR Measurement Requirements for 100 MHz to 6 GHz"</p> <p>Additional Documentation: c) DASy4S System Handbook</p> <p>Methods Applied and Interpretation of Parameters:</p> <ul style="list-style-type: none"> Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss assumes low reflected power. No uncertainty required. Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. SAR measured: SAR measured at the stated antenna input power. SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. <p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p> <p>Certificate No: Z22-60184 Page 1 of 4</p>																		
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																																																												
Power Meter NRP2	106277	24-Sep-21 (CTTL No. J21X08326)	Sep-22																																																												
Power sensor NRP8S	104291	24-Sep-21 (CTTL No. J21X08326)	Sep-22																																																												
Reference Probe EX3DV4	SN 7464	26-Jan-22 (SPEAG No. EX3-7464_Jan22)	Jan-23																																																												
DAEA	SN 1566	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23																																																												
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																																																												
Signal Generator E4438C	MV48071430	13-Jan-22 (CTTL No. J22X00409)	Jan-23																																																												
Network Analyzer E5071C	MV48110473	14-Jan-22 (CTTL No. J22X00409)	Jan-23																																																												
Calibrated by:	Name	Function	Signature																																																												
Reviewed by:	Lin Hao	SAR Test Engineer																																																													
Approved by:	Qi Dianyuan	SAR Project Leader																																																													
<div style="display: flex; justify-content: space-between;"> </div> <p>Address: Add: No.52 HuaYuanRoad, Haidian District, Beijing, 100191, P.R.China</p> <p>Client: SGS-CN Certificate No: Z22-60184</p> <h3>Measurement Conditions</h3> <p>DASy system configuration, as far as is given on page 1</p> <table border="1"> <thead> <tr> <th>DASy Version</th> <th>Configuration</th> <th>Value</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td>52.10.4</td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>15 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>0x, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>300 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table> <h3>Head TSL parameters</h3> <p>The following parameters and calculations were applied:</p> <table border="1"> <thead> <tr> <th>Nominal Head TSL parameters</th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>41.5</td> <td>0.97 mho/m</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><±1.0 °C</td> <td></td> <td></td> </tr> </tbody> </table> <h3>SAR result with Head TSL</h3> <table border="1"> <thead> <tr> <th>SAR averaged over 1 cm³ (1 g) of Head TSL</th> <th>Condition</th> <th>Value</th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>2.70 (W/kg)</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>11.0 (W/kg) ± 18.8 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm³ (10 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>1.75 (W/kg)</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>7.09 (W/kg) ± 16.7 % (k=2)</td> </tr> </tbody> </table> <p>Certificate No: Z22-60184 Page 1 of 4</p>	DASy Version	Configuration	Value	Extrapolation	Advanced Extrapolation	52.10.4	Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	15 mm	with Spacer	Zoom Scan Resolution	0x, dy, dz = 5 mm		Frequency	300 MHz ± 1 MHz		Nominal Head TSL parameters	Temperature	Permittivity	Conductivity	Measured Head TSL parameters	(22.0 ± 0.2) °C	41.5	0.97 mho/m	Head TSL temperature change during test	<±1.0 °C			SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	Value	SAR measured	250 mW input power	2.70 (W/kg)	SAR for nominal Head TSL parameters	normalized to 1W	11.0 (W/kg) ± 18.8 % (k=2)	SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		SAR measured	250 mW input power	1.75 (W/kg)	SAR for nominal Head TSL parameters	normalized to 1W	7.09 (W/kg) ± 16.7 % (k=2)	<div style="display: flex; justify-content: space-between;"> </div> <p>Address: Add: No.52 HuaYuanRoad, Haidian District, Beijing, 100191, P.R.China</p> <p>Client: SGS-CN Certificate No: Z22-60184</p> <h3>Appendix (Additional assessments outside the scope of CNAS L6070)</h3> <h4>Antenna Parameters with Head TSL</h4> <table border="1"> <thead> <tr> <th>Parameter</th> <th>Value</th> </tr> </thead> <tbody> <tr> <td>Impedance, transformed to feed point</td> <td>48 (1.0 - 8.4j)Ω</td> </tr> <tr> <td>Return Loss</td> <td>-23.3 dB</td> </tr> </tbody> </table> <h4>General Antenna Parameters and Design</h4> <table border="1"> <thead> <tr> <th>Parameter</th> <th>Value</th> </tr> </thead> <tbody> <tr> <td>Electrical Delay (line direction)</td> <td>1.312 ns</td> </tr> </tbody> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semi-rigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <h4>Additional EUT Data</h4> <table border="1"> <thead> <tr> <th>Manufacturer</th> <th>Value</th> </tr> </thead> <tbody> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </tbody> </table> <p>Certificate No: Z22-60184 Page 1 of 6</p>	Parameter	Value	Impedance, transformed to feed point	48 (1.0 - 8.4j)Ω	Return Loss	-23.3 dB	Parameter	Value	Electrical Delay (line direction)	1.312 ns	Manufacturer	Value	Manufactured by	SPEAG
DASy Version	Configuration	Value																																																													
Extrapolation	Advanced Extrapolation	52.10.4																																																													
Phantom	Triple Flat Phantom 5.1C																																																														
Distance Dipole Center - TSL	15 mm	with Spacer																																																													
Zoom Scan Resolution	0x, dy, dz = 5 mm																																																														
Frequency	300 MHz ± 1 MHz																																																														
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity																																																												
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.5	0.97 mho/m																																																												
Head TSL temperature change during test	<±1.0 °C																																																														
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	Value																																																													
SAR measured	250 mW input power	2.70 (W/kg)																																																													
SAR for nominal Head TSL parameters	normalized to 1W	11.0 (W/kg) ± 18.8 % (k=2)																																																													
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition																																																														
SAR measured	250 mW input power	1.75 (W/kg)																																																													
SAR for nominal Head TSL parameters	normalized to 1W	7.09 (W/kg) ± 16.7 % (k=2)																																																													
Parameter	Value																																																														
Impedance, transformed to feed point	48 (1.0 - 8.4j)Ω																																																														
Return Loss	-23.3 dB																																																														
Parameter	Value																																																														
Electrical Delay (line direction)	1.312 ns																																																														
Manufacturer	Value																																																														
Manufactured by	SPEAG																																																														



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgs.com.cn
(86-512)57355888 (86-512)57370818 sgs.china@sgs.com

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-4230603-2117
E-mail: cti@china.ttl.com

DASY5 Validation Report for Head TSL Date: 2022-06-07

Test Laboratory: TTL, Beijing, China
DUT: Dipole 900 MHz; Type: D900V2; Serial: D900V2 - SN: 14079
 Communication System: UTD 0, CW; Frequency: 900 MHz; Duty Cycle: 1:1
 Medium parameters used: $f = 900 \text{ MHz}$; $\sigma = 0.98 \text{ S/m}$; $\epsilon_r = 42.65$; $\rho = 1000 \text{ kg/m}^3$
 Phantom section: Right Section
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
 DASY5 Configuration:

- Probe: EX3DV4 - SN7464; ConvF(9.72, 9.72) @ 900 MHz; Calibrated: 2022-01-26
- Sensor-Surface: LAmn (Mechanical Surface Detection)
- Electronic: DA44 S01556; Calibrated: 2023-01-12
- Phantom: MFP_V5.1C (2dlog probe kit); Type: QD 000 P51 Cx; Serial: 1062
- DASY52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0; Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 59.81 V/m; Power Drift = -0.01 dB
 Peak SAR (extrapolated) = 4.20 W/kg
 SAR(1 g) = 2.79 W/kg; SAR(10 g) = 1.78 W/kg
 Smallest distance from peaks to all points 3 dB below = 16 mm
 Ratio of SAR at M2 to SAR at M1 = 65.8%
 Maximum value of SAR (measured) = 3.71 W/kg

Certificate No: Z22-60184 Page 9 of 6

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-4230603-2117
E-mail: cti@china.ttl.com

Impedance Measurement Plot for Head TSL

Certificate No: Z22-60184 Page 9 of 6

1.6 D1800V2 - SN 2d170

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-4230603-2117
E-mail: cti@china.ttl.com

Client: **SGS-CN** Certificate No: **Z22-60105**

CALIBRATION CERTIFICATE

Object: **D1800V2 - SN: 2d170**

Calibration Procedure(s): **FF-Z11-003-01**
 Calibration Procedures for dipole validation kits

Calibration date: **March 31, 2022**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility, environment temperature (23±3)°C and humidity <70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	108277	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No.EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23
Network Analyzer E5071C	MY48110873	14-Jan-22 (CTTL No.J22X00409)	Jan-23

Calibrated by: **Zhao Jing** SAR Test Engineer
 Reviewed by: **Lin Hao** SAR Test Engineer
 Approved by: **Qi Diqiyuan** SAR Project Leader

Issued: April 6, 2022
 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60105 Page 1 of 6

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-4230603-2117
E-mail: cti@china.ttl.com

Glossary:

TSL: tissue simulating liquid
 ConvF: sensitivity in TSL / NORM_{x,y,z}
 N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- KDB 855684, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60105 Page 1 of 6



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN_Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
 中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgsgroup.com.cn
 (86-512)57355888 (86-512)57370818 sgs.china@sgs.com

In Collaboration with
TTL Speag
 CALIBRATION LABORATORY

CAICT

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504
 E-mail: cti@china.ttl.com http://www.chinat.tl.com

Measurement Conditions
 DASYS system configuration, as far as not given on page 1.

DASY Version	DASY52	52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1800 MHz ± 1 MHz	

Head TSL parameters
 The following parameters and calculations were applied:

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	22.0 ± 0.2 °C	40.8 ± 8 %	1.41 mho/m ± 8 %
Head TSL temperature change during test	< 1.0 °C	—	—

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.73 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	38.9 W/kg ± 18.8 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	5.11 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	20.4 W/kg ± 18.7 % (k=2)

Certificate No: Z22-60105 Page 3 of 6

In Collaboration with
TTL Speag
 CALIBRATION LABORATORY

CAICT

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504
 E-mail: cti@china.ttl.com http://www.chinat.tl.com

Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	47.90 - 2.54jΩ
Return Loss	-29.4dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.116 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semi-rigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Certificate No: Z22-60105 Page 4 of 6

In Collaboration with
TTL Speag
 CALIBRATION LABORATORY

CAICT

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504
 E-mail: cti@china.ttl.com http://www.chinat.tl.com

DASY5 Validation Report for Head TSL Date: 2022-03-31
 Test Laboratory: TTL, Beijing, China
 DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN: 2d170
 Communication System: UID 0, CW; Frequency: 1800 MHz; Duty Cycle: 1:1
 Medium parameters used: f = 1800 MHz; σ = 1.41 S/m; ε = 40.62; ρ = 1000 kg/m³
 Phantom section: Right Section
 Measurement Standard: DASY5 (IEEE/ANSI C63.19-2007)
 DASY5 Configuration:

- Probe: EX3DV4 - SN7307; ConvF(8.34, 8.34, 8.34) @ 1800 MHz; Calibrated: 2021-05-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2022-01-12
- Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration/Zoom Scan (7x7x7)(7x7x7)Cube Ø: Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 98.14 V/m; Power Drift = 0.03 dB
 Peak SAR (extrapolated) = 18.2 W/kg
 SAR(1 g) = 9.73 W/kg; SAR(10 g) = 5.11 W/kg
 Smallest distance from peaks to all points 3 dB below = 10 mm
 Ratio of SAR at M2 to SAR at M1 = 54%
 Maximum value of SAR (measured) = 15.2 W/kg

0 dB = 15.2 W/kg = 11.82 dBW/kg

Certificate No: Z22-60105 Page 5 of 6

In Collaboration with
TTL Speag
 CALIBRATION LABORATORY

CAICT

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504
 E-mail: cti@china.ttl.com http://www.chinat.tl.com

Impedance Measurement Plot for Head TSL

Certificate No: Z22-60105 Page 6 of 6



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.
Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN_Doccheck@sgs.com
 No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
 中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgs.com.cn
 (86-512)57355888 (86-512)57370818 sgs.china@sgs.com

1.7 D1900V2 - SN 5d136

<p>Client: SGS-CN Certificate No: Z22-60185</p> <h3>CALIBRATION CERTIFICATE</h3> <p>Object: D1900V2 - SN: 5d136</p> <p>Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits</p> <p>Calibration date: June 7, 2022</p> <p>The calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility, environment temperature (23±0.1) and humidity <math>70\%</math>.</p> <p>Calibration Equipment used (M&E critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter NRP2</td> <td>106277</td> <td>24-Sep-21 (CTTL No. J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Power Sensor NRP65</td> <td>104291</td> <td>24-Sep-21 (CTTL No. J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EXSDV4</td> <td>SN 7464</td> <td>28-Jan-22 (SPEAG No. EX3-7464_Jan22)</td> <td>Jan-23</td> </tr> <tr> <td>DAEA</td> <td>SN 1658</td> <td>12-Jan-22 (CTTL-SPEAG No. Z22-60007)</td> <td>Jan-23</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Signal Generator E4438C</td> <td>MY48071430</td> <td>13-Jan-22 (CTTL No. J22X00409)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyser E5071C</td> <td>MY48110073</td> <td>14-Jan-22 (CTTL No. J22X00406)</td> <td>Jan-23</td> </tr> </tbody> </table> <p>Calibrated by: Zhao Jing, SAR Test Engineer</p> <p>Reviewed by: Lin Hao, SAR Test Engineer</p> <p>Approved by: Qi Danyuan, SAR Project Leader</p> <p>Issued: June 13, 2022</p> <p>The calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> <p>Certificate No: Z22-60185 Page 1 of 6</p>	Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Power Meter NRP2	106277	24-Sep-21 (CTTL No. J21X08326)	Sep-22	Power Sensor NRP65	104291	24-Sep-21 (CTTL No. J21X08326)	Sep-22	Reference Probe EXSDV4	SN 7464	28-Jan-22 (SPEAG No. EX3-7464_Jan22)	Jan-23	DAEA	SN 1658	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No. J22X00409)	Jan-23	Network Analyser E5071C	MY48110073	14-Jan-22 (CTTL No. J22X00406)	Jan-23	<p>Glossary:</p> <p>TSL: tissue simulating liquid</p> <p>ConvF: sensitivity in TSL / NORMx.y.z</p> <p>N/A: not applicable or not measured</p> <p>Calibration is Performed According to the Following Standards:</p> <p>a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-Held and Body-Mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020</p> <p>b) KDB 855884, "SAR Measurement Requirements for 100 MHz to 6 GHz"</p> <p>Additional Documentation:</p> <p>c) DAS4/S System Handbook</p> <p>Methods Applied and Interpretation of Parameters:</p> <ul style="list-style-type: none"> Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. SAR measured: SAR measured at the stated antenna input power. SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. <p>The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p> <p>Certificate No: Z22-60185 Page 2 of 6</p>																								
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																																																						
Power Meter NRP2	106277	24-Sep-21 (CTTL No. J21X08326)	Sep-22																																																						
Power Sensor NRP65	104291	24-Sep-21 (CTTL No. J21X08326)	Sep-22																																																						
Reference Probe EXSDV4	SN 7464	28-Jan-22 (SPEAG No. EX3-7464_Jan22)	Jan-23																																																						
DAEA	SN 1658	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23																																																						
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																																																						
Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No. J22X00409)	Jan-23																																																						
Network Analyser E5071C	MY48110073	14-Jan-22 (CTTL No. J22X00406)	Jan-23																																																						
<p>Measurement Conditions</p> <p>DASY system configuration, as far as not given on page 1:</p> <table border="1"> <thead> <tr> <th>DASY Version</th> <th>DASY52</th> <th>52.10.4</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Tribe Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>1900 MHz ± 1 kHz</td> <td></td> </tr> </tbody> </table> <p>Head TSL parameters</p> <p>The following parameters and calculations were applied:</p> <table border="1"> <thead> <tr> <th>Nominal Head TSL parameters</th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Measured Head TSL parameters</td> <td>22.0 ± 0.2 °C</td> <td>45.0</td> <td>1.42 mS/m</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td>+1.0 °C</td> <td></td> <td></td> </tr> </tbody> </table> <p>SAR result with Head TSL</p> <table border="1"> <thead> <tr> <th>SAR averaged over 1 cm² (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>9.66 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>40.8 W/kg ± 16.8 % (k=2)</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>SAR averaged over 10 cm² (10 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>5.18 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>20.8 W/kg ± 16.7 % (k=2)</td> </tr> </tbody> </table> <p>Certificate No: Z22-60185 Page 3 of 6</p>	DASY Version	DASY52	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Tribe Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	1900 MHz ± 1 kHz		Nominal Head TSL parameters	Temperature	Permittivity	Conductivity	Measured Head TSL parameters	22.0 ± 0.2 °C	45.0	1.42 mS/m	Head TSL temperature change during test	+1.0 °C			SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		SAR measured	250 mW input power	9.66 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	40.8 W/kg ± 16.8 % (k=2)	SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		SAR measured	250 mW input power	5.18 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	20.8 W/kg ± 16.7 % (k=2)	<p>Appendix (Additional assessments outside the scope of CNAS L0570)</p> <h3>Antenna Parameters with Head TSL</h3> <table border="1"> <tbody> <tr> <td>Impedance, transformed to feed point</td> <td>51.5Ω ± 1.5Ω(j)</td> </tr> <tr> <td>Return Loss</td> <td>22.4dB</td> </tr> </tbody> </table> <h3>General Antenna Parameters and Design</h3> <table border="1"> <tbody> <tr> <td>Electrical Delay (one direction)</td> <td>1.109 ns</td> </tr> </tbody> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semi-rigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as specified in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <h3>Additional EUT Data</h3> <table border="1"> <tbody> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </tbody> </table> <p>Certificate No: Z22-60185 Page 4 of 6</p>	Impedance, transformed to feed point	51.5Ω ± 1.5Ω(j)	Return Loss	22.4dB	Electrical Delay (one direction)	1.109 ns	Manufactured by	SPEAG
DASY Version	DASY52	52.10.4																																																							
Extrapolation	Advanced Extrapolation																																																								
Phantom	Tribe Flat Phantom 5.1C																																																								
Distance Dipole Center - TSL	10 mm	with Spacer																																																							
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																								
Frequency	1900 MHz ± 1 kHz																																																								
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity																																																						
Measured Head TSL parameters	22.0 ± 0.2 °C	45.0	1.42 mS/m																																																						
Head TSL temperature change during test	+1.0 °C																																																								
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition																																																								
SAR measured	250 mW input power	9.66 W/kg																																																							
SAR for nominal Head TSL parameters	normalized to 1W	40.8 W/kg ± 16.8 % (k=2)																																																							
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition																																																								
SAR measured	250 mW input power	5.18 W/kg																																																							
SAR for nominal Head TSL parameters	normalized to 1W	20.8 W/kg ± 16.7 % (k=2)																																																							
Impedance, transformed to feed point	51.5Ω ± 1.5Ω(j)																																																								
Return Loss	22.4dB																																																								
Electrical Delay (one direction)	1.109 ns																																																								
Manufactured by	SPEAG																																																								



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN_Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
 中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgs.com.cn
 (86-512)57355888 (86-512)57370818 sgs.china@sgs.com

DASY5 Validation Report for Head TSL
 Test Laboratory: CTTL, Beijing, China
 DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 54136
 Communication System: UTD 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1
 Medium parameters used: $f = 1900 \text{ MHz}$; $a = 1.385 \text{ S/m}$; $\epsilon = 39.85$; $\rho = 1000 \text{ kg/m}^3$
 Phantom section: Right Section
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
 DASY5 Configuration:
 • Probe: EX3DV4 - SN7464; ConvF(8,18, 8,18, 8,18) @ 1900 MHz; Calibrated: 2022-01-26
 • Sensor-Surface: 1.4mm (Mechanical Surface Detection)
 • Electronics: DAE4 Sn1556; Calibrated: 2022-01-12
 • Phantom: MFP_V3_IC (20kg probe III); Type: QD 000 P51 Cx; Serial: 1062
 • DASY5 52.10.4(1555); SEMCAD X.14.6-14(7501)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube D- Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 99.99 V/m; Power Drift = 0.04 dB
 Peak SAR (extrapolated) = 18.6 W/kg
 SAR(1 g) = 9.95 W/kg; SAR(10 g) = 5.18 W/kg
 Smallest distance from peaks to all points 3 dB below = 9.2 mm
 Ratio of SAR at M2 to SAR at M1 = 54.1%
 Maximum value of SAR (measured) = 15.6 W/kg

0 dB = 15.6 W/kg = 11.93 dBW/kg

Impedance Measurement Plot for Head TSL

Plot 1: Real and Imaginary parts of the impedance. The real part is approximately 1.00000 and the imaginary part is approximately -0.00000.

Plot 2: Smith chart showing the impedance measurement.

1.8 D2000V2 - SN 1041

Client: SGS-CN Certificate No: Z22-60186

Object: D2000V2 - SN 1041

Calibration Procedure(s): FF-Z11-003-01

Calibration date: June 6, 2022

The calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22±3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No. J21-K06328)	Sep-22
Power sensor NRP2S	104291	24-Sep-21 (CTTL No. J21-K06328)	Sep-22
Reference Probe EX3DVA	SN 7464	26-Jan-22 (SPEAG No. EX3-7464-Jan22)	Jan-23
DAEA	SN 1556	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No. J22X00408)	Jan-23
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No. J22X00408)	Jan-23

Calibrated by: Zhao Jing, SAR Test Engineer
 Reviewed by: Lin Hao, SAR Test Engineer
 Approved by: Qi Dianyan, SAR Project Leader

Glossary:

TSL: Issue simulating liquid
 ConvF: sensitivity in TSL / INORMx.y.z
 N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEC/IEEE 62209-1528, Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-Head and Body-Mounted Wireless Communication Devices; Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz), October 2020
- KDB 955664, SAR Measurement Requirements for 100 MHz to 6 GHz

Additional Documentation:

- DASY5/S System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
 中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgsgroup.com.cn
 (86-512)57355888 (86-512)57370818 sgs.china@sgs.com

In Collaboration with **TTL Calibration Laboratory** and **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-4239632-2117
 E-mail: emc@sgs.com.cn

Measurement Conditions
 DASYS system configuration, as for as not given on page 1.

DASY Version	DASYV2	52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom S.I.C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2000 MHz ± 1 MHz	

Head TSL parameters
 The following parameters and calculations were applied:

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.9 °C	40.0'	1.40 mho/cm
Measured Head TSL parameters	(22.9 ± 0.2) °C	40.2 ± 0.5 %	1.36 mho/cm ± 0.6 %
Head TSL temperature change during test	-1.0 °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	10.4 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	41.8 W/kg ± 18.8 % (n=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	5.30 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.3 W/kg ± 18.7 % (n=2)

Certificate No: Z22-60186 Page 3 of 6

In Collaboration with **TTL Calibration Laboratory** and **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-4239632-2117
 E-mail: emc@sgs.com.cn

Appendix (Additional assessments outside the scope of CNAS L6570)

Antenna Parameters with Head TSL

Impedance: transformed to feed point	48.40 ± 0.74(j)
Return Loss	-34 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.086 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semi-rigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

Additional EUT Data

Manufactured by	BPEAG
-----------------	-------

Certificate No: Z22-60186 Page 4 of 6

In Collaboration with **TTL Calibration Laboratory** and **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-4239632-2117
 E-mail: emc@sgs.com.cn

DASY5 Validation Report for Head TSL
 Date: 2022-06-06
 Test Laboratory: CTTL, Beijing, China
 DUT: Dipole 2000 MHz; Type: D2000V2; Serial: D2000V2 - SN: 1041
 Communication System: UFD 0; CW; Frequency: 2000 MHz; Duty Cycle: 1:1
 Medium parameters used: f = 2000 MHz; σ = 1.392 S/m; ε = 40.21; ρ = 1000 kg/m³
 Phantom section: Right Section
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
 DASY5 Configuration:

- Probe: EX3DV4 - SN7464; ConvF(R,2, 8,2) @ 2000 MHz; Calibrated: 2022-01-26
- Sensor Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DA64 Sn1556; Calibrated: 2022-01-12
- Phantom: MFP_V5.I.C (20dkg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY5: 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7); Cube 0; Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 103.4 V/m; Power Dfth = 0.03 dB
 Peak SAR (extrapolated) = 19.6 W/kg
 SAR(1 g) = 10.4 W/kg; SAR(10 g) = 5.3 W/kg
 Smallest distance from peaks to all points 3 dB below = 9.1 mm
 Ratio of SAR at M2 to SAR at M1 = 53.0%

Maximum value of SAR (measured) = 16.3 W/kg

0 dB = 16.3 W/kg = 12.12 dBW/kg

Certificate No: Z22-60186 Page 5 of 6

In Collaboration with **TTL Calibration Laboratory** and **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-4239632-2117
 E-mail: emc@sgs.com.cn

Impedance Measurement Plot for Head TSL

Certificate No: Z22-60186 Page 6 of 6



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN_Doccheck@sgs.com

No.10, Weiyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
 中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
 t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

1.9 D2300V2 - SN 1096

<p>Address: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2512 Fax: +86-10-42304633-2594 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn</p>		<p>Address: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2594 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn</p>	
<p>Client: SGS-CN Certificate No: Z22-60106</p>			
<p>CALIBRATION CERTIFICATE</p>			
Object	D2300V2 - SN 1096		
Calibration Procedure(s)	FF-Z11-003-01 Calibration Procedures for dipole validation kits		
Calibration date:	March 31, 2022		
<p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.</p> <p>Calibration Equipment used (M&TE critical for calibration)</p>			
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	108277	24-Sep-21 (CTTL No.J21X08328)	Sep-22
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08328)	Sep-22
Reference Probe EK30V4 DAE4	SN 7307 SN 1556	26-May-21 (SPEAG No.EK3-7307_May21) 12-Jan-22 (CTTL-SPEAG No.Z22-600007)	May-22 Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00408)	Jan-23
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No.J22X00408)	Jan-23
Calibrated by:	Name: Zhao Jing	Function: SAR Test Engineer	Signature: [Signature]
Reviewed by:	Name: Lin Hao	Function: SAR Test Engineer	Signature: [Signature]
Approved by:	Name: Qi Dianyan	Function: SAR Project Leader	Signature: [Signature]
<p>Issued: April 6, 2022</p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p>			
Certificate No: Z22-60106		Page 1 of 6	

<p>Address: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2594 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn</p>		<p>Address: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2594 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn</p>																			
<p>Measurement Conditions DASY system configuration, as far as not given on page 1</p> <table border="1"> <tr> <td>DASY Version</td> <td>DASY2</td> <td>52.10.4</td> </tr> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1G</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>(dx, dy, dz = 5 mm)</td> <td></td> </tr> <tr> <td>Frequency</td> <td>2300 MHz ± 1 MHz</td> <td></td> </tr> </table>				DASY Version	DASY2	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1G		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	(dx, dy, dz = 5 mm)		Frequency	2300 MHz ± 1 MHz	
DASY Version	DASY2	52.10.4																			
Extrapolation	Advanced Extrapolation																				
Phantom	Triple Flat Phantom 5.1G																				
Distance Dipole Center - TSL	10 mm	with Spacer																			
Zoom Scan Resolution	(dx, dy, dz = 5 mm)																				
Frequency	2300 MHz ± 1 MHz																				
<p>Head TSL parameters The following parameters and calculations were applied:</p> <table border="1"> <tr> <td></td> <td>Temperature</td> <td>Permittivity</td> <td>Conductivity</td> </tr> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>39.5</td> <td>1.67 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>39.8 ± 9 %</td> <td>1.70 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><1.0 °C</td> <td></td> <td></td> </tr> </table>					Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	39.5	1.67 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	39.8 ± 9 %	1.70 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C				
	Temperature	Permittivity	Conductivity																		
Nominal Head TSL parameters	22.0 °C	39.5	1.67 mho/m																		
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.8 ± 9 %	1.70 mho/m ± 6 %																		
Head TSL temperature change during test	<1.0 °C																				
<p>SAR result with Head TSL</p> <table border="1"> <tr> <td>SAR averaged over 1 cm² (1g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>12.4 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>48.2 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm² (10g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>5.88 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>23.4 W/kg ± 18.7 % (k=2)</td> </tr> </table>				SAR averaged over 1 cm ² (1g) of Head TSL	Condition		SAR measured	250 mW input power	12.4 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	48.2 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ² (10g) of Head TSL	Condition		SAR measured	250 mW input power	5.88 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	23.4 W/kg ± 18.7 % (k=2)
SAR averaged over 1 cm ² (1g) of Head TSL	Condition																				
SAR measured	250 mW input power	12.4 W/kg																			
SAR for nominal Head TSL parameters	normalized to 1W	48.2 W/kg ± 18.8 % (k=2)																			
SAR averaged over 10 cm ² (10g) of Head TSL	Condition																				
SAR measured	250 mW input power	5.88 W/kg																			
SAR for nominal Head TSL parameters	normalized to 1W	23.4 W/kg ± 18.7 % (k=2)																			
Certificate No: Z22-60106		Page 3 of 6																			

<p>Address: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2594 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn</p>		<p>Address: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2594 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn</p>	
<p>Glossary:</p> <p>TSL: Issue simulating liquid ConvF: sensitivity in TSL / NCF/Ma,y,z N/A: not applicable or not measured</p>			
<p>Calibration is Performed According to the Following Standards:</p> <p>a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020. b) KDB 855664, "SAR Measurement Requirements for 100 MHz to 8 GHz"</p>			
<p>Additional Documentation: c) DASY4/5 System Handbook</p>			
<p>Methods Applied and Interpretation of Parameters:</p> <ul style="list-style-type: none"> Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. SAR measured: SAR measured at the stated antenna input power. SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. 			
<p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p>			
Certificate No: Z22-60106		Page 2 of 6	

<p>Address: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2594 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn</p>		<p>Address: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2594 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn</p>					
<p>Appendix (Additional assessments outside the scope of CNAS L0570)</p>							
<p>Antenna Parameters with Head TSL</p> <table border="1"> <tr> <td>Impedance, transformed to feed point</td> <td>49.20; 4.59(j)</td> </tr> <tr> <td>Return Loss</td> <td>-26.9dB</td> </tr> </table>				Impedance, transformed to feed point	49.20; 4.59(j)	Return Loss	-26.9dB
Impedance, transformed to feed point	49.20; 4.59(j)						
Return Loss	-26.9dB						
<p>General Antenna Parameters and Design</p> <table border="1"> <tr> <td>Electrical Delay (one direction)</td> <td>1.083 ns</td> </tr> </table>				Electrical Delay (one direction)	1.083 ns		
Electrical Delay (one direction)	1.083 ns						
<p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p>							
<p>Additional EUT Data</p> <table border="1"> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </table>				Manufactured by	SPEAG		
Manufactured by	SPEAG						
Certificate No: Z22-60106		Page 4 of 6					





Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgs.com.cn
(86-512)57355888 (86-512)57370818 sgs.china@sgs.com

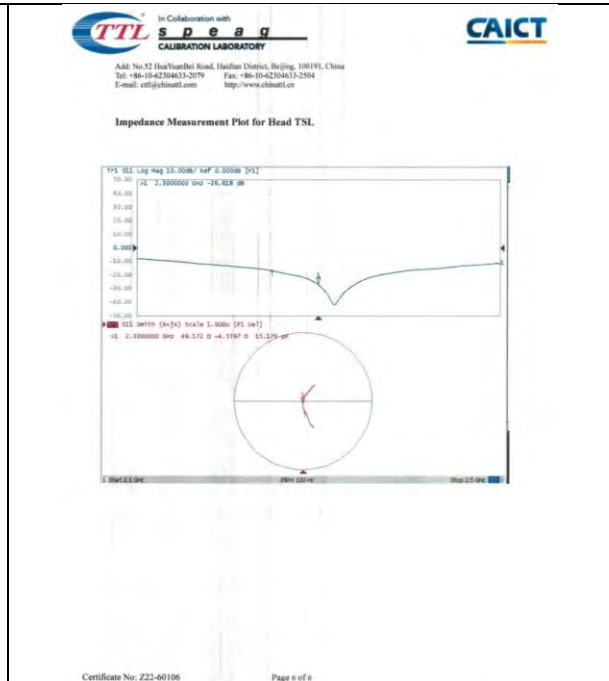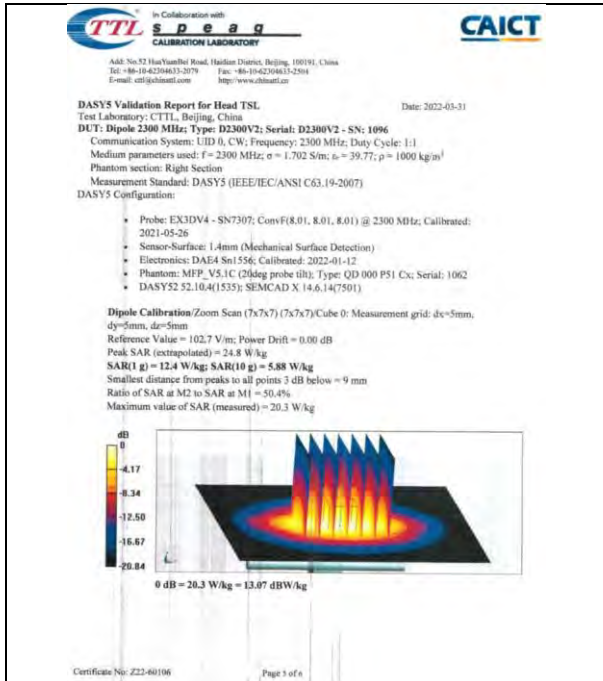

1.10 D2450V2 - SN 817

Client: SGS-CN Certificate No: Z22-60107

CALIBRATION CERTIFICATE

Object: D2450V2 - SN 817
 Calibration Procedure(s): FF-Z11-003-01
 Calibration date: April 1, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter: NRP2	108277	24-Sep-21 (CTTL No.J21X08320)	Sep-22
Power sensor: NRP8S	104291	24-Sep-21 (CTTL No.J21X08320)	Sep-22
Reference Probe: EX3DV4	SN 7307	25-May-21(SPEAG.No.EK3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG.No.Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator: E4438C	MY4007430	13-Jan-22 (CTTL No. J22X00400)	Jan-23
Network Analyzer: E5071C	MY48110873	14-Jan-22 (CTTL No. J22X00406)	Jan-23

Calibrated by: Zhao Jing (SAR Test Engineer)
 Reviewed by: Lin Hao (SAR Test Engineer)
 Approved by: Qi Dianyan (SAR Project Leader)

Issued: April 6, 2022

Glossary:
 TSL: tissue simulating liquid
 ConvF: sensitivity in TSL / NORMix.y.z
 N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:
 a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October, 2020
 b) KDB 656684, "SAR Measurement Requirements for 100 MHz to 5 GHz"

Additional Documentation:
 c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- **Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- **Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- **Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- **Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- **SAR measured:** SAR measured at the stated antenna input power.
- **SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- **SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor $k=2$ which for a normal distribution Corresponds to a coverage probability of approximately 95%.



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.
Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
 中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgsgroup.com.cn
 (86-512)57355888 (86-512)57370818 sgs.china@sgs.com

In Collaboration with **TTL Speaq** CALIBRATION LABORATORY and **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304633-3079 Fax: +86-10-42304633-2504
 E-mail: cn@china-test.com http://www.china-test.com

Measurement Conditions
 DASYS system configuration, as far as not given on page 1:

DASY Version	DASY52	52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

Head TSL parameters
 The following parameters and calculations were applied:

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.5 ± 6 %	1.79 mho/m ± 8 %
Head TSL temperature change during test	<+1.0 °C	—	—

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.2 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	53.0 W/kg ± 18.8 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	6.15 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.7 W/kg ± 18.7 % (k=2)

Certificate No: Z22-60107 Page 3 of 6

In Collaboration with **TTL Speaq** CALIBRATION LABORATORY and **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304633-3079 Fax: +86-10-42304633-2504
 E-mail: cn@china-test.com http://www.china-test.com

Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	52.1Ω ± 3.2Ω
Return Loss	-26.5dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.086 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard ferringid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Certificate No: Z22-60107 Page 4 of 6

In Collaboration with **TTL Speaq** CALIBRATION LABORATORY and **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304633-3079 Fax: +86-10-42304633-2504
 E-mail: cn@china-test.com http://www.china-test.com

DASY5 Validation Report for Head TSL Date: 2022-04-01

Test Laboratory: CTTL, Beijing, China
 DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 817
 Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1
 Medium parameters used: f = 2450 MHz; σ = 1.79 S/m; ε = 39.52; ρ = 1000 kg/m³
 Phantom section: Right Section
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
 DASY5 Configuration:

- Probe: EX3DV4 - SN7307; ConvF(7.75, 7.75) @ 2450 MHz; Calibrated: 2021-05-26
- Sensor-Surface: 1 Arm (Mechanical Surface Detection)
- Electronics: DA54 Sn1556; Calibrated: 2022-01-12
- Phantom: MFP_V5.1C (20kg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 104.6 V/m; Power Drift = -0.03 dB
 Peak SAR (extrapolated) = 27.0 W/kg
SAR(1 g) = 13.2 W/kg; SAR(10 g) = 6.15 W/kg
 Smallest distance from peaks to all points 3 dB below = 8.9 mm
 Ratio of SAR at M2 to SAR at M1 = -49.2%
 Maximum value of SAR (measured) = 22.1 W/kg

0 dB = 22.1 W/kg = 13.44 dBW/kg

Certificate No: Z22-60107 Page 5 of 6

In Collaboration with **TTL Speaq** CALIBRATION LABORATORY and **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304633-3079 Fax: +86-10-42304633-2504
 E-mail: cn@china-test.com http://www.china-test.com

Impedance Measurement Plot for Head TSL

Certificate No: Z22-60107 Page 6 of 6



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN_Doccheck@sgs.com

No. 10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
 中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

(86-512) 57355888 (86-512) 57370818 www.sgs.com.cn
 (86-512) 57355888 (86-512) 57370818 sgs.china@sgs.com

1.11 D2600V2 - SN 1158

<p>Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-42304633-2912 Fax: +86-10-42304633-2904 E-mail: csi@ttspeag.com.cn http://www.ttspeag.com</p> <p>Client: SGS-CN Certificate No: Z22-60108</p> <h3>CALIBRATION CERTIFICATE</h3> <p>Object: D2600V2 - SN 1158</p> <p>Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits</p> <p>Calibration date: March 31, 2022</p> <p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (23±3)°C and humidity<70%.</p> <p>Calibration Equipment used (M&TE critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter NRP2</td> <td>102577</td> <td>24-Sep-21 (CTTL No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP8S</td> <td>104291</td> <td>24-Sep-21 (CTTL No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX301VA</td> <td>SN 7307</td> <td>26-May-21(SPEAG.No.EX3-7307_May21)</td> <td>May-22</td> </tr> <tr> <td>DAE4</td> <td>SN 1556</td> <td>12-Jan-22(CTTL-SPEAG.No.Z22-60007)</td> <td>Jan-23</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Signal Generator E4438C</td> <td>MY49671430</td> <td>13-Jan-22 (CTTL No.Z22X00409)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MY48110673</td> <td>14-Jan-22 (CTTL No.Z22X00406)</td> <td>Jan-23</td> </tr> </tbody> </table> <p>Calibrated by: Zhao Jing SAR Test Engineer</p> <p>Reviewed by: Lin Hao SAR Test Engineer</p> <p>Approved by: Qi Dianyuan SAR Project Leader</p> <p>Issued: April 6, 2022</p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> <p>Certificate No: Z22-60108 Page 1 of 6</p>	Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Power Meter NRP2	102577	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Reference Probe EX301VA	SN 7307	26-May-21(SPEAG.No.EX3-7307_May21)	May-22	DAE4	SN 1556	12-Jan-22(CTTL-SPEAG.No.Z22-60007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY49671430	13-Jan-22 (CTTL No.Z22X00409)	Jan-23	Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.Z22X00406)	Jan-23	<p>Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2919 Fax: +86-10-42304633-2904 E-mail: csi@ttspeag.com.cn http://www.ttspeag.com</p> <p>Glossary: TSL: tissue simulating liquid ConvF: sensitivity in TSL / NORMx.y.z N/A: not applicable or not measured</p> <p>Calibration is Performed According to the Following Standards: a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"</p> <p>Additional Documentation: c) DASY4/S System Handbook</p> <p>Methods Applied and Interpretation of Parameters:</p> <ul style="list-style-type: none"> Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. SAR measured: SAR measured at the stated antenna input power. SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. <p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.</p> <p>Certificate No: Z22-60108 Page 2 of 6</p>																												
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																																																										
Power Meter NRP2	102577	24-Sep-21 (CTTL No.J21X08326)	Sep-22																																																										
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22																																																										
Reference Probe EX301VA	SN 7307	26-May-21(SPEAG.No.EX3-7307_May21)	May-22																																																										
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG.No.Z22-60007)	Jan-23																																																										
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																																																										
Signal Generator E4438C	MY49671430	13-Jan-22 (CTTL No.Z22X00409)	Jan-23																																																										
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.Z22X00406)	Jan-23																																																										
<p>Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-3079 Fax: +86-10-42304633-2904 E-mail: csi@ttspeag.com.cn http://www.ttspeag.com</p> <h3>Measurement Conditions</h3> <p>DASY system configuration, as far as not given on page 1</p> <table border="1"> <thead> <tr> <th>DASY Version</th> <th>DASY32</th> <th>52,10,4</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>5x, 6y, 6z = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>2600 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table> <h3>Head TSL parameters</h3> <p>The following parameters and calculations were applied:</p> <table border="1"> <thead> <tr> <th></th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>38.0</td> <td>1.96 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>38.7 ± 0.5 %</td> <td>1.96 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><1.0 °C</td> <td>---</td> <td>---</td> </tr> </tbody> </table> <h3>SAR result with Head TSL</h3> <table border="1"> <thead> <tr> <th>SAR averaged over 1 cm² (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>13.7 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>64.8 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm² (10 g) of Head TSL</td> <th>Condition</th> <th></th> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>8.12 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>24.5 W/kg ± 18.7 % (k=2)</td> </tr> </tbody> </table> <p>Certificate No: Z22-60108 Page 3 of 6</p>	DASY Version	DASY32	52,10,4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	5x, 6y, 6z = 5 mm		Frequency	2600 MHz ± 1 MHz			Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	38.0	1.96 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	38.7 ± 0.5 %	1.96 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	---	---	SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		SAR measured	250 mW input power	13.7 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	64.8 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		SAR measured	250 mW input power	8.12 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	24.5 W/kg ± 18.7 % (k=2)	<p>Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-3079 Fax: +86-10-42304633-2904 E-mail: csi@ttspeag.com.cn http://www.ttspeag.com</p> <h3>Appendix (Additional assessments outside the scope of CNAS L0570)</h3> <h4>Antenna Parameters with Head TSL</h4> <table border="1"> <thead> <tr> <th>Impedance, transformed to feed point</th> <th>49.90j - 6.49Ω</th> </tr> </thead> <tbody> <tr> <td>Return Loss</td> <td>-23.9dB</td> </tr> </tbody> </table> <h4>General Antenna Parameters and Design</h4> <table border="1"> <thead> <tr> <th>Electrical Delay (one direction)</th> <th>1.053 ns</th> </tr> </thead> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semi-rigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <h4>Additional EUT Data</h4> <table border="1"> <thead> <tr> <th>Manufactured by</th> <th>SPEAG</th> </tr> </thead> </table> <p>Certificate No: Z22-60108 Page 4 of 6</p>	Impedance, transformed to feed point	49.90j - 6.49Ω	Return Loss	-23.9dB	Electrical Delay (one direction)	1.053 ns	Manufactured by	SPEAG
DASY Version	DASY32	52,10,4																																																											
Extrapolation	Advanced Extrapolation																																																												
Phantom	Triple Flat Phantom 5.1C																																																												
Distance Dipole Center - TSL	10 mm	with Spacer																																																											
Zoom Scan Resolution	5x, 6y, 6z = 5 mm																																																												
Frequency	2600 MHz ± 1 MHz																																																												
	Temperature	Permittivity	Conductivity																																																										
Nominal Head TSL parameters	22.0 °C	38.0	1.96 mho/m																																																										
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.7 ± 0.5 %	1.96 mho/m ± 6 %																																																										
Head TSL temperature change during test	<1.0 °C	---	---																																																										
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition																																																												
SAR measured	250 mW input power	13.7 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	64.8 W/kg ± 18.8 % (k=2)																																																											
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition																																																												
SAR measured	250 mW input power	8.12 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	24.5 W/kg ± 18.7 % (k=2)																																																											
Impedance, transformed to feed point	49.90j - 6.49Ω																																																												
Return Loss	-23.9dB																																																												
Electrical Delay (one direction)	1.053 ns																																																												
Manufactured by	SPEAG																																																												



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgsgroup.com.cn
(86-512)57355888 (86-512)57370818 sgs.china@sgs.com

In Collaboration with **TTL Speag** CALIBRATION LABORATORY and **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62104613-2079 Fax: +86-10-62104613-2504
E-mail: cti@ttspeag.com http://www.ttspeag.com

DASY5 Validation Report for Head TSL Date: 2022-03-31

Test Laboratory: CTTL, Beijing, China
DUT: Dipole 2600 MHz; Type: D2600V2; Serial: D2600V2 - SN: 1158
Communication System: UID 0, CW; Frequency: 2600 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2600$ MHz; $\sigma = 1.955$ S/m; $\epsilon_r = 38.68$; $\rho = 1000$ kg/m³
Phantom section: Right Section
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
DASY5 Configuration:

- Probe: EX3DV4 - SN7307; ConvF(7.5, 7.5, 7.5) @ 2600 MHz; Calibrated: 2021-05-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2022-01-12
- Phantom: MFP-V5.1C (20deg probe tilt); Type: QD 000 P5) Cx; Serial: 1062
- DASY52.52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube @ Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 103.3 V/m; Power Drift = 0.04 dB
Peak SAR (extrapolated) = 29.0 W/kg
SAR(1 g) = 13.7 W/kg; SAR(10 g) = 6.12 W/kg
Smallest distance from peaks to all points 3 dB below = 8.9 mm
Ratio of SAR at M2 to SAR at M1 = 47.5%
Maximum value of SAR (measured) = 23.4 W/kg

0 dB = 23.4 W/kg = 13.69 dBW/kg

Certificate No: Z22-60108 Page 1 of 6

In Collaboration with **TTL Speag** CALIBRATION LABORATORY and **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62104613-2079 Fax: +86-10-62104613-2504
E-mail: cti@ttspeag.com http://www.ttspeag.com

Impedance Measurement Plot for Head TSL

Certificate No: Z22-60108 Page 6 of 6

1.12 D5GHZV2 - SN 1095

In Collaboration with **TTL Speag** CALIBRATION LABORATORY, **ILAC**, **CNAS**, **UKAS**, **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62104613-2079 Fax: +86-10-62104613-2504
E-mail: cti@ttspeag.com http://www.ttspeag.com

Client: **SGS-CN** Certificate No: **Z22-60187**

CALIBRATION CERTIFICATE

Object: D5GHZV2 - SN 1095

Calibration Procedure(s): FF-Z11-003-01
Calibration Procedures for dipole validation kits

Calibration date: June 1, 2022

The calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (23±1)°C and humidity < 70%.

Calibration Equipment used (MSTE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No. J211008326)	Sep-22
Power sensor NRP85	104291	24-Sep-21 (CTTL No. J211008326)	Sep-22
Reference Probe EX3DV4	SN 7464	26-Jan-22(SPEAG No. EX3-7484, Jan22)	Jan-23
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG No. Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No. J22X00406)	Jan-23
Network Analyzer E5071C	MY46110873	14-Jan-22 (CTTL No. J22X00406)	Jan-23

Calibrated by: Zhao Jing, SAR Test Engineer
Reviewed by: Lin Hao, SAR Test Engineer
Approved by: Qi Dianyan, SAR Project Leader

Issued: June 6, 2022
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60187 Page 1 of 10

In Collaboration with **TTL Speag** CALIBRATION LABORATORY and **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62104613-2079 Fax: +86-10-62104613-2504
E-mail: cti@ttspeag.com http://www.ttspeag.com

Glossary:

- TSL: Issue simulating liquid
- CompF: sensitivity in TSL: 1/MORMX,y,z
- N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEC/IEEE 62209-1528, "Measurement Procedure for the Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- KDB 665664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance station is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60187 Page 7 of 10



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN_Doccheck@sgs.com

No. 10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgsgroup.com.cn
(86-512)57355888 (86-512)57370818 sgs.china@sgs.com

In Collaboration with
T T L
CALIBRATION LABORATORY

Address: No. 57 HuaYuanBei Road, Huailin District, Beijing, 100191, China
Tel: +86-10-62320117
E-mail: ttt@ttml.com.cn http://www.ttml.com.cn

CAICT

Measurement Conditions
DA87 system configuration, see for as not given on page 1.

DA87 Version	DA87S2	32,10,4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom S,1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4 mm, dz = 1.4 mm	(Graded Ratio = 1.4 (Z direction))
Frequency	500 MHz ± 1 MHz 6300 MHz ± 1 MHz 3500 MHz ± 1 MHz 5600 MHz ± 1 MHz	

Head TSL parameters at 5200MHz
The following parameters and calculations were applied:

Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
	22.0 °C	35.9	4.68 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.4 ± 6 %	4.42 mho/m ± 6 %
Head TSL temperature change during test	-1.0 °C	—	—

SAR result with Head TSL at 5200MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition
SAR measured	250 mW input power 7.75 W/kg
SAR for nominal Head TSL parameters	normalized to 1W 77.8 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition
SAR measured	250 mW input power 2.22 W/kg
SAR for nominal Head TSL parameters	normalized to 1W 22.1 W/kg ± 24.2 % (k=2)

Certificate No: Z22-6018T Page 1 of 10

In Collaboration with
T T L
CALIBRATION LABORATORY

Address: No. 57 HuaYuanBei Road, Huailin District, Beijing, 100191, China
Tel: +86-10-62320117
E-mail: ttt@ttml.com.cn http://www.ttml.com.cn

CAICT

Head TSL parameters at 5300MHz
The following parameters and calculations were applied:

Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
	22.0 °C	35.9	4.76 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.2 ± 6 %	4.73 mho/m ± 6 %
Head TSL temperature change during test	-1.0 °C	—	—

SAR result with Head TSL at 5300MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition
SAR measured	100 mW input power 7.84 W/kg
SAR for nominal Head TSL parameters	normalized to 1W 78.1 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition
SAR measured	100 mW input power 2.27 W/kg
SAR for nominal Head TSL parameters	normalized to 1W 22.6 W/kg ± 24.2 % (k=2)

Head TSL parameters at 5500MHz
The following parameters and calculations were applied:

Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
	22.0 °C	35.8	4.88 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.8 ± 6 %	4.84 mho/m ± 6 %
Head TSL temperature change during test	-1.0 °C	—	—

SAR result with Head TSL at 5500MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition
SAR measured	100 mW input power 8.26 W/kg
SAR for nominal Head TSL parameters	normalized to 1W 82.6 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition
SAR measured	100 mW input power 2.34 W/kg
SAR for nominal Head TSL parameters	normalized to 1W 23.3 W/kg ± 24.2 % (k=2)

Certificate No: Z22-6018T Page 4 of 10

In Collaboration with
T T L
CALIBRATION LABORATORY

Address: No. 57 HuaYuanBei Road, Huailin District, Beijing, 100191, China
Tel: +86-10-62320117
E-mail: ttt@ttml.com.cn http://www.ttml.com.cn

CAICT

Head TSL parameters at 5600MHz
The following parameters and calculations were applied:

Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.7 ± 6 %	5.05 mho/m ± 6 %
Head TSL temperature change during test	-1.0 °C	—	—

SAR result with Head TSL at 5600MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition
SAR measured	100 mW input power 8.12 W/kg
SAR for nominal Head TSL parameters	normalized to 1W 80.8 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition
SAR measured	100 mW input power 2.38 W/kg
SAR for nominal Head TSL parameters	normalized to 1W 22.9 W/kg ± 24.2 % (k=2)

Head TSL parameters at 5800MHz
The following parameters and calculations were applied:

Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
	22.0 °C	35.3	5.27 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.4 ± 6 %	5.25 mho/m ± 6 %
Head TSL temperature change during test	-1.0 °C	—	—

SAR result with Head TSL at 5800MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition
SAR measured	100 mW input power 7.71 W/kg
SAR for nominal Head TSL parameters	normalized to 1W 76.7 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition
SAR measured	100 mW input power 2.16 W/kg
SAR for nominal Head TSL parameters	normalized to 1W 21.6 W/kg ± 24.2 % (k=2)

Certificate No: Z22-6018T Page 5 of 10

In Collaboration with
T T L
CALIBRATION LABORATORY

Address: No. 57 HuaYuanBei Road, Huailin District, Beijing, 100191, China
Tel: +86-10-62320117
E-mail: ttt@ttml.com.cn http://www.ttml.com.cn

CAICT

Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL at 5200MHz

Impedance, transformed to feed point	46.10-5.03jΩ
Return Loss	-23.6dB

Antenna Parameters with Head TSL at 5300MHz

Impedance, transformed to feed point	47.80-2.42jΩ
Return Loss	-23.5dB

Antenna Parameters with Head TSL at 5500MHz

Impedance, transformed to feed point	50.30-4.36jΩ
Return Loss	-27.4dB

Antenna Parameters with Head TSL at 5600MHz

Impedance, transformed to feed point	54.80-4.89jΩ
Return Loss	-24.6dB

Antenna Parameters with Head TSL at 5800MHz

Impedance, transformed to feed point	51.50-5.61jΩ
Return Loss	-24.6dB

Certificate No: Z22-6018T Page 6 of 10



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us by telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgs.com.cn
(86-512)57355888 (86-512)57370818 sgs.china@sgs.com

In Collaboration with
T T L
CALIBRATION LABORATORY

ADD: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62302117
E-mail: csl@ttsl.com.cn http://www.ttsl.com.cn

General Antenna Parameters and Design

Electrical Delay (one direction): 1.101 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The carrier conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

Additional EUT Data

Manufactured by: SPEAQ

Certificate No: Z22-60187 Page 1 of 10

In Collaboration with
T T L
CALIBRATION LABORATORY

ADD: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62302117
E-mail: csl@ttsl.com.cn http://www.ttsl.com.cn

DASY5 Validation Report for Head TSL

Test Laboratory: CTTL, Beijing, China
Date: 2022-04-01

DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1095

Communication System: CW; Frequency: 5200 MHz; Frequency: 5300 MHz; Frequency: 5500 MHz; Frequency: 5600 MHz; Frequency: 5800 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 5200 \text{ MHz}$; $\sigma = 4.82 \text{ S/m}$; $\epsilon = 35.39$; $\rho = 1000 \text{ kg/m}^3$

Medium parameters used: $f = 5300 \text{ MHz}$; $\sigma = 4.73 \text{ S/m}$; $\epsilon = 35.19$; $\rho = 1000 \text{ kg/m}^3$

Medium parameters used: $f = 5500 \text{ MHz}$; $\sigma = 4.939 \text{ S/m}$; $\epsilon = 34.83$; $\rho = 1000 \text{ kg/m}^3$

Medium parameters used: $f = 5600 \text{ MHz}$; $\sigma = 5.051 \text{ S/m}$; $\epsilon = 34.89$; $\rho = 1000 \text{ kg/m}^3$

Medium parameters used: $f = 5800 \text{ MHz}$; $\sigma = 5.247 \text{ S/m}$; $\epsilon = 34.42$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI CS3.16-2007)

DASY5 Configuration:

- Probe: EX3DV4 - SN7484; ConvF(5, 6, 5, 6) @ 5200 MHz; ConvF(5, 32, 5, 32) @ 5300 MHz; ConvF(5, 11, 5, 11) @ 5500 MHz; ConvF(4, 9, 4, 9) @ 5800 MHz; ConvF(5, 5, 5) @ 5600 MHz; Calibrated: 2022-01-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DA84 Sn1556; Calibrated: 2022-01-12
- Phantom: MFP_V5-1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration /Pin=100mW, d=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Reference Value = 60.80 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 29.8 W/kg

SAR(1g) = 7.73 W/kg; SAR(10g) = 2.22 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 66.8%

Maximum value of SAR (measured) = 19.3 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Reference Value = 61.08 V/m; Power Drift = -0.07 dB

Peak SAR (extrapolated) = 31.5 W/kg

SAR(1g) = 7.94 W/kg; SAR(10g) = 2.27 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 65.5%

Maximum value of SAR (measured) = 19.0 W/kg

Certificate No: Z22-60187 Page 4 of 10

In Collaboration with
T T L
CALIBRATION LABORATORY

ADD: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62302117
E-mail: csl@ttsl.com.cn http://www.ttsl.com.cn

Dipole Calibration /Pin=100mW, d=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Reference Value = 61.92 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 34.7 W/kg

SAR(1g) = 8.28 W/kg; SAR(10g) = 2.34 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 63.9%

Maximum value of SAR (measured) = 20.2 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Reference Value = 65.08 V/m; Power Drift = -0.07 dB

Peak SAR (extrapolated) = 35.3 W/kg

SAR(1g) = 8.12 W/kg; SAR(10g) = 2.3 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 62.5%

Maximum value of SAR (measured) = 19.1 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Reference Value = 62.13 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 34.8 W/kg

SAR(1g) = 7.71 W/kg; SAR(10g) = 2.16 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 61.6%

Maximum value of SAR (measured) = 18.7 W/kg

Certificate No: Z22-60187 Page 10 of 10

In Collaboration with
T T L
CALIBRATION LABORATORY

ADD: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62302117
E-mail: csl@ttsl.com.cn http://www.ttsl.com.cn

Impedance Measurement Plot for Head TSL

Certificate No: Z22-60187 Page 10 of 10



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us by telephone: (86-755) 8307 1443, or email: CN_Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)67355888 (86-512)67370818 www.sgs.com.cn
(86-512)67355888 (86-512)67370818 sgs.china@sgs.com

2 DAE4 - SN 1245

<p>Speag</p> <p>Schmid & Partner Engineering AG Zugzwangstrasse 43, 8004 Zurich, Switzerland Phone +41 (0) 43 930, Fax +41 (0) 43 973, info@speag.ch</p> <p>IMPORTANT NOTICE</p> <p>USAGE OF THE DAE4</p> <p>The DAE unit is a delicate, high precision instrument and requires careful treatment by the user. There are no serviceable parts inside the DAE. Special attention shall be given to the following points:</p> <p>Battery Exchange: The battery cover of the DAE4 unit is fixed using a screw, over tightening the screw may cause the threads inside the DAE to wear out.</p> <p>Shipping of the DAE: Before shipping the DAE to SPEAG for calibration, remove the batteries and pack the DAE in an anti-static bag. This anti-static bag shall then be packed into a larger box or container which protects the DAE from impacts during transportation. The package shall be marked to indicate that a fragile instrument is inside.</p> <p>E-Stop Failures: Touch detection may be malfunctioning due to broken magnets in the E-stop. Rough handling of the E-stop may lead to damage of these magnets. Touch and collision errors are often caused by dust and dirt accumulated in the E-stop. To prevent E-stop failure, the customer should always mount the probe to the DAE carefully and keep the DAE unit in a non-dusty environment if not used for measurements.</p> <p>Repair: Minor repairs are performed at no extra cost during the annual calibration. However, SPEAG reserves the right to charge for any repair especially if rough professional handling caused the defect.</p> <p>DASY Configuration Files: Since the exact values of the DAE input resistances, as measured during the calibration procedure of a DAE unit, are not used by the DASY software, a nominal value of 500 MOhm is given in the corresponding configuration file.</p> <p>Important Note: Warranty and calibration is void if the DAE unit is disassembled partly or fully by the Customer.</p> <p>Important Note: Never attempt to grease or oil the E-stop assembly. Cleaning and readjusting of the E-stop assembly is allowed by certified SPEAG personnel only and is part of the annual calibration procedure.</p> <p>Important Note: To prevent damage of the DAE probe connector pins, use great care when installing the probe to the DAE. Carefully connect the probe with the connector notch oriented in the mating position. Avoid any rotational movement of the probe body versus the DAE while turning the locking nut of the connector. The same care shall be used when disconnecting the probe from the DAE.</p> <p>TN_EH100306AE_DAE4.docx 07.03.2019</p>	<p>Calibration Laboratory of Schmid & Partner Engineering AG Zugzwangstrasse 43, 8004 Zurich, Switzerland</p> <p>Schweizerischer Kalibrierdienst C Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Accreditation No.: SCS 0108</p> <p>Client: SGS-CN (Auden) Certificate No.: DAE4-1245_May22</p> <p>CALIBRATION CERTIFICATE</p> <p>Object: DAE4 - SD 000 D04 BM - SN: 1245</p> <p>Calibration procedure(s): QA CAL-06 v30 Calibration procedure for the data acquisition electronics (DAE)</p> <p>Calibration date: May 30, 2022</p> <p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurement (SI). The measurement and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility, environment temperature (22 ± 1)°C and humidity < 70%.</p> <p>Calibration Equipment used (MATE critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Due Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Kelvin Multimeter Type 2001</td> <td>SN: SE10276</td> <td>31-Aug-21 (No:31368)</td> <td>Aug-22</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Check Date (in hours)</th> <th>Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>Auto DAE Calibration Unit</td> <td>SE LMS 05A AA 1001</td> <td>24-Jan-22 (in house check)</td> <td>In house check Jan-22</td> </tr> <tr> <td>Calibration box V3</td> <td>SE LMS 006 AA 1002</td> <td>24-Jan-22 (in house check)</td> <td>In house check Jan-22</td> </tr> </tbody> </table> <p>Calibrated by: Dominique Sailer (Name) / Laboratory Technician (Function) / <i>[Signature]</i> (Signature)</p> <p>Approved by: Steen Kuhn (Name) / Technical Manager (Function) / <i>[Signature]</i> (Signature)</p> <p>Issued: May 30, 2022</p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> <p>Certificate No: DAE4-1245_May22 Page 1 of 5</p>	Primary Standards	ID #	Due Date (Certificate No.)	Scheduled Calibration	Kelvin Multimeter Type 2001	SN: SE10276	31-Aug-21 (No:31368)	Aug-22	Secondary Standards	ID #	Check Date (in hours)	Scheduled Check	Auto DAE Calibration Unit	SE LMS 05A AA 1001	24-Jan-22 (in house check)	In house check Jan-22	Calibration box V3	SE LMS 006 AA 1002	24-Jan-22 (in house check)	In house check Jan-22
Primary Standards	ID #	Due Date (Certificate No.)	Scheduled Calibration																		
Kelvin Multimeter Type 2001	SN: SE10276	31-Aug-21 (No:31368)	Aug-22																		
Secondary Standards	ID #	Check Date (in hours)	Scheduled Check																		
Auto DAE Calibration Unit	SE LMS 05A AA 1001	24-Jan-22 (in house check)	In house check Jan-22																		
Calibration box V3	SE LMS 006 AA 1002	24-Jan-22 (in house check)	In house check Jan-22																		
<p>Calibration Laboratory of Schmid & Partner Engineering AG Zugzwangstrasse 43, 8004 Zurich, Switzerland</p> <p>Schweizerischer Kalibrierdienst C Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Accreditation No.: SCS 0108</p> <p>Glossary</p> <p>DAE: data acquisition electronics Connector angle: information used in DASY system to align probe sensor X to the robot coordinate system.</p> <p>Methods Applied and Interpretation of Parameters</p> <ul style="list-style-type: none"> DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range. Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required. The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty. <ul style="list-style-type: none"> DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement. Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement. Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage. AD Converter Values with inputs stored: Values on the internal AD converter corresponding to zero input voltage. Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements. Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance. Input resistance: Typical value for information; DAE input resistance at the connector, during internal auto-zeroing and during measurement. Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated. Power consumption: Typical value for information. Supply currents in various operating modes. <p>Certificate No: DAE4-1245_May22 Page 2 of 5</p>	<p>DC Voltage Measurement</p> <p>AD - Converter Resolution nominal High Range: 1LSB = 6 mV, full range = -100...+320 mV Low Range: 1LSB = 61 mV, full range = -1...+3mV DASY measurement parameters: Auto Zero-Time: 3 sec; Measuring time: 3 sec</p> <table border="1"> <thead> <tr> <th>Calibration Factors</th> <th>X</th> <th>Y</th> <th>Z</th> </tr> </thead> <tbody> <tr> <td>High Range</td> <td>405.265 ± 0.02% (k=2)</td> <td>403.974 ± 0.02% (k=2)</td> <td>406.092 ± 0.02% (k=2)</td> </tr> <tr> <td>Low Range</td> <td>3.99534 ± 1.50% (k=2)</td> <td>3.99508 ± 1.50% (k=2)</td> <td>4.01015 ± 1.50% (k=2)</td> </tr> </tbody> </table> <p>Connector Angle</p> <table border="1"> <thead> <tr> <th>Connector Angle to be used in DASY system</th> <th>30.0° ± 1°</th> </tr> </thead> </table> <p>Certificate No: DAE4-1245_May22 Page 3 of 5</p>	Calibration Factors	X	Y	Z	High Range	405.265 ± 0.02% (k=2)	403.974 ± 0.02% (k=2)	406.092 ± 0.02% (k=2)	Low Range	3.99534 ± 1.50% (k=2)	3.99508 ± 1.50% (k=2)	4.01015 ± 1.50% (k=2)	Connector Angle to be used in DASY system	30.0° ± 1°						
Calibration Factors	X	Y	Z																		
High Range	405.265 ± 0.02% (k=2)	403.974 ± 0.02% (k=2)	406.092 ± 0.02% (k=2)																		
Low Range	3.99534 ± 1.50% (k=2)	3.99508 ± 1.50% (k=2)	4.01015 ± 1.50% (k=2)																		
Connector Angle to be used in DASY system	30.0° ± 1°																				



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us by telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgs.com.cn
(86-512)57355888 (86-512)57370818 sgs.china@sgs.com

Appendix (Additional assessments outside the scope of SCS0108)

1. DC Voltage Linearity

High Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	19994.45	1.52	0.00
Channel X + Input	20004.58	2.22	0.01
Channel X - Input	-20000.14	1.12	-0.01
Channel Y + Input	19994.72	1.58	0.00
Channel Y + Input	20001.22	-1.00	-0.00
Channel Y - Input	-20003.05	-1.57	0.01
Channel Z + Input	19992.84	0.19	0.00
Channel Z + Input	20003.09	0.58	0.00
Channel Z - Input	-20001.73	-0.27	0.00

Low Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	2001.91	0.41	0.02
Channel X + Input	202.54	0.65	0.32
Channel X - Input	-197.86	0.07	-0.04
Channel Y + Input	2002.05	0.58	0.03
Channel Y + Input	201.27	-0.57	-0.28
Channel Y - Input	-199.23	-0.06	0.03
Channel Z + Input	2001.98	0.08	0.00
Channel Z + Input	200.09	-1.53	-0.76
Channel Z - Input	-199.89	-1.57	0.79

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Common mode Input Voltage (mV)	High Range Average Reading (µV)	Low Range Average Reading (µV)
Channel X	-3.87	-7.69
-200	9.12	7.79
Channel Y	-8.68	-9.28
-200	8.52	6.36
Channel Z	-5.36	-5.80
-200	3.58	3.08

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input Voltage (mV)	Channel X (µV)	Channel Y (µV)	Channel Z (µV)	
Channel X	200	-	4.07	-3.14
Channel Y	200	9.36	-	4.27
Channel Z	200	10.11	7.14	-

Certificate No: DAE4-1245_May22 Page 4 of 5

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15984	17040
Channel Y	16562	16768
Channel Z	16035	15668

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10MΩ	Average (µV)	min. Offset (µV)	max. Offset (µV)	Std. Deviation (µV)
Channel X	1.00	-0.15	1.93	0.45
Channel Y	-0.18	-1.28	0.94	0.45
Channel Z	-0.58	-2.61	0.58	0.60

6. Input Offset Current

Nominal input circuitry offset current on all channels: $-25nA$

7. Input Resistance (Typical values for information)

	Zeroing (ΩOhm)	Measuring (MΩhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+8	+14
Supply (- Vcc)	-0.01	-8	-9

Certificate No: DAE4-1245_May22 Page 5 of 5

3 EX3DV4 - SN 7346

Calibration Laboratory of Schmid & Partner Engineering AG
Zugstrasse 6, 8048 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is a member of the EA Multilateral Agreement for the recognition of calibration certificates

Client: **Auden** Certificate No: **EX3-7346_Mar22**

CALIBRATION CERTIFICATE

Object: **EX3DV4 - SN 7346**

Customer equipment: **QA CAL-01 v9; QA CAL-14 v6; QA CAL-23 v5; QA CAL-25 v7**
Calibration procedure for domestic E-field probes

Calibration date: **March 30, 2022**

This calibration certificate documents the laboratory's national standards, which realize the physical units of measurement (SI). The measurement and the uncertainties with confidence probability are given on the following pages and are part of this certificate.

All calibrations have been conducted in the above laboratory facility: environment temperature (22 ± 0.1°C and humidity = 70%).

Calibration Equipment used (MKT) (suitable for calibration):

Primary Standards	SI	Cal Date (Certificate No.)	Scheduled Calibration
Power meter MPP	SR 10079	09-Apr-21 (No. 211-0201-0302)	Apr-22
Power source MPP-29	SR 10324	09-Apr-21 (No. 211-0201-0301)	Apr-22
Power source MPP-291	SR 10324	09-Apr-21 (No. 211-0202)	Apr-22
Reference 200 mV generator	SR 02282 (200)	09-Apr-21 (No. 211-0204)	Apr-22
DASY	SR 460	13-Dec-21 (No. 048-460-3401)	Dec-22
Reference Probe ESD02	SR 393	07-Dec-21 (No. 033-393-0621)	Dec-22

Secondary Standards

SI	Check Date (in house)	Scheduled Date	
Power source E412B	SR 024126704	09-Apr-21 (in house check Jan-22)	in house check Jan-22
Power source E412A	SR 1Y4149487	05-Apr-21 (in house check Jan-22)	in house check Jan-22
Power source E412A	SR 00310161	05-Apr-21 (in house check Jan-22)	in house check Jan-22
RF generator HP 8447A	SR 0549431700	04-Apr-21 (in house check Jan-22)	in house check Jan-22
Network Analyzer B 8700A	SR 154190477	01-Mar-14 (in house check Dec-20)	in house check Dec-20

Calibrated by: **Steven Koller** Function: **Laboratory Technician** Signature: *[Signature]*

Approved by: **Steven Koller** Function: **Laboratory Manager** Signature: *[Signature]*

This calibration certificate shall not be reproduced, copied or in any way used without written approval of the laboratory.

Certificate No: EX3-7346_Mar22 Page 1 of 14

Calibration Laboratory of Schmid & Partner Engineering AG
Zugstrasse 6, 8048 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is a member of the EA Multilateral Agreement for the recognition of calibration certificates

Client: **Auden** Certificate No: **EX3-7346_Mar22**

CALIBRATION CERTIFICATE

Object: **EX3DV4 - SN 7346**

Customer equipment: **QA CAL-01 v9; QA CAL-14 v6; QA CAL-23 v5; QA CAL-25 v7**
Calibration procedure for domestic E-field probes

Calibration date: **March 30, 2022**

This calibration certificate documents the laboratory's national standards, which realize the physical units of measurement (SI). The measurement and the uncertainties with confidence probability are given on the following pages and are part of this certificate.

All calibrations have been conducted in the above laboratory facility: environment temperature (22 ± 0.1°C and humidity = 70%).

Calibration Equipment used (MKT) (suitable for calibration):

Primary Standards	SI	Cal Date (Certificate No.)	Scheduled Calibration
Power meter MPP	SR 10079	09-Apr-21 (No. 211-0201-0302)	Apr-22
Power source MPP-29	SR 10324	09-Apr-21 (No. 211-0201-0301)	Apr-22
Power source MPP-291	SR 10324	09-Apr-21 (No. 211-0202)	Apr-22
Reference 200 mV generator	SR 02282 (200)	09-Apr-21 (No. 211-0204)	Apr-22
DASY	SR 460	13-Dec-21 (No. 048-460-3401)	Dec-22
Reference Probe ESD02	SR 393	07-Dec-21 (No. 033-393-0621)	Dec-22

Secondary Standards

SI	Check Date (in house)	Scheduled Date	
Power source E412B	SR 024126704	09-Apr-21 (in house check Jan-22)	in house check Jan-22
Power source E412A	SR 1Y4149487	05-Apr-21 (in house check Jan-22)	in house check Jan-22
Power source E412A	SR 00310161	05-Apr-21 (in house check Jan-22)	in house check Jan-22
RF generator HP 8447A	SR 0549431700	04-Apr-21 (in house check Jan-22)	in house check Jan-22
Network Analyzer B 8700A	SR 154190477	01-Mar-14 (in house check Dec-20)	in house check Dec-20

Calibrated by: **Steven Koller** Function: **Laboratory Technician** Signature: *[Signature]*

Approved by: **Steven Koller** Function: **Laboratory Manager** Signature: *[Signature]*

This calibration certificate shall not be reproduced, copied or in any way used without written approval of the laboratory.

Certificate No: EX3-7346_Mar22 Page 1 of 14

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgsgroup.com.cn
(86-512)57355888 (86-512)57370818 sgs.china@sgs.com


<p>EX3DV4 - SN:7346 March 30, 2022</p> <p>DASY/EASY - Parameters of Probe: EX3DV4 - SN:7346</p> <p>Basic Calibration Parameters</p> <table border="1"> <thead> <tr> <th>Parameter</th> <th>Series X</th> <th>Series Y</th> <th>Series Z</th> <th>Unc. (k=2)</th> </tr> </thead> <tbody> <tr> <td>Norm. $\Delta V(V/mV)^2$</td> <td>0.45</td> <td>0.47</td> <td>0.61</td> <td>± 10.1%</td> </tr> <tr> <td>DCP (mV/V)</td> <td>101.4</td> <td>106.0</td> <td>108.9</td> <td></td> </tr> </tbody> </table> <p>Calibration Results for Modulation Response</p> <table border="1"> <thead> <tr> <th>UID</th> <th>Communication System Name</th> <th>dB</th> <th>dB</th> <th>dB</th> <th>dB</th> <th>dB</th> <th>dB</th> <th>Max. Unc. (k=2)</th> </tr> </thead> <tbody> <tr> <td>T005</td> <td>Fluke Waveform (200Hz, 10%)</td> <td>X</td> <td>0.00</td> <td>0.00</td> <td>1.00</td> <td>0.00</td> <td>143.9</td> <td>± 0.0%</td> </tr> <tr> <td>AAA</td> <td></td> <td>Y</td> <td>0.00</td> <td>0.00</td> <td>1.00</td> <td>0.00</td> <td>199.3</td> <td></td> </tr> <tr> <td></td> <td></td> <td>Z</td> <td>0.00</td> <td>0.00</td> <td>1.00</td> <td>0.00</td> <td>143.9</td> <td></td> </tr> <tr> <td>T005</td> <td>Fluke Waveform (200Hz, 10%)</td> <td>X</td> <td>3.33</td> <td>68.99</td> <td>11.08</td> <td>10.00</td> <td>86.0</td> <td>± 8.8%</td> </tr> <tr> <td>AAA</td> <td></td> <td>Y</td> <td>4.03</td> <td>79.70</td> <td>12.35</td> <td></td> <td>66.0</td> <td></td> </tr> <tr> <td></td> <td></td> <td>Z</td> <td>1.63</td> <td>64.25</td> <td>6.76</td> <td></td> <td>62.0</td> <td></td> </tr> <tr> <td>T005</td> <td>Fluke Waveform (200Hz, 20%)</td> <td>X</td> <td>3.00</td> <td>79.65</td> <td>11.31</td> <td>6.89</td> <td>80.0</td> <td>± 2.4%</td> </tr> <tr> <td>AAA</td> <td></td> <td>Y</td> <td>11.31</td> <td>81.32</td> <td>18.72</td> <td></td> <td>88.0</td> <td></td> </tr> <tr> <td></td> <td></td> <td>Z</td> <td>3.83</td> <td>69.90</td> <td>5.11</td> <td></td> <td>85.0</td> <td></td> </tr> <tr> <td>T005</td> <td>Fluke Waveform (200Hz, 40%)</td> <td>X</td> <td>7.41</td> <td>79.85</td> <td>12.61</td> <td>3.88</td> <td>95.0</td> <td>± 2.7%</td> </tr> <tr> <td>AAA</td> <td></td> <td>Y</td> <td>26.90</td> <td>81.62</td> <td>18.51</td> <td></td> <td>95.0</td> <td></td> </tr> <tr> <td></td> <td></td> <td>Z</td> <td>0.18</td> <td>138.39</td> <td>0.01</td> <td></td> <td>95.0</td> <td></td> </tr> <tr> <td>T005</td> <td>Fluke Waveform (200Hz, 80%)</td> <td>X</td> <td>2.72</td> <td>75.13</td> <td>9.50</td> <td>2.22</td> <td>126.9</td> <td>± 1.1%</td> </tr> <tr> <td>AAA</td> <td></td> <td>Y</td> <td>20.90</td> <td>81.58</td> <td>16.29</td> <td></td> <td>120.0</td> <td></td> </tr> <tr> <td></td> <td></td> <td>Z</td> <td>1.94</td> <td>126.51</td> <td>16.87</td> <td></td> <td>120.0</td> <td></td> </tr> <tr> <td>T005</td> <td>QPRK Waveform 1 MHz</td> <td>X</td> <td>1.47</td> <td>84.88</td> <td>13.82</td> <td>1.00</td> <td>150.0</td> <td>± 4.2%</td> </tr> <tr> <td>AAA</td> <td></td> <td>Y</td> <td>1.56</td> <td>68.27</td> <td>14.65</td> <td>0.00</td> <td>150.0</td> <td></td> </tr> <tr> <td></td> <td></td> <td>Z</td> <td>3.45</td> <td>61.88</td> <td>13.05</td> <td></td> <td>150.0</td> <td></td> </tr> <tr> <td>T005</td> <td>QPRK Waveform 10 MHz</td> <td>X</td> <td>2.08</td> <td>67.33</td> <td>13.38</td> <td></td> <td>150.0</td> <td>± 1.1%</td> </tr> <tr> <td>AAA</td> <td></td> <td>Y</td> <td>1.56</td> <td>68.27</td> <td>14.65</td> <td></td> <td>150.0</td> <td></td> </tr> <tr> <td></td> <td></td> <td>Z</td> <td>2.63</td> <td>68.51</td> <td>13.26</td> <td>0.01</td> <td>150.0</td> <td></td> </tr> <tr> <td>T005</td> <td>64-QAM Waveform, 500 MHz</td> <td>X</td> <td>2.63</td> <td>68.51</td> <td>13.26</td> <td>0.01</td> <td>150.0</td> <td>± 1.5%</td> </tr> <tr> <td>AAA</td> <td></td> <td>Y</td> <td>2.63</td> <td>68.51</td> <td>13.26</td> <td></td> <td>150.0</td> <td></td> </tr> <tr> <td></td> <td></td> <td>Z</td> <td>1.70</td> <td>64.72</td> <td>15.99</td> <td></td> <td>150.0</td> <td></td> </tr> <tr> <td>T005</td> <td>64-QAM Waveform, 40 Mhz</td> <td>X</td> <td>1.38</td> <td>66.82</td> <td>15.05</td> <td>0.00</td> <td>150.0</td> <td>± 0.8%</td> </tr> <tr> <td>AAA</td> <td></td> <td>Y</td> <td>1.38</td> <td>66.82</td> <td>15.05</td> <td></td> <td>150.0</td> <td></td> </tr> <tr> <td></td> <td></td> <td>Z</td> <td>2.70</td> <td>66.72</td> <td>14.74</td> <td></td> <td>150.0</td> <td></td> </tr> <tr> <td>T001</td> <td>WLAN CCK42 64-QAM, 4096Hz</td> <td>X</td> <td>4.71</td> <td>65.35</td> <td>12.77</td> <td>0.00</td> <td>150.0</td> <td>± 3.0%</td> </tr> <tr> <td>AAA</td> <td></td> <td>Y</td> <td>4.70</td> <td>65.54</td> <td>13.41</td> <td></td> <td>150.0</td> <td></td> </tr> <tr> <td></td> <td></td> <td>Z</td> <td>3.63</td> <td>66.16</td> <td>15.26</td> <td></td> <td>150.0</td> <td></td> </tr> </tbody> </table> <p>Note: For details on UID parameters see Appendix.</p> <p>The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p> <p>1) The uncertainties of Norm. ΔV do not affect the E field uncertainty within 10% (see Page 21 of 24).</p> <p>2) Numerical simulation parameter uncertainty not required.</p> <p>3) Uncertainty is determined using the most conservative (largest) possible response (indicated in the table) and is determined to the lowest of the listed values.</p> <p>Certificate No: EX3-7346_Mar22 Page 3 of 34</p>	Parameter	Series X	Series Y	Series Z	Unc. (k=2)	Norm. $\Delta V(V/mV)^2$	0.45	0.47	0.61	± 10.1%	DCP (mV/V)	101.4	106.0	108.9		UID	Communication System Name	dB	dB	dB	dB	dB	dB	Max. Unc. (k=2)	T005	Fluke Waveform (200Hz, 10%)	X	0.00	0.00	1.00	0.00	143.9	± 0.0%	AAA		Y	0.00	0.00	1.00	0.00	199.3				Z	0.00	0.00	1.00	0.00	143.9		T005	Fluke Waveform (200Hz, 10%)	X	3.33	68.99	11.08	10.00	86.0	± 8.8%	AAA		Y	4.03	79.70	12.35		66.0				Z	1.63	64.25	6.76		62.0		T005	Fluke Waveform (200Hz, 20%)	X	3.00	79.65	11.31	6.89	80.0	± 2.4%	AAA		Y	11.31	81.32	18.72		88.0				Z	3.83	69.90	5.11		85.0		T005	Fluke Waveform (200Hz, 40%)	X	7.41	79.85	12.61	3.88	95.0	± 2.7%	AAA		Y	26.90	81.62	18.51		95.0				Z	0.18	138.39	0.01		95.0		T005	Fluke Waveform (200Hz, 80%)	X	2.72	75.13	9.50	2.22	126.9	± 1.1%	AAA		Y	20.90	81.58	16.29		120.0				Z	1.94	126.51	16.87		120.0		T005	QPRK Waveform 1 MHz	X	1.47	84.88	13.82	1.00	150.0	± 4.2%	AAA		Y	1.56	68.27	14.65	0.00	150.0				Z	3.45	61.88	13.05		150.0		T005	QPRK Waveform 10 MHz	X	2.08	67.33	13.38		150.0	± 1.1%	AAA		Y	1.56	68.27	14.65		150.0				Z	2.63	68.51	13.26	0.01	150.0		T005	64-QAM Waveform, 500 MHz	X	2.63	68.51	13.26	0.01	150.0	± 1.5%	AAA		Y	2.63	68.51	13.26		150.0				Z	1.70	64.72	15.99		150.0		T005	64-QAM Waveform, 40 Mhz	X	1.38	66.82	15.05	0.00	150.0	± 0.8%	AAA		Y	1.38	66.82	15.05		150.0				Z	2.70	66.72	14.74		150.0		T001	WLAN CCK42 64-QAM, 4096Hz	X	4.71	65.35	12.77	0.00	150.0	± 3.0%	AAA		Y	4.70	65.54	13.41		150.0				Z	3.63	66.16	15.26		150.0		<p>EX3DV4 - SN:7346 March 30, 2022</p> <p>DASY/EASY - Parameters of Probe: EX3DV4 - SN:7346</p> <p>Sensor Model Parameters</p> <table border="1"> <thead> <tr> <th>CT</th> <th>C2</th> <th>T1</th> <th>T2</th> <th>T3</th> <th>T4</th> <th>T5</th> <th>T6</th> </tr> </thead> <tbody> <tr> <td>X</td> <td>39.2</td> <td>291.80</td> <td>35.10</td> <td>5.63</td> <td>0.03</td> <td>5.02</td> <td>1.42</td> </tr> <tr> <td>Y</td> <td>37.1</td> <td>270.84</td> <td>34.12</td> <td>6.29</td> <td>0.00</td> <td>5.01</td> <td>1.82</td> </tr> <tr> <td>Z</td> <td>9.7</td> <td>69.74</td> <td>33.37</td> <td>4.96</td> <td>0.00</td> <td>4.94</td> <td>0.61</td> </tr> </tbody> </table> <p>Other Probe Parameters</p> <table border="1"> <thead> <tr> <th>Parameter</th> <th>Value</th> </tr> </thead> <tbody> <tr> <td>Sensor Arrangement</td> <td>Triangular</td> </tr> <tr> <td>Connector Angle (°)</td> <td>-166.1</td> </tr> <tr> <td>Mechanical Surface Detection Mode</td> <td>enabled</td> </tr> <tr> <td>Optical Surface Detection Mode</td> <td>disabled</td> </tr> <tr> <td>Probe Overall Length</td> <td>237 mm</td> </tr> <tr> <td>Probe Body Diameter</td> <td>10 mm</td> </tr> <tr> <td>Tip Length</td> <td>9 mm</td> </tr> <tr> <td>Tip Diameter</td> <td>2.5 mm</td> </tr> <tr> <td>Probe Tip to Sensor X Calibration Point</td> <td>1 mm</td> </tr> <tr> <td>Probe Tip to Sensor Y Calibration Point</td> <td>1 mm</td> </tr> <tr> <td>Probe Tip to Sensor Z Calibration Point</td> <td>1 mm</td> </tr> <tr> <td>Recommended Measurement Distance from Surface</td> <td>1.4 mm</td> </tr> </tbody> </table> <p>Note: Measurement distance from surface can be increased to 3-4 mm for an Area Scan job.</p> <p>Certificate No: EX3-7346_Mar22 Page 4 of 34</p>	CT	C2	T1	T2	T3	T4	T5	T6	X	39.2	291.80	35.10	5.63	0.03	5.02	1.42	Y	37.1	270.84	34.12	6.29	0.00	5.01	1.82	Z	9.7	69.74	33.37	4.96	0.00	4.94	0.61	Parameter	Value	Sensor Arrangement	Triangular	Connector Angle (°)	-166.1	Mechanical Surface Detection Mode	enabled	Optical Surface Detection Mode	disabled	Probe Overall Length	237 mm	Probe Body Diameter	10 mm	Tip Length	9 mm	Tip Diameter	2.5 mm	Probe Tip to Sensor X Calibration Point	1 mm	Probe Tip to Sensor Y Calibration Point	1 mm	Probe Tip to Sensor Z Calibration Point	1 mm	Recommended Measurement Distance from Surface	1.4 mm
Parameter	Series X	Series Y	Series Z	Unc. (k=2)																																																																																																																																																																																																																																																																																																																																																													
Norm. $\Delta V(V/mV)^2$	0.45	0.47	0.61	± 10.1%																																																																																																																																																																																																																																																																																																																																																													
DCP (mV/V)	101.4	106.0	108.9																																																																																																																																																																																																																																																																																																																																																														
UID	Communication System Name	dB	dB	dB	dB	dB	dB	Max. Unc. (k=2)																																																																																																																																																																																																																																																																																																																																																									
T005	Fluke Waveform (200Hz, 10%)	X	0.00	0.00	1.00	0.00	143.9	± 0.0%																																																																																																																																																																																																																																																																																																																																																									
AAA		Y	0.00	0.00	1.00	0.00	199.3																																																																																																																																																																																																																																																																																																																																																										
		Z	0.00	0.00	1.00	0.00	143.9																																																																																																																																																																																																																																																																																																																																																										
T005	Fluke Waveform (200Hz, 10%)	X	3.33	68.99	11.08	10.00	86.0	± 8.8%																																																																																																																																																																																																																																																																																																																																																									
AAA		Y	4.03	79.70	12.35		66.0																																																																																																																																																																																																																																																																																																																																																										
		Z	1.63	64.25	6.76		62.0																																																																																																																																																																																																																																																																																																																																																										
T005	Fluke Waveform (200Hz, 20%)	X	3.00	79.65	11.31	6.89	80.0	± 2.4%																																																																																																																																																																																																																																																																																																																																																									
AAA		Y	11.31	81.32	18.72		88.0																																																																																																																																																																																																																																																																																																																																																										
		Z	3.83	69.90	5.11		85.0																																																																																																																																																																																																																																																																																																																																																										
T005	Fluke Waveform (200Hz, 40%)	X	7.41	79.85	12.61	3.88	95.0	± 2.7%																																																																																																																																																																																																																																																																																																																																																									
AAA		Y	26.90	81.62	18.51		95.0																																																																																																																																																																																																																																																																																																																																																										
		Z	0.18	138.39	0.01		95.0																																																																																																																																																																																																																																																																																																																																																										
T005	Fluke Waveform (200Hz, 80%)	X	2.72	75.13	9.50	2.22	126.9	± 1.1%																																																																																																																																																																																																																																																																																																																																																									
AAA		Y	20.90	81.58	16.29		120.0																																																																																																																																																																																																																																																																																																																																																										
		Z	1.94	126.51	16.87		120.0																																																																																																																																																																																																																																																																																																																																																										
T005	QPRK Waveform 1 MHz	X	1.47	84.88	13.82	1.00	150.0	± 4.2%																																																																																																																																																																																																																																																																																																																																																									
AAA		Y	1.56	68.27	14.65	0.00	150.0																																																																																																																																																																																																																																																																																																																																																										
		Z	3.45	61.88	13.05		150.0																																																																																																																																																																																																																																																																																																																																																										
T005	QPRK Waveform 10 MHz	X	2.08	67.33	13.38		150.0	± 1.1%																																																																																																																																																																																																																																																																																																																																																									
AAA		Y	1.56	68.27	14.65		150.0																																																																																																																																																																																																																																																																																																																																																										
		Z	2.63	68.51	13.26	0.01	150.0																																																																																																																																																																																																																																																																																																																																																										
T005	64-QAM Waveform, 500 MHz	X	2.63	68.51	13.26	0.01	150.0	± 1.5%																																																																																																																																																																																																																																																																																																																																																									
AAA		Y	2.63	68.51	13.26		150.0																																																																																																																																																																																																																																																																																																																																																										
		Z	1.70	64.72	15.99		150.0																																																																																																																																																																																																																																																																																																																																																										
T005	64-QAM Waveform, 40 Mhz	X	1.38	66.82	15.05	0.00	150.0	± 0.8%																																																																																																																																																																																																																																																																																																																																																									
AAA		Y	1.38	66.82	15.05		150.0																																																																																																																																																																																																																																																																																																																																																										
		Z	2.70	66.72	14.74		150.0																																																																																																																																																																																																																																																																																																																																																										
T001	WLAN CCK42 64-QAM, 4096Hz	X	4.71	65.35	12.77	0.00	150.0	± 3.0%																																																																																																																																																																																																																																																																																																																																																									
AAA		Y	4.70	65.54	13.41		150.0																																																																																																																																																																																																																																																																																																																																																										
		Z	3.63	66.16	15.26		150.0																																																																																																																																																																																																																																																																																																																																																										
CT	C2	T1	T2	T3	T4	T5	T6																																																																																																																																																																																																																																																																																																																																																										
X	39.2	291.80	35.10	5.63	0.03	5.02	1.42																																																																																																																																																																																																																																																																																																																																																										
Y	37.1	270.84	34.12	6.29	0.00	5.01	1.82																																																																																																																																																																																																																																																																																																																																																										
Z	9.7	69.74	33.37	4.96	0.00	4.94	0.61																																																																																																																																																																																																																																																																																																																																																										
Parameter	Value																																																																																																																																																																																																																																																																																																																																																																
Sensor Arrangement	Triangular																																																																																																																																																																																																																																																																																																																																																																
Connector Angle (°)	-166.1																																																																																																																																																																																																																																																																																																																																																																
Mechanical Surface Detection Mode	enabled																																																																																																																																																																																																																																																																																																																																																																
Optical Surface Detection Mode	disabled																																																																																																																																																																																																																																																																																																																																																																
Probe Overall Length	237 mm																																																																																																																																																																																																																																																																																																																																																																
Probe Body Diameter	10 mm																																																																																																																																																																																																																																																																																																																																																																
Tip Length	9 mm																																																																																																																																																																																																																																																																																																																																																																
Tip Diameter	2.5 mm																																																																																																																																																																																																																																																																																																																																																																
Probe Tip to Sensor X Calibration Point	1 mm																																																																																																																																																																																																																																																																																																																																																																
Probe Tip to Sensor Y Calibration Point	1 mm																																																																																																																																																																																																																																																																																																																																																																
Probe Tip to Sensor Z Calibration Point	1 mm																																																																																																																																																																																																																																																																																																																																																																
Recommended Measurement Distance from Surface	1.4 mm																																																																																																																																																																																																																																																																																																																																																																
<p>EX3DV4 - SN:7346 March 30, 2022</p> <p>DASY/EASY - Parameters of Probe: EX3DV4 - SN:7346</p> <p>Calibration Parameter Determined in Head Tissue Simulating Media</p> <table border="1"> <thead> <tr> <th>f (MHz)</th> <th>Relative Permittivity¹</th> <th>Conductivity (S/m)¹</th> <th>Const X</th> <th>Const Y</th> <th>Const Z</th> <th>Alpha²</th> <th>Depth³ (mm)</th> <th>Unc. (k=2)</th> </tr> </thead> <tbody> <tr> <td>750</td> <td>41.9</td> <td>0.69</td> <td>10.56</td> <td>10.56</td> <td>10.56</td> <td>0.55</td> <td>0.85</td> <td>± 12.0%</td> </tr> <tr> <td>835</td> <td>41.5</td> <td>0.90</td> <td>10.12</td> <td>10.12</td> <td>10.12</td> <td>0.42</td> <td>0.96</td> <td>± 12.0%</td> </tr> <tr> <td>900</td> <td>41.5</td> <td>0.97</td> <td>10.10</td> <td>10.10</td> <td>10.10</td> <td>0.53</td> <td>0.80</td> <td>± 12.0%</td> </tr> <tr> <td>1450</td> <td>40.5</td> <td>1.20</td> <td>9.26</td> <td>9.26</td> <td>9.26</td> <td>0.50</td> <td>0.80</td> <td>± 12.0%</td> </tr> <tr> <td>1750</td> <td>40.1</td> <td>1.37</td> <td>8.83</td> <td>8.83</td> <td>8.83</td> <td>0.34</td> <td>0.86</td> <td>± 12.0%</td> </tr> <tr> <td>1900</td> <td>40.0</td> <td>1.40</td> <td>8.48</td> <td>8.48</td> <td>8.48</td> <td>0.35</td> <td>0.95</td> <td>± 12.0%</td> </tr> <tr> <td>2000</td> <td>40.0</td> <td>1.40</td> <td>8.35</td> <td>8.35</td> <td>8.35</td> <td>0.34</td> <td>0.88</td> <td>± 12.0%</td> </tr> <tr> <td>2300</td> <td>39.5</td> <td>1.67</td> <td>7.86</td> <td>7.86</td> <td>7.86</td> <td>0.39</td> <td>0.90</td> <td>± 12.0%</td> </tr> <tr> <td>2450</td> <td>39.2</td> <td>1.80</td> <td>7.63</td> <td>7.63</td> <td>7.63</td> <td>0.41</td> <td>0.90</td> <td>± 12.0%</td> </tr> <tr> <td>2600</td> <td>39.0</td> <td>1.96</td> <td>7.33</td> <td>7.33</td> <td>7.33</td> <td>0.44</td> <td>0.90</td> <td>± 12.0%</td> </tr> <tr> <td>3300</td> <td>38.2</td> <td>2.71</td> <td>7.15</td> <td>7.15</td> <td>7.15</td> <td>0.30</td> <td>1.35</td> <td>± 13.1%</td> </tr> <tr> <td>3500</td> <td>37.9</td> <td>2.91</td> <td>7.14</td> <td>7.14</td> <td>7.14</td> <td>0.30</td> <td>1.35</td> <td>± 13.1%</td> </tr> <tr> <td>3700</td> <td>37.7</td> <td>3.12</td> <td>6.85</td> <td>6.85</td> <td>6.85</td> <td>0.30</td> <td>1.35</td> <td>± 13.1%</td> </tr> <tr> <td>3900</td> <td>37.5</td> <td>3.32</td> <td>6.71</td> <td>6.71</td> <td>6.71</td> <td>0.40</td> <td>1.60</td> <td>± 13.1%</td> </tr> <tr> <td>4100</td> <td>37.2</td> <td>3.53</td> <td>6.58</td> <td>6.58</td> <td>6.58</td> <td>0.40</td> <td>1.60</td> <td>± 13.1%</td> </tr> <tr> <td>4200</td> <td>37.1</td> <td>3.63</td> <td>6.30</td> <td>6.30</td> <td>6.30</td> <td>0.40</td> <td>1.70</td> <td>± 13.1%</td> </tr> <tr> <td>4400</td> <td>36.9</td> <td>3.84</td> <td>6.24</td> <td>6.24</td> <td>6.24</td> <td>0.40</td> <td>1.70</td> <td>± 13.1%</td> </tr> <tr> <td>4600</td> <td>36.7</td> <td>4.04</td> <td>6.11</td> <td>6.11</td> <td>6.11</td> <td>0.40</td> <td>1.70</td> <td>± 13.1%</td> </tr> <tr> <td>4800</td> <td>36.4</td> <td>4.25</td> <td>6.08</td> <td>6.08</td> <td>6.08</td> <td>0.40</td> <td>1.80</td> <td>± 13.1%</td> </tr> <tr> <td>4900</td> <td>36.3</td> <td>4.40</td> <td>5.84</td> <td>5.84</td> <td>5.84</td> <td>0.40</td> <td>1.80</td> <td>± 13.1%</td> </tr> <tr> <td>5200</td> <td>36.0</td> <td>4.66</td> <td>5.25</td> <td>5.25</td> <td>5.25</td> <td>0.40</td> <td>1.80</td> <td>± 13.1%</td> </tr> <tr> <td>5300</td> <td>35.9</td> <td>4.78</td> <td>5.12</td> <td>5.12</td> <td>5.12</td> <td>0.40</td> <td>1.80</td> <td>± 13.1%</td> </tr> <tr> <td>5500</td> <td>35.6</td> <td>4.98</td> <td>4.85</td> <td>4.85</td> <td>4.85</td> <td>0.40</td> <td>1.80</td> <td>± 13.1%</td> </tr> <tr> <td>5800</td> <td>35.5</td> <td>5.07</td> <td>4.70</td> <td>4.70</td> <td>4.70</td> <td>0.40</td> <td>1.80</td> <td>± 13.1%</td> </tr> <tr> <td>5900</td> <td>35.3</td> <td>5.27</td> <td>4.75</td> <td>4.75</td> <td>4.75</td> <td>0.40</td> <td>1.80</td> <td>± 13.1%</td> </tr> </tbody> </table> <p>1) Frequency validity above 300 MHz and ≤ 100 MHz only applies for DASY v4.4 and higher (see Page 21, slide 4) is restricted to ≤ 50 MHz. The uncertainty is the RSS of the Const uncertainty at calibration frequency and the uncertainty for the measured frequency validity. Frequency validity below 300 MHz is 10, 25, 40, 60 and 70 MHz for Const assessments at 30, 64, 128, 192 and 250 MHz respectively. Validity of Const assessed at 9 MHz and 9 MHz and Const assessed at 10 MHz is 10 MHz and 9 MHz frequency validity can be extended to a 10 MHz.</p> <p>2) All frequencies below 3 GHz, the validity of tissue parameters is, and it can be related to a 10% liquid compensation formula is applied to measured SARA values. All frequencies above 3 GHz, the validity of tissue parameters is, and it is restricted to 10%. The uncertainty is the RSS of the Const uncertainty for indicated target tissue parameters.</p> <p>3) Alpha values are determined during calibration. SRAIC warrants that the remaining deviation due to the boundary effect after compensation is always less than 1% for frequencies below 3 GHz and below $\pm 2\%$ for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.</p> <p>Certificate No: EX3-7346_Mar22 Page 5 of 34</p>	f (MHz)	Relative Permittivity ¹	Conductivity (S/m) ¹	Const X	Const Y	Const Z	Alpha ²	Depth ³ (mm)	Unc. (k=2)	750	41.9	0.69	10.56	10.56	10.56	0.55	0.85	± 12.0%	835	41.5	0.90	10.12	10.12	10.12	0.42	0.96	± 12.0%	900	41.5	0.97	10.10	10.10	10.10	0.53	0.80	± 12.0%	1450	40.5	1.20	9.26	9.26	9.26	0.50	0.80	± 12.0%	1750	40.1	1.37	8.83	8.83	8.83	0.34	0.86	± 12.0%	1900	40.0	1.40	8.48	8.48	8.48	0.35	0.95	± 12.0%	2000	40.0	1.40	8.35	8.35	8.35	0.34	0.88	± 12.0%	2300	39.5	1.67	7.86	7.86	7.86	0.39	0.90	± 12.0%	2450	39.2	1.80	7.63	7.63	7.63	0.41	0.90	± 12.0%	2600	39.0	1.96	7.33	7.33	7.33	0.44	0.90	± 12.0%	3300	38.2	2.71	7.15	7.15	7.15	0.30	1.35	± 13.1%	3500	37.9	2.91	7.14	7.14	7.14	0.30	1.35	± 13.1%	3700	37.7	3.12	6.85	6.85	6.85	0.30	1.35	± 13.1%	3900	37.5	3.32	6.71	6.71	6.71	0.40	1.60	± 13.1%	4100	37.2	3.53	6.58	6.58	6.58	0.40	1.60	± 13.1%	4200	37.1	3.63	6.30	6.30	6.30	0.40	1.70	± 13.1%	4400	36.9	3.84	6.24	6.24	6.24	0.40	1.70	± 13.1%	4600	36.7	4.04	6.11	6.11	6.11	0.40	1.70	± 13.1%	4800	36.4	4.25	6.08	6.08	6.08	0.40	1.80	± 13.1%	4900	36.3	4.40	5.84	5.84	5.84	0.40	1.80	± 13.1%	5200	36.0	4.66	5.25	5.25	5.25	0.40	1.80	± 13.1%	5300	35.9	4.78	5.12	5.12	5.12	0.40	1.80	± 13.1%	5500	35.6	4.98	4.85	4.85	4.85	0.40	1.80	± 13.1%	5800	35.5	5.07	4.70	4.70	4.70	0.40	1.80	± 13.1%	5900	35.3	5.27	4.75	4.75	4.75	0.40	1.80	± 13.1%	<p>EX3DV4 - SN:7346 March 30, 2022</p> <p>DASY/EASY - Parameters of Probe: EX3DV4 - SN:7346</p> <p>Calibration Parameter Determined in Head Tissue Simulating Media</p> <table border="1"> <thead> <tr> <th>f (MHz)</th> <th>Relative Permittivity¹</th> <th>Conductivity (S/m)¹</th> <th>Const X</th> <th>Const Y</th> <th>Const Z</th> <th>Alpha²</th> <th>Depth³ (mm)</th> <th>Unc. (k=2)</th> </tr> </thead> <tbody> <tr> <td>6500</td> <td>34.5</td> <td>6.07</td> <td>5.30</td> <td>5.30</td> <td>5.30</td> <td>0.20</td> <td>2.50</td> <td>± 18.0%</td> </tr> </tbody> </table> <p>1) Frequency validity above 6 GHz is ≤ 700 MHz. The uncertainty is the RSS of the Const uncertainty at calibration frequency and the uncertainty for the measured frequency band.</p> <p>2) As frequencies 6-10 GHz, the validity of tissue parameters is, and it can be related to a 10% liquid compensation formula is applied to measured SARA values. The uncertainty is the RSS of the Const uncertainty for indicated target tissue parameters.</p> <p>3) Alpha values are determined during calibration. SRAIC warrants that the remaining deviation due to the boundary effect after compensation is always less than 1% for frequencies below 3 GHz and below $\pm 2\%$ for frequencies between 3-6 GHz and below $\pm 4\%$ for frequencies between 6-10 GHz at any distance larger than half the probe tip diameter from the boundary.</p> <p>Certificate No: EX3-7346_Mar22 Page 6 of 34</p>	f (MHz)	Relative Permittivity ¹	Conductivity (S/m) ¹	Const X	Const Y	Const Z	Alpha ²	Depth ³ (mm)	Unc. (k=2)	6500	34.5	6.07	5.30	5.30	5.30	0.20	2.50	± 18.0%																																																																																																				
f (MHz)	Relative Permittivity ¹	Conductivity (S/m) ¹	Const X	Const Y	Const Z	Alpha ²	Depth ³ (mm)	Unc. (k=2)																																																																																																																																																																																																																																																																																																																																																									
750	41.9	0.69	10.56	10.56	10.56	0.55	0.85	± 12.0%																																																																																																																																																																																																																																																																																																																																																									
835	41.5	0.90	10.12	10.12	10.12	0.42	0.96	± 12.0%																																																																																																																																																																																																																																																																																																																																																									
900	41.5	0.97	10.10	10.10	10.10	0.53	0.80	± 12.0%																																																																																																																																																																																																																																																																																																																																																									
1450	40.5	1.20	9.26	9.26	9.26	0.50	0.80	± 12.0%																																																																																																																																																																																																																																																																																																																																																									
1750	40.1	1.37	8.83	8.83	8.83	0.34	0.86	± 12.0%																																																																																																																																																																																																																																																																																																																																																									
1900	40.0	1.40	8.48	8.48	8.48	0.35	0.95	± 12.0%																																																																																																																																																																																																																																																																																																																																																									
2000	40.0	1.40	8.35	8.35	8.35	0.34	0.88	± 12.0%																																																																																																																																																																																																																																																																																																																																																									
2300	39.5	1.67	7.86	7.86	7.86	0.39	0.90	± 12.0%																																																																																																																																																																																																																																																																																																																																																									
2450	39.2	1.80	7.63	7.63	7.63	0.41	0.90	± 12.0%																																																																																																																																																																																																																																																																																																																																																									
2600	39.0	1.96	7.33	7.33	7.33	0.44	0.90	± 12.0%																																																																																																																																																																																																																																																																																																																																																									
3300	38.2	2.71	7.15	7.15	7.15	0.30	1.35	± 13.1%																																																																																																																																																																																																																																																																																																																																																									
3500	37.9	2.91	7.14	7.14	7.14	0.30	1.35	± 13.1%																																																																																																																																																																																																																																																																																																																																																									
3700	37.7	3.12	6.85	6.85	6.85	0.30	1.35	± 13.1%																																																																																																																																																																																																																																																																																																																																																									
3900	37.5	3.32	6.71	6.71	6.71	0.40	1.60	± 13.1%																																																																																																																																																																																																																																																																																																																																																									
4100	37.2	3.53	6.58	6.58	6.58	0.40	1.60	± 13.1%																																																																																																																																																																																																																																																																																																																																																									
4200	37.1	3.63	6.30	6.30	6.30	0.40	1.70	± 13.1%																																																																																																																																																																																																																																																																																																																																																									
4400	36.9	3.84	6.24	6.24	6.24	0.40	1.70	± 13.1%																																																																																																																																																																																																																																																																																																																																																									
4600	36.7	4.04	6.11	6.11	6.11	0.40	1.70	± 13.1%																																																																																																																																																																																																																																																																																																																																																									
4800	36.4	4.25	6.08	6.08	6.08	0.40	1.80	± 13.1%																																																																																																																																																																																																																																																																																																																																																									
4900	36.3	4.40	5.84	5.84	5.84	0.40	1.80	± 13.1%																																																																																																																																																																																																																																																																																																																																																									
5200	36.0	4.66	5.25	5.25	5.25	0.40	1.80	± 13.1%																																																																																																																																																																																																																																																																																																																																																									
5300	35.9	4.78	5.12	5.12	5.12	0.40	1.80	± 13.1%																																																																																																																																																																																																																																																																																																																																																									
5500	35.6	4.98	4.85	4.85	4.85	0.40	1.80	± 13.1%																																																																																																																																																																																																																																																																																																																																																									
5800	35.5	5.07	4.70	4.70	4.70	0.40	1.80	± 13.1%																																																																																																																																																																																																																																																																																																																																																									
5900	35.3	5.27	4.75	4.75	4.75	0.40	1.80	± 13.1%																																																																																																																																																																																																																																																																																																																																																									
f (MHz)	Relative Permittivity ¹	Conductivity (S/m) ¹	Const X	Const Y	Const Z	Alpha ²	Depth ³ (mm)	Unc. (k=2)																																																																																																																																																																																																																																																																																																																																																									
6500	34.5	6.07	5.30	5.30	5.30	0.20	2.50	± 18.0%																																																																																																																																																																																																																																																																																																																																																									



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300 (86-512)57355888 (86-512)57370818 www.sgsgroup.com.cn
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300 (86-512)57355888 (86-512)57370818 sgs.china@sgs.com

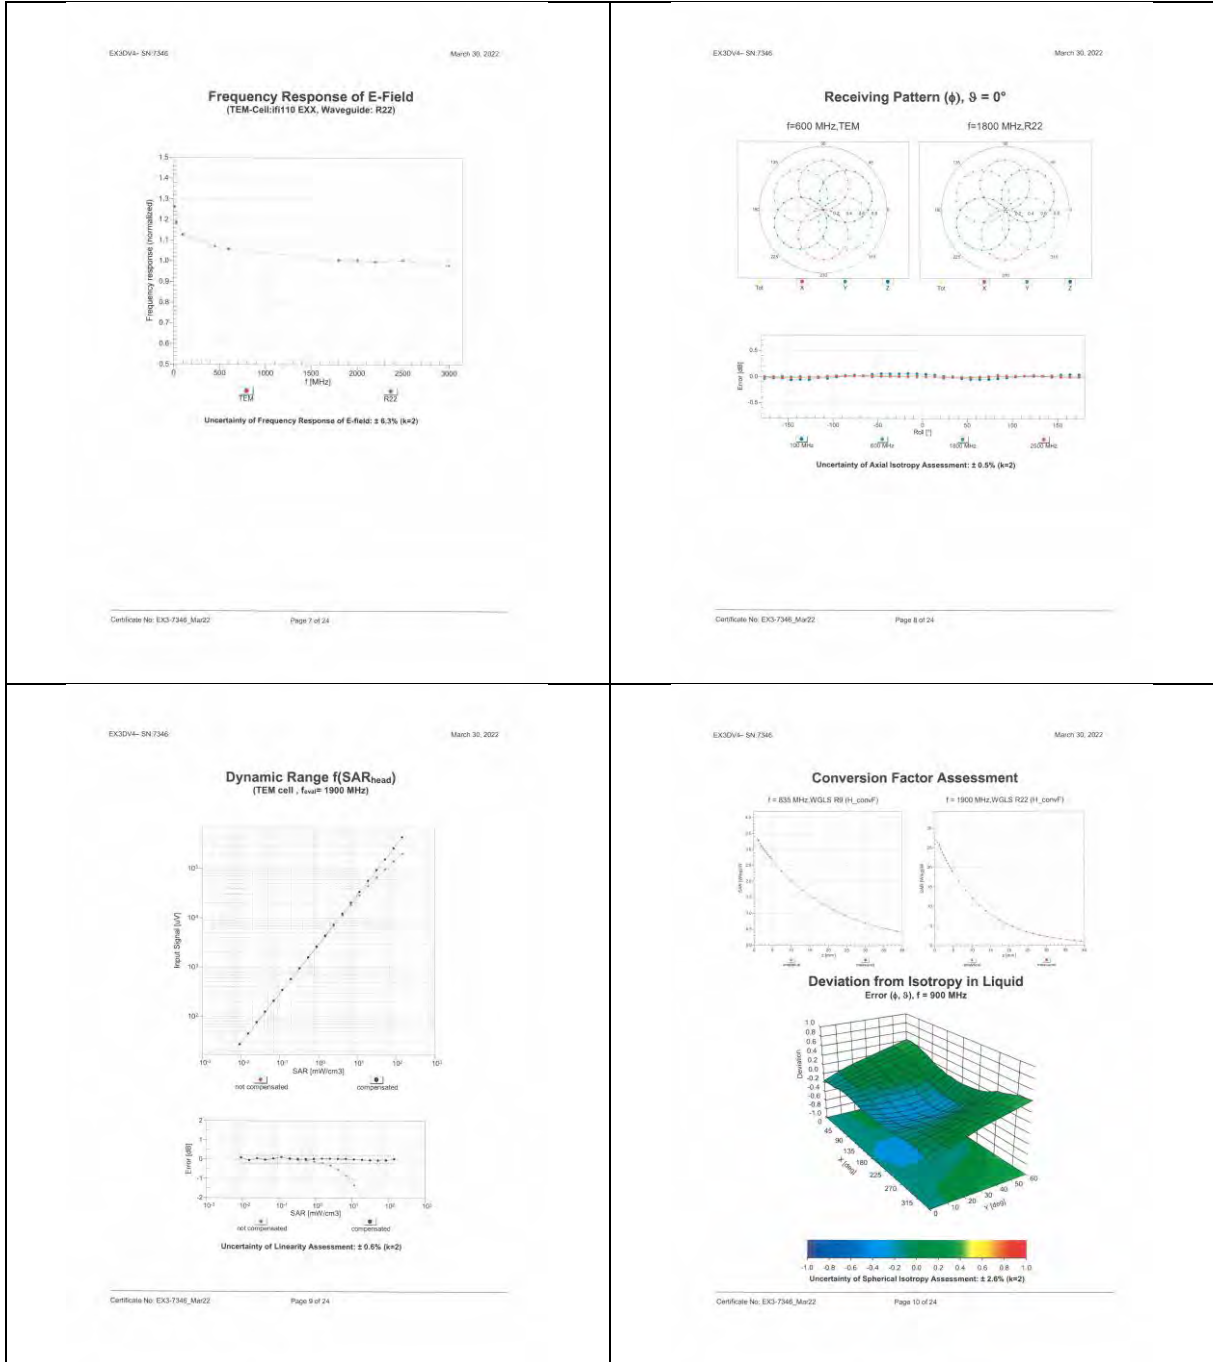

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN_Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300 t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
 中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300 t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com



Table with columns: Appendix: Modulation Calibration Parameters, UID, Rev, Commissioning System Name, Group, PASC (dB), Used (MHz), and a list of various modulation parameters and their values.

Table with columns: E3X7366-SN-7366, March 30, 2022, and a list of various modulation parameters and their values.

Table with columns: E3X7366-SN-7366, March 30, 2022, and a list of various modulation parameters and their values.

Table with columns: E3X7366-SN-7366, March 30, 2022, and a list of various modulation parameters and their values.

Unless otherwise agreed in writing, this document is issued by its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com/en/Terms-and-Conditions... Attention: To check the authenticity of testing/inspection report & certificate, please contact us by telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300 中国·江苏·昆山市留学生在创业园伟业路10号 邮编 215300



Table with columns: Item No., Description, Standard, Result, and Date. Includes items like 10414 AAA, 10415 AAA, etc., under EX3746-SN 7346.

Certificate No. EX3-7346_Mar22 Page 15 of 24

Table with columns: Item No., Description, Standard, Result, and Date. Includes items like 104899 AAF, 104900 AAF, etc., under EX3746-SN 7346.

Certificate No. EX3-7346_Mar22 Page 16 of 24

Table with columns: Item No., Description, Standard, Result, and Date. Includes items like 10547 AAC, 10548 AAC, etc., under EX3746-SN 7346.

Certificate No. EX3-7346_Mar22 Page 17 of 24

Table with columns: Item No., Description, Standard, Result, and Date. Includes items like 10605 AAC, 10606 AAC, etc., under EX3746-SN 7346.

Certificate No. EX3-7346_Mar22 Page 18 of 24



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed on leaf... Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300 (86-512)57355888 (86-512)57370818 www.sgsgrp.com.cn 中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300 (86-512)57355888 (86-512)57370818 sgs.kunshan@sgs.com

EX30V4 - SN 7346				March 30, 2022			
10673	AAC	IEEE 802.11a (20MHz, MCS2, 900-00)	WLAN	8.78	± 0.6 %		
10674	AAC	IEEE 802.11a (20MHz, MCS3, 900-00)	WLAN	8.74	± 0.6 %		
10675	AAC	IEEE 802.11a (20MHz, MCS4, 900-00)	WLAN	8.80	± 0.6 %		
10676	AAC	IEEE 802.11a (20MHz, MCS5, 900-00)	WLAN	8.77	± 0.6 %		
10677	AAC	IEEE 802.11a (20MHz, MCS6, 900-00)	WLAN	8.73	± 0.6 %		
10678	AAC	IEEE 802.11a (20MHz, MCS7, 900-00)	WLAN	8.78	± 0.6 %		
10679	AAC	IEEE 802.11a (20MHz, MCS8, 900-00)	WLAN	8.80	± 0.6 %		
10680	AAC	IEEE 802.11a (20MHz, MCS9, 900-00)	WLAN	8.80	± 0.6 %		
10681	AAC	IEEE 802.11a (20MHz, MCS10, 900-00)	WLAN	8.82	± 0.6 %		
10682	AAC	IEEE 802.11a (20MHz, MCS11, 900-00)	WLAN	8.83	± 0.6 %		
10683	AAC	IEEE 802.11a (20MHz, MCS12, 900-00)	WLAN	8.82	± 0.6 %		
10684	AAC	IEEE 802.11a (20MHz, MCS13, 900-00)	WLAN	8.20	± 0.6 %		
10685	AAC	IEEE 802.11a (20MHz, MCS14, 900-00)	WLAN	8.33	± 0.6 %		
10686	AAC	IEEE 802.11a (20MHz, MCS15, 900-00)	WLAN	8.28	± 0.6 %		
10687	AAC	IEEE 802.11a (20MHz, MCS16, 900-00)	WLAN	8.45	± 0.6 %		
10688	AAC	IEEE 802.11a (20MHz, MCS17, 900-00)	WLAN	8.29	± 0.6 %		
10689	AAC	IEEE 802.11a (20MHz, MCS18, 900-00)	WLAN	8.56	± 0.6 %		
10690	AAC	IEEE 802.11a (20MHz, MCS19, 900-00)	WLAN	8.29	± 0.6 %		
10691	AAC	IEEE 802.11a (20MHz, MCS20, 900-00)	WLAN	8.25	± 0.6 %		
10692	AAC	IEEE 802.11a (20MHz, MCS21, 900-00)	WLAN	8.29	± 0.6 %		
10693	AAC	IEEE 802.11a (20MHz, MCS22, 900-00)	WLAN	8.25	± 0.6 %		
10694	AAC	IEEE 802.11a (20MHz, MCS23, 900-00)	WLAN	8.37	± 0.6 %		
10695	AAC	IEEE 802.11a (40MHz, MCS8, 900-00)	WLAN	8.78	± 0.6 %		
10696	AAC	IEEE 802.11a (40MHz, MCS9, 900-00)	WLAN	8.81	± 0.6 %		
10697	AAC	IEEE 802.11a (40MHz, MCS10, 900-00)	WLAN	8.81	± 0.6 %		
10698	AAC	IEEE 802.11a (40MHz, MCS11, 900-00)	WLAN	8.89	± 0.6 %		
10699	AAC	IEEE 802.11a (40MHz, MCS12, 900-00)	WLAN	8.82	± 0.6 %		
10700	AAC	IEEE 802.11a (40MHz, MCS13, 900-00)	WLAN	8.73	± 0.6 %		
10701	AAC	IEEE 802.11a (40MHz, MCS14, 900-00)	WLAN	8.86	± 0.6 %		
10702	AAC	IEEE 802.11a (40MHz, MCS15, 900-00)	WLAN	8.70	± 0.6 %		
10703	AAC	IEEE 802.11a (40MHz, MCS16, 900-00)	WLAN	8.82	± 0.6 %		
10704	AAC	IEEE 802.11a (40MHz, MCS17, 900-00)	WLAN	8.86	± 0.6 %		
10705	AAC	IEEE 802.11a (40MHz, MCS18, 900-00)	WLAN	8.69	± 0.6 %		
10706	AAC	IEEE 802.11a (40MHz, MCS19, 900-00)	WLAN	8.86	± 0.6 %		
10707	AAC	IEEE 802.11a (40MHz, MCS20, 900-00)	WLAN	8.32	± 0.6 %		
10708	AAC	IEEE 802.11a (40MHz, MCS21, 900-00)	WLAN	8.55	± 0.6 %		
10709	AAC	IEEE 802.11a (40MHz, MCS22, 900-00)	WLAN	8.33	± 0.6 %		
10710	AAC	IEEE 802.11a (40MHz, MCS23, 900-00)	WLAN	8.29	± 0.6 %		
10711	AAC	IEEE 802.11a (40MHz, MCS24, 900-00)	WLAN	8.39	± 0.6 %		
10712	AAC	IEEE 802.11a (40MHz, MCS25, 900-00)	WLAN	8.67	± 0.6 %		
10713	AAC	IEEE 802.11a (40MHz, MCS26, 900-00)	WLAN	8.33	± 0.6 %		
10714	AAC	IEEE 802.11a (40MHz, MCS27, 900-00)	WLAN	8.36	± 0.6 %		
10715	AAC	IEEE 802.11a (40MHz, MCS28, 900-00)	WLAN	8.43	± 0.6 %		
10716	AAC	IEEE 802.11a (40MHz, MCS29, 900-00)	WLAN	8.30	± 0.6 %		
10717	AAC	IEEE 802.11a (40MHz, MCS30, 900-00)	WLAN	8.48	± 0.6 %		
10718	AAC	IEEE 802.11a (40MHz, MCS31, 900-00)	WLAN	8.24	± 0.6 %		
10719	AAC	IEEE 802.11a (40MHz, MCS32, 900-00)	WLAN	8.81	± 0.6 %		
10720	AAC	IEEE 802.11a (80MHz, MCS1, 900-00)	WLAN	8.87	± 0.6 %		
10721	AAC	IEEE 802.11a (80MHz, MCS2, 900-00)	WLAN	8.81	± 0.6 %		
10722	AAC	IEEE 802.11a (80MHz, MCS3, 900-00)	WLAN	8.55	± 0.6 %		
10723	AAC	IEEE 802.11a (80MHz, MCS4, 900-00)	WLAN	8.70	± 0.6 %		
10724	AAC	IEEE 802.11a (80MHz, MCS5, 900-00)	WLAN	8.80	± 0.6 %		
10725	AAC	IEEE 802.11a (80MHz, MCS6, 900-00)	WLAN	8.74	± 0.6 %		
10726	AAC	IEEE 802.11a (80MHz, MCS7, 900-00)	WLAN	8.72	± 0.6 %		
10727	AAC	IEEE 802.11a (80MHz, MCS8, 900-00)	WLAN	8.66	± 0.6 %		
10728	AAC	IEEE 802.11a (80MHz, MCS9, 900-00)	WLAN	8.65	± 0.6 %		

EX30V4 - SN 7346				March 30, 2022			
10729	AAC	IEEE 802.11a (80MHz, MCS10, 900-00)	WLAN	8.64	± 0.6 %		
10730	AAC	IEEE 802.11a (80MHz, MCS11, 900-00)	WLAN	8.87	± 0.6 %		
10731	AAC	IEEE 802.11a (80MHz, MCS12, 900-00)	WLAN	8.62	± 0.6 %		
10732	AAC	IEEE 802.11a (80MHz, MCS13, 900-00)	WLAN	8.46	± 0.6 %		
10733	AAC	IEEE 802.11a (80MHz, MCS14, 900-00)	WLAN	8.60	± 0.6 %		
10734	AAC	IEEE 802.11a (80MHz, MCS15, 900-00)	WLAN	8.25	± 0.6 %		
10735	AAC	IEEE 802.11a (80MHz, MCS16, 900-00)	WLAN	8.73	± 0.6 %		
10736	AAC	IEEE 802.11a (80MHz, MCS17, 900-00)	WLAN	8.67	± 0.6 %		
10737	AAC	IEEE 802.11a (80MHz, MCS18, 900-00)	WLAN	8.78	± 0.6 %		
10738	AAC	IEEE 802.11a (80MHz, MCS19, 900-00)	WLAN	8.48	± 0.6 %		
10739	AAC	IEEE 802.11a (80MHz, MCS20, 900-00)	WLAN	8.78	± 0.6 %		
10740	AAC	IEEE 802.11a (80MHz, MCS21, 900-00)	WLAN	8.68	± 0.6 %		
10741	AAC	IEEE 802.11a (80MHz, MCS22, 900-00)	WLAN	8.67	± 0.6 %		
10742	AAC	IEEE 802.11a (80MHz, MCS23, 900-00)	WLAN	8.43	± 0.6 %		
10743	AAC	IEEE 802.11a (80MHz, MCS24, 900-00)	WLAN	8.43	± 0.6 %		
10744	AAC	IEEE 802.11a (80MHz, MCS25, 900-00)	WLAN	8.16	± 0.6 %		
10745	AAC	IEEE 802.11a (80MHz, MCS26, 900-00)	WLAN	8.74	± 0.6 %		
10746	AAC	IEEE 802.11a (80MHz, MCS27, 900-00)	WLAN	8.63	± 0.6 %		
10747	AAC	IEEE 802.11a (80MHz, MCS28, 900-00)	WLAN	8.64	± 0.6 %		
10748	AAC	IEEE 802.11a (80MHz, MCS29, 900-00)	WLAN	8.80	± 0.6 %		
10749	AAC	IEEE 802.11a (80MHz, MCS30, 900-00)	WLAN	8.80	± 0.6 %		
10750	AAC	IEEE 802.11a (80MHz, MCS31, 900-00)	WLAN	8.82	± 0.6 %		
10751	AAC	IEEE 802.11a (80MHz, MCS32, 900-00)	WLAN	8.61	± 0.6 %		
10752	AAC	IEEE 802.11a (160MHz, MCS1, 900-00)	WLAN	9.02	± 0.6 %		
10753	AAC	IEEE 802.11a (160MHz, MCS2, 900-00)	WLAN	8.94	± 0.6 %		
10754	AAC	IEEE 802.11a (160MHz, MCS3, 900-00)	WLAN	8.77	± 0.6 %		
10755	AAC	IEEE 802.11a (160MHz, MCS4, 900-00)	WLAN	8.69	± 0.6 %		
10756	AAC	IEEE 802.11a (160MHz, MCS5, 900-00)	WLAN	8.58	± 0.6 %		
10757	AAC	IEEE 802.11a (160MHz, MCS6, 900-00)	WLAN	8.69	± 0.6 %		
10758	AAC	IEEE 802.11a (160MHz, MCS7, 900-00)	WLAN	8.49	± 0.6 %		
10759	AAC	IEEE 802.11a (160MHz, MCS8, 900-00)	WLAN	8.54	± 0.6 %		
10760	AAC	IEEE 802.11a (160MHz, MCS9, 900-00)	WLAN	8.54	± 0.6 %		
10761	AAC	IEEE 802.11a (160MHz, MCS10, 900-00)	WLAN	8.54	± 0.6 %		
10762	AAC	IEEE 802.11a (160MHz, MCS11, 900-00)	WLAN	8.51	± 0.6 %		
10763	AAC	IEEE 802.11a (160MHz, MCS12, 900-00)	WLAN	8.51	± 0.6 %		
10764	AAC	IEEE 802.11a (160MHz, MCS13, 900-00)	WLAN	8.51	± 0.6 %		
10765	AAC	IEEE 802.11a (160MHz, MCS14, 900-00)	WLAN	8.51	± 0.6 %		
10766	AAC	IEEE 802.11a (160MHz, MCS15, 900-00)	WLAN	8.51	± 0.6 %		
10767	AAC	IEEE 802.11a (160MHz, MCS16, 900-00)	WLAN	8.51	± 0.6 %		
10768	AAC	IEEE 802.11a (160MHz, MCS17, 900-00)	WLAN	8.51	± 0.6 %		
10769	AAC	IEEE 802.11a (160MHz, MCS18, 900-00)	WLAN	8.51	± 0.6 %		
10770	AAC	IEEE 802.11a (160MHz, MCS19, 900-00)	WLAN	8.51	± 0.6 %		
10771	AAC	IEEE 802.11a (160MHz, MCS20, 900-00)	WLAN	8.51	± 0.6 %		
10772	AAC	IEEE 802.11a (160MHz, MCS21, 900-00)	WLAN	8.51	± 0.6 %		
10773	AAC	IEEE 802.11a (160MHz, MCS22, 900-00)	WLAN	8.51	± 0.6 %		
10774	AAC	IEEE 802.11a (160MHz, MCS23, 900-00)	WLAN	8.51	± 0.6 %		
10775	AAC	IEEE 802.11a (160MHz, MCS24, 900-00)	WLAN	8.51	± 0.6 %		
10776	AAC	IEEE 802.11a (160MHz, MCS25, 900-00)	WLAN	8.51	± 0.6 %		
10777	AAC	IEEE 802.11a (160MHz, MCS26, 900-00)	WLAN	8.51	± 0.6 %		
10778	AAC	IEEE 802.11a (160MHz, MCS27, 900-00)	WLAN	8.51	± 0.6 %		
10779	AAC	IEEE 802.11a (160MHz, MCS28, 900-00)	WLAN	8.51	± 0.6 %		
10780	AAC	IEEE 802.11a (160MHz, MCS29, 900-00)	WLAN	8.51	± 0.6 %		
10781	AAC	IEEE 802.11a (160MHz, MCS30, 900-00)	WLAN	8.51	± 0.6 %		
10782	AAC	IEEE 802.11a (160MHz, MCS31, 900-00)	WLAN	8.51	± 0.6 %		
10783	AAC	IEEE 802.11a (160MHz, MCS32, 900-00)	WLAN	8.51	± 0.6 %		



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us by telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
 中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgsgroup.com.cn
 (86-512)57355888 (86-512)57370818 sgs.china@sgs.com

<p>EX3D14-- SN 7346</p> <p>March 30, 2022</p> <p>Continued on: EX3-D14_Mar22 Page 27 of 24</p>	<p>EX3D14-- SN 7346</p> <p>March 30, 2022</p> <table border="1"> <tr> <td>15985</td> <td>AAA</td> <td>50 NR DL (CP-QPOM, TM 3.1, 40 MHz, 64-QAM, 30 MHz)</td> <td>SG NR FR1 TDD</td> <td>9.54</td> <td>± 9.8 %</td> </tr> <tr> <td>15986</td> <td>AAA</td> <td>50 NR DL (CP-QPOM, TM 3.1, 50 MHz, 64-QAM, 30 MHz)</td> <td>SG NR FR1 TDD</td> <td>9.50</td> <td>± 9.8 %</td> </tr> <tr> <td>15987</td> <td>AAA</td> <td>50 NR DL (CP-QPOM, TM 3.1, 60 MHz, 64-QAM, 30 MHz)</td> <td>SG NR FR1 TDD</td> <td>9.53</td> <td>± 9.8 %</td> </tr> <tr> <td>15988</td> <td>AAA</td> <td>50 NR DL (CP-QPOM, TM 3.1, 70 MHz, 64-QAM, 30 MHz)</td> <td>SG NR FR1 TDD</td> <td>9.38</td> <td>± 9.8 %</td> </tr> <tr> <td>15989</td> <td>AAA</td> <td>50 NR DL (CP-QPOM, TM 3.1, 80 MHz, 64-QAM, 30 MHz)</td> <td>SG NR FR1 TDD</td> <td>9.33</td> <td>± 9.8 %</td> </tr> <tr> <td>15990</td> <td>AAA</td> <td>50 NR DL (CP-QPOM, TM 3.1, 90 MHz, 64-QAM, 30 MHz)</td> <td>SG NR FR1 TDD</td> <td>9.52</td> <td>± 9.8 %</td> </tr> </table> <p><small>* Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.</small></p> <p>Certificate No: EX3-7346_Mar22 Page 24 of 24</p>	15985	AAA	50 NR DL (CP-QPOM, TM 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.54	± 9.8 %	15986	AAA	50 NR DL (CP-QPOM, TM 3.1, 50 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.50	± 9.8 %	15987	AAA	50 NR DL (CP-QPOM, TM 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.53	± 9.8 %	15988	AAA	50 NR DL (CP-QPOM, TM 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.38	± 9.8 %	15989	AAA	50 NR DL (CP-QPOM, TM 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.33	± 9.8 %	15990	AAA	50 NR DL (CP-QPOM, TM 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.52	± 9.8 %
15985	AAA	50 NR DL (CP-QPOM, TM 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.54	± 9.8 %																																
15986	AAA	50 NR DL (CP-QPOM, TM 3.1, 50 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.50	± 9.8 %																																
15987	AAA	50 NR DL (CP-QPOM, TM 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.53	± 9.8 %																																
15988	AAA	50 NR DL (CP-QPOM, TM 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.38	± 9.8 %																																
15989	AAA	50 NR DL (CP-QPOM, TM 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.33	± 9.8 %																																
15990	AAA	50 NR DL (CP-QPOM, TM 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.52	± 9.8 %																																

4 Impedance and return loss

Dipole CLA150 SN 4025				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2021/4/26	-31.4	/	47.8	/
Dipole D450V3 SN 1103				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2021/4/21	-23	/	57.1	/



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN_Doccheck@sgs.com
 No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300 t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
 中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300 t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com