


Appendix D

Photographs


1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

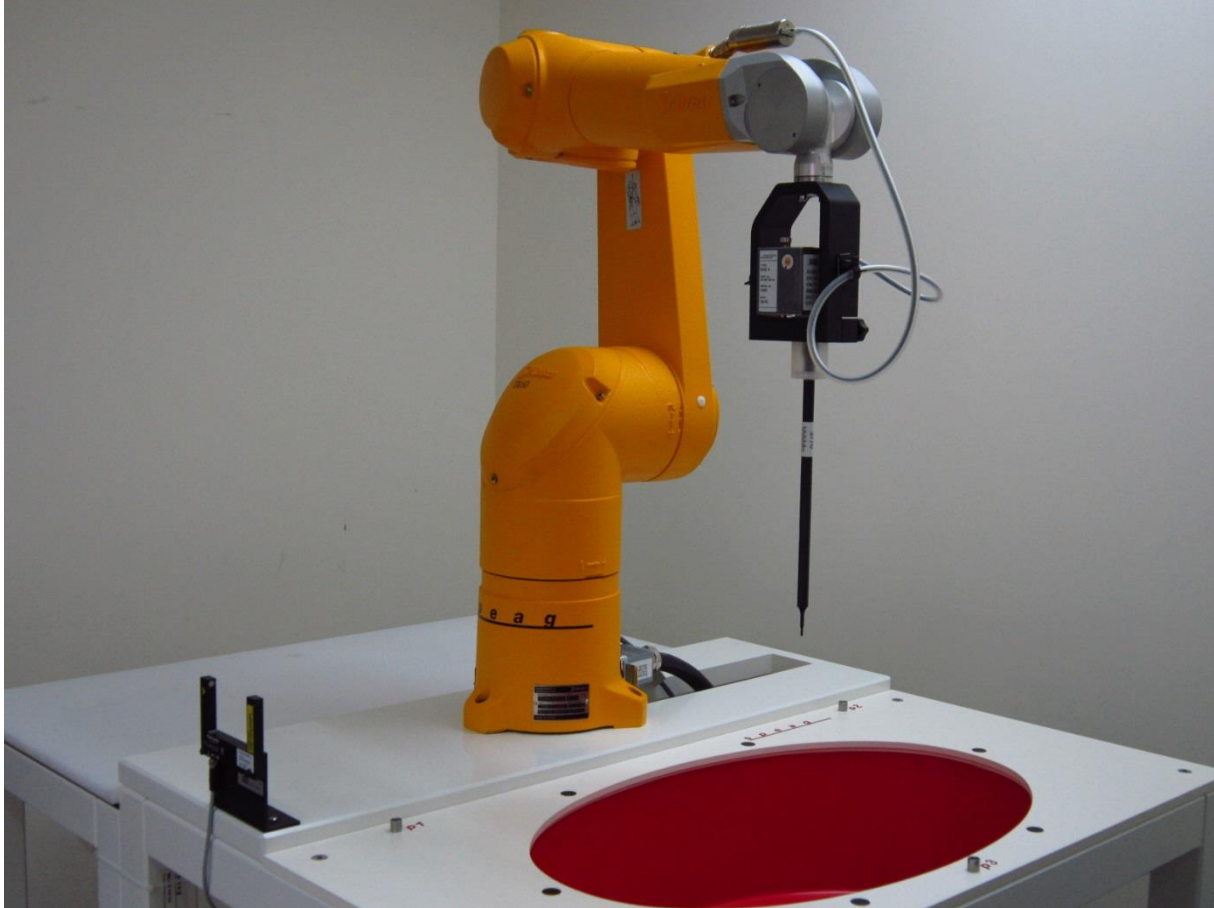


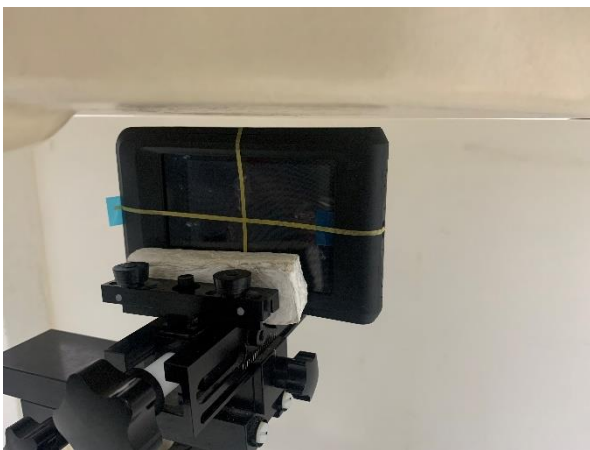
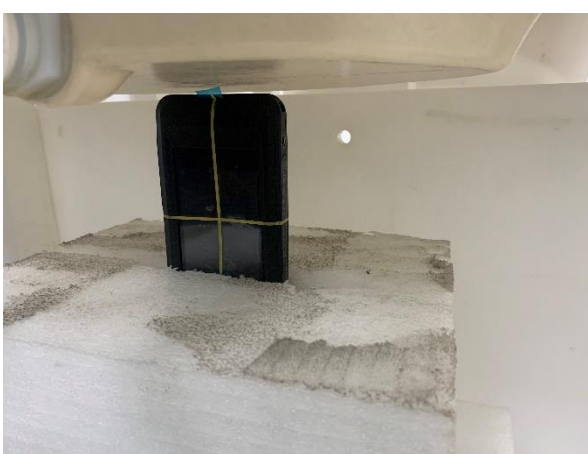
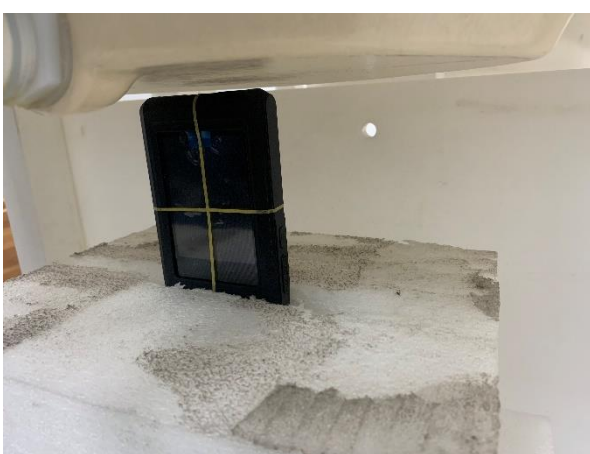


2. Photographs of Tissue Simulate Liquid

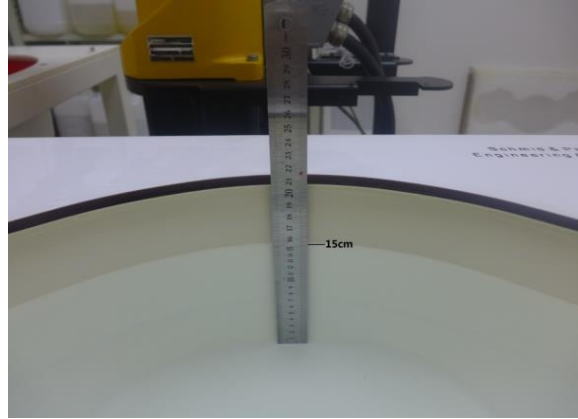Photo 1: Tissue Simulant Liquid for Head 2450



3. Photographs of EUT test position

<p>Photo 2: Front side 5mm</p>	<p>Photo 3: Back side 5mm</p>
	
<p>Photo 4: Left side 5mm</p>	<p>Photo 5: Right side 5mm</p>
	
<p>Photo 6: Top side 5mm</p>	<p>Photo 7: Bottom side 5mm</p>
	

4. EUT Constructional Details

Details please Refer to the <External Photos> & <Internal Photos>.