

Appendix D

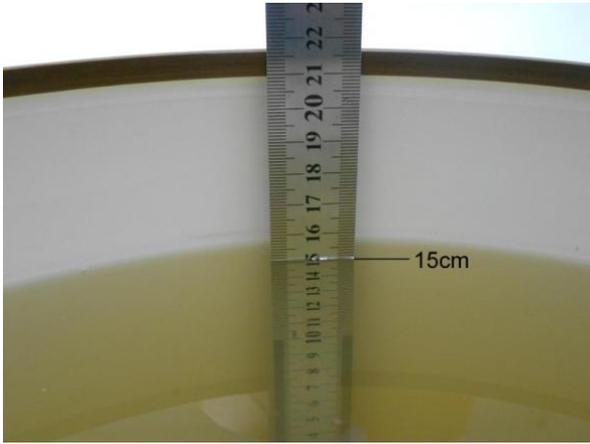
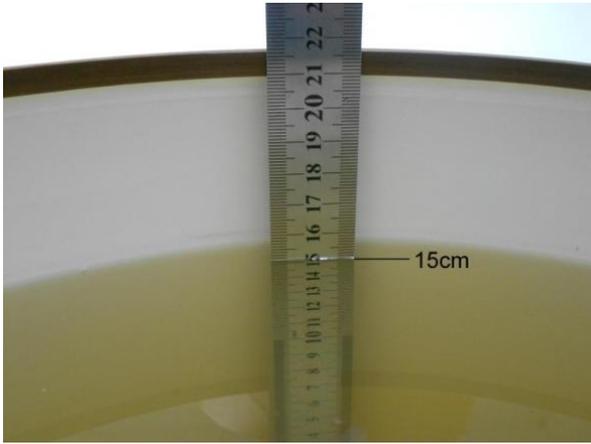
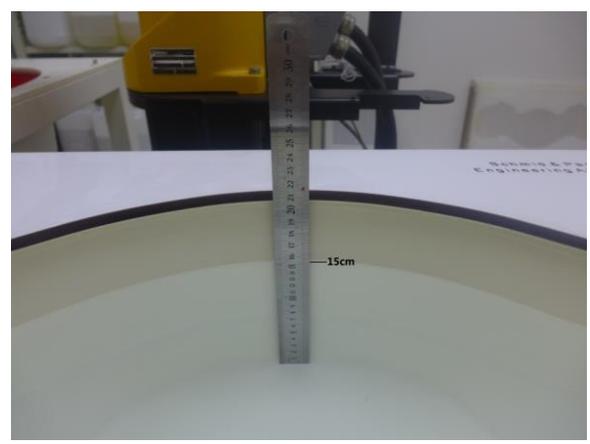
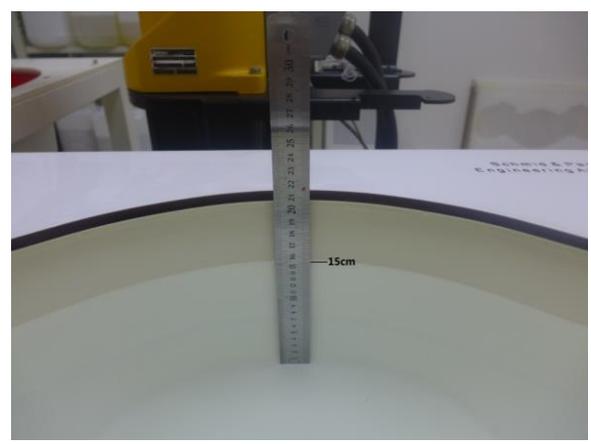
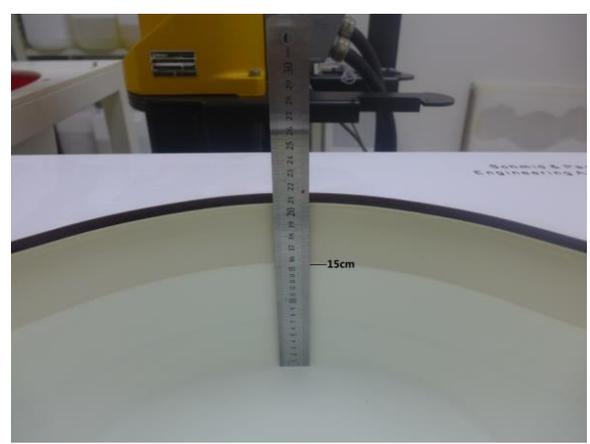
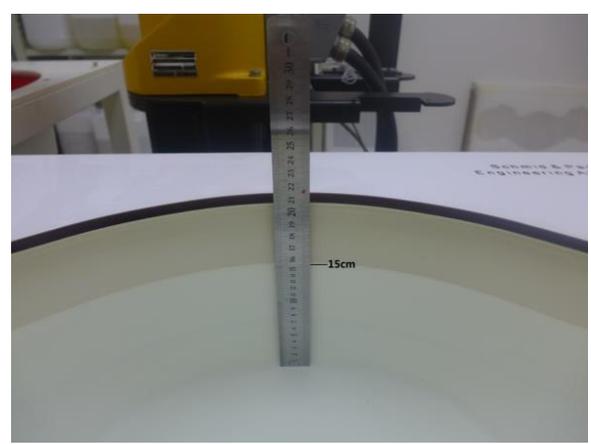
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

<p>Photo 1: Tissue Simulant Liquid for Head 750</p>	<p>Photo 2: Tissue Simulant Liquid for Head 835</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 1800</p>	<p>Photo 4: Tissue Simulant Liquid for Head 1900</p>
	
<p>Photo 5: Tissue Simulant Liquid for Head 2450</p>	<p>Photo 6: Tissue Simulant Liquid for Head 2600</p>
	

3. Photographs of EUT test position

Photo 7: Next to the mouth 10mm	Photo 8: Back side 0mm
 A close-up photograph of a black electronic device (likely a mobile phone) resting on a white foam block. The device is positioned horizontally, and the camera is positioned 10mm to the left of the mouth area. The device has a small oval-shaped area with the letters 'SMB' embossed on it.	 A close-up photograph of the same black electronic device resting on a white foam block. The camera is positioned directly behind the device (0mm distance) to capture the back side. The back of the device shows a camera lens and a flash. In the foreground, the tops of three black cylindrical test fixtures are visible.

4. EUT Constructional Details

Details please Refer to the <External Photos> & <Internal Photos>.