


### FCC ID Label Location

- FCC ID Label Placement Location

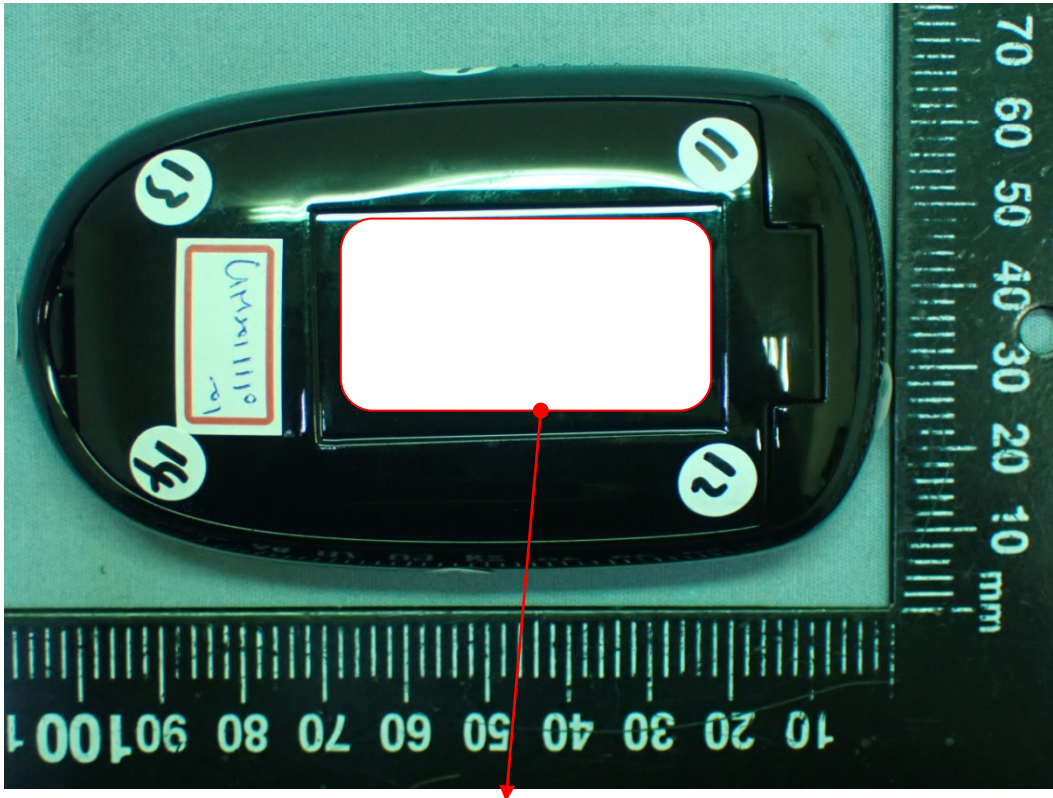

FCC ID Label Placement Location (EUT Bottom View)

- FCC ID Label Format

<b>ACEZIN GLUGold</b>
<b>Blood Glucose Meter Model: AM100 plus</b>
<b>FCC ID:2AYCBAM100PLUS</b>
<p>This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.</p>
<b>Ace Medical Technology Co., Ltd.</b> <small>No.52, Dinghu Rd., Gulshan Dist., Taoyuan City 33378, Taiwan</small>
<b>SN</b>
<b>P/N: M709-000000-XXX VER: 001</b>