1.6. D2600V2 Dipole Calibration Certificate

In Collabora	tion with CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CALC CA		中国认可 国际互认 校准 CALIBRATION
Add: No.52 HuaYuanBei Ro Tel: +86-10-62304633-2117 E-mail: emf@caict.ac.cn			CNAS L0570
Client HTW		Certificate No:	23J02Z80186
CALIBRATION CE	ERTIFICAT	E	
Object	D2600	V2 - SN: 1150	
Calibration Procedure(s)	FF-711	-003-01	
		tion Procedures for dipole validation kits	
Calibration date:		ber 7, 2023	
pages and are part of the ce	ertificate.	the uncertainties with confidence probabiling the closed laboratory facility: environment or calibration)	
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRP2	106276	15-May-23 (CTTL, No.J23X04183)	May-24
Power sensor NRP6A	101369	15-May-23 (CTTL, No.J23X04183)	May-24
Reference Probe EX3DV4	SN 3617	31-Mar-23(CTTL-SPEAG, No.Z23-60161	
DAE4	SN 1556	11-Jan-23(CTTL-SPEAG,No.Z23-60034)	
Secondary Standards	ID#	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	05-Jan-23 (CTTL, No. J23X00107)	Jan-24
NetworkAnalyzer E5071C	MY46110673	10-Jan-23 (CTTL, No. J23X00104)	Jan-24
	Name	Function	Signature
Calibrated by:	Zhao Jing	SAR Test Engineer	大変
Reviewed by:	Lin Hao	SAR Test Engineer	the and
Approved by:	Qi Dianyuan	SAR Project Leader	(tot)
		Issued: Do	ecember 12, 2023

Certificate No: 23J02Z80186

Page 1 of 6





Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORMx,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Page 2 of 6





Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2600 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.0	1.96 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	37.9 ± 6 %	1.99 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C		

SAR result with Head TSL

SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	14.3 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	56.4 W/kg ± 18.8 % (k=2)
SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	6.37 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	25.3 W/kg ± 18.7 % (<i>k</i> =2)

Certificate No: 23J02Z80186

Page 3 of 6





Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	48.1Ω- 4.67jΩ	
Return Loss	- 25.8dB	

General Antenna Parameters and Design

Electrical Delay (one direction)	1.048 ns	
----------------------------------	----------	--

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.


The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------


Certificate No: 23J02Z80186

Page 4 of 6

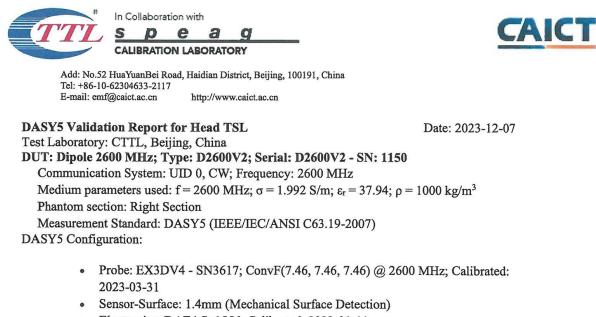

- Electronics: DAE4 Sn1556; Calibrated: 2023-01-11
- Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 101.9 V/m; Power Drift = -0.04 dB Peak SAR (extrapolated) = 30.6 W/kg SAR(1 g) = 14.3 W/kg; SAR(10 g) = 6.37 W/kg Smallest distance from peaks to all points 3 dB below = 8.5 mm Ratio of SAR at M2 to SAR at M1 = 47.4% Maximum value of SAR (measured) = 24.6 W/kg

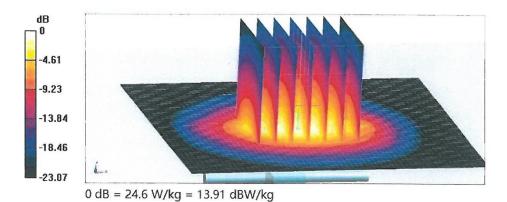


Certificate No: 23J02Z80186

Page 5 of 6





Impedance Measurement Plot for Head TSL

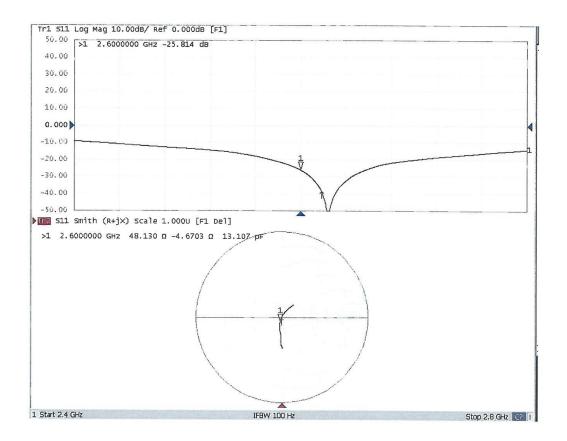

Certificate No: 23J02Z80186

Page 6 of 6

1.7. D5GHzV2 Dipole Calibration Certificate

	on with e a d		中国认可 国际互认 一人
	N LABORATORY		交准 ALIBRATION
Add: No.52 HuaYuanBei Road Tel: +86-10-62304633-2117 E-mail: emf@caict.ac.cn	d, Haidian District, http://www.caic.	Beijing, 100191	NAS L0570
Client HTW		Certificate No: 23	J02Z80187
ALIBRATION CE	RTIFICAT	Έ	
bject	D5GHz	2V2 - SN: 1273	
alibration Procedure(s)	FF-Z11	-003-01	
	Calibra	tion Procedures for dipole validation kits	
alibration date:	Decem	ber 6, 2023	
	surements and	traceability to national standards, which rea the uncertainties with confidence probability	
	conducted in t	he closed laboratory facility: environment or calibration)	temperature (22±3)℃ and
I calibrations have been c umidity<70%. alibration Equipment used (N	conducted in t	or calibration)	
I calibrations have been c umidity<70%. alibration Equipment used (N rimary Standards	conducted in the M&TE critical for		Scheduled Calibration
I calibrations have been c umidity<70%. alibration Equipment used (N rimary Standards Power Meter NRP2	Conducted in the M&TE critical for ID #	or calibration) Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration May-24
I calibrations have been c umidity<70%. alibration Equipment used (N imary Standards Power Meter NRP2 Power sensor NRP6A	Conducted in the M&TE critical for ID # 106276	Cal Date (Calibrated by, Certificate No.) 15-May-23 (CTTL, No.J23X04183)	Scheduled Calibration
I calibrations have been c umidity<70%. alibration Equipment used (N imary Standards Power Meter NRP2 Power sensor NRP6A Reference Probe EX3DV4	Conducted in the M&TE critical for the ID # 106276 101369	Cal Date (Calibrated by, Certificate No.) 15-May-23 (CTTL, No.J23X04183) 15-May-23 (CTTL, No.J23X04183)	Scheduled Calibration May-24 May-24
I calibrations have been c umidity<70%. alibration Equipment used (N rimary Standards Power Meter NRP2 Power sensor NRP6A Reference Probe EX3DV4 DAE4	Conducted in the M&TE critical for the M&TE	Cal Date (Calibrated by, Certificate No.) 15-May-23 (CTTL, No.J23X04183) 15-May-23 (CTTL, No.J23X04183) 31-Mar-23(CTTL-SPEAG,No.Z23-60161)	Scheduled Calibration May-24 May-24 Mar-24
I calibrations have been c umidity<70%. alibration Equipment used (N rimary Standards Power Meter NRP2 Power sensor NRP6A Reference Probe EX3DV4 DAE4 Secondary Standards	Conducted in the M&TE critical for ID # 106276 101369 SN 3617 SN 1556	Cal Date (Calibrated by, Certificate No.) 15-May-23 (CTTL, No.J23X04183) 15-May-23 (CTTL, No.J23X04183) 31-Mar-23(CTTL-SPEAG,No.Z23-60161) 11-Jan-23(CTTL-SPEAG,No.Z23-60034)	Scheduled Calibration May-24 May-24 Mar-24 Jan-24
I calibrations have been of umidity<70%. alibration Equipment used (N imary Standards Power Meter NRP2 Power sensor NRP6A Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	Conducted in the M&TE critical for the ID # 106276 101369 SN 3617 SN 1556 ID # ID #	Cal Date (Calibrated by, Certificate No.) 15-May-23 (CTTL, No.J23X04183) 15-May-23 (CTTL, No.J23X04183) 31-Mar-23(CTTL-SPEAG,No.Z23-60161) 11-Jan-23(CTTL-SPEAG,No.Z23-60034) Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration May-24 May-24 Mar-24 Jan-24 Scheduled Calibration
I calibrations have been or umidity<70%. alibration Equipment used (Norman Standards Power Meter NRP2 Power sensor NRP6A Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	Conducted in the M&TE critical for the formation of the f	Cal Date (Calibrated by, Certificate No.) 15-May-23 (CTTL, No.J23X04183) 15-May-23 (CTTL, No.J23X04183) 31-Mar-23(CTTL-SPEAG,No.Z23-60161) 11-Jan-23(CTTL-SPEAG,No.Z23-60034) Cal Date (Calibrated by, Certificate No.) 05-Jan-23 (CTTL, No. J23X00107) 10-Jan-23 (CTTL, No. J23X00104)	Scheduled Calibration May-24 May-24 Mar-24 Jan-24 Scheduled Calibration Jan-24 Jan-24
I calibrations have been of umidity<70%. alibration Equipment used (N imary Standards Power Meter NRP2 Power sensor NRP6A Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C NetworkAnalyzer E5071C	Conducted in the M&TE critical for the ID # 106276 101369 SN 3617 SN 1556 ID # MY49071430 MY46110673	Cal Date (Calibrated by, Certificate No.) 15-May-23 (CTTL, No.J23X04183) 15-May-23 (CTTL, No.J23X04183) 31-Mar-23(CTTL-SPEAG,No.Z23-60161) 11-Jan-23(CTTL-SPEAG,No.Z23-60034) Cal Date (Calibrated by, Certificate No.) 05-Jan-23 (CTTL, No. J23X00107)	Scheduled Calibration May-24 May-24 Mar-24 Jan-24 Scheduled Calibration Jan-24
I calibrations have been or umidity<70%. alibration Equipment used (N imary Standards Power Meter NRP2 Power sensor NRP6A Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C NetworkAnalyzer E5071C	Conducted in the M&TE critical for the formation of the f	Cal Date (Calibrated by, Certificate No.) 15-May-23 (CTTL, No.J23X04183) 15-May-23 (CTTL, No.J23X04183) 31-Mar-23(CTTL-SPEAG,No.Z23-60161) 11-Jan-23(CTTL-SPEAG,No.Z23-60034) Cal Date (Calibrated by, Certificate No.) 05-Jan-23 (CTTL, No. J23X00107) 10-Jan-23 (CTTL, No. J23X00104) Function	Scheduled Calibration May-24 May-24 Mar-24 Jan-24 Scheduled Calibration Jan-24 Jan-24
I calibrations have been or midity<70%. alibration Equipment used (Normal Standards Power Meter NRP2 Power sensor NRP6A Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C NetworkAnalyzer E5071C alibrated by: 2 eviewed by: 2	Conducted in the M&TE critical for ID # 106276 101369 SN 3617 SN 1556 ID # MY49071430 MY46110673 Name Zhao Jing	Cal Date (Calibrated by, Certificate No.) 15-May-23 (CTTL, No.J23X04183) 15-May-23 (CTTL, No.J23X04183) 31-Mar-23 (CTTL-SPEAG,No.Z23-60161) 11-Jan-23 (CTTL-SPEAG,No.Z23-60034) Cal Date (Calibrated by, Certificate No.) 05-Jan-23 (CTTL, No. J23X00107) 10-Jan-23 (CTTL, No. J23X00104) Function SAR Test Engineer	Scheduled Calibration May-24 May-24 Mar-24 Jan-24 Scheduled Calibration Jan-24 Jan-24
I calibrations have been or umidity<70%. alibration Equipment used (N imary Standards Power Meter NRP2 Power sensor NRP6A Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C NetworkAnalyzer E5071C	Conducted in the M&TE critical for ID # 106276 101369 SN 3617 SN 1556 ID # MY49071430 MY46110673 Name Zhao Jing	Cal Date (Calibrated by, Certificate No.) 15-May-23 (CTTL, No.J23X04183) 15-May-23 (CTTL, No.J23X04183) 31-Mar-23 (CTTL-SPEAG,No.Z23-60161) 11-Jan-23 (CTTL-SPEAG,No.Z23-60034) Cal Date (Calibrated by, Certificate No.) 05-Jan-23 (CTTL, No. J23X00107) 10-Jan-23 (CTTL, No. J23X00104) Function SAR Test Engineer	Scheduled Calib May-24 May-24 Mar-24 Jan-24 Scheduled Calibr Jan-24 Jan-24

Certificate No: 23J02Z80187

Page 1 of 8





Glossary	/:
----------	----

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORMx,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Page 2 of 8





Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	5250 MHz ± 1 MHz 5600 MHz ± 1 MHz 5750 MHz ± 1 MHz	

Head TSL parameters at 5250MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.9	4.71 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.1 ± 6 %	4.61 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C		

SAR result with Head TSL at 5250MHz

SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	7.79 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	77.5 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.19 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.8 W/kg ± 24.2 % (k=2)

Certificate No: 23J02Z80187

Page 3 of 8





Head TSL parameters at 5600MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.5 ± 6 %	4.98 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C		

SAR result with Head TSL at 5600MHz

SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.35 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	83.0 W/kg ± 24.4 % (<i>k</i> =2)
SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.35 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.3 W/kg ± 24.2 % (k=2)

Head TSL parameters at 5750MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.4	5.22 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.4 ± 6 %	5.14 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C		

SAR result with Head TSL at 5750MHz

SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	7.78 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	77.3 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.17 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.5 W/kg ± 24.2 % (k=2)

Certificate No: 23J02Z80187

Page 4 of 8





Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL at 5250MHz

Impedance, transformed to feed point	47.7Ω- 1.45jΩ
Return Loss	- 31.0dB

Antenna Parameters with Head TSL at 5600MHz

Impedance, transformed to feed point	52.2Ω+ 4.46jΩ
Return Loss	- 26.3dB

Antenna Parameters with Head TSL at 5750MHz

Impedance, transformed to feed point	51.0Ω+ 4.54jΩ	
Return Loss	- 26.7dB	_

General Antenna Parameters and Design

Electrical Delay (one direction)	1 000
	1.099 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

Additional EUT Data

Manufacture	
Manufactured by	SPEAG
	61 21/0

Certificate No: 23J02Z80187

Page 5 of 8





DASY5 Validation Report for Head TSL Test Laboratory: CTTL, Beijing, China

Date: 2023-12-06

DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1273 Communication System: CW; Frequency: 5250 MHz, Frequency: 5600 MHz, Frequency: 5750 MHz Medium parameters used: f = 5250 MHz; σ = 4.61 S/m; ϵ_r = 35.12; ρ = 1000 kg/m³ Medium parameters used: f = 5600 MHz; σ = 4.982 S/m; ϵ_r = 34.53; ρ = 1000 kg/m³ Medium parameters used: f = 5750 MHz; σ = 5.143 S/m; ϵ_r = 34.38; ρ = 1000 kg/m³ Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration:


- Probe: EX3DV4 SN3617; ConvF(5.5, 5.5, 5.5) @ 5250 MHz; ConvF(5.01, 5.01, 5.01) @ 5600 MHz; ConvF(5.15, 5.15, 5.15) @ 5750 MHz; Calibrated: 2023-03-31
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2023-01-11
- Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration /Pin=100mW, d=10mm, f=5250 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 68.44 V/m; Power Drift = -0.04 dB Peak SAR (extrapolated) = 31.7 W/kg SAR(1 g) = 7.79 W/kg; SAR(10 g) = 2.19 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 65% Maximum value of SAR (measured) = 19.1 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 68.83 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 36.9 W/kg SAR(1 g) = 8.35 W/kg; SAR(10 g) = 2.35 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 62.3% Maximum value of SAR (measured) = 21.0 W/kg

Certificate No: 23J02Z80187


Page 6 of 8





Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China E-mail: emf@caict.ac.cn http://www.caic.ac.cn

Dipole Calibration /Pin=100mW, d=10mm, f=5750 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 66.65 V/m; Power Drift = -0.03 dB Peak SAR (extrapolated) = 35.5 W/kg SAR(1 g) = 7.78 W/kg; SAR(10 g) = 2.17 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 61.2% Maximum value of SAR (measured) = 19.9 W/kg

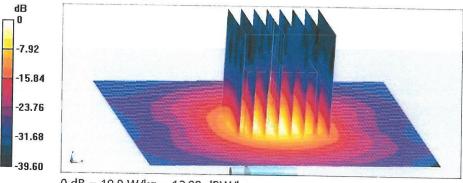

0 dB = 19.9 W/kg = 12.99 dBW/kg


Certificate No: 23J02Z80187

Page 7 of 8





Impedance Measurement Plot for Head TSL

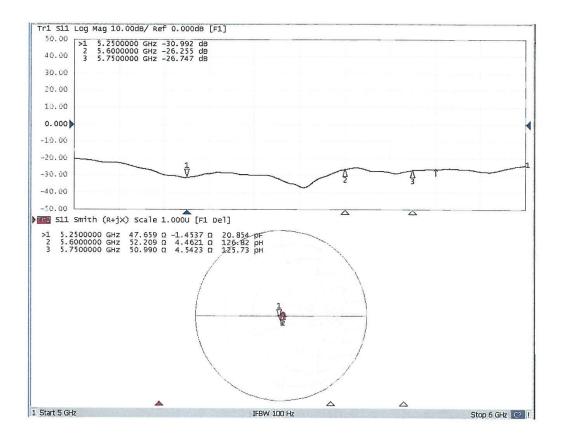

Certificate No: 23J02Z80187

Page 8 of 8