

Appendix D






Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid
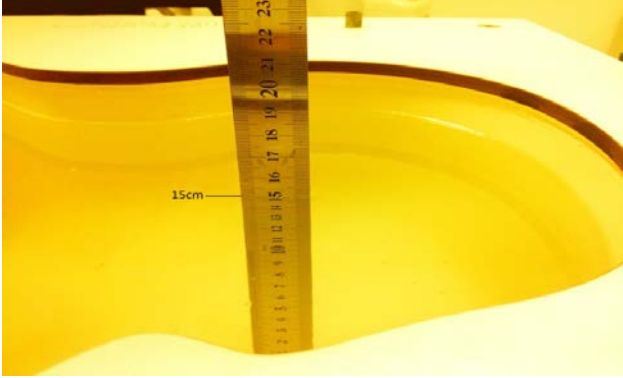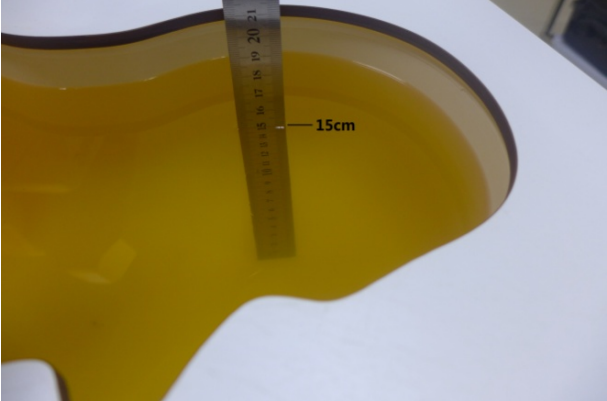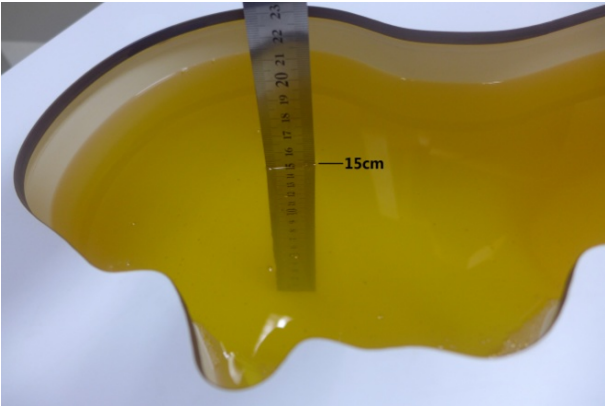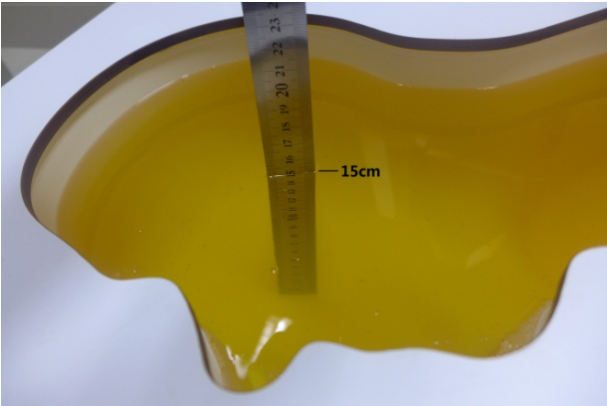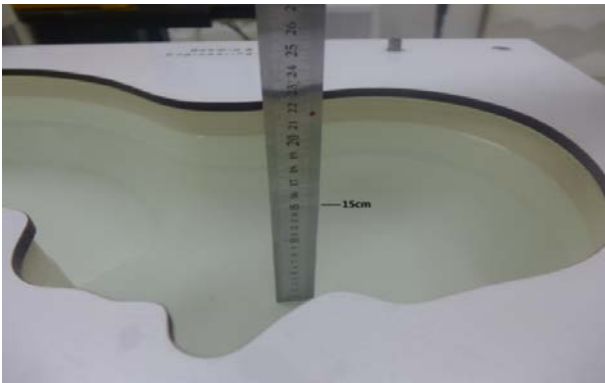
<p>Photo 1: Tissue Simulant Liquid for Head 835</p>	<p>Photo 2: Tissue Simulant Liquid for Head 1900</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 2450</p>	<p>Photo 4: Tissue Simulant Liquid for Head 2600</p>
	
<p>Photo 5: Tissue Simulant Liquid for Head 5G</p>	<p>NA</p>
	<p>NA</p>

3. Photographs of EUT test position

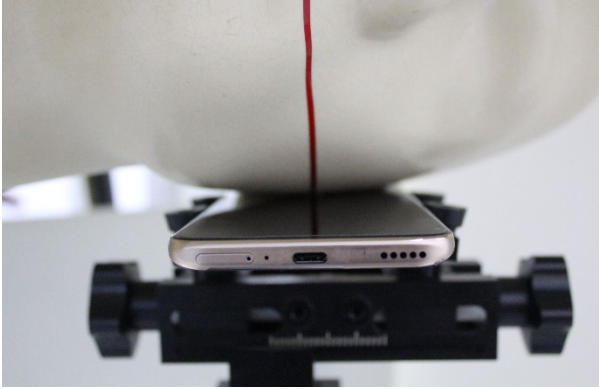
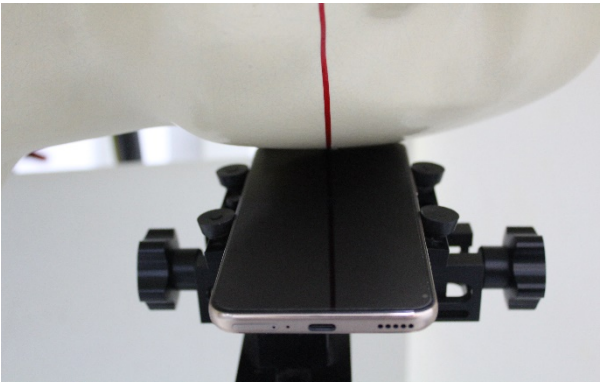
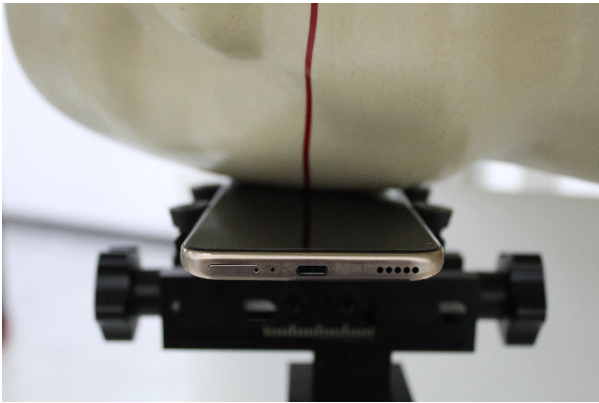
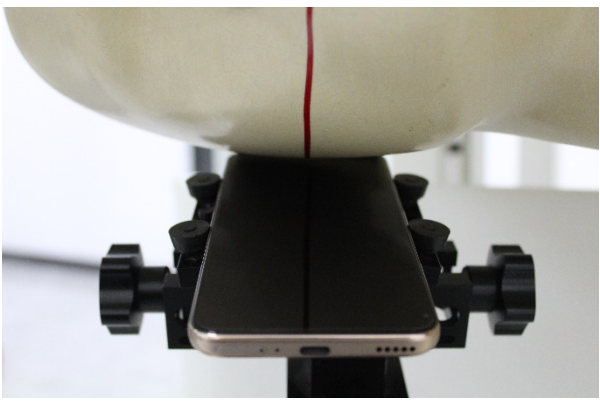
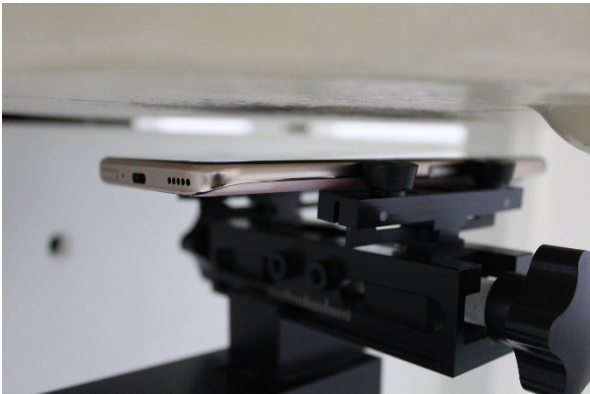
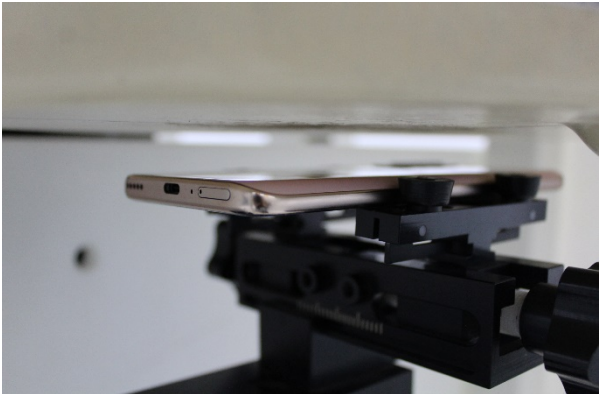
<p>Photo 6: Left touch cheek</p>	<p>Photo 7: Left tilted 15 degree</p>
	
<p>Photo 8: Right touch cheek</p>	<p>Photo 9: Right tilted 15 degree</p>
	
<p>Photo 10: Front side 15mm</p>	<p>Photo 11: Back side 15mm</p>
	

Photo 12: Front side 10mm

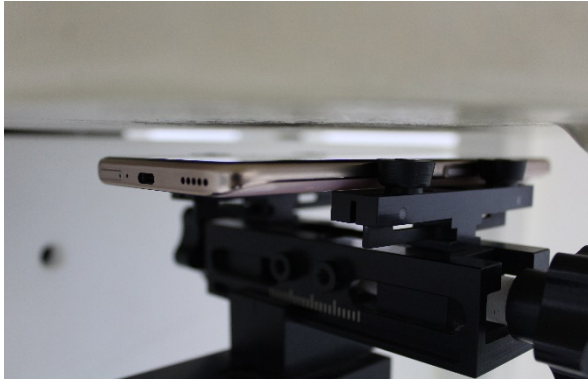


Photo 13: Back side 10mm

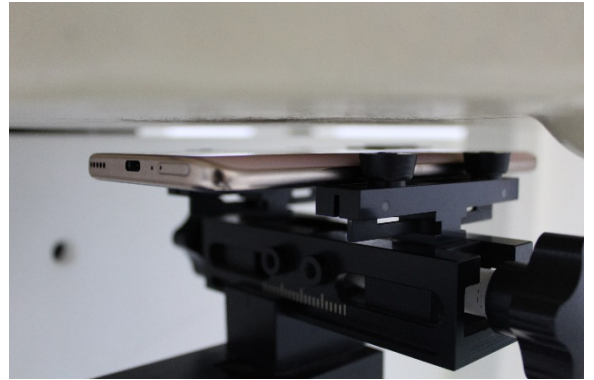


Photo 14: Left side 10mm



Photo 15: Right side 10mm



Photo 16: Top side 10mm



Photo 17: Bottom side 10mm



Photo 18: Front side 0mm

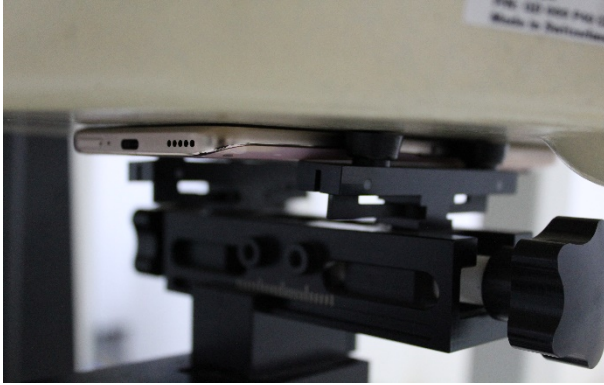


Photo 19: Back side 0mm

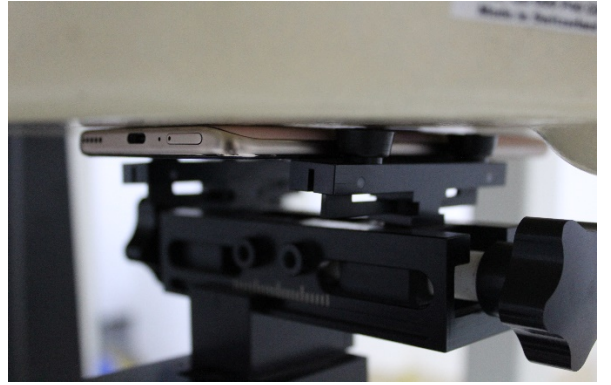


Photo 20: Right side 0mm


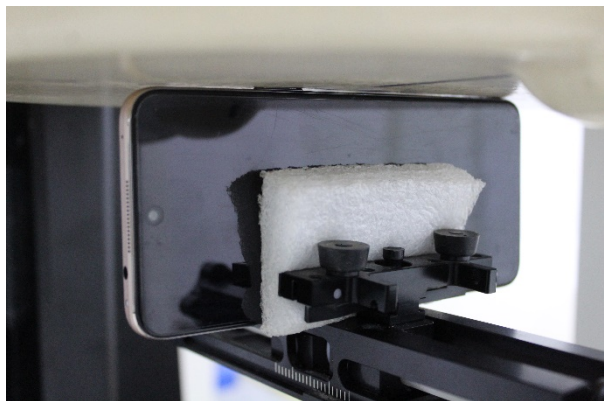


Photo 21: Top side 0mm



4. EUT Constructional Details

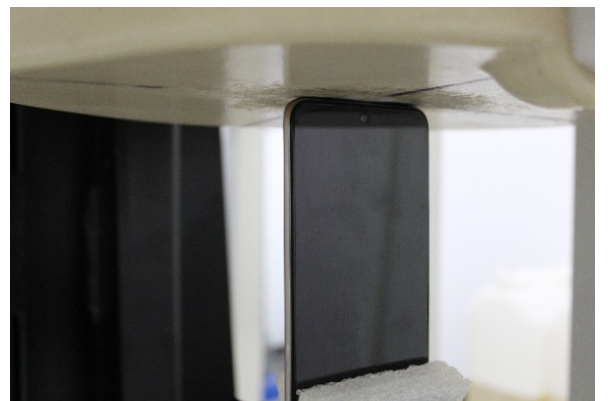