

Ms Andrea Hsia,
 Supervisor, BV CPS Taoyuan

17 May 2022

Implantable Closed Loop Stimulator CLS121 FCC ID Label Location

Per 47 CFR 95.2593(f)(2), in lieu of being placed directly on the transmitter, the FCC ID has been placed on both:

- The package label (Fig. 1) of the sealed package (Fig. 2) of the medical implant device; AND
- The user manual of the device (Fig.3).

Each unit is still physically labeled with a serial number.

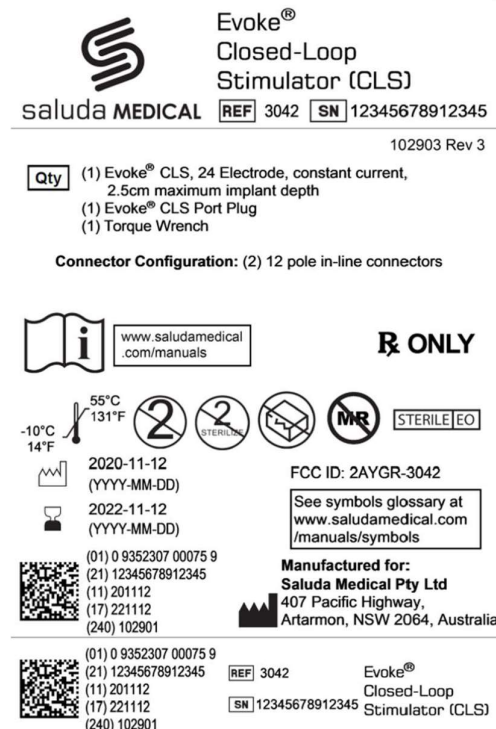


Fig. 1 CLS121 Package Label with FCC ID Label



Fig. 2 CLS121 Sealed Package with attached Package Label

Radio frequency communication	MICS band	402 - 405 MHz
	8 channels*	Centre frequency (MHz): 402.45, 402.75, 403.05, 403.35, 403.65, 403.95, 404.25, 404.55
	Transmit/Receive	
	Channel Bandwidth	300 kHz
	Modulation type	Frequency Shift Keying (FSK)
	Range	1.0 m (3.3 ft.)
	Effective Isotropic Radiated Power (EIRP)	25 μ W (-16.02 dBm) maximum
	FCC ID	2AYGR-3042

Fig. 3 User Manual Section 17.2.1, excerpt page 52