



Tap-2-Pair™

**Posey®**

**Single Patient Use 30-Day Wireless Chair Sensor Pad**  
for use with Sitter On Cue PRO™

**FIRST USE DATE:**

\_\_\_\_ / \_\_\_\_ / \_\_\_\_


**EXPIRATION DATE:**

\_\_\_\_ / \_\_\_\_ / \_\_\_\_

**USE THIS SIDE UP**

**1. Pair**

Locate and align pairing icons together

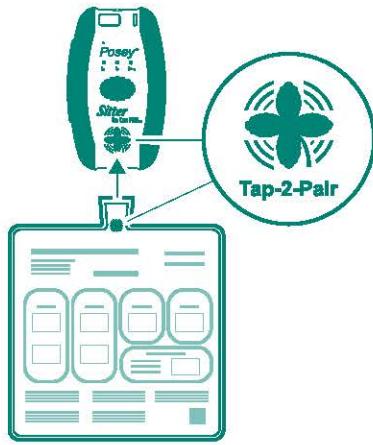


Blue light means paired





**2. Place**

Place green grip, then white pad

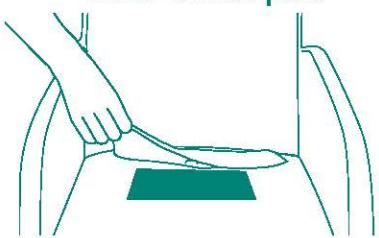


Position pad with neck facing back of chair or wheelchair

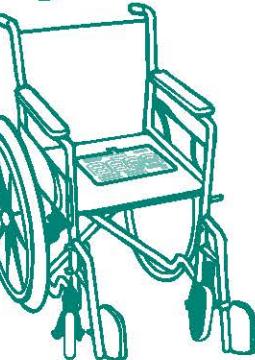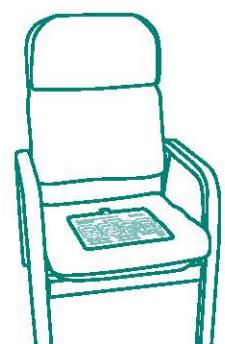


**3. Test**

Press pad and watch status light  
Green means go

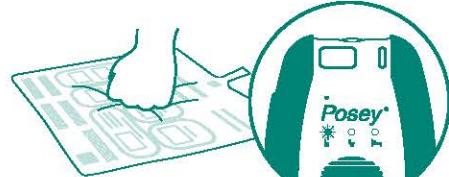

Release pad and listen for alarm

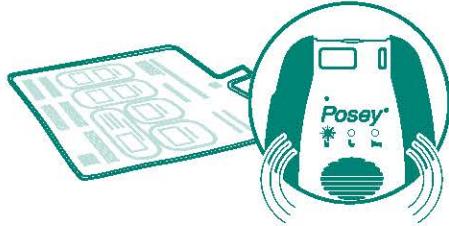

**4. Monitor**

Place patient on pad  
Green means go  
Blue light means paired



**Optional: Nurse Call Adapter**

Locate and align pairing icons together



Nurse Call Adapter blue light means paired

Plug into facility's nurse call system port

**Unpair**

- To replace sensor pad, press HOLD button to pause monitoring. Repeat steps 1-4.
- To unpair inactive sensor pad, select from these options:
  - Press and hold the MODE button
  - Turn off the fall monitor
  - Move the sensor pad outside the range of the fall monitor

**Cleaning**

Dampen (but DO NOT soak) a clean cloth with disinfectant. NEVER use any cleaning substance that contains Phenol, immerse in liquid, or sterilize with heat. Use a clean, DRY cloth to dry all parts.

**Discard**

Utilize electronic recycling programs. Sensor contains foam, electronic components, and a lithium battery. Consult Instructions for Use for additional discarding information.



**WARNING**

- Use only with chairs or wheelchairs
- Use only with Posey Sitter On Cue PRO Fall Monitor
- Ensure all parts of the system are operational before leaving patient unattended.
- This system does not prevent falls or injury from falls and is not a substitute for patient care.
- This product should be used in conjunction with your facility's falls management program.
- Never crease sensor pad. This will damage sensor pad and may cause false alarms or no alarm.

**WARRANTY USEFUL LIFE:**

Thirty (30) days from date of first use.

**FCC ID: 2AZB4-8309WL**

This device complies with part 15 of FCC Rules. Operation is subject to the following two conditions:

This device may not cause harmful interference, and this device must accept any interference received, including interference that may cause undesired operation.

L9608M Rev A 06142021



Caution: Consult Instructions for Use

[www.tap-2-pair.com](http://www.tap-2-pair.com)

For more information please visit  
[WWW.TIDIPRODUCTS.COM](http://WWW.TIDIPRODUCTS.COM)  
May be patented: see  
[www.tidiproducts.com/virtual-patent-marking](http://www.tidiproducts.com/virtual-patent-marking)

**REF** 8309WL - 30-Day Chair Pad, Wireless

**TIDI**  
Support Caregivers.  
Protect Patients.