

Product: Mimitakara hearing aid (with charging box)

Type Identification: DP-6EF, UP-6EF

**<EUT Standalone>**

**Photograph 1: Test Setup for Spurious Emissions (Front View 1)**



**Photograph 2: Test Setup for Spurious Emissions (Front View 2)**




Product: Mimitakara hearing aid (with charging box)

Type Identification: DP-6EF, UP-6EF

**Photograph 3: Test Setup for Spurious Emissions (Back View 1)**



**Photograph 4: Test Setup for Spurious Emissions (Back View 2)**

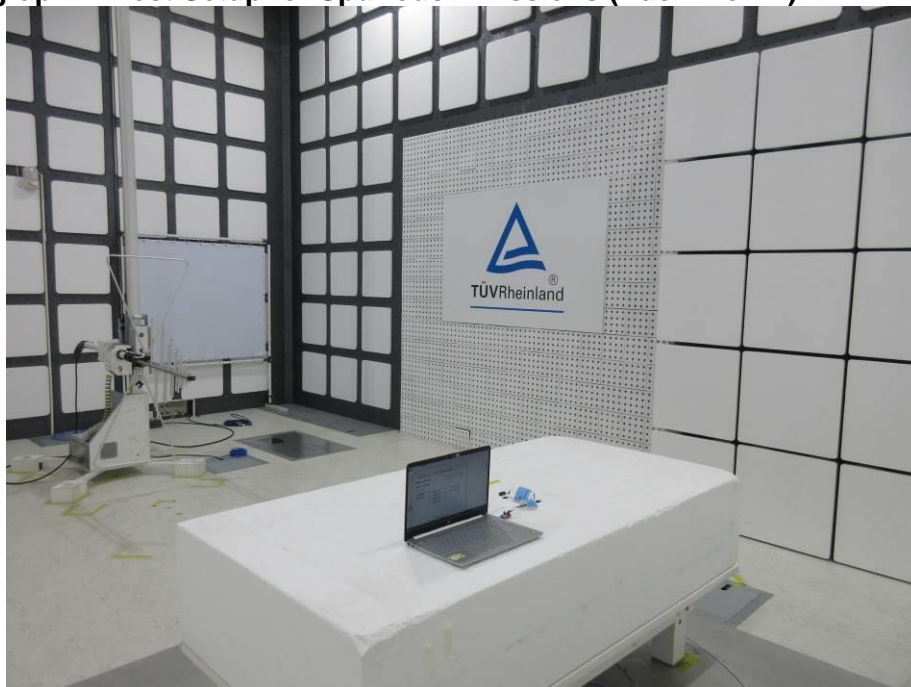

Product: Mimitakara hearing aid (with charging box)

Type Identification: DP-6EF, UP-6EF

**Photograph 5: Test Setup for Spurious Emissions (Back View 3)**



**Photograph 6: Test Setup for Spurious Emissions (Back View 4)**



Product: Mimitakara hearing aid (with charging box)

Type Identification: DP-6EF, UP-6EF

**<EUT with Charger box>**

**Photograph 7: Test Setup for Spurious Emissions (Front View 1)**



**Photograph 8: Test Setup for Spurious Emissions (Back View 1)**






Product: Mimitakara hearing aid (with charging box)

Type Identification: DP-6EF, UP-6EF

**Photograph 9: Test Setup for Spurious Emissions (Back View 2)**

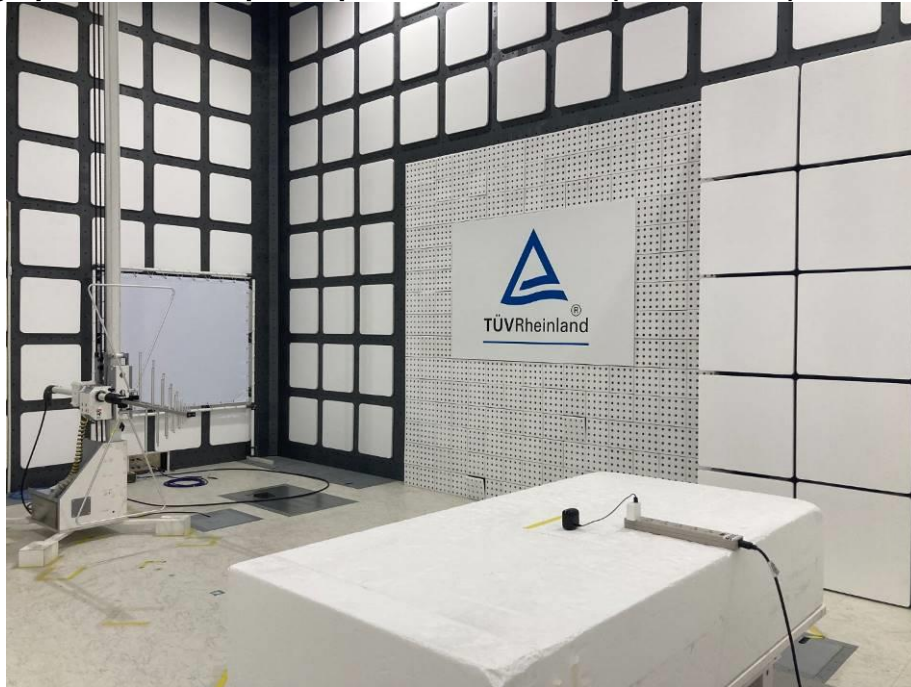

Product: Mimitakara hearing aid (with charging box)

Type Identification: DP-6EF, UP-6EF

**Photograph 10: Test Setup for Mains Conducted Emissions (Front View)**



**Photograph 11: Test Setup for Mains Conducted Emissions (Back View)**

