

FCC Composite Gain Test Report

TP-LINK CORPORATION PTE.,LTD

<http://www.tp-link.com>

7 Temasek Boulevard #29-03 Suntec Tower One, Singapore 038987



Copyright © 2022 By TP-Link CORPORATION PTE. LTD. All rights reserved.

The drawings, specifications and the data contained in this document are exclusively the property of TP-Link CORPORATION PTE. LTD. The information is intended for internal use only and is subject to change without any notice.

With no written permission from TP-Link CORPORATION PTE. LTD, this document, in parts or as a whole, shall not be reproduced, copied, or used in any form or by any means to make any derivatives such as translation, transformation, or adaptation, for any purpose whatever.




is a registered trademark of TP-Link CORPORATION PTE. LTD. Other brands and product names mentioned herein are trademarks or registered trademarks of their respective holders.

Warning

This document is intended for internal use only. A Non-Disclosure Agreement (NDA) approved by Chief Technology Officer (CTO) is required to release this document under any circumstances.

Basic Information

EUT Description:	AXE5400 Tri-Band Wi-Fi 6E Gaming Router		
Brand Name:	tp-link		
Model Name:	Archer GXE75		
Tested By:	Tan Yiyi 	Date:	2024/01/31

CONTENTS

1	Operation Mode and Antenna Information	4
1.1	EUT Operation Mode	4
1.2	Antenna Information	4
1.3	Test Frequency	5
2	Test System	5
2.1	Test Equipment	5
2.2	Test Software	5
3	Test Summary	6
3.1	Measurement Environment	6
3.2	Measurement Quantity	8
3.3	Test Method	8
3.4	Directional Gain Calculations	9
3.5	Test Procedure	10
4	Measured Value and Maximum Gain Positions	11
4.1	Antenna Number	11
4.2	6G	11
4.2.1	DG_1SS Max Value Position	11
4.2.2	DG_1SS Max Value Position Calculation	11
5	Test and Calculate Result	12
5.1	Antenna Test Result	12
5.2	Directional Gain Calculate Result	12
	Test Pattern	12
5.3	Antenna Pattern	12
6	Test Pattern	14

1 Operation Mode and Antenna Information

1.1 EUT Operation Mode

The Archer GXE75 is the Four-band wireless router of 4 internal antennas, of which 2 were 2.4G & 5G Dual-Band antennas and 2 were 6G antennas.

1.2 Antenna Information

The Antennas are internal , the Locations of Antennas are shown below:

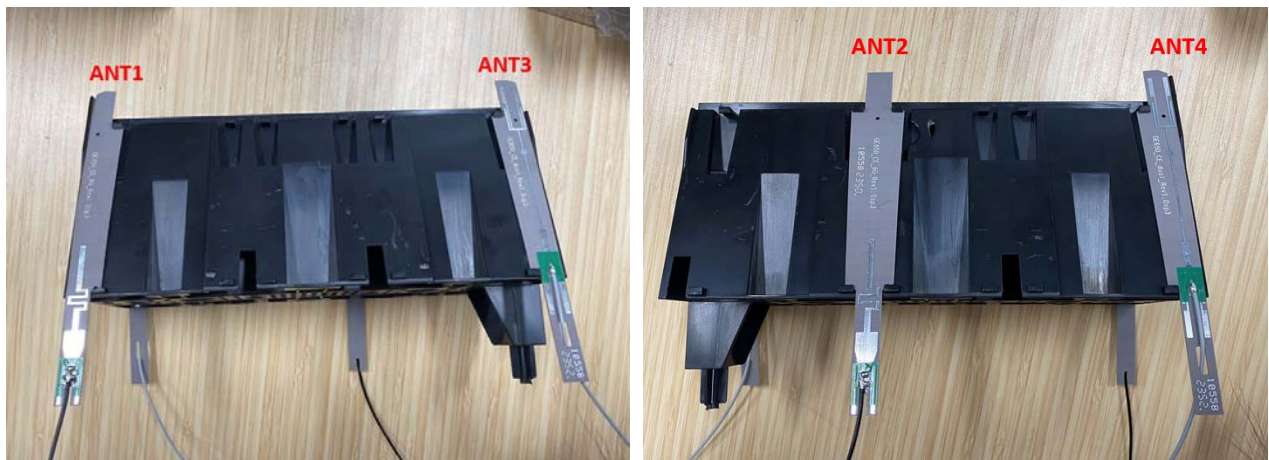


Figure 1-1 Locations of Antennas

The Antenna Information was shown below:

Table 1-1 Antenna Information

Antenna Position	Antenna Type	Connector	Mode of operation
Ant1	Franklin antenna	ipex	6G
Ant2	Franklin antenna	ipex	6G
Ant3	Dipole	ipex	2.4G&5G
Ant4	Dipole	ipex	2.4G&5G

1.3 Test Frequency

The Listed frequency of each bands are selected to represent each frequency bands.

Table 1-2 Test Frequency

Frequency Band(MHz)	Test Frequency(MHz)
5925-6425	6175
6425-6525	6475
6525-6875	6725
6875-7125	7025

2 Test System

2.1 Test Equipment

Table 2-1 Test Equipment

Equipment	Model	Manufacturer	S/N	Cali. Interval	Cali. Due Date
Chamber	Rayzone2800	GTS	MY53470435	12months	2025/04/15
Vector Network Analyzer	E5071C	Keysight	MY46315238	24months	2026/05/27

2.2 Test Software

Table 2-2 Test Software

Software	Version	Function
GTS MaxSign100	V2.1	Passive Antenna Measurements

3 Test Summary

3.1 Measurement Environment

This measurement experiment adopted an antenna near-field measurement system, and the diagram of the measurement system was shown in Figure 3-1. The excitation signal was generated by the Keysight E5071C (300kHz-20GHz). Under the control of the central computer, the probe rotated in the θ direction, and the EUT rotated in the ϕ direction with the turntable. The probe sampling frame received and collected signals in the near-field range of the EUT. The software system which was controlled by the central computer completed the processing, output and display of the test data.

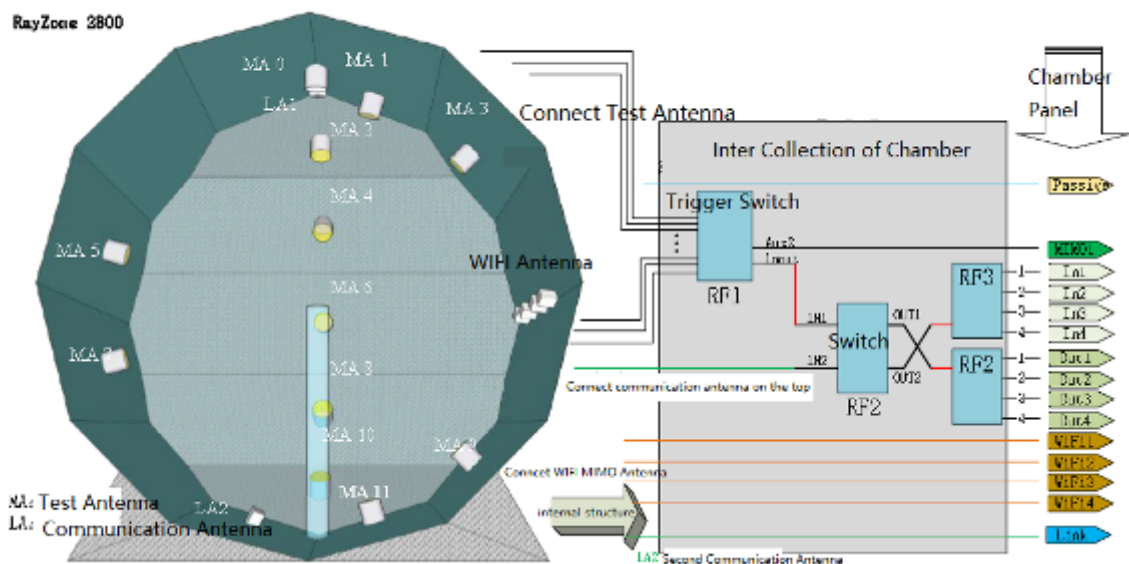


Figure 3-1 Schematic diagram of antenna near-field measurement system

The test site was a full anechoic chamber with a size of 3.0m×3.1m×2.97m, which was built by GTS Rayzone2800. All six surfaces of the anechoic chamber were pasted with absorbing materials. And the chamber was calibrated by the authoritative third-party lab every year. The antenna anechoic chamber measurement system adopted a 13-probe multi-probe system. The probe antennas were evenly distributed on the spherical surface surrounding the EUT, and their operating frequency was 600MHz~8.5GHz.

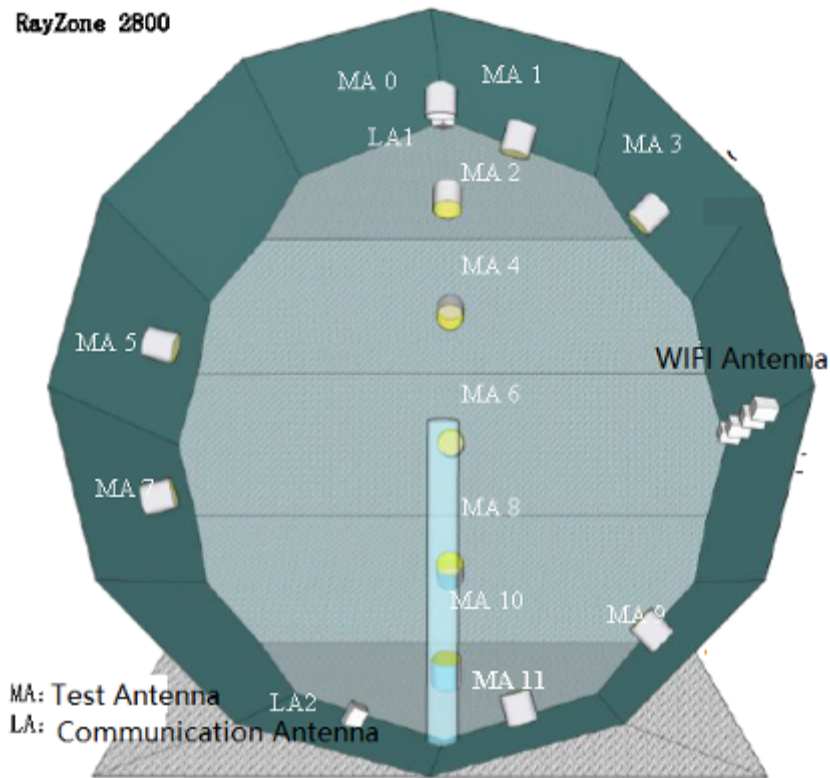


Figure 3-2 Antenna anechoic chamber for near-field measurement

During the measurement, the probe antennas were rotated in the θ direction under the control of the probe holder to sample the near-field data at the θ angle. At the same time, the EUT rotated with the turntable in the ϕ direction to sample the near field data at the ϕ angle. The system diagram was shown in Figure 3-3. From the sampling results, the EUT's near-field test data of θ component, ϕ component and total component could be obtained.

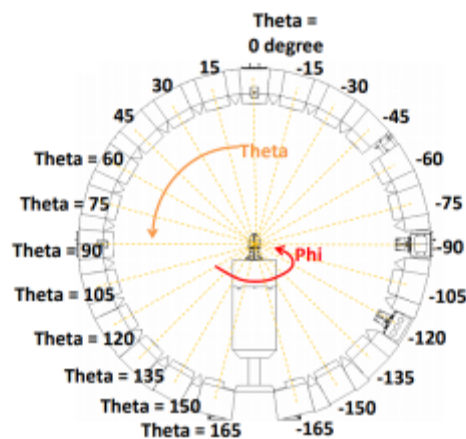


Figure 3-3 System diagram

Before the measurement, calibrated the vector network analyzer, and then connected the input end of each antenna to the output end of the vector network analyzer, and evenly the antennas to be measured. The Calibration information was shown in table 2-1.

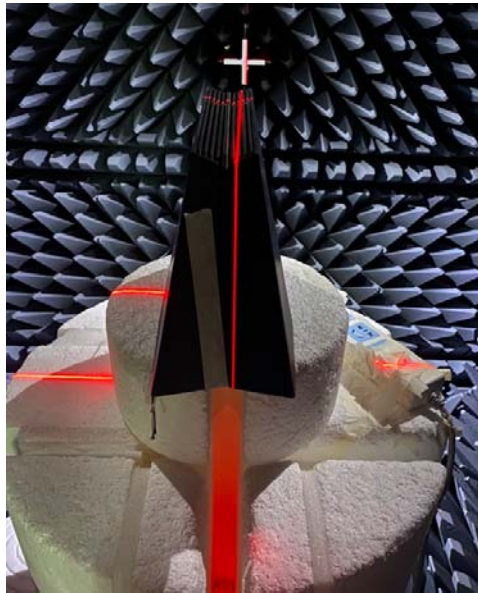


Figure 3-4 Antennas measurement diagram

Table 3-1 Calibration information

Measurement Class	Standard
Cal Type	2p/1-2
Cal Kit	N4691B

3.2 Measurement Quantity

In this measurement experiment, the Directional Gain was measured at a certain frequency interval within the whole frequency range. The measurement frequency interval of the 6G antennas was 50MHz.

3.3 Test Method

During the measurement, the probe antennas were rotated in the θ direction under the control of the probe holder to sample the near-field data at the θ angle. At the same time, the EUT rotated with the turntable in the φ direction to sample the near field data at the φ angle. The sampling accuracy was 15° . The system diagram was shown in Figure 2-6. From the sampling results, the EUT's near-field test data of θ component, φ component and total component could be obtained.

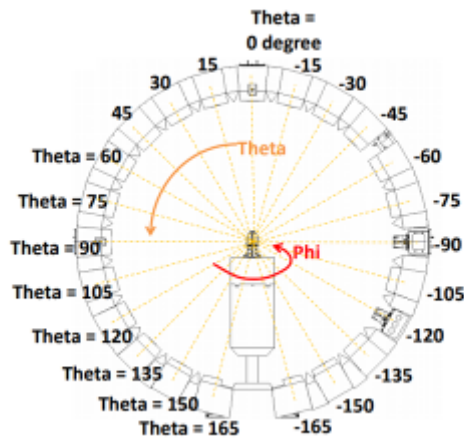


Figure 3-5 Test angle

3.4 Directional Gain Calculations

Multiple antennas system, each of which has one of two (or three) polarizations that are orthogonal to one another (i.e., cross polarized), The total gain—including array gain—is computed separately for each of the two (or three) polarizations using the procedures presented in this document. The highest of the total gains shall apply.

Theoretical Directional Gain represented the theoretical value calculated by formula 2-1. As we all know, the effect of array gain must be included in the calculation of overall directional antenna gain for devices that transmit on multiple outputs simultaneously in the same band, in the same or in overlapping frequency ranges. Therefore, in formula 2-1, the directional gain calculation needs to include all directions and all Frequencies and all Polarizations, and then take the maximum value as the final directional gain value. Therefore, the calculation formula of theoretical directional gain value can be modified as formula 2-2

$$\text{Directional Gain} = 10 \log \left[\frac{\sum_{j=1}^{N_{ANT}} (\sum_{k=1}^{N_{ANT}} g_{jk})^2}{N_{ANT}} \right] \quad (2-1)$$

Where

Nss = the number of independent spatial streams of data; NSS =1.

Nant = the total number of antennas: NANT =4 for 2.4G & 5G & 6G antennas

$g_{jk} = 10^{G_k/20}$ if the kth antenna is being fed by spatial stream j, or zero if it is not;

G_k is the gain in dBi of the kth antenna .

$$\text{Directional Gain} = \text{Maximum} \left[10 \log \left[\frac{\sum_{j=1}^{N_{ANT}} (\sum_{k=1}^{N_{ANT}} g_{jk})^2}{N_{ANT}} \right] \right] \quad (2-2)$$

Maximum function is the max directional gain overall directions and all frequency all polarizations.

3.5 Test Procedure

The calculation method of DG (Directional Gain) in this scheme is summarized as follows:

- 1) The antenna anechoic chamber is used to measure the gain of each antenna, the gain of each antenna at this angle is taken every 15° to calculate the Directional Gain;
- 2) Use formula below to calculate and the Directional Gain of the system at this angle is obtained

$$\text{Directional Gain} = 10 \log \left[\frac{\sum_{i=1}^{N_{ANT}} \sum_{\theta=1}^{N_{DIR}} G_{ANT}(\theta)}{N_{ANT}} \right] \tag{2-3}$$

- 3) For each frequency point, the Directional Gain value under 24 different angles can be obtained, and finally the maximum value is taken as the system Directional Gain value.

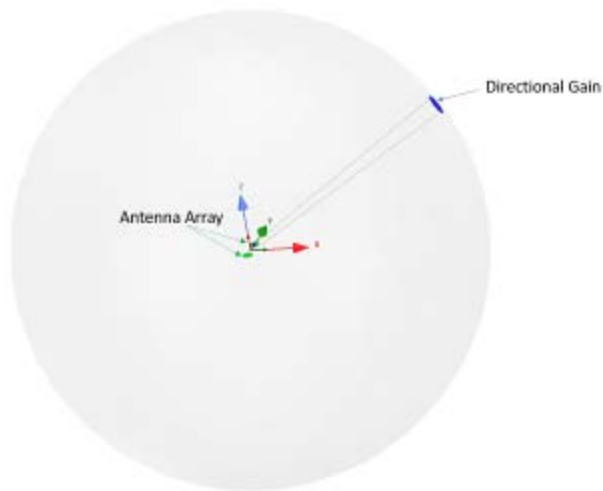


Figure 3-6 Directional Gain Calculation Sketch Map

4 Measured Value and Maximum Gain Positions

4.1 Antenna Number

The Antennas number for measured in the following section was shown below:

Table 4-1 Antennas number

Antenna Number	Antenna Position
	6G
Ant1	Ant1
Ant2	Ant2

4.2 6G

4.2.1 DG_1SS Max Value Position

Table 4-2 DG_1SS Max Value Position

Frequency(GHz)	6.175	6.475	6.725	7.025
Ant1(dBi)	0.75	2.45	2.45	2.39
Ant2(dBi)	0.17	-1.5	-1.3	-1.3
Polarization	Theta	Theta	Theta	Theta
Φ (°)	90	285	75	75
θ (°)	75	75	75	75

4.2.2 DG_1SS Max Value Position Calculation

Table 4-3 DG_1SS Max Value Position Calculation

Frequency(GHz)	6.175	6.475	6.725	7.025
Ant1[$10^{(G/20)}$]	$10^{(0.75/20)}$	$10^{(2.45/20)}$	$10^{(2.45/20)}$	$10^{(2.39/20)}$
Ant2[$10^{(G/20)}$]	$10^{(0.17/20)}$	$10^{(-1.5/20)}$	$10^{(-1.3/20)}$	$10^{(-1.3/20)}$
Ant1[$10^{(G/20)}$] value	1.09	1.326	1.326	1.317
Ant2[$10^{(G/20)}$] value	1.02	0.841	0.861	0.861
Sum of Ants Value(Antmax)	2.110	2.167	2.187	2.178
DG[$10 * \text{Log}(\text{Antmax}^2 / \text{Nant})$] (dBi)	3.475	3.708	3.786	3.750

5 Test and Calculate Result

5.1 Antenna Test Result

Table 5-1 Antenna Test Result

Frequency(GHz)	6.175	6.475	6.725	7.025
Ant1 MaxGain(dBi)	2.20	2.45	2.45	2.39
Ant2 MaxGain(dBi)	2.10	2.35	2.28	2.39
Ant1 Polarization/ Φ (°) / θ (°)	Theta/60/75	Theta/285/75	Theta/75/75	Theta/75/75
Ant2 Polarization/ Φ (°) / θ (°)	Theta/255/90	Theta/105/75	Theta/255/75	Theta/255/75
Max Gain(dBi)	2.20	2.45	2.45	2.39

5.2 Directional Gain Calculate Result

Table 5-2 Test & Calculate Result

Frequency Band(MHz)	Max Antenna Gain	Max Composite Gain	NSS	Polarization/ Φ (°) / θ (°)
5925-6425(6175)	2.20dBi	3.48dBi	1	Theta/90/75
6425-6525(6475)	2.45dBi	3.71dBi	1	Theta/285/75
6525-6875(6725)	2.45dBi	3.79dBi	1	Theta/75/75
6875-7125(7025)	2.39dBi	3.75dBi	1	Theta/75/75
5925-6425(6175)	2.20dBi	2.20dBi	2	Theta/60/75
6425-6525(6475)	2.45dBi	2.45dBi	2	Theta/285/75
6525-6875(6725)	2.45dBi	2.45dBi	2	Theta/75/75
6875-7125(7025)	2.39dBi	2.39dBi	2	Theta/75/75


Note:


1. Directional Gain(nss=2)= Directional Gain(nss=1)-6dB. If Directional Gain is less than max gain, use max gain as directional gain.

Test Pattern

5.3 Antenna Pattern

Ant1

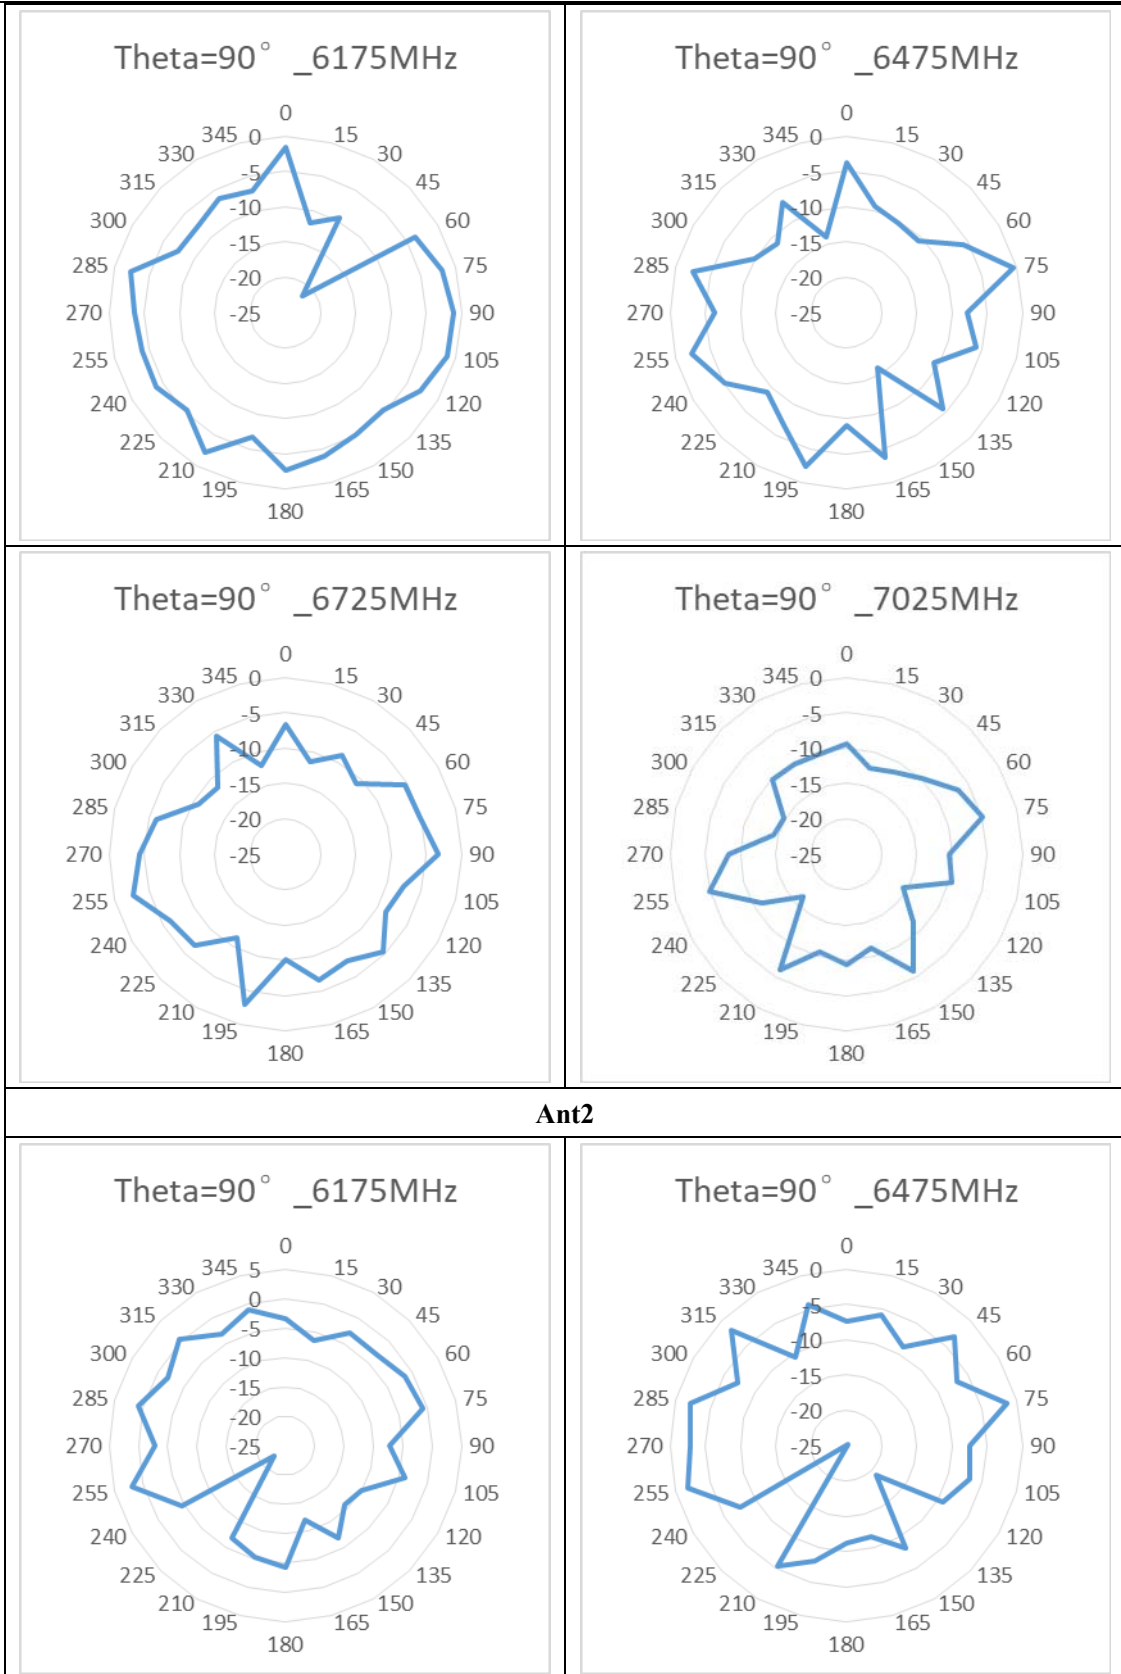

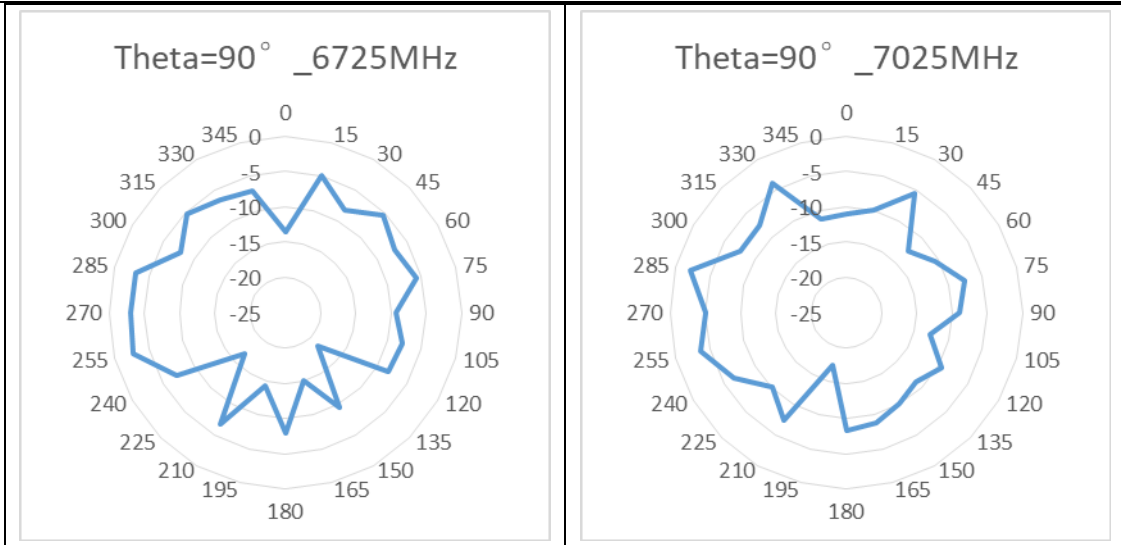

6 Test Pattern

Ant1													
Freq	6175												
Phi\Theta	0	15	30	45	60	75	90	105	120	135	150	165	180
0	-12.12	-11.27	-12.13	-4.55	-3.31	-2.87	-1.49	-7.96	-12.21	-14.71	-16.82	-21.19	-26.6
15	-11.73	-14.22	-8.6	-7.68	-8	-12.2	-11.74	-21.13	-19.85	-13.91	-18.31	-20.16	-26.6
30	-11.54	-13.97	-3.18	-6.89	-9.7	-3.76	-9.43	-10.36	-15.48	-18.62	-15.79	-23.56	-26.6
45	-11.37	-10.12	-3.02	-7.52	-6.32	-7.7	-21.59	-14.28	-21.39	-16.4	-19.05	-20.18	-26.6
60	-11.18	-8.79	-7.82	-12.75	-1.48	2.2	-3.66	-8.53	-20.19	-13.86	-18.88	-17.33	-26.6
75	-11.12	-9.31	-10.81	-12.85	-1.21	-0.11	-2.06	-6.73	-15.7	-12.79	-19.22	-17.24	-26.6
90	-11.54	-10.22	-10.79	-9.6	-0.28	0.75	-1.11	-9.01	-17.92	-13.86	-14.33	-16.77	-26.6
105	-11.5	-11.3	-11.22	-8.71	-2.92	-1.76	-1.15	-6.54	-19.87	-15.24	-14.7	-15.28	-26.6
120	-11.5	-13.23	-15.42	-7.65	-10.28	-1.15	-2.84	-13.23	-9.21	-15.05	-15.09	-14.66	-26.6
135	-11.35	-17.15	-12.97	-7.59	-9.72	-3.75	-5.5	-8.52	-12.43	-13.86	-13.5	-14.07	-26.6
150	-11.2	-21.02	-12.87	-8.68	1.19	-2.32	-5.05	-12.34	-14.12	-14.43	-17.11	-15.88	-26.6
165	-11.13	-18.65	-11.21	-6.14	-7.58	-3.4	-3.88	-6.12	-11.95	-13.67	-15.34	-19.26	-26.6
180	-11.56	-14.54	-8.93	-5.37	-0.92	-1.7	-2.58	-9.71	-12.06	-17.35	-15.9	-16.99	-26.6
195	-11.67	-11.06	-8.71	-8.83	-5.36	-4.23	-6.68	-8.05	-15.68	-13.94	-13.51	-16.4	-26.6
210	-12.1	-10.27	-9.43	-9.86	-2.68	-1.4	-2.12	-7.41	-15.96	-17.9	-13.61	-16.02	-26.6
225	-12.03	-11.21	-10.85	-8.12	-12.55	-2.08	-5.35	-5.61	-13.62	-20.79	-16.67	-12.23	-26.6
240	-11.94	-12.21	-16.08	-8.33	-6.18	-2.51	-3.82	-5.78	-10.32	-10.38	-25.6	-10.83	-26.6
255	-12.19	-11.4	-13.27	-12.93	-12.09	-4.56	-4	-3.44	-10.41	-13.88	-18.58	-12.35	-26.6
270	-12.15	-9.68	-11.29	-10.71	-7.42	-3.58	-3.56	-5.46	-11.38	-16.16	-17.01	-14.57	-26.6
285	-11.9	-8.53	-10.22	-5.66	-3.98	-0.5	-2.37	-9.08	-10.09	-12.19	-20.8	-14.02	-26.6
300	-12.15	-8.52	-9.38	-2.34	-4.5	-0.72	-7.5	-6.42	-9.13	-10.43	-18.87	-15.41	-26.6
315	-12.05	-9.97	-13.65	-4.05	-5.59	-3.53	-7.51	-12.65	-15.08	-14.34	-16.39	-19.67	-26.6
330	-11.91	-11.13	-13.37	-12	-6.45	-7.31	-6.25	-14.48	-14.02	-18.45	-15.13	-25.37	-26.6
345	-12.19	-10.92	-11.51	-5.41	-8.88	-1.67	-7.12	-11.78	-14.47	-21.62	-17.03	-26.6	-26.6



Ant2													
Freq	6175												
Phi\Theta	0	15	30	45	60	75	90	105	120	135	150	165	180
0	-15.02	-13.87	-12.3	-4.31	0.53	0.26	-3.39	-7.11	-8.59	-16.79	-15.43	-9.67	-23.16
15	-14.71	-15.6	-10.38	-10.41	-7.37	-2.52	-6.58	-8.76	-15.58	-21.63	-13.21	-11.44	-23.16
30	-15.02	-13.59	-18.15	-9.65	-3.18	-1.77	-2.89	-15.21	-11.89	-15.87	-23.09	-15.28	-23.16
45	-15.56	-11.63	-8.37	-6.77	-9.25	-2.45	-2.95	-5.4	-12.78	-12.8	-17.87	-17.35	-23.16
60	-14.97	-10.33	-9.82	-9.75	-4.14	-1.88	-1.5	-11.25	-12.01	-17.47	-15.13	-13.82	-23.16
75	-15.06	-9.81	-13.86	-17.36	-6.91	-2.27	-0.73	-7.5	-16.04	-20.28	-17.39	-15.12	-23.16
90	-15.34	-10.62	-12.89	-12.52	-4.93	0.17	-7.21	-4.84	-16.21	-15.32	-25.58	-18.97	-23.16
105	-15.01	-11.14	-8.39	-3.53	-0.59	1.46	-3.82	-7.02	-12.06	-20.34	-23.2	-14.73	-23.16
120	-15.13	-10.54	-6.03	-4.59	-3.57	-1.24	-9.94	-10.88	-17.66	-17.8	-16.96	-13.43	-23.16
135	-15.5	-10.63	-7.63	-5.4	-9.01	-8.85	-10.75	-19.59	-13.25	-20.06	-12.98	-10.48	-23.16
150	-14.99	-11.41	-9.68	-7.29	-6.77	-4.23	-6.93	-10.89	-16.59	-14.16	-11.55	-11.12	-23.16
165	-14.98	-11.53	-11.11	-8.71	-4.61	-3.55	-11.92	-10.71	-6.03	-12.8	-10.08	-15.83	-23.16
180	-15.55	-11.18	-11.45	-3.4	-5.4	-1.66	-4.17	-10.29	-12.9	-17.81	-13.59	-23.16	-23.16
195	-15.6	-12.64	-8.26	-3.67	-1.72	-4.42	-5.41	-6.99	-10.08	-19.05	-19.47	-21.75	-23.16
210	-15.58	-18.2	-6.71	-3.82	-8.28	-3.67	-6.91	-8.19	-15.78	-18.67	-17.94	-18.28	-23.16
225	-15.44	-14.67	-4.17	-5.18	-6.49	-11	-22.48	-17.26	-19.57	-20.55	-10.95	-18.5	-23.16
240	-14.83	-10.42	-5.85	-7.51	-3.72	1.2	-4.68	-9.48	-12.51	-10.96	-13.16	-13.76	-23.16
255	-15	-8.79	-9.36	-8.68	-4.33	0.44	2.1	-3.35	-14.13	-15.39	-17.54	-11.6	-23.16
270	-15.21	-8.89	-9.63	-5.94	-1.34	-0.05	-2.81	-7.41	-21.46	-17.65	-10.98	-12.26	-23.16
285	-15.26	-9.79	-9.94	-9.77	-1.25	0.41	0.93	-3.96	-22.03	-23.49	-11.7	-12.95	-23.16
300	-15.46	-10.79	-9.27	-7.95	-7.66	-1.01	-1.8	-9.85	-15.33	-13.78	-10.31	-12.23	-23.16
315	-15.5	-11.37	-8.22	-7.97	-10.73	-3.76	0.6	-2.86	-9.65	-15.87	-8.19	-12.12	-23.16
330	-14.81	-12.28	-9.36	-10.84	-0.95	-0.29	-3.14	-8.89	-9.65	-13.7	-10.3	-10.51	-23.16
345	-15.09	-12.97	-15.13	-8.32	-7.03	-3.4	-1.13	-4.96	-13.64	-14.66	-16.48	-10.49	-23.16

6175MHz Composite Gain													
Freq	6175												
Phi\Theta	0	15	30	45	60	75	90	105	120	135	150	165	180
0	-10.44	-9.46	-9.20	-1.42	1.83	1.85	0.62	-4.51	-7.20	-12.68	-13.09	-10.64	-21.70
15	-10.08	-11.87	-6.43	-5.93	-4.67	-3.07	-5.77	-9.90	-14.44	-13.93	-12.38	-11.74	-21.70
30	-10.10	-10.77	-4.76	-5.15	-2.83	0.30	-2.55	-9.44	-10.49	-14.13	-15.68	-15.46	-21.70
45	-10.20	-7.83	-2.28	-4.13	-4.65	-1.67	-5.00	-5.74	-13.05	-11.40	-15.43	-15.64	-21.70
60	-9.86	-6.52	-5.75	-8.11	0.30	3.41	0.50	-6.77	-12.16	-12.47	-13.79	-12.39	-21.70
75	-9.86	-6.55	-9.19	-11.81	-0.59	1.89	1.64	-4.10	-12.86	-12.74	-15.25	-13.11	-21.70
90	-10.22	-7.41	-8.77	-7.93	0.71	3.48	-0.62	-3.67	-14.01	-11.55	-15.24	-14.79	-21.70
105	-10.07	-8.21	-6.68	-2.73	1.33	3.01	0.63	-3.77	-12.10	-14.41	-14.94	-11.99	-21.70
120	-10.12	-8.77	-6.50	-2.98	-3.28	1.82	-2.67	-8.97	-9.44	-13.31	-12.96	-11.01	-21.70
135	-10.17	-10.28	-6.89	-3.42	-6.35	-2.92	-4.72	-9.39	-9.82	-13.41	-10.23	-9.08	-21.70
150	-9.88	-11.94	-8.12	-4.95	1.10	-0.21	-2.93	-8.57	-12.26	-11.28	-10.88	-10.17	-21.70
165	-9.83	-11.37	-8.15	-4.32	-2.96	-0.46	-3.99	-5.10	-5.48	-10.21	-9.31	-14.37	-21.70



180	-10.32	-9.69	-7.09	-1.32	0.14	1.33	-0.33	-6.98	-9.46	-14.57	-11.66	-16.53	-21.70
195	-10.40	-8.80	-5.47	-2.86	-0.34	-1.31	-3.01	-4.49	-9.43	-13.11	-12.98	-15.66	-21.70
210	-10.66	-10.35	-4.95	-3.31	-2.03	0.55	-1.18	-4.78	-12.86	-15.27	-12.50	-14.07	-21.70
225	-10.56	-9.76	-3.87	-3.52	-5.99	-2.43	-7.23	-6.60	-13.08	-17.66	-10.34	-11.80	-21.70
240	-10.26	-8.26	-6.53	-4.90	-1.85	2.55	-1.23	-4.42	-8.34	-7.65	-14.31	-9.16	-21.70
255	-10.47	-6.99	-8.09	-7.54	-4.36	1.31	2.59	-0.38	-9.06	-11.59	-15.03	-8.96	-21.70
270	-10.54	-6.27	-7.41	-4.99	-0.85	1.37	-0.17	-3.37	-12.02	-13.86	-10.47	-10.33	-21.70
285	-10.41	-6.13	-7.07	-4.46	0.50	2.98	2.45	-3.14	-11.14	-13.11	-12.10	-10.46	-21.70
300	-10.64	-6.57	-6.31	-1.69	-2.93	2.15	-1.18	-4.96	-8.68	-8.93	-10.57	-10.66	-21.70
315	-10.59	-7.63	-7.51	-2.78	-4.77	-0.63	0.47	-3.43	-8.94	-12.06	-8.35	-12.09	-21.70
330	-10.23	-8.68	-8.13	-8.39	-0.26	-0.10	-1.55	-8.23	-8.55	-12.74	-9.37	-12.08	-21.70
345	-10.51	-8.87	-10.12	-3.73	-4.90	0.52	-0.61	-4.71	-11.03	-14.45	-13.74	-12.24	-21.70

Ant1													
Freq	6475												
Phi\Theta	0	15	30	45	60	75	90	105	120	135	150	165	180
0	-21.69	-14.91	-8.58	-7.04	-7.92	0.53	-3.81	-8.73	-13.46	-17.6	-22.41	-18.34	-26.88
15	-21.97	-18.46	-13.65	-11.37	-9.06	-7.24	-9.47	-11.5	-16.42	-28.5	-24.41	-19.16	-26.88
30	-21.52	-11.91	-3.52	-8.22	-11.84	-9.13	-10.28	-15.3	-15.18	-17.58	-25.37	-23.12	-26.88
45	-20.97	-8.05	-5.57	-5.24	-5.32	-7.37	-10.63	-24.99	-18.56	-20.72	-20.2	-21.06	-26.88
60	-20.81	-7.67	-6.58	-6.55	-2.41	-2.46	-5.9	-10.86	-16.61	-21.8	-14.02	-21.67	-26.88
75	-21.03	-7.91	-7.01	-6.66	-0.84	-0.51	-0.48	-8.82	-18.29	-18.92	-13.26	-20.96	-26.88
90	-22.1	-8.7	-10.28	-9.18	-0.81	-1.63	-7.93	-10.74	-19.32	-18.38	-11.94	-23.25	-26.88
105	-21.61	-11.29	-19.02	-12.06	-3.52	-1.54	-6.02	-12.97	-20.74	-18.84	-13.5	-22.39	-26.88
120	-21.56	-14.54	-19.33	-11.62	-4.13	-5.75	-10.69	-11.05	-16.4	-15.52	-10.29	-21.04	-26.88
135	-20.98	-13.73	-12.53	-7.9	-6.23	-2.17	-5.67	-15.53	-13.76	-12.3	-11.69	-18.59	-26.88
150	-21.1	-12.76	-9.79	-3.78	-2.84	-7.25	-15.99	-10.5	-17.04	-13.37	-16.12	-16.34	-26.88
165	-22.65	-12.68	-8.7	-11.29	-2.97	-1.74	-3.69	-12.25	-15.79	-16.23	-17.88	-16.3	-26.88
180	-22.81	-12.46	-13.37	-4.7	-2.6	-3.37	-8.92	-11.6	-13.19	-18.04	-13.46	-15.06	-26.88
195	-22.83	-12.94	-8.7	-9.73	-2.81	-1.48	-2.42	-10.1	-18.48	-18.66	-17.41	-14.38	-26.88
210	-22.94	-14.06	-9.87	-5.18	-2.65	-3.76	-6.94	-12.46	-18.97	-12.75	-15.43	-15.95	-26.88
225	-23.51	-14.23	-17.77	-11.29	-6.31	-1.48	-9.12	-7.89	-10.51	-13.38	-11.78	-16.28	-26.88
240	-23.04	-12.92	-18.2	-5.04	-4.06	-2.6	-5.07	-7.02	-10.18	-15.49	-12.51	-16.29	-26.88
255	-22.25	-10.95	-17.4	-11.51	-9.49	-3.06	-2.28	-4.82	-15.36	-13.77	-19.37	-19.31	-26.88
270	-22.34	-9.53	-14.46	-14.83	-9.89	-5.44	-6.42	-5.71	-16.55	-13.49	-20.68	-20.02	-26.88
285	-23.3	-9.4	-13.56	-7.6	-3.31	2.45	-2.46	-8.21	-12.65	-12.99	-18.25	-19.43	-26.88
300	-22.88	-10.48	-11.33	-4.23	-3.6	-2.49	-9.9	-13.2	-14.67	-22.06	-23.53	-20.99	-26.88
315	-23.49	-12.71	-9.67	-5.62	-7.7	-6.46	-11.12	-16.9	-12.93	-16	-15.3	-26.88	-26.88
330	-22.59	-14.24	-12.63	-17.66	-10.63	-4.29	-6.85	-12.55	-20.11	-18.77	-12.42	-19.62	-26.88
345	-20.76	-14.75	-12.59	-10.33	-7.22	-6.21	-13.97	-19.06	-18.24	-21.81	-20.85	-19.77	-26.88

Ant2													
Freq	6475												



Phi\Theta	0	15	30	45	60	75	90	105	120	135	150	165	180
0	-17.58	-14.43	-14.86	-5.36	-3.33	-2.7	-7.29	-10.56	-14.45	-16.21	-21.61	-21.47	-25.84
15	-18.45	-15.38	-16.27	-16.65	-4.59	-3.23	-5.8	-10.09	-13.94	-22.13	-19.38	-17.9	-25.84
30	-18.94	-19.45	-11.44	-8.54	-4.68	-4.33	-8.87	-8.19	-13.66	-15.43	-20.56	-14.61	-25.84
45	-18.44	-19.93	-17.43	-13.21	-9.22	-3.31	-3.22	-12.55	-19.86	-19.81	-22.7	-15.14	-25.84
60	-18.82	-15.95	-22.11	-9.05	-4.72	-5.47	-6.92	-6.95	-20.05	-17.24	-19.17	-16.83	-25.84
75	-18.64	-13.43	-18.33	-12.01	-10.41	-2.38	-1.49	-14.17	-13.05	-16.59	-16.63	-18.71	-25.84
90	-18.57	-11.04	-15.21	-27.23	-6.86	-4.31	-7.52	-8.47	-19.52	-15.16	-19.38	-17.29	-25.84
105	-18.37	-10.06	-11.71	-9.64	-3.44	2.35	-6.9	-11.18	-13.01	-14.15	-15.89	-18.44	-25.84
120	-18.69	-11.72	-10.73	-6.44	-3.49	-2.39	-9.13	-11.74	-12.41	-17.43	-20.22	-20.29	-25.84
135	-18.27	-17.02	-10.57	-7.88	-7.56	-8.98	-19.07	-13.05	-27.34	-19	-17.19	-14.69	-25.84
150	-18.83	-20.06	-16.74	-15.18	-6.43	-2.59	-8.31	-16.48	-17.96	-26.88	-18.25	-15.73	-25.84
165	-18.59	-16.64	-14.62	-10.65	-7.06	-9.01	-11.73	-14.31	-13.32	-21.07	-18.39	-22.96	-25.84
180	-18.03	-14.39	-20.08	-8.31	-7.01	-3.81	-11.11	-10.29	-15.37	-17.41	-20.86	-25.84	-25.84
195	-17.64	-15.67	-17.12	-8.53	-8.4	-4.28	-8.01	-13.91	-19.06	-18.37	-22.7	-22.85	-25.84
210	-18.02	-16.72	-7.39	-7.35	-7.47	-7.47	-5.33	-10.48	-21.18	-19.12	-22.05	-20.75	-25.84
225	-18.1	-12.27	-7.29	-6.97	-8.81	-7.8	-25.29	-20.74	-14.52	-15.88	-13.67	-19.44	-25.84
240	-17.89	-10.95	-8.52	-8.79	-4.95	-2.48	-7.64	-9.45	-18.17	-14.15	-29.07	-14.93	-25.84
255	-17.36	-12.51	-9.8	-12.78	-4.1	-0.69	-1.74	-4.39	-14.84	-19.06	-16.03	-15.52	-25.84
270	-17.14	-14.12	-11.19	-17.64	-4.27	-1.25	-2.82	-5.54	-15.31	-19.52	-15.61	-20.32	-25.84
285	-17.71	-14.4	-15.06	-22.62	-6.14	-1.5	-2.02	-6.65	-15.8	-13.03	-18.36	-21.51	-25.84
300	-18.24	-14.53	-18.73	-16.97	-8.06	-5.12	-7.18	-11.14	-14.27	-14.17	-19.13	-16.48	-25.84
315	-18.25	-15.31	-15.4	-9.33	-10.1	-1.57	-1.82	-12.45	-17.88	-16.01	-14.52	-14.22	-25.84
330	-17.88	-17.52	-9.2	-8.73	-3.84	-8.54	-10.55	-10.91	-15.48	-15.01	-10.19	-13.99	-25.84
345	-17.39	-16.65	-8.7	-11.3	-2.49	-1.16	-4.28	-11.27	-17.71	-13.56	-15.22	-16.24	-25.84

6475MHz Composite Gain													
Freq	6475												
Phi\Theta	0	15	30	45	60	75	90	105	120	135	150	165	180
0	-16.38	-11.66	-8.15	-3.15	-2.31	2.07	-2.37	-6.59	-10.93	-13.87	-18.99	-16.75	-23.33
15	-17.02	-13.77	-11.85	-10.60	-3.53	-2.00	-4.43	-7.76	-12.08	-21.73	-18.53	-15.50	-23.33
30	-17.12	-11.88	-3.60	-5.37	-4.53	-3.39	-6.54	-8.03	-11.38	-13.43	-19.63	-14.85	-23.33
45	-16.60	-9.09	-6.61	-5.33	-4.04	-2.09	-3.15	-13.70	-16.18	-17.24	-18.35	-14.59	-23.33
60	-16.75	-7.85	-8.25	-4.70	-0.48	-0.82	-3.38	-5.68	-15.15	-16.21	-13.21	-15.91	-23.33
75	-16.74	-7.23	-7.93	-5.92	-1.36	1.62	2.04	-8.08	-12.27	-14.67	-11.77	-16.75	-23.33
90	-17.15	-6.78	-9.39	-11.17	-0.31	0.14	-4.71	-6.52	-16.41	-13.61	-11.88	-16.76	-23.33
105	-16.83	-7.64	-11.61	-7.76	-0.47	3.63	-3.44	-9.02	-13.03	-13.17	-11.60	-17.18	-23.33
120	-17.00	-10.01	-11.00	-5.64	-0.79	-0.90	-6.86	-8.38	-11.17	-13.41	-10.90	-17.65	-23.33
135	-16.51	-12.21	-8.48	-4.88	-3.86	-1.91	-7.00	-11.19	-15.12	-12.01	-11.00	-13.41	-23.33
150	-16.88	-12.65	-9.58	-4.72	-1.44	-1.60	-8.32	-9.97	-14.48	-14.72	-14.11	-13.02	-23.33
165	-17.37	-11.43	-8.15	-7.95	-1.77	-1.63	-3.80	-10.21	-11.46	-15.31	-15.12	-16.00	-23.33
180	-17.08	-10.36	-13.08	-3.31	-1.52	-0.58	-6.94	-7.91	-11.20	-14.71	-13.38	-15.86	-23.33
195	-16.84	-11.19	-8.92	-6.10	-2.15	0.24	-1.76	-8.79	-15.75	-15.50	-16.65	-14.61	-23.33



210	-17.13	-12.28	-5.53	-3.19	-1.72	-2.41	-3.09	-8.40	-16.99	-12.35	-15.11	-15.01	-23.33
225	-17.38	-10.18	-8.03	-5.85	-4.46	-1.07	-10.88	-9.12	-9.28	-11.53	-9.66	-14.71	-23.33
240	-17.08	-8.87	-9.07	-3.70	-1.48	0.47	-3.25	-5.14	-10.28	-11.78	-14.32	-12.57	-23.33
255	-16.46	-8.68	-9.78	-9.11	-3.37	1.22	1.00	-1.59	-12.09	-13.01	-14.53	-14.20	-23.33
270	-16.35	-8.51	-9.66	-13.11	-3.62	-0.08	-1.42	-2.61	-12.90	-12.98	-14.77	-17.16	-23.33
285	-17.05	-8.53	-11.27	-9.19	-1.60	3.71	0.77	-4.38	-11.07	-10.00	-15.29	-17.40	-23.33
300	-17.24	-9.26	-11.25	-5.44	-2.54	-0.70	-5.42	-9.10	-11.46	-14.24	-18.04	-15.44	-23.33
315	-17.47	-10.90	-9.06	-4.27	-5.81	-0.67	-2.27	-11.38	-12.05	-12.99	-11.89	-15.41	-23.33
330	-16.91	-12.72	-7.74	-9.08	-3.58	-3.15	-5.49	-8.68	-14.48	-13.68	-8.22	-13.35	-23.33
345	-15.90	-12.64	-7.42	-7.79	-1.53	-0.31	-4.83	-11.31	-14.96	-13.73	-14.58	-14.82	-23.33

Ant1													
Freq	6725												
Phi\Theta	0	15	30	45	60	75	90	105	120	135	150	165	180
0	-15.93	-16.26	-9.41	-5.96	-5.13	-0.65	-6.62	-9.02	-12.89	-14.82	-22.31	-17.92	-24.35
15	-16.61	-17.23	-6.63	-9.12	-9.38	-4.12	-11.37	-10.91	-13.63	-20.4	-26.6	-21.35	-24.35
30	-16.39	-8.53	-4.63	-6.38	-10.24	-11.51	-8.77	-18.33	-27.92	-17.9	-20.03	-21.84	-24.35
45	-16.57	-6.68	-6.86	-7.98	-5.6	-4.78	-10.82	-17.99	-15.19	-19.9	-16.54	-18.54	-24.35
60	-16.17	-8.64	-5.75	-7.91	-0.7	-3.01	-5.34	-9.73	-26.55	-14.12	-22.32	-18.97	-24.35
75	-15.6	-12.73	-8.92	-9.87	-1.65	2.45	-5.09	-9.43	-13.81	-17.63	-25.43	-19.92	-24.35
90	-15.89	-17.63	-11.39	-10.72	-4.37	-0.47	-3.26	-14.84	-12.62	-15.82	-22.9	-15.88	-24.35
105	-17.19	-19.51	-13.98	-11.19	-4.28	-1.86	-7.68	-12.27	-11.66	-10.69	-24.35	-15.11	-24.35
120	-16.59	-15.83	-17.7	-17.87	-5.29	-5.35	-8.63	-17.26	-7.76	-11.45	-17.08	-17.63	-24.35
135	-16.58	-12.76	-14.01	-10.82	-2.93	-1.55	-5.49	-17.23	-11.42	-20.54	-14.39	-17.3	-24.35
150	-15.83	-11.58	-12.1	-1.9	-3.66	-5.35	-7.49	-14.49	-13.12	-13.37	-13.32	-19.42	-24.35
165	-15.34	-11.39	-8.38	-9.77	-1.11	-1.8	-6.51	-14.52	-12.28	-15.3	-15.28	-21.88	-24.35
180	-15.47	-11.19	-10.52	-4.36	-3.58	-5.1	-10.02	-13.71	-13.37	-14.43	-17.53	-20.91	-24.35
195	-16.57	-12.36	-16.1	-9.9	-1.21	-0.62	-3.03	-13.67	-23.18	-16.85	-14.88	-17.35	-24.35
210	-15.83	-15.25	-13.39	-4.46	-1.78	-3.45	-11.43	-18.13	-21.53	-18.19	-17.03	-16.93	-24.35
225	-14.9	-18.21	-10.73	-9.33	-4.37	-2.55	-6.81	-16.99	-11.1	-14.67	-15.83	-15.22	-24.35
240	-14.38	-16.64	-14.66	-8.74	-3.18	-2.16	-6.09	-13.34	-16.58	-12.83	-13.83	-13.42	-24.35
255	-14.8	-15.11	-16.73	-12.35	-5.02	-3.63	-2.61	-10.97	-12.19	-14.72	-15.23	-15.24	-24.35
270	-15.51	-14.28	-14.07	-13.3	-18.38	-9.27	-4.42	-6.7	-12.71	-15.51	-16.99	-20.42	-24.35
285	-16.06	-13.41	-13.94	-8.47	-3.67	0.82	-6.11	-9.13	-15.4	-16.12	-16.49	-23.1	-24.35
300	-15.66	-13.06	-10.77	-4.88	-4.08	-2.58	-10.73	-12.56	-12.98	-17.64	-16.23	-18.1	-24.35
315	-14.9	-15.48	-9.94	-5.42	-6.52	-8.55	-11.53	-15.32	-20.72	-16.17	-14.65	-16.43	-24.35
330	-14.61	-21.92	-20.83	-13.05	-5.58	-2.76	-5.64	-14.72	-14.1	-18.53	-14.94	-19.05	-24.35
345	-15.04	-16.59	-14.88	-7.72	-9.19	-14.01	-11.92	-21.36	-16.21	-21.33	-23.32	-24.35	-24.35

Ant2													
Freq	6725												
Phi\Theta	0	15	30	45	60	75	90	105	120	135	150	165	180
0	-17.27	-16.41	-13.84	-6.01	-5.02	-6.2	-13.56	-15.29	-18.46	-13.1	-13.46	-10.52	-33.23



15	-17.14	-16.62	-18.01	-10.8	-2.11	-2.44	-4.88	-10.58	-14.88	-13.28	-24.48	-14.86	-33.23
30	-17.82	-16.51	-16.21	-9.19	-5.83	-7.81	-8.17	-13.46	-16.04	-18.12	-23.22	-20.55	-33.23
45	-17.66	-15.99	-14.7	-7.64	-5.18	-2.58	-5.46	-19.41	-17.94	-21.72	-19.42	-17.36	-33.23
60	-16.31	-14.2	-18.05	-13.27	-7.99	-6.51	-7.11	-13.82	-14.45	-20.92	-22.09	-18.81	-33.23
75	-15.95	-13.02	-22.87	-10.25	-8.19	-1.3	-5.83	-19.04	-18.98	-18.06	-21.3	-21.46	-33.23
90	-16.6	-12.75	-18.17	-16.29	-7.92	-8.43	-9.29	-17.18	-15.58	-14.11	-18.87	-18.78	-33.23
105	-17.04	-12.94	-11.95	-6.95	-1.97	0.39	-7.9	-12.24	-12.73	-13.89	-20.17	-16.25	-33.23
120	-17.6	-14.7	-11.7	-4.01	-1.12	-2.88	-8.12	-15.57	-16.71	-19.62	-16.28	-21.73	-33.23
135	-17.72	-17.07	-14.98	-7.24	-9.31	-16.9	-18.43	-13.42	-15.63	-14.46	-22.82	-22.89	-33.23
150	-16.43	-19.51	-17.64	-10.55	-5.33	-2.08	-9.57	-17.44	-20.19	-26.41	-20.17	-18.33	-33.23
165	-16.32	-18.16	-20.41	-12.08	-11.19	-16.34	-15.09	-17.58	-18.58	-23.01	-22.84	-19.1	-33.23
180	-16.97	-15.52	-16.51	-7.72	-5.31	-8.45	-7.9	-11.72	-12.49	-19.98	-20.95	-20.66	-33.23
195	-16.83	-19.07	-11.02	-10.1	-5.66	-4.37	-14.23	-22.9	-18.05	-19.12	-23.32	-17.93	-33.23
210	-16.58	-18.2	-9.2	-7.98	-8.79	-5.75	-6.67	-12.96	-12.83	-14.86	-19.76	-16.53	-33.23
225	-16.66	-12.92	-8.01	-8.26	-7.51	-7.41	-16.82	-13.47	-17.19	-10.8	-23.5	-22.33	-33.23
240	-16.67	-12.07	-5.75	-7.34	-4.27	-2.43	-7.3	-12.02	-14.82	-15.37	-12.68	-29.43	-33.23
255	-17.34	-12.95	-7.49	-10.35	-4.49	2.28	-2.64	-10.04	-14.38	-19.78	-14.49	-33.23	-33.23
270	-17.71	-14.3	-12.02	-14.57	-4.56	-0.02	-3.04	-12.45	-19.55	-14.46	-14.4	-24.47	-33.23
285	-16.93	-16.16	-20.11	-17.12	-5.43	-1.08	-3.1	-9.74	-13.01	-10.89	-13.22	-23.38	-33.23
300	-16.76	-18.25	-24.98	-17.26	-6.72	-7.61	-7.9	-14.1	-12	-11.03	-10.41	-21.71	-33.23
315	-16.62	-18.59	-20.02	-12.32	-4.84	-1.15	-5.24	-21.19	-16.64	-11.34	-14.84	-19.51	-33.23
330	-16.55	-17.36	-12.23	-5.67	-7.13	-10.42	-6.57	-15.99	-15.72	-13.69	-17.58	-18.36	-33.23
345	-16.87	-16.57	-8.84	-10.71	-0.18	-1.59	-7.05	-17.24	-9.38	-15.33	-15.58	-11.92	-33.23

6725MHz Composite Gain													
Freq	6725												
Phi\Theta	0	15	30	45	60	75	90	105	120	135	150	165	180
0	-13.56	-13.32	-8.34	-2.97	-2.06	0.02	-6.40	-8.59	-12.23	-10.91	-13.79	-10.44	-24.69
15	-13.86	-13.91	-7.57	-6.91	-2.00	-0.23	-4.52	-7.73	-11.22	-13.12	-22.47	-14.50	-24.69
30	-14.07	-8.62	-5.61	-4.66	-4.75	-6.45	-5.45	-12.55	-17.08	-15.00	-18.47	-18.16	-24.69
45	-14.09	-7.13	-6.91	-4.80	-2.38	-0.60	-4.72	-15.66	-13.45	-17.75	-14.85	-14.92	-24.69
60	-13.23	-7.97	-6.87	-7.17	-0.59	-1.57	-3.17	-8.53	-15.53	-13.86	-19.19	-15.88	-24.69
75	-12.76	-9.86	-10.34	-7.05	-1.31	3.79	-2.44	-9.96	-13.01	-14.83	-20.11	-17.65	-24.69
90	-13.23	-11.84	-11.12	-10.06	-2.95	-0.56	-2.75	-12.92	-10.96	-11.91	-17.64	-14.20	-24.69
105	-14.10	-12.61	-9.90	-5.80	-0.04	2.35	-4.78	-9.24	-9.17	-9.13	-19.00	-12.65	-24.69
120	-14.07	-12.24	-11.18	-5.42	0.05	-1.02	-5.36	-13.36	-8.12	-11.60	-13.66	-16.43	-24.69
135	-14.12	-11.64	-11.47	-5.84	-2.54	-3.19	-6.73	-12.11	-10.26	-13.97	-14.61	-16.64	-24.69
150	-13.11	-11.66	-11.43	-2.18	-1.44	-0.55	-5.46	-12.83	-12.94	-14.63	-13.08	-15.85	-24.69
165	-12.81	-11.12	-9.45	-7.84	-1.75	-3.32	-6.77	-12.91	-11.86	-15.32	-15.25	-17.37	-24.69
180	-13.18	-10.08	-10.00	-2.87	-1.39	-3.60	-5.89	-9.65	-9.91	-13.76	-16.06	-17.77	-24.69
195	-13.69	-12.07	-10.18	-6.99	-0.14	0.72	-3.93	-14.10	-17.23	-14.90	-15.10	-14.62	-24.69
210	-13.19	-13.59	-8.03	-3.03	-1.59	-1.51	-5.72	-12.16	-13.12	-13.36	-15.28	-13.72	-24.69
225	-12.73	-12.16	-6.25	-5.77	-2.79	-1.63	-7.44	-12.04	-10.61	-9.51	-15.83	-15.06	-24.69



240	-12.44	-11.05	-6.10	-5.00	-0.70	0.72	-3.66	-9.64	-12.65	-11.00	-10.23	-15.15	-24.69
255	-12.97	-10.95	-7.92	-8.28	-1.74	2.83	0.39	-7.48	-10.21	-13.88	-11.84	-17.22	-24.69
270	-13.53	-11.28	-9.97	-10.90	-5.96	-0.46	-0.69	-6.10	-12.46	-11.96	-12.59	-19.20	-24.69
285	-13.47	-11.67	-13.48	-8.75	-1.50	2.93	-1.46	-6.42	-11.11	-10.11	-11.69	-20.23	-24.69
300	-13.18	-12.26	-12.23	-6.02	-2.29	-1.73	-6.19	-10.29	-9.47	-10.71	-9.83	-16.71	-24.69
315	-12.71	-13.89	-10.58	-5.19	-2.63	-1.07	-4.82	-14.76	-15.43	-10.41	-11.73	-14.82	-24.69
330	-12.52	-16.33	-12.50	-5.59	-3.31	-2.76	-3.08	-12.32	-11.86	-12.77	-13.15	-15.69	-24.69
345	-12.90	-13.57	-8.33	-6.08	-0.56	-2.74	-6.14	-16.05	-9.13	-14.81	-15.60	-13.07	-24.69

Ant1													
Freq	7025												
Phi\Theta	0	15	30	45	60	75	90	105	120	135	150	165	180
0	-15.47	-23.32	-8.89	-4.33	-4.98	-2.2	-9.34	-18.05	-16.96	-21.8	-27.22	-23.71	-23.71
15	-15.06	-14.24	-8.07	-10.46	-7.72	-4.3	-12.3	-11.68	-26.07	-18.1	-16.4	-18.75	-23.71
30	-15.24	-10.12	-5.02	-6.34	-8.38	-11.48	-11.55	-25.99	-15.66	-22.05	-17.06	-15.65	-23.71
45	-15.41	-9.94	-4.72	-5.95	-2.98	-5.24	-9.78	-14.65	-19.67	-16.33	-18.12	-14.21	-23.71
60	-16.04	-9.85	-8.67	-6.64	-1.01	-1.75	-6.72	-21.09	-15.16	-13.62	-14.61	-14.51	-23.71
75	-16.73	-9.49	-8.69	-8.84	-2.63	2.39	-4.91	-15.98	-18.68	-12.3	-14.44	-16.14	-23.71
90	-15.88	-9.86	-9.15	-5.8	-2.12	0.26	-10.4	-23.41	-10.36	-12.74	-11.27	-15.68	-23.71
105	-16.25	-10.58	-17.08	-8.15	-3.09	-7.28	-9.51	-11.65	-10.15	-10.37	-10.54	-15.71	-23.71
120	-15.62	-10.84	-13.83	-15.17	-6.4	-8.36	-15.62	-10.38	-8.66	-9.3	-11.57	-16.16	-23.71
135	-15.59	-12.5	-7.43	-12.28	-3.36	-2.17	-11.44	-9.18	-6.35	-10.26	-14.09	-13.25	-23.71
150	-16.07	-14.09	-8.86	-2.75	-4.25	-4.23	-5.91	-10.73	-10.96	-11.88	-12.08	-13.7	-23.71
165	-16.42	-16.81	-9.8	-5.36	-0.7	-4.97	-11.23	-9.61	-8.86	-9.48	-9.95	-12.81	-23.71
180	-15.34	-21.31	-13.24	-7.92	-4.95	-8.03	-9.32	-14.95	-18.1	-15.33	-16.63	-14.3	-23.71
195	-16.35	-13.43	-18.98	-3.69	-0.64	-1.81	-10.62	-12.02	-13.54	-9.73	-15.24	-15.45	-23.71
210	-15.77	-12.84	-13.21	-7.69	-4.3	-2.97	-6.07	-12.55	-12.77	-20.64	-16.35	-15.46	-23.71
225	-16.11	-17.16	-13.19	-5.12	-2.97	-4.99	-16.45	-9.1	-10.97	-9.75	-16.87	-16.19	-23.71
240	-15.88	-17.87	-15.81	-11.66	-6.45	-5.39	-11.3	-8.32	-9.68	-9.23	-13.86	-16.52	-23.71
255	-15.44	-14.01	-17.44	-15.64	-7.11	-4.73	-4.88	-13.23	-9.3	-12.76	-13.43	-15.8	-23.71
270	-14.98	-13.41	-15.45	-8.68	-9.15	-6.85	-8.29	-13.49	-9.87	-14.34	-17.52	-17.41	-23.71
285	-15.13	-14.22	-13.78	-5.4	-1.22	-0.84	-14.3	-15.45	-13.93	-16.56	-22.76	-20.38	-23.71
300	-15.37	-13.08	-11.1	-3.83	-0.78	-1.8	-14.82	-21.49	-9.96	-17.35	-18.78	-20.09	-23.71
315	-15.92	-12.63	-10.23	-4.04	-10.18	-19.65	-10.16	-19.04	-19.58	-16.16	-16.08	-17.05	-23.71
330	-15.84	-13.71	-13.24	-7.77	-2.34	-3.88	-10.39	-11.91	-19.81	-18.4	-19.67	-17.58	-23.71
345	-15.68	-16.23	-24.1	-12.12	-9.75	-11.42	-10.37	-11.3	-16.16	-14.89	-15.05	-23.35	-23.71

Ant2													
Freq	7025												
Phi\Theta	0	15	30	45	60	75	90	105	120	135	150	165	180
0	-18.81	-20.99	-9.71	-5.61	-4.76	-8.13	-11.09	-14.37	-9.04	-8.47	-12.86	-10.01	-27.67
15	-17.42	-20.88	-11.13	-4.17	-0.17	-2.52	-9.87	-13.21	-17.39	-10.43	-11.38	-12.52	-27.67
30	-17.6	-18.78	-10.16	-9.09	-5.58	-3.24	-5.54	-17.61	-12.89	-16.77	-15.92	-15.96	-27.67



45	-17.41	-16.16	-10.61	-3.97	-1.74	-2.75	-12.56	-7.63	-13.87	-15.87	-13.42	-17.99	-27.67
60	-17.75	-15.13	-15.89	-7.47	-5.62	-3.87	-10.41	-10.98	-8.84	-13.58	-15.1	-17.39	-27.67
75	-17.64	-14.44	-14.02	-11.65	-6.28	-1.3	-7.71	-9.51	-8.08	-23.45	-17.2	-16.66	-27.67
90	-18.62	-16.9	-12.53	-10.6	-8.11	-4.33	-8.99	-11.51	-18.81	-11.55	-17.76	-12.45	-27.67
105	-18.48	-18.12	-11.31	-5.81	0.82	-0.36	-12.79	-12.6	-11.27	-15.98	-19.12	-13.11	-27.67
120	-18.87	-14.03	-8.5	-0.74	0	-4.01	-9.34	-17.99	-10.86	-16.84	-19.67	-18.95	-27.67
135	-18.83	-11.21	-11.5	-6.2	-7.78	-14.93	-11.07	-15.24	-13.87	-13.96	-22.53	-20.87	-27.67
150	-18.6	-13.44	-12.94	-8.03	-2.29	-1.72	-10.02	-20.52	-15.67	-14.72	-14.24	-22.37	-27.67
165	-18.3	-15.73	-25.08	-8.71	-5.69	-10.75	-8.76	-16.05	-15.71	-19.55	-24.62	-19.5	-27.67
180	-18.68	-15.17	-17.05	-5.35	-4.82	-5.23	-8.33	-9.65	-24.16	-19.66	-19.7	-19.42	-27.67
195	-18.45	-16.25	-9.93	-8.82	-2.04	-8.32	-17.25	-14.91	-11.82	-16.99	-20.38	-16.14	-27.67
210	-18.53	-12.67	-9.85	-6.52	-6.47	-4.02	-7.33	-12.87	-7.24	-9.2	-15.76	-13.12	-27.67
225	-17.85	-10.3	-6.09	-8.24	-3.66	-6.19	-10.08	-16.57	-13.45	-8.64	-20	-14.45	-27.67
240	-17.6	-10.48	-6.71	-5.86	-1.87	0.57	-6.57	-20.58	-11.01	-6.88	-10.82	-19.43	-27.67
255	-18.39	-11.77	-9.98	-9.8	-1.2	2.39	-3.65	-10.12	-9.84	-11.91	-13.15	-27.67	-27.67
270	-18.87	-12.29	-15.27	-11.6	-2.69	-1.07	-5.06	-15.9	-8.24	-8.22	-11.8	-18.6	-27.67
285	-17.4	-12.82	-13.33	-6.41	-4.86	-1.78	-2.04	-13.46	-6.11	-7.38	-12.06	-20.47	-27.67
300	-17.34	-13.87	-13.18	-8.74	-8.92	-8.07	-7.68	-8.05	-7.4	-5.86	-9.01	-21.59	-27.67
315	-16.68	-14.59	-12.85	-10.51	-2	-2.83	-7.56	-9.87	-9.43	-9.3	-9.46	-16.15	-27.67
330	-16.91	-16.13	-12.1	-3.67	-5.45	-2.93	-3.89	-12.11	-8.81	-7.69	-9.33	-15.75	-27.67
345	-17.73	-19.37	-6.84	-5.31	0.6	-3.07	-11.22	-10.51	-7.33	-8.63	-11.05	-10.55	-27.67

7025MHz Composite Gain													
Freq	7025												
Phi\Theta	0	15	30	45	60	75	90	105	120	135	150	165	180
0	-13.97	-19.07	-6.28	-1.94	-1.86	-1.66	-7.16	-13.01	-9.12	-9.79	-14.35	-11.39	-22.46
15	-13.15	-13.93	-6.46	-3.75	-0.14	-0.35	-7.99	-9.40	-17.68	-10.43	-10.52	-12.08	-22.46
30	-13.33	-10.40	-4.20	-4.60	-3.86	-3.41	-5.02	-17.82	-11.15	-16.00	-13.46	-12.79	-22.46
45	-13.34	-9.49	-4.16	-1.89	0.67	-0.90	-8.05	-7.44	-13.28	-13.09	-12.45	-12.89	-22.46
60	-13.84	-9.08	-8.54	-4.03	0.00	0.26	-5.36	-11.63	-8.43	-10.59	-11.84	-12.82	-22.46
75	-14.16	-8.61	-7.94	-7.12	-1.25	3.75	-3.19	-9.15	-8.84	-13.19	-12.70	-13.39	-22.46
90	-14.13	-9.68	-7.67	-4.86	-1.60	1.28	-6.66	-12.55	-10.59	-9.11	-10.91	-10.91	-22.46
105	-14.28	-10.55	-10.71	-3.89	2.09	-0.14	-7.99	-9.10	-7.68	-9.72	-10.80	-11.30	-22.46
120	-14.08	-9.28	-7.75	-2.24	0.39	-2.91	-8.91	-10.37	-6.68	-9.27	-11.70	-14.43	-22.46
135	-14.05	-8.82	-6.22	-5.71	-2.28	-3.38	-8.24	-8.68	-6.31	-8.90	-14.31	-13.24	-22.46
150	-14.23	-10.75	-7.65	-1.98	-0.20	0.13	-4.71	-11.30	-9.99	-10.17	-10.08	-13.99	-22.46
165	-14.30	-13.24	-11.43	-3.86	0.17	-4.38	-6.90	-9.24	-8.62	-10.12	-11.49	-12.52	-22.46
180	-13.84	-14.70	-11.93	-3.53	-1.87	-3.51	-5.80	-8.89	-17.60	-14.22	-15.02	-13.48	-22.46
195	-14.33	-11.72	-10.32	-2.87	1.70	-1.46	-10.31	-10.34	-9.63	-9.61	-14.42	-12.78	-22.46
210	-14.03	-9.74	-8.36	-4.08	-2.31	-0.47	-3.67	-9.70	-6.56	-10.15	-13.04	-11.20	-22.46
225	-13.93	-10.06	-5.92	-3.53	-0.30	-2.56	-9.68	-9.05	-9.11	-6.17	-15.28	-12.27	-22.46
240	-13.69	-10.40	-7.11	-5.27	-0.85	1.10	-5.61	-9.44	-7.31	-4.97	-9.20	-14.84	-22.46
255	-13.78	-9.81	-9.92	-9.23	-0.65	2.55	-1.23	-8.53	-6.56	-9.31	-10.28	-16.84	-22.46

270	-13.70	-9.82	-12.35	-7.01	-2.32	-0.48	-3.52	-11.60	-6.01	-7.74	-11.19	-14.97	-22.46
285	-13.18	-10.48	-10.54	-2.88	0.16	1.71	-3.16	-11.39	-6.16	-7.80	-12.85	-17.41	-22.46
300	-13.29	-10.46	-9.07	-2.93	-0.92	-1.37	-7.53	-9.38	-5.58	-6.82	-9.58	-17.80	-22.46
315	-13.28	-10.54	-8.43	-3.68	-2.15	-4.67	-5.75	-10.29	-10.09	-9.06	-9.14	-13.58	-22.46
330	-13.35	-11.83	-9.64	-2.47	-0.75	-0.38	-3.54	-9.00	-9.66	-8.48	-10.03	-13.61	-22.46
345	-13.63	-14.65	-8.73	-5.05	-0.11	-3.27	-7.77	-7.89	-7.66	-8.20	-9.81	-11.77	-22.46