

## Appendix C for KSCR231000179101

## Calibration Certificate

Object	Apply	No	Model	SN	Calibration Date	Due date of calibration
Dipole	<input type="checkbox"/>	1	CLA150	4025	2021/04/26	2024/04/25
	<input type="checkbox"/>	2	D450V3	1103	2021/04/21	2024/04/20
	<input type="checkbox"/>	3	D750V3	1188	2022/03/29	2025/03/28
	<input type="checkbox"/>	4	D835V2	4d114	2022/03/31	2025/03/30
	<input type="checkbox"/>	5	D900V2	1d079	2022/06/07	2025/06/06
	<input type="checkbox"/>	6	D1800V2	2d170	2022/03/31	2025/03/30
	<input type="checkbox"/>	7	D1900V2	5d136	2022/06/07	2025/06/06
	<input type="checkbox"/>	8	D2000V2	1041	2022/06/06	2025/06/05
	<input type="checkbox"/>	9	D2300V2	1096	2022/03/31	2025/03/30
	<input checked="" type="checkbox"/>	10	D2450V2	817	2022/04/01	2025/03/31
	<input type="checkbox"/>	11	D2600V2	1158	2022/03/31	2025/03/30
	<input checked="" type="checkbox"/>	12	D5GHzV2	1095	2022/06/01	2025/05/31
DAE	<input checked="" type="checkbox"/>	13	DAE4	1245	2023/04/25	2024/04/24
Probe	<input checked="" type="checkbox"/>	14	EX3DV4	7767	2022/10/28	2023/10/27

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.Doccheck@sgs.com](mailto:CN.Doccheck@sgs.com)

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300  
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 [www.sgsgroup.com.cn](http://www.sgsgroup.com.cn)  
t(86-512)57355888 f(86-512)57370818 [sgs.china@sgs.com](mailto:sgs.china@sgs.com)



# 1 Dipole

## 1.1 CLA150 - SN 4025

<p><b>Calibration Laboratory of</b> Schmid &amp; Partner Engineering AG Zürcherstrasse 45, 8004 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Client SGS-CN (Auden) Certificate No: CLA150-4025_Apr21</p> <p><b>CALIBRATION CERTIFICATE</b></p> <table border="1"> <tr> <td>Object</td> <td>CLA150 - SN: 4025</td> </tr> <tr> <td>Calibration procedure</td> <td>QA CAL-15.v9 Calibration Procedure for SAR Validation Sources below 700 MHz</td> </tr> <tr> <td>Calibration date</td> <td>April 26, 2021</td> </tr> <tr> <td colspan="2">This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</td> </tr> <tr> <td colspan="2">All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity &lt; 70%.</td> </tr> <tr> <td colspan="2">Calibration Equipment used (MATE: critical for calibration)</td> </tr> <tr> <td colspan="2"> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter NRP</td> <td>SN: 104/78</td> <td>09-Apr-21 (No. 217-03291/03292)</td> <td>Apr-22</td> </tr> <tr> <td>Power sensor NRP 291</td> <td>SN: 103/44</td> <td>09-Apr-21 (No. 217-03291)</td> <td>Apr-22</td> </tr> <tr> <td>Power sensor NRP 291</td> <td>SN: 103/45</td> <td>09-Apr-21 (No. 217-03291)</td> <td>Apr-22</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN: C20062 (200)</td> <td>09-Apr-21 (No. 217-03293)</td> <td>Apr-22</td> </tr> <tr> <td>Type-N/match combination</td> <td>SN: 310997 / 09377</td> <td>09-Apr-21 (No. 217-03294)</td> <td>Apr-22</td> </tr> <tr> <td>Reference Probe EX03W4</td> <td>SN: 3877</td> <td>30-Dec-20 (No. EX03-077, Dec-20)</td> <td>Dec-21</td> </tr> <tr> <td>D414</td> <td>SN: 664</td> <td>26-Jun-20 (No. D414-654, Jun-20)</td> <td>Jun-21</td> </tr> </tbody> </table> </td> </tr> <tr> <td colspan="2"> <table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Check Date (in house)</th> <th>Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>Power meter E4419B</td> <td>SN: GB41209874</td> <td>09-Apr-16 (in house check Jun-20)</td> <td>In house check: Jun-22</td> </tr> <tr> <td>Power sensor E4419B</td> <td>SN: MY41498067</td> <td>09-Apr-16 (in house check Jun-20)</td> <td>In house check: Jun-22</td> </tr> <tr> <td>Power sensor E4419A</td> <td>SN: 103/40</td> <td>09-Apr-16 (in house check Jun-20)</td> <td>In house check: Jun-22</td> </tr> <tr> <td>RF generator HP 8548C</td> <td>SN: US84040101700</td> <td>04-Aug-18 (in house check Jun-20)</td> <td>In house check: Jun-22</td> </tr> <tr> <td>Network Analyzer Agilent E8360A</td> <td>EN: US41061477</td> <td>31-Mar-14 (in house check Oct-20)</td> <td>In house check: Oct-21</td> </tr> </tbody> </table> </td> </tr> <tr> <td colspan="2"> <p>Calibrated by: Jeffrey Katzman Function: Laboratory Technician Signature: </p> <p>Approved by: Katica Pokovic Function: Technical Manager Signature: </p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> <p>Issued: April 26, 2021</p> </td> </tr> </table> <p>Certificate No: CLA150-4025_Apr21 Page 1 of 6</p>		Object	CLA150 - SN: 4025	Calibration procedure	QA CAL-15.v9 Calibration Procedure for SAR Validation Sources below 700 MHz	Calibration date	April 26, 2021	This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.		All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%.		Calibration Equipment used (MATE: critical for calibration)		<table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter NRP</td> <td>SN: 104/78</td> <td>09-Apr-21 (No. 217-03291/03292)</td> <td>Apr-22</td> </tr> <tr> <td>Power sensor NRP 291</td> <td>SN: 103/44</td> <td>09-Apr-21 (No. 217-03291)</td> <td>Apr-22</td> </tr> <tr> <td>Power sensor NRP 291</td> <td>SN: 103/45</td> <td>09-Apr-21 (No. 217-03291)</td> <td>Apr-22</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN: C20062 (200)</td> <td>09-Apr-21 (No. 217-03293)</td> <td>Apr-22</td> </tr> <tr> <td>Type-N/match combination</td> <td>SN: 310997 / 09377</td> <td>09-Apr-21 (No. 217-03294)</td> <td>Apr-22</td> </tr> <tr> <td>Reference Probe EX03W4</td> <td>SN: 3877</td> <td>30-Dec-20 (No. EX03-077, Dec-20)</td> <td>Dec-21</td> </tr> <tr> <td>D414</td> <td>SN: 664</td> <td>26-Jun-20 (No. D414-654, Jun-20)</td> <td>Jun-21</td> </tr> </tbody> </table>		Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration	Power meter NRP	SN: 104/78	09-Apr-21 (No. 217-03291/03292)	Apr-22	Power sensor NRP 291	SN: 103/44	09-Apr-21 (No. 217-03291)	Apr-22	Power sensor NRP 291	SN: 103/45	09-Apr-21 (No. 217-03291)	Apr-22	Reference 20 dB Attenuator	SN: C20062 (200)	09-Apr-21 (No. 217-03293)	Apr-22	Type-N/match combination	SN: 310997 / 09377	09-Apr-21 (No. 217-03294)	Apr-22	Reference Probe EX03W4	SN: 3877	30-Dec-20 (No. EX03-077, Dec-20)	Dec-21	D414	SN: 664	26-Jun-20 (No. D414-654, Jun-20)	Jun-21	<table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Check Date (in house)</th> <th>Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>Power meter E4419B</td> <td>SN: GB41209874</td> <td>09-Apr-16 (in house check Jun-20)</td> <td>In house check: Jun-22</td> </tr> <tr> <td>Power sensor E4419B</td> <td>SN: MY41498067</td> <td>09-Apr-16 (in house check Jun-20)</td> <td>In house check: Jun-22</td> </tr> <tr> <td>Power sensor E4419A</td> <td>SN: 103/40</td> <td>09-Apr-16 (in house check Jun-20)</td> <td>In house check: Jun-22</td> </tr> <tr> <td>RF generator HP 8548C</td> <td>SN: US84040101700</td> <td>04-Aug-18 (in house check Jun-20)</td> <td>In house check: Jun-22</td> </tr> <tr> <td>Network Analyzer Agilent E8360A</td> <td>EN: US41061477</td> <td>31-Mar-14 (in house check Oct-20)</td> <td>In house check: Oct-21</td> </tr> </tbody> </table>		Secondary Standards	ID #	Check Date (in house)	Scheduled Check	Power meter E4419B	SN: GB41209874	09-Apr-16 (in house check Jun-20)	In house check: Jun-22	Power sensor E4419B	SN: MY41498067	09-Apr-16 (in house check Jun-20)	In house check: Jun-22	Power sensor E4419A	SN: 103/40	09-Apr-16 (in house check Jun-20)	In house check: Jun-22	RF generator HP 8548C	SN: US84040101700	04-Aug-18 (in house check Jun-20)	In house check: Jun-22	Network Analyzer Agilent E8360A	EN: US41061477	31-Mar-14 (in house check Oct-20)	In house check: Oct-21	<p>Calibrated by: Jeffrey Katzman Function: Laboratory Technician Signature: </p> <p>Approved by: Katica Pokovic Function: Technical Manager Signature: </p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> <p>Issued: April 26, 2021</p>		<p><b>Calibration Laboratory of</b> Schmid &amp; Partner Engineering AG Zürcherstrasse 45, 8004 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p><b>Glossary:</b></p> <p>TSL tissue simulating liquid ConvF sensitivity in TSL / NORM x,y,z N/A not applicable or not measured</p> <p><b>Calibration is Performed According to the Following Standards:</b></p> <p>a) IEEE Std 2020-2018, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013</p> <p>b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016</p> <p>c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 300 MHz to 6 GHz)", March 2010</p> <p>d) KDB 665664, "SAR Measurement Requirements for 100 MHz to 6 GHz"</p> <p><b>Additional Documentation:</b></p> <p>e) DASY4/5 System Handbook</p> <p><b>Methods Applied and Interpretation of Parameters:</b></p> <ul style="list-style-type: none"> <li><b>Measurement Conditions:</b> Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.</li> <li><b>Antenna Parameters with TSL:</b> The source is mounted in a touch configuration below the center marking of the flat phantom.</li> <li><b>Return Loss:</b> This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.</li> <li><b>SAR measured:</b> SAR measured at the stated antenna input power.</li> <li><b>SAR normalized:</b> SAR as measured, normalized to an input power of 1 W at the antenna connector.</li> <li><b>SAR for nominal TSL parameters:</b> The measured TSL parameters are used to calculate the nominal SAR result.</li> </ul> <p>The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p> <p>Certificate No: CLA150-4025_Apr21 Page 2 of 6</p>	
Object	CLA150 - SN: 4025																																																																												
Calibration procedure	QA CAL-15.v9 Calibration Procedure for SAR Validation Sources below 700 MHz																																																																												
Calibration date	April 26, 2021																																																																												
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.																																																																													
All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%.																																																																													
Calibration Equipment used (MATE: critical for calibration)																																																																													
<table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter NRP</td> <td>SN: 104/78</td> <td>09-Apr-21 (No. 217-03291/03292)</td> <td>Apr-22</td> </tr> <tr> <td>Power sensor NRP 291</td> <td>SN: 103/44</td> <td>09-Apr-21 (No. 217-03291)</td> <td>Apr-22</td> </tr> <tr> <td>Power sensor NRP 291</td> <td>SN: 103/45</td> <td>09-Apr-21 (No. 217-03291)</td> <td>Apr-22</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN: C20062 (200)</td> <td>09-Apr-21 (No. 217-03293)</td> <td>Apr-22</td> </tr> <tr> <td>Type-N/match combination</td> <td>SN: 310997 / 09377</td> <td>09-Apr-21 (No. 217-03294)</td> <td>Apr-22</td> </tr> <tr> <td>Reference Probe EX03W4</td> <td>SN: 3877</td> <td>30-Dec-20 (No. EX03-077, Dec-20)</td> <td>Dec-21</td> </tr> <tr> <td>D414</td> <td>SN: 664</td> <td>26-Jun-20 (No. D414-654, Jun-20)</td> <td>Jun-21</td> </tr> </tbody> </table>		Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration	Power meter NRP	SN: 104/78	09-Apr-21 (No. 217-03291/03292)	Apr-22	Power sensor NRP 291	SN: 103/44	09-Apr-21 (No. 217-03291)	Apr-22	Power sensor NRP 291	SN: 103/45	09-Apr-21 (No. 217-03291)	Apr-22	Reference 20 dB Attenuator	SN: C20062 (200)	09-Apr-21 (No. 217-03293)	Apr-22	Type-N/match combination	SN: 310997 / 09377	09-Apr-21 (No. 217-03294)	Apr-22	Reference Probe EX03W4	SN: 3877	30-Dec-20 (No. EX03-077, Dec-20)	Dec-21	D414	SN: 664	26-Jun-20 (No. D414-654, Jun-20)	Jun-21																																												
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration																																																																										
Power meter NRP	SN: 104/78	09-Apr-21 (No. 217-03291/03292)	Apr-22																																																																										
Power sensor NRP 291	SN: 103/44	09-Apr-21 (No. 217-03291)	Apr-22																																																																										
Power sensor NRP 291	SN: 103/45	09-Apr-21 (No. 217-03291)	Apr-22																																																																										
Reference 20 dB Attenuator	SN: C20062 (200)	09-Apr-21 (No. 217-03293)	Apr-22																																																																										
Type-N/match combination	SN: 310997 / 09377	09-Apr-21 (No. 217-03294)	Apr-22																																																																										
Reference Probe EX03W4	SN: 3877	30-Dec-20 (No. EX03-077, Dec-20)	Dec-21																																																																										
D414	SN: 664	26-Jun-20 (No. D414-654, Jun-20)	Jun-21																																																																										
<table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Check Date (in house)</th> <th>Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>Power meter E4419B</td> <td>SN: GB41209874</td> <td>09-Apr-16 (in house check Jun-20)</td> <td>In house check: Jun-22</td> </tr> <tr> <td>Power sensor E4419B</td> <td>SN: MY41498067</td> <td>09-Apr-16 (in house check Jun-20)</td> <td>In house check: Jun-22</td> </tr> <tr> <td>Power sensor E4419A</td> <td>SN: 103/40</td> <td>09-Apr-16 (in house check Jun-20)</td> <td>In house check: Jun-22</td> </tr> <tr> <td>RF generator HP 8548C</td> <td>SN: US84040101700</td> <td>04-Aug-18 (in house check Jun-20)</td> <td>In house check: Jun-22</td> </tr> <tr> <td>Network Analyzer Agilent E8360A</td> <td>EN: US41061477</td> <td>31-Mar-14 (in house check Oct-20)</td> <td>In house check: Oct-21</td> </tr> </tbody> </table>		Secondary Standards	ID #	Check Date (in house)	Scheduled Check	Power meter E4419B	SN: GB41209874	09-Apr-16 (in house check Jun-20)	In house check: Jun-22	Power sensor E4419B	SN: MY41498067	09-Apr-16 (in house check Jun-20)	In house check: Jun-22	Power sensor E4419A	SN: 103/40	09-Apr-16 (in house check Jun-20)	In house check: Jun-22	RF generator HP 8548C	SN: US84040101700	04-Aug-18 (in house check Jun-20)	In house check: Jun-22	Network Analyzer Agilent E8360A	EN: US41061477	31-Mar-14 (in house check Oct-20)	In house check: Oct-21																																																				
Secondary Standards	ID #	Check Date (in house)	Scheduled Check																																																																										
Power meter E4419B	SN: GB41209874	09-Apr-16 (in house check Jun-20)	In house check: Jun-22																																																																										
Power sensor E4419B	SN: MY41498067	09-Apr-16 (in house check Jun-20)	In house check: Jun-22																																																																										
Power sensor E4419A	SN: 103/40	09-Apr-16 (in house check Jun-20)	In house check: Jun-22																																																																										
RF generator HP 8548C	SN: US84040101700	04-Aug-18 (in house check Jun-20)	In house check: Jun-22																																																																										
Network Analyzer Agilent E8360A	EN: US41061477	31-Mar-14 (in house check Oct-20)	In house check: Oct-21																																																																										
<p>Calibrated by: Jeffrey Katzman Function: Laboratory Technician Signature: </p> <p>Approved by: Katica Pokovic Function: Technical Manager Signature: </p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> <p>Issued: April 26, 2021</p>																																																																													
<p><b>Measurement Conditions</b> DASY system configuration, as far as not given on page 1.</p> <table border="1"> <tr> <td>DASY Version</td> <td>DASY5</td> <td>V32.10.4</td> </tr> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>EL44 Flat Phantom</td> <td>Shell thickness: 2 ± 0.2 mm</td> </tr> <tr> <td>EUT Positioning</td> <td>Touch Position</td> <td></td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy = 4.0 mm, dz = 1.4 mm</td> <td>Grated Ratio = 1.4 (Z direction)</td> </tr> <tr> <td>Frequency</td> <td>150 MHz ± 1 MHz</td> <td></td> </tr> </table> <p><b>Head TSL parameters</b> The following parameters and calculations were applied.</p> <table border="1"> <tr> <td>Nominal Head TSL parameters</td> <td>Temperature</td> <td>Permittivity</td> <td>Conductivity</td> </tr> <tr> <td>22.0 °C</td> <td>62.3</td> <td>0.78 mho/m</td> <td></td> </tr> <tr> <td>(22.0 ± 0.2) °C</td> <td>51.1 ± 6 %</td> <td>0.75 mho/m ± 6 %</td> <td></td> </tr> <tr> <td>Head TSL temperature change during test</td> <td>&lt; 0.5 °C</td> <td>---</td> <td>---</td> </tr> </table> <p><b>SAR result with Head TSL</b></p> <table border="1"> <tr> <td>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>1 W input power</td> <td>3.90 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>3.88 W/kg ± 18.4 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>1 W input power</td> <td>2.60 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>2.59 W/kg ± 18.0 % (k=2)</td> </tr> </table> <p>Certificate No: CLA150-4025_Apr21 Page 3 of 6</p>		DASY Version	DASY5	V32.10.4	Extrapolation	Advanced Extrapolation		Phantom	EL44 Flat Phantom	Shell thickness: 2 ± 0.2 mm	EUT Positioning	Touch Position		Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 1.4 mm	Grated Ratio = 1.4 (Z direction)	Frequency	150 MHz ± 1 MHz		Nominal Head TSL parameters	Temperature	Permittivity	Conductivity	22.0 °C	62.3	0.78 mho/m		(22.0 ± 0.2) °C	51.1 ± 6 %	0.75 mho/m ± 6 %		Head TSL temperature change during test	< 0.5 °C	---	---	SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition		SAR measured	1 W input power	3.90 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	3.88 W/kg ± 18.4 % (k=2)	SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition		SAR measured	1 W input power	2.60 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	2.59 W/kg ± 18.0 % (k=2)	<p><b>Appendix (Additional assessments outside the scope of SCS 0108)</b></p> <p><b>Antenna Parameters with Head TSL</b></p> <table border="1"> <tr> <td>Impedance, transformed to feed point:</td> <td>47.8 Ω ± 1.5 jΩ</td> </tr> <tr> <td>Return Loss:</td> <td>-31.4 dB</td> </tr> </table> <p><b>Additional EUT Data</b></p> <table border="1"> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </table> <p>Certificate No: CLA150-4025_Apr21 Page 4 of 6</p>		Impedance, transformed to feed point:	47.8 Ω ± 1.5 jΩ	Return Loss:	-31.4 dB	Manufactured by	SPEAG																
DASY Version	DASY5	V32.10.4																																																																											
Extrapolation	Advanced Extrapolation																																																																												
Phantom	EL44 Flat Phantom	Shell thickness: 2 ± 0.2 mm																																																																											
EUT Positioning	Touch Position																																																																												
Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 1.4 mm	Grated Ratio = 1.4 (Z direction)																																																																											
Frequency	150 MHz ± 1 MHz																																																																												
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity																																																																										
22.0 °C	62.3	0.78 mho/m																																																																											
(22.0 ± 0.2) °C	51.1 ± 6 %	0.75 mho/m ± 6 %																																																																											
Head TSL temperature change during test	< 0.5 °C	---	---																																																																										
SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition																																																																												
SAR measured	1 W input power	3.90 W/kg																																																																											
SAR for nominal Head TSL parameters	normalized to 1W	3.88 W/kg ± 18.4 % (k=2)																																																																											
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition																																																																												
SAR measured	1 W input power	2.60 W/kg																																																																											
SAR for nominal Head TSL parameters	normalized to 1W	2.59 W/kg ± 18.0 % (k=2)																																																																											
Impedance, transformed to feed point:	47.8 Ω ± 1.5 jΩ																																																																												
Return Loss:	-31.4 dB																																																																												
Manufactured by	SPEAG																																																																												



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To need the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.DocCheck@sgs.com](mailto:CN.DocCheck@sgs.com)

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300  
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 [www.sgsgroup.com.cn](http://www.sgsgroup.com.cn)  
t(86-512)57355888 f(86-512)57370818 [sgs.china@sgs.com](mailto:sgs.china@sgs.com)

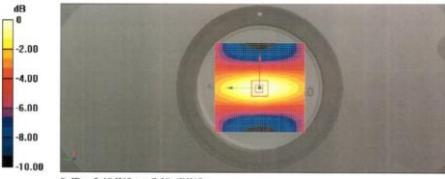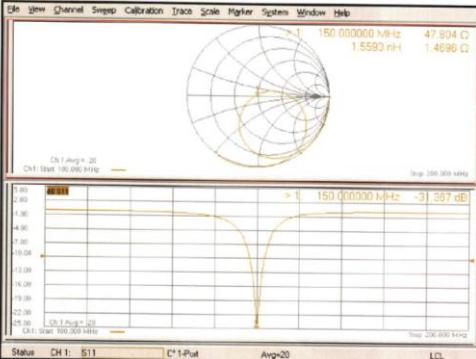

<p><b>DASY5 Validation Report for Head TSL</b></p> <p>Date: 26.04.2021</p> <p>Test Laboratory: SPEAG, Zurich, Switzerland</p> <p>DUT: CLA150; Type: CLA150; Serial: CLA150 - SN: 4025</p> <p>Communication System: UUD 0 - CW; Frequency: 150 MHz</p> <p>Medium parameters used: <math>\epsilon' = 150 \text{ MHz}</math>; <math>\epsilon_r = 0.76 \text{ S/m}</math>; <math>\sigma = 51.1 \text{ S/m}</math>; <math>\rho = 1000 \text{ kg/m}^3</math></p> <p>Phantom section: Flat Section</p> <p>Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)</p> <p>DASY52 Configuration:</p> <ul style="list-style-type: none"> <li>Probe: EX3DV4 - SN3877; ConvF(12.51, 12.51, 12.51) @ 150 MHz; Calibrated: 30.12.2020</li> <li>Sensor-Surface: 1.4mm (Mechanical Surface Detection)</li> <li>Electronics: DAB4 Suf654; Calibrated: 26.06.2020</li> <li>Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1003</li> <li>DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)</li> </ul> <p><b>CLA Calibration for HSL-LF Tissue/CLA150, touch configuration, Pin=1W/Zoom Scan, dist=1.4mm (8x10x8) /Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm</b></p> <p>Reference Value = 85.93 V/m; Power Drift = -0.02 dB</p> <p>Peak SAR (extrapolated) = 7.36 W/kg</p> <p>SAR(1 g) = 3.90 W/kg; SAR(10 g) = 2.00 W/kg</p> <p>Small distances tend to result in amounts 3 dB below; Larger than measurement grid (&gt;30mm)</p> <p>Ratio of SAR at M2 to SAR at M1 = 80.4%</p> <p>Maximum value of SAR (measured) = 5.48 W/kg</p> <p>0 dB = 5.48 W/kg = 7.39 dBW/kg</p>  <p>Certificates No: CLA150-4025_Apr21 Page 5 of 6</p>	 <p>Certificates No: CLA150-4025_Apr21 Page 6 of 6</p>
---	--

## 1.2 D450V3 - SN 1103

<p><b>Calibration Laboratory of</b> Schmid &amp; Partner Engineering AG Zughestrasse 43, 8004 Zurich, Switzerland</p> <p> </p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Client: SGS-CN (Auden) Certificate No: D450V3-1103_Apr21</p> <p><b>CALIBRATION CERTIFICATE</b></p> <p>Object: D450V3 - SN:1103</p> <p>Calibration procedure(s): QA CAL-15.v9 Calibration Procedure for SAR Validation Sources below 700 MHz</p> <p>Calibration date: April 21, 2021</p> <p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurement (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (29 ± 3)°C and humidity ~ 75%.</p> <p>Calibration Equipment used (M/TE critical for calibration):</p> <table border="1"> <tr> <td>Primary Standards</td> <td>ID #</td> <td>Cal Date (Certificate No.)</td> <td>Scheduled Calibration</td> </tr> <tr> <td>Power meter NIP</td> <td>SN: 100778</td> <td>09-Apr-21 (No. 217-0021-0320)</td> <td>Apr-22</td> </tr> <tr> <td>Power sensor NIP-291</td> <td>SN: 100284</td> <td>09-Apr-21 (No. 217-0021)</td> <td>Apr-22</td> </tr> <tr> <td>Power sensor NIP-291</td> <td>SN: 103219</td> <td>09-Apr-21 (No. 217-0021)</td> <td>Apr-22</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN: CC2652 (200)</td> <td>09-Apr-21 (No. 217-0043)</td> <td>Apr-22</td> </tr> <tr> <td>Type-N min-max combination</td> <td>SN: 310982 / 06327</td> <td>09-Apr-21 (No. 217-0044)</td> <td>Apr-22</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN: 3877</td> <td>30-Dec-20 (No. EX3-3077- Dec20)</td> <td>Dec-21</td> </tr> <tr> <td>DAE4</td> <td>SN: 954</td> <td>28-Jun-20 (No. DAE4-954_Jun20)</td> <td>Jun-21</td> </tr> </table> <table border="1"> <tr> <td>Secondary Standards</td> <td>ID #</td> <td>Check Date (in house)</td> <td>Scheduled Check</td> </tr> <tr> <td>Power meter E41198</td> <td>SN: G411290874</td> <td>09-Apr-16 (in house check Jun-20)</td> <td>In house check: Jun-22</td> </tr> <tr> <td>Power meter E41198</td> <td>SN: 9411290874</td> <td>09-Apr-16 (in house check Jun-20)</td> <td>In house check: Jun-22</td> </tr> <tr> <td>Power sensor E4412A</td> <td>SN: 200116019</td> <td>09-Apr-19 (in house check Jun-20)</td> <td>In house check: Jun-22</td> </tr> <tr> <td>RF generator HP 8648C</td> <td>EN: USR440-011700</td> <td>09-Aug-19 (in house check Jun-20)</td> <td>In house check: Jun-22</td> </tr> <tr> <td>Network Analyzer Agilent E3036A</td> <td>SN: US410960477</td> <td>31-Mar-14 (in house check Oct-20)</td> <td>In house check: Oct-21</td> </tr> </table> <p>Calibrated by: Name: Claudio Leutler Function: Laboratory Technician Signature: </p> <p>Approved by: Name: Katja Povacic Function: Technical Manager Signature: </p> <p>Issued: April 23, 2021</p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> <p>Certificates No: D450V3-1103_Apr21 Page 1 of 6</p>	Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration	Power meter NIP	SN: 100778	09-Apr-21 (No. 217-0021-0320)	Apr-22	Power sensor NIP-291	SN: 100284	09-Apr-21 (No. 217-0021)	Apr-22	Power sensor NIP-291	SN: 103219	09-Apr-21 (No. 217-0021)	Apr-22	Reference 20 dB Attenuator	SN: CC2652 (200)	09-Apr-21 (No. 217-0043)	Apr-22	Type-N min-max combination	SN: 310982 / 06327	09-Apr-21 (No. 217-0044)	Apr-22	Reference Probe EX3DV4	SN: 3877	30-Dec-20 (No. EX3-3077- Dec20)	Dec-21	DAE4	SN: 954	28-Jun-20 (No. DAE4-954_Jun20)	Jun-21	Secondary Standards	ID #	Check Date (in house)	Scheduled Check	Power meter E41198	SN: G411290874	09-Apr-16 (in house check Jun-20)	In house check: Jun-22	Power meter E41198	SN: 9411290874	09-Apr-16 (in house check Jun-20)	In house check: Jun-22	Power sensor E4412A	SN: 200116019	09-Apr-19 (in house check Jun-20)	In house check: Jun-22	RF generator HP 8648C	EN: USR440-011700	09-Aug-19 (in house check Jun-20)	In house check: Jun-22	Network Analyzer Agilent E3036A	SN: US410960477	31-Mar-14 (in house check Oct-20)	In house check: Oct-21	<p><b>Calibration Laboratory of</b> Schmid &amp; Partner Engineering AG Zughestrasse 43, 8004 Zurich, Switzerland</p> <p> </p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p><b>Glossary:</b></p> <ul style="list-style-type: none"> <li><b>TSL</b>: tissue simulating liquid</li> <li><b>ConvF</b>: sensitivity in TSL / NORM x,y,z</li> <li><b>N/A</b>: not applicable or not measured</li> </ul> <p><b>Calibration is Performed According to the Following Standards:</b></p> <ol style="list-style-type: none"> <li>IEEE Std 1628-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013</li> <li>IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016</li> <li>IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010</li> <li>KDB 605864, "SAR Measurement Requirements for 100 MHz to 6 GHz"</li> </ol> <p><b>Additional Documentation:</b></p> <ol style="list-style-type: none"> <li>DASY4/5 System Handbook</li> </ol> <p><b>Method Applied and Interpretation of Parameters:</b></p> <ul style="list-style-type: none"> <li><b>Measurement Conditions:</b> Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.</li> <li><b>Antenna Parameters with TSL:</b> The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.</li> <li><b>Peak Power Impedance and Return Loss:</b> These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.</li> <li><b>Electrical Delay:</b> One-way delay between the SMA connector and the antenna feed point. No uncertainty required.</li> <li><b>SAR measured:</b> SAR measured at the stated antenna input power.</li> <li><b>SAR normalized:</b> SAR as measured, normalized to an input power of 1 W at the antenna connector.</li> <li><b>SAR for nominal TSL parameters:</b> The measured TSL parameters are used to calculate the nominal SAR result.</li> </ul> <p>The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p> <p>Certificates No: D450V3-1103_Apr21 Page 2 of 6</p>
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration																																																						
Power meter NIP	SN: 100778	09-Apr-21 (No. 217-0021-0320)	Apr-22																																																						
Power sensor NIP-291	SN: 100284	09-Apr-21 (No. 217-0021)	Apr-22																																																						
Power sensor NIP-291	SN: 103219	09-Apr-21 (No. 217-0021)	Apr-22																																																						
Reference 20 dB Attenuator	SN: CC2652 (200)	09-Apr-21 (No. 217-0043)	Apr-22																																																						
Type-N min-max combination	SN: 310982 / 06327	09-Apr-21 (No. 217-0044)	Apr-22																																																						
Reference Probe EX3DV4	SN: 3877	30-Dec-20 (No. EX3-3077- Dec20)	Dec-21																																																						
DAE4	SN: 954	28-Jun-20 (No. DAE4-954_Jun20)	Jun-21																																																						
Secondary Standards	ID #	Check Date (in house)	Scheduled Check																																																						
Power meter E41198	SN: G411290874	09-Apr-16 (in house check Jun-20)	In house check: Jun-22																																																						
Power meter E41198	SN: 9411290874	09-Apr-16 (in house check Jun-20)	In house check: Jun-22																																																						
Power sensor E4412A	SN: 200116019	09-Apr-19 (in house check Jun-20)	In house check: Jun-22																																																						
RF generator HP 8648C	EN: USR440-011700	09-Aug-19 (in house check Jun-20)	In house check: Jun-22																																																						
Network Analyzer Agilent E3036A	SN: US410960477	31-Mar-14 (in house check Oct-20)	In house check: Oct-21																																																						

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To need the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.DocCheck@sgs.com](mailto:CN.DocCheck@sgs.com)

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300  
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 [www.sgsgroup.com.cn](http://www.sgsgroup.com.cn)  
t(86-512)57355888 f(86-512)57370818 [sgs.china@sgs.com](mailto:sgs.china@sgs.com)



<b>Measurement Conditions</b> DASY system configuration, as far as not given on page 1. <table border="1"> <tr><td>DASY Version</td><td>DASY5</td><td>V52.10.4</td></tr> <tr><td>Extrapolation</td><td colspan="2">Advanced Extrapolation</td></tr> <tr><td>Phantom</td><td>ELH Flat Phantom</td><td>Shell thickness: <math>2 \pm 0.2</math> mm</td></tr> <tr><td>Distance Dipole Center - TSL</td><td>15 mm</td><td>with Spacer</td></tr> <tr><td>Zoom Scan Resolution</td><td><math>\Delta x, \Delta y, \Delta z = 5</math> mm</td><td></td></tr> <tr><td>Frequency</td><td>450 MHz <math>\pm 1</math> MHz</td><td></td></tr> </table>		DASY Version	DASY5	V52.10.4	Extrapolation	Advanced Extrapolation		Phantom	ELH Flat Phantom	Shell thickness: $2 \pm 0.2$ mm	Distance Dipole Center - TSL	15 mm	with Spacer	Zoom Scan Resolution	$\Delta x, \Delta y, \Delta z = 5$ mm		Frequency	450 MHz $\pm 1$ MHz		<b>Appendix (Additional assessments outside the scope of SCS 0108)</b> <b>Antenna Parameters with Head TSL</b> <table border="1"> <tr><td>Impedance, transformed to feed point</td><td>57.1 <math>\Omega</math> - 2.8 <math>\text{j}\Omega</math></td></tr> <tr><td>Return Loss</td><td>-23.0 dB</td></tr> </table> <b>General Antenna Parameters and Design</b> <table border="1"> <tr><td>Electrical Delay (one direction)</td><td>1.346 ns</td></tr> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.</p> <p>The dipole is made of standard semi-gloss copper cable. The outer conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the arms, small end caps are added to the dipole arms in order to improve matching when loaded according to the test and explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.</p> <p>No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.</p>		Impedance, transformed to feed point	57.1 $\Omega$ - 2.8 $\text{j}\Omega$	Return Loss	-23.0 dB	Electrical Delay (one direction)	1.346 ns
DASY Version	DASY5	V52.10.4																									
Extrapolation	Advanced Extrapolation																										
Phantom	ELH Flat Phantom	Shell thickness: $2 \pm 0.2$ mm																									
Distance Dipole Center - TSL	15 mm	with Spacer																									
Zoom Scan Resolution	$\Delta x, \Delta y, \Delta z = 5$ mm																										
Frequency	450 MHz $\pm 1$ MHz																										
Impedance, transformed to feed point	57.1 $\Omega$ - 2.8 $\text{j}\Omega$																										
Return Loss	-23.0 dB																										
Electrical Delay (one direction)	1.346 ns																										
<b>Head TSL parameters</b> The following parameters and calculations were applied. <table border="1"> <tr><td>Nominal Head TSL parameters</td><td>22.0 <math>^{\circ}\text{C}</math></td><td>43.5</td><td>0.57 mho/m</td></tr> <tr><td>Measured Head TSL parameters</td><td>(22.0 <math>\pm 0.2</math> <math>^{\circ}\text{C}</math>)</td><td>43.1 <math>\pm 6\%</math></td><td>0.67 mho/m <math>\pm 6\%</math></td></tr> <tr><td>Head TSL temperature change during test</td><td>&lt; 0.5 <math>^{\circ}\text{C}</math></td><td>----</td><td>----</td></tr> </table>		Nominal Head TSL parameters	22.0 $^{\circ}\text{C}$	43.5	0.57 mho/m	Measured Head TSL parameters	(22.0 $\pm 0.2$ $^{\circ}\text{C}$ )	43.1 $\pm 6\%$	0.67 mho/m $\pm 6\%$	Head TSL temperature change during test	< 0.5 $^{\circ}\text{C}$	----	----	<b>Additional EUT Data</b> <table border="1"> <tr><td>Manufactured by</td><td>SPEAG</td></tr> </table>		Manufactured by	SPEAG										
Nominal Head TSL parameters	22.0 $^{\circ}\text{C}$	43.5	0.57 mho/m																								
Measured Head TSL parameters	(22.0 $\pm 0.2$ $^{\circ}\text{C}$ )	43.1 $\pm 6\%$	0.67 mho/m $\pm 6\%$																								
Head TSL temperature change during test	< 0.5 $^{\circ}\text{C}$	----	----																								
Manufactured by	SPEAG																										
<b>SAR result with Head TSL</b> <table border="1"> <tr><td>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>250 mW input power</td><td>1.14 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>4.88 W/kg <math>\pm 18.1\%</math> (Ko2)</td></tr> </table> <table border="1"> <tr><td>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>250 mW input power</td><td>0.797 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>3.08 W/kg <math>\pm 17.6\%</math> (Ko2)</td></tr> </table>		SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	SAR measured	250 mW input power	1.14 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	4.88 W/kg $\pm 18.1\%$ (Ko2)	SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	SAR measured	250 mW input power	0.797 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	3.08 W/kg $\pm 17.6\%$ (Ko2)	Certificate No: D450V3-1103_Apr21 Page 3 of 6									
SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition																										
SAR measured	250 mW input power	1.14 W/kg																									
SAR for nominal Head TSL parameters	normalized to 1W	4.88 W/kg $\pm 18.1\%$ (Ko2)																									
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition																										
SAR measured	250 mW input power	0.797 W/kg																									
SAR for nominal Head TSL parameters	normalized to 1W	3.08 W/kg $\pm 17.6\%$ (Ko2)																									
<b>DASY5 Validation Report for Head TSL</b> Test Laboratory: SPEAG, Zurich, Switzerland DUT: Dipole 450 MHz; Type: D450V3; Serial: D450V3 - SN:1103 Communication System: UUD 0 - CW; Frequency: 450 MHz Medium parameters used: $\epsilon' = 450$ MHz; $\sigma = 0.87$ S/m; $\epsilon_r = 43.1$ ; $\rho = 1000$ kg/m <sup>3</sup> Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011) DASY52 Configuration: <ul style="list-style-type: none"> <li>Probe: EX3DV4 - SN3877; ConvF(10.64, 10.64, 10.64) @ 450 MHz; Calibrated: 30.12.2020</li> <li>Sensor-Surface: 1.4mm (Mechanical Surface Detection)</li> <li>Electronics: DAE4 Sn654; Calibrated: 26.06.2020</li> <li>Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1003</li> <li>DASY52.52.10.4(1527); SEMCAD X 14.6.14(7483)</li> </ul> <b>Dipole Calibration for Head Tissue/d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 8</b> Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 39.18 V/m; Power Drift $\approx$ 0.08 dB Peak SAR (extrapolated) = 1.76 W/kg SAR(1 g) = 1.14 W/kg; SAR(10 g) = 0.767 W/kg Smallest distance from peaks to all points 3 dB below: Larger than measurement grid Ratio of SAR at M2 to SAR at M1 = 64.9% Maximum value of SAR (measured) = 1.53 W/kg		Certificate No: D450V3-1103_Apr21 Page 4 of 6																									
Certificate No: D450V3-1103_Apr21 Page 5 of 6		Certificate No: D450V3-1103_Apr21 Page 6 of 6																									

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

If you need the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.Doccheck@sgs.com](mailto:CN.Doccheck@sgs.com)

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300  
 中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 [www.sgsgroup.com.cn](http://www.sgsgroup.com.cn)  
 t(86-512)57355888 f(86-512)57370818 [sgs.china@sgs.com](mailto:sgs.china@sgs.com)



## 1.3 D750V3 - SN 1188

    <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-62305012 Fax: +86-10-62304633-2594 E-mail: cttf@chinaitt.com http://www.chinaitt.com</p> <p>Client: SGS-CN Certificate No: Z22-60103</p> <p><b>CALIBRATION CERTIFICATE</b></p> <p>Object: D750V3 - SN: 1188</p> <p>Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits</p> <p>Calibration date: March 29, 2022</p> <p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibration have been conducted in the closed laboratory facility: environment temperature (22±3)°C; and humidity&lt;70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> <table border="1"> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> <tr> <td>Power Meter NRP2</td> <td>105277</td> <td>24-Sep-21 (CTTL, No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP8S</td> <td>104291</td> <td>24-Sep-21 (CTTL, No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN 7307</td> <td>26-May-21 (SPEAG No. EX3-7307, May21)</td> <td>May-22</td> </tr> <tr> <td>DAE4</td> <td>SN 1556</td> <td>12-Jan-22 (CTTL-SPEAG, No.Z22-60007)</td> <td>Jan-23</td> </tr> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> <tr> <td>Signal Generator E4438C</td> <td>MY49071430</td> <td>13-Jan-22 (CTTL, No.J22X04049)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MY46110673</td> <td>14-Jan-22 (CTTL, No.J22X04046)</td> <td>Jan-23</td> </tr> </table> <table border="1"> <tr> <td>Calibrated by:</td> <td>Name: Zhao Jing</td> <td>Function: SAR Test Engineer</td> <td>Signature: </td> </tr> <tr> <td>Reviewed by:</td> <td>Name: Lin Hao</td> <td>Function: SAR Test Engineer</td> <td>Signature: </td> </tr> <tr> <td>Approved by:</td> <td>Name: Qi Dianyuan</td> <td>Function: SAR Project Leader</td> <td>Signature: </td> </tr> </table> <p>Issued: April 3, 2022</p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p>		Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Power Meter NRP2	105277	24-Sep-21 (CTTL, No.J21X08326)	Sep-22	Power sensor NRP8S	104291	24-Sep-21 (CTTL, No.J21X08326)	Sep-22	Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No. EX3-7307, May21)	May-22	DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG, No.Z22-60007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL, No.J22X04049)	Jan-23	Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL, No.J22X04046)	Jan-23	Calibrated by:	Name: Zhao Jing	Function: SAR Test Engineer	Signature: 	Reviewed by:	Name: Lin Hao	Function: SAR Test Engineer	Signature: 	Approved by:	Name: Qi Dianyuan	Function: SAR Project Leader	Signature: 	    <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2594 E-mail: cttf@chinaitt.com http://www.chinaitt.com</p> <p><b>Glossary:</b> TSL tissue simulating liquid ConvF sensitivity in TSL / NORMx,y,z N/A not applicable or not measured</p> <p><b>Calibration is Performed According to the Following Standards:</b></p> <ul style="list-style-type: none"> <li>a) IEC/IEEE 62209-1528, "Measurement Procedure for the Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices - Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020</li> <li>b) KDB 655864, "SAR Measurement Requirements for 100 MHz to 6 GHz"</li> </ul> <p><b>Additional Documentation:</b></p> <ul style="list-style-type: none"> <li>c) DASY4/5 System handbook</li> </ul> <p><b>Methods Applied and Interpretation of Parameters:</b></p> <ul style="list-style-type: none"> <li>• <b>Measurement Conditions:</b> Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.</li> <li>• <b>Antenna Parameters with TSL:</b> The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.</li> <li>• <b>Feed Point Impedance and Return Loss:</b> These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measured value at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.</li> <li>• <b>Electrical Delay:</b> One-way delay between the SMA connector and the antenna feed point. No uncertainty required.</li> <li>• <b>SAR measured:</b> SAR measured at the stated antenna input power.</li> <li>• <b>SAR normalized:</b> SAR as measured, normalized to an input power of 1 W at the antenna connector.</li> <li>• <b>SAR for nominal TSL parameters:</b> The measured TSL parameters are used to calculate the nominal SAR result.</li> </ul> <p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.</p>																
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																											
Power Meter NRP2	105277	24-Sep-21 (CTTL, No.J21X08326)	Sep-22																																																											
Power sensor NRP8S	104291	24-Sep-21 (CTTL, No.J21X08326)	Sep-22																																																											
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No. EX3-7307, May21)	May-22																																																											
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG, No.Z22-60007)	Jan-23																																																											
Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																											
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL, No.J22X04049)	Jan-23																																																											
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL, No.J22X04046)	Jan-23																																																											
Calibrated by:	Name: Zhao Jing	Function: SAR Test Engineer	Signature: 																																																											
Reviewed by:	Name: Lin Hao	Function: SAR Test Engineer	Signature: 																																																											
Approved by:	Name: Qi Dianyuan	Function: SAR Project Leader	Signature: 																																																											
<p>Certificate No: Z22-60103 Page 1 of 6</p> <p>   <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2594 E-mail: cttf@chinaitt.com http://www.chinaitt.com</p> <p><b>Measurement Conditions</b> DASY system configuration, as far as not given on page 1.</p> <table border="1"> <tr> <td>DASY Version</td> <td>DASY52</td> <td>VS2.10.4</td> </tr> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>15 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>750 MHz ± 1 MHz</td> <td></td> </tr> </table> <p><b>Head TSL parameters</b> The following parameters and calculations were applied.</p> <table border="1"> <tr> <td></td> <td>Temperature</td> <td>Permittivity</td> <td>Conductivity</td> </tr> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>42.0</td> <td>0.90 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>41.4 ± 6 %</td> <td>0.89 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td>&lt;1.0 °C</td> <td>---</td> <td>---</td> </tr> </table> <p><b>SAR result with Head TSL</b></p> <table border="1"> <tr> <td>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>250 mW Input power</td> <td>2.07 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>8.27 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>250 mW Input power</td> <td>1.37 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>5.48 W/kg ± 18.7 % (k=2)</td> </tr> </table> </p>		DASY Version	DASY52	VS2.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	15 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	750 MHz ± 1 MHz			Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	42.0	0.90 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	41.4 ± 6 %	0.89 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	---	---	SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition		SAR measured	250 mW Input power	2.07 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	8.27 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition		SAR measured	250 mW Input power	1.37 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	5.48 W/kg ± 18.7 % (k=2)	<p>Certificate No: Z22-60103 Page 2 of 6</p> <p>   <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2594 E-mail: cttf@chinaitt.com http://www.chinaitt.com</p> <p><b>Appendix (Additional assessments outside the scope of CNAS L0570)</b></p> <p><b>Antenna Parameters with Head TSL</b></p> <table border="1"> <tr> <td>Impedance, transformed to feed point</td> <td>53.6Ω-1.13jΩ</td> </tr> <tr> <td>Return Loss</td> <td>-28.7dB</td> </tr> </table> <p><b>General Antenna Parameters and Design</b></p> <table border="1"> <tr> <td>Electrical Delay (one direction)</td> <td>0.947 ns</td> </tr> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this modification, as long as it is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p><b>Additional EUT Data</b></p> <table border="1"> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </table> </p>	Impedance, transformed to feed point	53.6Ω-1.13jΩ	Return Loss	-28.7dB	Electrical Delay (one direction)	0.947 ns	Manufactured by	SPEAG
DASY Version	DASY52	VS2.10.4																																																												
Extrapolation	Advanced Extrapolation																																																													
Phantom	Triple Flat Phantom 5.1C																																																													
Distance Dipole Center - TSL	15 mm	with Spacer																																																												
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																													
Frequency	750 MHz ± 1 MHz																																																													
	Temperature	Permittivity	Conductivity																																																											
Nominal Head TSL parameters	22.0 °C	42.0	0.90 mho/m																																																											
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.4 ± 6 %	0.89 mho/m ± 6 %																																																											
Head TSL temperature change during test	<1.0 °C	---	---																																																											
SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition																																																													
SAR measured	250 mW Input power	2.07 W/kg																																																												
SAR for nominal Head TSL parameters	normalized to 1W	8.27 W/kg ± 18.8 % (k=2)																																																												
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition																																																													
SAR measured	250 mW Input power	1.37 W/kg																																																												
SAR for nominal Head TSL parameters	normalized to 1W	5.48 W/kg ± 18.7 % (k=2)																																																												
Impedance, transformed to feed point	53.6Ω-1.13jΩ																																																													
Return Loss	-28.7dB																																																													
Electrical Delay (one direction)	0.947 ns																																																													
Manufactured by	SPEAG																																																													


Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.Doccheck@sgs.com](mailto:CN.Doccheck@sgs.com)


No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300  
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 [www.sgsgroup.com.cn](http://www.sgsgroup.com.cn)  
t(86-512)57355888 f(86-512)57370818 [sgs.china@sgs.com](mailto:sgs.china@sgs.com)



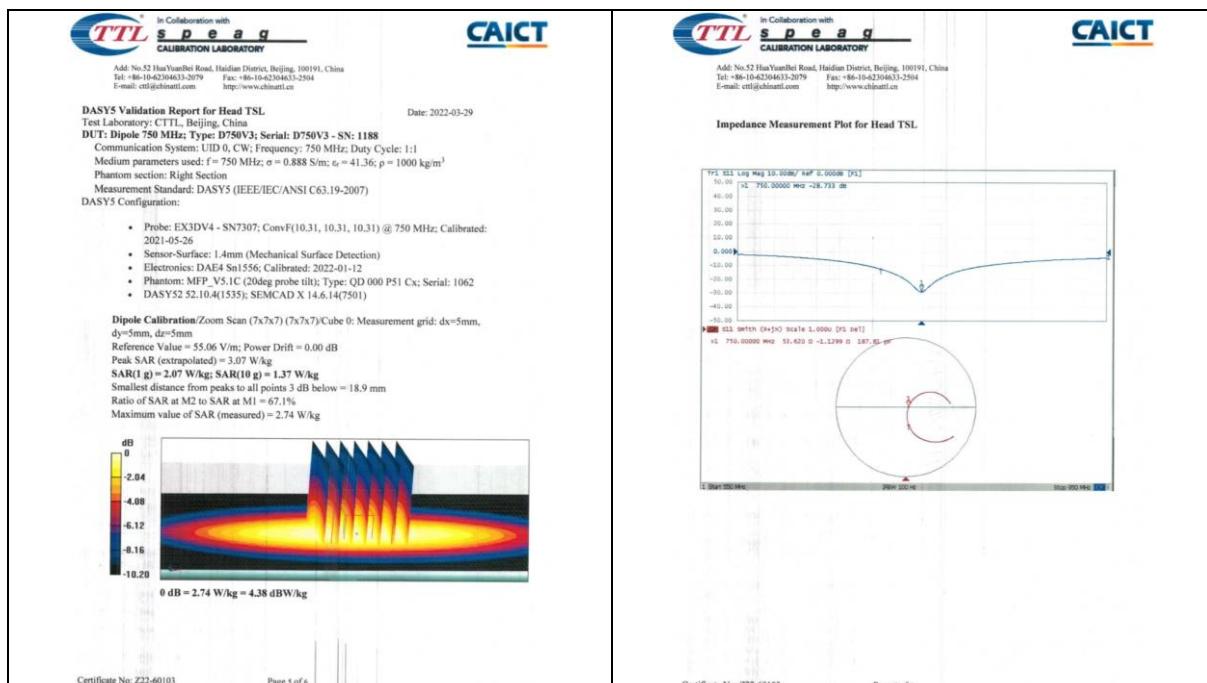

## 1.4 D835V2 - SN 4d114

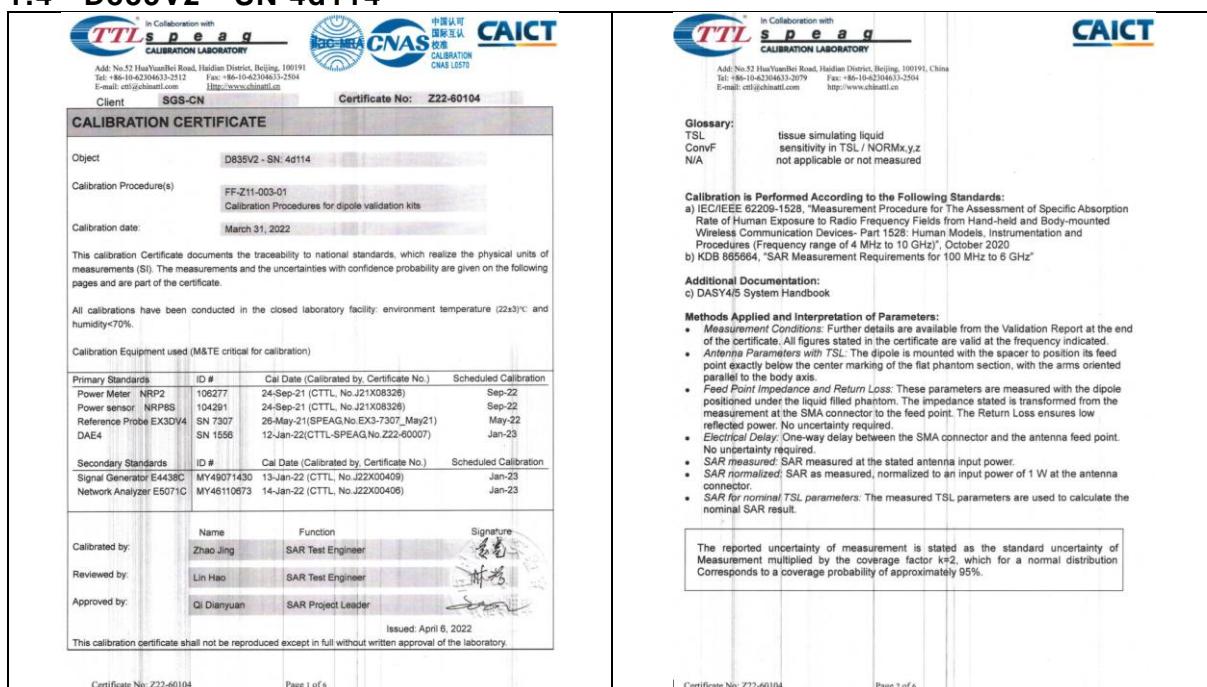



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Please note that the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.Doccheck@sgs.com](mailto:CN.Doccheck@sgs.com)

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300  
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 [www.sgsgroup.com.cn](http://www.sgsgroup.com.cn)  
t(86-512)57355888 f(86-512)57370818 [sgs.china@sgs.com](mailto:sgs.china@sgs.com)

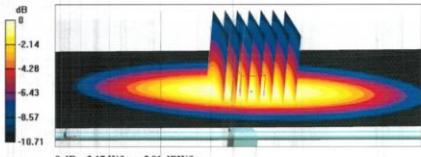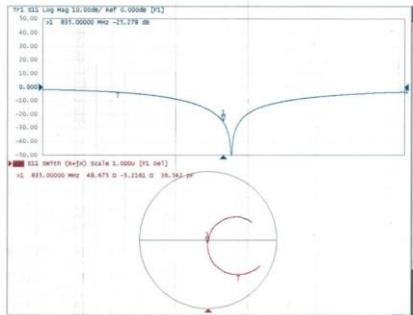

<div style="text-align: center;">  <p>In Collaboration with <b>CAICT</b></p> <p>Add: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: ctit@chinatec.cn http://www.chinatec.cn</p> <p><b>Measurement Conditions</b> DASY system configuration, as far as not given on page 1.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>DASY Version</td><td>DASY52</td><td>V52.10.4</td></tr> <tr><td>Extrapolation</td><td>Advanced Extrapolation</td><td></td></tr> <tr><td>Phantom</td><td>Triple Flat Phantom 5.1C</td><td></td></tr> <tr><td>Distance Dipole Center - TSL</td><td>15 mm</td><td>with Spacer</td></tr> <tr><td>Zoom Scan Resolution</td><td>dx, dy, dz = 5 mm</td><td></td></tr> <tr><td>Frequency</td><td>835 MHz ± 1 MHz</td><td></td></tr> </table> <p><b>Head TSL parameters</b> The following parameters and calculations were applied.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>41.5</td><td>0.90 mho/m</td></tr> <tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>41.0 ± 6 %</td><td>0.91 mho/m ± 6 %</td></tr> <tr><td>Head TSL temperature change during test</td><td>&lt;1.0 °C</td><td>—</td><td>—</td></tr> </table> <p><b>SAR result with Head TSL</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</td><td>Condition</td><td></td></tr> <tr><td>SAR measured</td><td>250 mW input power</td><td>2.37 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>9.49 W/kg ± 18.8 % (n=2)</td></tr> <tr><td>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</td><td>Condition</td><td></td></tr> <tr><td>SAR measured</td><td>250 mW input power</td><td>1.54 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>6.12 W/kg ± 18.7 % (n=2)</td></tr> </table> </div>	DASY Version	DASY52	V52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	15 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	835 MHz ± 1 MHz		Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	41.0 ± 6 %	0.91 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition		SAR measured	250 mW input power	2.37 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	9.49 W/kg ± 18.8 % (n=2)	SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition		SAR measured	250 mW input power	1.54 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	6.12 W/kg ± 18.7 % (n=2)	<div style="text-align: center;">  <p>In Collaboration with <b>CAICT</b></p> <p>Add: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: ctit@chinatec.cn http://www.chinatec.cn</p> <p><b>Appendix (Additional assessments outside the scope of CNAS L0570)</b></p> <p><b>Antenna Parameters with Head TSL</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Impedance, transformed to feed point</td><td>48.7Ω-5.22jΩ</td></tr> <tr><td>Return Loss</td><td>-25.3dB</td></tr> </table> <p><b>General Antenna Parameters and Design</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Electrical Delay (one direction)</td><td>1.307 ns</td></tr> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semi-rigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the standard. The antenna is not loaded according to the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p><b>Additional EUT Data</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Manufactured by</td><td>SPEAG</td></tr> </table> </div>	Impedance, transformed to feed point	48.7Ω-5.22jΩ	Return Loss	-25.3dB	Electrical Delay (one direction)	1.307 ns	Manufactured by	SPEAG
DASY Version	DASY52	V52.10.4																																																							
Extrapolation	Advanced Extrapolation																																																								
Phantom	Triple Flat Phantom 5.1C																																																								
Distance Dipole Center - TSL	15 mm	with Spacer																																																							
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																								
Frequency	835 MHz ± 1 MHz																																																								
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m																																																						
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.0 ± 6 %	0.91 mho/m ± 6 %																																																						
Head TSL temperature change during test	<1.0 °C	—	—																																																						
SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition																																																								
SAR measured	250 mW input power	2.37 W/kg																																																							
SAR for nominal Head TSL parameters	normalized to 1W	9.49 W/kg ± 18.8 % (n=2)																																																							
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition																																																								
SAR measured	250 mW input power	1.54 W/kg																																																							
SAR for nominal Head TSL parameters	normalized to 1W	6.12 W/kg ± 18.7 % (n=2)																																																							
Impedance, transformed to feed point	48.7Ω-5.22jΩ																																																								
Return Loss	-25.3dB																																																								
Electrical Delay (one direction)	1.307 ns																																																								
Manufactured by	SPEAG																																																								
Certificate No: Z22-60104 Page 2 of 6																																																									
<div style="display: flex; justify-content: space-around;"> <div style="text-align: center;">  <p>In Collaboration with <b>CAICT</b></p> <p>Add: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: ctit@chinatec.cn http://www.chinatec.cn</p> <p>DASY5's Variation Report for Head TSL Test Laboratory: CCAICT, Beijing China Date: 2022-03-31</p> <p><b>DUT:</b> Dipole 835 MHz; <b>Type:</b> DR35V2; <b>Serial:</b> DR35V2 - SN: 4d114 Communication System: UID 0; CW; Frequency: 835 MHz; Duty Cycle: 1:1 Medium parameters used: <math>\epsilon' = 835 \text{ MHz}</math>; <math>\sigma = 0.907 \text{ S/m}</math>; <math>\tau_s = 40.98</math>; <math>\rho = 1000 \text{ kg/m}^3</math> Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration:  <ul style="list-style-type: none"> <li>• Probe: EX3DV4 - SN7307; ConvF(10.13, 10.13, 10.13) @ 835 MHz; Calibrated: 2021-05-26</li> <li>• Sensor-Surface: 1.4mm (Mechanical Surface Detection)</li> <li>• Electronics: DAE4-Sn1556; Calibrated: 2022-01-12</li> <li>• Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062</li> <li>• DASY52 S2.10.4(1535); SEMCAD X 14.6.14(7501)</li> </ul> <p><b>Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0:</b> Measurement grid: <math>dx=5\text{mm}</math>, <math>dy=5\text{mm}</math>, <math>dz=5\text{mm}</math> Reference Value = 57.88 V/m; Power Drift = 0.04 dB Peak SAR (extrapolated) = 2.37 W/kg; SAR(10 g) = 1.54 W/kg Smallest distance from peaks to all points 3 dB below = 15.8 mm Ratio of SAR at M2 to SAR at M1 = 66.2% Maximum value of SAR (measured) = 3.17 W/kg</p>  <p>0 dB = 3.17 W/kg = 5.01 dBW/kg</p> </p></div> <div style="text-align: center;">  <p>Impedance Measurement Plot for Head TSL</p> <p>Y-axis: 50.00, 40.00, 30.00, 20.00, 10.00, 0.000, -10.00, -20.00, -30.00, -40.00, -50.00</p> <p>X-axis: 833.00000 MHz, 48.477 D -3.226jΩ, 16.563-μF</p> <p>Plot title: Y21 S21 Log Mag 10.00000/ Ref 1.00000 [Y21]</p> <p>Plot description: Y21 S21 Smith (X+jY) Scale 1.00000 [Y21, S21]</p> </div> </div>																																																									
Certificate No: Z22-60104 Page 5 of 6																																																									
Certificate No: Z22-60104 Page 6 of 6																																																									

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.


Attention: To need the authenticity of testing /Inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.Doccheck@sgs.com](mailto:CN.Doccheck@sgs.com)

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300  
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn  
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com



## 1.5 D900V2 - SN 1d079

    <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-62796531-2117 E-mail: offi@caict.ac.cn <a href="http://www.caict.ac.cn">http://www.caict.ac.cn</a></p> <p>Client SGS-CN Certificate No: Z22-60184</p> <p><b>CALIBRATION CERTIFICATE</b></p> <p>Object D900V2 - SN: 1d079</p> <p>Calibration Procedure(s) FF-Z11-003-01 Calibration Procedures for dipole validation kits</p> <p>Calibration date: June 7, 2022</p> <p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility, environment temperature (22±5)°C and humidity&lt;70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter NIP82</td> <td>10277</td> <td>24-Jan-21 (CTTL, No. J22X0026)</td> <td>Sept-22</td> </tr> <tr> <td>Power sensor NIP85</td> <td>10491</td> <td>24-Sep-21 (CTTL, No. J21X0326)</td> <td>Sept-22</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN 7464</td> <td>26-Jan-22(SPEAG No EX3-7464, Jan22)</td> <td>Jan-23</td> </tr> <tr> <td>DAE4</td> <td>SN 1558</td> <td>12-Jan-22(CTTL-SPEAG No Z22-8007)</td> <td>Jan-23</td> </tr> <tr> <td>Secondary Standards</td> <td>ID #</td> <td>Cal Date (Calibrated by, Certificate No.)</td> <td>Scheduled Calibration</td> </tr> <tr> <td>Signal Generator E4438C</td> <td>MY49071430</td> <td>13-Jan-22 (CTTL, No. J22X00409)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MY46110673</td> <td>14-Jan-22 (CTTL, No. J22X00406)</td> <td>Jan-23</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Calibrated by:</th> <th>Name</th> <th>Function</th> <th>Signature</th> </tr> </thead> <tbody> <tr> <td>Zhao Jing</td> <td>SAR Test Engineer</td> <td></td> <td></td> </tr> <tr> <td>Reviewed by:</td> <td>Lin Hao</td> <td>SAR Test Engineer</td> <td></td> </tr> <tr> <td>Approved by:</td> <td>Qi Dianyuan</td> <td>SAR Project Leader</td> <td></td> </tr> </tbody> </table> <p>Issued: June 13, 2022</p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> <p>Certificate No: Z22-60184 Page 1 of 6</p>	Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Power Meter NIP82	10277	24-Jan-21 (CTTL, No. J22X0026)	Sept-22	Power sensor NIP85	10491	24-Sep-21 (CTTL, No. J21X0326)	Sept-22	Reference Probe EX3DV4	SN 7464	26-Jan-22(SPEAG No EX3-7464, Jan22)	Jan-23	DAE4	SN 1558	12-Jan-22(CTTL-SPEAG No Z22-8007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL, No. J22X00409)	Jan-23	Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL, No. J22X00406)	Jan-23	Calibrated by:	Name	Function	Signature	Zhao Jing	SAR Test Engineer			Reviewed by:	Lin Hao	SAR Test Engineer		Approved by:	Qi Dianyuan	SAR Project Leader		  <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62796531-3217 E-mail: offi@caict.ac.cn <a href="http://www.caict.ac.cn">http://www.caict.ac.cn</a></p> <p><b>Glossary:</b> TSL tissue simulating liquid ConvF sensitivity in TSL / NORMxyz N/A not applicable or not measured</p> <p><b>Calibration is Performed According to the Following Standards:</b> a) IEC/IEEE 62209-1528, "Measurement Procedure for the Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDB 895994, "SAR Measurement Requirements for 100 MHz to 6 GHz"</p> <p><b>Additional Documentation:</b> o DASY4.5 System Handbook</p> <p><b>Methods Applied and Interpretation of Parameters:</b></p> <ul style="list-style-type: none"> <li>• <b>Antenna Configuration:</b> Further details are available from the Validation Report at the end of the certificate. All parameters in the certificate are valid at the frequency indicated.</li> <li>• <b>Antenna Parameters with TSL:</b> The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.</li> <li>• <b>Impedance and Return Loss:</b> These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance value is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.</li> <li>• <b>Time Delay:</b> One-way delay between the SMA connector and the antenna feed point.</li> <li>• <b>No uncertainty required.</b></li> <li>• <b>SAR measured:</b> SAR measured at the stated antenna input power.</li> <li>• <b>SAR normalized:</b> SAR as measured, normalized to an input power of 1 W at the antenna connector.</li> <li>• <b>SAR for nominal TSL parameters:</b> The measured TSL parameters are used to calculate the nominal SAR result.</li> </ul> <div style="border: 1px solid black; padding: 5px; margin-top: 10px;"> <p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p> </div> <p>Certificate No: Z22-60184 Page 2 of 6</p>												
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																										
Power Meter NIP82	10277	24-Jan-21 (CTTL, No. J22X0026)	Sept-22																																																										
Power sensor NIP85	10491	24-Sep-21 (CTTL, No. J21X0326)	Sept-22																																																										
Reference Probe EX3DV4	SN 7464	26-Jan-22(SPEAG No EX3-7464, Jan22)	Jan-23																																																										
DAE4	SN 1558	12-Jan-22(CTTL-SPEAG No Z22-8007)	Jan-23																																																										
Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																										
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL, No. J22X00409)	Jan-23																																																										
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL, No. J22X00406)	Jan-23																																																										
Calibrated by:	Name	Function	Signature																																																										
Zhao Jing	SAR Test Engineer																																																												
Reviewed by:	Lin Hao	SAR Test Engineer																																																											
Approved by:	Qi Dianyuan	SAR Project Leader																																																											
  <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62796531-2117 E-mail: offi@caict.ac.cn <a href="http://www.caict.ac.cn">http://www.caict.ac.cn</a></p> <p><b>Measurement system configuration, as far as not given on page 1:</b></p> <table border="1"> <thead> <tr> <th>DASY Version</th> <th>DASY92</th> <th>52.10.4</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>15 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>900 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table> <p><b>Head TSL parameters</b> The following parameters and calculations were applied.</p> <table border="1"> <thead> <tr> <th></th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>41.5</td> <td>0.97 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>42.1 ± 6 %</td> <td>0.98 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td>&lt;1.0 °C</td> <td>---</td> <td>---</td> </tr> </tbody> </table> <p><b>SAR result with Head TSL</b></p> <table border="1"> <thead> <tr> <th>SAR measured over 1 cm<sup>3</sup> (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>250 mW input power</td> <td></td> <td>2.76 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters normalized to 1W</td> <td></td> <td>11.0 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <td>SAR measured over 10 cm<sup>3</sup> (10 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>250 mW input power</td> <td></td> <td>1.78 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters normalized to 1W</td> <td></td> <td>7.09 W/kg ± 18.7 % (k=2)</td> </tr> </tbody> </table> <p>Certificate No: Z22-60184 Page 3 of 6</p>	DASY Version	DASY92	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple flat Phantom 5.1C		Distance Dipole Center - TSL	15 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	900 MHz ± 1 MHz			Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	41.5	0.97 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	42.1 ± 6 %	0.98 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	---	---	SAR measured over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition		250 mW input power		2.76 W/kg	SAR for nominal Head TSL parameters normalized to 1W		11.0 W/kg ± 18.8 % (k=2)	SAR measured over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition		250 mW input power		1.78 W/kg	SAR for nominal Head TSL parameters normalized to 1W		7.09 W/kg ± 18.7 % (k=2)	  <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62796531-3217 E-mail: offi@caict.ac.cn <a href="http://www.caict.ac.cn">http://www.caict.ac.cn</a></p> <p><b>Appendix (Additional assessments outside the scope of CNAS L0570)</b></p> <p><b>Antenna Parameters with Head TSL</b></p> <table border="1"> <thead> <tr> <th>Impedance, transformed to feed point</th> <th>48.10- 8.49jΩ</th> </tr> </thead> <tbody> <tr> <td>Return Loss</td> <td>-23.3 dB</td> </tr> </tbody> </table> <p><b>General Antenna Parameters and Design</b></p> <table border="1"> <thead> <tr> <th>Electrical Delay (one direction)</th> <th>1.312 ns</th> </tr> </thead> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard enrigid coaxial cable. The center conductor of the testing line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded with the liquid phantom explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The dipole impedance is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p><b>Additional EUT Data</b></p> <table border="1"> <thead> <tr> <th>Manufactured by</th> <th>SPEAG</th> </tr> </thead> </table> <p>Certificate No: Z22-60184 Page 4 of 6</p>	Impedance, transformed to feed point	48.10- 8.49jΩ	Return Loss	-23.3 dB	Electrical Delay (one direction)	1.312 ns	Manufactured by	SPEAG
DASY Version	DASY92	52.10.4																																																											
Extrapolation	Advanced Extrapolation																																																												
Phantom	Triple flat Phantom 5.1C																																																												
Distance Dipole Center - TSL	15 mm	with Spacer																																																											
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																												
Frequency	900 MHz ± 1 MHz																																																												
	Temperature	Permittivity	Conductivity																																																										
Nominal Head TSL parameters	22.0 °C	41.5	0.97 mho/m																																																										
Measured Head TSL parameters	(22.0 ± 0.2) °C	42.1 ± 6 %	0.98 mho/m ± 6 %																																																										
Head TSL temperature change during test	<1.0 °C	---	---																																																										
SAR measured over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition																																																												
250 mW input power		2.76 W/kg																																																											
SAR for nominal Head TSL parameters normalized to 1W		11.0 W/kg ± 18.8 % (k=2)																																																											
SAR measured over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition																																																												
250 mW input power		1.78 W/kg																																																											
SAR for nominal Head TSL parameters normalized to 1W		7.09 W/kg ± 18.7 % (k=2)																																																											
Impedance, transformed to feed point	48.10- 8.49jΩ																																																												
Return Loss	-23.3 dB																																																												
Electrical Delay (one direction)	1.312 ns																																																												
Manufactured by	SPEAG																																																												


Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To need the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.Doccheck@sgs.com](mailto:CN.Doccheck@sgs.com)

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300  
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 [www.sgsgroup.com.cn](http://www.sgsgroup.com.cn)  
t(86-512)57355888 f(86-512)57370818 [sgs.china@sgs.com](mailto:sgs.china@sgs.com)



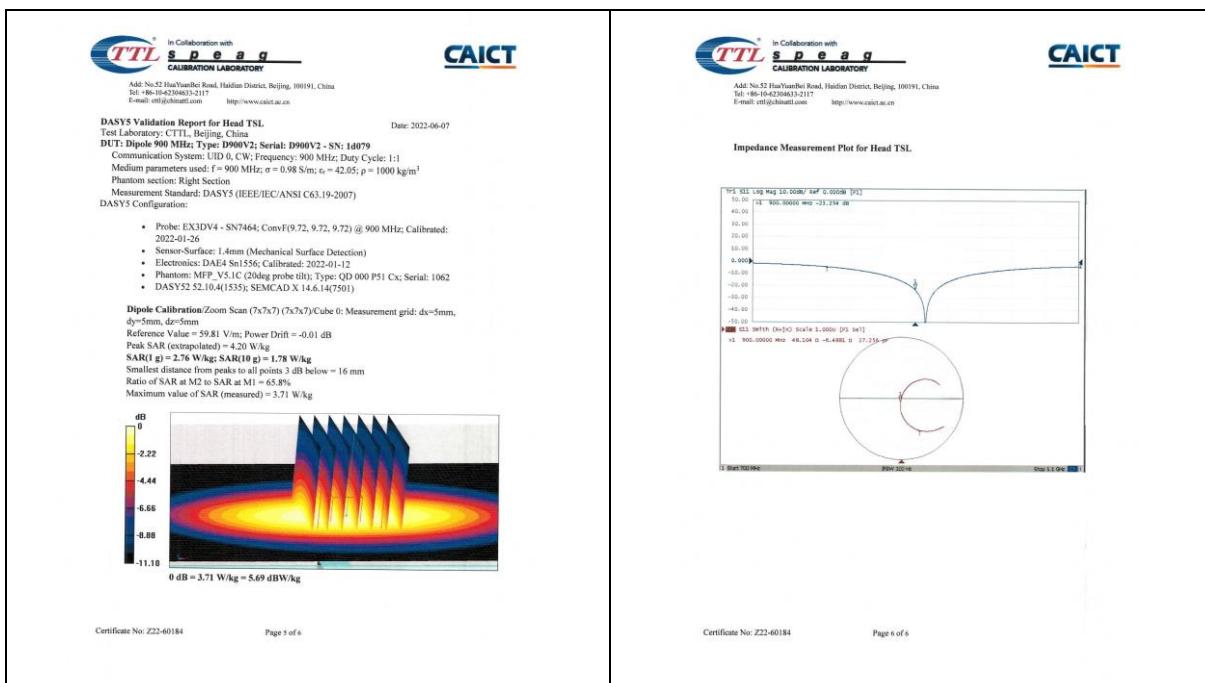

## 1.6 D1800V2 - SN 2d170

**TTL speag CALIBRATION LABORATORY**  
Add: No.52 HuaYanBei Road, Haidian District, Beijing, 100191  
Tel: +86-10-62304633-2112 Fax: +86-10-62304633-2504  
E-mail: cttl@caict.ac.cn <http://www.caict.ac.cn>

**CNAS** 中国认可 国家认可 CALIBRATION CNAS LIST

Client	SGS-CN	Certificate No:	Z22-60105
<b>CALIBRATION CERTIFICATE</b>			
Object	D1800V2 - SN: 2d170		
Calibration Procedure(s)	FF-Z11-003-01 Calibration Procedures for dipole validation kits		
Calibration date:	March 31, 2022		
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL, No.J21X08326)	Sep-22
Power sensor NRP85	104291	24-Sep-21 (CTTL, No.J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-22 (SPEAG No.EK-7307, May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL, No.J22X00409)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL, No.J22X00406)	Jan-23
Calibrated by:	Name	Function	Signature
Reviewed by:			
Approved by:			
Issued: April 6, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			

Certificate No: Z22-60105 Page 1 of 6

**TTL speag CALIBRATION LABORATORY**  
Add: No.52 HuaYanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@caict.ac.cn <http://www.caict.ac.cn>

**CAICT**

**Glossary:**  
TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORMx.y.z  
N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**  
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedure (Frequency range of 4 MHz to 10 GHz)", October 2020  
b) KDB 865864, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**  
c) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**  
• **Measuring Configuration:** Further details are available from the Validation Report at the end of the certificate. All figures in the certificate are valid at the frequency indicated.  
• **Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.  
• **Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measured value at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.  
• **Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.  
• **SAR measured:** SAR measured at the stated antenna input power.  
• **SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.  
• **SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60105 Page 2 of 6

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Please note that the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.Doccheck@sgs.com](mailto:CN.Doccheck@sgs.com)

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300  
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)5735888 f(86-512)57370818 [www.sgsgroup.com.cn](http://www.sgsgroup.com.cn)  
t(86-512)5735888 f(86-512)57370818 [sgs.china@sgs.com](mailto:sgs.china@sgs.com)



<p><b>TTL</b> <b>s p e a g</b> CALIBRATION LABORATORY</p> <p>Add: No.53 HuaYanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304613-2079 Fax: +86-10-62304613-2504 E-mail: ctt@chinattl.com http://www.chinattl.cn</p> <p><b>Measurement Conditions</b> DASY5 system configuration, as far as not given on page 1.</p> <table border="1"> <tr><td>DASY Version</td><td>DASY52</td><td>52.10.4</td></tr> <tr><td>Extrapolation</td><td>Advanced Extrapolation</td><td></td></tr> <tr><td>Phantom</td><td>Triple Flat Phantom 5.1C</td><td></td></tr> <tr><td>Distance Dipole Center - TSL</td><td>10 mm</td><td>with Spacer</td></tr> <tr><td>Zoom Scan Resolution</td><td>dx, dy, dz = 5 mm</td><td></td></tr> <tr><td>Frequency</td><td>1800 MHz ± 1 MHz</td><td></td></tr> </table> <p><b>Head TSL parameters</b> The following parameters and calculations were applied.</p> <table border="1"> <tr><th></th><th>Temperature</th><th>Permittivity</th><th>Conductivity</th></tr> <tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>40.0</td><td>1.40 mho/m</td></tr> <tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>40.6 ± 6 %</td><td>1.41 mho/m ± 6 %</td></tr> <tr><td>Head TSL temperature change during test</td><td>&lt;1.0 °C</td><td>—</td><td>—</td></tr> </table> <p><b>SAR result with Head TSL</b></p> <table border="1"> <tr><th>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</th><th>Condition</th></tr> <tr><td>SAR measured</td><td>250 mW input power 9.73 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W 38.9 W/kg ± 18.8 % (k=2)</td></tr> <tr><th>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</th><th>Condition</th></tr> <tr><td>SAR measured</td><td>250 mW input power 5.11 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W 20.4 W/kg ± 18.7 % (k=2)</td></tr> </table>	DASY Version	DASY52	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	1800 MHz ± 1 MHz			Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	40.6 ± 6 %	1.41 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	SAR measured	250 mW input power 9.73 W/kg	SAR for nominal Head TSL parameters	normalized to 1W 38.9 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	SAR measured	250 mW input power 5.11 W/kg	SAR for nominal Head TSL parameters	normalized to 1W 20.4 W/kg ± 18.7 % (k=2)	<p><b>CAICT</b></p> <p><b>TTL</b> <b>s p e a g</b> CALIBRATION LABORATORY</p> <p>Add: No.53 HuaYanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304613-2079 Fax: +86-10-62304613-2504 E-mail: ctt@chinattl.com http://www.chinattl.cn</p> <p><b>Appendix (Additional assessments outside the scope of CNAS L0570)</b></p> <p><b>Antenna Parameters with Head TSL</b></p> <table border="1"> <tr><td>Impedance, transformed to feed point</td><td>47.90- 2.54jΩ</td></tr> <tr><td>Return Loss</td><td>-29.4dB</td></tr> </table> <p><b>General Antenna Parameters and Design</b></p> <table border="1"> <tr><td>Electrical Delay (one direction)</td><td>1.116 ns</td></tr> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the standard. The overall dipole design is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p><b>Additional EUT Data</b></p> <table border="1"> <tr><td>Manufactured by</td><td>SPEAG</td></tr> </table>	Impedance, transformed to feed point	47.90- 2.54jΩ	Return Loss	-29.4dB	Electrical Delay (one direction)	1.116 ns	Manufactured by	SPEAG
DASY Version	DASY52	52.10.4																																																					
Extrapolation	Advanced Extrapolation																																																						
Phantom	Triple Flat Phantom 5.1C																																																						
Distance Dipole Center - TSL	10 mm	with Spacer																																																					
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																						
Frequency	1800 MHz ± 1 MHz																																																						
	Temperature	Permittivity	Conductivity																																																				
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m																																																				
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.6 ± 6 %	1.41 mho/m ± 6 %																																																				
Head TSL temperature change during test	<1.0 °C	—	—																																																				
SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition																																																						
SAR measured	250 mW input power 9.73 W/kg																																																						
SAR for nominal Head TSL parameters	normalized to 1W 38.9 W/kg ± 18.8 % (k=2)																																																						
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition																																																						
SAR measured	250 mW input power 5.11 W/kg																																																						
SAR for nominal Head TSL parameters	normalized to 1W 20.4 W/kg ± 18.7 % (k=2)																																																						
Impedance, transformed to feed point	47.90- 2.54jΩ																																																						
Return Loss	-29.4dB																																																						
Electrical Delay (one direction)	1.116 ns																																																						
Manufactured by	SPEAG																																																						
<p>Certificate No: Z22-60105 Page 3 of 6</p> <p><b>TTL</b> <b>s p e a g</b> CALIBRATION LABORATORY</p> <p>Add: No.53 HuaYanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304613-2079 Fax: +86-10-62304613-2504 E-mail: ctt@chinattl.com http://www.chinattl.cn</p> <p><b>DASY5 Validation Report for Head TSL</b> Test Laboratory: CTTL, Beijing, China Date: 2022-03-31</p> <p><b>DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN: 2d170</b> Communication System: UUD 0, CW; Frequency: 1800 MHz; Duty Cycle: 1:1 Medium parameters used: <math>\epsilon = 1800 \text{ MHz}</math>; <math>\sigma = 1.411 \text{ S/m}</math>; <math>\epsilon_r = 40.62</math>; <math>\rho = 1000 \text{ kg/m}^3</math> Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)</p> <p><b>DASY5 Configuration:</b></p> <ul style="list-style-type: none"> <li>Probe: EX3DV4 - SNT307; ConvF(8.34, 8.34, 8.34) @ 1800 MHz; Calibrated: 2021-05-26</li> <li>Sensor-Surface: 1.4mm (Mechanical Surface Detection)</li> <li>Electronics: DAE4 Sn1556; Calibrated: 2022-01-12</li> <li>Phantom: MFP_V3.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062</li> <li>DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)</li> </ul> <p><b>Probe Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm</b> Reference Value = 98.14 V/m; Power Drift = 0.03 dB Peak SAR (1 g) = 9.73 W/kg; SAR(10 g) = 38.9 W/kg Smallest distance from peaks to all points 3 dB below = 10 mm Ratio of SAR at M2 to SAR at M1 = 54% Maximum value of SAR (measured) = 15.2 W/kg</p> <p><b>Figure:</b> A 3D heatmap showing SAR distribution. The color scale ranges from -17.12 dB to 0 dB. The peak SAR value is 15.2 W/kg, which is 11.82 dBW/kg.</p>																																																							
<p>Certificate No: Z22-60105 Page 5 of 6</p> <p><b>CAICT</b></p> <p><b>TTL</b> <b>s p e a g</b> CALIBRATION LABORATORY</p> <p>Add: No.53 HuaYanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304613-2079 Fax: +86-10-62304613-2504 E-mail: ctt@chinattl.com http://www.chinattl.cn</p> <p><b>Impedance Measurement Plot for Head TSL</b></p>																																																							
<p>Certificate No: Z22-60105 Page 6 of 6</p>																																																							

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To need the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.Doccheck@sgs.com](mailto:CN.Doccheck@sgs.com)

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300  
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 [www.sgsgroup.com.cn](http://www.sgsgroup.com.cn)  
t(86-512)57355888 f(86-512)57370818 [sgs.china@sgs.com](mailto:sgs.china@sgs.com)



## 1.7 D1900V2 - SN 5d136

  <p>In Collaboration with SGS SPEAG CALIBRATION LABORATORY Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-62904532-2117 E-mail: sfl@caict.ac.cn <a href="http://www.caict.ac.cn">http://www.caict.ac.cn</a></p> <p>Client: SGS-CN Certificate No: Z22-60185</p> <p><b>CALIBRATION CERTIFICATE</b></p> <p>Object: D1900V2 - SN: 5d136</p> <p>Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits</p> <p>Calibration date: June 7, 2022</p> <p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility, environment temperature (22±5)°C and humidity&lt;70%.</p> <p>Calibration Equipment used (M&amp;TE criteria for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power sensor NRP2</td> <td>102277</td> <td>24-Sep-21 (CTTL No.J22X00409)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP85</td> <td>104291</td> <td>24-Sep-21 (CTTL No.J21X00326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN 7464</td> <td>26-Jan-22 (SPEAG No EX3-7464, Jan22)</td> <td>Jan-23</td> </tr> <tr> <td>DAEA</td> <td>SN 1558</td> <td>12-Jan-22 (CTTL-SPEAG No 222-60007)</td> <td>Jan-23</td> </tr> <tr> <td>Secondary Standards</td> <td>ID #</td> <td>Cal Date (Calibrated by, Certificate No.)</td> <td>Scheduled Calibration</td> </tr> <tr> <td>Signal Generator E4438C</td> <td>MY49071430</td> <td>13-Jan-22 (CTTL No.J22X00409)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MY48110673</td> <td>14-Jan-22 (CTTL No.J22X00406)</td> <td>Jan-23</td> </tr> </tbody> </table> <p>Calibrated by: Zhao Jing SAR Test Engineer </p> <p>Reviewed by: Lin Hao SAR Test Engineer </p> <p>Approved by: Qi Danyuan SAR Project Leader </p> <p>Issued: June 13, 2022</p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p>	Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Power sensor NRP2	102277	24-Sep-21 (CTTL No.J22X00409)	Sep-22	Power sensor NRP85	104291	24-Sep-21 (CTTL No.J21X00326)	Sep-22	Reference Probe EX3DV4	SN 7464	26-Jan-22 (SPEAG No EX3-7464, Jan22)	Jan-23	DAEA	SN 1558	12-Jan-22 (CTTL-SPEAG No 222-60007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23	Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00406)	Jan-23	 <p>In Collaboration with CAICT CALIBRATION LABORATORY Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62904532-2117 E-mail: sfl@caict.ac.cn <a href="http://www.caict.ac.cn">http://www.caict.ac.cn</a></p> <p><b>Glossary:</b></p> <p>TSL: tissue simulating liquid Conv/F: sensitivity in TSL / NORMix.y.z N/A: not applicable or not measured</p> <p><b>Calibration is Performed According to the Following Standards:</b></p> <p>a) IEC/IEEE 62209-1528, "Measurement Procedure for the Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Personal Communication Devices- Part 1528: Human Models, Instrumentation and Procedure (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"</p> <p><b>Additional Documentation:</b></p> <p>c) DASY4.3 System Handbook</p> <p><b>Methods Applied and Interpretation of Parameters:</b></p> <ul style="list-style-type: none"> <li>Measurement Conditions: Further details are available from the Validation Report at the end of this document. All figures and tables are valid at the frequency indicated.</li> <li>Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.</li> <li>Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transferred from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflection power. No uncertainty required.</li> <li>Electrical Delay: The electrical delay between the SMA connector and the antenna feed point.</li> <li>No uncertainty required.</li> <li>SAR measured: SAR measured at the stated antenna input power.</li> <li>SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna</li> <li>SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.</li> </ul> <p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p>																																																																																
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																																																																														
Power sensor NRP2	102277	24-Sep-21 (CTTL No.J22X00409)	Sep-22																																																																																																														
Power sensor NRP85	104291	24-Sep-21 (CTTL No.J21X00326)	Sep-22																																																																																																														
Reference Probe EX3DV4	SN 7464	26-Jan-22 (SPEAG No EX3-7464, Jan22)	Jan-23																																																																																																														
DAEA	SN 1558	12-Jan-22 (CTTL-SPEAG No 222-60007)	Jan-23																																																																																																														
Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																																																																														
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23																																																																																																														
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00406)	Jan-23																																																																																																														
<p>Certificate No: Z22-60185 Page 1 of 6</p> <p><b>Measurement Conditions</b> DASY system configuration, as far as not given on page 1.</p> <table border="1"> <thead> <tr> <th>DASY Version</th> <th>DASY2</th> <th>52.10.4</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>1900 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table> <p><b>Head TSL parameters</b> The following parameters and calculations were applied.</p> <table border="1"> <thead> <tr> <th></th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>23.0 °C</td> <td>40.0</td> <td>1.40 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>39.9 ± 6 %</td> <td>1.39 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td>41.0 °C</td> <td>—</td> <td>—</td> </tr> </tbody> </table> <p><b>SAR result with Head TSL</b></p> <table border="1"> <thead> <tr> <th>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>9.95 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>40.0 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <th>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>5.10 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>20.8 W/kg ± 18.7 % (k=2)</td> </tr> </tbody> </table> <p>Certificate No: Z22-60185 Page 2 of 6</p>	DASY Version	DASY2	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	1900 MHz ± 1 MHz			Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	23.0 °C	40.0	1.40 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	39.9 ± 6 %	1.39 mho/m ± 6 %	Head TSL temperature change during test	41.0 °C	—	—	SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition		SAR measured	250 mW input power	9.95 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	40.0 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition		SAR measured	250 mW input power	5.10 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	20.8 W/kg ± 18.7 % (k=2)	<p><b>Measurement Conditions</b> DASY system configuration, as far as not given on page 1.</p> <table border="1"> <thead> <tr> <th>DASY Version</th> <th>DASY2</th> <th>52.10.4</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>1900 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table> <p><b>Head TSL parameters</b> The following parameters and calculations were applied.</p> <table border="1"> <thead> <tr> <th></th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>23.0 °C</td> <td>40.0</td> <td>1.40 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>39.9 ± 6 %</td> <td>1.39 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td>41.0 °C</td> <td>—</td> <td>—</td> </tr> </tbody> </table> <p><b>SAR result with Head TSL</b></p> <table border="1"> <thead> <tr> <th>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>9.95 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>40.0 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <th>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>5.10 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>20.8 W/kg ± 18.7 % (k=2)</td> </tr> </tbody> </table> <p><b>Antenna Parameters with Head TSL</b></p> <table border="1"> <thead> <tr> <th>Impedance, Transformed to feed point</th> <th>51.20 ± 7.98 jΩ</th> </tr> </thead> <tbody> <tr> <td>Return Loss</td> <td>-22.4 dB</td> </tr> </tbody> </table> <p><b>General Antenna Parameters and Design</b></p> <table border="1"> <thead> <tr> <th>Electrical Delay (one direction)</th> <th>1.109 ns</th> </tr> </thead> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-biases. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded. The antenna is positioned as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change, because the antenna length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p><b>Additional EUT Data</b></p> <table border="1"> <thead> <tr> <th>Manufactured by</th> <th>SPEAG</th> </tr> </thead> </table> <p>Certificate No: Z22-60185 Page 4 of 6</p>	DASY Version	DASY2	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	1900 MHz ± 1 MHz			Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	23.0 °C	40.0	1.40 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	39.9 ± 6 %	1.39 mho/m ± 6 %	Head TSL temperature change during test	41.0 °C	—	—	SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition		SAR measured	250 mW input power	9.95 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	40.0 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition		SAR measured	250 mW input power	5.10 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	20.8 W/kg ± 18.7 % (k=2)	Impedance, Transformed to feed point	51.20 ± 7.98 jΩ	Return Loss	-22.4 dB	Electrical Delay (one direction)	1.109 ns	Manufactured by	SPEAG
DASY Version	DASY2	52.10.4																																																																																																															
Extrapolation	Advanced Extrapolation																																																																																																																
Phantom	Triple Flat Phantom 5.1C																																																																																																																
Distance Dipole Center - TSL	10 mm	with Spacer																																																																																																															
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																																																																																
Frequency	1900 MHz ± 1 MHz																																																																																																																
	Temperature	Permittivity	Conductivity																																																																																																														
Nominal Head TSL parameters	23.0 °C	40.0	1.40 mho/m																																																																																																														
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.9 ± 6 %	1.39 mho/m ± 6 %																																																																																																														
Head TSL temperature change during test	41.0 °C	—	—																																																																																																														
SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition																																																																																																																
SAR measured	250 mW input power	9.95 W/kg																																																																																																															
SAR for nominal Head TSL parameters	normalized to 1W	40.0 W/kg ± 18.8 % (k=2)																																																																																																															
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition																																																																																																																
SAR measured	250 mW input power	5.10 W/kg																																																																																																															
SAR for nominal Head TSL parameters	normalized to 1W	20.8 W/kg ± 18.7 % (k=2)																																																																																																															
DASY Version	DASY2	52.10.4																																																																																																															
Extrapolation	Advanced Extrapolation																																																																																																																
Phantom	Triple Flat Phantom 5.1C																																																																																																																
Distance Dipole Center - TSL	10 mm	with Spacer																																																																																																															
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																																																																																
Frequency	1900 MHz ± 1 MHz																																																																																																																
	Temperature	Permittivity	Conductivity																																																																																																														
Nominal Head TSL parameters	23.0 °C	40.0	1.40 mho/m																																																																																																														
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.9 ± 6 %	1.39 mho/m ± 6 %																																																																																																														
Head TSL temperature change during test	41.0 °C	—	—																																																																																																														
SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition																																																																																																																
SAR measured	250 mW input power	9.95 W/kg																																																																																																															
SAR for nominal Head TSL parameters	normalized to 1W	40.0 W/kg ± 18.8 % (k=2)																																																																																																															
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition																																																																																																																
SAR measured	250 mW input power	5.10 W/kg																																																																																																															
SAR for nominal Head TSL parameters	normalized to 1W	20.8 W/kg ± 18.7 % (k=2)																																																																																																															
Impedance, Transformed to feed point	51.20 ± 7.98 jΩ																																																																																																																
Return Loss	-22.4 dB																																																																																																																
Electrical Delay (one direction)	1.109 ns																																																																																																																
Manufactured by	SPEAG																																																																																																																


Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To need the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com


No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300  
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 [www.sgsgroup.com.cn](http://www.sgsgroup.com.cn)  
t(86-512)57355888 f(86-512)57370818 [sgs.china@sgs.com](mailto:sgs.china@sgs.com)



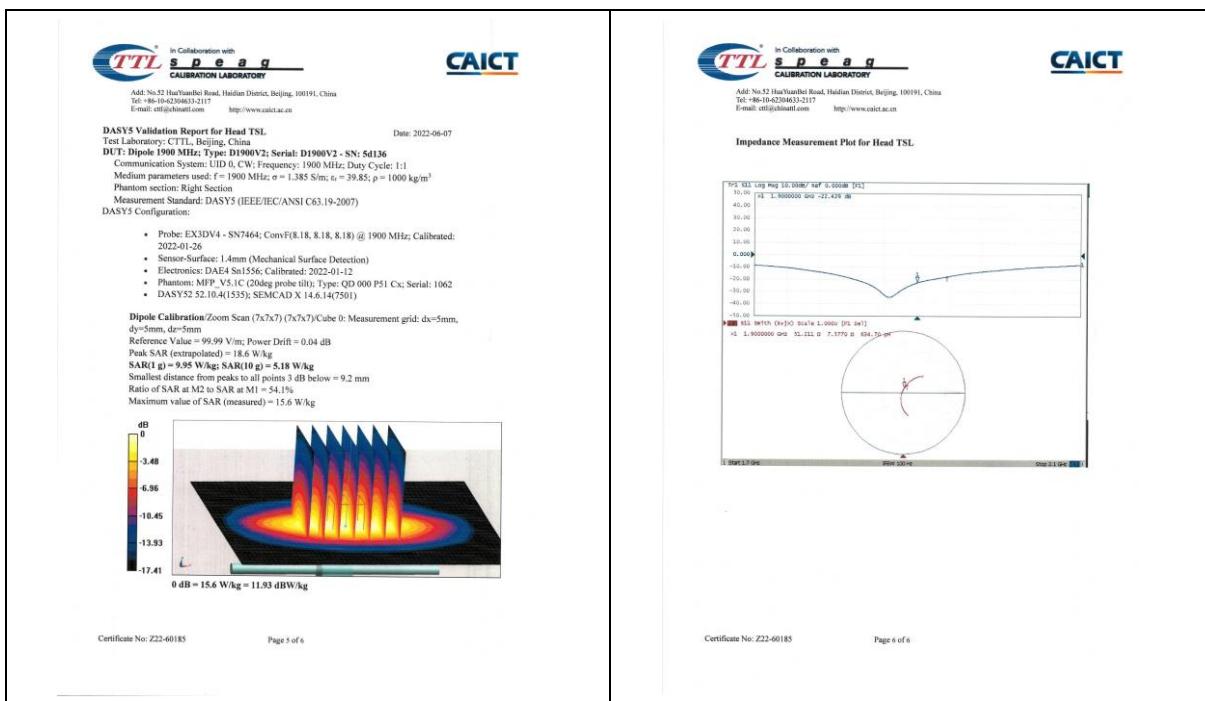

## 1.8 D2000V2 - SN 1041

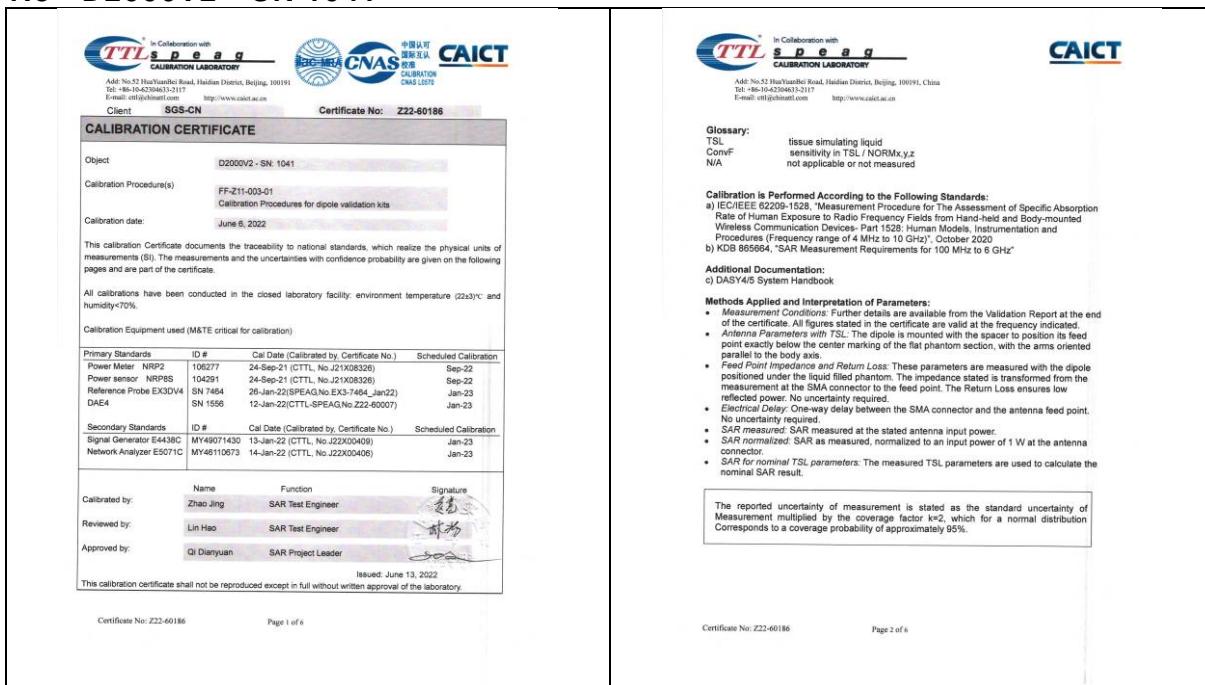



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention is drawn to the authenticity of testing /Inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.DocCheck@sgs.com](mailto:CN.DocCheck@sgs.com)



No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300  
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 [www.sgsgroup.com.cn](http://www.sgsgroup.com.cn)  
t(86-512)57355888 f(86-512)57370818 [sgs.china@sgs.com](mailto:sgs.china@sgs.com)
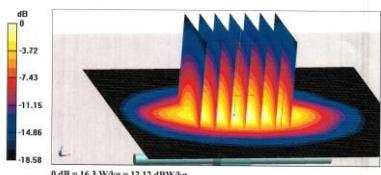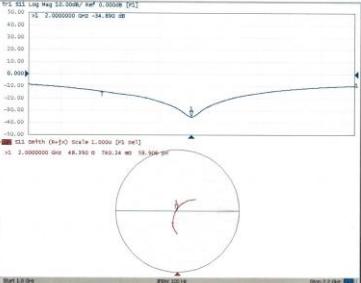
<div style="text-align: center;">  <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: cttl@chinatll.com <a href="http://www.caict.ac.cn">http://www.caict.ac.cn</a></p> <p><b>Measurement Conditions</b> DASY system configuration, as far as given on page 1.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>DASY Version</td><td>DASY52</td><td>52.10.4</td></tr> <tr><td>Extrapolation</td><td>Advanced Extrapolation</td><td></td></tr> <tr><td>Phantom</td><td>Triple Hat Phantom 5.1C</td><td></td></tr> <tr><td>Distance Dipole Center - TSL</td><td>10 mm</td><td>with Spacer</td></tr> <tr><td>Zoom Scan Resolution</td><td>dx, dy, dz = 5 mm</td><td></td></tr> <tr><td>Frequency</td><td>2000 MHz ± 1 MHz</td><td></td></tr> </table> <p><b>Head TSL parameters</b> The following parameters and calculations were applied:</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Temperature</td><td>Permittivity</td><td>Conductivity</td></tr> <tr><td>22.0 °C</td><td>40.0</td><td>1.40 mho/m</td></tr> <tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>40.2 ± 6 % 1.39 mho/m ± 6 %</td></tr> <tr><td>Head TSL temperature change during test</td><td>&lt;1.0 °C</td><td>—</td></tr> </table> <p><b>SAR result with Head TSL</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>250 mW input power</td><td>10.4 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>41.8 W/kg ± 18.8 % (n=2)</td></tr> <tr><td>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>250 mW input power</td><td>5.30 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>21.3 W/kg ± 18.7 % (n=2)</td></tr> </table> </div>	DASY Version	DASY52	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Hat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	2000 MHz ± 1 MHz		Temperature	Permittivity	Conductivity	22.0 °C	40.0	1.40 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	40.2 ± 6 % 1.39 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	SAR measured	250 mW input power	10.4 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	41.8 W/kg ± 18.8 % (n=2)	SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	SAR measured	250 mW input power	5.30 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	21.3 W/kg ± 18.7 % (n=2)	<div style="text-align: center;">  <p><b>in Collaboration with</b> <b>TTL speag</b> <b>CALIBRATION LABORATORY</b> Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: cttl@chinatll.com <a href="http://www.caict.ac.cn">http://www.caict.ac.cn</a></p> <p><b>Appendix (Additional assessments outside the scope of CNAS L0570)</b></p> <p><b>Antenna Parameters with Head TSL</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Impedance, transformed to feed port</td><td>48.40+ 0.74jΩ</td></tr> <tr><td>Return Loss</td><td>-34.9dB</td></tr> </table> <p><b>General Antenna Parameters and Design</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Electric Delay (one direction)</td><td>1.088 ns</td></tr> </table> <p>After long time use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semirigid coaxial cable. The center conductor of the testing line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded with a phantom. See "Antenna Parameters" paragraph. Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still adapted to the phantom.</p> <p>No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p><b>Additional EUT Data</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Manufactured by</td><td>SPEAG</td></tr> </table> </div>	Impedance, transformed to feed port	48.40+ 0.74jΩ	Return Loss	-34.9dB	Electric Delay (one direction)	1.088 ns	Manufactured by	SPEAG
DASY Version	DASY52	52.10.4																																																					
Extrapolation	Advanced Extrapolation																																																						
Phantom	Triple Hat Phantom 5.1C																																																						
Distance Dipole Center - TSL	10 mm	with Spacer																																																					
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																						
Frequency	2000 MHz ± 1 MHz																																																						
Temperature	Permittivity	Conductivity																																																					
22.0 °C	40.0	1.40 mho/m																																																					
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.2 ± 6 % 1.39 mho/m ± 6 %																																																					
Head TSL temperature change during test	<1.0 °C	—																																																					
SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition																																																						
SAR measured	250 mW input power	10.4 W/kg																																																					
SAR for nominal Head TSL parameters	normalized to 1W	41.8 W/kg ± 18.8 % (n=2)																																																					
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition																																																						
SAR measured	250 mW input power	5.30 W/kg																																																					
SAR for nominal Head TSL parameters	normalized to 1W	21.3 W/kg ± 18.7 % (n=2)																																																					
Impedance, transformed to feed port	48.40+ 0.74jΩ																																																						
Return Loss	-34.9dB																																																						
Electric Delay (one direction)	1.088 ns																																																						
Manufactured by	SPEAG																																																						
Certificate No: Z22-60186      Page 3 of 6																																																							
Certificate No: Z22-60186      Page 4 of 6																																																							
<div style="text-align: center;">  <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: cttl@chinatll.com <a href="http://www.caict.ac.cn">http://www.caict.ac.cn</a></p> <p><b>DASY5 Validation Report for Head TSL</b> Test Laboratory: CTTL, Beijing, China DUT: Dipole 2000 MHz, Type: D2000V2; Serial: D2000V2 - SN: 1041 Customer Selection: UUD 0, CW, Frequency: 2000 MHz, Duty Cycle: 1:1 Medium parameters used: f = 2000 MHz, ε = 1.392 Sim, σ = 40.21; ρ = 1000 kg/m<sup>3</sup> Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration:</p> <ul style="list-style-type: none"> <li>• Probe: EX304V4 - SN7464; ConvF(8.2, 8.2, 8.2) @ 2000 MHz; Calibrated: 2022-01-26</li> <li>• Sensor-Surface: 1.4mm (Mechanical Surface Detection)</li> <li>• Electronics: DAE4 Snt156; Calibrated: 2022-01-12</li> <li>• Phantom: MPP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062</li> <li>• DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)</li> </ul> <p><b>Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm</b> Reference Value = 103.4 V/m, Power Drift = 0.03 dB Peak SAR (extrapolated) = 19.6 W/kg SAR(1 g) = 10.4 W/kg; SAR(10 g) = 5.3 W/kg Smallest distance from peaks to all points 3 dB below = 9.1 mm Ratio of SAR at M2 to SAR at M1 = 53.6% Maximum value of SAR (measured) = 16.3 W/kg</p>  </div>	<div style="text-align: center;">  <p><b>in Collaboration with</b> <b>TTL speag</b> <b>CALIBRATION LABORATORY</b> Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: cttl@chinatll.com <a href="http://www.caict.ac.cn">http://www.caict.ac.cn</a></p> <p><b>Impedance Measurement Plot for Head TSL</b></p>  </div>																																																						
Certificate No: Z22-60186      Page 5 of 6																																																							
Certificate No: Z22-60186      Page 6 of 6																																																							

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To need the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.Doccheck@sgs.com](mailto:CN.Doccheck@sgs.com)



Compliance Certification Services (Kunshan) Inc.  
EMC Laboratory

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300  
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 [www.sgsgroup.com.cn](http://www.sgsgroup.com.cn)  
t(86-512)57355888 f(86-512)57370818 [sgs.china@sgs.com](mailto:sgs.china@sgs.com)


## 1.9 D2300V2 - SN 1096

    <p>Object: D2300V2 - SN: 1096</p> <p>Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits</p> <p>Calibration date: March 31, 2022</p> <p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity &lt;70%.</p> <p>Calibration Equipment used (MATE critical for calibration)</p> <table border="1"> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> <tr> <td>Power Meter NRP2</td> <td>106277</td> <td>24-Sep-21 (CTTL, No. J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP8S</td> <td>104291</td> <td>24-Sep-21 (CTTL, No. J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN 7307</td> <td>26-May-21 (SPEAG No.EK3-7307, May21)</td> <td>May-22</td> </tr> <tr> <td>DAE4</td> <td>SN 1556</td> <td>12-Jan-22 (CTTL-SPEAG No.222-60007)</td> <td>Jan-23</td> </tr> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> <tr> <td>Signal Generator E4438C</td> <td>MY49071430</td> <td>13-Jan-22 (CTTL, No. J22X00409)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MY46110673</td> <td>14-Jan-22 (CTTL, No. J22X00406)</td> <td>Jan-23</td> </tr> </table> <table border="1"> <tr> <th>Calibrated by:</th> <th>Name</th> <th>Function</th> <th>Signature</th> </tr> <tr> <td>Zhao Jing</td> <td>SAR Test Engineer</td> <td></td> <td></td> </tr> <tr> <th>Reviewed by:</th> <td>Lin Hao</td> <td>SAR Test Engineer</td> <td></td> </tr> <tr> <th>Approved by:</th> <td>Qi Dianyuan</td> <td>SAR Project Leader</td> <td></td> </tr> </table> <p>Issued: April 6, 2022</p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p>		Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Power Meter NRP2	106277	24-Sep-21 (CTTL, No. J21X08326)	Sep-22	Power sensor NRP8S	104291	24-Sep-21 (CTTL, No. J21X08326)	Sep-22	Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No.EK3-7307, May21)	May-22	DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.222-60007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL, No. J22X00409)	Jan-23	Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL, No. J22X00406)	Jan-23	Calibrated by:	Name	Function	Signature	Zhao Jing	SAR Test Engineer			Reviewed by:	Lin Hao	SAR Test Engineer		Approved by:	Qi Dianyuan	SAR Project Leader		  <p>Object: D2300V2 - SN: 1096</p> <p>Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits</p> <p>Calibration date: March 31, 2022</p> <p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity &lt;70%.</p> <p>Calibration Equipment used (MATE critical for calibration)</p> <table border="1"> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> <tr> <td>Power Meter NRP2</td> <td>106277</td> <td>24-Sep-21 (CTTL, No. J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP8S</td> <td>104291</td> <td>24-Sep-21 (CTTL, No. J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN 7307</td> <td>26-May-21 (SPEAG No.EK3-7307, May21)</td> <td>May-22</td> </tr> <tr> <td>DAE4</td> <td>SN 1556</td> <td>12-Jan-22 (CTTL-SPEAG No.222-60007)</td> <td>Jan-23</td> </tr> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> <tr> <td>Signal Generator E4438C</td> <td>MY49071430</td> <td>13-Jan-22 (CTTL, No. J22X00409)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MY46110673</td> <td>14-Jan-22 (CTTL, No. J22X00406)</td> <td>Jan-23</td> </tr> </table> <table border="1"> <tr> <th>Calibrated by:</th> <th>Name</th> <th>Function</th> <th>Signature</th> </tr> <tr> <td>Zhao Jing</td> <td>SAR Test Engineer</td> <td></td> <td></td> </tr> <tr> <th>Reviewed by:</th> <td>Lin Hao</td> <td>SAR Test Engineer</td> <td></td> </tr> <tr> <th>Approved by:</th> <td>Qi Dianyuan</td> <td>SAR Project Leader</td> <td></td> </tr> </table> <p>Issued: April 6, 2022</p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p>	Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Power Meter NRP2	106277	24-Sep-21 (CTTL, No. J21X08326)	Sep-22	Power sensor NRP8S	104291	24-Sep-21 (CTTL, No. J21X08326)	Sep-22	Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No.EK3-7307, May21)	May-22	DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.222-60007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL, No. J22X00409)	Jan-23	Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL, No. J22X00406)	Jan-23	Calibrated by:	Name	Function	Signature	Zhao Jing	SAR Test Engineer			Reviewed by:	Lin Hao	SAR Test Engineer		Approved by:	Qi Dianyuan	SAR Project Leader	
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																																																															
Power Meter NRP2	106277	24-Sep-21 (CTTL, No. J21X08326)	Sep-22																																																																																															
Power sensor NRP8S	104291	24-Sep-21 (CTTL, No. J21X08326)	Sep-22																																																																																															
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No.EK3-7307, May21)	May-22																																																																																															
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.222-60007)	Jan-23																																																																																															
Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																																																															
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL, No. J22X00409)	Jan-23																																																																																															
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL, No. J22X00406)	Jan-23																																																																																															
Calibrated by:	Name	Function	Signature																																																																																															
Zhao Jing	SAR Test Engineer																																																																																																	
Reviewed by:	Lin Hao	SAR Test Engineer																																																																																																
Approved by:	Qi Dianyuan	SAR Project Leader																																																																																																
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																																																															
Power Meter NRP2	106277	24-Sep-21 (CTTL, No. J21X08326)	Sep-22																																																																																															
Power sensor NRP8S	104291	24-Sep-21 (CTTL, No. J21X08326)	Sep-22																																																																																															
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No.EK3-7307, May21)	May-22																																																																																															
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.222-60007)	Jan-23																																																																																															
Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																																																															
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL, No. J22X00409)	Jan-23																																																																																															
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL, No. J22X00406)	Jan-23																																																																																															
Calibrated by:	Name	Function	Signature																																																																																															
Zhao Jing	SAR Test Engineer																																																																																																	
Reviewed by:	Lin Hao	SAR Test Engineer																																																																																																
Approved by:	Qi Dianyuan	SAR Project Leader																																																																																																
<p>Certificate No: Z22-60106 Page 1 of 6</p> <p><b>Measurement Conditions</b> DASY system configuration, as far as not given on page 1</p> <table border="1"> <tr> <td>DASY Version</td> <td>DASY2</td> <td>52.10.4</td> </tr> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz &lt; 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>2300 MHz ± 1 MHz</td> <td></td> </tr> </table> <p><b>Head TSL parameters</b> The following parameters and calculations were applied.</p> <table border="1"> <tr> <td></td> <td>Temperature</td> <td>Permittivity</td> <td>Conductivity</td> </tr> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>39.5</td> <td>1.67 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>39.8 ± 6 %</td> <td>1.70 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td>&lt;1.0 °C</td> <td>—</td> <td>—</td> </tr> </table> <p><b>SAR result with Head TSL</b></p> <table border="1"> <tr> <td>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>12.4 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>49.2 W/kg ± 18.8 % (R=2)</td> </tr> <tr> <td>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>5.88 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>23.4 W/kg ± 18.7 % (R=2)</td> </tr> </table>		DASY Version	DASY2	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz < 5 mm		Frequency	2300 MHz ± 1 MHz			Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	39.5	1.67 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	39.8 ± 6 %	1.70 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition		SAR measured	250 mW input power	12.4 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	49.2 W/kg ± 18.8 % (R=2)	SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition		SAR measured	250 mW input power	5.88 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	23.4 W/kg ± 18.7 % (R=2)	<p>Certificate No: Z22-60106 Page 2 of 6</p> <p><b>Methods Applied and Interpretation of Parameters:</b></p> <ul style="list-style-type: none"> <li>Measurement Procedure: Further details are available from the Validation Report at the end of the certificate. All figures given in the certificate are valid at the frequency indicated.</li> <li>Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.</li> <li>Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the feed point to the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.</li> <li>Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.</li> <li>SAR measured: SAR measured at the stated antenna input power.</li> <li>SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.</li> <li>SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.</li> </ul> <p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p>																																												
DASY Version	DASY2	52.10.4																																																																																																
Extrapolation	Advanced Extrapolation																																																																																																	
Phantom	Triple Flat Phantom 5.1C																																																																																																	
Distance Dipole Center - TSL	10 mm	with Spacer																																																																																																
Zoom Scan Resolution	dx, dy, dz < 5 mm																																																																																																	
Frequency	2300 MHz ± 1 MHz																																																																																																	
	Temperature	Permittivity	Conductivity																																																																																															
Nominal Head TSL parameters	22.0 °C	39.5	1.67 mho/m																																																																																															
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.8 ± 6 %	1.70 mho/m ± 6 %																																																																																															
Head TSL temperature change during test	<1.0 °C	—	—																																																																																															
SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition																																																																																																	
SAR measured	250 mW input power	12.4 W/kg																																																																																																
SAR for nominal Head TSL parameters	normalized to 1W	49.2 W/kg ± 18.8 % (R=2)																																																																																																
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition																																																																																																	
SAR measured	250 mW input power	5.88 W/kg																																																																																																
SAR for nominal Head TSL parameters	normalized to 1W	23.4 W/kg ± 18.7 % (R=2)																																																																																																
<p>Certificate No: Z22-60106 Page 3 of 6</p> <p><b>Appendix (Additional assessments outside the scope of CNAS L0570)</b></p> <p><b>Antenna Parameters with Head TSL</b></p> <table border="1"> <tr> <td>Impedance, transformed to feed point</td> <td>49.2D-4.56jΩ</td> </tr> <tr> <td>Return Loss</td> <td>-26.6dB</td> </tr> </table> <p><b>General Antenna Parameters and Design</b></p> <table border="1"> <tr> <td>Electrical Delay (one direction)</td> <td>1.083 ns</td> </tr> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the standard. The antenna parameters in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p><b>Additional EUT Data</b></p> <table border="1"> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </table>		Impedance, transformed to feed point	49.2D-4.56jΩ	Return Loss	-26.6dB	Electrical Delay (one direction)	1.083 ns	Manufactured by	SPEAG	<p>Certificate No: Z22-60106 Page 4 of 6</p>																																																																																								
Impedance, transformed to feed point	49.2D-4.56jΩ																																																																																																	
Return Loss	-26.6dB																																																																																																	
Electrical Delay (one direction)	1.083 ns																																																																																																	
Manufactured by	SPEAG																																																																																																	

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention is drawn to the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.Doccheck@sgs.com](mailto:CN.Doccheck@sgs.com)



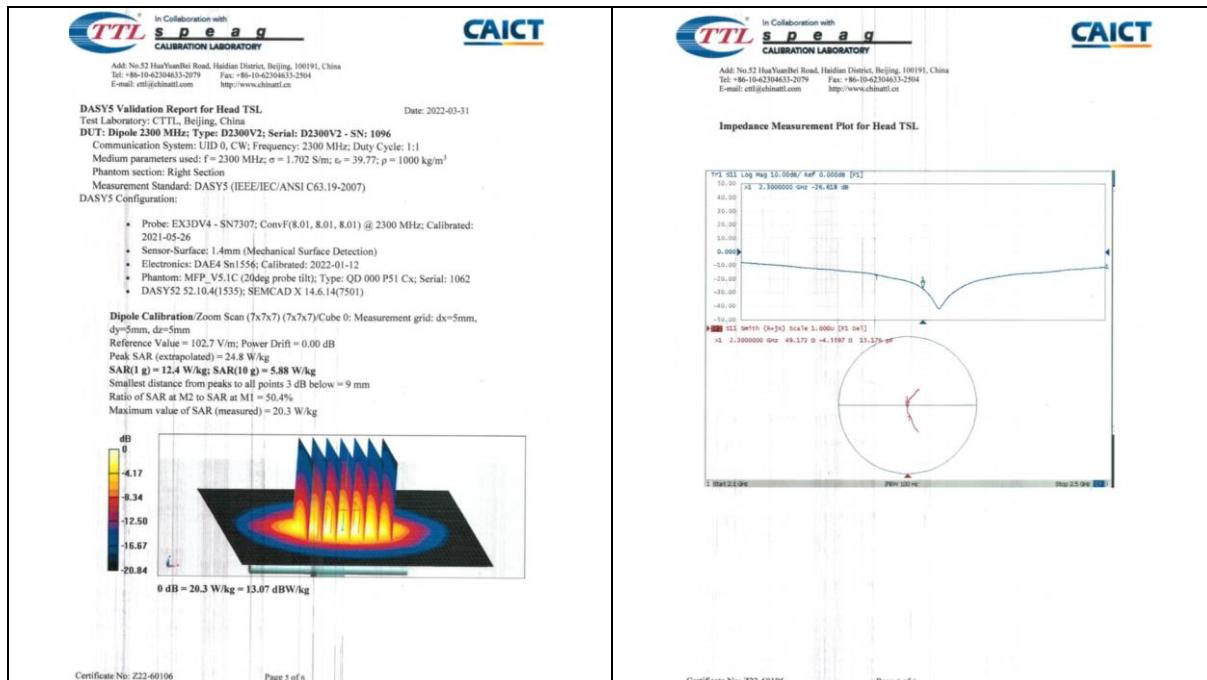

## 1.10 D2450V2 - SN 817





Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Please note that the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.Doccheck@sgs.com](mailto:CN.Doccheck@sgs.com)

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300  
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 [www.sgsgroup.com.cn](http://www.sgsgroup.com.cn)  
t(86-512)57355888 f(86-512)57370818 [sgs.china@sgs.com](mailto:sgs.china@sgs.com)

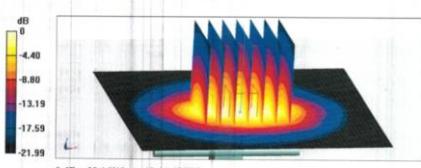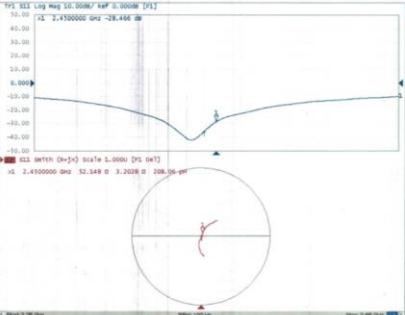

 <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: ctfl@chinattl.com http://www.chinattl.cn</p> <p><b>Measurement Conditions</b> DASY system configuration, as far as not given on page 1.</p> <table border="1"> <tr><td>DASY Version</td><td>DASY2</td><td>52.10.4</td></tr> <tr><td>Extrapolation</td><td>Advanced Extrapolation</td><td></td></tr> <tr><td>Phantom</td><td>Triple Flat Phantom 5.1C</td><td></td></tr> <tr><td>Distance Dipole Center - TSL</td><td>10 mm</td><td>with Spacer</td></tr> <tr><td>Zoom Scan Resolution</td><td>dx, dy, dz = 5 mm</td><td></td></tr> <tr><td>Frequency</td><td>2450 MHz ± 1 MHz</td><td></td></tr> </table> <p><b>Head TSL parameters</b> The following parameters and calculations were applied.</p> <table border="1"> <tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>39.2</td><td>1.80 mho/m</td></tr> <tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>39.5 ± 6 %</td><td>1.79 mho/m ± 6 %</td></tr> <tr><td>Head TSL temperature change during test</td><td>&lt;1.0 °C</td><td>—</td><td>—</td></tr> </table> <p><b>SAR result with Head TSL</b></p> <table border="1"> <tr><td>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</td><td>Condition</td><td></td></tr> <tr><td>SAR measured</td><td>250 mW input power</td><td>13.2 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>83.0 W/kg ± 18.8 % (k=2)</td></tr> <tr><td>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</td><td>Condition</td><td></td></tr> <tr><td>SAR measured</td><td>250 mW input power</td><td>6.15 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>24.7 W/kg ± 18.7 % (k=2)</td></tr> </table>		DASY Version	DASY2	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	2450 MHz ± 1 MHz		Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	39.5 ± 6 %	1.79 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition		SAR measured	250 mW input power	13.2 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	83.0 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition		SAR measured	250 mW input power	6.15 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	24.7 W/kg ± 18.7 % (k=2)	 <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: ctfl@chinattl.com http://www.chinattl.cn</p> <p><b>Appendix (Additional assessments outside the scope of CNAS L0570)</b></p> <p><b>Antenna Parameters with Head TSL</b></p> <table border="1"> <tr><td>Impedance, transformed to feed point</td><td>52.10+ 3.29jΩ</td></tr> <tr><td>Return Loss</td><td>-28.5dB</td></tr> </table> <p><b>General Antenna Parameters and Design</b></p> <table border="1"> <tr><td>Electrical Delay (one direction)</td><td>1.066 ns</td></tr> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the standard. The dipole arms are soldered to the printed circuit board. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p><b>Additional EUT Data</b></p> <table border="1"> <tr><td>Manufactured by</td><td>SPEAG</td></tr> </table>		Impedance, transformed to feed point	52.10+ 3.29jΩ	Return Loss	-28.5dB	Electrical Delay (one direction)	1.066 ns	Manufactured by	SPEAG
DASY Version	DASY2	52.10.4																																																									
Extrapolation	Advanced Extrapolation																																																										
Phantom	Triple Flat Phantom 5.1C																																																										
Distance Dipole Center - TSL	10 mm	with Spacer																																																									
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																										
Frequency	2450 MHz ± 1 MHz																																																										
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m																																																								
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.5 ± 6 %	1.79 mho/m ± 6 %																																																								
Head TSL temperature change during test	<1.0 °C	—	—																																																								
SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition																																																										
SAR measured	250 mW input power	13.2 W/kg																																																									
SAR for nominal Head TSL parameters	normalized to 1W	83.0 W/kg ± 18.8 % (k=2)																																																									
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition																																																										
SAR measured	250 mW input power	6.15 W/kg																																																									
SAR for nominal Head TSL parameters	normalized to 1W	24.7 W/kg ± 18.7 % (k=2)																																																									
Impedance, transformed to feed point	52.10+ 3.29jΩ																																																										
Return Loss	-28.5dB																																																										
Electrical Delay (one direction)	1.066 ns																																																										
Manufactured by	SPEAG																																																										
<p>Certificate No: Z22-60107 Page 3 of 6</p>  <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: ctfl@chinattl.com http://www.chinattl.cn</p> <p><b>DASY3 Validation Report for Head TSL</b> Test Laboratory: CTTL, Beijing China DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 817 Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium parameters used: <math>\epsilon' = 2450</math> MHz, <math>\sigma = 1.79</math> S/m, <math>\epsilon_r = 39.52</math>, <math>\rho = 1000</math> kg/m<sup>3</sup> Phantom section: Right Section Measurement Standard: DASY3 (IEEE/IEC/ANSI C63.19-2007) DASY3 Configuration:</p> <ul style="list-style-type: none"> <li>Probe: EX3DV4 - SN7307; ConvF(7.75, 7.75, 7.75) @ 2450 MHz; Calibrated: 2021-05-26</li> <li>Sensor-Surface: 1.4mm (Mechanical Surface Detection)</li> <li>Electronics: DAE4 Sn1556; Calibrated: 2022-01-12</li> <li>Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062</li> <li>DASY2 52.10.4(535); SEMCAD X 14.6.147(550)</li> </ul> <p>Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)Cu/0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 104.6 V/m; Power Drift = -0.03 dB Peak SAR (1 g) = 13.2 W/kg; SAR(10 g) = 6.15 W/kg Smallest distance from peaks to all points 3 dB below = 8.9 mm Ratio of SAR at M2 to SAR at M1 = 49.2% Maximum value of SAR (measured) = 22.1 W/kg</p> <p></p>		<p>Certificate No: Z22-60107 Page 4 of 6</p>  <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: ctfl@chinattl.com http://www.chinattl.cn</p> <p><b>Impedance Measurement Plot for Head TSL</b></p> <p></p>																																																									



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To need the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.Doccheck@sgs.com](mailto:CN.Doccheck@sgs.com)

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300  
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 [www.sgsgroup.com.cn](http://www.sgsgroup.com.cn)  
t(86-512)57355888 f(86-512)57370818 [sgs.china@sgs.com](mailto:sgs.china@sgs.com)


## 1.11 D2600V2 - SN 1158

 <p>In Collaboration with <b>TTL speag</b> CALIBRATION LABORATORY</p> <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504 E-mail: ctt@chinattl.com <a href="http://www.chinattl.com">http://www.chinattl.com</a></p> <p>Client: SGS-CN Certificate No: Z22-60108</p> <p><b>CALIBRATION CERTIFICATE</b></p> <p>Object: D2600V2 - SN: 1158</p> <p>Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits</p> <p>Calibration date: March 31, 2022</p> <p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity &gt;70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> <tr> <td>Power Meter NRP2</td> <td>106277</td> <td>24-Sep-21 (CTTL, No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP8</td> <td>104291</td> <td>24-Sep-21 (CTTL, No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN 7307</td> <td>26-May-21 (SPEAG No. EX3-7307-May21)</td> <td>May-22</td> </tr> <tr> <td>DAE4</td> <td>SN 1556</td> <td>12-Jan-22 (CTTL-SPEAG No. Z22-60007)</td> <td>Jan-23</td> </tr> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> <tr> <td>Signal Generator E4438C</td> <td>MY49071430</td> <td>13-Jan-22 (CTTL, No.J22X04049)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MY46110673</td> <td>14-Jan-22 (CTTL, No.J22X04046)</td> <td>Jan-23</td> </tr> </table> <p>Calibrated by: Zhao Jing (Signature)</p> <p>Reviewed by: Lin Hao (Signature)</p> <p>Approved by: Qi Dianyuan (Signature)</p> <p>Issued: April 6, 2022</p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p>	Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Power Meter NRP2	106277	24-Sep-21 (CTTL, No.J21X08326)	Sep-22	Power sensor NRP8	104291	24-Sep-21 (CTTL, No.J21X08326)	Sep-22	Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No. EX3-7307-May21)	May-22	DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL, No.J22X04049)	Jan-23	Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL, No.J22X04046)	Jan-23	 <p>In Collaboration with <b>TTL speag</b> CALIBRATION LABORATORY</p> <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: ctt@chinattl.com <a href="http://www.chinattl.com">http://www.chinattl.com</a></p> <p><b>Glossary:</b> TSL tissue simulating liquid ConvF sensitivity in TSL / NORMx,y,z N/A not applicable or not measured</p> <p><b>Calibration is Performed According to the Following Standards:</b></p> <ul style="list-style-type: none"> <li>a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices - Part 1528: Human Models, Instrumentation and Procedure (Frequency range of 4 MHz to 10 GHz)", October 2020</li> <li>b) KDB 655664, "SAR Measurement Requirements for 100 MHz to 6 GHz"</li> </ul> <p><b>Additional Documentation:</b></p> <ul style="list-style-type: none"> <li>c) DASY4/S System Handbook</li> </ul> <p><b>Methods Applied and Interpretation of Parameters:</b></p> <ul style="list-style-type: none"> <li>• <b>Measurement Conditions:</b> Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.</li> <li>• <b>Antenna Parameters with TSL:</b> The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.</li> <li>• <b>Feed Point Impedance and Return Loss:</b> These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measured at the SMA connector to the feed point. The Return Loss ensures low reflected power. No de-embedding required.</li> <li>• <b>Electrical Delay:</b> One-way delay between the SMA connector and the antenna feed point. No uncertainty required.</li> <li>• <b>SAR measured:</b> SAR measured at the stated antenna input power.</li> <li>• <b>SAR normalized:</b> SAR as measured, normalized to an input power of 1 W at the antenna connector.</li> <li>• <b>SAR for nominal TSL parameters:</b> The measured TSL parameters are used to calculate the nominal SAR result.</li> </ul> <p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.</p>																														
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																												
Power Meter NRP2	106277	24-Sep-21 (CTTL, No.J21X08326)	Sep-22																																																												
Power sensor NRP8	104291	24-Sep-21 (CTTL, No.J21X08326)	Sep-22																																																												
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No. EX3-7307-May21)	May-22																																																												
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23																																																												
Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																												
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL, No.J22X04049)	Jan-23																																																												
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL, No.J22X04046)	Jan-23																																																												
<p>Certificate No: Z22-60108 Page 1 of 6</p> <p><b>Measurement Conditions</b> DASY system configuration, as far as not given on page 1.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td>DASY Version</td> <td>DASY52</td> <td>52.10.4</td> </tr> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz &lt; 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>2600 MHz ± 1 MHz</td> <td></td> </tr> </table> <p><b>Head TSL parameters</b> The following parameters and calculations were applied:</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td></td> <td>Temperature</td> <td>Permittivity</td> <td>Conductivity</td> </tr> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>39.0</td> <td>1.96 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>38.7 ± 6 %</td> <td>1.96 mho/m ± 8 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td>&lt;1.0 °C</td> <td>—</td> <td>—</td> </tr> </table> <p><b>SAR result with Head TSL</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>13.7 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>54.8 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>6.12 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>24.5 W/kg ± 18.7 % (k=2)</td> </tr> </table>		DASY Version	DASY52	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz < 5 mm		Frequency	2600 MHz ± 1 MHz			Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	39.0	1.96 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	38.7 ± 6 %	1.96 mho/m ± 8 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition		SAR measured	250 mW input power	13.7 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	54.8 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition		SAR measured	250 mW input power	6.12 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	24.5 W/kg ± 18.7 % (k=2)	<p>Certificate No: Z22-60108 Page 2 of 6</p> <p><b>Appendix (Additional assessments outside the scope of CNAS L0570)</b></p> <p><b>Antenna Parameters with Head TSL</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td>Impedance, transformed to feed point</td> <td>49.9Ω-6.49Ω</td> </tr> <tr> <td>Return Loss</td> <td>-23.8dB</td> </tr> </table> <p><b>General Antenna Parameters and Design</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td>Electrical Delay (one direction)</td> <td>1.053 ns</td> </tr> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the test conditions mentioned in the "Measurement Conditions" paragraph. The SAR data are not affected by the change. The overall dipole is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p><b>Additional EUT Data</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </table>		Impedance, transformed to feed point	49.9Ω-6.49Ω	Return Loss	-23.8dB	Electrical Delay (one direction)	1.053 ns	Manufactured by	SPEAG
DASY Version	DASY52	52.10.4																																																													
Extrapolation	Advanced Extrapolation																																																														
Phantom	Triple Flat Phantom 5.1C																																																														
Distance Dipole Center - TSL	10 mm	with Spacer																																																													
Zoom Scan Resolution	dx, dy, dz < 5 mm																																																														
Frequency	2600 MHz ± 1 MHz																																																														
	Temperature	Permittivity	Conductivity																																																												
Nominal Head TSL parameters	22.0 °C	39.0	1.96 mho/m																																																												
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.7 ± 6 %	1.96 mho/m ± 8 %																																																												
Head TSL temperature change during test	<1.0 °C	—	—																																																												
SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition																																																														
SAR measured	250 mW input power	13.7 W/kg																																																													
SAR for nominal Head TSL parameters	normalized to 1W	54.8 W/kg ± 18.8 % (k=2)																																																													
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition																																																														
SAR measured	250 mW input power	6.12 W/kg																																																													
SAR for nominal Head TSL parameters	normalized to 1W	24.5 W/kg ± 18.7 % (k=2)																																																													
Impedance, transformed to feed point	49.9Ω-6.49Ω																																																														
Return Loss	-23.8dB																																																														
Electrical Delay (one direction)	1.053 ns																																																														
Manufactured by	SPEAG																																																														
<p>Certificate No: Z22-66108 Page 3 of 6</p>		<p>Certificate No: Z22-66108 Page 4 of 6</p>																																																													


Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.Doccheck@sgs.com](mailto:CN.Doccheck@sgs.com)



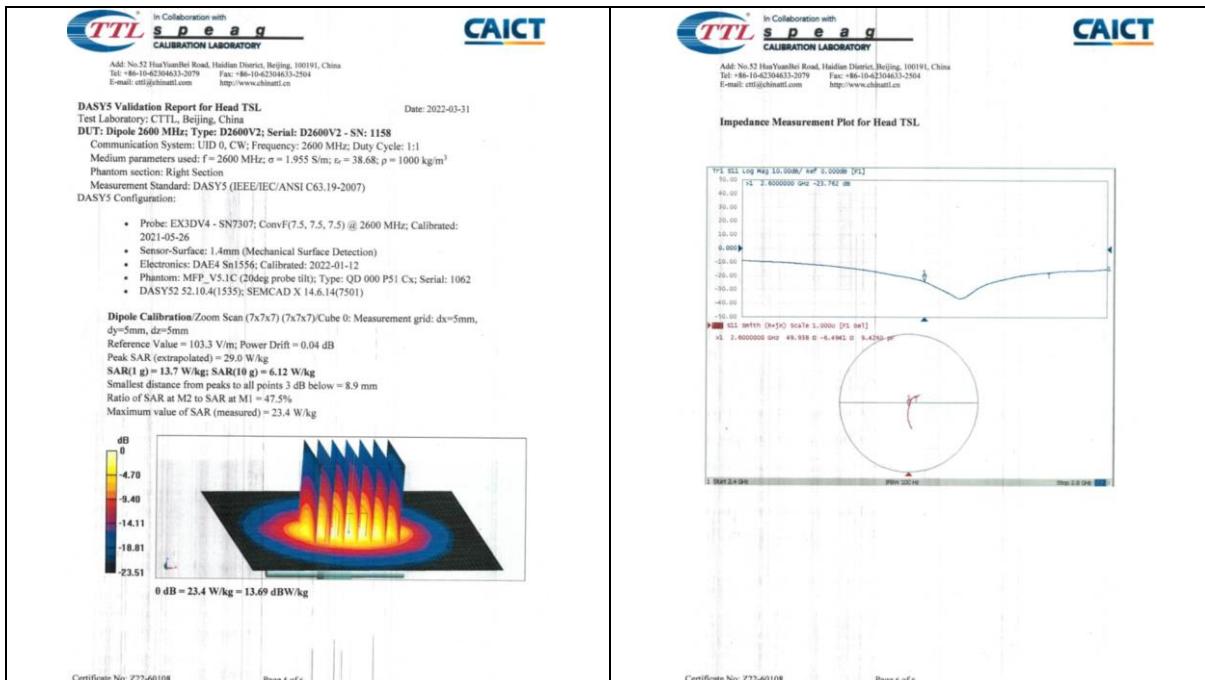

## 1.12 D5GHzV2 - SN 1095

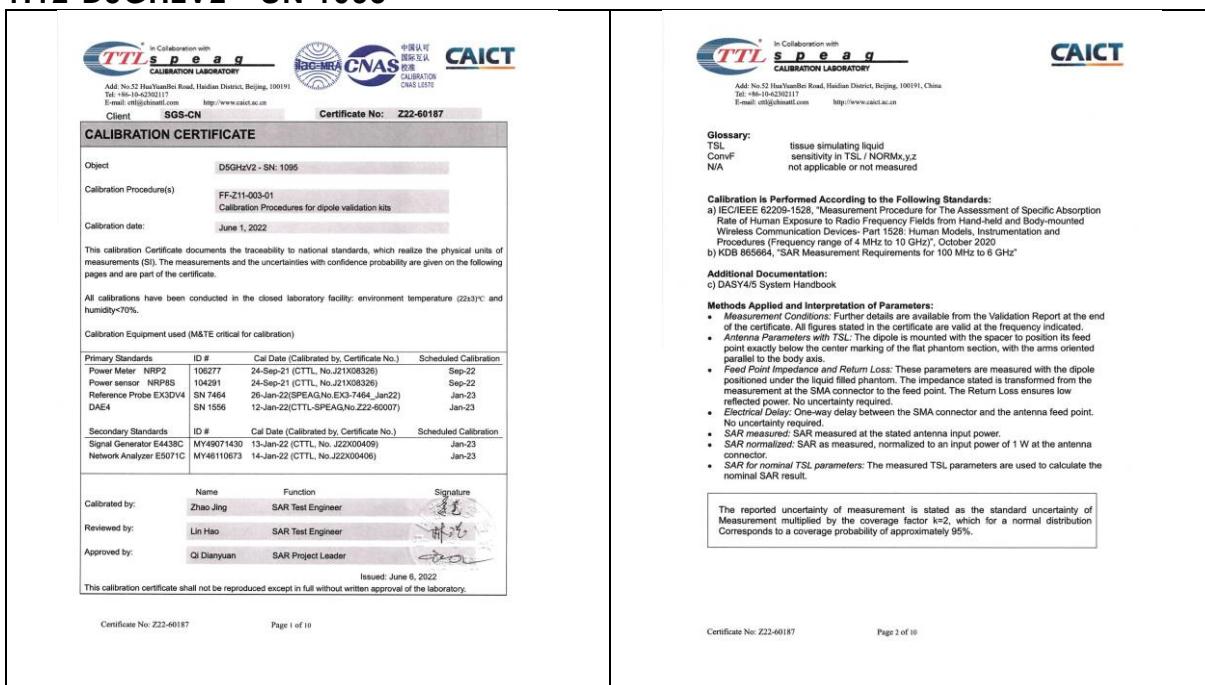

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Please note that the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.Doccheck@sgs.com](mailto:CN.Doccheck@sgs.com)

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300  
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 [www.sgsgroup.com.cn](http://www.sgsgroup.com.cn)  
t(86-512)57355888 f(86-512)57370818 [sgs.china@sgs.com](mailto:sgs.china@sgs.com)

<div style="text-align: center;">  <p>In Collaboration with <b>CAICT</b></p> <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: cict@caict.ac.cn <a href="http://www.caict.ac.cn">http://www.caict.ac.cn</a></p> <p><b>Measurement Conditions</b> DASY system configuration, as far as not given on page 1.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>DASY Version</td><td>DASY32</td><td>52.10.4</td></tr> <tr><td>Extrapolation</td><td>Advanced Extrapolation</td><td></td></tr> <tr><td>Phantom</td><td>Triple Flat Phantom 5.1C</td><td></td></tr> <tr><td>Distance Dipole Center - TSL</td><td>10 mm</td><td>with Spacer</td></tr> <tr><td>Zoom Scan Resolution</td><td>dx, dy = 4 mm, dz = 1.4 mm</td><td>Graded Ratio = 1.4 (Z direction)</td></tr> <tr><td>Frequency</td><td>2000 MHz ± 1 MHz 5300 MHz ± 1 MHz 5500 MHz ± 1 MHz 5600 MHz ± 1 MHz 5800 MHz ± 1 MHz</td><td></td></tr> </table> <p><b>Head TSL parameters at 5200MHz</b> The following parameters and calculations were applied.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td></td><td>Temperature</td><td>Permittivity</td><td>Conductivity</td></tr> <tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>36.0</td><td>4.66 mho/m</td></tr> <tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>35.4 ± 6 %</td><td>4.62 mho/m ± 6 %</td></tr> <tr><td>Head TSL temperature change during test</td><td>&lt;1.0 °C</td><td>—</td><td>—</td></tr> </table> <p><b>SAR result with Head TSL at 5200MHz</b> SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL Condition</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>SAR measured</td><td>250 mW input power</td><td>7.79 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>77.6 W/kg ± 24.4 % (k=2)</td></tr> </table> <p><b>SAR result with Head TSL at 5200MHz</b> SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL Condition</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>SAR measured</td><td>250 mW input power</td><td>2.22 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>22.1 W/kg ± 24.2 % (k=2)</td></tr> </table> </div>	DASY Version	DASY32	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy = 4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)	Frequency	2000 MHz ± 1 MHz 5300 MHz ± 1 MHz 5500 MHz ± 1 MHz 5600 MHz ± 1 MHz 5800 MHz ± 1 MHz			Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	36.0	4.66 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	35.4 ± 6 %	4.62 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR measured	250 mW input power	7.79 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	77.6 W/kg ± 24.4 % (k=2)	SAR measured	250 mW input power	2.22 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	22.1 W/kg ± 24.2 % (k=2)	<div style="text-align: center;">  <p>In Collaboration with <b>CAICT</b></p> <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: cict@caict.ac.cn <a href="http://www.caict.ac.cn">http://www.caict.ac.cn</a></p> <p><b>Head TSL parameters at 5300MHz</b> The following parameters and calculations were applied.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td></td><td>Temperature</td><td>Permittivity</td><td>Conductivity</td></tr> <tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>35.6</td><td>4.76 mho/m</td></tr> <tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>35.2 ± 6 %</td><td>4.73 mho/m ± 6 %</td></tr> <tr><td>Head TSL temperature change during test</td><td>&lt;1.0 °C</td><td>—</td><td>—</td></tr> </table> <p><b>SAR result with Head TSL at 5300MHz</b> SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL Condition</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>SAR measured</td><td>100 mW input power</td><td>7.94 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>78.1 W/kg ± 24.4 % (k=2)</td></tr> </table> <p><b>SAR result with Head TSL at 5300MHz</b> SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL Condition</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>SAR measured</td><td>100 mW input power</td><td>2.27 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>22.6 W/kg ± 24.2 % (k=2)</td></tr> </table> </div>		Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	35.6	4.76 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	35.2 ± 6 %	4.73 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR measured	100 mW input power	7.94 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	78.1 W/kg ± 24.4 % (k=2)	SAR measured	100 mW input power	2.27 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	22.6 W/kg ± 24.2 % (k=2)		
DASY Version	DASY32	52.10.4																																																																											
Extrapolation	Advanced Extrapolation																																																																												
Phantom	Triple Flat Phantom 5.1C																																																																												
Distance Dipole Center - TSL	10 mm	with Spacer																																																																											
Zoom Scan Resolution	dx, dy = 4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)																																																																											
Frequency	2000 MHz ± 1 MHz 5300 MHz ± 1 MHz 5500 MHz ± 1 MHz 5600 MHz ± 1 MHz 5800 MHz ± 1 MHz																																																																												
	Temperature	Permittivity	Conductivity																																																																										
Nominal Head TSL parameters	22.0 °C	36.0	4.66 mho/m																																																																										
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.4 ± 6 %	4.62 mho/m ± 6 %																																																																										
Head TSL temperature change during test	<1.0 °C	—	—																																																																										
SAR measured	250 mW input power	7.79 W/kg																																																																											
SAR for nominal Head TSL parameters	normalized to 1W	77.6 W/kg ± 24.4 % (k=2)																																																																											
SAR measured	250 mW input power	2.22 W/kg																																																																											
SAR for nominal Head TSL parameters	normalized to 1W	22.1 W/kg ± 24.2 % (k=2)																																																																											
	Temperature	Permittivity	Conductivity																																																																										
Nominal Head TSL parameters	22.0 °C	35.6	4.76 mho/m																																																																										
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.2 ± 6 %	4.73 mho/m ± 6 %																																																																										
Head TSL temperature change during test	<1.0 °C	—	—																																																																										
SAR measured	100 mW input power	7.94 W/kg																																																																											
SAR for nominal Head TSL parameters	normalized to 1W	78.1 W/kg ± 24.4 % (k=2)																																																																											
SAR measured	100 mW input power	2.27 W/kg																																																																											
SAR for nominal Head TSL parameters	normalized to 1W	22.6 W/kg ± 24.2 % (k=2)																																																																											
<p>Certificate No: Z22-60187 <span style="float: right;">Page 3 of 10</span></p>																																																																													
<p>Certificate No: Z22-60187 <span style="float: right;">Page 4 of 10</span></p>																																																																													
<div style="text-align: center;">  <p>In Collaboration with <b>CAICT</b></p> <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: cict@caict.ac.cn <a href="http://www.caict.ac.cn">http://www.caict.ac.cn</a></p> <p><b>Head TSL parameters at 5600MHz</b> The following parameters and calculations were applied.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td></td><td>Temperature</td><td>Permittivity</td><td>Conductivity</td></tr> <tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>35.5</td><td>5.07 mho/m</td></tr> <tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>34.7 ± 6 %</td><td>5.05 mho/m ± 6 %</td></tr> <tr><td>Head TSL temperature change during test</td><td>&lt;1.0 °C</td><td>—</td><td>—</td></tr> </table> <p><b>SAR result with Head TSL at 5600MHz</b> SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL Condition</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>SAR measured</td><td>100 mW input power</td><td>8.12 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>80.8 W/kg ± 24.4 % (k=2)</td></tr> </table> <p><b>SAR result with Head TSL at 5600MHz</b> SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL Condition</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>SAR measured</td><td>100 mW input power</td><td>2.30 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>22.8 W/kg ± 24.2 % (k=2)</td></tr> </table> <p><b>Head TSL parameters at 5800MHz</b> The following parameters and calculations were applied.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td></td><td>Temperature</td><td>Permittivity</td><td>Conductivity</td></tr> <tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>35.3</td><td>5.27 mho/m</td></tr> <tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>34.4 ± 6 %</td><td>5.25 mho/m ± 6 %</td></tr> <tr><td>Head TSL temperature change during test</td><td>&lt;1.0 °C</td><td>—</td><td>—</td></tr> </table> <p><b>SAR result with Head TSL at 5800MHz</b> SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL Condition</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>SAR measured</td><td>100 mW input power</td><td>7.71 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>76.7 W/kg ± 24.4 % (k=2)</td></tr> </table> <p><b>SAR result with Head TSL at 5800MHz</b> SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL Condition</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>SAR measured</td><td>100 mW input power</td><td>2.16 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>21.5 W/kg ± 24.2 % (k=2)</td></tr> </table> </div>		Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	34.7 ± 6 %	5.05 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR measured	100 mW input power	8.12 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	80.8 W/kg ± 24.4 % (k=2)	SAR measured	100 mW input power	2.30 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	22.8 W/kg ± 24.2 % (k=2)		Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	35.3	5.27 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	34.4 ± 6 %	5.25 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR measured	100 mW input power	7.71 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	76.7 W/kg ± 24.4 % (k=2)	SAR measured	100 mW input power	2.16 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	21.5 W/kg ± 24.2 % (k=2)	<div style="text-align: center;">  <p>In Collaboration with <b>CAICT</b></p> <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: cict@caict.ac.cn <a href="http://www.caict.ac.cn">http://www.caict.ac.cn</a></p> <p><b>Appendix (Additional assessments outside the scope of CNAS L0570)</b></p> <p><b>Antenna Parameters with Head TSL at 5200MHz</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Impedance, transformed to feed point</td><td>46.10- 5.03jΩ</td></tr> <tr><td>Return Loss</td><td>-23.8dB</td></tr> </table> <p><b>Antenna Parameters with Head TSL at 5300MHz</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Impedance, transformed to feed point</td><td>47.80- 2.42jΩ</td></tr> <tr><td>Return Loss</td><td>-29.5dB</td></tr> </table> <p><b>Antenna Parameters with Head TSL at 5500MHz</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Impedance, transformed to feed point</td><td>50.30- 4.26jΩ</td></tr> <tr><td>Return Loss</td><td>-27.4dB</td></tr> </table> <p><b>Antenna Parameters with Head TSL at 5600MHz</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Impedance, transformed to feed point</td><td>54.50- 4.80jΩ</td></tr> <tr><td>Return Loss</td><td>-24.0dB</td></tr> </table> <p><b>Antenna Parameters with Head TSL at 5800MHz</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Impedance, transformed to feed point</td><td>51.50- 5.61jΩ</td></tr> <tr><td>Return Loss</td><td>-24.9dB</td></tr> </table> </div>	Impedance, transformed to feed point	46.10- 5.03jΩ	Return Loss	-23.8dB	Impedance, transformed to feed point	47.80- 2.42jΩ	Return Loss	-29.5dB	Impedance, transformed to feed point	50.30- 4.26jΩ	Return Loss	-27.4dB	Impedance, transformed to feed point	54.50- 4.80jΩ	Return Loss	-24.0dB	Impedance, transformed to feed point	51.50- 5.61jΩ	Return Loss	-24.9dB
	Temperature	Permittivity	Conductivity																																																																										
Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m																																																																										
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.7 ± 6 %	5.05 mho/m ± 6 %																																																																										
Head TSL temperature change during test	<1.0 °C	—	—																																																																										
SAR measured	100 mW input power	8.12 W/kg																																																																											
SAR for nominal Head TSL parameters	normalized to 1W	80.8 W/kg ± 24.4 % (k=2)																																																																											
SAR measured	100 mW input power	2.30 W/kg																																																																											
SAR for nominal Head TSL parameters	normalized to 1W	22.8 W/kg ± 24.2 % (k=2)																																																																											
	Temperature	Permittivity	Conductivity																																																																										
Nominal Head TSL parameters	22.0 °C	35.3	5.27 mho/m																																																																										
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.4 ± 6 %	5.25 mho/m ± 6 %																																																																										
Head TSL temperature change during test	<1.0 °C	—	—																																																																										
SAR measured	100 mW input power	7.71 W/kg																																																																											
SAR for nominal Head TSL parameters	normalized to 1W	76.7 W/kg ± 24.4 % (k=2)																																																																											
SAR measured	100 mW input power	2.16 W/kg																																																																											
SAR for nominal Head TSL parameters	normalized to 1W	21.5 W/kg ± 24.2 % (k=2)																																																																											
Impedance, transformed to feed point	46.10- 5.03jΩ																																																																												
Return Loss	-23.8dB																																																																												
Impedance, transformed to feed point	47.80- 2.42jΩ																																																																												
Return Loss	-29.5dB																																																																												
Impedance, transformed to feed point	50.30- 4.26jΩ																																																																												
Return Loss	-27.4dB																																																																												
Impedance, transformed to feed point	54.50- 4.80jΩ																																																																												
Return Loss	-24.0dB																																																																												
Impedance, transformed to feed point	51.50- 5.61jΩ																																																																												
Return Loss	-24.9dB																																																																												
<p>Certificate No: Z22-60187 <span style="float: right;">Page 5 of 10</span></p>																																																																													
<p>Certificate No: Z22-60187 <span style="float: right;">Page 6 of 10</span></p>																																																																													

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To need the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.Deecheck@sgs.com](mailto:CN.Deecheck@sgs.com)

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300  
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)5735888 f(86-512)57370818 [www.sgsgroup.com.cn](http://www.sgsgroup.com.cn)  
t(86-512)5735888 f(86-512)57370818 [sgs.china@sgs.com](mailto:sgs.china@sgs.com)



<div style="text-align: center;">  <p>In Collaboration with <b>TTL speag</b> CALIBRATION LABORATORY</p> <p>Add: No.52 HuYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42302117 E-mail: ctttgj@sohu.com http://www.caict.ac.cn</p> <p><b>General Antenna Parameters and Design</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 50%;">Electrical Delay (one direction)</td> <td style="width: 50%;">1.101 ns</td> </tr> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semi rigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded with a specific load. The dipole arms are not soldered to the center conductor. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p><b>Additional EUT Data</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 50%;">Manufactured by</td> <td style="width: 50%;">SPEAG</td> </tr> </table> </div>	Electrical Delay (one direction)	1.101 ns	Manufactured by	SPEAG	<div style="text-align: center;">  <p><b>CAICT</b></p> <p>In Collaboration with <b>TTL speag</b> CALIBRATION LABORATORY</p> <p>Add: No.52 HuYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42302117 E-mail: ctttgj@sohu.com http://www.caict.ac.cn</p> <p><b>DASYS Report for Head TSL</b></p> <p>DUT: Dipole 5GHz; Type: DSGHv2; Serial: 1095 Communication System: CW; Frequency: 5200 MHz; Frequency: 5300 MHz; Frequency: 5500 MHz; Frequency: 5600 MHz; Frequency: 5800 MHz; Duty Cycle: 1:1 Medium parameters used: f = 5200 MHz; <math>\sigma</math> = 4.62 S/m; <math>\epsilon</math> = 35.39; <math>\rho</math> = 1000 kg/m<sup>3</sup> Medium parameters used: f = 5300 MHz; <math>\sigma</math> = 4.73 S/m; <math>\epsilon</math> = 35.19; <math>\rho</math> = 1000 kg/m<sup>3</sup> Medium parameters used: f = 5500 MHz; <math>\sigma</math> = 4.82 S/m; <math>\epsilon</math> = 34.49; <math>\rho</math> = 1000 kg/m<sup>3</sup> Medium parameters used: f = 5600 MHz; <math>\sigma</math> = 5.01 S/m; <math>\epsilon</math> = 34.89; <math>\rho</math> = 1000 kg/m<sup>3</sup> Medium parameters used: f = 5800 MHz; <math>\sigma</math> = 5.247 S/m; <math>\epsilon</math> = 34.42; <math>\rho</math> = 1000 kg/m<sup>3</sup> Phantom section: Right Section Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007) DASYS Configuration:<ul style="list-style-type: none"> <li>• Probe: EX3DV4 - SN7464; ConvF(5.6, 5.6, 5.6) @ 5200 MHz; ConvF(5.32, 5.32, 5.32) @ 5300 MHz; ConvF(5.11, 5.11, 5.11) @ 5500 MHz; ConvF(4.91, 4.91, 4.91) @ 5600 MHz; ConvF(5, 5, 5) @ 5800 MHz;</li> <li>• Calibrated: 2022-01-26</li> <li>• Sensor-Surface: 1.4mm (Mechanical Surface Detection)</li> <li>• Electronics: DAE4 Sn11556; Calibrated: 2022-01-12</li> <li>• Probe: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062</li> <li>• DASYS52.10.14(1535); SEMCAD X 14.6.14(7501)</li> </ul> <p>Dipole Calibration (Pin=100mW, d=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 61.92 V/m; Power Drift = -0.06 dB Peak SAR (extrapolated) = 29.1 W/kg SAR(1 g) = 7.79 W/kg; SAR(10 g) = 2.33 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 66.8% Maximum value of SAR (measured) = 18.3 W/kg</p> <p>Dipole Calibration (Pin=100mW, d=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 61.08 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 31.5 W/kg SAR(1 g) = 8.07 W/kg; SAR(10 g) = 2.47 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 65.5% Maximum value of SAR (measured) = 19.0 W/kg</p> </p></div>
Electrical Delay (one direction)	1.101 ns				
Manufactured by	SPEAG				
<p>Certificate No: Z22-60187 Page 7 of 10</p> <p>Certificate No: Z22-60187 Page 8 of 10</p>					
<p>Certificate No: Z22-60187 Page 9 of 10</p> <p>Certificate No: Z22-60187 Page 10 of 10</p>					



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention is drawn to the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.Doccheck@sgs.com](mailto:CN.Doccheck@sgs.com)

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300  
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 [www.sgsgroup.com.cn](http://www.sgsgroup.com.cn)  
t(86-512)57355888 f(86-512)57370818 [sgs.china@sgs.com](mailto:sgs.china@sgs.com)

## 2 DAE4 - SN 910

<div style="border: 1px solid black; padding: 10px;"> <p style="text-align: center;">  <b>TTL</b> In Collaboration with <b>CAICT</b>   <b>CNAS</b> 中国认可 国际互认  <b>CAICT</b> CALIBRATION CNAS B379         </p> <p>Client : <b>Auden</b> Certificate No: Z22-60275</p> <p><b>CALIBRATION CERTIFICATE</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 10%;">Object</td> <td style="width: 90%;">DAE4 - SN: 910</td> </tr> <tr> <td>Calibration Procedure(s)</td> <td>FF-Z11-002-01 Calibration Procedure for the Data Acquisition Electronics (DAE4)</td> </tr> <tr> <td>Calibration date:</td> <td>July 14, 2022</td> </tr> <tr> <td colspan="2">           This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.            All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C; and humidity&lt;70%.         </td> </tr> <tr> <td colspan="2">           Calibration Equipment used (M&amp;TE critical for calibration)           <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 10%;">Primary Standards</td> <td style="width: 10%;">ID #</td> <td style="width: 10%;">Cal Date(Calibrated by, Certificate No.)</td> <td style="width: 10%;">Scheduled Calibration</td> </tr> <tr> <td>Process Calibrator 753</td> <td>1971018</td> <td>14-Jun-22 (CTTL, No.J22X04180)</td> <td>Jun-23</td> </tr> </table> </td> </tr> <tr> <td>Calibrated by:</td> <td>Name: Yu Zongying, Function: SAR Test Engineer, Signature: </td> </tr> <tr> <td>Reviewed by:</td> <td>Name: Lin Hao, Function: SAR Test Engineer, Signature: </td> </tr> <tr> <td>Approved by:</td> <td>Name: Qi Danyuan, Function: SAR Project Leader, Signature: </td> </tr> <tr> <td colspan="2" style="text-align: center;">Issued: July 20, 2022</td> </tr> <tr> <td colspan="2">           This calibration certificate shall not be reproduced except in full without written approval of the laboratory.         </td> </tr> </table> </div> <p style="text-align: center;">Certificate No: Z22-60275 Page 1 of 3</p>	Object	DAE4 - SN: 910	Calibration Procedure(s)	FF-Z11-002-01 Calibration Procedure for the Data Acquisition Electronics (DAE4)	Calibration date:	July 14, 2022	This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C; and humidity<70%.		Calibration Equipment used (M&TE critical for calibration) <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 10%;">Primary Standards</td> <td style="width: 10%;">ID #</td> <td style="width: 10%;">Cal Date(Calibrated by, Certificate No.)</td> <td style="width: 10%;">Scheduled Calibration</td> </tr> <tr> <td>Process Calibrator 753</td> <td>1971018</td> <td>14-Jun-22 (CTTL, No.J22X04180)</td> <td>Jun-23</td> </tr> </table>		Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration	Process Calibrator 753	1971018	14-Jun-22 (CTTL, No.J22X04180)	Jun-23	Calibrated by:	Name: Yu Zongying, Function: SAR Test Engineer, Signature: 	Reviewed by:	Name: Lin Hao, Function: SAR Test Engineer, Signature: 	Approved by:	Name: Qi Danyuan, Function: SAR Project Leader, Signature: 	Issued: July 20, 2022		This calibration certificate shall not be reproduced except in full without written approval of the laboratory.		<div style="border: 1px solid black; padding: 10px;"> <p style="text-align: center;">  <b>TTL</b> In Collaboration with <b>CAICT</b>   <b>CNAS</b> 中国认可 国际互认  <b>CAICT</b> CALIBRATION LABORATORY         </p> <p>Add: No.52 HuaYanBei Road, Haidian District, Beijing, 100191, China            Tel: +86-10-62360633-2117            E-mail: emf@caict.ac.cn <a href="http://www.caict.ac.cn">http://www.caict.ac.cn</a></p> <p><b>Glossary:</b>  <b>DAE</b> data acquisition electronics  <b>Connector angle</b> information used in DASY system to align probe sensor X to the robot coordinate system.</p> <p><b>Methods Applied and Interpretation of Parameters:</b></p> <ul style="list-style-type: none"> <li>• <b>DC Voltage Measurement:</b> Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.</li> <li>• <b>Connector angle:</b> The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.</li> <li>• The report provide only calibration results for DAE, it does not contain other performance test results.</li> </ul> </div> <p style="text-align: center;">Certificate No: Z22-60275 Page 2 of 3</p>
Object	DAE4 - SN: 910																												
Calibration Procedure(s)	FF-Z11-002-01 Calibration Procedure for the Data Acquisition Electronics (DAE4)																												
Calibration date:	July 14, 2022																												
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C; and humidity<70%.																													
Calibration Equipment used (M&TE critical for calibration) <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 10%;">Primary Standards</td> <td style="width: 10%;">ID #</td> <td style="width: 10%;">Cal Date(Calibrated by, Certificate No.)</td> <td style="width: 10%;">Scheduled Calibration</td> </tr> <tr> <td>Process Calibrator 753</td> <td>1971018</td> <td>14-Jun-22 (CTTL, No.J22X04180)</td> <td>Jun-23</td> </tr> </table>		Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration	Process Calibrator 753	1971018	14-Jun-22 (CTTL, No.J22X04180)	Jun-23																				
Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration																										
Process Calibrator 753	1971018	14-Jun-22 (CTTL, No.J22X04180)	Jun-23																										
Calibrated by:	Name: Yu Zongying, Function: SAR Test Engineer, Signature: 																												
Reviewed by:	Name: Lin Hao, Function: SAR Test Engineer, Signature: 																												
Approved by:	Name: Qi Danyuan, Function: SAR Project Leader, Signature: 																												
Issued: July 20, 2022																													
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.																													
<div style="border: 1px solid black; padding: 10px;"> <p style="text-align: center;">  <b>TTL</b> In Collaboration with <b>CAICT</b>   <b>CNAS</b> 中国认可 国际互认  <b>CAICT</b> CALIBRATION LABORATORY         </p> <p>Add: No.52 HuaYanBei Road, Haidian District, Beijing, 100191, China            Tel: +86-10-62360633-2117            E-mail: emf@caict.ac.cn <a href="http://www.caict.ac.cn">http://www.caict.ac.cn</a></p> <p><b>DC Voltage Measurement</b>            A/D - Converter Resolution nominal            High Range: 1LSB = 5.12V, full range = -100...+300 mV            Low Range: 1LSB = 61.44mV, full range = -10...+30mV            DASY measurement parameters: Auto Zero Time: 3 sec, Measuring time: 3 sec</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <th>Calibration Factors</th> <th>X</th> <th>Y</th> <th>Z</th> </tr> <tr> <td>High Range</td> <td>403.347 ± 0.15% (k=2)</td> <td>402.769 ± 0.15% (k=2)</td> <td>403.242 ± 0.15% (k=2)</td> </tr> <tr> <td>Low Range</td> <td>3.98151 ± 0.7% (k=2)</td> <td>3.94044 ± 0.7% (k=2)</td> <td>3.94827 ± 0.7% (k=2)</td> </tr> </table> <p><b>Connector Angle</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 10%;">Connector Angle to be used in DASY system</td> <td style="width: 90%;">269° ± 1°</td> </tr> </table> </div>		Calibration Factors	X	Y	Z	High Range	403.347 ± 0.15% (k=2)	402.769 ± 0.15% (k=2)	403.242 ± 0.15% (k=2)	Low Range	3.98151 ± 0.7% (k=2)	3.94044 ± 0.7% (k=2)	3.94827 ± 0.7% (k=2)	Connector Angle to be used in DASY system	269° ± 1°														
Calibration Factors	X	Y	Z																										
High Range	403.347 ± 0.15% (k=2)	402.769 ± 0.15% (k=2)	403.242 ± 0.15% (k=2)																										
Low Range	3.98151 ± 0.7% (k=2)	3.94044 ± 0.7% (k=2)	3.94827 ± 0.7% (k=2)																										
Connector Angle to be used in DASY system	269° ± 1°																												
<div style="border: 1px solid black; padding: 10px;"> <p style="text-align: center;">Certificate No: Z22-60275 Page 3 of 3</p> </div>																													

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Please note that the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.Doccheck@sgs.com](mailto:CN.Doccheck@sgs.com)




3 EX3DV4 - SN 7767

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overhead, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from, excepting all their rights and obligations under the transaction documents. This document cannot be reproduced in whole or in part, in any form, without the prior written permission of the Company. Any unauthorized copying, transmission, distribution, or appearance of this document is unlawful and offenders may be prosecuted to the full extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.DocCheck@sgs.com](mailto:CN.DocCheck@sgs.com)

中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn  
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

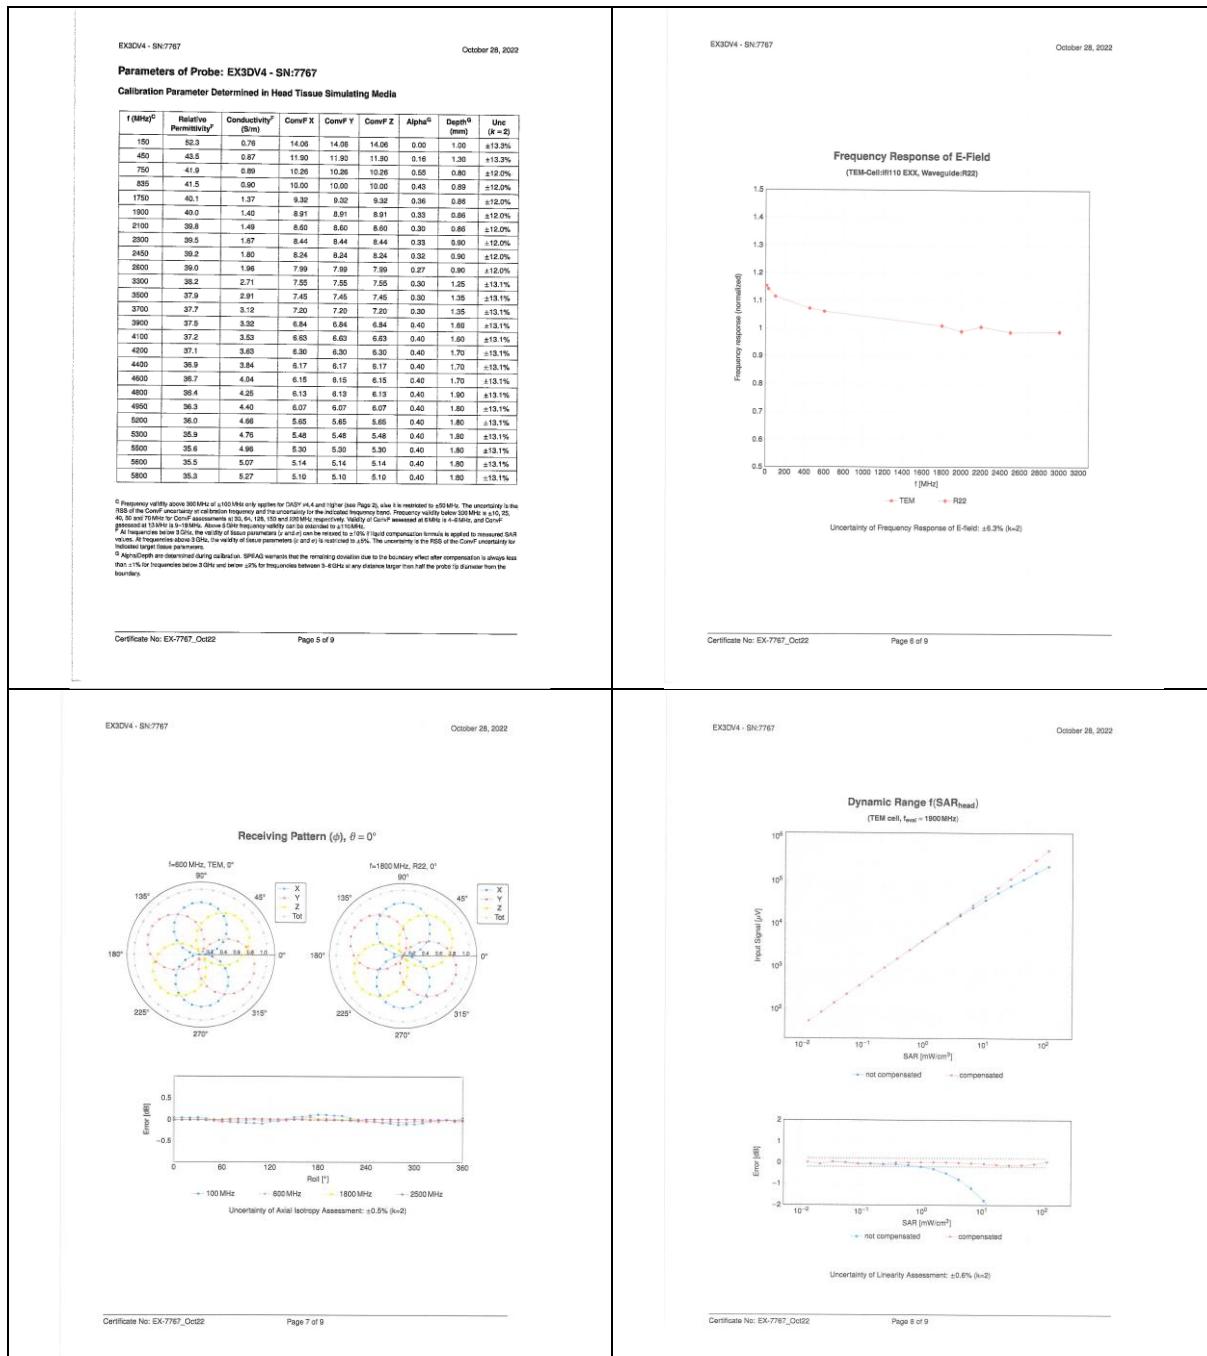


Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To need the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com



No.10, Weive Road, Innovation Park, Kunshan, Jiangsu, China 215300  
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn  
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

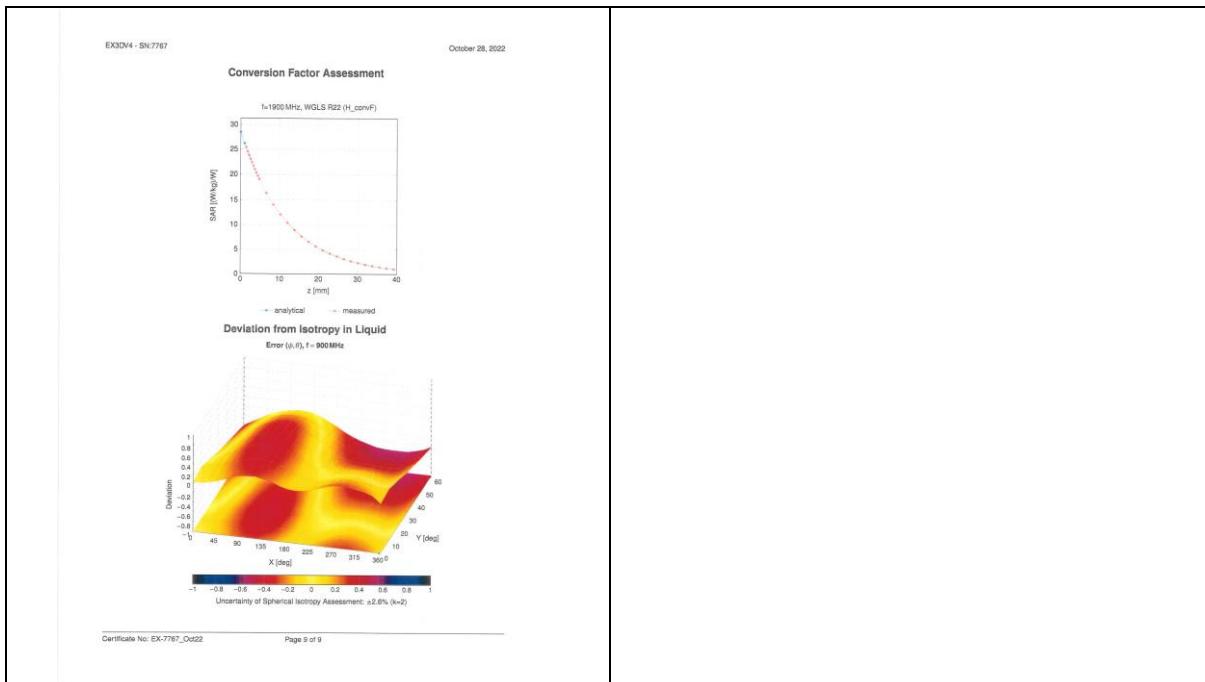

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.Doccheck@sgs.com](mailto:CN.Doccheck@sgs.com)



#### 4 Impedance and return loss

Dipole CLA150 SN 4025				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2021/4/26	-31.4	/	47.8	/
2022/4/26	-32.5	-3.5%	47.1	0.7
2023/4/26	-32.3	-2.87%	46.5	1.3
Dipole D450V3 SN 1103				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2021/4/21	-23	/	57.1	/
2022/4/26	-23.4	-1.74%	56.6	0.5
2023/4/26	-23.9	-3.91%	56.2	0.9
Dipole D750V3 SN 1188				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2022/3/29	-28.7	/	53.6	/
2023/3/29	-28.3	1.39%	53.2	0.4
Dipole D835V2 SN 4d114				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2022/3/31	-25.3	/	48.7	/
2023/3/31	-24.6	2.77%	49.1	0.4
Dipole D900V2 SN 1d079				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2022/6/7	-23.3	/	48.1	/
2023/6/7	-23.6	-1.29%	48.3	0.2
Dipole D1800V2 SN 2d170				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2022/3/31	-29.4	/	47.9	/
2023/3/31	-28.9	1.70%	47.2	0.7
Dipole D1900V2 SN 5d136				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2022/6/7	-22.4	/	51.2	/
2023/6/7	-22.9	-2.23%	51.6	-0.4
Dipole D2000V2 SN 1041				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2022/6/6	-34.9	/	48.4	/
2023/6/6	-33.5	4.01%	49.1	-0.7
Dipole D2300V2 SN 1096				

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To need the authenticity of testing /Inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.Doccheck@sgs.com](mailto:CN.Doccheck@sgs.com)

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300  
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 [www.sgsgroup.com.cn](http://www.sgsgroup.com.cn)  
t(86-512)57355888 f(86-512)57370818 [sgs.china@sgs.com](mailto:sgs.china@sgs.com)



Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2022/3/31	-26.6	/	49.2	/
2023/3/31	-27.1	-1.88%	49.4	0.2
Dipole D2450V2 SN 817				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2022/4/1	-28.5	/	52.1	/
2023/4/1	-28.0	1.75%	51.6	0.5
Dipole D2600V2 SN 1158				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2022/3/31	-23.8	/	49.9	/
2023/3/31	-23.3	2.10%	50.3	0.4
Dipole D5GHzV2 SN 1095 for 5200				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2022/6/1	-23.6	/	46.1	/
2023/6/1	-23.1	2.12%	45.6	0.5
Dipole D5GHzV2 SN 1095 for 5300				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2022/6/1	-29.5	/	47.8	/
2023/6/1	-28.8	2.37%	46.9	0.9
Dipole D5GHzV2 SN 1095 for 5500				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2022/6/1	-27.4	/	50.3	/
2023/6/1	-27.6	-0.73%	50.8	-0.5
Dipole D5GHzV2 SN 1095 for 5600				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2022/6/1	-24.0	/	54.5	/
2023/6/1	-23.6	1.67%	54.9	-0.4
Dipole D5GHzV2 SN 1095 for 5800				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2022/6/1	-24.9	/	51.5	/
2023/6/1	-24.3	2.41%	51.0	0.5

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To need the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: [CN.Doccheck@sgs.com](mailto:CN.Doccheck@sgs.com)

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300  
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 [www.sgsgroup.com.cn](http://www.sgsgroup.com.cn)  
t(86-512)57355888 f(86-512)57370818 [sgs.china@sgs.com](mailto:sgs.china@sgs.com)

