



# Appendix D

## Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details



## 1. SAR measurement System





## 2. Photographs of Tissue Simulate Liquid


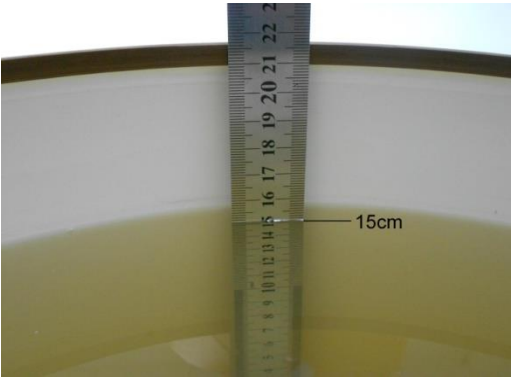
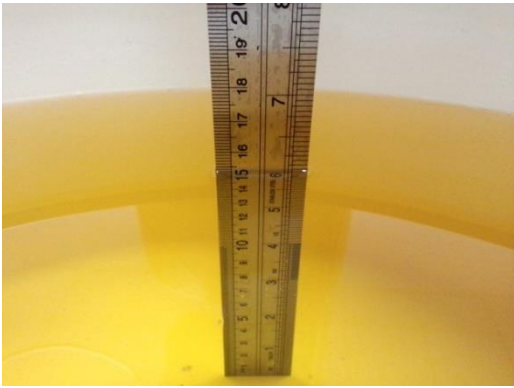



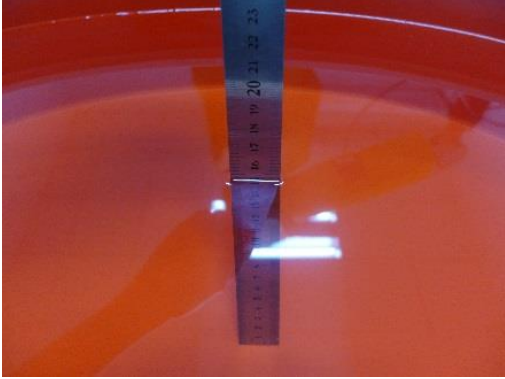

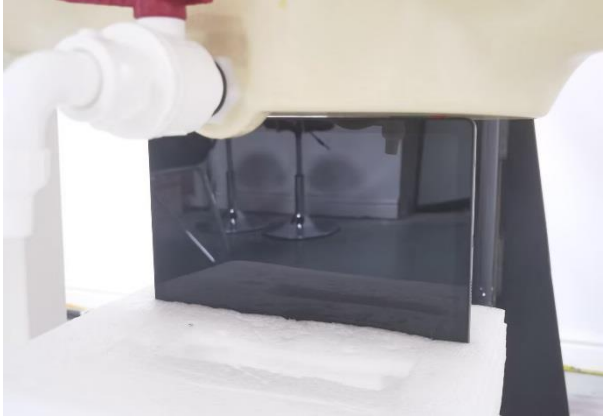


<p><b>Photo 1: Tissue Simulant Liquid for Head 750</b></p>	<p><b>Photo 2: Tissue Simulant Liquid for Head 835</b></p>
	
<p><b>Photo 3: Tissue Simulant Liquid for Head 1750</b></p>	<p><b>Photo 4: Tissue Simulant Liquid for Head 1900</b></p>
	
<p><b>Photo 5: Tissue Simulant Liquid for Head 2450</b></p>	<p><b>Photo 6: Tissue Simulant Liquid for Head 2600</b></p>
	



Photo 7: Tissue Simulant Liquid for Head 5000	NA
	NA



### 3. Photographs of EUT test position

<p>Photo 8: Rear side 0mm</p>	<p>Photo 9: Right side 0mm</p>
	
<p>Photo 10: Top side 0mm</p>	<p>Photo 11: Bottom side 0mm</p>
	



## 4. EUT Constructional Details

