


Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

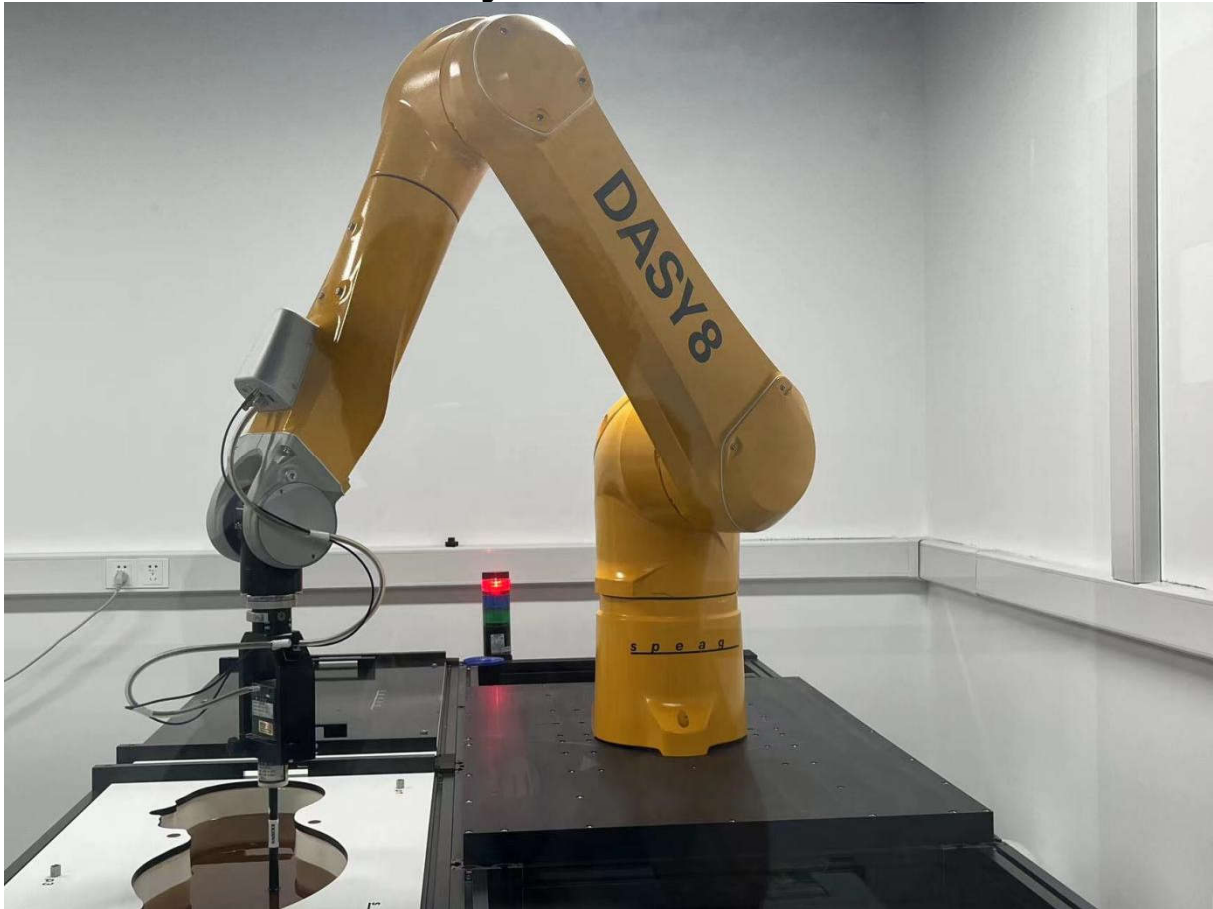

2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for HBBL600-10000MHz	NA
 A photograph showing a cross-section of a curved, translucent container filled with a yellowish, viscous liquid. A metal ruler is placed vertically against the container to provide a scale. The ruler markings show centimeters from 6 to 12. The liquid level is approximately at the 10 cm mark. The container has a blue outer rim.	NA

3. Photographs of EUT test position

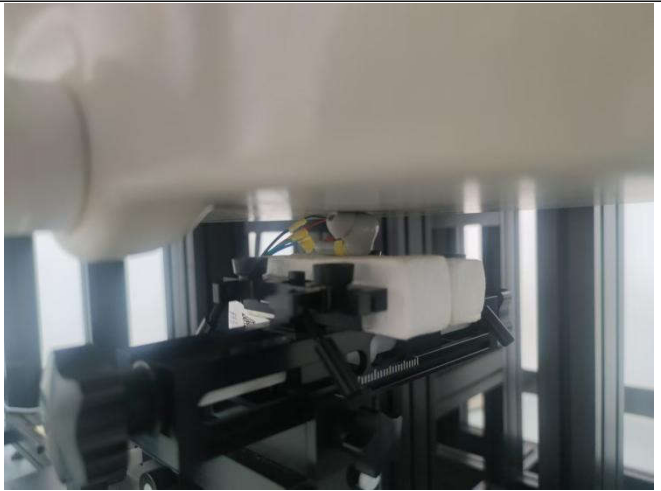
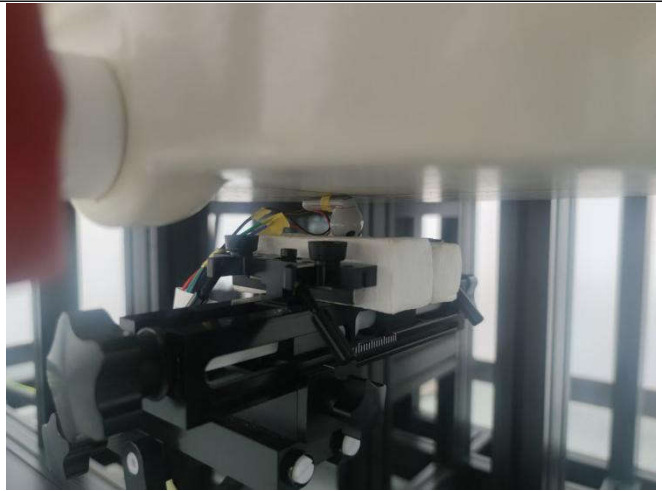
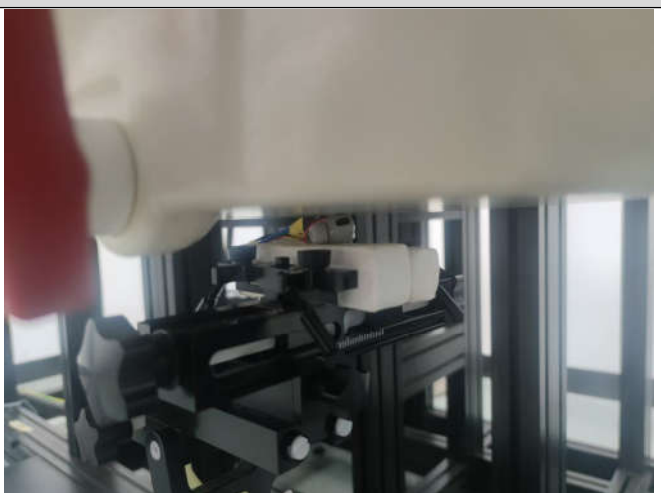
Photo 2: Left ear Front side 0mm	Photo 3: Left ear Back side 0mm
	
Photo 4: Left ear Left side 0mm	Photo 5: Left ear Right side 0mm
	
Photo 6: Left ear Top side 0mm	Photo 7: Left ear Bottom side 0mm
	

Photo 8: Right ear Front side 0mm

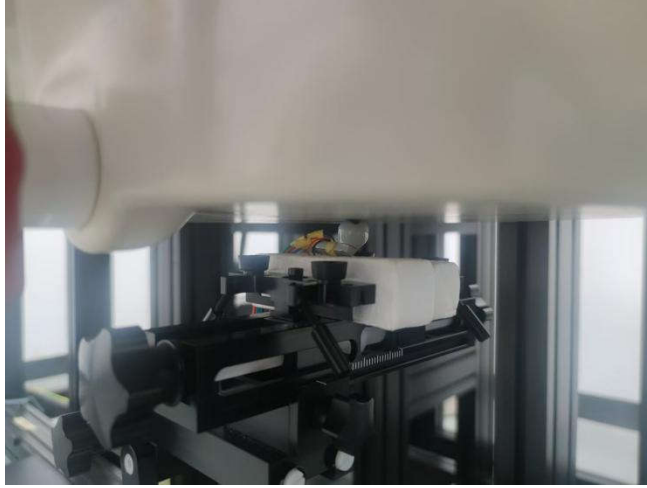


Photo 9: Right ear Back side 0mm

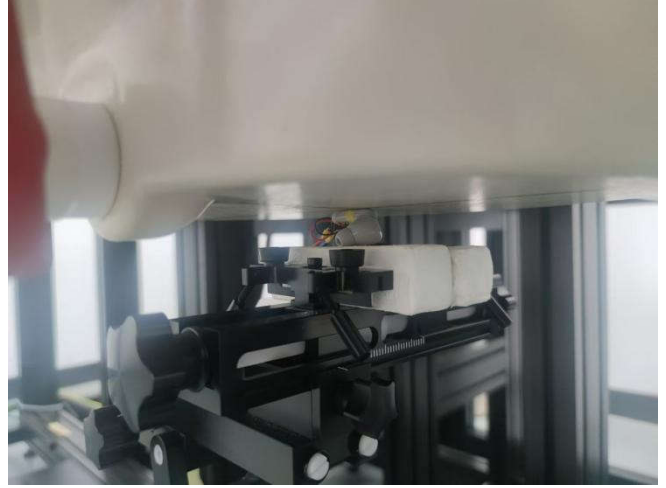


Photo 10: Right ear Left side 0mm

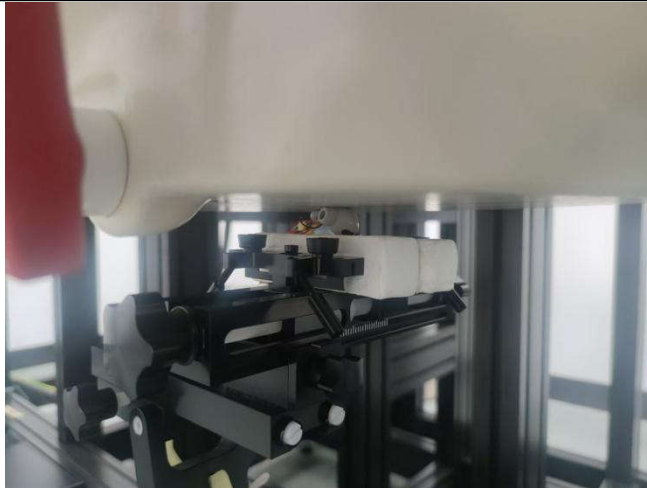


Photo 11: Right ear Right side 0mm

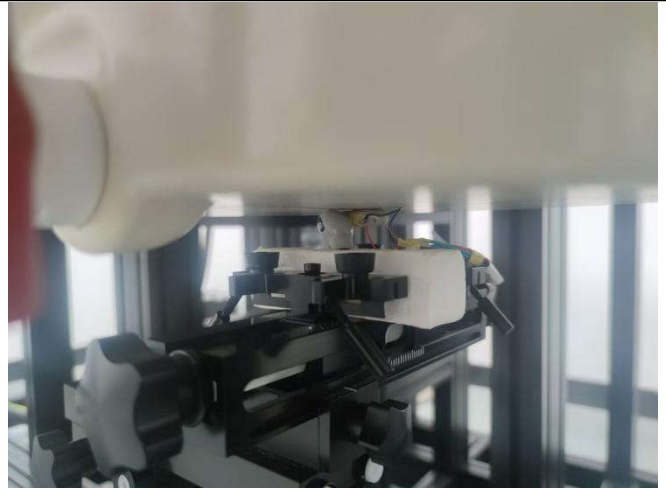


Photo 12: Right ear Top side 0mm



Photo 13: Right ear Bottom side 0mm



4. EUT Constructional Details

Photo 14: Left ear Front View

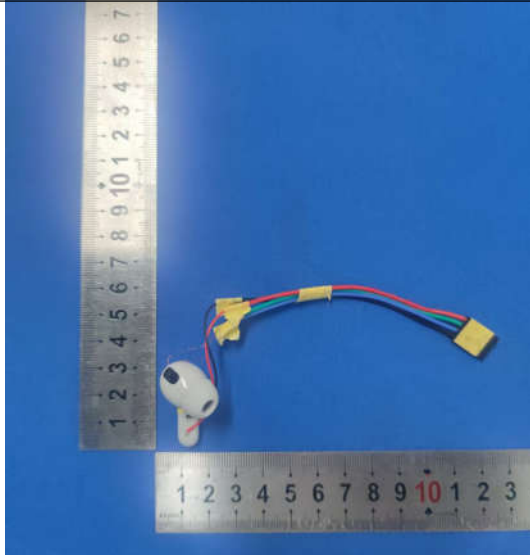


Photo 15: Left ear Back View

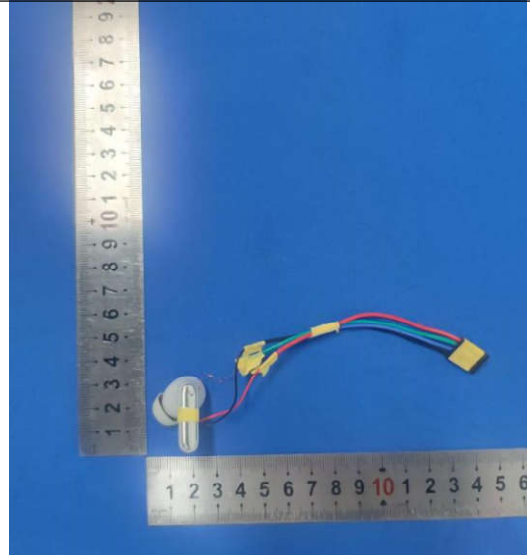


Photo 16: Right ear Front View

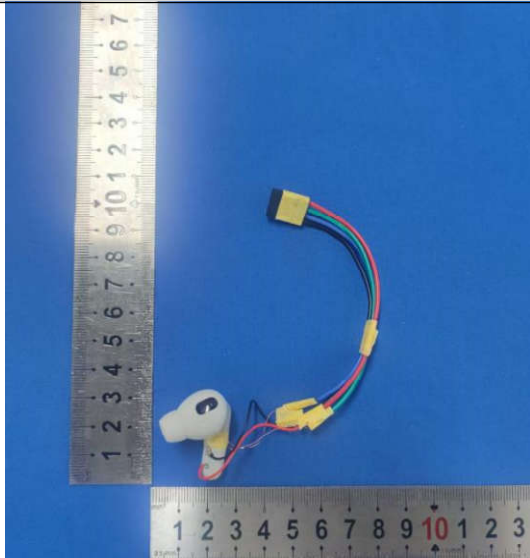


Photo 17: Right ear Back View

