



**Impedance Plot for SN 29/15 DIP 2G450-393  
2450 Head**

Calibrated impedance:  $52.3\Omega + 3.4j\Omega$ ; Measurement impedance:  $50.0\Omega + 5.0j\Omega$  (within 5Ω)

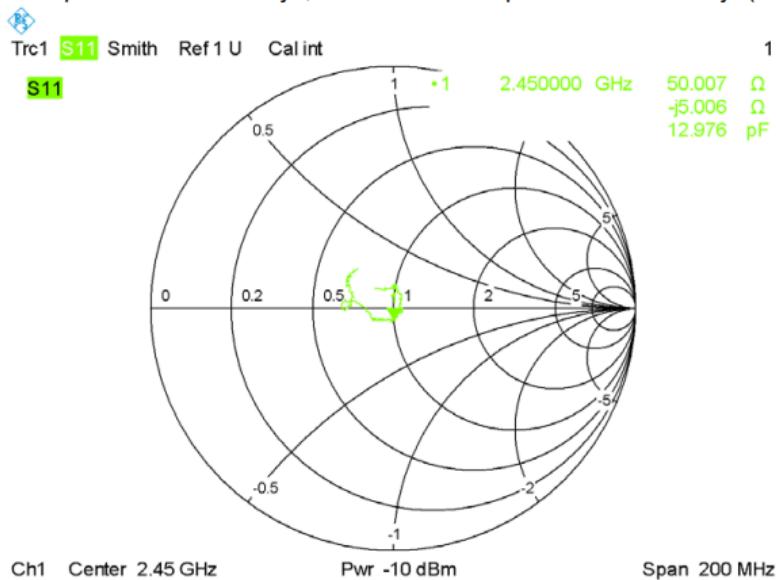

Date: 21.FEB.2024 19:04:50

Calibrated return loss: -27.80dB; Measurement return loss: -26.75dB (within 20%)

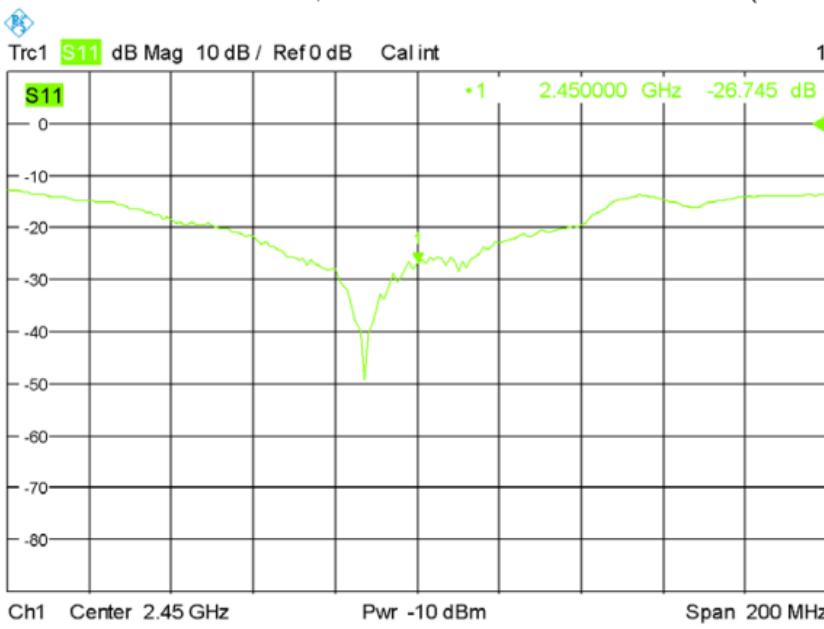

Date: 26.FEB.2024 19:28:46

Report having not been signed by authorized approver, or having been altered without authorization, or having not been stamped by the "Dedicated Test" is deemed to be invalid. Copying or excerpting portion of, or altering the content of the report is not permitted without the written authorization of AGC and the report apply only to the tested sample. Any objections to report issued by AGC should be submitted to AGC within 15days after the issuance of inquiry of validity or verification of the test report should be addressed to AGC by agc01@agccert.com.