

## Head Tissue Simulating Liquids

Head Tissue	Parameters according to IEEE Std 1528-2013 / IEC 62209 / FCC KDB 865664 D01		
<b>Narrow-Band Solutions (±5% tolerance)</b>	<b>Product</b>	<b>Test Frequency (MHz)</b>	<b>Main Ingredients</b>
	HSL300V2	300	Water, Sugar
	HSL450V2	450	Water, Sugar
	HSL750V2	750	Water, Sugar
	HSL900V2	835, 900	Water, Sugar
	HSL1450V2	1450, 1500, 1640	Water, DGBE
	HSL1750V2	1750	Water, DGBE
	HSL1800V2	1800, 1900	Water, DGBE
	HSL1900V2	1900	Water, DGBE
	HSL1950V2	1950, 2000	Water, DGBE
HSL2450V2	2450, 2600	Water, DGBE	
<b>Broad-Band Solutions (±5% tolerance)</b>	<b>Product</b>	<b>Test Frequency (MHz)</b>	<b>Main Ingredients</b>
	HBBL30-250V3	30-250	Water, Tween
	HBBL1350-1850V3	1400-1800	Water, Tween
	HBBL1550-1950V3	1750-1900	Water, Tween
	HBBL1900-3800V3	1950-3000	Water, Tween
	HBBL3500-5800V5	3500-5800	Water, Oil

## Body Tissue Simulating Liquids

Body Tissue (Muscle)	Parameters according to FCC KDB 865664 D01		
<b>Narrow-Band Solutions (±5% tolerance)</b>	<b>Product</b>	<b>Test Frequency (MHz)</b>	<b>Main Ingredients</b>
	MSL300V2	300	Water, Sugar
	MSL450V2	400, 450	Water, Sugar
	MSL750V2	750	Water, Sugar
	MSL900V2	835, 900	Water, Sugar
	MSL1450V2	1450, 1500, 1640	Water, DGBE
	MSL1750V2	1750	Water, DGBE
	MSL1800V2	1800, 1900	Water, DGBE
	MSL1900V2	1900	Water, DGBE
	MSL1950V2	1950, 2100	Water, DGBE
MSL2450V2	2450, 2600	Water, DGBE	
<b>Broad-Band Solutions (±5% tolerance)</b>	<b>Product</b>	<b>Test Frequency (MHz)</b>	<b>Main Ingredients</b>
	MBBL130-250V3	130-250	Water, Tween
	MBBL1350-1850V3	1350-1800	Water, Tween
	MBBL1550-1950V3	1550-1850	Water, Tween
	MBBL1900-3800V3	1950-3800	Water, Tween
	MBBL3500-5800V5	3500-5800	Water, Oil

Zeughausstrasse 43, 8004 Zurich, Switzerland  
 Phone +41 44 245 9700, Fax +41 44 245 9779  
 info@speag.com, http://www.speag.com

## Measurement Certificate / Material Test

Item Name	<b>Head Tissue Simulating Liquid (HSL750V2)</b>
Product No.	SL AAH 075 AA (Charge: 140210-5)
Manufacturer	SPEAG

### Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

### Setup Validation

Validation results were within  $\pm 2.5\%$  towards the target values of Methanol.

### Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



### Test Condition

Ambient	Environment temperatur ( $22 \pm 3$ )°C and humidity < 70%.
TSL Temperature	22°C
Test Date	12-Feb-14
Operator	IEN

### Additional Information

TSL Density	1.284 g/cm <sup>3</sup>
TSL Heat-capacity	2.701 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	$\Delta$ -eps	$\Delta$ -sigma
600	44.4	23.49	0.78	42.7	0.88	3.9	-11.1
625	44.1	23.23	0.81	42.6	0.88	3.5	-8.6
650	43.7	22.96	0.83	42.5	0.89	3.0	-6.2
675	43.3	22.68	0.85	42.3	0.89	2.4	-4.1
700	42.9	22.40	0.87	42.2	0.89	1.7	-1.9
725	42.6	22.25	0.90	42.1	0.89	1.3	0.7
<b>750</b>	<b>42.3</b>	<b>22.10</b>	<b>0.92</b>	<b>41.9</b>	<b>0.89</b>	<b>0.9</b>	<b>3.2</b>
775	42.0	21.89	0.94	41.8	0.90	0.4	5.4
800	41.6	21.67	0.96	41.7	0.90	-0.1	7.5
825	41.3	21.55	0.99	41.6	0.91	-0.6	9.0
838	41.2	21.49	1.00	41.5	0.91	-0.8	9.8
850	41.1	21.42	1.01	41.5	0.92	-1.1	10.6
875	40.8	21.29	1.04	41.5	0.94	-1.8	9.9
900	40.5	21.15	1.06	41.5	0.97	-2.5	9.2
925	40.2	21.01	1.08	41.5	0.98	-3.1	10.0
950	39.9	20.87	1.10	41.4	0.99	-3.7	10.9
975	39.6	20.79	1.13	41.4	1.00	-4.3	12.2
1000	39.4	20.71	1.15	41.3	1.01	-4.8	13.5

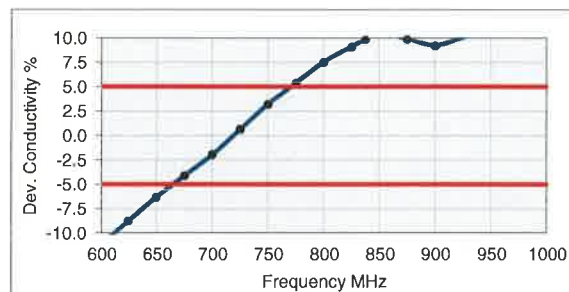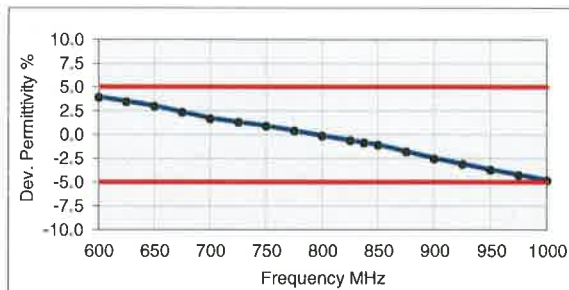

Zeughausstrasse 43, 8004 Zurich, Switzerland  
 Phone +41 44 245 9700, Fax +41 44 245 9779  
 info@speag.com, http://www.speag.com

**Measurement Certificate / Material Test**

Item Name	<b>Head Tissue Simulating Liquid (HSL900V2)</b>
Product No.	SL AAH 090 BB (Charge: 140205-4)
Manufacturer	SPEAG

**Measurement Method**

TSL dielectric parameters measured using calibrated OCP probe.

**Setup Validation**

Validation results were within  $\pm 2.5\%$  towards the target values of Methanol.

**Target Parameters**

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



**Test Condition**

Ambient	Environment temperatur ( $22 \pm 3$ )°C and humidity < 70%.
TSL Temperature	22°C
Test Date	12-Feb-14
Operator	IEN

**Additional Information**

TSL Density	1.280 g/cm <sup>3</sup>
TSL Heat-capacity	2.942 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	$\Delta$ -eps	$\Delta$ -sigma
700	42.9	19.58	0.76	42.2	0.89	1.6	-14.3
725	42.6	19.52	0.79	42.1	0.89	1.2	-11.7
750	42.3	19.47	0.81	41.9	0.89	0.8	-9.1
775	41.9	19.35	0.83	41.8	0.90	0.3	-6.8
800	41.6	19.23	0.86	41.7	0.90	-0.3	-4.6
825	41.3	19.18	0.88	41.6	0.91	-0.7	-2.9
<b>838</b>	<b>41.1</b>	<b>19.16</b>	<b>0.89</b>	<b>41.5</b>	<b>0.91</b>	<b>-1.0</b>	<b>-2.1</b>
850	41.0	19.13	0.90	41.5	0.92	-1.2	-1.2
875	40.7	19.07	0.93	41.5	0.94	-1.9	-1.6
<b>900</b>	<b>40.4</b>	<b>19.00</b>	<b>0.95</b>	<b>41.5</b>	<b>0.97</b>	<b>-2.7</b>	<b>-1.9</b>
925	40.1	18.92	0.97	41.5	0.98	-3.3	-0.9
950	39.8	18.85	1.00	41.4	0.99	-3.9	0.2
975	39.6	18.82	1.02	41.4	1.00	-4.4	1.6
1000	39.3	18.80	1.05	41.3	1.01	-5.0	3.0
1025	39.0	18.71	1.07	41.3	1.03	-5.5	4.0
1050	38.8	18.62	1.09	41.2	1.04	-6.0	5.0
1075	38.5	18.59	1.11	41.2	1.05	-6.5	6.3
1100	38.3	18.55	1.14	41.2	1.06	-7.0	7.5
1125	38.0	18.50	1.16	41.1	1.07	-7.5	8.5
1150	37.8	18.44	1.18	41.1	1.08	-8.0	9.6
1175	37.5	18.39	1.20	41.0	1.09	-8.4	10.6
1200	37.3	18.35	1.22	41.0	1.10	-8.9	11.6

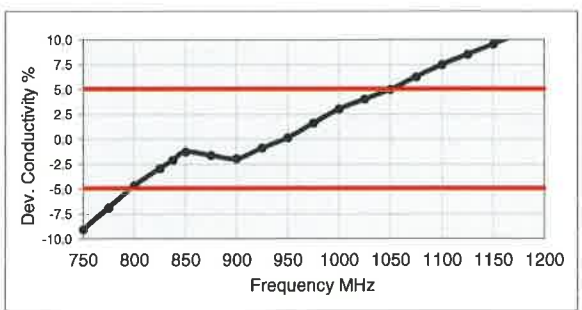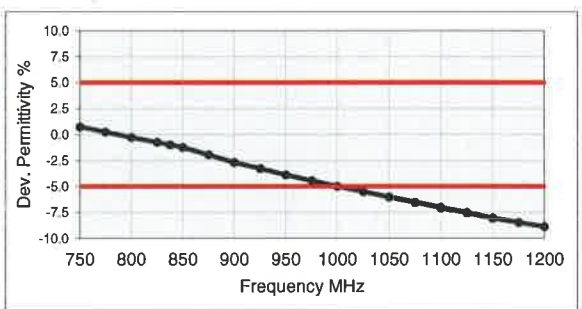

Zeughausstrasse 43, 8004 Zurich, Switzerland  
 Phone +41 44 245 9700, Fax +41 44 245 9779  
 info@speag.com, http://www.speag.com

## Measurement Certificate / Material Test

Item Name **Head Tissue Simulating Liquid (HBBL1550-1950V3)**  
 Product No. SL AAH 181 AA (Charge: 140206-3)  
 Manufacturer SPEAG

### Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

### Setup Validation

Validation results were within  $\pm 2.5\%$  towards the target values of Methanol.

### Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



### Test Condition

Ambient Environment temperatur ( $22 \pm 3$ )°C and humidity < 70%.  
 TSL Temperature 22°C  
 Test Date 12-Feb-14  
 Operator IEN

### Additional Information

TSL Density 1.052 g/cm<sup>3</sup>  
 TSL Heat-capacity 3.322 kJ/(kg\*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	$\Delta$ -eps	$\Delta$ -sigma
1500	40.8	13.29	1.11	40.4	1.23	0.9	-9.7
1525	40.7	13.34	1.13	40.4	1.24	0.7	-8.9
1550	40.6	13.38	1.15	40.4	1.26	0.6	-8.2
1575	40.5	13.41	1.17	40.3	1.27	0.4	-7.5
1600	40.4	13.44	1.20	40.3	1.28	0.2	-6.9
1625	40.3	13.48	1.22	40.3	1.30	0.1	-6.2
1650	40.2	13.53	1.24	40.2	1.31	-0.1	-5.4
1675	40.1	13.54	1.26	40.2	1.33	-0.3	-5.0
1700	40.0	13.55	1.28	40.2	1.34	-0.4	-4.5
1725	39.9	13.60	1.30	40.1	1.36	-0.6	-3.8
1750	39.8	13.64	1.33	40.1	1.37	-0.7	-3.1
1775	39.7	13.67	1.35	40.0	1.39	-0.9	-2.6
1800	39.6	13.70	1.37	40.0	1.40	-1.0	-2.0
1825	39.5	13.75	1.40	40.0	1.40	-1.2	-0.3
1850	39.4	13.81	1.42	40.0	1.40	-1.5	1.5
1875	39.3	13.84	1.44	40.0	1.40	-1.7	3.1
1900	39.2	13.88	1.47	40.0	1.40	-2.0	4.8
1925	39.1	13.92	1.49	40.0	1.40	-2.2	6.5
1950	39.0	13.97	1.52	40.0	1.40	-2.4	8.3
1975	38.9	14.01	1.54	40.0	1.40	-2.6	10.0
2000	38.8	14.05	1.56	40.0	1.40	-2.9	11.6

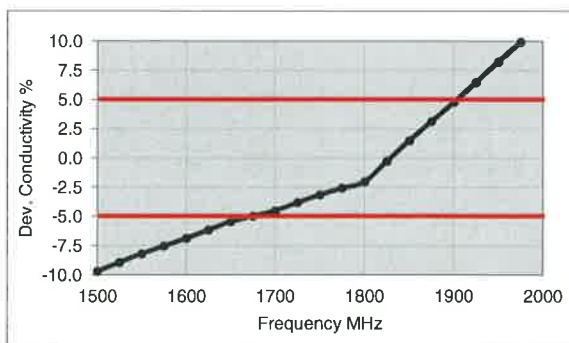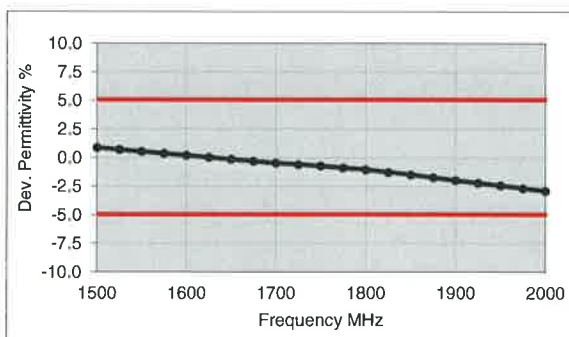

Zeughausstrasse 43, 8004 Zurich, Switzerland  
 Phone +41 44 245 9700, Fax +41 44 245 9779  
 info@speag.com, http://www.speag.com

## Measurement Certificate / Material Test

Item Name **Head Tissue Simulating Liquid (HBBL1900-3800V3)**  
 Product No. SL AAH 196 AB (Charge: 131212-1)  
 Manufacturer SPEAG

### Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

### Setup Validation

Validation results were within  $\pm 2.5\%$  towards the target values of Methanol.

### Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



### Test Condition

Ambient Environment temperatur ( $22 \pm 3$ )°C and humidity < 70%.  
 TSL Temperature 22°C  
 Test Date 18-Dec-13  
 Operator IEN

### Additional Information

TSL Density 1.054 g/cm<sup>3</sup>  
 TSL Heat-capacity 3.389 kJ/(kg\*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	$\Delta$ -eps	$\Delta$ -sigma
1900	41.0	12.2	1.3	40.0	1.4	2.5	-7.9
1950	40.8	12.3	1.3	40.0	1.4	2.1	-4.7
2000	40.7	12.4	1.4	40.0	1.4	1.7	-1.3
2050	40.5	12.6	1.4	39.9	1.4	1.6	-0.6
2100	40.4	12.7	1.5	39.8	1.5	1.4	-0.6
2150	40.2	12.8	1.5	39.7	1.5	1.2	-0.4
2200	40.0	12.9	1.6	39.6	1.6	1.0	0.1
2250	39.9	13.0	1.6	39.6	1.6	0.8	0.4
2300	39.7	13.2	1.7	39.5	1.7	0.5	1.3
2350	39.5	13.3	1.7	39.4	1.7	0.3	1.8
2400	39.3	13.5	1.8	39.3	1.8	0.1	2.4
2450	39.1	13.6	1.9	39.2	1.8	-0.1	2.8
2500	39.0	13.7	1.9	39.1	1.9	-0.4	2.6
2550	38.8	13.8	2.0	39.1	1.9	-0.6	2.7
2600	38.6	14.0	2.0	39.0	2.0	-1.0	2.8
2650	38.4	14.0	2.1	38.9	2.0	-1.4	2.5
2700	38.2	14.2	2.1	38.9	2.1	-1.7	2.7
2750	38.0	14.3	2.2	38.8	2.1	-2.1	2.5
2800	37.8	14.4	2.2	38.8	2.2	-2.4	2.6
2850	37.6	14.5	2.3	38.7	2.2	-2.7	2.6
2900	37.5	14.6	2.4	38.6	2.3	-2.9	2.6
2950	37.3	14.6	2.4	38.6	2.3	-3.3	2.5
3000	37.1	14.7	2.5	38.5	2.4	-3.6	2.3
3050	36.9	14.8	2.5	38.4	2.5	-3.9	2.6
3100	36.7	14.9	2.6	38.4	2.5	-4.3	2.6
3150	36.6	15.0	2.6	38.3	2.6	-4.6	2.8
3200	36.4	15.0	2.7	38.3	2.6	-4.9	2.8
3250	36.2	15.1	2.7	38.2	2.7	-5.2	3.0
3300	36.1	15.2	2.8	38.2	2.7	-5.5	3.0
3350	35.9	15.2	2.8	38.1	2.8	-5.8	2.9
3400	35.7	15.3	2.9	38.0	2.8	-6.0	2.8
3450	35.6	15.3	2.9	38.0	2.9	-6.3	2.8
3500	35.4	15.4	3.0	37.9	2.9	-6.6	2.8
3550	35.3	15.4	3.0	37.9	3.0	-6.9	2.9
3600	35.1	15.5	3.1	37.8	3.0	-7.2	2.9
3650	34.9	15.5	3.2	37.8	3.1	-7.5	2.9
3700	34.7	15.6	3.2	37.7	3.1	-7.8	3.2
3750	34.6	15.7	3.3	37.6	3.2	-8.1	3.2
3800	34.5	15.7	3.3	37.6	3.2	-8.3	3.4
3850	34.3	15.8	3.4	37.5	3.3	-8.5	3.2

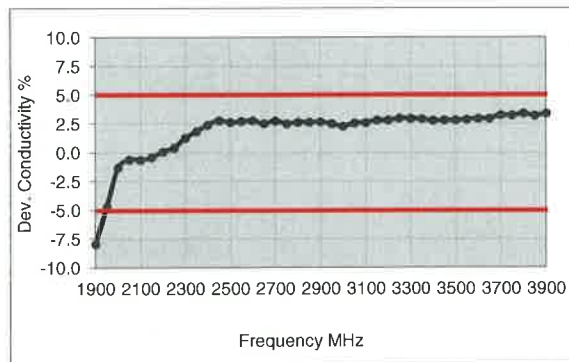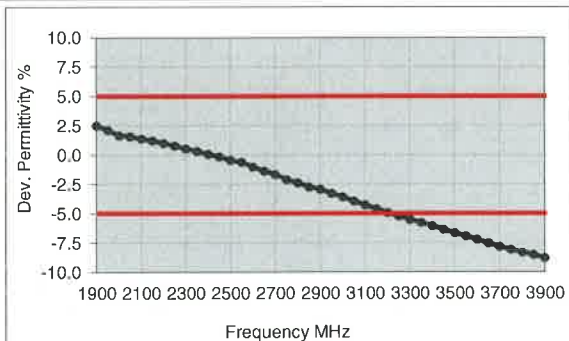

## Measurement Certificate / Material Test

Item Name	Head Tissue Simulating Liquid (HBBL3500-5800V5)
Product No.	SL AAH 502 AB (Charge: 130123-1)
Manufacturer	SPEAG

### Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

### Setup Validation

Validation results were within  $\pm 2.5\%$  towards the target values of Methanol.

### Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



### Test Condition

Ambient Environment temperatur ( $22 \pm 3$ )°C and humidity < 70%.  
 TSL Temperature 22°C  
 Test Date 23-Jan-13  
 Operator DI

### Additional Information

TSL Density 0.985 g/cm<sup>3</sup>  
 TSL Heat-capacity 3.383 kJ/(kg\*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	$\Delta$ -eps	$\Delta$ -sigma
3400	38.8	15.03	2.84	38.0	2.81	1.9	1.2
<b>3500</b>	<b>38.6</b>	<b>15.00</b>	<b>2.92</b>	<b>37.9</b>	<b>2.91</b>	<b>1.8</b>	<b>0.3</b>
3600	38.5	14.98	3.00	37.8	3.02	1.7	-0.5
<b>3700</b>	<b>38.4</b>	<b>14.97</b>	<b>3.08</b>	<b>37.7</b>	<b>3.12</b>	<b>1.7</b>	<b>-1.2</b>
3800	38.2	14.95	3.16	37.6	3.22	1.7	-1.8
3900	38.1	14.96	3.25	37.5	3.32	1.7	-2.3
4000	38.0	14.99	3.34	37.4	3.43	1.8	-2.6
4100	37.9	15.03	3.43	37.2	3.53	1.8	-2.8
4200	37.8	15.06	3.52	37.1	3.63	1.8	-3.0
4300	37.7	15.13	3.62	37.0	3.73	1.8	-3.1
4400	37.6	15.20	3.72	36.9	3.84	1.8	-3.0
4500	37.4	15.23	3.81	36.8	3.94	1.7	-3.2
4600	37.3	15.30	3.92	36.7	4.04	1.6	-3.1
4700	37.1	15.35	4.01	36.6	4.14	1.5	-3.1
4800	37.0	15.41	4.11	36.4	4.25	1.5	-3.1
4850	36.9	15.45	4.17	36.4	4.30	1.5	-3.0
4900	36.8	15.49	4.22	36.3	4.35	1.4	-2.9
4950	36.8	15.51	4.27	36.3	4.40	1.4	-2.9
5000	36.7	15.54	4.32	36.2	4.45	1.4	-2.9
5050	36.6	15.57	4.37	36.2	4.50	1.3	-2.8
5100	36.6	15.60	4.42	36.1	4.55	1.3	-2.8
5150	36.5	15.63	4.48	36.0	4.60	1.2	-2.7
<b>5200</b>	<b>36.4</b>	<b>15.67</b>	<b>4.53</b>	<b>36.0</b>	<b>4.66</b>	<b>1.2</b>	<b>-2.6</b>
5250	36.3	15.68	4.58	35.9	4.71	1.1	-2.7
5300	36.2	15.71	4.63	35.9	4.76	1.0	-2.6
5350	36.2	15.74	4.68	35.8	4.81	1.0	-2.6
5400	36.1	15.78	4.74	35.8	4.86	0.9	-2.5
5450	36.0	15.78	4.78	35.7	4.91	0.9	-2.6
<b>5500</b>	<b>36.0</b>	<b>15.79</b>	<b>4.83</b>	<b>35.6</b>	<b>4.96</b>	<b>0.9</b>	<b>-2.6</b>
5550	35.9	15.84	4.89	35.6	5.01	0.9	-2.5
5600	35.8	15.86	4.94	35.5	5.07	0.8	-2.5
5650	35.8	15.91	5.00	35.5	5.12	0.8	-2.2
5700	35.7	15.91	5.05	35.4	5.17	0.8	-2.4
5750	35.6	15.97	5.11	35.4	5.22	0.7	-2.1
<b>5800</b>	<b>35.5</b>	<b>15.98</b>	<b>5.16</b>	<b>35.3</b>	<b>5.27</b>	<b>0.7</b>	<b>-2.1</b>
5850	35.5	16.01	5.21	35.3	5.34	0.5	-2.4
5900	35.4	16.05	5.27	35.3	5.40	0.3	-2.4

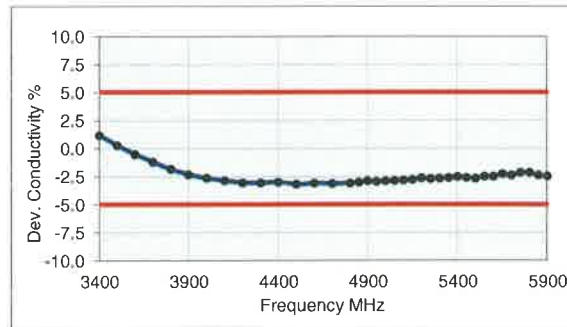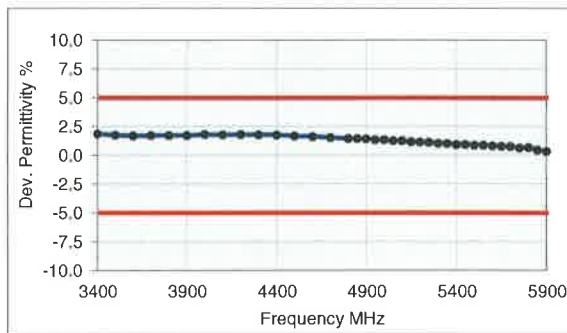

Zeughausstrasse 43, 8004 Zurich, Switzerland  
 Phone +41 44 245 9700, Fax +41 44 245 9779  
 info@speag.com, http://www.speag.com

## Measurement Certificate / Material Test

Item Name **Body Tissue Simulating Liquid (MSL750V2)**  
 Product No. SL AAM 075 (Charge: 120831-2)  
 Manufacturer SPEAG

### Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

### Setup Validation

Validation results were within  $\pm 2.5\%$  towards the target values of Methanol.

### Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



### Test Condition

Ambient Environment temperatur ( $22 \pm 3$ )°C and humidity < 70%.  
 TSL Temperature 22°C  
 Test Date 5-Sep-12  
 Operator CL

### Additional Information

TSL Density 1.212 g/cm<sup>3</sup>  
 TSL Heat-capacity 3.006 kJ/(kg\*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	$\Delta$ -eps	$\Delta$ -sigma
600	57.4	24.67	0.82	56.1	0.95	2.2	-13.5
625	57.1	24.34	0.85	56.0	0.95	1.9	-11.3
650	56.8	24.01	0.87	55.9	0.96	1.6	-9.1
675	56.6	23.71	0.89	55.8	0.96	1.3	-7.1
700	56.3	23.41	0.91	55.7	0.96	1.0	-5.0
725	56.0	23.20	0.94	55.6	0.96	0.7	-2.7
<b>750</b>	<b>55.8</b>	<b>22.99</b>	<b>0.96</b>	<b>55.5</b>	<b>0.96</b>	<b>0.5</b>	<b>-0.4</b>
775	55.5	22.81	0.98	55.4	0.97	0.2	1.9
800	55.3	22.64	1.01	55.3	0.97	-0.1	4.2
825	55.1	22.47	1.03	55.2	0.98	-0.3	5.5
838	54.9	22.39	1.04	55.2	0.98	-0.5	6.1
850	54.8	22.31	1.05	55.2	0.99	-0.6	6.7
875	54.6	22.19	1.08	55.1	1.02	-0.9	6.0
900	54.4	22.07	1.10	55.0	1.05	-1.1	5.2
925	54.1	21.96	1.13	55.0	1.06	-1.5	6.3
950	53.9	21.85	1.15	54.9	1.08	-1.9	7.4
975	53.7	21.75	1.18	54.9	1.09	-2.2	8.5
1000	53.5	21.64	1.20	54.8	1.10	-2.5	9.6

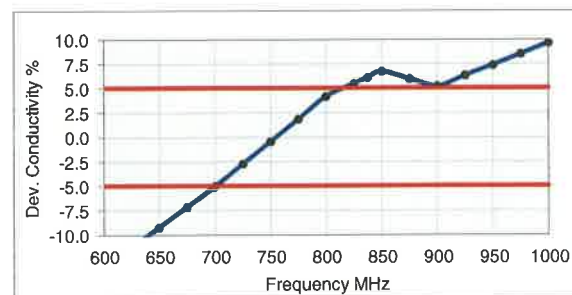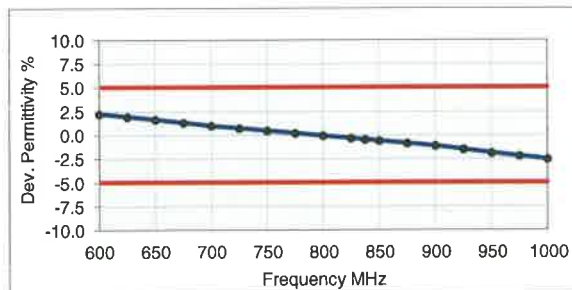

Zeughausstrasse 43, 8004 Zurich, Switzerland  
 Phone +41 44 245 9700, Fax +41 44 245 9779  
 info@speag.com, http://www.speag.com

## Measurement Certificate / Material Test

Item Name **Body Tissue Simulating Liquid (MSL900V2)**  
 Product No. SL AAM 090 CA (Charge: 140124-1)  
 Manufacturer SPEAG

### Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

### Setup Validation

Validation results were within  $\pm 2.5\%$  towards the target values of Methanol.

### Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



### Test Condition

Ambient Environment temperatur ( $22 \pm 3$ )°C and humidity < 70%.  
 TSL Temperature 22°C  
 Test Date 29-Jan-14  
 Operator IEN

### Additional Information

TSL Density 1.208 g/cm<sup>3</sup>  
 TSL Heat-capacity 3.113 kJ/(kg\*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ-eps	Δ-sigma
700	56.5	22.21	0.86	55.7	0.96	1.4	-9.9
725	56.3	22.03	0.89	55.6	0.96	1.1	-7.6
750	56.0	21.85	0.91	55.5	0.96	0.9	-5.4
775	55.8	21.71	0.94	55.4	0.97	0.6	-3.1
800	55.5	21.57	0.96	55.3	0.97	0.3	-0.8
825	55.3	21.47	0.99	55.2	0.98	0.1	0.8
<b>838</b>	<b>55.2</b>	<b>21.42</b>	<b>1.00</b>	<b>55.2</b>	<b>0.98</b>	<b>-0.1</b>	<b>1.5</b>
850	55.1	21.37	1.01	55.2	0.99	-0.2	2.2
875	54.8	21.28	1.04	55.1	1.02	-0.5	1.6
<b>900</b>	<b>54.6</b>	<b>21.19</b>	<b>1.06</b>	<b>55.0</b>	<b>1.05</b>	<b>-0.8</b>	<b>1.0</b>
925	54.3	21.10	1.09	55.0	1.06	-1.1	2.1
950	54.1	21.01	1.11	54.9	1.08	-1.5	3.2
975	53.9	20.96	1.14	54.9	1.09	-1.8	4.6
1000	53.7	20.90	1.16	54.8	1.10	-2.1	5.9
1025	53.5	20.82	1.19	54.8	1.11	-2.4	7.0
1050	53.3	20.75	1.21	54.7	1.12	-2.7	8.1
1075	53.0	20.70	1.24	54.7	1.13	-3.0	9.4
1100	52.8	20.66	1.26	54.7	1.14	-3.4	10.6
1125	52.6	20.57	1.29	54.6	1.15	-3.7	11.5
1150	52.4	20.48	1.31	54.6	1.17	-3.9	12.4
1175	52.2	20.47	1.34	54.5	1.18	-4.2	13.7
1200	52.0	20.46	1.37	54.5	1.19	-4.5	15.0

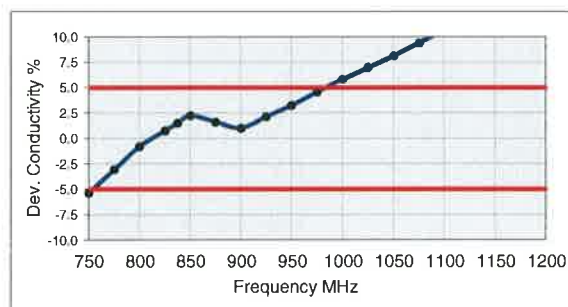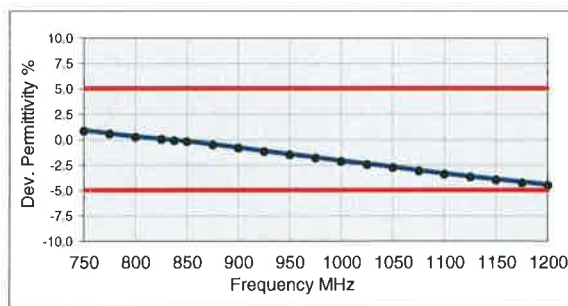



Zeughausstrasse 43, 8004 Zurich, Switzerland  
 Phone +41 44 245 9700, Fax +41 44 245 9779  
 info@speag.com, http://www.speag.com

## Measurement Certificate / Material Test

Item Name **Body Tissue Simulating Liquid (MBBL1550-1950V3)**  
 Product No. SL AAM 181 AA (Charge: 140218-3)  
 Manufacturer SPEAG

### Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

### Setup Validation

Validation results were within  $\pm 2.5\%$  towards the target values of Methanol.

### Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



### Test Condition

Ambient Environment temperatur ( $22 \pm 3$ )°C and humidity < 70%.  
 TSL Temperature 22°C  
 Test Date 19-Feb-14  
 Operator IEN

### Additional Information

TSL Density 1.042 g/cm<sup>3</sup>  
 TSL Heat-capacity 3.475 kJ/(kg\*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-ε'	HP-ε''	sigma	eps	sigma	Δ-eps	Δ-sigma
1500	53.5	14.88	1.24	53.9	1.33	-0.9	-6.7
1525	53.4	14.88	1.26	53.9	1.35	-0.9	-6.2
1550	53.4	14.89	1.28	53.9	1.36	-1.0	-5.8
1575	53.2	14.89	1.30	53.8	1.38	-1.1	-5.3
1600	53.1	14.90	1.33	53.8	1.39	-1.2	-4.8
1625	53.1	14.89	1.35	53.8	1.41	-1.2	-4.5
1650	53.0	14.88	1.37	53.7	1.43	-1.3	-4.2
1675	52.9	14.86	1.38	53.6	1.44	-1.3	-3.9
1700	52.9	14.84	1.40	53.6	1.46	-1.3	-3.7
1725	52.8	14.87	1.43	53.5	1.47	-1.3	-3.1
1750	52.7	14.90	1.45	53.4	1.49	-1.4	-2.6
1775	52.6	14.90	1.47	53.4	1.50	-1.4	-2.2
1800	52.8	14.91	1.49	53.3	1.52	-1.4	-1.8
1825	52.5	14.99	1.52	53.3	1.52	-1.5	0.1
1850	52.4	15.07	1.55	53.3	1.52	-1.7	2.0
1875	52.3	15.06	1.57	53.3	1.52	-1.8	3.3
1900	52.3	15.05	1.59	53.3	1.52	-1.9	4.6
1925	52.2	15.09	1.62	53.3	1.52	-2.1	6.3
1950	52.1	15.13	1.64	53.3	1.52	-2.2	8.0
1975	52.1	15.17	1.67	53.3	1.52	-2.3	9.7
2000	52.0	15.21	1.69	53.3	1.52	-2.4	11.3

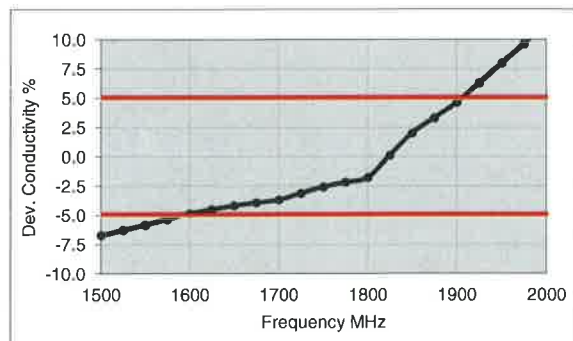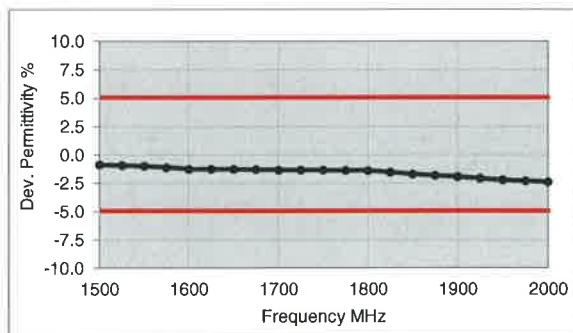

Zeughausstrasse 43, 8004 Zurich, Switzerland  
 Phone +41 44 245 9700, Fax +41 44 245 9779  
 info@speag.com, http://www.speag.com

## Measurement Certificate / Material Test

Item Name	Body Tissue Simulating Liquid (MBBL1900-3800V3)
Product No.	SL AAM 196 AB (Charge: 140219-3)
Manufacturer	SPEAG

### Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

### Setup Validation

Validation results were within  $\pm 2.5\%$  towards the target values of Methanol.

### Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.

### Test Condition



Ambient	Environment temperatur ( $22 \pm 3$ )°C and humidity < 70%.
TSL Temperature	22°C
Test Date	19-Feb-14
Operator	IEN

### Additional Information

TSL Density 1.036 g/cm<sup>3</sup>

TSL Heat-capacity 3.508 kJ/(kg\*K)

f [MHz]	Measured			Target		Diff. to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	$\Delta$ -eps	$\Delta$ -sigma
1900	53.5	13.3	1.41	53.3	1.52	0.5	-7.3
1950	53.4	13.4	1.46	53.3	1.52	0.2	-4.1
2000	53.3	13.5	1.51	53.3	1.52	0.0	-0.8
2050	53.2	13.6	1.55	53.2	1.57	0.0	-1.1
2100	53.1	13.7	1.60	53.2	1.62	-0.1	-0.7
2150	53.0	13.8	1.65	53.1	1.66	-0.2	-0.9
2200	52.8	13.9	1.70	53.0	1.71	-0.4	-0.5
2250	52.7	14.0	1.76	53.0	1.76	-0.4	0.0
2300	52.6	14.2	1.82	52.9	1.81	-0.6	0.7
2350	52.4	14.4	1.88	52.8	1.85	-0.7	1.3
2400	52.3	14.5	1.94	52.8	1.90	-0.9	2.0
2450	52.2	14.7	2.00	52.7	1.95	-1.0	2.4
2500	52.0	14.8	2.05	52.6	2.02	-1.1	1.6
2550	52.0	14.8	2.10	52.6	2.09	-1.1	0.3
2600	51.8	15.0	2.17	52.5	2.16	-1.4	0.1
2650	51.6	15.1	2.23	52.4	2.23	-1.6	-0.3
2700	51.5	15.2	2.29	52.4	2.30	-1.8	-0.8
2750	51.2	15.3	2.34	52.3	2.38	-2.1	-1.5
2800	51.1	15.4	2.40	52.3	2.45	-2.2	-1.7
2850	50.9	15.6	2.47	52.2	2.52	-2.4	-2.0
2900	50.8	15.7	2.53	52.1	2.59	-2.5	-2.2
2950	50.7	15.8	2.59	52.1	2.66	-2.7	-2.8
3000	50.5	15.9	2.65	52.0	2.73	-2.8	-3.0
3050	50.4	16.0	2.71	51.9	2.79	-3.0	-2.9
3100	50.2	16.1	2.78	51.9	2.85	-3.2	-2.4
3150	50.1	16.2	2.85	51.8	2.91	-3.3	-2.0
3200	49.9	16.3	2.90	51.7	2.96	-3.6	-2.1
3250	49.8	16.5	2.98	51.7	3.02	-3.6	-1.5
3300	49.6	16.5	3.02	51.6	3.08	-3.8	-1.8
3350	49.5	16.6	3.09	51.5	3.14	-3.9	-1.5
3400	49.4	16.6	3.15	51.5	3.20	-4.0	-1.5
3450	49.2	16.7	3.21	51.4	3.26	-4.2	-1.4
3500	49.1	16.8	3.28	51.3	3.31	-4.3	-1.0
3550	48.9	16.9	3.34	51.3	3.37	-4.5	-0.9
3600	48.8	17.1	3.42	51.2	3.43	-4.6	-0.4
3650	48.7	17.1	3.47	51.1	3.49	-4.8	-0.5
3700	48.5	17.2	3.55	51.1	3.55	-4.9	0.0
3750	48.4	17.3	3.61	51.0	3.61	-5.0	0.0
3800	48.3	17.4	3.67	50.9	3.66	-5.1	0.1
3850	48.2	17.5	3.74	50.8	3.72	-5.2	0.5

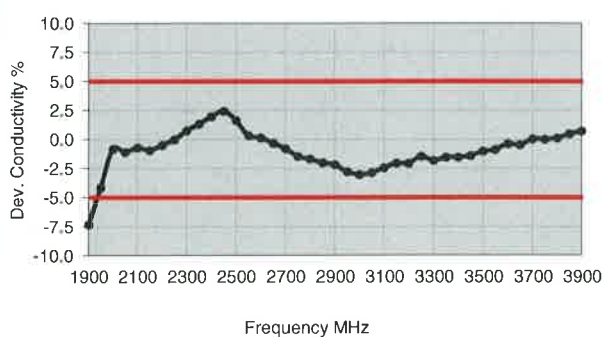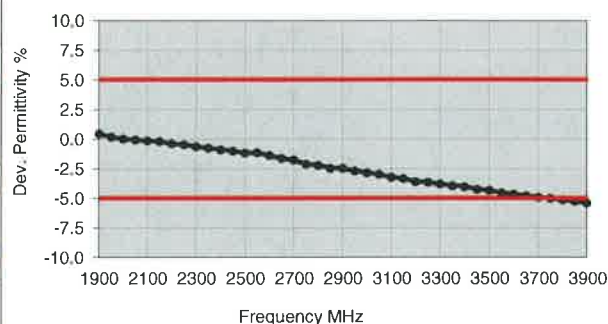

Zeughausstrasse 43, 8004 Zurich, Switzerland  
 Phone +41 44 245 9700, Fax +41 44 245 9779  
 info@speag.com, http://www.speag.com

## Measurement Certificate / Material Test

Item Name **Body Tissue Simulating Liquid (MBBL3500-5800V5)**  
 Product No. SL AAM 501 EA (Charge: 140114-1)  
 Manufacturer SPEAG

### Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

### Setup Validation

Validation results were within  $\pm 2.5\%$  towards the target values of Methanol.

### Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.

### Test Condition

Ambient Environment temperatur ( $22 \pm 3$ )°C and humidity < 70%.  
 TSL Temperature 22°C  
 Test Date 15-Jan-14  
 Operator IEN

### Additional Information

TSL Density 0.996 g/cm<sup>3</sup>  
 TSL Heat-capacity 3.765 kJ/(kg\*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ-eps	Δ-sigma
3400	52.2	16.63	3.14	51.5	3.20	1.4	-1.8
<b>3500</b>	<b>52.0</b>	<b>16.67</b>	<b>3.25</b>	<b>51.3</b>	<b>3.31</b>	<b>1.3</b>	<b>-1.9</b>
3600	51.9	16.74	3.35	51.2	3.43	1.4	-2.4
<b>3700</b>	<b>51.7</b>	<b>16.81</b>	<b>3.46</b>	<b>51.1</b>	<b>3.55</b>	<b>1.3</b>	<b>-2.5</b>
3800	51.6	16.90	3.57	50.9	3.66	1.3	-2.6
3900	51.5	16.99	3.69	50.8	3.78	1.4	-2.4
4000	51.3	17.08	3.80	50.6	3.90	1.3	-2.5
4100	51.2	17.18	3.92	50.5	4.01	1.4	-2.4
4200	51.1	17.32	4.05	50.4	4.13	1.4	-2.0
4300	50.9	17.47	4.18	50.2	4.25	1.3	-1.6
4400	50.8	17.61	4.31	50.1	4.37	1.4	-1.3
4500	50.6	17.73	4.44	50.0	4.48	1.3	-0.9
4600	50.4	17.86	4.57	49.8	4.60	1.1	-0.6
4700	50.3	18.00	4.71	49.7	4.72	1.2	-0.1
4800	50.1	18.14	4.84	49.6	4.83	1.1	0.2
4850	50.0	18.20	4.91	49.5	4.89	1.0	0.4
4900	49.9	18.28	4.98	49.4	4.95	1.0	0.6
4950	49.8	18.31	5.04	49.4	5.01	0.9	0.7
5000	49.7	18.38	5.11	49.3	5.07	0.8	0.9
5050	49.6	18.44	5.18	49.2	5.12	0.8	1.1
5100	49.5	18.50	5.25	49.2	5.18	0.7	1.3
5150	49.4	18.57	5.32	49.1	5.24	0.6	1.5
<b>5200</b>	<b>49.4</b>	<b>18.63</b>	<b>5.39</b>	<b>49.0</b>	<b>5.30</b>	<b>0.8</b>	<b>1.7</b>
5250	49.3	18.68	5.46	48.9	5.36	0.7	1.9
5300	49.2	18.75	5.53	48.9	5.42	0.7	2.1
5350	49.1	18.79	5.59	48.8	5.47	0.6	2.1
5400	49.0	18.86	5.66	48.7	5.53	0.5	2.3
5450	48.9	18.90	5.73	48.7	5.59	0.5	2.5
<b>5500</b>	<b>48.8</b>	<b>18.94</b>	<b>5.80</b>	<b>48.6</b>	<b>5.65</b>	<b>0.4</b>	<b>2.7</b>
5550	48.7	19.01	5.87	48.5	5.71	0.3	2.8
5600	48.7	19.06	5.94	48.5	5.77	0.5	3.0
5650	48.6	19.13	6.01	48.4	5.82	0.4	3.2
5700	48.5	19.18	6.08	48.3	5.88	0.3	3.3
5750	48.4	19.26	6.16	48.3	5.94	0.3	3.7
<b>5800</b>	<b>48.3</b>	<b>19.30</b>	<b>6.23</b>	<b>48.2</b>	<b>6.00</b>	<b>0.2</b>	<b>3.8</b>
5850	48.2	19.37	6.30	48.1	6.06	0.1	4.0
5900	48.1	19.43	6.38	48.1	6.12	0.1	4.3

