



HCT Co., Ltd.

74, Seoicheon-ro 578beon-gil, Majang-myeon, Icheon-si, Gyeonggi-do, 17383 KOREA
Tel. +82 31 634 6300 Fax. +82 31 645 6401

<h1 style="margin: 0;">Appendix A: Test Setup Photo</h1>	<p>FCC ID A3LSMA725F</p> <p>File No. HCT-RF-2101-FC047-P HCT-RF-2101-FC052-P HCT-RF-2101-FC048-P HCT-RF-2101-FC053-P HCT-RF-2101-FC049-P HCT-RF-2101-FC054-P HCT-RF-2101-FC050-P HCT-RF-2101-FC051-P</p>
--	--


REVISION HISTORY

The revision history for this document is shown in table.


Revision No.	Date of Issue	Description
0	January 15, 2021	Initial Release
1	January 22, 2021	Revised the setup photo on 4~5 page

File	HCT-RF-2101-FC047-P	HCT-RF-2101-FC048-P	HCT-RF-2101-FC049-P	HCT-RF-2101-FC050-P	HCT-RF-2101-FC051-P
No.	HCT-RF-2101-FC052-P	HCT-RF-2101-FC053-P	HCT-RF-2101-FC054-P		


1. Radiated Test Setup Photo

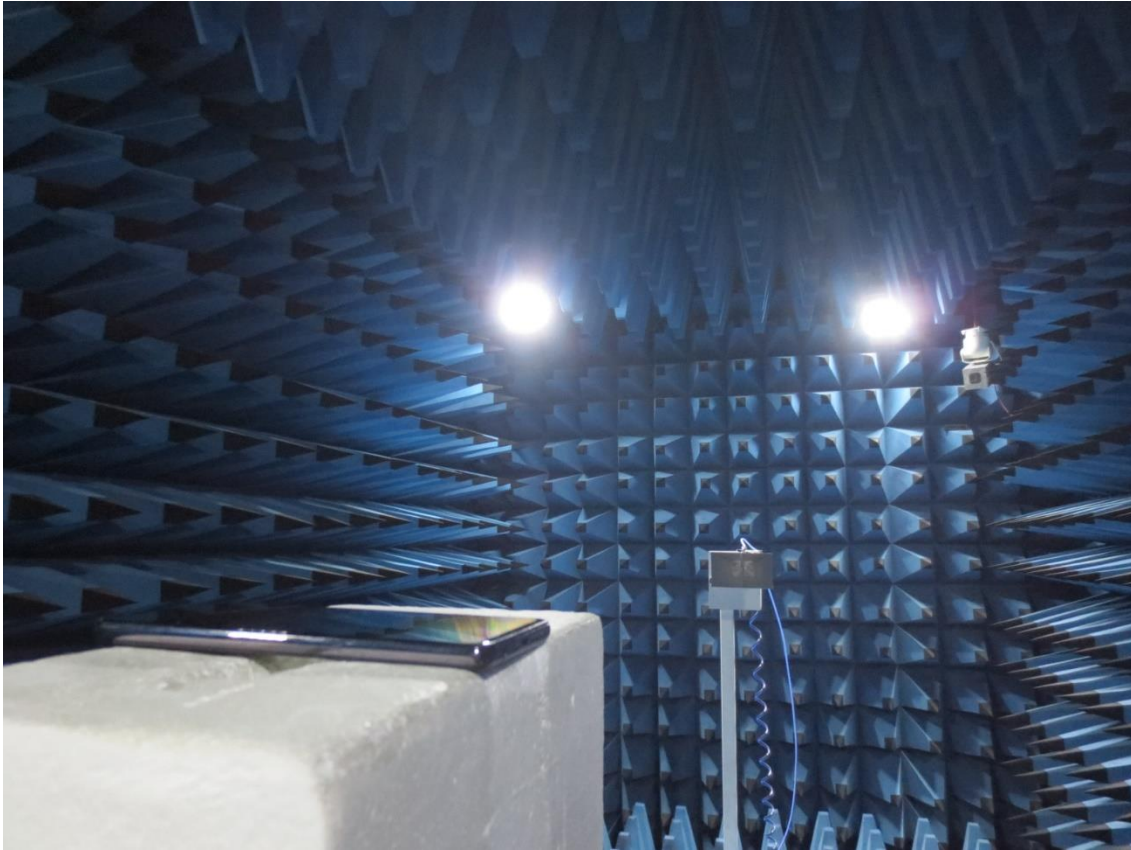


File	HCT-RF-2101-FC047-P	HCT-RF-2101-FC048-P	HCT-RF-2101-FC049-P	HCT-RF-2101-FC050-P	HCT-RF-2101-FC051-P
No.	HCT-RF-2101-FC052-P	HCT-RF-2101-FC053-P	HCT-RF-2101-FC054-P		

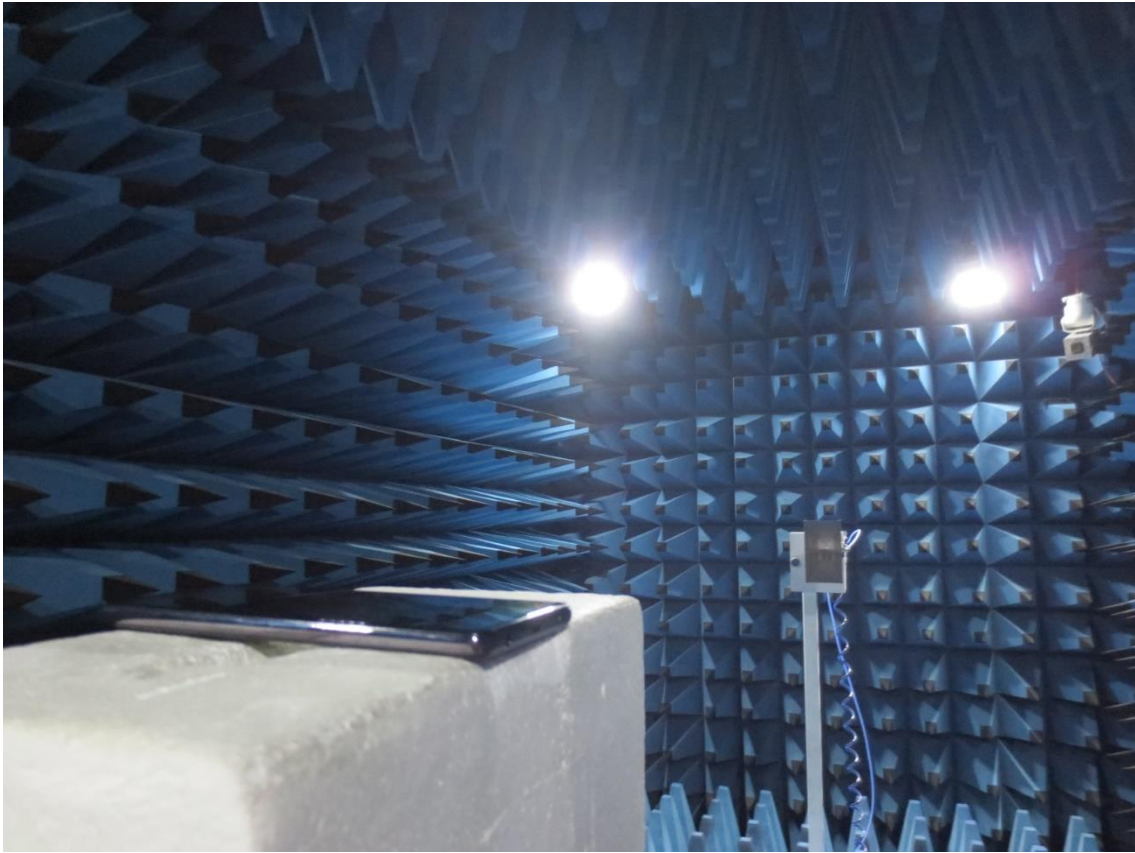


File	HCT-RF-2101-FC047-P	HCT-RF-2101-FC048-P	HCT-RF-2101-FC049-P	HCT-RF-2101-FC050-P	HCT-RF-2101-FC051-P
No.	HCT-RF-2101-FC052-P	HCT-RF-2101-FC053-P	HCT-RF-2101-FC054-P		

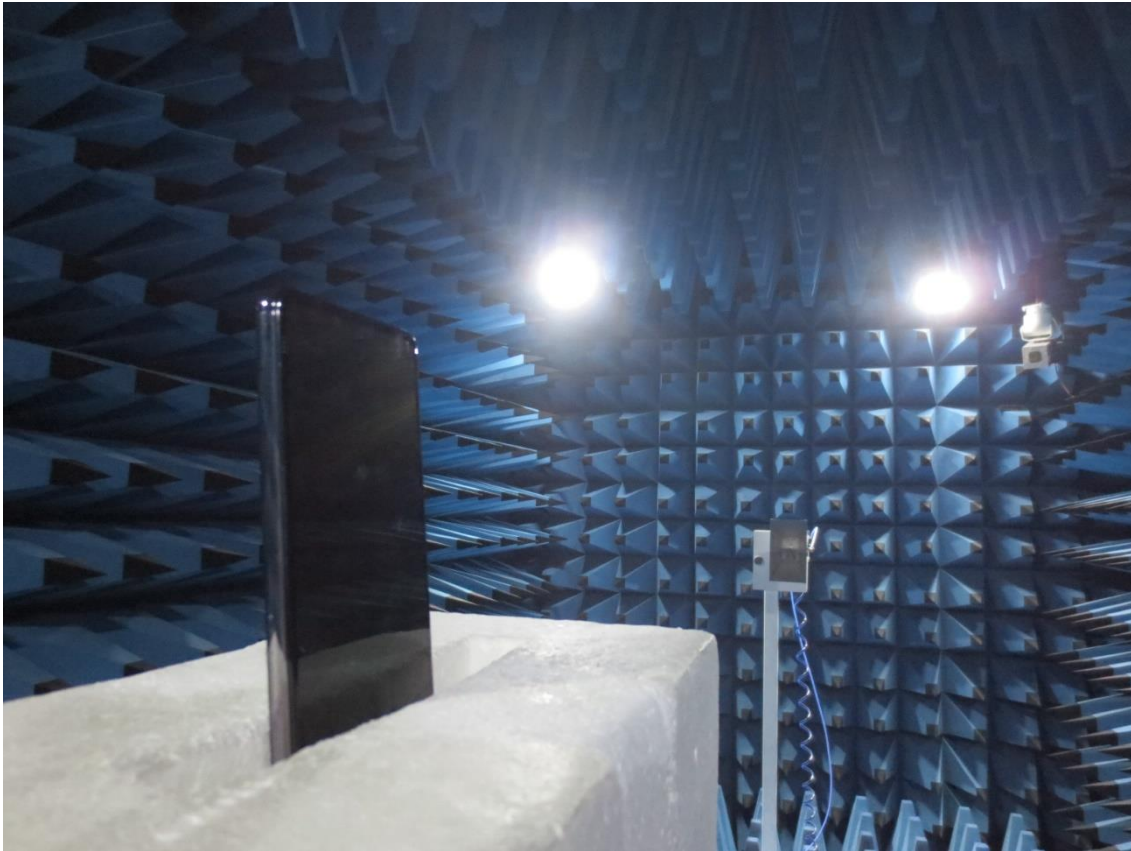


File	HCT-RF-2101-FC047-P	HCT-RF-2101-FC048-P	HCT-RF-2101-FC049-P	HCT-RF-2101-FC050-P	HCT-RF-2101-FC051-P
No.	HCT-RF-2101-FC052-P	HCT-RF-2101-FC053-P	HCT-RF-2101-FC054-P		

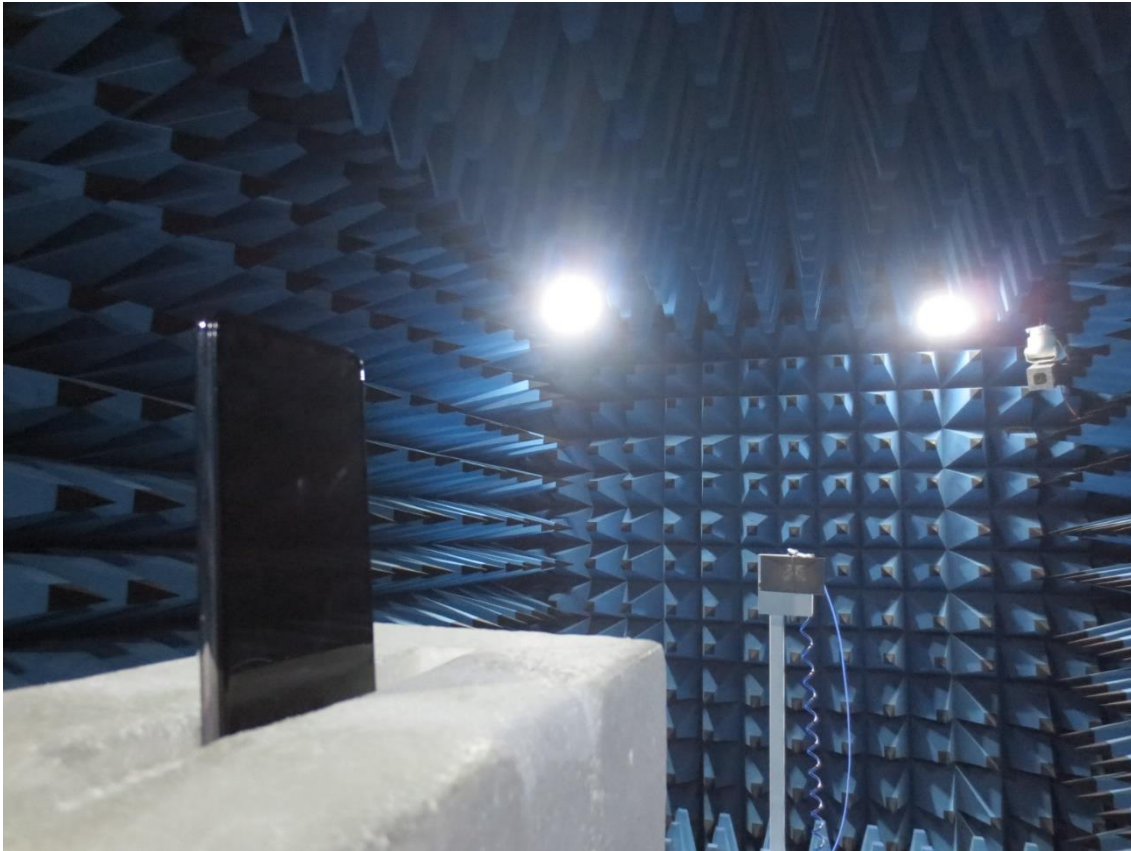


File	HCT-RF-2101-FC047-P	HCT-RF-2101-FC048-P	HCT-RF-2101-FC049-P	HCT-RF-2101-FC050-P	HCT-RF-2101-FC051-P
No.	HCT-RF-2101-FC052-P	HCT-RF-2101-FC053-P	HCT-RF-2101-FC054-P		

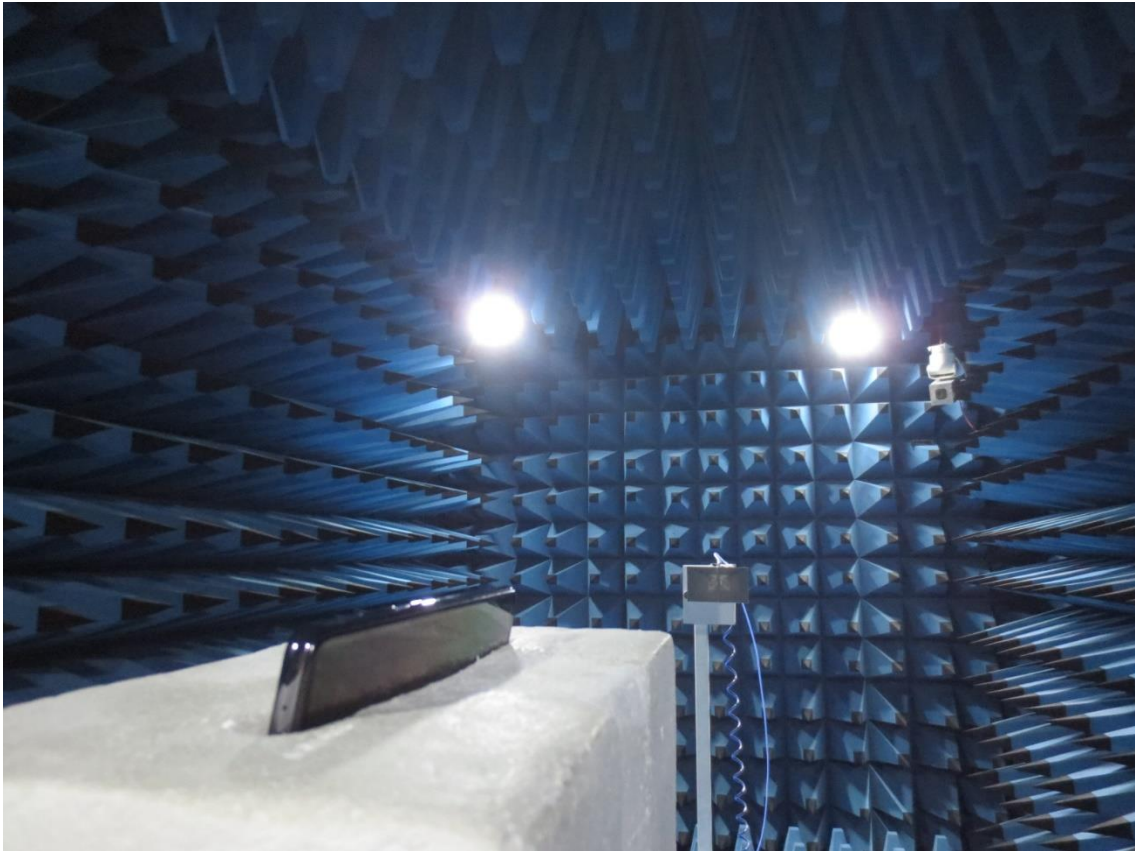


File	HCT-RF-2101-FC047-P	HCT-RF-2101-FC048-P	HCT-RF-2101-FC049-P	HCT-RF-2101-FC050-P	HCT-RF-2101-FC051-P
No.	HCT-RF-2101-FC052-P	HCT-RF-2101-FC053-P	HCT-RF-2101-FC054-P		

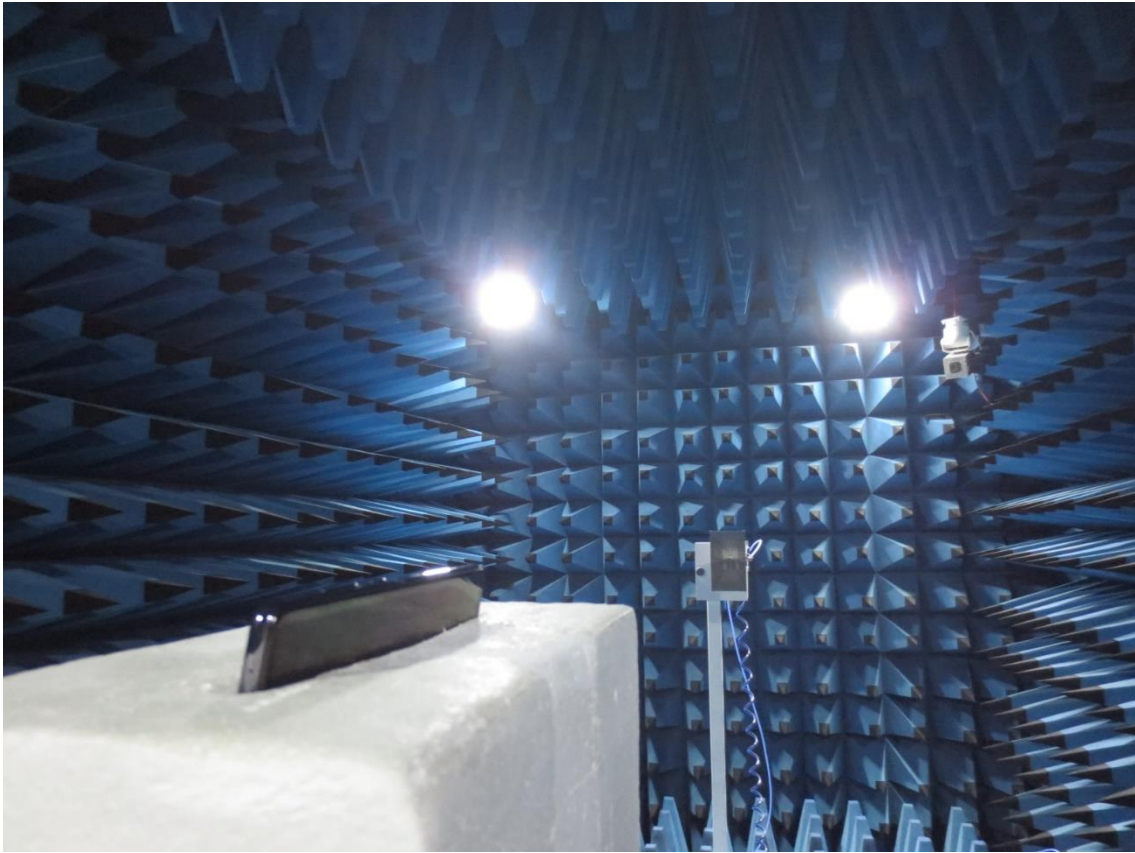


File	HCT-RF-2101-FC047-P	HCT-RF-2101-FC048-P	HCT-RF-2101-FC049-P	HCT-RF-2101-FC050-P	HCT-RF-2101-FC051-P
No.	HCT-RF-2101-FC052-P	HCT-RF-2101-FC053-P	HCT-RF-2101-FC054-P		

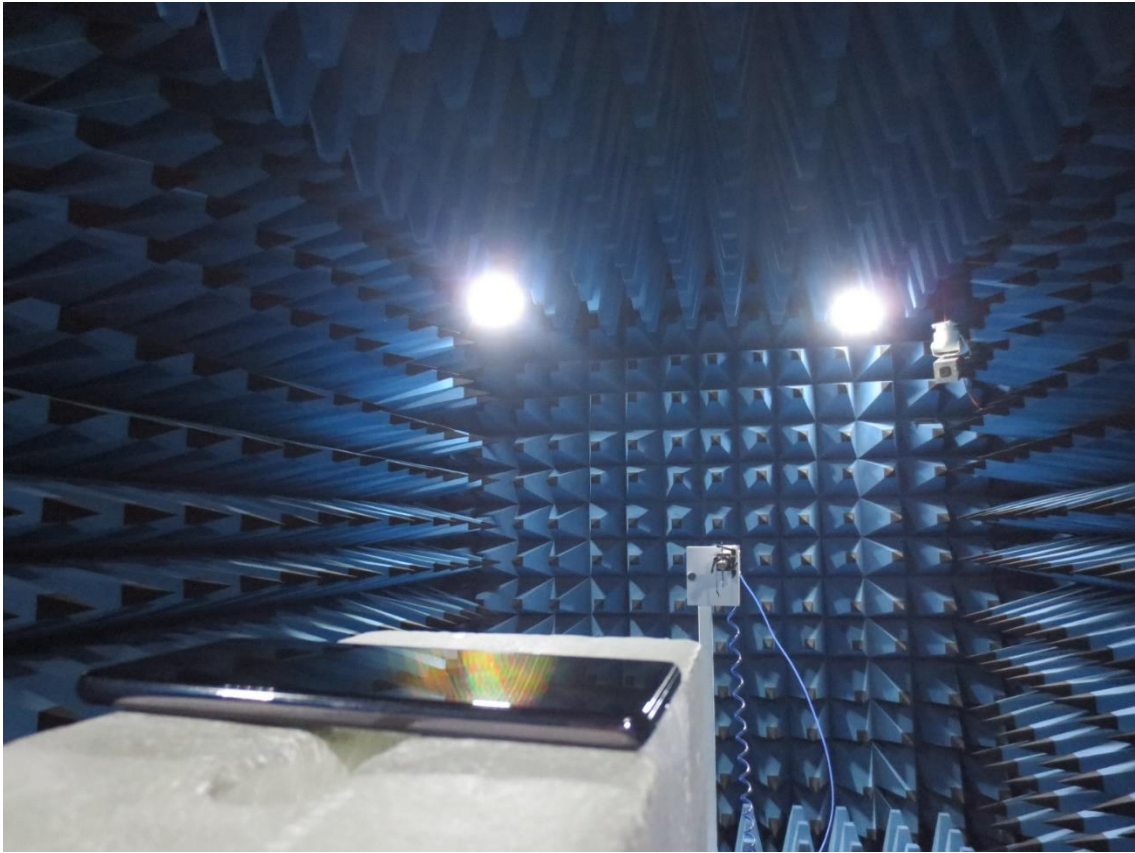


File	HCT-RF-2101-FC047-P	HCT-RF-2101-FC048-P	HCT-RF-2101-FC049-P	HCT-RF-2101-FC050-P	HCT-RF-2101-FC051-P
No.	HCT-RF-2101-FC052-P	HCT-RF-2101-FC053-P	HCT-RF-2101-FC054-P		

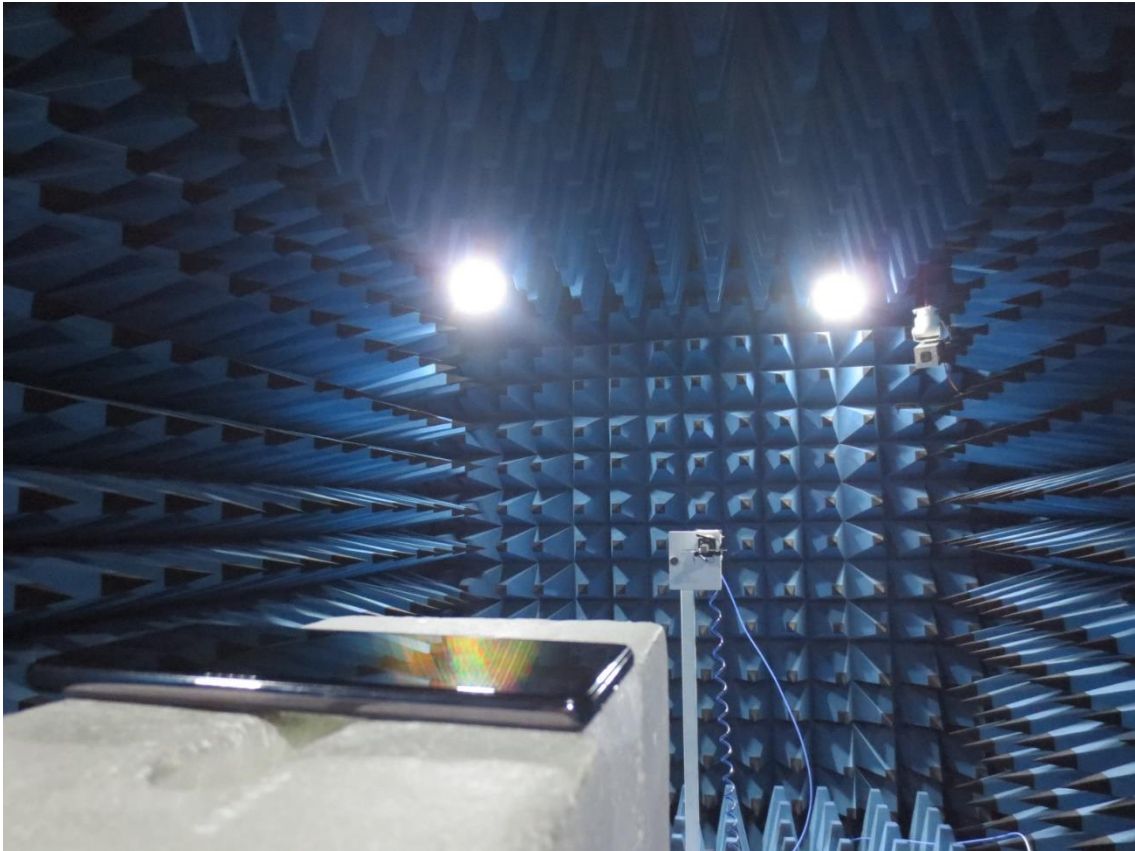


File	HCT-RF-2101-FC047-P	HCT-RF-2101-FC048-P	HCT-RF-2101-FC049-P	HCT-RF-2101-FC050-P	HCT-RF-2101-FC051-P
No.	HCT-RF-2101-FC052-P	HCT-RF-2101-FC053-P	HCT-RF-2101-FC054-P		

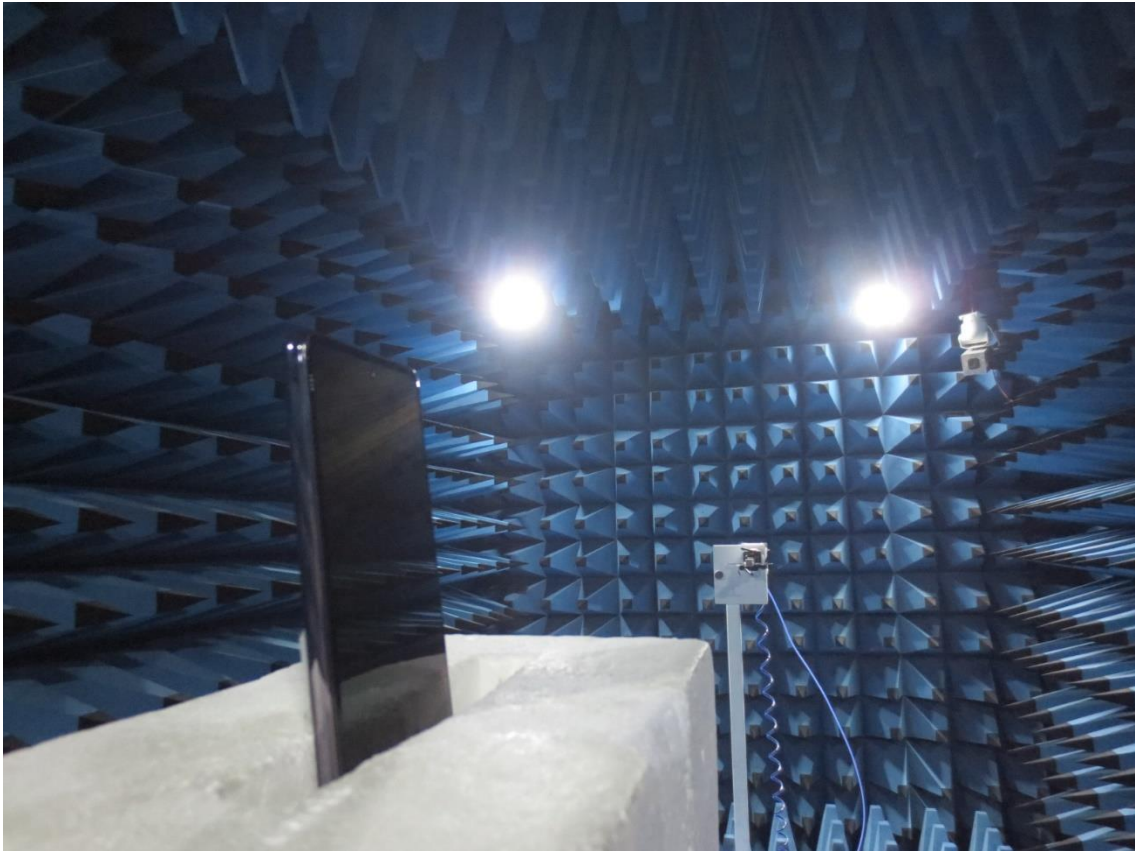


File	HCT-RF-2101-FC047-P	HCT-RF-2101-FC048-P	HCT-RF-2101-FC049-P	HCT-RF-2101-FC050-P	HCT-RF-2101-FC051-P
No.	HCT-RF-2101-FC052-P	HCT-RF-2101-FC053-P	HCT-RF-2101-FC054-P		

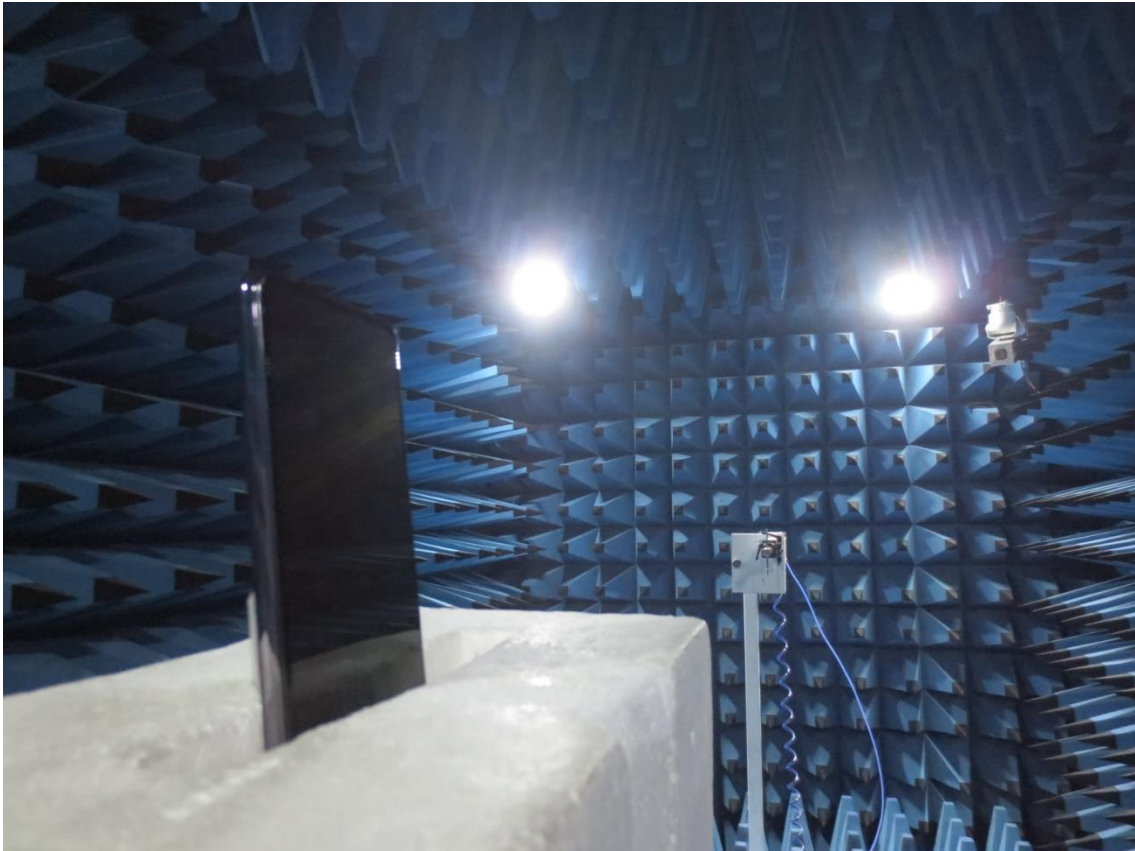

File	HCT-RF-2101-FC047-P	HCT-RF-2101-FC048-P	HCT-RF-2101-FC049-P	HCT-RF-2101-FC050-P	HCT-RF-2101-FC051-P
No.	HCT-RF-2101-FC052-P	HCT-RF-2101-FC053-P	HCT-RF-2101-FC054-P		

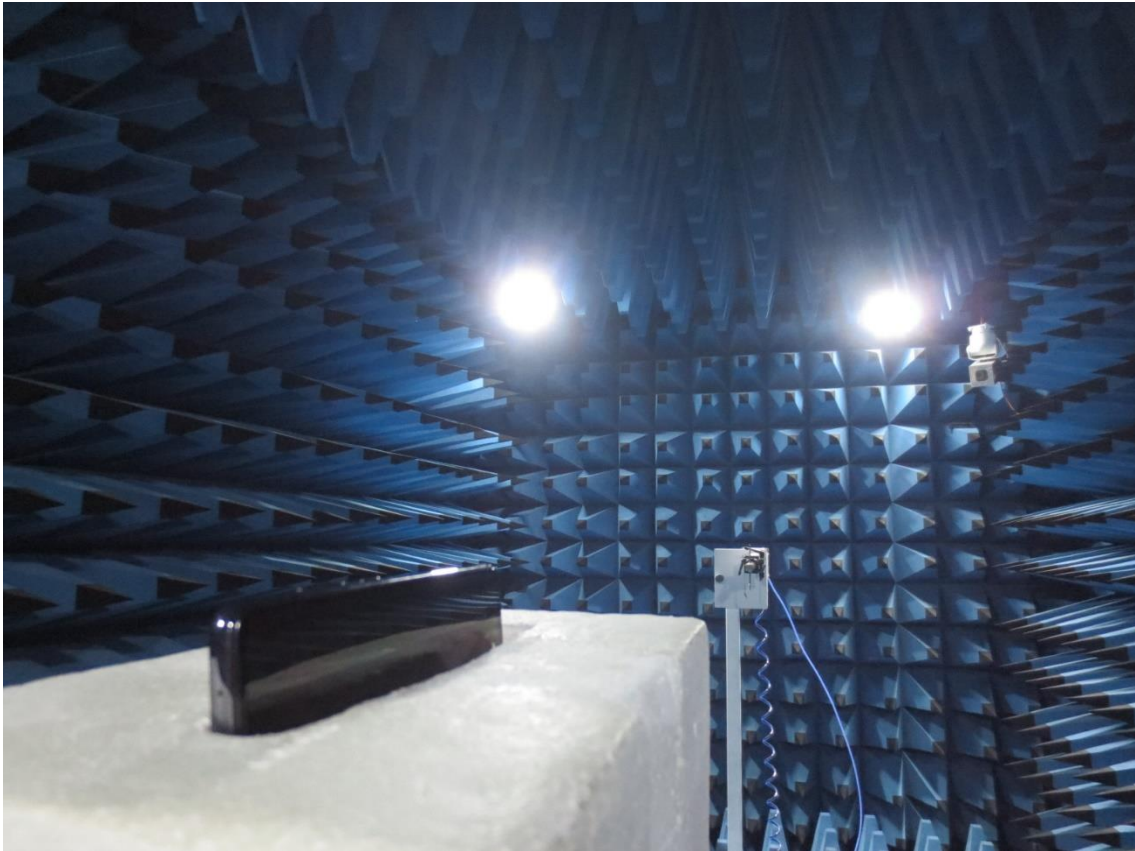

File	HCT-RF-2101-FC047-P	HCT-RF-2101-FC048-P	HCT-RF-2101-FC049-P	HCT-RF-2101-FC050-P	HCT-RF-2101-FC051-P
No.	HCT-RF-2101-FC052-P	HCT-RF-2101-FC053-P	HCT-RF-2101-FC054-P		

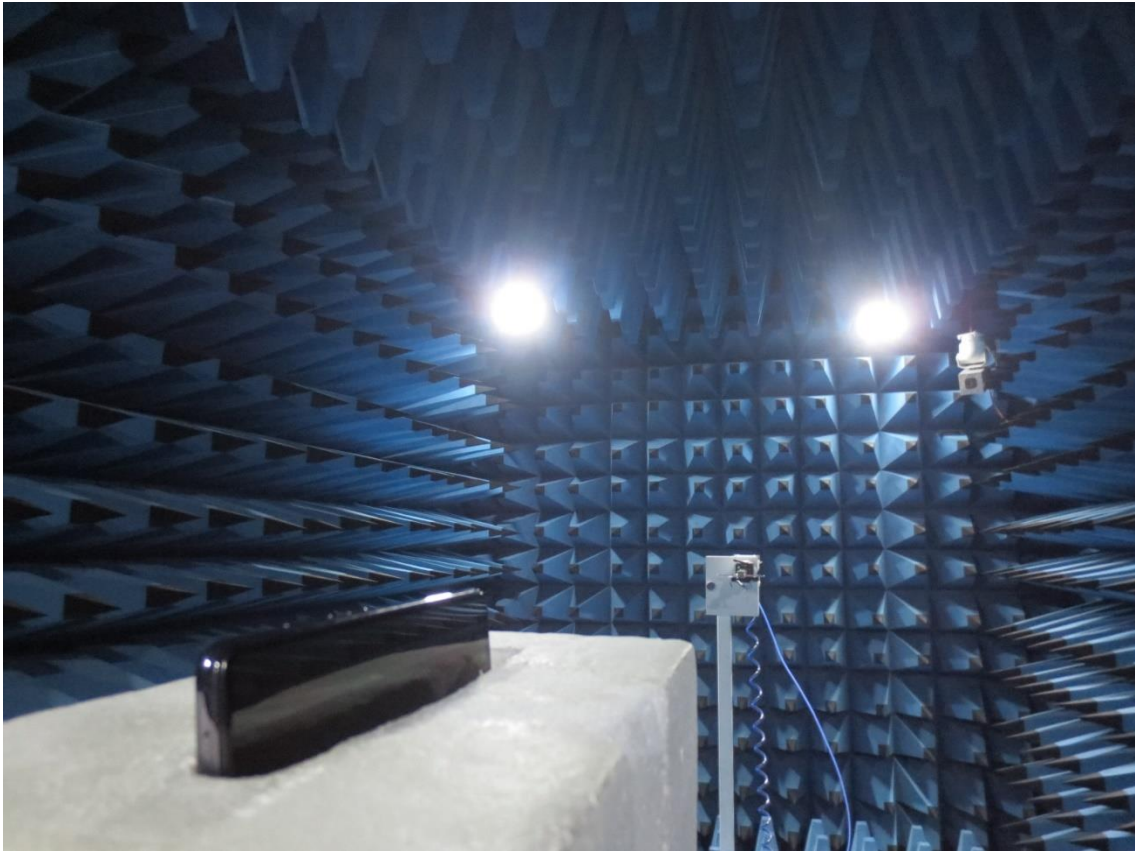

File	HCT-RF-2101-FC047-P	HCT-RF-2101-FC048-P	HCT-RF-2101-FC049-P	HCT-RF-2101-FC050-P	HCT-RF-2101-FC051-P
No.	HCT-RF-2101-FC052-P	HCT-RF-2101-FC053-P	HCT-RF-2101-FC054-P		

2. Conducted Test Setup Photo



File	HCT-RF-2101-FC047-P	HCT-RF-2101-FC048-P	HCT-RF-2101-FC049-P	HCT-RF-2101-FC050-P	HCT-RF-2101-FC051-P
No.	HCT-RF-2101-FC052-P	HCT-RF-2101-FC053-P	HCT-RF-2101-FC054-P		