

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

**Glossary:**

TSL	tissue simulating liquid
NORM <sub>x,y,z</sub>	sensitivity in free space
ConvF	sensitivity in TSL / NORM <sub>x,y,z</sub>
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization $\varphi$	$\varphi$ rotation around probe axis
Polarization $\theta$	$\theta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

**Calibration is Performed According to the Following Standards:**

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Methods Applied and Interpretation of Parameters:**

- NORM<sub>x,y,z</sub>:** Assessed for E-field polarization  $\theta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not affect the E<sup>2</sup>-field uncertainty inside TSL (see below ConvF).
- NORM(f)<sub>x,y,z</sub> = NORM<sub>x,y,z</sub> \* frequency\_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>x,y,z</sub>:** DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR:** PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; D<sub>x,y,z</sub>; VR<sub>x,y,z</sub>:** A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters:** Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy):** in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset:** The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle:** The angle is assessed using the information gained by determining the NORM<sub>x</sub> (no uncertainty required).

EX3DV4 – SN:3863

April 25, 2018

# Probe EX3DV4

## SN:3863

Manufactured: February 2, 2012  
Calibrated: April 25, 2018

Calibrated for DASY/EASY Systems  
(Note: non-compatible with DASY2 system!)

EX3DV4- SN:3863

April 25, 2018

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3863

### Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ( $\mu\text{V}/(\text{V/m})^2$ ) <sup>A</sup>	0.35	0.34	0.45	$\pm 10.1\%$
DCP (mV) <sup>B</sup>	99.7	103.9	103.3	

### Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Unc <sup>C</sup> (k=2)
0	CW	X	0.0	0.0	1.0	0.00	151.1	$\pm 3.5\%$
		Y	0.0	0.0	1.0		153.4	
		Z	0.0	0.0	1.0		149.6	

Note: For details on UID parameters see Appendix.

### Sensor Model Parameters

	C1 fF	C2 fF	$\alpha$ $\text{V}^{-1}$	T1 $\text{ms}\cdot\text{V}^{-2}$	T2 $\text{ms}\cdot\text{V}^{-1}$	T3 ms	T4 $\text{V}^{-2}$	T5 $\text{V}^{-1}$	T6
X	35.70	266.3	35.57	18.74	0.500	5.000	0.445	0.515	1.000
Y	23.67	174.6	34.99	6.322	0.441	5.000	1.481	0.043	1.003
Z	41.62	317.3	36.81	8.754	0.711	5.047	0.519	0.469	1.008

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of Norm X,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside T5L (see Pages 5 and 6).

<sup>B</sup> Numerical linearization parameters; uncertainty not required.

<sup>C</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4- SN:3863

April 25, 2018

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3863

### Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth (mm) <sup>G</sup>	Unc (k=2)
150	52.3	0.76	12.22	12.22	12.22	0.00	1.00	± 13.3 %
450	43.5	0.87	10.92	10.92	10.92	0.14	1.20	± 13.3 %
750	41.9	0.89	10.20	10.20	10.20	0.61	0.80	± 12.0 %
835	41.5	0.90	9.95	9.95	9.95	0.50	0.80	± 12.0 %
900	41.5	0.97	9.67	9.67	9.67	0.32	1.07	± 12.0 %
1450	40.5	1.20	8.78	8.78	8.78	0.34	0.80	± 12.0 %
1750	40.1	1.37	8.45	8.45	8.45	0.42	0.80	± 12.0 %
1900	40.0	1.40	8.19	8.19	8.19	0.36	0.80	± 12.0 %
2300	39.5	1.67	7.77	7.77	7.77	0.34	0.86	± 12.0 %
2450	39.2	1.80	7.62	7.62	7.62	0.36	0.85	± 12.0 %
2800	39.0	1.96	7.19	7.19	7.19	0.36	0.93	± 12.0 %
5250	35.9	4.71	5.04	5.04	5.04	0.40	1.80	± 13.1 %
5600	35.5	5.07	4.68	4.68	4.68	0.40	1.80	± 13.1 %
5750	35.4	5.22	5.08	5.08	5.08	0.40	1.80	± 13.1 %

<sup>C</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:3863

April 25, 2018

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3863

### Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth (mm)	Unc (k=2)
150	61.9	0.80	11.86	11.86	11.86	0.00	1.00	± 13.3 %
450	56.7	0.94	10.78	10.78	10.78	0.08	1.20	± 13.3 %
750	55.5	0.96	10.02	10.02	10.02	0.37	0.89	± 12.0 %
835	55.2	0.97	9.66	9.66	9.66	0.42	0.91	± 12.0 %
1750	53.4	1.49	8.18	8.18	8.18	0.40	0.80	± 12.0 %
1900	53.3	1.52	7.84	7.84	7.84	0.34	0.80	± 12.0 %
2300	52.9	1.81	7.68	7.68	7.68	0.29	0.90	± 12.0 %
2450	52.7	1.95	7.48	7.48	7.48	0.27	0.97	± 12.0 %
2600	52.5	2.16	7.27	7.27	7.27	0.17	1.05	± 12.0 %
5250	48.9	5.36	4.41	4.41	4.41	0.50	1.90	± 13.1 %
5600	48.5	5.77	3.88	3.88	3.88	0.50	1.90	± 13.1 %
5750	48.3	5.94	4.21	4.21	4.21	0.50	1.90	± 13.1 %

<sup>C</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.


<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.



EX3DV4-- SN:3863

April 25, 2018

### Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

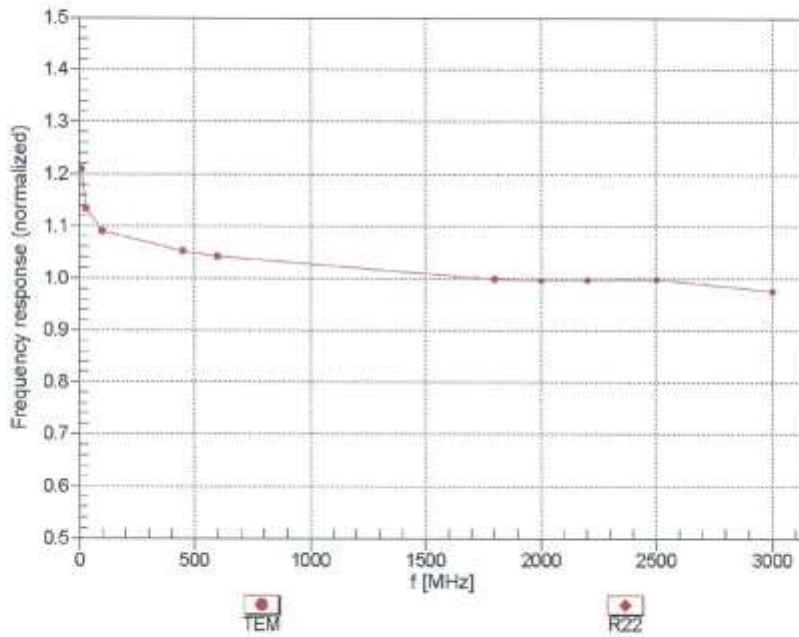

Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  (k=2)



EX3DV4- SN:3863

April 25, 2018

**Receiving Pattern ( $\phi$ ),  $\theta = 0^\circ$**

f=600 MHz,TEM

f=1800 MHz,R22

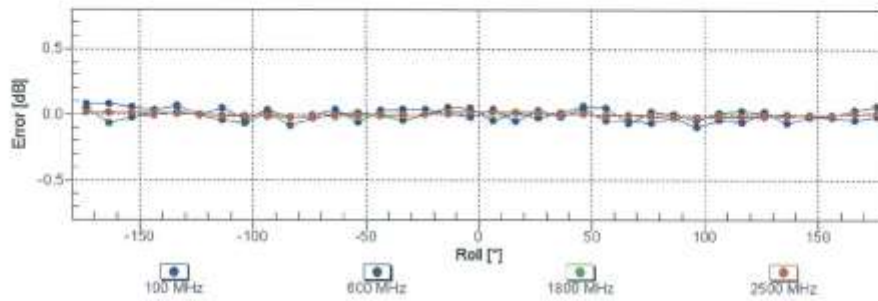
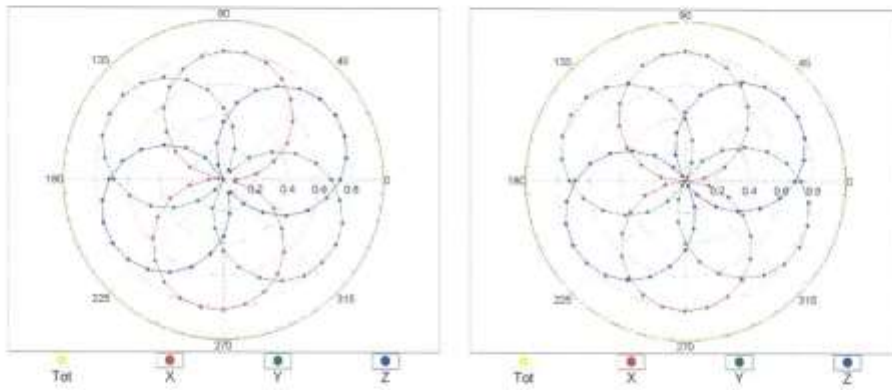


Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  (k=2)

EX3DV4- SN:3863

April 25, 2018

**Dynamic Range  $f(SAR_{head})$**   
(TEM cell ,  $f_{eval}=1900$  MHz)

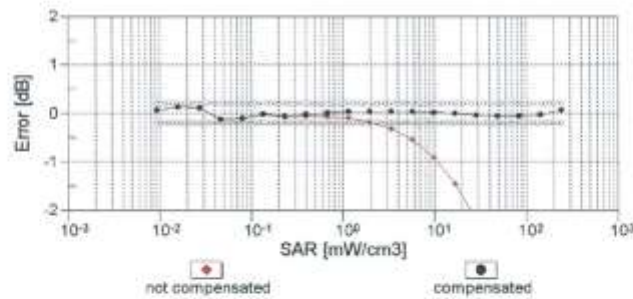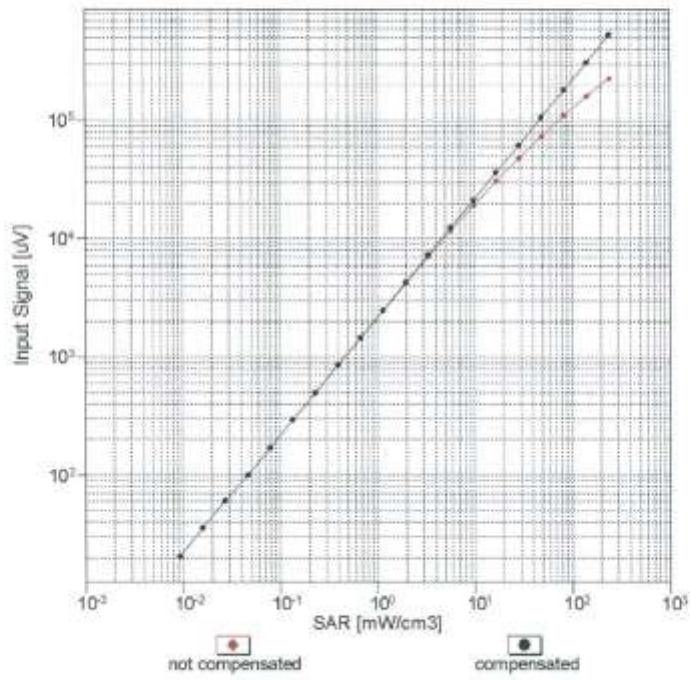


Uncertainty of Linearity Assessment:  $\pm 0.6\%$  (k=2)



EX3DV4- SN:3863



April 25, 2018

### Conversion Factor Assessment

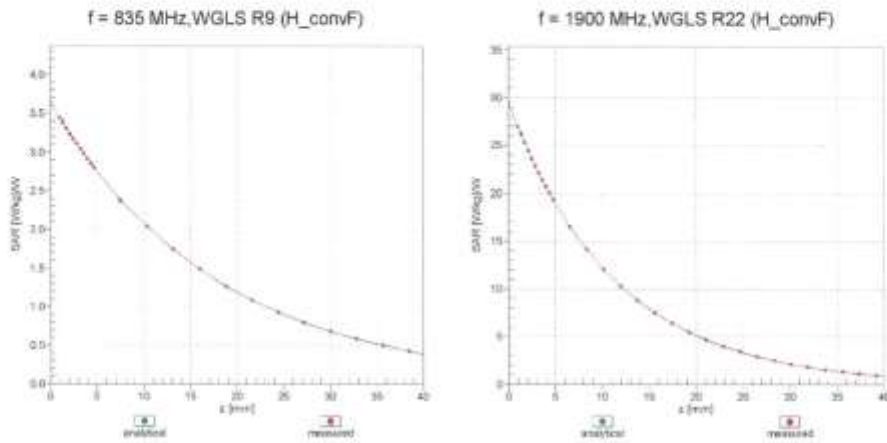

### Deviation from Isotropy in Liquid

Error ( $\phi$ ,  $\theta$ ), f = 900 MHz

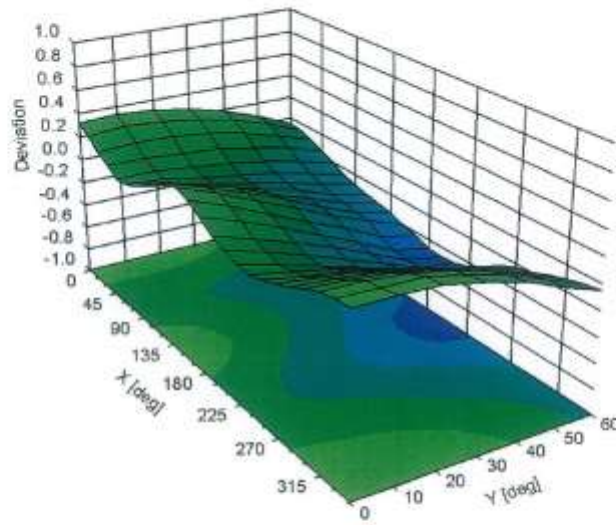

EX3DV4- SN:3863

April 25, 2018

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3863

### Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	106.5
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

EX3DV4- SN:3863

April 25, 2018

**Appendix: Modulation Calibration Parameters**

UID	Communication System Name		A dB	B dB $\mu$ V	C	D dB	VR mV	Max Unc <sup>E</sup> (k=2)
0	CW	X	0.00	0.00	1.00	0.00	151.1	$\pm 3.5\%$
		Y	0.00	0.00	1.00		153.4	
		Z	0.00	0.00	1.00		149.6	
10010- CAA	SAR Validation (Square, 100ms, 10ms)	X	11.00	70.00	30.00	10.00	20.0	$\pm 9.6\%$
		Y	1.74	62.86	8.09		20.0	
		Z	2.07	64.28	9.36		20.0	
10011- CAB	UMTS-FDD (WCDMA)	X	0.92	66.96	14.69	0.00	150.0	$\pm 9.6\%$
		Y	1.23	73.72	17.72		150.0	
		Z	0.82	64.81	13.15		150.0	
10012- CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps)	X	1.13	63.96	15.00	0.41	150.0	$\pm 9.6\%$
		Y	1.12	65.21	15.97		150.0	
		Z	1.04	62.64	14.13		150.0	
10013- CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps)	X	4.66	66.70	16.87	1.46	150.0	$\pm 9.6\%$
		Y	4.41	67.26	17.07		150.0	
		Z	4.70	66.40	16.80		150.0	
10021- DAC	GSM-FDD (TDMA, GMSK)	X	9.09	79.88	16.40	9.39	50.0	$\pm 9.6\%$
		Y	45.23	97.58	21.17		50.0	
		Z	100.00	110.54	25.67		50.0	
10023- DAC	GPRS-FDD (TDMA, GMSK, TN 0)	X	6.78	76.49	15.24	9.57	50.0	$\pm 9.6\%$
		Y	9.44	80.59	16.39		50.0	
		Z	67.36	105.58	24.50		50.0	
10024- DAC	GPRS-FDD (TDMA, GMSK, TN 0-1)	X	11.10	81.86	15.87	6.56	60.0	$\pm 9.6\%$
		Y	100.00	103.67	20.95		60.0	
		Z	100.00	108.28	23.45		60.0	
10025- DAC	EDGE-FDD (TDMA, 8PSK, TN 0)	X	3.31	63.37	21.37	12.57	50.0	$\pm 9.6\%$
		Y	4.23	71.81	26.71		50.0	
		Z	3.77	66.74	23.69		50.0	
10026- DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1)	X	9.84	92.28	31.76	9.56	60.0	$\pm 9.6\%$
		Y	5.96	83.99	29.74		60.0	
		Z	7.19	86.26	30.24		60.0	
10027- DAC	GPRS-FDD (TDMA, GMSK, TN 0-1-2)	X	100.00	101.03	19.83	4.80	80.0	$\pm 9.6\%$
		Y	100.00	103.59	20.13		80.0	
		Z	100.00	106.91	22.02		80.0	
10028- DAC	GPRS-FDD (TDMA, GMSK, TN 0-1-2-3)	X	100.00	100.43	19.05	3.55	100.0	$\pm 9.6\%$
		Y	100.00	104.67	19.92		100.0	
		Z	100.00	105.33	20.65		100.0	
10029- DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1-2)	X	6.41	82.79	27.10	7.80	80.0	$\pm 9.6\%$
		Y	4.05	75.66	25.13		80.0	
		Z	4.75	77.36	25.50		80.0	
10030- CAA	IEEE 802.15.1 Bluetooth (GFSK, DH1)	X	5.26	74.89	13.09	5.30	70.0	$\pm 9.6\%$
		Y	100.00	100.23	18.93		70.0	
		Z	100.00	105.72	21.80		70.0	
10031- CAA	IEEE 802.15.1 Bluetooth (GFSK, DH3)	X	4.88	76.31	11.58	1.68	100.0	$\pm 9.6\%$
		Y	0.28	61.23	5.16		100.0	
		Z	0.39	62.06	6.02		100.0	

EX3DV4- SN:3863

April 25, 2018

10032-CAA	IEEE 802.15.1 Bluetooth (GFSK, DH5)	X	99.99	93.80	14.65	1.17	100.0	± 9.6 %
		Y	0.14	60.00	3.64		100.0	
		Z	0.18	60.00	3.83		100.0	
10033-CAA	IEEE 802.15.1 Bluetooth (PI/4-DQPSK, DH1)	X	6.63	80.89	18.62	5.30	70.0	± 9.6 %
		Y	3.59	74.26	15.11		70.0	
		Z	6.50	84.64	21.35		70.0	
10034-CAA	IEEE 802.15.1 Bluetooth (PI/4-DQPSK, DH3)	X	2.35	71.30	13.76	1.88	100.0	± 9.6 %
		Y	0.91	63.27	8.36		100.0	
		Z	1.79	70.18	14.28		100.0	
10035-CAA	IEEE 802.15.1 Bluetooth (PI/4-DQPSK, DH5)	X	1.70	69.13	12.72	1.17	100.0	± 9.6 %
		Y	0.67	61.91	7.34		100.0	
		Z	1.29	67.25	12.66		100.0	
10036-CAA	IEEE 802.15.1 Bluetooth (8-DPSK, DH1)	X	8.29	83.97	19.70	5.30	70.0	± 9.6 %
		Y	4.28	76.54	16.01		70.0	
		Z	8.57	88.94	22.82		70.0	
10037-CAA	IEEE 802.15.1 Bluetooth (8-DPSK, DH3)	X	2.17	70.51	13.42	1.88	100.0	± 9.6 %
		Y	0.85	62.76	8.13		100.0	
		Z	1.68	69.54	13.98		100.0	
10038-CAA	IEEE 802.15.1 Bluetooth (8-DPSK, DH5)	X	1.73	69.53	13.00	1.17	100.0	± 9.6 %
		Y	0.68	62.14	7.59		100.0	
		Z	1.29	67.51	12.89		100.0	
10039-CAB	CDMA2000 (1xRTT, RC1)	X	1.20	68.00	12.32	0.00	150.0	± 9.6 %
		Y	0.40	60.00	5.73		150.0	
		Z	1.08	65.78	11.49		150.0	
10042-CAB	IS-54 / IS-136 FDD (TDMA/FDM, PI/4-DQPSK, Halfrate)	X	3.96	71.13	12.28	7.78	50.0	± 9.6 %
		Y	4.33	73.40	12.83		50.0	
		Z	20.63	89.92	18.82		50.0	
10044-CAA	IS-91/EIA/TIA-553 FDD (FDMA, FM)	X	0.03	118.44	11.49	0.00	150.0	± 9.6 %
		Y	0.03	123.41	0.47		150.0	
		Z	0.10	121.86	6.25		150.0	
10048-CAA	DECT (TDD, TDMA/FDM, GFSK, Full Slot, 24)	X	4.53	70.04	14.07	13.80	25.0	± 9.6 %
		Y	4.85	69.08	13.50		25.0	
		Z	9.31	78.44	18.09		25.0	
10049-CAA	DECT (TDD, TDMA/FDM, GFSK, Double Slot, 12)	X	5.00	72.36	13.87	10.79	40.0	± 9.6 %
		Y	4.95	72.19	13.60		40.0	
		Z	10.49	82.35	18.31		40.0	
10056-CAA	UMTS-TDD (TD-SCDMA, 1.28 Mcps)	X	9.88	83.19	19.98	9.03	50.0	± 9.6 %
		Y	7.80	79.96	18.01		50.0	
		Z	13.55	90.17	23.36		50.0	
10058-DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1-2-3)	X	4.96	77.96	24.46	6.55	100.0	± 9.6 %
		Y	3.33	72.13	22.83		100.0	
		Z	3.78	73.24	22.95		100.0	
10059-CAB	IEEE 802.11b WIFI 2.4 GHz (DSSS, 2 Mbps)	X	1.19	65.20	15.58	0.61	110.0	± 9.6 %
		Y	1.14	66.22	16.48		110.0	
		Z	1.06	63.47	14.60		110.0	
10060-CAB	IEEE 802.11b WIFI 2.4 GHz (DSSS, 5.5 Mbps)	X	18.28	106.21	26.40	1.30	110.0	± 9.6 %
		Y	100.00	142.43	36.78		110.0	
		Z	2.88	84.70	20.89		110.0	



EX3DV4- SN:3863

April 25, 2018

10061-CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 11 Mbps)	X	3.45	61.46	21.39	2.04	110.0	± 9.6 %
		Y	2.51	81.17	22.36		110.0	
		Z	1.97	74.69	19.49		110.0	
10062-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps)	X	4.45	66.68	16.34	0.49	100.0	± 9.6 %
		Y	4.22	67.27	16.54		100.0	
		Z	4.49	66.34	16.21		100.0	
10063-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps)	X	4.47	66.76	16.42	0.72	100.0	± 9.6 %
		Y	4.23	67.37	16.64		100.0	
		Z	4.51	66.43	16.31		100.0	
10064-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 12 Mbps)	X	4.71	66.95	16.61	0.86	100.0	± 9.6 %
		Y	4.42	67.49	16.78		100.0	
		Z	4.77	66.69	16.54		100.0	
10065-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 18 Mbps)	X	4.59	66.82	16.68	1.21	100.0	± 9.6 %
		Y	4.30	67.26	16.81		100.0	
		Z	4.65	66.56	16.62		100.0	
10066-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 24 Mbps)	X	4.60	66.82	16.82	1.46	100.0	± 9.6 %
		Y	4.29	67.17	16.89		100.0	
		Z	4.66	66.58	16.78		100.0	
10067-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 36 Mbps)	X	4.89	67.08	17.27	2.04	100.0	± 9.6 %
		Y	4.52	67.29	17.26		100.0	
		Z	4.96	66.83	17.27		100.0	
10068-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 48 Mbps)	X	4.93	67.01	17.42	2.55	100.0	± 9.6 %
		Y	4.61	67.41	17.54		100.0	
		Z	5.00	66.81	17.45		100.0	
10069-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 54 Mbps)	X	4.99	67.04	17.61	2.67	100.0	± 9.6 %
		Y	4.63	67.31	17.64		100.0	
		Z	5.07	66.84	17.65		100.0	
10071-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 9 Mbps)	X	4.76	66.78	17.15	1.99	100.0	± 9.6 %
		Y	4.51	67.31	17.34		100.0	
		Z	4.79	66.48	17.11		100.0	
10072-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 12 Mbps)	X	4.72	67.04	17.33	2.30	100.0	± 9.6 %
		Y	4.43	67.41	17.46		100.0	
		Z	4.76	66.75	17.30		100.0	
10073-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 18 Mbps)	X	4.80	67.25	17.65	2.83	100.0	± 9.6 %
		Y	4.51	67.66	17.82		100.0	
		Z	4.82	66.92	17.62		100.0	
10074-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 24 Mbps)	X	4.81	67.22	17.80	3.30	100.0	± 9.6 %
		Y	4.56	67.77	18.04		100.0	
		Z	4.81	66.83	17.77		100.0	
10075-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 36 Mbps)	X	4.84	67.27	18.05	3.82	90.0	± 9.6 %
		Y	4.60	67.82	18.29		90.0	
		Z	4.85	66.90	18.05		90.0	
10076-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 48 Mbps)	X	4.88	67.16	18.22	4.15	90.0	± 9.6 %
		Y	4.64	67.67	18.44		90.0	
		Z	4.88	66.75	18.20		90.0	
10077-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 54 Mbps)	X	4.92	67.26	18.33	4.30	90.0	± 9.6 %
		Y	4.68	67.80	18.56		90.0	
		Z	4.90	66.83	18.30		90.0	



EX3DV4- SN:3863

April 25, 2018

10081-CAB	CDMA2000 (1xRTT, RC3)	X	0.57	63.24	9.45	0.00	150.0	± 9.6 %
		Y	0.29	60.00	5.08		150.0	
		Z	0.55	61.98	8.86		150.0	
10082-CAB	IS-54 / IS-136 FDD (TDMA/FDM, PI/4-DQPSK, Fullrate)	X	0.85	60.00	4.39	4.77	80.0	± 9.6 %
		Y	0.61	60.00	3.29		80.0	
		Z	0.85	61.10	4.43		80.0	
10090-DAC	GPRS-FDD (TDMA, GMSK, TN 0-4)	X	11.01	81.80	15.86	6.56	80.0	± 9.6 %
		Y	100.00	103.71	20.98		80.0	
		Z	100.00	108.37	23.51		80.0	
10097-CAB	UMTS-FDD (HSDPA)	X	1.75	68.14	15.41	0.00	150.0	± 9.6 %
		Y	2.15	73.36	17.10		150.0	
		Z	1.61	66.21	14.35		150.0	
10098-CAB	UMTS-FDD (HSUPA, Subtest 2)	X	1.71	68.07	15.37	0.00	150.0	± 9.6 %
		Y	2.11	73.35	17.12		150.0	
		Z	1.57	66.13	14.31		150.0	
10099-DAC	EDGE-FDD (TDMA, 8PSK, TN 0-4)	X	9.91	92.40	31.80	9.56	60.0	± 9.6 %
		Y	6.00	84.12	29.79		60.0	
		Z	7.24	86.38	30.27		60.0	
10100-CAD	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	X	2.91	69.93	16.52	0.00	150.0	± 9.6 %
		Y	2.94	71.66	17.64		150.0	
		Z	2.79	68.74	15.72		150.0	
10101-CAD	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM)	X	3.05	67.27	15.75	0.00	150.0	± 9.6 %
		Y	2.96	68.14	16.32		150.0	
		Z	3.02	66.65	15.31		150.0	
10102-CAD	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM)	X	3.16	67.31	15.88	0.00	150.0	± 9.6 %
		Y	3.06	68.19	16.41		150.0	
		Z	3.13	66.69	15.44		150.0	
10103-CAD	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	X	6.17	75.27	19.83	3.98	65.0	± 9.6 %
		Y	5.02	74.56	20.07		65.0	
		Z	5.58	74.23	19.78		65.0	
10104-CAD	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM)	X	6.38	74.05	20.09	3.98	65.0	± 9.6 %
		Y	4.96	71.85	19.45		65.0	
		Z	5.51	71.89	19.54		65.0	
10105-CAD	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM)	X	5.67	71.78	19.42	3.98	65.0	± 9.6 %
		Y	4.68	70.50	19.12		65.0	
		Z	5.40	71.34	19.60		65.0	
10108-CAE	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X	2.50	69.27	16.35	0.00	150.0	± 9.6 %
		Y	2.53	71.57	17.63		150.0	
		Z	2.41	68.02	15.51		150.0	
10109-CAE	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM)	X	2.70	67.24	15.61	0.00	150.0	± 9.6 %
		Y	2.63	68.68	16.24		150.0	
		Z	2.66	66.45	15.11		150.0	
10110-CAE	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, QPSK)	X	1.99	68.44	15.79	0.00	150.0	± 9.6 %
		Y	2.06	71.55	17.06		150.0	
		Z	1.92	67.04	14.92		150.0	
10111-CAE	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM)	X	2.45	68.57	15.90	0.00	150.0	± 9.6 %
		Y	2.57	71.53	16.67		150.0	
		Z	2.35	67.12	15.16		150.0	

EX3DV4- SN:3863

April 25, 2018

10112-CAE	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM)	X	2.83	67.33	15.71	0.00	150.0	± 9.6 %
		Y	2.76	68.82	16.33		150.0	
		Z	2.79	66.53	15.22		150.0	
10113-CAE	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, 64-QAM)	X	2.60	68.79	16.07	0.00	150.0	± 9.6 %
		Y	2.70	71.55	16.71		150.0	
		Z	2.50	67.36	15.35		150.0	
10114-CAC	IEEE 802.11n (HT Greenfield, 13.5 Mbps, BPSK)	X	4.91	67.08	16.35	0.00	150.0	± 9.6 %
		Y	4.70	67.41	16.61		150.0	
		Z	4.96	66.85	16.19		150.0	
10115-CAC	IEEE 802.11n (HT Greenfield, 81 Mbps, 16-QAM)	X	5.16	67.16	16.39	0.00	150.0	± 9.6 %
		Y	4.93	67.53	16.63		150.0	
		Z	5.21	66.93	16.24		150.0	
10116-CAC	IEEE 802.11n (HT Greenfield, 135 Mbps, 64-QAM)	X	5.00	67.28	16.38	0.00	150.0	± 9.6 %
		Y	4.76	67.61	16.63		150.0	
		Z	5.04	67.03	16.21		150.0	
10117-CAC	IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)	X	4.91	67.04	16.35	0.00	150.0	± 9.6 %
		Y	4.68	67.32	16.58		150.0	
		Z	4.93	66.73	16.15		150.0	
10118-CAC	IEEE 802.11n (HT Mixed, 81 Mbps, 16-QAM)	X	5.23	67.34	16.49	0.00	150.0	± 9.6 %
		Y	4.94	67.52	16.63		150.0	
		Z	5.30	67.14	16.35		150.0	
10119-CAC	IEEE 802.11n (HT Mixed, 135 Mbps, 64-QAM)	X	4.99	67.27	16.39	0.00	150.0	± 9.6 %
		Y	4.77	67.61	16.64		150.0	
		Z	5.03	67.00	16.20		150.0	
10140-CAD	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	X	3.18	67.31	15.78	0.00	150.0	± 9.6 %
		Y	3.06	68.22	16.30		150.0	
		Z	3.16	66.70	15.36		150.0	
10141-CAD	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	X	3.31	67.51	16.00	0.00	150.0	± 9.6 %
		Y	3.20	68.53	16.55		150.0	
		Z	3.29	66.86	15.57		150.0	
10142-CAD	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, QPSK)	X	1.75	68.36	15.09	0.00	150.0	± 9.6 %
		Y	1.78	71.06	15.42		150.0	
		Z	1.66	66.67	14.20		150.0	
10143-CAD	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM)	X	2.25	68.96	15.03	0.00	150.0	± 9.6 %
		Y	1.94	68.81	13.51		150.0	
		Z	2.12	67.21	14.32		150.0	
10144-CAD	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, 64-QAM)	X	1.90	65.74	12.89	0.00	150.0	± 9.6 %
		Y	1.39	63.90	10.43		150.0	
		Z	1.92	65.05	12.71		150.0	
10145-CAE	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK)	X	0.74	61.13	7.80	0.00	150.0	± 9.6 %
		Y	0.44	60.00	4.49		150.0	
		Z	0.83	61.47	8.46		150.0	
10146-CAE	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	X	0.98	60.10	6.33	0.00	150.0	± 9.6 %
		Y	0.63	60.00	3.77		150.0	
		Z	1.32	62.30	8.56		150.0	
10147-CAE	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	X	1.02	60.37	6.56	0.00	150.0	± 9.6 %
		Y	0.63	60.00	3.82		150.0	
		Z	1.41	62.99	9.03		150.0	

EX3DV4- SN:3863

April 25, 2018

10149-CAD	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM)	X	2.71	67.32	15.67	0.00	150.0	± 9.6 %
		Y	2.64	68.79	16.31		150.0	
		Z	2.67	66.51	15.16		150.0	
10150-CAD	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, 64-QAM)	X	2.84	67.40	15.76	0.00	150.0	± 9.6 %
		Y	2.77	68.91	16.39		150.0	
		Z	2.80	66.59	15.26		150.0	
10151-CAD	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	X	7.05	79.01	21.24	3.98	65.0	± 9.6 %
		Y	5.45	78.07	21.33		65.0	
		Z	5.61	76.01	20.56		65.0	
10152-CAD	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM)	X	5.87	73.88	19.52	3.98	65.0	± 9.6 %
		Y	4.45	71.66	18.62		65.0	
		Z	5.02	71.71	19.09		65.0	
10153-CAD	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 64-QAM)	X	6.39	75.31	20.54	3.98	65.0	± 9.6 %
		Y	4.89	73.20	19.71		65.0	
		Z	5.39	72.79	19.96		65.0	
10154-CAE	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	X	2.04	68.90	16.07	0.00	150.0	± 9.6 %
		Y	2.13	72.17	17.39		150.0	
		Z	1.95	67.39	15.15		150.0	
10155-CAE	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM)	X	2.46	68.61	15.94	0.00	150.0	± 9.6 %
		Y	2.59	71.66	16.74		150.0	
		Z	2.35	67.14	15.18		150.0	
10156-CAE	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, QPSK)	X	1.56	68.06	14.48	0.00	150.0	± 9.6 %
		Y	1.39	68.73	13.43		150.0	
		Z	1.48	66.30	13.62		150.0	
10157-CAE	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM)	X	1.70	65.86	12.52	0.00	150.0	± 9.6 %
		Y	1.07	62.55	8.97		150.0	
		Z	1.71	65.08	12.35		150.0	
10158-CAE	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, 64-QAM)	X	2.62	68.90	16.14	0.00	150.0	± 9.6 %
		Y	2.73	71.76	16.82		150.0	
		Z	2.51	67.43	15.40		150.0	
10159-CAE	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, 64-QAM)	X	1.78	66.23	12.74	0.00	150.0	± 9.6 %
		Y	1.10	62.56	8.97		150.0	
		Z	1.78	65.42	12.58		150.0	
10160-CAD	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, QPSK)	X	2.55	68.64	16.16	0.00	150.0	± 9.6 %
		Y	2.51	70.60	17.09		150.0	
		Z	2.49	67.55	15.47		150.0	
10161-CAD	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM)	X	2.73	67.38	15.64	0.00	150.0	± 9.6 %
		Y	2.66	68.98	16.16		150.0	
		Z	2.69	66.51	15.14		150.0	
10162-CAD	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, 64-QAM)	X	2.84	67.62	15.79	0.00	150.0	± 9.6 %
		Y	2.77	69.32	16.34		150.0	
		Z	2.80	66.72	15.29		150.0	
10166-CAE	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK)	X	3.17	68.43	18.19	3.01	150.0	± 9.6 %
		Y	2.74	68.67	18.97		150.0	
		Z	3.37	69.16	18.82		150.0	
10167-CAE	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM)	X	3.80	70.92	18.39	3.01	150.0	± 9.6 %
		Y	3.27	72.46	19.76		150.0	
		Z	4.11	71.94	19.16		150.0	



EX3DV4- SN:3863

April 25, 2018

10168-CAE	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, 64-QAM)	X	4.33	73.72	20.04	3.01	150.0	± 9.6 %
		Y	3.93	76.52	22.01		150.0	
		Z	4.68	74.75	20.78		150.0	
10169-CAD	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	X	2.69	67.32	17.58	3.01	150.0	± 9.6 %
		Y	2.43	68.05	18.61		150.0	
		Z	2.79	68.16	18.34		150.0	
10170-CAD	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM)	X	3.59	72.54	19.67	3.01	150.0	± 9.6 %
		Y	3.51	76.45	22.16		150.0	
		Z	3.83	74.10	20.71		150.0	
10171-AAD	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, 64-QAM)	X	2.93	68.40	16.78	3.01	150.0	± 9.6 %
		Y	2.63	70.44	18.33		150.0	
		Z	3.08	69.59	17.69		150.0	
10172-CAD	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	X	4.62	78.65	22.60	6.02	65.0	± 9.6 %
		Y	2.94	76.24	23.12		65.0	
		Z	6.04	85.62	26.43		65.0	
10173-CAD	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM)	X	7.73	84.08	22.65	6.02	65.0	± 9.6 %
		Y	6.63	89.25	25.64		65.0	
		Z	9.82	91.06	26.34		65.0	
10174-CAD	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 64-QAM)	X	3.91	73.33	18.34	6.02	65.0	± 9.6 %
		Y	5.35	84.73	23.41		65.0	
		Z	6.55	83.31	23.20		65.0	
10175-CAE	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	X	2.66	67.02	17.32	3.01	150.0	± 9.6 %
		Y	2.39	67.72	18.33		150.0	
		Z	2.76	67.84	18.07		150.0	
10176-CAE	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM)	X	3.60	72.56	19.68	3.01	150.0	± 9.6 %
		Y	3.51	76.48	22.17		150.0	
		Z	3.84	74.12	20.72		150.0	
10177-CAG	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, QPSK)	X	2.67	67.15	17.41	3.01	150.0	± 9.6 %
		Y	2.41	67.82	18.40		150.0	
		Z	2.78	67.99	18.17		150.0	
10178-CAE	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM)	X	3.57	72.39	19.58	3.01	150.0	± 9.6 %
		Y	3.49	76.32	22.09		150.0	
		Z	3.80	73.91	20.61		150.0	
10179-CAE	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, 64-QAM)	X	3.21	70.22	18.03	3.01	150.0	± 9.6 %
		Y	3.01	73.21	20.07		150.0	
		Z	3.41	71.63	19.02		150.0	
10180-CAE	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, 64-QAM)	X	2.92	68.36	16.75	3.01	150.0	± 9.6 %
		Y	2.63	70.42	18.31		150.0	
		Z	3.08	69.53	17.64		150.0	
10181-CAD	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	X	2.67	67.13	17.40	3.01	150.0	± 9.6 %
		Y	2.40	67.81	18.39		150.0	
		Z	2.78	67.97	18.16		150.0	
10182-CAD	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM)	X	3.57	72.37	19.57	3.01	150.0	± 9.6 %
		Y	3.48	76.29	22.07		150.0	
		Z	3.79	73.86	20.60		150.0	
10183-AAC	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, 64-QAM)	X	2.92	68.34	16.74	3.01	150.0	± 9.6 %
		Y	2.63	70.39	18.30		150.0	
		Z	3.07	69.51	17.63		150.0	

EX3DV4- SN:3863

April 25, 2018

10184-CAD	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, QPSK)	X	2.68	67.17	17.42	3.01	150.0	± 9.6 %
		Y	2.41	67.84	18.41		150.0	
		Z	2.79	68.01	18.18		150.0	
10185-CAD	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM)	X	3.58	72.44	19.61	3.01	150.0	± 9.6 %
		Y	3.50	76.39	22.12		150.0	
		Z	3.81	73.96	20.64		150.0	
10186-AAD	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, 64-QAM)	X	2.93	68.39	16.77	3.01	150.0	± 9.6 %
		Y	2.64	70.46	18.34		150.0	
		Z	3.09	69.57	17.67		150.0	
10187-CAE	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK)	X	2.69	67.25	17.51	3.01	150.0	± 9.6 %
		Y	2.43	67.98	18.53		150.0	
		Z	2.80	68.08	18.26		150.0	
10188-CAE	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM)	X	3.69	73.08	19.99	3.01	150.0	± 9.6 %
		Y	3.64	77.24	22.59		150.0	
		Z	3.94	74.67	21.05		150.0	
10189-AAE	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, 64-QAM)	X	2.99	68.75	17.02	3.01	150.0	± 9.6 %
		Y	2.71	70.95	18.66		150.0	
		Z	3.15	69.99	17.95		150.0	
10193-CAC	IEEE 802.11n (HT Greenfield, 6.5 Mbps, BPSK)	X	4.32	66.74	16.06	0.00	150.0	± 9.6 %
		Y	4.14	67.59	16.37		150.0	
		Z	4.34	66.29	15.83		150.0	
10194-CAC	IEEE 802.11n (HT Greenfield, 39 Mbps, 16-QAM)	X	4.46	66.98	16.19	0.00	150.0	± 9.6 %
		Y	4.24	67.67	16.48		150.0	
		Z	4.50	66.57	15.96		150.0	
10195-CAC	IEEE 802.11n (HT Greenfield, 65 Mbps, 64-QAM)	X	4.50	66.99	16.21	0.00	150.0	± 9.6 %
		Y	4.25	67.61	16.46		150.0	
		Z	4.54	66.61	15.99		150.0	
10196-CAC	IEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)	X	4.31	66.74	16.05	0.00	150.0	± 9.6 %
		Y	4.11	67.51	16.32		150.0	
		Z	4.34	66.32	15.83		150.0	
10197-CAC	IEEE 802.11n (HT Mixed, 39 Mbps, 16-QAM)	X	4.47	66.98	16.20	0.00	150.0	± 9.6 %
		Y	4.24	67.66	16.48		150.0	
		Z	4.51	66.59	15.97		150.0	
10198-CAC	IEEE 802.11n (HT Mixed, 65 Mbps, 64-QAM)	X	4.49	66.99	16.21	0.00	150.0	± 9.6 %
		Y	4.24	67.60	16.45		150.0	
		Z	4.53	66.62	15.99		150.0	
10219-CAC	IEEE 802.11n (HT Mixed, 7.2 Mbps, BPSK)	X	4.26	66.77	16.02	0.00	150.0	± 9.6 %
		Y	4.07	67.62	16.34		150.0	
		Z	4.28	66.34	15.79		150.0	
10220-CAC	IEEE 802.11n (HT Mixed, 43.3 Mbps, 16-QAM)	X	4.47	66.94	16.18	0.00	150.0	± 9.6 %
		Y	4.23	67.62	16.46		150.0	
		Z	4.50	66.55	15.96		150.0	
10221-CAC	IEEE 802.11n (HT Mixed, 72.2 Mbps, 64-QAM)	X	4.51	66.94	16.20	0.00	150.0	± 9.6 %
		Y	4.26	67.58	16.45		150.0	
		Z	4.55	66.56	15.98		150.0	
10222-CAC	IEEE 802.11n (HT Mixed, 15 Mbps, BPSK)	X	4.88	67.02	16.33	0.00	150.0	± 9.6 %
		Y	4.67	67.32	16.57		150.0	
		Z	4.90	66.72	16.13		150.0	



EX3DV4- SN:3863

April 25, 2018

10223-CAC	IEEE 802.11n (HT Mixed, 90 Mbps, 16-QAM)	X	5.15	67.21	16.44	0.00	150.0	± 9.6 %
		Y	4.85	67.37	16.57		150.0	
		Z	5.20	66.97	16.28		150.0	
10224-CAC	IEEE 802.11n (HT Mixed, 150 Mbps, 64-QAM)	X	4.92	67.13	16.32	0.00	150.0	± 9.6 %
		Y	4.70	67.49	16.58		150.0	
		Z	4.94	66.83	16.11		150.0	
10225-CAB	UMTS-FDD (HSPA+)	X	2.60	66.16	14.83	0.00	150.0	± 9.6 %
		Y	2.41	67.00	14.35		150.0	
		Z	2.59	65.42	14.54		150.0	
10226-CAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM)	X	8.23	85.19	23.12	6.02	65.0	± 9.6 %
		Y	7.42	91.37	26.44		65.0	
		Z	10.58	92.51	26.91		65.0	
10227-CAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 64-QAM)	X	7.55	82.84	21.72	6.02	65.0	± 9.6 %
		Y	6.51	87.87	24.49		65.0	
		Z	10.25	90.62	25.65		65.0	
10228-CAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK)	X	6.67	85.48	25.12	6.02	65.0	± 9.6 %
		Y	3.69	80.81	24.99		65.0	
		Z	6.44	87.27	27.13		65.0	
10229-CAB	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM)	X	7.78	84.18	22.69	6.02	65.0	± 9.6 %
		Y	6.69	89.39	25.70		65.0	
		Z	9.90	91.18	26.39		65.0	
10230-CAB	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 64-QAM)	X	7.14	81.92	21.34	6.02	65.0	± 9.6 %
		Y	5.85	86.04	23.80		65.0	
		Z	9.54	89.32	25.15		65.0	
10231-CAB	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, QPSK)	X	6.36	84.50	24.69	6.02	65.0	± 9.6 %
		Y	3.53	79.82	24.51		65.0	
		Z	6.16	86.30	26.70		65.0	
10232-CAD	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM)	X	7.77	84.16	22.68	6.02	65.0	± 9.6 %
		Y	6.68	89.37	25.69		65.0	
		Z	9.88	91.16	26.38		65.0	
10233-CAD	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 64-QAM)	X	7.13	81.90	21.33	6.02	65.0	± 9.6 %
		Y	5.83	85.99	23.79		65.0	
		Z	9.51	89.29	25.14		65.0	
10234-CAD	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK)	X	6.09	83.61	24.25	6.02	65.0	± 9.6 %
		Y	3.42	79.13	24.11		65.0	
		Z	5.93	85.47	26.28		65.0	
10235-CAD	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM)	X	7.78	84.19	22.69	6.02	65.0	± 9.6 %
		Y	6.68	89.41	25.71		65.0	
		Z	9.89	91.19	26.39		65.0	
10236-CAD	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 64-QAM)	X	7.18	81.98	21.35	6.02	65.0	± 9.6 %
		Y	5.91	86.16	23.84		65.0	
		Z	9.62	89.44	25.18		65.0	
10237-CAD	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	X	6.36	84.53	24.70	6.02	65.0	± 9.6 %
		Y	3.52	79.81	24.52		65.0	
		Z	6.16	86.34	26.72		65.0	
10238-CAD	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM)	X	7.75	84.14	22.67	6.02	65.0	± 9.6 %
		Y	6.66	89.35	25.68		65.0	
		Z	9.86	91.13	26.37		65.0	

EX3DV4- SN:3863

April 25, 2018

10239-CAD	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 64-QAM)	X	7.11	81.87	21.32	6.02	65.0	± 9.6 %
		Y	5.81	85.95	23.78		65.0	
		Z	9.48	89.25	25.13		65.0	
10240-CAD	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	X	6.34	84.51	24.69	6.02	65.0	± 9.6 %
		Y	3.52	79.81	24.52		65.0	
		Z	6.14	86.30	26.70		65.0	
10241-CAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM)	X	7.98	81.00	24.33	6.98	65.0	± 9.6 %
		Y	6.14	81.54	25.53		65.0	
		Z	7.26	79.71	24.64		65.0	
10242-CAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 64-QAM)	X	6.47	76.99	22.66	6.98	65.0	± 9.6 %
		Y	4.99	77.45	23.83		65.0	
		Z	6.91	78.72	24.15		65.0	
10243-CAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK)	X	5.40	74.34	22.44	6.98	65.0	± 9.6 %
		Y	4.21	73.63	23.07		65.0	
		Z	5.61	75.34	23.62		65.0	
10244-CAB	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM)	X	3.76	67.79	12.85	3.98	65.0	± 9.6 %
		Y	1.87	62.25	8.40		65.0	
		Z	4.41	71.62	16.01		65.0	
10245-CAB	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 64-QAM)	X	3.71	67.43	12.64	3.98	65.0	± 9.6 %
		Y	1.87	62.05	8.24		65.0	
		Z	4.30	70.99	15.67		65.0	
10246-CAB	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, QPSK)	X	4.05	72.21	15.44	3.98	65.0	± 9.6 %
		Y	1.80	64.42	10.44		65.0	
		Z	3.80	73.10	16.90		65.0	
10247-CAD	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM)	X	4.44	71.15	15.84	3.98	65.0	± 9.6 %
		Y	2.54	65.63	11.89		65.0	
		Z	4.00	70.77	16.63		65.0	
10248-CAD	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 64-QAM)	X	4.38	70.57	15.58	3.98	65.0	± 9.6 %
		Y	2.50	65.09	11.62		65.0	
		Z	4.00	70.27	16.39		65.0	
10249-CAD	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, QPSK)	X	6.22	78.94	19.39	3.98	65.0	± 9.6 %
		Y	3.43	72.93	16.18		65.0	
		Z	5.02	77.51	19.84		65.0	
10250-CAD	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM)	X	6.14	76.63	20.38	3.98	65.0	± 9.6 %
		Y	4.51	74.09	18.97		65.0	
		Z	5.00	73.95	19.97		65.0	
10251-CAD	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 64-QAM)	X	5.56	73.72	18.77	3.98	65.0	± 9.6 %
		Y	3.95	70.70	16.95		65.0	
		Z	4.76	71.87	18.65		65.0	
10252-CAD	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	X	7.45	81.83	21.98	3.98	65.0	± 9.6 %
		Y	5.54	80.55	21.60		65.0	
		Z	5.55	78.23	21.33		65.0	
10253-CAD	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM)	X	5.77	73.44	19.25	3.98	65.0	± 9.6 %
		Y	4.37	71.25	18.16		65.0	
		Z	4.94	71.30	18.85		65.0	
10254-CAD	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 64-QAM)	X	6.22	74.67	20.11	3.98	65.0	± 9.6 %
		Y	4.73	72.48	19.03		65.0	
		Z	5.27	72.27	19.61		65.0	

EX3DV4- SN:3863

April 25, 2018

10255-CAD	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, QPSK)	X	6.76	78.48	21.18	3.98	65.0	± 9.6 %
		Y	5.16	77.25	20.99		65.0	
		Z	5.37	75.38	20.49		65.0	
10256-CAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	X	2.78	64.16	9.93	3.98	65.0	± 9.6 %
		Y	1.36	60.00	5.83		65.0	
		Z	3.18	67.02	12.70		65.0	
10257-CAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	X	2.75	63.84	9.69	3.98	65.0	± 9.6 %
		Y	1.38	60.00	5.75		65.0	
		Z	3.11	66.43	12.31		65.0	
10258-CAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK)	X	2.69	66.45	11.77	3.98	65.0	± 9.6 %
		Y	1.25	60.72	7.00		65.0	
		Z	2.70	67.95	13.57		65.0	
10259-CAB	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM)	X	5.09	73.24	17.52	3.98	65.0	± 9.6 %
		Y	3.20	68.61	14.39		65.0	
		Z	4.40	72.05	17.89		65.0	
10260-CAB	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 64-QAM)	X	5.09	72.94	17.39	3.98	65.0	± 9.6 %
		Y	3.20	68.30	14.22		65.0	
		Z	4.44	71.81	17.78		65.0	
10261-CAB	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, QPSK)	X	6.43	79.43	20.17	3.98	65.0	± 9.6 %
		Y	4.14	75.58	18.12		65.0	
		Z	5.00	77.05	20.16		65.0	
10262-CAD	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM)	X	6.11	76.51	20.31	3.98	65.0	± 9.6 %
		Y	4.48	73.95	18.88		65.0	
		Z	4.98	73.88	19.92		65.0	
10263-CAD	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 64-QAM)	X	5.55	73.70	18.77	3.98	65.0	± 9.6 %
		Y	3.94	70.69	16.95		65.0	
		Z	4.76	71.84	18.64		65.0	
10264-CAD	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, QPSK)	X	7.33	81.55	21.85	3.98	65.0	± 9.6 %
		Y	5.45	80.22	21.44		65.0	
		Z	5.49	78.02	21.23		65.0	
10265-CAD	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM)	X	5.87	73.86	19.53	3.98	65.0	± 9.6 %
		Y	4.46	71.68	18.63		65.0	
		Z	5.02	71.71	19.09		65.0	
10266-CAD	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM)	X	6.39	75.29	20.53	3.98	65.0	± 9.6 %
		Y	4.89	73.18	19.70		65.0	
		Z	5.38	72.78	19.95		65.0	
10267-CAD	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X	7.04	78.96	21.22	3.98	65.0	± 9.6 %
		Y	5.43	77.99	21.30		65.0	
		Z	5.60	75.97	20.54		65.0	
10268-CAD	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	X	6.56	74.07	20.20	3.98	65.0	± 9.6 %
		Y	5.15	72.08	19.58		65.0	
		Z	5.68	71.86	19.63		65.0	
10269-CAD	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	X	6.55	73.70	20.08	3.98	65.0	± 9.6 %
		Y	5.19	71.84	19.47		65.0	
		Z	5.68	71.51	19.52		65.0	
10270-CAD	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	X	6.77	76.24	20.42	3.98	65.0	± 9.6 %
		Y	5.40	75.25	20.50		65.0	
		Z	5.66	73.75	19.79		65.0	



EX3DV4- SN:3863

April 25, 2018

10274-CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.10)	X	2.43	66.71	14.85	0.00	150.0	± 9.6 %
		Y	2.33	68.15	14.74		150.0	
		Z	2.38	65.72	14.40		150.0	
10275-CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.4)	X	1.47	67.75	15.10	0.00	150.0	± 9.6 %
		Y	1.72	72.43	16.90		150.0	
		Z	1.36	65.94	13.97		150.0	
10277-CAA	PHS (QPSK)	X	1.92	60.08	5.51	9.03	50.0	± 9.6 %
		Y	1.38	58.77	3.99		50.0	
		Z	1.98	60.78	6.41		50.0	
10278-CAA	PHS (QPSK, BW 884MHz, Roll-off 0.5)	X	3.08	65.19	10.55	9.03	50.0	± 9.6 %
		Y	2.17	61.96	7.67		50.0	
		Z	3.52	67.85	12.76		50.0	
10279-CAA	PHS (QPSK, BW 884MHz, Roll-off 0.38)	X	3.15	65.40	10.71	9.03	50.0	± 9.6 %
		Y	2.20	62.03	7.77		50.0	
		Z	3.61	68.12	12.94		50.0	
10290-AAB	CDMA2000, RC1, SO55, Full Rate	X	0.92	64.86	10.52	0.00	150.0	± 9.6 %
		Y	0.39	60.00	5.42		150.0	
		Z	0.92	63.92	10.28		150.0	
10291-AAB	CDMA2000, RC3, SO55, Full Rate	X	0.56	63.07	9.34	0.00	150.0	± 9.6 %
		Y	0.29	60.00	5.06		150.0	
		Z	0.54	61.87	8.78		150.0	
10292-AAB	CDMA2000, RC3, SO32, Full Rate	X	0.78	67.26	11.80	0.00	150.0	± 9.6 %
		Y	0.28	60.00	5.38		150.0	
		Z	0.61	63.79	10.15		150.0	
10293-AAB	CDMA2000, RC3, SO3, Full Rate	X	2.07	78.82	16.86	0.00	150.0	± 9.6 %
		Y	0.39	62.28	7.09		150.0	
		Z	0.82	67.12	12.27		150.0	
10295-AAB	CDMA2000, RC1, SO3, 1/8th Rate 25 fr.	X	10.77	83.93	21.20	9.03	50.0	± 9.6 %
		Y	21.51	90.17	21.22		50.0	
		Z	9.58	84.17	22.47		50.0	
10297-AAC	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	X	2.52	69.39	16.43	0.00	150.0	± 9.6 %
		Y	2.55	71.75	17.73		150.0	
		Z	2.42	68.12	15.58		150.0	
10298-AAC	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, QPSK)	X	1.11	64.88	11.35	0.00	150.0	± 9.6 %
		Y	0.56	60.19	6.52		150.0	
		Z	1.13	64.17	11.22		150.0	
10299-AAC	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM)	X	1.42	62.80	9.08	0.00	150.0	± 9.6 %
		Y	0.76	60.00	5.28		150.0	
		Z	1.91	65.84	11.56		150.0	
10300-AAC	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, 64-QAM)	X	1.21	60.93	7.40	0.00	150.0	± 9.6 %
		Y	0.73	60.00	4.72		150.0	
		Z	1.52	62.72	9.26		150.0	
10301-AAA	IEEE 802.16e WIMAX (29:18, 5ms, 10MHz, QPSK, PUSC)	X	4.38	65.24	17.03	4.17	50.0	± 9.6 %
		Y	4.10	66.08	16.99		50.0	
		Z	4.53	65.17	17.06		50.0	
10302-AAA	IEEE 802.16e WIMAX (29:18, 5ms, 10MHz, QPSK, PUSC, 3 CTRL symbols)	X	4.87	65.87	17.74	4.96	50.0	± 9.6 %
		Y	4.52	66.36	17.57		50.0	
		Z	5.00	65.70	17.71		50.0	

EX3DV4- SN:3863

April 25, 2018

10303-AAA	IEEE 802.16e WIMAX (31:15, 5ms, 10MHz, 64QAM, PUSC)	X	4.64	65.56	17.55	4.96	50.0	± 9.6 %
		Y	4.40	66.71	17.70		50.0	
		Z	4.76	65.34	17.52		50.0	
10304-AAA	IEEE 802.16e WIMAX (29:18, 5ms, 10MHz, 64QAM, PUSC)	X	4.47	65.53	17.12	4.17	50.0	± 9.6 %
		Y	4.17	66.24	17.01		50.0	
		Z	4.56	65.19	17.01		50.0	
10305-AAA	IEEE 802.16e WIMAX (31:15, 10ms, 10MHz, 64QAM, PUSC, 15 symbols)	X	4.18	67.59	18.77	6.02	35.0	± 9.6 %
		Y	3.89	67.96	17.61		35.0	
		Z	4.33	67.73	19.13		35.0	
10306-AAA	IEEE 802.16e WIMAX (29:18, 10ms, 10MHz, 64QAM, PUSC, 18 symbols)	X	4.44	66.50	18.52	6.02	35.0	± 9.6 %
		Y	4.15	67.24	17.98		35.0	
		Z	4.60	66.59	18.78		35.0	
10307-AAA	IEEE 802.16e WIMAX (29:18, 10ms, 10MHz, QPSK, PUSC, 18 symbols)	X	4.34	66.59	18.45	6.02	35.0	± 9.6 %
		Y	4.05	67.23	17.84		35.0	
		Z	4.50	66.72	18.72		35.0	
10308-AAA	IEEE 802.16e WIMAX (29:18, 10ms, 10MHz, 16QAM, PUSC)	X	4.32	66.82	18.60	6.02	35.0	± 9.6 %
		Y	4.06	67.54	18.06		35.0	
		Z	4.48	66.95	18.87		35.0	
10309-AAA	IEEE 802.16e WiMAX (29:18, 10ms, 10MHz, 16QAM, AMC 2x3, 18 symbols)	X	4.46	66.56	18.61	6.02	35.0	± 9.6 %
		Y	4.17	67.31	18.10		35.0	
		Z	4.64	66.74	18.90		35.0	
10310-AAA	IEEE 802.16e WiMAX (29:18, 10ms, 10MHz, QPSK, AMC 2x3, 18 symbols)	X	4.40	66.58	18.52	6.02	35.0	± 9.6 %
		Y	4.14	67.40	18.05		35.0	
		Z	4.55	66.87	18.78		35.0	
10311-AAC	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	X	2.88	68.63	16.10	0.00	150.0	± 9.6 %
		Y	2.88	70.38	17.20		150.0	
		Z	2.77	67.46	15.32		150.0	
10313-AAA	iDEN 1:3	X	3.55	71.03	14.37	6.99	70.0	± 9.6 %
		Y	2.76	72.05	15.47		70.0	
		Z	2.49	69.17	14.17		70.0	
10314-AAA	iDEN 1:6	X	6.09	81.23	20.99	10.00	30.0	± 9.6 %
		Y	7.74	88.37	24.07		30.0	
		Z	3.89	76.29	19.81		30.0	
10315-AAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 96pc duty cycle)	X	1.04	63.85	14.96	0.17	150.0	± 9.6 %
		Y	1.05	65.58	16.18		150.0	
		Z	0.96	62.52	14.00		150.0	
10316-AAB	IEEE 802.11g WiFi 2.4 GHz (ERP-OFDM, 6 Mbps, 96pc duty cycle)	X	4.35	66.66	16.11	0.17	150.0	± 9.6 %
		Y	4.12	67.27	16.33		150.0	
		Z	4.39	66.31	15.96		150.0	
10317-AAC	IEEE 802.11a WiFi 5 GHz (OFDM, 6 Mbps, 96pc duty cycle)	X	4.35	66.66	16.11	0.17	150.0	± 9.6 %
		Y	4.12	67.27	16.33		150.0	
		Z	4.39	66.31	15.96		150.0	
10400-AAD	IEEE 802.11ac WiFi (20MHz, 64-QAM, 99pc duty cycle)	X	4.42	66.96	16.15	0.00	150.0	± 9.6 %
		Y	4.13	67.43	16.34		150.0	
		Z	4.47	66.60	15.95		150.0	
10401-AAD	IEEE 802.11ac WiFi (40MHz, 64-QAM, 99pc duty cycle)	X	5.08	66.77	16.17	0.00	150.0	± 9.6 %
		Y	5.02	67.75	16.71		150.0	
		Z	5.22	66.85	16.19		150.0	



EX3DV4- SN:3863

April 25, 2018

10402-AAD	IEEE 802.11ac WiFi (80MHz, 64-QAM, 99pc duty cycle)	X	5.43	67.35	16.36	0.00	150.0	± 9.6 %
		Y	5.23	67.61	16.59		150.0	
		Z	5.46	67.09	16.19		150.0	
10403-AAB	CDMA2000 (1xEV-DO, Rev. 0)	X	0.92	64.86	10.52	0.00	115.0	± 9.6 %
		Y	0.39	60.00	5.42		115.0	
		Z	0.92	63.92	10.28		115.0	
10404-AAB	CDMA2000 (1xEV-DO, Rev. A)	X	0.92	64.86	10.52	0.00	115.0	± 9.6 %
		Y	0.39	60.00	5.42		115.0	
		Z	0.92	63.92	10.28		115.0	
10406-AAB	CDMA2000, RC3, SO32, SCH0, Full Rate	X	6.61	82.29	18.19	0.00	100.0	± 9.6 %
		Y	100.00	99.95	18.83		100.0	
		Z	45.79	108.43	26.26		100.0	
10410-AAD	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9, Subframe Conf=4)	X	3.30	74.41	15.15	3.23	80.0	± 9.6 %
		Y	16.11	98.20	22.53		80.0	
		Z	23.06	102.83	25.32		80.0	
10415-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	X	0.96	62.96	14.43	0.00	150.0	± 9.6 %
		Y	0.99	64.96	15.77		150.0	
		Z	0.90	61.91	13.52		150.0	
10416-AAA	IEEE 802.11g WiFi 2.4 GHz (ERP-OFDM, 6 Mbps, 99pc duty cycle)	X	4.32	66.73	16.13	0.00	150.0	± 9.6 %
		Y	4.11	67.43	16.39		150.0	
		Z	4.34	66.32	15.91		150.0	
10417-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps, 99pc duty cycle)	X	4.32	66.73	16.13	0.00	150.0	± 9.6 %
		Y	4.11	67.43	16.39		150.0	
		Z	4.34	66.32	15.91		150.0	
10418-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 99pc duty cycle, Long preamble)	X	4.31	66.93	16.18	0.00	150.0	± 9.6 %
		Y	4.10	67.68	16.50		150.0	
		Z	4.33	66.49	15.93		150.0	
10419-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 99pc duty cycle, Short preamble)	X	4.33	66.86	16.17	0.00	150.0	± 9.6 %
		Y	4.11	67.59	16.46		150.0	
		Z	4.35	66.43	15.93		150.0	
10422-AAB	IEEE 802.11n (HT Greenfield, 7.2 Mbps, BPSK)	X	4.43	66.84	16.18	0.00	150.0	± 9.6 %
		Y	4.21	67.51	16.45		150.0	
		Z	4.46	66.43	15.95		150.0	
10423-AAB	IEEE 802.11n (HT Greenfield, 43.3 Mbps, 16-QAM)	X	4.56	67.09	16.27	0.00	150.0	± 9.6 %
		Y	4.30	67.73	16.52		150.0	
		Z	4.61	66.71	16.06		150.0	
10424-AAB	IEEE 802.11n (HT Greenfield, 72.2 Mbps, 64-QAM)	X	4.49	67.05	16.24	0.00	150.0	± 9.6 %
		Y	4.23	67.65	16.49		150.0	
		Z	4.53	66.66	16.03		150.0	
10425-AAB	IEEE 802.11n (HT Greenfield, 15 Mbps, BPSK)	X	5.11	67.24	16.43	0.00	150.0	± 9.6 %
		Y	4.85	67.48	16.62		150.0	
		Z	5.16	66.98	16.26		150.0	
10426-AAB	IEEE 802.11n (HT Greenfield, 90 Mbps, 16-QAM)	X	5.13	67.32	16.47	0.00	150.0	± 9.6 %
		Y	4.90	67.67	16.71		150.0	
		Z	5.18	67.07	16.30		150.0	

EX3DV4- SN:3863

April 25, 2018

10427-AAB	IEEE 802.11n (HT Greenfield, 150 Mbps, 64-QAM)	X	5.10	67.11	16.36	0.00	150.0	± 9.6 %
		Y	4.87	67.47	16.61		150.0	
		Z	5.17	66.96	16.24		150.0	
10430-AAB	LTE-FDD (OFDMA, 5 MHz, E-TM 3.1)	X	4.40	73.18	18.78	0.00	150.0	± 9.6 %
		Y	5.18	77.79	19.68		150.0	
		Z	4.07	70.86	17.81		150.0	
10431-AAB	LTE-FDD (OFDMA, 10 MHz, E-TM 3.1)	X	3.93	67.31	16.00	0.00	150.0	± 9.6 %
		Y	3.67	68.21	16.08		150.0	
		Z	3.97	66.78	15.76		150.0	
10432-AAB	LTE-FDD (OFDMA, 15 MHz, E-TM 3.1)	X	4.25	67.14	16.17	0.00	150.0	± 9.6 %
		Y	4.00	67.91	16.40		150.0	
		Z	4.29	66.70	15.93		150.0	
10433-AAB	LTE-FDD (OFDMA, 20 MHz, E-TM 3.1)	X	4.51	67.08	16.27	0.00	150.0	± 9.6 %
		Y	4.26	67.71	16.52		150.0	
		Z	4.55	66.70	16.05		150.0	
10434-AAA	W-CDMA (BS Test Model 1, 64 DPCH)	X	4.57	74.23	18.62	0.00	150.0	± 9.6 %
		Y	4.96	77.01	18.39		150.0	
		Z	4.13	71.55	17.59		150.0	
10435-AAC	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	3.22	74.05	14.97	3.23	80.0	± 9.6 %
		Y	12.58	95.13	21.66		80.0	
		Z	20.50	101.13	24.83		80.0	
10447-AAB	LTE-FDD (OFDMA, 5 MHz, E-TM 3.1, Clipping 44%)	X	3.16	67.07	14.83	0.00	150.0	± 9.6 %
		Y	2.72	66.94	13.70		150.0	
		Z	3.20	66.46	14.68		150.0	
10448-AAB	LTE-FDD (OFDMA, 10 MHz, E-TM 3.1, Clipping 44%)	X	3.80	67.10	15.87	0.00	150.0	± 9.6 %
		Y	3.57	68.05	15.99		150.0	
		Z	3.82	66.56	15.62		150.0	
10449-AAB	LTE-FDD (OFDMA, 15 MHz, E-TM 3.1, Clipping 44%)	X	4.09	66.98	16.07	0.00	150.0	± 9.6 %
		Y	3.88	67.77	16.33		150.0	
		Z	4.12	66.51	15.82		150.0	
10450-AAB	LTE-FDD (OFDMA, 20 MHz, E-TM 3.1, Clipping 44%)	X	4.31	66.86	16.12	0.00	150.0	± 9.6 %
		Y	4.10	67.50	16.40		150.0	
		Z	4.33	66.45	15.89		150.0	
10451-AAA	W-CDMA (BS Test Model 1, 64 DPCH, Clipping 44%)	X	2.96	66.79	14.05	0.00	150.0	± 9.6 %
		Y	2.28	65.25	11.94		150.0	
		Z	3.03	66.33	14.05		150.0	
10456-AAB	IEEE 802.11ac WiFi (160MHz, 64-QAM, 99pc duty cycle)	X	6.03	67.73	16.57	0.00	150.0	± 9.6 %
		Y	6.14	68.84	17.23		150.0	
		Z	6.09	67.66	16.51		150.0	
10457-AAA	UMTS-FDD (DC-HSDPA)	X	3.67	65.47	15.85	0.00	150.0	± 9.6 %
		Y	3.57	66.44	16.21		150.0	
		Z	3.66	65.00	15.61		150.0	
10458-AAA	CDMA2000 (1xEV-DO, Rev. B, 2 carriers)	X	3.82	71.77	16.94	0.00	150.0	± 9.6 %
		Y	2.33	66.01	12.18		150.0	
		Z	3.66	70.24	16.55		150.0	
10459-AAA	CDMA2000 (1xEV-DO, Rev. B, 3 carriers)	X	5.04	70.06	18.38	0.00	150.0	± 9.6 %
		Y	4.33	69.08	16.37		150.0	
		Z	4.93	68.74	17.97		150.0	

EX3DV4- SN:3863

April 25, 2018

10460-AAA	UMTS-FDD (WCDMA, AMR)	X	0.62	68.06	15.67	0.00	150.0	± 9.6 %
		Y	1.52	80.43	21.00		150.0	
		Z	0.70	65.12	13.61		150.0	
10461-AAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	1.71	68.46	13.76	3.29	80.0	± 9.6 %
		Y	18.73	104.14	25.37		80.0	
		Z	16.72	101.23	25.84		80.0	
10462-AAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	0.95	60.00	7.25	3.23	80.0	± 9.6 %
		Y	0.26	55.18	3.00		80.0	
		Z	1.02	61.47	8.87		80.0	
10463-AAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	0.96	60.00	6.79	3.23	80.0	± 9.6 %
		Y	3.83	65.07	6.10		80.0	
		Z	0.88	60.00	7.59		80.0	
10464-AAA	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	1.35	65.72	12.06	3.23	80.0	± 9.6 %
		Y	3.75	82.77	18.52		80.0	
		Z	9.51	92.26	22.65		80.0	
10465-AAA	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	0.95	60.00	7.20	3.23	80.0	± 9.6 %
		Y	0.25	55.06	2.87		80.0	
		Z	0.96	60.91	8.53		80.0	
10466-AAA	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	0.97	60.00	6.75	3.23	80.0	± 9.6 %
		Y	3.08	64.36	5.91		80.0	
		Z	0.88	60.00	7.54		80.0	
10467-AAC	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	1.38	66.05	12.23	3.23	80.0	± 9.6 %
		Y	4.97	86.13	19.58		80.0	
		Z	11.48	94.80	23.39		80.0	
10468-AAC	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	0.95	60.00	7.22	3.23	80.0	± 9.6 %
		Y	0.26	55.12	2.95		80.0	
		Z	0.97	61.07	8.63		80.0	
10469-AAC	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	0.96	60.00	6.75	3.23	80.0	± 9.6 %
		Y	3.73	65.04	6.11		80.0	
		Z	0.88	60.00	7.54		80.0	
10470-AAC	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	1.38	66.03	12.21	3.23	80.0	± 9.6 %
		Y	5.04	86.32	19.63		80.0	
		Z	11.56	94.91	23.42		80.0	
10471-AAC	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	0.95	60.00	7.21	3.23	80.0	± 9.6 %
		Y	0.25	55.11	2.92		80.0	
		Z	0.97	61.03	8.59		80.0	
10472-AAC	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	0.96	60.00	6.74	3.23	80.0	± 9.6 %
		Y	8.84	67.69	6.73		80.0	
		Z	0.88	60.00	7.53		80.0	
10473-AAC	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	1.37	66.01	12.20	3.23	80.0	± 9.6 %
		Y	4.94	86.08	19.55		80.0	
		Z	11.45	94.77	23.37		80.0	
10474-AAC	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	0.94	60.00	7.21	3.23	80.0	± 9.6 %
		Y	0.25	55.09	2.91		80.0	
		Z	0.96	61.01	8.58		80.0	
10475-AAC	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	0.96	60.00	6.74	3.23	80.0	± 9.6 %
		Y	5.48	65.71	6.11		80.0	
		Z	0.88	60.00	7.53		80.0	



EX3DV4-- SN:3863

April 25, 2018

10477-AAC	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	0.94	60.00	7.19	3.23	80.0	± 9.6 %
		Y	0.25	55.02	2.82		80.0	
		Z	0.95	60.87	8.49		80.0	
10478-AAC	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	0.96	60.00	6.73	3.23	80.0	± 9.6 %
		Y	0.28	53.97	1.35		80.0	
		Z	0.88	60.00	7.52		80.0	
10479-AAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	3.21	72.74	16.33	3.23	80.0	± 9.6 %
		Y	39.60	110.75	27.52		80.0	
		Z	6.66	84.68	21.96		80.0	
10480-AAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	2.08	64.62	11.24	3.23	80.0	± 9.6 %
		Y	1.03	61.93	8.80		80.0	
		Z	4.36	74.13	16.27		80.0	
10481-AAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	1.78	62.75	10.02	3.23	80.0	± 9.6 %
		Y	0.84	60.00	7.33		80.0	
		Z	3.24	70.04	14.31		80.0	
10482-AAA	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	1.73	64.95	12.00	2.23	80.0	± 9.6 %
		Y	0.84	60.00	7.70		80.0	
		Z	1.75	65.57	13.09		80.0	
10483-AAA	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	1.61	61.02	9.13	2.23	80.0	± 9.6 %
		Y	1.09	60.00	6.49		80.0	
		Z	2.56	66.79	13.19		80.0	
10484-AAA	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	1.61	60.82	9.02	2.23	80.0	± 9.6 %
		Y	1.11	60.00	6.48		80.0	
		Z	2.45	66.04	12.85		80.0	
10485-AAC	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	2.62	70.06	15.66	2.23	80.0	± 9.6 %
		Y	1.92	68.50	13.94		80.0	
		Z	2.29	68.71	15.73		80.0	
10486-AAC	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	2.37	65.68	13.03	2.23	80.0	± 9.6 %
		Y	1.24	60.58	8.96		80.0	
		Z	2.33	65.68	13.73		80.0	
10487-AAC	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	2.37	65.34	12.86	2.23	80.0	± 9.6 %
		Y	1.24	60.28	8.75		80.0	
		Z	2.35	65.41	13.59		80.0	
10488-AAC	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	3.19	71.23	17.45	2.23	80.0	± 9.6 %
		Y	2.91	73.05	18.24		80.0	
		Z	2.77	69.32	17.00		80.0	
10489-AAC	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.21	68.38	16.16	2.23	80.0	± 9.6 %
		Y	2.80	68.89	15.94		80.0	
		Z	2.91	66.98	15.94		80.0	
10490-AAC	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.28	68.24	16.11	2.23	80.0	± 9.6 %
		Y	2.81	68.47	15.72		80.0	
		Z	3.00	66.92	15.92		80.0	
10491-AAC	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	3.47	70.14	17.34	2.23	80.0	± 9.6 %
		Y	3.03	70.90	17.92		80.0	
		Z	3.12	68.57	16.90		80.0	
10492-AAC	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.59	67.96	16.53	2.23	80.0	± 9.6 %
		Y	3.13	68.26	16.56		80.0	
		Z	3.32	66.68	16.23		80.0	



EX3DV4-- SN:3863

April 25, 2018

10493-AAC	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.65	67.84	16.48	2.23	80.0	± 9.6 %
		Y	3.17	68.05	16.43		80.0	
		Z	3.39	66.61	16.21		80.0	
10494-AAC	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	3.72	71.32	17.72	2.23	80.0	± 9.6 %
		Y	3.26	72.17	16.50		80.0	
		Z	3.30	69.67	17.25		80.0	
10495-AAC	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.62	68.25	16.75	2.23	80.0	± 9.6 %
		Y	3.18	68.50	16.94		80.0	
		Z	3.33	66.95	16.42		80.0	
10496-AAC	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.71	68.07	16.72	2.23	80.0	± 9.6 %
		Y	3.25	68.28	16.85		80.0	
		Z	3.43	66.81	16.39		80.0	
10497-AAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	1.07	60.00	8.19	2.23	80.0	± 9.6 %
		Y	0.87	60.00	5.66		80.0	
		Z	1.16	61.09	9.64		80.0	
10498-AAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	1.24	60.00	7.11	2.23	80.0	± 9.6 %
		Y	1.51	60.00	4.12		80.0	
		Z	1.24	60.00	7.97		80.0	
10499-AAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	1.26	60.00	6.97	2.23	80.0	± 9.6 %
		Y	1.84	60.00	3.85		80.0	
		Z	1.26	60.00	7.82		80.0	
10500-AAA	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	2.86	70.59	16.41	2.23	80.0	± 9.6 %
		Y	2.47	71.37	16.06		80.0	
		Z	2.47	68.90	16.23		80.0	
10501-AAA	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	2.77	67.13	14.41	2.23	80.0	± 9.6 %
		Y	1.82	64.08	11.77		80.0	
		Z	2.61	66.45	14.70		80.0	
10502-AAA	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	2.80	66.92	14.24	2.23	80.0	± 9.6 %
		Y	1.80	63.62	11.44		80.0	
		Z	2.65	66.33	14.58		80.0	
10503-AAC	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	3.15	71.01	17.34	2.23	80.0	± 9.6 %
		Y	2.85	72.73	18.09		80.0	
		Z	2.74	69.14	16.90		80.0	
10504-AAC	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.18	68.25	16.09	2.23	80.0	± 9.6 %
		Y	2.77	68.71	15.84		80.0	
		Z	2.89	66.89	15.87		80.0	
10505-AAC	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.26	68.13	16.04	2.23	80.0	± 9.6 %
		Y	2.78	68.31	15.63		80.0	
		Z	2.99	66.63	15.86		80.0	
10506-AAC	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	3.68	71.16	17.64	2.23	80.0	± 9.6 %
		Y	3.23	71.98	18.40		80.0	
		Z	3.28	69.54	17.18		80.0	
10507-AAC	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.60	68.17	16.71	2.23	80.0	± 9.6 %
		Y	3.16	68.41	16.88		80.0	
		Z	3.32	66.89	16.38		80.0	

EX3DV4- SN:3863

April 25, 2018

10508-AAC	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.69	67.98	16.67	2.23	80.0	± 9.6 %
		Y	3.23	68.18	16.79		80.0	
		Z	3.42	66.74	16.35		80.0	
10509-AAC	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	4.09	70.27	17.38	2.23	80.0	± 9.6 %
		Y	3.57	70.54	17.94		80.0	
		Z	3.72	68.92	16.97		80.0	
10510-AAC	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	4.09	67.97	16.86	2.23	80.0	± 9.6 %
		Y	3.56	67.74	16.96		80.0	
		Z	3.82	66.86	16.53		80.0	
10511-AAC	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	4.17	67.81	16.83	2.23	80.0	± 9.6 %
		Y	3.64	67.61	16.92		80.0	
		Z	3.90	66.70	16.51		80.0	
10512-AAC	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	4.18	71.35	17.66	2.23	80.0	± 9.6 %
		Y	3.66	71.82	18.28		80.0	
		Z	3.77	69.95	17.25		80.0	
10513-AAC	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.98	68.10	16.91	2.23	80.0	± 9.6 %
		Y	3.47	67.78	17.03		80.0	
		Z	3.70	66.98	16.58		80.0	
10514-AAC	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	4.02	67.80	16.84	2.23	80.0	± 9.6 %
		Y	3.52	67.49	16.93		80.0	
		Z	3.75	66.69	16.51		80.0	
10515-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 99pc duty cycle)	X	0.92	63.12	14.48	0.00	150.0	± 9.6 %
		Y	0.96	65.32	15.94		150.0	
		Z	0.86	62.01	13.50		150.0	
10516-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5 Mbps, 99pc duty cycle)	X	0.54	70.00	16.71	0.00	150.0	± 9.6 %
		Y	2.46	99.33	28.61		150.0	
		Z	0.41	65.69	13.40		150.0	
10517-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 11 Mbps, 99pc duty cycle)	X	0.76	64.84	14.98	0.00	150.0	± 9.6 %
		Y	0.86	68.98	17.56		150.0	
		Z	0.68	63.15	13.53		150.0	
10518-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps, 99pc duty cycle)	X	4.31	66.83	16.12	0.00	150.0	± 9.6 %
		Y	4.10	67.60	16.42		150.0	
		Z	4.33	66.40	15.88		150.0	
10519-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 12 Mbps, 99pc duty cycle)	X	4.45	66.99	16.21	0.00	150.0	± 9.6 %
		Y	4.21	67.71	16.46		150.0	
		Z	4.49	66.60	15.99		150.0	
10520-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 18 Mbps, 99pc duty cycle)	X	4.31	66.93	16.12	0.00	150.0	± 9.6 %
		Y	4.08	67.63	16.41		150.0	
		Z	4.35	66.53	15.90		150.0	
10521-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 24 Mbps, 99pc duty cycle)	X	4.24	66.89	16.10	0.00	150.0	± 9.6 %
		Y	4.01	67.52	16.35		150.0	
		Z	4.28	66.50	15.87		150.0	
10522-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 36 Mbps, 99pc duty cycle)	X	4.29	67.01	16.19	0.00	150.0	± 9.6 %
		Y	4.02	67.52	16.36		150.0	
		Z	4.34	66.64	15.98		150.0	

EX3DV4- SN:3863

April 25, 2018

10523-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 48 Mbps, 99pc duty cycle)	X	4.22	67.02	16.12	0.00	150.0	± 9.6 %
		Y	4.02	67.85	16.48		150.0	
		Z	4.24	66.53	15.84		150.0	
10524-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 54 Mbps, 99pc duty cycle)	X	4.25	66.98	16.19	0.00	150.0	± 9.6 %
		Y	4.00	67.65	16.47		150.0	
		Z	4.28	66.56	15.95		150.0	
10525-AAB	IEEE 802.11ac WiFi (20MHz, MCS0, 99pc duty cycle)	X	4.28	66.09	15.82	0.00	150.0	± 9.6 %
		Y	4.09	66.89	16.17		150.0	
		Z	4.29	65.63	15.56		150.0	
10526-AAB	IEEE 802.11ac WiFi (20MHz, MCS1, 99pc duty cycle)	X	4.40	66.37	15.93	0.00	150.0	± 9.6 %
		Y	4.16	67.06	16.24		150.0	
		Z	4.43	65.94	15.69		150.0	
10527-AAB	IEEE 802.11ac WiFi (20MHz, MCS2, 99pc duty cycle)	X	4.33	66.34	15.87	0.00	150.0	± 9.6 %
		Y	4.12	67.09	16.20		150.0	
		Z	4.36	65.89	15.62		150.0	
10528-AAB	IEEE 802.11ac WiFi (20MHz, MCS3, 99pc duty cycle)	X	4.35	66.35	15.90	0.00	150.0	± 9.6 %
		Y	4.12	67.05	16.21		150.0	
		Z	4.37	65.91	15.65		150.0	
10529-AAB	IEEE 802.11ac WiFi (20MHz, MCS4, 99pc duty cycle)	X	4.35	66.35	15.90	0.00	150.0	± 9.6 %
		Y	4.12	67.05	16.21		150.0	
		Z	4.37	65.91	15.65		150.0	
10531-AAB	IEEE 802.11ac WiFi (20MHz, MCS6, 99pc duty cycle)	X	4.31	66.37	15.88	0.00	150.0	± 9.6 %
		Y	4.07	67.03	16.17		150.0	
		Z	4.35	65.96	15.64		150.0	
10532-AAB	IEEE 802.11ac WiFi (20MHz, MCS7, 99pc duty cycle)	X	4.19	66.23	15.81	0.00	150.0	± 9.6 %
		Y	3.98	66.94	16.12		150.0	
		Z	4.22	65.81	15.56		150.0	
10533-AAB	IEEE 802.11ac WiFi (20MHz, MCS8, 99pc duty cycle)	X	4.35	66.43	15.91	0.00	150.0	± 9.6 %
		Y	4.13	67.21	16.24		150.0	
		Z	4.38	65.98	15.65		150.0	
10534-AAB	IEEE 802.11ac WiFi (40MHz, MCS0, 99pc duty cycle)	X	4.91	66.34	15.97	0.00	150.0	± 9.6 %
		Y	4.69	66.74	16.24		150.0	
		Z	4.94	66.04	15.77		150.0	
10535-AAB	IEEE 802.11ac WiFi (40MHz, MCS1, 99pc duty cycle)	X	4.95	66.47	16.03	0.00	150.0	± 9.6 %
		Y	4.71	66.81	16.28		150.0	
		Z	4.99	66.21	15.85		150.0	
10536-AAB	IEEE 802.11ac WiFi (40MHz, MCS2, 99pc duty cycle)	X	4.84	66.47	16.01	0.00	150.0	± 9.6 %
		Y	4.62	66.84	16.27		150.0	
		Z	4.87	66.16	15.80		150.0	
10537-AAB	IEEE 802.11ac WiFi (40MHz, MCS3, 99pc duty cycle)	X	4.90	66.47	16.01	0.00	150.0	± 9.6 %
		Y	4.71	66.93	16.32		150.0	
		Z	4.93	66.13	15.79		150.0	
10538-AAB	IEEE 802.11ac WiFi (40MHz, MCS4, 99pc duty cycle)	X	4.97	66.42	16.03	0.00	150.0	± 9.6 %
		Y	4.73	66.75	16.26		150.0	
		Z	5.00	66.13	15.84		150.0	
10540-AAB	IEEE 802.11ac WiFi (40MHz, MCS6, 99pc duty cycle)	X	4.90	66.38	16.03	0.00	150.0	± 9.6 %
		Y	4.67	66.70	16.26		150.0	
		Z	4.93	66.11	15.84		150.0	



EX3DV4-- SN:3863

April 25, 2018

10541-AAB	IEEE 802.11ac WiFi (40MHz, MCS7, 99pc duty cycle)	X	4.88	66.31	15.97	0.00	150.0	± 9.6 %
		Y	4.67	66.70	16.23		150.0	
		Z	4.91	66.01	15.77		150.0	
10542-AAB	IEEE 802.11ac WiFi (40MHz, MCS8, 99pc duty cycle)	X	5.04	66.41	16.04	0.00	150.0	± 9.6 %
		Y	4.80	66.76	16.28		150.0	
		Z	5.07	66.11	15.85		150.0	
10543-AAB	IEEE 802.11ac WiFi (40MHz, MCS9, 99pc duty cycle)	X	5.11	66.49	16.11	0.00	150.0	± 9.6 %
		Y	4.85	66.80	16.33		150.0	
		Z	5.14	66.14	15.89		150.0	
10544-AAB	IEEE 802.11ac WiFi (80MHz, MCS0, 99pc duty cycle)	X	5.25	66.42	15.96	0.00	150.0	± 9.6 %
		Y	5.07	66.65	16.18		150.0	
		Z	5.27	66.15	15.78		150.0	
10545-AAB	IEEE 802.11ac WiFi (80MHz, MCS1, 99pc duty cycle)	X	5.42	66.84	16.13	0.00	150.0	± 9.6 %
		Y	5.21	67.04	16.34		150.0	
		Z	5.45	66.60	15.96		150.0	
10546-AAB	IEEE 802.11ac WiFi (80MHz, MCS2, 99pc duty cycle)	X	5.28	66.54	15.99	0.00	150.0	± 9.6 %
		Y	5.09	66.74	16.19		150.0	
		Z	5.31	66.30	15.82		150.0	
10547-AAB	IEEE 802.11ac WiFi (80MHz, MCS3, 99pc duty cycle)	X	5.36	66.65	16.04	0.00	150.0	± 9.6 %
		Y	5.22	67.07	16.36		150.0	
		Z	5.39	66.38	15.86		150.0	
10548-AAB	IEEE 802.11ac WiFi (80MHz, MCS4, 99pc duty cycle)	X	5.50	67.24	16.31	0.00	150.0	± 9.6 %
		Y	5.18	67.11	16.36		150.0	
		Z	5.58	67.16	16.22		150.0	
10550-AAB	IEEE 802.11ac WiFi (80MHz, MCS6, 99pc duty cycle)	X	5.34	66.72	16.10	0.00	150.0	± 9.6 %
		Y	5.22	67.23	16.45		150.0	
		Z	5.36	66.42	15.90		150.0	
10551-AAB	IEEE 802.11ac WiFi (80MHz, MCS7, 99pc duty cycle)	X	5.28	66.50	15.95	0.00	150.0	± 9.6 %
		Y	5.06	66.66	16.14		150.0	
		Z	5.33	66.34	15.82		150.0	
10552-AAB	IEEE 802.11ac WiFi (80MHz, MCS8, 99pc duty cycle)	X	5.26	66.54	15.97	0.00	150.0	± 9.6 %
		Y	5.07	66.82	16.21		150.0	
		Z	5.27	66.23	15.76		150.0	
10553-AAB	IEEE 802.11ac WiFi (80MHz, MCS9, 99pc duty cycle)	X	5.31	66.48	15.97	0.00	150.0	± 9.6 %
		Y	5.11	66.71	16.17		150.0	
		Z	5.34	66.23	15.80		150.0	
10554-AAC	IEEE 802.11ac WiFi (160MHz, MCS0, 99pc duty cycle)	X	5.67	66.75	16.04	0.00	150.0	± 9.6 %
		Y	5.52	66.90	16.21		150.0	
		Z	5.69	66.52	15.88		150.0	
10555-AAC	IEEE 802.11ac WiFi (160MHz, MCS1, 99pc duty cycle)	X	5.76	66.97	16.13	0.00	150.0	± 9.6 %
		Y	5.58	67.06	16.29		150.0	
		Z	5.80	66.79	16.00		150.0	
10556-AAC	IEEE 802.11ac WiFi (160MHz, MCS2, 99pc duty cycle)	X	5.80	67.08	16.18	0.00	150.0	± 9.6 %
		Y	5.63	67.23	16.36		150.0	
		Z	5.83	66.86	16.03		150.0	
10557-AAC	IEEE 802.11ac WiFi (160MHz, MCS3, 99pc duty cycle)	X	5.76	66.95	16.13	0.00	150.0	± 9.6 %
		Y	5.57	67.06	16.29		150.0	
		Z	5.78	66.73	15.96		150.0	



EX3DV4- SN:3863

April 25, 2018

10558-AAC	IEEE 802.11ac WiFi (160MHz, MCS4, 99pc duty cycle)	X	5.77	67.00	16.18	0.00	150.0	± 9.6 %
		Y	5.54	66.98	16.27		150.0	
		Z	5.82	66.87	16.07		150.0	
10560-AAC	IEEE 802.11ac WiFi (160MHz, MCS6, 99pc duty cycle)	X	5.79	66.93	16.18	0.00	150.0	± 9.6 %
		Y	5.57	66.97	16.30		150.0	
		Z	5.82	66.74	16.04		150.0	
10561-AAC	IEEE 802.11ac WiFi (160MHz, MCS7, 99pc duty cycle)	X	5.72	66.92	16.20	0.00	150.0	± 9.6 %
		Y	5.51	66.95	16.32		150.0	
		Z	5.75	66.73	16.07		150.0	
10562-AAC	IEEE 802.11ac WiFi (160MHz, MCS8, 99pc duty cycle)	X	5.77	67.08	16.28	0.00	150.0	± 9.6 %
		Y	5.56	67.09	16.39		150.0	
		Z	5.83	66.98	16.19		150.0	
10563-AAC	IEEE 802.11ac WiFi (160MHz, MCS9, 99pc duty cycle)	X	5.87	67.06	16.24	0.00	150.0	± 9.6 %
		Y	5.77	67.47	16.55		150.0	
		Z	5.92	66.90	16.12		150.0	
10564-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 9 Mbps, 99pc duty cycle)	X	4.62	66.82	16.22	0.46	150.0	± 9.6 %
		Y	4.39	67.43	16.46		150.0	
		Z	4.66	66.47	16.04		150.0	
10565-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 12 Mbps, 99pc duty cycle)	X	4.82	67.25	16.56	0.46	150.0	± 9.6 %
		Y	4.56	67.87	16.81		150.0	
		Z	4.86	66.91	16.38		150.0	
10566-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 18 Mbps, 99pc duty cycle)	X	4.65	67.05	16.34	0.46	150.0	± 9.6 %
		Y	4.40	67.63	16.58		150.0	
		Z	4.70	66.72	16.17		150.0	
10567-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 24 Mbps, 99pc duty cycle)	X	4.70	67.52	16.78	0.46	150.0	± 9.6 %
		Y	4.46	68.13	17.04		150.0	
		Z	4.73	67.13	16.55		150.0	
10568-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 36 Mbps, 99pc duty cycle)	X	4.54	66.72	16.04	0.46	150.0	± 9.6 %
		Y	4.23	67.04	16.12		150.0	
		Z	4.60	66.47	15.91		150.0	
10569-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 48 Mbps, 99pc duty cycle)	X	4.69	67.76	16.91	0.46	150.0	± 9.6 %
		Y	4.48	68.53	17.28		150.0	
		Z	4.70	67.29	16.65		150.0	
10570-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 54 Mbps, 99pc duty cycle)	X	4.68	67.52	16.79	0.46	150.0	± 9.6 %
		Y	4.43	68.13	17.07		150.0	
		Z	4.72	67.10	16.55		150.0	
10571-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 90pc duty cycle)	X	1.13	64.43	15.18	0.46	130.0	± 9.6 %
		Y	1.09	65.61	16.13		130.0	
		Z	1.02	62.91	14.24		130.0	
10572-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 90pc duty cycle)	X	1.14	65.04	15.56	0.46	130.0	± 9.6 %
		Y	1.11	66.40	16.63		130.0	
		Z	1.02	63.36	14.54		130.0	
10573-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5 Mbps, 90pc duty cycle)	X	2.01	84.38	21.80	0.46	130.0	± 9.6 %
		Y	35.15	138.74	38.20		130.0	
		Z	0.86	72.57	16.97		130.0	
10574-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 11 Mbps, 90pc duty cycle)	X	1.29	71.29	18.68	0.46	130.0	± 9.6 %
		Y	1.41	75.83	21.40		130.0	
		Z	1.02	67.46	16.65		130.0	

EX3DV4- SN:3863

April 25, 2018

10575-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 90pc duty cycle)	X	4.40	66.56	16.20	0.46	130.0	± 9.6 %
		Y	4.16	67.14	16.39		130.0	
		Z	4.44	66.24	16.07		130.0	
10576-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 9 Mbps, 90pc duty cycle)	X	4.43	66.78	16.30	0.46	130.0	± 9.6 %
		Y	4.20	67.45	16.55		130.0	
		Z	4.46	66.42	16.14		130.0	
10577-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 12 Mbps, 90pc duty cycle)	X	4.59	67.02	16.46	0.46	130.0	± 9.6 %
		Y	4.33	67.64	16.68		130.0	
		Z	4.64	66.69	16.31		130.0	
10578-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 18 Mbps, 90pc duty cycle)	X	4.50	67.20	16.59	0.46	130.0	± 9.6 %
		Y	4.26	67.87	16.85		130.0	
		Z	4.54	66.83	16.41		130.0	
10579-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 24 Mbps, 90pc duty cycle)	X	4.24	66.27	15.75	0.46	130.0	± 9.6 %
		Y	3.96	66.67	15.85		130.0	
		Z	4.30	66.02	15.65		130.0	
10580-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 36 Mbps, 90pc duty cycle)	X	4.27	66.31	15.76	0.46	130.0	± 9.6 %
		Y	3.95	66.55	15.77		130.0	
		Z	4.34	66.08	15.68		130.0	
10581-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 48 Mbps, 90pc duty cycle)	X	4.41	67.27	16.55	0.46	130.0	± 9.6 %
		Y	4.19	68.04	16.88		130.0	
		Z	4.44	66.86	16.35		130.0	
10582-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 54 Mbps, 90pc duty cycle)	X	4.16	66.00	15.50	0.46	130.0	± 9.6 %
		Y	3.86	66.35	15.58		130.0	
		Z	4.23	65.78	15.42		130.0	
10583-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps, 90pc duty cycle)	X	4.40	66.56	16.20	0.46	130.0	± 9.6 %
		Y	4.16	67.14	16.39		130.0	
		Z	4.44	66.24	16.07		130.0	
10584-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps, 90pc duty cycle)	X	4.43	66.78	16.30	0.46	130.0	± 9.6 %
		Y	4.20	67.45	16.55		130.0	
		Z	4.46	66.42	16.14		130.0	
10585-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 12 Mbps, 90pc duty cycle)	X	4.59	67.02	16.46	0.46	130.0	± 9.6 %
		Y	4.33	67.64	16.68		130.0	
		Z	4.64	66.69	16.31		130.0	
10586-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 18 Mbps, 90pc duty cycle)	X	4.50	67.20	16.59	0.46	130.0	± 9.6 %
		Y	4.26	67.87	16.85		130.0	
		Z	4.54	66.83	16.41		130.0	
10587-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 24 Mbps, 90pc duty cycle)	X	4.24	66.27	15.75	0.46	130.0	± 9.6 %
		Y	3.96	66.67	15.85		130.0	
		Z	4.30	66.02	15.65		130.0	
10588-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 36 Mbps, 90pc duty cycle)	X	4.27	66.31	15.76	0.46	130.0	± 9.6 %
		Y	3.95	66.55	15.77		130.0	
		Z	4.34	66.08	15.68		130.0	
10589-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 48 Mbps, 90pc duty cycle)	X	4.41	67.27	16.55	0.46	130.0	± 9.6 %
		Y	4.19	68.04	16.88		130.0	
		Z	4.44	66.86	16.35		130.0	
10590-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 54 Mbps, 90pc duty cycle)	X	4.16	66.00	15.50	0.46	130.0	± 9.6 %
		Y	3.86	66.35	15.58		130.0	
		Z	4.23	65.78	15.42		130.0	

EX3DV4- SN:3863

April 25, 2018

10591-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS0, 90pc duty cycle)	X	4.56	66.67	16.34	0.46	130.0	± 9.6 %
		Y	4.32	67.28	16.57		130.0	
		Z	4.59	66.33	16.20		130.0	
10592-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS1, 90pc duty cycle)	X	4.67	66.95	16.47	0.46	130.0	± 9.6 %
		Y	4.40	67.50	16.68		130.0	
		Z	4.73	66.64	16.33		130.0	
10593-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS2, 90pc duty cycle)	X	4.59	66.81	16.31	0.46	130.0	± 9.6 %
		Y	4.33	67.38	16.52		130.0	
		Z	4.64	66.52	16.18		130.0	
10594-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS3, 90pc duty cycle)	X	4.65	67.01	16.49	0.46	130.0	± 9.6 %
		Y	4.38	67.56	16.71		130.0	
		Z	4.70	66.70	16.35		130.0	
10595-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS4, 90pc duty cycle)	X	4.61	66.98	16.39	0.46	130.0	± 9.6 %
		Y	4.34	67.53	16.61		130.0	
		Z	4.66	66.65	16.24		130.0	
10596-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS5, 90pc duty cycle)	X	4.54	66.93	16.37	0.46	130.0	± 9.6 %
		Y	4.25	67.39	16.55		130.0	
		Z	4.60	66.62	16.23		130.0	
10597-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS6, 90pc duty cycle)	X	4.49	66.79	16.22	0.46	130.0	± 9.6 %
		Y	4.22	67.27	16.39		130.0	
		Z	4.55	66.50	16.09		130.0	
10598-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS7, 90pc duty cycle)	X	4.49	67.08	16.53	0.46	130.0	± 9.6 %
		Y	4.26	67.70	16.78		130.0	
		Z	4.53	66.74	16.37		130.0	
10599-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS0, 90pc duty cycle)	X	5.23	67.11	16.59	0.46	130.0	± 9.6 %
		Y	5.12	67.88	17.03		130.0	
		Z	5.27	66.86	16.46		130.0	
10600-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS1, 90pc duty cycle)	X	5.32	67.43	16.72	0.46	130.0	± 9.6 %
		Y	5.06	67.70	16.91		130.0	
		Z	5.40	67.28	16.64		130.0	
10601-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS2, 90pc duty cycle)	X	5.23	67.24	16.64	0.46	130.0	± 9.6 %
		Y	5.01	67.64	16.90		130.0	
		Z	5.29	67.02	16.53		130.0	
10602-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS3, 90pc duty cycle)	X	5.32	67.24	16.55	0.46	130.0	± 9.6 %
		Y	5.04	67.46	16.72		130.0	
		Z	5.42	67.18	16.53		130.0	
10603-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS4, 90pc duty cycle)	X	5.39	67.57	16.87	0.46	130.0	± 9.6 %
		Y	5.05	67.60	16.95		130.0	
		Z	5.48	67.46	16.80		130.0	
10604-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS5, 90pc duty cycle)	X	5.28	67.19	16.65	0.46	130.0	± 9.6 %
		Y	5.00	67.36	16.79		130.0	
		Z	5.37	67.14	16.62		130.0	
10605-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS6, 90pc duty cycle)	X	5.31	67.30	16.70	0.46	130.0	± 9.6 %
		Y	5.01	67.43	16.83		130.0	
		Z	5.39	67.19	16.65		130.0	
10606-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS7, 90pc duty cycle)	X	5.10	66.73	16.26	0.46	130.0	± 9.6 %
		Y	4.93	67.27	16.59		130.0	
		Z	5.13	66.48	16.14		130.0	



EX3DV4- SN:3863

April 25, 2018

10607-AAB	IEEE 802.11ac WiFi (20MHz, MCS0, 90pc duty cycle)	X	4.40	66.00	15.99	0.46	130.0	± 9.6 %
		Y	4.19	66.71	16.28		130.0	
		Z	4.43	65.63	15.81		130.0	
10608-AAB	IEEE 802.11ac WiFi (20MHz, MCS1, 90pc duty cycle)	X	4.54	66.32	16.13	0.46	130.0	± 9.6 %
		Y	4.28	66.94	16.39		130.0	
		Z	4.59	65.99	15.97		130.0	
10609-AAB	IEEE 802.11ac WiFi (20MHz, MCS2, 90pc duty cycle)	X	4.43	66.14	15.93	0.46	130.0	± 9.6 %
		Y	4.18	66.77	16.19		130.0	
		Z	4.48	65.81	15.78		130.0	
10610-AAB	IEEE 802.11ac WiFi (20MHz, MCS3, 90pc duty cycle)	X	4.48	66.33	16.12	0.46	130.0	± 9.6 %
		Y	4.24	66.96	16.39		130.0	
		Z	4.53	65.98	15.95		130.0	
10611-AAB	IEEE 802.11ac WiFi (20MHz, MCS4, 90pc duty cycle)	X	4.40	66.11	15.95	0.46	130.0	± 9.6 %
		Y	4.14	66.70	16.20		130.0	
		Z	4.44	65.77	15.79		130.0	
10612-AAB	IEEE 802.11ac WiFi (20MHz, MCS5, 90pc duty cycle)	X	4.38	66.21	15.97	0.46	130.0	± 9.6 %
		Y	4.09	66.68	16.16		130.0	
		Z	4.44	65.90	15.83		130.0	
10613-AAB	IEEE 802.11ac WiFi (20MHz, MCS6, 90pc duty cycle)	X	4.37	66.02	15.81	0.46	130.0	± 9.6 %
		Y	4.10	66.52	16.00		130.0	
		Z	4.44	65.75	15.68		130.0	
10614-AAB	IEEE 802.11ac WiFi (20MHz, MCS7, 90pc duty cycle)	X	4.36	66.31	16.11	0.46	130.0	± 9.6 %
		Y	4.12	66.94	16.38		130.0	
		Z	4.40	65.96	15.94		130.0	
10615-AAB	IEEE 802.11ac WiFi (20MHz, MCS8, 90pc duty cycle)	X	4.38	65.89	15.68	0.46	130.0	± 9.6 %
		Y	4.11	66.48	15.90		130.0	
		Z	4.44	65.80	15.55		130.0	
10616-AAB	IEEE 802.11ac WiFi (40MHz, MCS0, 90pc duty cycle)	X	5.04	66.30	16.17	0.46	130.0	± 9.6 %
		Y	4.81	66.63	16.40		130.0	
		Z	5.08	66.07	16.04		130.0	
10617-AAB	IEEE 802.11ac WiFi (40MHz, MCS1, 90pc duty cycle)	X	5.07	66.41	16.20	0.46	130.0	± 9.6 %
		Y	4.82	66.67	16.40		130.0	
		Z	5.15	66.26	16.12		130.0	
10618-AAB	IEEE 802.11ac WiFi (40MHz, MCS2, 90pc duty cycle)	X	4.99	66.49	16.26	0.46	130.0	± 9.6 %
		Y	4.75	66.78	16.46		130.0	
		Z	5.04	66.28	16.14		130.0	
10619-AAB	IEEE 802.11ac WiFi (40MHz, MCS3, 90pc duty cycle)	X	5.01	66.29	16.09	0.46	130.0	± 9.6 %
		Y	4.79	66.70	16.36		130.0	
		Z	5.05	66.06	15.96		130.0	
10620-AAB	IEEE 802.11ac WiFi (40MHz, MCS4, 90pc duty cycle)	X	5.07	66.29	16.14	0.46	130.0	± 9.6 %
		Y	4.80	66.49	16.29		130.0	
		Z	5.13	66.09	16.03		130.0	
10621-AAB	IEEE 802.11ac WiFi (40MHz, MCS5, 90pc duty cycle)	X	5.09	66.45	16.35	0.46	130.0	± 9.6 %
		Y	4.85	66.75	16.57		130.0	
		Z	5.15	66.25	16.23		130.0	
10622-AAB	IEEE 802.11ac WiFi (40MHz, MCS6, 90pc duty cycle)	X	5.08	66.53	16.39	0.46	130.0	± 9.6 %
		Y	4.83	66.78	16.59		130.0	
		Z	5.14	66.36	16.28		130.0	



EX3DV4- SN:3863

April 25, 2018

10623-AAB	IEEE 802.11ac WiFi (40MHz, MCS7, 90pc duty cycle)	X	4.96	66.05	15.99	0.46	130.0	± 9.6 %
		Y	4.74	66.39	16.22		130.0	
		Z	5.02	65.88	15.90		130.0	
10624-AAB	IEEE 802.11ac WiFi (40MHz, MCS8, 90pc duty cycle)	X	5.16	66.32	16.20	0.46	130.0	± 9.6 %
		Y	4.91	66.60	16.40		130.0	
		Z	5.22	66.13	16.10		130.0	
10625-AAB	IEEE 802.11ac WiFi (40MHz, MCS9, 90pc duty cycle)	X	5.25	66.46	16.34	0.46	130.0	± 9.6 %
		Y	5.01	66.87	16.61		130.0	
		Z	5.43	66.66	16.42		130.0	
10626-AAB	IEEE 802.11ac WiFi (80MHz, MCS0, 90pc duty cycle)	X	5.37	66.32	16.13	0.46	130.0	± 9.6 %
		Y	5.18	66.52	16.32		130.0	
		Z	5.41	66.14	16.02		130.0	
10627-AAB	IEEE 802.11ac WiFi (80MHz, MCS1, 90pc duty cycle)	X	5.59	66.90	16.39	0.46	130.0	± 9.6 %
		Y	5.36	67.08	16.58		130.0	
		Z	5.64	66.75	16.30		130.0	
10628-AAB	IEEE 802.11ac WiFi (80MHz, MCS2, 90pc duty cycle)	X	5.36	66.27	16.00	0.46	130.0	± 9.6 %
		Y	5.15	66.43	16.17		130.0	
		Z	5.41	66.15	15.92		130.0	
10629-AAB	IEEE 802.11ac WiFi (80MHz, MCS3, 90pc duty cycle)	X	5.46	66.45	16.06	0.46	130.0	± 9.6 %
		Y	5.33	66.94	16.43		130.0	
		Z	5.50	66.26	15.96		130.0	
10630-AAB	IEEE 802.11ac WiFi (80MHz, MCS4, 90pc duty cycle)	X	5.68	67.33	16.53	0.46	130.0	± 9.6 %
		Y	5.30	67.01	16.48		130.0	
		Z	5.83	67.48	16.58		130.0	
10631-AAB	IEEE 802.11ac WiFi (80MHz, MCS5, 90pc duty cycle)	X	5.68	67.46	16.80	0.46	130.0	± 9.6 %
		Y	5.39	67.46	16.91		130.0	
		Z	5.77	67.39	16.74		130.0	
10632-AAB	IEEE 802.11ac WiFi (80MHz, MCS6, 90pc duty cycle)	X	5.60	67.13	16.65	0.46	130.0	± 9.6 %
		Y	5.50	67.73	17.05		130.0	
		Z	5.63	66.87	16.50		130.0	
10633-AAB	IEEE 802.11ac WiFi (80MHz, MCS7, 90pc duty cycle)	X	5.39	66.38	16.10	0.46	130.0	± 9.6 %
		Y	5.16	66.54	16.27		130.0	
		Z	5.48	66.37	16.07		130.0	
10634-AAB	IEEE 802.11ac WiFi (80MHz, MCS8, 90pc duty cycle)	X	5.42	66.59	16.25	0.46	130.0	± 9.6 %
		Y	5.22	66.83	16.48		130.0	
		Z	5.46	66.38	16.13		130.0	
10635-AAB	IEEE 802.11ac WiFi (80MHz, MCS9, 90pc duty cycle)	X	5.26	65.75	15.53	0.46	130.0	± 9.6 %
		Y	5.03	65.88	15.68		130.0	
		Z	5.33	65.66	15.49		130.0	
10636-AAC	IEEE 802.11ac WiFi (160MHz, MCS0, 90pc duty cycle)	X	5.80	66.66	16.21	0.46	130.0	± 9.6 %
		Y	5.64	66.80	16.37		130.0	
		Z	5.84	66.53	16.13		130.0	
10637-AAC	IEEE 802.11ac WiFi (160MHz, MCS1, 90pc duty cycle)	X	5.91	66.96	16.34	0.46	130.0	± 9.6 %
		Y	5.72	67.05	16.49		130.0	
		Z	5.98	66.89	16.30		130.0	
10638-AAC	IEEE 802.11ac WiFi (160MHz, MCS2, 90pc duty cycle)	X	5.94	67.02	16.35	0.46	130.0	± 9.6 %
		Y	5.77	67.21	16.55		130.0	
		Z	5.96	66.86	16.26		130.0	

EX3DV4- SN:3863

April 25, 2018

10639-AAC	IEEE 802.11ac WiFi (160MHz, MCS3, 90pc duty cycle)	X	5.90	66.90	16.34	0.46	130.0	± 9.6 %
		Y	5.70	66.99	16.48		130.0	
		Z	5.95	66.78	16.26		130.0	
10640-AAC	IEEE 802.11ac WiFi (160MHz, MCS4, 90pc duty cycle)	X	5.85	66.77	16.21	0.46	130.0	± 9.6 %
		Y	5.60	66.70	16.28		130.0	
		Z	5.94	66.77	16.19		130.0	
10641-AAC	IEEE 802.11ac WiFi (160MHz, MCS5, 90pc duty cycle)	X	5.95	66.85	16.27	0.46	130.0	± 9.6 %
		Y	5.73	66.88	16.38		130.0	
		Z	6.01	66.77	16.22		130.0	
10642-AAC	IEEE 802.11ac WiFi (160MHz, MCS6, 90pc duty cycle)	X	5.98	67.10	16.57	0.46	130.0	± 9.6 %
		Y	5.76	67.11	16.68		130.0	
		Z	6.04	66.98	16.50		130.0	
10643-AAC	IEEE 802.11ac WiFi (160MHz, MCS7, 90pc duty cycle)	X	5.82	66.74	16.27	0.46	130.0	± 9.6 %
		Y	5.59	66.71	16.35		130.0	
		Z	5.88	66.67	16.23		130.0	
10644-AAC	IEEE 802.11ac WiFi (160MHz, MCS8, 90pc duty cycle)	X	5.88	66.93	16.39	0.46	130.0	± 9.6 %
		Y	5.65	66.92	16.48		130.0	
		Z	5.97	66.98	16.39		130.0	
10645-AAC	IEEE 802.11ac WiFi (160MHz, MCS9, 90pc duty cycle)	X	6.00	66.98	16.38	0.46	130.0	± 9.6 %
		Y	5.89	67.36	16.67		130.0	
		Z	6.11	67.04	16.40		130.0	
10646-AAD	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK, UL Subframe=2,7)	X	10.64	95.54	31.22	9.30	60.0	± 9.6 %
		Y	4.79	84.10	28.76		60.0	
		Z	10.44	97.20	33.10		60.0	
10647-AAC	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, UL Subframe=2,7)	X	9.38	93.52	30.68	9.30	60.0	± 9.6 %
		Y	4.24	81.79	27.97		60.0	
		Z	9.23	95.05	32.51		60.0	
10648-AAA	CDMA2000 (1x Advanced)	X	0.45	60.96	7.58	0.00	150.0	± 9.6 %
		Y	0.27	60.00	4.46		150.0	
		Z	0.46	60.51	7.45		150.0	
10652-AAB	LTE-TDD (OFDMA, 5 MHz, E-TM 3.1, Clipping 44%)	X	3.44	66.86	15.90	2.23	80.0	± 9.6 %
		Y	3.11	67.55	15.78		80.0	
		Z	3.23	65.63	15.61		80.0	
10653-AAB	LTE-TDD (OFDMA, 10 MHz, E-TM 3.1, Clipping 44%)	X	4.00	66.30	16.33	2.23	80.0	± 9.6 %
		Y	3.63	66.57	16.36		80.0	
		Z	3.80	65.27	16.02		80.0	
10654-AAB	LTE-TDD (OFDMA, 15 MHz, E-TM 3.1, Clipping 44%)	X	4.02	65.95	16.40	2.23	80.0	± 9.6 %
		Y	3.68	66.02	16.44		80.0	
		Z	3.82	64.96	16.07		80.0	
10655-AAB	LTE-TDD (OFDMA, 20 MHz, E-TM 3.1, Clipping 44%)	X	4.10	65.87	16.44	2.23	80.0	± 9.6 %
		Y	3.77	65.78	16.47		80.0	
		Z	3.89	64.93	16.12		80.0	
10658-AAA	Pulse Waveform (200Hz, 10%)	X	3.96	69.40	12.41	10.00	50.0	± 9.6 %
		Y	3.54	68.64	11.84		50.0	
		Z	6.60	76.50	15.95		50.0	
10659-AAA	Pulse Waveform (200Hz, 20%)	X	3.35	69.24	11.38	6.99	60.0	± 9.6 %
		Y	2.54	68.41	10.67		60.0	
		Z	15.62	86.85	17.81		60.0	

EX3DV4- SN:3863

April 25, 2018

10660-AAA	Pulse Waveform (200Hz, 40%)	X	3.13	70.75	10.92	3.98	80.0	± 9.6 %
		Y	2.65	71.33	10.38		80.0	
		Z	100.00	100.70	18.97		80.0	
10661-AAA	Pulse Waveform (200Hz, 60%)	X	3.01	72.21	10.50	2.22	100.0	± 9.6 %
		Y	0.47	62.70	6.02		100.0	
		Z	0.86	65.62	7.78		100.0	
10662-AAA	Pulse Waveform (200Hz, 80%)	X	0.23	60.01	4.55	0.97	120.0	± 9.6 %
		Y	0.53	60.44	2.25		120.0	
		Z	0.27	60.00	2.59		120.0	

<sup>2</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

## Attachment 7. – Dipole Calibration Data



**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**S** Service suisse d'étalonnage  
**C** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **HCT (Dymstec)**

Certificate No: **D750V3-1014\_Aug18**

**CALIBRATION CERTIFICATE**

Object **D750V3 - SN:1014**

Calibration procedure(s) **QA CAL-05.v10  
Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **August 14, 2018**

결재	담당자	와인자
	<i>[Signature]</i>	<i>[Signature]</i>
직위/성명	GW 175243	GW 175243
일 자	2018. 10. 23	2018. 10. 23

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-18 (No. 217-02672/02673)	Apr-19
Power sensor NRP-Z91	SN: 103244	04-Apr-18 (No. 217-02672)	Apr-19
Power sensor NRP-Z91	SN: 103245	04-Apr-18 (No. 217-02673)	Apr-19
Reference 20 dB Attenuator	SN: 5058 (20k)	04-Apr-18 (No. 217-02682)	Apr-19
Type-N mismatch combination	SN: 5047.2 / 06327	04-Apr-18 (No. 217-02683)	Apr-19
Reference Probe EX3DV4	SN: 7349	30-Dec-17 (No. EX3-7349_Dec17)	Dec-18
DAE4	SN: 601	26-Oct-17 (No. DAE4-601_Oct17)	Oct-18

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: GB37480704	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-16)	In house check: Oct-18
Network Analyzer Agilent EB358A	SN: US41080477	31-Mar-14 (in house check Oct-17)	In house check: Oct-18

Calibrated by:	Name	Function	Signature
	Manu Seitz	Laboratory Technician	<i>[Signature]</i>
Approved by:	Katja Pokovic	Technical Manager	<i>[Signature]</i>

Issued: August 14, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

**Glossary:**

TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORM x,y,z  
N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- e) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.1
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	750 MHz ± 1 MHz	

**Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.9	0.89 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.9 ± 6 %	0.89 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

**SAR result with Head TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.05 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>8.15 W/kg ± 17.0 % (k=2)</b>

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.33 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>5.30 W/kg ± 16.5 % (k=2)</b>

**Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.5	0.96 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	55.0 ± 6 %	0.96 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

**SAR result with Body TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.15 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	<b>8.58 W/kg ± 17.0 % (k=2)</b>

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.41 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	<b>5.63 W/kg ± 16.5 % (k=2)</b>



**Appendix (Additional assessments outside the scope of SCS 0108)**

**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	56.4 $\Omega$ + 6.4 j $\Omega$
Return Loss	- 21.4 dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	50.3 $\Omega$ + 1.0 j $\Omega$
Return Loss	- 39.6 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.035 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	March 22, 2010



**DASY5 Validation Report for Head TSL**

Date: 14.08.2018

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN:1014**

Communication System: UID 0 - CW; Frequency: 750 MHz

Medium parameters used:  $f = 750$  MHz;  $\sigma = 0.89$  S/m;  $\epsilon_r = 40.9$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(10.22, 10.22, 10.22) @ 750 MHz; Calibrated: 30.12.2017
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 4.9 (front); Type: QD 00L P49 AA; Serial: 1001
- DASY52 52.10.1(1476); SEMCAD X 14.6.11(7439)

**Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 59.30 V/m; Power Drift = -0.04 dB

Peak SAR (extrapolated) = 3.10 W/kg


**SAR(1 g) = 2.05 W/kg; SAR(10 g) = 1.33 W/kg**

Maximum value of SAR (measured) = 2.76 W/kg

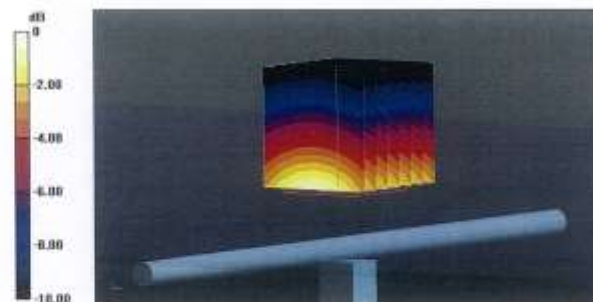

0 dB = 2.76 W/kg = 4.41 dBW/kg

**Impedance Measurement Plot for Head TSL**

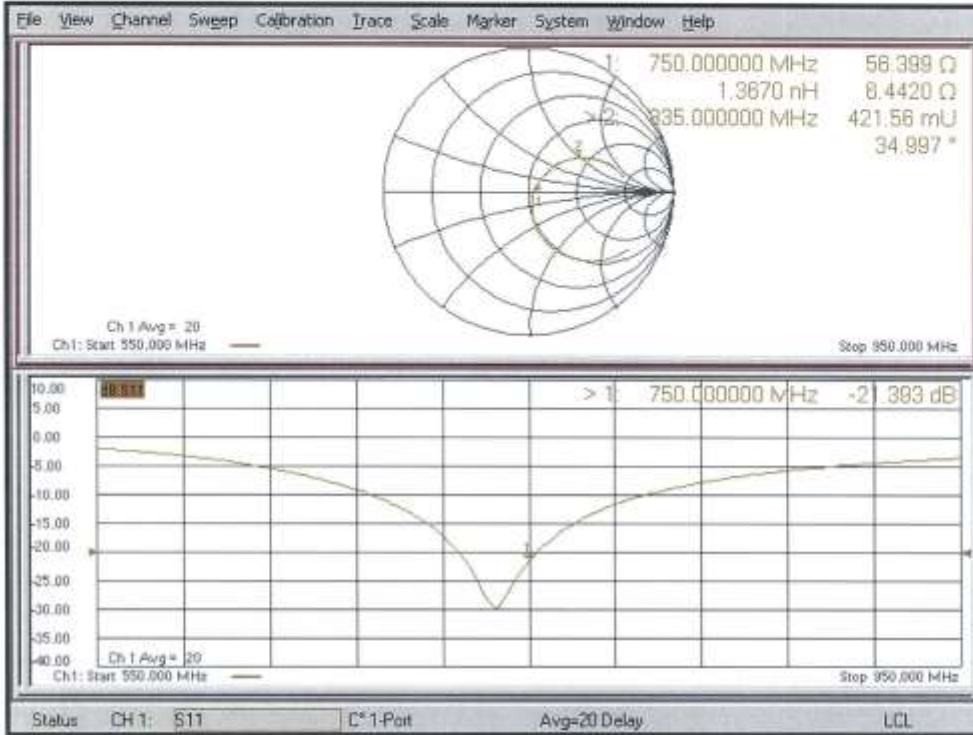

**DASY5 Validation Report for Body TSL**

Date: 14.08.2018

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN:1014**

Communication System: UID 0 - CW; Frequency: 750 MHz

Medium parameters used:  $f = 750 \text{ MHz}$ ;  $\sigma = 0.96 \text{ S/m}$ ;  $\epsilon_r = 55$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(10.19, 10.19, 10.19) @ 750 MHz; Calibrated: 30.12.2017
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 4.9 (Back); Type: QD 00R P49 AA; Serial: 1005
- DASY52 52.10.1(1476); SEMCAD X 14.6.11(7439)

**Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 57.92 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 3.20 W/kg

**SAR(1 g) = 2.15 W/kg; SAR(10 g) = 1.41 W/kg**


Maximum value of SAR (measured) = 2.85 W/kg

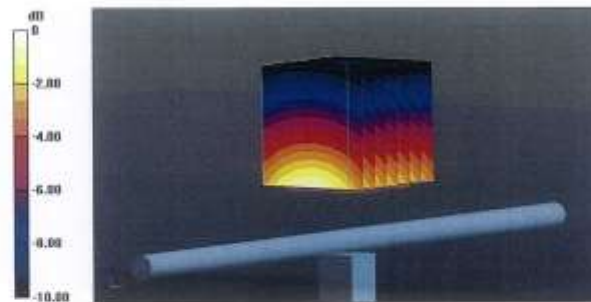

0 dB = 2.85 W/kg = 4.55 dBW/kg



**Impedance Measurement Plot for Body TSL**

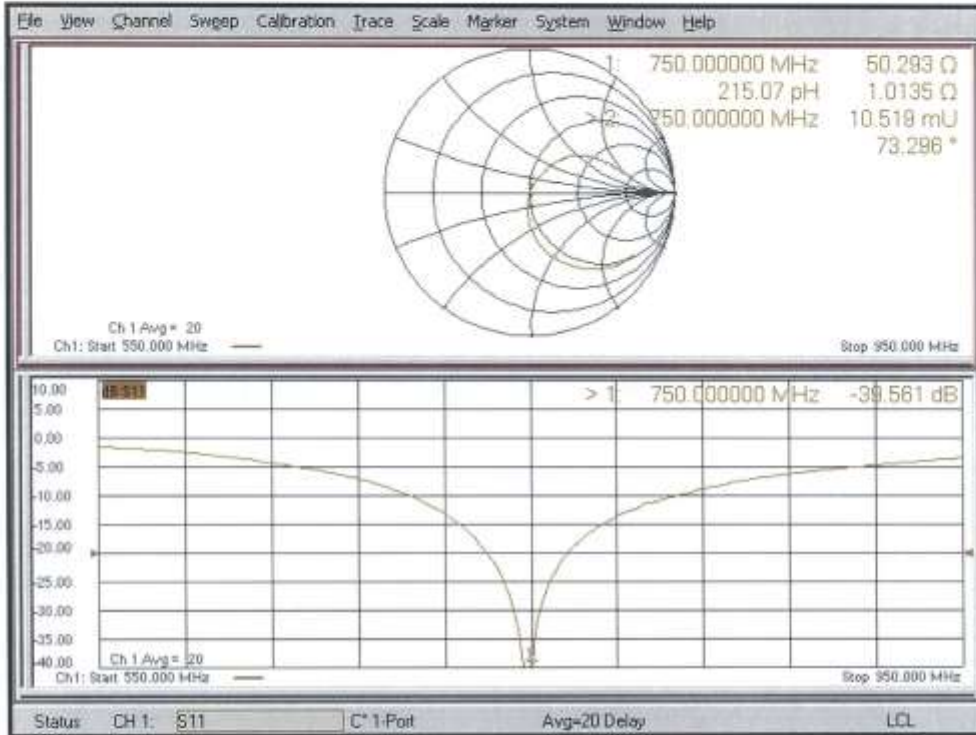

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**S** Service suisse d'étalonnage  
**C** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **HCT (Dymstec)**

Certificate No: **D835V2-4d165\_Sep18**

**CALIBRATION CERTIFICATE**

		검 재	단 당 자	화 인 자																																																								
Object	D835V2 - SN:4d165																																																											
Calibration procedure(s)	QA CAL-05.v10 Calibration procedure for dipole validation kits above 700 MHz	이위성명 SW 1개씩 일자 2018/10/05		김기 / 김우현 2018/10/5																																																								
Calibration date:	September 18, 2018																																																											
<p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity &lt; 70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter NRP</td> <td>SN: 104778</td> <td>04-Apr-18 (No. 217-02672/02673)</td> <td>Apr-19</td> </tr> <tr> <td>Power sensor NRP-Z91</td> <td>SN: 103244</td> <td>04-Apr-18 (No. 217-02672)</td> <td>Apr-19</td> </tr> <tr> <td>Power sensor NRP-Z91</td> <td>SN: 103245</td> <td>04-Apr-18 (No. 217-02673)</td> <td>Apr-19</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN: 5058 (20k)</td> <td>04-Apr-18 (No. 217-02682)</td> <td>Apr-19</td> </tr> <tr> <td>Type-N mismatch combination</td> <td>SN: 5047.2 / 06327</td> <td>04-Apr-18 (No. 217-02683)</td> <td>Apr-19</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN: 7349</td> <td>30-Dec-17 (No. EX3-7349_Dec17)</td> <td>Dec-18</td> </tr> <tr> <td>DAE4</td> <td>SN: 601</td> <td>26-Oct-17 (No. DAE4-601_Oct17)</td> <td>Oct-18</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Check Date (in house)</th> <th>Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>Power meter EPM-442A</td> <td>SN: GB37480704</td> <td>07-Oct-15 (in house check Oct-16)</td> <td>In house check: Oct-18</td> </tr> <tr> <td>Power sensor HP 8481A</td> <td>SN: US37292783</td> <td>07-Oct-15 (in house check Oct-16)</td> <td>In house check: Oct-18</td> </tr> <tr> <td>Power sensor HP 8481A</td> <td>SN: MY41092317</td> <td>07-Oct-15 (in house check Oct-16)</td> <td>In house check: Oct-18</td> </tr> <tr> <td>RF generator R&amp;S SMT-06</td> <td>SN: 100972</td> <td>15-Jun-15 (in house check Oct-16)</td> <td>In house check: Oct-18</td> </tr> <tr> <td>Network Analyzer Agilent E8358A</td> <td>SN: US41080477</td> <td>31-Mar-14 (in house check Oct-17)</td> <td>In house check: Oct-18</td> </tr> </tbody> </table>					Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration	Power meter NRP	SN: 104778	04-Apr-18 (No. 217-02672/02673)	Apr-19	Power sensor NRP-Z91	SN: 103244	04-Apr-18 (No. 217-02672)	Apr-19	Power sensor NRP-Z91	SN: 103245	04-Apr-18 (No. 217-02673)	Apr-19	Reference 20 dB Attenuator	SN: 5058 (20k)	04-Apr-18 (No. 217-02682)	Apr-19	Type-N mismatch combination	SN: 5047.2 / 06327	04-Apr-18 (No. 217-02683)	Apr-19	Reference Probe EX3DV4	SN: 7349	30-Dec-17 (No. EX3-7349_Dec17)	Dec-18	DAE4	SN: 601	26-Oct-17 (No. DAE4-601_Oct17)	Oct-18	Secondary Standards	ID #	Check Date (in house)	Scheduled Check	Power meter EPM-442A	SN: GB37480704	07-Oct-15 (in house check Oct-16)	In house check: Oct-18	Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-16)	In house check: Oct-18	Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-16)	In house check: Oct-18	RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-16)	In house check: Oct-18	Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-17)	In house check: Oct-18
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration																																																									
Power meter NRP	SN: 104778	04-Apr-18 (No. 217-02672/02673)	Apr-19																																																									
Power sensor NRP-Z91	SN: 103244	04-Apr-18 (No. 217-02672)	Apr-19																																																									
Power sensor NRP-Z91	SN: 103245	04-Apr-18 (No. 217-02673)	Apr-19																																																									
Reference 20 dB Attenuator	SN: 5058 (20k)	04-Apr-18 (No. 217-02682)	Apr-19																																																									
Type-N mismatch combination	SN: 5047.2 / 06327	04-Apr-18 (No. 217-02683)	Apr-19																																																									
Reference Probe EX3DV4	SN: 7349	30-Dec-17 (No. EX3-7349_Dec17)	Dec-18																																																									
DAE4	SN: 601	26-Oct-17 (No. DAE4-601_Oct17)	Oct-18																																																									
Secondary Standards	ID #	Check Date (in house)	Scheduled Check																																																									
Power meter EPM-442A	SN: GB37480704	07-Oct-15 (in house check Oct-16)	In house check: Oct-18																																																									
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-16)	In house check: Oct-18																																																									
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-16)	In house check: Oct-18																																																									
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-16)	In house check: Oct-18																																																									
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-17)	In house check: Oct-18																																																									
Calibrated by:	Name: Jeton Kastrati Function: Laboratory Technician	Signature:																																																										
Approved by:	Name: Katja Pokovic Function: Technical Manager	Signature:																																																										
Issued: September 18, 2018																																																												
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.																																																												

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**S** Service suisse d'étalonnage  
**C** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

**Glossary:**

TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORM x,y,z  
N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- e) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.



### Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.1
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz ± 1 MHz	

### Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.6 ± 6 %	0.91 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

### SAR result with Head TSL

<b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>	Condition	
SAR measured	250 mW input power	2.38 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>9.41 W/kg ± 17.0 % (k=2)</b>
<b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b>	condition	
SAR measured	250 mW input power	1.53 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>6.06 W/kg ± 16.5 % (k=2)</b>

### Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.2	0.97 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	55.4 ± 6 %	0.99 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

### SAR result with Body TSL

<b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Body TSL</b>	Condition	
SAR measured	250 mW input power	2.41 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	<b>9.50 W/kg ± 17.0 % (k=2)</b>
<b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Body TSL</b>	condition	
SAR measured	250 mW input power	1.57 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	<b>6.21 W/kg ± 16.5 % (k=2)</b>

**Appendix (Additional assessments outside the scope of SCS 0108)**

**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	50.5 $\Omega$ - 5.3 j $\Omega$
Return Loss	- 25.5 dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	45.5 $\Omega$ - 7.6 j $\Omega$
Return Loss	- 20.7 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.436 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	December 28, 2012

**DASY5 Validation Report for Head TSL**

Date: 18.09.2018

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:4d165**

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used:  $f = 835$  MHz;  $\sigma = 0.91$  S/m;  $\epsilon_r = 40.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(9.9, 9.9, 9.9) @ 835 MHz; Calibrated: 30.12.2017
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 4.9 (front); Type: QD 00L P49 AA; Serial: 1001
- DASY52 52.10.1(1476); SEMCAD X 14.6.11(7439)

**Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 65.64 V/m; Power Drift = 0.08 dB

Peak SAR (extrapolated) = 3.70 W/kg

SAR(1 g) = 2.38 W/kg; SAR(10 g) = 1.53 W/kg


Maximum value of SAR (measured) = 3.24 W/kg

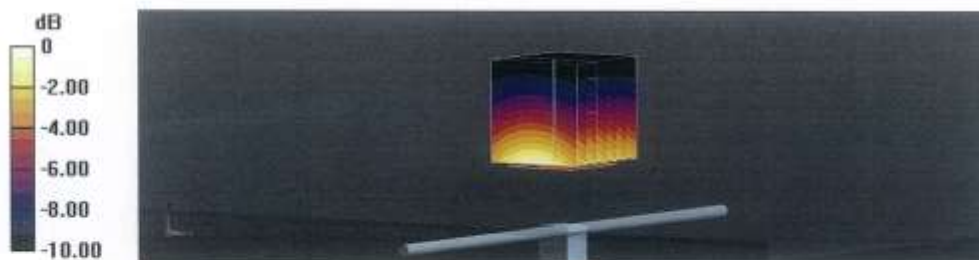

0 dB = 3.24 W/kg = 5.11 dBW/kg



**Impedance Measurement Plot for Head TSL**

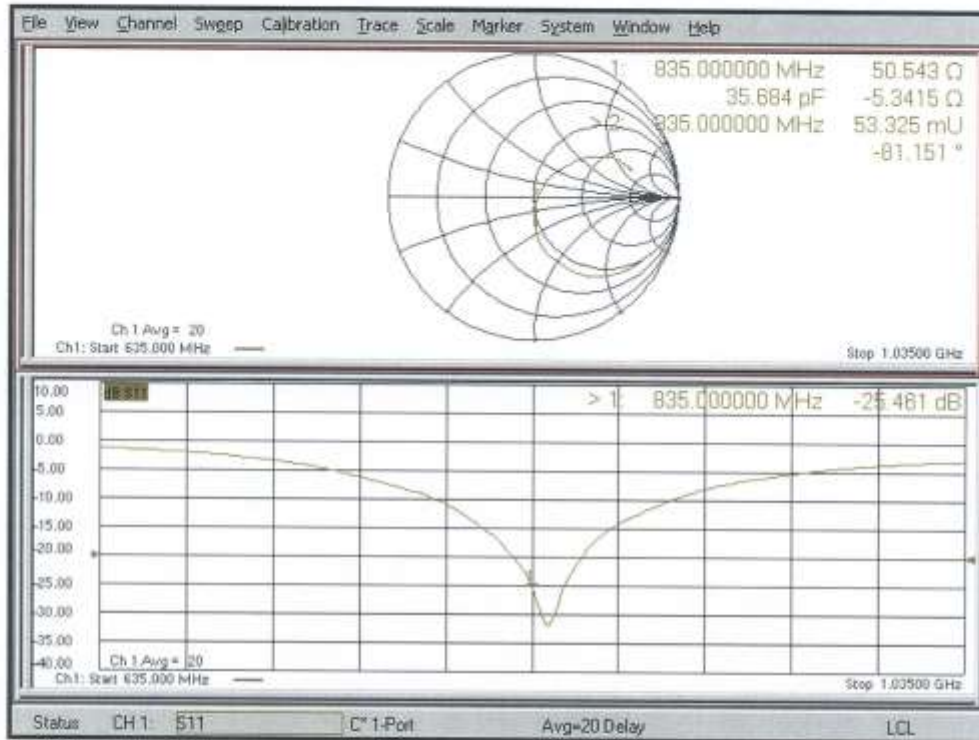

**DASY5 Validation Report for Body TSL**

Date: 18.09.2018

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:4d165**

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used:  $f = 835 \text{ MHz}$ ;  $\sigma = 0.99 \text{ S/m}$ ;  $\epsilon_r = 55.4$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(10.05, 10.05, 10.05) @ 835 MHz; Calibrated: 30.12.2017
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 4.9 (Back); Type: QD 00R P49 AA; Serial: 1005
- DASY52 52.10.1(1476); SEMCAD X 14.6.11(7439)

**Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 60.86 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 3.62 W/kg


**SAR(1 g) = 2.41 W/kg; SAR(10 g) = 1.57 W/kg**

Maximum value of SAR (measured) = 3.22 W/kg

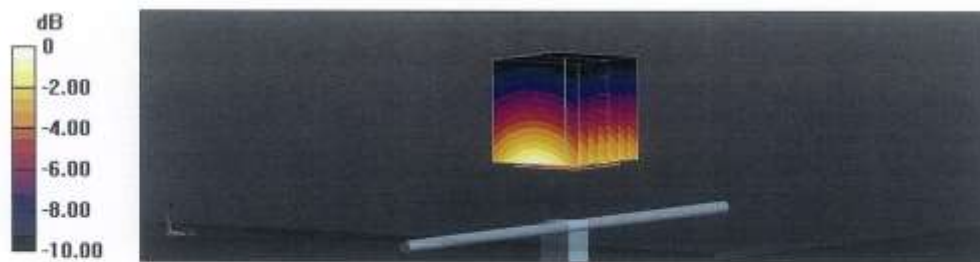

0 dB = 3.22 W/kg = 5.08 dBW/kg

**Impedance Measurement Plot for Body TSL**

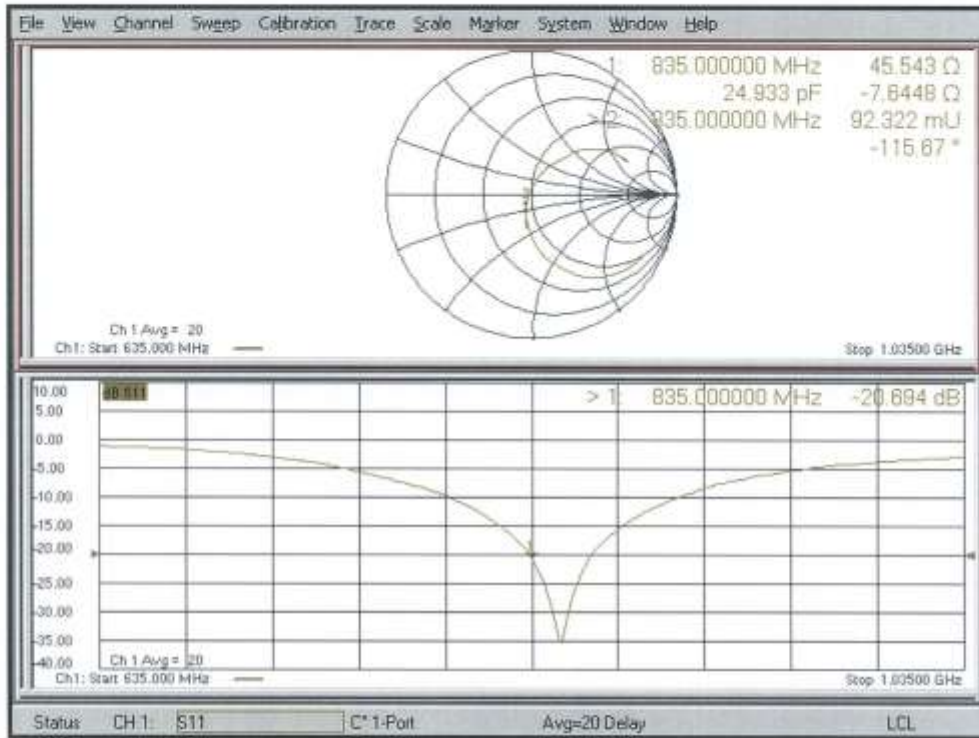

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **HCT (Dymstec)**

Certificate No: **D1800V2-2d006\_Nov17**

**CALIBRATION CERTIFICATE**

Object	D1800V2 - SN:2d006	<table border="1"> <tr> <td>설 재</td> <td>담당자 S.W. 김서준 2017. 11. 15</td> <td>확인자 HCT 인종남 2017. 12. 15</td> </tr> </table>		설 재	담당자 S.W. 김서준 2017. 11. 15	확인자 HCT 인종남 2017. 12. 15																																																					
설 재	담당자 S.W. 김서준 2017. 11. 15	확인자 HCT 인종남 2017. 12. 15																																																									
Calibration procedure(s)	QA CAL-05.v9 Calibration procedure for dipole validation kits above 700 MHz																																																										
Calibration date:	November 15, 2017																																																										
<p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity &lt; 70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter NRP</td> <td>SN: 104778</td> <td>04-Apr-17 (No. 217-02521/02522)</td> <td>Apr-18</td> </tr> <tr> <td>Power sensor NRP-Z91</td> <td>SN: 103244</td> <td>04-Apr-17 (No. 217-02521)</td> <td>Apr-18</td> </tr> <tr> <td>Power sensor NRP-Z91</td> <td>SN: 103245</td> <td>04-Apr-17 (No. 217-02522)</td> <td>Apr-18</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN: 5058 (20k)</td> <td>07-Apr-17 (No. 217-02528)</td> <td>Apr-18</td> </tr> <tr> <td>Type-N mismatch combination</td> <td>SN: 5047.2 / 06327</td> <td>07-Apr-17 (No. 217-02529)</td> <td>Apr-18</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN: 7349</td> <td>31-May-17 (No. EX3-7349_May17)</td> <td>May-18</td> </tr> <tr> <td>DAE4</td> <td>SN: 601</td> <td>26-Oct-17 (No. DAE4-601_Oct17)</td> <td>Oct-18</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Check Date (in house)</th> <th>Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>Power meter EPM-442A</td> <td>SN: G837480704</td> <td>07-Oct-15 (in house check Oct-16)</td> <td>In house check: Oct-18</td> </tr> <tr> <td>Power sensor HP 8481A</td> <td>SN: US37292783</td> <td>07-Oct-15 (in house check Oct-16)</td> <td>In house check: Oct-18</td> </tr> <tr> <td>Power sensor HP 8481A</td> <td>SN: MY41092317</td> <td>07-Oct-15 (in house check Oct-16)</td> <td>In house check: Oct-18</td> </tr> <tr> <td>RF generator R&amp;S SMT-06</td> <td>SN: 100972</td> <td>15-Jun-15 (in house check Oct-16)</td> <td>In house check: Oct-18</td> </tr> <tr> <td>Network Analyzer HP 8753E</td> <td>SN: US37390585</td> <td>18-Oct-01 (in house check Oct-17)</td> <td>In house check: Oct-18</td> </tr> </tbody> </table>				Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration	Power meter NRP	SN: 104778	04-Apr-17 (No. 217-02521/02522)	Apr-18	Power sensor NRP-Z91	SN: 103244	04-Apr-17 (No. 217-02521)	Apr-18	Power sensor NRP-Z91	SN: 103245	04-Apr-17 (No. 217-02522)	Apr-18	Reference 20 dB Attenuator	SN: 5058 (20k)	07-Apr-17 (No. 217-02528)	Apr-18	Type-N mismatch combination	SN: 5047.2 / 06327	07-Apr-17 (No. 217-02529)	Apr-18	Reference Probe EX3DV4	SN: 7349	31-May-17 (No. EX3-7349_May17)	May-18	DAE4	SN: 601	26-Oct-17 (No. DAE4-601_Oct17)	Oct-18	Secondary Standards	ID #	Check Date (in house)	Scheduled Check	Power meter EPM-442A	SN: G837480704	07-Oct-15 (in house check Oct-16)	In house check: Oct-18	Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-16)	In house check: Oct-18	Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-16)	In house check: Oct-18	RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-16)	In house check: Oct-18	Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-17)	In house check: Oct-18
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration																																																								
Power meter NRP	SN: 104778	04-Apr-17 (No. 217-02521/02522)	Apr-18																																																								
Power sensor NRP-Z91	SN: 103244	04-Apr-17 (No. 217-02521)	Apr-18																																																								
Power sensor NRP-Z91	SN: 103245	04-Apr-17 (No. 217-02522)	Apr-18																																																								
Reference 20 dB Attenuator	SN: 5058 (20k)	07-Apr-17 (No. 217-02528)	Apr-18																																																								
Type-N mismatch combination	SN: 5047.2 / 06327	07-Apr-17 (No. 217-02529)	Apr-18																																																								
Reference Probe EX3DV4	SN: 7349	31-May-17 (No. EX3-7349_May17)	May-18																																																								
DAE4	SN: 601	26-Oct-17 (No. DAE4-601_Oct17)	Oct-18																																																								
Secondary Standards	ID #	Check Date (in house)	Scheduled Check																																																								
Power meter EPM-442A	SN: G837480704	07-Oct-15 (in house check Oct-16)	In house check: Oct-18																																																								
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-16)	In house check: Oct-18																																																								
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-16)	In house check: Oct-18																																																								
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-16)	In house check: Oct-18																																																								
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-17)	In house check: Oct-18																																																								
Calibrated by:	Name: Michael Weber Function: Laboratory Technician	Signature:																																																									
Approved by:	Name: Kalja Pokovic Function: Technical Manager	Signature:																																																									
<p>Issued: November 15, 2017</p>																																																											
<p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p>																																																											



**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

**Glossary:**

TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORM x,y,z  
N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- e) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.0
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1800 MHz ± 1 MHz	

**Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.7 ± 6 %	1.38 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

**SAR result with Head TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.63 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>38.8 W/kg ± 17.0 % (k=2)</b>

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.01 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>20.1 W/kg ± 16.5 % (k=2)</b>

**Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	52.5 ± 6 %	1.52 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

**SAR result with Body TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.75 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	<b>38.9 W/kg ± 17.0 % (k=2)</b>

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.09 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	<b>20.3 W/kg ± 16.5 % (k=2)</b>

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with Head TSL**

Impedance, transformed to feed point	46.6 $\Omega$ - 7.3 j $\Omega$
Return Loss	- 21.7 dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	42.9 $\Omega$ - 6.0 j $\Omega$
Return Loss	- 20.0 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.208 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	July 23, 2001

**DASY5 Validation Report for Head TSL**

Date: 15.11.2017

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN:2d006**

Communication System: UID 0 - CW; Frequency: 1800 MHz

Medium parameters used:  $f = 1800$  MHz;  $\sigma = 1.38$  S/m;  $\epsilon_r = 39.7$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.56, 8.56, 8.56); Calibrated: 31.05.2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

**Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 108.6 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 18.2 W/kg


SAR(1 g) = 9.63 W/kg; SAR(10 g) = 5.01 W/kg

Maximum value of SAR (measured) = 14.9 W/kg

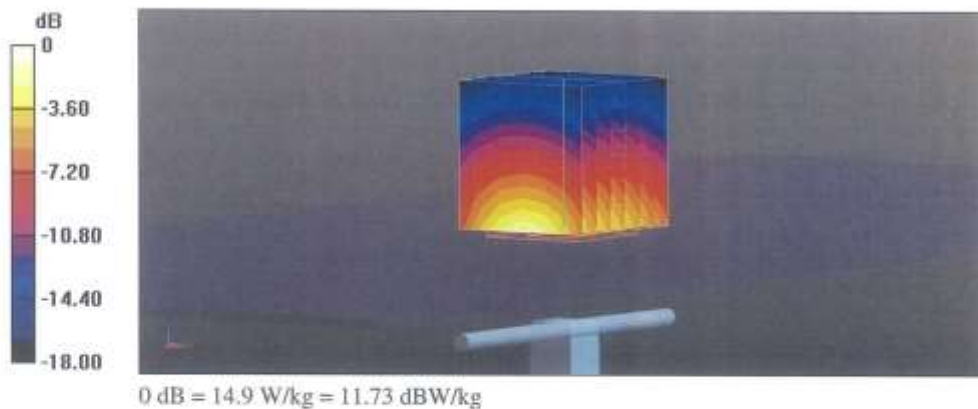



Impedance Measurement Plot for Head TSL

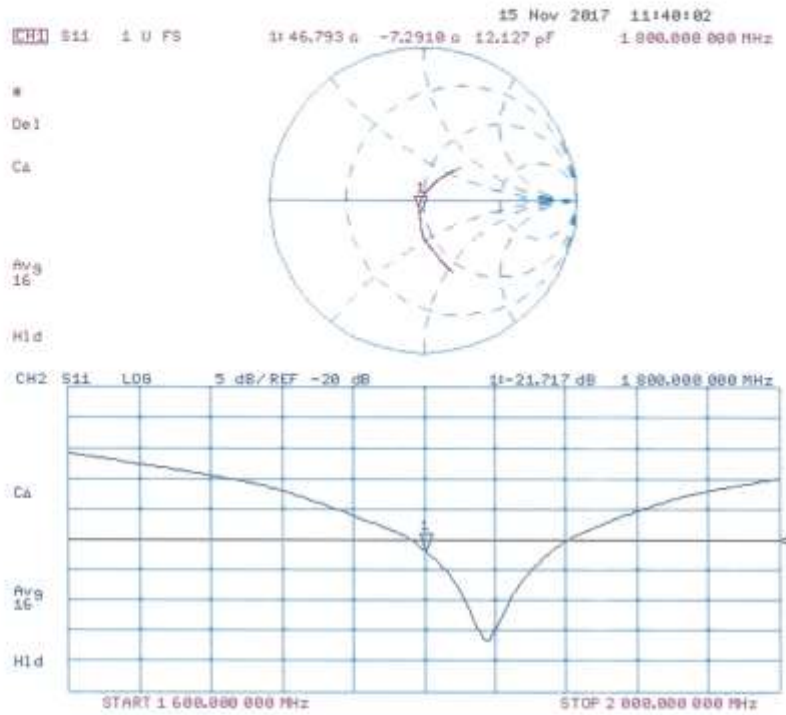

**DASY5 Validation Report for Body TSL**

Date: 15.11.2017

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN:2d006**

Communication System: UID 0 - CW; Frequency: 1800 MHz

Medium parameters used:  $f = 1800$  MHz;  $\sigma = 1.52$  S/m;  $\epsilon_r = 52.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.38, 8.38, 8.38); Calibrated: 31.05.2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

**Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 102.8 V/m; Power Drift = -0.09 dB

Peak SAR (extrapolated) = 17.5 W/kg


**SAR(1 g) = 9.75 W/kg; SAR(10 g) = 5.09 W/kg**

Maximum value of SAR (measured) = 14.5 W/kg

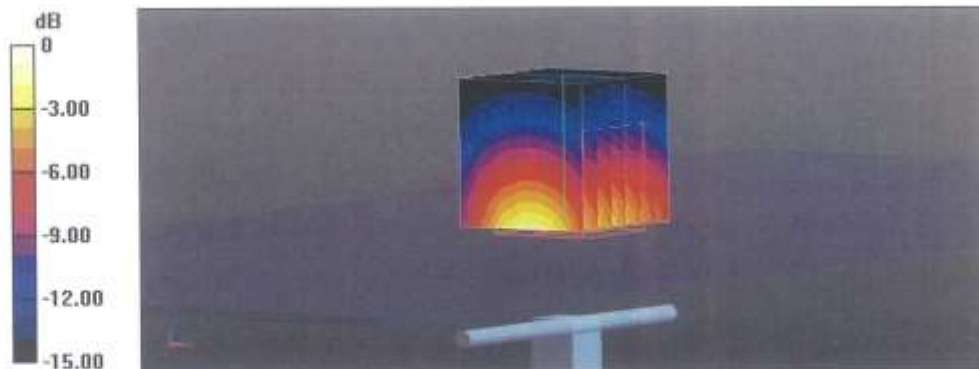

0 dB = 14.5 W/kg = 11.61 dBW/kg

Impedance Measurement Plot for Body TSL

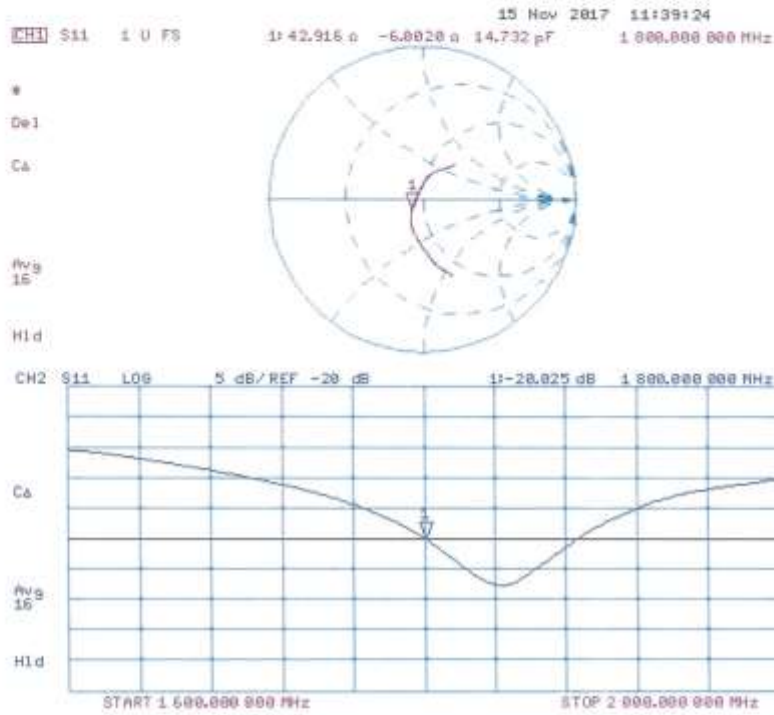

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **HCT (Dymstec)**

Certificate No: **D1900V2-5d061\_Mar18**

CALIBRATION CERTIFICATE																																																											
Object:	D1900V2 - SN:5d061																																																										
Calibration procedure(s):	QA CAL-05.v10 Calibration procedure for dipole validation kits above 700 MHz																																																										
Calibration date:	March 15, 2018																																																										
<table border="1"> <tr> <td>결</td> <td>담당자</td> <td>확인자</td> </tr> <tr> <td>제</td> <td><i>[Signature]</i></td> <td><i>[Signature]</i></td> </tr> </table>				결	담당자	확인자	제	<i>[Signature]</i>	<i>[Signature]</i>																																																		
결	담당자	확인자																																																									
제	<i>[Signature]</i>	<i>[Signature]</i>																																																									
<p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity &lt; 70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter NRP</td> <td>SN: 104778</td> <td>04-Apr-17 (No. 217-02521/02522)</td> <td>Apr-18</td> </tr> <tr> <td>Power sensor NRP-Z91</td> <td>SN: 103244</td> <td>04-Apr-17 (No. 217-02521)</td> <td>Apr-18</td> </tr> <tr> <td>Power sensor NRP-Z91</td> <td>SN: 103245</td> <td>04-Apr-17 (No. 217-02522)</td> <td>Apr-18</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN: 5068 (20k)</td> <td>07-Apr-17 (No. 217-02528)</td> <td>Apr-18</td> </tr> <tr> <td>Type-N mismatch combination</td> <td>SN: 5047.2 / 06327</td> <td>07-Apr-17 (No. 217-02529)</td> <td>Apr-18</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN: 7349</td> <td>30-Dec-17 (No. EX3-7349_Dec17)</td> <td>Dec-18</td> </tr> <tr> <td>DAE4</td> <td>SN: 601</td> <td>26-Oct-17 (No. DAE4-601_Oct17)</td> <td>Oct-18</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Check Date (in house)</th> <th>Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>Power meter EPM-442A</td> <td>SN: GB37480704</td> <td>07-Oct-15 (in house check Oct-16)</td> <td>In house check: Oct-18</td> </tr> <tr> <td>Power sensor HP 8481A</td> <td>SN: US37292783</td> <td>07-Oct-15 (in house check Oct-16)</td> <td>In house check: Oct-18</td> </tr> <tr> <td>Power sensor HP 8481A</td> <td>SN: MY41092317</td> <td>07-Oct-15 (in house check Oct-16)</td> <td>In house check: Oct-18</td> </tr> <tr> <td>RF generator R&amp;S SMT-06</td> <td>SN: 100972</td> <td>15-Jun-15 (in house check Oct-16)</td> <td>In house check: Oct-18</td> </tr> <tr> <td>Network Analyzer HP 8753E</td> <td>SN: US37390585</td> <td>18-Oct-01 (in house check Oct-17)</td> <td>In house check: Oct-18</td> </tr> </tbody> </table>				Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration	Power meter NRP	SN: 104778	04-Apr-17 (No. 217-02521/02522)	Apr-18	Power sensor NRP-Z91	SN: 103244	04-Apr-17 (No. 217-02521)	Apr-18	Power sensor NRP-Z91	SN: 103245	04-Apr-17 (No. 217-02522)	Apr-18	Reference 20 dB Attenuator	SN: 5068 (20k)	07-Apr-17 (No. 217-02528)	Apr-18	Type-N mismatch combination	SN: 5047.2 / 06327	07-Apr-17 (No. 217-02529)	Apr-18	Reference Probe EX3DV4	SN: 7349	30-Dec-17 (No. EX3-7349_Dec17)	Dec-18	DAE4	SN: 601	26-Oct-17 (No. DAE4-601_Oct17)	Oct-18	Secondary Standards	ID #	Check Date (in house)	Scheduled Check	Power meter EPM-442A	SN: GB37480704	07-Oct-15 (in house check Oct-16)	In house check: Oct-18	Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-16)	In house check: Oct-18	Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-16)	In house check: Oct-18	RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-16)	In house check: Oct-18	Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-17)	In house check: Oct-18
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration																																																								
Power meter NRP	SN: 104778	04-Apr-17 (No. 217-02521/02522)	Apr-18																																																								
Power sensor NRP-Z91	SN: 103244	04-Apr-17 (No. 217-02521)	Apr-18																																																								
Power sensor NRP-Z91	SN: 103245	04-Apr-17 (No. 217-02522)	Apr-18																																																								
Reference 20 dB Attenuator	SN: 5068 (20k)	07-Apr-17 (No. 217-02528)	Apr-18																																																								
Type-N mismatch combination	SN: 5047.2 / 06327	07-Apr-17 (No. 217-02529)	Apr-18																																																								
Reference Probe EX3DV4	SN: 7349	30-Dec-17 (No. EX3-7349_Dec17)	Dec-18																																																								
DAE4	SN: 601	26-Oct-17 (No. DAE4-601_Oct17)	Oct-18																																																								
Secondary Standards	ID #	Check Date (in house)	Scheduled Check																																																								
Power meter EPM-442A	SN: GB37480704	07-Oct-15 (in house check Oct-16)	In house check: Oct-18																																																								
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-16)	In house check: Oct-18																																																								
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-16)	In house check: Oct-18																																																								
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-16)	In house check: Oct-18																																																								
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-17)	In house check: Oct-18																																																								
Calibrated by:	Name Claudio Leubler	Function Laboratory Technician	Signature <i>[Signature]</i>																																																								
Approved by:	Katja Pokovic	Technical Manager	<i>[Signature]</i>																																																								
<p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> <p style="text-align: right;">Issued: March 15, 2018</p>																																																											



**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

**Glossary:**

TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORM x,y,z  
N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- e) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

### Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.0
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

### Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.5 ± 6 %	1.37 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.68 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	40.1 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.19 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.0 W/kg ± 16.5 % (k=2)

### Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	55.2 ± 6 %	1.47 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

### SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.64 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	39.6 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.14 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	20.9 W/kg ± 16.5 % (k=2)

**Appendix (Additional assessments outside the scope of SCS 0108)**

**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	51.4 $\Omega$ + 8.2 j $\Omega$
Return Loss	- 24.0 dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	47.7 $\Omega$ + 4.8 j $\Omega$
Return Loss	- 25.1 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.194 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	December 10, 2004

**DASY5 Validation Report for Head TSL**

Date: 15.03.2018

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d061**

Communication System: UID 0 - CW; Frequency: 1900 MHz

Medium parameters used:  $f = 1900$  MHz;  $\sigma = 1.37$  S/m;  $\epsilon_r = 40.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.18, 8.18, 8.18); Calibrated: 30.12.2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

**Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 107.8 V/m; Power Drift = -0.09 dB

Peak SAR (extrapolated) = 18.3 W/kg


SAR(1 g) = 9.88 W/kg; SAR(10 g) = 5.19 W/kg

Maximum value of SAR (measured) = 15.1 W/kg

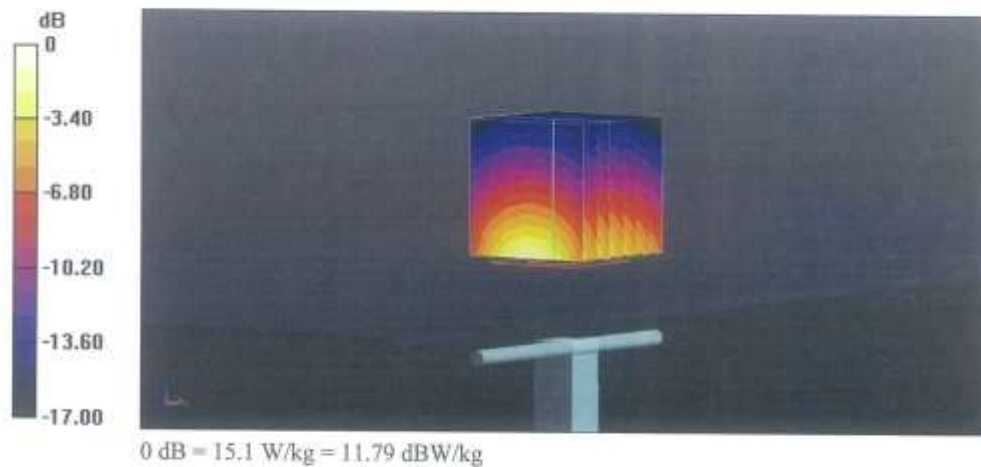



Impedance Measurement Plot for Head TSL

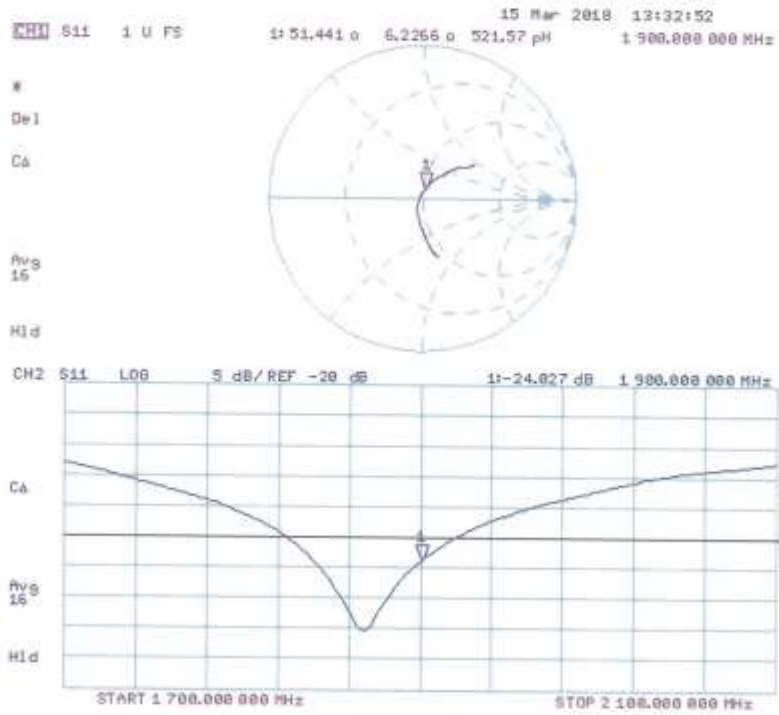

**DASY5 Validation Report for Body TSL**

Date: 15.03.2018

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d061**

Communication System: UID 0 - CW; Frequency: 1900 MHz

Medium parameters used:  $f = 1900$  MHz;  $\sigma = 1.47$  S/m;  $\epsilon_r = 55.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.15, 8.15, 8.15); Calibrated: 30.12.2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

**Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 101.9 V/m; Power Drift = -0.04 dB


Peak SAR (extrapolated) = 17.1 W/kg

SAR(1 g) = 9.64 W/kg; SAR(10 g) = 5.14 W/kg

Maximum value of SAR (measured) = 13.9 W/kg

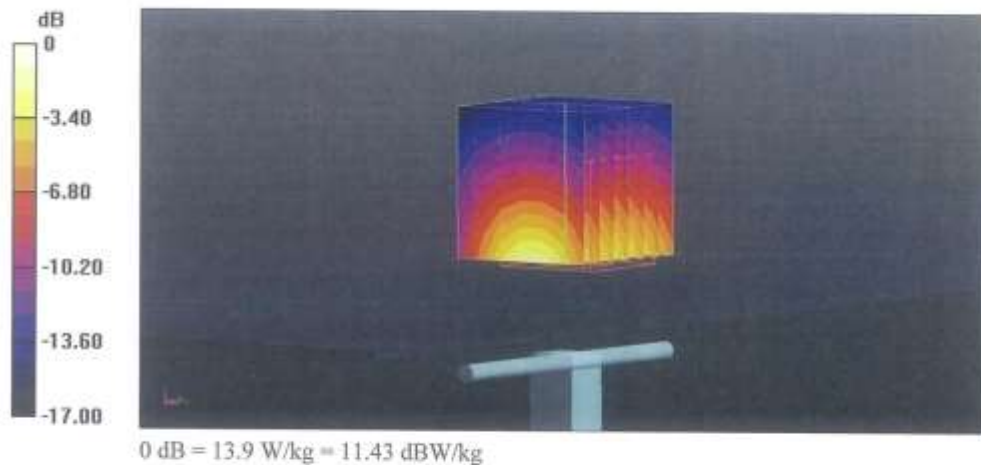

Impedance Measurement Plot for Body TSL

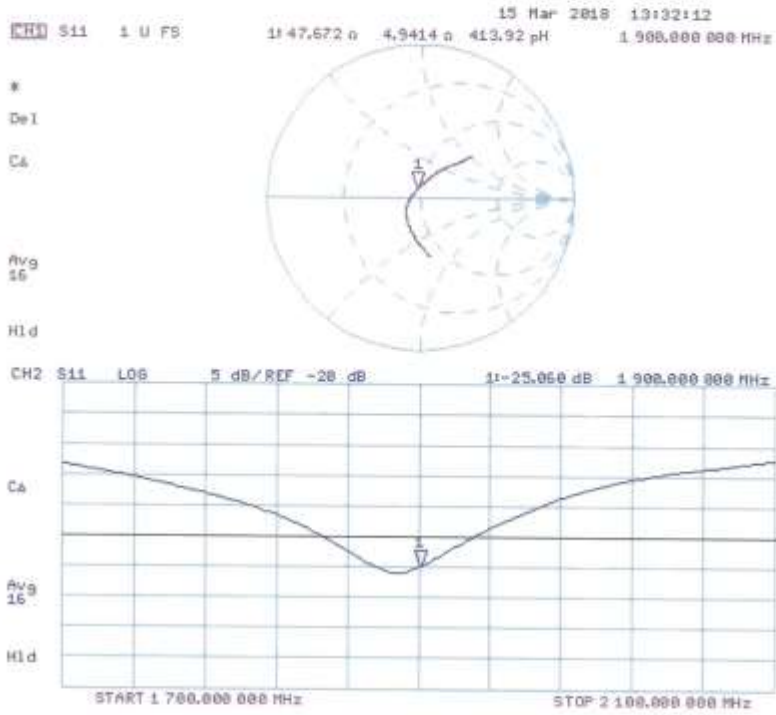

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**S** Service suisse d'étalonnage  
**C** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client: **HCT (Dymstec)**

Certificate No: **D2450V2-965\_Feb18**

**CALIBRATION CERTIFICATE**

Object: **D2450V2 - SN:965**

Calibration procedure(s): **QA CAL-05.v9  
Calibration procedure for dipole validation kits above 700 MHz.**

Calibration date: **February 16, 2018.**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-17 (No. 217-02521/02522)	Apr-18
Power sensor NRP-Z91	SN: 103244	04-Apr-17 (No. 217-02521)	Apr-18
Power sensor NRP-Z91	SN: 103245	04-Apr-17 (No. 217-02522)	Apr-18
Reference 20 dB Attenuator	SN: 5058 (20k)	07-Apr-17 (No. 217-02528)	Apr-18
Type-N mismatch combination	SN: 5047.2 / 06327	07-Apr-17 (No. 217-02529)	Apr-18
Reference Probe EX3DV4	SN: 7349	30-Dec-17 (No. EX3-7349_Dec17)	Dec-18
DAE4	SN: 601	26-Oct-17 (No. DAE4-601_Oct17)	Oct-18
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: GB37480704	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-16)	In house check: Oct-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-17)	In house check: Oct-18

Calibrated by: **Michael Weber** (Name), **Laboratory Technician** (Function), *M. Weber* (Signature)

Approved by: **Katja Pokovic** (Name), **Technical Manager** (Function), *K. Pokovic* (Signature)

Issued: February 19, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

결	담당자	확인자
재	<i>X Jim</i>	<i>JH</i>
확인/일	6W 183.06	6J 183.06
일 자	2018 1 23.06	2018 1 23.06



**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 0108**

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

**Glossary:**

TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORM x,y,z  
N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- e) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.0
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

**Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	37.9 ± 6 %	1.87 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

**SAR result with Head TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.1 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	51.1 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.07 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.9 W/kg ± 16.5 % (k=2)

**Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	51.4 ± 6 %	2.04 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

**SAR result with Body TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	12.9 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	50.2 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.98 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	23.6 W/kg ± 16.5 % (k=2)

**Appendix (Additional assessments outside the scope of SCS 0108)**

**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	54.9 $\Omega$ + 4.2 j $\Omega$
Return Loss	- 24.2 dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	50.9 $\Omega$ + 6.3 j $\Omega$
Return Loss	- 24.0 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.163 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	November 19, 2014

**DASY5 Validation Report for Head TSL**

Date: 16.02.2018

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 965**

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.87$  S/m;  $\epsilon_r = 37.9$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.88, 7.88, 7.88); Calibrated: 30.12.2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

**Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 112.7 V/m; Power Drift = -0.05 dB

Peak SAR (extrapolated) = 26.2 W/kg


**SAR(1 g) = 13.1 W/kg; SAR(10 g) = 6.07 W/kg**

Maximum value of SAR (measured) = 20.7 W/kg

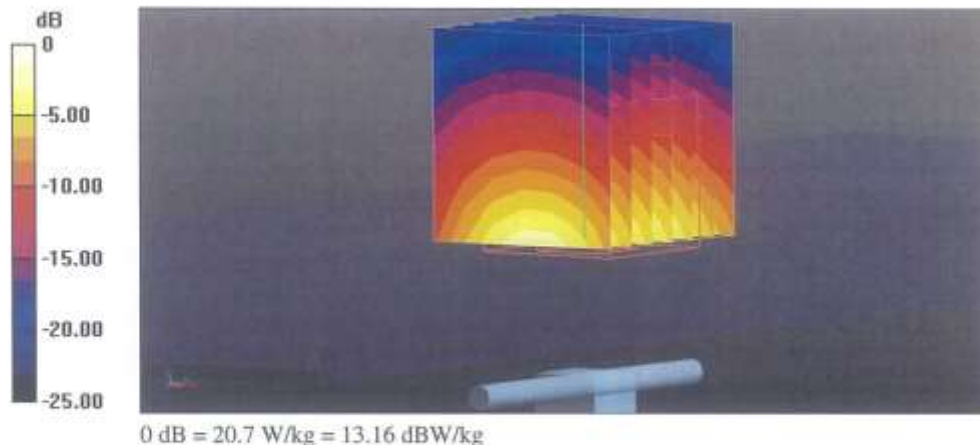



**Impedance Measurement Plot for Head TSL**

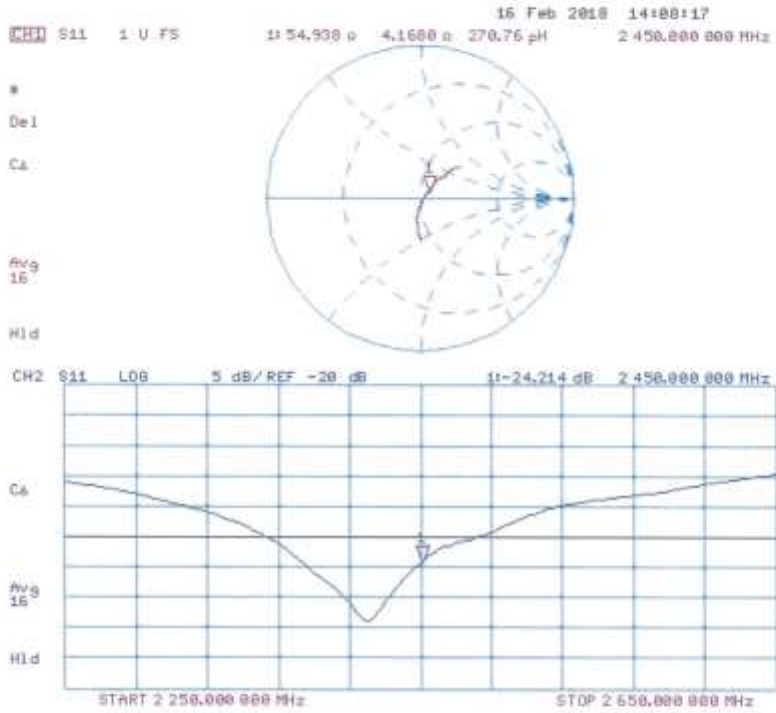

**DASY5 Validation Report for Body TSL**

Date: 16.02.2018

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 965**

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 2.04$  S/m;  $\epsilon_r = 51.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.01, 8.01, 8.01); Calibrated: 30.12.2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

**Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 104.7 V/m; Power Drift = -0.03 dB


Peak SAR (extrapolated) = 25.8 W/kg

**SAR(1 g) = 12.9 W/kg; SAR(10 g) = 5.98 W/kg**

Maximum value of SAR (measured) = 20.0 W/kg

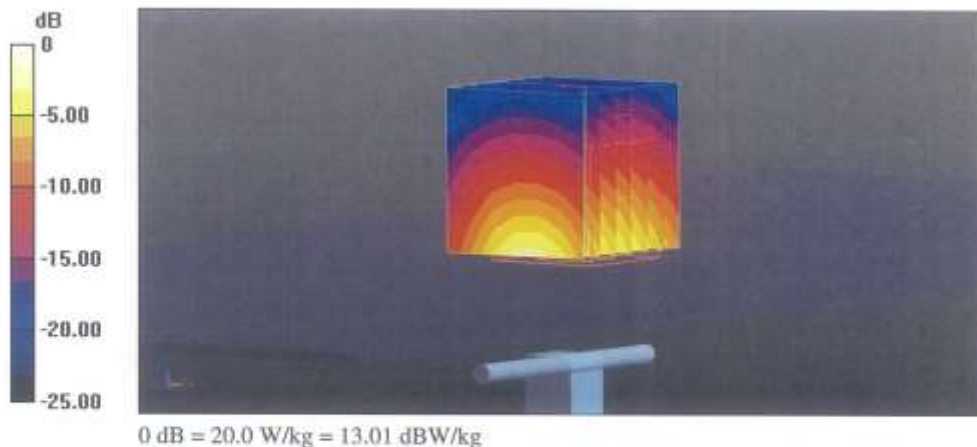

Impedance Measurement Plot for Body TSL

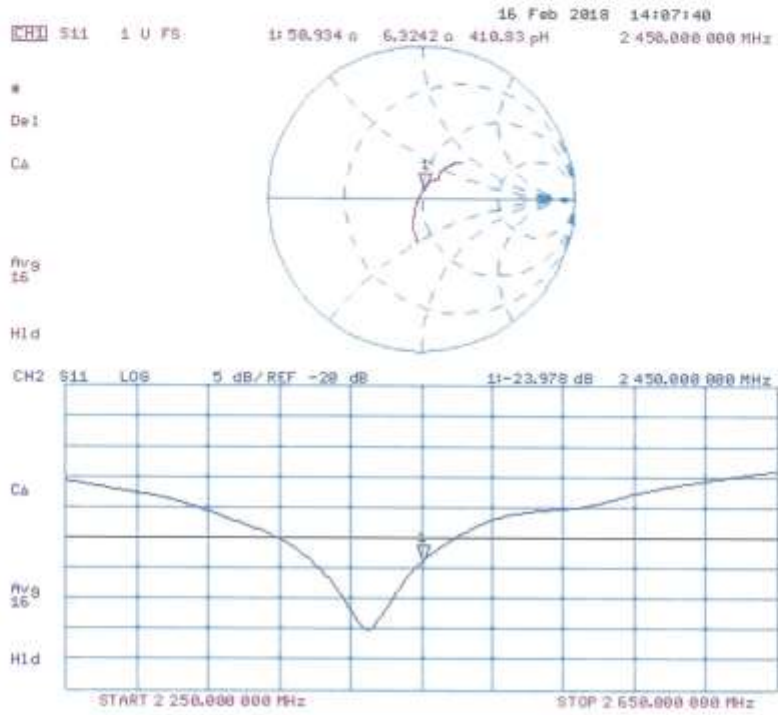

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**S** Service suisse d'étalonnage  
**C** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **HCT (Dymstec)**

Certificate No: **D2600V2-1106\_Dec17**

**CALIBRATION CERTIFICATE**

Object **D2600V2 - SN:1106**

Calibration procedure(s) **QA CAL-05.v9  
Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **December 15, 2017**

결 재	담당자 <i>[Signature]</i> 2018. 01. 04 김정민	확인자 <i>[Signature]</i> 2018. 01. 04 김정민
--------	--	--

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-17 (No. 217-02521/02522)	Apr-18
Power sensor NRP-Z91	SN: 103244	04-Apr-17 (No. 217-02521)	Apr-18
Power sensor NRP-Z91	SN: 103245	04-Apr-17 (No. 217-02522)	Apr-18
Reference 20 dB Attenuator	SN: 5058 (20K)	07-Apr-17 (No. 217-02528)	Apr-18
Type-N mismatch combination	SN: 5047.2 / 06327	07-Apr-17 (No. 217-02529)	Apr-18
Reference Probe EX3DV4	SN: 7349	31-May-17 (No. EX3-7349_May17)	May-18
DAE4	SN: 601	26-Oct-17 (No. DAE4-601_Oct17)	Oct-18
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: GB37480704	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-16)	In house check: Oct-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-17)	In house check: Oct-18

Calibrated by: **Leif Klysner** (Name), **Laboratory Technician** (Function), *[Signature]* (Signature)

Approved by: **Katja Pokovic** (Name), **Technical Manager** (Function), *[Signature]* (Signature)

Issued: December 18, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

**Glossary:**

TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORM x,y,z  
N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- e) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.0
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2600 MHz ± 1 MHz	

**Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.0	1.96 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	37.1 ± 6 %	2.03 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

**SAR result with Head TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	14.5 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>56.4 W/kg ± 17.0 % (k=2)</b>

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.35 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>25.0 W/kg ± 16.5 % (k=2)</b>

**Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.5	2.16 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	51.0 ± 6 %	2.22 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

**SAR result with Body TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.9 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	<b>54.6 W/kg ± 17.0 % (k=2)</b>

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	6.13 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	<b>24.2 W/kg ± 16.5 % (k=2)</b>

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with Head TSL**

Impedance, transformed to feed point	47.8 $\Omega$ - 8.3 j $\Omega$
Return Loss:	- 21.2 dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	44.7 $\Omega$ - 5.9 j $\Omega$
Return Loss:	- 21.6 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.150 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the 'Measurement Conditions' paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	February 18, 2015

**DASY5 Validation Report for Head TSL**

Date: 15.12.2017

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2600 MHz; Type: D2600V2; Serial: D2600V2 - SN: 1106**

Communication System: UID 0 - CW; Frequency: 2600 MHz

Medium parameters used:  $f = 2600$  MHz;  $\sigma = 2.03$  S/m;  $\epsilon_r = 37.1$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.96, 7.96, 7.96); Calibrated: 31.05.2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

**Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 113.0 V/m; Power Drift = -0.07 dB

Peak SAR (extrapolated) = 32.1 W/kg


SAR(1 g) = 14.5 W/kg; SAR(10 g) = 6.35 W/kg

Maximum value of SAR (measured) = 23.6 W/kg

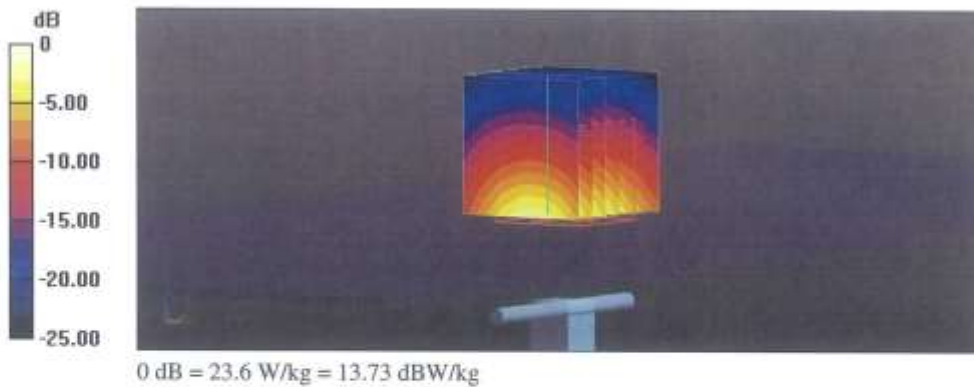



Impedance Measurement Plot for Head TSL

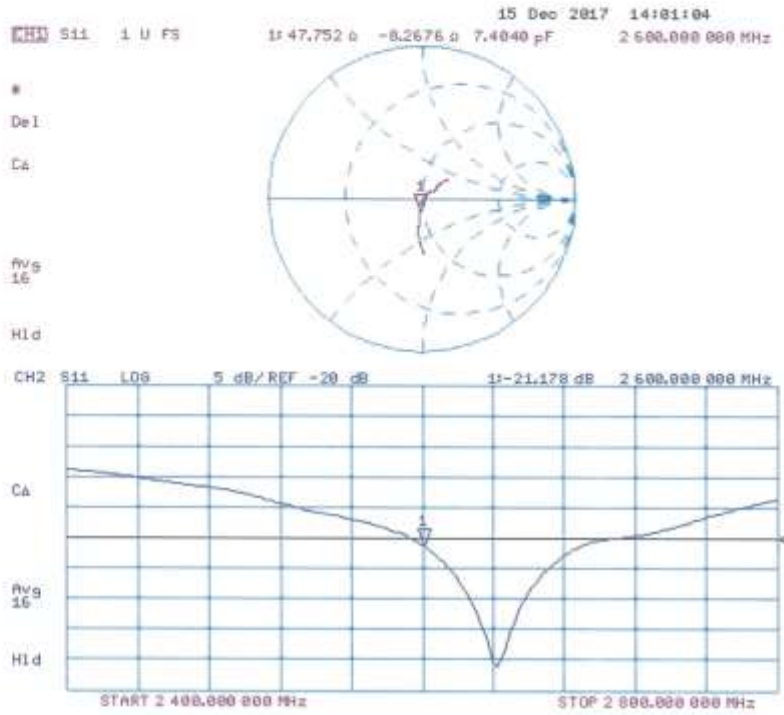

**DASY5 Validation Report for Body TSL**

Date: 15.12.2017

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2600 MHz; Type: D2600V2; Serial: D2600V2 - SN: 1106**

Communication System: UID 0 - CW; Frequency: 2600 MHz

Medium parameters used:  $f = 2600$  MHz;  $\sigma = 2.22$  S/m;  $\epsilon_r = 51$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.94, 7.94, 7.94); Calibrated: 31.05.2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

**Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 104.4 V/m; Power Drift = -0.08 dB


Peak SAR (extrapolated) = 29.9 W/kg

**SAR(1 g) = 13.9 W/kg; SAR(10 g) = 6.13 W/kg**

Maximum value of SAR (measured) = 22.4 W/kg

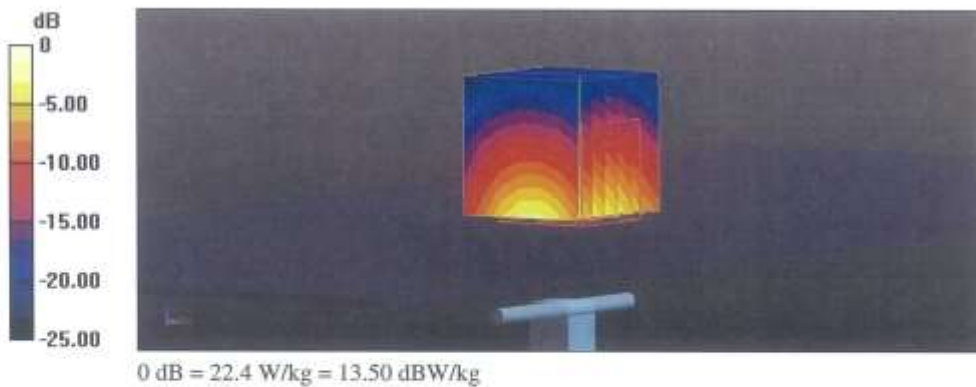

Impedance Measurement Plot for Body TSL

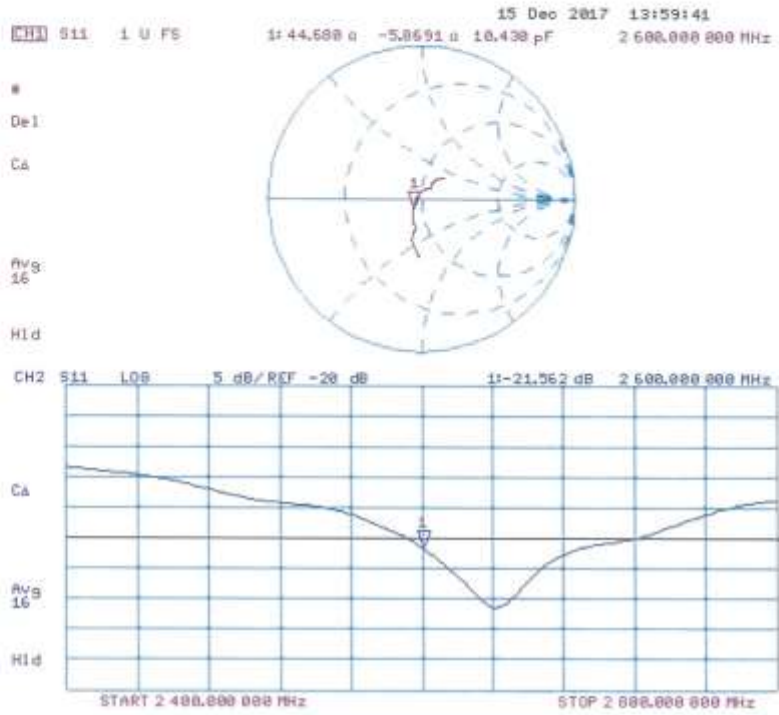

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**S** Service suisse d'étalonnage  
**C** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **HCT (Dymstec)**

Certificate No: **D5GHzV2-1107\_Dec17**

**CALIBRATION CERTIFICATE**

Object	D5GHzV2 - SN:1107
Calibration procedure(s)	QA CAL-22.v2 Calibration procedure for dipole validation kits between 3-6 GHz
Calibration date:	December 14, 2017

결 재	담당자  2018. 01. 04 SW 강지호	확인자  2018. 1. 4 61 김동진
--------	-----------------------------------	---------------------------------

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104776	04-Apr-17 (No. 217-02521/02522)	Apr-18
Power sensor NRP-Z91	SN: 103244	04-Apr-17 (No. 217-02521)	Apr-18
Power sensor NRP-Z91	SN: 103245	04-Apr-17 (No. 217-02522)	Apr-18
Reference 20 dB Attenuator	SN: 5056 (20k)	07-Apr-17 (No. 217-02528)	Apr-18
Type-N mismatch combination	SN: 5047.2 / 06327	07-Apr-17 (No. 217-02529)	Apr-18
Reference Probe EX3DV4	SN: 3503	31-Dec-16 (No. EX3-3503_Dec16)	Dec-17
DAE4	SN: 601	26-Oct-17 (No. DAE4-601_Oct17)	Oct-18

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: GB37480704	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-16)	In house check: Oct-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-17)	In house check: Oct-18

Calibrated by:	Name Michael Weber	Function Laboratory Technician	Signature 
----------------	-----------------------	-----------------------------------	---------------

Approved by:	Name Katja Pokovic	Function Technical Manager	Signature 
--------------	-----------------------	-------------------------------	---------------

Issued: December 14, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

**Glossary:**

TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORM x,y,z  
N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- e) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.0
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	5250 MHz ± 1 MHz 5600 MHz ± 1 MHz 5750 MHz ± 1 MHz	

**Head TSL parameters at 5250 MHz**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.9	4.71 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.7 ± 6 %	4.56 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

**SAR result with Head TSL at 5250 MHz**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.15 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>81.3 W/kg ± 19.9 % (k=2)</b>

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.34 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>23.3 W/kg ± 19.5 % (k=2)</b>

**Head TSL parameters at 5600 MHz**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.2 ± 6 %	4.91 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Head TSL at 5600 MHz**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.43 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>84.0 W / kg ± 19.9 % (k=2)</b>

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.41 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>24.0 W/kg ± 19.5 % (k=2)</b>

**Head TSL parameters at 5750 MHz**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.4	5.22 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.0 ± 6 %	5.07 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Head TSL at 5750 MHz**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.09 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>80.6 W/kg ± 19.9 % (k=2)</b>

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.30 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>22.9 W/kg ± 19.5 % (k=2)</b>

**Body TSL parameters at 5250 MHz**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.9	5.36 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	47.1 ± 6 %	5.51 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Body TSL at 5250 MHz**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.79 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	77.4 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.17 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	21.5 W/kg ± 19.5 % (k=2)

**Body TSL parameters at 5600 MHz**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.5	5.77 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	46.5 ± 6 %	5.97 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Body TSL at 5600 MHz**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	8.09 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	80.3 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.26 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	22.4 W/kg ± 19.5 % (k=2)



**Body TSL parameters at 5750 MHz**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.3	5.94 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	46.2 ± 6 %	6.18 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Body TSL at 5750 MHz**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.65 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	75.9 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.13 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	21.1 W/kg ± 19.5 % (k=2)

**Appendix (Additional assessments outside the scope of SCS 0108)**

**Antenna Parameters with Head TSL at 5250 MHz**

Impedance, transformed to feed point	49.8 Ω - 6.7 jΩ
Return Loss	- 23.5 dB

**Antenna Parameters with Head TSL at 5600 MHz**

Impedance, transformed to feed point	54.6 Ω - 2.4 jΩ
Return Loss	- 26.0 dB

**Antenna Parameters with Head TSL at 5750 MHz**

Impedance, transformed to feed point	55.6 Ω - 2.6 jΩ
Return Loss	- 24.6 dB

**Antenna Parameters with Body TSL at 5250 MHz**

Impedance, transformed to feed point	48.4 Ω - 5.2 jΩ
Return Loss	- 25.1 dB

**Antenna Parameters with Body TSL at 5600 MHz**

Impedance, transformed to feed point	55.4 Ω - 2.6 jΩ
Return Loss	- 25.0 dB

**Antenna Parameters with Body TSL at 5750 MHz**

Impedance, transformed to feed point	55.7 Ω - 3.1 jΩ
Return Loss	- 24.3 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.196 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	March 11, 2011

**DASY5 Validation Report for Head TSL**

Date: 14.12.2017

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole D5GHzV2; Type: D5GHzV2; Serial: D5GHzV2 - SN:1107**

Communication System: UID 0 - CW; Frequency: 5250 MHz, Frequency: 5600 MHz, Frequency: 5750 MHz

Medium parameters used:  $f = 5250$  MHz;  $\sigma = 4.56$  S/m;  $\epsilon_r = 35.7$ ;  $\rho = 1000$  kg/m<sup>3</sup>,Medium parameters used:  $f = 5600$  MHz;  $\sigma = 4.91$  S/m;  $\epsilon_r = 35.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>,Medium parameters used:  $f = 5750$  MHz;  $\sigma = 5.07$  S/m;  $\epsilon_r = 35$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(5.58, 5.58, 5.58); Calibrated: 31.12.2016, ConvF(5.09, 5.09, 5.09); Calibrated: 31.12.2016, ConvF(5.02, 5.02, 5.02); Calibrated: 31.12.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

**Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5250 MHz/Zoom Scan,****dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 71.55 V/m; Power Drift = -0.09 dB

Peak SAR (extrapolated) = 30.5 W/kg

**SAR(1 g) = 8.15 W/kg; SAR(10 g) = 2.34 W/kg**

Maximum value of SAR (measured) = 19.1 W/kg

**Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan,****dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 71.65 V/m; Power Drift = -0.07 dB

Peak SAR (extrapolated) = 33.4 W/kg

**SAR(1 g) = 8.43 W/kg; SAR(10 g) = 2.41 W/kg**

Maximum value of SAR (measured) = 20.2 W/kg


**Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5750 MHz/Zoom Scan,****dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 69.75 V/m; Power Drift = -0.09 dB

Peak SAR (extrapolated) = 32.8 W/kg


**SAR(1 g) = 8.09 W/kg; SAR(10 g) = 2.3 W/kg**

Maximum value of SAR (measured) = 19.6 W/kg

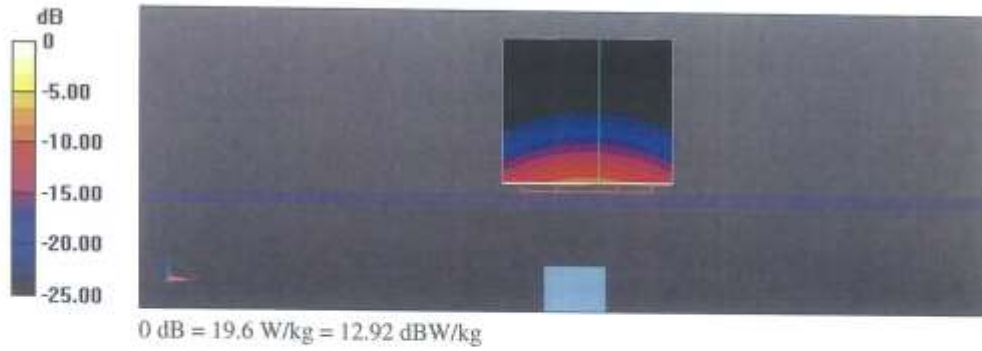



Impedance Measurement Plot for Head TSL

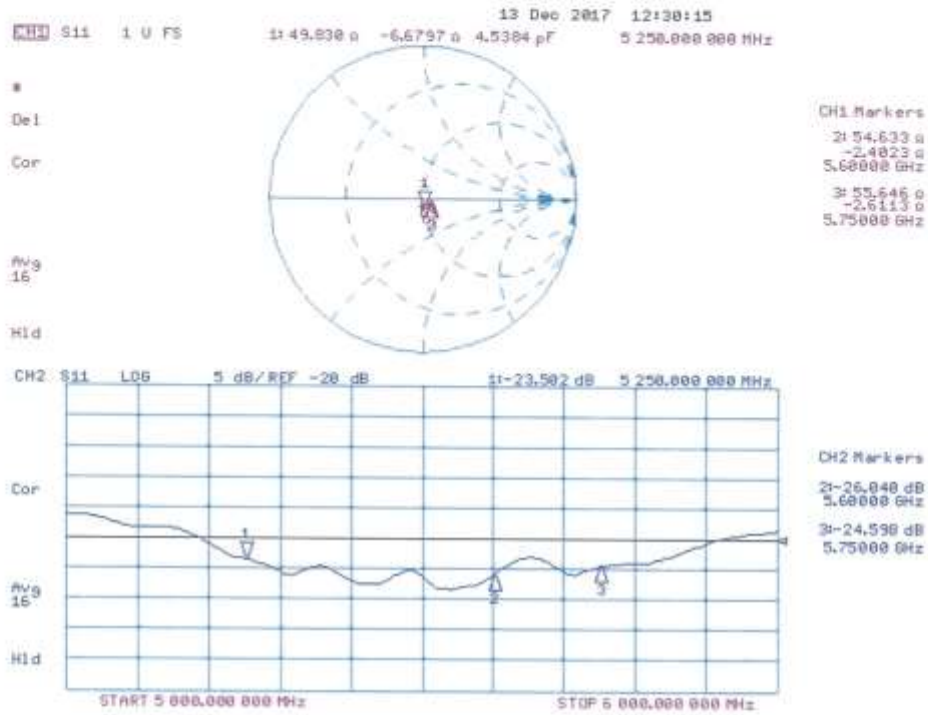

**DASY5 Validation Report for Body TSL**

Date: 13.12.2017

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole D5GHzV2; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1107**

Communication System: UID 0 - CW; Frequency: 5250 MHz, Frequency: 5600 MHz, Frequency: 5750 MHz  
Medium parameters used:  $f = 5250$  MHz;  $\sigma = 5.51$  S/m;  $\epsilon_r = 47.1$ ;  $\rho = 1000$  kg/m<sup>3</sup>,  
Medium parameters used:  $f = 5600$  MHz;  $\sigma = 5.97$  S/m;  $\epsilon_r = 46.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>,  
Medium parameters used:  $f = 5750$  MHz;  $\sigma = 6.18$  S/m;  $\epsilon_r = 46.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section  
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

**DASY52 Configuration:**

- Probe: EX3DV4 - SN3503; ConvF(5.14, 5.14, 5.14); Calibrated: 31.12.2016, ConvF(4.57, 4.57, 4.57); Calibrated: 31.12.2016, ConvF(4.51, 4.51, 4.51); Calibrated: 31.12.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

**Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5250 MHz/Zoom Scan,****dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 66.06 V/m; Power Drift = -0.04 dB

Peak SAR (extrapolated) = 30.6 W/kg

**SAR(1 g) = 7.79 W/kg; SAR(10 g) = 2.17 W/kg**

Maximum value of SAR (measured) = 18.5 W/kg

**Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan,****dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 64.93 V/m; Power Drift = -0.07 dB

Peak SAR (extrapolated) = 34.6 W/kg

**SAR(1 g) = 8.09 W/kg; SAR(10 g) = 2.26 W/kg**

Maximum value of SAR (measured) = 19.9 W/kg


**Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5750 MHz/Zoom Scan,****dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 62.90 V/m; Power Drift = -0.08 dB


Peak SAR (extrapolated) = 34.0 W/kg

**SAR(1 g) = 7.65 W/kg; SAR(10 g) = 2.13 W/kg**

Maximum value of SAR (measured) = 19.0 W/kg

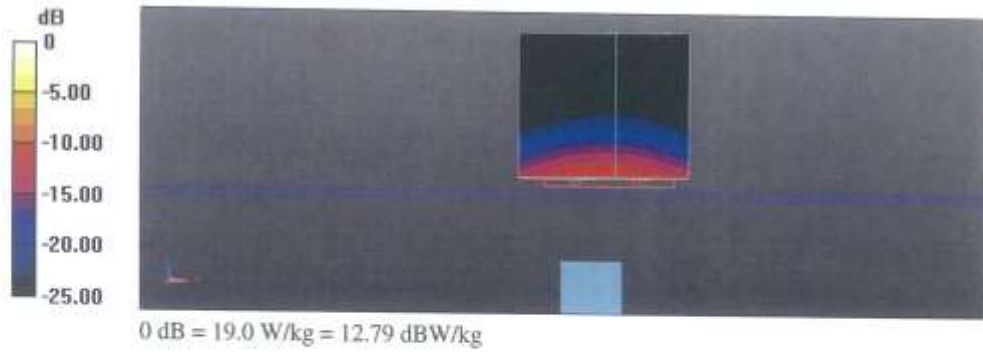

Impedance Measurement Plot for Body TSL

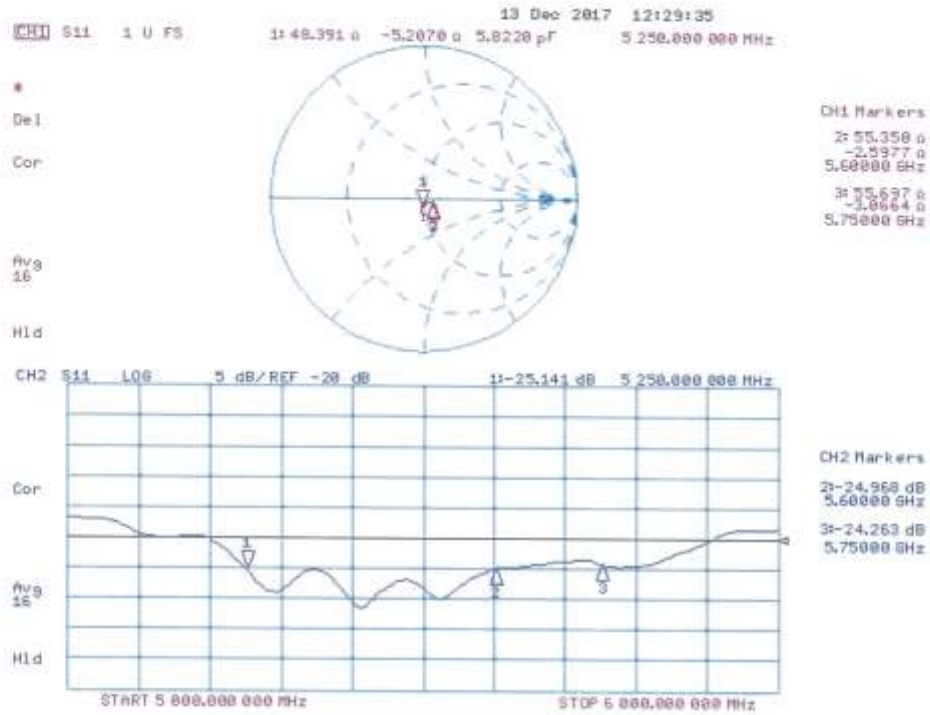



Schmid & Partner Engineering AG

**s p e a g**

Zeughausstrasse 43, 8004 Zurich, Switzerland  
Phone +41 44 245 9700, Fax +41 44 245 9779  
info@speag.com, http://www.speag.com

**Certificate of conformity / First Article Inspection**

Item	Triple Modular Flat Phantom V5.1
Type No	QD 000 P51 C
Series No	1100 and higher
Manufacturer / Origin	Untersee Composites Knebelstrasse 8, CH-8268 Mannenbach, Switzerland

**Tests**

The sub-units of item 1100 are identified with the designation 1100/1, 1100/2 and 1100/3. Tests were conducted on all 3 sub-units of this phantom.

Test	Requirement	Details	Units tested
Material thickness	Compliant with the standard requirements.	2 mm +/- 0.2 mm 30 points over the bottom area	all
Material parameters	Dielectric parameters for required frequencies	200 MHz – 6 GHz - Relative permittivity 3 - 5 Loss tangent < 0.05.	Material sample
Material resistivity	The material is compatible with the liquids defined in the standards if handled and cleaned according to the instructions.	DGBE based simulating liquids. Observe Technical Note for material compatibility.	Material Samples
Shape	Internal dimensions	Internal height: > 175 mm Bottom internal length: 280 mm Bottom internal width: 175 mm Nominal filling height: 155 mm Nominal volume: 9.2 l	Pre-series, design
Sagging	Depending on standard	No initial sagging (negative preshaped, change < 0.5 mm)	1100/2

**Standards**

- [1] IEEE 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- [2] IEC 62209 – 1, "Specific Absorption Rate (SAR) in the frequency range of 300 MHz to 3 GHz – Measurement Procedure, Part 1: Hand-held mobile wireless communication devices", February 2005
- [3] IEC 62209 – 2, "Evaluation of Human Exposure to Radio Frequency Fields from Handheld and Body-Mounted Wireless Communication Devices in the Frequency Range of 30 MHz to 6 GHz: Human models, Instrumentation and Procedures, Part 2: Procedure to determine the Specific Absorption Rate (SAR) for ... including accessories and multiple transmitters", March 2010
- [4] KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Conformity**

Based on the dimensions and sample tests above, we certify that this item is in compliance with the standards [1] to [4] for frequencies > 700 MHz, if operated according to the specific requirements.

Date 16.07.2015

Signature / Stamp

**s p e a g**

Schmid & Partner Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland  
Phone +41 44 245 9700, Fax +41 44 245 9779  
info@speag.com, http://www.speag.com