

Head Tissue Simulating Liquids

Head Tissue	Parameters according to IEEE Std 1528-2013 / IEC 62209 / FCC KDB 865664 D01		
Narrow-Band Solutions (±5% tolerance)	Product	Test Frequency (MHz)	Main Ingredients
	HSL300V2	300	Water, Sugar
	HSL450V2	450	Water, Sugar
	HSL750V2	750	Water, Sugar
	HSL900V2	835, 900	Water, Sugar
	HSL1450V2	1450, 1500, 1640	Water, DGBE
	HSL1750V2	1750	Water, DGBE
	HSL1800V2	1800, 1900	Water, DGBE
	HSL1900V2	1900	Water, DGBE
	HSL1950V2	1950, 2000	Water, DGBE
HSL2450V2	2450, 2600	Water, DGBE	
Broad-Band Solutions (±5% tolerance)	Product	Test Frequency (MHz)	Main Ingredients
	HBBL30-250V3	30-250	Water, Tween
	HBBL1350-1850V3	1400-1800	Water, Tween
	HBBL1550-1950V3	1750-1900	Water, Tween
	HBBL1900-3800V3	1950-3000	Water, Tween
	HBBL3500-5800V5	3500-5800	Water, Oil

Body Tissue Simulating Liquids

Body Tissue (Muscle)	Parameters according to FCC KDB 865664 D01		
Narrow-Band Solutions (±5% tolerance)	Product	Test Frequency (MHz)	Main Ingredients
	MSL300V2	300	Water, Sugar
	MSL450V2	400, 450	Water, Sugar
	MSL750V2	750	Water, Sugar
	MSL900V2	835, 900	Water, Sugar
	MSL1450V2	1450, 1500, 1640	Water, DGBE
	MSL1750V2	1750	Water, DGBE
	MSL1800V2	1800, 1900	Water, DGBE
	MSL1900V2	1900	Water, DGBE
	MSL1950V2	1950, 2100	Water, DGBE
MSL2450V2	2450, 2600	Water, DGBE	
Broad-Band Solutions (±5% tolerance)	Product	Test Frequency (MHz)	Main Ingredients
	MBBL130-250V3	130-250	Water, Tween
	MBBL1350-1850V3	1350-1800	Water, Tween
	MBBL1550-1950V3	1550-1850	Water, Tween
	MBBL1900-3800V3	1950-3800	Water, Tween
	MBBL3500-5800V5	3500-5800	Water, Oil

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speag.com, http://www.speag.com

Measurement Certificate / Material Test

Item Name	Head Tissue Simulating Liquid (HSL750V2)
Product No.	SL AAH 075 AA (Charge: 140210-5)
Manufacturer	SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



Test Condition

Ambient	Environment temperatur (22 ± 3)°C and humidity < 70%.
TSL Temperature	22°C
Test Date	12-Feb-14
Operator	IEN

Additional Information

TSL Density	1.284 g/cm ³
TSL Heat-capacity	2.701 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ -eps	Δ -sigma
600	44.4	23.49	0.78	42.7	0.88	3.9	-11.1
625	44.1	23.23	0.81	42.6	0.88	3.5	-8.6
650	43.7	22.96	0.83	42.5	0.89	3.0	-6.2
675	43.3	22.68	0.85	42.3	0.89	2.4	-4.1
700	42.9	22.40	0.87	42.2	0.89	1.7	-1.9
725	42.6	22.25	0.90	42.1	0.89	1.3	0.7
750	42.3	22.10	0.92	41.9	0.89	0.9	3.2
775	42.0	21.89	0.94	41.8	0.90	0.4	5.4
800	41.6	21.67	0.96	41.7	0.90	-0.1	7.5
825	41.3	21.55	0.99	41.6	0.91	-0.6	9.0
838	41.2	21.49	1.00	41.5	0.91	-0.8	9.8
850	41.1	21.42	1.01	41.5	0.92	-1.1	10.6
875	40.8	21.29	1.04	41.5	0.94	-1.8	9.9
900	40.5	21.15	1.06	41.5	0.97	-2.5	9.2
925	40.2	21.01	1.08	41.5	0.98	-3.1	10.0
950	39.9	20.87	1.10	41.4	0.99	-3.7	10.9
975	39.6	20.79	1.13	41.4	1.00	-4.3	12.2
1000	39.4	20.71	1.15	41.3	1.01	-4.8	13.5

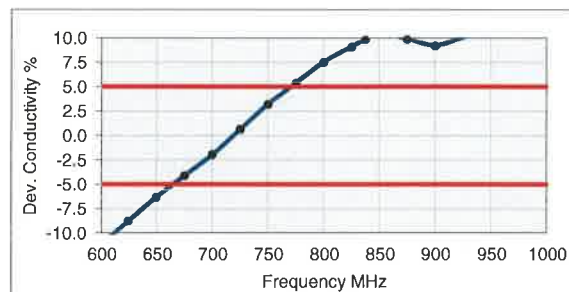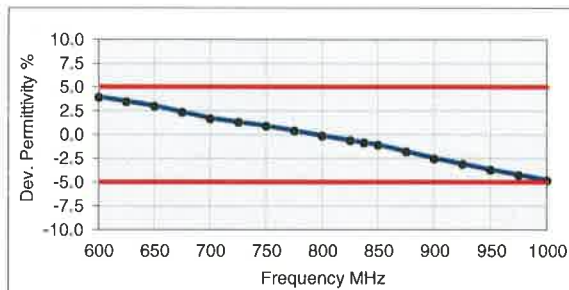

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speag.com, http://www.speag.com

Measurement Certificate / Material Test

Item Name	Head Tissue Simulating Liquid (HSL900V2)
Product No.	SL AAH 090 BB (Charge: 140205-4)
Manufacturer	SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



Test Condition

Ambient	Environment temperatur (22 ± 3)°C and humidity < 70%.
TSL Temperature	22°C
Test Date	12-Feb-14
Operator	IEN

Additional Information

TSL Density	1.280 g/cm ³
TSL Heat-capacity	2.942 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ -eps	Δ -sigma
700	42.9	19.58	0.76	42.2	0.89	1.6	-14.3
725	42.6	19.52	0.79	42.1	0.89	1.2	-11.7
750	42.3	19.47	0.81	41.9	0.89	0.8	-9.1
775	41.9	19.35	0.83	41.8	0.90	0.3	-6.8
800	41.6	19.23	0.86	41.7	0.90	-0.3	-4.6
825	41.3	19.18	0.88	41.6	0.91	-0.7	-2.9
838	41.1	19.16	0.89	41.5	0.91	-1.0	-2.1
850	41.0	19.13	0.90	41.5	0.92	-1.2	-1.2
875	40.7	19.07	0.93	41.5	0.94	-1.9	-1.6
900	40.4	19.00	0.95	41.5	0.97	-2.7	-1.9
925	40.1	18.92	0.97	41.5	0.98	-3.3	-0.9
950	39.8	18.85	1.00	41.4	0.99	-3.9	0.2
975	39.6	18.82	1.02	41.4	1.00	-4.4	1.6
1000	39.3	18.80	1.05	41.3	1.01	-5.0	3.0
1025	39.0	18.71	1.07	41.3	1.03	-5.5	4.0
1050	38.8	18.62	1.09	41.2	1.04	-6.0	5.0
1075	38.5	18.59	1.11	41.2	1.05	-6.5	6.3
1100	38.3	18.55	1.14	41.2	1.06	-7.0	7.5
1125	38.0	18.50	1.16	41.1	1.07	-7.5	8.5
1150	37.8	18.44	1.18	41.1	1.08	-8.0	9.6
1175	37.5	18.39	1.20	41.0	1.09	-8.4	10.6
1200	37.3	18.35	1.22	41.0	1.10	-8.9	11.6

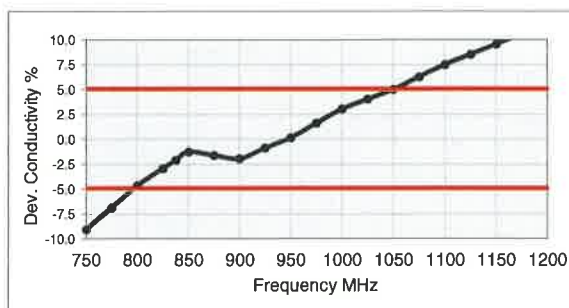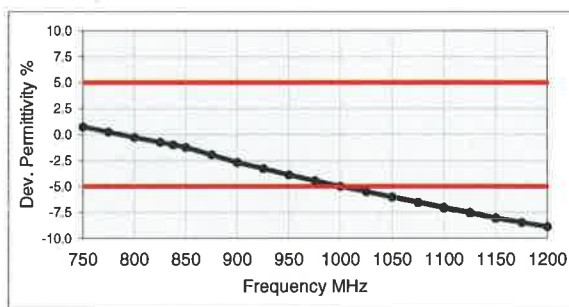

Measurement Certificate / Material Test

Item Name	Head Tissue Simulating Liquid (HSL 1900)
Product No.	SL AAH 190 AA (Charge: 120112-1)
Manufacturer	SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe (type DAK).

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.

Test Condition



Ambient Condition 22°C ; 30% humidity
 TSL Temperature 22°C
 Test Date 18-Jan-12

Additional Information

TSL Density 0.985 g/cm³
 TSL Heat-capacity 3.710 kJ/(kg*K)

Results

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ-eps	Δ-sigma
1600	41.2	12.84	1.14	40.3	1.28	2.1	-11.0
1613	41.1	12.88	1.16	40.3	1.29	2.0	-10.5
1625	41.1	12.93	1.17	40.3	1.30	1.9	-10.0
1638	41.0	12.97	1.18	40.3	1.31	1.8	-9.5
1650	40.9	13.01	1.19	40.2	1.31	1.8	-9.1
1663	40.9	13.05	1.21	40.2	1.32	1.7	-8.6
1675	40.8	13.10	1.22	40.2	1.33	1.6	-8.1
1688	40.8	13.14	1.23	40.2	1.33	1.4	-7.6
1700	40.7	13.18	1.25	40.2	1.34	1.3	-7.1
1713	40.6	13.22	1.26	40.1	1.35	1.2	-6.7
1725	40.6	13.25	1.27	40.1	1.36	1.1	-6.3
1738	40.5	13.28	1.28	40.1	1.36	1.0	-5.9
1750	40.5	13.31	1.30	40.1	1.37	0.9	-5.5
1763	40.4	13.35	1.31	40.1	1.38	0.9	-5.1
1775	40.4	13.38	1.32	40.0	1.39	0.8	-4.7
1788	40.3	13.41	1.33	40.0	1.39	0.7	-4.3
1800	40.3	13.44	1.35	40.0	1.40	0.6	-3.9
1813	40.2	13.48	1.36	40.0	1.40	0.5	-2.9
1825	40.2	13.52	1.37	40.0	1.40	0.4	-2.0
1838	40.1	13.55	1.39	40.0	1.40	0.3	-1.0
1850	40.1	13.59	1.40	40.0	1.40	0.1	-0.1
1863	40.0	13.63	1.41	40.0	1.40	0.0	0.9
1875	39.9	13.67	1.43	40.0	1.40	-0.1	1.9
1888	39.9	13.71	1.44	40.0	1.40	-0.3	2.9
1900	39.8	13.75	1.45	40.0	1.40	-0.4	3.8
1913	39.8	13.79	1.47	40.0	1.40	-0.5	4.8
1925	39.7	13.83	1.48	40.0	1.40	-0.7	5.8
1938	39.7	13.86	1.49	40.0	1.40	-0.8	6.7
1950	39.6	13.90	1.51	40.0	1.40	-0.9	7.7
1975	39.5	13.97	1.53	40.0	1.40	-1.2	9.6
2000	39.4	14.04	1.56	40.0	1.40	-1.5	11.6

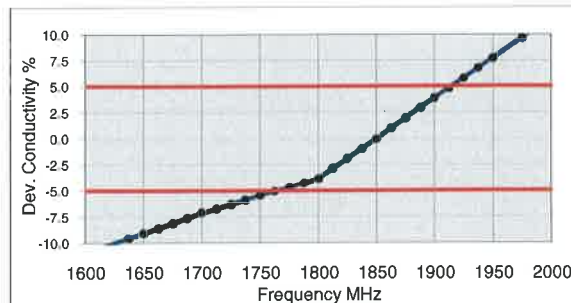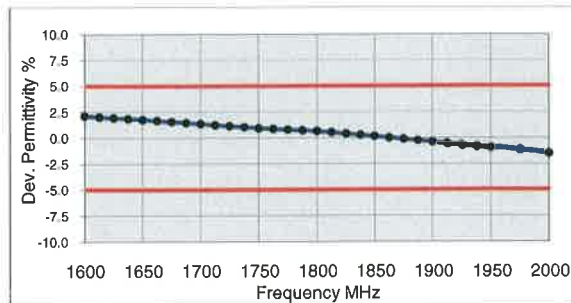

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speag.com, http://www.speag.com

Measurement Certificate / Material Test

Item Name	Head Tissue Simulating Liquid (HSL2450V2)
Product No.	SL AAH 245 BA (Charge: 130430-3)
Manufacturer	SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



Test Condition

Ambient	Environment temperatur (22 ± 3)°C and humidity < 70%.
TSL Temperature	23°C
Test Date	2-May-13
Operator	CL

Additional Information

TSL Density	0.988 g/cm ³
TSL Heat-capacity	3.680 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ -eps	Δ -sigma
1900	41.6	11.98	1.27	40.0	1.40	4.0	-9.6
1925	41.5	12.06	1.29	40.0	1.40	3.8	-7.7
1950	41.4	12.15	1.32	40.0	1.40	3.5	-5.9
1975	41.3	12.24	1.35	40.0	1.40	3.3	-3.9
2000	41.2	12.34	1.37	40.0	1.40	3.0	-1.9
2025	41.1	12.44	1.40	40.0	1.42	2.9	-1.5
2050	41.0	12.54	1.43	39.9	1.44	2.8	-1.0
2075	40.9	12.62	1.46	39.9	1.47	2.6	-0.6
2100	40.8	12.71	1.48	39.8	1.49	2.5	-0.3
2125	40.7	12.80	1.51	39.8	1.51	2.3	0.1
2150	40.6	12.88	1.54	39.7	1.53	2.2	0.5
2175	40.5	12.97	1.57	39.7	1.56	2.0	0.9
2200	40.4	13.05	1.60	39.6	1.58	1.9	1.3
2225	40.3	13.13	1.63	39.6	1.60	1.7	1.6
2250	40.2	13.21	1.65	39.6	1.62	1.6	1.9
2275	40.1	13.30	1.68	39.5	1.64	1.5	2.4
2300	40.0	13.39	1.71	39.5	1.67	1.3	2.8
2325	39.9	13.48	1.74	39.4	1.69	1.2	3.2
2350	39.8	13.56	1.77	39.4	1.71	1.0	3.6
2375	39.7	13.64	1.80	39.3	1.73	0.9	4.0
2400	39.6	13.72	1.83	39.3	1.76	0.8	4.3
2425	39.5	13.80	1.86	39.2	1.78	0.6	4.8
2450	39.4	13.89	1.89	39.2	1.80	0.5	5.2
2475	39.3	13.96	1.92	39.2	1.83	0.3	5.2
2500	39.2	14.03	1.95	39.1	1.85	0.1	5.2
2525	39.1	14.12	1.98	39.1	1.88	-0.1	5.4
2550	39.0	14.22	2.02	39.1	1.91	-0.3	5.6
2575	38.9	14.28	2.05	39.0	1.94	-0.5	5.6
2600	38.7	14.34	2.07	39.0	1.96	-0.7	5.6
2625	38.6	14.41	2.10	39.0	1.99	-0.9	5.7
2650	38.5	14.48	2.13	38.9	2.02	-1.1	5.8
2675	38.4	14.55	2.17	38.9	2.05	-1.3	5.9
2700	38.3	14.62	2.20	38.9	2.07	-1.4	6.0

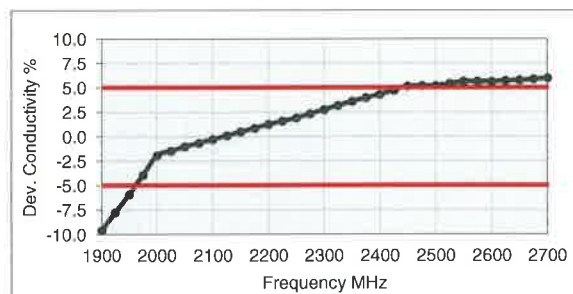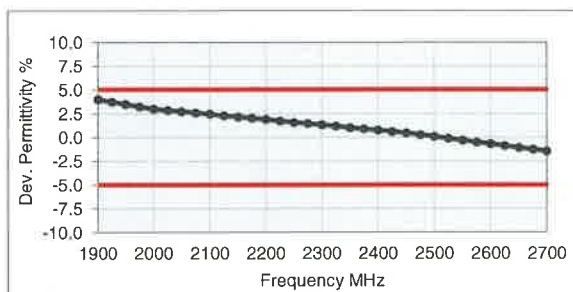

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speag.com, http://www.speag.com

Measurement Certificate / Material Test

Item Name **Body Tissue Simulating Liquid (MSL750V2)**
 Product No. SL AAM 075 (Charge: 120831-2)
 Manufacturer SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



Test Condition

Ambient Environment temperatur (22 ± 3)°C and humidity < 70%.
 TSL Temperature 22°C
 Test Date 5-Sep-12
 Operator CL

Additional Information

TSL Density 1.212 g/cm³
 TSL Heat-capacity 3.006 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ -eps	Δ -sigma
600	57.4	24.67	0.82	56.1	0.95	2.2	-13.5
625	57.1	24.34	0.85	56.0	0.95	1.9	-11.3
650	56.8	24.01	0.87	55.9	0.96	1.6	-9.1
675	56.6	23.71	0.89	55.8	0.96	1.3	-7.1
700	56.3	23.41	0.91	55.7	0.96	1.0	-5.0
725	56.0	23.20	0.94	55.6	0.96	0.7	-2.7
750	55.8	22.99	0.96	55.5	0.96	0.5	-0.4
775	55.5	22.81	0.98	55.4	0.97	0.2	1.9
800	55.3	22.64	1.01	55.3	0.97	-0.1	4.2
825	55.1	22.47	1.03	55.2	0.98	-0.3	5.5
838	54.9	22.39	1.04	55.2	0.98	-0.5	6.1
850	54.8	22.31	1.05	55.2	0.99	-0.6	6.7
875	54.6	22.19	1.08	55.1	1.02	-0.9	6.0
900	54.4	22.07	1.10	55.0	1.05	-1.1	5.2
925	54.1	21.96	1.13	55.0	1.06	-1.5	6.3
950	53.9	21.85	1.15	54.9	1.08	-1.9	7.4
975	53.7	21.75	1.18	54.9	1.09	-2.2	8.5
1000	53.5	21.64	1.20	54.8	1.10	-2.5	9.6

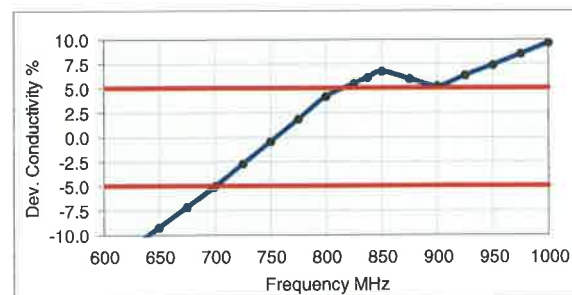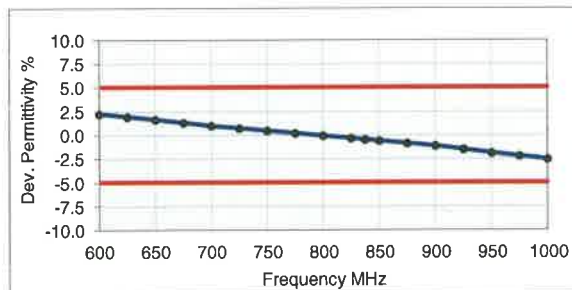

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speag.com, http://www.speag.com

Measurement Certificate / Material Test

Item Name	Body Tissue Simulating Liquid (MSL900V2)
Product No.	SL AAM 090 CA (Charge: 140124-1)
Manufacturer	SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



Test Condition

Ambient	Environment temperatur (22 ± 3)°C and humidity < 70%.
TSL Temperature	22°C
Test Date	29-Jan-14
Operator	IEN

Additional Information

TSL Density	1.208 g/cm ³
TSL Heat-capacity	3.113 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ-eps	Δ-sigma
700	56.5	22.21	0.86	55.7	0.96	1.4	-9.9
725	56.3	22.03	0.89	55.6	0.96	1.1	-7.6
750	56.0	21.85	0.91	55.5	0.96	0.9	-5.4
775	55.8	21.71	0.94	55.4	0.97	0.6	-3.1
800	55.5	21.57	0.96	55.3	0.97	0.3	-0.8
825	55.3	21.47	0.99	55.2	0.98	0.1	0.8
838	55.2	21.42	1.00	55.2	0.98	-0.1	1.5
850	55.1	21.37	1.01	55.2	0.99	-0.2	2.2
875	54.8	21.28	1.04	55.1	1.02	-0.5	1.6
900	54.6	21.19	1.06	55.0	1.05	-0.8	1.0
925	54.3	21.10	1.09	55.0	1.06	-1.1	2.1
950	54.1	21.01	1.11	54.9	1.08	-1.5	3.2
975	53.9	20.96	1.14	54.9	1.09	-1.8	4.6
1000	53.7	20.90	1.16	54.8	1.10	-2.1	5.9
1025	53.5	20.82	1.19	54.8	1.11	-2.4	7.0
1050	53.3	20.75	1.21	54.7	1.12	-2.7	8.1
1075	53.0	20.70	1.24	54.7	1.13	-3.0	9.4
1100	52.8	20.66	1.26	54.7	1.14	-3.4	10.6
1125	52.6	20.57	1.29	54.6	1.15	-3.7	11.5
1150	52.4	20.48	1.31	54.6	1.17	-3.9	12.4
1175	52.2	20.47	1.34	54.5	1.18	-4.2	13.7
1200	52.0	20.46	1.37	54.5	1.19	-4.5	15.0

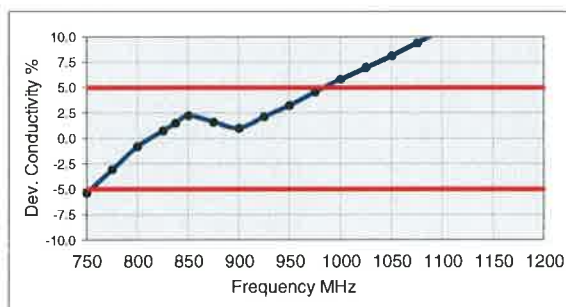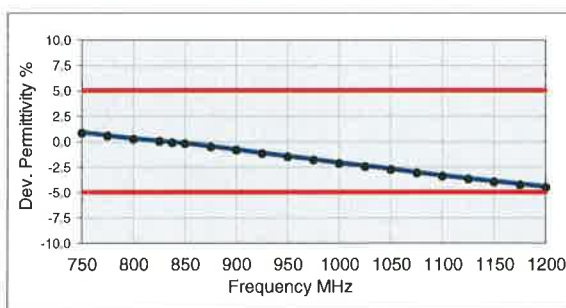

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speag.com, http://www.speag.com

Measurement Certificate / Material Test

Item Name	Body Tissue Simulating Liquid (MSL1900V2)
Product No.	SL AAM 190 (Charge: 120913-1)
Manufacturer	SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



Test Condition

Ambient	Environment temperatur (22 ± 3)°C and humidity < 70%.
TSL Temperature	22°C
Test Date	20-Sep-12
Operator	CL

Additional Information

TSL Density	0.996 g/cm ³
TSL Heat-capacity	3.947 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ -eps	Δ -sigma
1600	54.1	13.80	1.23	53.8	1.39	0.5	-11.8
1613	54.1	13.84	1.24	53.8	1.40	0.5	-11.4
1625	54.0	13.87	1.25	53.8	1.41	0.5	-11.0
1638	54.0	13.91	1.27	53.7	1.42	0.5	-10.6
1650	53.9	13.95	1.28	53.7	1.43	0.4	-10.2
1663	53.9	13.99	1.29	53.7	1.43	0.4	-9.7
1675	53.8	14.02	1.31	53.6	1.44	0.4	-9.3
1688	53.8	14.06	1.32	53.6	1.45	0.4	-8.9
1700	53.8	14.10	1.33	53.6	1.46	0.4	-8.4
1713	53.7	14.14	1.35	53.5	1.46	0.3	-8.0
1725	53.7	14.19	1.36	53.5	1.47	0.3	-7.6
1738	53.6	14.23	1.38	53.5	1.48	0.3	-7.1
1750	53.6	14.27	1.39	53.4	1.49	0.3	-6.7
1763	53.5	14.31	1.40	53.4	1.50	0.3	-6.2
1775	53.5	14.35	1.42	53.4	1.50	0.3	-5.8
1788	53.5	14.40	1.43	53.3	1.51	0.2	-5.3
1800	53.4	14.44	1.45	53.3	1.52	0.2	-4.9
1813	53.4	14.48	1.46	53.3	1.52	0.2	-3.9
1825	53.3	14.52	1.47	53.3	1.52	0.1	-3.0
1838	53.3	14.56	1.49	53.3	1.52	0.0	-2.0
1850	53.3	14.61	1.50	53.3	1.52	-0.1	-1.1
1863	53.2	14.65	1.52	53.3	1.52	-0.1	-0.1
1875	53.2	14.69	1.53	53.3	1.52	-0.2	0.8
1888	53.1	14.74	1.55	53.3	1.52	-0.3	1.8
1900	53.1	14.78	1.56	53.3	1.52	-0.4	2.8
1913	53.0	14.83	1.58	53.3	1.52	-0.5	3.8
1925	53.0	14.87	1.59	53.3	1.52	-0.5	4.8
1938	53.0	14.91	1.61	53.3	1.52	-0.6	5.7
1950	52.9	14.95	1.62	53.3	1.52	-0.7	6.7
1975	52.8	15.03	1.65	53.3	1.52	-0.9	8.7
2000	52.7	15.11	1.68	53.3	1.52	-1.0	10.6

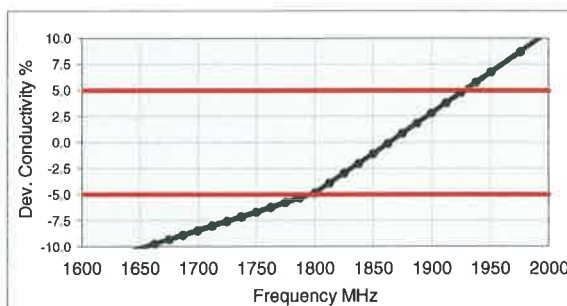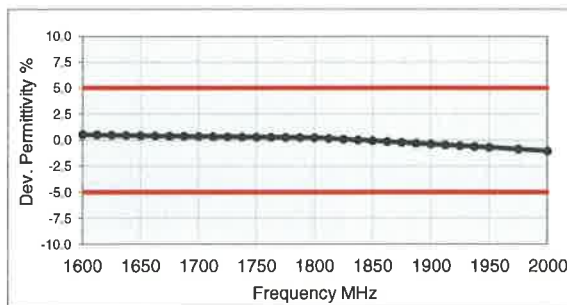

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speag.com, http://www.speag.com

Measurement Certificate / Material Test

Item Name **Body Tissue Simulating Liquid (MSL2450V2)**
 Product No. SL AAM 245 BA (Charge: 130510-2)
 Manufacturer SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.

Test Condition

Ambient Environment temperatur (22 ± 3)°C and humidity < 70%.
 TSL Temperature 22°C
 Test Date 15-May-13
 Operator IEN

Additional Information

TSL Density 0.996 g/cm³
 TSL Heat-capacity 3.987 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ-eps	Δ-sigma
1900	52.4	12.21	1.29	53.3	1.52	-1.7	-15.1
1925	52.3	12.32	1.32	53.3	1.52	-1.9	-13.2
1950	52.2	12.43	1.35	53.3	1.52	-2.1	-11.3
1975	52.1	12.55	1.38	53.3	1.52	-2.2	-9.3
2000	52.0	12.67	1.41	53.3	1.52	-2.4	-7.3
2025	51.9	12.75	1.44	53.3	1.54	-2.5	-6.9
2050	51.8	12.84	1.46	53.2	1.57	-2.6	-6.6
2075	51.7	12.96	1.50	53.2	1.59	-2.7	-6.0
2100	51.7	13.09	1.53	53.2	1.62	-2.8	-5.4
2125	51.6	13.17	1.56	53.1	1.64	-2.9	-5.0
2150	51.5	13.25	1.58	53.1	1.66	-3.0	-4.7
2175	51.4	13.37	1.62	53.1	1.69	-3.1	-4.1
2200	51.3	13.50	1.65	53.0	1.71	-3.3	-3.5
2225	51.2	13.58	1.68	53.0	1.74	-3.3	-3.1
2250	51.2	13.65	1.71	53.0	1.76	-3.3	-2.8
2275	51.1	13.78	1.74	52.9	1.78	-3.5	-2.2
2300	51.0	13.90	1.78	52.9	1.81	-3.6	-1.5
2325	50.9	14.01	1.81	52.9	1.83	-3.7	-1.0
2350	50.9	14.12	1.85	52.8	1.85	-3.8	-0.5
2375	50.7	14.21	1.88	52.8	1.88	-3.9	0.0
2400	50.6	14.31	1.91	52.8	1.90	-4.1	0.5
2425	50.5	14.44	1.95	52.7	1.93	-4.2	1.1
2450	50.5	14.56	1.99	52.7	1.95	-4.3	1.9
2475	50.4	14.64	2.02	52.7	1.99	-4.4	1.6
2500	50.3	14.72	2.05	52.6	2.02	-4.5	1.3
2525	50.2	14.79	2.08	52.6	2.06	-4.6	1.0
2550	50.1	14.86	2.11	52.6	2.09	-4.7	0.7
2575	50.0	15.00	2.15	52.5	2.13	-4.8	1.0
2600	49.9	15.14	2.19	52.5	2.16	-4.9	1.2
2625	49.8	15.23	2.22	52.5	2.20	-5.1	1.2
2650	49.6	15.33	2.26	52.4	2.23	-5.3	1.2
2675	49.6	15.45	2.30	52.4	2.27	-5.4	1.3
2700	49.5	15.56	2.34	52.4	2.30	-5.5	1.4

