

APPENDIX B: SYSTEM VERIFICATION

PCTEST

DUT: Dipole 750.0 MHz; Type: D750V3 - SN1003

Communication System: UID: 0, CW; Frequency: 750.0 MHz
Medium: 750 Head; Medium parameters used:
f = 750.0 MHz; cond = 0.907 S/m; perm = 43.8; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 01/06/2022; Ambient Temp: 22.9°C; Tissue Temp: 21.9°C

Probe: EX3DV4 - SN7406; ConvF:(10.08,10.08,10.08); Calibrated: 2021-07-20
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1676; Calibrated: 2021-06-21
Phantom: Twin-SAM V8.0; Serial: 2058
Measurement SW: DASY Module SAR V16.0.0.65

750 MHz System Verification at 23 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.65 W/kg

SAR(1 g) = 1.64 W/kg

Deviation (1 g) = -6.61%

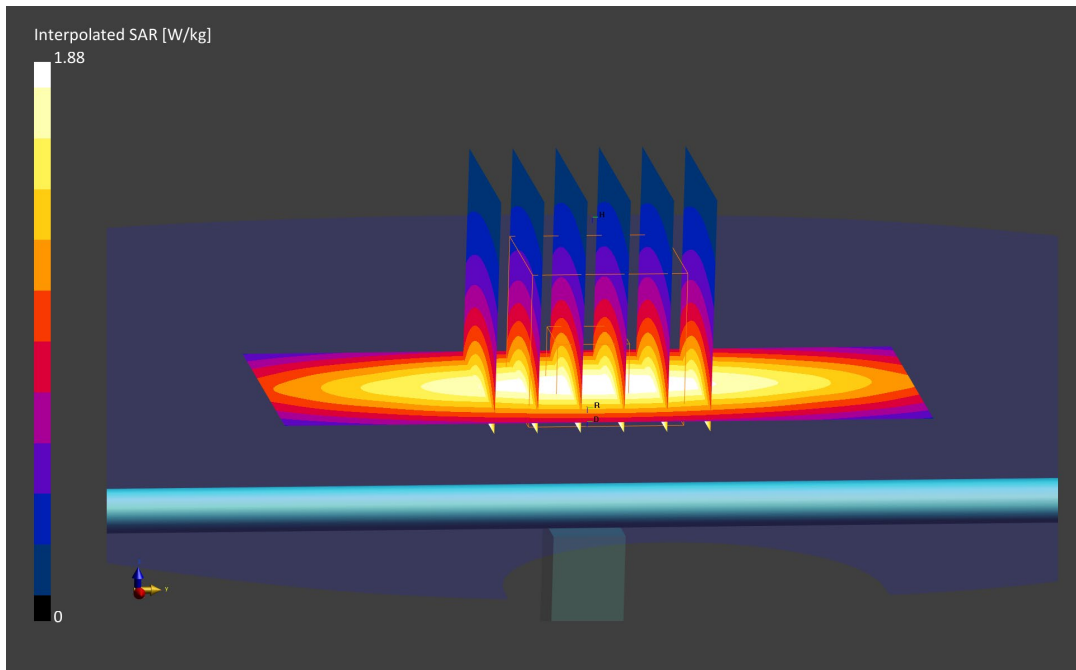

PCTEST

DUT: Dipole 835.0 MHz; Type: D835V2 - SN4d132

Communication System: UID: 0, CW; Frequency: 835.0 MHz
Medium: 835 Head; Medium parameters used:
f = 835.0 MHz; cond = 0.938 S/m; perm = 43.6; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 01/06/2022; Ambient Temp: 22.9°C; Tissue Temp: 21.9°C

Probe: EX3DV4 - SN7406; ConvF:(9.68,9.68,9.68); Calibrated: 2021-07-20
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1676; Calibrated: 2021-06-21
Phantom: Twin-SAM V8.0; Serial: 2058
Measurement SW: DASY Module SAR V16.0.0.65

835 MHz System Verification at 23 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 3.07 W/kg

SAR(1 g) = 2.00 W/kg

Deviation (1 g) = 3.52%

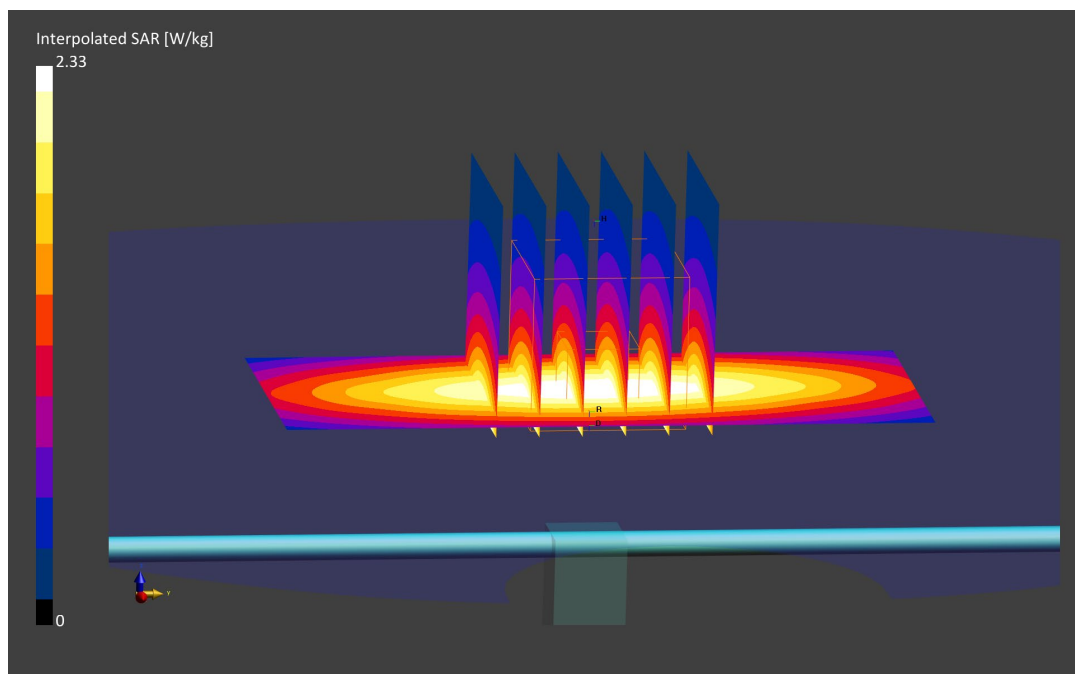

PCTEST

DUT: Dipole 1750.0 MHz; Type: D1750V2 - SN1148

Communication System: UID: 0, CW; Frequency: 1750.0 MHz
Medium: 1750 Head; Medium parameters used:
f = 1750.0 MHz; cond = 1.38 S/m; perm = 41.8; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/04/2022; Ambient Temp: 23.3°C; Tissue Temp: 21.4°C

Probe: EX3DV4 - SN7406; ConvF:(8.26,8.26,8.26); Calibrated: 2021-07-20
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1676; Calibrated: 2021-06-21
Phantom: Twin-SAM V8.0; Serial: 2058
Measurement SW: DASY Module SAR V16.0.0.65

1750 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.36 W/kg

SAR(1 g) = 3.89 W/kg

Deviation (1 g) = 8.36%

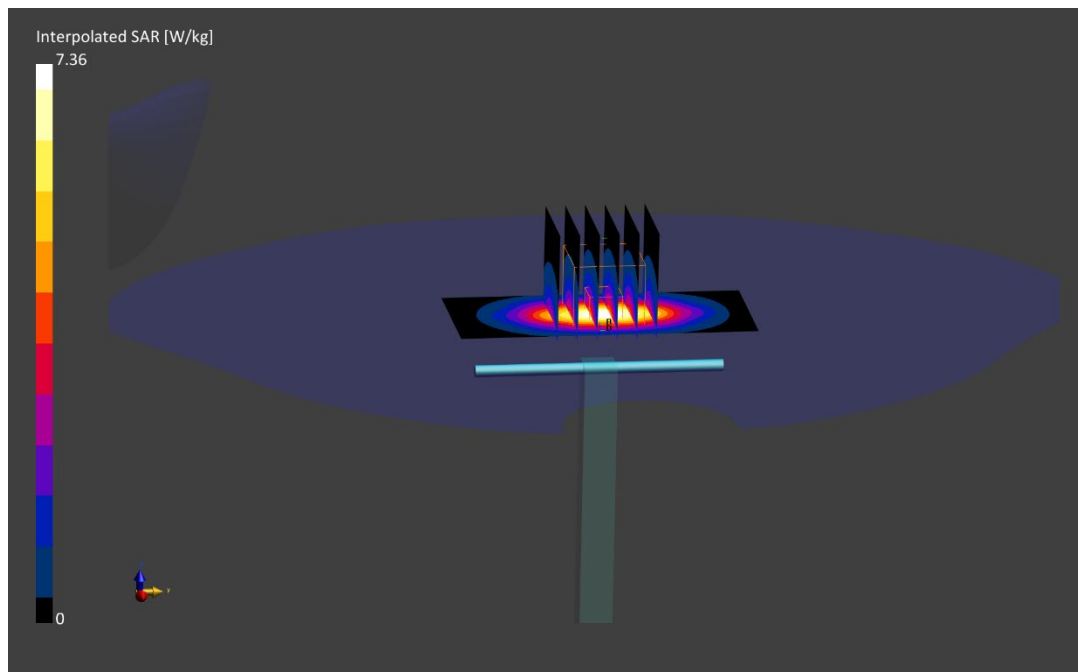

PCTEST

DUT: Dipole 1750.0 MHz; Type: D1750V2 – SN1008

Communication System: UID:0; CW; Frequency: 1750.0 MHz
Medium: 1750 Head; Medium parameters used:
f = 1750.0 MHz; cond = 1.38 S/m; perm = 40.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/12/2022; Ambient Temp: 22.7°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7410; ConvF:(8.34,8.34,8.34); Calibrated: 2021-07-20
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1583; Calibrated: 2021-07-13
Phantom: Twin-SAM V5.0; Serial: 1792
Measurement SW: DASY Module SAR V16.0.0.116

1750 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.22 W/kg

SAR(1 g) = 3.79 W/kg

Deviation (1 g) = 1.34%

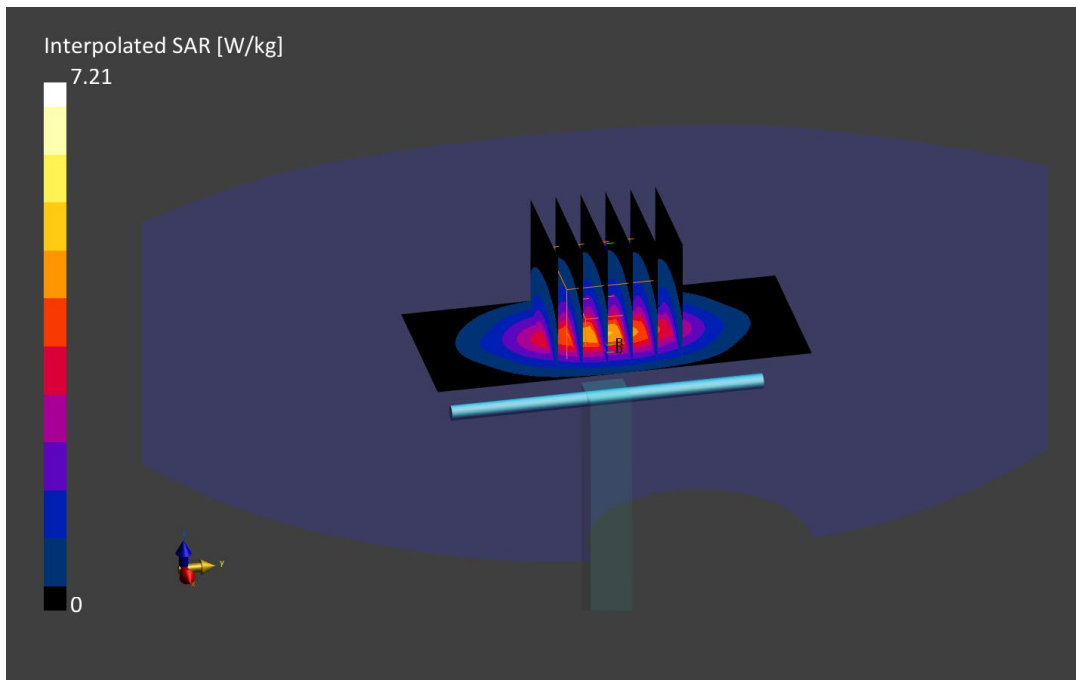

PCTEST

DUT: Dipole 1900.0 MHz; Type: D1900V2 - SN5d080

Communication System: UID: 0, CW; Frequency: 1900.0 MHz
Medium: 1900 Head; Medium parameters used:
f = 1900.0 MHz; cond = 1.45 S/m; perm = 40.0; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/09/2022; Ambient Temp: 21.5°C; Tissue Temp: 21.8°C

Probe: EX3DV4 - SN7660; ConvF:(9.06,9.06,9.06); Calibrated: 2021-06-28
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1677; Calibrated: 2021-06-22
Phantom: Twin-SAM V8.0; Serial: 2056
Measurement SW: DASY Module SAR V16.0.0.65

1900 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 8.03 W/kg

SAR(1 g) = 4.01 W/kg

Deviation (1 g) = -0.99%

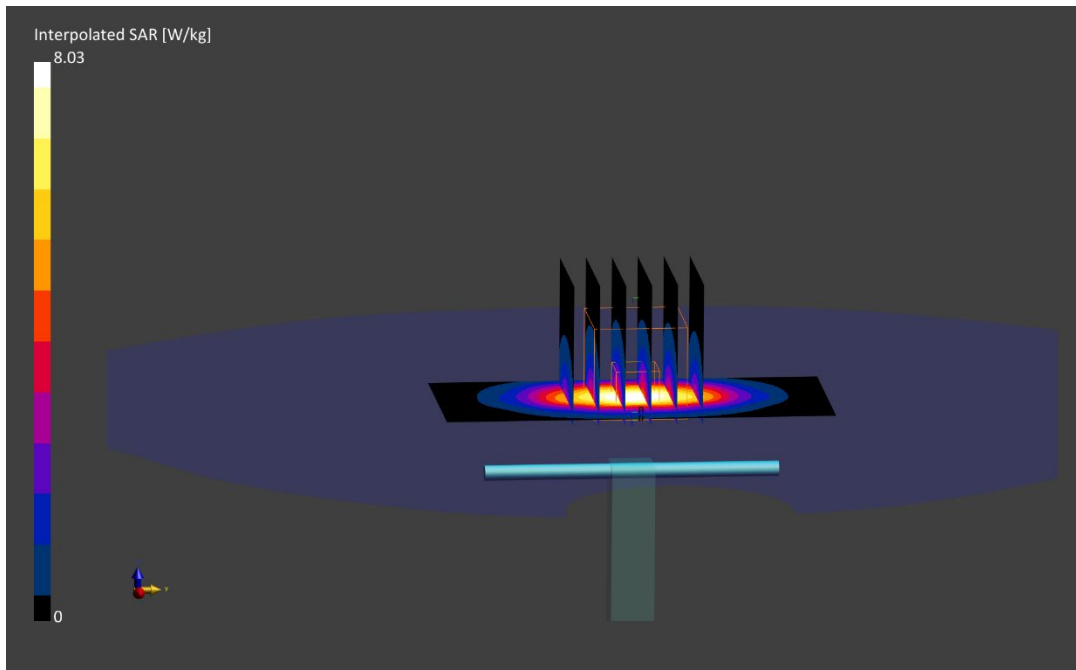

PCTEST

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN797

Communication System: UID: 0, CW; Frequency: 2450.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2450.0 MHz; cond = 1.85 S/m; perm = 38.8; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/12/2022; Ambient Temp: 24.3°C; Tissue Temp: 22.5°C

Probe: EX3DV4 - SN7538; ConvF:(7.58,7.58,7.58); Calibrated: 2021-11-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1323; Calibrated: 2021-11-10
Phantom: Twin-SAM V5.0; Serial: 1648
Measurement SW: DASY Module SAR V16.0.0.116

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.7 W/kg

SAR(1 g) = 5.44 W/kg

Deviation (1 g) = 3.82%

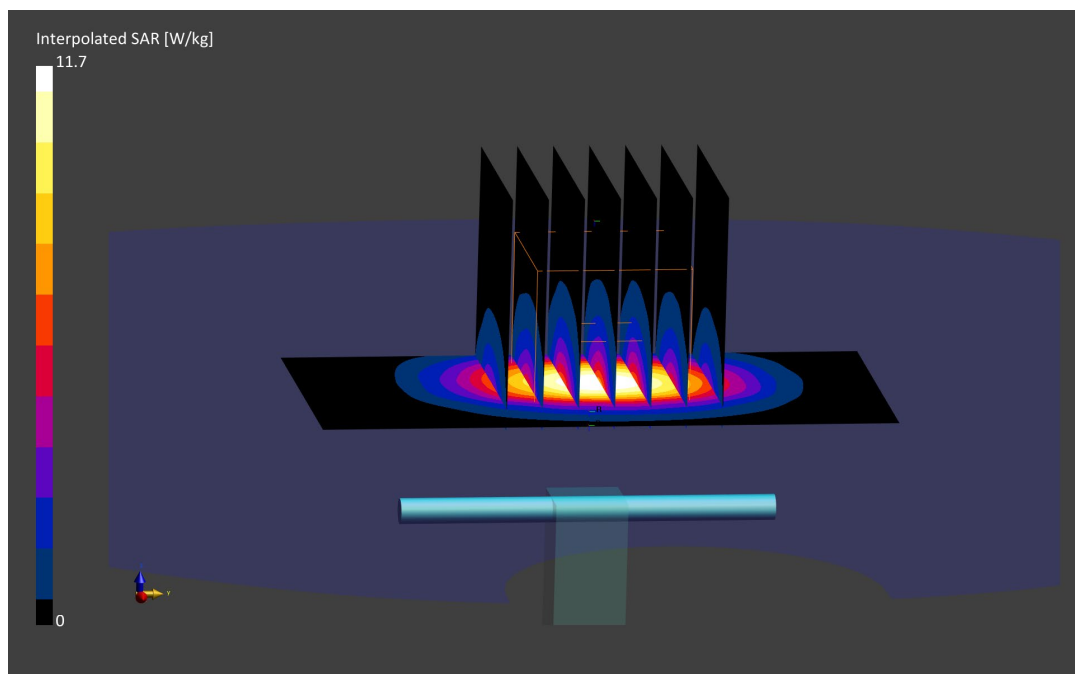

PCTEST

DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1064

Communication System: UID: 0, CW; Frequency: 2600.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2600.0 MHz; cond = 1.99 S/m; perm = 38.8; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/28/2022; Ambient Temp: 19.5°C; Tissue Temp: 19.2°C

Probe: EX3DV4 - SN7552; ConvF:(7.1,7.1,7.1); Calibrated: 2021-09-20
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1680; Calibrated: 2021-08-04
Phantom: Twin-SAM V8.0; Serial: 2065
Measurement SW: DASY Module SAR V16.0.0.65

2600 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.6 W/kg

SAR(1 g) = 5.84 W/kg

Deviation (1 g) = 0.52%

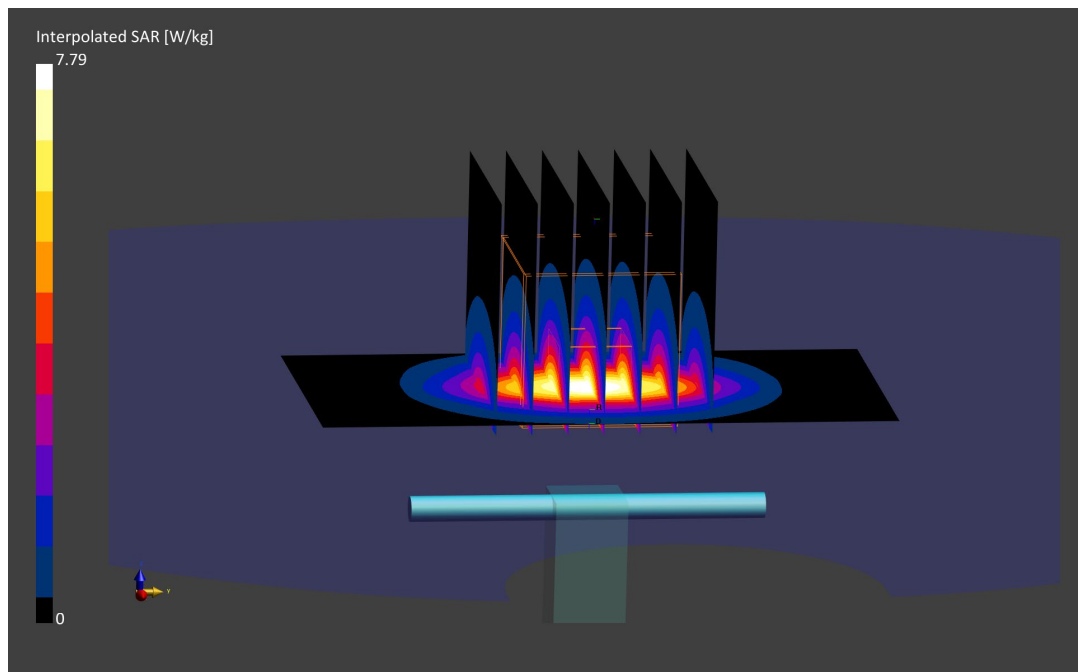

PCTEST

DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1191

Communication System: UID: 0, CW; Frequency: 5250.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5250.0 MHz; cond = 4.56 S/m; perm = 34.6; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/25/2022; Ambient Temp: 20.1°C; Tissue Temp: 19.6°C

Probe: EX3DV4 - SN7668; ConvF:(5.1,5.1,5.1); Calibrated: 2021-08-04
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1272; Calibrated: 2021-03-18
Phantom: Twin-SAM V8.0; Serial: 20063
Measurement SW: DASY Module SAR V16.0.0.116

5250 MHz System Verification at 17 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 14.3 W/kg

SAR(1 g) = 3.65 W/kg

Deviation (1 g) = -8.29%

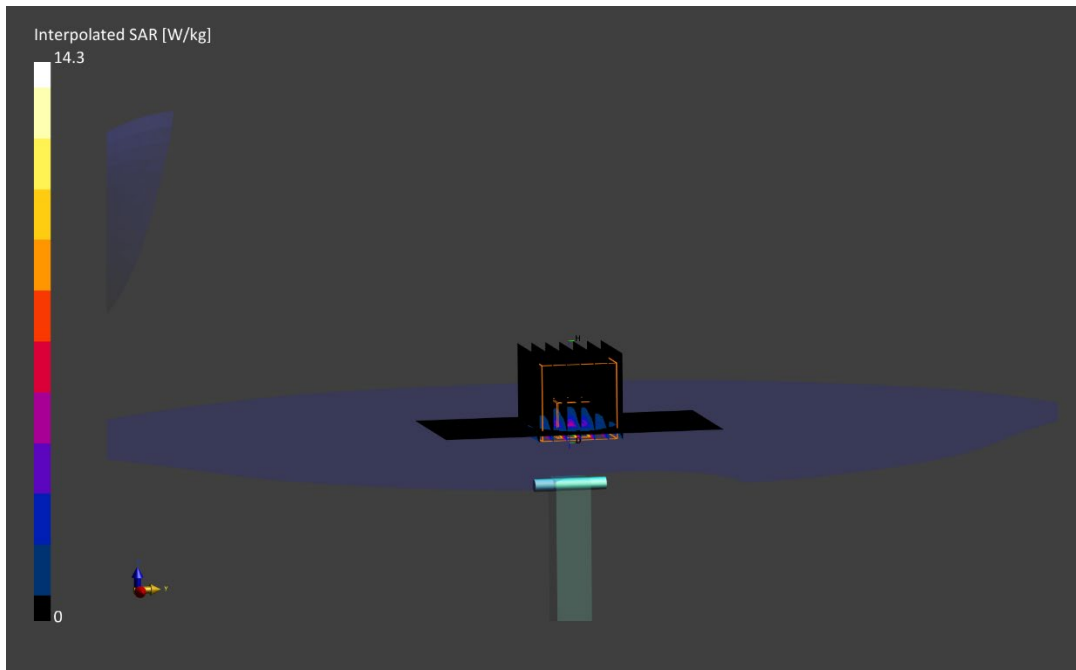

PCTEST

DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1191

Communication System: UID: 0, CW; Frequency: 5600.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5600.0 MHz; cond = 4.94 S/m; perm = 34.0; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/25/2022; Ambient Temp: 20.1°C; Tissue Temp: 19.6°C

Probe: EX3DV4 - SN7668; ConvF:(4.51,4.51,4.51); Calibrated: 2021-08-04
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1272; Calibrated: 2021-03-18
Phantom: Twin-SAM V8.0; Serial: 20063
Measurement SW: DASY Module SAR V16.0.0.116

5600 MHz System Verification at 17 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.9 W/kg

SAR(1 g) = 3.99 W/kg

Deviation (1 g) = -2.80%

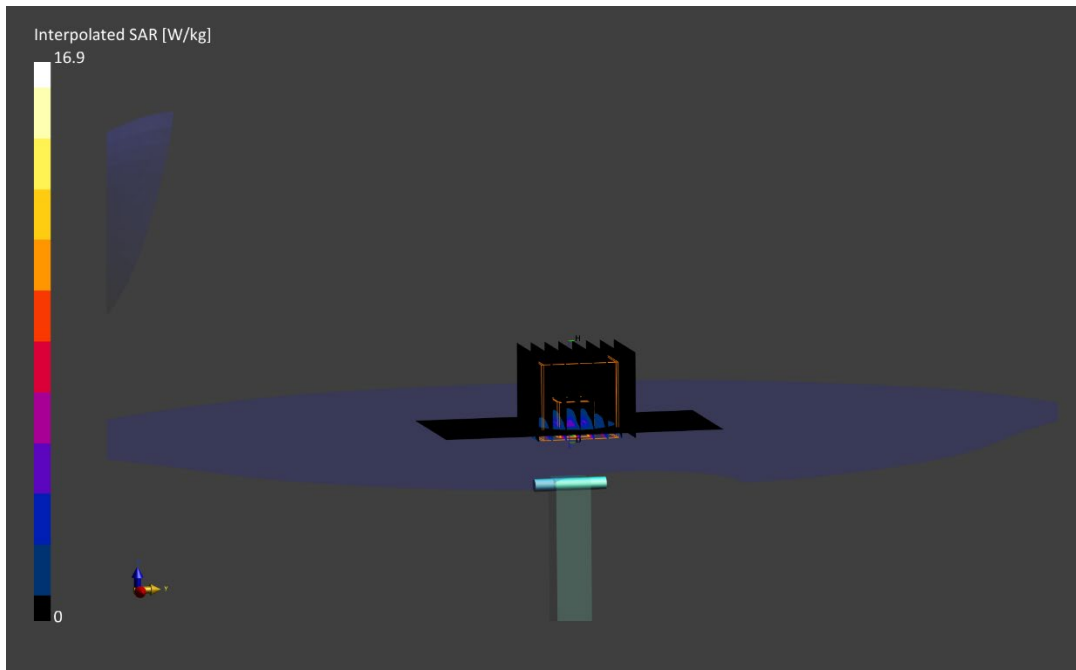

PCTEST

DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1191

Communication System: UID: 0, CW; Frequency: 5750.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5750.0 MHz; cond = 5.11 S/m; perm = 33.8; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/25/2022; Ambient Temp: 20.1°C; Tissue Temp: 19.6°C

Probe: EX3DV4 - SN7668; ConvF:(4.68,4.68,4.68); Calibrated: 2021-08-04
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1272; Calibrated: 2021-03-18
Phantom: Twin-SAM V8.0; Serial: 20063
Measurement SW: DASY Module SAR V16.0.0.116

5750 MHz System Verification at 17 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 15.8 W/kg

SAR(1 g) = 3.67 W/kg

Deviation (1 g) = -6.14%

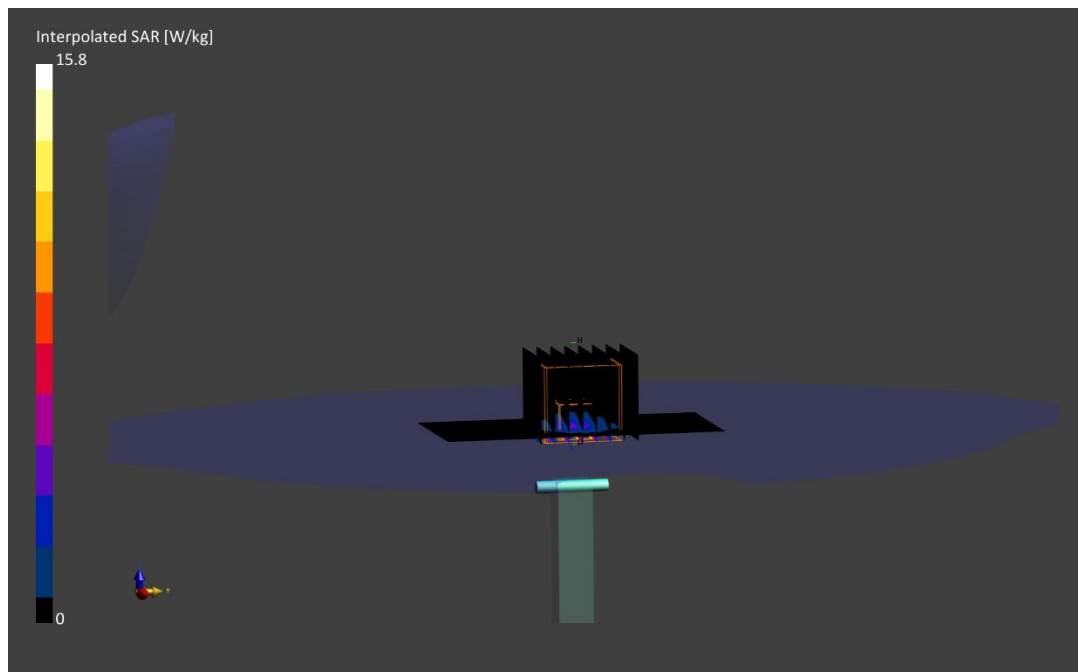

PCTEST

DUT: Dipole 750.0 MHz; Type: D750V3 - SN1161

Communication System: UID: 0, CW; Frequency: 750.0 MHz
Medium: 750 Body; Medium parameters used:
f = 750.0 MHz; cond = 0.943 S/m; perm = 54.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 01/10/2022; Ambient Temp: 20.3°C; Tissue Temp: 20.3°C

Probe: EX3DV4 - SN7661; ConvF:(10.26,10.26,10.26); Calibrated: 2021-06-28
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1450; Calibrated: 2021-08-16
Phantom: Twin-SAM V5.0; Serial: 1692
Measurement SW: DASY Module SAR V16.0.0.116

750 MHz System Verification at 23 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.90 W/kg

SAR(1 g) = 1.83 W/kg

Deviation (1 g) = 4.10%

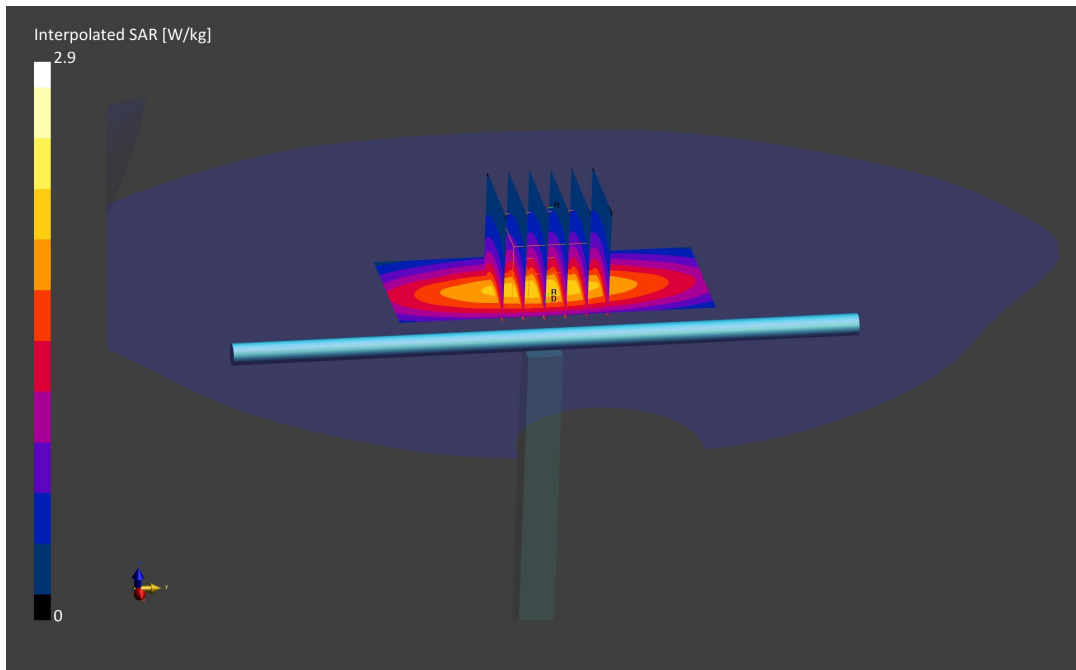

PCTEST

DUT: Dipole 835.0 MHz; Type: D835V2 - SN4d132

Communication System: UID: 0, CW; Frequency: 835.0 MHz
Medium: 835 Body; Medium parameters used:
f = 835.0 MHz; cond = 0.988 S/m; perm = 54.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 01/05/2022; Ambient Temp: 24.4°C; Tissue Temp: 21.8°C

Probe: EX3DV4 - SN7538; ConvF:(9.99,9.99,9.99); Calibrated: 2021-11-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1323; Calibrated: 2021-11-10
Phantom: Twin-SAM V5.0; Serial: 1648
Measurement SW: DASY Module SAR V16.0.0.116

835 MHz System Verification at 23 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 3.29 W/kg

SAR(1 g) = 2.13 W/kg

Deviation (1 g) = 8.56%

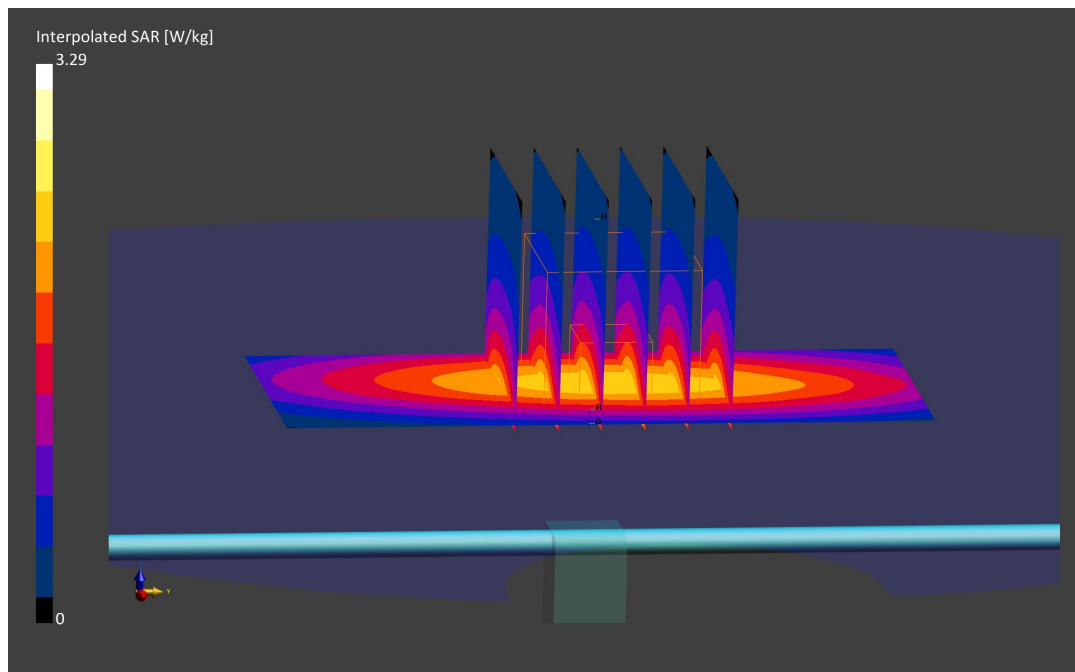

PCTEST

DUT: Dipole 835.0 MHz; Type: D835V2 - SN4d047

Communication System: UID: 0, CW; Frequency: 835.0 MHz
Medium: 835 Body; Medium parameters used:
f = 835.0 MHz; cond = 1.00 S/m; perm = 54.4; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 01/07/2022; Ambient Temp: 22.2°C; Tissue Temp: 21.9°C

Probe: EX3DV4 - SN7538; ConvF:(9.99,9.99,9.99); Calibrated: 2021-11-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1323; Calibrated: 2021-11-10
Phantom: Twin-SAM V5.0; Serial: 1648
Measurement SW: DASY Module SAR V16.0.0.116

835 MHz System Verification at 23 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.90 W/kg

SAR(1 g) = 1.91 W/kg

Deviation (1 g) = 0.84%

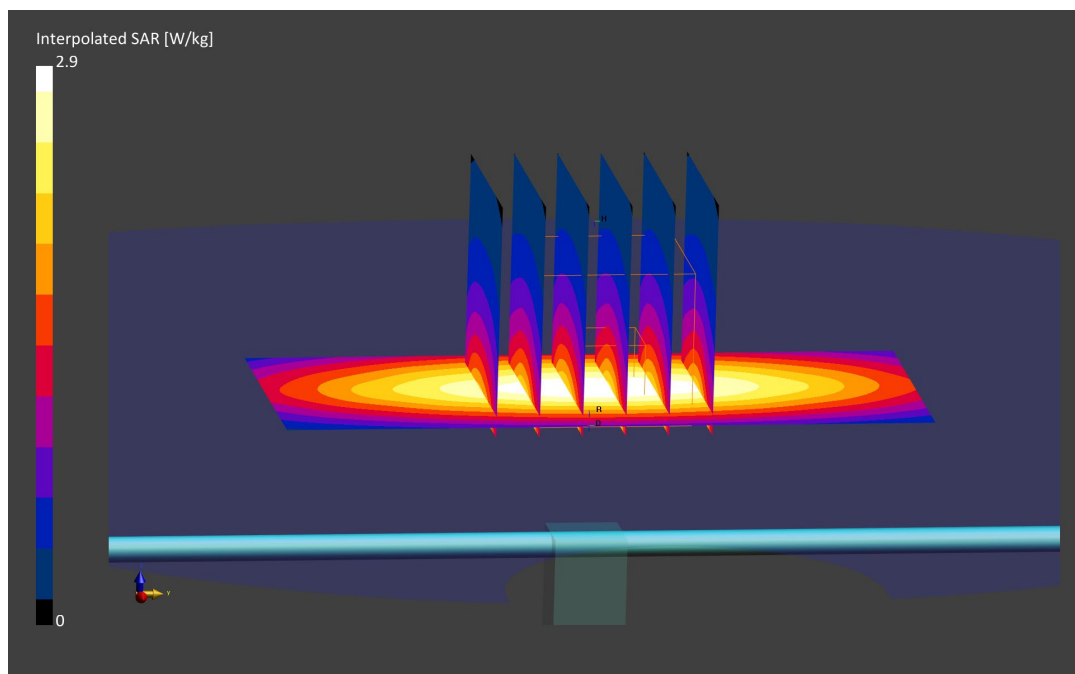

PCTEST

DUT: Dipole 835.0 MHz; Type: D835V2 - SN4d133

Communication System: UID: 0, CW; Frequency: 835.0 MHz
Medium: 835 Body; Medium parameters used:
f = 835.0 MHz; cond = 0.971 S/m; perm = 54.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 01/10/2022; Ambient Temp: 21.1°C; Tissue Temp: 19.9°C

Probe: EX3DV4 - SN7538; ConvF:(9.99,9.99,9.99); Calibrated: 2021-11-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1323; Calibrated: 2021-11-10
Phantom: Twin-SAM V5.0; Serial: 1648
Measurement SW: DASY Module SAR V16.0.0.116

835 MHz System Verification at 23 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 3.00 W/kg

SAR(1 g) = 1.99 W/kg

Deviation (1 g) = 2.68%

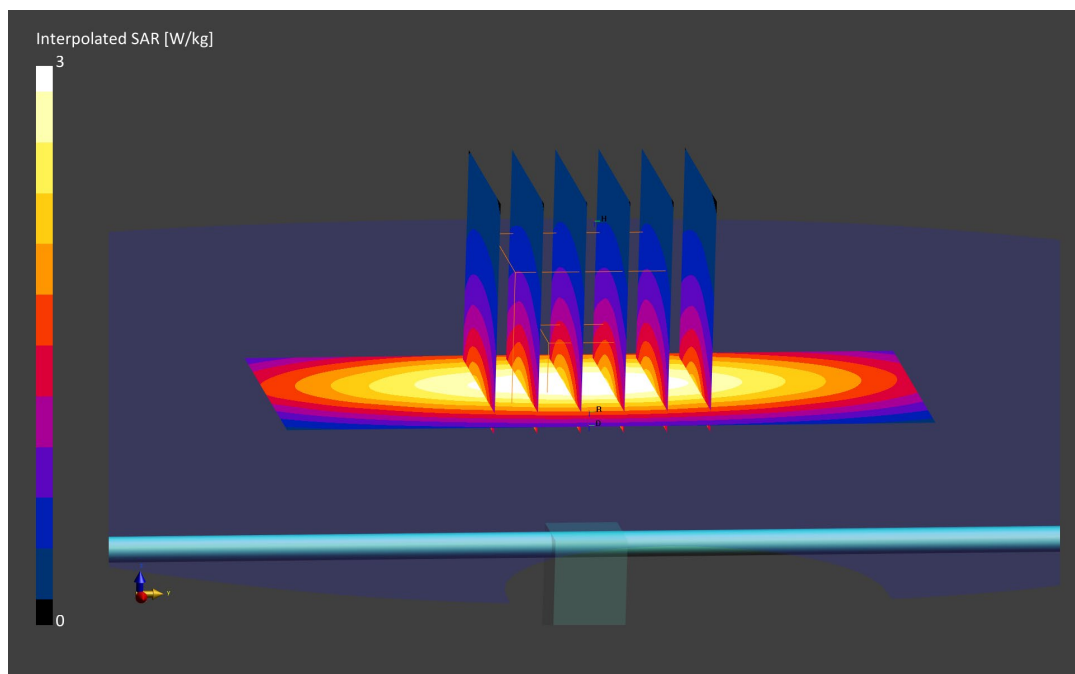

PCTEST

DUT: Dipole 1750.0 MHz; Type: D1765V2 - SN1008

Communication System: UID: 0, CW; Frequency: 1750.0 MHz
Medium: 1750 Body; Medium parameters used:
f = 1750.0 MHz; cond = 1.48 S/m; perm = 53.3; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/10/2022; Ambient Temp: 23.5°C; Tissue Temp: 21.2°C

Probe: EX3DV4 - SN7670; ConvF:(8.36,8.36,8.36); Calibrated: 2021-08-05
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1681; Calibrated: 2021-08-03
Phantom: Twin-SAM V8.0; Serial: 1966
Measurement SW: DASY Module SAR V16.0.0.116

1750 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.29 W/kg

SAR(1 g) = 3.82 W/kg; SAR(10 g) = 2.03 W/kg

Deviation (1 g) = 1.06%; Deviation (10 g) = 2.01%

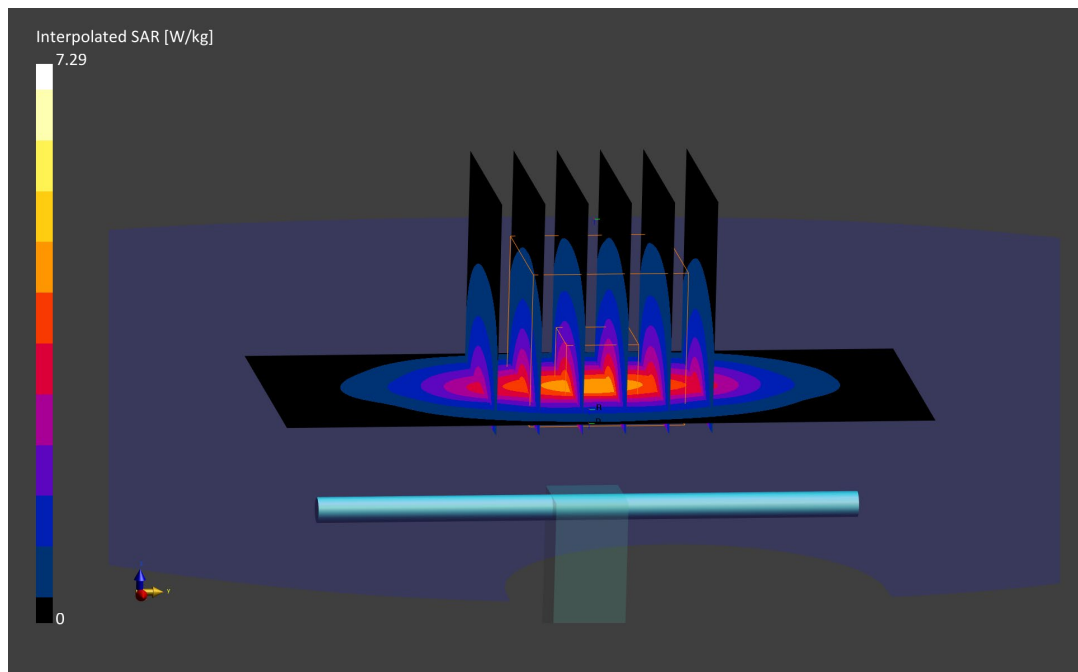

PCTEST

DUT: Dipole 1750.0 MHz; Type: D1765V2 - SN1008

Communication System: UID: 0, CW; Frequency: 1750.0 MHz
Medium: 1750 Body; Medium parameters used:
f = 1750.0 MHz; cond = 1.51 S/m; perm = 53.3; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/13/2022; Ambient Temp: 21.5°C; Tissue Temp: 19.5°C

Probe: EX3DV4 - SN7670; ConvF:(8.36,8.36,8.36); Calibrated: 2021-08-05
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1681; Calibrated: 2021-08-03
Phantom: Twin-SAM V8.0; Serial: 1966
Measurement SW: DASY Module SAR V16.0.0.116

1750 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 6.90 W/kg

SAR(1 g) = 3.73 W/kg; SAR(10 g) = 1.98 W/kg

Deviation (1 g) = -1.32%; Deviation (10 g) = -0.50%

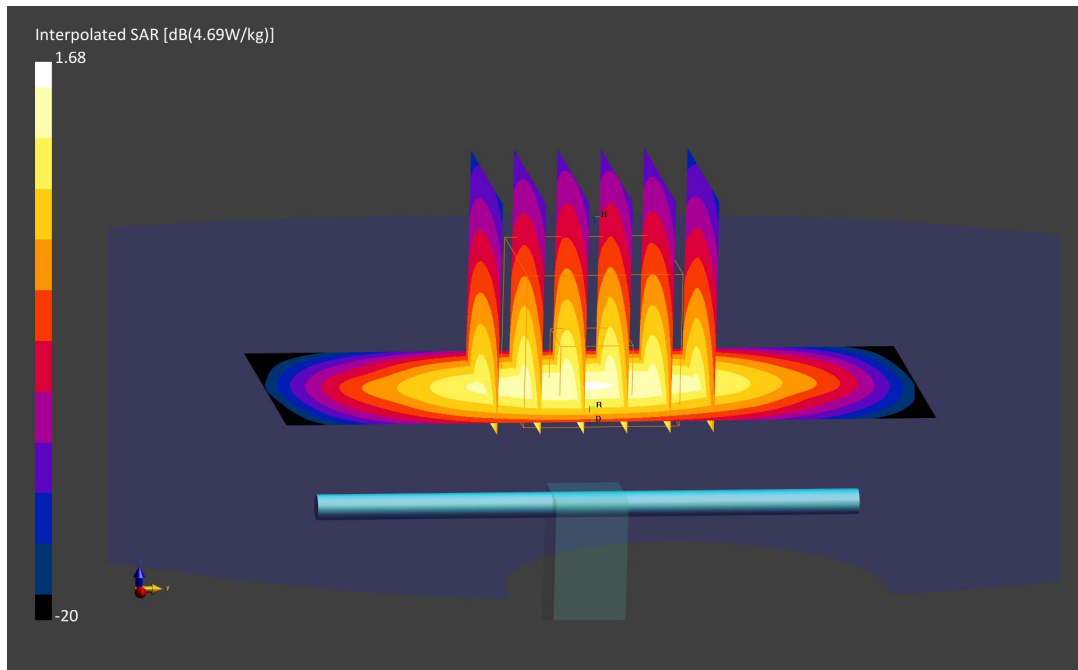

PCTEST

DUT: Dipole 1900.0 MHz; Type: D1900V2 - SN5d080

Communication System: UID: 0, CW; Frequency: 1900.0 MHz
Medium: 1900 Body; Medium parameters used:
f = 1900.0 MHz; cond = 1.53 S/m; perm = 51.3; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/03/2022; Ambient Temp: 20.3°C; Tissue Temp: 20.8°C

Probe: EX3DV4 - SN7410; ConvF:(7.7,7.7,7.7); Calibrated: 2021-07-20
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1583; Calibrated: 2021-07-13
Phantom: Twin-SAM V5.0; Serial: 1792
Measurement SW: DASY Module SAR V16.0.0.116

1900 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.30 W/kg

SAR(1 g) = 3.99 W/kg

Deviation (1 g) = -1.97%

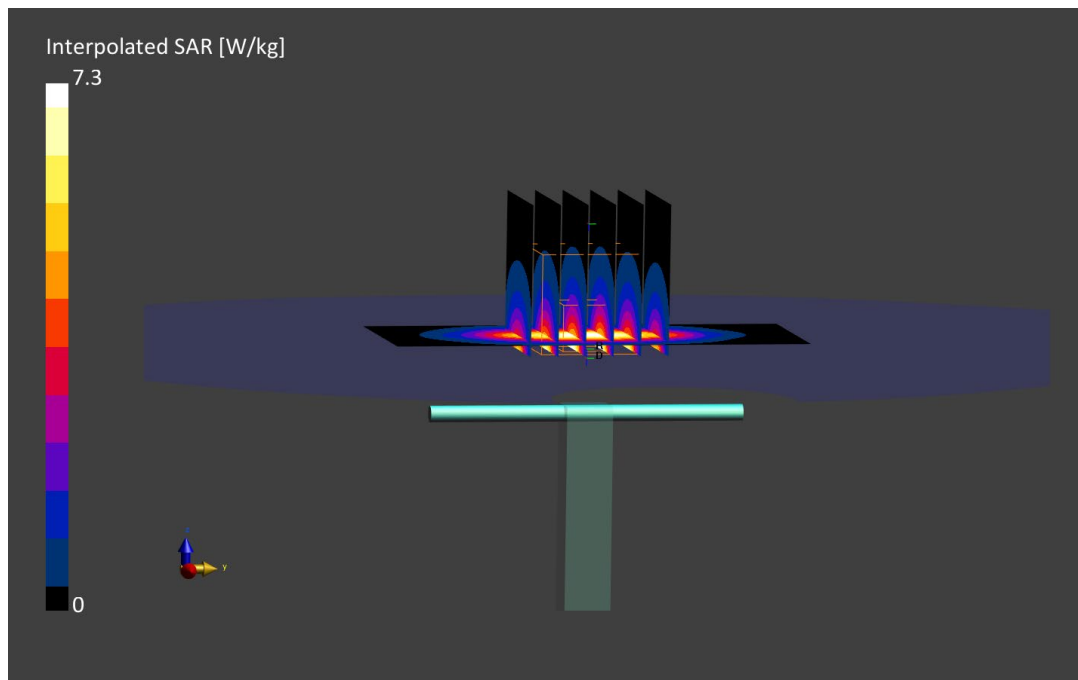

PCTEST

DUT: Dipole 1900.0 MHz; Type: D1900V2 - SN5d080

Communication System: UID: 0, CW; Frequency: 1900.0 MHz
Medium: 1900 Body; Medium parameters used:
f = 1900.0 MHz; cond = 1.53 S/m; perm = 51.5; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/05/2022; Ambient Temp: 20.4°C; Tissue Temp: 20.5°C

Probe: EX3DV4 - SN7410; ConvF:(7.7,7.7,7.7); Calibrated: 2021-07-20
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1583; Calibrated: 2021-07-13
Phantom: Twin-SAM V5.0; Serial: 1792
Measurement SW: DASY Module SAR V16.0.0.116

1900 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.75 W/kg

SAR(1 g) = 4.20 W/kg; SAR(10 g) = 2.15 W/kg

Deviation (1 g) = 3.19%; Deviation (10 g) = 0.47%

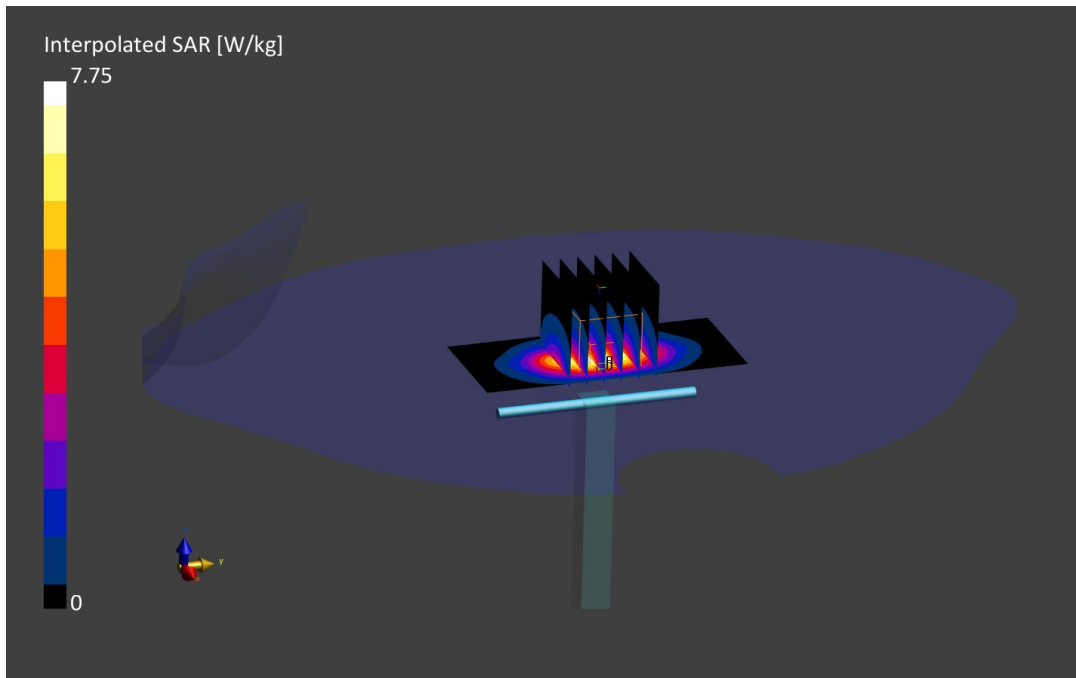

PCTEST

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN981

Communication System: UID: 0, CW; Frequency: 2450.0 MHz
Medium: 2450 Body; Medium parameters used:
f = 2450.0 MHz; cond = 1.91 S/m; perm = 53.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/04/2022; Ambient Temp: 22.4°C; Tissue Temp: 22.1°C

Probe: EX3DV4 - SN3914; ConvF:(7.33,7.33,7.33); Calibrated: 2021-05-18
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn728; Calibrated: 2021-05-11
Phantom: Twin-SAM V5.0; Serial: 1873
Measurement SW: DASY Module SAR V16.0.0.116

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.5 W/kg

SAR(1 g) = 4.87 W/kg

Deviation (1 g) = -3.18%

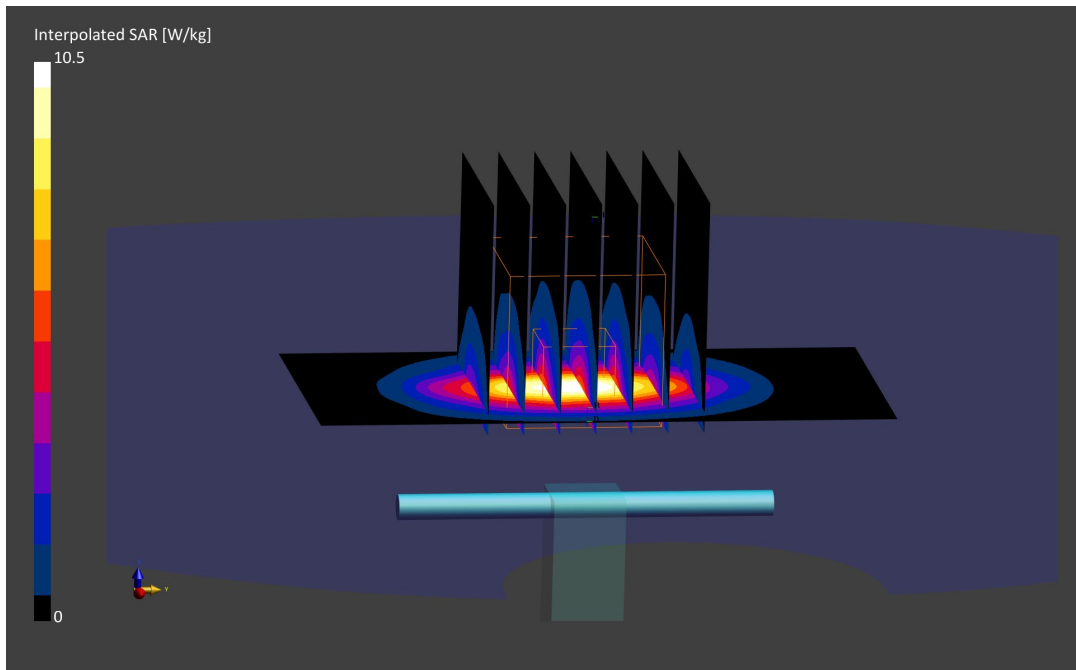

PCTEST

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN719

Communication System: UID: 0, CW; Frequency: 2450.0 MHz
Medium: 2450 Body; Medium parameters used:
f = 2450.0 MHz; cond = 1.99 S/m; perm = 51.1; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/09/2022; Ambient Temp: 21.9°C; Tissue Temp: 21.9°C

Probe: EX3DV4 - SN3914; ConvF:(7.33,7.33,7.33); Calibrated: 2021-05-18
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn728; Calibrated: 2021-05-11
Phantom: Twin-SAM V5.0; Serial: 1873
Measurement SW: DASY Module SAR V16.0.0.116

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.8 W/kg

SAR(1 g) = 5.09 W/kg

Deviation (1 g) = 1.19%

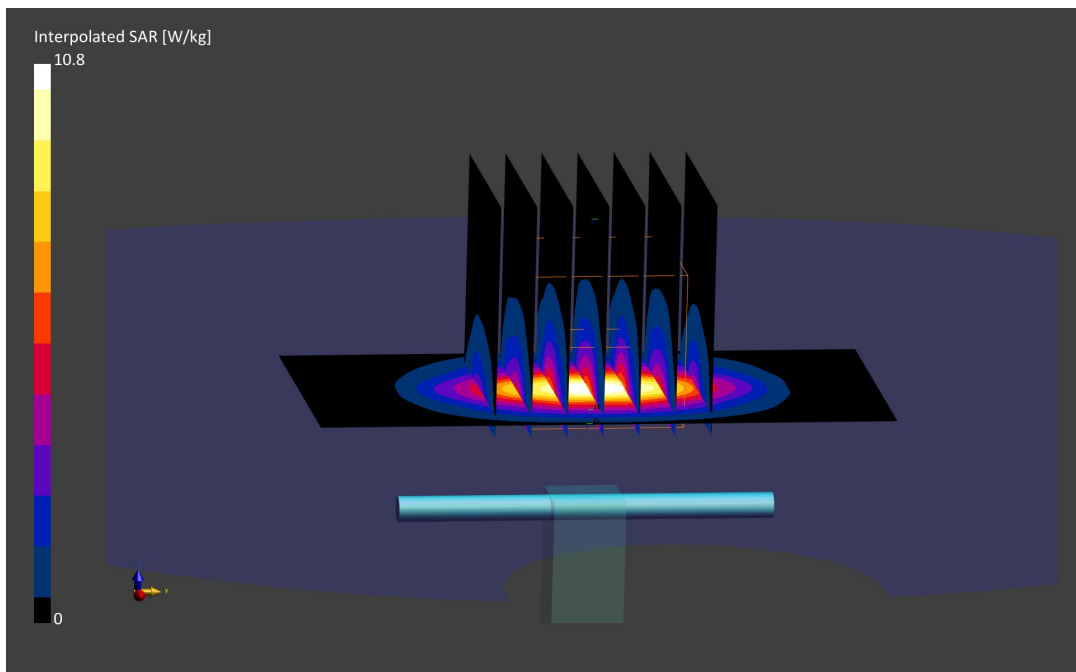

PCTEST

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN719

Communication System: UID: 0, CW; Frequency: 2450.0 MHz
Medium: 2450 Body; Medium parameters used:
f = 2450.0 MHz; cond = 2.01 S/m; perm = 50.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/28/2022; Ambient Temp: 22.0°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7409; ConvF:(7.38,7.38,7.38); Calibrated: 2021-06-21
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1334; Calibrated: 2021-06-15
Phantom: Twin-SAM V5.0; Serial: 1759
Measurement SW: DASY Module SAR V16.0.0.116

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.7 W/kg

SAR(10 g) = 2.30 W/kg

Deviation (10 g) = -6.88%

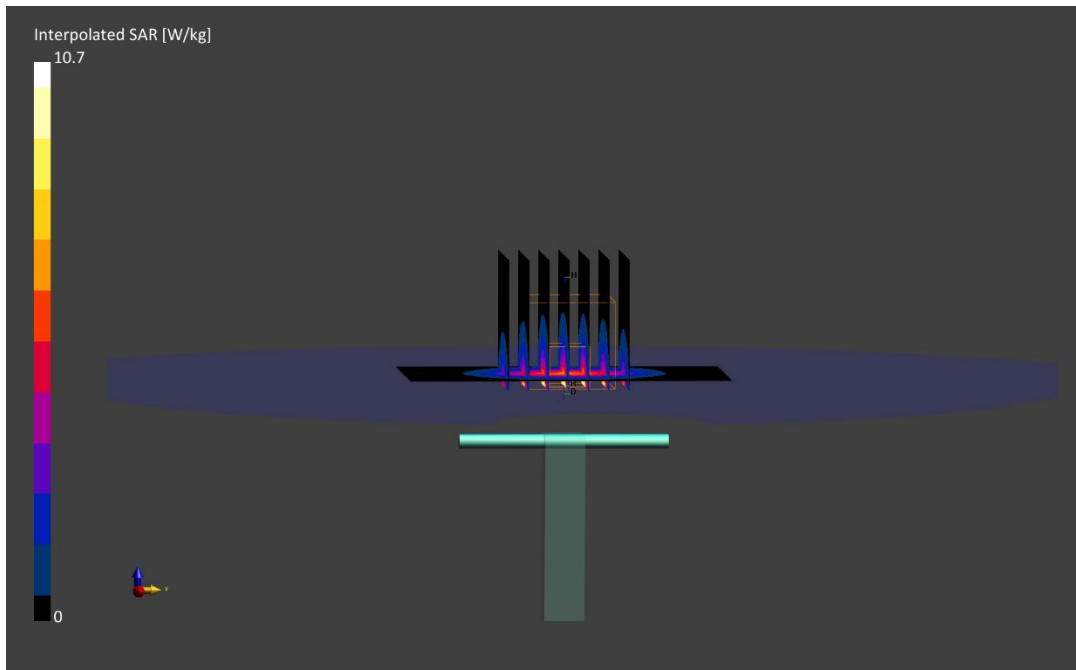

PCTEST

DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1004

Communication System: UID: 0, CW; Frequency: 2600.0 MHz
Medium: 2450 Body; Medium parameters used:
f = 2600.0 MHz; cond = 2.14 S/m; perm = 50.0; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/28/2022; Ambient Temp: 22.0°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7409; ConvF:(7.24,7.24,7.24); Calibrated: 2021-06-21
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1334; Calibrated: 2021-06-15
Phantom: Twin-SAM V5.0; Serial: 1759
Measurement SW: DASY Module SAR V16.0.0.116

2600 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.9 W/kg

SAR(1 g) = 5.54 W/kg; SAR(10 g) = 2.44 W/kg

Deviation (1 g) = 0.00%; Deviation (10 g) = -1.61%

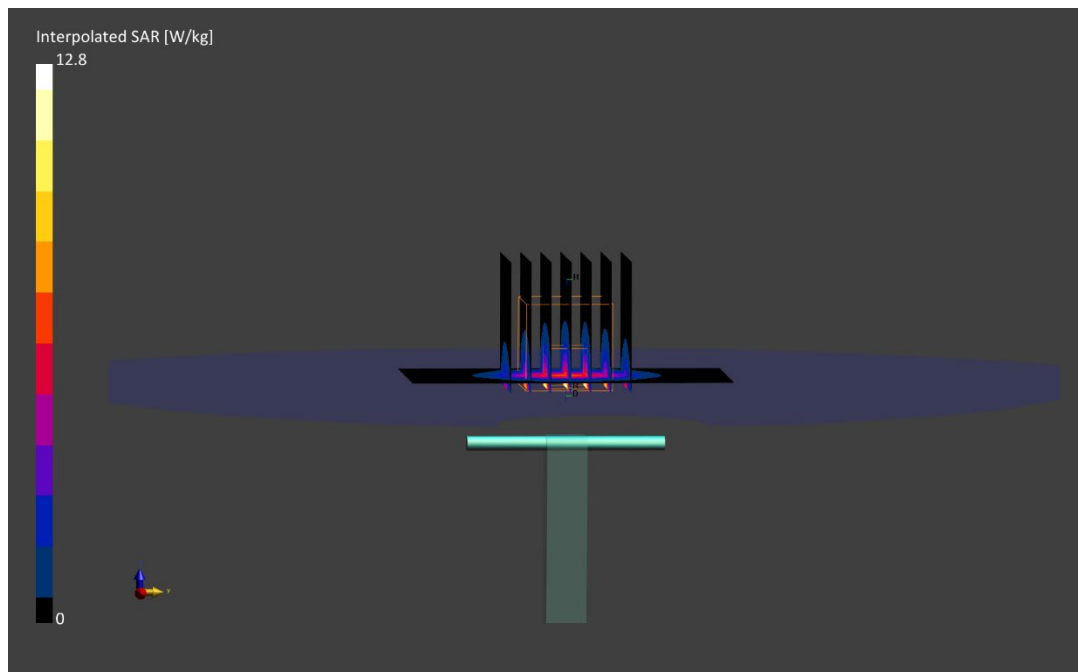

PCTEST

DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1191

Communication System: UID: 0, CW; Frequency: 5250.0 MHz
Medium: 5200-5800 Body; Medium parameters used:
f = 5250.0 MHz; cond = 5.42 S/m; perm = 48.1; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/25/2022; Ambient Temp: 23.4°C; Tissue Temp: 22.0°C

Probe: EX3DV4 - SN7357; ConvF:(4.6,4.6,4.6); Calibrated: 2021-04-19
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1407; Calibrated: 2021-04-07
Phantom: Twin-SAM V5.0; Serial: 1757
Measurement SW: DASY Module SAR V16.0.0.116

5250 MHz System Verification at 17 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 14.4 W/kg

SAR(1 g) = 3.74 W/kg; SAR(10 g) = 1.06 W/kg

Deviation (1 g) = 0.94%; Deviation (10 g) = 1.92%

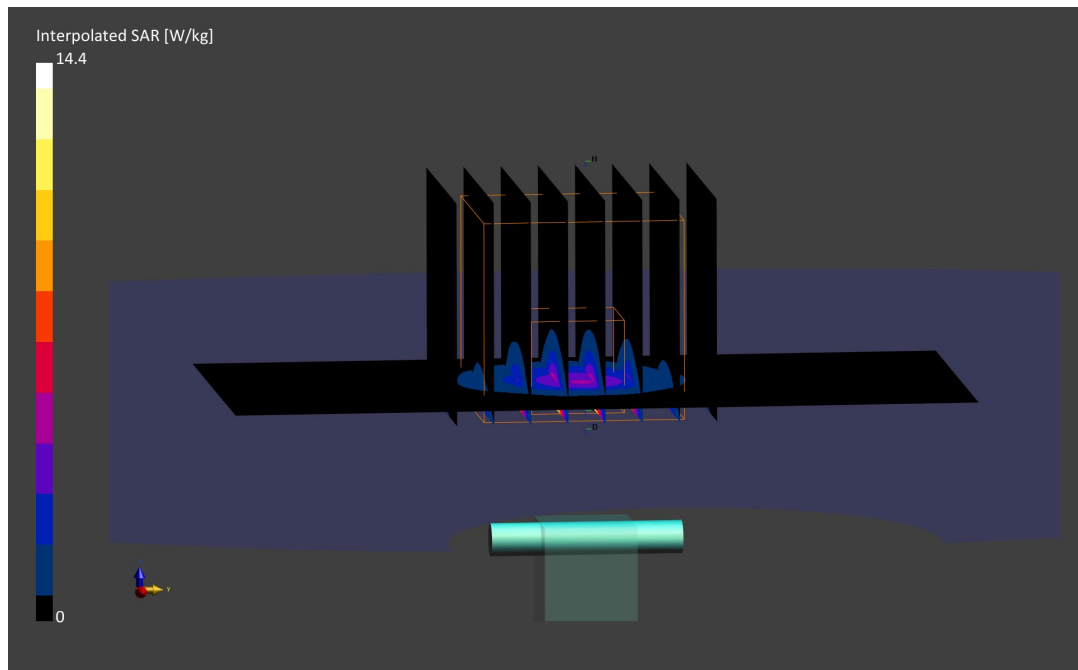

PCTEST

DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1191

Communication System: UID: 0, CW; Frequency: 5600.0 MHz
Medium: 5200-5800 Body; Medium parameters used:
f = 5600.0 MHz; cond = 5.93 S/m; perm = 47.4; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/25/2022; Ambient Temp: 23.4°C; Tissue Temp: 22.0°C

Probe: EX3DV4 - SN7357; ConvF:(4.1,4.1,4.1); Calibrated: 2021-04-19
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1407; Calibrated: 2021-04-07
Phantom: Twin-SAM V5.0; Serial: 1757
Measurement SW: DASY Module SAR V16.0.0.116

5600 MHz System Verification at 17 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.2 W/kg

SAR(1 g) = 3.85 W/kg; SAR(10 g) = 1.08 W/kg

Deviation (1 g) = 0.13%; Deviation (10 g) = 1.41%

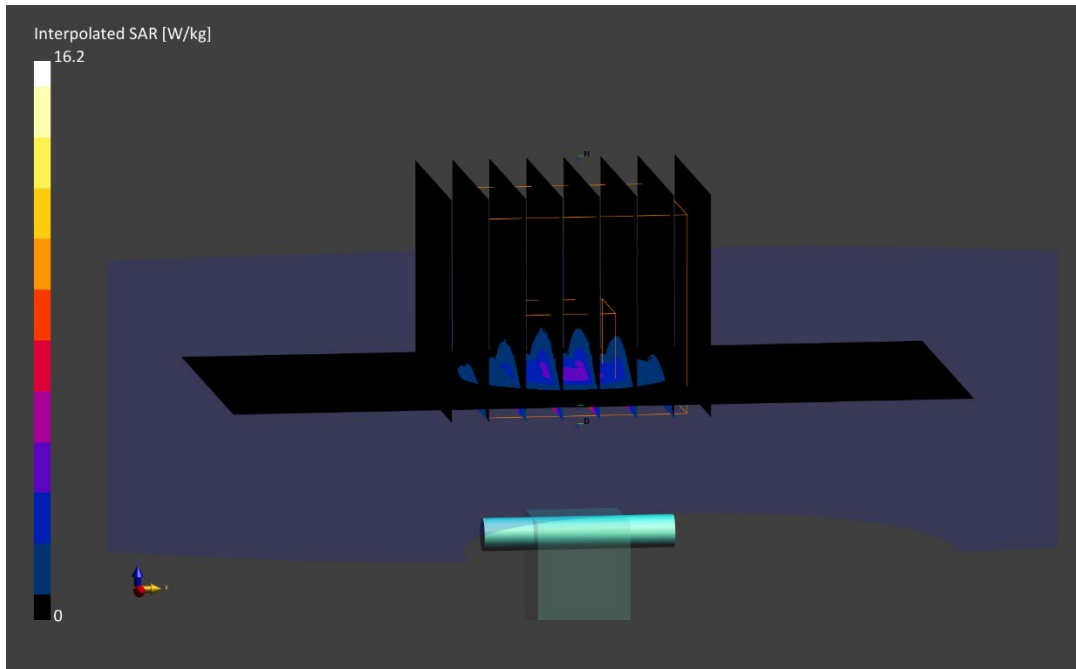

PCTEST

DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1191

Communication System: UID: 0, CW; Frequency: 5750.0 MHz
Medium: 5200-5800 Body; Medium parameters used:
f = 5750.0 MHz; cond = 6.15 S/m; perm = 47.1; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/25/2022; Ambient Temp: 23.4°C; Tissue Temp: 22.0°C

Probe: EX3DV4 - SN7357; ConvF:(4.12,4.12,4.12); Calibrated: 2021-04-19
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1407; Calibrated: 2021-04-07
Phantom: Twin-SAM V5.0; Serial: 1757
Measurement SW: DASY Module SAR V16.0.0.116

5750 MHz System Verification at 17 dBm (50 mW)

Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 15.8 W/kg

SAR(1 g) = 3.68 W/kg; SAR(10 g) = 1.03 W/kg

Deviation (1 g) = -1.08%; Deviation (10 g) = -0.48%

