



HCT Co., Ltd.

74, Seoicheon-ro 578beon-gil, Majang-myeon, Icheon-si, Gyeonggi-do, 17383 KOREA
Tel. +82 31 634 6300 Fax. +82 31 645 6401

Appendix A:
Test Setup
Photo

FCC ID/IC
A3LSMR825/649E-SMR825

File No.
HCT-RF-1907-FI026-P HCT-RF-1907-FI027-P
HCT-RF-1907-FI028-P HCT-RF-1907-FI029-P
HCT-RF-1907-FI030-P HCT-RF-1907-FI031-P
HCT-RF-1907-FI032-P HCT-RF-1907-FI033-P
HCT-RF-1907-FI034-P

REVISION HISTORY

The revision history for this document is shown in table.

Revision No.	Date of Issue	Description
0	July 29, 2019	Initial Release


File No.	HCT-RF-1907-FI026-P	HCT-RF-1907-FI027-P	HCT-RF-1907-FI028-P	HCT-RF-1907-FI029-P	HCT-RF-1907-FI030-P
	HCT-RF-1907-FI031-P	HCT-RF-1907-FI032-P	HCT-RF-1907-FI033-P	HCT-RF-1907-FI034-P	

1. Radiated Test Setup Photo

1.1. stand alone




File	HCT-RF-1907-FI026-P	HCT-RF-1907-FI027-P	HCT-RF-1907-FI028-P	HCT-RF-1907-FI029-P	HCT-RF-1907-FI030-P
No.	HCT-RF-1907-FI031-P	HCT-RF-1907-FI032-P	HCT-RF-1907-FI033-P	HCT-RF-1907-FI034-P	

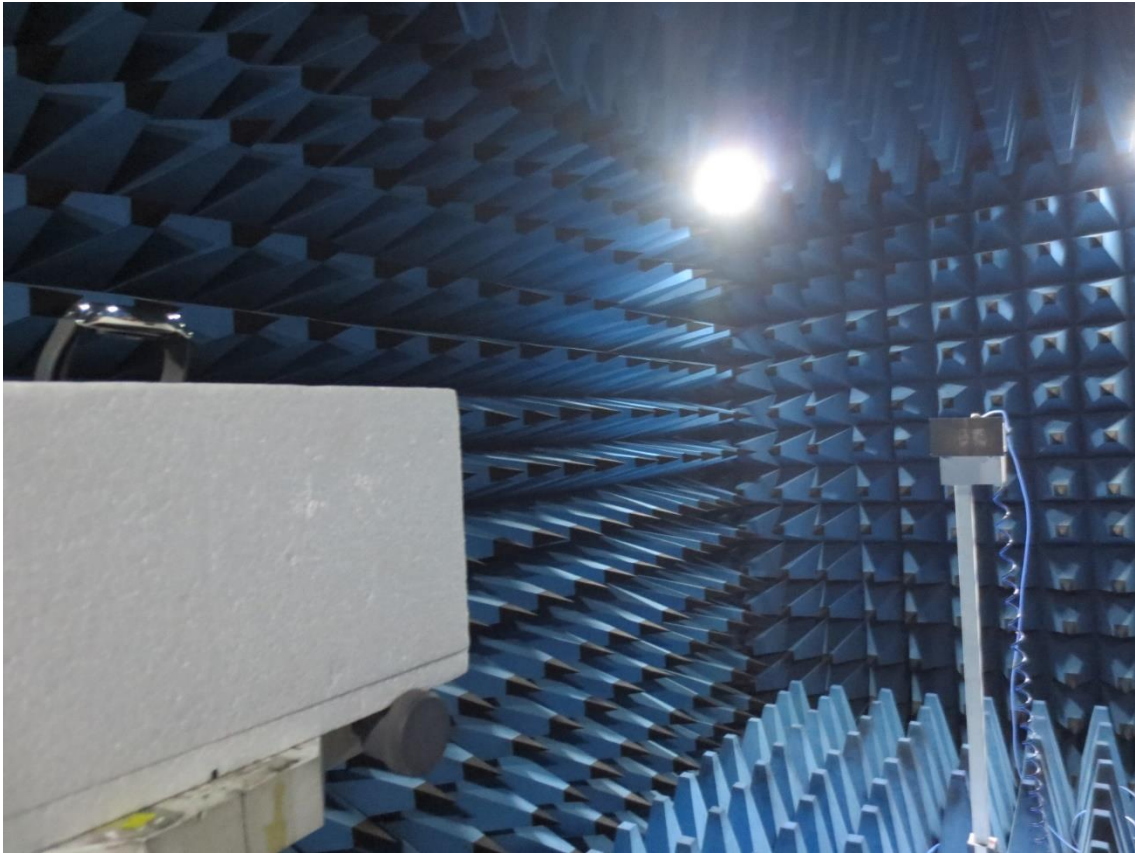


File	HCT-RF-1907-FI026-P	HCT-RF-1907-FI027-P	HCT-RF-1907-FI028-P	HCT-RF-1907-FI029-P	HCT-RF-1907-FI030-P
No.	HCT-RF-1907-FI031-P	HCT-RF-1907-FI032-P	HCT-RF-1907-FI033-P	HCT-RF-1907-FI034-P	




File	HCT-RF-1907-FI026-P	HCT-RF-1907-FI027-P	HCT-RF-1907-FI028-P	HCT-RF-1907-FI029-P	HCT-RF-1907-FI030-P
No.	HCT-RF-1907-FI031-P	HCT-RF-1907-FI032-P	HCT-RF-1907-FI033-P	HCT-RF-1907-FI034-P	

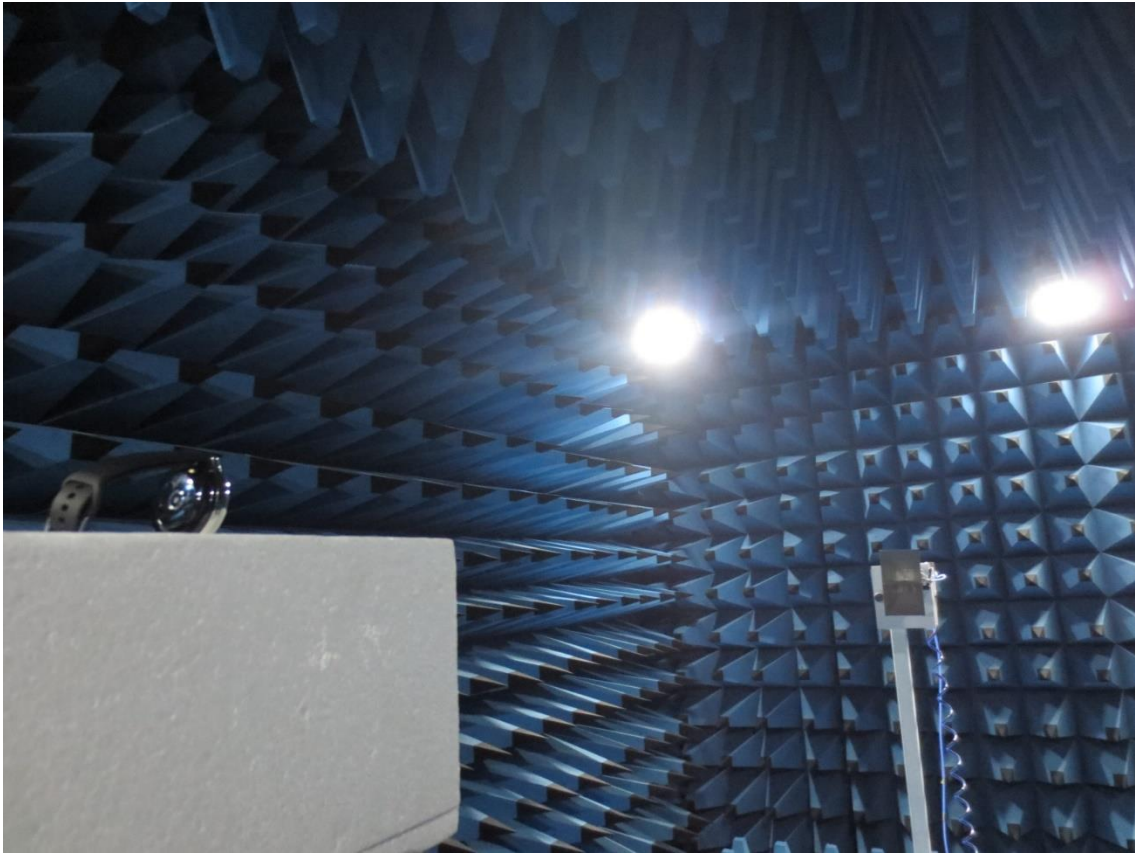


File	HCT-RF-1907-FI026-P	HCT-RF-1907-FI027-P	HCT-RF-1907-FI028-P	HCT-RF-1907-FI029-P	HCT-RF-1907-FI030-P
No.	HCT-RF-1907-FI031-P	HCT-RF-1907-FI032-P	HCT-RF-1907-FI033-P	HCT-RF-1907-FI034-P	

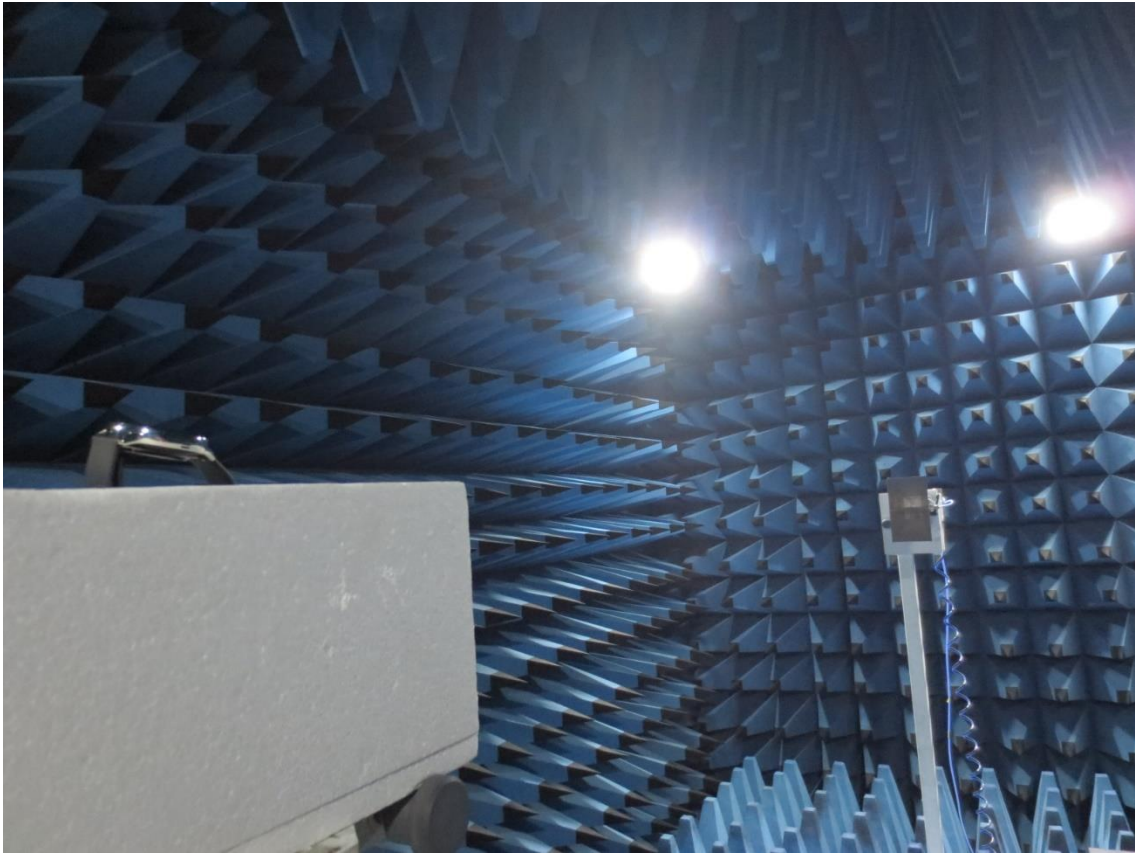


File	HCT-RF-1907-FI026-P	HCT-RF-1907-FI027-P	HCT-RF-1907-FI028-P	HCT-RF-1907-FI029-P	HCT-RF-1907-FI030-P
No.	HCT-RF-1907-FI031-P	HCT-RF-1907-FI032-P	HCT-RF-1907-FI033-P	HCT-RF-1907-FI034-P	

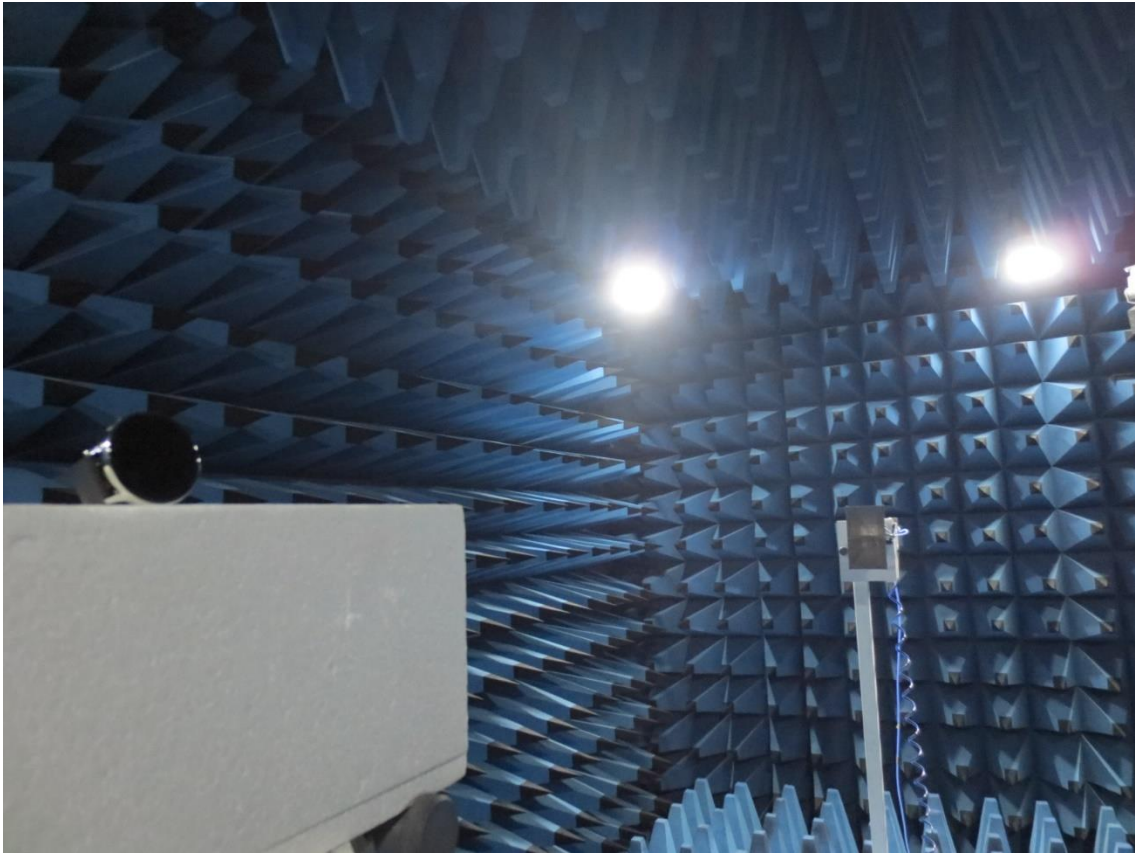


File	HCT-RF-1907-FI026-P	HCT-RF-1907-FI027-P	HCT-RF-1907-FI028-P	HCT-RF-1907-FI029-P	HCT-RF-1907-FI030-P
No.	HCT-RF-1907-FI031-P	HCT-RF-1907-FI032-P	HCT-RF-1907-FI033-P	HCT-RF-1907-FI034-P	

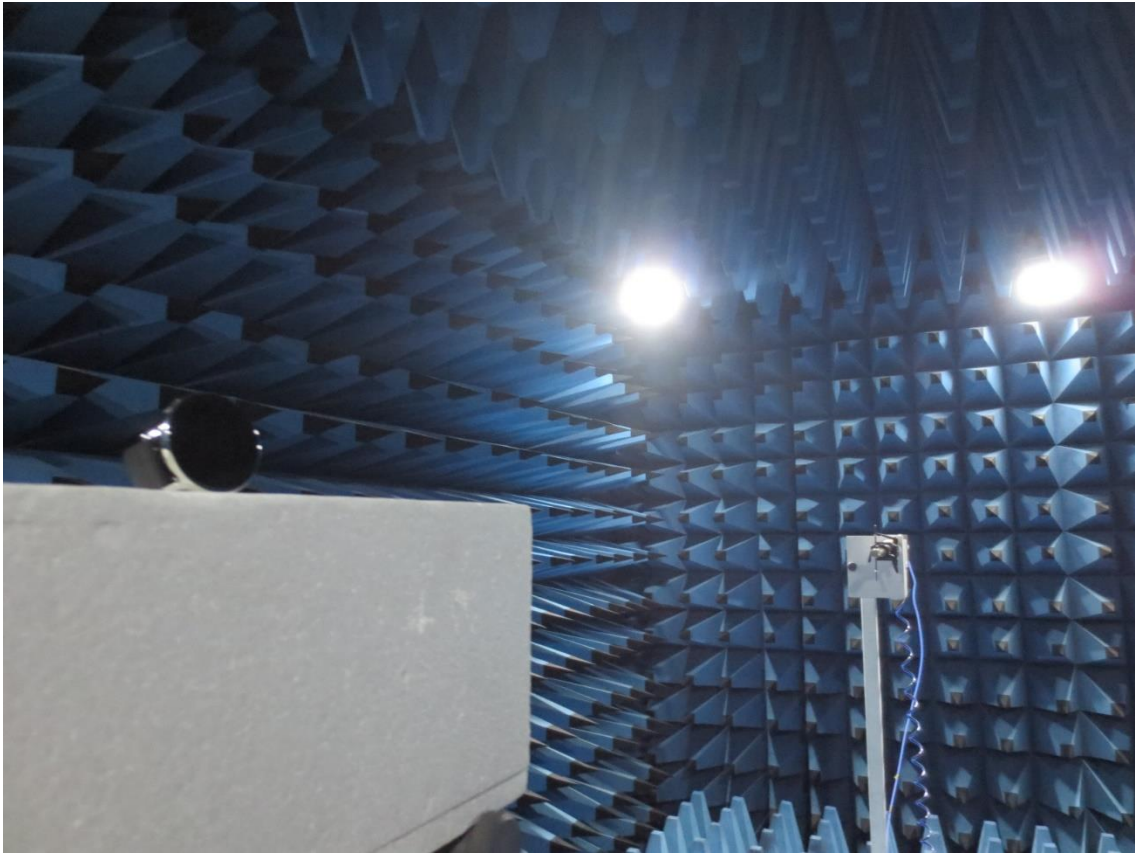


File	HCT-RF-1907-FI026-P	HCT-RF-1907-FI027-P	HCT-RF-1907-FI028-P	HCT-RF-1907-FI029-P	HCT-RF-1907-FI030-P
No.	HCT-RF-1907-FI031-P	HCT-RF-1907-FI032-P	HCT-RF-1907-FI033-P	HCT-RF-1907-FI034-P	

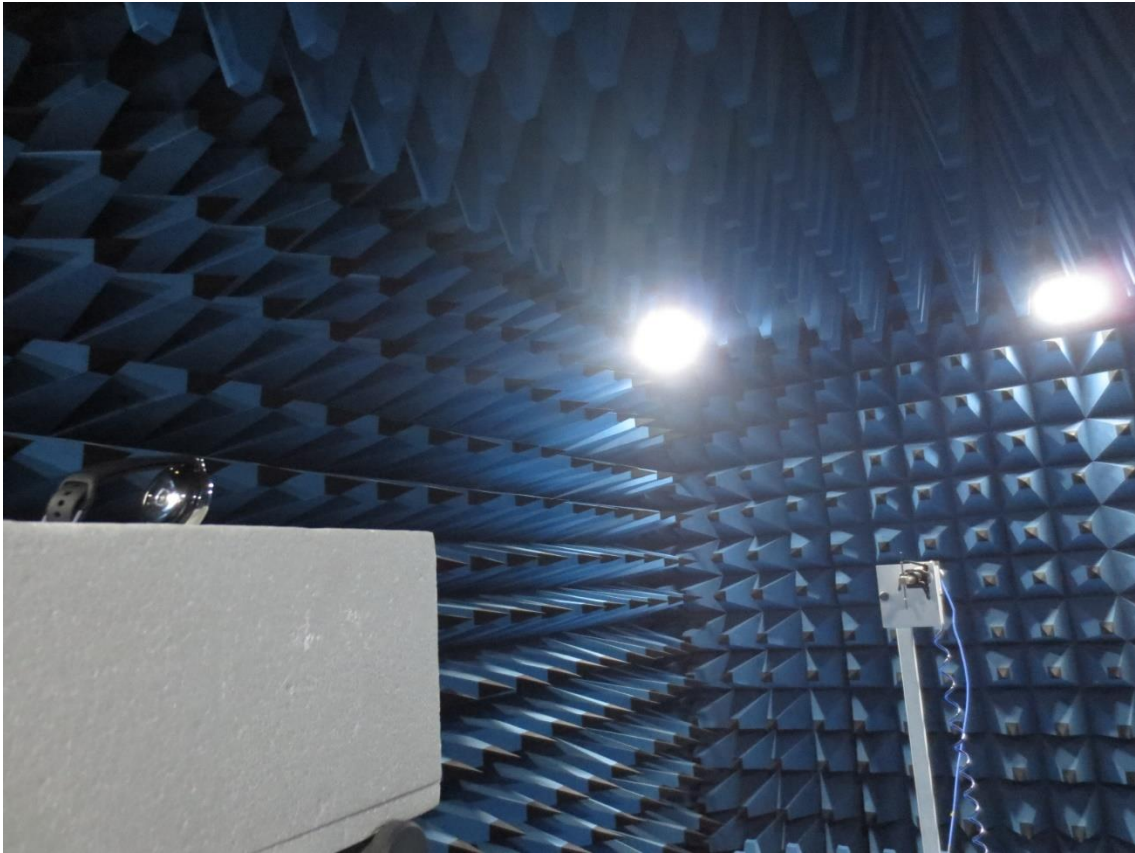


File	HCT-RF-1907-FI026-P	HCT-RF-1907-FI027-P	HCT-RF-1907-FI028-P	HCT-RF-1907-FI029-P	HCT-RF-1907-FI030-P
No.	HCT-RF-1907-FI031-P	HCT-RF-1907-FI032-P	HCT-RF-1907-FI033-P	HCT-RF-1907-FI034-P	

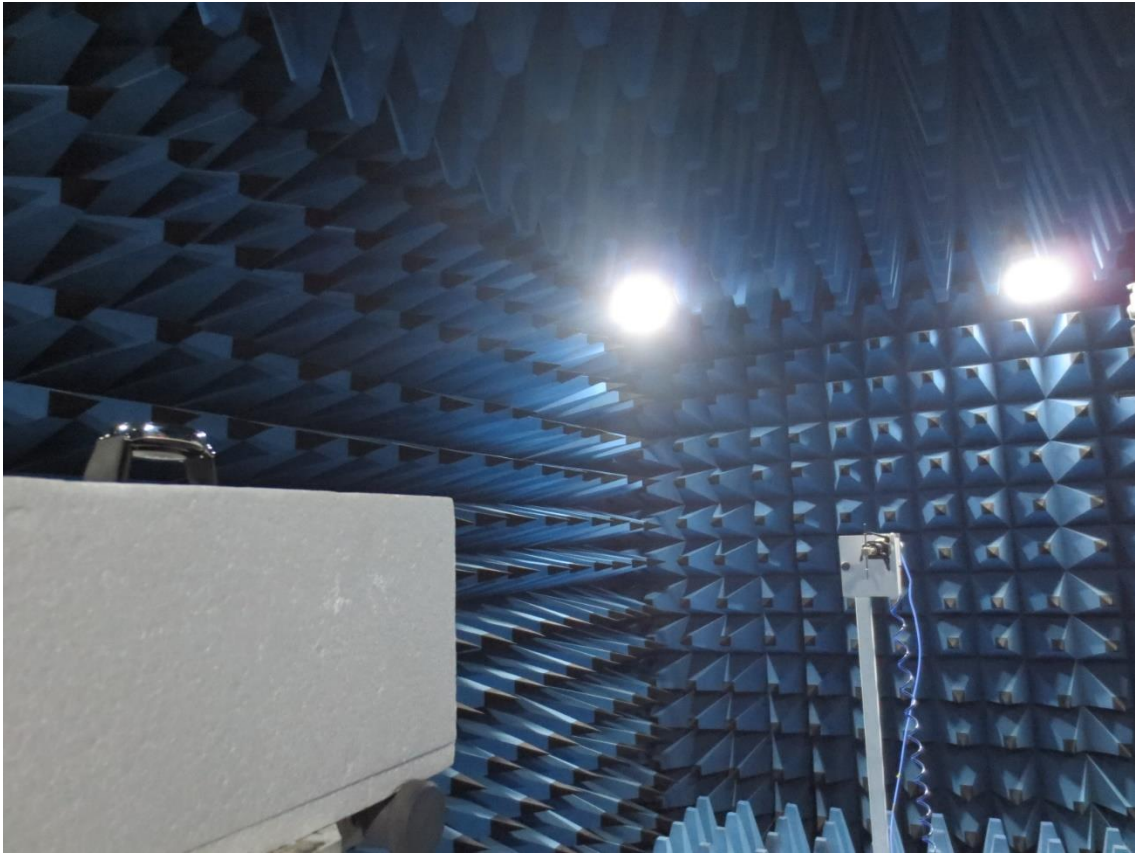


File	HCT-RF-1907-FI026-P	HCT-RF-1907-FI027-P	HCT-RF-1907-FI028-P	HCT-RF-1907-FI029-P	HCT-RF-1907-FI030-P
No.	HCT-RF-1907-FI031-P	HCT-RF-1907-FI032-P	HCT-RF-1907-FI033-P	HCT-RF-1907-FI034-P	

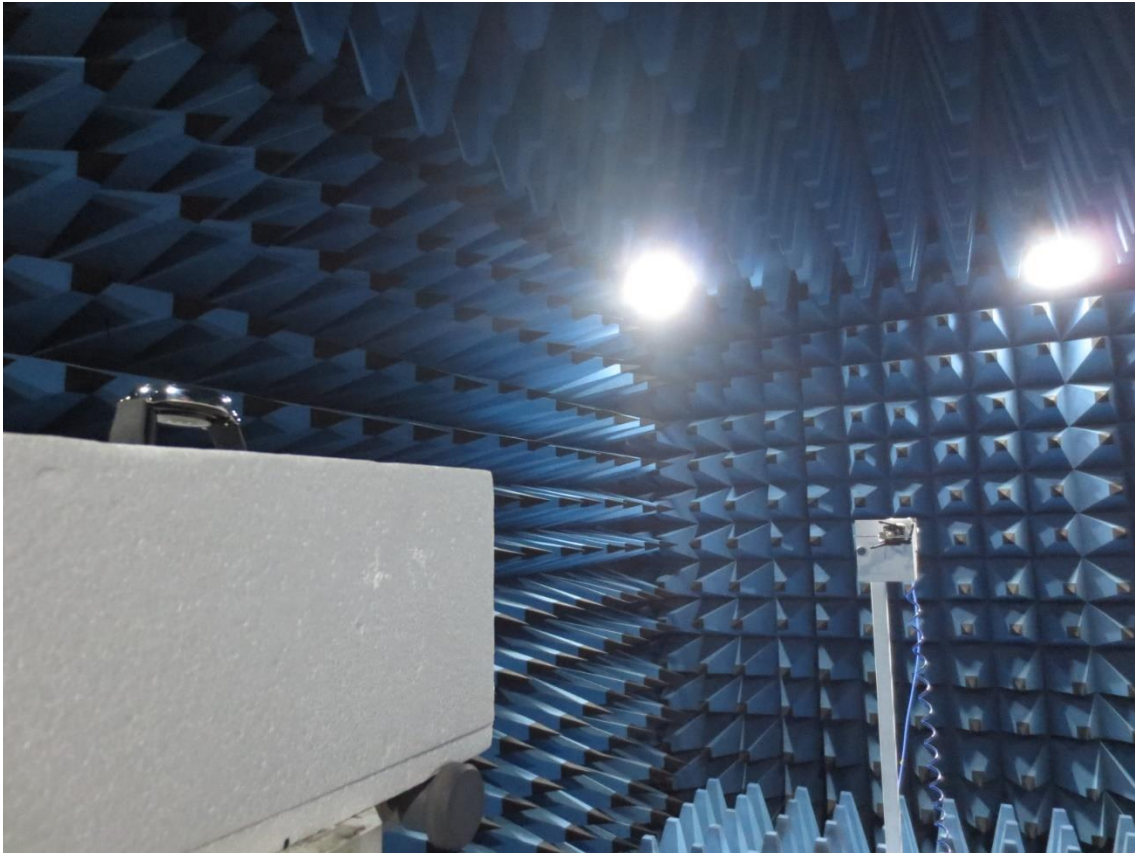

File	HCT-RF-1907-FI026-P	HCT-RF-1907-FI027-P	HCT-RF-1907-FI028-P	HCT-RF-1907-FI029-P	HCT-RF-1907-FI030-P
No.	HCT-RF-1907-FI031-P	HCT-RF-1907-FI032-P	HCT-RF-1907-FI033-P	HCT-RF-1907-FI034-P	

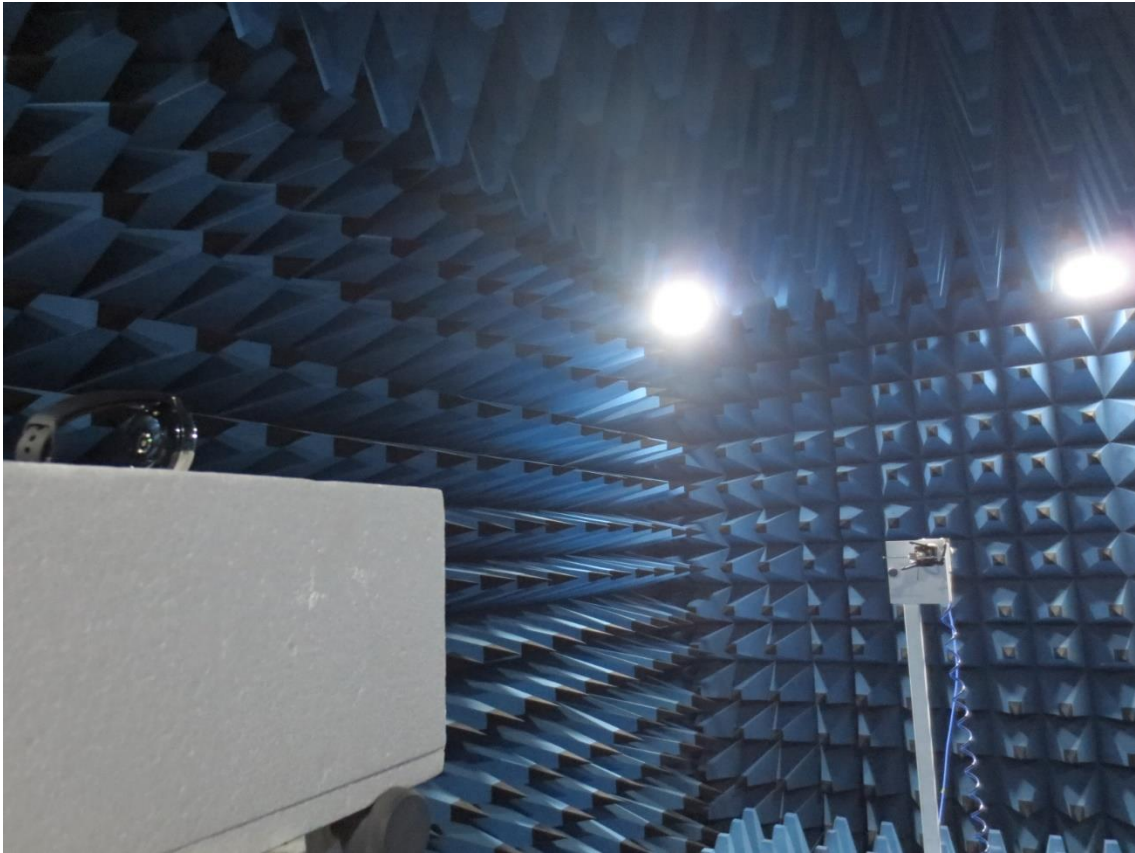

File	HCT-RF-1907-FI026-P	HCT-RF-1907-FI027-P	HCT-RF-1907-FI028-P	HCT-RF-1907-FI029-P	HCT-RF-1907-FI030-P
No.	HCT-RF-1907-FI031-P	HCT-RF-1907-FI032-P	HCT-RF-1907-FI033-P	HCT-RF-1907-FI034-P	

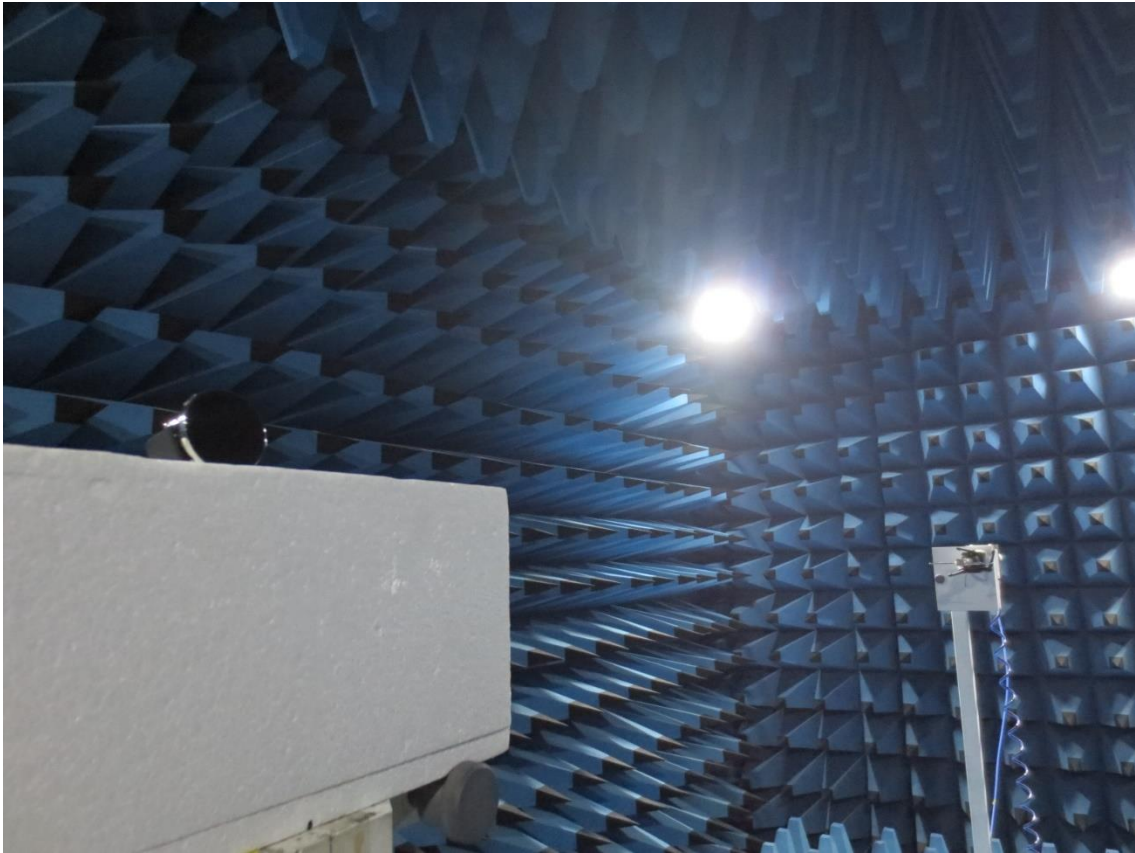


File	HCT-RF-1907-FI026-P	HCT-RF-1907-FI027-P	HCT-RF-1907-FI028-P	HCT-RF-1907-FI029-P	HCT-RF-1907-FI030-P
No.	HCT-RF-1907-FI031-P	HCT-RF-1907-FI032-P	HCT-RF-1907-FI033-P	HCT-RF-1907-FI034-P	

1.2 wireless charging dock




File	HCT-RF-1907-FI026-P	HCT-RF-1907-FI027-P	HCT-RF-1907-FI028-P	HCT-RF-1907-FI029-P	HCT-RF-1907-FI030-P
No.	HCT-RF-1907-FI031-P	HCT-RF-1907-FI032-P	HCT-RF-1907-FI033-P	HCT-RF-1907-FI034-P	

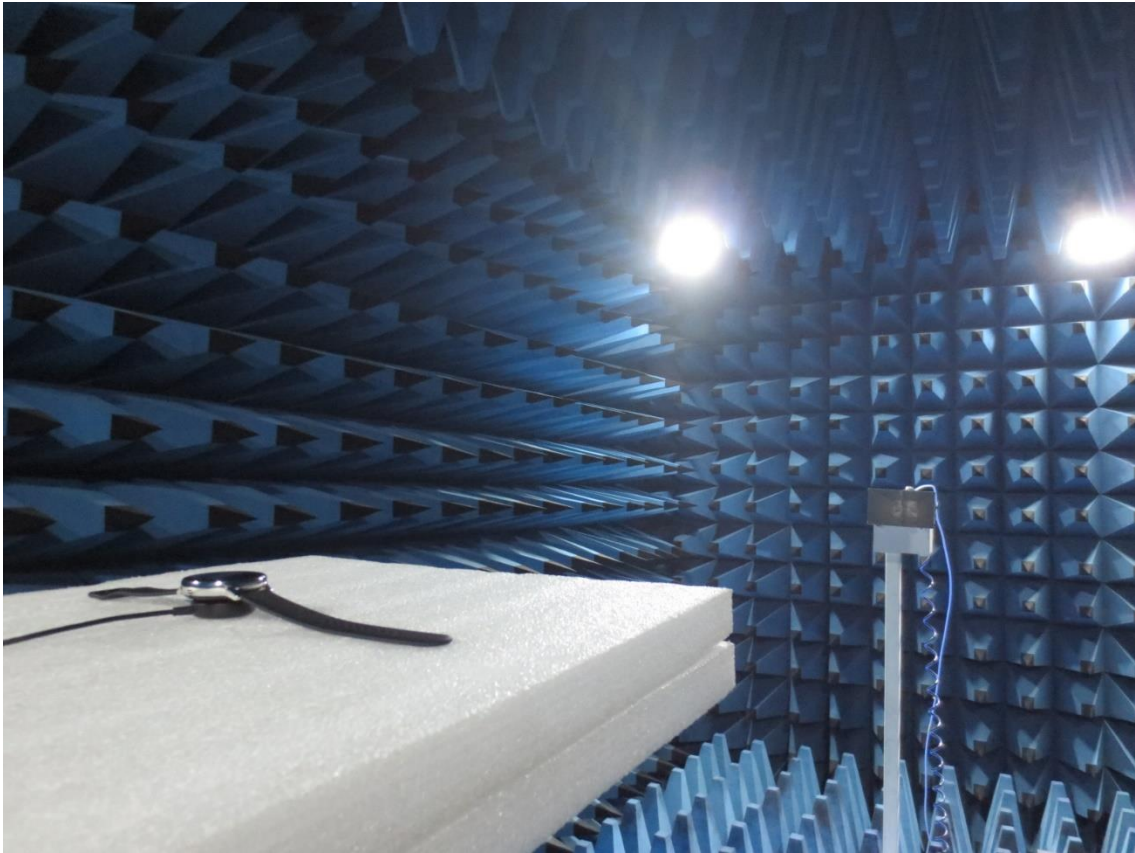

File	HCT-RF-1907-FI026-P	HCT-RF-1907-FI027-P	HCT-RF-1907-FI028-P	HCT-RF-1907-FI029-P	HCT-RF-1907-FI030-P
No.	HCT-RF-1907-FI031-P	HCT-RF-1907-FI032-P	HCT-RF-1907-FI033-P	HCT-RF-1907-FI034-P	




File	HCT-RF-1907-FI026-P	HCT-RF-1907-FI027-P	HCT-RF-1907-FI028-P	HCT-RF-1907-FI029-P	HCT-RF-1907-FI030-P
No.	HCT-RF-1907-FI031-P	HCT-RF-1907-FI032-P	HCT-RF-1907-FI033-P	HCT-RF-1907-FI034-P	

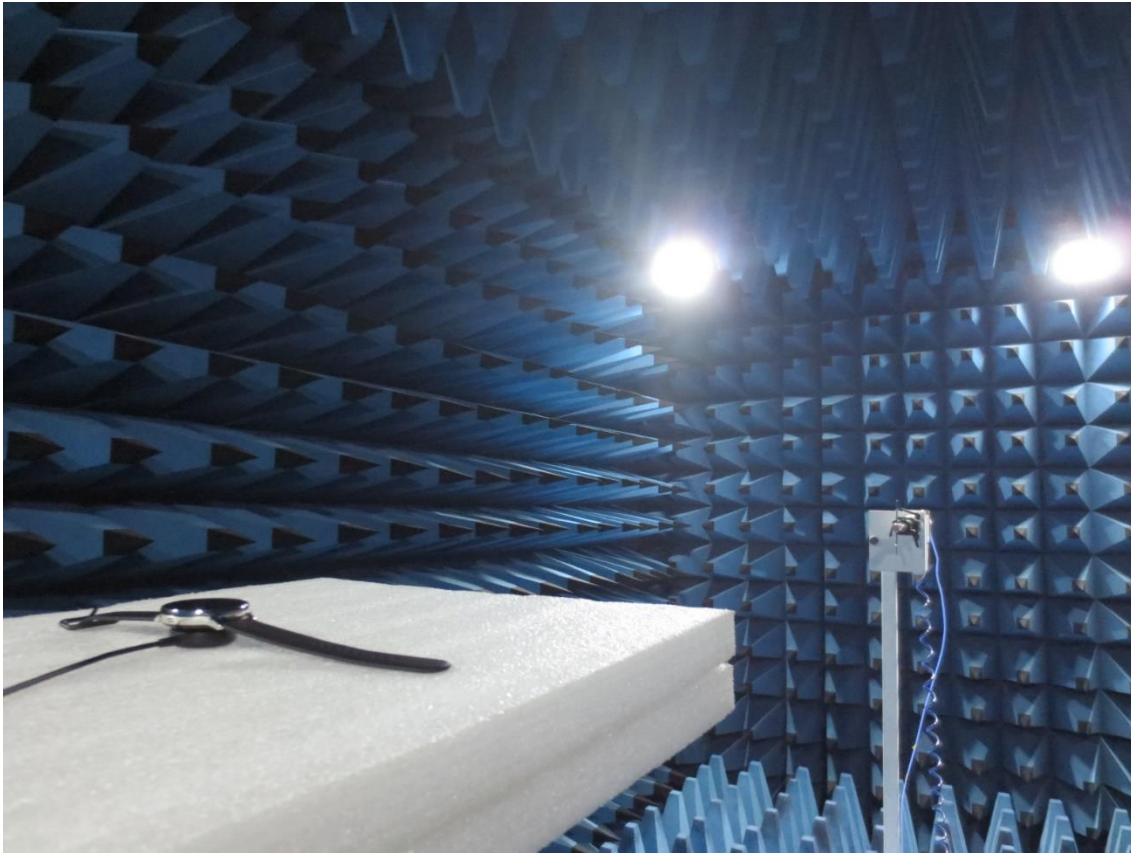

File	HCT-RF-1907-FI026-P	HCT-RF-1907-FI027-P	HCT-RF-1907-FI028-P	HCT-RF-1907-FI029-P	HCT-RF-1907-FI030-P
No.	HCT-RF-1907-FI031-P	HCT-RF-1907-FI032-P	HCT-RF-1907-FI033-P	HCT-RF-1907-FI034-P	

2. Conducted Test Setup Photo

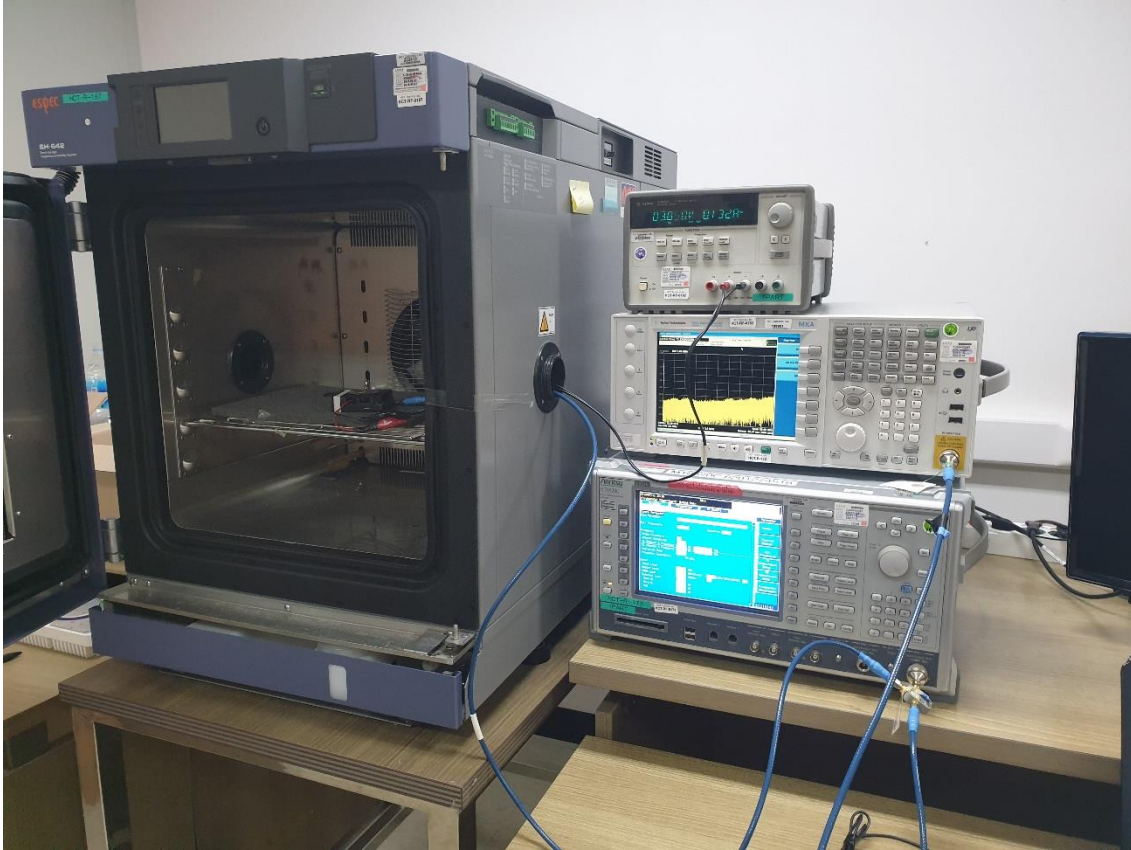

File	HCT-RF-1907-FI026-P	HCT-RF-1907-FI027-P	HCT-RF-1907-FI028-P	HCT-RF-1907-FI029-P	HCT-RF-1907-FI030-P
No.	HCT-RF-1907-FI031-P	HCT-RF-1907-FI032-P	HCT-RF-1907-FI033-P	HCT-RF-1907-FI034-P	