# APPENDIX C: SAR TISSUE SPECIFICATIONS

## Measurement Procedure for Tissue verification:

1) The network analyzer and probe system was configured and calibrated.
2) The probe was immersed in the tissue. The tissue was placed in a nonmetallic container. Trapped air bubbles beneath the flange were minimized by placing the probe at a slight angle.
3) The complex admittance with respect to the probe aperture was measured
4) The complex relative permittivity $\varepsilon_r'$ can be calculated from the below equation (Pournaropoulos and Misra):

$$Y = \frac{j2\omega\varepsilon_r\varepsilon_0}{\left[\ln(b/a)\right]^2}\int_a^b\int_a^b\int_0^\pi \cos\phi' \frac{\exp\left[-j\omega r(\mu_0\varepsilon_r'\varepsilon_0)^{1/2}\right]}{r} d\phi' d\rho' d\rho$$

where $Y$ is the admittance of the probe in contact with the sample, the primed and unprimed coordinates refer to source and observation points, respectively, $r^2 = \rho^2 + \rho'^2 - 2\rho\rho'\cos\phi'$, $\omega$ is the angular frequency, and $j = \sqrt{-1}$.

**3 Composition / Information on ingredients**

**3.2 Mixtures**
**Description:** Aqueous solution with surfactants and inhibitors
**Declarable, or hazardous components:**

| | | |
|---|---|---|
| CAS: 107-21-1<br>EINECS: 203-473-3<br>Reg.nr.: 01-2119456816-28-0000 | **Ethanediol**<br>STOT RE 2, H373;<br>Acute Tox. 4, H302 | >1.0-4.9% |
| CAS: 68608-26-4<br>EINECS: 271-781-5<br>Reg.nr.: 01-2119527859-22-0000 | **Sodium petroleum sulfonate**<br>Eye Irrit. 2, H319 | < 2.9% |
| CAS: 107-41-5<br>EINECS: 203-489-0<br>Reg.nr.: 01-2119539582-35-0000 | **Hexylene Glycol / 2-Methyl-pentane-2,4-diol**<br>Skin Irrit. 2, H315; Eye Irrit. 2, H319 | < 2.9% |
| CAS: 68920-66-1<br>NLP: 500-236-9<br>Reg.nr.: 01-2119489407-26-0000 | **Alkoxylated alcohol, > $C_{16}$**<br>Aquatic Chronic 2, H411;<br>Skin Irrit. 2, H315; Eye Irrit. 2, H319 | < 2.0% |

**Additional information:**
For the wording of the listed risk phrases refer to section 16.
Not mentioned CAS-, EINECS- or registration numbers are to be regarded as Proprietary/Confidential.
The specific chemical identity and/or exact percentage concentration of proprietary components is withheld as a trade secret.

**Figure C-1**

Note: Liquid recipes are proprietary SPEAG. Since the composition is approximate to the actual liquids utilized, the manufacturer tissue-equivalent liquid data sheets are provided below.



© 2022 PCTEST

Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland
Phone +41 44 245 9700, Fax +41 44 245 9779
info@speag.com, http://www.speag.com

**Measurement Certificate / Material Test**

| | |
|---|---|
| Item Name | **Body Tissue Simulating Liquid (MBBL600-6000V6)** |
| Product No. | SL AAM U16 BC (Batch: 200803-1) |
| Manufacturer | SPEAG |

**Measurement Method**

TSL dielectric parameters measured using calibrated DAK probe.

**Target Parameters**

Target parameters as defined in the KDB 865664 compliance standard.

**Test Condition**

| | |
|---|---|
| Ambient Condition | 22°C ; 30% humidity |
| TSL Temperature | 22°C |
| Test Date | 6-Aug-20 |
| Operator | CL |

**Additional Information**

TSL Density
TSL Heat-capacity

**Results**

| | Measured | | | Target | | Diff.to Target [%] | |
|---|---|---|---|---|---|---|---|
| f [MHz] | e' | e'' | sigma | eps | sigma | Δ-eps | Δ-sigma |
| 600 | 56.3 | 26.8 | 0.89 | 56.1 | 0.95 | 0.3 | -6.3 |
| 750 | 55.8 | 22.6 | 0.94 | 55.5 | 0.96 | 0.5 | -2.1 |
| 800 | 55.7 | 21.6 | 0.96 | 55.3 | 0.97 | 0.7 | -1.0 |
| 825 | 55.7 | 21.1 | 0.97 | 55.2 | 0.98 | 0.8 | -1.0 |
| 835 | 55.7 | 20.9 | 0.98 | 55.1 | 0.99 | 1.0 | -0.5 |
| 850 | 55.6 | 20.7 | 0.98 | 55.2 | 0.99 | 0.8 | -1.0 |
| 900 | 55.5 | 19.9 | 1.00 | 55.0 | 1.05 | 0.9 | -4.8 |
| 1400 | 54.7 | 15.9 | 1.24 | 54.1 | 1.28 | 1.1 | -3.1 |
| 1450 | 54.6 | 15.8 | 1.27 | 54.0 | 1.30 | 1.1 | -2.3 |
| 1600 | 54.4 | 15.3 | 1.36 | 53.8 | 1.39 | 1.1 | -2.2 |
| 1625 | 54.4 | 15.3 | 1.38 | 53.8 | 1.41 | 1.2 | -2.1 |
| 1640 | 54.4 | 15.2 | 1.39 | 53.7 | 1.42 | 1.3 | -2.1 |
| 1650 | 54.3 | 15.2 | 1.39 | 53.7 | 1.43 | 1.1 | -2.8 |
| 1700 | 54.2 | 15.1 | 1.43 | 53.6 | 1.46 | 1.2 | -2.1 |
| 1750 | 54.2 | 15.0 | 1.46 | 53.4 | 1.49 | 1.4 | -2.0 |
| 1800 | 54.1 | 14.9 | 1.50 | 53.3 | 1.52 | 1.5 | -1.3 |
| 1810 | 54.1 | 14.9 | 1.51 | 53.3 | 1.52 | 1.5 | -0.7 |
| 1825 | 54.1 | 14.9 | 1.52 | 53.3 | 1.52 | 1.5 | 0.0 |
| 1850 | 54.0 | 14.9 | 1.53 | 53.3 | 1.52 | 1.3 | 0.7 |
| 1900 | 54.0 | 14.8 | 1.57 | 53.3 | 1.52 | 1.3 | 3.3 |
| 1950 | 53.9 | 14.8 | 1.60 | 53.3 | 1.52 | 1.1 | 5.3 |
| 2000 | 53.8 | 14.8 | 1.64 | 53.3 | 1.52 | 0.9 | 7.9 |
| 2050 | 53.8 | 14.7 | 1.68 | 53.2 | 1.57 | 1.1 | 7.0 |
| 2100 | 53.7 | 14.7 | 1.72 | 53.2 | 1.62 | 1.0 | 6.2 |
| 2150 | 53.7 | 14.7 | 1.76 | 53.1 | 1.66 | 1.1 | 6.0 |
| 2200 | 53.6 | 14.7 | 1.80 | 53.0 | 1.71 | 1.1 | 5.3 |
| 2250 | 53.5 | 14.8 | 1.85 | 53.0 | 1.76 | 1.0 | 5.1 |
| 2300 | 53.5 | 14.8 | 1.89 | 52.9 | 1.81 | 1.1 | 4.4 |
| 2350 | 53.4 | 14.8 | 1.94 | 52.8 | 1.85 | 1.1 | 4.9 |
| 2400 | 53.3 | 14.8 | 1.98 | 52.8 | 1.90 | 1.0 | 4.2 |
| 2450 | 53.3 | 14.9 | 2.03 | 52.7 | 1.95 | 1.1 | 4.1 |
| 2500 | 53.2 | 14.9 | 2.07 | 52.6 | 2.02 | 1.1 | 2.5 |
| 2550 | 53.1 | 15.0 | 2.12 | 52.6 | 2.09 | 1.0 | 1.4 |
| 2600 | 53.0 | 15.0 | 2.17 | 52.5 | 2.16 | 0.9 | 0.5 |

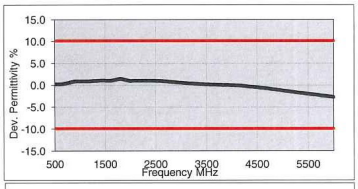


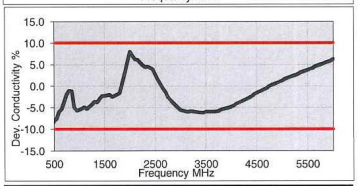


| | | | | | | | |
|---|---|---|---|---|---|---|---|
| 3500 | 51.4 | 16.0 | 3.11 | 51.3 | 3.31 | 0.2 | -6.0 |
| 3700 | 51.1 | 16.2 | 3.34 | 51.1 | 3.55 | 0.1 | -5.9 |
| 5200 | 48.3 | 18.7 | 5.42 | 49.0 | 5.30 | -1.5 | 2.3 |
| 5250 | 48.2 | 18.8 | 5.50 | 49.0 | 5.36 | -1.6 | 2.5 |
| 5300 | 48.1 | 18.9 | 5.57 | 48.9 | 5.42 | -1.7 | 2.8 |
| 5500 | 47.7 | 19.2 | 5.86 | 48.6 | 5.65 | -2.0 | 3.8 |
| 5600 | 47.5 | 19.3 | 6.01 | 48.5 | 5.77 | -2.1 | 4.2 |
| 5700 | 47.3 | 19.4 | 6.16 | 48.3 | 5.88 | -2.3 | 4.8 |
| 5800 | 47.0 | 19.6 | 6.32 | 48.2 | 6.00 | -2.4 | 5.3 |
| 6000 | 46.6 | 19.8 | 6.62 | 47.9 | 6.23 | -2.7 | 6.3 |
| 6500 | | | | | | | |
| 7000 | | | | | | | |
| 7500 | | | | | | | |
| 8000 | | | | | | | |
| 8500 | | | | | | | |
| 9000 | | | | | | | |
| 9500 | | | | | | | |
| 10000 | | | | | | | |

**Figure C-2**
**600 – 5800 MHz Body Tissue Equivalent Matter**



© 2022 PCTEST

Schmid & Partner Engineering AG
s p e a g
Zeughausstrasse 43, 8004 Zurich, Switzerland
Phone +41 44 245 9700, Fax +41 44 245 9779
info@speag.com, http://www.speag.com

## Measurement Certificate / Material Test

| | |
|---|---|
| Item Name | **Head Tissue Simulating Liquid (HBBL600-10000V6)** |
| Product No. | SL AAH U16 BC (Batch: 200805-4) |
| Manufacturer | SPEAG |

**Measurement Method**

TSL dielectric parameters measured using calibrated DAK probe.

**Target Parameters**

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.

**Test Condition**

| | |
|---|---|
| Ambient Condition | 22°C ; 30% humidity |
| TSL Temperature | 22°C |
| Test Date | 6-Aug-20 |
| Operator | CL |

**Additional Information**

TSL Density
TSL Heat-capacity

**Results**

| | Measured | | | Target | | Diff.to Target [%] | |
|---|---|---|---|---|---|---|---|
| f [MHz] | ε' | ε'' | sigma | eps | sigma | Δ-eps | Δ-sigma |
| 600 | 44.7 | 25.7 | 0.86 | 42.7 | 0.88 | 4.6 | -2.5 |
| 750 | 44.1 | 21.7 | 0.90 | 41.9 | 0.89 | 5.1 | 0.7 |
| 800 | 44.0 | 20.7 | 0.92 | 41.7 | 0.90 | 5.6 | 2.5 |
| 825 | 43.9 | 20.3 | 0.93 | 41.6 | 0.91 | 5.6 | 2.6 |
| 835 | 43.9 | 20.1 | 0.94 | 41.5 | 0.91 | 5.7 | 3.1 |
| 850 | 43.8 | 19.9 | 0.94 | 41.5 | 0.92 | 5.5 | 2.6 |
| 900 | 43.7 | 19.1 | 0.96 | 41.5 | 0.97 | 5.3 | -1.0 |
| 1400 | 42.7 | 15.1 | 1.18 | 40.6 | 1.18 | 5.2 | 0.0 |
| 1450 | 42.6 | 14.9 | 1.20 | 40.5 | 1.20 | 5.2 | 0.0 |
| 1600 | 42.4 | 14.4 | 1.28 | 40.3 | 1.28 | 5.2 | -0.3 |
| 1625 | 42.4 | 14.4 | 1.30 | 40.3 | 1.30 | 5.3 | 0.1 |
| 1640 | 42.4 | 14.3 | 1.31 | 40.3 | 1.31 | 5.3 | 0.3 |
| 1650 | 42.3 | 14.3 | 1.31 | 40.2 | 1.31 | 5.1 | -0.2 |
| 1700 | 42.2 | 14.2 | 1.34 | 40.2 | 1.34 | 5.1 | -0.2 |
| 1750 | 42.2 | 14.1 | 1.37 | 40.1 | 1.37 | 5.3 | -0.1 |
| 1800 | 42.1 | 14.0 | 1.40 | 40.0 | 1.40 | 5.3 | 0.0 |
| 1810 | 42.1 | 14.0 | 1.41 | 40.0 | 1.40 | 5.3 | 0.7 |
| 1825 | 42.1 | 13.9 | 1.42 | 40.0 | 1.40 | 5.3 | 1.4 |
| 1850 | 42.0 | 13.9 | 1.43 | 40.0 | 1.40 | 5.0 | 2.1 |
| 1900 | 41.9 | 13.8 | 1.46 | 40.0 | 1.40 | 4.7 | 4.3 |
| 1950 | 41.9 | 13.8 | 1.49 | 40.0 | 1.40 | 4.7 | 6.4 |
| 2000 | 41.8 | 13.7 | 1.53 | 40.0 | 1.40 | 4.5 | 9.3 |
| 2050 | 41.7 | 13.7 | 1.56 | 39.9 | 1.44 | 4.5 | 8.0 |
| 2100 | 41.7 | 13.7 | 1.60 | 39.8 | 1.49 | 4.7 | 7.5 |
| 2150 | 41.6 | 13.6 | 1.63 | 39.7 | 1.53 | 4.7 | 6.3 |
| 2200 | 41.5 | 13.6 | 1.67 | 39.6 | 1.58 | 4.7 | 5.8 |
| 2250 | 41.5 | 13.6 | 1.70 | 39.6 | 1.62 | 4.9 | 4.8 |
| 2300 | 41.4 | 13.6 | 1.74 | 39.5 | 1.67 | 4.9 | 4.4 |
| 2350 | 41.3 | 13.6 | 1.78 | 39.4 | 1.71 | 4.9 | 4.0 |
| 2400 | 41.2 | 13.6 | 1.82 | 39.3 | 1.76 | 4.9 | 3.7 |
| 2450 | 41.2 | 13.6 | 1.85 | 39.2 | 1.80 | 5.1 | 2.8 |
| 2500 | 41.1 | 13.6 | 1.89 | 39.1 | 1.85 | 5.0 | 1.9 |
| 2550 | 41.0 | 13.7 | 1.94 | 39.1 | 1.91 | 4.9 | 1.6 |
| 2600 | 40.9 | 13.7 | 1.98 | 39.0 | 1.96 | 4.8 | 0.8 |
| 3500 | 39.4 | 14.2 | 2.77 | 37.9 | 2.91 | 3.7 | -5.1 |
| 3700 | 39.0 | 14.3 | 2.95 | 37.7 | 3.12 | 3.5 | -5.3 |
| 5200 | 36.4 | 15.9 | 4.61 | 36.0 | 4.66 | 1.3 | -1.0 |
| 5250 | 36.4 | 16.0 | 4.67 | 35.9 | 4.71 | 1.2 | -0.9 |
| 5300 | 36.3 | 16.0 | 4.72 | 35.9 | 4.76 | 1.1 | -0.7 |
| 5500 | 35.9 | 16.2 | 4.96 | 35.6 | 4.96 | 0.7 | -0.1 |
| 5600 | 35.7 | 16.3 | 5.07 | 35.5 | 5.07 | 0.5 | 0.2 |
| 5700 | 35.5 | 16.4 | 5.19 | 35.4 | 5.17 | 0.3 | 0.4 |
| 5800 | 35.4 | 16.5 | 5.31 | 35.3 | 5.27 | 0.1 | 0.7 |
| 6000 | 35.0 | 16.6 | 5.54 | 35.1 | 5.48 | -0.2 | 1.2 |
| 6500 | 34.1 | 17.1 | 6.17 | 34.5 | 6.07 | -1.1 | 1.6 |
| 7000 | 33.2 | 17.4 | 6.78 | 33.9 | 6.65 | -2.0 | 2.0 |
| 7500 | 32.3 | 17.7 | 7.40 | 33.3 | 7.24 | -2.9 | 2.2 |
| 8000 | 31.5 | 18.0 | 8.01 | 32.7 | 7.84 | -3.8 | 2.2 |
| 8500 | 30.6 | 18.2 | 8.63 | 32.1 | 8.45 | -4.7 | 2.1 |
| 9000 | 29.8 | 18.4 | 9.24 | 31.5 | 9.08 | -5.6 | 1.8 |
| 9500 | 29.0 | 18.6 | 9.84 | 31.0 | 9.71 | -6.5 | 1.3 |
| 10000 | 28.1 | 18.8 | 10.44 | 30.4 | 10.36 | -7.4 | 0.8 |

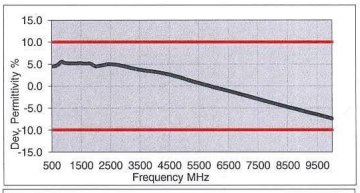


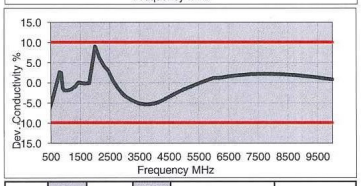


**Figure C-3**
**600 – 5800 MHz Head Tissue Equivalent Matter**



© 2022 PCTEST