

APPENDIX D: SAR TISSUE SPECIFICATIONS

Measurement Procedure for Tissue verification:

- 1) The network analyzer and probe system was configured and calibrated.
- 2) The probe was immersed in the tissue. The tissue was placed in a nonmetallic container. Trapped air bubbles beneath the flange were minimized by placing the probe at a slight angle.
- 3) The complex admittance with respect to the probe aperture was measured
- 4) The complex relative permittivity ϵ can be calculated from the below equation (Pournaropoulos and Misra):

$$Y = \frac{j2\omega\varepsilon_{r}\varepsilon_{0}}{\left[\ln(b/a)\right]^{2}} \int_{a}^{b} \int_{a}^{b} \int_{0}^{\pi} \cos\phi' \frac{\exp\left[-j\omega r(\mu_{0}\varepsilon_{r}\varepsilon_{0})^{1/2}\right]}{r} d\phi' d\rho' d\rho$$

where Y is the admittance of the probe in contact with the sample, the primed and unprimed coordinates refer to source and observation points, respectively, $r^2 = \rho^2 + \rho'^2 - 2\rho\rho'\cos\phi'$, ω is the angular frequency, and $j = \sqrt{-1}$.

3 Composition / Information on ingredients

3.2 Mixtures

Description: Aqueous solution with surfactants and inhibitors

Declarable, or nazardous compon	ients:	
CAS: 107-21-1	Ethanediol	>1.0-4.9%
EINECS: 203-473-3	STOT RE 2, H373;	
Reg.nr.: 01-2119456816-28-0000	Acute Tox. 4, H302	
CAS: 68608-26-4	Sodium petroleum sulfonate	< 2.9%
EINECS: 271-781-5	Eye Irrit. 2, H319	
Reg.nr.: 01-2119527859-22-0000		
CAS: 107-41-5	Hexylene Glycol / 2-Methyl-pentane-2,4-diol	< 2.9%
EINECS: 203-489-0	Skin Irrit. 2, H315; Eye Irrit. 2, H319	
Reg.nr.: 01-2119539582-35-0000		
CAS: 68920-66-1	Alkoxylated alcohol, > C ₁₆	< 2.0%
NLP: 500-236-9	Aquatic Chronic 2, H411;	
Reg.nr.: 01-2119489407-26-0000	Skin Irrit. 2, H315; Eye Irrit. 2, H319	

Additional information:

withheld as a trade secret.

For the wording of the listed risk phrases refer to section 16.

Not mentioned CAS-, EINECS- or registration numbers are to be regarded as Proprietary/Confidential. The specific chemical identity and/or exact percentage concentration of proprietary components is

Figure D-1

Note: Liquid recipes are proprietary SPEAG. Since the composition is approximate to the actual liquids utilized, the manufacturer tissue-equivalent liquid data sheets are provided below.

FCC ID A3LSMS911JPN	SAR EVALUATION REPORT	Approved by: Technical Manager
DUT Type: Portable Handset		APPENDIX D: Page 1 of 4



Schmid & Partner Engineering AG

S p e a g

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 44 245 9700, Fax +41 44 245 9779 www.speag.swiss, info@speag.swiss

Measurement Certificate / Material Test

Body Tissue Simulating Liquid (MBBL600-6000V6) SL AAM U16 BC (Batch: 210621-3)

Item Name Product No.

SPEAG Manufacturer

Measurement Method

TSL dielectric parameters measured using calibrated DAK probe.

Target Parameters

Target parameters as defined in the KDB 865664 compliance standard.

Test Condition

Ambient Condition 22°C; 30% humidity

TSL Temperature 22°C Test Date 23-Jun-21 WM

Operator Additional Information
TSL Density

TSL Heat-capacity

700	Measu	red		Targe	t	Diff.to Targ	get [%]	15.0							
[MHz]	e'	e"	sigma	-	sigma	∆-eps	∆-sigma	10.0					-		
600	55.7	26.7	0.89	56.1	0.95	-0.7	-6.3	%							
750	55.3	22.5	0.94	55.5	0.96	-0.4	-2.1	TE OO							
800	55.1	21.5	0.96	55.3	0.97	-0.4	-1.0	0.0 0.0 0.0						_	_
325	55.1	21.1	0.97	55.2	0.98	-0.3	-1.0								
35	55.1	20.8	0.97	55.1	0.99	0.0	-1.5	10.0 €					177		
350	55.0	20.6	0.97	55.2	0.99	-0.3	-2.0	-15.0	500	1500	2500	3500	4500	550	0
900	54.9	19.9	0.99	55.0	1.05	-0.2	-5.7	`		1000	Freque	3500 ency MHz	1000		_
400	54.1	15.9	1.24	54.1	1.28	0.0	-3.1	15.0	T						
450	54.0	15.7	1.27	54.0	1.30	0.0	-2.3	10.0							_
600	53.8	15.3	1.36	53.8	1.39	0.0	-2.2	%	-	1	-				
625	53.8	15.2	1.38	53.8	1.41	0.1	-2.1	Conductivity 2.0 2.0			1				
640	53.8	15.2	1.39	53.7	1.42	0.1	-2.1	-5.0	1	Land	1				
350	53.7	15.1	1.39	53.7	1.43	0.0	-2.8		1			_			
700	53.7	15.0	1.42	53.6	1.46	0.3	-2.7	5-10.0		History	1 301	175 5			
750	53.6	14.9	1.45	53.4	1.49	0.3	-2.7	-15.0	500	1500	2500	3500	4500	550	10
800	53.5	14.9	1.49	53.3	1.52	0.4	-2.0				Freque	ncy MHz			_
310	53.5	14.9	1.50	53.3	1.52	0.4	-1.3	3500	50.9	15.9	3.10	51.3	3.31	-0.9	-6
325	53.5	14.8	1.51	53.3	1.52	0.4	-0.7	3700	50.6	16.2	3.33	51.1	3.55	-1.0	-6
350	53.5	14.8	1.52	53.3	1.52	0.4	0.0	5200	47.7	18.6	5.39	49.0	5.30	-2.6	1.
900	53.4	14.8	1.56	53.3	1.52	0.2	2.6	5250	47.6	18.7	5.46	49.0	5.36	-2.7	1.
950	53.4	14.7	1.60	53.3	1.52	0.2	5.3	5300	47.5	18.8	5.54	48.9	5.42	-2.8	2
000	53.3	14.7	1.63	53.3	1.52	0.0	7.2	5500	47.1	19.1	5.83	48.6	5.65	-3.0	3
050	53.3	14.7	1.67	53.2	1.57	0.1	6.4	5600	46.9	19.2	5.98	48.5	5.77	-3.2	3
2100	53.2	14.7	1.71	53.2	1.62	0.1	5.6	5700	46.7	19.3	6.13	48.3	5.88	-3.3	4
2150	53.1	14.7	1.75	53.1	1.66	0.0	5.4	5800	46.5	19.4	6.27	48.2	6.00	-3.5	4
200	53.1	14.7	1.80	53.0	1.71	0.1	5.3	6000	46.1	19.7	6.57	47.9	6.23	-3.7	5
2250	53.0	14.7	1.84	53.0	1.76	0.1	4.5	6500			The se				
2300	52.9	14.7	1.88	52.9	1.81	0.0	3.9	7000						ĺ	
2350	52.9	14.8	1.93	52.8	1.85	0.1	4.3	7500						ĺ	
2400	52.8	14.8	1.98	52.8	1.90	0.1	4.2	8000							
2450	52.7	14.8	2.02	52.7	1.95	0.0	3.6	8500							
500	52.6	14.9	2.07	52.6	2.02	-0.1	2.5	9000			12.0				
2550	52.5	14.9	2.12	52.6	2.09	-0.1	1.4	9500							
2600	52.5	15.0	2.16	52.5	2.16	0.0	0.0	10000			May 1				

Figure D-2 600 - 6000 MHz Body Tissue Equivalent Matter

FCC ID A3LSMS911JPN	SAR EVALUATION REPORT	Approved by: Technical Manager
DUT Type: Portable Handset		APPENDIX D: Page 2 of 4



Schmid & Partner Engineering AG

s peag

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 44 245 9700, Fax +41 44 245 9779 www.speag.swiss, info@speag.swiss

Measurement Certificate / Material Test

Head Tissue Simulating Liquid (HBBL600-10000V6)

Product No. SL AAH U16 BC (Batch: 210629-3)

Manufacturer SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated DAK probe.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.

Test Condition

Ambient Condition 22°C; 30% humidity

TSL Temperature 22°C Operator WM

Additional Information

TSL Density

TSL Heat-capacity

	Measu	ired		Targe	et	Diff.to Target [%]			
f [MHz]	e'	е"	sigma	eps	sigma	∆-eps	∆-sigma		
600	44.7	25.5	0.85	42.7	0.88	4.6	-3.6		
750	44.1	21.6	0.90	41.9	0.89	5.1	0.7		
800	44.0	20.6	0.92	41.7	0.90	5.6	2.5		
825	44.0	20.2	0.93	41.6	0.91	5.8	2.6		
835	44.0	20.0	0.93	41.5	0.91	5.9	2.0		
850	43.9	19.8	0.93	41.5	0.92	5.8	1.5		
900	43.8	19.0	0.95	41.5	0.97	5.5	-2.1		
1400	42.8	15.1	1.18	40.6	1.18	5.4	0.0		
1450	42.7	14.9	1.20	40.5	1.20	5.4	0.0		
1600	42.4	14.4	1.28	40.3	1.28	5.2	-0.3		
1625	42.4	14.3	1.30	40.3	1.30	5.3	0.1		
1640	42.4	14.3	1.31	40.3	1.31	5.3	0.3		
1650	42.3	14.3	1.31	40.2	1.31	5.1	-0.2		
1700	42.3	14.2	1.34	40.2	1.34	5.3	-0.2		
1750	42.2	14.1	1.37	40.1	1.37	5.3	-0.1		
1800	42.1	14.0	1.40	40.0	1.40	5.3	0.0		
1810	42.1	13.9	1.41	40.0	1.40	5.3	0.7		
1825	42.1	13.9	1.42	40.0	1.40	5.3	1.4		
1850	42.0	13.9	1.43	40.0	1.40	5.0	2.1		
1900	42.0	13.8	1.46	40.0	1.40	5.0	4.3		
1950	41.9	13.8	1.49	40.0	1.40	4.7	6.4		
2000	41.8	13.7	1.53	40.0	1.40	4.5	9.3		
2050	41.8	13.7	1.56	39.9	1.44	4.7	8.0		
2100	41.7	13.7	1.59	39.8	1.49	4.7	6.8		
2150	41.6	13.6	1.63	39.7	1.53	4.7	6.3		
2200	41.6	13.6	1.67	39.6	1.58	4.9	5.8		
2250	41.5	13.6	1.70	39.6	1.62	4.9	4.8		
2300	41.4	13.6	1.74	39.5	1.67	4.9	4.4		
2350	41.3	13.6	1.78	39.4	1.71	4.9	4.0		
2400	41.3	13.6	1.82	39.3	1.76	5.1	3.7		
2450	41.2	13.6	1.86	39.2	1.80	5.1	3.3		
2500	41.1	13.6	1.90	39.1	1.85	5.0	2.5		
2550	41.0	13.7	1.94	39.1	1.91	4.9	1.6		
2600	41.0	13.7	1.98	39.0	1.96	5.1	0.8		

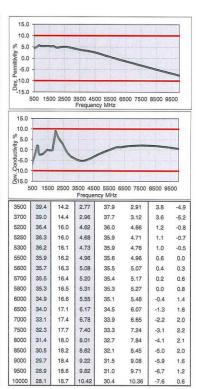


Figure D-3 600 - 10000 MHz Head Tissue Equivalent Matter

FCC ID A3LSMS911JPN	SMS911JPN SAR EVALUATION REPORT	
DUT Type: Portable Handset		APPENDIX D: Page 3 of 4



Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 44 245 9700, Fax +41 44 245 9779 www.speag.swiss, info@speag.swiss Measurement Certificate / Material Test Head Tissue Simulating Liquid (HBBL4-250V3) item Name Product No. SL AAH 005 AD (Batch: 210601-1) Manufacturer SPEAG Measurement Method
TSL dielectric parameters measured using calibrated DAK probe. $\begin{tabular}{ll} Setup Validation \\ \hline Validation results were within $\pm 2.5\%$ towards the target values of Methanol. \\ \hline \end{tabular}$ Target Parameters
Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards Test Condition
Ambient
TSL Temperature Environment temperatur (22 ± 3)°C and humidity < 70%. 3-Jun-21 Test Date WM Additional Information TSL Density 1.042 g/cm3
TSL Heat-capacity 3.574 kJ/(kg*K) 10.0 -7.5 -5.0 -2.5 -0.0 -Dev. Permitthity % -2.5 -5.0 -7.5 -10.0 5 25 45 65 7.5 5.0 2.5 -2.5 -10.0 105 125 145 165 185 205 225 245 Frequency MHz

e a

s p

9

Figure D-4
5 – 250 MHz Head Tissue Equivalent Matter

Pana 1 of 1

FCC ID A3LSMS911JPN	SAR EVALUATION REPORT	Approved by: Technical Manager	
DUT Type: Portable Handset		APPENDIX D: Page 4 of 4	