APPENDIX B: SYSTEM VERIFICATION PLOTS

ELEMENT

DUT: Dipole 6500.0 MHz; Type: D6.5GHzV2 - SN1018

Communication System: UID: 0, CW; Frequency: 6500.0 MHz
Medium: 6000 Head; Medium parameters used:
f = 6500.0 MHz; cond = 6.29 S/m; perm = 35.3; density = 1000 kg/m^3
Phantom Section: Flat; Space: 5 mm

Test Date: 01/17/2023; Ambient Temp: 22.6°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN3914; ConvF:(5.5,5.5,5.5); Calibrated: 2022-05-17
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn728; Calibrated: 2022-05-10
Phantom: Twin-SAM V5.0; Serial: 1759
Measurement SW: DASY Module SAR V16.2.0.1425

6500.0 MHz System Verification at 14.0 dBm (25 mW)

Area Scan (51.0 x 85.0): Measurement grid: dx=8.5 mm, dy=8.5 mm
Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=3.4 mm, dy=3.4 mm, dz=1.4 mm; Graded Ratio: 1.4
Peak SAR (extrapolated) = 47.3 W/kg
SAR(1 g) = 7.20 W/kg; SAR(10 g) = 1.30 W/kg; APD(4 cm^2) = 31.8 W/m^2
Deviation (1 g) = -1.71%; Deviation (10 g) = -3.88%; Deviation (4 cm^2) = -2.90%

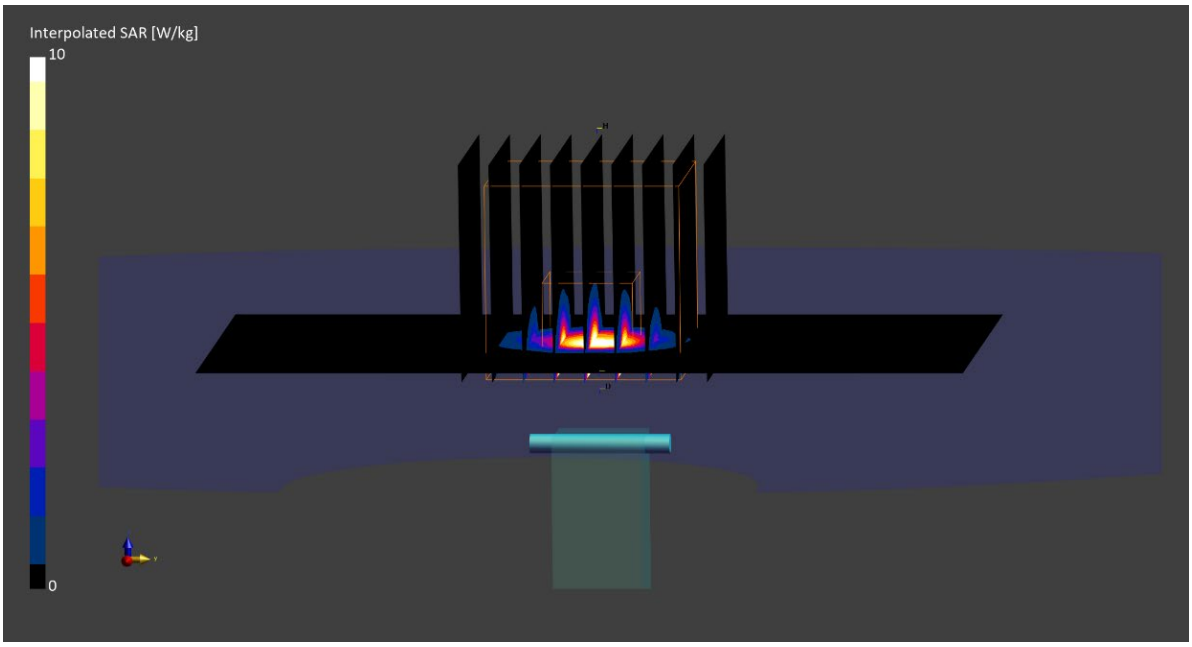

ELEMENT

DUT: Dipole 6500.0 MHz; Type: D6.5GHzV2 - SN1018

Communication System: UID: 0, CW; Frequency: 6500.0 MHz
Medium: 6000 Head; Medium parameters used:
f = 6500.0 MHz; cond = 6.29 S/m; perm = 34.5; density = 1000 kg/m^3
Phantom Section: Flat; Space: 5 mm

Test Date: 01/19/2023; Ambient Temp: 22.7°C; Tissue Temp: 21.2°C

Probe: EX3DV4 - SN3914; ConvF:(5.5,5.5,5.5); Calibrated: 2022-05-17
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn728; Calibrated: 2022-05-10
Phantom: Twin-SAM V5.0; Serial: 1759
Measurement SW: DASY Module SAR V16.2.0.1425

6500.0 MHz System Verification at 14.0 dBm (25 mW)

Area Scan (51.0 x 85.0): Measurement grid: dx=8.5 mm, dy=8.5 mm
Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=3.4 mm, dy=3.4 mm, dz=1.4 mm; Graded Ratio: 1.4
Peak SAR (extrapolated) = 48.6 W/kg
SAR(1 g) = 7.41 W/kg; SAR(10 g) = 1.34 W/kg; APD(4 cm^2) = 32.7 W/m^2
Deviation (1 g) = 1.16%; Deviation (10 g) = -0.92%; Deviation (4 cm^2) = -0.15%

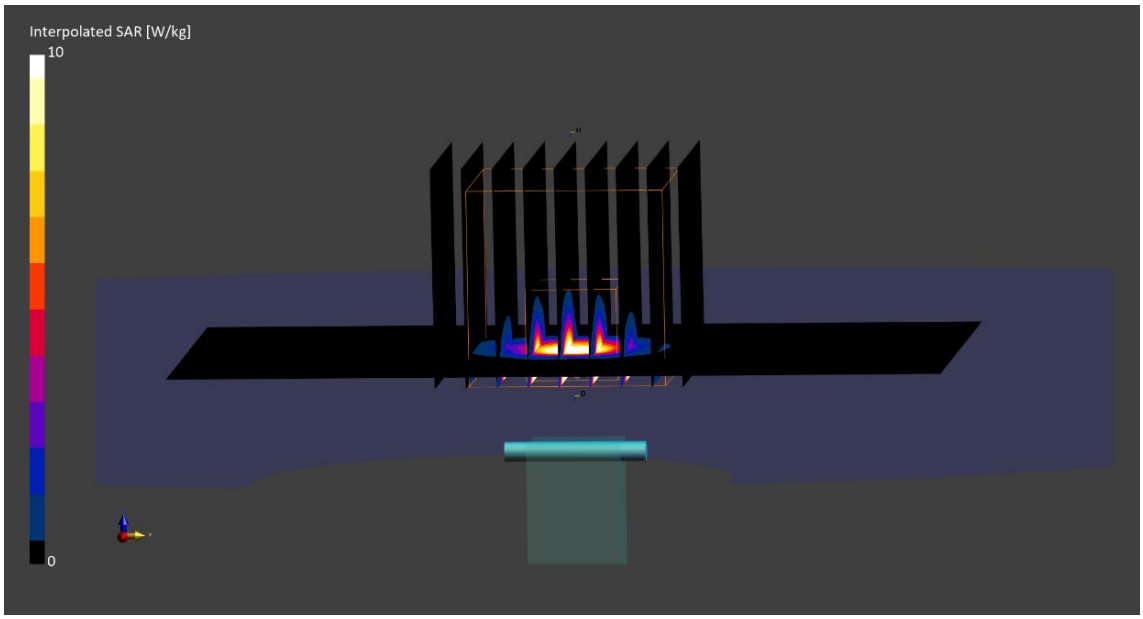

ELEMENT

DUT: Dipole 8000.0 MHz; Type: D8GHzV2 - SN1007

Communication System: UID: 0, CW; Frequency: 8000.0 MHz
Medium: 6000 Head; Medium parameters used:
f = 8000.0 MHz; cond = 8.17 S/m; perm = 31.8; density = 1000 kg/m^3
Phantom Section: Flat; Space: 5 mm

Test Date: 01/19/2023; Ambient Temp: 22.7°C; Tissue Temp: 21.2°C

Probe: EX3DV4 - SN3914; ConvF:(5.4,5.4,5.4); Calibrated: 2022-05-17
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn728; Calibrated: 2022-05-10
Phantom: Twin-SAM V5.0; Serial: 1759
Measurement SW: DASY Module SAR V16.2.0.1425

8000.0 MHz System Verification at 14.0 dBm (25 mW)

Area Scan (52.0 x 91.0): Measurement grid: dx=6.5 mm, dy=6.5 mm
Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=2.7 mm, dy=2.7 mm, dz=1.3 mm; Graded Ratio: 1.4
Peak SAR (extrapolated) = 60.7 W/kg
SAR(1 g) = 6.91 W/kg; SAR(10 g) = 1.14 W/kg; APD(4 cm^2) = 28.0 W/m^2
Deviation (1 g) = 5.50%; Deviation (10 g) = 3.35%; Deviation (4 cm^2) = 2.75%

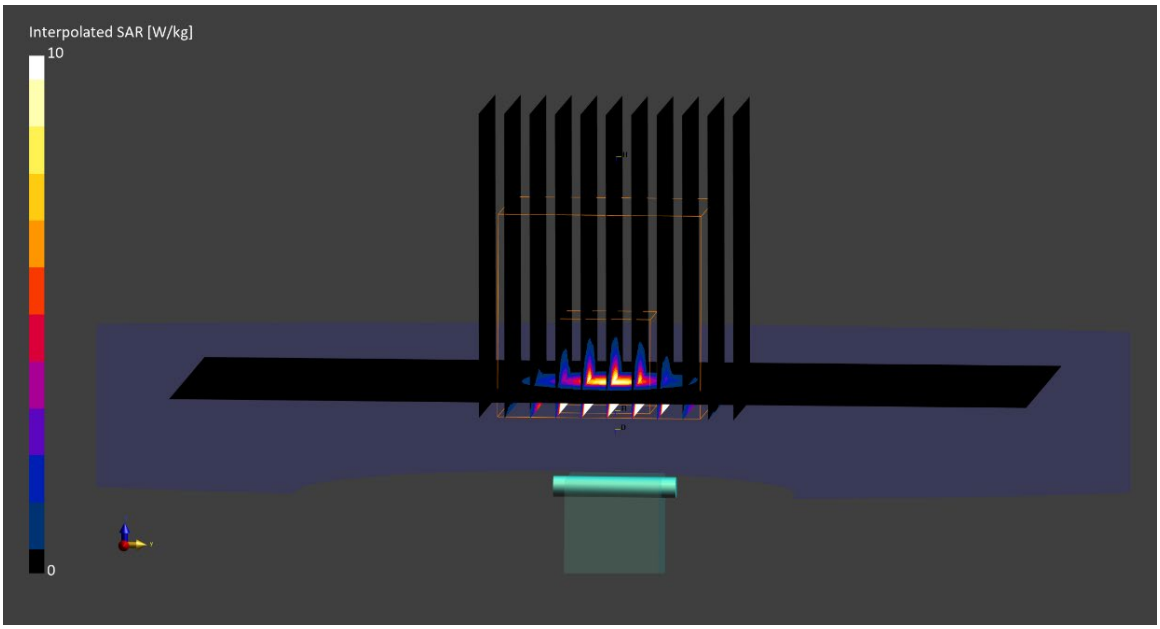

Element

Date: 12/12/2022

10 GHz System Verification

Device Under Test Properties

DUT	Serial Number
10 GHz Verification Source	1004

Exposure Conditions

Phantom Section	Position	Test Distance [mm]	Band	Frequency [MHz]
5G	FRONT	10.00	Validation band	10000.0

Hardware Setup

Probe, Calibration Date	DAE, Calibration Date
EUmmWV3 - SN9407, 10/17/2022	DAE4ip SN1638, 10/13/2022

Software Setup

Software	Software Version
cDASY6 Module mmWave	3.0.0.841

Scans Setup

Scan Type	5G Scan
Grid Extents [mm]	120 x 120
Grid Steps [lambda]	0.25 x 0.25
Sensor Surface [mm]	10.00

Measurement Results

Scan Type	5G Scan
Avg. Area [cm²]	4.00
pS_{tot} avg [W/m²]	50.4
pS_n avg [W/m²]	50.3
E_{peak} [V/m]	145
Deviation pStot (dB)	0.09
Deviation pSn (dB)	0.08

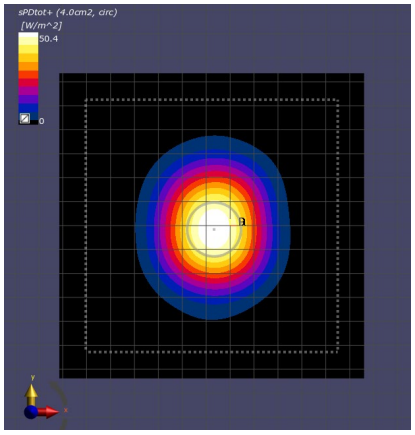

10 GHz System Verification

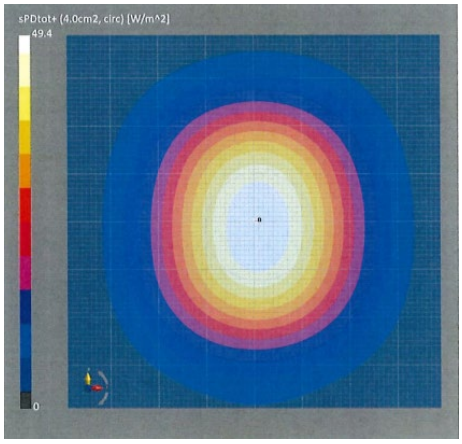

Calibration Certificate

Element

Date: 12/21/2022

10 GHz System Verification

Device Under Test Properties

DUT	Serial Number
10 GHz Verification Source	1004

Exposure Conditions

Phantom Section	Position	Test Distance [mm]	Band	Frequency [MHz]
5G	FRONT	10.00	Validation band	10000.0

Hardware Setup

Probe, Calibration Date	DAE, Calibration Date
EUmmWV4 - SN9541, 05/19/2022	DAE4ip SN1639, 11/16/2022

Software Setup

Software	Software Version
cDASY6 Module mmWave	3.0.0.841

Scans Setup

Scan Type	5G Scan
Grid Extents [mm]	120 x 120
Grid Steps [lambda]	0.25 x 0.25
Sensor Surface [mm]	10.00

Measurement Results

Scan Type	5G Scan
Avg. Area [cm²]	4.00
pS_{tot} avg [W/m²]	55.6
pS_n avg [W/m²]	55.3
E_{peak} [V/m]	152
Deviation pStot (dB)	0.51
Deviation pSn (dB)	0.49

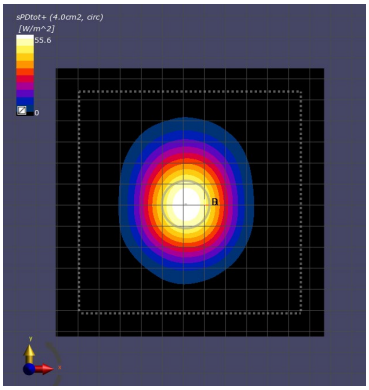

10 GHz System Verification

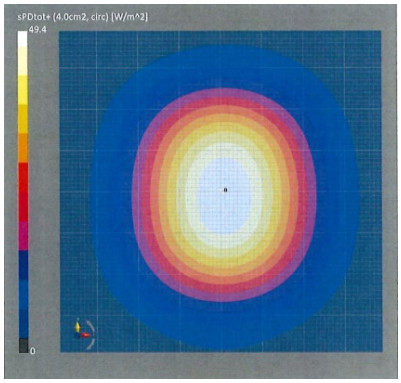

Calibration Certificate