



HCT Co., Ltd.

74, Seoicheon-ro 578beon-gil, Majang-myeon, Icheon-si, Gyeonggi-do, 17383 KOREA
Tel. +82 31 634 6300 Fax. +82 31 645 6401

Appendix A:
Test Setup
Photo

FCC ID
A3LSMX616B

File No.

HCT-RF-2307-FC001-P	HCT-RF-2307-FC005-P	HCT-RF-2307-FC009-P
HCT-RF-2307-FC002-P	HCT-RF-2307-FC006-P	HCT-RF-2307-FC010-P
HCT-RF-2307-FC003-P	HCT-RF-2307-FC007-P	HCT-RF-2307-FC011-P
HCT-RF-2307-FC004-P	HCT-RF-2307-FC008-P	

REVISION HISTORY

The revision history for this document is shown in table.

Revision No.	Date of Issue	Description
0	July 13, 2023	Initial Release

HCT-RF-2307-FC001-P	HCT-RF-2307-FC002-P	HCT-RF-2307-FC003-P	HCT-RF-2307-FC004-P	HCT-RF-2307-FC005-P
HCT-RF-2307-FC006-P	HCT-RF-2307-FC007-P	HCT-RF-2307-FC008-P	HCT-RF-2307-FC009-P	HCT-RF-2307-FC010-P
HCT-RF-2307-FC011-P				


1. Radiated Test Setup Photo




File No.	HCT-RF-2307-FC001-P	HCT-RF-2307-FC002-P	HCT-RF-2307-FC003-P	HCT-RF-2307-FC004-P	HCT-RF-2307-FC005-P
	HCT-RF-2307-FC006-P	HCT-RF-2307-FC007-P	HCT-RF-2307-FC008-P	HCT-RF-2307-FC009-P	HCT-RF-2307-FC010-P
	HCT-RF-2307-FC011-P				



File No.	HCT-RF-2307-FC001-P	HCT-RF-2307-FC002-P	HCT-RF-2307-FC003-P	HCT-RF-2307-FC004-P	HCT-RF-2307-FC005-P
	HCT-RF-2307-FC006-P	HCT-RF-2307-FC007-P	HCT-RF-2307-FC008-P	HCT-RF-2307-FC009-P	HCT-RF-2307-FC010-P
	HCT-RF-2307-FC011-P				

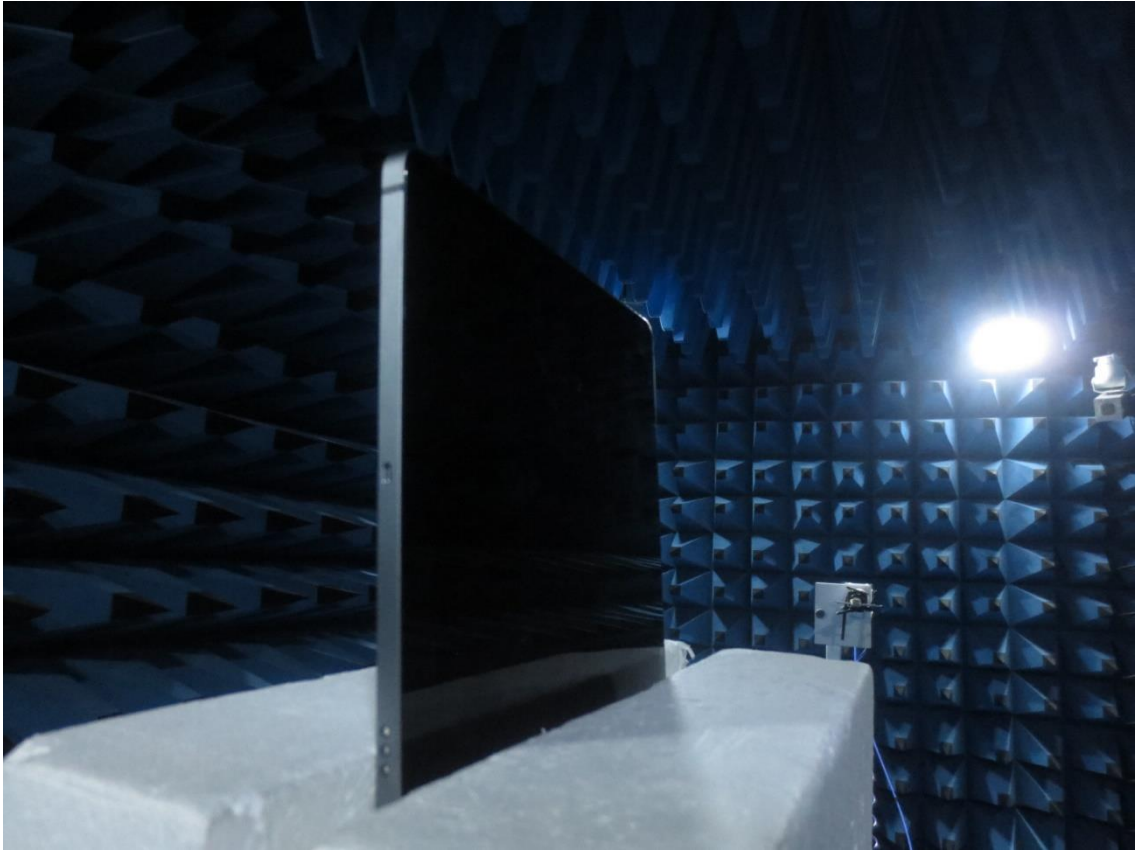

File No.	HCT-RF-2307-FC001-P	HCT-RF-2307-FC002-P	HCT-RF-2307-FC003-P	HCT-RF-2307-FC004-P	HCT-RF-2307-FC005-P
	HCT-RF-2307-FC006-P	HCT-RF-2307-FC007-P	HCT-RF-2307-FC008-P	HCT-RF-2307-FC009-P	HCT-RF-2307-FC010-P
	HCT-RF-2307-FC011-P				

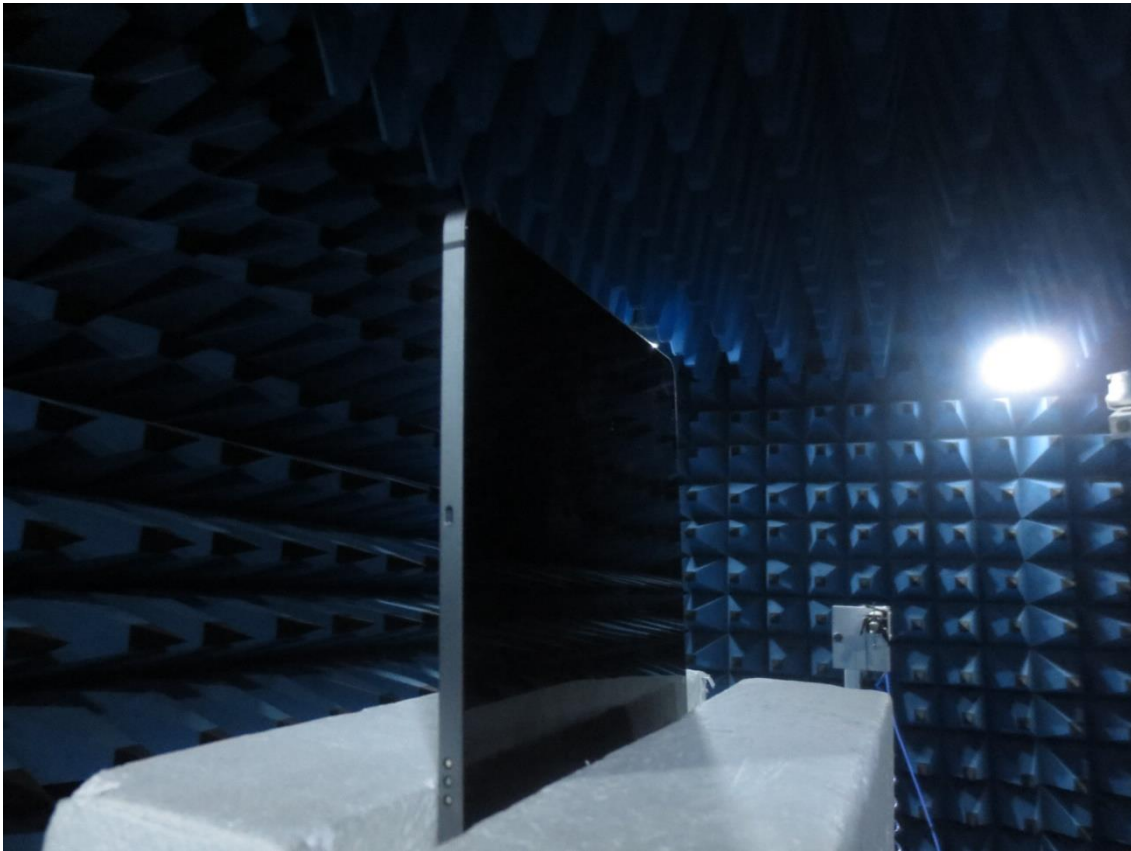

File
No.


HCT-RF-2307-FC001-P
HCT-RF-2307-FC006-P
HCT-RF-2307-FC011-P

HCT-RF-2307-FC002-P
HCT-RF-2307-FC007-P

HCT-RF-2307-FC003-P
HCT-RF-2307-FC008-P

HCT-RF-2307-FC004-P
HCT-RF-2307-FC009-P

HCT-RF-2307-FC005-P
HCT-RF-2307-FC010-P

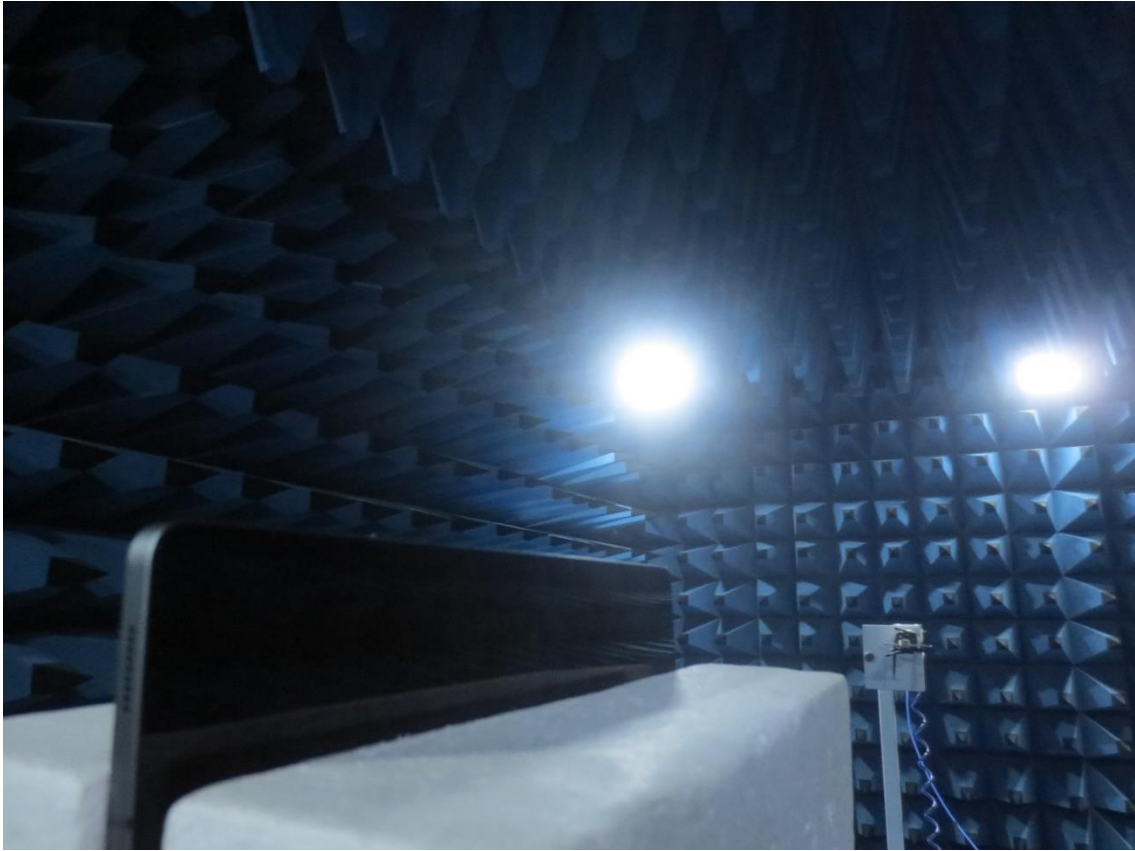

File No.	HCT-RF-2307-FC001-P	HCT-RF-2307-FC002-P	HCT-RF-2307-FC003-P	HCT-RF-2307-FC004-P	HCT-RF-2307-FC005-P
	HCT-RF-2307-FC006-P	HCT-RF-2307-FC007-P	HCT-RF-2307-FC008-P	HCT-RF-2307-FC009-P	HCT-RF-2307-FC010-P
	HCT-RF-2307-FC011-P				



File No.	HCT-RF-2307-FC001-P	HCT-RF-2307-FC002-P	HCT-RF-2307-FC003-P	HCT-RF-2307-FC004-P	HCT-RF-2307-FC005-P
	HCT-RF-2307-FC006-P	HCT-RF-2307-FC007-P	HCT-RF-2307-FC008-P	HCT-RF-2307-FC009-P	HCT-RF-2307-FC010-P
	HCT-RF-2307-FC011-P				



File
No.


HCT-RF-2307-FC001-P
HCT-RF-2307-FC006-P
HCT-RF-2307-FC011-P

HCT-RF-2307-FC002-P
HCT-RF-2307-FC007-P


HCT-RF-2307-FC003-P
HCT-RF-2307-FC008-P

HCT-RF-2307-FC004-P
HCT-RF-2307-FC009-P

HCT-RF-2307-FC005-P
HCT-RF-2307-FC010-P

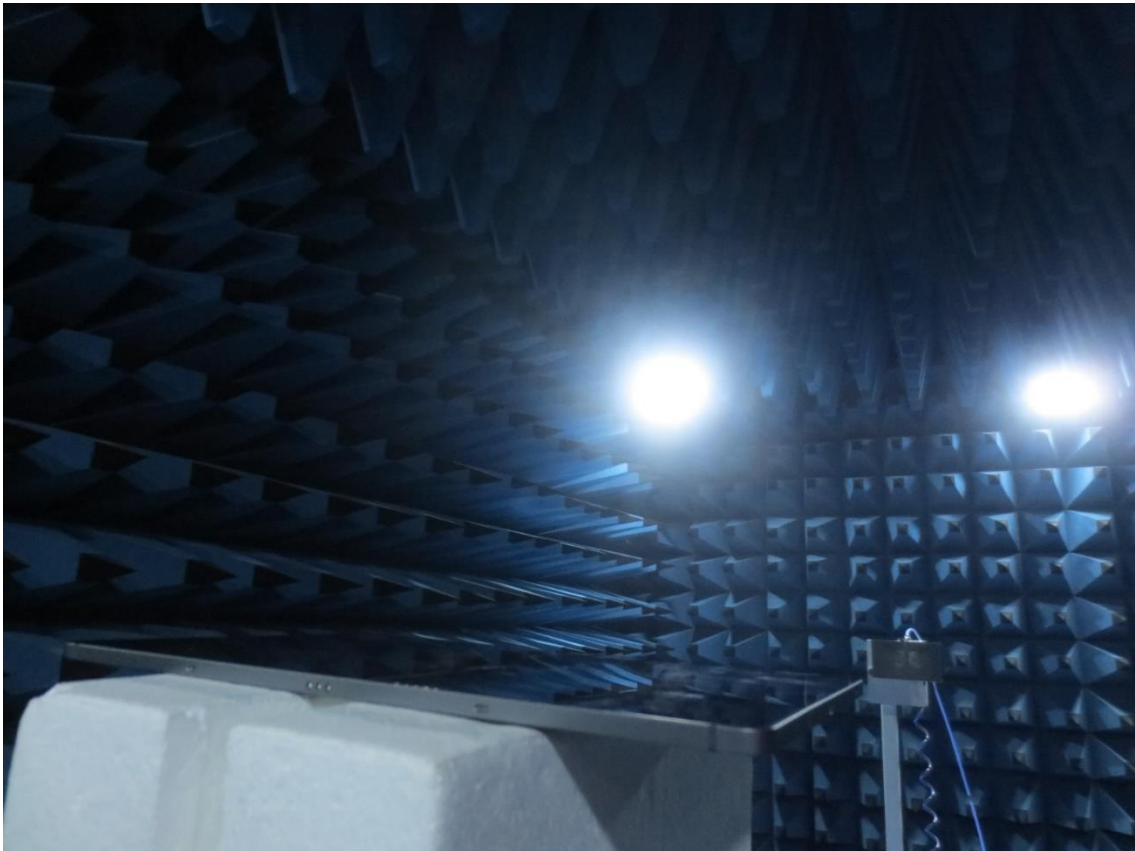

File No.	HCT-RF-2307-FC001-P	HCT-RF-2307-FC002-P	HCT-RF-2307-FC003-P	HCT-RF-2307-FC004-P	HCT-RF-2307-FC005-P
	HCT-RF-2307-FC006-P	HCT-RF-2307-FC007-P	HCT-RF-2307-FC008-P	HCT-RF-2307-FC009-P	HCT-RF-2307-FC010-P
	HCT-RF-2307-FC011-P				

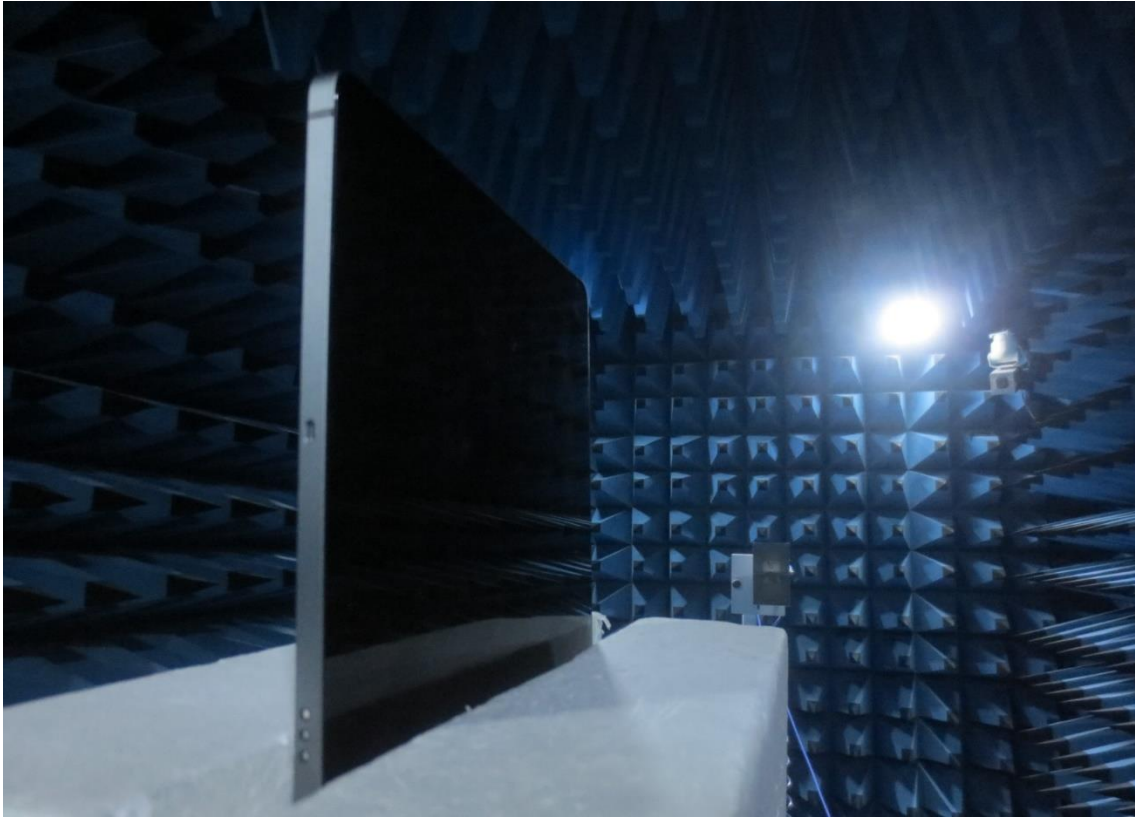

File
No.


HCT-RF-2307-FC001-P
HCT-RF-2307-FC006-P
HCT-RF-2307-FC011-P

HCT-RF-2307-FC002-P
HCT-RF-2307-FC007-P

HCT-RF-2307-FC003-P
HCT-RF-2307-FC008-P

HCT-RF-2307-FC004-P
HCT-RF-2307-FC009-P

HCT-RF-2307-FC005-P
HCT-RF-2307-FC010-P

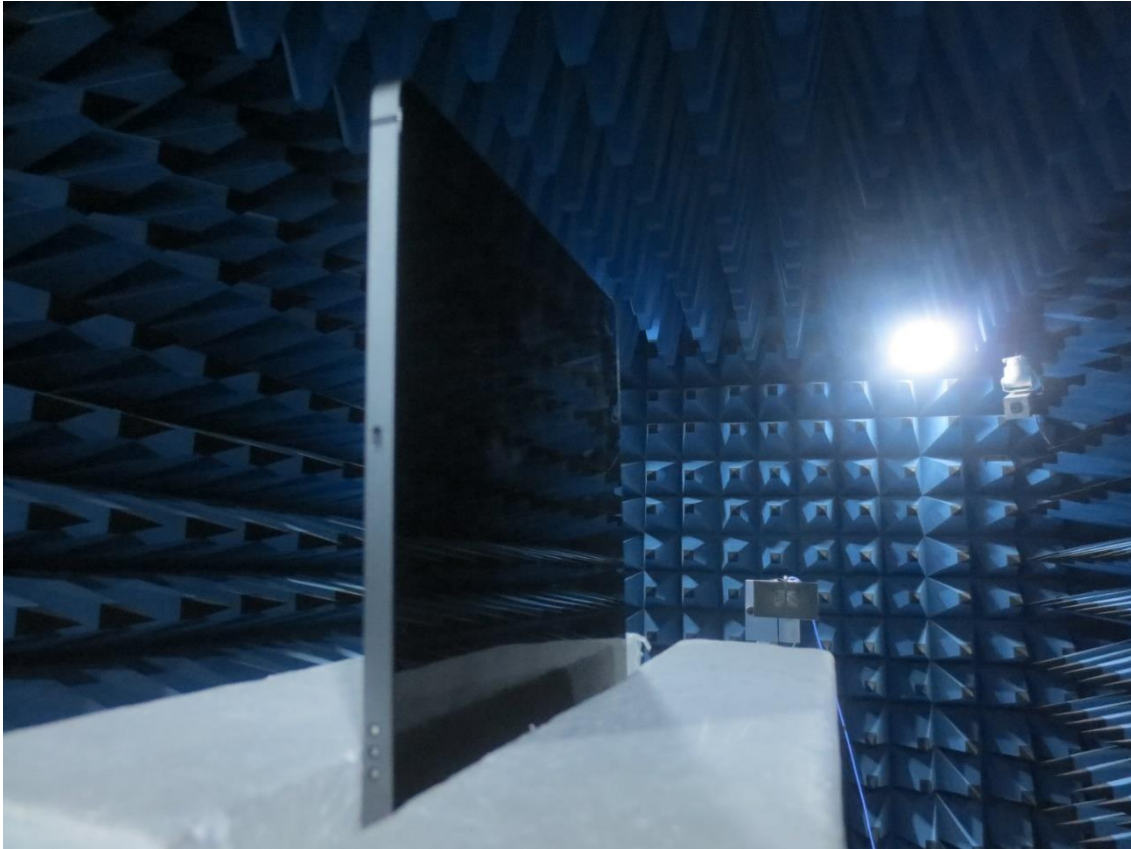

File
No.


HCT-RF-2307-FC001-P
HCT-RF-2307-FC006-P
HCT-RF-2307-FC011-P

HCT-RF-2307-FC002-P
HCT-RF-2307-FC007-P


HCT-RF-2307-FC003-P
HCT-RF-2307-FC008-P

HCT-RF-2307-FC004-P
HCT-RF-2307-FC009-P

HCT-RF-2307-FC005-P
HCT-RF-2307-FC010-P

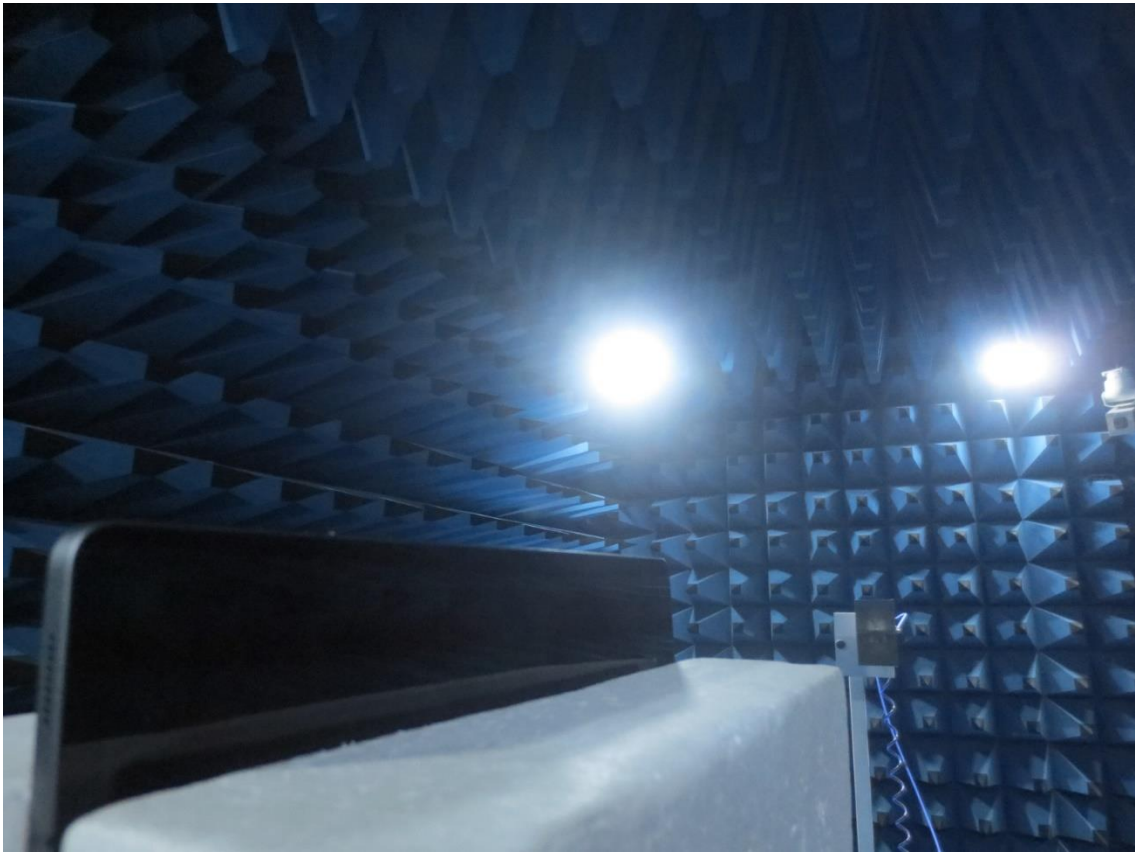

File No.	HCT-RF-2307-FC001-P	HCT-RF-2307-FC002-P	HCT-RF-2307-FC003-P	HCT-RF-2307-FC004-P	HCT-RF-2307-FC005-P
	HCT-RF-2307-FC006-P	HCT-RF-2307-FC007-P	HCT-RF-2307-FC008-P	HCT-RF-2307-FC009-P	HCT-RF-2307-FC010-P
	HCT-RF-2307-FC011-P				

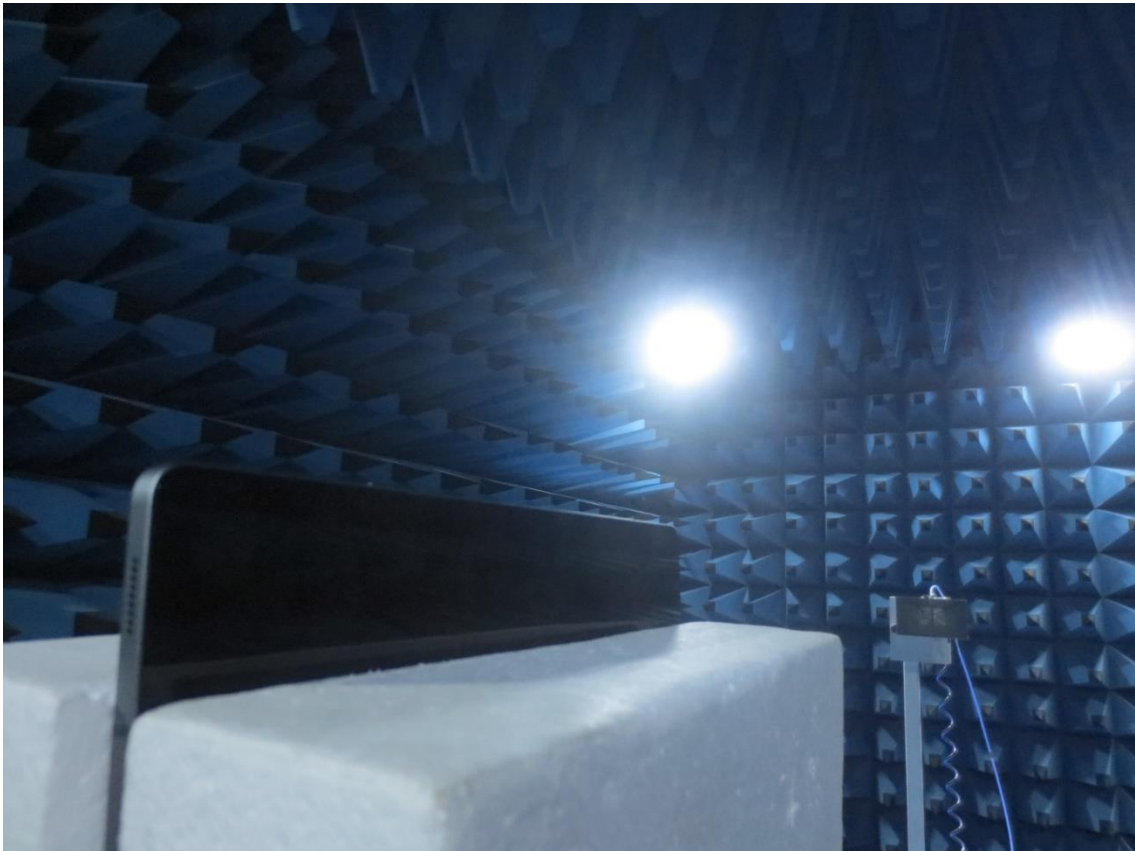

File
No.

HCT-RF-2307-FC001-P
HCT-RF-2307-FC006-P
HCT-RF-2307-FC011-P

HCT-RF-2307-FC002-P
HCT-RF-2307-FC007-P

HCT-RF-2307-FC003-P
HCT-RF-2307-FC008-P

HCT-RF-2307-FC004-P
HCT-RF-2307-FC009-P

HCT-RF-2307-FC005-P
HCT-RF-2307-FC010-P



File
No.


HCT-RF-2307-FC001-P
HCT-RF-2307-FC006-P
HCT-RF-2307-FC011-P

HCT-RF-2307-FC002-P
HCT-RF-2307-FC007-P


HCT-RF-2307-FC003-P
HCT-RF-2307-FC008-P

HCT-RF-2307-FC004-P
HCT-RF-2307-FC009-P

HCT-RF-2307-FC005-P
HCT-RF-2307-FC010-P

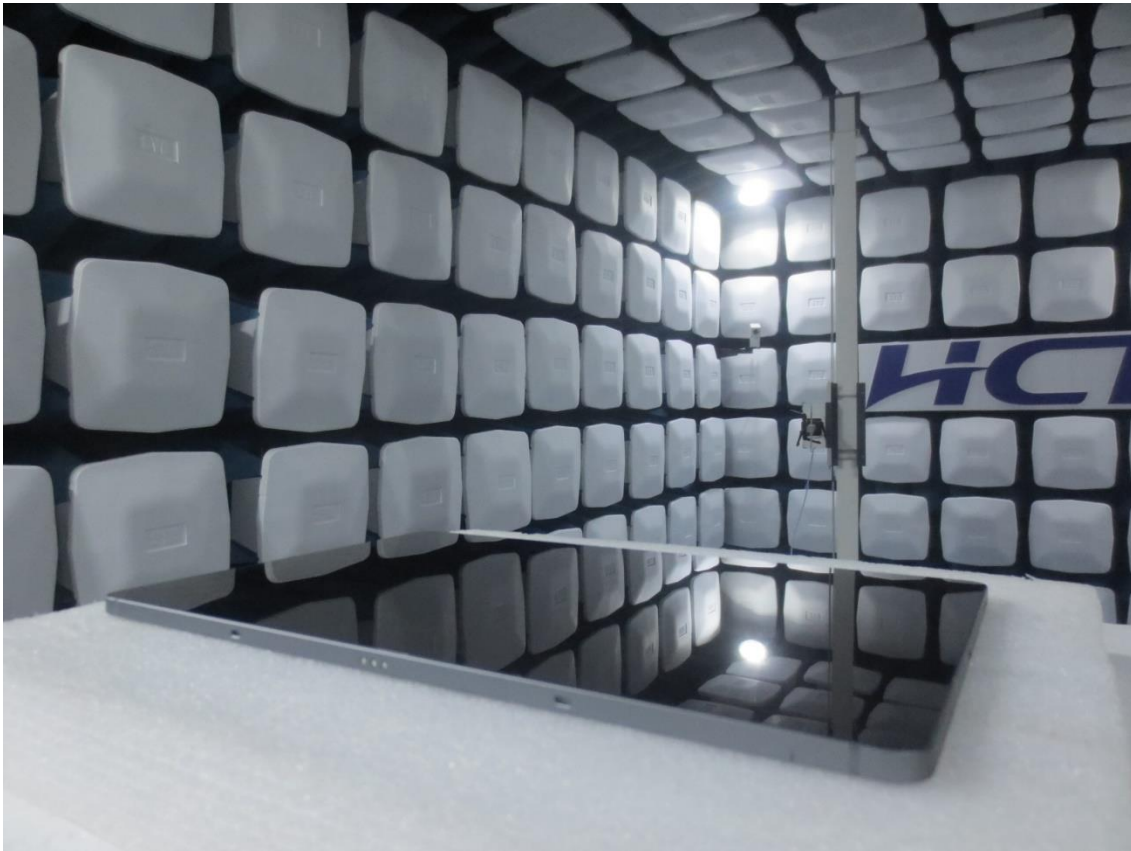

File No.	HCT-RF-2307-FC001-P	HCT-RF-2307-FC002-P	HCT-RF-2307-FC003-P	HCT-RF-2307-FC004-P	HCT-RF-2307-FC005-P
	HCT-RF-2307-FC006-P	HCT-RF-2307-FC007-P	HCT-RF-2307-FC008-P	HCT-RF-2307-FC009-P	HCT-RF-2307-FC010-P
	HCT-RF-2307-FC011-P				

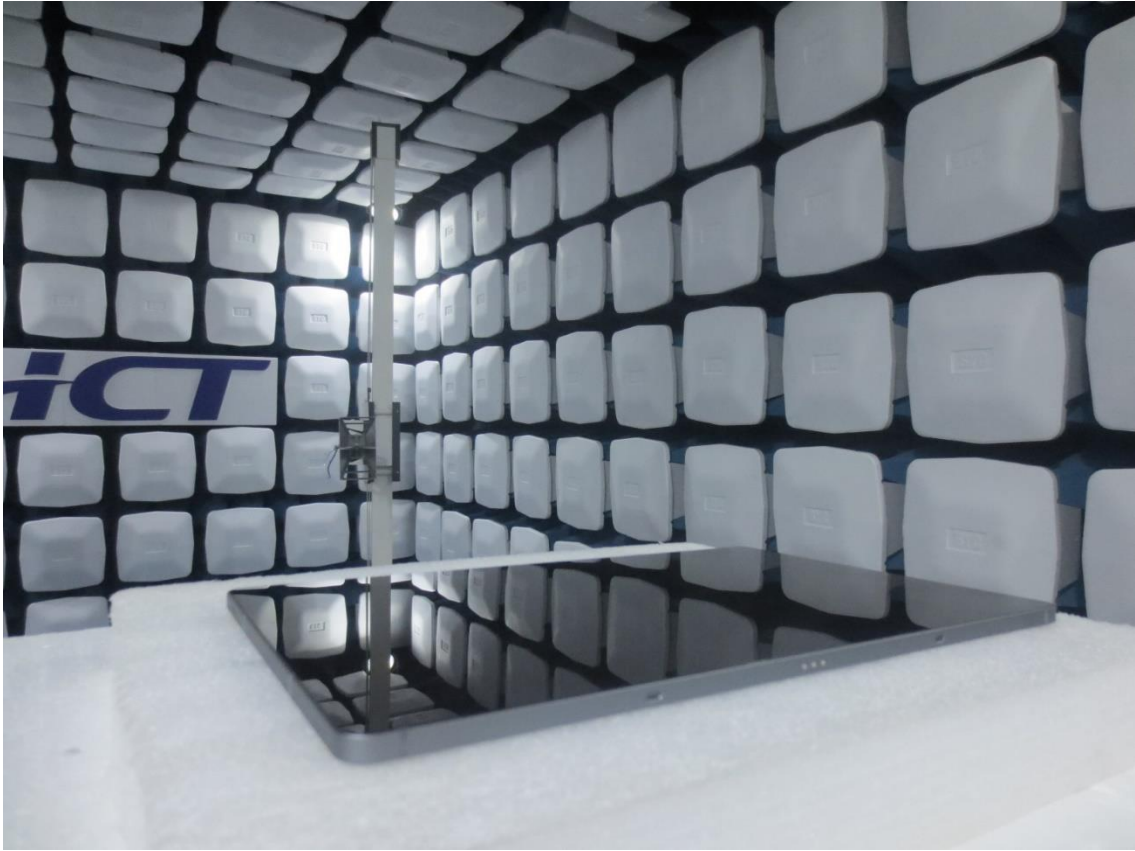

File
No.


HCT-RF-2307-FC001-P
HCT-RF-2307-FC006-P
HCT-RF-2307-FC011-P

HCT-RF-2307-FC002-P
HCT-RF-2307-FC007-P

HCT-RF-2307-FC003-P
HCT-RF-2307-FC008-P

HCT-RF-2307-FC004-P
HCT-RF-2307-FC009-P

HCT-RF-2307-FC005-P
HCT-RF-2307-FC010-P

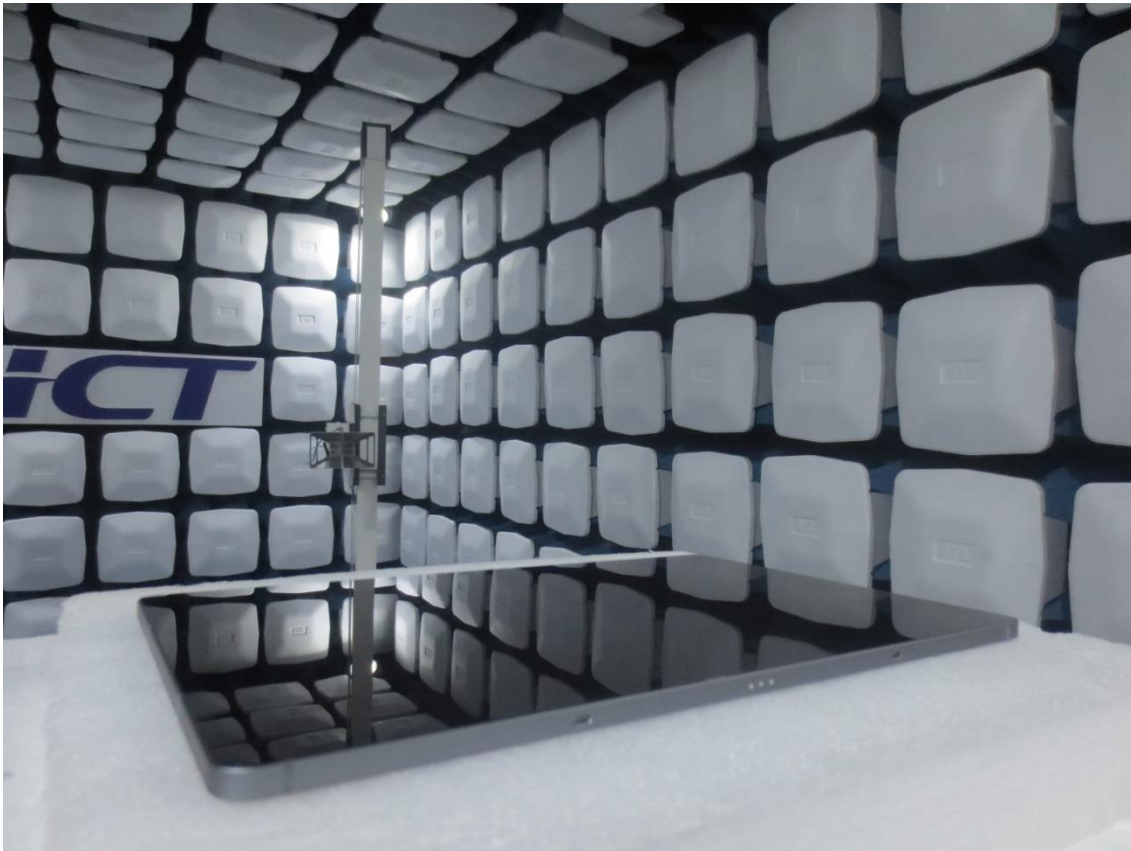

File
No.

HCT-RF-2307-FC001-P
HCT-RF-2307-FC006-P
HCT-RF-2307-FC011-P

HCT-RF-2307-FC002-P
HCT-RF-2307-FC007-P

HCT-RF-2307-FC003-P
HCT-RF-2307-FC008-P

HCT-RF-2307-FC004-P
HCT-RF-2307-FC009-P

HCT-RF-2307-FC005-P
HCT-RF-2307-FC010-P



File
No.


HCT-RF-2307-FC001-P
HCT-RF-2307-FC006-P
HCT-RF-2307-FC011-P

HCT-RF-2307-FC002-P
HCT-RF-2307-FC007-P

HCT-RF-2307-FC003-P
HCT-RF-2307-FC008-P

HCT-RF-2307-FC004-P
HCT-RF-2307-FC009-P

HCT-RF-2307-FC005-P
HCT-RF-2307-FC010-P

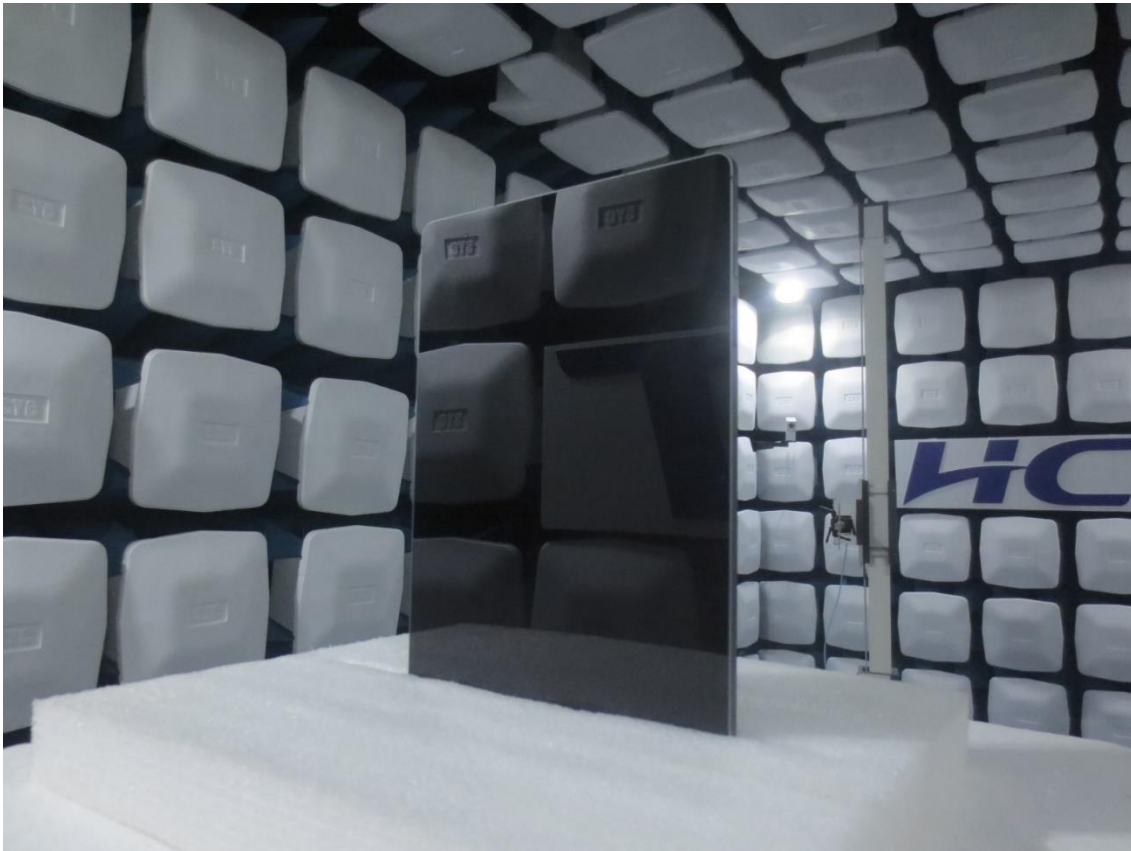

File
No.


HCT-RF-2307-FC001-P
HCT-RF-2307-FC006-P
HCT-RF-2307-FC011-P

HCT-RF-2307-FC002-P
HCT-RF-2307-FC007-P

HCT-RF-2307-FC003-P
HCT-RF-2307-FC008-P

HCT-RF-2307-FC004-P
HCT-RF-2307-FC009-P

HCT-RF-2307-FC005-P
HCT-RF-2307-FC010-P

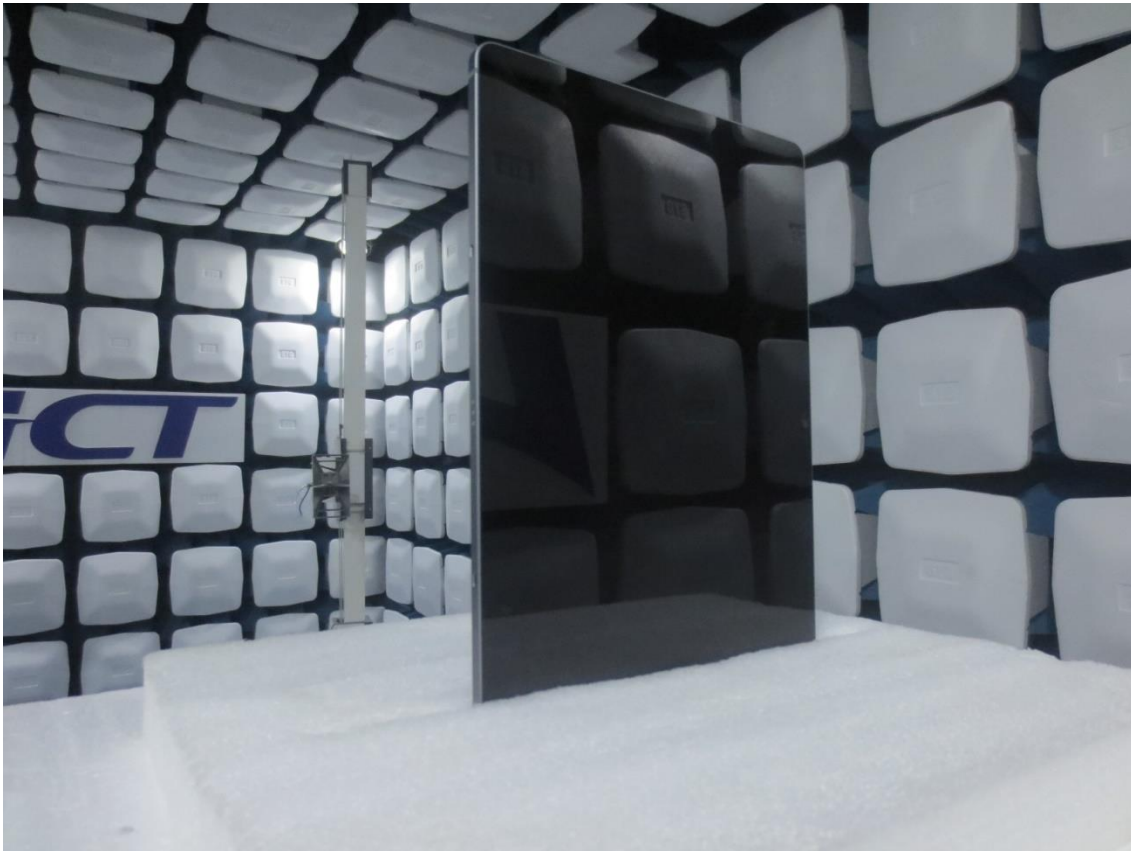

File
No.


HCT-RF-2307-FC001-P
HCT-RF-2307-FC006-P
HCT-RF-2307-FC011-P

HCT-RF-2307-FC002-P
HCT-RF-2307-FC007-P

HCT-RF-2307-FC003-P
HCT-RF-2307-FC008-P

HCT-RF-2307-FC004-P
HCT-RF-2307-FC009-P

HCT-RF-2307-FC005-P
HCT-RF-2307-FC010-P

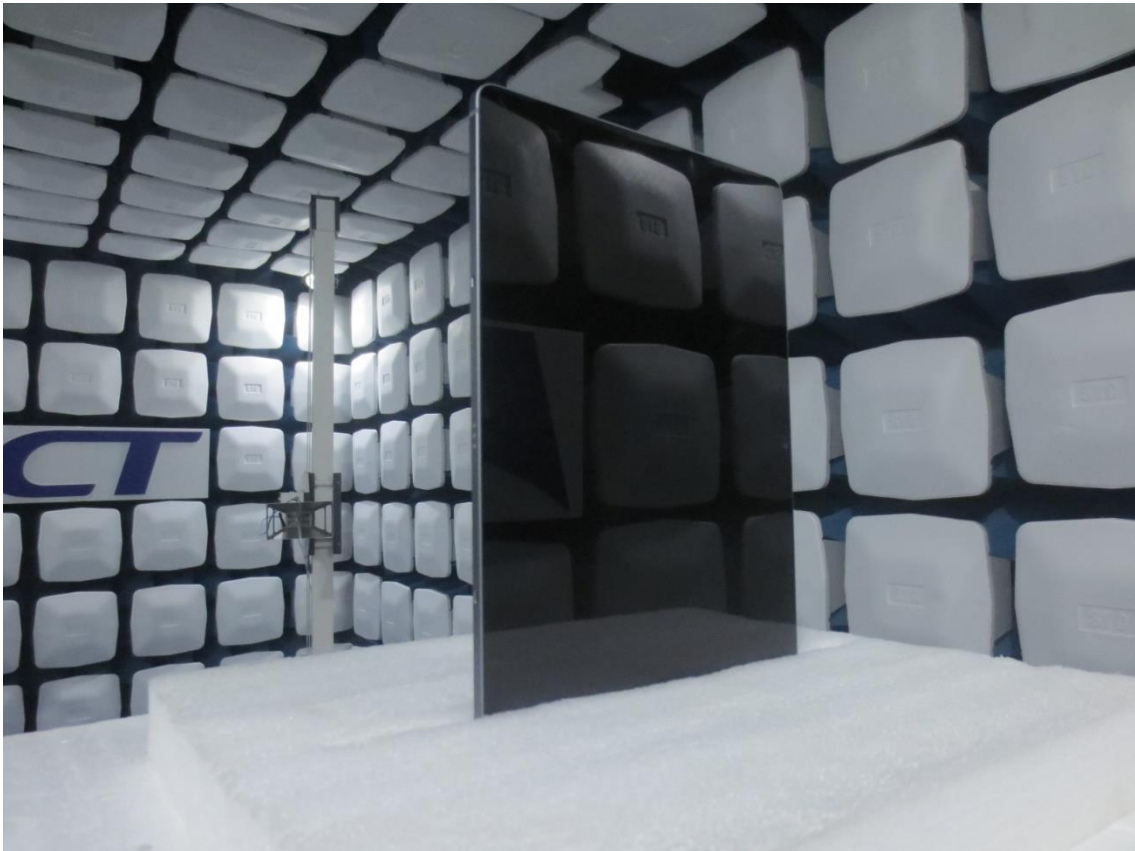

File
No.


HCT-RF-2307-FC001-P
HCT-RF-2307-FC006-P
HCT-RF-2307-FC011-P

HCT-RF-2307-FC002-P
HCT-RF-2307-FC007-P

HCT-RF-2307-FC003-P
HCT-RF-2307-FC008-P

HCT-RF-2307-FC004-P
HCT-RF-2307-FC009-P

HCT-RF-2307-FC005-P
HCT-RF-2307-FC010-P

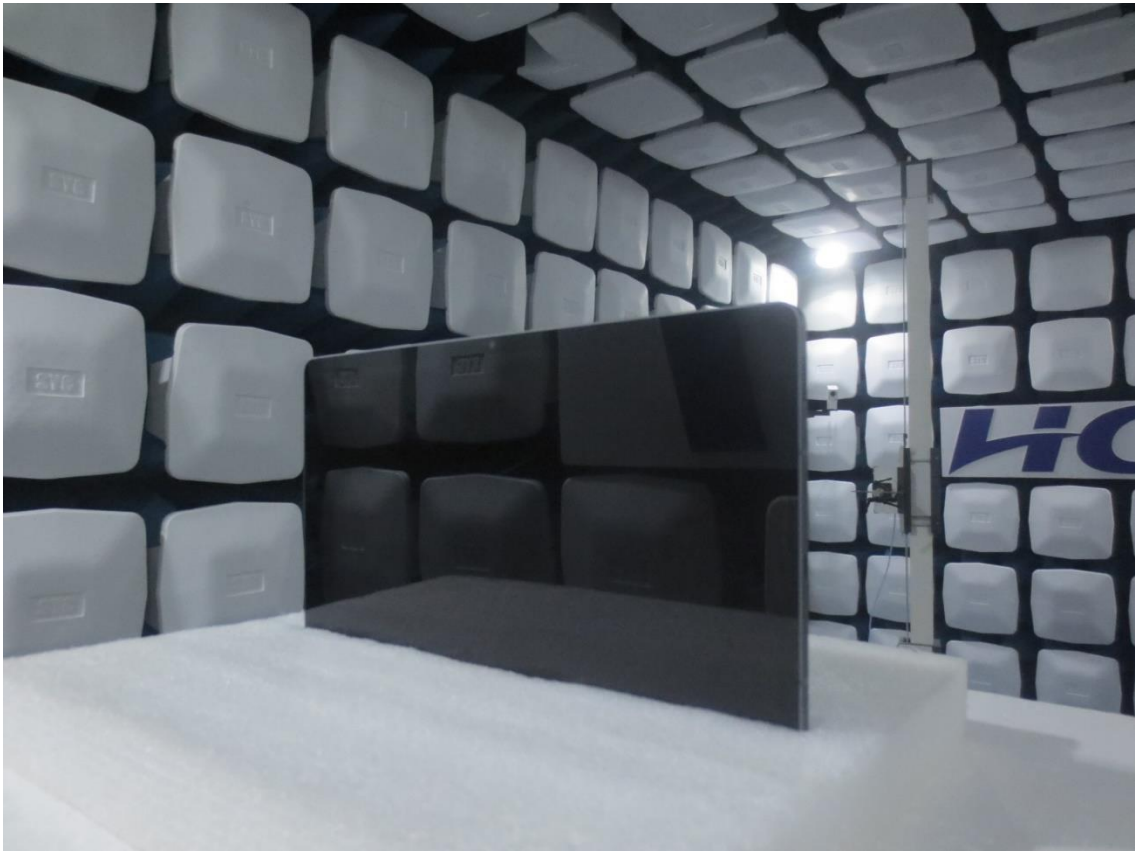

File
No.

HCT-RF-2307-FC001-P
HCT-RF-2307-FC006-P
HCT-RF-2307-FC011-P

HCT-RF-2307-FC002-P
HCT-RF-2307-FC007-P

HCT-RF-2307-FC003-P
HCT-RF-2307-FC008-P

HCT-RF-2307-FC004-P
HCT-RF-2307-FC009-P

HCT-RF-2307-FC005-P
HCT-RF-2307-FC010-P



File
No.


HCT-RF-2307-FC001-P
HCT-RF-2307-FC006-P
HCT-RF-2307-FC011-P

HCT-RF-2307-FC002-P
HCT-RF-2307-FC007-P

HCT-RF-2307-FC003-P
HCT-RF-2307-FC008-P

HCT-RF-2307-FC004-P
HCT-RF-2307-FC009-P

HCT-RF-2307-FC005-P
HCT-RF-2307-FC010-P

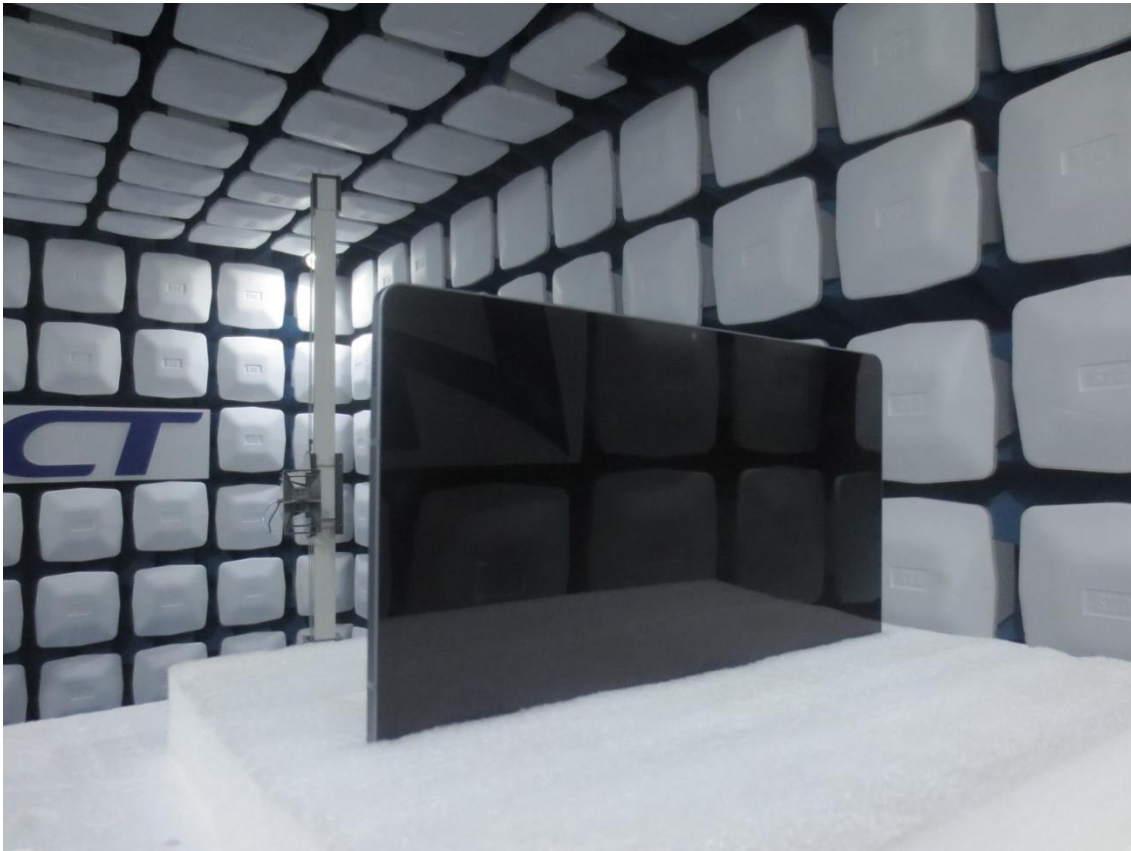

File
No.

HCT-RF-2307-FC001-P
HCT-RF-2307-FC006-P
HCT-RF-2307-FC011-P

HCT-RF-2307-FC002-P
HCT-RF-2307-FC007-P

HCT-RF-2307-FC003-P
HCT-RF-2307-FC008-P

HCT-RF-2307-FC004-P
HCT-RF-2307-FC009-P

HCT-RF-2307-FC005-P
HCT-RF-2307-FC010-P



File
No.

HCT-RF-2307-FC001-P
HCT-RF-2307-FC006-P
HCT-RF-2307-FC011-P


HCT-RF-2307-FC002-P
HCT-RF-2307-FC007-P

HCT-RF-2307-FC003-P
HCT-RF-2307-FC008-P

HCT-RF-2307-FC004-P
HCT-RF-2307-FC009-P

HCT-RF-2307-FC005-P
HCT-RF-2307-FC010-P

2. Conducted Test Setup Photo

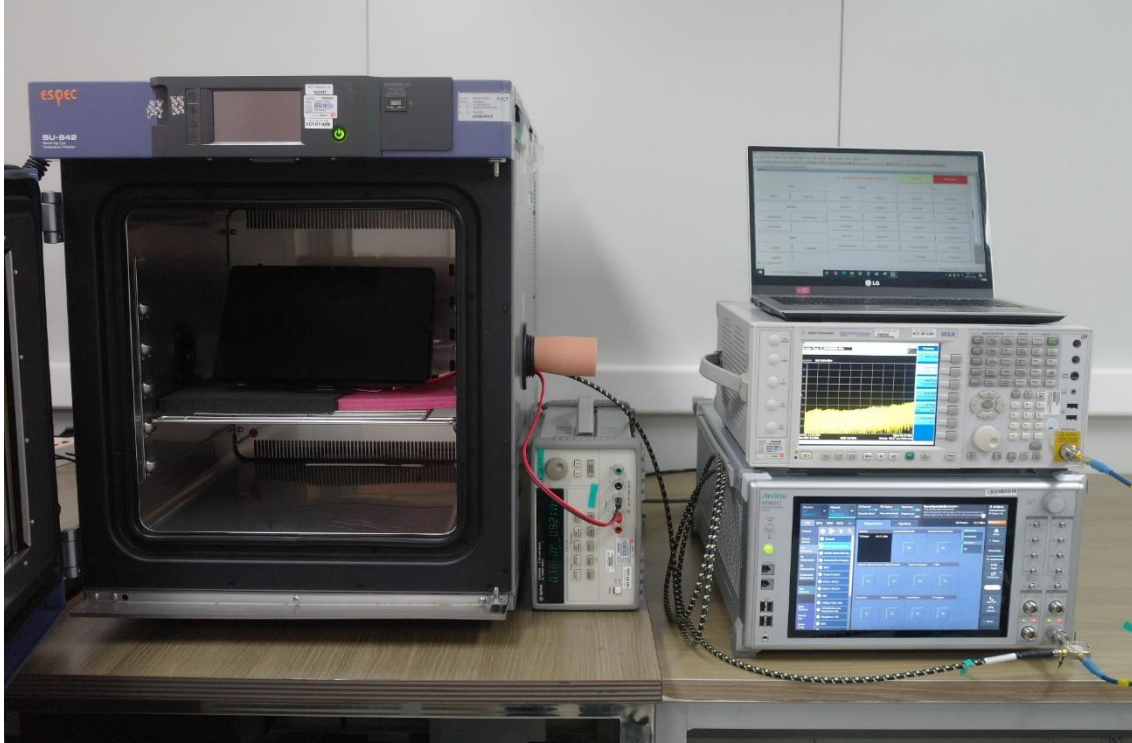

File
No.

HCT-RF-2307-FC001-P
HCT-RF-2307-FC006-P
HCT-RF-2307-FC011-P

HCT-RF-2307-FC002-P
HCT-RF-2307-FC007-P

HCT-RF-2307-FC003-P
HCT-RF-2307-FC008-P

HCT-RF-2307-FC004-P
HCT-RF-2307-FC009-P

HCT-RF-2307-FC005-P
HCT-RF-2307-FC010-P