(Incoming)


Software used for measurement Item Type

Measurement Studio Professional Edition
MixerCertification


**Version** 2013 7\_15

Remark

#### 1.1 Deviation between actual and previous conversion loss

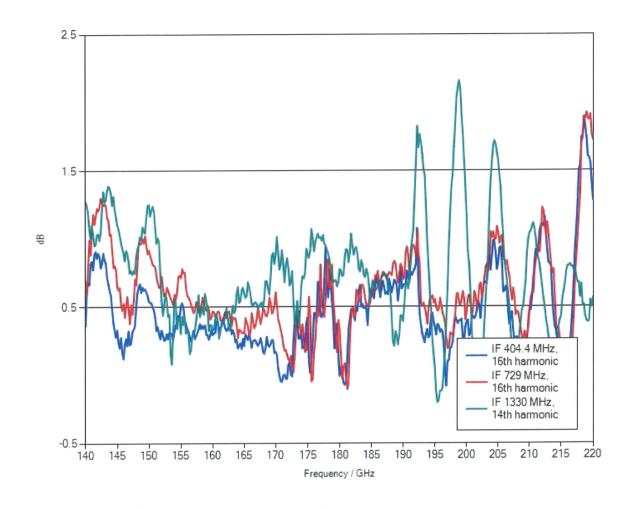


# Calibration Laboratory of Microwave Measuring Equipment of MWMLab

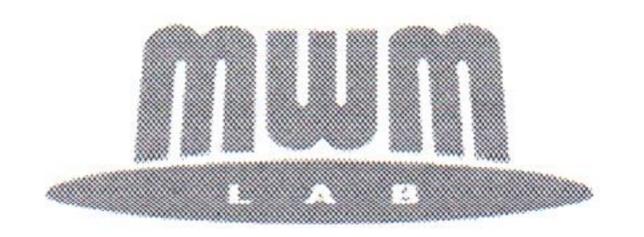



## Calibration certificate

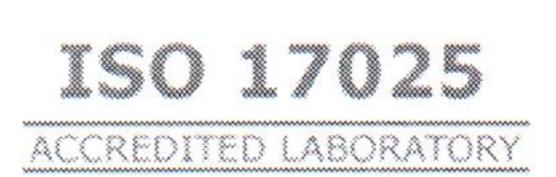



Accreditation certificate No.

Nº BY/112 5.0065

of

09.01.2015

Certificate number 36-21 Date when calibrated 06.07.2021 Page 1 of 2

Item calibrated

Antenna QWH-UPRR00 # 1410300003

Customer

Sporton International Inc.

Method of calibration

GOST 20271.1, MK KL 8.2-16

All measurements are traceable to the SI units which are realized by national measurement standards of NMI and state standards of RF. Gain measurements above 178 GHz are to confirm operation functionality and traceable only to MWMLab standards and OML. This certificate shall not be reproduced, except in full. Any publication extracts from the calibration certificate requires written permission of the issuing calibration laboratory of microwave measuring equipment.



/ Technical manager Date of issue 06.07.2021

### Calibration Certificate

Certificate number

36-21

Page 2 of 2

Calibration is performed by using

| Cambiani | campianton is perior med by using         |                   |                   |                       |                       |
|----------|---|-------------------|-------------------|-----------------------|-----------------------|
| Model    | Model Description                         | Equipment ID      | Cal Due Date      | Certificate<br>Number | Trace Value           |
| M1-11    | Calibrator of power with wattmeter M3-22A | 841202/<br>037410 | 08 December 2021  | 3882-43               | RF Power              |
| M 568    | Reference power meter                     | 164               | 24 March 2022     | 1/111-175-20          | RF Power              |
| G4-161   | Signal generator                          | 3                 | 12 October 2021   | 20-20                 | RF Power              |
| MG3694C  | Signal generator                          | 133805            | 11 September 2021 | 2726-43               | RF Power<br>Frequency |
| V7-34    | Universal voltmeter                       | 0067787           | 23 September 2021 | 2742-42               | DC Voltage            |
| RCH3-72  | Frequency meter                           | 931200            | 18 September 2021 | 2822-43               | Frequency             |
| P6-133   | Horn antenna                              | 15005             | 23 September 2021 | 2374-43               | Gain                  |
| P6-11B   | Measuring horn antenna                    | 08051             | 23 September 2021 | 2370-43               | Gain                  |

Calibration conditions

Temperature: 23.8 °C.

Humidity: 43.2 %.

Pressure:

100.1 kPa.


Calibration results are given in the measurement report # 36-21

| # | Parameter       | Specifications required | Specifications tested and measured |
|---|-----------------|-------------------------|------------------------------------|
| 1 | Frequency range | 40 – 60 GHz             | Corresponds                        |
| 2 | Antenna Gain    | 22.5* dBi               | Corresponds (Table 1)              |
| 3 | Antenna Factor  | 42 dB/m                 | Corresponds (Table 1)              |

<sup>\* –</sup> Expanded uncertainty of measurements 2.0 dB.

The uncertainty evaluation has been performed in accordance with ISO/IEC Guide 98-3:2008 (GUM). The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k such that the coverage probability corresponds to approximately 95 %. This probability corresponds to a coverage factor of k=2 for a normal distribution.

Signature of the person who has performed calibration

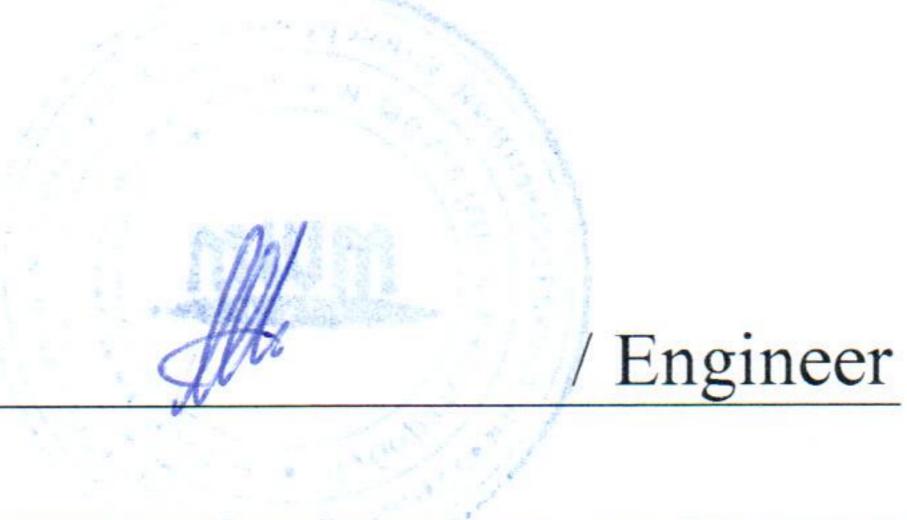

Phone/Fax: +375 17 293-84-96/E-mail: info@mwmlab.com

Calibration Laboratory of Microwave Measuring Equipment

Accreditation certificate No. BY/112 5.0065

Address: 6, P. Brovki str., Minsk

220013, Belarus

Phone/Fax: +375 17 2938496



#### MEASUREMENT REPORT # 36-21

July 6, 2021

| Customer:                    | Sporton International Inc.      |
|------------------------------|---------------------------------|
| Item calibrated:             | Antenna QWH-UPRR00 # 1410300003 |
| Method of calibration:       | GOST 20271.1, MK KL 8.2-16      |
| Number of samples:           | One                             |
| Delivery date of the sample: | 21.06.2021                      |
| Date of calibration:         | From 21.06.2021 to 06.07.2021   |

#### MEASUREMENT REPORT # 36-21

06.07.2021

Page 2 of 2

#### MEASUREMENT CONDITIONS

Temperature: 23.8 °C Humidity: 43.2 % Pressure: 100.1 kPa

MEASUREMENT EQUIPMENT

| WILLIAM DOUBLINE DOUBLINE |   |                   |                   |                       |                       |
|---------------------------|---|-------------------|-------------------|-----------------------|-----------------------|
| Model                     | Model Description                         | Equipment ID      | Cal Due Date      | Certificate<br>Number | Trace Value           |
| M1-11                     | Calibrator of power with wattmeter M3-22A | 841202/<br>037410 | 08 December 2021  | 3882-43               | RF Power              |
| M 568                     | Reference power meter                     | 164               | 24 March 2022     | 1/111-175-20          | RF Power              |
| G4-161                    | Signal generator                          | 3                 | 12 October 2021   | 20-20                 | RF Power              |
| MG3694C                   | Signal generator                          | 133805            | 11 September 2021 |                       | RF Power<br>Frequency |
| V7-34                     | Universal voltmeter                       | 0067787           | 23 September 2021 | 2742-42               | DC Voltage            |
| RCH3-72                   | Frequency meter                           | 931200            | 18 September 2021 | 2822-43               | Frequency             |
| P6-133                    | Horn antenna                              | 15005             | 23 September 2021 | 2374-43               | Gain                  |
| P6-11B                    | Measuring horn antenna                    | 08051             | 23 September 2021 | 2370-43               | Gain                  |

#### MEASUREMENT RESULTS

Distance between tested and generating antenna 2.0 m.

Table 1

| Frequency, GHz   | 40    | 50    | 60    |
|--|-------|-------|-------|
| Power density of electromagnetic field, W/m <sup>2</sup> | 0.050 | 0.070 | 0.070 |
| Maximum level of measured power, dBm                     | -14.3 | -14.2 | -15.8 |
| Gain, dBi  | 22.3  | 22.8  | 22.8  |
| Expanded uncertainty, dB                                 | 2.0   | 2.0   | 2.0   |
| Antenna Factor, dB/m                                     | 40.0  | 41.5  | 43.0  |

The uncertainty evaluation has been performed in accordance with ISO/IEC Guide 98-3:2008 (GUM). The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k such that the coverage probability corresponds to approximately 95%. This probability corresponds to a coverage factor of k=2 for a normal distribution.

Engineer

This measurement report issued in duplicate and sent to:

1. Sporton International Inc.

2. Calibration Laboratory of Microwave Measuring Equipment

Duplication of Measurement report (complete or partial) must be authorized by the laboratory.

#### Calibration Laboratory of Microwave Measuring Equipment of MWMLab





### Calibration certificate



ISO 17025



Accreditation certificate No.

No BY/112 5.0065

09.01.2015

Certificate number 38-21 Date when calibrated 06.07.2021 Page 1 of 2

Item calibrated

Antenna QWH-EPRR00 # 1372000000

Customer

Sporton International Inc.

Method of calibration

GOST 20271.1, MK KL 8.2-16

All measurements are traceable to the SI units which are realized by national measurement standards of NMI and state standards of RF. Gain measurements above 178 GHz are to confirm operation functionality and traceable only to MWMLab standards and OML. This certificate shall not be reproduced, except in full. Any publication extracts from the calibration certificate requires written permission of the issuing calibration laboratory of microwave measuring equipment.

Authorising signature

/ Technical manager

Date of issue 06.07.2021

MWM Lab. BSUIR, 6, P.Brovki str., Minsk, 220013, Belarus

Phone/Fax: +375 17 293-84-96/E-mail: info@mwmlab.com