

Probe ES3DV2

SN:3022

Manufactured:	April 15, 2003
Last calibration:	September 24, 2004

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

DASY - Parameters of Probe: ES3DV2 SN:3022

Sensitivity in Free Space

NormX	1.00 $\mu\text{V}/(\text{V}/\text{m})^2$
NormY	1.04 $\mu\text{V}/(\text{V}/\text{m})^2$
NormZ	0.98 $\mu\text{V}/(\text{V}/\text{m})^2$

Diode Compression

DCP X	95	mV
DCP Y	95	mV
DCP Z	95	mV

Sensitivity in Tissue Simulating Liquid

Head 900 MHz $\epsilon_r = 41.5 \pm 5\%$ $\sigma = 0.97 \pm 5\%$ mho/m

Valid for f=800-1000 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

ConvF X	6.1 $\pm 9.5\%$ (k=2)	Boundary effect:
ConvF Y	6.1 $\pm 9.5\%$ (k=2)	Alpha 0.32
ConvF Z	6.1 $\pm 9.5\%$ (k=2)	Depth 1.65

Head 1800 MHz $\epsilon_r = 40.0 \pm 5\%$ $\sigma = 1.40 \pm 5\%$ mho/m

Valid for f=1710-1910 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

ConvF X	5.0 $\pm 9.5\%$ (k=2)	Boundary effect:
ConvF Y	5.0 $\pm 9.5\%$ (k=2)	Alpha 0.25
ConvF Z	5.0 $\pm 9.5\%$ (k=2)	Depth 2.30

Boundary Effect

Head 900 MHz Typical SAR gradient: 5 % per mm





Probe Tip to Boundary		1 mm	2 mm
SAR _{ba} [%] Without Correction Algorithm		5.5	2.5
SAR _{ba} [%] With Correction Algorithm		0.1	0.4


Head 1800 MHz Typical SAR gradient: 10 % per mm

Probe Tip to Boundary		1 mm	2 mm
SAR _{ba} [%] Without Correction Algorithm		7.1	4.4
SAR _{ba} [%] With Correction Algorithm		0.0	0.1


Sensor Offset

Probe Tip to Sensor Center	2.0	mm
----------------------------	------------	----

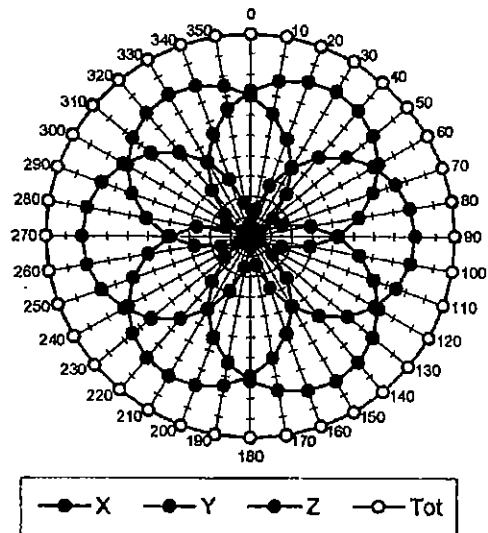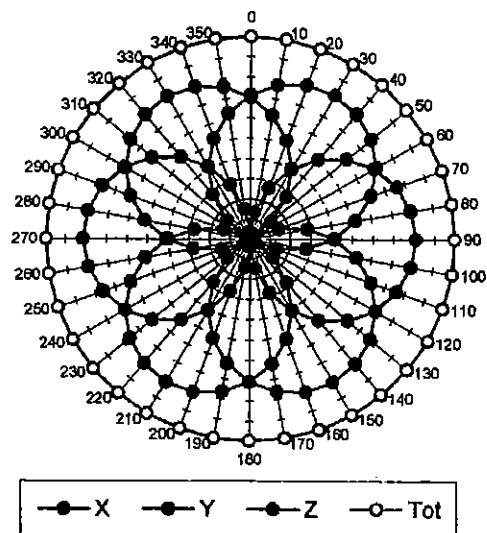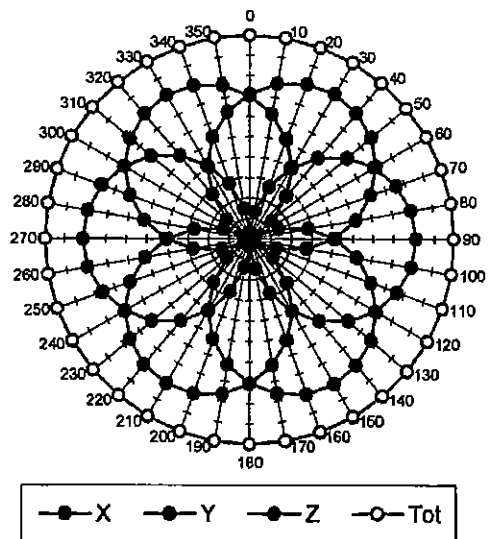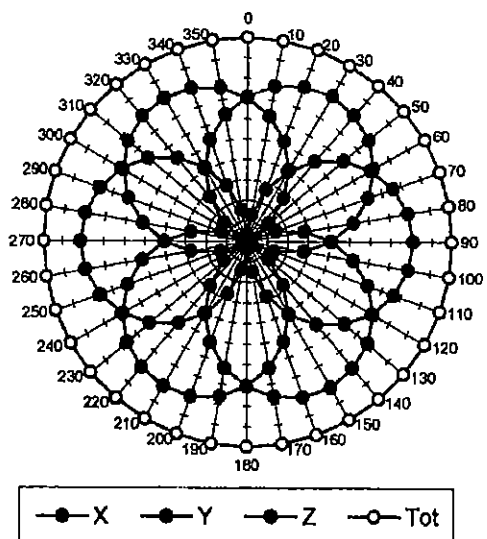
Receiving Pattern (ϕ , $\theta = 0^\circ$)**f = 30 MHz, TEM cell ifi110****f = 100 MHz, TEM cell ifi110****f = 300 MHz, TEM cell ifi110****f = 900 MHz, TEM cell ifi110**

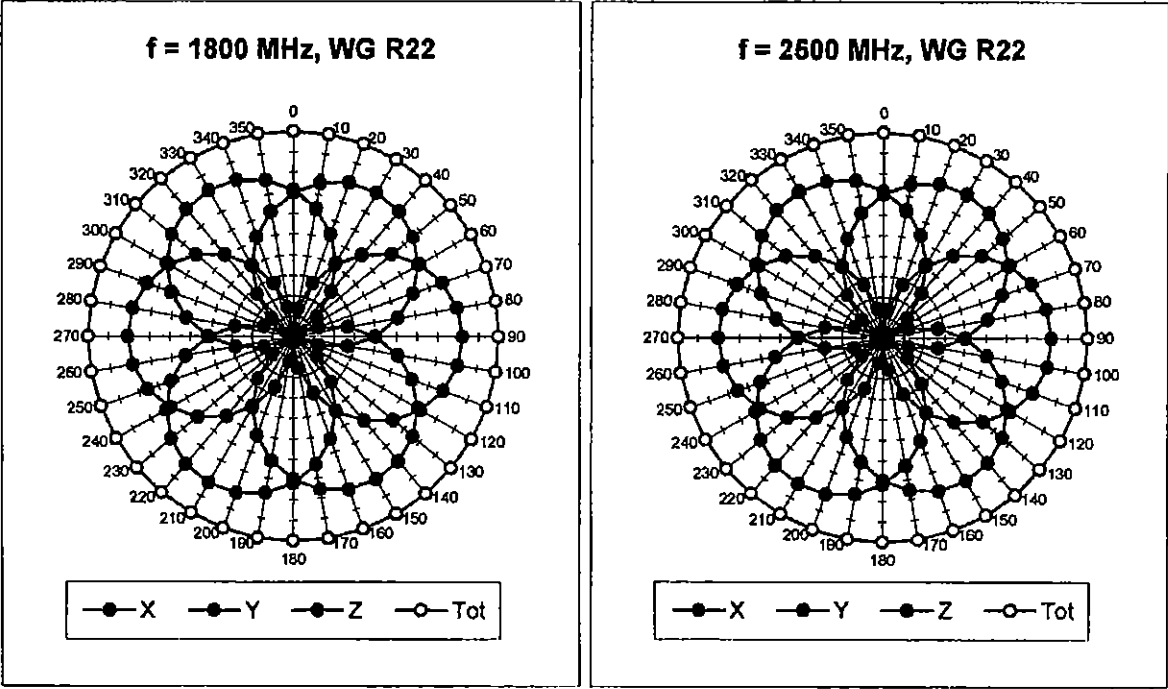



Isotropy Error (ϕ), $\theta = 0^\circ$

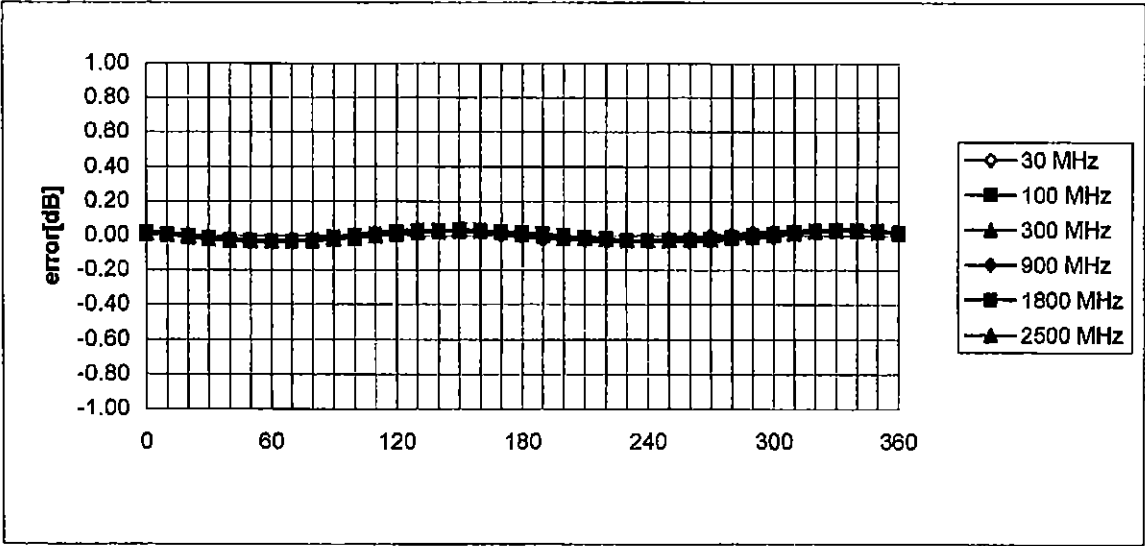


Frequency Response of E-Field
(TEM-Cell:ifi110, Waveguide R22)

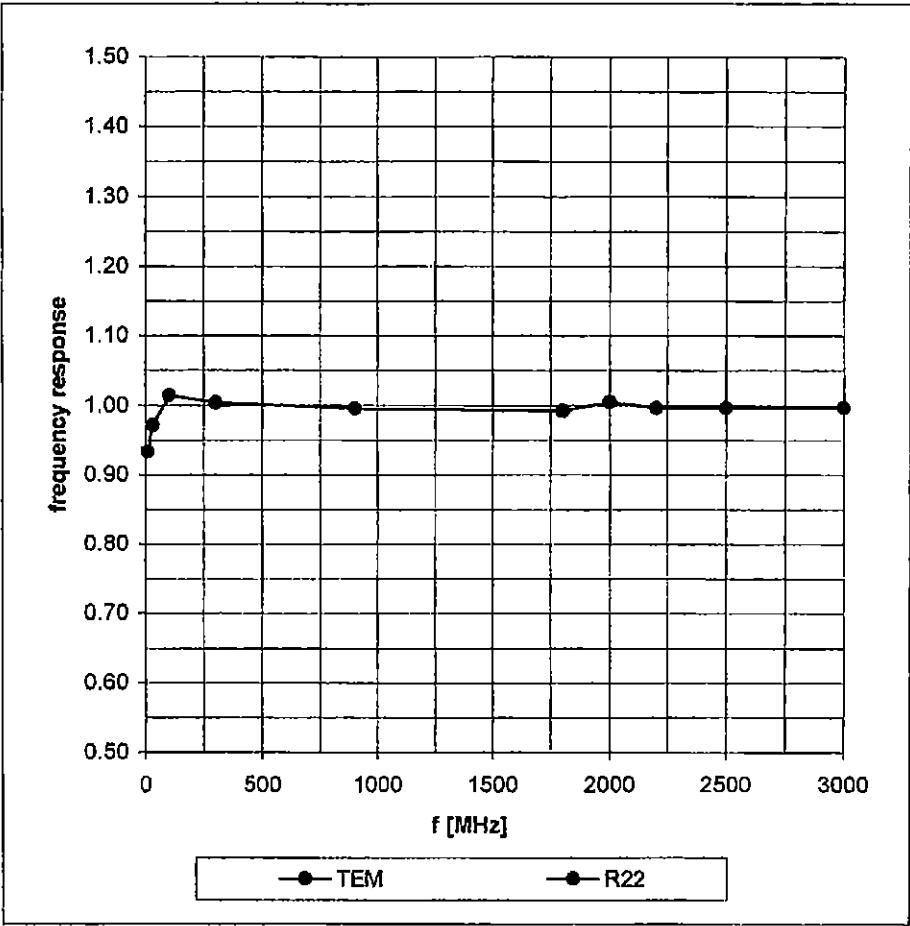

Dynamic Range f(SAR_{brain})
(Waveguide R22)

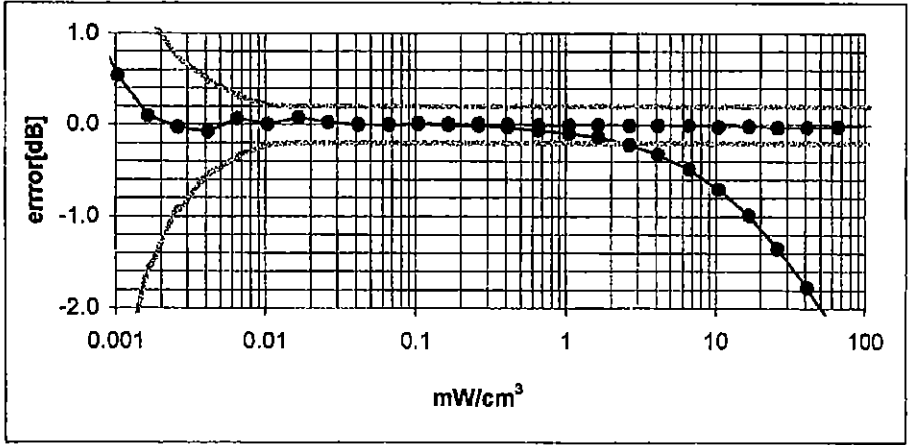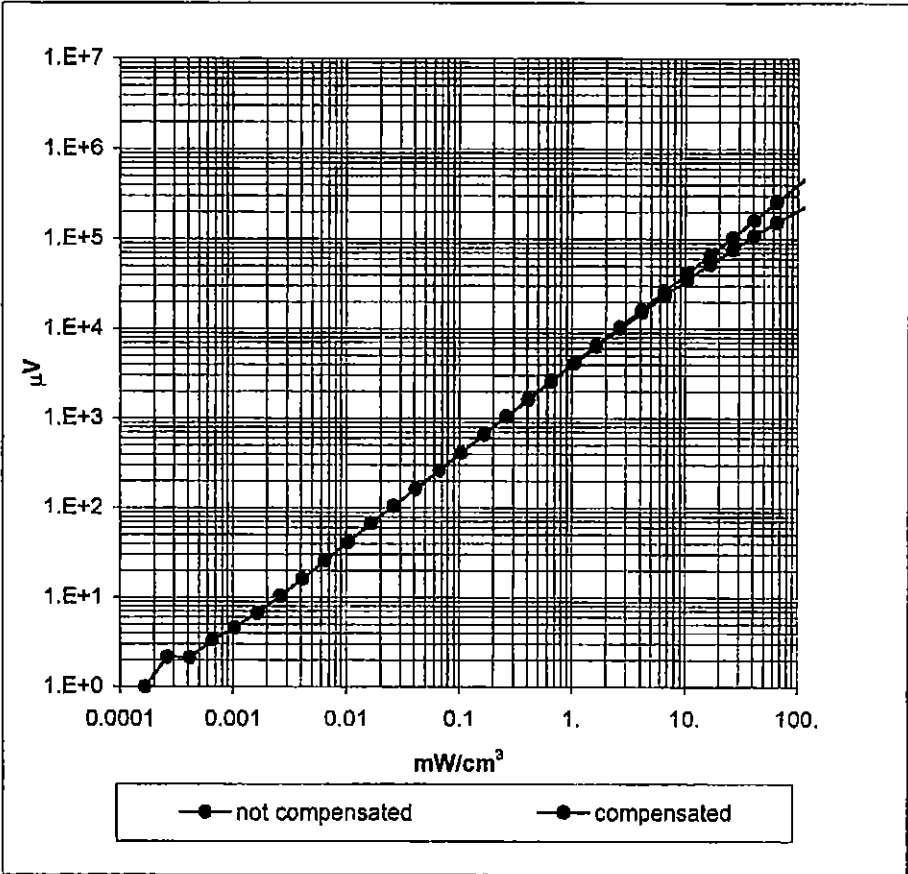

Conversion Factor Assessment

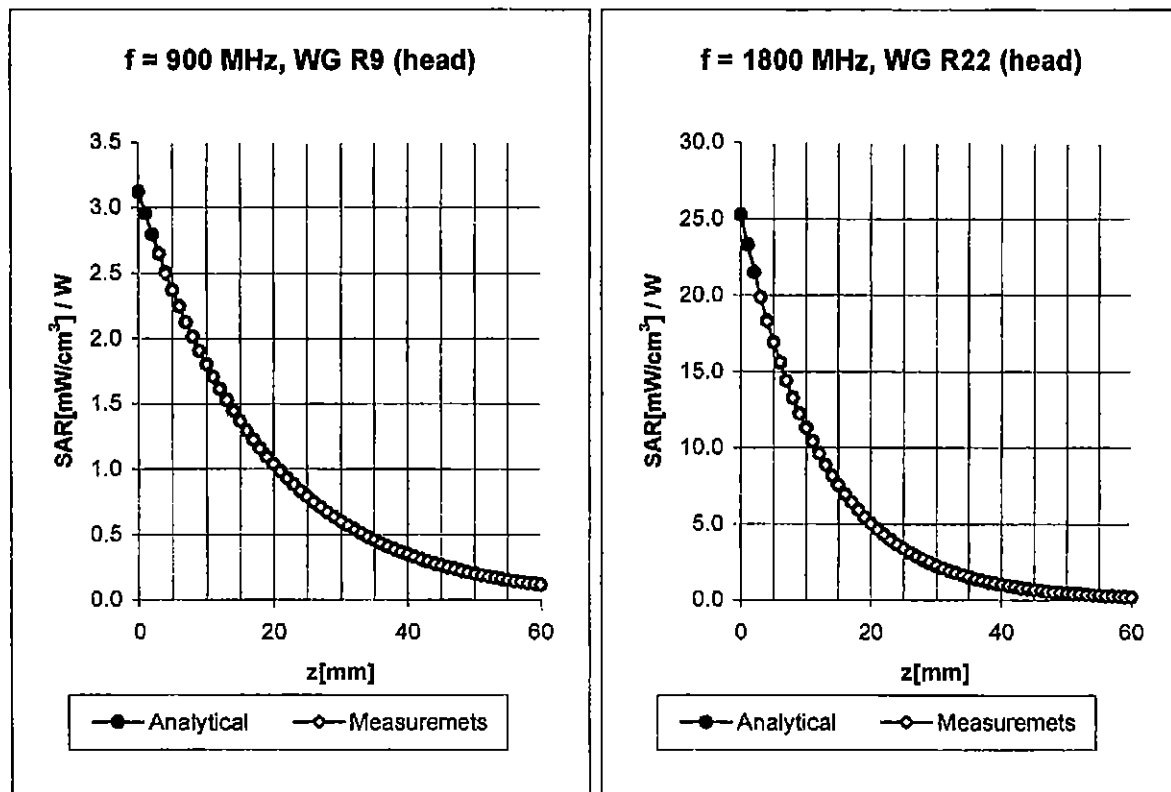

Head 900 MHz $\epsilon_r = 41.5 \pm 5\%$ $\sigma = 0.97 \pm 5\% \text{ mho/m}$

Valid for f=800-1000 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X


ConvF X	6.1 $\pm$ 9.5% (k=2)	Boundary effect:	
ConvF Y	6.1 $\pm$ 9.5% (k=2)	Alpha	0.32
ConvF Z	6.1 $\pm$ 9.5% (k=2)	Depth	1.65

Head **1800 MHz** **$\epsilon_r = 40.0 \pm 5\%$** **$\sigma = 1.40 \pm 5\%$ mho/m**

Valid for f=1710-1910 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

ConvF X	5.0 $\pm$ 9.5% (k=2)	Boundary effect:	
ConvF Y	5.0 $\pm$ 9.5% (k=2)	Alpha	0.25
ConvF Z	5.0 $\pm$ 9.5% (k=2)	Depth	2.30

Conversion Factor Assessment

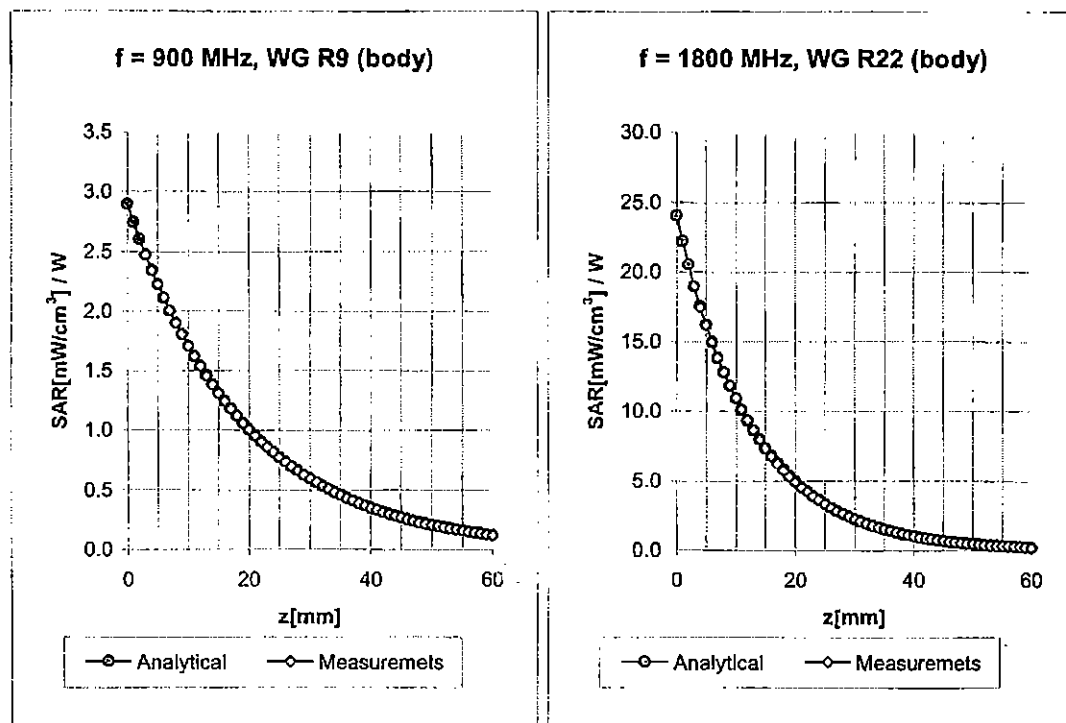

Body 900 MHz $\epsilon_r = 55.0 \pm 5\%$ $\sigma = 1.05 \pm 5\% \text{ mho/m}$

Valid for $f=800\text{-}1000$ MHz with Body Tissue Simulating Liquid according to OET 65 Suppl. C


ConvF X	6.0 $\pm 9.5\%$ ($k=2$)	Boundary effect:	
ConvF Y	6.0 $\pm 9.5\%$ ($k=2$)	Alpha	0.38
ConvF Z	6.0 $\pm 9.5\%$ ($k=2$)	Depth	1.47

Body 1800 MHz $\epsilon_r = 53.3 \pm 5\%$ $\sigma = 1.52 \pm 5\% \text{ mho/m}$

Valid for $f=1710\text{-}1910$ MHz with Body Tissue Simulating Liquid according to OET 65 Suppl. C

ConvF X	4.5 $\pm 9.5\%$ ($k=2$)	Boundary effect:	
ConvF Y	4.5 $\pm 9.5\%$ ($k=2$)	Alpha	0.22
ConvF Z	4.5 $\pm 9.5\%$ ($k=2$)	Depth	3.42

Conversion Factor Assessment

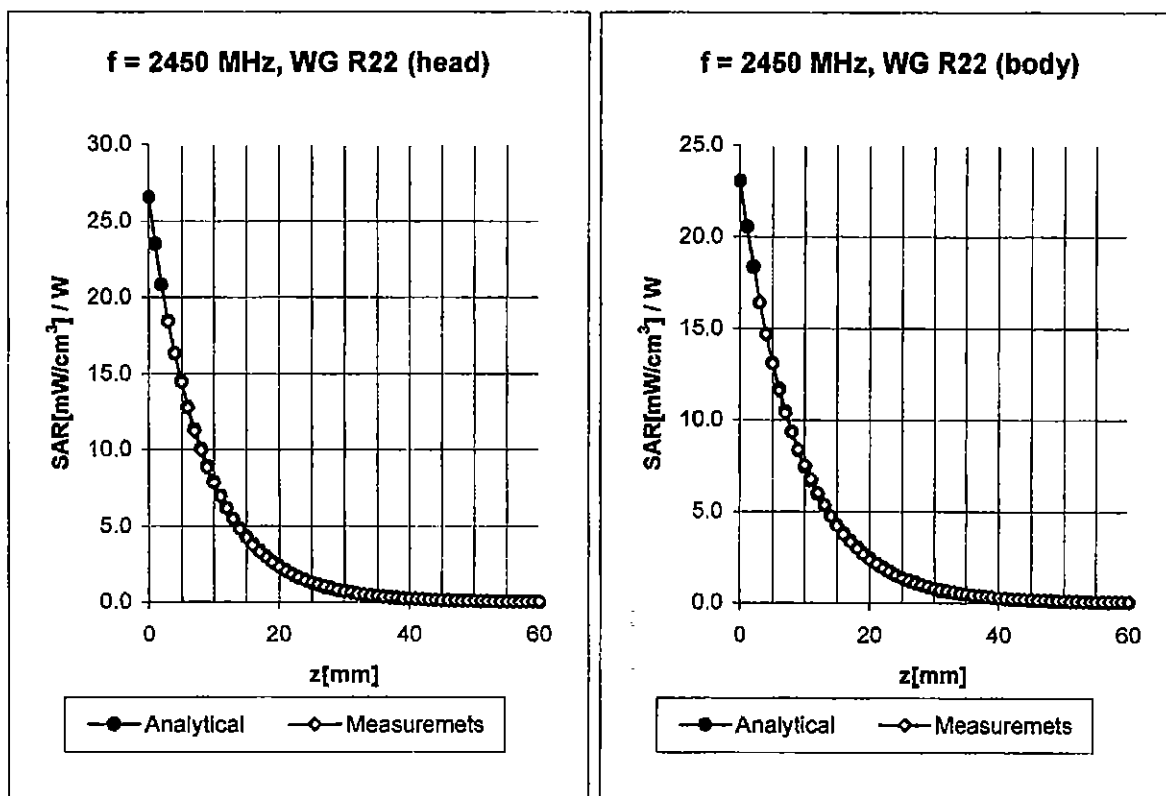

Head **2450 MHz** $\epsilon_r = 39.2 \pm 5\%$ $\sigma = 1.80 \pm 5\%$ mho/m

Valid for f=2400-2500 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X


ConvF X	4.5 $\pm 9.5\%$ (k=2)	Boundary effect:
ConvF Y	4.5 $\pm 9.5\%$ (k=2)	Alpha 0.42
ConvF Z	4.5 $\pm 9.5\%$ (k=2)	Depth 1.56

Body **2450 MHz** $\epsilon_r = 52.7 \pm 5\%$ $\sigma = 1.95 \pm 5\%$ mho/m

Valid for f=2400-2500 MHz with Body Tissue Simulating Liquid according to OET 65 Suppl. C

ConvF X	4.2 $\pm 9.5\%$ (k=2)	Boundary effect:
ConvF Y	4.2 $\pm 9.5\%$ (k=2)	Alpha 0.42
ConvF Z	4.2 $\pm 9.5\%$ (k=2)	Depth 1.65

Conversion Factor Assessment

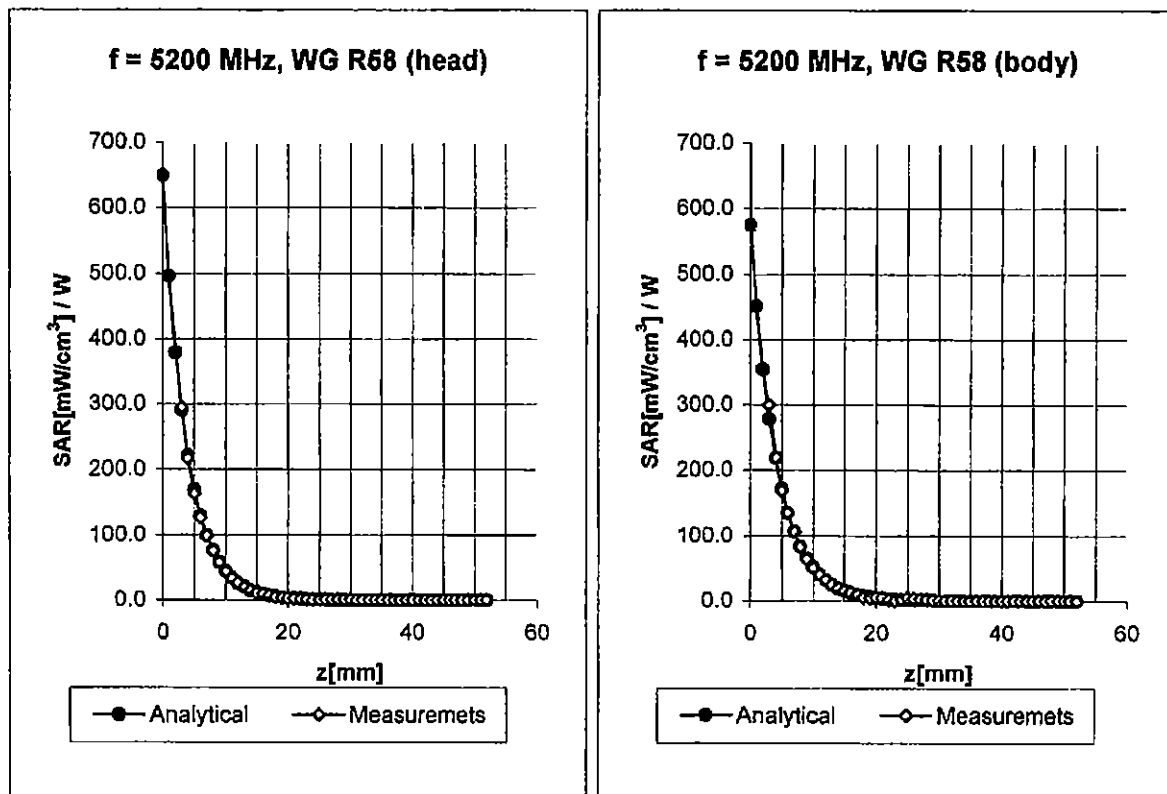

Head **5200 MHz** $\epsilon_r = 36.0 \pm 5\%$ $\sigma = 4.66 \pm 5\%$ mho/m

Valid for f=4940-5460 MHz with Head Tissue Simulating Liquid according to OET65-SuppC


ConvF X	2.60 $\pm 16.6\%$ (k=2)	Boundary effect:	
ConvF Y	2.60 $\pm 16.6\%$ (k=2)	Alpha	0.93
ConvF Z	2.60 $\pm 16.6\%$ (k=2)	Depth	1.50

Body **5200 MHz** $\epsilon_r = 49.0 \pm 5\%$ $\sigma = 5.30 \pm 5\%$ mho/m

Valid for f=4940-5460 MHz with Body Tissue Simulating Liquid according to OET65-SuppC

ConvF X	1.80 $\pm 16.6\%$ (k=2)	Boundary effect:	
ConvF Y	1.80 $\pm 16.6\%$ (k=2)	Alpha	1.05
ConvF Z	1.80 $\pm 16.6\%$ (k=2)	Depth	1.60

Conversion Factor Assessment

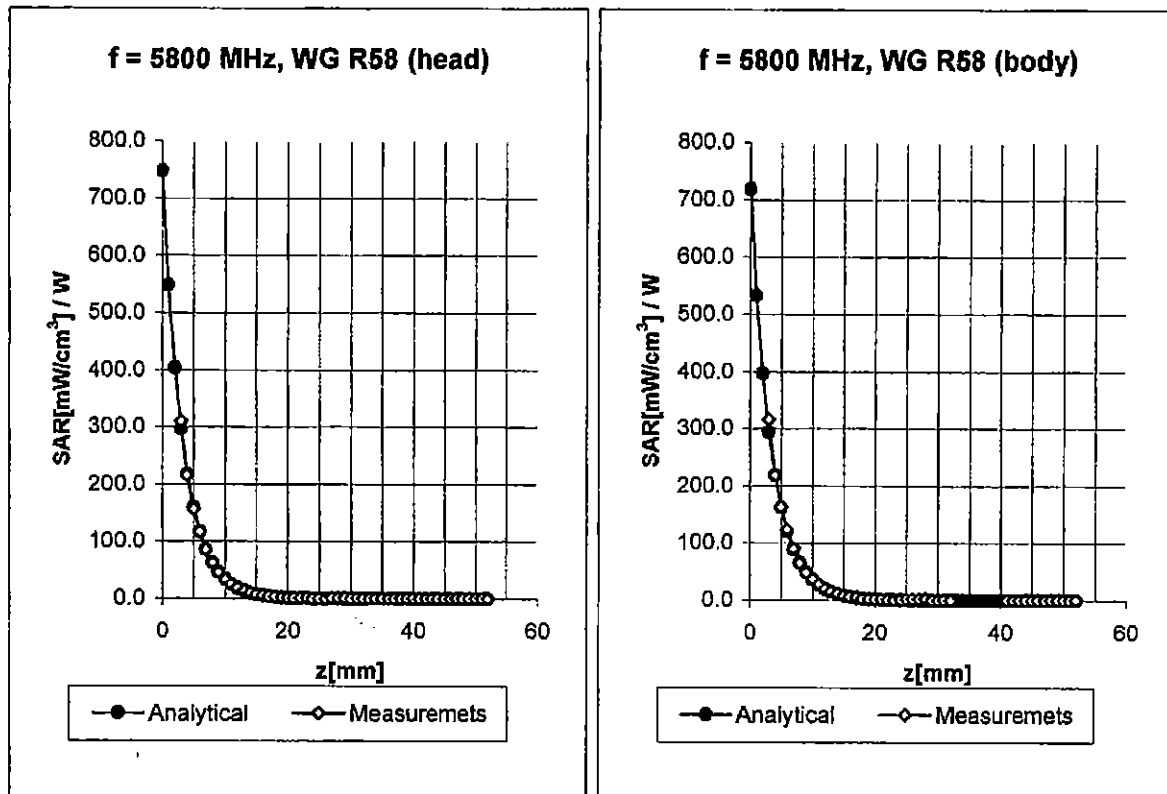

Head **5800 MHz** $\epsilon_r = 35.3 \pm 5\%$ $\sigma = 5.27 \pm 5\% \text{ mho/m}$

Valid for f=5510-6090 MHz with Head Tissue Simulating Liquid according to OET65-SuppC

ConvF X	2.15 $\pm 16.6\%$ (k=2)	Boundary effect:
ConvF Y	2.15 $\pm 16.6\%$ (k=2)	Alpha 1.04
ConvF Z	2.15 $\pm 16.6\%$ (k=2)	Depth 1.50

Body **5800 MHz** $\epsilon_r = 48.2 \pm 5\%$ $\sigma = 6.0 \pm 5\% \text{ mho/m}$

Valid for f=5510-6090 MHz with Body Tissue Simulating Liquid according to OET65-SuppC

ConvF X	1.57 $\pm 16.6\%$ (k=2)	Boundary effect:
ConvF Y	1.57 $\pm 16.6\%$ (k=2)	Alpha 1.15
ConvF Z	1.57 $\pm 16.6\%$ (k=2)	Depth 1.70

Deviation from Isotropy in HSL

Error ($\theta\phi$), $f = 900$ MHz

