

***APPENDIX "C" – PROBE CALIBRATION***

# Probe ET3DV6

**SN:1387**

Manufactured:	September 21, 1999
Last calibration:	September 22, 1999

Calibrated for System DASY3

**DASY3 - Parameters of Probe: ET3DV6 SN:1387**

## Sensitivity in Free Space

NomX	<b>1.55</b> $\mu\text{V}/(\text{V}/\text{m})^2$
NomY	<b>1.65</b> $\mu\text{V}/(\text{V}/\text{m})^2$
NormZ	<b>1.64</b> $\mu\text{V}/(\text{V}/\text{m})^2$

## Diode Compression

DCP X	<b>98</b> mV
DCP Y	<b>98</b> mV
DCP Z	<b>98</b> mV

## Sensitivity in Tissue Simulating Liquid

**Brain**                      **450 MHz**                       $\epsilon_r = 48 \pm 5\%$                        $\sigma = 0.50 \pm 10\%$  mho/m

ConvF X	<b>6.76</b> extrapolated	Boundary effect:
ConvF Y	<b>6.76</b> extrapolated	Alpha <b>0.30</b>
ConvF Z	<b>6.76</b> extrapolated	Depth <b>2.52</b>

**Brain**                      **900 MHz**                       $\epsilon_r = 42.5 \pm 5\%$                        $\sigma = 0.86 \pm 10\%$  mho/m

ConvF X	<b>6.34</b> $\pm 7\%$ (k=2)	Boundary effect:
ConvF Y	<b>6.34</b> $\pm 7\%$ (k=2)	Alpha <b>0.47</b>
ConvF Z	<b>6.34</b> $\pm 7\%$ (k=2)	Depth <b>2.25</b>

**Brain**                      **1500 MHz**                       $\epsilon_r = 41 \pm 5\%$                        $\sigma = 1.32 \pm 10\%$  mho/m

ConvF X	<b>5.78</b> interpolated	Boundary effect:
ConvF Y	<b>5.78</b> interpolated	Alpha <b>0.69</b>
ConvF Z	<b>5.78</b> interpolated	Depth <b>1.88</b>

**Brain**                      **1800 MHz**                       $\epsilon_r = 41 \pm 5\%$                        $\sigma = 1.69 \pm 10\%$  mho/m


ConvF X	<b>5.50</b> $\pm 7\%$ (k=2)	Boundary effect:
ConvF Y	<b>5.50</b> $\pm 7\%$ (k=2)	Alpha <b>0.81</b>
ConvF Z	<b>5.50</b> $\pm 7\%$ (k=2)	Depth <b>1.70</b>

## Sensor Offset


Probe Tip to Sensor Center	<b>2.7</b>	mm
Optical Surface Detection	<b>1.6 <math>\pm</math> 0.2</b>	mm

## Receiving Pattern ( $\phi$ ), $\theta = 0^\circ$


**f = 30 MHz, TEM cell ifi110**

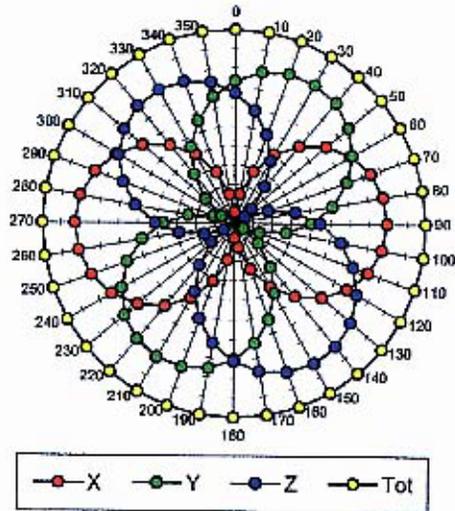


**f = 100 MHz, TEM cell ifi110**

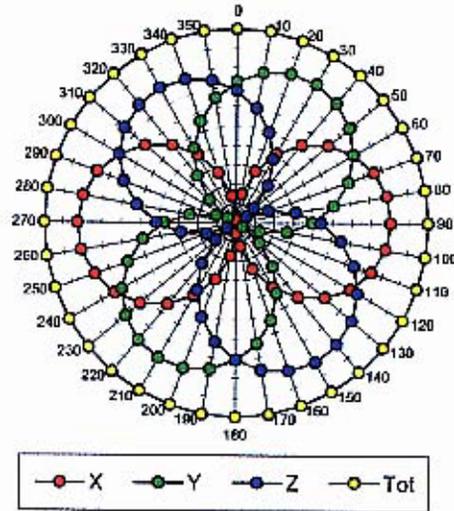


**f = 300 MHz, TEM cell ifi110**

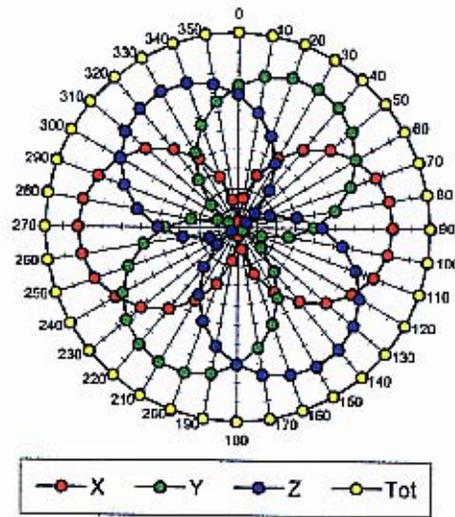


**f = 900 MHz, TEM cell ifi110**

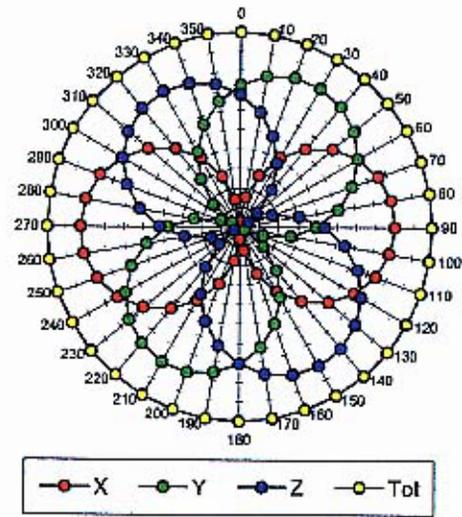

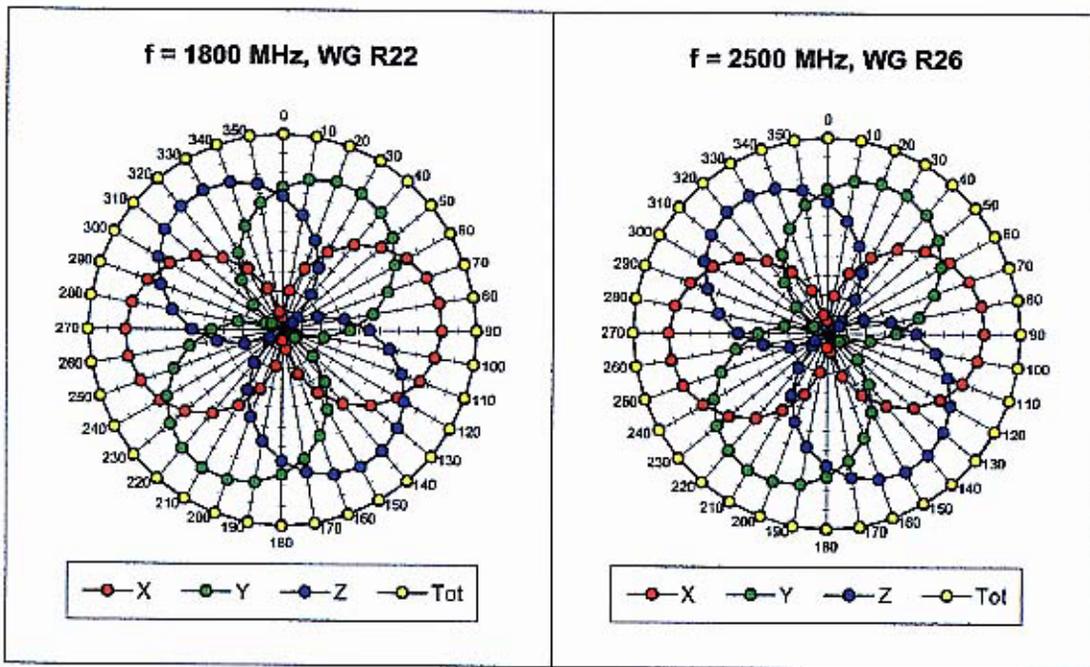

Isotropy Error ( $\phi$ ),  $\theta = 0^\circ$

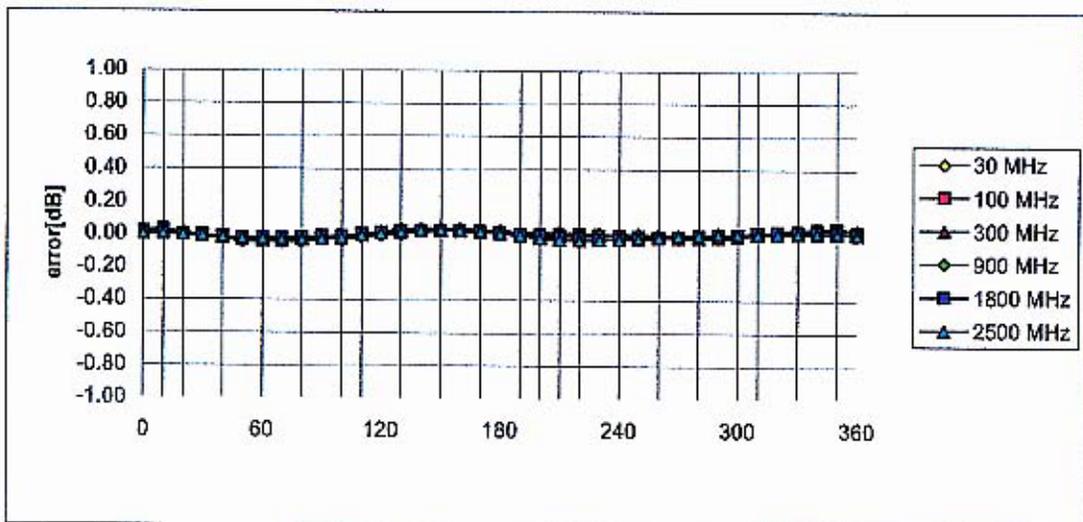

## Frequency Response of E-Field

( TEM-Cell:ifi110, Waveguide R22, R26 )

