

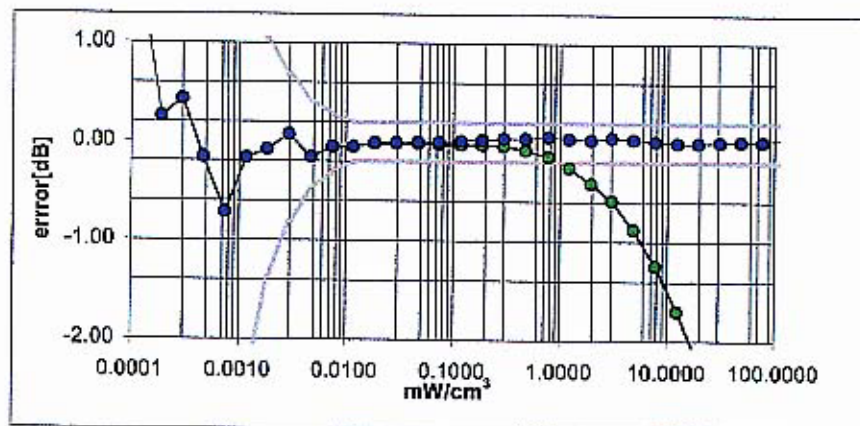



Dynamic Range $f(\text{SAR}_{\text{brain}})$ (TEM-Cell:ifi110)

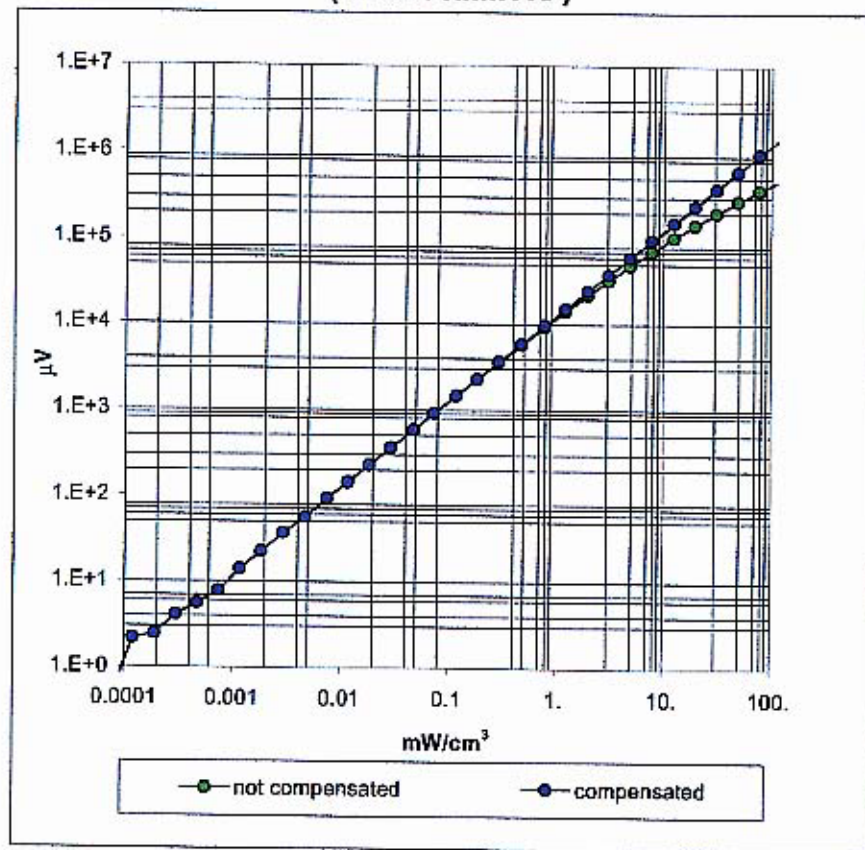

Conversion Factor Assessment


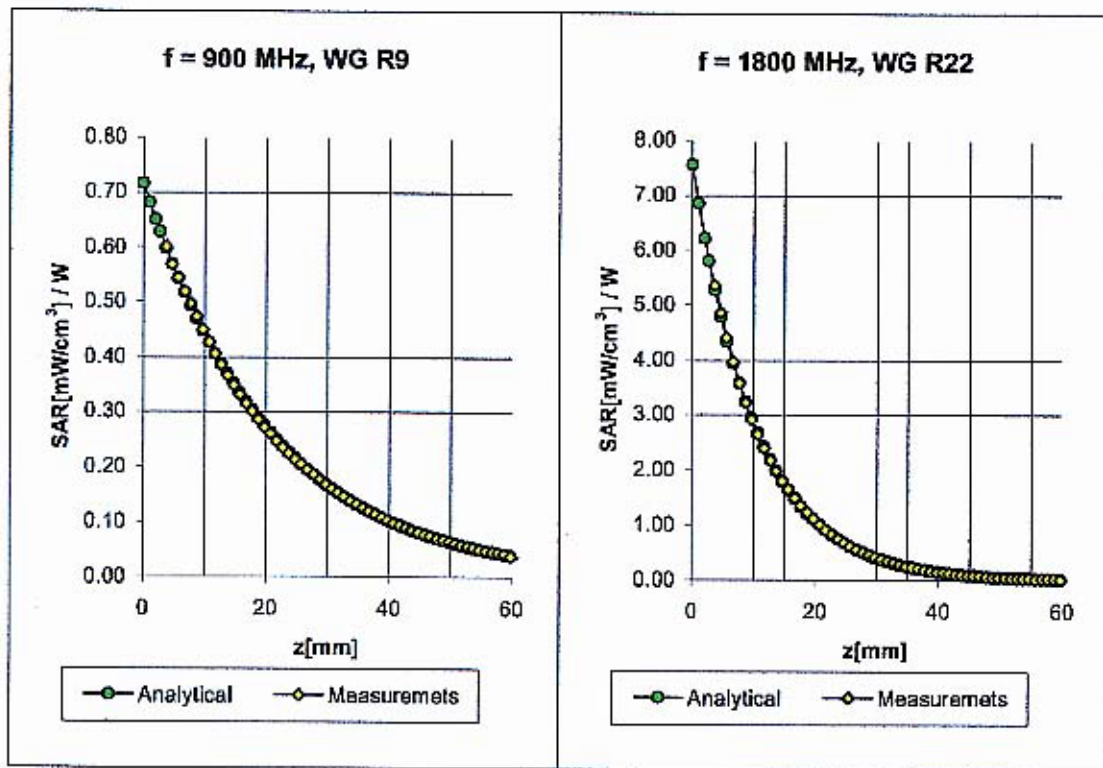


Receiving Pattern (ϕ) (in brain tissue, $z = 5$ mm)

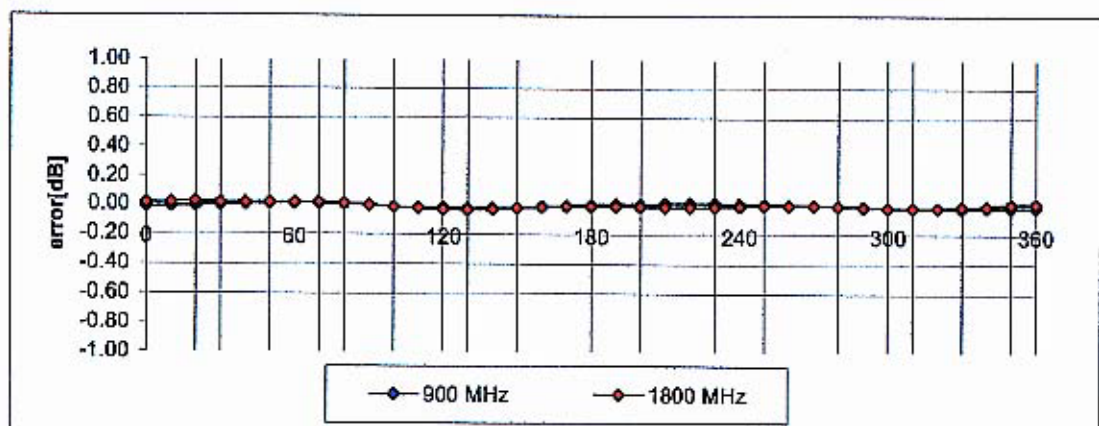

APPENDIX "D" – TEST SETUP PHOTOGRAPHS

FACE-HELD SAR TEST SETUP PHOTOGRAPHS
4.0cm Separation Distance

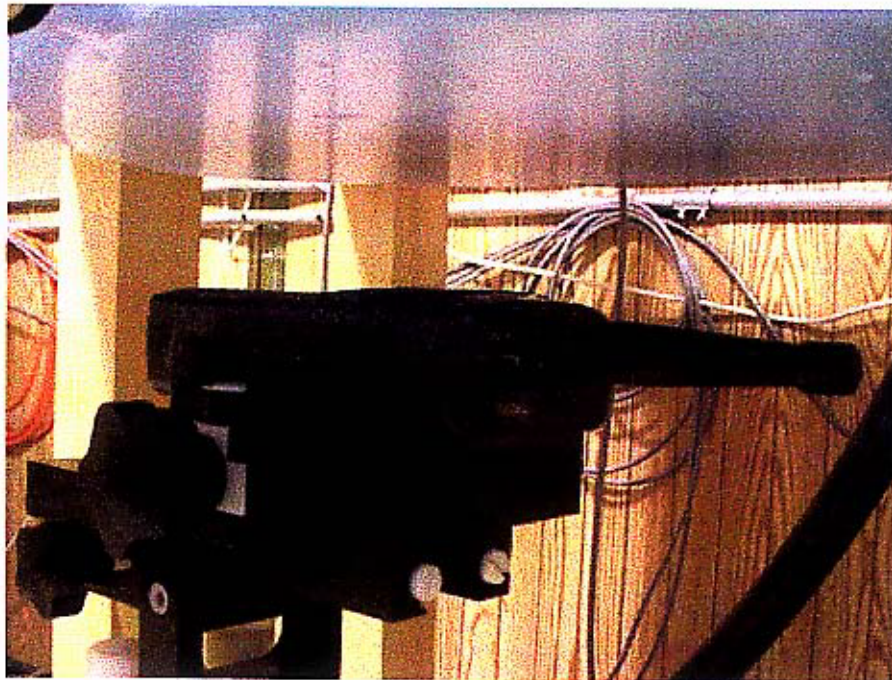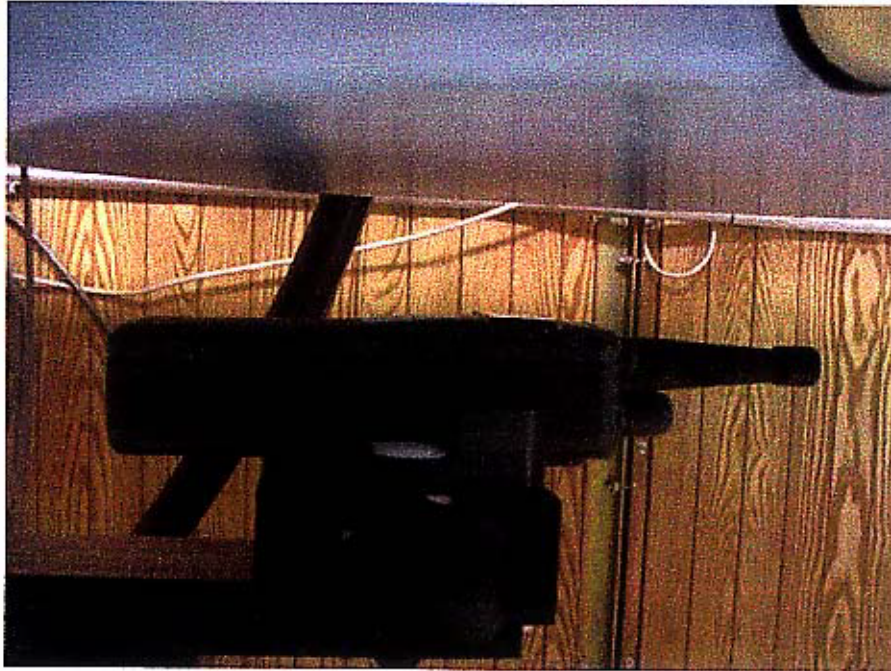

BODY-WORN SAR TEST SETUP PHOTOGRAPHS
0.8cm Separation Distance with Belt-Clip

