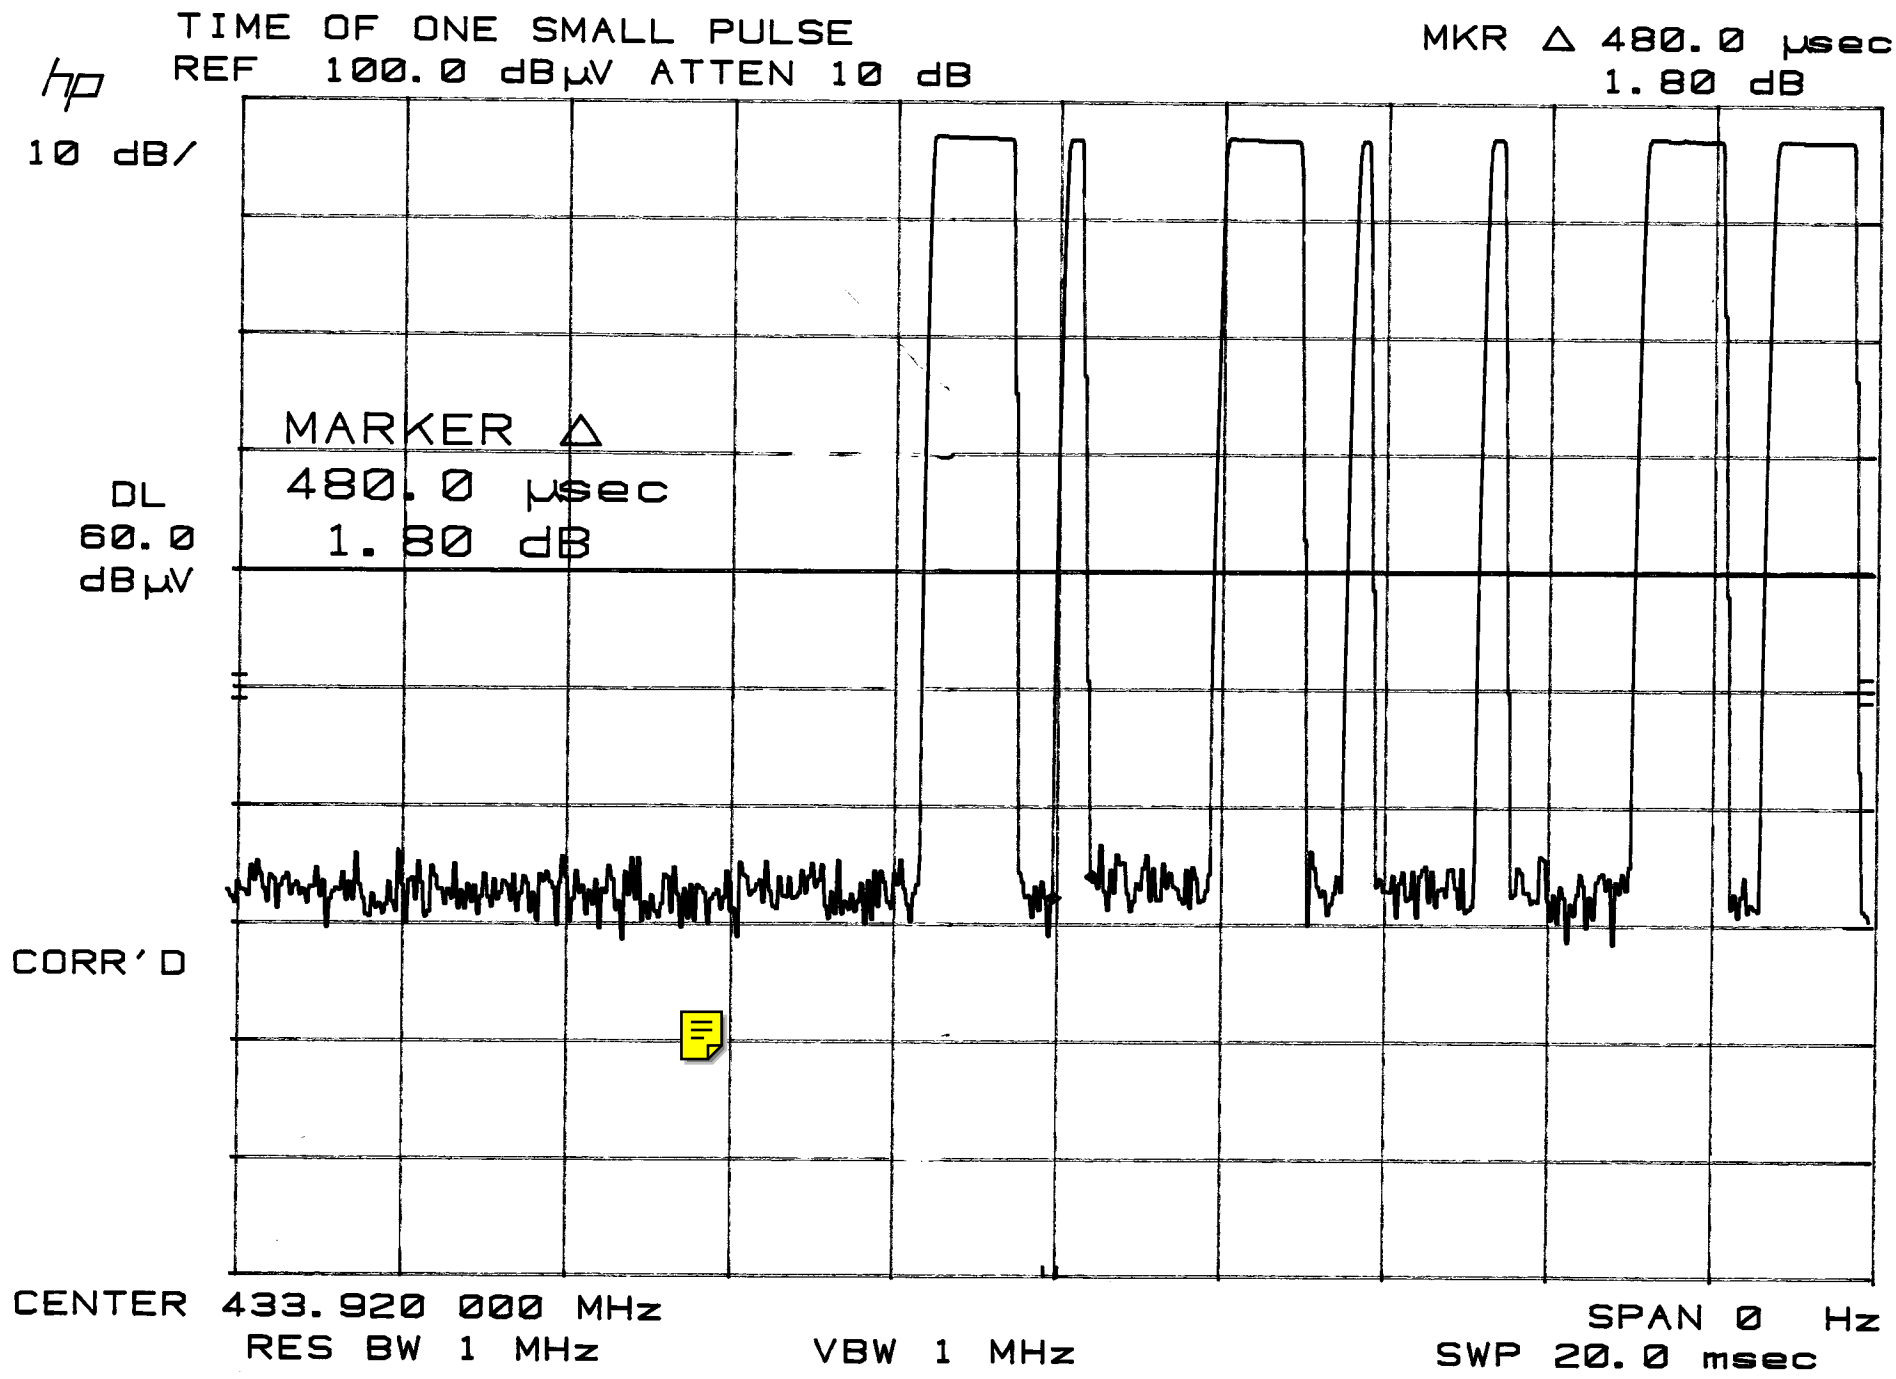
TIME OF ONE SMALL PULSE
REF 100.0 dBμV ATTEN 10 dB
MKR Δ 480.0 μsec
1.80 dB
10 dB/
MARKER Δ
480.0 μsec
1.80 dB
DL
60.0
dBμV
CORR'D
CENTER 433.920 000 MHz
RES BW 1 MHz
VBW 1 MHz
SPAN 0 Hz
SWP 20.0 msec

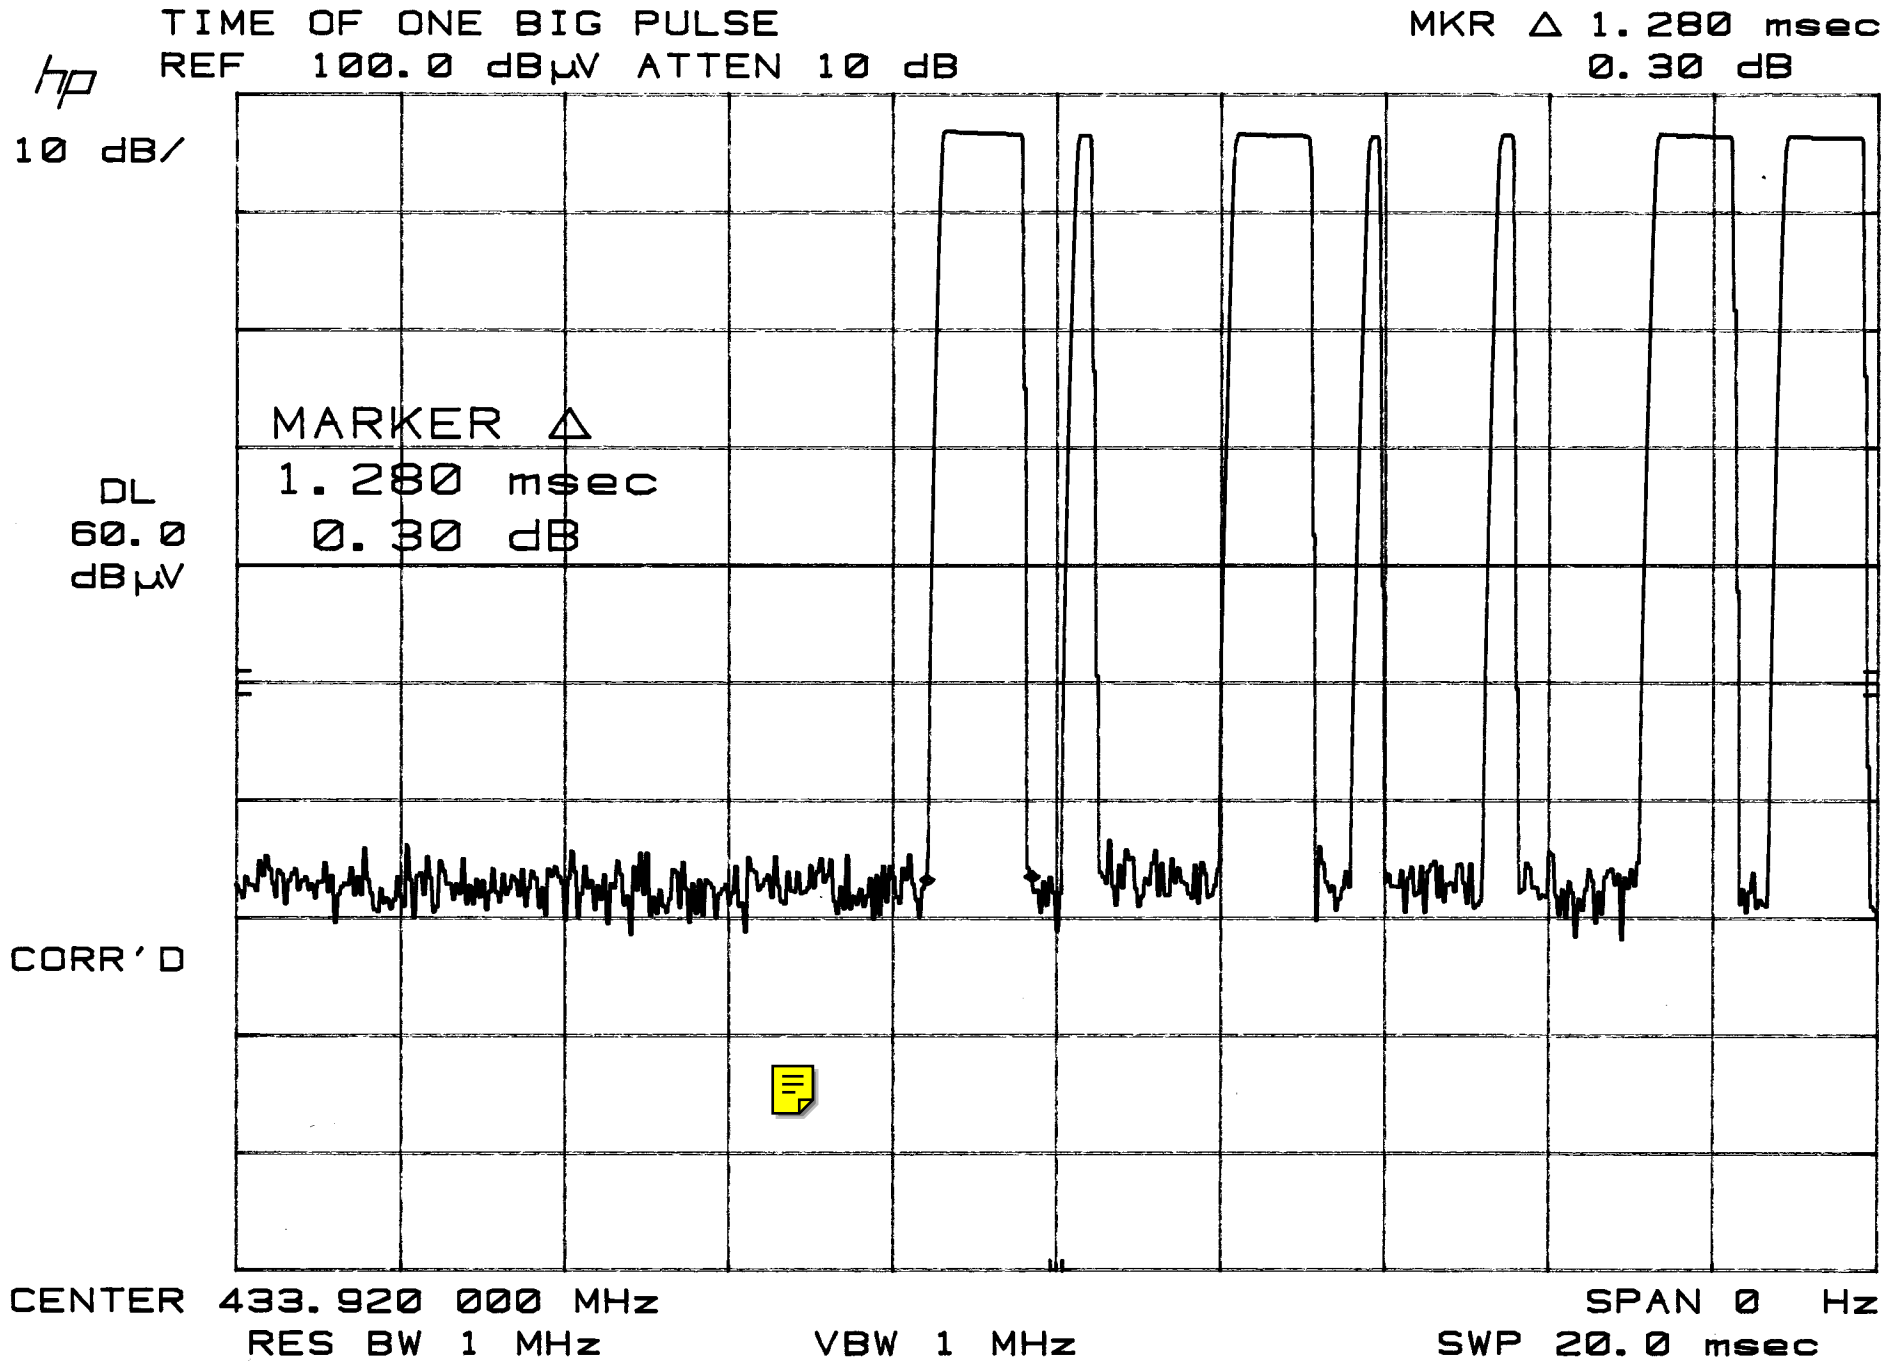
TIME OF ONE BIG PULSE
REF 100.0 dBμV ATTEN 10 dB
MKR Δ 1.280 msec
0.30 dB
10 dB/
MARKER Δ
1.280 msec
0.30 dB
DL
60.0
dBμV
CORR'D
CENTER 433.920 000 MHz
RES BW 1 MHz
VBW 1 MHz
SPAN 0 Hz
SWP 20.0 msec

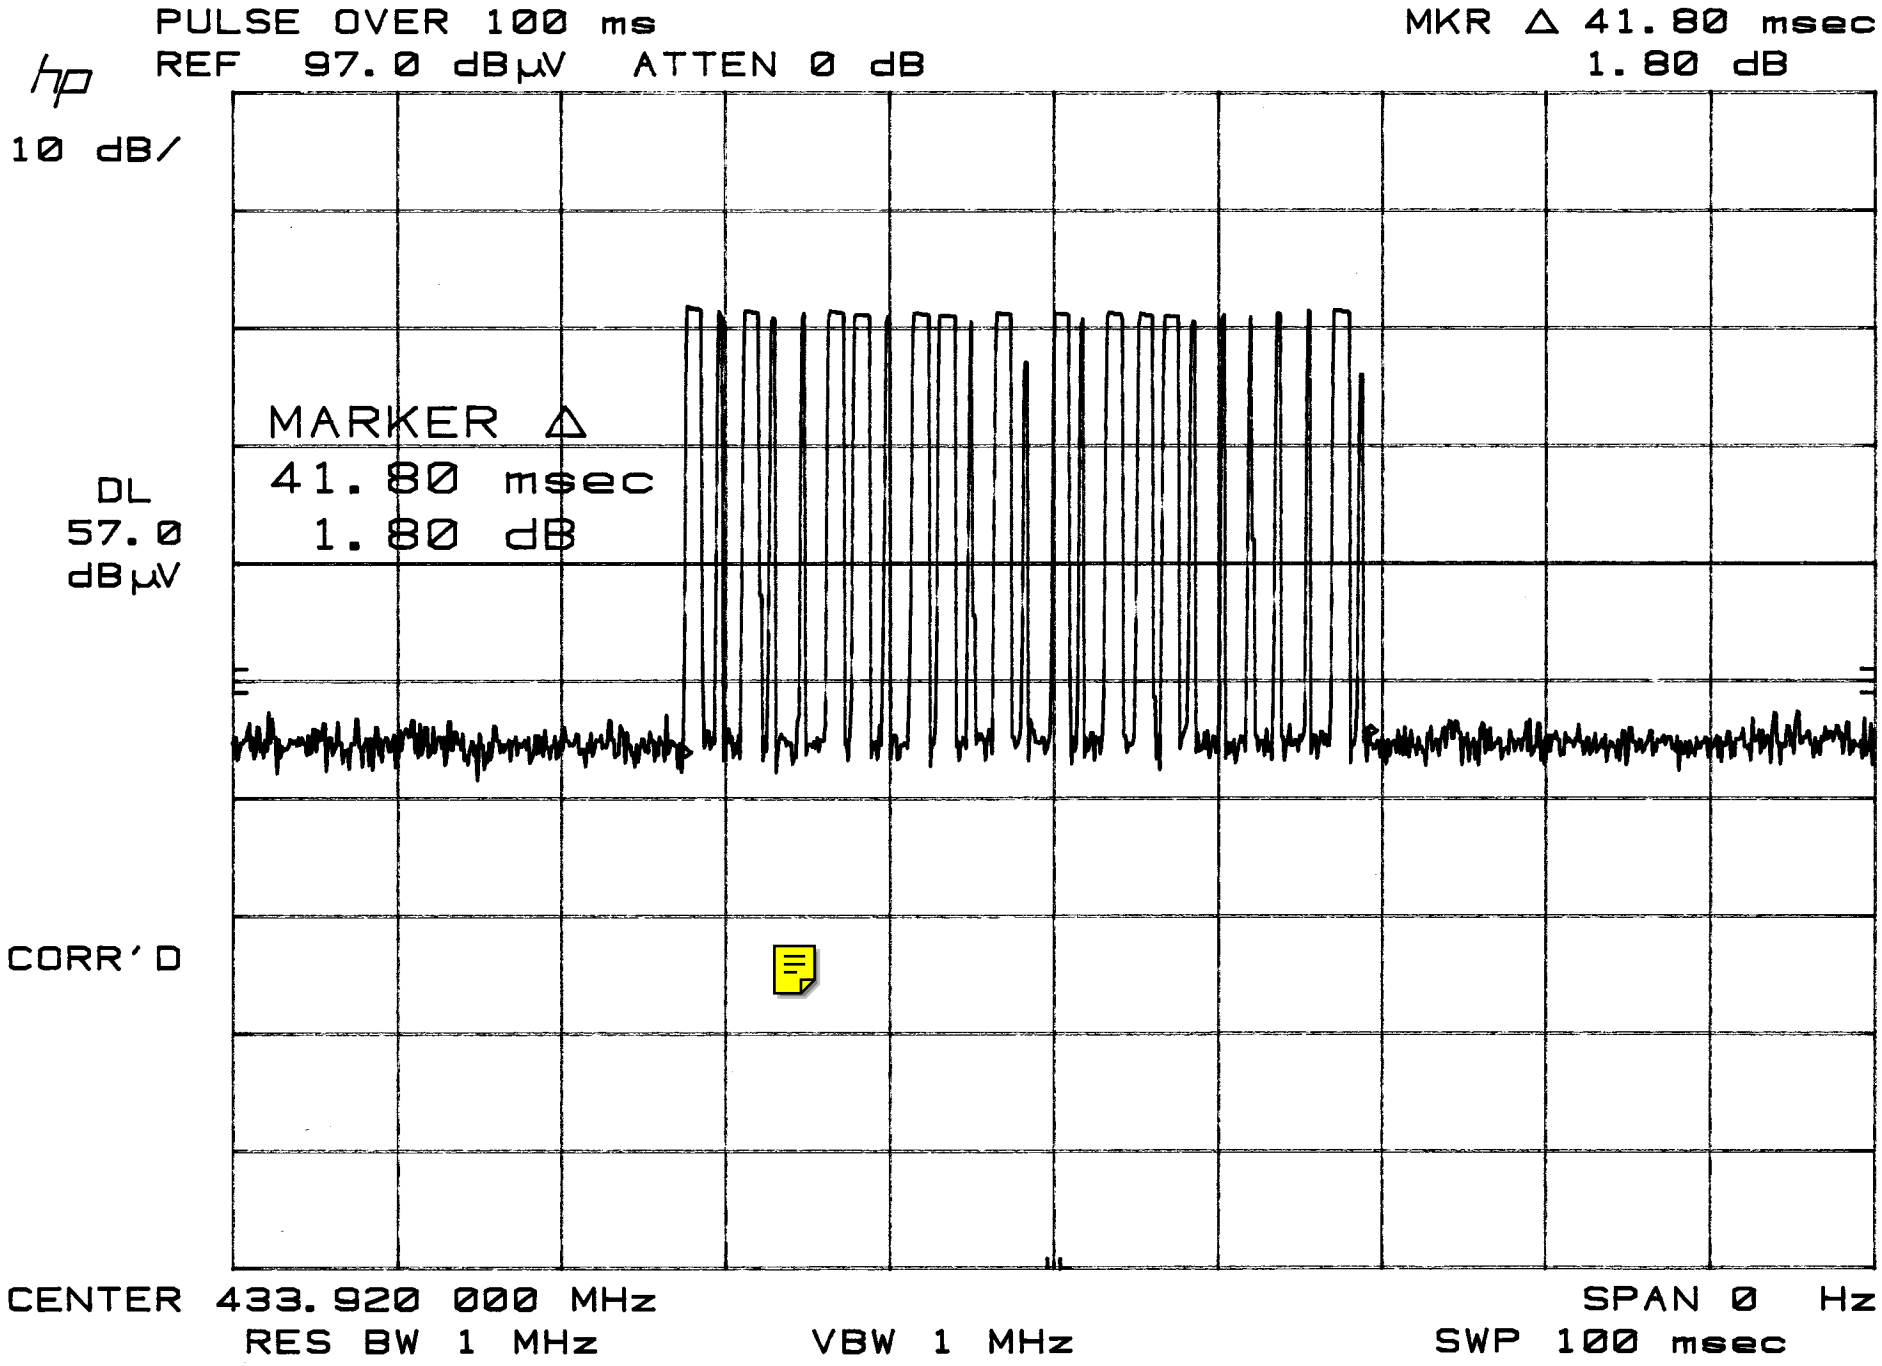
PULSE OVER 100 ms
REF 97.0 dBμV ATTEN 0 dB
MKR Δ 41.80 msec
1.80 dB
10 dB/
MARKER Δ
41.80 msec
1.80 dB
DL
57.0
dBμV
CORR'D
CENTER 433.920 000 MHz
RES BW 1 MHz
VBW 1 MHz
SPAN 0 Hz
SWP 100 msec