

835MHz Brain Dipole Validation

SAM Phantom; Flat Section; Probe:ET3DV6 - SN1677; ConvF(6.70,6.70,6.70)


Med. Parameters 835 MHz Brain: $\sigma = 0.91$ mho/m $\epsilon_r = 40.0$ $\rho = 1.00$ g/cm³; Antenna Position -- Out; Crest Factor 1.0

SAR (1g): 2.47 mW/g ± 0.00 dB, SAR (10g): 1.56 mW/g ± 0.00 dB

835MHz Brain Dipole Validation (D835V2 S/N: 406)

Frequency: 835 MHz; Antenna Input Power: 250 [mW]; Ambient Temp. = 22.3°C / Meas. Tissue Temp. = 22.2°C

PCTEST Brain Tissue Simulating Liquid [08/05/2002]

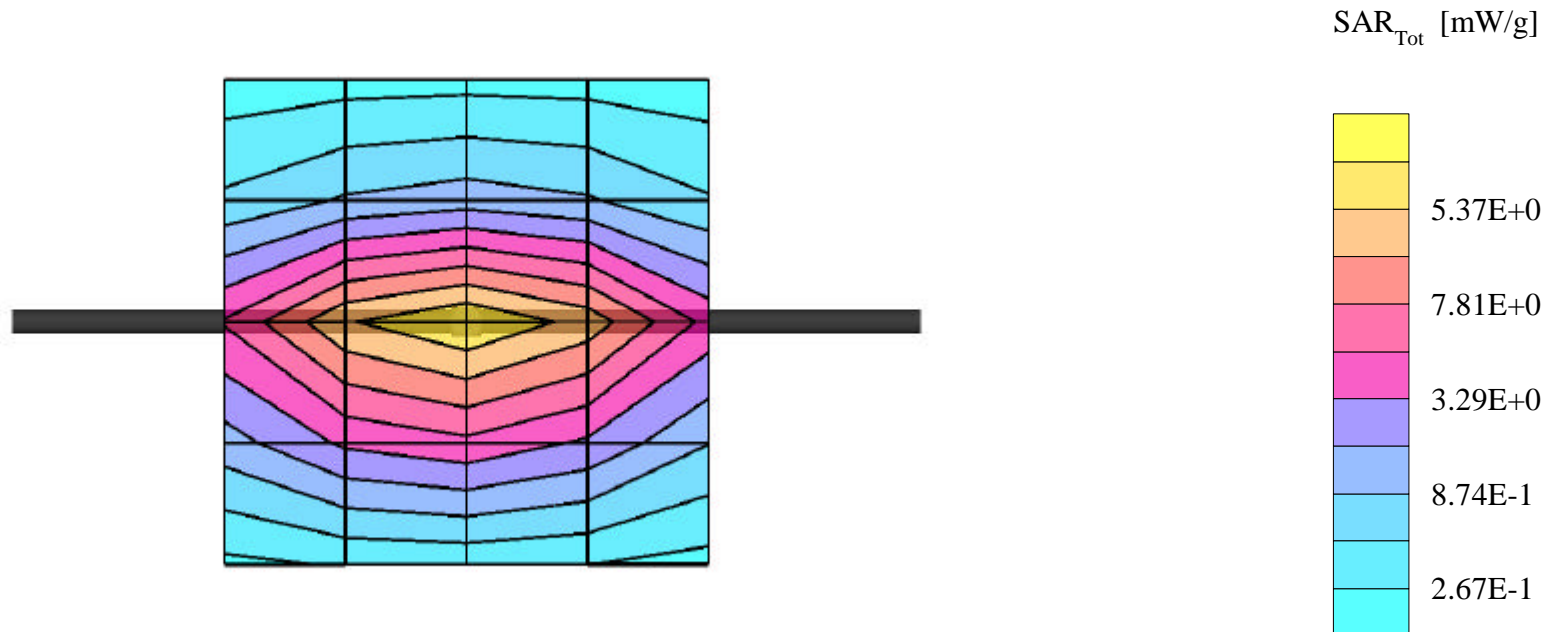


1900MHz Brain Dipole Validation

SAM Phantom; Flat Section; Probe:ET3DV6 - SN1677; ConvF(5.30,5.30,5.30)

Med. Parameters 1900 MHz Brain: $\sigma = 1.45$ mho/m $\epsilon_r = 41.8$ $\rho = 1.00$ g/cm³; Antenna Position -- Out; Crest Factor 1.0
SAR (1g): 9.96 mW/g, SAR (10g): 5.05 mW/g

1900MHz Brain Dipole Validation (D1900V2 S/N: 502)

Frequency: 1900 MHz; Antenna Input Power: 250 [mW]; Ambient Temp. = 22.3°C / Meas. Tissue Temp. = 22.2°
PCTEST Brain Tissue Simulating Liquid [08/06/2002]

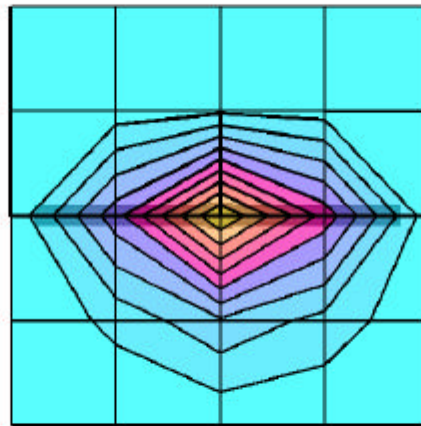

SAR_{Tot} [mW/g]

