

MFA **M. Flom Associates, Inc. - Global Compliance Center**
3356 North San Marcos Place, Suite 107, Chandler, Arizona 85225-7176
www.mflom.com general@mflom.com (480) 926-3100, FAX: 926-3598

Date: September 28, 2000

Federal Communications Commission
Via Electronic Filing

Attention: Authorization & Evaluation Division

Applicant: Icom Incorporated
Equipment: IC-F40GT-2 and IC-F4GS-2
FCC ID: AFJIC-F40G-2
FCC Rules: 47 CFR 1.1307, Environmental Assessment

Gentlemen:

On behalf of the Applicant, enclosed please find the Supplemental Test Data Report and all pertinent documentation, the whole for Environmental Assessment of the referenced equipment as shown.

We trust the same is in order. Should you need any further information, kindly contact the writer who is authorized to act as agent.

Sincerely yours,



Morton Flom, P. Eng.

enclosure(s)
cc: Applicant
MF/cvr

MFA **M. Flom Associates, Inc. - Global Compliance Center**
3356 North San Marcos Place, Suite 107, Chandler, Arizona 85225-7176
www.mflom.com general@mflom.com (480) 926-3100, FAX: 926-3598

ENVIRONMENTAL ASSESSMENT

FOR

PORTABLES

Held to Face and/or Belt-Clip Operation

for

FCC ID: FCC ID: AFJIC-F40G-2

Model: IC-F40GT-2 and IC-F4GS-2

to

FEDERAL COMMUNICATIONS COMMISSION

DATE OF REPORT: September 28, 2000

ON THE BEHALF OF THE APPLICANT:

Icom Incorporated

AT THE REQUEST OF:

P.O. UPS 6/2/00

Icom America, Inc.
2380 - 116th Ave. N. E.
P.O. C-90029
Bellevue, Washington 98009-9029

Attention of:

Masaaki Takahashi, Product Development Manager
m-takahashi@icomamerica.com
(800) 872-4266; (425) 454-8155; FAX: -1509

SUPERVISED BY:




Morton Flom, P. Eng.

TABLE OF CONTENTS

<u>DESCRIPTION</u>	<u>PAGE</u>
Test Report	1
EUT Description and Specifications	2
R.F. Power Output	4
Probe Calibration	5
True Induced Voltage	6
Conductivity, Brain Tissue	7
Peak SAR - Brain Tissue	8
Conductivity - Muscle Tissue	9
Annex A	

PAGE NO. 1 of 9.

Required information per ISO/IEC Guide 25-1990, paragraph 13.2:

- a) TEST REPORT (SUPPLEMENTAL)
- b) Laboratory: M. Flom Associates, Inc.
 (FCC: 31040/SIT) 3356 N. San Marcos Place, Suite 107
 (Canada: IC 2044) Chandler, AZ 85225
- c) Report Number: d0090055
- d) Client: Icom America, Inc.
 2380 - 116th Ave. N. E.
 P.O. C-90029
 Bellevue, Washington 98009-9029
- e) Identification: IC-F40GT-2 and IC-F4GS-2
 FCC ID: AFJIC-F40G-2
 Description: UHF FM Handheld Transceiver
- f) EUT Condition: Not required unless specified in individual tests.
- g) Report Date: September 28, 2000
 EUT Received: June 2, 2000
- h, j, k): As indicated in individual tests.
- i) Sampling method: No sampling procedure used.
- l) Uncertainty: In accordance with MFA internal quality manual.
- m) Supervised by: 
 Morton Flom, P. Eng.
- n) Results: The results presented in this report relate only to the item tested.
- o) Reproduction: This report must not be reproduced, except in full, without written permission from this laboratory.

PAGE NO.

2 of 9.

IDENTIFICATION OF THE EQUIPMENT UNDER TEST (EUT)NAME AND ADDRESS OF APPLICANT:

Icom Incorporated
1-6-19 Kamikurazukuri
Hirano-ku
Osaka, Japan 547

MANUFACTURER:

Applicant

FREQUENCY RANGE, MHz:

450 to 490

WATTS:

4 W. Max, Conducted

ANTENNA TYPE:

1/4 Wave

SUPPLIED:

Yes

INTEGRAL:

No


GAIN:

0 db, reference to dipole

MODULATION:

F3E

M. Flom Associates, Inc. is accredited by the American Association for Laboratory Association (A2LA) as shown in the scope below.



THE AMERICAN ASSOCIATION FOR LABORATORY ACCREDITATION

ACCREDITED LABORATORY

A2LA has accredited


M. FLOM ASSOCIATES, INC.
Chandler, AZ

for technical competence in the field of

Electrical (EMC) Testing


The accreditation covers the specific tests and types of tests listed on the agreed scope of accreditation. This laboratory meets the requirements of ISO/IEC Guide 25-1990 "General Requirements for the Competence of Calibration and Testing Laboratories" (equivalent to relevant requirements of the ISO 9000 series of standards) and any additional program requirements in the identified field of testing.

Presented this 24th day of November, 1998.



Peter Abjorn
President
For the Accreditation Council
Certificate Number 1008.01
Valid to December 31, 2000

For tests or types of tests to which this accreditation applies, please refer to the laboratory's Electrical (EMC) Scope of Accreditation



American Association for Laboratory Accreditation

SCOPE OF ACCREDITATION TO ISO/IEC GUIDE 25-1990 AND EN 45001

M. FLOM ASSOCIATES, INC.
Electronic Testing Laboratory
3356 North San Marcos Place, Suite 107
Chandler, AZ 85225
Morton Flom Phone: 480 926 3100

ELECTRICAL (EMC)

Valid to: December 31, 2000 Certificate Number: 1008-01

In recognition of the successful completion of the A2LA evaluation process, accreditation is granted to this laboratory to perform the following electromagnetic compatibility tests:

Tests	Standard(s)
RF Emissions	FCC Part 15 (Subparts B and C) using ANSI C63 4-1992; CISPR 11; CISPR 13; CISPR 14; CISPR 22; EN 55011; EN 55013; EN 55014; EN 55022; EN 50081-1; EN 50081-2; FCC Part 18; ICES-003; AS/NZS 1044; AS/NZS 1053; AS/NZS 3548; AS/NZS 4251.1; CNS 13438
RF Immunity	EN 50082-1; EN 50082-2; AS/NZS 4251.1
Radiated Susceptibility	EN 61000-4-3; ENV 50140; ENV 50204; IEC 1000-4-3; IEC 801-3
ESD	EN 61000-4-2; IEC 1000-4-2; IEC 801-2
EFT	EN 61000-4-4; IEC 1000-4-4; IEC 801-4
Surge	EN 61000-4-5; ENV 50142; IEC 1000-4-5; IEC 801-5
47 CFR (FCC)	2, 21, 22, 23, 24, 74, 80, 87, 90, 95, 97

Revised 2/2/2000

Peter Abjorn

5301 Buckeystown Pike, Suite 350 • Frederick, MD 21704-8370 • Phone: 301 644 3248 • Fax: 301 662 2974

"This laboratory is accredited by the American Association for Laboratory Accreditation (A2LA) and the results shown in this report have been determined in accordance with the laboratory's terms of accreditation unless stated otherwise in the report."

Should this report contain any data for tests for which we are not accredited, or which have been undertaken by a subcontractor that is not A2LA accredited, such data would not covered by this laboratory's A2LA accreditation.

PAGE NO.

4 of 9.

R.F. Power Output

Conducted = Yes

Radiated = N/A

<u>Frequency, MHz</u>	<u>Watts, Conducted</u>
450.05	3.507
470.05	3.548
489.95	4.130

After each measurement: 1) Checked Battery Voltage
2) Checked Power Output

PAGE NO.

5 of 9.

Probe Calibration

Probe	Narda 8021B
Calibrated	June 2000
TEM Cell	Fischer Model JM2 TEM
Cross-Sectional Dimensions	15.2 x 9.9 cm
Flux Density	1 milliwatt/cm ²
Feed Power, (free space field)	150.5 milliwatts

At each frequency of interest, the probe is subjected to this free space field. The combined output of the 3 orthogonal outputs is measured.

<u>MHz</u>	<u>Feed Power, mW</u>	<u>Calibration, mV</u>
450.05	150.5	10.09
470.05	150.5	9.61
489.95	150.5	9.44

Field Strength of free space = 0.661 V/cm

PAGE NO.

6 of 9.

True Induced Voltage

<u>Test Data</u>	<u>Measured, millivolts</u>	<u>True Induced Voltage V</u>
450.05	17.99	1.177
470.05	20.28	1.394
489.95	17.80	1.245

Sample Calculation:

For 470.05 MHz

$$\begin{aligned} \text{measured} &= 20.28 \text{ mV} \\ \text{calibration} &= 9.61 \text{ mV} \\ \text{true induced voltage} &= (20.28/9.61) \times 0.661 \\ &= 1.3949 \text{ volts} \end{aligned}$$

PAGE NO.

7 of 9.

Conductivity, σ , Brain Tissue

$$\sigma = e'' \times 8.854 \times 2\pi \times \text{frequency}$$

measured at each frequency with HP85070B network analyzer
and software

<u>MHz</u>	<u>e''</u>	<u>σ, mho/m</u>
470.05	24.77	0.620
470.05	24.34	0.636
489.95	23.77	0.648

Density, ρ

Material density is mass divided by volume.

For tissue material, $\rho = 1.3 \text{ (kg/m}^3\text{)}$ approximately.

PAGE NO.

8 of 9.

Peak SAR - Brain Tissue

$$\text{SAR} = \frac{|E|^2 \times \sigma}{\rho} \text{ w/kg}$$

MHz	Induced Voltage V	Conductivity s/m	SAR w/kg
450.05	1.177	0.620	0.661
470.05	1.394	0.636	0.951
489.95	1.245	0.648	0.773

Uncertainty:

Probe position = $\pm 1\%$
 Volumetric = $\pm 4\%$
 Device positioning = $\pm 5\%$
 Dist., Probe tip to phantom surface = $1 \pm 0.2 \text{ mm}$

EUT Foam cradle - Photo attached

Foam spacers, surface to phantom = 2.5 cm

Conductivity - Muscle Tissue

<u>MHz</u>	<u>e''</u>	<u>Conductivity, (s/m) (mho/m)</u>
450.05	34.44	0.862
470.05	33.68	0.881
489.95	32.97	0.897

Sample Calculation, Conductivity
 $32.97 \times 8.854 \times 2\pi \times 489.95 = 0.897$
 Uncertainty = 5%

Peak SAR


$$SAR = \frac{|E|^2 \times \sigma}{\rho} \text{ w/kg}$$

<u>MHz</u>	<u>Induced Voltage V</u>	<u>Conductivity s/m</u>	<u>SAR w/kg</u>
450.05	0.902	0.862	0.539
450.05	1.024	0.881	0.711
489.95	0.924	0.897	0.589


ANNEX A

<u>DESCRIPTION</u>	<u>PAGE</u>
Test Set-Ups	1
Test Instrumentation	2
Description of Phantom	3
Simulated Tissue	6
Determining SAR	7


Probe Calibration

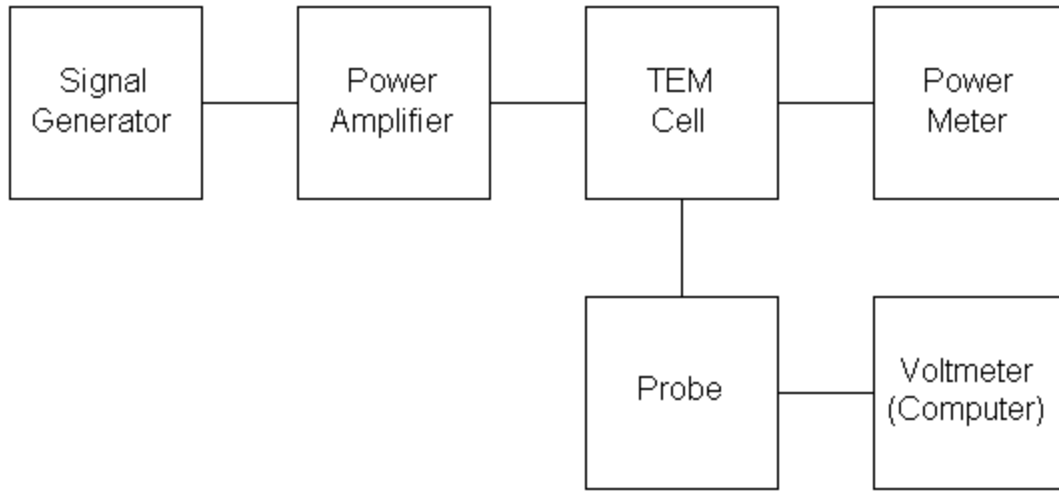

Measurement of ϵ''

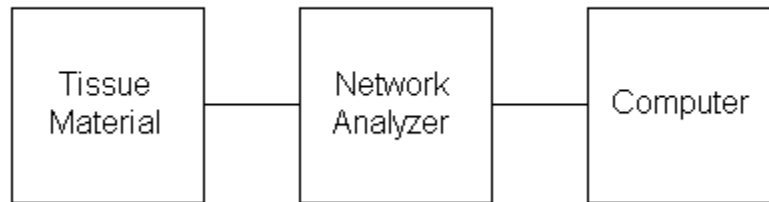

Measurement of SAR

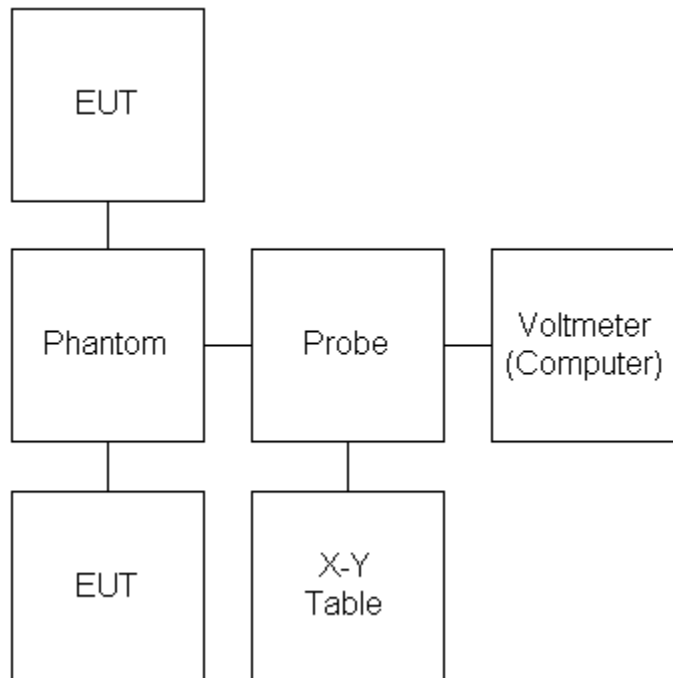

PAGE NO.

2 of 7.

Test Instrumentation

<u>Equipment</u>	<u>Model/Serial No. (as app.)</u>	<u>Cal. Date</u>
1. Signal Generator	HP8640B	Aug. 2000
2. Power Amplifier	Amplifier Research 50W1000A	June 2000
3. Probe	Narda 8021B S/N 04019	June 2000
4. Power Meter	HP436A S/N 2709A16776	June 2000
5. Network Analyzer	HP85070B S/N 103410A00514	June 2000
6. TEM Cell	Fischer JM2TEM S/N 2004	April 2000
7. Phantom	Lab Design Fiber Glass, with 1 cm grid	N/A
8. X-Y Table, Precision	ENCO P/N 201-2826	Not Req'd
9. Computer	Pentium Pro	Not Req'd
10. Precision Thermometer	Guideline 5150 S/N 6485	
11. Foam Cradle	Lab Design, 2.5 cm spacer	N/A

PAGE NO.

3 of 7.

Description Of Phantom

Material: Fiber Glass


Thickness: 2 mm \pm 0.5 mm


L x W x D, cm: 24.13 x 20.0 x 13.33, \pm 1 mm

Dielectric Constant: 3.4 kg/m³

Conductivity: 1.2 x 10⁻⁴

Grid of Phantom Bottom: 16 x 16 cm, graduated 1 cm squares

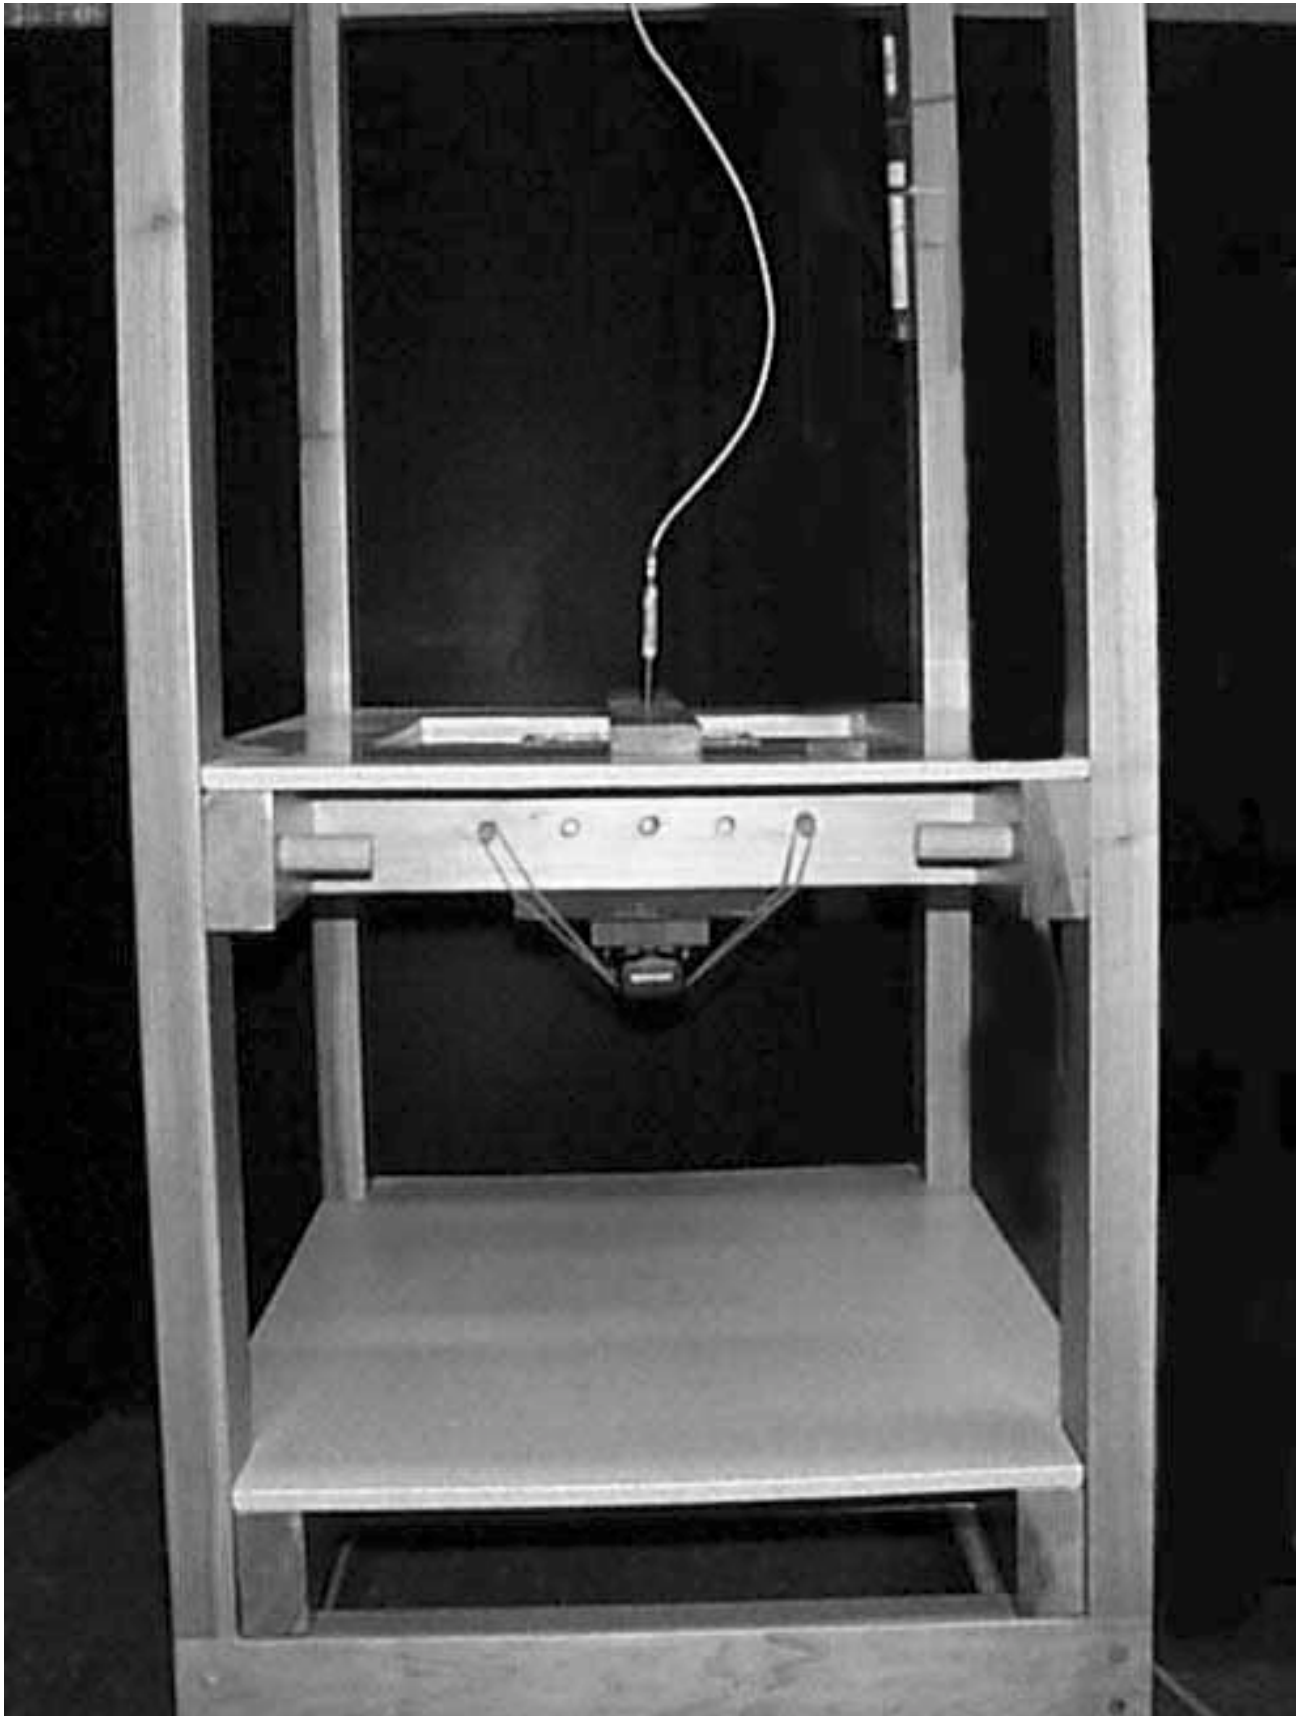

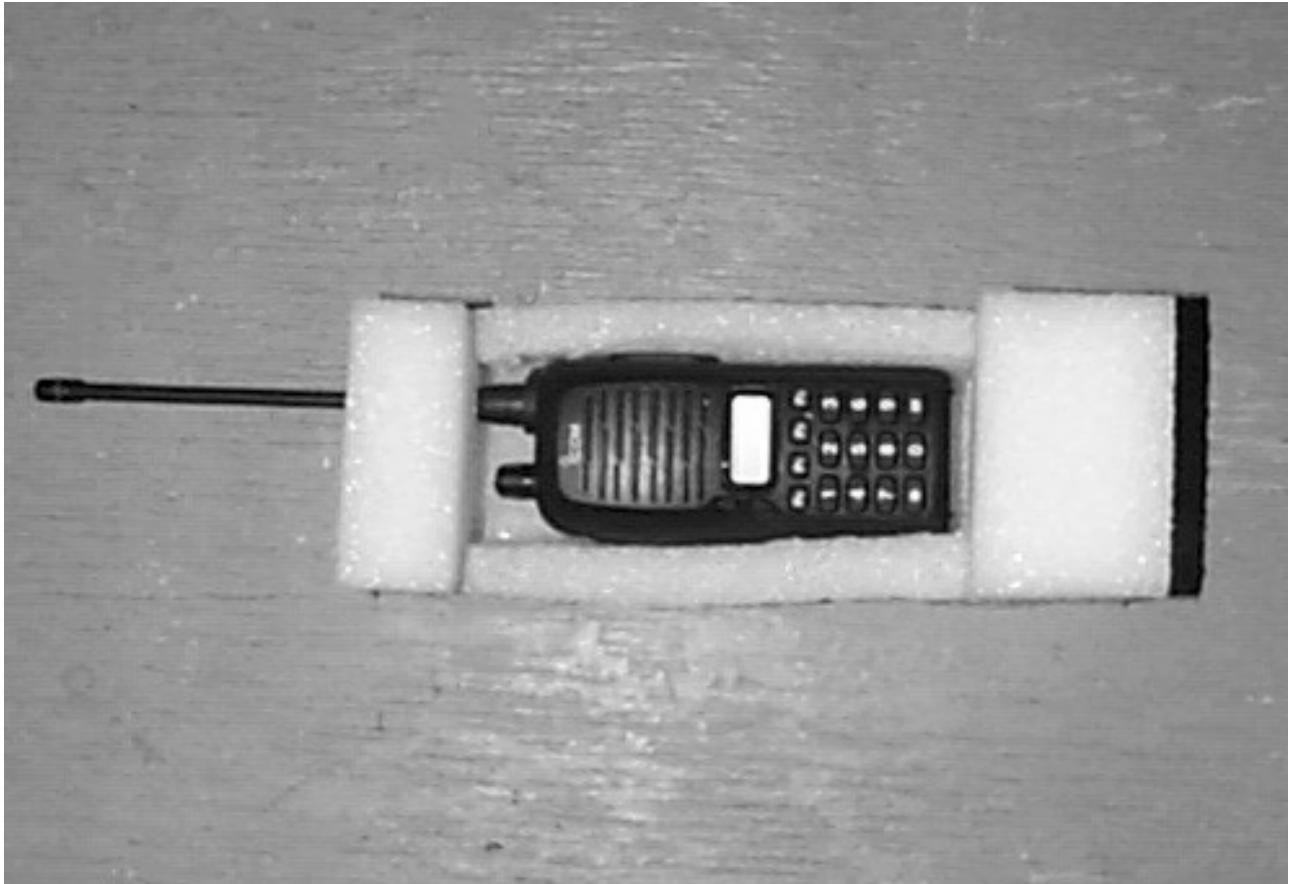

PAGE NO.

6 of 7.

Simulated Tissue - Compositions Solutions

1. Brain Tissue: See Below
2. Muscle Tissue: See Below

MFA Lab Report

Recipe and Preparation: 400 - 500 MHz

The table lists the compositions and conductivity of liquid muscle and brain based on George Hartsgrove and Colleagues in University of Ottawa Ref.; Bioelectromagnetics 8:29-36 (1987). The conductivities are within a 5% target value.

Frequency 400-500 MHz

<u>Ingredient</u>	<u>Muscle Mixture</u>	<u>Brain Mixture</u>
Water	38.56%	42.92%
Sugar	56.32%	58.42%
Salt	3.95%	1.00%
HEC	0.98%	0.30%
Bactericide	0.19%	0.10%
Conductivity	0.832	0.545

1. Weigh all ingredients accurately
2. Heat water 40°C
3. Add salt to bactericide while stirring
4. Add sugar
5. Continue to stir and add hydroxyethylcellulose (HEC)
6. Remove from heat
7. Continue to stir until mixture thickens
8. Let cool to room temperature
9. Keep in closed container when not in use


Method for Determining Value of SAR

Initially a coarse scan is performed over an area of 5 cm x 5 cm closest to the antenna port. The course scan is used to determine the location of the max value using the X - Y table. The center of this location is used to perform a more detailed scan over a 1.5 cm x 1.5 cm grid. Neighboring 1 cm x 1 cm grids are then checked for possibility of higher values.

X - Y Table

Repeatability: >10% of 1 cm
 Resolution: >10% of 1 cm

Grid of Bottom of Phantom

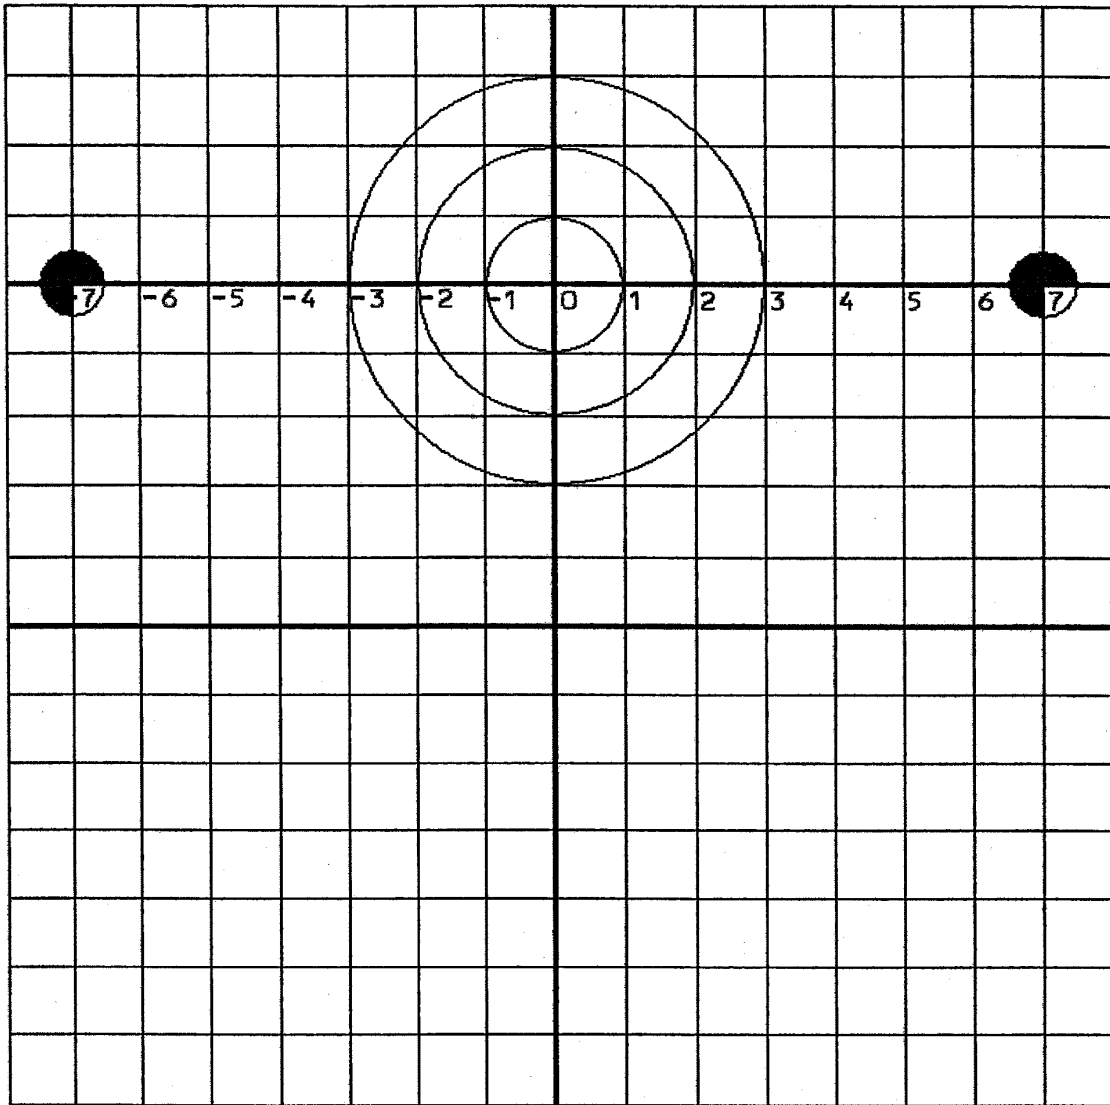

TESTIMONIAL
AND
STATEMENT OF CERTIFICATION

THIS IS TO CERTIFY THAT:

1. THAT the application was prepared either by, or under the direct supervision of, the undersigned.
2. THAT the technical data supplied with the application was taken under my direction and supervision.
3. THAT the data was obtained on representative units, randomly selected.
4. THAT, to the best of my knowledge and belief, the facts set forth in the application and accompanying technical data are true and correct.

CERTIFYING ENGINEER:



Morton Flom, P. Eng.