

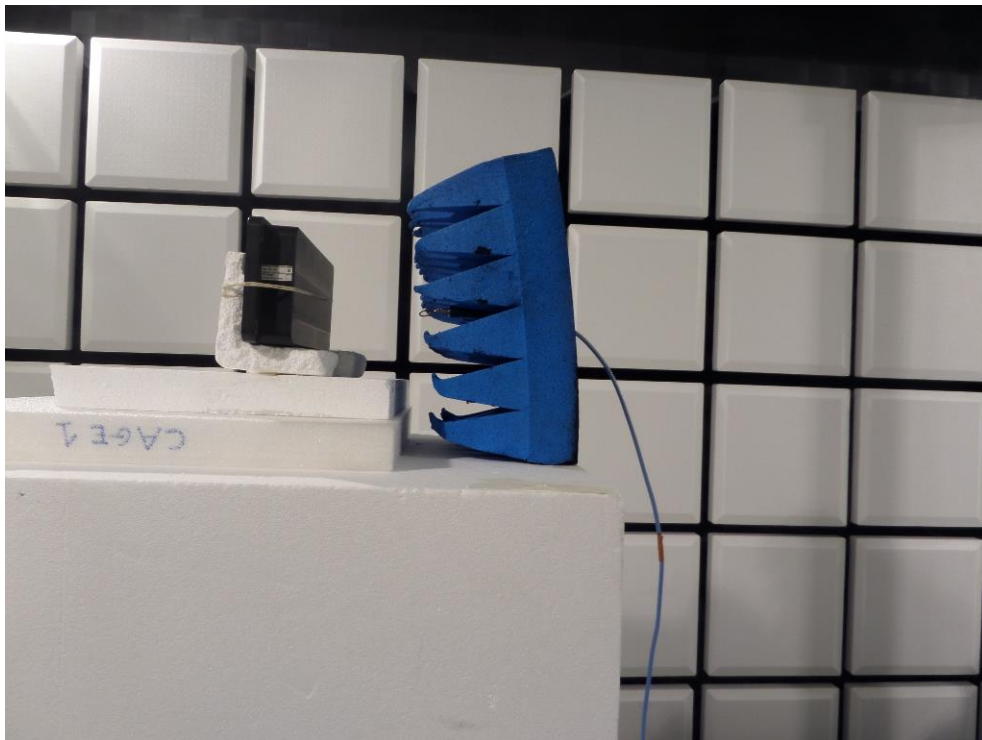


Calibration

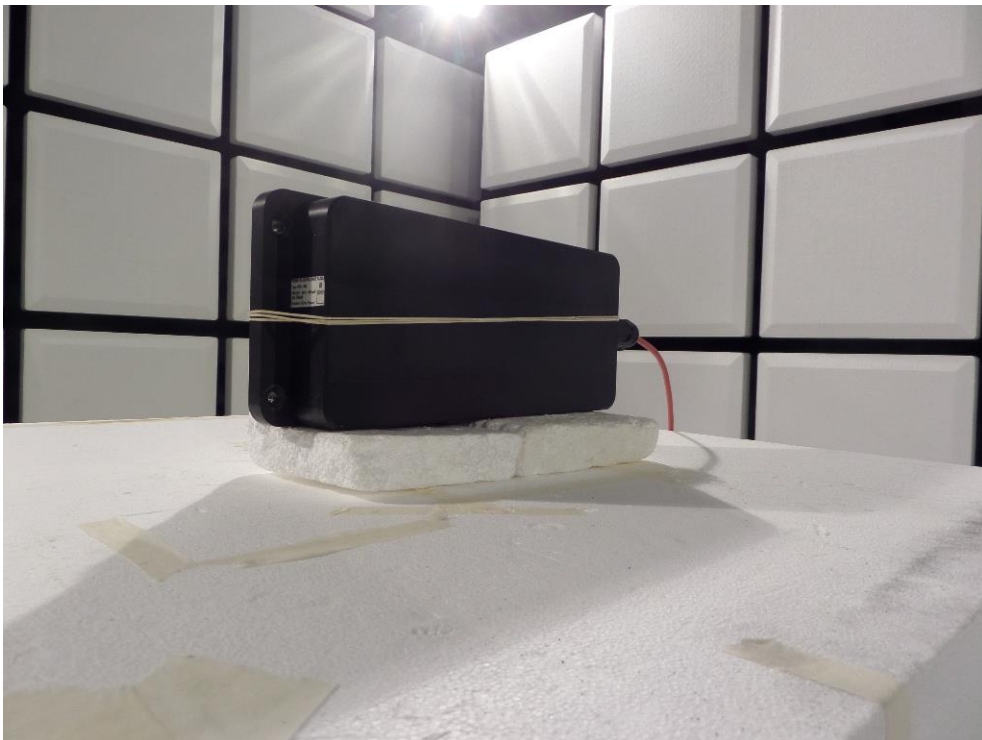

Test in anechoic room

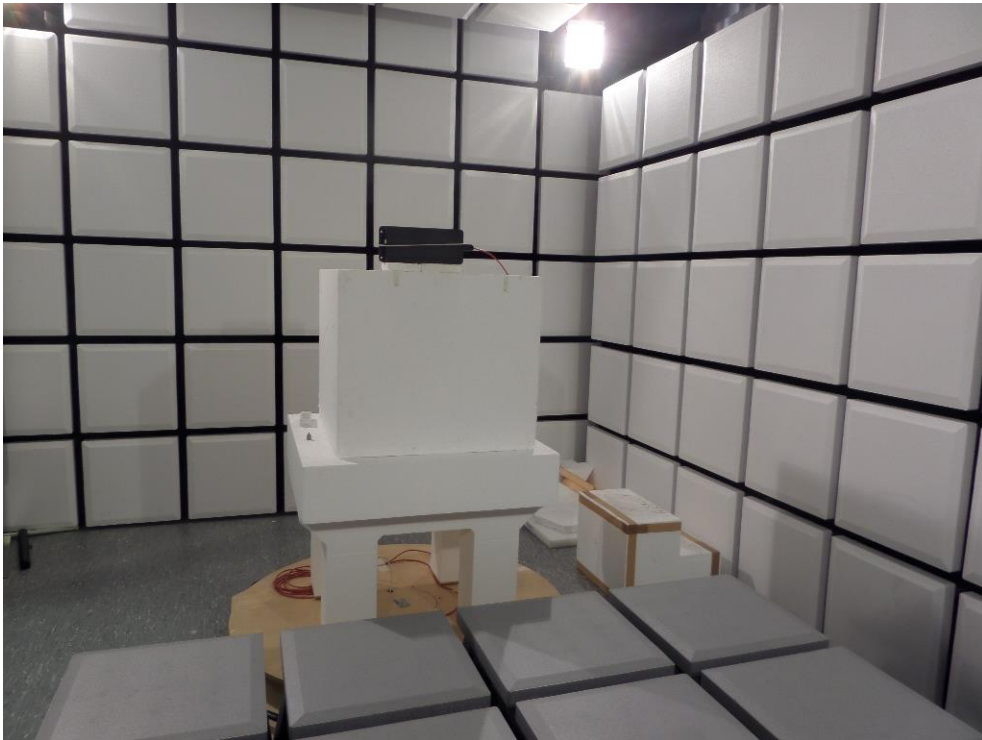

Test in Open test area



Conducted measurement

