

SAR Test Report

| Product Name | : | Bluetooth USB Adapter |
|--------------|---|-----------------------|
| Model No. | : | BT600C |
| FCC ID | : | AL8-BT600C |
| IC | : | 457A-BT600C |

Applicant : Plantronics,Inc. Address : 345 Encinal Street,Santa Cruz,CA 95060,USA

| Date of Receipt | : | Feb. 26, 2018 |
|-----------------|---|------------------------------|
| Test Date | : | Mar. 15, 2018~ Mar. 15, 2018 |
| Issued Date | : | Mar. 26, 2018 |
| Report No. | : | 1822065R-HP-US-P03V01 |
| Report Version | : | V1.0 |

The test results relate only to the samples tested.

The test results shown in the test report are traceable to the national/international standard through the calibration of the equipment and evaluated measurement uncertainty herein.

This report must not be used to claim product endorsement by TAF, A2LA any agency of the government. The test report shall not be reproduced without the written approval of DEKRA Testing and Certification (Suzhou) Co., Ltd.



Test Report Certification

Issued Date: Mar. 26, 2018 Report No: 1822065R-HP-US-P03V01



| Product Name | : Bluetooth USB Adapter |
|---------------------|---|
| Applicant | : Plantronics, Inc. |
| Address | : 345 Encinal Street, Santa Cruz, CA 95060, USA |
| Manufacturer | Plantronics, Inc. |
| Address | : 345 Encinal Street, Santa Cruz, CA 95060, USA |
| Model No. | : BT600C |
| FCC ID | : AL8-BT600C |
| IC | : 457A-BT600C |
| Brand Name | : Plantronics |
| EUT Voltage | : DC 5V |
| Applicable Standard | FCC KDB Publication 248227 D01v02r02 |
| | FCC KDB Publication 447498 D01v06 |
| | FCC KDB Publication 447498 D02v02r01 |
| | FCC KDB Publication 865664 D01v01r04 |
| | IEEE Std. 1528-2013 |
| | |
| | FCC 47CFR §2.1093 |
| | ANSI C95.1-2005 |
| | RSS - 102 Issue 5: 2015 |
| | IEC 62209-2: 2010 |
| Test Result | : Max. SAR Measurement (1g) |
| | Body: 0.332 W/kg for 100% duty cycle; 0.083 W/kg for 25% duty cycle |
| Performed Location | : DEKRA Testing and Certification (Suzhou) Co., Ltd. |
| | No.99 Hongye Rd., Suzhou Industrial Park, Suzhou,215006, |
| | Jiangsu,China |
| | TEL: +86-512-6251-5088 / FAX: +86-512-6251-5098 |
| | FCC Designation Number: CN1199 |
| | IC Lab Code: 4075B |
| | |
| | Leve Tark |
| Documented By | Kathy Feng |
| | 0 0 |
| | (Project Assistant: Kathy Feng) |
| | T L J |
| Reviewed By | ack 2 hong |
| | $\langle \rangle$ |
| | (Senior Engineer: Jack Zhang) |
| Approved By | Harry 2han |
| | |
| | (Engineering Manager: Harry Zhao) |
| | |
| | |
| | |



TABLE OF CONTENTS

| De | script | ion | Page |
|----|--------|---|------|
| 1. | GENE | RAL INFORMATION | 6 |
| | 1.1. | EUT Description | 6 |
| | 1.2. | Test Environment | 9 |
| | 1.3. | Power Reduction for SAR | 9 |
| | 1.4. | Guidance Documents | 9 |
| 2. | SAR M | IEASUREMENT SYSTEM | 10 |
| | 2.1. | DASY5 System Description | 10 |
| | 2.1.1. | Applications | 11 |
| | 2.1.2. | Area Scans | 11 |
| | 2.1.3. | Zoom Scan (Cube Scan Averaging) | 11 |
| | 2.1.4. | Uncertainty of Inter-/Extrapolation and Averaging | 11 |
| | 2.2. | DASY5 E-Field Probe | 12 |
| | 2.2.1. | Isotropic E-Field Probe Specification | 12 |
| | 2.3. | Boundary Detection Unit and Probe Mounting Device | 13 |
| | 2.4. | DATA Acquisition Electronics (DAE) and Measurement Server | 13 |
| | 2.5. | Robot | 14 |
| | 2.6. | Light Beam Unit | 14 |
| | 2.7. | Device Holder | 15 |
| | 2.8. | SAM Twin Phantom | 15 |
| 3. | TISSU | E SIMULATING LIQUID | 16 |
| | 3.1. | The composition of the tissue simulating liquid | 16 |
| | 3.2. | Tissue Calibration Result | 17 |
| | 3.3. | Tissue Dielectric Parameters for Head and Body Phantoms | 19 |
| 4. | SAR M | EASUREMENT PROCEDURE | 20 |
| | 4.1. | SAR System Validation | 20 |
| | 4.1.1. | Validation Dipoles | 20 |
| | 4.1.2. | Validation Result | 21 |
| | 4.2. | SAR Measurement Procedure | 22 |
| | 4.3. | SAR Measurement Conditions for 802.11 Device | 23 |
| | 4.3.1. | Duty Factor Control | 23 |
| | 4.3.2. | Initial Test Position SAR Test Reduction Procedure | 23 |
| 5. | SAR E | XPOSURE LIMITS | 24 |



| 6. | TEST E | EQUIPMENT LIST | 25 |
|-----|---------|---------------------------------|----|
| 7. | MEASU | JREMENT UNCERTAINTY | 26 |
| 8. | CONDU | JCTED POWER MEASUREMENT | 29 |
| 9. | TEST F | PROCEDURES | 31 |
| | 9.1. | SAR Test Results Summary | 31 |
| | 9.2. | Test position and configuration | 34 |
| APP | | A. SAR SYSTEM VALIDATION DATA | 35 |
| APP | ENDIX I | B. SAR MEASUREMENT DATA | 36 |
| APP | | C. PROBE CALIBRATION DATA | 47 |
| APP | ENDIX I | D. DIPOLE CALIBRATION DATA | 58 |
| APP | ENDIX I | E. DAE CALIBRATION DATA | 66 |



History of This Test Report

| REPORT NO. | VERSION | DESCRIPTION | ISSUED DATE |
|-----------------------|---------|-----------------------|---------------|
| 1822065R-HP-US-P03V01 | V1.0 | Initial Issued Report | Mar. 26, 2018 |
| | | | |
| | | | |
| | | | |



1. General Information

1.1. EUT Description

| | 1 | | | |
|-------------------------|--|--|--|--|
| Product Name | Bluetooth USB Adapter | | | |
| Model No. | BT600C | | | |
| Working Voltage | DC 5V | | | |
| Test Voltage | AC120V/60Hz | | | |
| Bluetooth Specification | V3.0/ V4.0 | | | |
| Frequency Range | 2402- 2480 MHz | | | |
| Channel Number | V3.0: 79 | | | |
| | V4.0: 40 | | | |
| Channel Separation | V3.0: 1MHz | | | |
| | V4.0: 2MHz | | | |
| Type of Modulation | V3.0: GFSK, Pi/4 DQPSK, 8DPSK | | | |
| Type of Modulation | V4.0: GFSK | | | |
| Data Rate | V3.0: 1Mbps(GFSK), 2Mbps(Pi/4 DQPSK), 3Mbps(8DPSK) | | | |
| | V4.0: 1Mbps(GFSK) | | | |
| Antenna Type | Reference to Antenna List | | | |
| Peak Antenna Gain | Reference to Antenna List | | | |



| Bluetooth | Bluetooth Working Frequency of Each Channel: (For V3.0) | | | | | | | |
|-----------|---|---------|-----------|---------|-----------|---------|-----------|--|
| Channel | Frequency | Channel | Frequency | Channel | Frequency | Channel | Frequency | |
| 00 | 2402 MHz | 01 | 2403 MHz | 02 | 2404 MHz | 03 | 2405 MHz | |
| 04 | 2406 MHz | 05 | 2407 MHz | 06 | 2408 MHz | 07 | 2409 MHz | |
| 08 | 2410 MHz | 09 | 2411 MHz | 10 | 2412 MHz | 11 | 2413 MHz | |
| 12 | 2414 MHz | 13 | 2415 MHz | 14 | 2416 MHz | 15 | 2417 MHz | |
| 16 | 2418 MHz | 17 | 2419 MHz | 18 | 2420 MHz | 19 | 2421 MHz | |
| 20 | 2422 MHz | 21 | 2423 MHz | 22 | 2424 MHz | 23 | 2425 MHz | |
| 24 | 2426 MHz | 25 | 2427 MHz | 26 | 2428 MHz | 27 | 2429 MHz | |
| 28 | 2430 MHz | 29 | 2431 MHz | 30 | 2432 MHz | 31 | 2433 MHz | |
| 32 | 2434 MHz | 33 | 2435 MHz | 34 | 2436 MHz | 35 | 2437 MHz | |
| 36 | 2438 MHz | 37 | 2439 MHz | 38 | 2440 MHz | 39 | 2441 MHz | |
| 40 | 2442 MHz | 41 | 2443 MHz | 42 | 2444 MHz | 43 | 2445 MHz | |
| 44 | 2446 MHz | 45 | 2447 MHz | 46 | 2448 MHz | 47 | 2449 MHz | |
| 48 | 2450 MHz | 49 | 2451 MHz | 50 | 2452 MHz | 51 | 2453 MHz | |
| 52 | 2454 MHz | 53 | 2455 MHz | 54 | 2456 MHz | 55 | 2457 MHz | |
| 56 | 2458 MHz | 57 | 2459 MHz | 58 | 2460 MHz | 59 | 2461 MHz | |
| 60 | 2462 MHz | 61 | 2463 MHz | 62 | 2464 MHz | 63 | 2465 MHz | |
| 64 | 2466 MHz | 65 | 2467 MHz | 66 | 2468 MHz | 67 | 2469 MHz | |
| 68 | 2470 MHz | 69 | 2471 MHz | 70 | 2472 MHz | 71 | 2473 MHz | |
| 72 | 2474 MHz | 73 | 2475 MHz | 74 | 2476 MHz | 75 | 2477 MHz | |
| 76 | 2478 MHz | 77 | 2479 MHz | 78 | 2480 MHz | N/A | N/A | |

| Bluetooth Working Frequency of Each Channel: (For V4.0) | | | | | | | |
|---|-----------|---------|-----------|---------|-----------|---------|-----------|
| Channel | Frequency | Channel | Frequency | Channel | Frequency | Channel | Frequency |
| 00 | 2402 MHz | 01 | 2404 MHz | 02 | 2406 MHz | 03 | 2408 MHz |
| 04 | 2410 MHz | 05 | 2412 MHz | 06 | 2414 MHz | 07 | 2416 MHz |
| 08 | 2418 MHz | 09 | 2420 MHz | 10 | 2422 MHz | 11 | 2424 MHz |
| 12 | 2426 MHz | 13 | 2428 MHz | 14 | 2430 MHz | 15 | 2432 MHz |
| 16 | 2434 MHz | 17 | 2436 MHz | 18 | 2438 MHz | 19 | 2440 MHz |
| 20 | 2442 MHz | 21 | 2444 MHz | 22 | 2446 MHz | 23 | 2448 MHz |
| 24 | 2450 MHz | 25 | 2452 MHz | 26 | 2454 MHz | 27 | 2456 MHz |
| 28 | 2458 MHz | 29 | 2460 MHz | 30 | 2462 MHz | 31 | 2464 MHz |
| 32 | 2466 MHz | 33 | 2468 MHz | 34 | 2470 MHz | 35 | 2472 MHz |
| 36 | 2474 MHz | 37 | 2476 MHz | 38 | 2478 MHz | 39 | 2480 MHz |



Antenna List

| Model No. | N/A | N/A | | | | | | |
|----------------------|-------------|-------------------------------------|-------------|----------------------------|--|--|--|--|
| Antenna manufacturer | N/A | J/A | | | | | | |
| Antenna Delivery | \boxtimes | ☐ 1*TX+1*RX ☐ 2*TX+2*RX ☐ 3*TX+3*RX | | | | | | |
| Antenna technology | \boxtimes | SISO | | | | | | |
| | | | | Basic | | | | |
| | | MIMO | | CDD | | | | |
| | | | | Beam-forming | | | | |
| | |] External 🔲 Dipole | | | | | | |
| Antenna Type | | Internal | | SMD | | | | |
| | | | | PIFA | | | | |
| | | | | РСВ | | | | |
| | | | \boxtimes | Ceramic Chip Antenna | | | | |
| | | | | Metal plate type F antenna | | | | |
| Antenna Gain | 1.54 | 1.54dBi | | | | | | |



1.2. Test Environment

Ambient conditions in the laboratory:

| Items | Required | Actual |
|------------------|----------|--------|
| Temperature (°C) | 18-25 | 21.5±2 |
| Humidity (%RH) | 30-70 | 52 |

1.3. Power Reduction for SAR

There is no power reduction used for any band/mode implemented in this device for SAR purposes.

1.4. Guidance Documents

1) FCC KDB Publication 447498 D01v06 (General SAR Guidance)

2) FCC KDB Publication 447498 D02v02r01 (SAR Measurement Procedures for USB Dongle Transmitters)

3) FCC KDB Publication 865664 D01v01r04(SAR measurement 100 MHz to 6 GHz)

4) FCC KDB Publication 248227 D01v02r02 (SAR Considerations for 802.11 Devices)

5) RSS 102 Issue5 Radio Frequency (RF) Exposure Compliance of Radiocommunication Apparatus (All Frequency Bands)

6) IEEE Std. 1528-2013 (IEEE Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques)


7) IEC 62209-2: 2010 (Human exposure to radio frequency fields from hand- held and bodymounted wireless communication devices — Human models, instrumentation, and procedures)

8) FCC 47CFR §2.1093 Radiofrequency radiation exposure evaluation: portable devices

9) ANSI C95.1-2005 - IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz

2. SAR Measurement System

2.1. DASY5 System Description

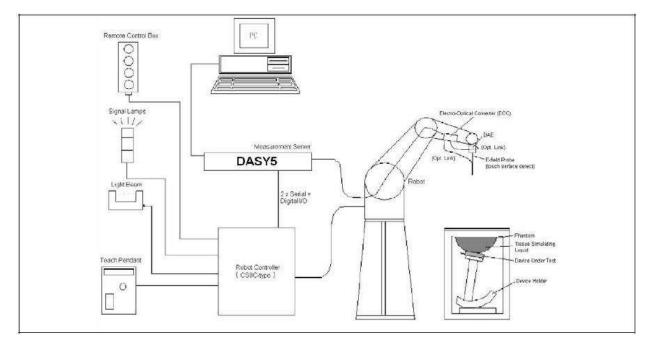

The DASY5 system for performing compliance tests consists of the following items:

- A standard high precision 6-axis robot with controller, teach pendant and software.
 An arm extension for accommodating the data acquisition electronics (DAE).
- A data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- The Electro-optical converter (EOC) performs the conversion from optical to electrical signals for the digital communication to the DAE. To use optical surface detection, a special version of the EOC is required. The EOC signal is transmitted to the measurement server.
- The Light Beam used is for probe alignment. This improves the (absolute) accuracy of the probe positioning.
- > A computer running WinXP and the DASY5 software.
- Remote control and teach pendant as well as additional circuitry for robot safety such as warning lamps, etc.
- The phantom, the device holder and other accessories according to the targeted measurement.



2.1.1. Applications

Predefined procedures and evaluations for automated compliance testing with all worldwide standards, e.g., IEEE 1528, OET 65, IEC 62209-1, IEC 62209-2, EN 50360, EN 50383 and others.

2.1.2. Area Scans

Area scans are defined prior to the measurement process being executed with a user defined variable spacing between each measurement point (integral) allowing low uncertainty measurements to be conducted. Scans defined for FCC applications utilize a 10mm² step integral, with 1mm interpolation used to locate the peak SAR area used for zoom scan assessments.

When an Area Scan has measured all reachable points, it computes the field maxima found in the scanned area, within a range of the global maximum. The range (in dB) is specified in the standards for compliance testing. For example, a 2 dB range is required in IEEE 1528-2003, EN 50361 and IEC 62209 standards, whereby 3 dB is a requirement when compliance is assessed in accordance with the ARIB standard (Japan).

2.1.3. Zoom Scan (Cube Scan Averaging)

Zoom Scans are used to assess the peak spatial SAR values within a cubic averaging volume containing 1 g and 10 g of simulated tissue. A density of 1000 kg/m³ is used to represent the head and body tissue density and not the phantom liquid density, in order to be consistent with the definition of the liquid dielectric properties, i.e. the side length of the 1 g cube is 10mm, with the side length of the 10 g cube 21,5mm.

The zoom scan integer steps can be user defined so as to reduce uncertainty, but normal practice for typical test applications utilize a physical step of 7x7x7 (5mmx5mmx5mm) providing a volume of 30mm in the X & Y axis, and 30mm in the Z axis.

2.1.4. Uncertainty of Inter-/Extrapolation and Averaging

In order to evaluate the uncertainty of the interpolation, extrapolation and averaged SAR calculation algorithms of the Postprocessor, DASY5 allows the generation of measurement grids which are artificially predefined by analytically based test functions. Therefore, the grids of area scans and zoom scans can be filled with uncertainty test data, according to the SAR benchmark functions of IEEE 1528. The three analytical functions shown in equations as below are used to describe the possible range of the expected SAR distributions for the tested handsets. The field gradients are covered by the spatially flat distribution f1, the spatially steep distribution f3 and f2 accounts for H-field cancellation on the phantom/tissue surface.



$$f_1(x, y, z) = Ae^{-\frac{z}{2a}}\cos^2\left(\frac{\pi}{2}\frac{\sqrt{x'^2 + y'^2}}{5a}\right)$$
$$f_2(x, y, z) = Ae^{-\frac{z}{a}}\frac{a^2}{a^2 + x'^2}\left(3 - e^{-\frac{2z}{a}}\right)\cos^2\left(\frac{\pi}{2}\frac{y'}{3a}\right)$$
$$f_3(x, y, z) = A\frac{a^2}{\frac{a^2}{4} + x'^2 + y'^2}\left(e^{-\frac{2z}{a}} + \frac{a^2}{2(a+2z)^2}\right)$$

2.2. DASY5 E-Field Probe

The SAR measurement is conducted with the dosimetric probe manufactured by SPEAG. The probe is specially designed and calibrated for use in liquid with high permittivity. The dosimetric probe has special calibration in liquid at different frequency.

SPEAG conducts the probe calibration in compliance with international and national standards (e.g. IEEE 1528, EN 62209-1, IEC 62209, etc.) under ISO 17025. The calibration data are in Appendix D.

| Model | EX3DV4 | | | | | | |
|---------------|---|----------------------|--|--|--|--|--|
| Construction | Symmetrical design with triangular core Built-in shielding against static charges PEEK enclosure material (resistant to organic solvents, e.g., DGBE) | | | | | | |
| Frequency | 10 MHz to 6 GHz | | | | | | |
| Directivity | Linearity: ± 0.2 dB (30 MHz to 6 GHz) ± 0.3 dB in HSL (rotation around probe axis) ± 0.5 dB in tissue material (rotation normal to probe axis) | / | | | | | |
| Dynamic Range | 10 μ W/g to 100 mW/g Linearity: ± 0.2 dB (noise: typically < 1 μ W/g) | 1 | | | | | |
| Dimensions | Overall length: 330 mm (Tip: 20 mm) Tip diameter: 2.5 mm (Body: 12 mm) Typical distance from probe tip to dipole centers: 1 mm | | | | | | |
| Application | High precision dosimetric measurements in an (e.g., very strong gradient fields). Only probe whic testing for frequencies up to 6 GHz with precision | h enables compliance | | | | | |

2.2.1. Isotropic E-Field Probe Specification



2.3. Boundary Detection Unit and Probe Mounting Device

The DASY probes use a precise connector and an additional holder for the probe, consisting of a plastic tube and a flexible silicon ring to center the probe. The connector at the DAE is flexibly mounted and held in the default position with magnets and springs. Two switching systems in the connector mount detect frontal and lateral probe collisions and trigger the necessary software response.

2.4. DATA Acquisition Electronics (DAE) and Measurement Server


The data acquisition electronics (DAE) consists of a highly sensitive electrometer-grade preamplifier with autozeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit.

Transmission to the measurement server is accomplished through an optical downlink for data and status information as well as an optical uplink for commands and the clock. The input impedance of the DAE4 is 200M Ohm; the inputs

are symmetrical and floating. Common mode rejection is above 80dB.

The DASY5 measurement server is based on a PC/104 CPU board with a 400MHz intel ULV Celeron, 128MB chipdisk and 128MB RAM. The necessary circuits for communication with the DAE electronics box, as well as the 16 bit AD converter system for optical detection and digital I/O interface are contained on the DASY5 I/O board, which is directly connected to the PC/104 bus of the CPU board.





2.5. Robot

The DASY5 system uses the high precision robots TX90 XL type out of the newer series from Stäubli SA (France). For the 6-axis controller DASY5 system, the CS8C robot controller version from Stäubli is used.

The XL robot series have many features that are important for our application:

- High precision (repeatability 0.02 mm)
- High reliability (industrial design)
- Jerk-free straight movements
- Low ELF interference (the closed metallic construction shields against motor control fields)
- ➢ 6-axis controller

2.6. Light Beam Unit

The light beam switch allows automatic "tooling" of the probe. During the process, the actual position of the probe tip with respect to the robot arm is measured, as well as the probe length and the horizontal probe offset. The software then corrects all movements, such that the robot coordinates are valid for the probe tip.

The repeatability of this process is better than 0.1 mm. If a position has been taught with an aligned probe, the same position will be reached with another aligned probe within 0.1 mm, even if the other probe has different dimensions. During probe rotations, the probe tip will keep its actual position.









2.7. Device Holder

The DASY5 device holder is designed to cope with different positions given in the standard. It has two scales for the device rotation (with respect to the body axis) and the device inclination (with respect to the line between the ear reference points). The rotation center for both scales is the ear reference point (EPR).

Thus the device needs no repositioning when changing the angles.

The DASY5 device holder has been made out of low-loss POM material having the following dielectric parameters: relative permittivity $\varepsilon r = 3$ and loss tangent $\delta = 0.02$. The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered.



2.8. SAM Twin Phantom

The SAM twin phantom is a fiberglass shell phantom with 2mm shell thickness (except the ear region where shell thickness increases to 6mm). It has three measurement areas:

- Left head
- Right head
- Flat phantom



The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections. A white cover is provided to tap the phantom during off-periods to prevent water evaporation and changes in the liquid parameters. On the phantom tip, three reference markers are provided to identify the phantom position with respect to the robot.



3. Tissue Simulating Liquid

3.1. The composition of the tissue simulating liquid

| INGREDIENT | 2450MHz |
|--------------|---------|
| (% Weight) | Body |
| Water | 73.2 |
| Salt | 0.04 |
| Sugar | 0.00 |
| HEC | 0.00 |
| Preventol | 0.00 |
| DGBE | 26.7 |
| Triton X-100 | 0.00 |



3.2. Tissue Calibration Result

The dielectric parameters of the liquids were verified prior to the SAR evaluation using DASY5 Dielectric Probe Kit and Agilent Vector Network Analyzer E5071C

| Body Tissue Simulant Measurement | | | | | | | | | | |
|----------------------------------|------------------|---------------------------|--------------|--------------|--|--|--|--|--|--|
| Frequency | Description | Dielectric Parameters Tis | | Tissue Temp. | | | | | | |
| [MHz] | Description | εr | σ [s/m] | [°C] | | | | | | |
| | Reference result | 52.7 | 1.95 | N/A | | | | | | |
| 2450 MHz | ± 5% window | 50.07 to 55.34 | 1.85 to 2.05 | IN/75 | | | | | | |
| | 03-15-2018 | 52.04 | 1.95 | 21.0 | | | | | | |
| | | | | | | | | | | |



| | Body Tissue Simulant Measurement (Test Data: 03-15-2018) | | | | | | | | | | | | |
|--------------------|--|-----------------------|-------------------|---------------------------------------|-------|-------|----------------|----------------------|--|--|--|--|--|
| | | Dielectric Parameters | | | | | | | | | | | |
| Frequency [MHz] | Channel Permittivity Condu | | Conductivity σ | Permittivity Target ε _r | , , , | | Delta (σ) % | Tissue Temp. [°C] | | | | | |
| 2402 | Low CH | 52.25 | 1.88 | 53.14 | 1.87 | -1.67 | 0.53 | 21.0 | | | | | |
| 2441 | Mid CH | 52.08 | 1.94 | 52.76 | 1.94 | -1.29 | 0.00 | 21.0 | | | | | |
| 2450 | Mid CH | 52.04 | 1.95 | 52.70 | 1.95 | -1.25 | 0.00 | 21.0 | | | | | |
| 2480 | High CH | 51.93 | 1.99 | 52.52 | 1.98 | -1.12 | 0.51 | 21.0 | | | | | |

Note:

1.The delta (ϵ_{r}) and (σ) are within ±5%, delta SAR value was not calculated in this report.

2.As per IEC 62209-2 Annex F, the SAR correction factor is given by:

 $\Delta SAR = c_{\epsilon} \Delta \varepsilon_{r} + c_{\sigma} \Delta \sigma$

For the1g average SAR $C\epsilon$ and $C\sigma$ are given by:

 $C\epsilon = -7.854 x 10^{-4} f^{3} + 9.402 x 10^{-3} f^{2} - 2.742 x 10^{-2} f - 0.2026$

 $C\sigma = 9.804 x 10^{-3} f^{3} - 8.661 x 10^{-2} f^{2} + 2.981 x 10^{-2} f + 0.7829$

Where f is the frequency in GHz.

| | Body Tissue Simulant Measurement (Test Data: 03-15-2018) | | | | | | | | | | | | |
|--------------------|--|------------------------------|--------------|-------|------|------------|------|--|--|--|--|--|--|
| Frequency | | | Tissue Temp. | | | | | | | | | | |
| Frequency [MHz] | Channel | Delta (ε _r) % | Delta (σ) % | Cε | Сσ | Delta SAR% | [°C] | | | | | | |
| 2402 | Low CH | -1.67 | 0.53 | -0.23 | 0.49 | 0.26 | 21.0 | | | | | | |
| 2441 | Mid CH | -1.29 | 0.00 | -0.22 | 0.48 | 0 | 21.0 | | | | | | |
| 2450 | Mid CH | -1.25 | 0.00 | -0.22 | 0.48 | 0 | 21.0 | | | | | | |
| 2480 | High CH | -1.12 | 0.51 | -0.22 | 0.47 | 0.24 | 21.0 | | | | | | |

Note: The Δ SAR refers to the percent change in SAR relative to the percent change in dielectric properties versus the target values. Anegative Δ SAR would translate to a lower measured SAR value than what would be measured if using dielectric properties equal to the target values. A positive Δ SAR would translate to a higher measured SAR value than what would be measured if using dielectric properties equal to the target values. SAR correction shall not be made when the Δ SAR has a positive sign to provide a conservative SAR value. The SAR is only corrected when Δ SAR has a negative sign.



3.3. Tissue Dielectric Parameters for Head and Body Phantoms

The head tissue dielectric parameters recommended by the IEEE SCC-34/SC-2 in P1528 have been incorporated in the following table. These head parameters are derived from planar layer models simulating the highest expected SAR for the dielectric properties and tissue thickness variations in a human head. Other head and body tissue parameters that have not been specified in P1528 are derived from the tissue dielectric parameters computed from the 4-Cole-Cole equations described in Reference [12] and extrapolated according to the head parameters specified in P1528.

| Target Frequency | He | ad | Body | | |
|------------------|------|---------|------|---------|--|
| (MHz) | ٤r | σ (S/m) | ٤r | σ (S/m) | |
| 150 | 52.3 | 0.76 | 61.9 | 0.80 | |
| 300 | 45.3 | 0.87 | 58.2 | 0.92 | |
| 450 | 43.5 | 0.87 | 56.7 | 0.94 | |
| 835 | 41.5 | 0.90 | 55.2 | 0.97 | |
| 900 | 41.5 | 0.97 | 55.0 | 1.05 | |
| 915 | 41.5 | 0.98 | 55.0 | 1.06 | |
| 1450 | 40.5 | 1.20 | 54.0 | 1.30 | |
| 1610 | 40.3 | 1.29 | 53.8 | 1.40 | |
| 1800 – 2000 | 40.0 | 1.40 | 53.3 | 1.52 | |
| 2450 | 39.2 | 1.80 | 52.7 | 1.95 | |
| 3000 | 38.5 | 2.40 | 52.0 | 2.73 | |
| 5800 | 35.3 | 5.27 | 48.2 | 6.00 | |


(ε_r = relative permittivity, σ = conductivity and ρ = 1000 kg/m³)



4. SAR Measurement Procedure

4.1. SAR System Validation

4.1.1. Validation Dipoles



The dipoles used is based on the IEEE-1528 standard, and is complied with mechanical and electrical specifications in line with the requirements of both IEEE and FCC Supplement C. the table below provides details for the mechanical and electrical specifications for the dipoles.

| Frequency | L (mm) | h (mm) | d (mm) |
|-----------|--------|--------|--------|
| 2450MHz | 53.5 | 30.4 | 3.6 |



4.1.2. Validation Result

| System Performance Check at 2450MHz Validation Dipole: D2450V2, SN: 839 Body | | | | | | | | | | |
|---|--|------------------------|------------------------|----------------------|--|--|--|--|--|--|
| Frequency [MHz] | Description | SAR [w/kg] 1g | SAR [w/kg] 10g | Tissue Temp. [°C] | | | | | | |
| 2450 MHz | Reference result ± 10% window | 49.8 44.82 to 54.78 | 23.3 20.97 to 25.63 | N/A | | | | | | |
| | 03-15-2018 | 50.0 | 22.76 | 21.0 | | | | | | |
| Note: All SAR | Note: All SAR values are normalized to 1W forward power. | | | | | | | | | |



4.2. SAR Measurement Procedure

The DASY 5 calculates SAR using the following equation,

$$SAR = \frac{\sigma |\mathbf{E}|^2}{\rho}$$

 σ : represents the simulated tissue conductivity

 $\boldsymbol{\rho}:$ represents the tissue density

The EUT is set to transmit at the required power in line with product specification, at each frequency relating to the LOW, MID, and HIGH channel settings.

Pre-scans are made on the device to establish the location for the transmitting antenna, using a large area scan in either air or tissue simulation fluid.

The EUT is placed against the Universal Phantom where the maximum area scan dimensions are larger than the physical size of the resonating antenna. When the scan size is not large enough to cover the peak SAR distribution, it is modified by either extending the area scan size in both the X and Y directions, or the device is shifted within the predefined area.

The area scan is then run to establish the peak SAR location (interpolated resolution set at 1mm²) which is then used to orient the center of the zoom scan. The zoom scan is then executed and the 1g and 10g averages are derived from the zoom scan volume (interpolated resolution set at 1mm³).



4.3. SAR Measurement Conditions for 802.11 Device

4.3.1. Duty Factor Control

Unless it is permitted by specific KDB procedures or continuous transmission is specifically restricted by the device, the reported SAR must be scaled to 100% transmission duty factor to determine compliance at the maximum tune-up tolerance limit.

4.3.2. Initial Test Position SAR Test Reduction Procedure

DSSS and OFDM configurations are considered separately according to the required SAR procedures. SAR is measured in the initial test position using the 802.11 transmission mode configuration required by the DSSS procedure or initial test configuration and subsequent test configuration(s) according to the OFDM procedures.16 The initial test position procedure is described in the following:

When the reported SAR of the initial test position is ≤ 0.4 W/kg, further SAR measurement is not required for the other (remaining) test positions in that exposure configuration and 802.11 transmission mode combinations within the frequency band or aggregated band. SAR is also not required for that exposure configuration in the subsequent test configuration(s).

a) When the reported SAR of the initial test position is > 0.4 W/kg, SAR is repeated for the 802.11 transmission mode configuration tested in the initial test position using subsequent highest extrapolated or estimated 1-g SAR conditions determined by area scans or next closest/smallest test separation distance and maximum RF coupling test positions based on manufacturer justification, on the highest maximum output power channel, until the reported SAR is \leq 0.8 W/kg or all required test positions (left, right, touch, tilt or subsequent surfaces and edges) are tested.

b) For all positions/configurations tested using the initial test position and subsequent test positions, when the reported SAR is > 0.8 W/kg, SAR is measured for these test positions/configurations on the subsequent next highest measured output power channel(s) until the reported SAR is \leq 1.2 W/kg or all required channels are tested.

Additional power measurements may be required for this step, which should be limited to those necessary for identifying the subsequent highest output power channels.



5. SAR Exposure Limits

SAR assessments have been made in line with the requirements of IEEE-1528, FCC Supplement C, and comply with ANSI/IEEE C95.1-1992 "Uncontrolled Environments" limits. These limits apply to a location which is deemed as "Uncontrolled Environment" which can be described as a situation where the general public may be exposed to an RF source with no prior knowledge or control over their exposure.

| Type Exposure | Uncontrolled |
|--|-------------------|
| | Environment Limit |
| Spatial Peak SAR (1g cube tissue for brain or body) | 1.60 W/kg |
| Spatial Average SAR (whole body) | 0.08 W/kg |
| Spatial Peak SAR (10g for hands, feet, ankles and wrist) | 4.00 W/kg |

Limits for General Population/Uncontrolled Exposure (W/kg)



6. Test Equipment List

| Instrument | Manufacturer | Model No. | Serial No. | Cali. Due Date |
|------------------------|--------------|---------------|-----------------|----------------|
| Stäubli Robot TX60L | Stäubli | TX60L | F10/5C90A1/A/01 | N/A |
| Controller | Stäubli | SP1 | S-0034 | N/A |
| Dipole Validation Kits | Speag | D2450V2 | 839 | 2019.02.08 |
| SAM Twin Phantom | Speag | SAM | TP-1561/1562 | N/A |
| Device Holder | Speag | SD 000 H01 HA | N/A | N/A |
| Data | Speag | DAE4 | 905 | 2018.06.19 |
| Acquisition Electronic | | | | |
| E-Field Probe | Speag | EX3DV4 | 3661 | 2018.05.04 |
| SAR Software | Speag | DASY5 | V5.2 Build 162 | N/A |
| Power Amplifier | Mini-Circuit | ZVA-183-S+ | N657400950 | N/A |
| Directional Coupler | Agilent | 778D | 20160 | N/A |
| Universal Radio | R&S | CMU 200 | 117088 | 2019.03.10 |
| Communication Tester | | | | |
| Vector Network | Agilent | E5071C | MY48367267 | 2019.03.10 |
| Signal Generator | Agilent | E4438C | MY49070163 | 2019.03.10 |
| Power Meter | Anritsu | ML2495A | 0905006 | 2018.10.14 |
| Wide Bandwidth Sensor | Anritsu | MA2411B | 0846014 | 2018.10.14 |



7. Measurement Uncertainty

| DASY5 | Uncerta | ainty ac | cordin | g to IEI | EE std. | 1528-201 | 13 | |
|-------------------------|-----------|-----------|------------|----------|----------|------------|--------|------|
| Measurement uncertainty | for 300 M | Hz to 3 G | Hz aver | aged ove | r 1 gram | / 10 gram. | | |
| Error Description | Uncert. | Prob. | Div. | (Ci) | (Ci) | Std. | Std. | (Vi) |
| | value | Dist. | | 1g | 10g | Unc. | Unc. | Veff |
| | | | | | | (1g) | (10g) | |
| Measurement System | | | | | | | | |
| Probe Calibration | ±6.0% | Ν | 1 | 1 | 1 | ±6.0% | ±6.0% | 8 |
| Axial Isotropy | ±4.7% | R | $\sqrt{3}$ | 0.7 | 0.7 | ±1.9% | ±1.9% | 8 |
| Hemispherical Isotropy | ±9.6% | R | $\sqrt{3}$ | 0.7 | 0.7 | ±3.9% | ±3.9% | ∞ |
| Boundary Effects | ±1.0% | R | $\sqrt{3}$ | 1 | 1 | ±0.6% | ±0.6% | ∞ |
| Linearity | ±4.7% | R | $\sqrt{3}$ | 1 | 1 | ±2.7% | ±2.7% | ∞ |
| System Detection Limits | ±1.0% | R | $\sqrt{3}$ | 1 | 1 | ±0.6% | ±0.6% | ∞ |
| Readout Electronics | ±0.3% | N | 1 | 1 | 1 | ±0.3% | ±0.3% | ∞ |
| Response Time | ±0.8% | R | $\sqrt{3}$ | 1 | 1 | ±0.5% | ±0.5% | ∞ |
| Integration Time | ±2.6% | R | $\sqrt{3}$ | 1 | 1 | ±1.5% | ±1.5% | ∞ |
| RF Ambient Noise | ±3.0% | R | $\sqrt{3}$ | 1 | 1 | ±1.7% | ±1.7% | ∞ |
| RF Ambient Reflections | ±3.0% | R | $\sqrt{3}$ | 1 | 1 | ±1.7% | ±1.7% | ∞ |
| Probe Positioner | ±0.4% | R | $\sqrt{3}$ | 1 | 1 | ±0.2% | ±0.2% | ∞ |
| Probe Positioning | ±2.9% | R | $\sqrt{3}$ | 1 | 1 | ±1.7% | ±1.7% | ∞ |
| Max. SAR Eval. | ±1.0% | R | $\sqrt{3}$ | 1 | 1 | ±0.6% | ±0.6% | ∞ |
| Test Sample Related | | 1 | 1 | | | 1 | | 1 |
| Device Positioning | ±2.9% | N | 1 | 1 | 1 | ±2.9% | ±2.9% | 145 |
| Device Holder | ±3.6% | N | 1 | 1 | 1 | ±3.6% | ±3.6% | 5 |
| Power Drift | ±5.0% | R | $\sqrt{3}$ | 1 | 1 | ±2.9% | ±2.9% | ∞ |
| Phantom and Setup | | 1 | 1 | | | 1 | | 1 |
| Phantom Uncertainty | ±4.0% | R | $\sqrt{3}$ | 1 | 1 | ±2.3% | ±2.3% | ∞ |
| Liquid Conductivity | . 5.00/ | | 12 | 0.04 | 0.40 | .4.00/ | .4.00/ | |
| (target) | ±5.0% | R | $\sqrt{3}$ | 0.64 | 0.43 | ±1.8% | ±1.2% | ∞ |
| Liquid Conductivity | ±2.5% | N | 1 | 0.64 | 0.43 | ±1.6% | ±1.1% | ∞ |
| (meas.) | ±2.576 | IN | 1 | 0.04 | 0.43 | ±1.070 | ±1.170 | ~ |
| Liquid Permittivity | ±5.0% | R | √3 | 0.6 | 0.49 | ±1.7% | ±1.4% | ∞ |
| (target) | 10.0 /0 | | .4.2 | 0.0 | 0.49 | ±1.7 /0 | ±1.470 | |
| Liquid Permittivity | ±2.5% | N | 1 | 0.6 | 0.49 | ±1.5% | ±1.2% | ∞ |
| (meas.) | ±2.070 | | | 0.0 | 0.43 | ±1.070 | ±1.270 | |
| Combined Std. Uncertai | inty | | | | | ±11.0% | ±10.8% | 387 |
| Expanded STD Uncertai | inty | | | | | ±22.0% | ±21.5% | |



| DASY5 | Uncerta | inty ac | cording | g to IEE | E std. | 1528-201 | 3 | |
|-------------------------|-----------|----------|------------|-----------|-----------|----------|---------|------|
| Measurement uncertainty | for 3 GHz | to 6 GHz | z average | ed over 1 | gram / 10 |) gram. | | |
| Error Description | Uncert. | Prob. | Div. | (Ci) | (Ci) | Std. | Std. | (Vi) |
| | value | Dist. | | 1g | 10g | Unc. | Unc. | Veff |
| | | | | | | (1g) | (10g) | |
| Measurement System | | | | | | | | |
| Probe Calibration | ±6.55% | Ν | 1 | 1 | 1 | ±6.55% | ±6.55% | 8 |
| Axial Isotropy | ±4.7% | R | √3 | 0.7 | 0.7 | ±1.9% | ±1.9% | 8 |
| Hemispherical Isotropy | ±9.6% | R | √3 | 0.7 | 0.7 | ±3.9% | ±3.9% | 8 |
| Boundary Effects | ±2.0% | R | $\sqrt{3}$ | 1 | 1 | ±1.2% | ±1.2% | ∞ |
| Linearity | ±4.7% | R | $\sqrt{3}$ | 1 | 1 | ±2.7% | ±2.7% | ∞ |
| System Detection Limits | ±1.0% | R | $\sqrt{3}$ | 1 | 1 | ±0.6% | ±0.6% | ∞ |
| Readout Electronics | ±0.3% | Ν | 1 | 1 | 1 | ±0.3% | ±0.3% | ∞ |
| Response Time | ±0.8% | R | $\sqrt{3}$ | 1 | 1 | ±0.5% | ±0.5% | ∞ |
| Integration Time | ±2.6% | R | $\sqrt{3}$ | 1 | 1 | ±1.5% | ±1.5% | ∞ |
| RF Ambient Noise | ±3.0% | R | $\sqrt{3}$ | 1 | 1 | ±1.7% | ±1.7% | ∞ |
| RF Ambient Reflections | ±3.0% | R | $\sqrt{3}$ | 1 | 1 | ±1.7% | ±1.7% | ∞ |
| Probe Positioner | ±0.8% | R | $\sqrt{3}$ | 1 | 1 | ±0.5% | ±0.5% | ∞ |
| Probe Positioning | ±9.9% | R | $\sqrt{3}$ | 1 | 1 | ±5.7% | ±5.7% | ∞ |
| Max. SAR Eval. | ±4.0% | R | $\sqrt{3}$ | 1 | 1 | ±2.3% | ±2.3% | ∞ |
| Test Sample Related | | | | | | | | |
| Device Positioning | ±2.9% | Ν | 1 | 1 | 1 | ±2.9% | ±2.9% | 145 |
| Device Holder | ±3.6% | N | 1 | 1 | 1 | ±3.6% | ±3.6% | 5 |
| Power Drift | ±5.0% | R | $\sqrt{3}$ | 1 | 1 | ±2.9% | ±2.9% | ∞ |
| Phantom and Setup | | • | • | | | | | • |
| Phantom Uncertainty | ±4.0% | R | $\sqrt{3}$ | 1 | 1 | ±2.3% | ±2.3% | ∞ |
| Liquid Conductivity | . 5.00/ | D | 12 | 0.04 | 0.42 | .4.00/ | .1.00/ | |
| (target) | ±5.0% | R | $\sqrt{3}$ | 0.64 | 0.43 | ±1.8% | ±1.2% | ∞ |
| Liquid Conductivity | ±2.5% | N | 1 | 0.64 | 0.43 | ±1.6% | ±1.1% | ∞ |
| (meas.) | ±2.3% | IN | 1 | 0.04 | 0.43 | ±1.0% | ±1.1% | ~ |
| Liquid Permittivity | ±5.0% | R | $\sqrt{3}$ | 0.6 | 0.49 | ±1.7% | ±1.4% | ∞ |
| (target) | ±3.0 /⁄0 | | γ3 | 0.0 | 0.49 | ±1.7 /0 | ±1.4 /0 | |
| Liquid Permittivity | ±2.5% | N | 1 | 0.6 | 0.49 | ±1.5% | ±1.2% | 8 |
| (meas.) | 12.070 | | | 0.0 | 0.73 | 1.070 | 1.270 | |
| Combined Std. Uncertai | nty | | | | | ±12.8% | ±12.6% | 330 |
| Expanded STD Uncertai | nty | | | | | ±25.6% | ±25.2% | |



| DASY5 | Uncertair | nty acco | ording | to IEC 6 | 62209-2 | /2010 | | |
|--------------------------------|--------------|----------|------------|----------|----------|--------|--------|------|
| Measurement uncertainty for 30 |) MHz to 6 G | Hz avera | ged over | 1 gram / | 10 gram. | | | |
| Error Description | Uncert. | Prob. | Div. | (Ci) | (Ci) | Std. | Std. | (Vi) |
| | Value | Dist. | | 1g | 10g | Unc. | Unc. | Veff |
| | | | | | | (1g) | (10g) | |
| Measurement System | | | | | | | | |
| Probe Calibration | ±6.5% | Ν | 1 | 1 | 1 | ±6.5% | ±6.5% | 8 |
| Axial Isotropy | ±4.7% | R | $\sqrt{3}$ | 0.7 | 0.7 | ±1.9% | ±1.9% | 8 |
| Hemispherical Isotropy | ±9.6% | R | $\sqrt{3}$ | 0.7 | 0.7 | ±3.9% | ±3.9% | ∞ |
| Boundary Effects | ±2.0% | R | $\sqrt{3}$ | 1 | 1 | ±1.2% | ±1.2% | ∞ |
| Linearity | ±4.7% | R | $\sqrt{3}$ | 1 | 1 | ±2.7% | ±2.7% | ∞ |
| Modulation Response | ±2.4% | R | $\sqrt{3}$ | 1 | 1 | ±1.4% | ±1.4% | ∞ |
| System Detection Limits | ±1.0% | R | √3 | 1 | 1 | ±0.6% | ±0.6% | ∞ |
| Readout Electronics | ±0.3% | Ν | 1 | 1 | 1 | ±0.3% | ±0.3% | ∞ |
| Response Time | ±0.8% | R | $\sqrt{3}$ | 1 | 1 | ±0.5% | ±0.5% | ∞ |
| Integration Time | ±2.6% | R | $\sqrt{3}$ | 1 | 1 | ±1.5% | ±1.5% | ∞ |
| RF Ambient Noise | ±3.0% | R | $\sqrt{3}$ | 1 | 1 | ±1.7% | ±1.7% | ∞ |
| RF Ambient Reflections | ±3.0% | R | $\sqrt{3}$ | 1 | 1 | ±1.7% | ±1.7% | ∞ |
| Probe Positioner | ±0.8% | R | $\sqrt{3}$ | 1 | 1 | ±0.5% | ±0.5% | ∞ |
| Probe Positioning | ±6.7% | R | $\sqrt{3}$ | 1 | 1 | ±3.9% | ±3.9% | ∞ |
| Post-processing | ±4.0% | R | $\sqrt{3}$ | 1 | 1 | ±2.3% | ±2.3% | ∞ |
| Test Sample Related | | | | • | | • | | • |
| Test Sample Positioning | ±2.9% | Ν | 1 | 1 | 1 | ±2.9% | ±2.9% | 145 |
| Device Holder | ±3.6% | Ν | 1 | 1 | 1 | ±3.6% | ±3.6% | 5 |
| Power Drift | ±0.0% | R | $\sqrt{3}$ | 1 | 1 | ±0.0% | ±0.0% | ∞ |
| Power Scaling | ±5.0% | R | $\sqrt{3}$ | 1 | 1 | ±2.9% | ±2.9% | ∞ |
| Phantom and Setup | | | · | | | | | |
| Phantom Uncertainty | ±7.9% | R | $\sqrt{3}$ | 1 | 1 | ±4.6% | ±4.6% | ∞ |
| SAR correction | ±1.9% | R | $\sqrt{3}$ | 1 | 1 | ±1.1% | ±0.9% | ∞ |
| Liquid Conductivity (meas.) | ±2.5% | Ν | 1 | 0.78 | 0.71 | ±2.0% | ±1.8% | ∞ |
| Liquid Permittivity (meas.) | ±2.5% | Ν | 1 | 0.26 | 0.26 | ±0.6% | ±0.7% | ∞ |
| Temp. unc Conductivity | ±5.2% | R | $\sqrt{3}$ | 0.78 | 0.71 | ±2.3% | ±2.1% | ∞ |
| Temp. unc Permittivity | ±0.8% | R | $\sqrt{3}$ | 0.23 | 0.26 | ±0.1% | ±0.1% | ∞ |
| Combined Std. Uncertainty | | | | | | ±12.8% | ±12.7% | 748 |
| Expanded STD Uncertainty | | | | | | ±25.6% | ±25.4% | |



8. Conducted Power Measurement

For BT 3.0

| Test Mode | Frequency (MHz) | Avg. Burst Power (dBm) | Max. Power (dBm) | Scaling Factor |
|--------------------------|--------------------|---------------------------|---------------------|-------------------|
| | 2402 | 8.25 | 8.5 | 1.059 |
| 1Mbps(GFSK_DH5) | 2441 | 8.07 | 8.5 | 1.104 |
| | 2480 | 7.94 | 8.5 | 1.138 |
| | 2402 | 8.05 | 8.5 | 1.109 |
| 2Mbps(Pi/4 DQPSK_DH5) | 2441 | 8.19 | 8.5 | 1.074 |
| | 2480 | 7.83 | 8.5 | 1.167 |
| | 2402 | 8.13 | 8.5 | 1.089 |
| 3Mbps(8DPSK_DH5) | 2441 | 8.21 | 8.5 | 1.069 |
| | 2480 | 7.82 | 8.5 | 1.169 |

For BT 4.0

| Test Mode | Frequency (MHz) | Avg. Burst Power (dBm) | Max. Power (dBm) | Scaling Factor |
|--------------|--------------------|---------------------------|---------------------|-------------------|
| | 2402 | 3.49 | 4.0 | 1.125 |
| 1Mbps(GFSK) | 2440 | 5.49 | 6.0 | 1.125 |
| | 2480 | 5.61 | 6.0 | 1.094 |



Duty cycle:

| Test Mode | Duty Cycle(%) |
|-----------|---------------|
| DH5 | 77.2 |
| 2DH5 | 77.4 |
| 3DH5 | 77.4 |
| BT4.0 | 63.5 |

Note1: All the conducted power had already scaled to 100% duty cycle.

2: The maximum duty cycle which transmit by the RF tool is showed above, so each modes of the SAR was needed scaled to 100% duty cycle.



9. Test Procedures

9.1. SAR Test Results Summary

| SAR ME | ASUREM | IENT | | | | | | | | | |
|--|-------------------------|------------------------|---------------------------------|--|---------------------------|-------------------------|-----------------------|--------------------|----------------------------------|---------------------|--|
| Ambient Temperature (°C) : 21.5 ± 2 | | | | | Relative Humidity (%): 52 | | | | | | |
| Liquid Temperature (°C) : 21.0 ± 2 | | | | | Depth | of Liqui | d (cm):>′ | 15 | | | |
| Product: E | Bluetooth | USB Adapte | er | | | | | | | | |
| Frequency | /: 2402 ~ 2 | 2480 MHz | | | | | | | | | |
| Test Mode: DH5 | | | | | | | | | | | |
| Test Position Body (0mm gap) | Antenn a Position | Frequenc y (MHz) | Conducte d Power (dBm) | | Power Drift <±0.2) | SAR 1g (W/kg) | Scalin g Factor | Duty Facto r | Reporte d SAR 1g (W/kg) | Limit (W/kg) | |
| Horizonta I Up | Fixed | 2441 | 8.07 | | 0.03 | 0.097 | 1.104 | 1.295 | 0.139 | 1.6 | |
| Horizonta I Down | Fixed | 2441 | 8.07 | | 0.03 | 0.179 | 1.104 | 1.295 | 0.256 | 1.6 | |
| Vertical Front | Fixed | 2441 | 8.07 | | 0.19 | 0.126 | 1.104 | 1.295 | 0.180 | 1.6 | |
| Vertical Back | Fixed | 2441 | 8.07 | | -0.12 | 0.021 | 1.104 | 1.295 | 0.030 | 1.6 | |
| Tip | Fixed | 2441 | 8.07 | | 0.01 | 0.048 | 1.104 | 1.295 | 0.069 | 1.6 | |
| Horizonta I Down | Fixed | 2402 | 8.25 | | 0.18 | 0.225 | 1.138 | 1.295 | 0.332 | 1.6 | |
| Horizonta I Down | Fixed | 2480 | 7.94 | | 0.09 | 0.129 | 1.059 | 1.295 | 0.177 | 1.6 | |
| Test Mode: 2DH5 | | | | | | | | | | | |
| Horizonta I Down | Fixed | 2441 | 8.19 | | 0.19 | 0.140 | 1.074 | 1.292 | 0.194 | 1.6 | |
| Test Mode: 3DH5 | | | | | | | | | | | |
| Horizonta I Down | Fixed | 2441 | 8.21 | | 0.01 | 0.139 | 1.069 | 1.292 | 0.192 | 1.6 | |
| Test Mode: BLE | | | | | | | | | | | |
| Horizonta I Down | Fixed | 2480 | 5.61 | | 0.14 | 0.068 | 1.094 | 1.575 | 0.117 | 1.6 | |

Г



| SAR MEASUF | REMENT | | | | | | | | |
|---------------------------------------|---------------------|---------------------------|-----------------------------|---------------------------|-----|-------------------------|-----------------|--|--|
| Ambient Tempe | rature (°C | Relative Humidity (%): 52 | | | | | | | |
| Liquid Tempera | ture (°C) : | Depth of | Liquid (cm):>1 | 5 | | | | | |
| Product: Blueto | oth USB A | dapter | | | | | | | |
| Frequency: 240 | 2 ~ 2480 I | MHz | | | | | | | |
| Test Mode: DH5 | | | | | | | | | |
| Test Position Body (0mm gap) | Antenna Position | Frequency (MHz) | Conducted Power (dBm) | Reported SAR 1g (W/kg) | | Scaled SAR (25% d/c) | Limit (W/kg) | | |
| Horizontal Up | Fixed | 2441 | 8.07 | 0.1 | 39 | 0.035 | | | |
| Horizontal Down | Fixed | 2441 | 8.07 | 0.256 | | 0.256 0.064 | | | |
| Vertical Front | Fixed | 2441 | 8.07 | 0.1 | 80 | 0.045 | 1.6 | | |
| Vertical Back | Fixed | 2441 | 8.07 0.03 | |)30 | 0.008 | 1.6 | | |
| Тір | Fixed | 2441 | 8.07 | 8.07 0.00 | | 0.017 | 1.6 | | |
| Horizontal Down | Fixed | 2402 | 8.25 | 0.332 | | 0.083 | 1.6 | | |
| Horizontal Down | Fixed | 2480 | 7.94 | 0.177 | | 0.044 | 1.6 | | |
| Test Mode: 2DH5 | 5 | | | | | | | | |
| Horizontal Down | Fixed | 2441 | 8.19 | 0.194 | | 4 0.049 | | | |
| Test Mode: 3DH5 | | | | | | | | | |
| Horizontal Down | Fixed | 2441 | 8.21 | 0.192 | | 0.048 | 1.6 | | |
| Test Mode: BLE | | | | | | | | | |
| Horizontal Down | Fixed | 2480 | 5.61 | 0.117 | | 0.117 0.029 | | | |

Note 1: * - Repeated at the highest measured SAR according to the FCC KDB 865664

2: When the reported SAR of the initial test position is > 0.4 W/kg, on the highest maximum output power channel, until the reported SAR is \leq 0.8 W/kg or all required test positions (Front, Horizontal Down and edges) are tested.

3: For all positions/configurations tested using the initial test position and subsequent test positions, when the reported SAR is > 0.8 W/kg, SAR is measured for these test positions/configurations on the subsequent next highest measured output power channel(s) until the reported SAR is \leq 1.2 W/kg or



all required channels are tested.

4: The justification for SAR scaling to 25% factor shown in the above data table is based on the following rationale provided by Plantronics: The "most transmitter on percentage" steady-state transmitside RF mode that a headset that we ship these days would be modulating in GFSK (the least efficient) SCO, and for steady-state operation (ignoring transient states) HV1, that being a 64kbit/sec net transmit data-stream. The duty cycle would be: 240 bits payload (no payload header is present) 68 bits shortened access code (since no payload header follows) 4 bits ramping margin which, at 1.0uS/bit GFSK, is then 312uS with the transmitter on sent every 1250uS, or a duty cycle of 25%.



9.2. Test position and configuration

1. Liquid tissue depth was at least 15.0 cm for all frequencies.

2. The manufacturer has confirmed that the device(s) tested have the same physical, mechanical and thermal characteristics and are within operational tolerances expected for production units.

3. SAR results were scaled to the maximum allowed power to demonstrate compliance per FCC KDB Publication 447498 D01v06.

4. SAR were performed with Horizontal Up, Horizontal Down, Vertical Front, Vertical Back, Tip according to KDB 447498 D02v02r01.



Appendix A. SAR System Validation Data

Date/Time: 03/15/2018

Test Laboratory: DEKRA Lab System Check body 2450MHz **DUT: Dipole 2450 MHz D2450V2; Type: D2450V2** Communication System: UID 0, CW; Communication System Band: D2450(2450MHz); Duty Cycle: 1:1; Frequency: 2450 MHz; Medium parameters used: f = 2450 MHz; σ = 1.95 S/m; ϵ r = 52.04; ρ = 1000 kg/m3; Phantom section: Flat Section ; Input Power=250mW Ambient temperature (°C): 21.5, Liquid temperature (°C): 21.0 DASY5 Configuration:

- Probe: EX3DV4 SN3661; ConvF(7.54, 7.54, 7.54); Calibrated: 05/05/2017;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn905; Calibrated: 20/06/2017
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Configuration/System Check Body 2450MHz/Area Scan (7x11x1): Measurement grid: dx=10mm,


dy=10mm;Maximum value of SAR (measured) = 12.8 W/kg

Configuration/System Check Body 2450MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm,

dy=5mm, dz=5mm;Reference Value = 81.40 V/m; Power Drift = 0.18 dB

Peak SAR (extrapolated) = 25.3 W/kg

SAR(1 g) = 12.5 W/kg; SAR(10 g) = 5.69 W/kg; Maximum value of SAR (measured) = 14.4 W/kg

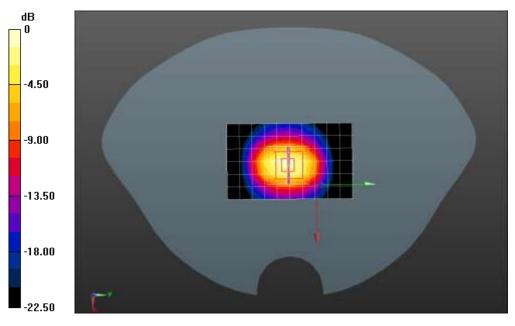

0 dB = 14.4 W/kg = 11.58 dBW/kg



Appendix B. SAR measurement Data

Date/Time: 03/15/2018

Test Laboratory: DEKRA Lab Bluetooth 2441MHz Body DH5 Horizontal Up **DUT: Bluetooth USB Adapter; Type: BT600C** Communication System: UID 0, Bluetooth (0); Communication System Band: ISM Band; Duty Cycle: 1:1.0; Frequency: 2441 MHz; Medium parameters used: f = 2441 MHz; σ = 1.94 S/m; ϵ r = 52.08; ρ = 1000 kg/m3 ; Phantom section: Flat Section Ambient temperature (°C): 21.5, Liquid temperature (°C): 21.0 DASY5 Configuration:

- Probe: EX3DV4 SN3661; ConvF(7.54, 7.54, 7.54); Calibrated: 05/05/2017;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn905; Calibrated: 20/06/2017
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)


Configuration/Bluetooth 2441MHz DH5 Body Horizontal Up/Area Scan (7x7x1): Measurement grid:

dx=12mm, dy=12mm;Maximum value of SAR (measured) = 0.111 W/kg

Configuration/Bluetooth 2441MHz DH5 Body Horizontal Up/Zoom Scan (5x5x7)/Cube

0: Measurement grid: dx=8mm, dy=8mm, dz=5mm;Reference Value = 3.088 V/m; Power Drift = 0.03 dB Peak SAR (extrapolated) = 0.281 W/kg

SAR(1 g) = 0.097 W/kg; SAR(10 g) = 0.041 W/kg

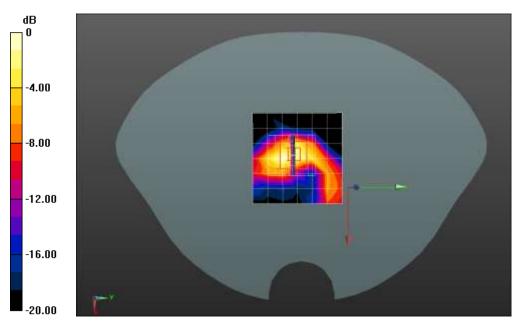

0 dB = 0.111 W/kg = -9.55 dBW/kg



Test Laboratory: DEKRA Lab

Bluetooth 2441MHz Body DH5 Horizontal Down

DUT: Bluetooth USB Adapter; Type: BT600C

Communication System: UID 0, Bluetooth (0); Communication System Band: ISM Band; Duty Cycle: 1:1.0; Frequency: 2441 MHz; Medium parameters used: f = 2441 MHz; $\sigma = 1.94$ S/m; $\epsilon r = 52.08; \rho = 1000$ kg/m3; Phantom section: Flat Section

Ambient temperature (°C): 21.5, Liquid temperature (°C): 21.0 DASY5 Configuration:


- Probe: EX3DV4 SN3661; ConvF(7.54, 7.54, 7.54); Calibrated: 05/05/2017;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn905; Calibrated: 20/06/2017
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)


Configuration/Bluetooth 2441MHz DH5 Body Horizontal Down/Area Scan (7x7x1): Measurement grid:

dx=12mm, dy=12mm;Maximum value of SAR (measured) = 0.139 W/kg

Configuration/Bluetooth 2441MHz DH5 Body Horizontal Down/Zoom Scan (5x5x7)/Cube

0: Measurement grid: dx=8mm, dy=8mm, dz=5mm;Reference Value = 2.069 V/m; Power Drift = 0.03 dB Peak SAR (extrapolated) = 0.552 W/kg



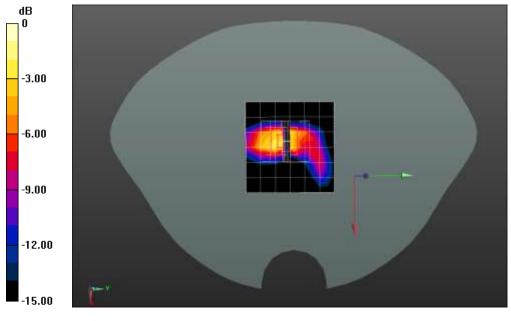

0 dB = 0.218 W/kg = -6.62 dBW/kg



Test Laboratory: DEKRA Lab Bluetooth 2441MHz Body DH5 Vertical Front **DUT: Bluetooth USB Adapter; Type: BT600C** Communication System: UID 0, Bluetooth (0); Communication System Band: ISM Band; Duty Cycle: 1:1.0; Frequency: 2441 MHz; Medium parameters used: f = 2441 MHz; σ = 1.94 S/m; εr = 52.08;ρ = 1000 kg/m3 ; Phantom section: Flat Section Ambient temperature (°C): 21.5, Liquid temperature (°C): 21.0

DASY5 Configuration:

- Probe: EX3DV4 SN3661; ConvF(7.54, 7.54, 7.54); Calibrated: 05/05/2017;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn905; Calibrated: 20/06/2017
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Configuration/Bluetooth 2441MHz DH5 Body Vertical Front/Area Scan (7x7x1): Measurement grid:

dx=12mm, dy=12mm;Maximum value of SAR (measured) = 0.110 W/kg

Configuration/Bluetooth 2441MHz DH5 Body Vertical Front/Zoom Scan (5x5x7)/Cube


0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 3.576 V/m; Power Drift = 0.19 dB

Peak SAR (extrapolated) = 0.294 W/kg

SAR(1 g) = 0.126 W/kg; SAR(10 g) = 0.050 W/kg

Maximum value of SAR (measured) = 0.148 W/kg

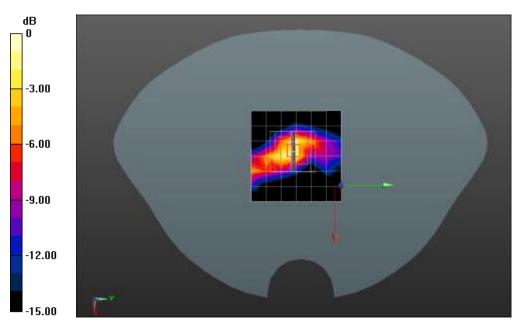

0 dB = 0.148 W/kg = -8.30 dBW/kg



Test Laboratory: DEKRA Lab Bluetooth 2441MHz Body DH5 Vertical Back **DUT: Bluetooth USB Adapter; Type: BT600C** Communication System: UID 0, Bluetooth (0); Communication System Band: ISM Band; Duty Cycle: 1:1.0; Frequency: 2441 MHz; Medium parameters used: f = 2441 MHz; σ = 1.94 S/m; ϵ r = 52.08; ρ = 1000 kg/m3 ; Phantom section: Flat Section Ambient temperature (°C): 21.5, Liquid temperature (°C): 21.0 DASY5 Configuration:

- Probe: EX3DV4 SN3661; ConvF(7.54, 7.54, 7.54); Calibrated: 05/05/2017;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn905; Calibrated: 20/06/2017
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Configuration/Bluetooth 2441MHz DH5 Body Vertical Back/Area Scan (7x7x1): Measurement grid:

dx=12mm, dy=12mm;Maximum value of SAR (measured) = 0.0171 W/kg


Configuration/Bluetooth 2441MHz DH5 Body Vertical Back/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 1.957 V/m; Power Drift = -0.12 dB

Peak SAR (extrapolated) = 0.0530 W/kg

SAR(1 g) = 0.021 W/kg; SAR(10 g) = 0.00724 W/kg

Maximum value of SAR (measured) = 0.0227 W/kg

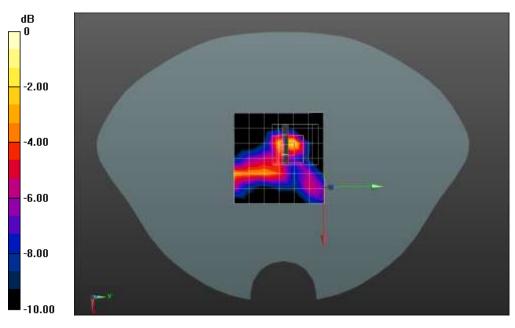

0 dB = 0.0227 W/kg = -16.44 dBW/kg



Test Laboratory: DEKRA Lab Bluetooth 2441MHz Body DH5 Tip **DUT: Bluetooth USB Adapter; Type: BT600C** Communication System: UID 0, Bluetooth (0); Communication System Band: ISM Band; Duty Cycle: 1:1.0; Frequency: 2441 MHz; Medium parameters used: f = 2441 MHz; σ = 1.94 S/m; εr = 52.08; ρ = 1000

kg/m3 ; Phantom section: Flat Section

Ambient temperature (°C): 21.5, Liquid temperature (°C): 21.0

DASY5 Configuration:

- Probe: EX3DV4 SN3661; ConvF(7.54, 7.54, 7.54); Calibrated: 05/05/2017;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn905; Calibrated: 20/06/2017
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Configuration/Bluetooth 2441MHz DH5 Body Tip/Area Scan (7x7x1): Measurement grid: dx=12mm,

dy=12mm;Maximum value of SAR (measured) = 0.0472 W/kg

Configuration/Bluetooth 2441MHz DH5 Body Tip/Zoom Scan (5x5x7)/Cube 0: Measurement grid:


dx=8mm, dy=8mm, dz=5mm

Reference Value = 5.379 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 0.102 W/kg

SAR(1 g) = 0.048 W/kg; SAR(10 g) = 0.018 W/kg

Maximum value of SAR (measured) = 0.0641 W/kg

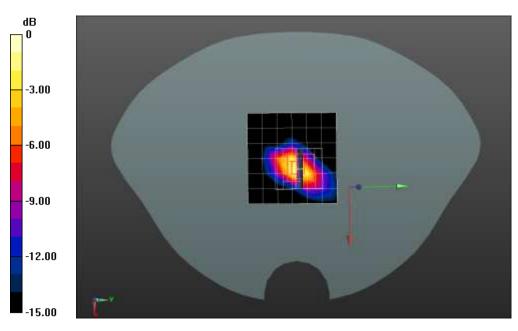

0 dB = 0.0641 W/kg = -11.93 dBW/kg



Test Laboratory: DEKRA Lab Bluetooth 2402MHz Body DH5 Horizontal Down **DUT: Bluetooth USB Adapter; Type: BT600C** Communication System: UID 0, Bluetooth (0); Communication System Band: ISM Band; Duty Cycle: 1:1.0; Frequency: 2402 MHz; Medium parameters used: f = 2402 MHz; σ = 1.88 S/m; ϵ r = 52.25; ρ = 1000 kg/m3 ; Phantom section: Flat Section Ambient temperature (°C): 21.5, Liquid temperature (°C): 21.0 DASY5 Configuration:

- Probe: EX3DV4 SN3661; ConvF(7.54, 7.54, 7.54); Calibrated: 05/05/2017;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn905; Calibrated: 20/06/2017
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Configuration/Bluetooth 2402MHz DH5 Body Horizontal Down/Area Scan (7x7x1): Measurement grid:

dx=12mm, dy=12mm;Maximum value of SAR (measured) = 0.171 W/kg

Configuration/Bluetooth 2402MHz DH5 Body Horizontal Down/Zoom Scan (5x5x7)/Cube


0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 2.259 V/m; Power Drift = 0.18 dB

Peak SAR (extrapolated) = 0.720 W/kg

SAR(1 g) = 0.225 W/kg; SAR(10 g) = 0.081 W/kg

Maximum value of SAR (measured) = 0.271 W/kg

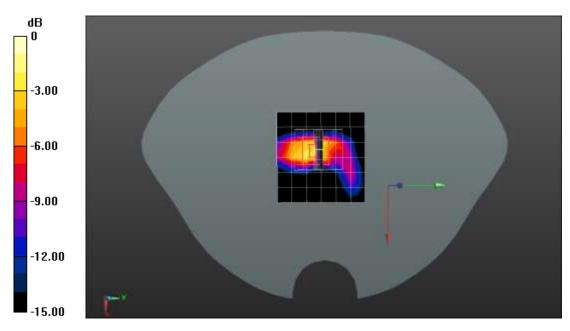

0 dB = 0.271 W/kg = -5.67 dBW/kg



Test Laboratory: DEKRA Lab Bluetooth 2480MHz Body DH5 Horizontal Down **DUT: Bluetooth USB Adapter; Type: BT600C** Communication System: UID 0, Bluetooth (0); Communication System Band: ISM Band; Duty Cycle: 1:1.0; Frequency: 2480 MHz; Medium parameters used: f = 2480 MHz; σ = 1.99 S/m; ϵ r = 51.93; ρ = 1000 kg/m3 ; Phantom section: Flat Section Ambient temperature (°C): 21.5, Liquid temperature (°C): 21.0 DASY5 Configuration:

- Probe: EX3DV4 SN3661; ConvF(7.54, 7.54, 7.54); Calibrated: 05/05/2017;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn905; Calibrated: 20/06/2017
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Configuration/Bluetooth 2480MHz DH5 Body Horizontal Down/Area Scan (7x7x1): Measurement grid:

dx=12mm, dy=12mm;Maximum value of SAR (measured) = 0.100 W/kg

Configuration/Bluetooth 2480MHz DH5 Body Horizontal Down/Zoom Scan (5x5x7)/Cube


0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 1.866 V/m; Power Drift = 0.09 dB

Peak SAR (extrapolated) = 0.366 W/kg

SAR(1 g) = 0.129 W/kg; SAR(10 g) = 0.048 W/kg

Maximum value of SAR (measured) = 0.159 W/kg

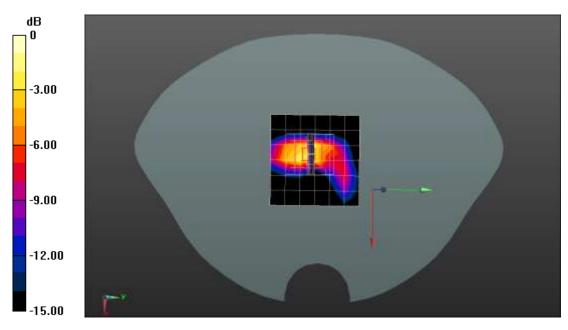

0 dB = 0.159 W/kg = -7.99 dBW/kg



Test Laboratory: DEKRA Lab Bluetooth 2441MHz Body 2DH5 Horizontal Down **DUT: Bluetooth USB Adapter; Type: BT600C** Communication System: UID 0, Wi-Fi (0); Communication System Band: 802.11b; Duty Cycle: 1:1.0; Frequency: 2441 MHz; Medium parameters used: f = 2441 MHz; $\sigma = 1.94$ S/m; $\epsilon r = 52.08; \rho = 1000$ kg/m3; Phantom section: Flat Section Ambient temperature (°C): 21.5, Liquid temperature (°C): 21.0 DASY5 Configuration:

- Probe: EX3DV4 SN3661; ConvF(7.54, 7.54, 7.54); Calibrated: 05/05/2017;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn905; Calibrated: 20/06/2017
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Configuration/ Bluetooth 2441MHz Body 2DH5 Horizontal Down/Area Scan (7x7x1): Measurement

grid: dx=12mm, dy=12mm;Maximum value of SAR (measured) = 0.141 W/kg

Configuration/ Bluetooth 2441MHz Body 2DH5 Horizontal Down/Zoom Scan (5x5x7)/Cube


0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 7.009 V/m; Power Drift = 0.19 dB

Peak SAR (extrapolated) = 0.437 W/kg

SAR(1 g) = 0.140 W/kg; SAR(10 g) = 0.050 W/kg

Maximum value of SAR (measured) = 0.162 W/kg

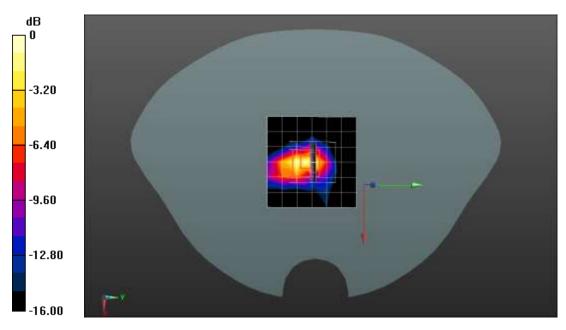

0 dB = 0.162 W/kg = -7.90 dBW/kg



Test Laboratory: DEKRA Lab Bluetooth 2441MHz Body 3DH5 Horizontal Down **DUT: Bluetooth USB Adapter; Type: BT600C** Communication System: UID 0, Wi-Fi (0); Communication System Band: 802.11b; Duty Cycle: 1:1.0; Frequency: 2441 MHz; Medium parameters used: f = 2441 MHz; $\sigma = 1.94$ S/m; $\epsilon r = 52.08$; $\rho = 1000$ kg/m3; Phantom section: Flat Section Ambient temperature (°C): 21.5, Liquid temperature (°C): 21.0 DASY5 Configuration:

- Probe: EX3DV4 SN3661; ConvF(7.54, 7.54, 7.54); Calibrated: 05/05/2017;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn905; Calibrated: 20/06/2017
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Configuration/ Bluetooth 2441MHz body 3DH5 Horizontal Down/Area Scan (7x7x1): Measurement

grid: dx=12mm, dy=12mm;Maximum value of SAR (measured) = 0.150 W/kg

Configuration/ Bluetooth 2441MHz body 3DH5 Horizontal Down/Zoom Scan (5x5x7)/Cube


0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 6.492 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 0.401 W/kg

SAR(1 g) = 0.139 W/kg; SAR(10 g) = 0.051 W/kg

Maximum value of SAR (measured) = 0.161 W/kg

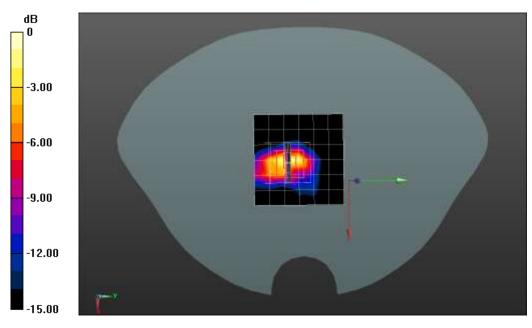

0 dB = 0.161 W/kg = -7.93 dBW/kg



Test Laboratory: DEKRA Lab Bluetooth 2480MHz Body BLE Horizontal Down **DUT: Bluetooth USB Adapter; Type: BT600C** Communication System: UID 0, Bluetooth (0); Communication System Band: BLE; Duty Cycle: 1:1.0; Frequency: 2480 MHz; Medium parameters used: f = 2480 MHz; σ = 1.99 S/m; ϵ r = 51.93; ρ = 1000 kg/m3; Phantom section: Flat Section Ambient temperature (°C): 21.5, Liquid temperature (°C): 21.0 DASY5 Configuration:

- Probe: EX3DV4 SN3661; ConvF(7.54, 7.54, 7.54); Calibrated: 05/05/2017;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn905; Calibrated: 20/06/2017
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Configuration/Bluetooth 2480MHz Body BLE Horizontal Down/Area Scan (7x7x1): Measurement grid:

dx=12mm, dy=12mm;Maximum value of SAR (measured) = 0.0521 W/kg

Configuration/Bluetooth 2480MHz Body BLE Horizontal Down/Zoom Scan (5x5x7)/Cube


0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 4.251 V/m; Power Drift = 0.14 dB

Peak SAR (extrapolated) = 0.244 W/kg

SAR(1 g) = 0.068 W/kg; SAR(10 g) = 0.023 W/kg


Maximum value of SAR (measured) = 0.0650 W/kg

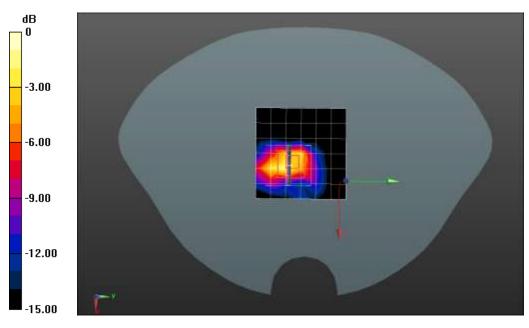

0 dB = 0.0650 W/kg = -11.87 dBW/kg




2450 Body

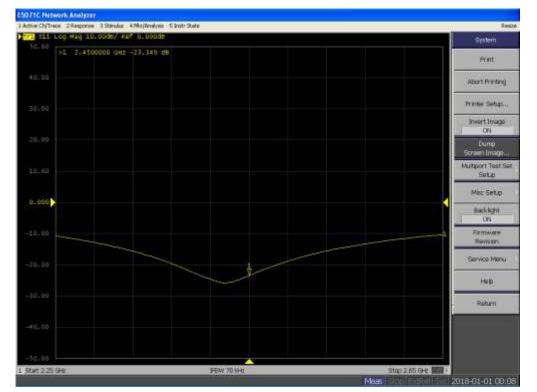

Calibrated return loss: -23.882 dB; Measured return loss: -23.349dB (within 20%)

Calibrated impedance: 50.244 Ω ; Measured impedance: 49.316 Ω (within 5 Ω)

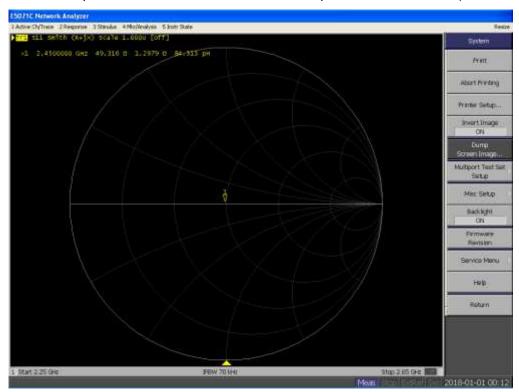

Appendix C. Probe Calibration Data

| | | t, Beijing, 100191, China | CNAS LOS |
|--|--|---|---|
| Tel: +86-10-6230463 | | | |
| E-mail: cttl@chinattl Client Aude | and a second | Certificate No: Z17-9 | 7051 |
| Chern | The sufficiency of | | |
| CALIBRATION CE | RIFICATE | | |
| Dbject | EX3DV4 | - SN:3661 | |
| Calibration Procedure(s) | FF 744 0 | | |
| | FF-Z11-0 Calibratio | 04-01 on Procedures for Dosimetric E-field Probes | |
| | | | |
| Calibration date: | May 05, 2 | 2017 | |
| neasurements(SI). The mea | Company of the second state of the second state | a state of the first sector in the second distance of the second s | a given on the following |
| ages and are part of the ce I calibrations have been | rtificate. | e uncertainties with confidence probability ar e closed laboratory facility: environment to | |
| bages and are part of the centry of the cent | rtificate. conducted in th (M&TE critical for | e closed laboratory facility: environment to calibration) | emperature(22±3)℃ and |
| ages and are part of the central calibrations have been unidity<70%. Calibration Equipment used Primary Standards | rtificate. conducted in th (M&TE critical for ID # (| e closed laboratory facility: environment to calibration) Cal Date(Calibrated by, Certificate No.) | emperature(22±3) [°] C and Scheduled Calibration |
| ages and are part of the central calibrations have been umidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 | rtificate. conducted in th (M&TE critical for ID # (101919 | e closed laboratory facility: environment to calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-16 (CTTL, No.J16X04777) | emperature(22±3) [°] C and Scheduled Calibration Jun-17 |
| ages and are part of the central calibrations have been umidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 | rtificate. conducted in th (M&TE critical for ID # () 101919 101547 | e closed laboratory facility: environment to calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-16 (CTTL, No.J16X04777) 27-Jun-16 (CTTL, No.J16X04777) | emperature(22±3) [°] C and Scheduled Calibration Jun-17 Jun-17 |
| ages and are part of the central calibrations have been umidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 | rtificate. conducted in th (M&TE critical for ID # (101919 101547 101548 | e closed laboratory facility: environment to calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-16 (CTTL, No.J16X04777) 27-Jun-16 (CTTL, No.J16X04777) 27-Jun-16 (CTTL, No.J16X04777) | emperature(22±3) [°] C and Scheduled Calibration Jun-17 Jun-17 Jun-17 |
| ages and are part of the cer II calibrations have been umidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference10dBAttenuator | rtificate. conducted in th (M&TE critical for ID # (0) 101919 101547 101548 18N50W-10dB | e closed laboratory facility: environment to calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-16 (CTTL, No.J16X04777) 27-Jun-16 (CTTL, No.J16X04777) 27-Jun-16 (CTTL, No.J16X04777) 13-Mar-16(CTTL,No.J16X01547) | emperature(22±3)℃ and Scheduled Calibration Jun-17 Jun-17 Jun-17 Mar-18 |
| ages and are part of the cer II calibrations have been umidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference10dBAttenuator Reference20dBAttenuator | rtificate. conducted in th (M&TE critical for ID # (101919 101547 101548 18N50W-10dB 18N50W-20dB | e closed laboratory facility: environment to calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-16 (CTTL, No.J16X04777) 27-Jun-16 (CTTL, No.J16X04777) 13-Mar-16(CTTL, No.J16X01547) 13-Mar-16(CTTL, No.J16X01548) | emperature(22±3)℃ and Scheduled Calibration Jun-17 Jun-17 Jun-17 Mar-18 Mar-18 |
| ages and are part of the cer II calibrations have been umidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference10dBAttenuator | rtificate. conducted in th (M&TE critical for ID # (0) 101919 101547 101548 18N50W-10dB | e closed laboratory facility: environment to calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-16 (CTTL, No.J16X04777) 27-Jun-16 (CTTL, No.J16X04777) 27-Jun-16 (CTTL, No.J16X04777) 13-Mar-16(CTTL,No.J16X01547) | emperature(22±3)℃ and Scheduled Calibration Jun-17 Jun-17 Jun-17 Mar-18 |
| ages and are part of the cer all calibrations have been umidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference10dBAttenuator Reference20dBAttenuator Reference Probe EX3DV4 DAE4 | rtificate. conducted in th (M&TE critical for ID # (101919 101547 101548 18N50W-10dB 18N50W-20dB SN 7433 SN 549 | e closed laboratory facility: environment to calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-16 (CTTL, No.J16X04777) 27-Jun-16 (CTTL, No.J16X04777) 27-Jun-16 (CTTL, No.J16X04777) 13-Mar-16(CTTL, No.J16X01547) 13-Mar-16(CTTL, No.J16X01548) 26-Sep-16(SPEAG, No.EX3-7433_Sep16) 13-Dec-16(SPEAG, No.DAE4-549_Dec16) | emperature(22±3) ¹ C and Scheduled Calibration Jun-17 Jun-17 Jun-17 Mar-18 Mar-18 Sep-17 Dec -17 |
| ages and are part of the cer unidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference10dBAttenuator Reference20dBAttenuator Reference Probe EX3DV4 DAE4 Secondary Standards | rtificate. conducted in th (M&TE critical for ID # (0) 101919 101547 101548 18N50W-10dB 18N50W-20dB SN 7433 SN 549 ID # | e closed laboratory facility: environment to calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-16 (CTTL, No.J16X04777) 27-Jun-16 (CTTL, No.J16X04777) 27-Jun-16 (CTTL, No.J16X04777) 13-Mar-16(CTTL, No.J16X01547) 13-Mar-16(CTTL, No.J16X01548) 26-Sep-16(SPEAG,No.EX3-7433_Sep16) 13-Dec-16(SPEAG, No.DAE4-549_Dec16) Cal Date(Calibrated by, Certificate No.) | emperature(22±3) [°] C and Scheduled Calibration Jun-17 Jun-17 Jun-17 Mar-18 Mar-18 Sep-17 Dec -17 Scheduled Calibration |
| ages and are part of the cer II calibrations have been umidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference10dBAttenuator Reference20dBAttenuator Reference Probe EX3DV4 DAE4 Secondary Standards SignalGeneratorMG3700A | rtificate. conducted in th (M&TE critical for ID # () 101919 101547 101548 18N50W-10dB 18N50W-20dB SN 7433 SN 549 ID # 6201052605 | e closed laboratory facility: environment to calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-16 (CTTL, No.J16X04777) 27-Jun-16 (CTTL, No.J16X04777) 13-Mar-16(CTTL, No.J16X01547) 13-Mar-16(CTTL, No.J16X01548) 26-Sep-16(SPEAG,No.EX3-7433_Sep16) 13-Dec-16(SPEAG, No.DAE4-549_Dec16) Cal Date(Calibrated by, Certificate No.) 27-Jun-16 (CTTL, No.J16X04776) | emperature(22±3) ¹ C and Scheduled Calibration Jun-17 Jun-17 Jun-17 Mar-18 Mar-18 Sep-17 Dec -17 Scheduled Calibration Jun-17 |
| ages and are part of the cer all calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference10dBAttenuator Reference20dBAttenuator Reference20dBAttenuator Reference Probe EX3DV4 DAE4 Secondary Standards SignalGeneratorMG3700A Network Analyzer E5071C | rtificate. conducted in th (M&TE critical for ID # (0) 101919 101547 101548 18N50W-10dB 18N50W-20dB SN 7433 SN 549 ID # | e closed laboratory facility: environment te calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-16 (CTTL, No.J16X04777) 27-Jun-16 (CTTL, No.J16X04777) 27-Jun-16 (CTTL, No.J16X04777) 13-Mar-16(CTTL, No.J16X01547) 13-Mar-16(CTTL, No.J16X01548) 26-Sep-16(SPEAG, No.DAE4-549_Dec16) 13-Dec-16(SPEAG, No.DAE4-549_Dec16) Cal Date(Calibrated by, Certificate No.) 27-Jun-16 (CTTL, No.J16X04776) 13-Jan-17 (CTTL, No.J17X00285) | emperature(22±3) [°] C and Scheduled Calibration Jun-17 Jun-17 Jun-17 Mar-18 Mar-18 Sep-17 Dec -17 Scheduled Calibration Jun-17 Jan -18 |
| ages and are part of the cer all calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference10dBAttenuator Reference20dBAttenuator Reference20dBAttenuator Reference Probe EX3DV4 DAE4 Secondary Standards SignalGeneratorMG3700A Network Analyzer E5071C | rtificate. conducted in th (M&TE critical for ID # () 101919 101547 101548 18N50W-10dB 18N50W-20dB SN 7433 SN 549 ID # 6201052605 MY46110673 | e closed laboratory facility: environment to calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-16 (CTTL, No.J16X04777) 27-Jun-16 (CTTL, No.J16X04777) 13-Mar-16(CTTL, No.J16X01547) 13-Mar-16(CTTL, No.J16X01548) 26-Sep-16(SPEAG,No.EX3-7433_Sep16) 13-Dec-16(SPEAG, No.DAE4-549_Dec16) Cal Date(Calibrated by, Certificate No.) 27-Jun-16 (CTTL, No.J16X04776) | emperature(22±3) [°] C and Scheduled Calibration Jun-17 Jun-17 Jun-17 Mar-18 Mar-18 Sep-17 Dec -17 Scheduled Calibration Jun-17 |
| ages and are part of the cer all calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference10dBAttenuator Reference20dBAttenuator Reference Probe EX3DV4 DAE4 Secondary Standards SignalGeneratorMG3700A Network Analyzer E5071C | rtificate. conducted in th (M&TE critical for ID # (0) 101919 101547 101548 18N50W-10dB 18N50W-20dB SN 7433 SN 549 ID # 6201052605 MY46110673 Name | e closed laboratory facility: environment to calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-16 (CTTL, No.J16X04777) 27-Jun-16 (CTTL, No.J16X04777) 13-Mar-16(CTTL, No.J16X01547) 13-Mar-16(CTTL, No.J16X01548) 26-Sep-16(SPEAG,No.EX3-7433_Sep16) 13-Dec-16(SPEAG, No.DAE4-549_Dec16) Cal Date(Calibrated by, Certificate No.) 27-Jun-16 (CTTL, No.J16X04776) 13-Jan-17 (CTTL, No.J17X00285) Function | emperature(22±3) [°] C and Scheduled Calibration Jun-17 Jun-17 Jun-17 Mar-18 Mar-18 Sep-17 Dec -17 Scheduled Calibration Jun-17 Jan -18 |

Certificate No: Z17-97051

Page 1 of 11





 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2218
 Fax: +86-10-62304633-2209

 E-mail: ettl@chinattl.com
 Http://www.chinattl.cn

Glossary:

| TSL | tissue simulating liquid |
|----------------|--|
| NORMx,y,z | sensitivity in free space |
| ConvF | sensitivity in TSL / NORMx,y,z |
| DCP | diode compression point |
| CF | crest factor (1/duty_cycle) of the RF signal |
| A,B,C,D | modulation dependent linearization parameters |
| Polarization Φ | Φ rotation around probe axis |
| Polarization 0 | θ rotation around an axis that is in the plane normal to probe axis (at measurement center), |
| | θ=0 is normal to probe axis |

Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300MHz to 3GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010

d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"


Methods Applied and Interpretation of Parameters:

- NORMx, y,z: Assessed for E-field polarization θ=0 (f≤900MHz in TEM-cell; f>1800MHz: waveguide). NORMx, y,z are only intermediate values, i.e., the uncertainties of NORMx, y,z does not effect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x, y, z = NORMx, y, z* frequency_response (see Frequency Response Chart). This
 linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the
 frequency response is included in the stated uncertainty of ConvF.
- DCPx, y, z: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- Ax, y,z; Bx, y,z; Cx, y,z; VRx, y,z:A,B,C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f≤800MHz) and inside waveguide using analytical field distributions based on power measurements for f >800MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty valued are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from±50MHz to±100MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the
 probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No: Z17-97051

Page 2 of 11





 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2218
 Fax: +86-10-62304633-2209

 E-mail: cttl@chinattl.com
 Http://www.chinattl.cn

Probe EX3DV4

SN: 3661

Calibrated: May 05, 2017

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

Certificate No: Z17-97051

Page 3 of 11





DASY/EASY – Parameters of Probe: EX3DV4 – SN: 3661

Basic Calibration Parameters

| | Sensor X | Sensor Y | Sensor Z | Unc (k=2) |
|---|----------|----------|----------|-----------|
| Norm(µV/(V/m) ²) ^A | 0.48 | 0.52 | 0.48 | ±10.0% |
| DCP(mV) ⁸ | 101.6 | 100.2 | 102.2 | |

Modulation Calibration Parameters

| UID | Communication System Name | | A dB | B dBõV | c | D dB | VR mV | Unc ^E (k=2) |
|-----|------------------------------|---|---------|-----------|-----|---------|----------|---------------------------|
| 0 | CW | X | 0.0 | 0.0 | 1.0 | 0.00 | 201.4 | ±2.0% |
| | | Y | 0.0 | 0.0 | 1.0 | | 213.0 | |
| | | z | 0.0 | 0.0 | 1.0 | | 202.8 | |

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X, Y, Z do not affect the E²-field uncertainty inside TSL (see Page 5 and Page 6). ^B Numerical linearization parameter: uncertainty not required.

^E Uncertainly is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Certificate No: Z17-97051

Page 4 of 11





 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2218
 Fax: +86-10-62304633-2209

 E-mail: ettl@chinattl.com
 Http://www.chinattl.cn

DASY/EASY – Parameters of Probe: EX3DV4 – SN: 3661

| f [MHz] ^C | Relative Permittivity ^F | Conductivity (S/m) ^F | ConvF X | ConvF Y | ConvF Z | Alpha ^G | Depth ^G (mm) | Unct. (k=2) |
|----------------------|---------------------------------------|------------------------------------|---------|---------|---------|--------------------|----------------------------|----------------|
| 750 | 41.9 | 0.89 | 9.89 | 9.89 | 9.89 | 0.30 | 0.85 | ±12.1% |
| 835 | 41.5 | 0.90 | 9.57 | 9.57 | 9.57 | 0.13 | 1.40 | ±12.1% |
| 900 | 41.5 | 0.97 | 9.73 | 9.73 | 9.73 | 0.13 | 1.36 | ±12.1% |
| 1750 | 40.1 | 1.37 | 8.47 | 8.47 | 8.47 | 0.17 | 1.36 | ±12.1% |
| 1900 | 40.0 | 1.40 | 8.10 | 8.10 | 8.10 | 0.21 | 1.10 | ±12.1% |
| 2000 | 40.0 | 1.40 | 8.09 | 8.09 | 8.09 | 0.20 | 1.11 | ±12.1% |
| 2300 | 39.5 | 1.67 | 7.93 | 7.93 | 7.93 | 0.39 | 0.83 | ±12.1% |
| 2450 | 39.2 | 1.80 | 7.64 | 7.64 | 7.64 | 0.43 | 0.82 | ±12.1% |
| 2600 | 39.0 | 1.96 | 7.35 | 7.35 | 7.35 | 0.55 | 0.71 | ±12.1% |
| 3500 | 37.9 | 2.91 | 7.23 | 7.23 | 7.23 | 0.53 | 0.84 | ±13.3% |
| 5250 | 35.9 | 4.71 | 5.36 | 5.36 | 5.36 | 0.40 | 1.30 | ±13.3% |
| 5600 | 35.5 | 5.07 | 4.88 | 4.88 | 4.88 | 0.40 | 1.50 | ±13.3% |
| 5750 | 35.4 | 5.22 | 4.87 | 4.87 | 4.87 | 0.40 | 1.50 | ±13.3% |

Calibration Parameter Determined in Head Tissue Simulating Media

^C Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^F At frequency below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than \pm 1% for frequencies below 3 GHz and below \pm 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.





 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2218
 Fax: +86-10-62304633-2209

 E-mail: ettl@chinattl.com
 <u>Http://www.chinattl.cn</u>

DASY/EASY – Parameters of Probe: EX3DV4 – SN: 3661

| f [MHz] ^C | Relative Permittivity ^F | Conductivity (S/m) ^F | ConvF X | ConvF Y | ConvF Z | Alpha ^G | Depth ^G (mm) | Unct. (k=2) |
|----------------------|---------------------------------------|------------------------------------|---------|---------|---------|--------------------|----------------------------|----------------|
| 750 | 55.5 | 0.96 | 9.85 | 9.85 | 9.85 | 0.30 | 0.90 | ±12.1% |
| 835 | 55.2 | 0.97 | 9.60 | 9.60 | 9.60 | 0.16 | 1.43 | ±12.1% |
| 900 | 55.0 | 1.05 | 9.69 | 9.69 | 9.69 | 0.20 | 1.19 | ±12.1% |
| 1750 | 53.4 | 1.49 | 8.26 | 8.26 | 8.26 | 0.22 | 1.11 | ±12.1% |
| 1900 | 53.3 | 1.52 | 7.88 | 7.88 | 7.88 | 0.15 | 1.55 | ±12.1% |
| 2000 | 53.3 | 1.52 | 7.92 | 7.92 | 7.92 | 0.21 | 1.24 | ±12.1% |
| 2300 | 52.9 | 1.81 | 7.81 | 7.81 | 7.81 | 0.37 | 1.05 | ±12.1% |
| 2450 | 52.7 | 1.95 | 7.54 | 7.54 | 7.54 | 0.29 | 1.46 | ±12.1% |
| 2600 | 52.5 | 2.16 | 7.45 | 7.45 | 7.45 | 0.32 | 1.19 | ±12.1% |
| 3500 | 51.3 | 3.31 | 6.67 | 6.67 | 6.67 | 0.59 | 0.94 | ±13.3% |
| 5250 | 48.9 | 5.36 | 4.94 | 4.94 | 4.94 | 0.50 | 1.45 | ±13.3% |
| 5600 | 48.5 | 5.77 | 4.32 | 4.32 | 4.32 | 0.55 | 1.35 | ±13.3% |
| 5750 | 48.3 | 5.94 | 4.52 | 4.52 | 4.52 | 0.55 | 1.75 | ±13.3% |

Calibration Parameter Determined in Body Tissue Simulating Media

^C Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^F At frequency below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters. ^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Page 6 of 11






 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2218
 Fax: +86-10-62304633-2209

 E-mail: cttl@chinattl.com
 Http://www.chinattl.cn

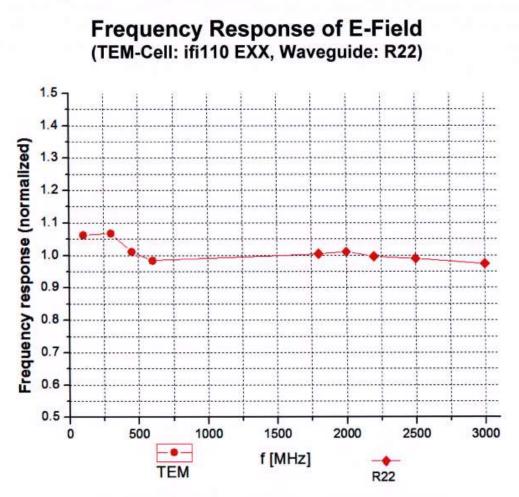

Uncertainty of Frequency Response of E-field: ±7.4% (k=2)

Certificate No: Z17-97051

Page 7 of 11





 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China


 Tel: +86-10-62304633-2218
 Fax: +86-10-62304633-2209


 E-mail: cttl@chinattl.com
 Http://www.chinattl.cn

Receiving Pattern (Φ), θ=0°

f=600 MHz, TEM

f=1800 MHz, R22

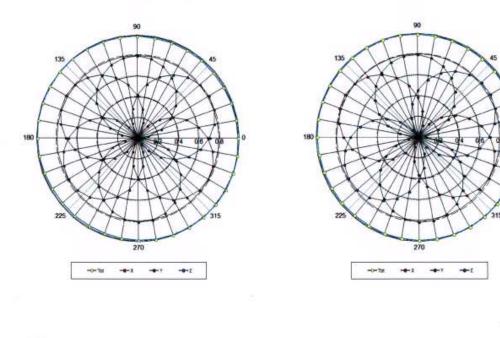


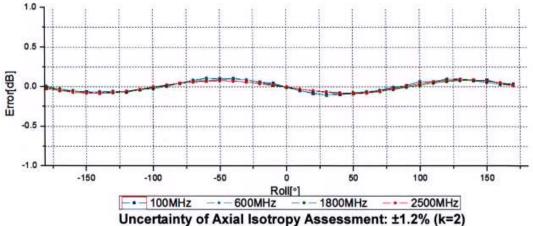


Certificate No: Z17-97051

Page 8 of 11




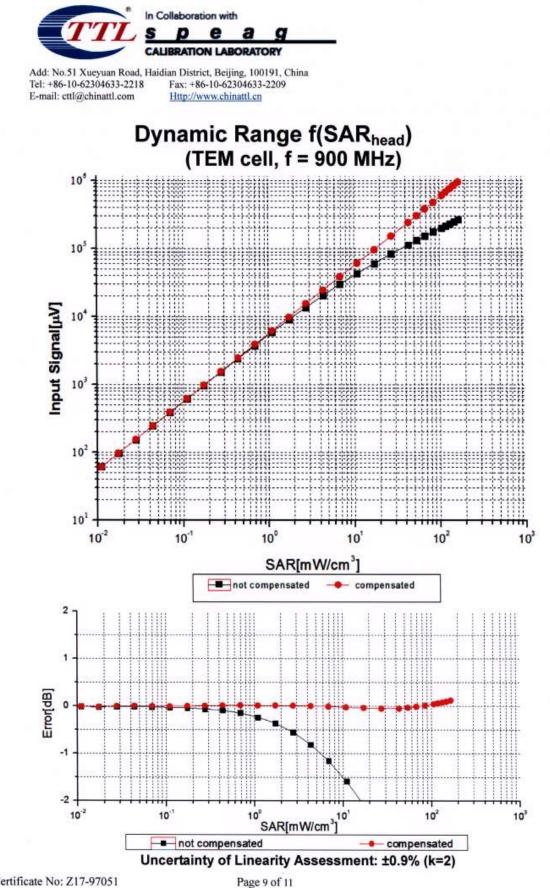









 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China


 Tel: +86-10-62304633-2218
 Fax: +86-10-62304633-2209

 E-mail: cttl@chinattl.com
 <u>Http://www.chinattl.cn</u>


Conversion Factor Assessment

f=900 MHz, WGLS R9(H convF)

f=1750 MHz, WGLS R22(H_convF)

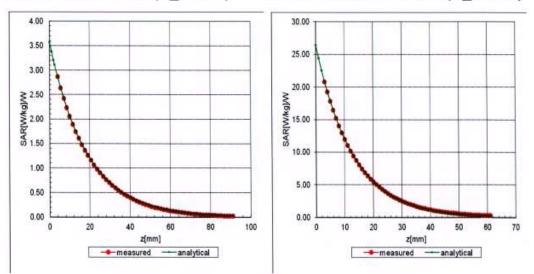

Deviation from Isotropy in Liquid

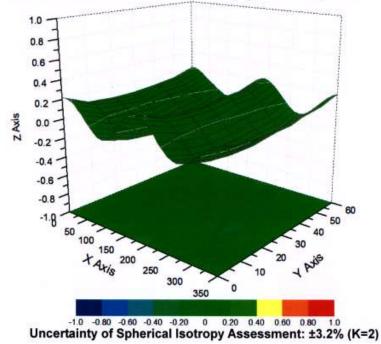

Certificate No: Z17-97051

Page 10 of 11





 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2218
 Fax: +86-10-62304633-2209

 E-mail: cttl@chinattl.com
 <u>Http://www.chinattl.cn</u>

DASY/EASY – Parameters of Probe: EX3DV4 – SN: 3661

Other Probe Parameters

| Sensor Arrangement | Triangular |
|---|------------|
| Connector Angle (°) | 129.5 |
| Mechanical Surface Detection Mode | enabled |
| Optical Surface Detection Mode | disable |
| Probe Overall Length | 337mm |
| Probe Body Diameter | 10mm |
| Tip Length | 9mm |
| Tip Diameter | 2.5mm |
| Probe Tip to Sensor X Calibration Point | 1mm |
| Probe Tip to Sensor Y Calibration Point | 1mm |
| Probe Tip to Sensor Z Calibration Point | 1mm |
| Recommended Measurement Distance from Surface | 1.4mm |

Page 11 of 11



Appendix D. Dipole Calibration Data

| Schmid & Partner Engineering AG Leughausstrasse 43, 8004 Zuric | y of h, Switzerland | ILAC MRA | Schweizerischer Kallbrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service |
|--|--|---|---|
| Accredited by the Swiss Accredita The Swiss Accreditation Service Multilateral Agreement for the re | e is one of the signatorie | is to the EA. | Accreditation No.: SCS 0108 |
| Client QTK-CN (Aude | | | No: D2450V2-839_Feb16 |
| CALIBRATION C | ERTIFICATE | | |
| Object | D2450V2 - SN: 8 | 39 | |
| Calibration procedure(s) | QA CAL-05.v9 Calibration proce | dure for dipole validation kits at | pove 700 MHz |
| | Calibration prove | | |
| Calibration date: | February 09, 201 | 6 | |
| The measurements and the unce | rtainties with confidence p | ional standards, which realize the physical or robability are given on the following pages or ry facility: environment temperature (22 ± 3) | and are part of the certificate. |
| The measurements and the unce All calibrations have been conduc | rtainties with confidence p cted in the closed laborato | robability are given on the following pages a | and are part of the certificale. PC and humidity < 70%. |
| The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T | rtainties with confidence p cted in the closed laborato | robability are given on the following pages a | and are part of the certificate. PC and humidity < 70%. Scheduled Calibration |
| The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPM-442A | rtainties with confidence p tool in the closed laborato FE critical for calibration) ID a GB37480704 | robability are given on the following pages (ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 07-Oct-15 (No. 217-02222) | and are part of the certificate. PC and humidity < 70%. Scheduled Calibration Oct-16 |
| The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPM-442A Power sensor HP 8481A | rtainties with confidence p tred in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 | robability are given on the following pages (ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) | and are part of the certificate. PC and humidity < 70%. Scheduled Calibration Oct-16 Oct-16 |
| The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A | rtainties with confidence p tred in the closed laborato TE critical for calibration) ID a GB37480704 US37292783 MY41092317 | robability are given on the following pages (ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223) | and are part of the certificate. PC and humidity < 70%. Scheduled Calibration Oct-16 Oct-16 Oct-16 Oct-16 |
| The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator | rtainties with confidence p top in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 MY41092317 SN: 5058 (20k) | robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223) 01-Apr-15 (No. 217-02131) | and are part of the certificate. PC and humidity < 70%. Scheduled Calibration Oct-16 Oct-16 Oct-16 Mar-16 |
| The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination | rtainties with confidence p tool in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5047.2 / 06327 | robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223) 01-Apr-15 (No. 217-02134) | and are part of the certificate. PC and humidity < 70%. Scheduled Calibration Oct-16 Oct-16 Mar-16 Mar-16 Mar-16 |
| The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 | rtainties with confidence p top in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 MY41092317 SN: 5058 (20k) | robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223) 01-Apr-15 (No. 217-02131) | and are part of the certificate. PC and humidity < 70%. Scheduled Calibration Oct-16 Oct-16 Oct-16 Mar-16 |
| The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power mater EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 | rtainties with confidence p tod in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 50547.2 / 06327 SN: 7349 SN: 601 | robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223) 01-Apr-15 (No. 217-02134) 01-Apr-15 (No. 217-02134) 31-Dec-15 (No. EX3-7349_Dec15) 30-Dec-15 (No. DAE4-601_Dec15) | and are part of the certificate. PC and humidity < 70%. Scheduled Calibration Oct-16 Oct-16 Oct-16 Mar-16 Mar-16 Dec-16 |
| The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T <u>Primary Standards</u> Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards | rtainties with confidence p tod in the closed laborato FE critical for calibration) ID # GB37480704 US37292783 MY41092317 SN: 5047.2 / 06327 SN: 5047.2 / 06327 SN: 7349 SN: 601 ID # | robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223) 01-Apr-15 (No. 217-02134) 01-Apr-15 (No. 217-02134) 01-Apr-15 (No. 217-02134) 31-Dec-15 (No. DAE4-601_Dec15) 30-Dec-15 (No. DAE4-601_Dec15) Check Date (in house) | and are part of the certificate. PC and humidity < 70%. Scheduled Calibration Oct-16 Oct-16 Oct-16 Mar-16 Mar-16 Dec-16 Dec-16 Dec-16 |
| The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards RF generator R&S SMT-06 | rtainties with confidence p tod in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 MY41092317 SN: 5054.24 / 06327 SN: 5047.2 / 06327 SN: 7349 SN: 601 | robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223) 01-Apr-15 (No. 217-02134) 01-Apr-15 (No. 217-02134) 31-Dec-15 (No. EX3-7349_Dec15) 30-Dec-15 (No. DAE4-601_Dec15) | and are part of the certificate. PC and humidity < 70%. Scheduled Calibration Oct-16 Oct-16 Oct-16 Mar-16 Dec-16 Dec-16 Dec-16 Dec-16 Scheduled Check |
| The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards RF generator R&S SMT-06 | rtainties with confidence p tool in the closed laborato ID # GB37480704 US37292783 MY41062317 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 5047.2 / 0747 SN: 5047.2 / 0747 SN: 5047.2 / | Cal Date (Certificate No.) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223) 01-Apr-15 (No. 217-02134) 31-Dec-15 (No. 217-02134) 30-Dec-15 (No. 217-02134) 30-Dec-15 (No. DAE4-601_Dec15) 30-Dec-15 (No. DAE4-601_Dec15) 15-Jun-15 (in house check Jun-15) 18-Oct-01 (in house check Jun-15) | and are part of the certificate. PC and humidity < 70%. Scheduled Calibration Oct-16 Oct-16 Mar-16 Mar-16 Dec-16 Dec-16 Dec-16 Dec-18 Scheduled Check In house check: Jun-18 In house check: Oct-16 |
| The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards RF generator R&S SMT-06 Network Analyzer HP 8753E | rtainties with confidence p ted in the closed laborato IE critical for calibration) ID # GB37480704 US37292783 MY41062317 SN: 5058 (20k) SN: 5058 (20k | robability are given on the following pages a ry facility: environment temperature (22 ± 3) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223) 01-Apr-15 (No. 217-0223) 01-Apr-15 (No. 217-02134) 31-Dec-15 (No. 217-02134) 31-Dec-15 (No. EX3-7349_Dec15) 30-Dec-15 (No. DAE4-601_Dec15) Check Date (in house) 15-Jun-15 (in house check Jun-15) 18-Oct-01 (in house check Jun-15) Function | and are part of the certificate. PC and humidity < 70%. Scheduled Calibration Oct-16 Oct-16 Oct-16 Mar-16 Dec-16 Dec-16 Dec-16 Dec-16 Dec-16 Dec-16 Dec-16 Dec-16 Dec-18 In house check: Jun-18 |
| The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards RF generator R&S SMT-06 | rtainties with confidence p tool in the closed laborato ID # GB37480704 US37292783 MY41062317 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 5047.2 / 0747 SN: 5047.2 / 0747 SN: 5047.2 / | Cal Date (Certificate No.) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223) 01-Apr-15 (No. 217-02134) 31-Dec-15 (No. 217-02134) 30-Dec-15 (No. 217-02134) 30-Dec-15 (No. DAE4-601_Dec15) 30-Dec-15 (No. DAE4-601_Dec15) 15-Jun-15 (in house check Jun-15) 18-Oct-01 (in house check Jun-15) | and are part of the certificate. PC and humidity < 70%. Scheduled Calibration Oct-16 Oct-16 Mar-16 Mar-16 Dec-16 Dec-16 Dec-16 Dec-18 Scheduled Check In house check: Jun-18 In house check: Oct-16 |
| The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards RF generator R&S SMT-06 Network Analyzer HP 6753E Calibrated by: | rtainties with confidence p ted in the closed laborato IE critical for calibration) ID # GB37480704 US37292783 MY41062317 SN: 5058 (20k) SN: 5058 (20k | robability are given on the following pages a ry facility: environment temperature (22 ± 3) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223) 01-Apr-15 (No. 217-0223) 01-Apr-15 (No. 217-02134) 31-Dec-15 (No. 217-02134) 31-Dec-15 (No. EX3-7349_Dec15) 30-Dec-15 (No. DAE4-601_Dec15) Check Date (in house) 15-Jun-15 (in house check Jun-15) 18-Oct-01 (in house check Jun-15) Function | and are part of the certificate. PC and humidity < 70%. Scheduled Calibration Oct-16 Oct-16 Mar-16 Mar-16 Dec-16 Dec-16 Dec-16 Dec-18 Scheduled Check In house check: Jun-18 In house check: Oct-16 |
| The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards RF generator R&S SMT-06 Network Analyzer HP 8753E | rtainties with confidence p ted in the closed laborato FE critical for calibration) ID # GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5058 (20k) Name Michael Weber | Cal Date (Certificate No.) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223) 01-Apr-15 (No. 217-02134) 31-Dec-15 (No. EX3-7349_Dec15) 30-Dec-15 (No. DAE4-601_Dec15) Check Date (in house) 15-Jun-15 (in house check Jun-15) 18-Oct-01 (in house check Oct-15) Function Laboratory Technician | and are part of the certificate. PC and humidity < 70%. Scheduled Calibration Oct-16 Oct-16 Mar-16 Mar-16 Dec-16 Dec-16 Dec-16 Dec-18 Scheduled Check In house check: Jun-18 In house check: Oct-16 |

Certificate No: D2450V2-839_Feb16

Page 1 of 8



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura

S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

| TSL | tissue simulating liquid |
|-------|---------------------------------|
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A | not applicable or not measured |

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D2450V2-839_Feb16

Page 2 of 8



Measurement Conditions

DASY system configuration, as far as not given on page 1.

| DASY5 | V52.8.8 |
|------------------------|--|
| Advanced Extrapolation | |
| Modular Flat Phantom | |
| 10 mm | with Spacer |
| dx, dy, dz = 5 mm | |
| 2450 MHz ± 1 MHz | |
| | Advanced Extrapolation Modular Flat Phantom 10 mm dx, dy, dz = 5 mm |

Head TSL parameters

The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|---|-----------------|-----------------|------------------|
| Nominal Head TSL parameters | 22.0 "C | 39.2 | 1.80 mho/m |
| Measured Head TSL parameters | (22.0 ± 0.2) °C | 38.7 ± 6 % | 1.84 mho/m ± 6 % |
| Head TSL temperature change during test | < 0.5 °C | 2 : | **** |

SAR result with Head TSL

| SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | |
|---|---------------------------------|--------------------------|
| SAR measured | 250 mW input power | 13.0 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 51.3 W/kg ± 17.0 % (k=2) |
| | | |
| | | |
| SAR averaged over 10 cm ³ (10 g) of Head TSL | condition | |
| SAR averaged over 10 cm ³ (10 g) of Head TSL SAR measured | condition 250 mW input power | 6.03 W/kg |

Body TSL parameters

| | Temperature | Permittivity | Conductivity |
|---|-----------------|--------------|------------------|
| Nominal Body TSL parameters | 22.0 °C | 52.7 | 1.95 mho/m |
| Measured Body TSL parameters | (22.0 ± 0.2) °C | 52.9 ± 6 % | 2.00 mho/m ± 6 % |
| Body TSL temperature change during test | < 0.5 °C | | |

SAR result with Body TSL

| SAR averaged over 1 cm ³ (1 g) of Body TSL | Condition | |
|---|---------------------------------|--------------------------|
| SAR measured | 250 mW input power | 12.6 W/kg |
| SAR for nominal Body TSL parameters | normalized to 1W | 49.8 W/kg ± 17.0 % (k=2) |
| | | |
| SAR averaged over 10 cm ³ (10 g) of Body TSL | condition | |
| SAR averaged over 10 cm ³ (10 g) of Body TSL SAR measured | condition 250 mW input power | 5.87 W/kg |

Certificate No: D2450V2-839_Feb16

Page 3 of 8



Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

| Impedance, transformed to feed point | 55.4 Ω + 2.0 jΩ | |
|--------------------------------------|-----------------|--|
| Return Loss | - 25.2 dB | |

Antenna Parameters with Body TSL

| Impedance, transformed to feed point | 50.2 Ω + 6.4 jΩ | |
|--------------------------------------|-----------------|--|
| Return Loss | - 23.9 dB | |

General Antenna Parameters and Design

| Electrical Delay (one direction) | 1,143 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the teedpoint may be damaged.

Additional EUT Data

| Manufactured by | SPEAG |
|-----------------|---------------|
| Manufactured on | July 20, 2009 |

Certificate No: D2450V2-839_Feb16

Page 4 of 8



Date: 08.02.2016

DASY5 Validation Report for Head TSL

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 839


Communication System: UID 0 - CW; Frequency: 2450 MHz Medium parameters used: f = 2450 MHz; $\sigma = 1.84$ S/m; $\varepsilon_r = 38.7$; $\rho = 1000$ kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 SN7349; ConvF(7.76, 7.76, 7.76); Calibrated: 31.12.2015;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.12.2015
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 113.0 V/m; Power Drift = 0.00 dB Peak SAR (extrapolated) = 26.2 W/kg SAR(1 g) = 13 W/kg; SAR(10 g) = 6.03 W/kg Maximum value of SAR (measured) = 21.2 W/kg

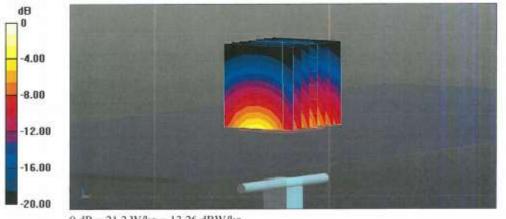

0 dB = 21.2 W/kg = 13.26 dBW/kg

Certificate No: D2450V2-839_Feb16

Page 5 of 8



Impedance Measurement Plot for Head TSL 8 Feb 2016 16:25:34 CHI Sii 3× 55.436 n 2.8659 g 138.30 pH 2 458.000 000 MHz 1 U FS ٠ De I Cit AV9 HId 3-25.200 dB 2,450.000 000 MHz CH2 \$11 108 5 dB/REF -20 dB CΔ fw9 16 Hld START 2 250,000 000 MHz STOP 2 550,000 000 MHz Certificate No: D2450V2-839_Feb16 Page 6 of 8



DASY5 Validation Report for Body TSL

Date: 09.02.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 839


Communication System: UID 0 - CW; Frequency: 2450 MHz Medium parameters used: f = 2450 MHz; $\sigma = 2$ S/m; $\epsilon_r = 52.9$; $\rho = 1000$ kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 SN7349; ConvF(7.79, 7.79, 7.79); Calibrated: 31.12.2015;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- · Electronics: DAE4 Sn601; Calibrated: 30.12.2015
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

```
Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 105.1 V/m; Power Drift = 0.02 dB
Peak SAR (extrapolated) = 25.0 W/kg
SAR(1 g) = 12.6 W/kg; SAR(10 g) = 5.87 W/kg
Maximum value of SAR (measured) = 20.4 W/kg
```

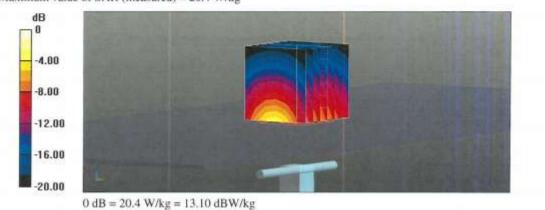


Certificate No: D2450V2-839_Feb16

Page 7 of 8



Impedance Measurement Plot for Body TSL

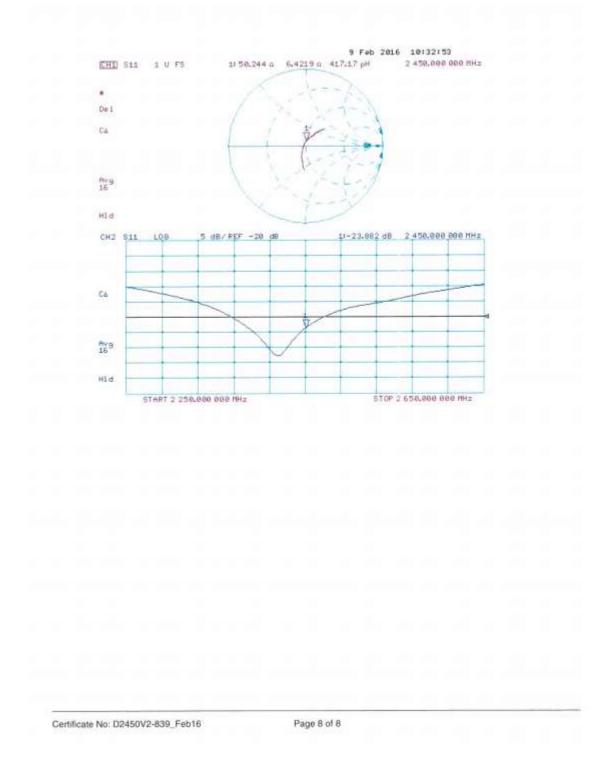



Appendix E. DAE Calibration Data

Calibration Laboratory of Schweizerischer Kalibrierdienst S Schmid & Partner Service suisse d'étalonnage C Engineering AG Servizio svizzero di taratura S Zeughausstrasse 43, 8004 Zurich, Switzerland Swiss Calibration Service Accreditation No.: SCS 0108 Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Certificate No: DAE4-905_Jun17 Auden Client CALIBRATION CERTIFICATE DAE4 - SD 000 D04 BK - SN: 905 Object Calibration procedure(s) QA CAL-06.v29 Calibration procedure for the data acquisition electronics (DAE) Calibration date: June 20, 2017 This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards ID # Cal Date (Certificate No.) Scheduled Calibration Keithley Multimeter Type 2001 SN: 0810278 09-Sep-16 (No: 19065) Sep-17 Secondary Standards 1D # Check Date (in house) Scheduled Check Auto DAE Calibration Unit SE UWS 053 AA 1001 05-Jan-17 (in house check) In house check: Jan-18 Calibrator Box V2.1 SE UMS 006 AA 1002 05-Jan-17 (in house check) In house check: Jan-18 Name Function Signature Calibrated by: Adrian Gehring Technician Approved by: Fin Bomholt Deputy Technical Manager Issued: June 20, 2017 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: DAE4-905_Jun17

Page 1 of 5



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst C Service suisse d'étalonnage Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 0108

S

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary

DAE Connector angle

data acquisition electronics information used in DASY system to align probe sensor X to the robot coordinate system.

Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a
 result from the performance test and require no uncertainty.
 - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
 - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
 - Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
 - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
 - Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
 - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
 - Input resistance: Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
 - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
 - Power consumption: Typical value for information. Supply currents in various operating modes.

Certificate No: DAE4-905_Jun17

Page 2 of 5



DC Voltage Measurement

| High Range: | 1LSB = | 6.1µV. | full range = | -100+300 mV |
|-------------|--------|--------|--------------|-------------|
| Low Range: | 1LSB = | 61nV . | full range = | -1+3mV |

| Calibration Factors | X | Y | z |
|----------------------------|-----------------------|-----------------------|-----------------------|
| High Range | 404.721 ± 0.02% (k=2) | 405.268 ± 0.02% (k=2) | 404.851 ± 0.02% (k=2) |
| Low Range | 3.98068 ± 1.50% (k=2) | 4.00246 ± 1.50% (k=2) | 3.99754 ± 1.50% (k=2) |

Connector Angle

| Connector Angle to be used in DASY system | 354.5 ° ± 1 ° |
|---|---------------|
|---|---------------|

Certificate No: DAE4-905_Jun17

Page 3 of 5



Appendix (Additional assessments outside the scope of SCS0108)

1. DC Voltage Linearity

| High Range | Reading (µV) | Difference (µV) | Error (%) |
|-------------------|--------------|-----------------|-----------|
| Channel X + Input | 199996.25 | -0.60 | -0.00 |
| Channel X + Input | 20001.67 | 0.52 | 0.00 |
| Channel X - Input | -19998.88 | 2.53 | -0.01 |
| Channel Y + Input | 199996.33 | -0.75 | -0.00 |
| Channel Y + Input | 19998.79 | -2.45 | -0.01 |
| Channel Y - Input | -20002.09 | -0.62 | 0.00 |
| Channel Z + Input | 199995.15 | -1.57 | -0.00 |
| Channel Z + Input | 19996.71 | -4.45 | -0.02 |
| Channel Z - Input | -20001.98 | -0.37 | 0.00 |
| | | | |

| Low Range | Reading (µV) | Difference (µV) | Error (%) |
|-------------------|--------------|-----------------|-----------|
| Channel X + Input | 2000.79 | 0.11 | 0.01 |
| Channel X + Input | 201.36 | 0.33 | 0.17 |
| Channel X - Input | -198.42 | 0.41 | -0.20 |
| Channel Y + Input | 2000.79 | -0.01 | -0.00 |
| Channel Y + Input | 200.91 | -0.27 | -0.13 |
| Channel Y - Input | -199.35 | -0.63 | 0.32 |
| Channel Z + Input | 2001.00 | 0.33 | 0.02 |
| Channel Z + Input | 199.44 | -1.66 | -0.83 |
| Channel Z - Input | -199.14 | -0.37 | 0.19 |
| | | | |

2. Common mode sensitivity DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| | Common mode Input Voltage (mV) | High Range Average Reading (μV) | Low Range Average Reading (µV) |
|-----------|-----------------------------------|------------------------------------|-----------------------------------|
| Channel X | 200 | 9.41 | 7.73 |
| | - 200 | -6.56 | -8.41 |
| Channel Y | 200 | 8.46 | 8.23 |
| | - 200 | -9.72 | -9.42 |
| Channel Z | 200 | 1.58 | 1.34 |
| | - 200 | -2.91 | -3.32 |

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| | Input Voltage (mV) | Channel X (µV) | Channel Y (µV) | Channel Z (µV) |
|-----------|--------------------|----------------|----------------|----------------|
| Channel X | 200 | | 5.63 | -1.36 |
| Channel Y | 200 | 9.50 | | 7.28 |
| Channel Z | 200 | 9.85 | 6.92 | |

Certificate No: DAE4-905_Jun17

Page 4 of 5



4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| | High Range (LSB) | Low Range (LSB) |
|-----------|------------------|-----------------|
| Channel X | 15903 | 17398 |
| Channel Y | 16151 | 16064 |
| Channel Z | 16372 | 16417 |

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10MΩ

| | Average (µV) | min. Offset (µV) | max. Offset (μV) | Std. Deviation (µV) |
|-----------|--------------|------------------|------------------|------------------------|
| Channel X | 1.16 | 0.21 | 1.96 | 0.29 |
| Channel Y | -0.77 | -1.64 | -0.02 | 0.31 |
| Channel Z | -0.55 | -3.10 | 1.08 | 0.51 |

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

| | Zeroing (kOhm) | Measuring (MOhm) |
|-----------|----------------|------------------|
| Channel X | 200 | 200 |
| Channel Y | 200 | 200 |
| Channel Z | 200 | 200 |

8. Low Battery Alarm Voltage (Typical values for information)

| Typical values | Alarm Level (VDC) | |
|----------------|-------------------|---|
| Supply (+ Vcc) | +7.9 | |
| Supply (- Vcc) | -7.6 | - |

9. Power Consumption (Typical values for information)

| Typical values | Switched off (mA) | Stand by (mA) | Transmitting (mA) |
|----------------|-------------------|---------------|-------------------|
| Supply (+ Vcc) | +0.01 | +6 | +14 |
| Supply (- Vcc) | -0.01 | -8 | -9 |

Certificate No: DAE4-905_Jun17

Page 5 of 5