


Appendix D

Photographs


1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

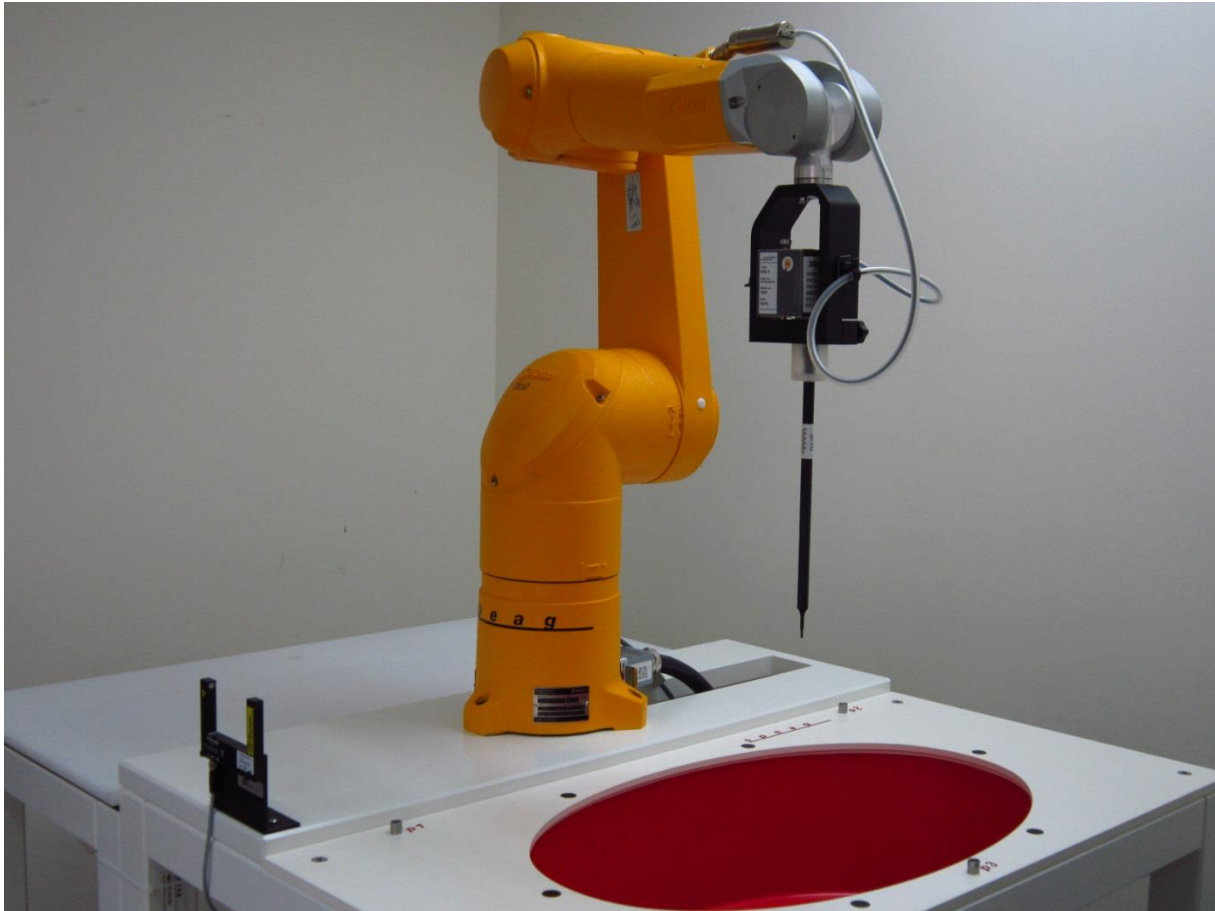





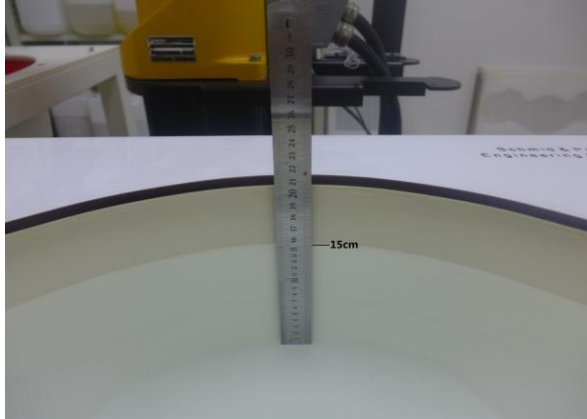

2. Photographs of Tissue Simulate Liquid





Photo 1: Tissue Simulant Liquid for Head 2450



3. Photographs of EUT test position

<p>Photo 2: Front Side 0mm</p>	<p>Photo 3: Back Side 0mm</p>
	
<p>Photo 4: Left Side 0mm</p>	<p>Photo 5: Right Side 0mm</p>
	
<p>Photo 6: Top Side 0mm</p>	<p>Photo 7: Bottom Side 0mm</p>
	

4. EUT Constructional Details

<p>Photo 1: Front View</p>	<p>Photo 2: Back View</p>
	
<p>Photo 3: Left View</p>	<p>Photo 4: Right View</p>
	
<p>Photo 5: Top View</p>	<p>Photo 6: Bottom View</p>
