

DECLARATION OF COMPLIANCE SAR RF EXPOSURE EVALUATION

| | |
|--|---|
| <p><u>Test Lab</u></p> <p>CELLTECH LABS INC. Testing and Engineering Services 1955 Moss Court Kelowna, B.C. Canada V1Y 9L3 Phone: 250-448-7047 Fax: 250-448-7046 e-mail: info@celltechlabs.com web site: www.celltechlabs.com</p> | <p><u>Applicant Information</u></p> <p>KENWOOD USA CORPORATION 3975 John Creek Court, Suite 300 Suwanee, GA 30024 United States</p> |
| <p>FCC IDENTIFIER: ALH34713110 IC IDENTIFIER: 282D-34713110 Model(s): TK-3170-K, TK-3170-K4, TK-3173-K</p> | |
| <p>Rule Part(s): FCC 47 CFR §2.1093; IC RSS-102 Issue 1 (Provisional) Test Procedure(s): FCC OET Bulletin 65, Supplement C (Edition 01-01) Device Classification: Licensed Non-Broadcast Transmitter Held to Face (TNF) Device Description: Portable FM UHF PTT Radio Transceiver</p> | |
| <p>Modulation: FM (UHF) Tx Frequency Range: 450 - 490 MHz Max. RF Output Power Measured: 36.48 dBm Conducted (450.05 MHz) 36.40 dBm Conducted (470.05 MHz) 36.37 dBm Conducted (489.95 MHz)</p> <p>Antenna Type(s) Tested: Stubby 450 - 490 MHz (P/N: KRA-17M) Stubby 470 - 512 MHz (P/N: KRA-17M2) Stubby 440 - 490 MHz (P/N: KRA-23M) Stubby 470 - 520 MHz (P/N: KRA-23M2) Whip 440 - 490 MHz (P/N: KRA-27M) Whip 470 - 520 MHz (P/N: KRA-27M2)</p> <p>Battery Type(s) Tested: Alkaline 1.5 V AA x6 (Battery Case P/N: KBP-5) (1. Duracell Procell 2850 mAh, 2. Energizer E91 2850 mAh) Li-ion 7.4 V, 1400 mAh (P/N: KNB-35L) Li-ion 7.4 V, 1400 mAh (P/N: KNB-24L) Ni-Cd 7.2 V, 1200 mAh (P/N: KNB-25A) Ni-MH 7.2 V, 2000 mAh (P/N: KNB-26N)</p> | |
| <p>Body-Worn Accessories Tested: Plastic Belt-Clip with Metal Spring (P/N: KBH-12) Speaker-Microphone (P/N: KMC-17) Headset (P/N: KHS-21)</p> | |
| <p>Max. SAR Levels Evaluated: Face-held: 3.91 W/kg (50% Duty Cycle) Body-worn: 6.16 W/kg (50% Duty Cycle)</p> | |

Celltech Labs Inc. declares under its sole responsibility that this wireless portable device has demonstrated compliance with the Specific Absorption Rate (SAR) RF exposure requirements specified in FCC 47 CFR §2.1093 and Health Canada's Safety Code 6. The device was tested in accordance with the measurement standards and procedures specified in FCC OET Bulletin 65, Supplement C (Edition 01-01) and Industry Canada RSS-102 Issue 1 (Provisional) for the Occupational / Controlled Exposure environment. All measurements were performed in accordance with the SAR system manufacturer recommendations.

I attest to the accuracy of data. All measurements were performed by me or were made under my supervision and are correct to the best of my knowledge and belief. I assume full responsibility for the completeness of these measurements and vouch for the qualifications of all persons taking them.

This test report shall not be reproduced partially, or in full, without the prior written approval of Celltech Labs Inc. The results and statements contained in this report pertain only to the device(s) evaluated.

Performed By:



Spencer Watson
Compliance Technologist
Celltech Labs Inc.

Reviewed By:



Russell W. Pipe
Senior Compliance Technologist
Celltech Labs Inc.



| TABLE OF CONTENTS | | |
|--------------------------|---|--------------|
| 1.0 | INTRODUCTION..... | 3 |
| 2.0 | DESCRIPTION OF DUT..... | 3 |
| 3.0 | SAR MEASUREMENT SYSTEM..... | 4 |
| 4.0 | MEASUREMENT SUMMARY..... | 5-11 |
| 5.0 | DETAILS OF SAR EVALUATION..... | 12 |
| 6.0 | EVALUATION PROCEDURES..... | 12 |
| 7.0 | SYSTEM PERFORMANCE CHECK..... | 13 |
| 8.0 | SIMULATED EQUIVALENT TISSUES..... | 14 |
| 9.0 | SAR SAFETY LIMITS..... | 14 |
| 10.0 | ROBOT SYSTEM SPECIFICATIONS..... | 15 |
| 11.0 | PROBE SPECIFICATION..... | 16 |
| 12.0 | PLANAR PHANTOM..... | 16 |
| 13.0 | VALIDATION PHANTOM..... | 16 |
| 14.0 | DEVICE HOLDER..... | 16 |
| 15.0 | TEST EQUIPMENT LIST..... | 17 |
| 16.0 | MEASUREMENT UNCERTAINTIES..... | 18-19 |
| 17.0 | REFERENCES..... | 20 |
| | APPENDIX A - SAR MEASUREMENT DATA..... | 21 |
| | APPENDIX B - SYSTEM PERFORMANCE CHECK DATA..... | 22 |
| | APPENDIX C - SYSTEM VALIDATION PROCEDURES..... | 23 |
| | APPENDIX D - PROBE CALIBRATION..... | 24 |
| | APPENDIX E - MEASURED FLUID DIELECTRIC PARAMETERS..... | 25 |
| | APPENDIX F - SAR TEST SETUP & DUT PHOTOGRAPHS..... | 26 |

1.0 INTRODUCTION

This measurement report demonstrates compliance of the Kenwood USA Corporation Models: TK-3170-K, TK-3170-K4, TK-3173-K Portable FM UHF PTT Radio Transceiver FCC ID: ALH34713110 with the SAR (Specific Absorption Rate) RF exposure requirements specified in FCC 47 CFR §2.1093 (see reference [1]), and Health Canada's Safety Code 6 (see reference [2]) for the Occupational / Controlled Exposure environment. The measurement procedures described in FCC OET Bulletin 65, Supplement C (Edition 01-01) (see reference [3]) and IC RSS-102 Issue 1 (Provisional) (see reference [4]), were employed. A description of the product, operating configuration, detailed summary of the test results, methodology and procedures used in the evaluation, equipment used, and the various provisions of the rules are included within this test report.

2.0 DESCRIPTION OF DEVICE UNDER TEST (DUT)

| | | | | |
|--------------------------------------|---|---------------------|--------------------|----------------------------|
| FCC Rule Part(s) | 47 CFR §2.1093 | | | |
| IC Rule Part(s) | RSS-102 Issue 1 (Provisional) | | | |
| Test Procedure(s) | FCC OET Bulletin 65, Supplement C (Edition 01-01) | | | |
| Device Classification | Licensed Non-Broadcast Transmitter Held to Face (TNF) | | | |
| Device Type | Portable FM UHF PTT Radio Transceiver | | | |
| FCC IDENTIFIER | ALH34713110 | | | |
| IC IDENTIFIER | 282D-34713110 | | | |
| Model(s) | TK-3170-K | TK-3170-K4 | TK-3173-K | |
| Serial No. | 1S-U1-21 | Identical Prototype | | |
| Modulation | FM (UHF) | | | |
| Tx Frequency Range | 450 - 490 MHz | | | |
| Max. RF Output Power Measured | 36.48 dBm | Conducted | 450.05 MHz | |
| | 36.40 dBm | Conducted | 470.05 MHz | |
| | 36.37 dBm | Conducted | 489.95 MHz | |
| Antenna Type(s) Tested | Stubby | KRA-17M | Length: 82 mm | 450 - 490 MHz |
| | Stubby | KRA-17M2 | Length: 78 mm | 470 - 512 MHz |
| | Stubby | KRA-23M | Length: 83 mm | 440 - 490 MHz |
| | Stubby | KRA-23M2 | Length: 83 mm | 470 - 520 MHz |
| | Whip | KRA-27M | Length: 153 mm | 400 - 490 MHz |
| | Whip | KRA-27M2 | Length: 143 mm | 470 - 520 MHz |
| Battery Type(s) Tested | Alkaline | 1.5 V AA (x6) | Duracell 2850 mAh | Battery Case P/N: KBP-5 |
| | | | Energizer 2850 mAh | |
| | Li-ion | 7.4 V, 1400 mAh | | P/N: KNB-35L |
| | Li-ion | 7.4 V, 1400 mAh | | P/N: KNB-24L |
| | Ni-Cd | 7.2 V, 1200 mAh | | P/N: KNB-25A |
| Ni-MH | 7.2 V, 2000 mAh | | P/N: KNB-26N | |
| Body-Worn Accessories Tested | Plastic Belt-Clip with Metal Spring | | P/N: KBH-12 | |
| | Speaker-Microphone | | P/N: KMC-17 | |
| | Headset | | P/N: KHS-21 | |

3.0 SAR MEASUREMENT SYSTEM

Celltech Labs Inc. SAR measurement facility utilizes the Dosimetric Assessment System (DASY™) manufactured by Schmid & Partner Engineering AG (SPEAG™) of Zurich, Switzerland. The DASY4 measurement system is comprised of the measurement server, robot controller, computer, near-field probe, probe alignment sensor, specific anthropomorphic mannequin (SAM) phantom, and various planar phantoms for brain and/or body SAR evaluations. The robot is a six-axis industrial robot performing precise movements to position the probe to the location (points) of maximum electromagnetic field (EMF). A cell controller system contains the power supply, robot controller, teach pendant (Joystick), and remote control, is used to drive the robot motors. The Staubli robot is connected to the cell controller to allow software manipulation of the robot. A data acquisition electronic (DAE) circuit performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. is connected to the Electro-optical coupler (EOC). The EOC performs the conversion from the optical into digital electric signal of the DAE and transfers data to the DASY4 measurement server. The DAE4 utilizes a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16-bit AD-converter and a command decoder and control logic unit. Transmission to the DASY4 measurement server is accomplished through an optical downlink for data and status information and an optical uplink for commands and clock lines. The mechanical probe-mounting device includes two different sensor systems for frontal and sidewise probe contacts. The sensor systems are also used for mechanical surface detection and probe collision detection. The robot uses its own controller with a built in VME-bus computer.



DASY4 SAR Measurement System with validation phantom



DASY4 SAR Measurement System with Plexiglas planar phantom

4.0 MEASUREMENT SUMMARY

FACE-HELD SAR EVALUATION RESULTS

| Freq. (MHz) | Chan. | Test Mode | Antenna Type | Antenna Part No. | Battery Type | Separation Distance to Planar Phantom (cm) | Cond. Power Before Test (dBm) | Measured SAR 1g (W/kg) | | SAR Drift During Test (dB) | Scaled SAR 1g (W/kg) | |
|-------------|-------|-----------|--------------|------------------|----------------|--|-------------------------------|------------------------|------|----------------------------|----------------------|------|
| | | | | | | | | Duty Cycle | | | Duty Cycle | |
| | | | | | | | | 100% | 50% | | 100% | 50% |
| 470.05 | Mid | CW | Stubby | KRA-17M | KBP-5 Duracell | 2.5 | 36.21 | 6.36 | 3.18 | -0.895 | 7.82 | 3.91 |
| 470.05 | Mid | CW | Stubby | KRA-17M | KNB-35L Li-ion | 2.5 | 36.34 | 7.23 | 3.62 | -0.00492 | 7.24 | 3.62 |
| 470.05 | Mid | CW | Stubby | KRA-17M | KNB-24L Li-ion | 2.5 | 36.27 | 6.91 | 3.46 | -0.161 | 7.17 | 3.59 |
| 470.05 | Mid | CW | Stubby | KRA-17M | KNB-25A Ni-Cd | 2.5 | 36.36 | 7.24 | 3.62 | -0.138 | 7.47 | 3.74 |
| 470.05 | Mid | CW | Stubby | KRA-17M | KNB-26N Ni-MH | 2.5 | 36.33 | 7.04 | 3.52 | -0.130 | 7.25 | 3.63 |
| 489.95 | High | CW | Stubby | KRA-17M2 | KBP-5 Duracell | 2.5 | 36.05 | 5.20 | 2.60 | -1.12 | 6.73 | 3.36 |
| 470.05 | Mid | CW | Whip | KRA-27M | KBP-5 Duracell | 2.5 | 36.22 | 5.68 | 2.84 | -0.842 | 6.90 | 3.45 |
| 470.05 | Mid | CW | Whip | KRA-27M | KNB-35L Li-ion | 2.5 | 36.35 | 6.20 | 3.10 | -0.137 | 6.40 | 3.20 |
| 470.05 | Mid | CW | Whip | KRA-27M | KNB-24L Li-ion | 2.5 | 36.18 | 5.87 | 2.94 | -0.241 | 6.20 | 3.10 |
| 470.05 | Mid | CW | Whip | KRA-27M | KNB-25A Ni-Cd | 2.5 | 36.26 | 6.15 | 3.08 | -0.211 | 6.46 | 3.23 |
| 470.05 | Mid | CW | Whip | KRA-27M | KNB-26N Ni-MH | 2.5 | 36.29 | 6.16 | 3.08 | -0.222 | 6.48 | 3.24 |
| 489.95 | High | CW | Whip | KRA-27M2 | KBP-5 Duracell | 2.5 | 36.02 | 5.00 | 2.50 | -1.03 | 6.34 | 3.17 |

ANSI / IEEE C95.1 1999 - SAFETY LIMIT
Spatial Peak - Controlled Exposure / Occupational
BRAIN: 8.0 W/kg (averaged over 1 gram)

| | | | | | |
|--|--------------------|------|-----------------------------|-----------------------------|------|
| Test Date | October 20, 2004 | | Relative Humidity | 34 | % |
| Measured Fluid Type | 450 MHz Brain | | Atmospheric Pressure | 101.5 | kPa |
| Dielectric Constant ϵ_r | IEEE Target | | Ambient Temperature | 23.6 | °C |
| | 43.5 | ± 5% | 44.0 | Fluid Temperature | 22.9 |
| Conductivity σ (mho/m) | IEEE Target | | Fluid Depth | ≥ 15 | cm |
| | 0.87 | ± 5% | 0.87 | ρ (Kg/m ³) | 1000 |

Note(s):

- The measurement results were obtained with the DUT tested in the conditions described in this report. Detailed measurement data and plots showing the maximum SAR location of the DUT are reported in Appendix A.
- If the scaled SAR levels at the mid channel (50% duty cycle) were ≥ 3 dB below the SAR limit, SAR evaluation for the low and high channels was optional per FCC OET Bulletin 65, Supplement C, Edition 01-01 (see reference [3]).
- The power drifts measured by the DASY4 system for the duration of the SAR evaluations were added to the measured SAR levels to report scaled SAR results as shown in the above table.
- The ambient and fluid temperatures were measured prior to, and during, the fluid dielectric parameter check and the SAR evaluation. The temperatures reported were consistent for all measurement periods.
- The dielectric parameters of the simulated tissue mixture were measured prior to the evaluation using an HP 85070C Dielectric Probe Kit and an HP 8753E Network Analyzer (see Appendix E for printout of measured fluid dielectric parameters).
- The SAR evaluations were performed within 24 hours of the system performance check.

MEASUREMENT SUMMARY (Cont.)

FACE-HELD SAR EVALUATION RESULTS

| Freq. (MHz) | Chan. | Test Mode | Antenna Type | Antenna Part No. | Battery Type | Separation Distance to Planar Phantom (cm) | Cond. Power Before Test (dBm) | Measured SAR 1g (W/kg) | | SAR Drift During Test (dB) | Scaled SAR 1g (W/kg) | |
|-------------|-------|-----------|--------------|------------------|----------------|--|-------------------------------|------------------------|------|----------------------------|----------------------|------|
| | | | | | | | | Duty Cycle | | | Duty Cycle | |
| | | | | | | | | 100% | 50% | | 100% | 50% |
| 470.05 | Mid | CW | Stubby | KRA-23M | KBP-5 Duracell | 2.5 | 36.16 | 6.02 | 3.01 | -0.979 | 7.54 | 3.77 |
| 470.05 | Mid | CW | Stubby | KRA-23M | KNB-35L Li-ion | 2.5 | 36.25 | 6.88 | 3.44 | -0.123 | 7.08 | 3.54 |
| 470.05 | Mid | CW | Stubby | KRA-23M | KNB-24L Li-ion | 2.5 | 36.18 | 6.42 | 3.21 | -0.308 | 6.89 | 3.45 |
| 470.05 | Mid | CW | Stubby | KRA-23M | KNB-25A Ni-Cd | 2.5 | 36.26 | 6.64 | 3.32 | -0.562 | 7.56 | 3.78 |
| 470.05 | Mid | CW | Stubby | KRA-23M | KNB-26N Ni-MH | 2.5 | 36.23 | 6.76 | 3.38 | -0.582 | 7.73 | 3.86 |
| 489.95 | High | CW | Stubby | KRA-23M2 | KNB-26N Ni-MH | 2.5 | 36.25 | 5.73 | 2.87 | -0.599 | 6.58 | 3.29 |

ANSI / IEEE C95.1 1999 - SAFETY LIMIT
Spatial Peak - Controlled Exposure / Occupational
BRAIN: 8.0 W/kg (averaged over 1 gram)

| | | | | | |
|--|--------------------|-----------------|-----------------------------|-----------------------------|------|
| Test Date | October 21, 2004 | | Relative Humidity | 33 | % |
| Measured Fluid Type | 450 MHz Brain | | Atmospheric Pressure | 101.9 | kPa |
| Dielectric Constant ϵ_r | IEEE Target | Measured | Ambient Temperature | 23.7 | °C |
| | 43.5 | ± 5% | 43.5 | Fluid Temperature | 23.3 |
| Conductivity σ (mho/m) | IEEE Target | Measured | Fluid Depth | ≥ 15 | cm |
| | 0.87 | ± 5% | 0.86 | ρ (Kg/m ³) | 1000 |

Note(s):

- The measurement results were obtained with the DUT tested in the conditions described in this report. Detailed measurement data and plots showing the maximum SAR location of the DUT are reported in Appendix A.
- If the scaled SAR levels at the mid channel (50% duty cycle) were ≥ 3 dB below the SAR limit, SAR evaluation for the low and high channels was optional per FCC OET Bulletin 65, Supplement C, Edition 01-01 (see reference [3]).
- The power drifts measured by the DASY4 system for the duration of the SAR evaluations were added to the measured SAR levels to report scaled SAR results as shown in the above table.
- The ambient and fluid temperatures were measured prior to, and during, the fluid dielectric parameter check and the SAR evaluation. The temperatures reported were consistent for all measurement periods.
- The dielectric parameters of the simulated tissue mixture were measured prior to the evaluation using an HP 85070C Dielectric Probe Kit and an HP 8753E Network Analyzer (see Appendix E for printout of measured fluid dielectric parameters).
- The SAR evaluations were performed within 24 hours of the system performance check.

MEASUREMENT SUMMARY (Cont.)

BODY-WORN SAR EVALUATION RESULTS

| Freq. (MHz) | Chan. | Test Mode | Antenna Type | Antenna Part No. | Battery Type | Body-worn Accessories | Separation Distance to Planar Phantom (cm) | Cond. Power Before Test (dBm) | Measured SAR 1g (W/kg) | | SAR Drift During Test (dB) | Scaled SAR 1g (W/kg) | |
|-------------|-------|-----------|--------------|------------------|----------------|-----------------------|--|-------------------------------|------------------------|------|----------------------------|----------------------|------|
| | | | | | | | | | Duty Cycle | | | Duty Cycle | |
| | | | | | | | | | 100% | 50% | | 100% | 50% |
| 470.05 | Mid | CW | Whip | KRA-27M | KBP-5 Duracell | Speaker-Mic Belt-Clip | 1.0 | 36.15 | 8.74 | 4.37 | -0.904 | 10.8 | 5.38 |
| 470.05 | Mid | CW | Whip | KRA-27M | KNB-35L Li-ion | Speaker-Mic Belt-Clip | 1.4 | 36.20 | 9.67 | 4.84 | -0.169 | 10.1 | 5.03 |
| 470.05 | Mid | CW | Whip | KRA-27M | KNB-24L Li-ion | Speaker-Mic Belt-Clip | 1.4 | 36.18 | 8.75 | 4.38 | -0.304 | 9.38 | 4.69 |
| 470.05 | Mid | CW | Whip | KRA-27M | KNB-25A Ni-Cd | Speaker-Mic Belt-Clip | 0.9 | 36.25 | 9.70 | 4.85 | -0.307 | 10.4 | 5.21 |
| 470.05 | Mid | CW | Whip | KRA-27M | KNB-26N Ni-MH | Speaker-Mic Belt-Clip | 0.9 | 36.28 | 9.46 | 4.73 | -0.285 | 10.1 | 5.05 |
| 450.05 | Low | CW | Whip | KRA-27M | KBP-5 Duracell | Speaker-Mic Belt-Clip | 1.0 | 36.30 | 6.90 | 3.45 | -0.615 | 7.95 | 3.97 |
| 489.95 | High | CW | Whip | KRA-27M | KBP-5 Duracell | Speaker-Mic Belt-Clip | 1.0 | 36.05 | 7.41 | 3.71 | -0.953 | 9.23 | 4.61 |
| 489.95 | High | CW | Whip | KRA-27M2 | KBP-5 Duracell | Speaker-Mic Belt-Clip | 1.0 | 36.01 | 8.05 | 4.03 | -1.06 | 10.3 | 5.14 |

ANSI / IEEE C95.1 1999 - SAFETY LIMIT
Spatial Peak - Controlled Exposure / Occupational
BODY: 8.0 W/kg (averaged over 1 gram)

| | | | | | |
|--|--------------------|------|-----------------------------|-----------------------------|------|
| Test Date | October 21, 2004 | | Relative Humidity | 32 | % |
| Measured Fluid Type | 450 MHz Body | | Atmospheric Pressure | 101.8 | kPa |
| Dielectric Constant ϵ_r | IEEE Target | | Ambient Temperature | 24.5 | °C |
| | 56.7 | ± 5% | 57.1 | Fluid Temperature | 23.6 |
| Conductivity σ (mho/m) | IEEE Target | | Fluid Depth | ≥ 15 | cm |
| | 0.94 | ± 5% | 0.91 | ρ (Kg/m ³) | 1000 |

Note(s):

- The measurement results were obtained with the DUT tested in the conditions described in this report. Detailed measurement data and plots showing the maximum SAR location of the DUT are reported in Appendix A.
- If the scaled SAR levels at the mid channel (50% duty cycle) were ≥ 3 dB below the SAR limit, SAR evaluation for the low and high channels was optional per FCC OET Bulletin 65, Supplement C, Edition 01-01 (see reference [3]).
- The power drifts measured by the DAS4 system for the duration of the SAR evaluations were added to the measured SAR levels to report scaled SAR results as shown in the above table.
- The ambient and fluid temperatures were measured prior to, and during, the fluid dielectric parameter check and the SAR evaluation. The temperatures reported were consistent for all measurement periods.
- The dielectric parameters of the simulated tissue mixture were measured prior to the evaluation using an HP 85070C Dielectric Probe Kit and an HP 8753E Network Analyzer (see Appendix E for printout of measured fluid dielectric parameters).
- The SAR evaluations were performed within 24 hours of the system performance check.

MEASUREMENT SUMMARY (Cont.)

BODY-WORN SAR EVALUATION RESULTS

| Freq. (MHz) | Chan. | Test Mode | Antenna Type | Antenna Part No. | Battery Type | Body-worn Accessories | Separation Distance to Planar Phantom (cm) | Cond. Power Before Test (dBm) | Measured SAR 1g (W/kg) | | SAR Drift During Test (dB) | Scaled SAR 1g (W/kg) | |
|-------------|-------|-----------|--------------|------------------|----------------|-----------------------|--|-------------------------------|------------------------|------|----------------------------|----------------------|------|
| | | | | | | | | | Duty Cycle | | | Duty Cycle | |
| | | | | | | | | | 100% | 50% | | 100% | 50% |
| 470.05 | Mid | CW | Whip | KRA-27M | KBP-5 Duracell | Headset Belt-Clip | 1.0 | 36.26 | 7.73 | 3.87 | -0.845 | 9.39 | 4.70 |
| 470.05 | Mid | CW | Whip | KRA-27M | KNB-35L Li-ion | Headset Belt-Clip | 1.4 | 36.36 | 8.68 | 4.34 | -0.125 | 8.93 | 4.47 |
| 470.05 | Mid | CW | Whip | KRA-27M | KNB-24L Li-ion | Headset Belt-Clip | 1.4 | 36.32 | 8.40 | 4.20 | -0.293 | 8.99 | 4.49 |
| 470.05 | Mid | CW | Whip | KRA-27M | KNB-25A Ni-Cd | Headset Belt-Clip | 0.9 | 36.35 | 9.25 | 4.63 | -0.274 | 9.85 | 4.93 |
| 470.05 | Mid | CW | Whip | KRA-27M | KNB-26N Ni-MH | Headset Belt-Clip | 0.9 | 36.36 | 8.62 | 4.31 | -0.231 | 9.09 | 4.55 |
| 450.05 | Low | CW | Whip | KRA-27M | KNB-25A Ni-Cd | Headset Belt-Clip | 0.9 | 36.47 | 7.03 | 3.52 | -0.0683 | 7.14 | 3.57 |
| 489.95 | High | CW | Whip | KRA-27M | KNB-25A Ni-Cd | Headset Belt-Clip | 0.9 | 36.37 | 8.51 | 4.26 | -0.453 | 9.45 | 4.72 |
| 489.95 | High | CW | Whip | KRA-27M2 | KNB-25A Ni-Cd | Headset Belt-Clip | 0.9 | 36.33 | 9.06 | 4.53 | -0.448 | 10.0 | 5.02 |
| 470.05 | Mid | CW | Stubby | KRA-23M | KBP-5 Duracell | Headset Belt-Clip | 1.0 | 36.24 | 8.09 | 4.05 | -1.01 | 10.2 | 5.10 |
| 470.05 | Mid | CW | Stubby | KRA-23M | KNB-35L Li-ion | Headset Belt-Clip | 1.4 | 36.37 | 10.5 | 5.25 | -0.293 | 11.2 | 5.62 |
| 470.05 | Mid | CW | Stubby | KRA-23M | KNB-24L Li-ion | Headset Belt-Clip | 1.4 | 36.34 | 9.00 | 4.50 | -0.468 | 10.0 | 5.01 |
| 470.05 | Mid | CW | Stubby | KRA-23M | KNB-25A Ni-Cd | Headset Belt-Clip | 0.9 | 36.29 | 9.04 | 4.52 | -0.453 | 10.0 | 5.02 |
| 470.05 | Mid | CW | Stubby | KRA-23M | KNB-26N Ni-MH | Headset Belt-Clip | 0.9 | 36.28 | 9.72 | 4.86 | -0.597 | 11.2 | 5.58 |
| 450.05 | Low | CW | Stubby | KRA-23M | KNB-35L Li-ion | Headset Belt-Clip | 1.4 | 36.43 | 6.96 | 3.48 | 0.0469 | 6.96 | 3.48 |
| 489.95 | High | CW | Stubby | KRA-23M | KNB-35L Li-ion | Headset Belt-Clip | 1.4 | 36.18 | 7.40 | 3.70 | -0.323 | 7.97 | 3.99 |
| 489.95 | High | CW | Stubby | KRA-23M2 | KNB-35L Li-ion | Headset Belt-Clip | 1.4 | 36.21 | 9.54 | 4.77 | -0.311 | 10.2 | 5.12 |

ANSI / IEEE C95.1 1999 - SAFETY LIMIT
Spatial Peak - Controlled Exposure / Occupational
BODY: 8.0 W/kg (averaged over 1 gram)

| | | | | | |
|--|--------------------|-----------------|-----------------------------|---|------|
| Test Date | October 22, 2004 | | Relative Humidity | 33 | % |
| Measured Fluid Type | 450 MHz Body | | Atmospheric Pressure | 101.3 | kPa |
| Dielectric Constant ϵ_r | IEEE Target | Measured | Ambient Temperature | 23.9 | °C |
| | 56.7 | ± 5% | 56.6 | Fluid Temperature | 23.1 |
| Conductivity σ (mho/m) | IEEE Target | Measured | Fluid Depth | ≥ 15 | cm |
| | 0.94 | ± 5% | 0.90 | ρ (Kg/m³) | 1000 |

Note(s):

- The measurement results were obtained with the DUT tested in the conditions described in this report. Detailed measurement data and plots showing the maximum SAR location of the DUT are reported in Appendix A.
- If the scaled SAR levels at the mid channel (50% duty cycle) were ≥ 3 dB below the SAR limit, SAR evaluation for the low and high channels was optional per FCC OET Bulletin 65, Supplement C, Edition 01-01 (see reference [3]).
- The power drifts measured by the DASY4 system for the duration of the SAR evaluations were added to the measured SAR levels to report scaled SAR results as shown in the above table.
- The ambient and fluid temperatures were measured prior to, and during, the fluid dielectric parameter check and the SAR evaluation. The temperatures reported were consistent for all measurement periods.
- The dielectric parameters of the simulated tissue mixture were measured prior to the evaluation using an HP 85070C Dielectric Probe Kit and an HP 8753E Network Analyzer (see Appendix E for printout of measured fluid dielectric parameters).
- The SAR evaluations were performed within 24 hours of the system performance check.

MEASUREMENT SUMMARY (Cont.)

BODY-WORN SAR EVALUATION RESULTS

| Test Date(s) | Freq. (MHz) | Chan. | Test Mode | Antenna Type | Antenna Part No. | Battery Type | Body-worn Accessories | Separation Distance to Planar Phantom (cm) | Cond. Power Before Test (dBm) | Measured SAR 1g (W/kg) | | SAR Drift During Test (dB) | Scaled SAR 1g (W/kg) | |
|--------------|-------------|-------|-----------|--------------|------------------|----------------|-----------------------|--|-------------------------------|------------------------|------|----------------------------|----------------------|------|
| | | | | | | | | | | Duty Cycle | | | Duty Cycle | |
| | | | | | | | | | | 100% | 50% | | 100% | 50% |
| Oct-22 | 470.05 | Mid | CW | Stubby | KRA-23M | KBP-5 Duracell | Speaker-Mic Belt-Clip | 1.0 | 36.22 | 8.08 | 4.04 | -1.18 | 10.6 | 5.30 |
| Oct-22 | 470.05 | Mid | CW | Stubby | KRA-23M | KNB-35L Li-ion | Speaker-Mic Belt-Clip | 1.4 | 36.31 | 10.3 | 5.15 | -0.328 | 11.1 | 5.55 |
| Oct-22 | 470.05 | Mid | CW | Stubby | KRA-23M | KNB-24L Li-ion | Speaker-Mic Belt-Clip | 1.4 | 36.24 | 9.17 | 4.59 | -0.501 | 10.3 | 5.15 |
| Oct-22 | 470.05 | Mid | CW | Stubby | KRA-23M | KNB-25A Ni-Cd | Speaker-Mic Belt-Clip | 0.9 | 36.30 | 9.24 | 4.62 | -0.531 | 10.4 | 5.22 |
| Oct-22 | 470.05 | Mid | CW | Stubby | KRA-23M | KNB-26N Ni-MH | Speaker-Mic Belt-Clip | 0.9 | 36.27 | 9.00 | 4.50 | -0.536 | 10.2 | 5.09 |
| Oct-22 | 450.05 | Low | CW | Stubby | KRA-23M | KNB-35L Li-ion | Speaker-Mic Belt-Clip | 1.4 | 36.39 | 7.38 | 3.69 | 0.0709 | 7.38 | 3.69 |
| Oct-22 | 489.95 | High | CW | Stubby | KRA-23M | KNB-35L Li-ion | Speaker-Mic Belt-Clip | 1.4 | 36.15 | 6.95 | 3.48 | -0.381 | 7.59 | 3.79 |
| Oct-23 | 489.95 | High | CW | Stubby | KRA-23M2 | KNB-35L Li-ion | Speaker-Mic Belt-Clip | 1.4 | 36.24 | 9.22 | 4.61 | -0.291 | 9.86 | 4.93 |

ANSI / IEEE C95.1 1999 - SAFETY LIMIT
Spatial Peak - Controlled Exposure / Occupational
BODY: 8.0 W/kg (averaged over 1 gram)

| Test Date(s) | October 22, 2004 | | October 23, 2004 | | Test Date(s) | Oct-22 | Oct-23 | Unit |
|----------------------------------|------------------|----------|------------------|----------|-----------------------------|--------|--------|------|
| Measured Fluid Type | 450 MHz Body | | 450 MHz Body | | Relative Humidity | 33 | 31 | % |
| Dielectric Constant ϵ_r | IEEE Target | Measured | IEEE Target | Measured | Atmospheric Pressure | 101.3 | 101.7 | kPa |
| | 56.7 ± 5% | 56.6 | 56.7 ± 5% | 56.8 | Ambient Temperature | 23.9 | 23.2 | °C |
| Conductivity σ (mho/m) | 450 MHz Body | | 450 MHz Body | | Fluid Temperature | 23.1 | 23.2 | °C |
| | IEEE Target | Measured | IEEE Target | Measured | Fluid Depth | ≥ 15 | ≥ 15 | cm |
| | 0.94 ± 5% | 0.90 | 0.94 ± 5% | 0.90 | ρ (Kg/m ³) | 1000 | | |

Note(s):

- The measurement results were obtained with the DUT tested in the conditions described in this report. Detailed measurement data and plots showing the maximum SAR location of the DUT are reported in Appendix A.
- If the scaled SAR levels at the mid channel (50% duty cycle) were ≥ 3 dB below the SAR limit, SAR evaluation for the low and high channels was optional per FCC OET Bulletin 65, Supplement C, Edition 01-01 (see reference [3]).
- The power drifts measured by the DASY4 system for the duration of the SAR evaluations were added to the measured SAR levels to report scaled SAR results as shown in the above table.
- The ambient and fluid temperatures were measured prior to, and during, the fluid dielectric parameter check and the SAR evaluation. The temperatures reported were consistent for all measurement periods.
- The dielectric parameters of the simulated tissue mixture were measured prior to the evaluation using an HP 85070C Dielectric Probe Kit and an HP 8753E Network Analyzer (see Appendix E for printout of measured fluid dielectric parameters).
- The SAR evaluations were performed within 24 hours of the system performance check.

MEASUREMENT SUMMARY (Cont.)

BODY-WORN SAR EVALUATION RESULTS

| Freq. (MHz) | Chan. | Test Mode | Antenna Type | Antenna Part No. | Battery Type | Body-worn Accessories | Separation Distance to Planar Phantom (cm) | Cond. Power Before Test (dBm) | Measured SAR 1g (W/kg) | | SAR Drift During Test (dB) | Scaled SAR 1g (W/kg) | |
|-------------|-------|-----------|--------------|------------------|----------------|-----------------------|--|-------------------------------|------------------------|------|----------------------------|----------------------|------|
| | | | | | | | | | Duty Cycle | | | Duty Cycle | |
| | | | | | | | | | 100% | 50% | | 100% | 50% |
| 470.05 | Mid | CW | Stubby | KRA-17M | KBP-5 Duracell | Headset Belt-Clip | 1.0 | 36.29 | 8.81 | 4.41 | -1.07 | 11.3 | 5.64 |
| 470.05 | Mid | CW | Stubby | KRA-17M | KNB-35L Li-ion | Headset Belt-Clip | 1.4 | 36.40 | 11.6 | 5.8 | -0.141 | 12.0 | 5.99 |
| 470.05 | Mid | CW | Stubby | KRA-17M | KNB-24L Li-ion | Headset Belt-Clip | 1.4 | 36.29 | 10.1 | 5.05 | -0.370 | 11.0 | 5.50 |
| 470.05 | Mid | CW | Stubby | KRA-17M | KNB-25A Ni-Cd | Headset Belt-Clip | 0.9 | 36.35 | 10.5 | 5.25 | -0.358 | 11.4 | 5.70 |
| 470.05 | Mid | CW | Stubby | KRA-17M | KNB-26N Ni-MH | Headset Belt-Clip | 0.9 | 36.39 | 10.7 | 5.35 | -0.453 | 11.9 | 5.94 |
| 450.05 | Low | CW | Stubby | KRA-17M | KNB-35L Li-ion | Headset Belt-Clip | 1.4 | 36.48 | 6.03 | 3.02 | -0.0295 | 6.07 | 3.04 |
| 489.95 | High | CW | Stubby | KRA-17M | KNB-35L Li-ion | Headset Belt-Clip | 1.4 | 36.27 | 8.80 | 4.40 | -0.368 | 9.58 | 4.79 |
| 489.95 | High | CW | Stubby | KRA-17M2 | KNB-35L Li-ion | Headset Belt-Clip | 1.4 | 36.24 | 10.2 | 5.10 | -0.250 | 10.8 | 5.40 |

ANSI / IEEE C95.1 1999 - SAFETY LIMIT
Spatial Peak - Controlled Exposure / Occupational
BODY: 8.0 W/kg (averaged over 1 gram)

| | | | | | | |
|--|--------------------|------|-----------------|---|-------|-----|
| Test Date | October 23, 2004 | | | Relative Humidity | 31 | % |
| Measured Fluid Type | 450 MHz Body | | | Atmospheric Pressure | 101.7 | kPa |
| Dielectric Constant ϵ_r | IEEE Target | | Measured | Ambient Temperature | 23.2 | °C |
| | 56.7 | ± 5% | 56.8 | Fluid Temperature | 23.2 | °C |
| Conductivity σ (mho/m) | IEEE Target | | Measured | Fluid Depth | ≥ 15 | cm |
| | 0.94 | ± 5% | 0.90 | ρ (Kg/m³) | 1000 | |

Note(s):

- The measurement results were obtained with the DUT tested in the conditions described in this report. Detailed measurement data and plots showing the maximum SAR location of the DUT are reported in Appendix A.
- If the scaled SAR levels at the mid channel (50% duty cycle) were ≥ 3 dB below the SAR limit, SAR evaluation for the low and high channels was optional per FCC OET Bulletin 65, Supplement C, Edition 01-01 (see reference [3]).
- The power drifts measured by the DASY4 system for the duration of the SAR evaluations were added to the measured SAR levels to report scaled SAR results as shown in the above table.
- The ambient and fluid temperatures were measured prior to, and during, the fluid dielectric parameter check and the SAR evaluation. The temperatures reported were consistent for all measurement periods.
- The dielectric parameters of the simulated tissue mixture were measured prior to the evaluation using an HP 85070C Dielectric Probe Kit and an HP 8753E Network Analyzer (see Appendix E for printout of measured fluid dielectric parameters).
- The SAR evaluations were performed within 24 hours of the system performance check.

MEASUREMENT SUMMARY (Cont.)

BODY-WORN SAR EVALUATION RESULTS

| Test Date | Freq. (MHz) | Chan. | Test Mode | Antenna Type | Antenna Part No. | Battery Type | Body-worn Accessories | Separation Distance to Planar Phantom (cm) | Cond. Power Before Test (dBm) | Measured SAR 1g (W/kg) | | SAR Drift During Test (dB) | Scaled SAR 1g (W/kg) | |
|-----------|-------------|-------|-----------|--------------|------------------|------------------|-----------------------|--|-------------------------------|------------------------|------|----------------------------|----------------------|------|
| | | | | | | | | | | Duty Cycle | | | Duty Cycle | |
| | | | | | | | | | | 100% | 50% | | 100% | 50% |
| Oct-23 | 470.05 | Mid | CW | Stubby | KRA-17M | KBP-5 Duracell | Speaker-Mic Belt-Clip | 1.0 | 36.27 | 9.03 | 4.52 | -1.08 | 11.6 | 5.79 |
| Oct-23 | 470.05 | Mid | CW | Stubby | KRA-17M | KNB-35L Li-ion | Speaker-Mic Belt-Clip | 1.4 | 36.38 | 11.7 | 5.85 | -0.222 | 12.3 | 6.16 |
| Oct-24 | 470.05 | Mid | CW | Stubby | KRA-17M | KNB-24L Li-ion | Speaker-Mic Belt-Clip | 1.4 | 36.26 | 10.3 | 5.15 | -0.402 | 11.3 | 5.65 |
| Oct-24 | 470.05 | Mid | CW | Stubby | KRA-17M | KNB-25A Ni-Cd | Speaker-Mic Belt-Clip | 0.9 | 36.40 | 11.0 | 5.50 | -0.443 | 12.2 | 6.09 |
| Oct-24 | 470.05 | Mid | CW | Stubby | KRA-17M | KNB-26N Ni-MH | Speaker-Mic Belt-Clip | 0.9 | 36.36 | 10.7 | 5.35 | -0.429 | 11.8 | 5.91 |
| Oct-24 | 450.05 | Low | CW | Stubby | KRA-17M | KNB-35L Li-ion | Speaker-Mic Belt-Clip | 1.4 | 36.36 | 6.47 | 3.24 | -0.0440 | 6.54 | 3.27 |
| Oct-24 | 489.95 | High | CW | Stubby | KRA-17M | KNB-35L Li-ion | Speaker-Mic Belt-Clip | 1.4 | 36.15 | 7.97 | 3.99 | -0.435 | 8.81 | 4.40 |
| Oct-24 | 489.95 | High | CW | Stubby | KRA-17M2 | KNB-35L Li-ion | Speaker-Mic Belt-Clip | 1.4 | 36.16 | 9.59 | 4.80 | -0.304 | 10.3 | 5.14 |
| Oct-24 | 470.05 | Mid | CW | Stubby | KRA-17M | KBP-5 Energizer* | Speaker-Mic Belt-Clip | 1.0 | 36.13 | 9.19 | 4.60 | -1.09 | 11.8 | 5.91 |

ANSI / IEEE C95.1 1999 - SAFETY LIMIT
Spatial Peak - Controlled Exposure / Occupational
BODY: 8.0 W/kg (averaged over 1 gram)

| Test Date(s) | October 23, 2004 | | October 24, 2004 | | Test Date(s) | Oct-23 | Oct-24 | Unit |
|----------------------------------|------------------|-----------|------------------|----------|-----------------------------|-----------|-----------|--------------------|
| Measured Fluid Type | 450 MHz Body | | 450 MHz Body | | Relative Humidity | 31 | 31 | % |
| Dielectric Constant ϵ_r | IEEE Target | Measured | IEEE Target | Measured | Atmospheric Pressure | 101.7 | 102.2 | kPa |
| | 56.7 | $\pm 5\%$ | 56.8 | 56.7 | Ambient Temperature | 23.2 | 23.5 | $^{\circ}\text{C}$ |
| Conductivity σ (mho/m) | 450 MHz Body | | 450 MHz Body | | Fluid Temperature | 23.2 | 22.7 | $^{\circ}\text{C}$ |
| | IEEE Target | Measured | IEEE Target | Measured | Fluid Depth | ≥ 15 | ≥ 15 | cm |
| | 0.94 | $\pm 5\%$ | 0.90 | 0.94 | ρ (Kg/m ³) | 1000 | | |

Note(s):

1. The measurement results were obtained with the DUT tested in the conditions described in this report. Detailed measurement data and plots showing the maximum SAR location of the DUT are reported in Appendix A.
 2. If the scaled SAR levels at the mid channel (50% duty cycle) were ≥ 3 dB below the SAR limit, SAR evaluation for the low and high channels was optional per FCC OET Bulletin 65, Supplement C, Edition 01-01 (see reference [3]).
 3. The power drifts measured by the DASY4 system for the duration of the SAR evaluations were added to the measured SAR levels to report scaled SAR results as shown in the above table.
 4. A SAR-versus-Time power drift evaluation was performed in the test configuration that reported the maximum-scaled SAR level (body-worn, mid channel, Li-ion Battery, Stubby Antenna P/N: KRA-17M, with Speaker-Mic and Belt-Clip accessories). See Appendix A (SAR Test Plots) for SAR-versus-Time power drift evaluation plot.
 5. The ambient and fluid temperatures were measured prior to, and during, the fluid dielectric parameter check and the SAR evaluation. The temperatures reported were consistent for all measurement periods.
 6. The dielectric parameters of the simulated tissue mixture were measured prior to the evaluation using an HP 85070C Dielectric Probe Kit and an HP 8753E Network Analyzer (see Appendix E for printout of measured fluid dielectric parameters).
 7. The SAR evaluations were performed within 24 hours of the system performance check.
- * The DUT was evaluated for SAR with Duracell Procell alkaline batteries. To report a SAR comparison between alternate alkaline battery types, the maximum scaled SAR level configuration evaluated with Duracell Procell alkaline batteries (Mid Channel, Stubby Antenna P/N: KRA-17M, with Speaker-Mic and Belt-Clip accessories) was repeated using Energizer E91 alkaline batteries as shown in the above table.

5.0 DETAILS OF SAR EVALUATION

The Kenwood USA Corporation Models: TK-3170-K, TK-3170-K4, TK-3173-K Portable FM UHF PTT Radio Transceiver FCC ID: ALH34713110 was compliant for localized Specific Absorption Rate (Occupational / Controlled Exposure) based on the test provisions and conditions described below. The detailed test setup photographs are shown in Appendix F.

1. The DUT was evaluated in a face-held configuration with the front of the radio placed parallel to the outer surface of the planar phantom. A 2.5 cm separation distance was maintained between the front side of the DUT and the outer surface of the planar phantom for the duration of the tests.
2. The DUT was evaluated in a body-worn configuration with the back of the radio placed parallel to the outer surface of the planar phantom. The attached belt-clip accessory was touching the planar phantom. With the Alkaline Battery Case the belt-clip accessory provided a 1.0 cm separation distance between the back of the DUT and the outer surface of the planar phantom. With the Li-ion battery the belt-clip accessory provided a 1.4 cm separation distance between the back of the DUT and the outer surface of the planar phantom. With the Ni-Cd and Ni-MH batteries, the belt-clip accessory provided a 0.9 cm separation distance between the back of the DUT and the outer surface of the planar phantom. The DUT was evaluated for body-worn SAR with the speaker-microphone and headset audio accessories connected consecutively.
3. The conducted power levels were measured before each test using a Gigatronics 8652A Universal Power Meter according to the procedures described in FCC 47 CFR §2.1046. It was noted that the power levels measured with the alkaline batteries resulted in up to 8% lower conducted power levels than with the Li-ion, NiMH, and NiCd batteries. The power measurement procedure was consistent for all battery types and measurement durations, therefore it was determined that the power measurements taken with alkaline batteries were reporting a worst-case conducted power level.
4. A SAR-versus-Time power drift evaluation was performed in the test configuration that reported the highest scaled SAR level (Body-Worn, Mid Channel, Stubby Antenna P/N: KRA-17M, Li-ion Battery, and Speaker-Microphone audio accessory). See Appendix A (SAR Test Plots) for SAR-versus-Time power drift evaluation plot.
5. The area scan evaluation was performed with a fully charged battery. After the area scan was completed the radio was cooled down to room temperature and the battery was replaced with a fully charged battery prior to the zoom scan evaluation.
6. The DUT was tested in unmodulated continuous transmit operation (Continuous Wave mode at 100% duty cycle) with the transmit key constantly depressed. For a push-to-talk device the 50% duty cycle compensation reported assumes a transmit/receive cycle of equal time base.
7. The ambient and fluid temperatures were measured prior to, and during, the fluid dielectric parameter check and the SAR evaluation. The temperatures reported were consistent for all measurement periods.
8. The dielectric parameters of the simulated tissue mixture were measured prior to the evaluation using an HP 85070C Dielectric Probe Kit and an HP 8753E Network Analyzer (see Appendix E for printout of measured fluid dielectric parameters).
9. The SAR evaluations were performed using a Plexiglas planar phantom.
10. A stack of low-density, low-loss dielectric foamed polystyrene was used in place of the device holder.

6.0 EVALUATION PROCEDURES

- a. (i) The evaluation was performed in the applicable area of the phantom depending on the type of device being tested. For devices held to the ear during normal operation, both the left and right ear positions were evaluated using the SAM phantom.
(ii) For body-worn and face-held devices a planar phantom was used.
- b. The SAR was determined by a pre-defined procedure within the DASY4 software. Upon completion of a reference and optical surface check, the exposed region of the phantom was scanned near the inner surface with a grid spacing of 15mm x 15mm.
An area scan was determined as follows:
- c. Based on the defined area scan grid, a more detailed grid is created to increase the points by a factor of 10. The interpolation function then evaluates all field values between corresponding measurement points.
- d. A linear search is applied to find all the candidate maxima. Subsequently, all maxima are removed that are >2 dB from the global maximum. The remaining maxima are then used to position the cube scans.
A 1g and 10g spatial peak SAR was determined as follows:
- e. Extrapolation is used to find the points between the dipole center of the probe and the surface of the phantom. This data cannot be measured, since the center of the dipoles is 2.7 mm away from the tip of the probe and the distance between the surface and the lowest measuring point is 1.4 mm (see probe calibration document in Appendix D). The extrapolation was based on trivariate quadratics computed from the previously calculated 3D interpolated points nearest the phantom surface.
- f. Interpolated data is used to calculate the average SAR over 1g and 10g cubes by spatially discretizing the entire measured cube. The volume used to determine the averaged SAR is a 1mm grid (42875 interpolated points).
- g. A zoom scan volume of 32 mm x 32 mm x 30 mm (5 x 5 x 7 points) centered at the peak SAR location determined from the area scan is used for all zoom scans for devices with a transmit frequency < 800 MHz. Zoom scans for frequencies ≥ 800 MHz are determined with a scan volume of 30 mm x 30 mm x 30 mm (7 x 7 x 7) to ensure complete capture of the peak spatial-average SAR.

7.0 SYSTEM PERFORMANCE CHECK

Prior to the SAR evaluation a system check was performed using a planar phantom with a 450MHz dipole (see Appendix C for system validation procedure). The dielectric parameters of the simulated tissue mixture were measured prior to the system performance check using an HP 85070C Dielectric Probe Kit and an HP 8753E Network Analyzer (see Appendix E for printout of measured fluid dielectric parameters). A forward power of 250mW was applied to the dipole and the system was verified to a tolerance of $\pm 10\%$ (see Appendix B for system performance check test plots).

| SYSTEM PERFORMANCE CHECK | | | | | | | | | | | | | |
|--------------------------|----------------------|---------------------|--------------|----------------------------------|----------|-------------------------------|----------|-----------------------------|-----------------|------------------|------------------|------------|---------------------|
| Test Date | 450MHz Equiv. Tissue | SAR 1g (W/kg) | | Dielectric Constant ϵ_r | | Conductivity σ (mho/m) | | ρ (Kg/m ³) | Amb. Temp. (°C) | Fluid Temp. (°C) | Fluid Depth (cm) | Humid. (%) | Barom. Press. (kPa) |
| | | IEEE Target | Measured | IEEE Target | Measured | IEEE Target | Measured | | | | | | |
| 10/20/04 | Brain | 1.23 ($\pm 10\%$) | 1.27 (+3.3%) | 43.5 $\pm 5\%$ | 44.0 | 0.87 $\pm 5\%$ | 0.87 | 1000 | 23.6 | 22.9 | ≥ 15 | 36 | 101.6 |
| 10/21/04 | Brain | 1.23 ($\pm 10\%$) | 1.25 (+1.6%) | 43.5 $\pm 5\%$ | 43.5 | 0.87 $\pm 5\%$ | 0.86 | 1000 | 23.8 | 23.3 | ≥ 15 | 32 | 101.9 |
| 10/22/04 | Brain | 1.23 ($\pm 10\%$) | 1.26 (+2.4%) | 43.5 $\pm 5\%$ | 43.3 | 0.87 $\pm 5\%$ | 0.86 | 1000 | 23.5 | 23.5 | ≥ 15 | 32 | 101.3 |
| 10/23/04 | Brain | 1.23 ($\pm 10\%$) | 1.27 (+3.3%) | 43.5 $\pm 5\%$ | 43.4 | 0.87 $\pm 5\%$ | 0.86 | 1000 | 23.0 | 22.8 | ≥ 15 | 32 | 101.9 |
| 10/24/04 | Brain | 1.23 ($\pm 10\%$) | 1.27 (+3.3%) | 43.5 $\pm 5\%$ | 43.5 | 0.87 $\pm 5\%$ | 0.85 | 1000 | 23.3 | 22.8 | ≥ 15 | 32 | 102.2 |

Note(s):

1. The ambient and fluid temperatures were measured prior to, and during, the fluid dielectric parameter check and the system performance check. The temperatures listed in the table above were consistent for all measurement periods.


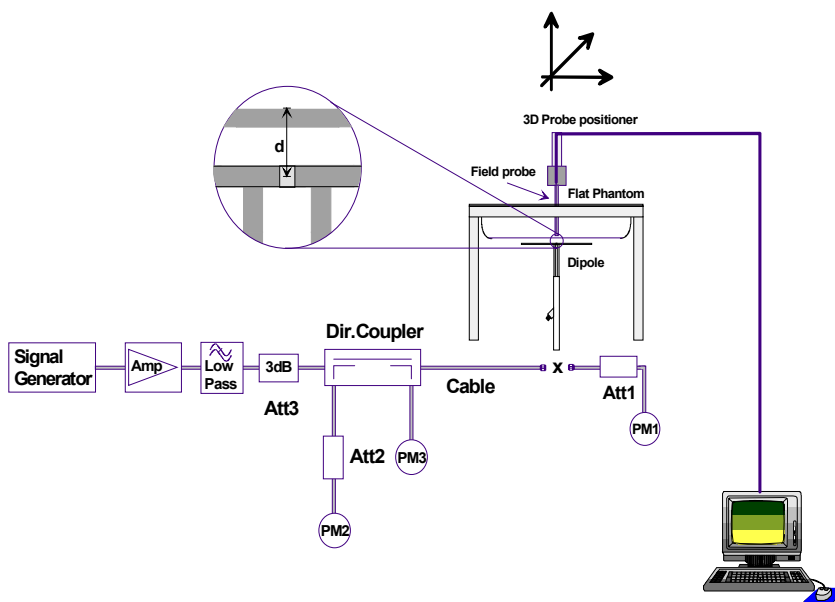


Figure 1. System Performance Check Setup Diagram

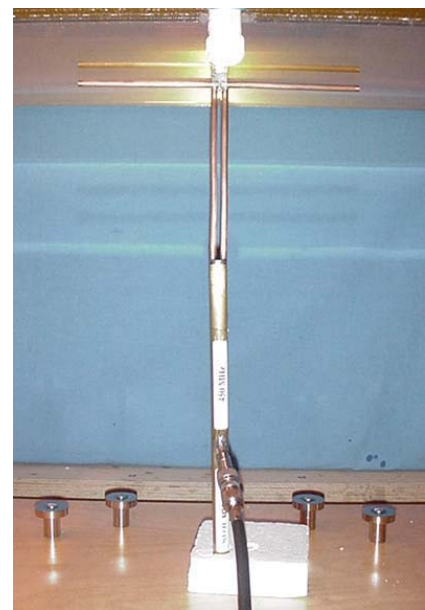

450MHz Dipole Setup

8.0 SIMULATED EQUIVALENT TISSUES

The 450MHz simulated tissue mixtures consist of a viscous gel using hydroxyethylcellulose (HEC) gelling agent and saline solution. Preservation with a bactericide is added and visual inspection is made to ensure air bubbles are not trapped during the mixing process. The fluid was prepared and measured for dielectric parameters (permittivity and conductivity) according to standardized procedures.

| SIMULATED TISSUE MIXTURES | | |
|---------------------------|-------------------------------|----------------|
| INGREDIENT | 450 MHz Brain | 450 MHz Body |
| | System Check & DUT Evaluation | DUT Evaluation |
| Water | 38.56 % | 52.00 % |
| Sugar | 56.32 % | 45.65 % |
| Salt | 3.95 % | 1.75 % |
| HEC | 0.98 % | 0.50 % |
| Bactericide | 0.19 % | 0.10 % |

9.0 SAR SAFETY LIMITS

| EXPOSURE LIMITS | SAR (W/kg) | |
|---|--|--|
| | (General Population / Uncontrolled Exposure Environment) | (Occupational / Controlled Exposure Environment) |
| Spatial Average (averaged over the whole body) | 0.08 | 0.4 |
| Spatial Peak (averaged over any 1g of tissue) | 1.60 | 8.0 |
| Spatial Peak (hands/wrists/feet/ankles averaged over 10g) | 4.0 | 20.0 |

Notes:

1. Uncontrolled environments are defined as locations where there is potential exposure of individuals who have no knowledge or control of their potential exposure.
2. Controlled environments are defined as locations where there is potential exposure of individuals who have knowledge of their potential exposure and can exercise control over their exposure.

10.0 ROBOT SYSTEM SPECIFICATIONS

Specifications

POSITIONER: Stäubli Unimation Corp. Robot Model: RX60L
Repeatability: 0.02 mm
No. of axis: 6

Data Acquisition Electronic (DAE) System

Cell Controller

Processor: AMD Athlon XP 2400+
Clock Speed: 2.0 GHz
Operating System: Windows XP Professional

Data Converter

Features: Signal Amplifier, multiplexer, A/D converter, and control logic
Software: DASY4 software
Connecting Lines: Optical downlink for data and status info.
 Optical uplink for commands and clock

DASY4 Measurement Server

Function: Real-time data evaluation for field measurements and surface detection
Hardware: PC/104 166MHz Pentium CPU; 32 MB chipdisk; 64 MB RAM
Connections: COM1, COM2, DAE, Robot, Ethernet, Service Interface

E-Field Probe

Model: ET3DV6
Serial No.: 1590
Construction: Triangular core fiber optic detection system
Frequency: 10 MHz to 6 GHz
Linearity: ± 0.2 dB (30 MHz to 3 GHz)

Phantom(s)

Evaluation Phantom

Type: Planar Phantom
Shell Material: Plexiglas
Bottom Thickness: 2.0 mm \pm 0.1 mm
Outer Dimensions: 75.0 cm (L) x 22.5 cm (W) x 20.5 cm (H); Back Plane: 25.7 cm (H)

Validation Phantom (≤ 450 MHz)

Type: Planar Phantom
Shell Material: Plexiglas
Bottom Thickness: 6.2 mm \pm 0.1 mm
Outer Dimensions: 86.0 cm (L) x 39.5 cm (W) x 21.8 cm (H)

11.0 PROBE SPECIFICATION (ET3DV6)

| | |
|--------------------|--|
| Construction: | Symmetrical design with triangular core Built-in shielding against static charges PEEK enclosure material (resistant to organic solvents, e.g. glycol) |
| Calibration: | In air from 10 MHz to 2.5 GHz In brain simulating tissue at frequencies of 900 MHz and 1.8 GHz (accuracy $\pm 8\%$) |
| Frequency: | 10 MHz to > 6 GHz; Linearity: ± 0.2 dB (30 MHz to 3 GHz) |
| Directivity: | ± 0.2 dB in brain tissue (rotation around probe axis) ± 0.4 dB in brain tissue (rotation normal to probe axis) |
| Dynamic Range: | 5 μ W/g to > 100 mW/g; Linearity: ± 0.2 dB |
| Surface Detection: | ± 0.2 mm repeatability in air and clear liquids over diffuse reflecting surfaces |
| Dimensions: | Overall length: 330 mm Tip length: 16 mm Body diameter: 12 mm Tip diameter: 6.8 mm Distance from probe tip to dipole centers: 2.7 mm |
| Application: | General dosimetry up to 3 GHz Compliance tests of mobile phone |



ET3DV6 E-Field Probe

12.0 PLANAR PHANTOM

The planar phantom is constructed of Plexiglas material with a 2.0 mm shell thickness for face-held and body-worn SAR evaluations of handheld and body-worn radio transceivers. The planar phantom is mounted on the side of the DASY4 compact system table.



Planar Phantom

13.0 VALIDATION PLANAR PHANTOM

The validation planar phantom is constructed of Plexiglas material with a 6.0 mm shell thickness for system validations at 450MHz and below. The validation planar phantom is mounted in the table of the DASY4 compact system.



Validation Planar Phantom

14.0 DEVICE HOLDER

The DASY4 device holder has two scales for device rotation (with respect to the body axis) and the device inclination (with respect to the line between the ear openings). The plane between the ear openings and the mouth tip has a rotation angle of 65° . The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections.



Device Holder

15.0 TEST EQUIPMENT LIST

| TEST EQUIPMENT | SERIAL NO. | CALIBRATION DATE |
|--|------------|------------------|
| Schmid & Partner DASY4 System | - | - |
| DASY4 Measurement Server | 1078 | N/A |
| -Robot | 599396-01 | N/A |
| DAE3 | 353 | Dec 2003 |
| DAE3 | 370 | May 2004 |
| -ET3DV6 E-Field Probe | 1387 | Mar 2004 |
| -ET3DV6 E-Field Probe | 1590 | May 2004 |
| -300MHz Validation Dipole | 135 | Oct 2004 |
| -450MHz Validation Dipole | 136 | Nov 2003 |
| -835MHz Validation Dipole | 411 | Mar 2004 |
| -900MHz Validation Dipole | 054 | June 2004 |
| -1800MHz Validation Dipole | 247 | June 2004 |
| -1900MHz Validation Dipole | 151 | June 2004 |
| -2450MHz Validation Dipole | 150 | Sept 2004 |
| -SAM Phantom V4.0C | 1033 | N/A |
| -Barski Planar Phantom | 03-01 | N/A |
| -Plexiglas Planar Phantom | 161 | N/A |
| -Validation Planar Phantom | 137 | N/A |
| HP 85070C Dielectric Probe Kit | N/A | N/A |
| Gigatronics 8651A Power Meter | 8650137 | April 2004 |
| Gigatronics 8652A Power Meter | 1835267 | April 2004 |
| Gigatronics 80701A Power Sensor | 1833535 | April 2004 |
| Gigatronics 80701A Power Sensor | 1833542 | April 2004 |
| Gigatronics 80701A Power Sensor | 1834350 | April 2004 |
| HP E4408B Spectrum Analyzer | US39240170 | Dec 2003 |
| HP 8594E Spectrum Analyzer | 3543A02721 | April 2004 |
| HP 8753E Network Analyzer | US38433013 | April 2004 |
| HP 8648D Signal Generator | 3847A00611 | April 2004 |
| Amplifier Research 5S1G4 Power Amplifier | 26235 | N/A |

16.0 MEASUREMENT UNCERTAINTIES

| UNCERTAINTY BUDGET FOR DEVICE EVALUATION | | | | | | |
|--|-------------------------|--------------------------|---------|-------------|---------------------------------|--------------------|
| Error Description | Uncertainty Value ±% | Probability Distribution | Divisor | C_i 1g | Standard Uncertainty ±% (1g) | V_i Or V_{eff} |
| Measurement System | | | | | | |
| Probe calibration | ± 4.0 | Normal | 1 | 1 | ± 4.0 | ∞ |
| Axial isotropy of the probe | ± 4.7 | Rectangular | √3 | (1- C_p) | ± 1.9 | ∞ |
| Spherical isotropy of the probe | ± 9.6 | Rectangular | √3 | (C_p) | ± 3.9 | ∞ |
| Spatial resolution | ± 0.0 | Rectangular | √3 | 1 | ± 0.0 | ∞ |
| Boundary effects | ± 5.5 | Rectangular | √3 | 1 | ± 3.2 | ∞ |
| Probe linearity | ± 4.7 | Rectangular | √3 | 1 | ± 2.7 | ∞ |
| Detection limit | ± 1.0 | Rectangular | √3 | 1 | ± 0.6 | ∞ |
| Readout electronics | ± 1.0 | Normal | 1 | 1 | ± 1.0 | ∞ |
| Response time | ± 0.8 | Rectangular | √3 | 1 | ± 0.5 | ∞ |
| Integration time | ± 1.4 | Rectangular | √3 | 1 | ± 0.8 | ∞ |
| RF ambient conditions | ± 3.0 | Rectangular | √3 | 1 | ± 1.7 | ∞ |
| Mech. constraints of robot | ± 0.4 | Rectangular | √3 | 1 | ± 0.2 | ∞ |
| Probe positioning | ± 2.9 | Rectangular | √3 | 1 | ± 1.7 | ∞ |
| Extrapolation & integration | ± 3.9 | Rectangular | √3 | 1 | ± 2.3 | ∞ |
| Test Sample Related | | | | | | |
| Device positioning | ± 6.0 | Normal | √3 | 1 | ± 6.7 | 12 |
| Device holder uncertainty | ± 5.0 | Normal | √3 | 1 | ± 5.9 | 8 |
| Power drift | ± 5.0 | Rectangular | √3 | | ± 2.9 | ∞ |
| Phantom and Setup | | | | | | |
| Phantom uncertainty | ± 4.0 | Rectangular | √3 | 1 | ± 2.3 | ∞ |
| Liquid conductivity (target) | ± 5.0 | Rectangular | √3 | 0.6 | ± 1.7 | ∞ |
| Liquid conductivity (measured) | ± 5.0 | Rectangular | √3 | 0.6 | ± 1.7 | ∞ |
| Liquid permittivity (target) | ± 5.0 | Rectangular | √3 | 0.6 | ± 1.7 | ∞ |
| Liquid permittivity (measured) | ± 5.0 | Rectangular | √3 | 0.6 | ± 1.7 | ∞ |
| Combined Standard Uncertainty | | | | | ± 13.03 | |
| Expanded Uncertainty (k=2) | | | | | ± 26.07 | |

Measurement Uncertainty Table in accordance with IEEE Standard 1528-2003 (see reference [5])

MEASUREMENT UNCERTAINTIES (Cont.)

| UNCERTAINTY BUDGET FOR SYSTEM VALIDATION | | | | | | |
|--|-------------------------|--------------------------|---------|-------------|---------------------------------|--------------------|
| Error Description | Uncertainty Value ±% | Probability Distribution | Divisor | C_i 1g | Standard Uncertainty ±% (1g) | V_i OR V_{eff} |
| Measurement System | | | | | | |
| Probe calibration | ± 4.0 | Normal | 1 | 1 | ± 4.0 | ∞ |
| Axial isotropy of the probe | ± 4.7 | Rectangular | √3 | (1- C_p) | ± 1.9 | ∞ |
| Spherical isotropy of the probe | ± 9.6 | Rectangular | √3 | (C_p) | ± 3.9 | ∞ |
| Spatial resolution | ± 0.0 | Rectangular | √3 | 1 | ± 0.0 | ∞ |
| Boundary effects | ± 5.5 | Rectangular | √3 | 1 | ± 3.2 | ∞ |
| Probe linearity | ± 4.7 | Rectangular | √3 | 1 | ± 2.7 | ∞ |
| Detection limit | ± 1.0 | Rectangular | √3 | 1 | ± 0.6 | ∞ |
| Readout electronics | ± 1.0 | Normal | 1 | 1 | ± 1.0 | ∞ |
| Response time | ± 0.8 | Rectangular | √3 | 1 | ± 0.5 | ∞ |
| Integration time | ± 1.4 | Rectangular | √3 | 1 | ± 0.8 | ∞ |
| RF ambient conditions | ± 3.0 | Rectangular | √3 | 1 | ± 1.7 | ∞ |
| Mech. constraints of robot | ± 0.4 | Rectangular | √3 | 1 | ± 0.2 | ∞ |
| Probe positioning | ± 2.9 | Rectangular | √3 | 1 | ± 1.7 | ∞ |
| Extrapolation & integration | ± 3.9 | Rectangular | √3 | 1 | ± 2.3 | ∞ |
| Dipole | | | | | | |
| Dipole Axis to Liquid Distance | ± 2.0 | Rectangular | √3 | 1 | ± 1.2 | ∞ |
| Input Power | ± 4.7 | Rectangular | √3 | 1 | ± 2.7 | ∞ |
| Phantom and Setup | | | | | | |
| Phantom uncertainty | ± 4.0 | Rectangular | √3 | 1 | ± 2.3 | ∞ |
| Liquid conductivity (target) | ± 5.0 | Rectangular | √3 | 0.6 | ± 1.7 | ∞ |
| Liquid conductivity (measured) | ± 5.0 | Rectangular | √3 | 0.6 | ± 1.7 | ∞ |
| Liquid permittivity (target) | ± 5.0 | Rectangular | √3 | 0.6 | ± 1.7 | ∞ |
| Liquid permittivity (measured) | ± 5.0 | Rectangular | √3 | 0.6 | ± 1.7 | ∞ |
| Combined Standard Uncertainty | | | | | ± 9.58 | |
| Expanded Uncertainty (k=2) | | | | | ± 19.16 | |

Measurement Uncertainty Table in accordance with IEEE Standard 1528-2003 (see reference [5])

17.0 REFERENCES

- [1] Federal Communications Commission, "Radiofrequency radiation exposure evaluation: portable devices", Rule Part 47 CFR §2.1093: 1999.
- [2] Health Canada, "Limits of Human Exposure to Radiofrequency Electromagnetic Fields in the Frequency Range from 3 kHz to 300 GHz", Safety Code 6.
- [3] Federal Communications Commission, "Evaluating Compliance with FCC Guidelines for Human Exposure to Radio frequency Electromagnetic Fields", OET Bulletin 65, Supplement C (Edition 01-01), FCC, Washington, D.C.: June 2001.
- [4] Industry Canada, "Evaluation Procedure for Mobile and Portable Radio Transmitters with respect to Health Canada's Safety Code 6 for Exposure of Humans to Radio Frequency Fields", Radio Standards Specification RSS-102 Issue 1 (Provisional): September 1999.
- [5] IEEE Std 1528-2003, "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques": June 2003.

| | |
|------------------|-----------------------|
| Test Report S/N: | 101204ALH-T569-S90U |
| Test Date(s): | October 20-24, 2004 |
| Test Type: | FCC/IC SAR Evaluation |

APPENDIX B - SYSTEM PERFORMANCE CHECK DATA

Date Tested: 10/20/04

System Performance Check - 450 MHz Dipole

DUT: Dipole 450 MHz; Model: D450V2; Type: System Performance Check; Serial: 136; Calibrated: 11/04/2003

Ambient Temp: 23.6 °C; Fluid Temp: 22.9 °C; Barometric Pressure: 101.6 kPa; Humidity: 36%

Communication System: CW
 Forward Conducted Power: 250mW
 Frequency: 450 MHz; Duty Cycle: 1:1
 Medium: HSL450 ($\sigma = 0.87$ mho/m; $\epsilon_r = 44.0$; $\rho = 1000$ kg/m³)


- Probe: ET3DV6 - SN1590; ConvF(7.5, 7.5, 7.5); Calibrated: 24/05/2004
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn370; Calibrated: 14/05/2004
- Phantom: Validation Planar; Type: Plexiglas; Serial: 137
- Measurement SW: DASY4, V4.3 Build 22; Postprocessing SW: SEMCAD, V1.8 Build 127

450 MHz System Performance Check/Area Scan (6x11x1):


Measurement grid: dx=15mm, dy=15mm

450 MHz System Performance Check/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 39.6 V/m; Power Drift = -0.1 dB
 Peak SAR (extrapolated) = 2.17 W/kg
SAR(1 g) = 1.27 mW/g; SAR(10 g) = 0.824 mW/g

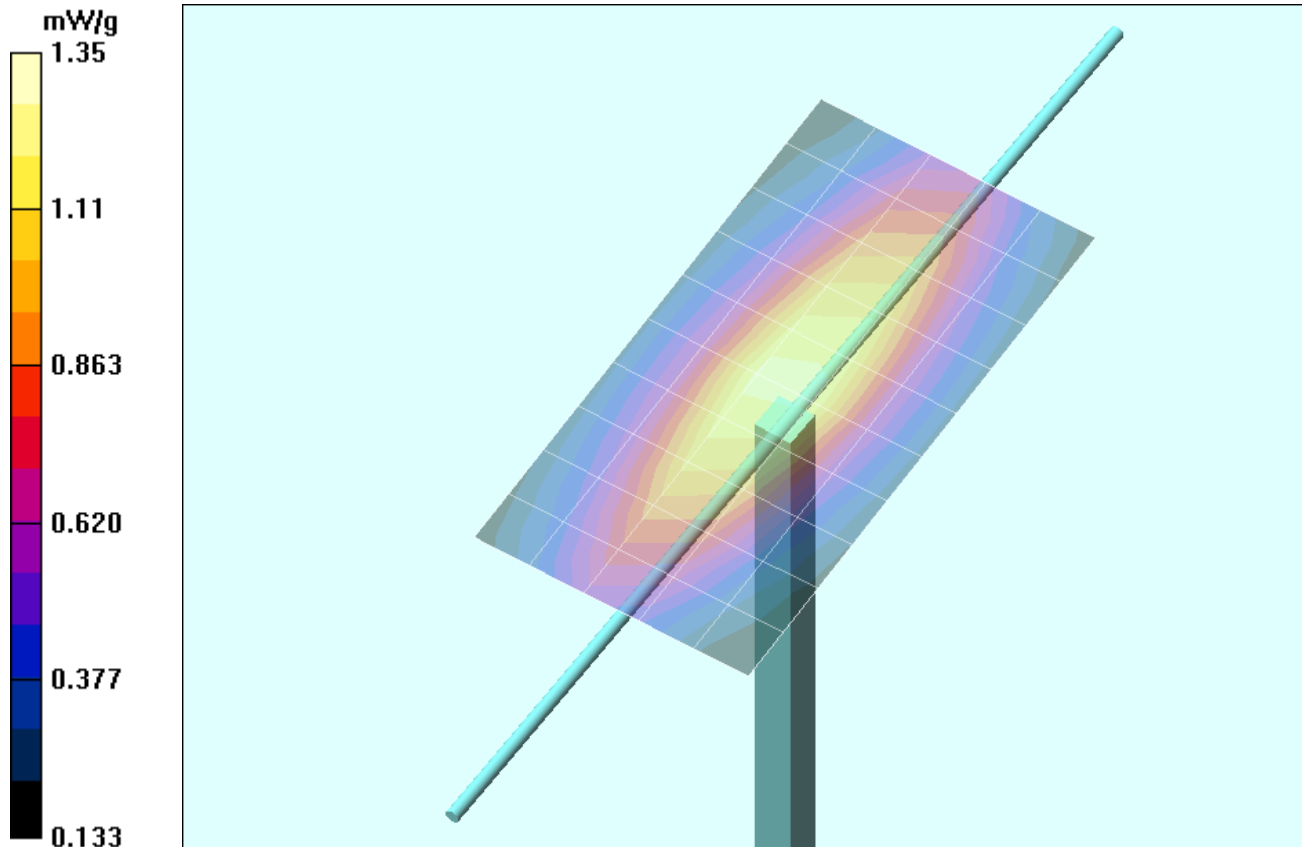

Z-Axis Scan

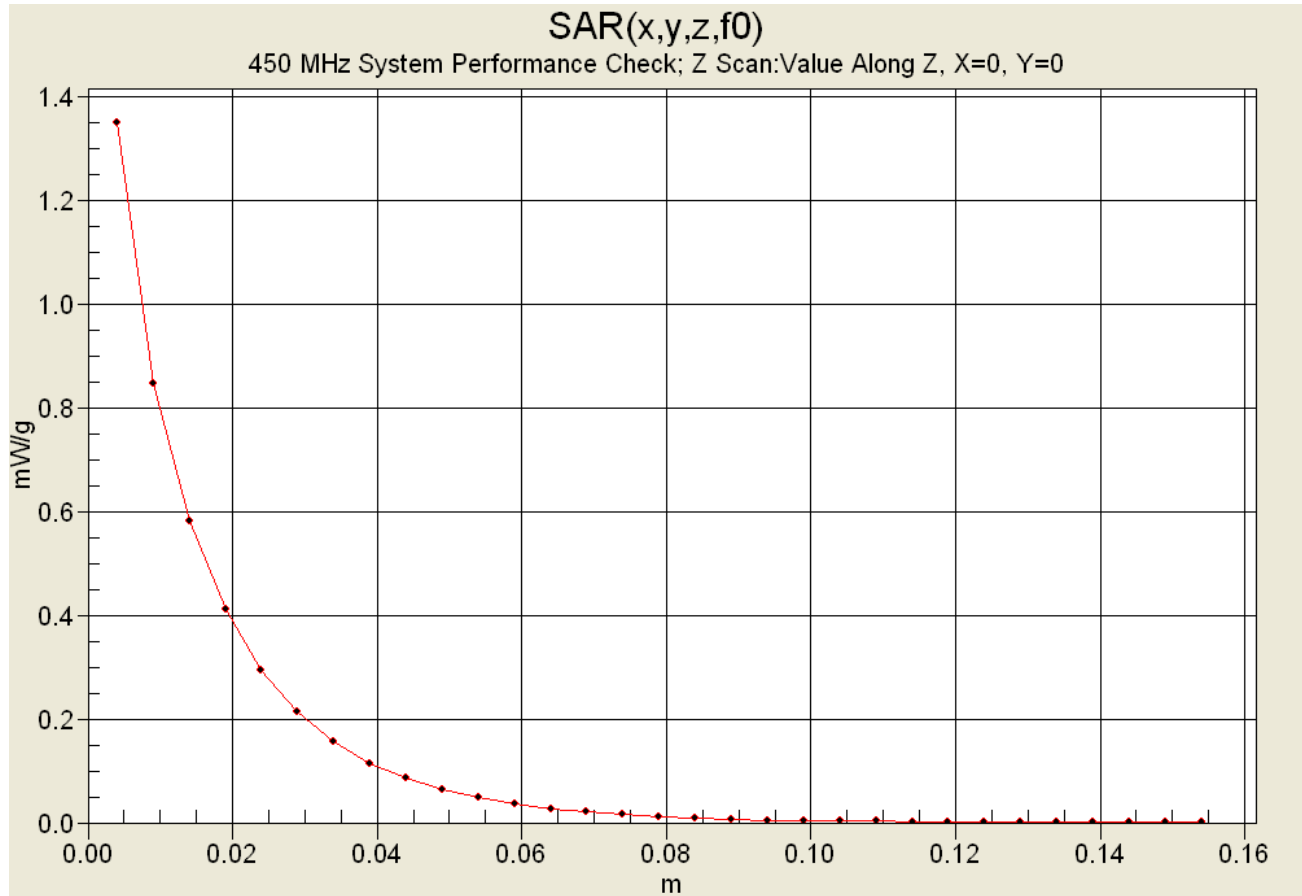

Date Tested: 10/21/04

System Performance Check - 450 MHz Dipole

DUT: Dipole 450 MHz; Model: D450V2; Type: System Performance Check; Serial: 136; Calibrated: 11/04/2003

Ambient Temp: 23.8 °C; Fluid Temp: 23.3 °C; Barometric Pressure: 101.9 kPa; Humidity: 32%

Communication System: CW
 Forward Conducted Power: 250mW
 Frequency: 450 MHz; Duty Cycle: 1:1
 Medium: HSL450 ($\sigma = 0.86$ mho/m; $\epsilon_r = 43.5$; $\rho = 1000$ kg/m³)


- Probe: ET3DV6 - SN1590; ConvF(7.5, 7.5, 7.5); Calibrated: 24/05/2004
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn370; Calibrated: 14/05/2004
- Phantom: Validation Planar; Type: Plexiglas; Serial: 137
- Measurement SW: DASY4, V4.3 Build 22; Postprocessing SW: SEMCAD, V1.8 Build 127

450 MHz System Performance Check/Area Scan (6x11x1):


Measurement grid: dx=15mm, dy=15mm

450 MHz System Performance Check/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 39.5 V/m; Power Drift = -0.0 dB
 Peak SAR (extrapolated) = 2.13 W/kg
SAR(1 g) = 1.25 mW/g; SAR(10 g) = 0.809 mW/g

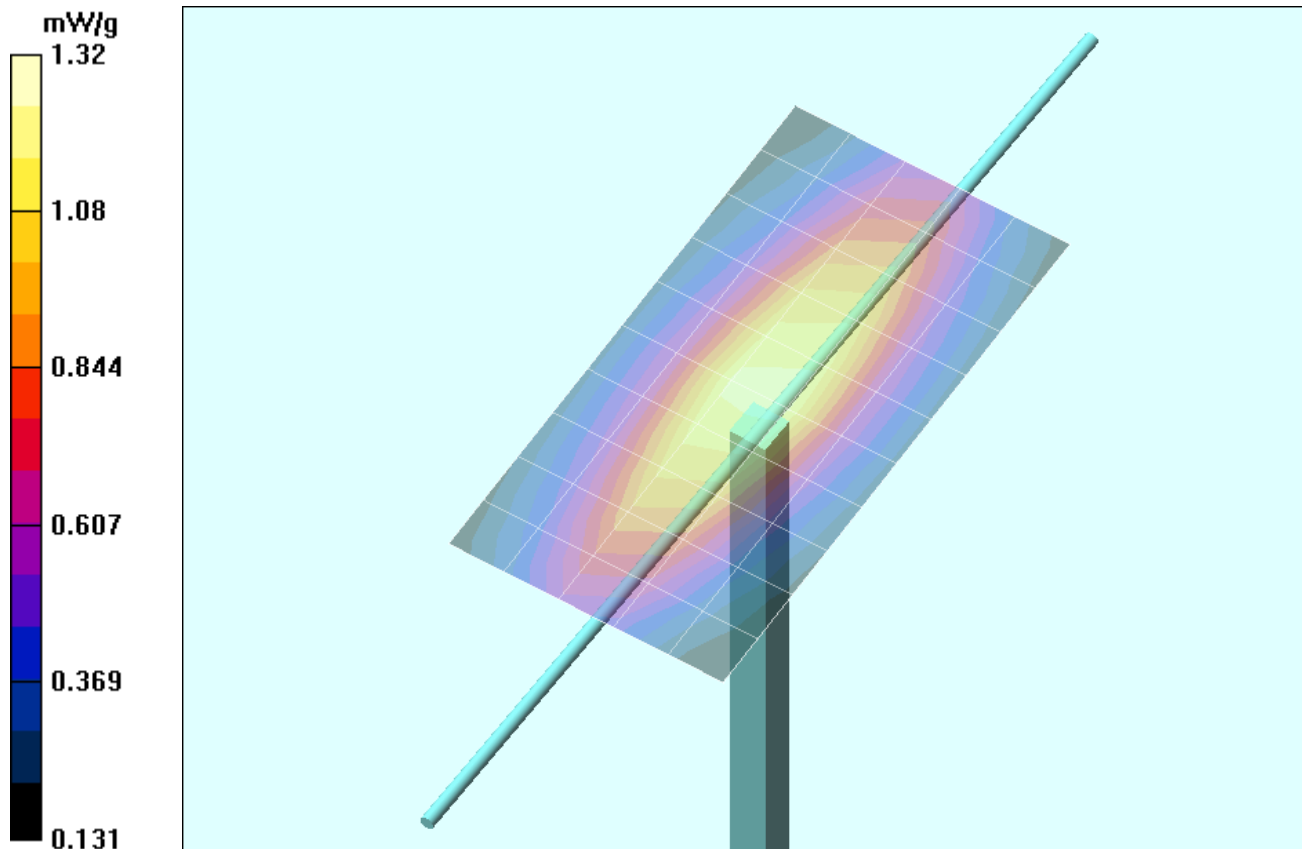

Z-Axis Scan

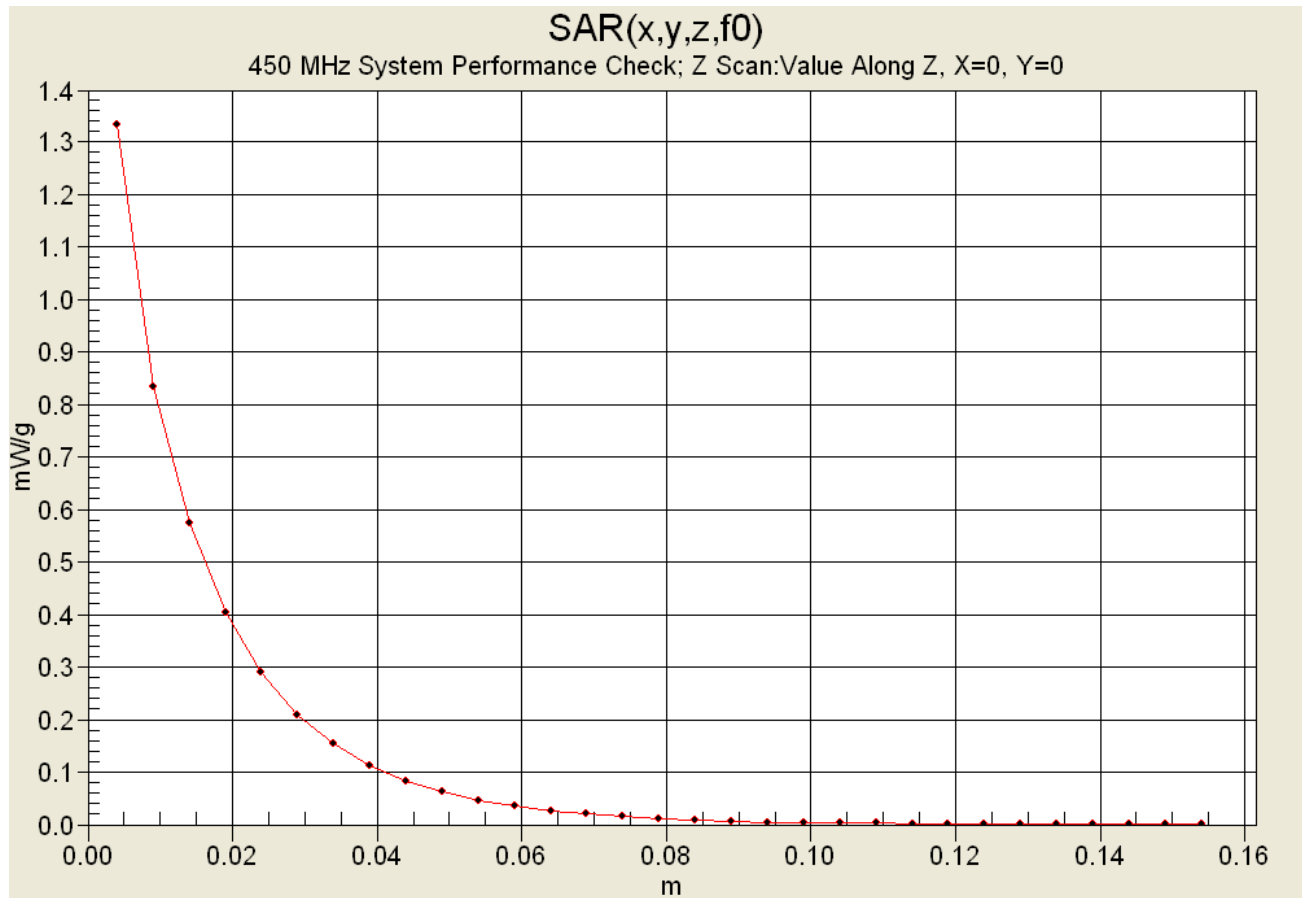

Date Tested: 10/22/04

System Performance Check - 450 MHz Dipole

DUT: Dipole 450 MHz; Model: D450V2; Type: System Performance Check; Serial: 136; Calibrated: 11/04/2003

Ambient Temp: 23.5 °C; Fluid Temp: 23.5 °C; Barometric Pressure: 101.3 kPa; Humidity: 32%

Communication System: CW
 Forward Conducted Power: 250mW
 Frequency: 450 MHz; Duty Cycle: 1:1
 Medium: HSL450 ($\sigma = 0.86$ mho/m; $\epsilon_r = 43.3$; $\rho = 1000$ kg/m³)


- Probe: ET3DV6 - SN1590; ConvF(7.5, 7.5, 7.5); Calibrated: 24/05/2004
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn370; Calibrated: 14/05/2004
- Phantom: Validation Planar; Type: Plexiglas; Serial: 137
- Measurement SW: DASY4, V4.3 Build 22; Postprocessing SW: SEMCAD, V1.8 Build 127

450 MHz System Performance Check/Area Scan (6x11x1):


Measurement grid: dx=15mm, dy=15mm

450 MHz System Performance Check/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 39.3 V/m; Power Drift = -0.0 dB
 Peak SAR (extrapolated) = 2.15 W/kg
SAR(1 g) = 1.26 mW/g; SAR(10 g) = 0.816 mW/g

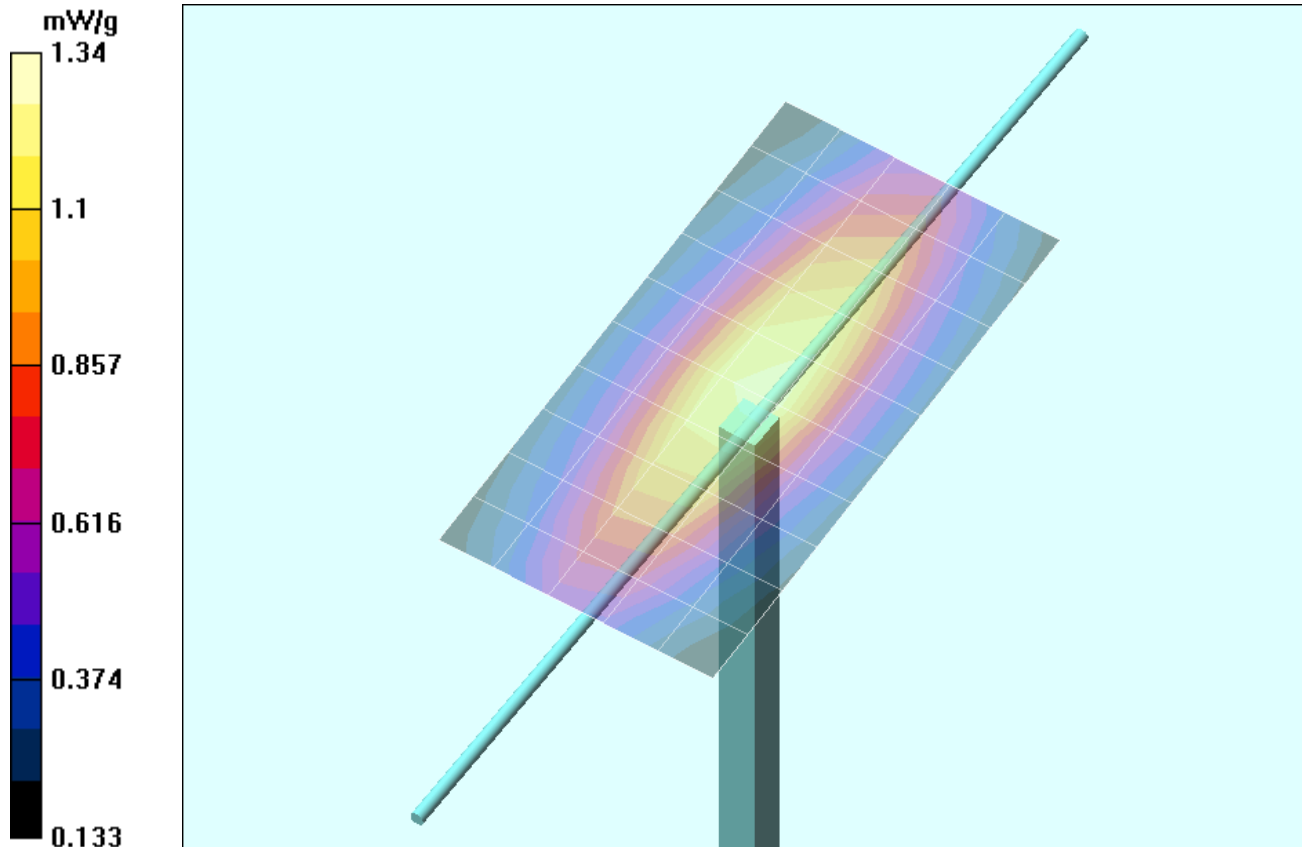

Z-Axis Scan

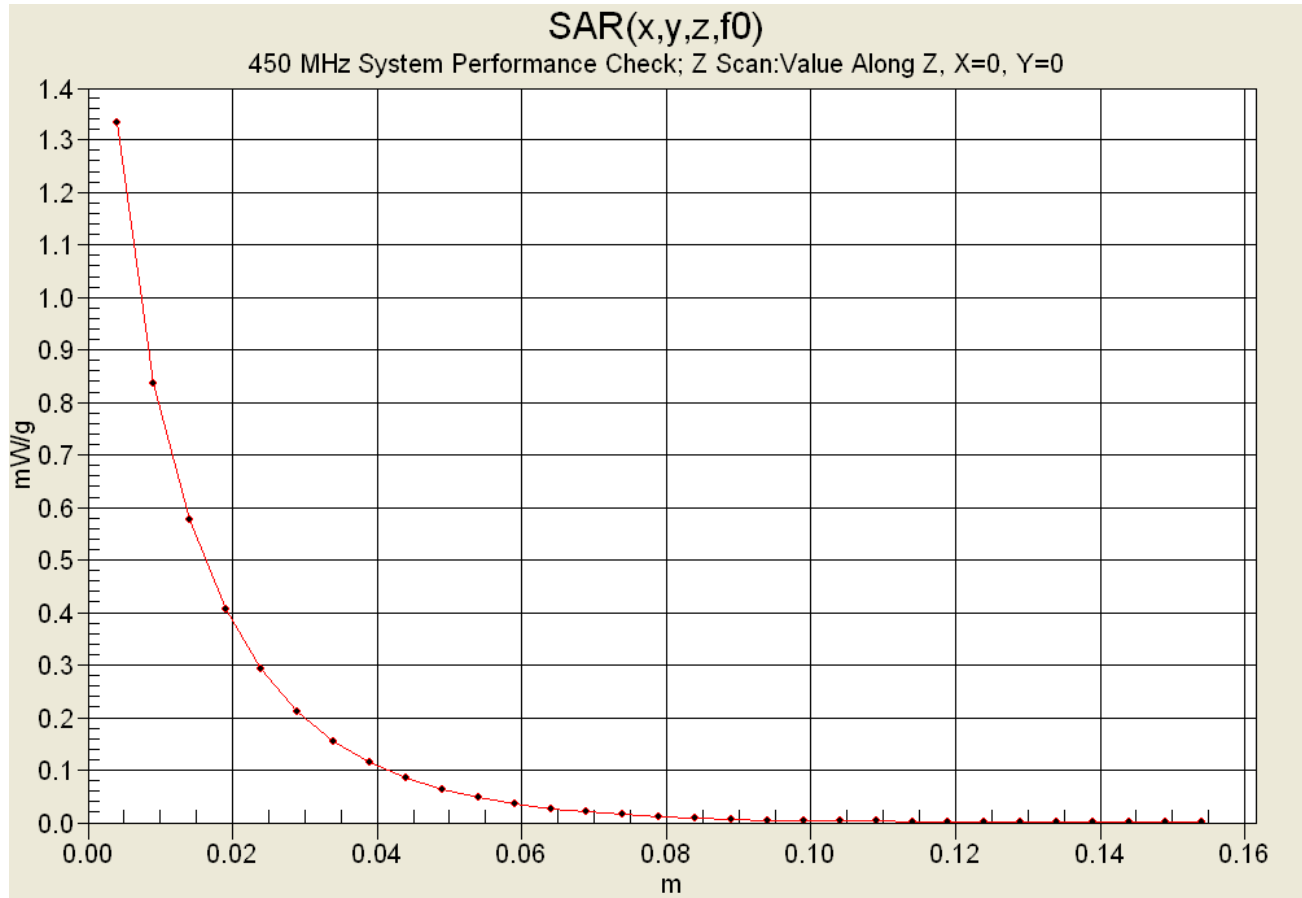

Date Tested: 10/23/04

System Performance Check - 450 MHz Dipole

DUT: Dipole 450 MHz; Model: D450V2; Type: System Performance Check; Serial: 136; Calibrated: 11/04/2003

Ambient Temp: 23.0 °C; Fluid Temp: 22.8 °C; Barometric Pressure: 101.9 kPa; Humidity: 32%

Communication System: CW
 Forward Conducted Power: 250mW
 Frequency: 450 MHz; Duty Cycle: 1:1
 Medium: HSL450 ($\sigma = 0.86$ mho/m; $\epsilon_r = 43.4$; $\rho = 1000$ kg/m³)


- Probe: ET3DV6 - SN1590; ConvF(7.5, 7.5, 7.5); Calibrated: 24/05/2004
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn370; Calibrated: 14/05/2004
- Phantom: Validation Planar; Type: Plexiglas; Serial: 137
- Measurement SW: DASY4, V4.3 Build 22; Postprocessing SW: SEMCAD, V1.8 Build 127

450 MHz System Performance Check/Area Scan (6x11x1):


Measurement grid: dx=15mm, dy=15mm

450 MHz System Performance Check/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 39.8 V/m; Power Drift = -0.0 dB
 Peak SAR (extrapolated) = 2.15 W/kg
SAR(1 g) = 1.27 mW/g; SAR(10 g) = 0.828 mW/g

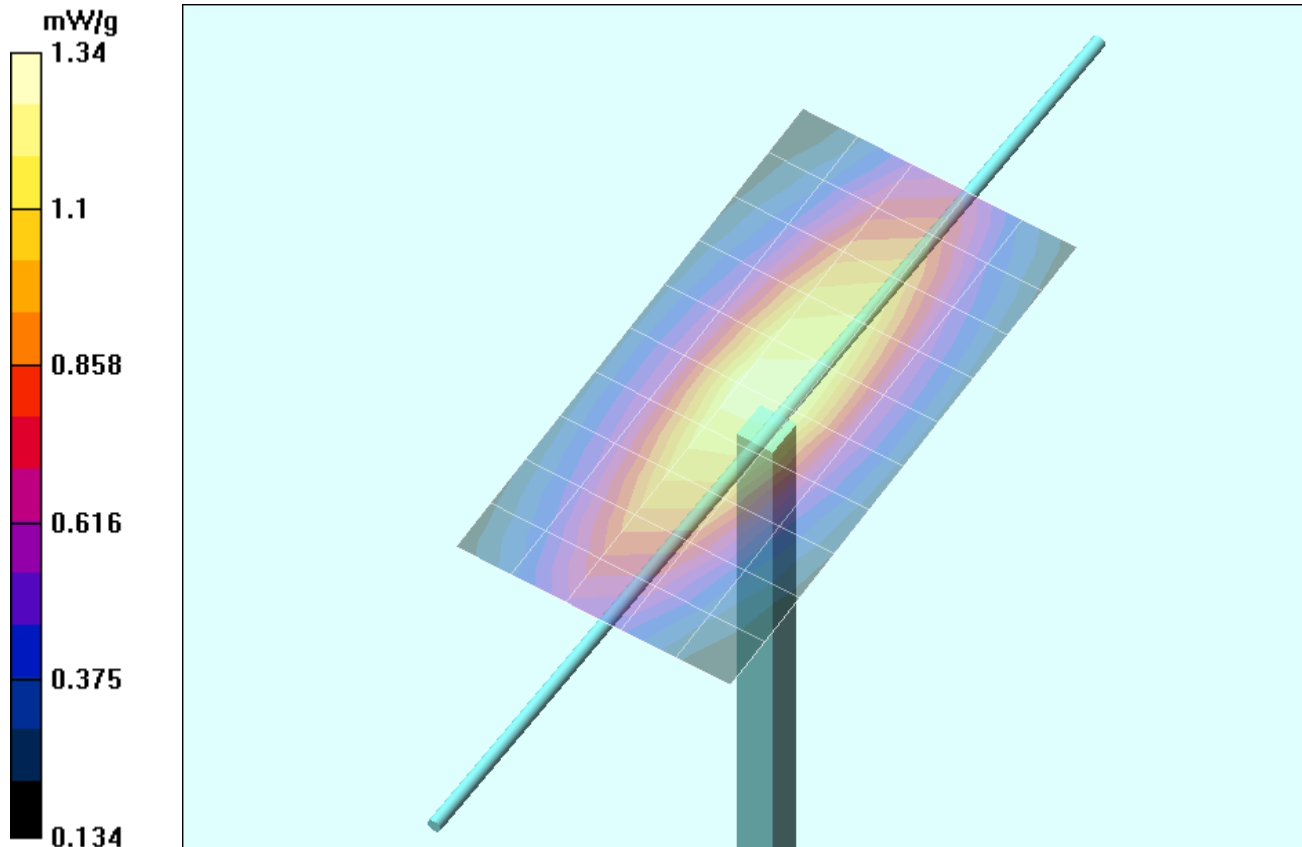

Z-Axis Scan

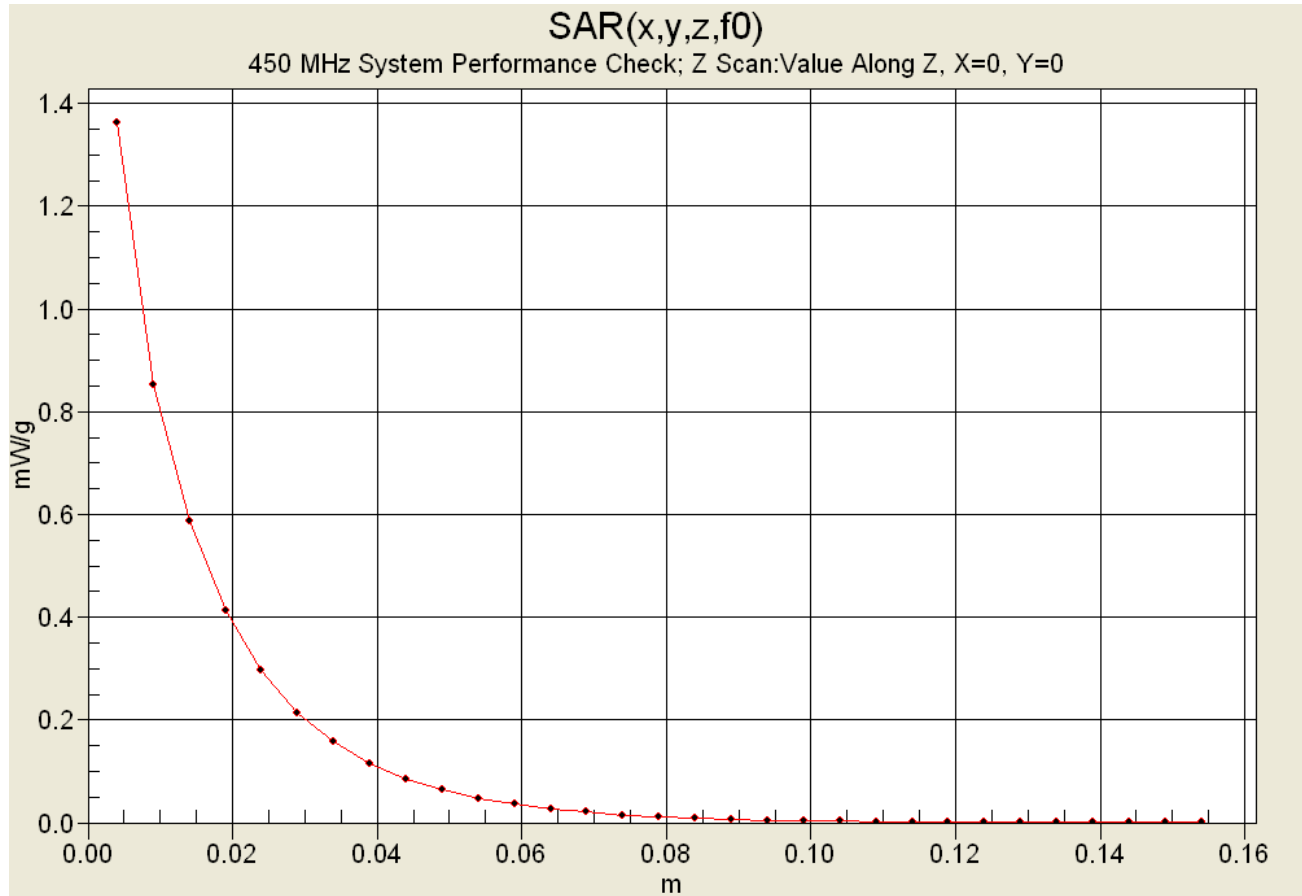

Date Tested: 10/24/04

System Performance Check - 450 MHz Dipole

DUT: Dipole 450 MHz; Model: D450V2; Type: System Performance Check; Serial: 136; Calibrated: 11/04/2003

Ambient Temp: 23.3 °C; Fluid Temp: 22.8 °C; Barometric Pressure: 102.2 kPa; Humidity: 32%

Communication System: CW
 Forward Conducted Power: 250mW
 Frequency: 450 MHz; Duty Cycle: 1:1
 Medium: HSL450 ($\sigma = 0.85$ mho/m; $\epsilon_r = 43.5$; $\rho = 1000$ kg/m³)


- Probe: ET3DV6 - SN1590; ConvF(7.5, 7.5, 7.5); Calibrated: 24/05/2004
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn370; Calibrated: 14/05/2004
- Phantom: Validation Planar; Type: Plexiglas; Serial: 137
- Measurement SW: DASY4, V4.3 Build 22; Postprocessing SW: SEMCAD, V1.8 Build 127

450 MHz System Performance Check/Area Scan (6x11x1):


Measurement grid: dx=15mm, dy=15mm

450 MHz System Performance Check/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 39.9 V/m; Power Drift = -0.0 dB
 Peak SAR (extrapolated) = 2.17 W/kg
SAR(1 g) = 1.27 mW/g; SAR(10 g) = 0.821 mW/g

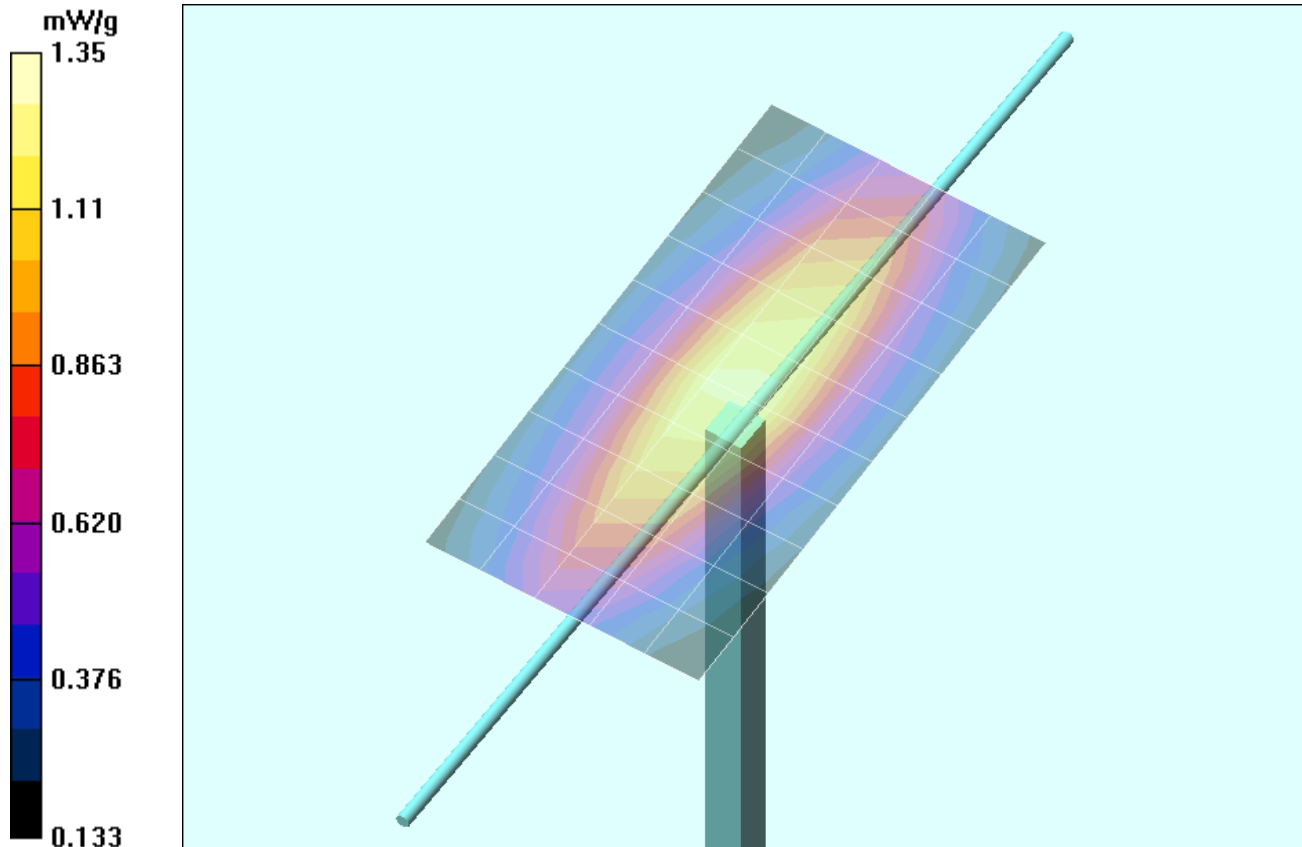

Z-Axis Scan

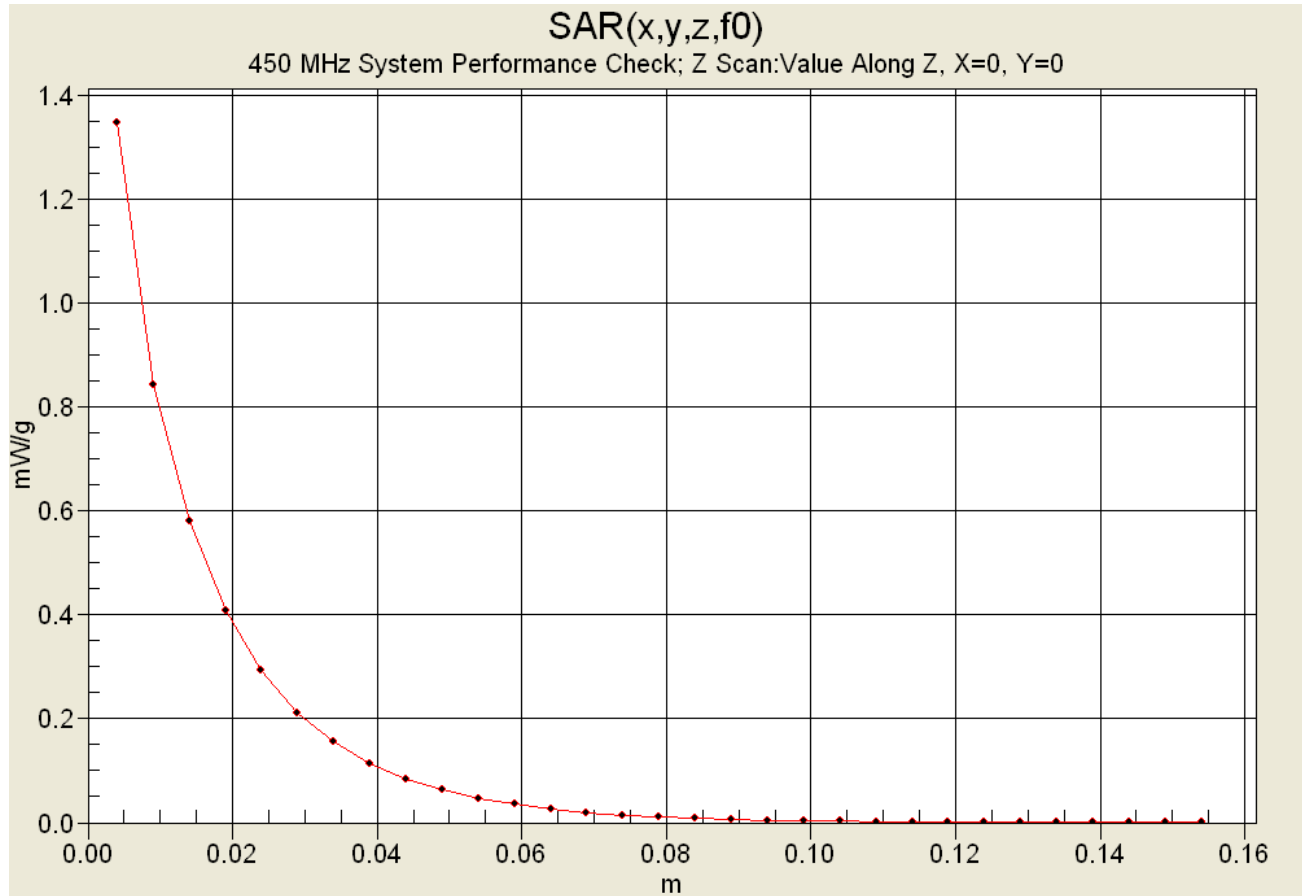

| | |
|------------------|-----------------------|
| Test Report S/N: | 101204ALH-T569-S90U |
| Test Date(s): | October 20-24, 2004 |
| Test Type: | FCC/IC SAR Evaluation |

APPENDIX C - SYSTEM VALIDATION

450MHz SYSTEM VALIDATION DIPOLE

Type:

450MHz Validation Dipole

Serial Number:

136

Place of Calibration:

Celltech Labs Inc.

Date of Calibration:

November 4, 2003

Celltech Labs Inc. hereby certifies that this device has been calibrated on the date indicated above.

Calibrated by:

Spencer Watson

Approved by:

Russell W. Pope

1. Dipole Construction & Electrical Characteristics


The validation dipole was constructed in accordance with the IEEE Std “Recommended Practice for Determining the Spatial-Peak Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques”. The electrical properties were measured using an HP 8753E Network Analyzer. The network analyzer was calibrated to the validation dipole N-type connector feed point using an HP85032E Type N calibration kit. The dipole was placed parallel to a planar phantom at a separation distance of 15.0mm from the simulating fluid using a loss-less dielectric spacer. The measured input impedance is:

Feed point impedance at 450MHz $\text{Re}\{Z\} = 49.982\Omega$


$\text{Im}\{Z\} = 7.2324\Omega$

Return Loss at 450MHz


-22.597dB

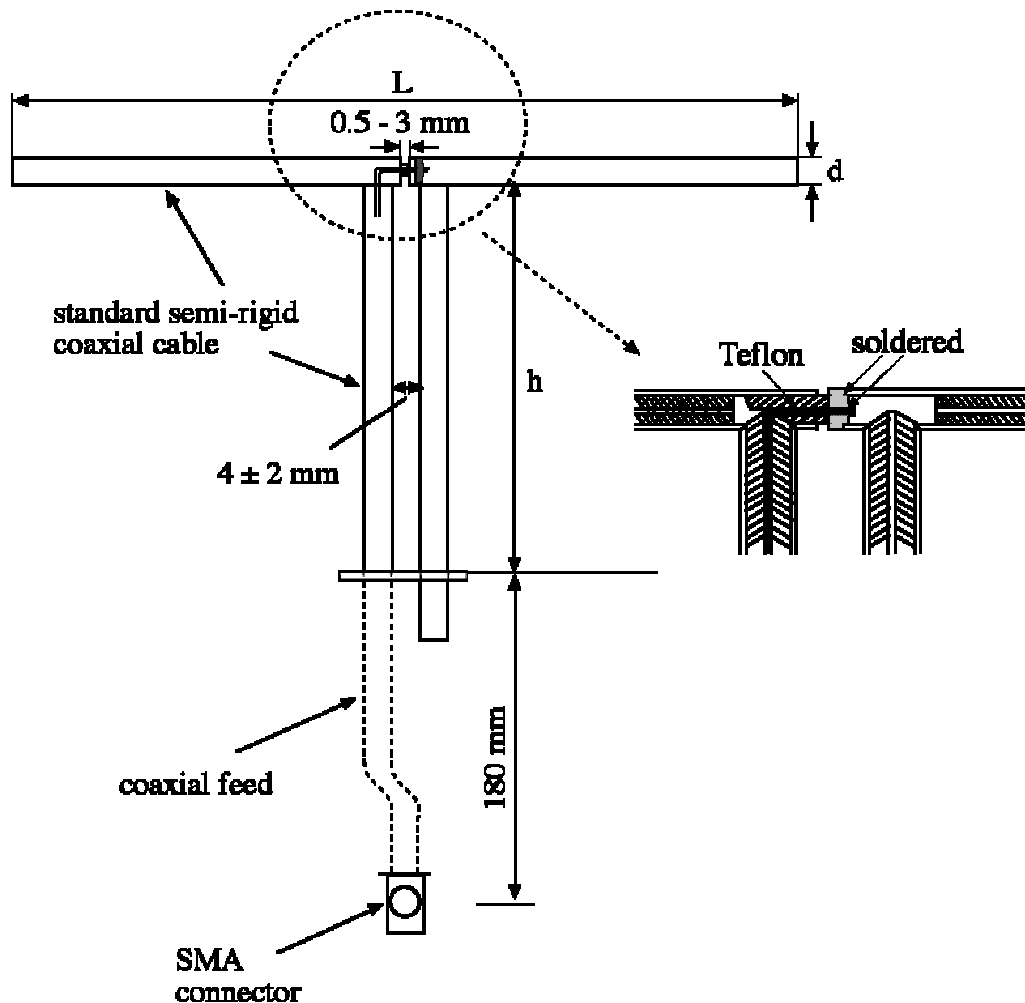

CH1 S11 1 U FS 1: 49.982 Ω 7.2324 Ω 2.5579 nH 4 Nov 2003 12:04:21 450.000 000 MHz

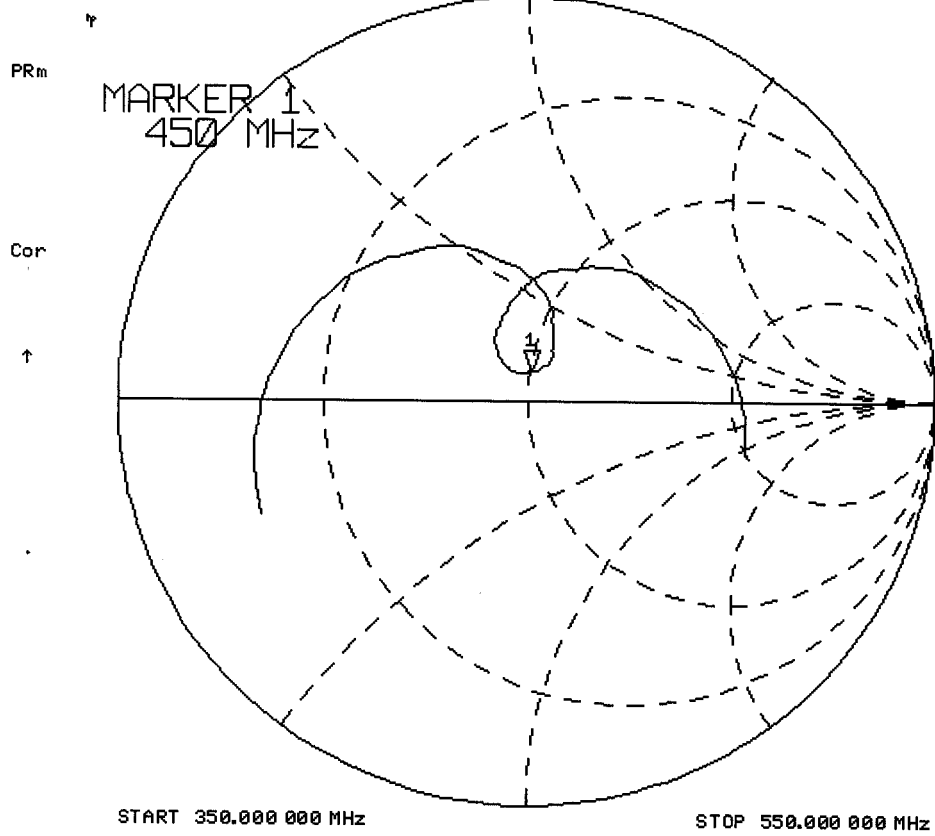

[CH1] S11 LOG 10 dB/REF 0 dB 4 Nov 2003 12:06:24
1:-22.597 dB 450.000 000 MHz

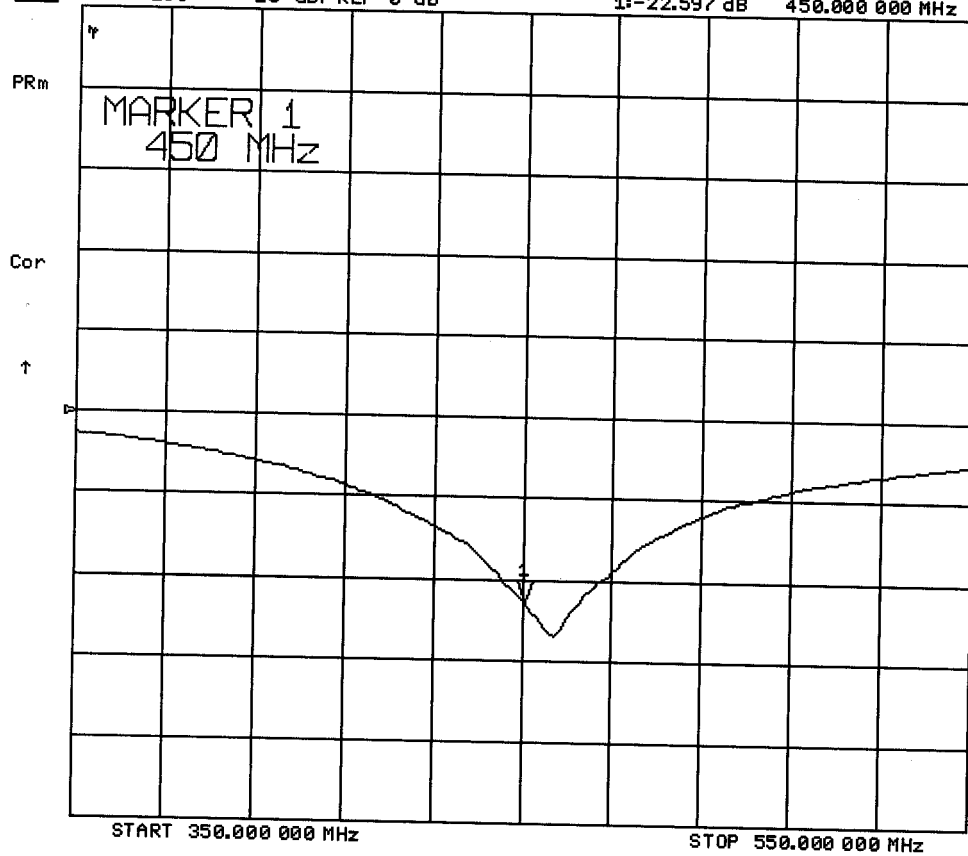

2. Validation Dipole Dimensions

| Frequency (MHz) | L (mm) | h (mm) | d (mm) |
|-----------------|--------|--------|--------|
| 300 | 420.0 | 250.0 | 6.2 |
| 450 | 288.0 | 167.0 | 6.2 |
| 835 | 161.0 | 89.8 | 3.6 |
| 900 | 149.0 | 83.3 | 3.6 |
| 1450 | 89.1 | 51.7 | 3.6 |
| 1800 | 72.0 | 41.7 | 3.6 |
| 1900 | 68.0 | 39.5 | 3.6 |
| 2000 | 64.5 | 37.5 | 3.6 |
| 2450 | 51.8 | 30.6 | 3.6 |
| 3000 | 41.5 | 25.0 | 3.6 |




3. Validation Phantom

The validation phantom was constructed using relatively low-loss tangent Plexiglas material. The inner dimensions of the phantom are as follows:

Length: 83.5 cm
 Width: 36.9 cm
 Height: 21.8 cm

The bottom section of the validation phantom is constructed of 6.2 ± 0.1 mm Plexiglas.

4. Dimensions of Plexiglas Planar Phantom

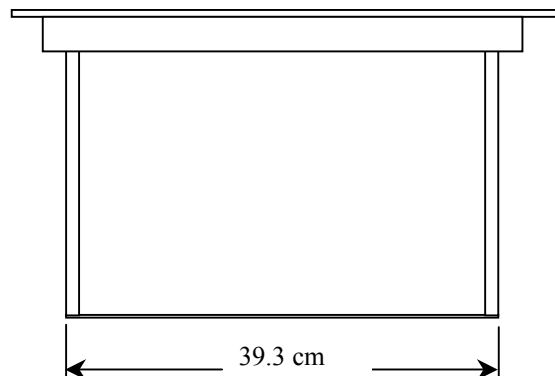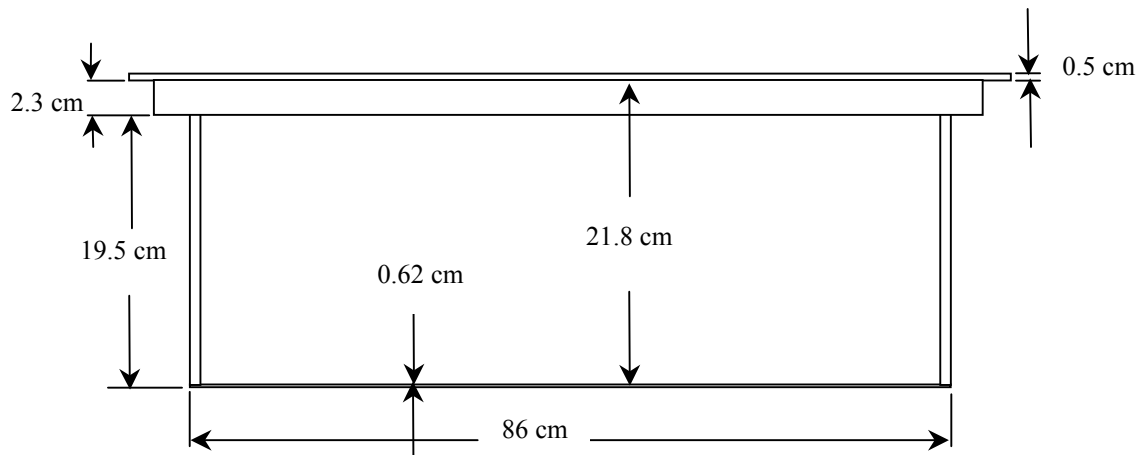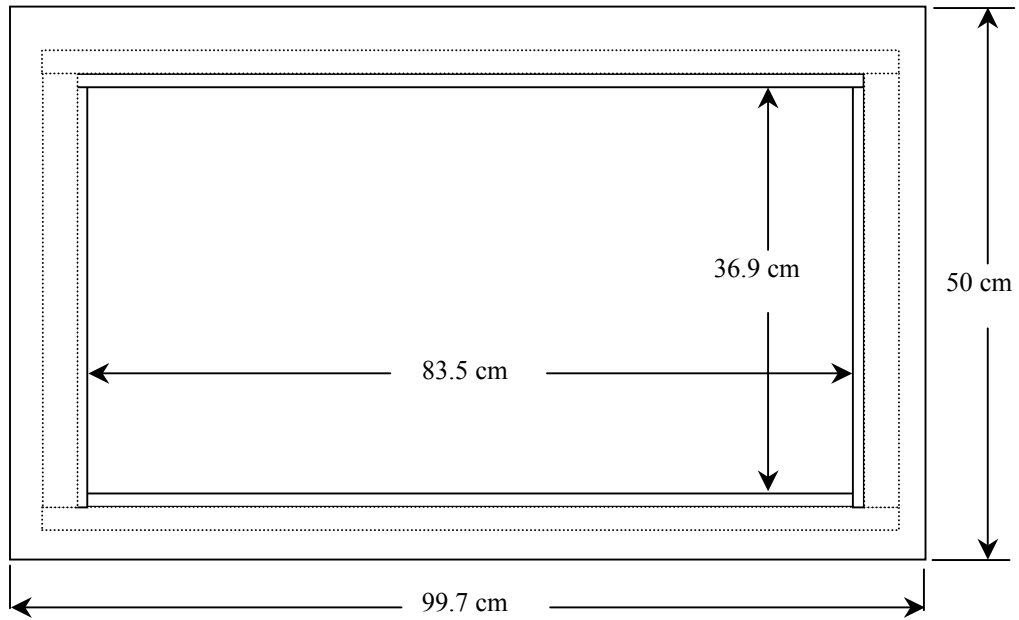

5. 450MHz System Validation Setup



450MHz System Validation Setup



6. Measurement Conditions

The planar phantom was filled with brain simulating tissue having the following parameters at 450MHz:

Relative Permittivity: 43.7
 Conductivity: 0.88 mho/m
 Fluid Temperature: 22.0 °C
 Fluid Depth: ≥ 15.0 cm

Environmental Conditions:


Ambient Temperature: 22.1 °C
 Humidity: 49 %
 Barometric Pressure: 102.8 kPa

The 450MHz simulated brain tissue mixture consists of the following ingredients:

| Ingredient | Percentage by weight |
|--|--|
| Water | 38.56% |
| Sugar | 56.32% |
| Salt | 3.95% |
| HEC | 0.98% |
| Dowicil 75 | 0.19% |
| 450MHz Target Dielectric Parameters at 22 °C | $\epsilon_r = 43.5$ $\sigma = 0.87 \text{ S/m}$ |

7. SAR Measurement

The SAR measurement was performed with the E-field probe in mechanical detection mode only. The setup and determination of the forward power into the dipole was performed using the following procedures.

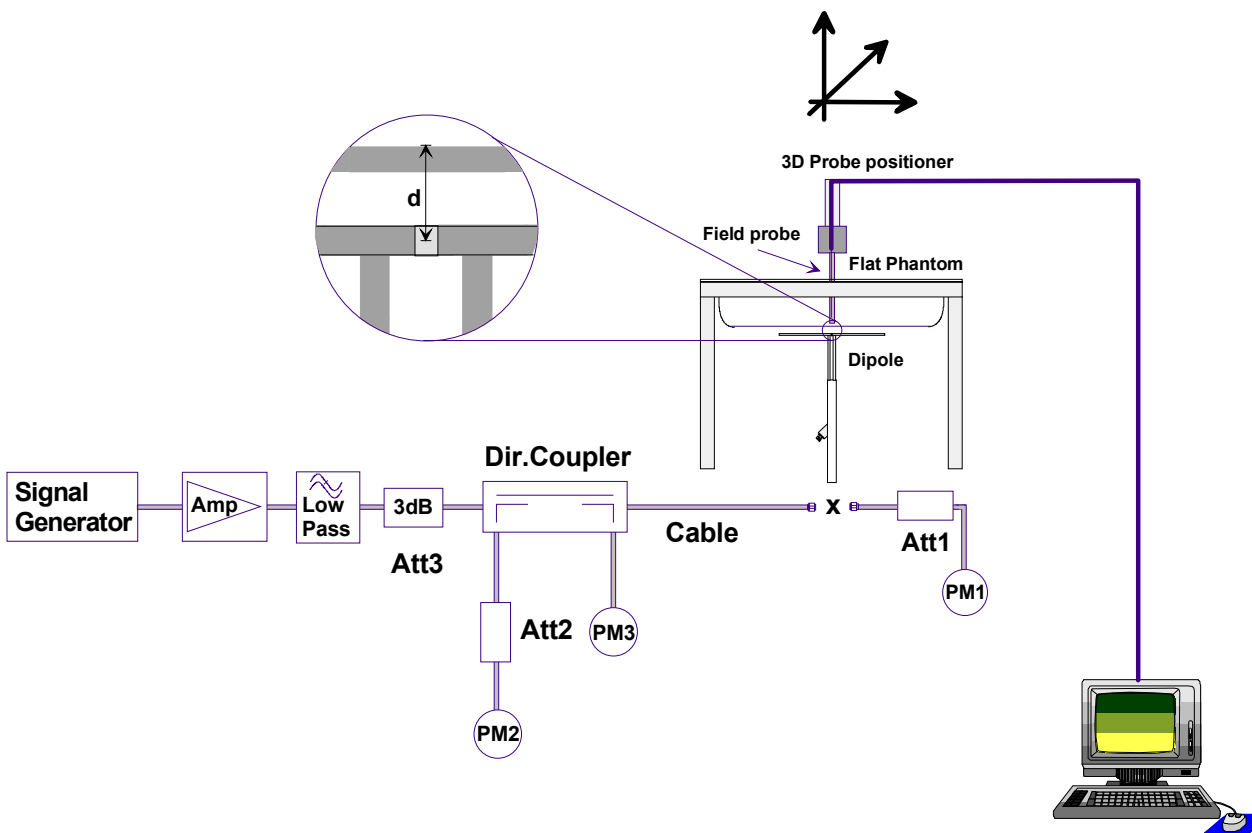

First the power meter PM1 (including attenuator Att1) is connected to the cable to measure the forward power at the location of the dipole connector (X). The signal generator is adjusted for the desired forward power at the dipole connector (taking into account the attenuation of Att1) as read by power meter PM2. After connecting the cable to the dipole, the signal generator is readjusted for the same reading at power meter PM2. If the signal generator does not allow adjustment in 0.01dB steps, the remaining difference at PM2 must be taken into consideration. PM3 records the reflected power from the dipole to ensure that the value is not changed from the previous value. The reflected power should be 20dB below the forward power.

8. Validation Dipole SAR Test Results

Ten SAR measurements were performed in order to achieve repeatability and to establish an average target value.

| Validation Measurement | SAR @ 0.25W Input averaged over 1g | SAR @ 1W Input averaged over 1g | SAR @ 0.25W Input averaged over 10g | SAR @ 1W Input averaged over 10g | Peak SAR @ 0.25W Input |
|------------------------|------------------------------------|---------------------------------|-------------------------------------|----------------------------------|------------------------|
| Test 1 | 1.29 | 5.16 | 0.810 | 3.24 | 2.28 |
| Test 2 | 1.31 | 5.24 | 0.827 | 3.31 | 2.31 |
| Test 3 | 1.30 | 5.20 | 0.823 | 3.29 | 2.29 |
| Test 4 | 1.30 | 5.20 | 0.822 | 3.29 | 2.29 |
| Test 5 | 1.29 | 5.16 | 0.819 | 3.28 | 2.28 |
| Test 6 | 1.30 | 5.20 | 0.826 | 3.30 | 2.28 |
| Test 7 | 1.31 | 5.24 | 0.826 | 3.30 | 2.30 |
| Test 8 | 1.31 | 5.24 | 0.829 | 3.32 | 2.30 |
| Test 9 | 1.30 | 5.20 | 0.822 | 3.29 | 2.28 |
| Test 10 | 1.31 | 5.24 | 0.822 | 3.29 | 2.33 |
| Average Value | 1.30 | 5.21 | 0.823 | 3.29 | 2.29 |

The results have been normalized to 1W (forward power) into the dipole.

IEEE Target over 1cm³ (1g) of tissue: 1.23 mW/g (+/- 10%)

Averaged over 1cm (1g) of tissue: 5.21 mW/g

Averaged over 10cm (10g) of tissue: 3.29 mW/g

Test Date: 11/04/03

DUT: Dipole 450MHz; Model: D450V2; Type: System Performance Check; Serial: 136

Ambient Temp: 22.1°C; Fluid Temp: 22.0°C; Barometric Pressure: 102.8 kPa; Humidity: 49%

Communication System: CW
Forward Conducted Power: 250 mW
Frequency: 450 MHz; Duty Cycle: 1:1
Medium: HSL450 ($\sigma = 0.88$ mho/m, $\epsilon_r = 43.7$, $\rho = 1000$ kg/m³)

- Probe: ET3DV6 - SN1387; ConvF(7.5, 7.5, 7.5); Calibrated: 26/02/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn370; Calibrated: 19/05/2003
- Phantom: Validation Planar; Type: Plexiglas; Serial: 137
- Measurement SW: DASy4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 116

450 MHz Validation/Area Scan (6x11x1): Measurement grid: dx=15mm, dy=15mm

Reference Value = 39 V/m

Power Drift = -0.08 dB

Maximum value of SAR = 1.3 mW/g


450 MHz Validation/Zoom Scan 8 (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm


Peak SAR (extrapolated) = 2.28 W/kg

SAR(1 g) = 1.3 mW/g; SAR(10 g) = 0.822 mW/g

Reference Value = 39 V/m

Power Drift = 0.08 dB

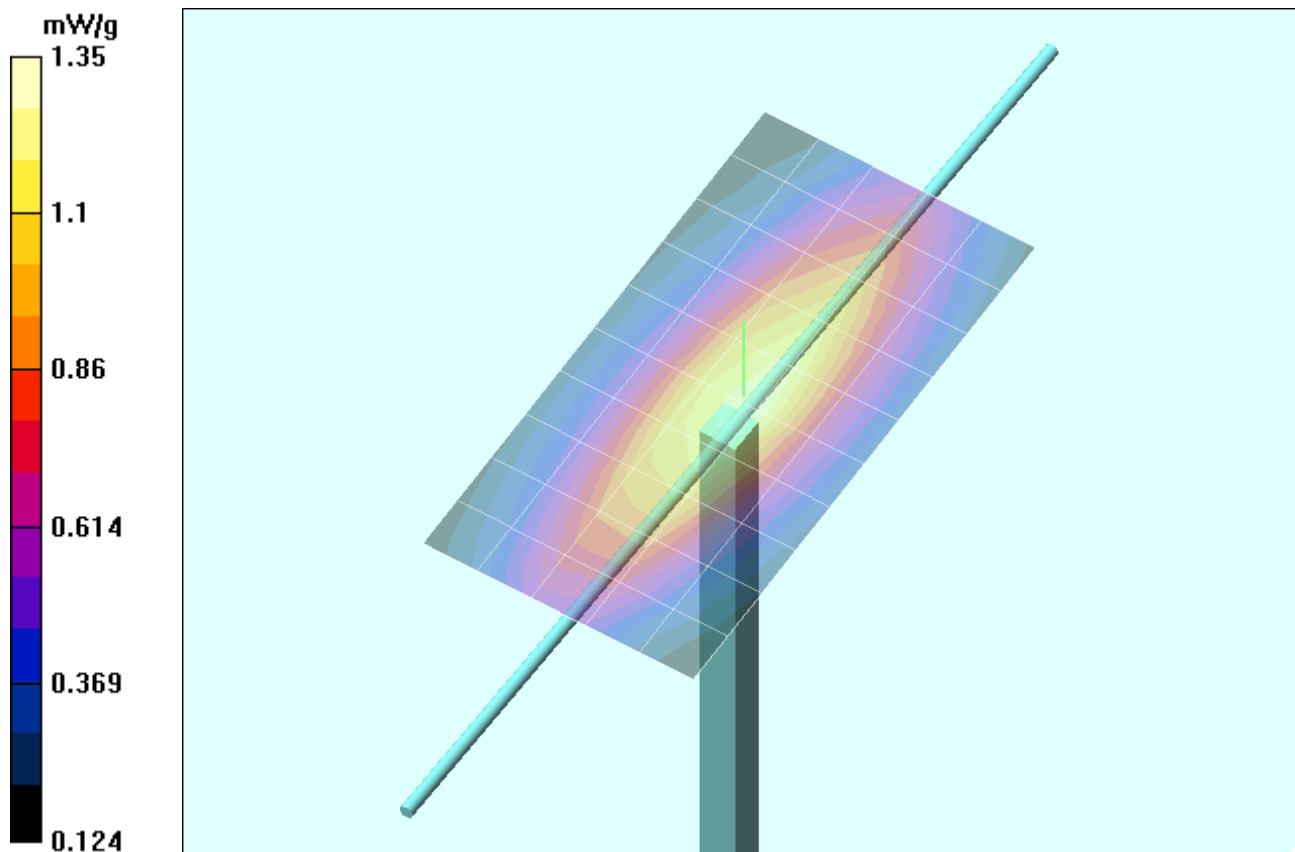

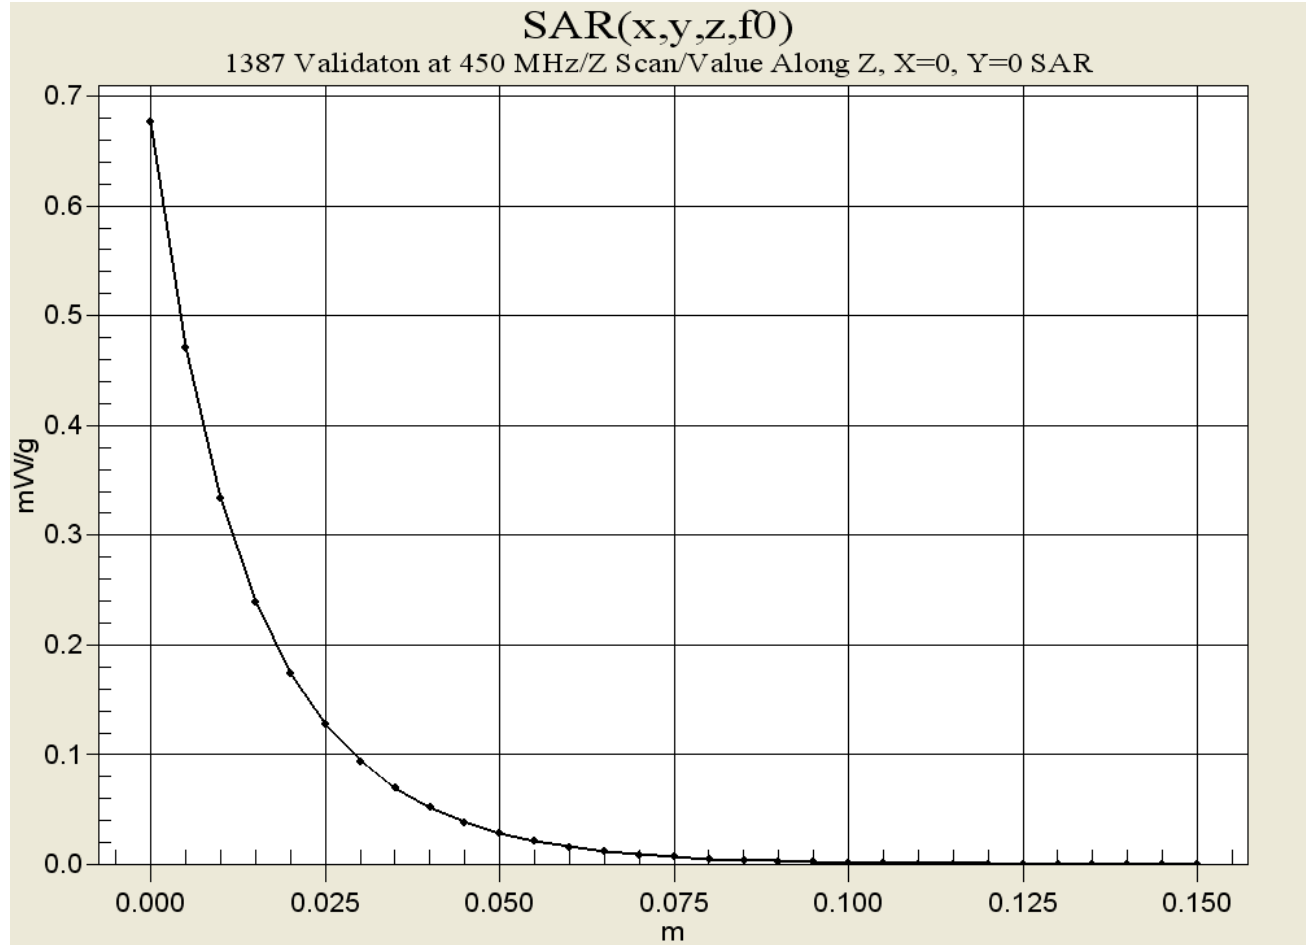

450MHz System Validation

Measured Fluid Dielectric Parameters (Brain)

November 04, 2003

| Frequency | ϵ' | ϵ'' |
|----------------|-------------|--------------|
| 350.000000 MHz | 46.2660 | 40.8224 |
| 360.000000 MHz | 45.9937 | 40.0986 |
| 370.000000 MHz | 45.7556 | 39.4543 |
| 380.000000 MHz | 45.5625 | 38.7387 |
| 390.000000 MHz | 45.2820 | 38.1140 |
| 400.000000 MHz | 45.0146 | 37.4981 |
| 410.000000 MHz | 44.7508 | 36.9734 |
| 420.000000 MHz | 44.5046 | 36.4917 |
| 430.000000 MHz | 44.2494 | 35.9460 |
| 440.000000 MHz | 43.9621 | 35.5647 |
| 450.000000 MHz | 43.7384 | 35.2106 |
| 460.000000 MHz | 43.5513 | 34.7930 |
| 470.000000 MHz | 43.2846 | 34.3970 |
| 480.000000 MHz | 43.0654 | 33.9576 |
| 490.000000 MHz | 42.8566 | 33.6391 |
| 500.000000 MHz | 42.6744 | 33.2270 |
| 510.000000 MHz | 42.5036 | 32.8459 |
| 520.000000 MHz | 42.3492 | 32.5261 |
| 530.000000 MHz | 42.1783 | 32.1727 |
| 540.000000 MHz | 41.9985 | 31.7385 |
| 550.000000 MHz | 41.8097 | 31.4862 |

| | |
|------------------|-----------------------|
| Test Report S/N: | 101204ALH-T569-S90U |
| Test Date(s): | October 20-24, 2004 |
| Test Type: | FCC/IC SAR Evaluation |

APPENDIX D - PROBE CALIBRATION

Client **Celltech Labs**

CALIBRATION CERTIFICATE

Object(s) **ET3DV6 - SN:1590**

Calibration procedure(s) **QA CAL-01.v2
Calibration procedure for dosimetric E-field probes**

Calibration date: **May 24, 2004**

Condition of the calibrated item **In Tolerance (according to the specific calibration document)**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature 22 +/- 2 degrees Celsius and humidity < 75%.

Calibration Equipment used (M&TE critical for calibration)

| Model Type | ID # | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
|-----------------------------------|----------------|---|------------------------|
| Power meter EPM E4419B | GB41293874 | 5-May-04 (METAS, No 251-00388) | May-05 |
| Power sensor E4412A | MY41495277 | 5-May-04 (METAS, No 251-00388) | May-05 |
| Reference 20 dB Attenuator | SN: 5086 (20b) | 3-May-04 (METAS, No 251-00389) | May-05 |
| Fluke Process Calibrator Type 702 | SN: 6295803 | 8-Sep-03 (Sintrel SCS No. E-030020) | Sep-04 |
| Power sensor HP 8481A | MY41092180 | 18-Sep-02 (SPEAG, in house check Oct-03) | In house check: Oct 05 |
| RF generator HP 8684C | US3642U01700 | 4-Aug-99 (SPEAG, in house check Aug-02) | In house check: Aug-05 |
| Network Analyzer HP 8753E | US37390585 | 18-Oct-01 (SPEAG, in house check Oct-03) | In house check: Oct 05 |

Calibrated by: **Name: Nico Vetterli, Function: Technician, Signature: [Handwritten Signature]**

Approved by: **Name: Katja Pokovic, Function: Laboratory Director, Signature: [Handwritten Signature]**

Date issued: May 24, 2004

This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed.

Probe ET3DV6

SN:1590

| | |
|------------------|----------------|
| Manufactured: | March 19, 2001 |
| Last calibrated: | May 15, 2003 |
| Recalibrated: | May 24, 2004 |

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

DASY - Parameters of Probe: ET3DV6 SN:1590

| Sensitivity in Free Space | | Diode Compression ^A | |
|---------------------------|--|--------------------------------|-------|
| NormX | 1.85 $\mu\text{V}/(\text{V}/\text{m})^2$ | DCP X | 91 mV |
| NormY | 2.01 $\mu\text{V}/(\text{V}/\text{m})^2$ | DCP Y | 91 mV |
| NormZ | 1.73 $\mu\text{V}/(\text{V}/\text{m})^2$ | DCP Z | 91 mV |

Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 7.

Boundary Effect

Head 900 MHz Typical SAR gradient: 5 % per mm

| | | | |
|---|------------------------------|--------|--------|
| Sensor Center to Phantom Surface Distance | | 3.7 mm | 4.7 mm |
| SAR _{be} [%] | Without Correction Algorithm | 8.0 | 4.4 |
| SAR _{be} [%] | With Correction Algorithm | 0.1 | 0.2 |

Head 1800 MHz Typical SAR gradient: 10 % per mm

| | | | |
|---|------------------------------|--------|--------|
| Sensor Center to Phantom Surface Distance | | 3.7 mm | 4.7 mm |
| SAR _{be} [%] | Without Correction Algorithm | 12.2 | 8.5 |
| SAR _{be} [%] | With Correction Algorithm | 0.2 | 0.1 |

Sensor Offset


| | |
|----------------------------|--------------|
| Probe Tip to Sensor Center | 2.7 mm |
| Optical Surface Detection | in tolerance |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.




^A numerical linearization parameter: uncertainty not required

Frequency Response of E-Field

(TEM-Cell:ifi110, Waveguide R22)


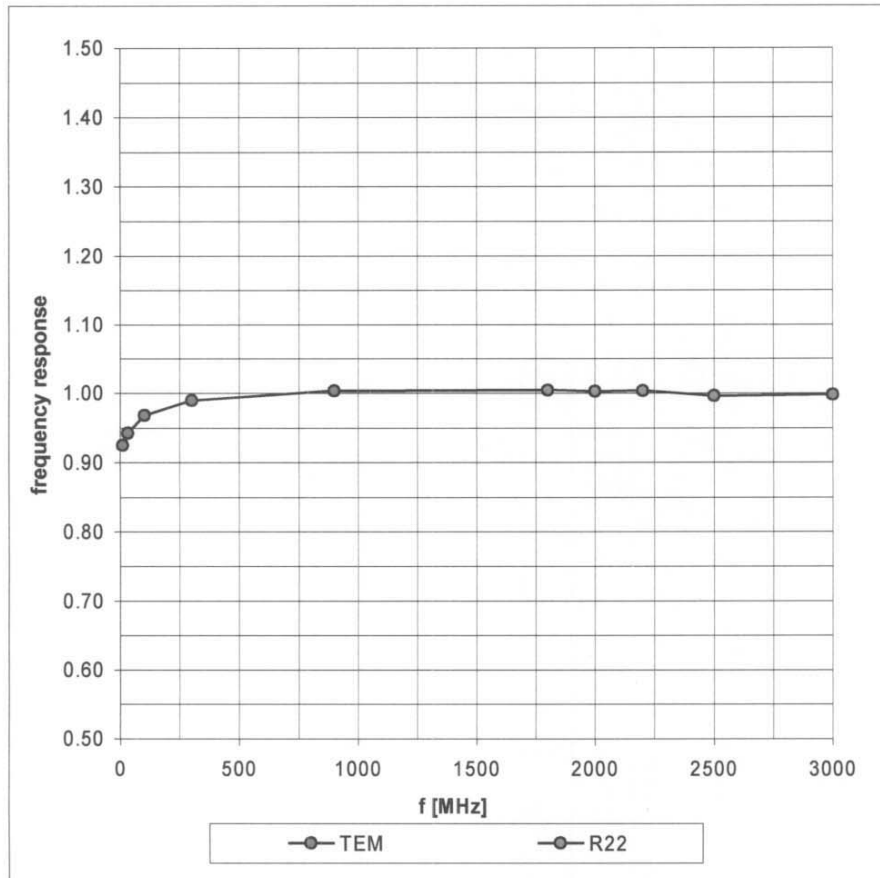


Receiving Pattern (ϕ), $\theta = 0^\circ$

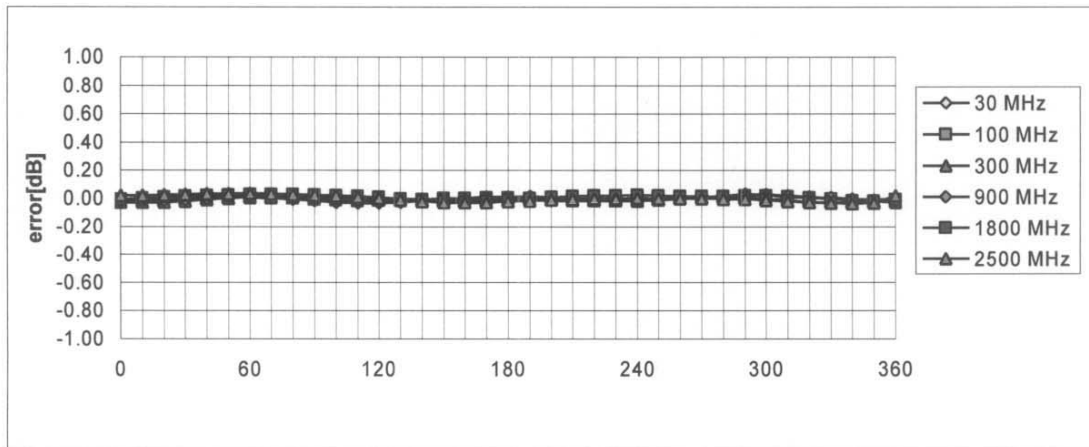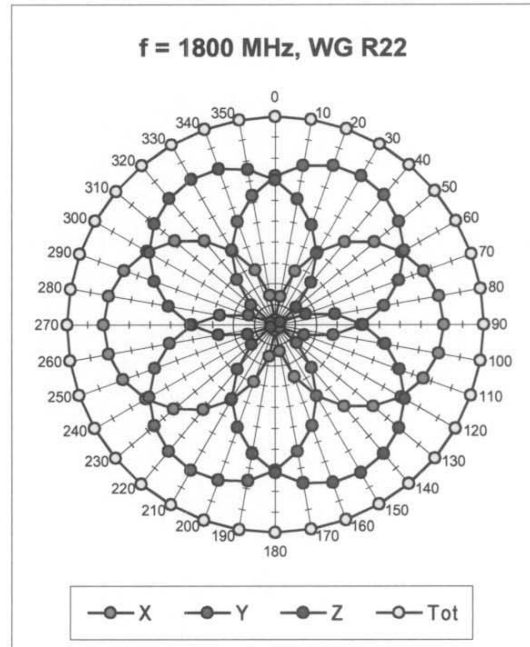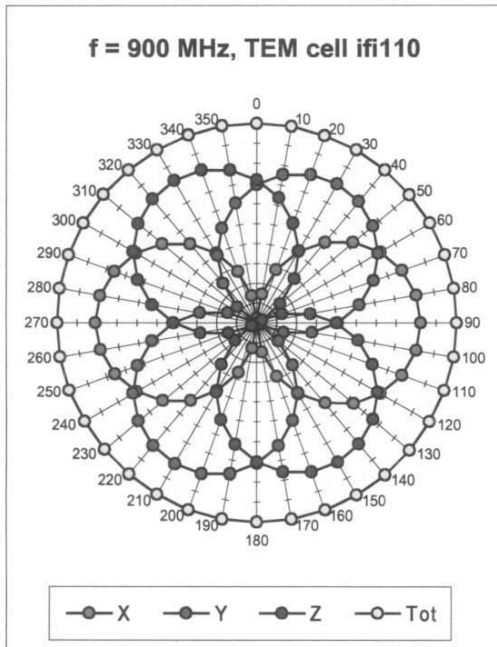



Axial Isotropy Error $\lt; \pm 0.2 \text{ dB}$

Dynamic Range f(SAR_{head}) (Waveguide R22)

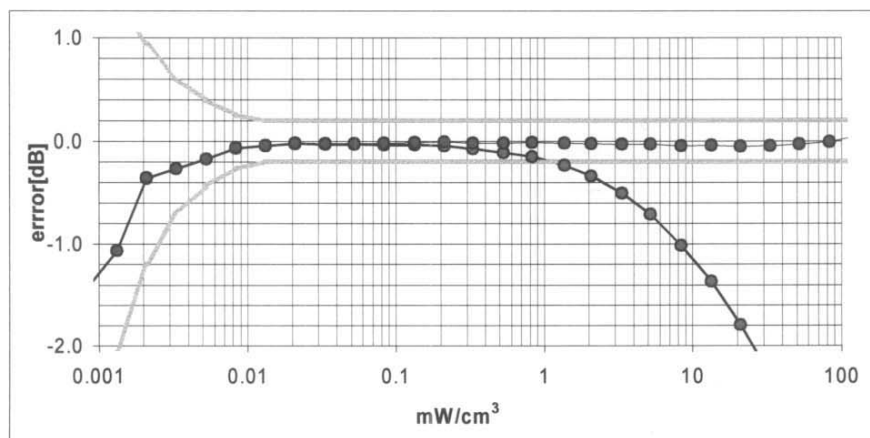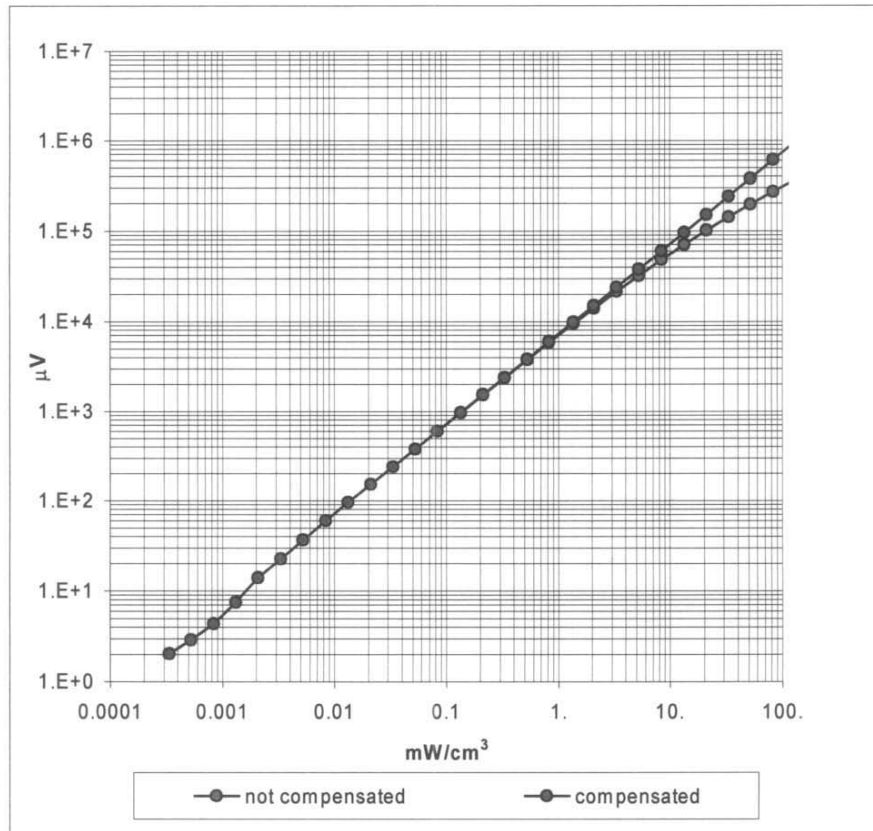

Probe Linearity Error < ± 0.2 dB

Conversion Factor Assessment

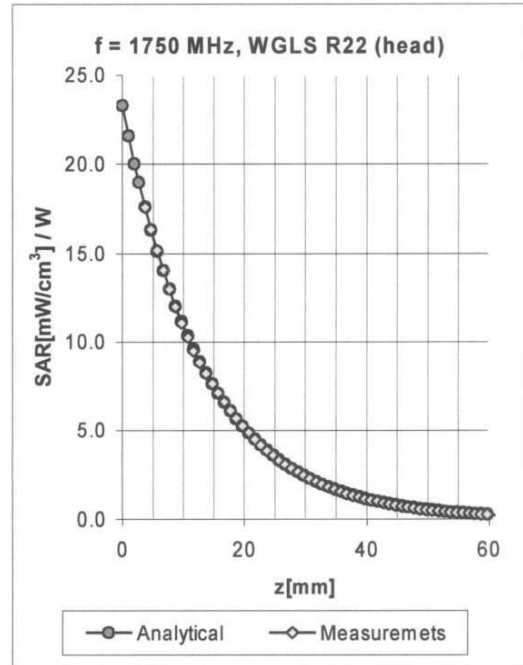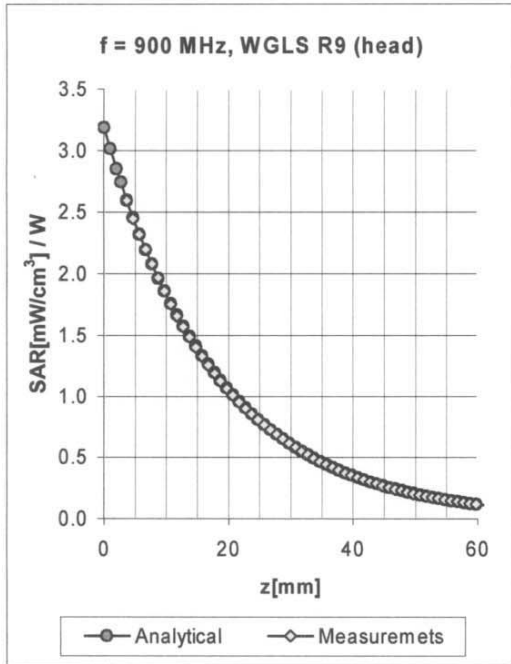


| f [MHz] | Validity [MHz] ^B | Tissue | Permittivity | Conductivity | Alpha | Depth | ConvF | Uncertainty |
|---------|-----------------------------|--------|--------------|--------------|-------|-------|--------------|-------------|
| 835 | 750-950 | Head | 41.5 ± 5% | 0.90 ± 5% | 0.68 | 1.64 | 6.71 ± 11.9% | (k=2) |
| 1750 | 1700-1800 | Head | 40.0 ± 5% | 1.40 ± 5% | 0.43 | 2.67 | 5.28 ± 9.7% | (k=2) |
| 1900 | 1850-1950 | Head | 40.0 ± 5% | 1.40 ± 5% | 0.46 | 2.81 | 5.03 ± 9.7% | (k=2) |
| 2450 | 2400-2500 | Head | 39.2 ± 5% | 1.80 ± 5% | 0.81 | 1.95 | 4.44 ± 9.7% | (k=2) |
| 835 | 750-950 | Body | 55.2 ± 5% | 0.97 ± 5% | 0.49 | 1.99 | 6.54 ± 11.9% | (k=2) |
| 1750 | 1700-1800 | Body | 53.3 ± 5% | 1.52 ± 5% | 0.50 | 2.87 | 4.68 ± 9.7% | (k=2) |
| 1900 | 1850-1950 | Body | 53.3 ± 5% | 1.52 ± 5% | 0.52 | 2.93 | 4.58 ± 9.7% | (k=2) |
| 2450 | 2400-2500 | Body | 52.7 ± 5% | 1.95 ± 5% | 0.91 | 1.78 | 4.22 ± 9.7% | (k=2) |

^B The total standard uncertainty is calculated as root-sum-square of standard uncertainty of the Conversion Factor at calibration frequency and the standard uncertainty for the indicated frequency band.

Deviation from Isotropy in HSL

Error (θ, ϕ), $f = 900$ MHz

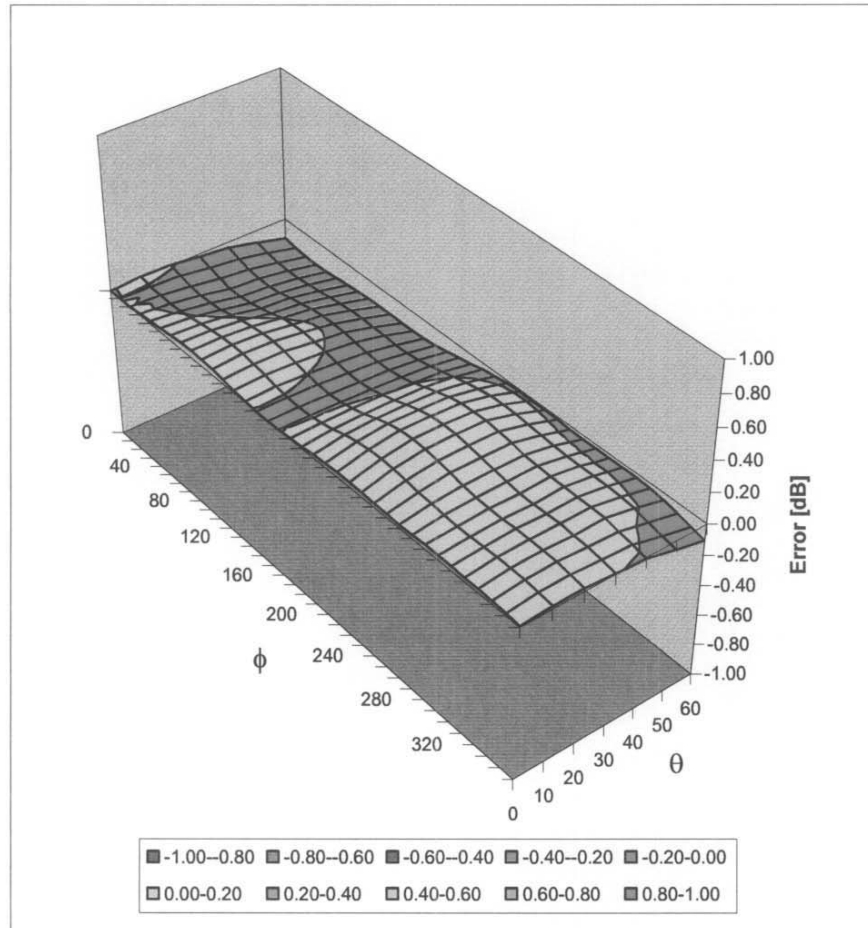

Spherical Isotropy Error $< \pm 0.4$ dB

Additional Conversion Factors for Dosimetric E-Field Probe

Type:

ET3DV6

Serial Number:

1590

Place of Assessment:

Zurich

Date of Assessment:


May 25, 2004

Probe Calibration Date:

May 24, 2004

Schmid & Partner Engineering AG hereby certifies that conversion factor(s) of this probe have been evaluated on the date indicated above. The assessment was performed using the FDTD numerical code SEMCAD of Schmid & Partner Engineering AG. Since the evaluation is coupled with measured conversion factors, it has to be recalculated yearly, i.e., following the re-calibration schedule of the probe. The uncertainty of the numerical assessment is based on the extrapolation from measured value at 900 MHz or at 1800 MHz.

Assessed by:



Dosimetric E-Field Probe ET3DV6 SN:1590Conversion factor (\pm standard deviation)

| | | | |
|----------------|-------|--------------------------------|---|
| 150 MHz | ConvF | 9.1 \pm 8% | $\epsilon_r = 52.3 \pm 5\%$ $\sigma = 0.76 \pm 5\%$ mho/m (head tissue) |
| 300 MHz | ConvF | 7.9 \pm 8% | $\epsilon_r = 45.3 \pm 5\%$ $\sigma = 0.87 \pm 5\%$ mho/m (head tissue) |
| 450 MHz | ConvF | 7.5 \pm 8% | $\epsilon_r = 43.5 \pm 5\%$ $\sigma = 0.87 \pm 5\%$ mho/m (head tissue) |
| 150 MHz | ConvF | 8.8 \pm 8% | $\epsilon_r = 61.9 \pm 5\%$ $\sigma = 0.80 \pm 5\%$ mho/m (body tissue) |
| 450 MHz | ConvF | 7.7 \pm 8% | $\epsilon_r = 56.7 \pm 5\%$ $\sigma = 0.94 \pm 5\%$ mho/m (body tissue) |

Important Note:

For numerically assessed probe conversion factors, parameters Alpha and Delta in the DASY software must have the following entries: Alpha = 0 and Delta = 1.

Please see also Section 4.7 of the DASY4 Manual.

| | |
|------------------|-----------------------|
| Test Report S/N: | 101204ALH-T569-S90U |
| Test Date(s): | October 20-24, 2004 |
| Test Type: | FCC/IC SAR Evaluation |

APPENDIX E - MEASURED FLUID DIELECTRIC PARAMETERS

450 MHz System Performance Check & DUT Evaluation (Face)

Measured Fluid Dielectric Parameters (Brain)

October 20, 2004

| Frequency | e' | e'' |
|----------------|---------|---------|
| 350.000000 MHz | 46.4441 | 40.4550 |
| 360.000000 MHz | 46.1177 | 39.7237 |
| 370.000000 MHz | 45.8431 | 39.1833 |
| 380.000000 MHz | 45.6592 | 38.4835 |
| 390.000000 MHz | 45.4329 | 37.8138 |
| 400.000000 MHz | 45.1993 | 37.3249 |
| 410.000000 MHz | 44.9621 | 36.7377 |
| 420.000000 MHz | 44.7606 | 36.1932 |
| 430.000000 MHz | 44.4798 | 35.6564 |
| 440.000000 MHz | 44.2192 | 35.1798 |
| 450.000000 MHz | 43.9729 | 34.7886 |
| 460.000000 MHz | 43.7210 | 34.4712 |
| 470.000000 MHz | 43.5087 | 34.1079 |
| 480.000000 MHz | 43.2986 | 33.7598 |
| 490.000000 MHz | 43.0088 | 33.4051 |
| 500.000000 MHz | 42.7762 | 33.0220 |
| 510.000000 MHz | 42.5868 | 32.6473 |
| 520.000000 MHz | 42.3825 | 32.3391 |
| 530.000000 MHz | 42.2262 | 31.9861 |
| 540.000000 MHz | 42.0457 | 31.6028 |
| 550.000000 MHz | 41.9143 | 31.2871 |

450 MHz System Performance Check & DUT Evaluation (Face)

Measured Fluid Dielectric Parameters (Brain)

October 21, 2004

| Frequency | ϵ' | ϵ'' |
|----------------|-------------|--------------|
| 350.000000 MHz | 45.9099 | 39.9901 |
| 360.000000 MHz | 45.5994 | 39.2952 |
| 370.000000 MHz | 45.4525 | 38.7065 |
| 380.000000 MHz | 45.2669 | 38.1859 |
| 390.000000 MHz | 45.0034 | 37.8097 |
| 400.000000 MHz | 44.7155 | 37.1637 |
| 410.000000 MHz | 44.4632 | 36.5444 |
| 420.000000 MHz | 44.2163 | 35.9639 |
| 430.000000 MHz | 43.9795 | 35.3895 |
| 440.000000 MHz | 43.7226 | 34.9401 |
| 450.000000 MHz | 43.4754 | 34.5473 |
| 460.000000 MHz | 43.3226 | 34.2218 |
| 470.000000 MHz | 43.0673 | 33.9446 |
| 480.000000 MHz | 42.8164 | 33.6265 |
| 490.000000 MHz | 42.5299 | 33.2415 |
| 500.000000 MHz | 42.2314 | 32.9263 |
| 510.000000 MHz | 42.0842 | 32.5491 |
| 520.000000 MHz | 41.9602 | 32.1821 |
| 530.000000 MHz | 41.7926 | 31.8201 |
| 540.000000 MHz | 41.6273 | 31.3519 |
| 550.000000 MHz | 41.4032 | 31.0986 |

450 MHz DUT Evaluation (Body)

Measured Fluid Dielectric Parameters (Muscle)

October 21, 2004

| Frequency | ϵ' | ϵ'' |
|----------------|-------------|--------------|
| 350.000000 MHz | 58.6177 | 43.0377 |
| 360.000000 MHz | 58.3982 | 42.2875 |
| 370.000000 MHz | 58.1995 | 41.4694 |
| 380.000000 MHz | 57.9892 | 40.7382 |
| 390.000000 MHz | 57.8263 | 40.0449 |
| 400.000000 MHz | 57.7721 | 39.4488 |
| 410.000000 MHz | 57.6538 | 38.7233 |
| 420.000000 MHz | 57.5736 | 38.1843 |
| 430.000000 MHz | 57.4301 | 37.5601 |
| 440.000000 MHz | 57.2973 | 37.0180 |
| 450.000000 MHz | 57.0705 | 36.5550 |
| 460.000000 MHz | 56.9234 | 36.1606 |
| 470.000000 MHz | 56.7408 | 35.6972 |
| 480.000000 MHz | 56.5579 | 35.2430 |
| 490.000000 MHz | 56.3208 | 34.8358 |
| 500.000000 MHz | 56.1232 | 34.4883 |
| 510.000000 MHz | 55.9650 | 34.1282 |
| 520.000000 MHz | 55.7907 | 33.8182 |
| 530.000000 MHz | 55.6931 | 33.4520 |
| 540.000000 MHz | 55.6121 | 33.0041 |
| 550.000000 MHz | 55.5176 | 32.7254 |

450 MHz System Performance Check

Measured Fluid Dielectric Parameters (Brain)

October 22, 2004

| Frequency | e' | e'' |
|----------------|---------|---------|
| 350.000000 MHz | 45.3801 | 39.6430 |
| 360.000000 MHz | 45.1262 | 38.8494 |
| 370.000000 MHz | 44.8599 | 38.2234 |
| 380.000000 MHz | 44.6925 | 37.6719 |
| 390.000000 MHz | 44.4927 | 37.2167 |
| 400.000000 MHz | 44.2972 | 36.7209 |
| 410.000000 MHz | 44.1137 | 36.2473 |
| 420.000000 MHz | 43.9093 | 35.7792 |
| 430.000000 MHz | 43.7721 | 35.2446 |
| 440.000000 MHz | 43.5529 | 34.8320 |
| 450.000000 MHz | 43.2793 | 34.3714 |
| 460.000000 MHz | 43.0357 | 33.9179 |
| 470.000000 MHz | 42.7777 | 33.4865 |
| 480.000000 MHz | 42.5202 | 33.1090 |
| 490.000000 MHz | 42.1455 | 32.6978 |
| 500.000000 MHz | 41.8503 | 32.3769 |
| 510.000000 MHz | 41.5978 | 32.0462 |
| 520.000000 MHz | 41.4525 | 31.8094 |
| 530.000000 MHz | 41.3304 | 31.5778 |
| 540.000000 MHz | 41.2225 | 31.2174 |
| 550.000000 MHz | 41.0970 | 30.9585 |

450 MHz DUT Evaluation (Body)

Measured Fluid Dielectric Parameters (Muscle)

October 22, 2004

| Frequency | ϵ' | ϵ'' |
|----------------|-------------|--------------|
| 350.000000 MHz | 58.0021 | 42.3560 |
| 360.000000 MHz | 57.7280 | 41.5672 |
| 370.000000 MHz | 57.5589 | 40.8589 |
| 380.000000 MHz | 57.3966 | 40.1507 |
| 390.000000 MHz | 57.2843 | 39.4454 |
| 400.000000 MHz | 57.2496 | 38.8002 |
| 410.000000 MHz | 57.1622 | 38.1502 |
| 420.000000 MHz | 57.0575 | 37.6120 |
| 430.000000 MHz | 56.9383 | 37.0293 |
| 440.000000 MHz | 56.8046 | 36.5510 |
| 450.000000 MHz | 56.5972 | 36.0113 |
| 460.000000 MHz | 56.4093 | 35.6677 |
| 470.000000 MHz | 56.2102 | 35.1844 |
| 480.000000 MHz | 55.9877 | 34.7704 |
| 490.000000 MHz | 55.7430 | 34.3777 |
| 500.000000 MHz | 55.5711 | 34.0370 |
| 510.000000 MHz | 55.4175 | 33.6707 |
| 520.000000 MHz | 55.2868 | 33.3793 |
| 530.000000 MHz | 55.1567 | 33.0649 |
| 540.000000 MHz | 55.0655 | 32.6868 |
| 550.000000 MHz | 55.0057 | 32.3610 |

450 MHz System Performance Check

Measured Fluid Dielectric Parameters (Brain)

October 23, 2004

| Frequency | ϵ' | ϵ'' |
|----------------|-------------|--------------|
| 350.000000 MHz | 45.7729 | 40.0313 |
| 360.000000 MHz | 45.3739 | 39.3362 |
| 370.000000 MHz | 45.1563 | 38.6786 |
| 380.000000 MHz | 44.9662 | 38.0733 |
| 390.000000 MHz | 44.7405 | 37.4606 |
| 400.000000 MHz | 44.4812 | 36.9876 |
| 410.000000 MHz | 44.2627 | 36.4303 |
| 420.000000 MHz | 44.1101 | 35.9896 |
| 430.000000 MHz | 43.9169 | 35.4282 |
| 440.000000 MHz | 43.7002 | 34.9818 |
| 450.000000 MHz | 43.4161 | 34.5284 |
| 460.000000 MHz | 43.2093 | 34.2029 |
| 470.000000 MHz | 43.0215 | 33.7716 |
| 480.000000 MHz | 42.8115 | 33.3796 |
| 490.000000 MHz | 42.4683 | 32.9740 |
| 500.000000 MHz | 42.1925 | 32.5921 |
| 510.000000 MHz | 41.9587 | 32.3027 |
| 520.000000 MHz | 41.7807 | 31.9994 |
| 530.000000 MHz | 41.6029 | 31.6595 |
| 540.000000 MHz | 41.4919 | 31.3046 |
| 550.000000 MHz | 41.2500 | 31.0715 |

450 MHz DUT Evaluation (Body)

Measured Fluid Dielectric Parameters (Muscle)

October 23, 2004

| Frequency | ϵ' | ϵ'' |
|----------------|-------------|--------------|
| 350.000000 MHz | 58.3728 | 42.2720 |
| 360.000000 MHz | 58.0943 | 41.5182 |
| 370.000000 MHz | 57.9564 | 40.8484 |
| 380.000000 MHz | 57.8730 | 40.2013 |
| 390.000000 MHz | 57.6876 | 39.6344 |
| 400.000000 MHz | 57.5656 | 39.0187 |
| 410.000000 MHz | 57.4712 | 38.2482 |
| 420.000000 MHz | 57.3525 | 37.6674 |
| 430.000000 MHz | 57.2254 | 37.0230 |
| 440.000000 MHz | 57.0144 | 36.5287 |
| 450.000000 MHz | 56.8265 | 36.0602 |
| 460.000000 MHz | 56.7106 | 35.5867 |
| 470.000000 MHz | 56.4923 | 35.2168 |
| 480.000000 MHz | 56.2301 | 34.8086 |
| 490.000000 MHz | 55.9861 | 34.5194 |
| 500.000000 MHz | 55.8322 | 34.1182 |
| 510.000000 MHz | 55.6868 | 33.7295 |
| 520.000000 MHz | 55.6118 | 33.4056 |
| 530.000000 MHz | 55.5158 | 33.0472 |
| 540.000000 MHz | 55.4341 | 32.6319 |
| 550.000000 MHz | 55.2661 | 32.3142 |

450 MHz System Performance Check

Measured Fluid Dielectric Parameters (Brain)

October 24, 2004

| Frequency | ϵ' | ϵ'' |
|----------------|-------------|--------------|
| 350.000000 MHz | 45.9174 | 39.5864 |
| 360.000000 MHz | 45.6161 | 38.9816 |
| 370.000000 MHz | 45.3750 | 38.3796 |
| 380.000000 MHz | 45.2510 | 37.7493 |
| 390.000000 MHz | 45.0326 | 37.0988 |
| 400.000000 MHz | 44.8065 | 36.4815 |
| 410.000000 MHz | 44.6100 | 35.7264 |
| 420.000000 MHz | 44.3088 | 35.1713 |
| 430.000000 MHz | 44.0665 | 34.6048 |
| 440.000000 MHz | 43.8294 | 34.2638 |
| 450.000000 MHz | 43.5432 | 33.8997 |
| 460.000000 MHz | 43.2842 | 33.6309 |
| 470.000000 MHz | 42.9890 | 33.3446 |
| 480.000000 MHz | 42.7982 | 33.0814 |
| 490.000000 MHz | 42.5558 | 32.7688 |
| 500.000000 MHz | 42.3496 | 32.4125 |
| 510.000000 MHz | 42.1609 | 32.0176 |
| 520.000000 MHz | 42.0258 | 31.6122 |
| 530.000000 MHz | 41.8630 | 31.2104 |
| 540.000000 MHz | 41.6823 | 30.7711 |
| 550.000000 MHz | 41.5047 | 30.4951 |

450 MHz DUT Evaluation (Body)

Measured Fluid Dielectric Parameters (Muscle)

October 24, 2004

| Frequency | ϵ' | ϵ'' |
|----------------|-------------|--------------|
| 350.000000 MHz | 59.0372 | 42.3676 |
| 360.000000 MHz | 58.8213 | 41.6658 |
| 370.000000 MHz | 58.6414 | 40.9821 |
| 380.000000 MHz | 58.5950 | 40.2525 |
| 390.000000 MHz | 58.4174 | 39.4596 |
| 400.000000 MHz | 58.2791 | 38.7385 |
| 410.000000 MHz | 58.1348 | 37.9674 |
| 420.000000 MHz | 57.9498 | 37.2884 |
| 430.000000 MHz | 57.7888 | 36.6538 |
| 440.000000 MHz | 57.6263 | 36.1821 |
| 450.000000 MHz | 57.3534 | 35.7904 |
| 460.000000 MHz | 57.2113 | 35.5198 |
| 470.000000 MHz | 57.0030 | 35.2004 |
| 480.000000 MHz | 56.8775 | 34.8852 |
| 490.000000 MHz | 56.7193 | 34.5533 |
| 500.000000 MHz | 56.5760 | 34.1782 |
| 510.000000 MHz | 56.4135 | 33.7696 |
| 520.000000 MHz | 56.3477 | 33.3194 |
| 530.000000 MHz | 56.2089 | 32.8347 |
| 540.000000 MHz | 56.0940 | 32.3360 |
| 550.000000 MHz | 55.9554 | 32.0268 |