


11/29/01

**Sharp (M/N: UX-CL220) (Left Tilt, Low/Ch-1/2405M, 50% Duty Cycle)**

Generic Twin Phantom; Section: Position: ; Frequency: 2450 MHz  
Probe: ET3DV6 - SN1577; ConvF(4.90,4.90,4.90); Crest factor: 1.0; Head 2450MHz:  $\sigma = 1.88 \text{ mho/m}$   $\epsilon_r = 39.5$   $\rho = 1.00 \text{ g/cm}^3$   
; 0  
Z-Axis: Dx = 0.0, Dy = 0.0, Dz = 2.0

Liquid Temperature: 23.8°C

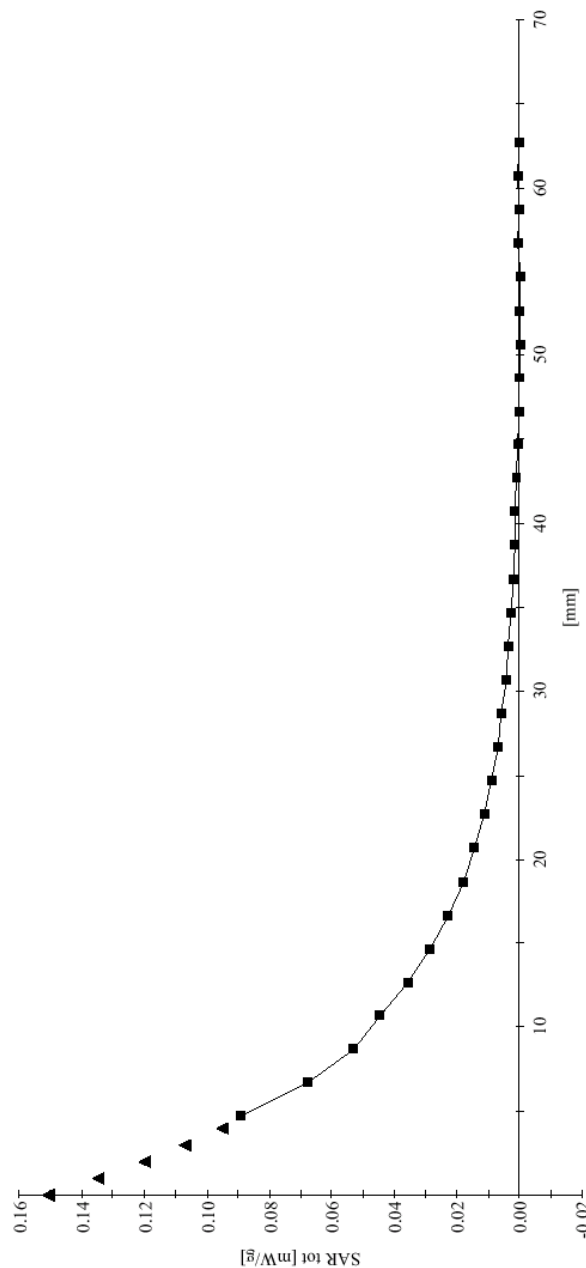


COMPLIANCE CERTIFICATION SERVICES

11/30/01

# Sharp (M/N: UX-CL220) (Right Cheek, High/Ch-40/2475M, 50% Duty Cycle)

Generic Twin Phantom: Right Cheek Section; Position: (72°, 65°); Frequency: 2450 MHz  
Probe: ET3DV6 - SN1577; ConvF(4,90,4,90,4,90); Crest factor: 1.0; Head 2450MHz:  $\sigma = 1.88$  mho/m  $\epsilon_r = 39.5$   $\rho = 1.00$  g/cm<sup>3</sup>  
Cube 5x5x7: SAR (1g): 0.0568 mW/g; SAR (10g): 0.0288 mW/g; (Worst-case extrapolation)  
Coarse: Dx = 15.0, Dy = 15.0, Dz = 10.0

Liquid Temperature: 23.2°C

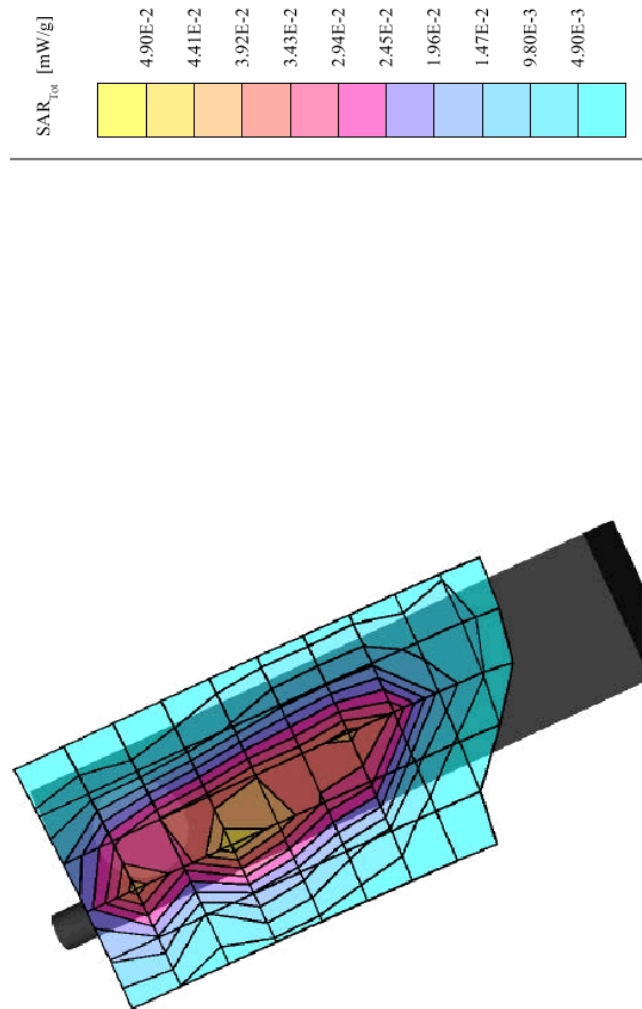


COMPLIANCE CERTIFICATION SERVICES

11/30/01

**Sharp (M/N: UX-CL220) (Right Cheek, High/Ch-40/2475M, 50% Duty Cycle)**

Generic Twin Phantom; Section; Position: ; Frequency: 2450 MHz  
Probe: ET3DV6 - SNI577; ConvF(4.90,4.90,4.90); Crest factor: 1.0; Head 2450MHz:  $\sigma = 1.88$  mho/m  $\epsilon_r = 39.5$   $\rho = 1.00$  g/cm<sup>3</sup>  
; , 0  
Z-Axis: Dx = 0.0, Dy = 0.0, Dz = 2.0

Liquid Temperature: 23.2°C

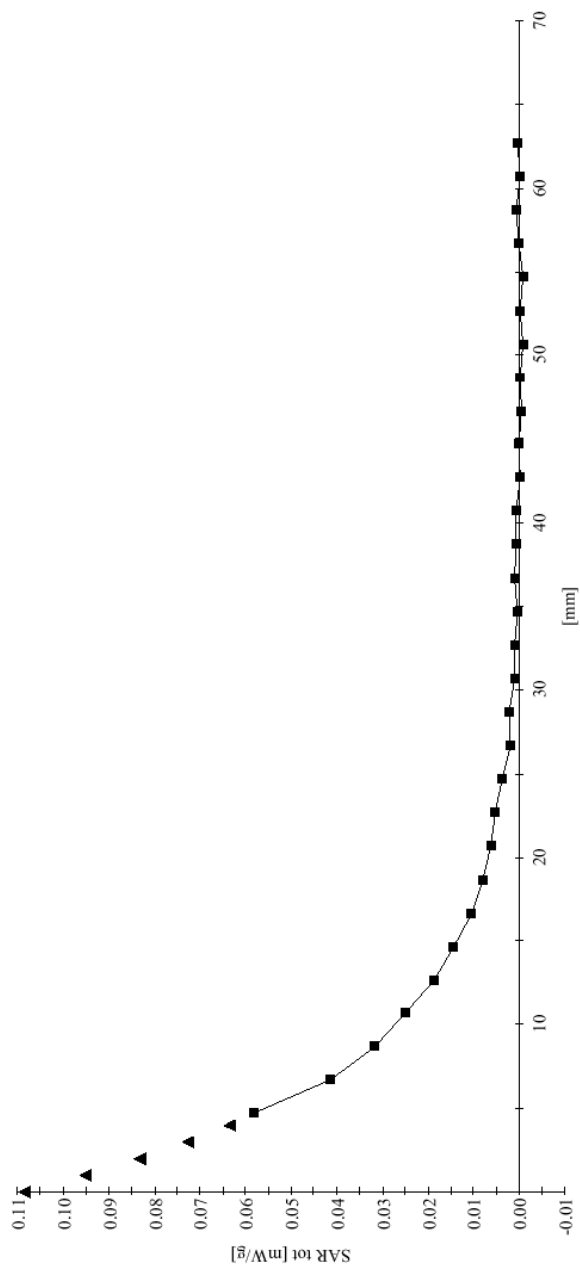


COMPLIANCE CERTIFICATION SERVICES

11/30/01

# Sharp (M/N: UX-CL220) (Right Tilt, High/Ch-40/2475M, 50% Duty Cycle)

Generic Twin Phantom; Right Hand Section; Position: (80° 65°); Frequency: 2450 MHz  
Probe: ET3DV6 - SN1577; ConvF(4.90,4.90,4.90); Crest factor: 1.0; Head 2450MHz:  $\sigma = 1.88$  mho/m  $\epsilon_r = 39.5$   $\rho = 1.00$  g/cm<sup>3</sup>  
Cube 5x5x7: SAR (1g): 0.0827 mW/g, SAR (10g): 0.0424 mW/g, (Worst-case extrapolation)  
Coarse: Dx = 20.0, Dy = 20.0, Dz = 10.0

Liquid Temperature: 23.4°C

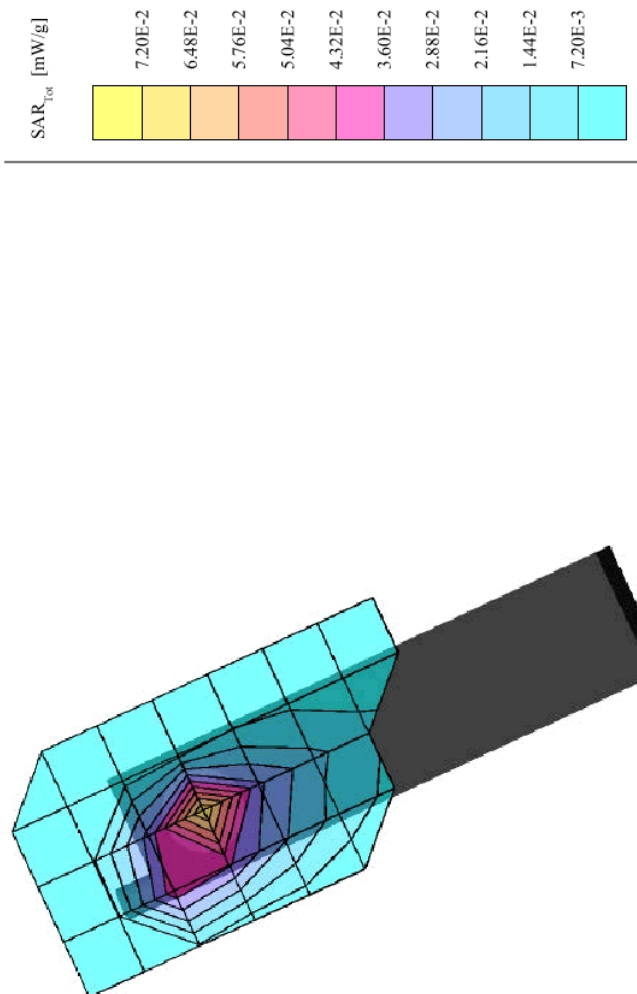


COMPLIANCE CERTIFICATION SERVICES

11/30/01

**Sharp (M/N: UX-CL220) (Right Tilt, High/Ch-40/2475M, 50% Duty Cycle)**

Generic Twin Phantom; Section; Position; Frequency: 2450 MHz  
Probe: ET3DV6 - SN1577; ConvF(4.90,4.90,4.90); Crest factor: 1.0; Head 2450MHz:  $\sigma = 1.88 \text{ mho/m}$   $\epsilon_r = 39.5$   $\rho = 1.00 \text{ g/cm}^3$   
; 0  
Z-Axis: Dx = 0.0, Dy = 0.0, Dz = 2.0

Liquid Temperature: 23.4°C

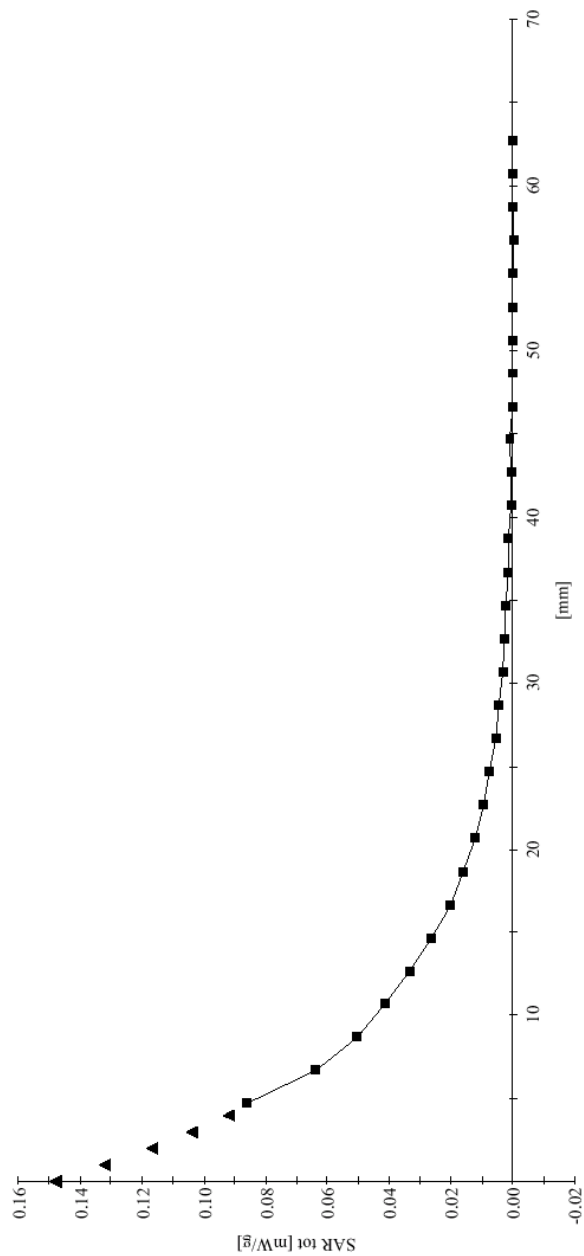


COMPLIANCE CERTIFICATION SERVICES

11/30/01

**Sharp (M/N: UX-CL220) (Body Configuration, 15mm Separation, High/Ch-40/2475M, 50% Duty Cycle)**

Generic Twin Phantom; Flat Section; Position: (270°, 270°); Frequency: 2450 MHz  
Probe: ET3DV6 - SN1577M; ConvF(4.40,4.40,4.40); Crest factor: 1.0; Muscle 2450 MHz:  $\sigma = 2.02$  mho/m  $\epsilon_r = 51.5$   $\rho = 1.00$  g/cm<sup>3</sup>  
Cube 5x5x7: SAR (1g): 0.0131 mW/g; SAR (10g): 0.0066 mW/g; (Worst-case extrapolation)  
Coarse: Dx = 20.0, Dy = 20.0, Dz = 10.0

Liquid Temperature: 23.2°C

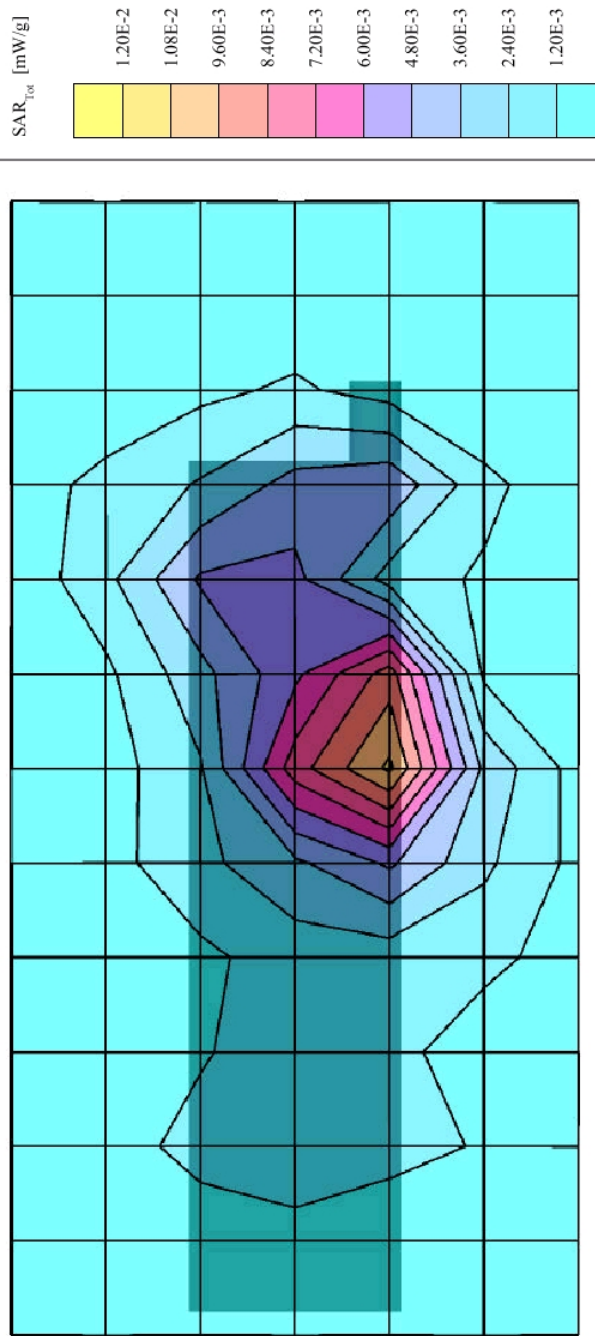


COMPLIANCE CERTIFICATION SERVICES

11/30/01

**Sharp (M/N: UX-CL220) (Body Configuration, 15mm Separation, High/Ch-40/2475M, 50% Duty Cycle)**

Generic Twin Phantom; Section: Position: ; Frequency: 2450 MHz  
Probe: ET3DV6 - SNI577M; ConvF(4.40,4.40,4.40); Crest factor: 1.0; Muscle 2450 MHz:  $\sigma = 2.02 \text{ mho/m}$   $\epsilon_r = 51.5$   $\rho = 1.00 \text{ g/cm}^3$   
; , 0  
Z-Axis: Dx = 0.0, Dy = 0.0, Dz = 2.0

Liquid Temperature: 23.2°C

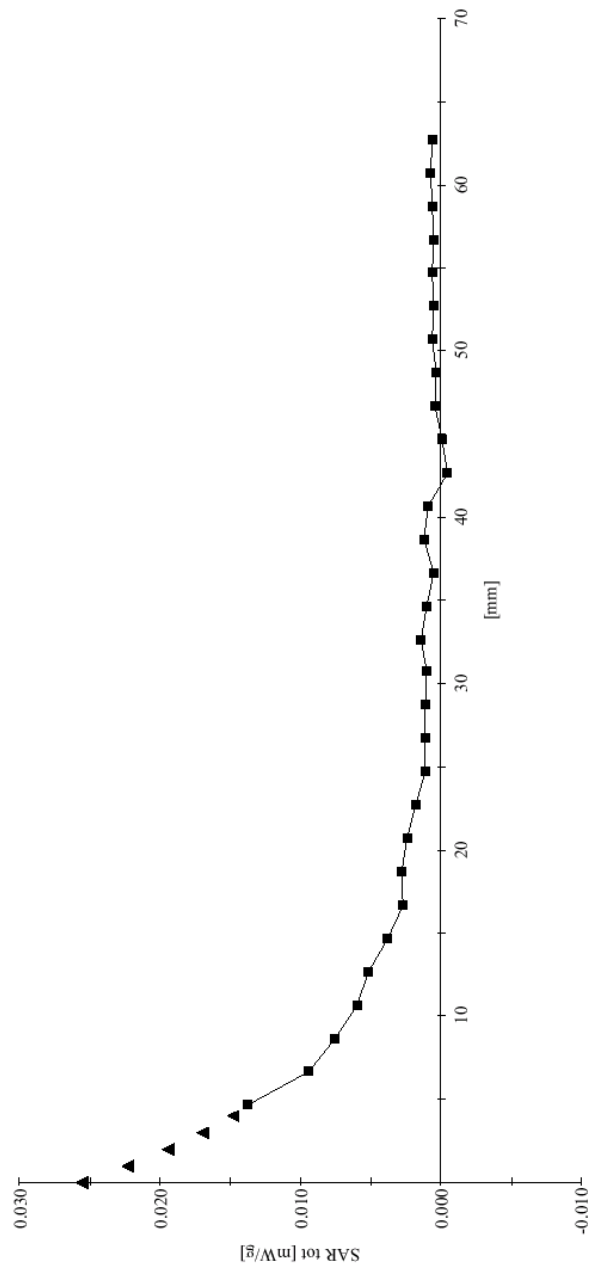

COMPLIANCE CERTIFICATION SERVICES

## 7. REFERENCES

- [1] Federal Communications Commission, \Report and order: Guidelines for evaluating the environmental effects of radiofrequency radiation", Tech. Rep. FCC 96-326, FCC, Washington, D.C. 20554, 1996.
- [2] David L. Means Kwok Chan, Robert F. Cleveland, \Evaluating compliance with FCC guidelines for human exposure to radiofrequency electromagnetic fields", Tech. Rep., Federal Communication Commission, Office of Engineering & Technology, Washington, DC, 1997.
- [3] Thomas Schmid, Oliver Egger, and Niels Kuster, \Automated E-field scanning system for dosimetric assessments", IEEE Transactions on Microwave Theory and Techniques, vol. 44, pp. 105{113, Jan. 1996.
- [4] Niels Kuster, Ralph Kastle, and Thomas Schmid, \Dosimetric evaluation of mobile communications equipment with known precision", IEICE Transactions on Communications, vol. E80-B, no. 5, pp. 645{652, May 1997.
- [5] CENELEC, \Considerations for evaluating of human exposure to electromagnetic fields (EMFs) from mobile telecommunication equipment (MTE) in the frequency range 30MHz - 6GHz", Tech. Rep., CENELEC, European Committee for Electrotechnical Standardization, Brussels, 1997.
- [6] ANSI, ANSI/IEEE C95.1-1992: IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz, The Institute of Electrical and Electronics Engineers, Inc., New York, NY 10017, 1992.
- [7] Katja Pokovic, Thomas Schmid, and Niels Kuster, \Robust setup for precise calibration of E-field probes in tissue simulating liquids at mobile communications frequencies", in ICECOM \_ 97, Dubrovnik, October 15{17, 1997, pp. 120{124.
- [8] Katja Pokovic, Thomas Schmid, and Niels Kuster, \E-field probe with improved isotropy in brain simulating liquids", in Proceedings of the ELMAR, Zadar, Croatia, 23{25 June, 1996, pp. 172{175.
- [9] Volker Hombach, Klaus Meier, Michael Burkhardt, Eberhard K. uhn, and Niels Kuster, \The dependence of EM energy absorption upon human head modeling at 900 MHz", IEEE Transactions on Microwave Theory and Techniques, vol. 44, no. 10, pp. 1865{1873, Oct. 1996.
- [10] Klaus Meier, Ralf Kastle, Volker Hombach, Roger Tay, and Niels Kuster, \The dependence of EM energy absorption upon human head modeling at 1800 MHz", IEEE Transactions on Microwave Theory and Techniques, Oct. 1997, in press.
- [11] W. Gander, Computermathematik, Birkhaeuser, Basel, 1992.
- [12] W. H. Press, S. A. Teukolsky, W. T. Vetterling, and B. P. Flannery, Numerical Recipes in C, The Art of Scientific Computing, Second Edition, Cambridge University Press, 1992..Dosimetric Evaluation of Sample device, month 1998 9
- [13] NIS81 NAMAS, \The treatment of uncertainty in EMC measurement", Tech. Rep., NAMAS Executive, National Physical Laboratory, Teddington, Middlesex, England, 1994.
- [14] Barry N. Taylor and Christ E. Kuyatt, \Guidelines for evaluating and expressing the uncertainty of NIST measurement results", Tech. Rep., National Institute of Standards and Technology, 1994..Dosimetric Evaluation of Sample device, month 1998 10


## 8. APPENDIX

### 8.1. EUT PHOTOS

#### External Photos



**Internal Photo**

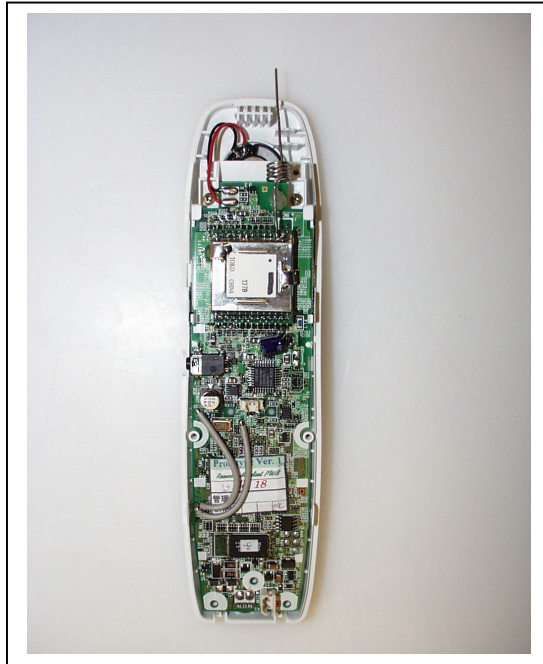

## 8.2 EQUIPMENTS LIST & CALIBRATION INFO

| Type / Model                         | Cal. Date | S/N:            |
|--------------------------------------|-----------|-----------------|
| DASY3 Professional Dosimetric System | N/A       |                 |
| Robot RX90BL                         | N/A       | F00/5H31A1/A/01 |
| Robot Controller                     | N/A       | D22134001-1     |
| Teach Pendant                        | N/A       | 321             |
| Dell Computer Optiplex GX110         | N/A       |                 |
| Pentium III, Windows NT              | N/A       |                 |
| SPEAG EDC3                           | N/A       |                 |
| SPEAG DAE3                           | 4/27/01   | 421             |
| SPEAG E-Field Probe ET3DV6           | 4/20/01   | 1577            |
| SPEAG E-Field Probe ET3DV6           | 4/20/01   | 1578            |
| SPEAG Dummy Probe                    | N/A       |                 |
| SPEAG Generic Twin Phantom           | N/A       |                 |
| SPEAG Light Alignment Sensor         | N/A       | 261             |
| SPEAG Validation Dipole D1800V2      | 4/19/01   | 294             |
| SPEAG Validation Dipole D900V2       | 4/17/01   | 108             |
| Brain Equivalent Matter (800MHz)     | Daily     |                 |
| Brain Equivalent Matter (1900MHz)    | Daily     |                 |
| Muscle Equivalent Matter (800MHz)    | Daily     |                 |
| Muscle Equivalent Matter (1900MHz)   | Daily     |                 |
| Robot Table                          | N/A       |                 |
| Phone Holder                         | N/A       |                 |
| Phantom Cover                        | N/A       |                 |
| HP Spectrum Analyzer HP8593GM        | 6/20/01   | 3009A00791      |
| Microwave Amp. Model: ZHL-42W        | N/A       | D072701-5       |
| Power Meter HP436A                   | 4/2/01    | 2709A29209      |
| Power Sensor HP8482A                 | 4/2/01    | 2349A08568      |
| Signal Generator HP-83732B           | 3/21/01   | US13449049      |
| Network Analyzer HP-8753ES           | 7/28/01   | MY40001647      |
| Dielectric Probe Kit HP85070A        | N/A       |                 |

### 8.3 IEEE SCC-34/SC-2 P1528 RECOMMENDED TISSUE DIELECTRIC PARAMETERS

The head tissue dielectric parameters recommended by the IEEE SCC-34/SC-2 in P1528 have been incorporated in the following table. These head parameters are derived from planar layer models simulating the highest expected SAR for the dielectric properties and tissue thickness variations in a human head. Other head and body tissue parameters that have not been specified in P1528 are derived from the tissue dielectric parameters computed from the 4-Cole-Cole equations and extrapolated according to the head parameters specified in P1528.

| Target Frequency | Head         |                | Body         |                |
|------------------|--------------|----------------|--------------|----------------|
| (MHz)            | $\epsilon_r$ | $\sigma$ (S/m) | $\epsilon_r$ | $\sigma$ (S/m) |
| 150              | 52.3         | 0.76           | 61.9         | 0.80           |
| 300              | 45.3         | 0.87           | 58.2         | 0.92           |
| 450              | 43.5         | 0.87           | 56.7         | 0.94           |
| 835              | 41.5         | 0.90           | 55.2         | 0.97           |
| 900              | 41.5         | 0.97           | 55.0         | 1.05           |
| 915              | 41.5         | 0.98           | 55.0         | 1.06           |
| 1450             | 40.5         | 1.20           | 54.0         | 1.30           |
| 1610             | 40.3         | 1.29           | 53.8         | 1.40           |
| 1800 – 2000      | 40.0         | 1.40           | 53.3         | 1.52           |
| 2450             | 39.2         | 1.80           | 52.7         | 1.95           |
| 3000             | 38.5         | 2.40           | 52.0         | 2.73           |
| 5800             | 35.3         | 5.27           | 48.2         | 6.00           |

( $\epsilon_r$  = relative permittivity,  $\sigma$  = conductivity and  $\rho$  = 1000 kg/m<sup>3</sup>)

## 8.4      EQUIPMENTS CALIBRATION CERTIFICATE

### **Schmid & Partner Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

### **Calibration Certificate**

#### **Dosimetric E-Field Probe**

Type:

**ET3DV6**

Serial Number:

**1577**

Place of Calibration:

**Zurich**

Date of Calibration:

**Apr. 20, 2001**

Calibration Interval:

**12 months**

Schmid & Partner Engineering AG hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of Schmid & Partner Engineering AG.

Wherever applicable, the standards used in the calibration process are traceable to international standards. In all other cases the standards of the Laboratory for EMF and Microwave Electronics at the Swiss Federal Institute of Technology (ETH) in Zurich, Switzerland have been applied.

Calibrated by:

*Michael Meriana*

Approved by:

*Robert Kofler*

**Schmid & Partner  
Engineering AG**

---

**DASY - DOSIMETRIC ASSESSMENT SYSTEM**

**CALIBRATION REPORT**

**DATA ACQUISITION ELECTRONICS**

**MODEL:** DAE3 V1

**SERIAL NUMBER:** 427

This Data Acquisition Unit was calibrated and tested using a FLUKE 702 Process Calibrator. Calibration and verification were performed at an ambient temperature of  $23 \pm 5$  °C and a relative humidity of < 70%.

Measurements were performed using the standard DASY software for converting binary values, offset compensation and noise filtering. Software settings are indicated in the reports.

Results from this calibration relate only to the unit calibrated.

**Calibrated by:** E. Meyer

**Calibration Date:** April 27, 2001

**DASY Software Version:** DASY3 V3.1c