

Appendix 1 – System Performance Check Plots

Test Laboratory: JAPAN QUALITY ASSURANCE ORGANIZATION

System Performance Check

DUT: Dipole 900 MHz; Type: D900V2; Serial: 153

Frequency: 835 MHz; Duty Cycle: 1:1

Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C

Medium parameters used: $f = 835$ MHz; $\sigma = 0.991$ S/m; $\epsilon_r = 54.717$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Probe: ET3DV6 - SN1679; ConvF(6.33, 6.33, 6.33); Calibrated: 8/12/2015;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn508; Calibrated: 11/23/2015
- Phantom: SAM v4.0 SN1194; Type: QD000P40CA; Serial: TP 1194
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Dipole/Input 250 mW/Area Scan (9x9x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (measured) = 2.64 W/kg



Dipole/Input 250 mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 53.58 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 3.45 W/kg

SAR(1 g) = 2.44 W/kg; SAR(10 g) = 1.62 W/kg

Maximum value of SAR (measured) = 2.65 W/kg

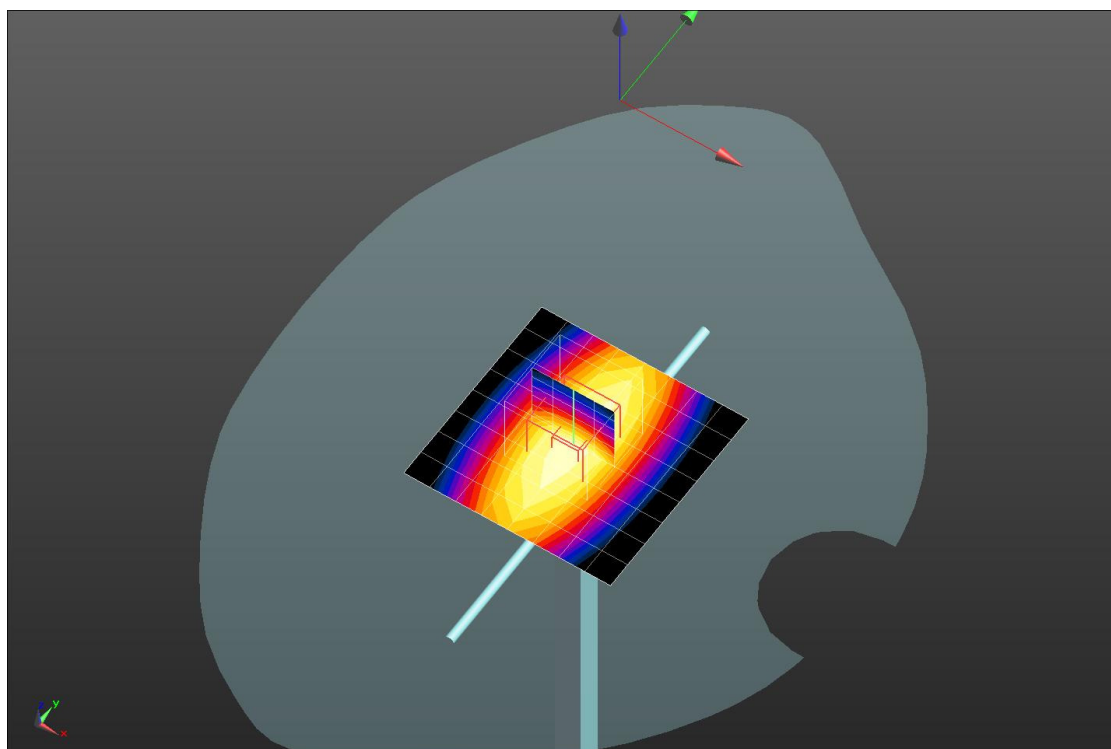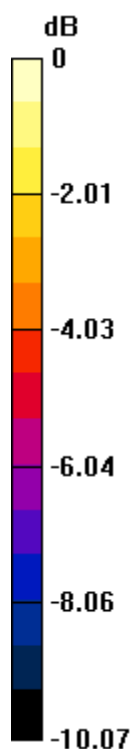

0 dB = 2.65 W/kg = 4.23 dBW/kg

Test Laboratory: JAPAN QUALITY ASSURANCE ORGANIZATION

System Performance Check

DUT: Dipole 900 MHz; Type: D900V2; Serial: 153

Frequency: 835 MHz; Duty Cycle: 1:1

Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C

Medium parameters used: $f = 835 \text{ MHz}$; $\sigma = 0.902 \text{ S/m}$; $\epsilon_r = 40.828$; $\rho = 1000 \text{ kg/m}^3$

DASY5 Configuration:

- Probe: ET3DV6 - SN1679; ConvF(6.4, 6.4, 6.4); Calibrated: 8/12/2015;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn508; Calibrated: 11/23/2015
- Phantom: SAM v4.0 SN1194; Type: QD000P40CA; Serial: TP 1194
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Dipole/Input 250 mW/Area Scan (9x9x1): Measurement grid: $dx=10\text{mm}$, $dy=10\text{mm}$

Maximum value of SAR (measured) = 2.53 W/kg



Dipole/Input 250 mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 54.48 V/m; Power Drift = 0.12 dB

Peak SAR (extrapolated) = 3.43 W/kg

SAR(1 g) = 2.38 W/kg; SAR(10 g) = 1.56 W/kg

Maximum value of SAR (measured) = 2.57 W/kg

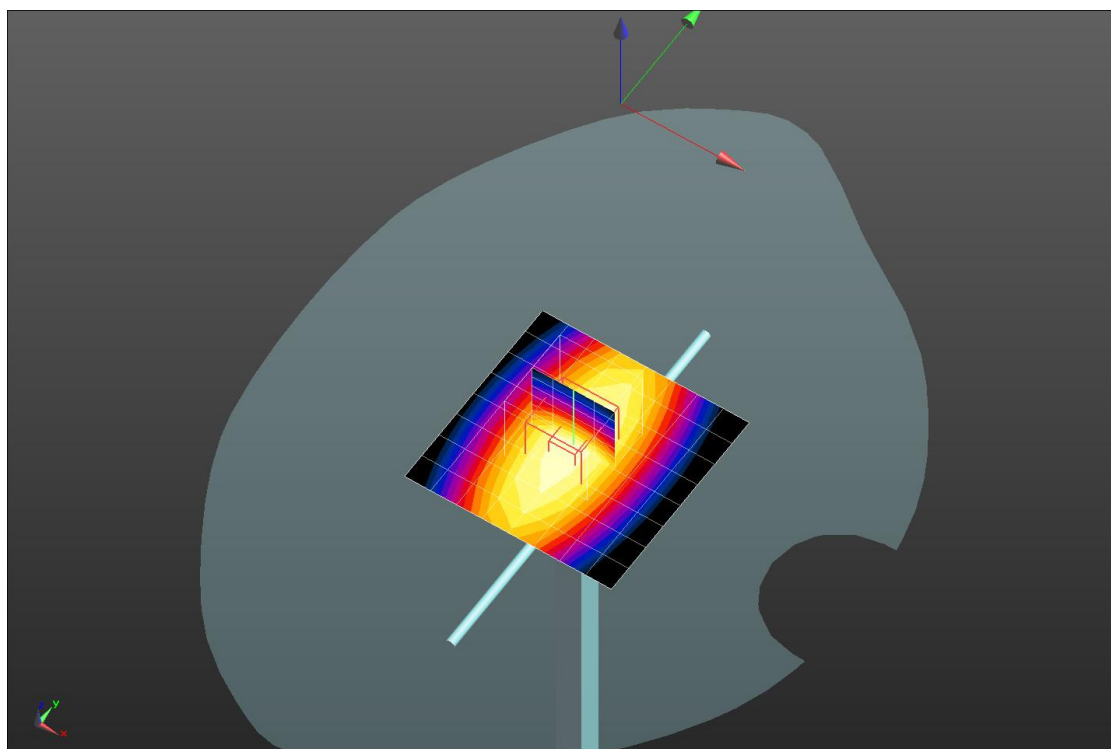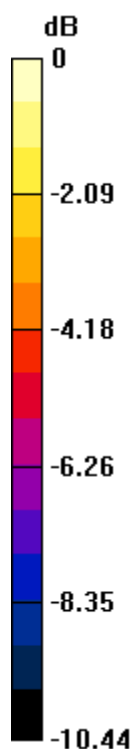

0 dB = 2.57 W/kg = 4.10 dBW/kg

Test Laboratory: JAPAN QUALITY ASSURANCE ORGANIZATION

System Performance Check

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d112

Frequency: 1900 MHz; Duty Cycle: 1:1

Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.529$ S/m; $\epsilon_r = 52.684$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Probe: ET3DV6 - SN1679; ConvF(4.6, 4.6, 4.6); Calibrated: 8/12/2015;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn508; Calibrated: 11/23/2015
- Phantom: SAM v4.0 SN1194; Type: QD000P40CA; Serial: TP 1194
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Dipole/Input 250 mW/Area Scan (9x9x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (measured) = 10.5 W/kg



Dipole/Input 250 mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 89.02 V/m; Power Drift = 0.15 dB

Peak SAR (extrapolated) = 15.3 W/kg

SAR(1 g) = 9.51 W/kg; SAR(10 g) = 5.12 W/kg

Maximum value of SAR (measured) = 10.8 W/kg

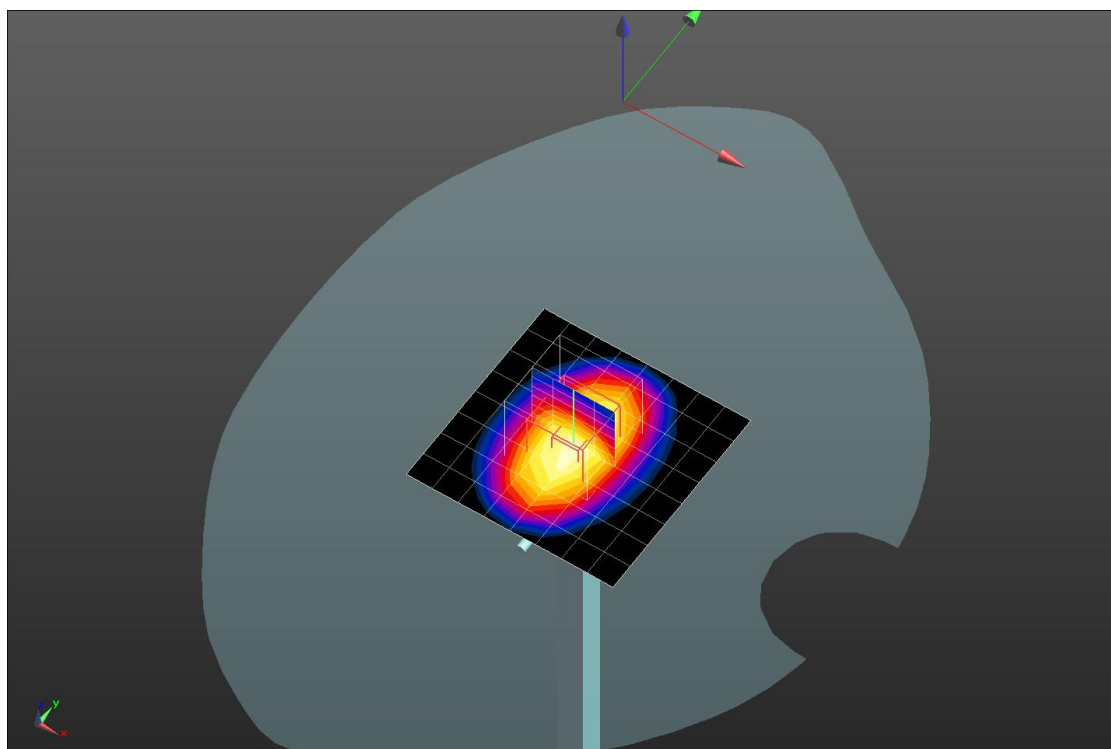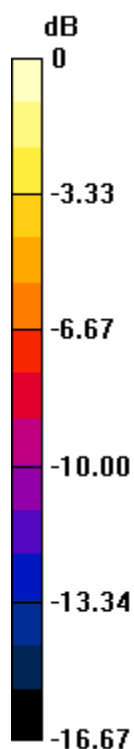

0 dB = 10.8 W/kg = 10.33 dBW/kg

Test Laboratory: JAPAN QUALITY ASSURANCE ORGANIZATION

System Performance Check

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d112

Frequency: 1900 MHz; Duty Cycle: 1:1

Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.393$ S/m; $\epsilon_r = 39.78$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Probe: ET3DV6 - SN1679; ConvF(5.08, 5.08, 5.08); Calibrated: 8/12/2015;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn508; Calibrated: 11/23/2015
- Phantom: SAM v4.0 SN1194; Type: QD000P40CA; Serial: TP 1194
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Dipole/Input 250 mW/Area Scan (9x9x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (measured) = 10.4 W/kg



Dipole/Input 250 mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 91.61 V/m; Power Drift = 0.09 dB

Peak SAR (extrapolated) = 16.0 W/kg

SAR(1 g) = 9.52 W/kg; SAR(10 g) = 5.1 W/kg

Maximum value of SAR (measured) = 10.8 W/kg

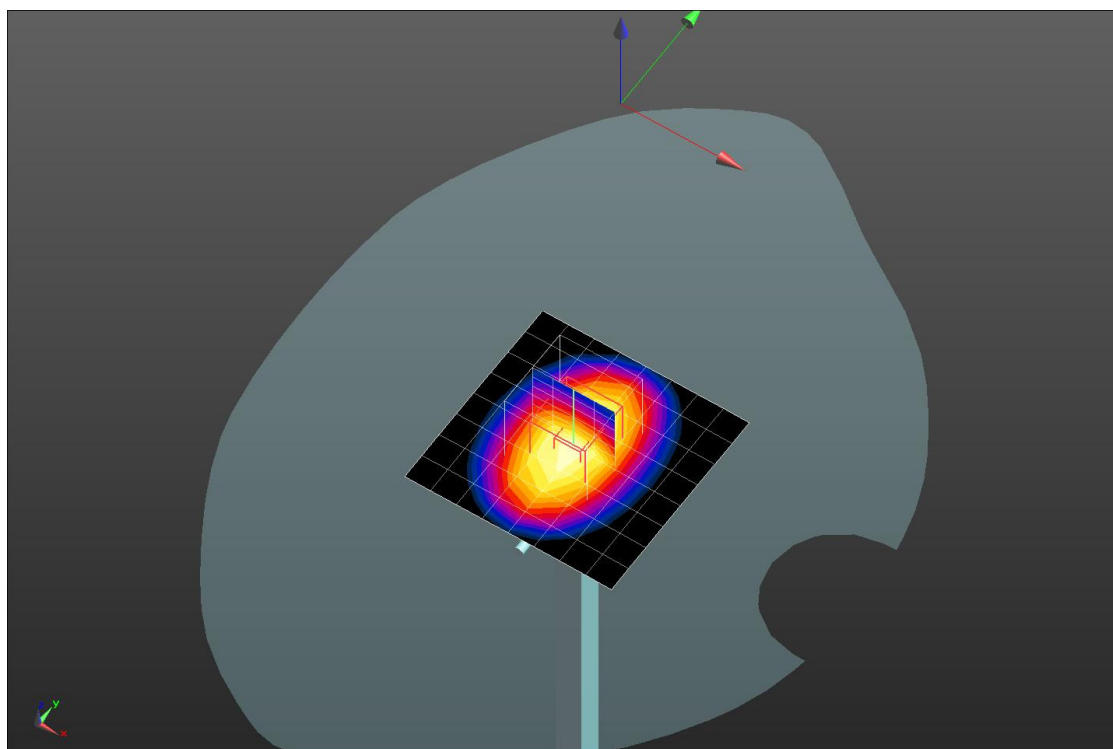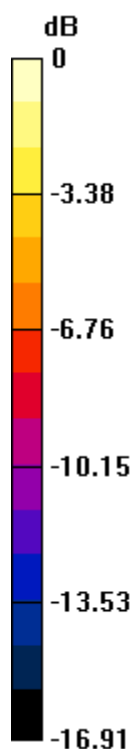

0 dB = 10.8 W/kg = 10.33 dBW/kg

Test Laboratory: JAPAN QUALITY ASSURANCE ORGANIZATION

System Performance Check

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: 714

Frequency: 2450 MHz; Duty Cycle: 1:1

Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.974$ S/m; $\epsilon_r = 51.611$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Probe: EX3DV4 - SN7321; ConvF(7.09, 7.09, 7.09); Calibrated: 8/18/2015;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn508; Calibrated: 11/23/2015
- Phantom: SAM v4.0 SN1194; Type: QD000P40CA; Serial: TP 1194
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Dipole/Input 250 mW/Area Scan (9x9x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (measured) = 19.8 W/kg



Dipole/Input 250 mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 102.3 V/m; Power Drift = 0.08 dB

Peak SAR (extrapolated) = 26.3 W/kg

SAR(1 g) = 13.3 W/kg; SAR(10 g) = 6.3 W/kg

Maximum value of SAR (measured) = 20.1 W/kg

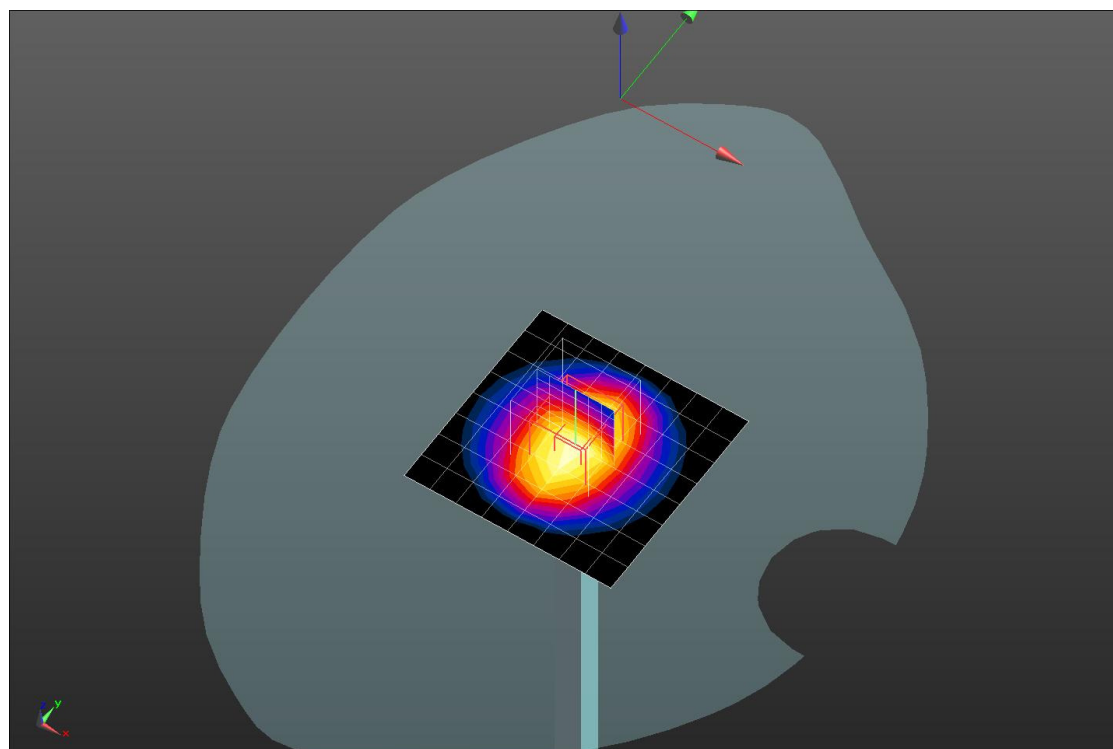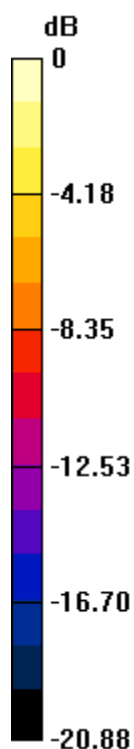

0 dB = 20.1 W/kg = 13.03 dBW/kg

Test Laboratory: JAPAN QUALITY ASSURANCE ORGANIZATION

System Performance Check

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: 714

Frequency: 2450 MHz; Duty Cycle: 1:1

Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.846$ S/m; $\epsilon_r = 37.757$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Probe: EX3DV4 - SN7321; ConvF(7, 7, 7); Calibrated: 8/18/2015;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn508; Calibrated: 11/23/2015
- Phantom: SAM v4.0 SN1194; Type: QD000P40CA; Serial: TP 1194
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Dipole/Input 250 mW/Area Scan (9x9x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (measured) = 20.0 W/kg



Dipole/Input 250 mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 106.0 V/m; Power Drift = 0.05 dB

Peak SAR (extrapolated) = 27.1 W/kg

SAR(1 g) = 13.1 W/kg; SAR(10 g) = 6.05 W/kg

Maximum value of SAR (measured) = 20.2 W/kg

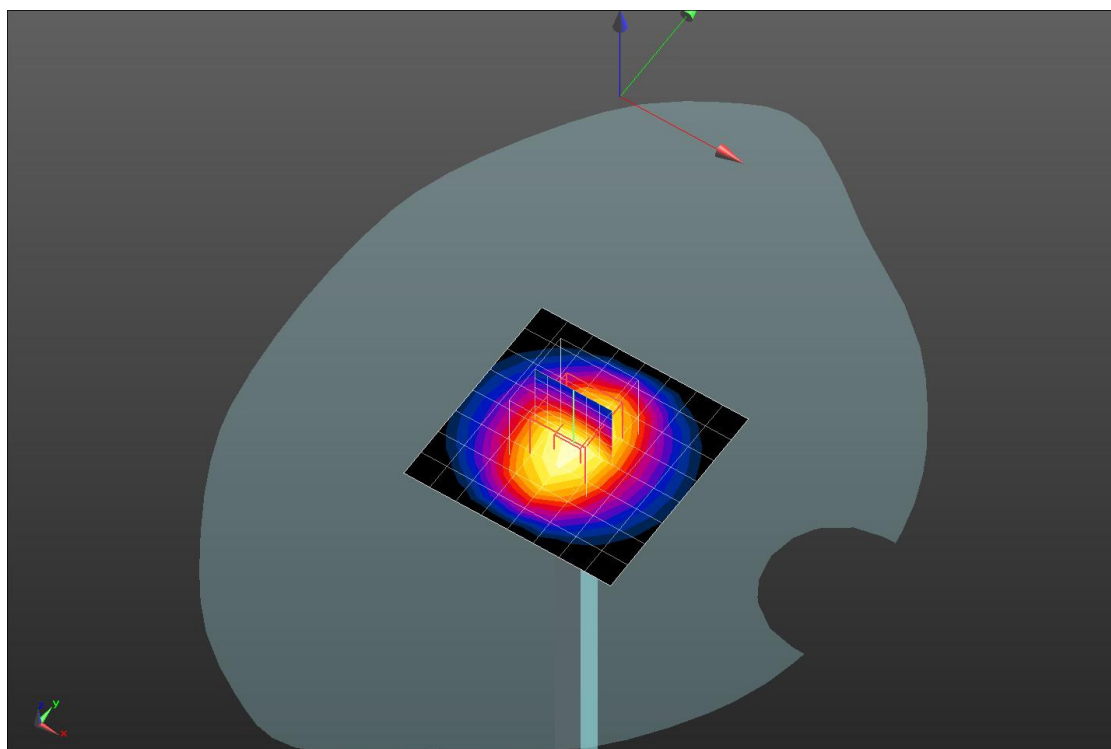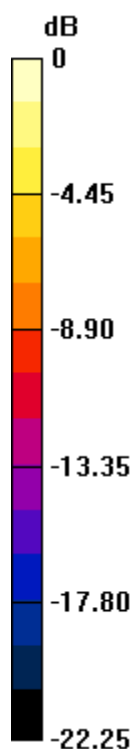

0 dB = 20.2 W/kg = 13.05 dBW/kg