

APPENDIX C - DIPOLE CALIBRATION

450MHz SYSTEM VALIDATION DIPOLE

Type:

450MHz Validation Dipole

Serial Number:

136

Place of Calibration:

Celltech Research Inc.

Date of Calibration:


October 17, 2001


Celltech Research Inc. hereby certifies that this device has been calibrated on the date indicated above.

Calibrated by:



Approved by:

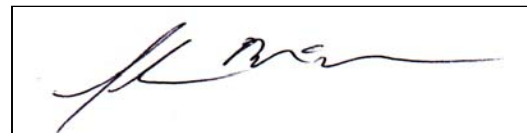

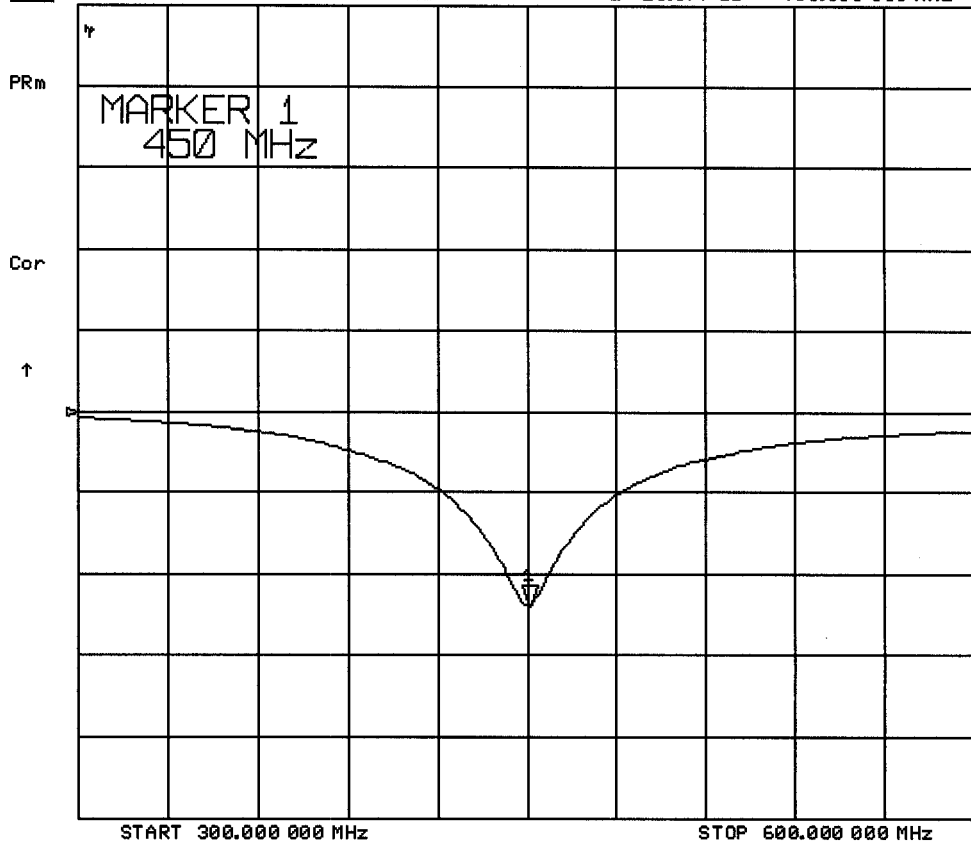

START 300.000 000 MHz

STOP 600.000 000 MHz

CH1 S11 1 U FS

1: 48.291 Ω 5.9902 Ω 2.1186 nH


11 Oct 2001 15:34:54

450.000 000 MHz

PRm

MARKER 1
450 MHz

Cor

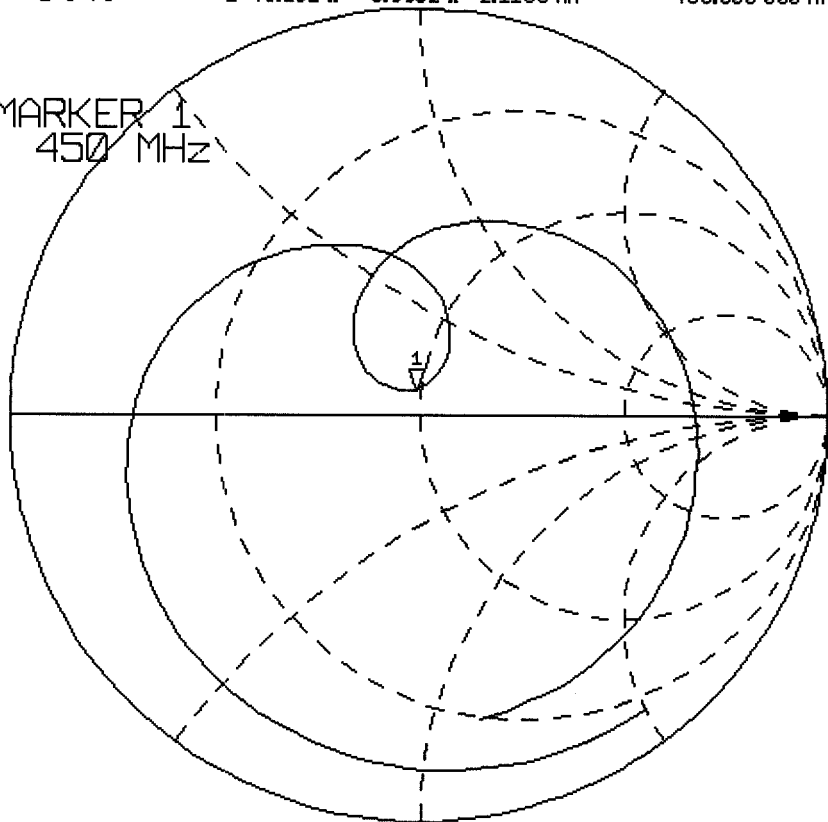

START 300.000 000 MHz

STOP 500.000 000 MHz

Validation Dipole Dimensions

Frequency (MHz)	L (mm)	h (mm)	d (mm)
300	420.0	250.0	6.2
450	288.0	167.0	6.2
835	161.0	89.8	3.6
900	149.0	83.3	3.6
1450	89.1	51.7	3.6
1800	72.0	41.7	3.6
1900	68.0	39.5	3.6
2000	64.5	37.5	3.6
2450	51.8	30.6	3.6
3000	41.5	25.0	3.6




2. Validation Phantom

The validation phantom was constructed using relatively low-loss tangent Plexiglas material. The dimensions of the phantom are as follows:

Length: 83.5 cm
Width: 36.9 cm
Height: 21.8 cm

The bottom of the phantom is constructed of 6.2 ± 0.1 mm Plexiglas.

Dimensions of Plexiglas Planar Phantom

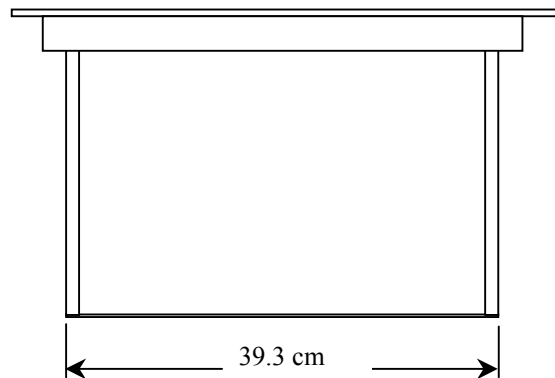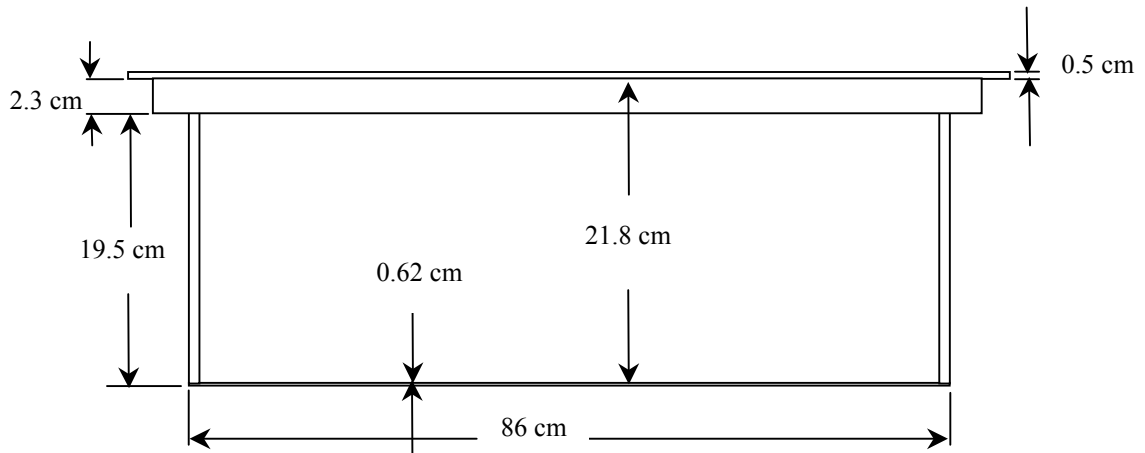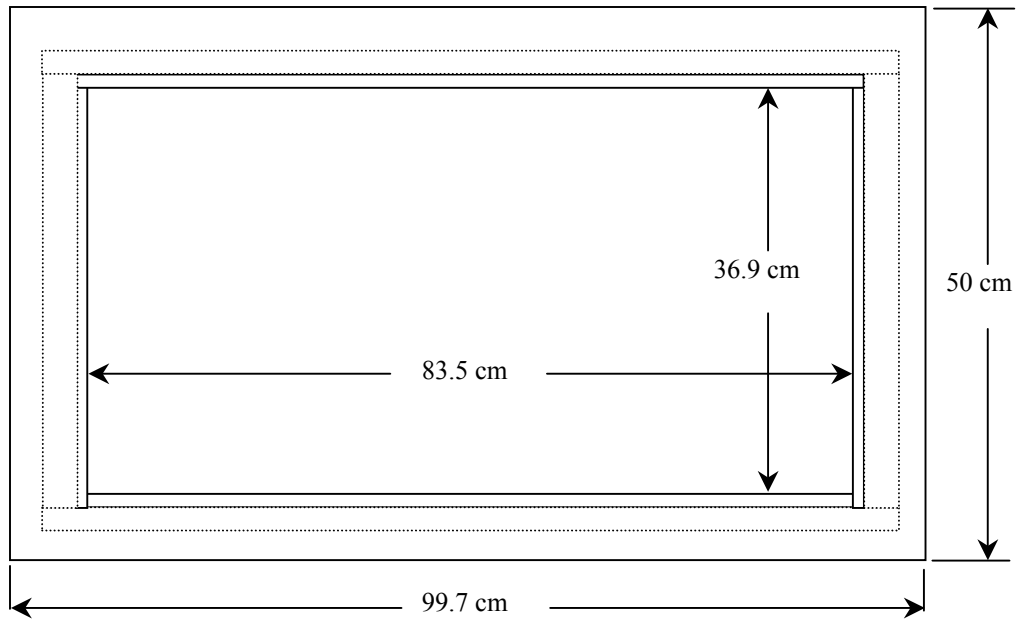

450MHz Dipole Calibration Photo



450MHz Dipole Calibration Photo



3. Measurement Conditions

The planar phantom was filled with brain simulating tissue having the following electrical parameters at 450MHz:


Relative Permittivity:	43.8	± 5%
Conductivity:	0.86 mho/m	± 5%
Temperature:	23.1°C	

The 450MHz simulating tissue consists of the following ingredients:

Ingredient	Percentage by weight
Water	38.56%
Sugar	56.32%
Salt	3.95%
HEC	0.98%
Dowicil 75	0.19%
Target Dielectric Parameters at 22°C	$\epsilon_r = 43.5$ $\sigma = 0.87 \text{ S/m}$

4. SAR Measurement

The SAR measurement was performed with the E-field probe in mechanical detection mode only. The setup and determination of the forward power into the dipole was performed using the following procedures.

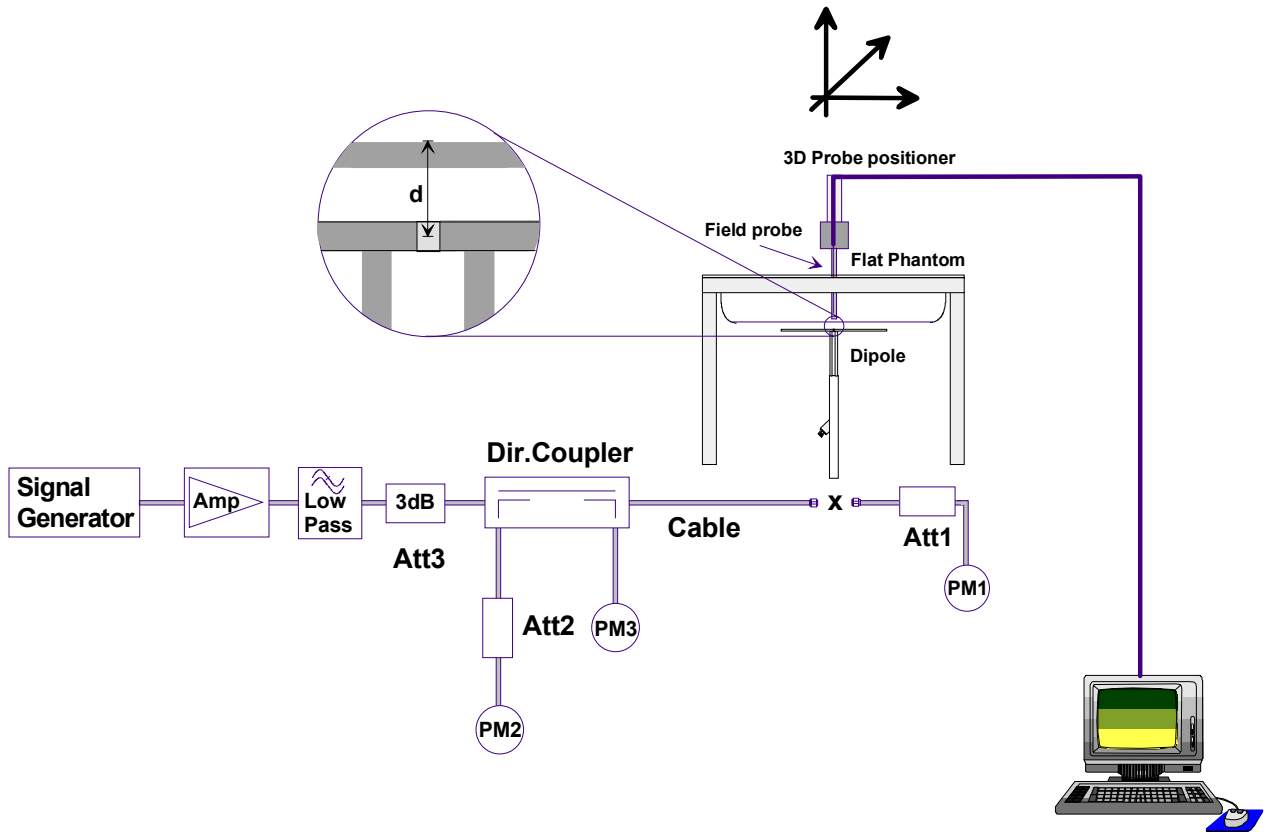

First the power meter PM1 (including attenuator Att1) is connected to the cable to measure the forward power at the location of the dipole connector (X). The signal generator is adjusted for the desired forward power at the dipole connector (taking into account the attenuation of Att1) as read by power meter PM2. After connecting the cable to the dipole, the signal generator is readjusted for the same reading at power meter PM2. If the signal generator does not allow adjustment in 0.01dB steps, the remaining difference at PM2 must be taken into consideration. PM3 records the reflected power from the dipole to ensure that the value is not changed from the previous value. The reflected power should be 20dB below the forward power.

Ten SAR measurements were performed in order to achieve repeatability and to establish an average target value.

Validation Dipole SAR Test Results

Validation Measurement	SAR @ 0.25W Input averaged over 1g	SAR @ 1W Input averaged over 1g	SAR @ 0.25W Input averaged over 10g	SAR @ 1W Input averaged over 10g	Peak SAR @ 0.25W Input
Test 1	1.47	5.88	0.971	3.88	2.31
Test 2	1.43	5.72	0.949	3.80	2.25
Test 3	1.45	5.80	0.961	3.84	2.27
Test 4	1.44	5.76	0.954	3.82	2.26
Test 5	1.46	5.84	0.969	3.88	2.29
Test 6	1.42	5.68	0.939	3.76	2.23
Test 7	1.45	5.80	0.960	3.84	2.27
Test 8	1.41	5.64	0.928	3.71	2.22
Test 9	1.43	5.72	0.950	3.80	2.25
Test10	1.46	5.84	0.971	3.88	2.29
Average Value	1.44	5.77	0.946	3.82	2.26


The results have been normalized to 1W (forward power) into the dipole.

Averaged over 1cm (1g) of tissue: 5.77 mW/g

Averaged over 10cm (10g) of tissue: 3.82 mW/g

Validation Dipole 450MHz, d = 15 mm

Frequency: 450 MHz; Antenna Input Power: 250 [mW]
Flat Phantom; Planar Section
Probe: ET3DV6 - SNI590; ConvF(7.36,7.36,7.36); Crest factor: 1.0
450 MHz Brain: $\sigma = 0.87$ mho/m $\epsilon_r = 43.5$ $\rho = 1.00$ g/cm³
Cube 5x5x7: Peak: 2.34 mW/g, SAR (1g): 1.47 mW/g, SAR (10g): 0.963 mW/g, (Worst-case extrapolation)
Penetration depth: 12.3 (10.7, 14.4) [mm]
Powerdrift: 0.02 dB
Calibration Date: Oct. 17, 2001

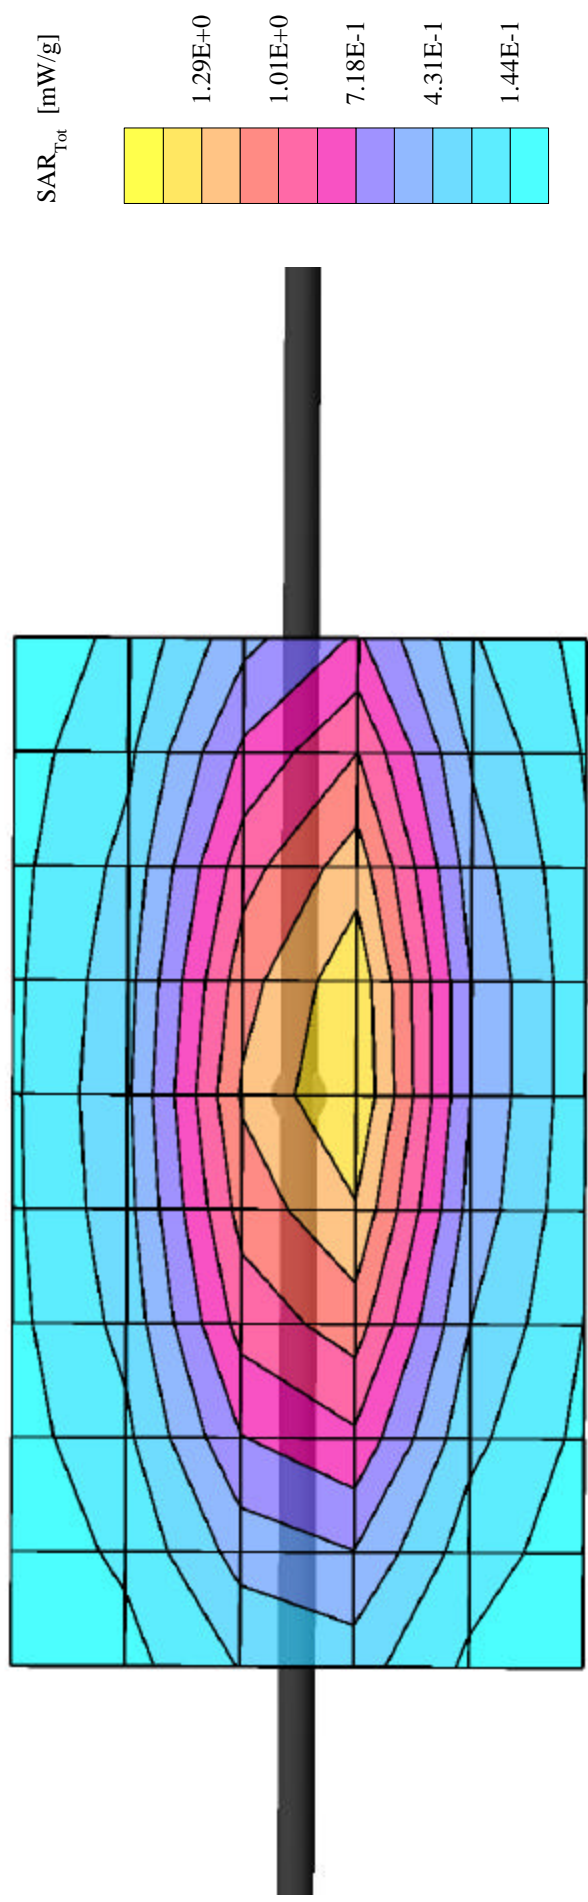


Validation Dipole 450MHz, d = 15 mm

Flat Phantom; Planar Section

Probe: ET3DV6 - SNI590; ConvF(7.36,7.36,7.36); Crest factor: 1.0
450 MHz Brain: $\sigma = 0.87$ mho/m $\epsilon_r = 43.5$ $\rho = 1.00$ g/cm³

Z-Axis: Dx = 0.0, Dy = 0.0, Dz = 5.0

Test Date: October 17, 2001
conducted power: 250 mW

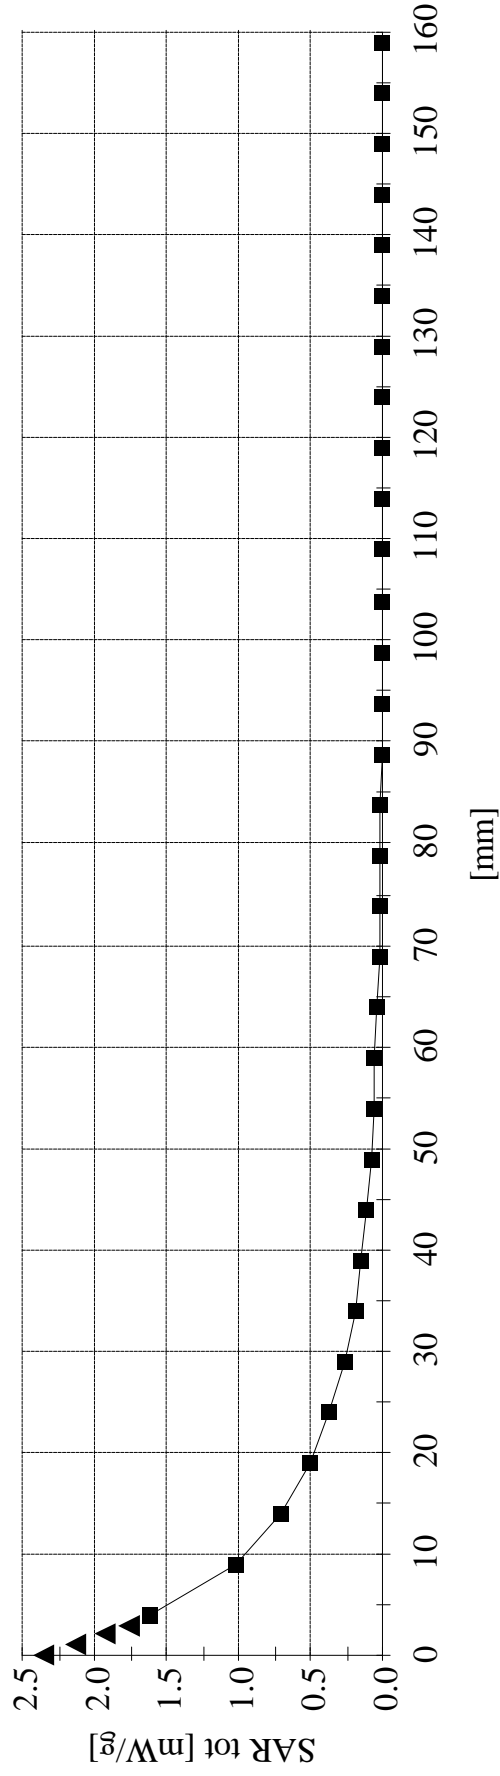

APPENDIX D - PROBE CALIBRATION

Probe ET3DV6

SN:1590

Manufactured:	March 19, 2001
Calibrated:	March 26, 2001

Calibrated for System DASY3

DASY3 - Parameters of Probe: ET3DV6 SN:1590

Sensitivity in Free Space

NormX	1.77 $\mu\text{V}/(\text{V}/\text{m})^2$
NormY	1.91 $\mu\text{V}/(\text{V}/\text{m})^2$
NormZ	1.67 $\mu\text{V}/(\text{V}/\text{m})^2$

Diode Compression

DCP X	100 mV
DCP Y	100 mV
DCP Z	100 mV

Sensitivity in Tissue Simulating Liquid

Head **450 MHz** $\epsilon_r = 43.5 \pm 5\%$ $S = 0.87 \pm 10\%$ mho/m

ConvF X	7.36 extrapolated	Boundary effect:
ConvF Y	7.36 extrapolated	Alpha 0.29
ConvF Z	7.36 extrapolated	Depth 2.72

Head **900 MHz** $\epsilon_r = 42 \pm 5\%$ $S = 0.97 \pm 10\%$ mho/m

ConvF X	6.83 $\pm 7\%$ (k=2)	Boundary effect:
ConvF Y	6.83 $\pm 7\%$ (k=2)	Alpha 0.37
ConvF Z	6.83 $\pm 7\%$ (k=2)	Depth 2.48

Head **1500 MHz** $\epsilon_r = 40.4 \pm 5\%$ $S = 1.23 \pm 10\%$ mho/m

ConvF X	6.13 interpolated	Boundary effect:
ConvF Y	6.13 interpolated	Alpha 0.47
ConvF Z	6.13 interpolated	Depth 2.17

Head **1800 MHz** $\epsilon_r = 40 \pm 5\%$ $S = 1.40 \pm 10\%$ mho/m

ConvF X	5.78 $\pm 7\%$ (k=2)	Boundary effect:
ConvF Y	5.78 $\pm 7\%$ (k=2)	Alpha 0.53
ConvF Z	5.78 $\pm 7\%$ (k=2)	Depth 2.01

Sensor Offset

Probe Tip to Sensor Center	2.7	mm
Optical Surface Detection	1.2 \pm 0.2	mm

ET3DV6 SN:1590

DASY3 - Parameters of Probe: ET3DV6 SN: 1590

Body **450 MHz** **$e_r = 56.7 \pm 5\%$** **$\sigma = 0.94 \pm 10\%$ mho/m**

ConvF X **7.23** extrapolated

ConvF Y **7.23** extrapolated

ConvF Z **7.23** extrapolated

Body **900 MHz** **$e_r = 55.0 \pm 5\%$** **$\sigma = 1.05 \pm 10\%$ mho/m**

ConvF X **6.61** $\pm 7\%$ (k=2)

ConvF Y **6.61** $\pm 7\%$ (k=2)

ConvF Z **6.61** $\pm 7\%$ (k=2)

Body **1500 MHz** **$e_r = 54.0 \pm 5\%$** **$\sigma = 1.30 \pm 10\%$ mho/m**

ConvF X **5.78** interpolated

ConvF Y **5.78** interpolated

ConvF Z **5.78** interpolated

Body **1800 MHz** **$e_r = 53.3 \pm 5\%$** **$\sigma = 1.52 \pm 10\%$ mho/m**


ConvF X **5.36** $\pm 7\%$ (k=2)

ConvF Y **5.36** $\pm 7\%$ (k=2)


ConvF Z **5.36** $\pm 7\%$ (k=2)

Receiving Pattern (f), $q = 0^\circ$


f = 30 MHz, TEM cell ifi110

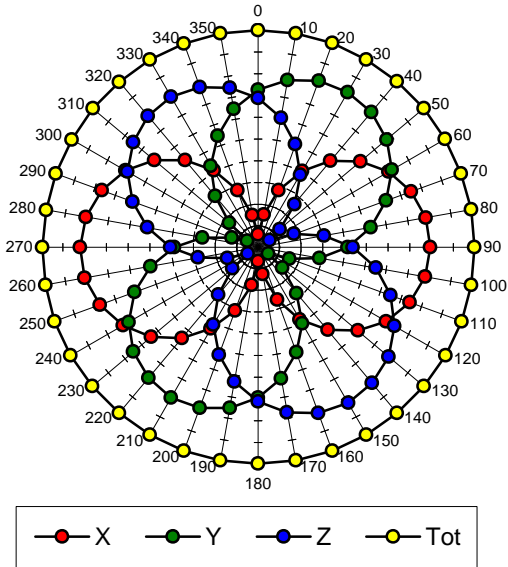


f = 100 MHz, TEM cell ifi110

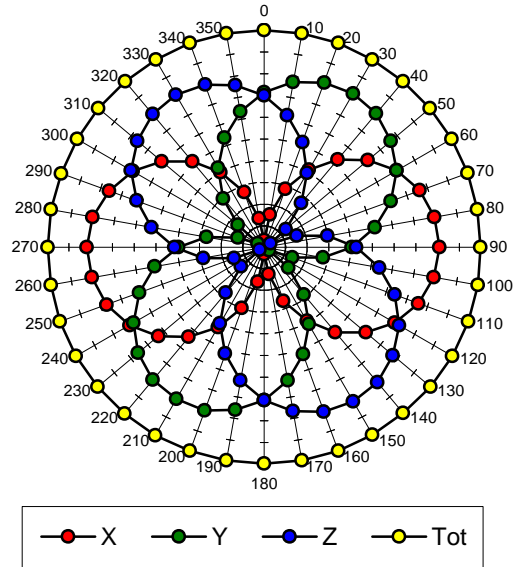


f = 300 MHz, TEM cell ifi110

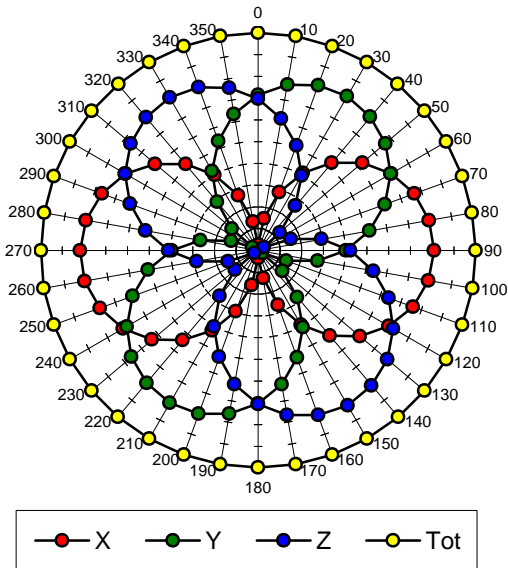


f = 900 MHz, TEM cell ifi110

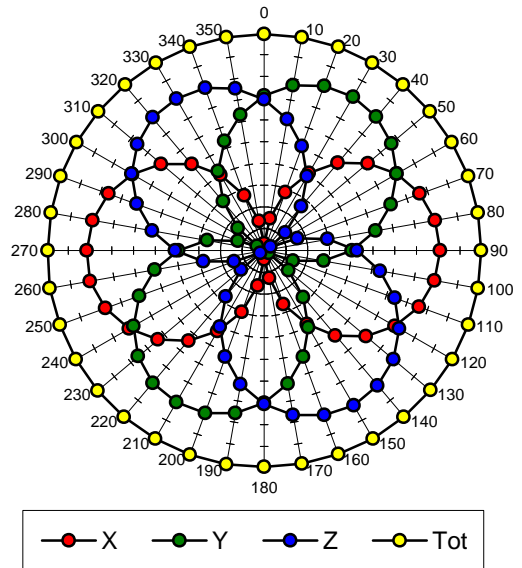

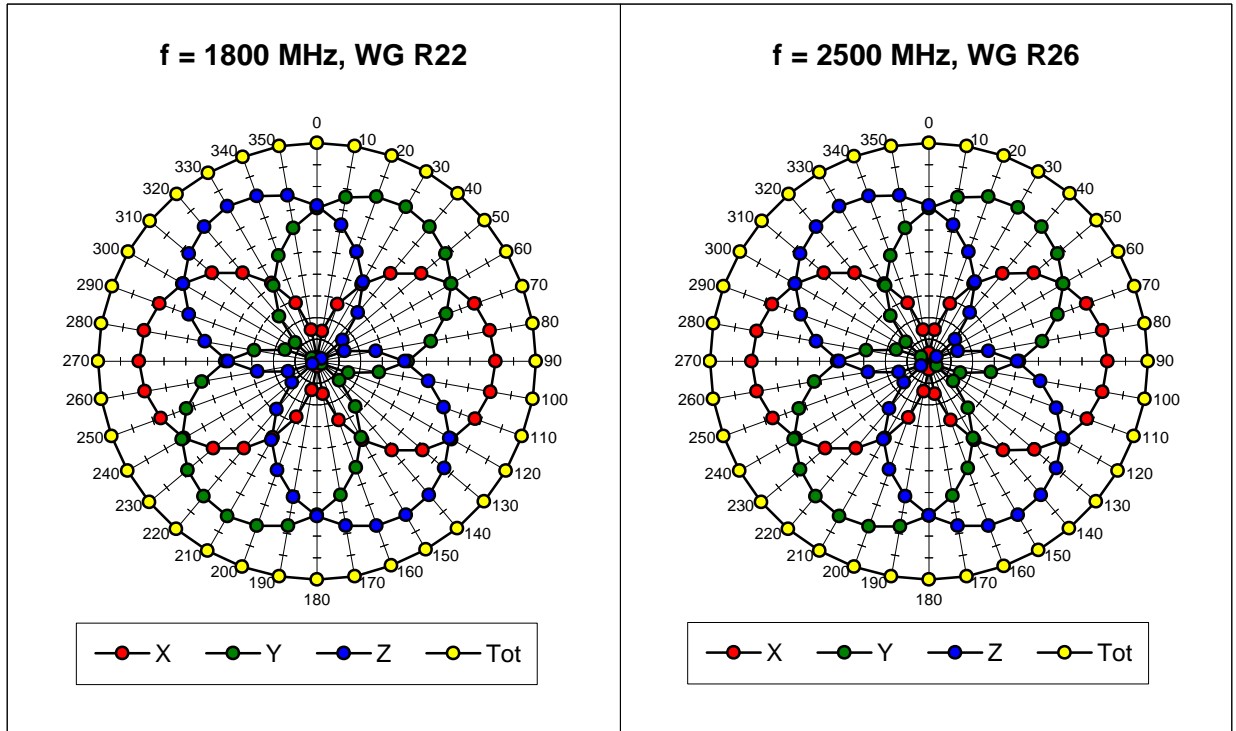


Isotropy Error (f), q = 0°


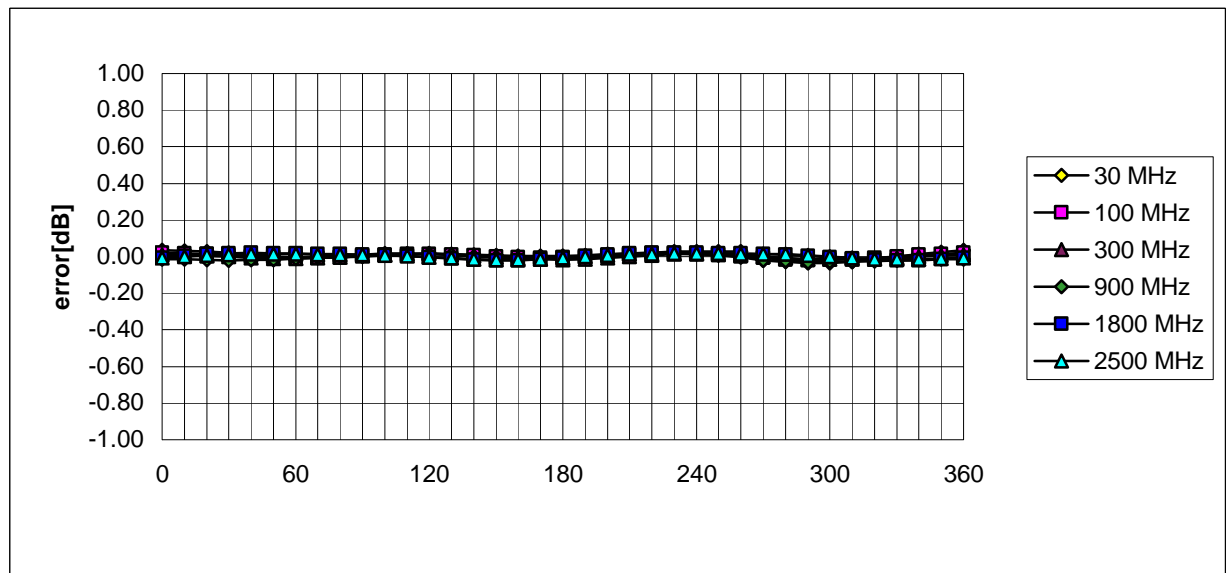


Frequency Response of E-Field


(TEM-Cell:ifi110, Waveguide R22)

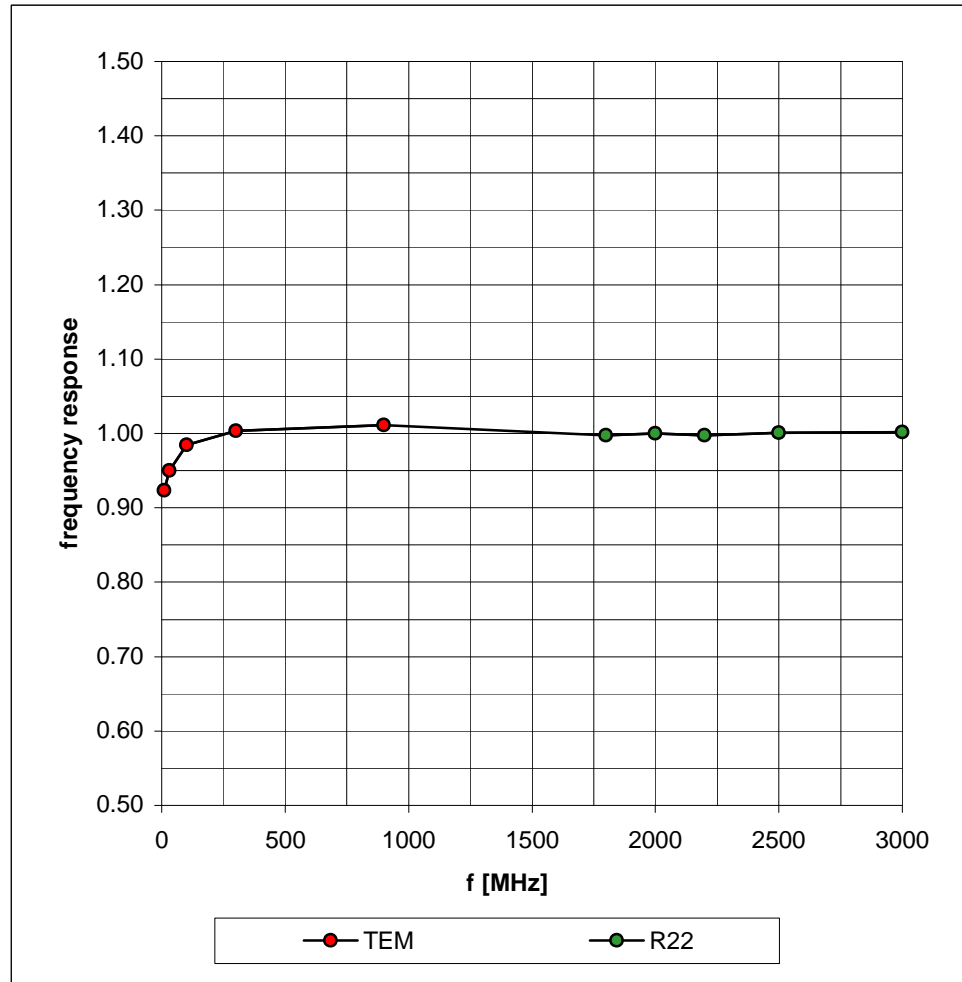

Dynamic Range f(SAR_{brain}) (TEM-Cell:ifi110)

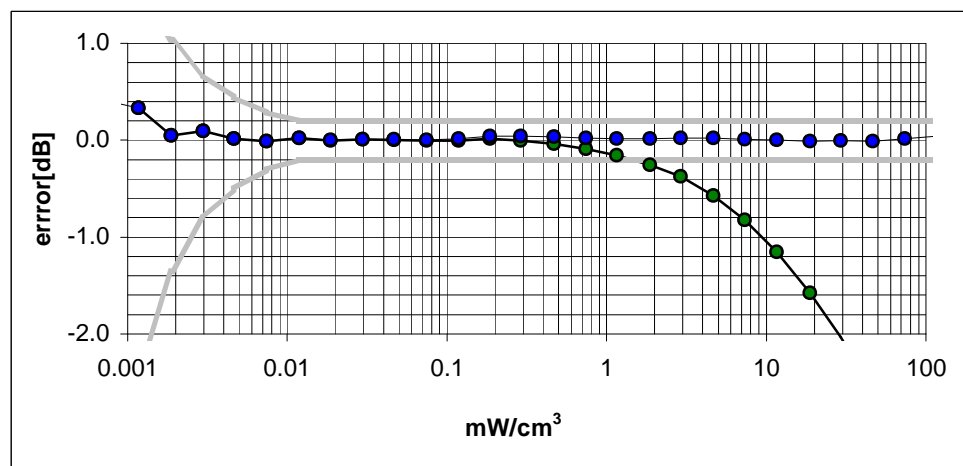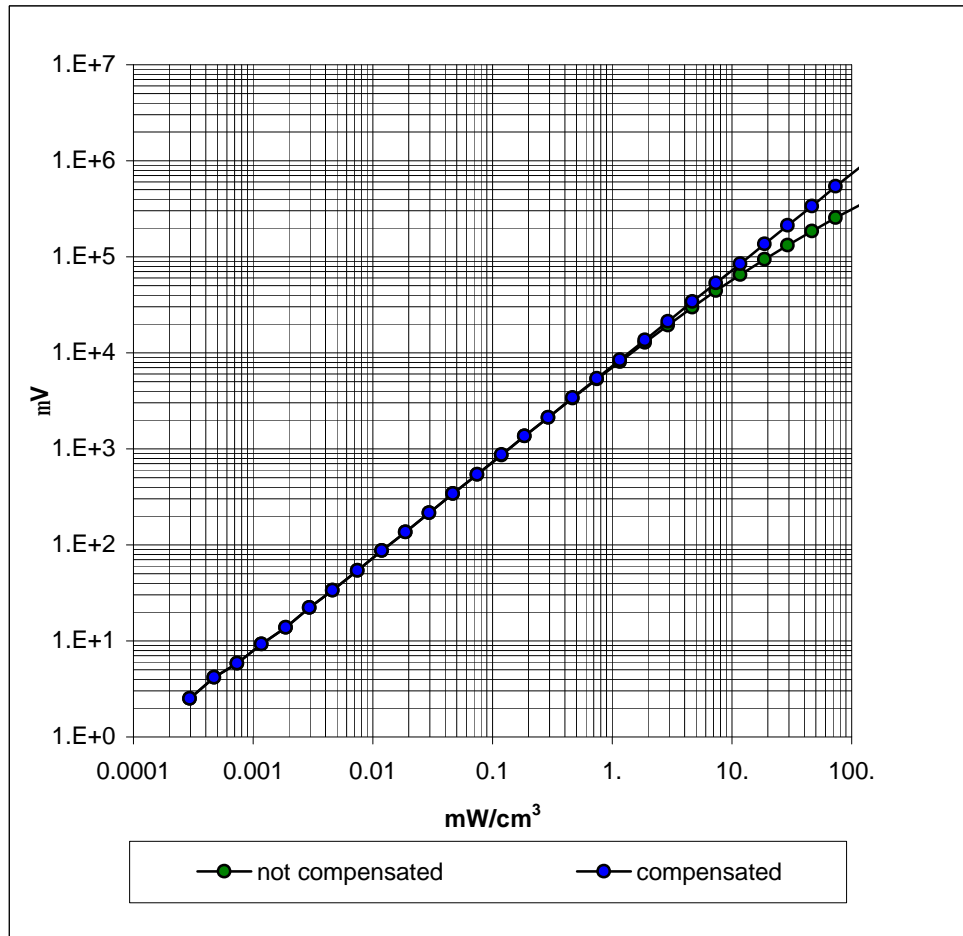


Conversion Factor Assessment

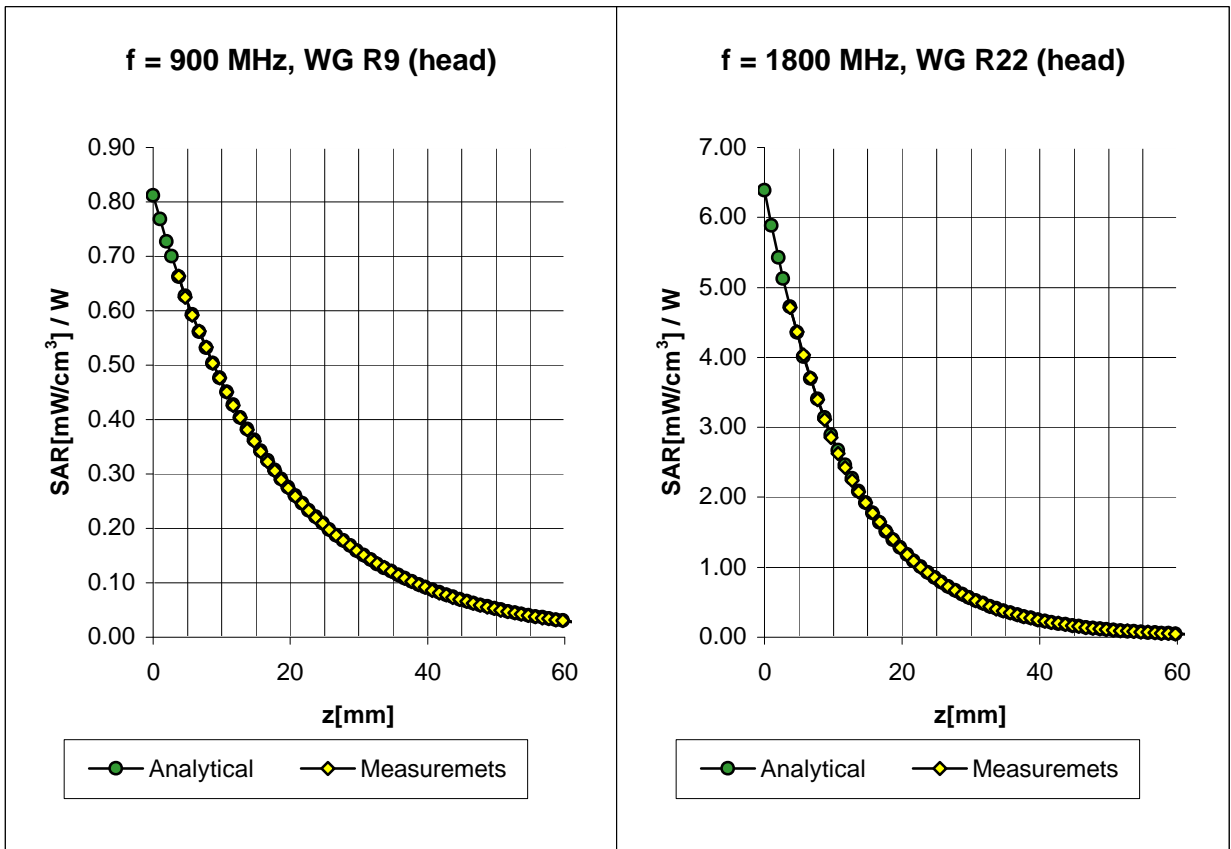

ET3DV6 SN:1590

Deviation from Isotropy in HSL

Error (qf), $f = 900$ MHz

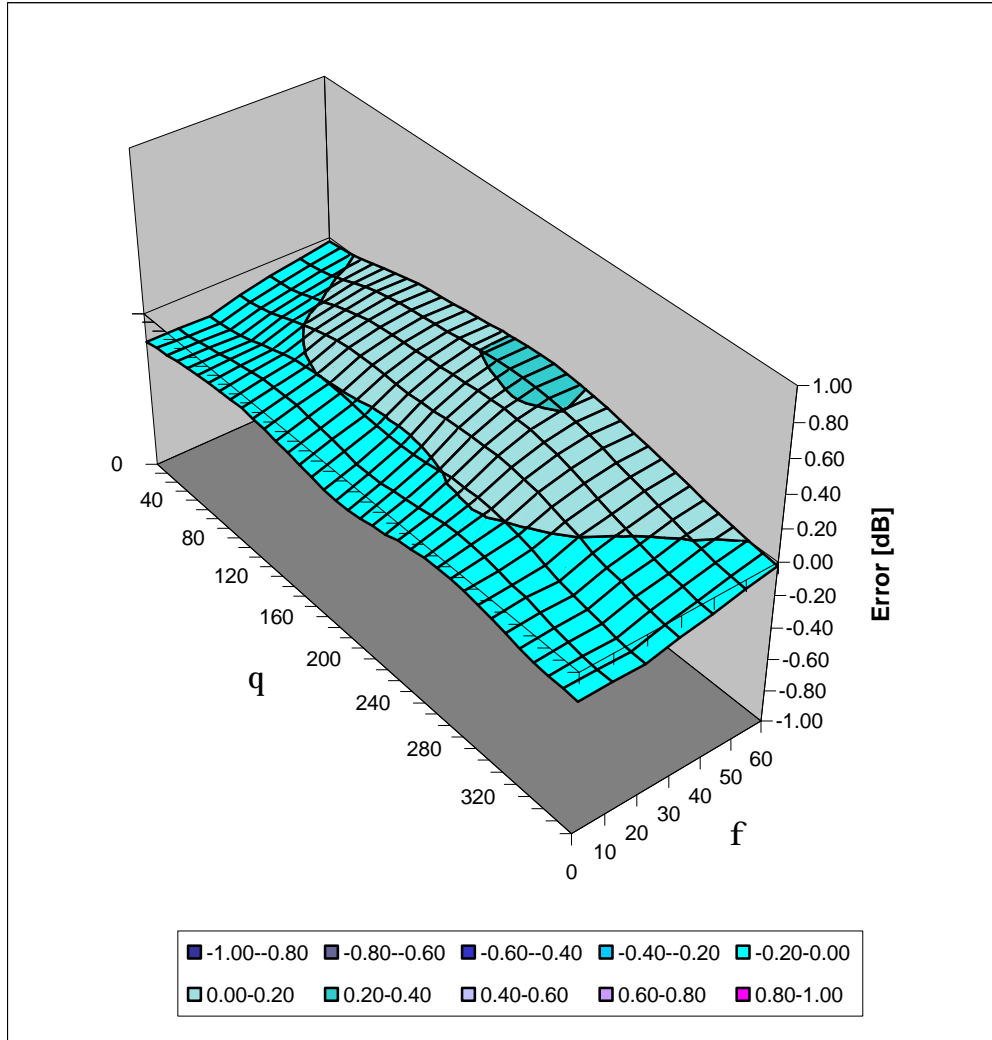

APPENDIX E - MEASURED LIQUID DIELECTRIC PARAMETERS

450MHz System Validation & EUT Evaluation

Measured Liquid Dielectric Parameters (Brain)

March 14, 2002

Frequency	ϵ'	ϵ''
400.000000 MHz	45.2787	37.4392
402.000000 MHz	45.1498	37.3431
404.000000 MHz	45.1355	37.1692
406.000000 MHz	45.0463	37.0492
408.000000 MHz	45.0185	36.9215
410.000000 MHz	45.0110	36.7919
412.000000 MHz	44.9069	36.6982
414.000000 MHz	44.8833	36.5936
416.000000 MHz	44.8205	36.4958
418.000000 MHz	44.7692	36.3369
420.000000 MHz	44.7244	36.2186
422.000000 MHz	44.6995	36.0984
424.000000 MHz	44.6390	36.0045
426.000000 MHz	44.6148	35.8863
428.000000 MHz	44.5400	35.7571
430.000000 MHz	44.5071	35.6424
432.000000 MHz	44.4247	35.5851
434.000000 MHz	44.4169	35.4392
436.000000 MHz	44.3547	35.3803
438.000000 MHz	44.2989	35.2344
440.000000 MHz	44.3035	35.1668
442.000000 MHz	44.2415	35.1004
444.000000 MHz	44.1709	35.0361
446.000000 MHz	44.1209	34.9787
448.000000 MHz	44.0798	34.8545
450.000000 MHz	44.0525	34.7573
452.000000 MHz	43.9862	34.6484
454.000000 MHz	43.9804	34.6240
456.000000 MHz	43.9390	34.5499
458.000000 MHz	43.8933	34.5048
460.000000 MHz	43.8679	34.4109
462.000000 MHz	43.7877	34.3174
464.000000 MHz	43.8148	34.2623
466.000000 MHz	43.7946	34.1970
468.000000 MHz	43.6689	34.0950

450MHz EUT Evaluation

Measured Liquid Dielectric Parameters (Body)

March 14, 2002

Frequency	e'	e''
400.000000 MHz	58.7243	40.4457
402.000000 MHz	58.7710	40.3509
404.000000 MHz	58.6960	40.1738
406.000000 MHz	58.6663	40.0109
408.000000 MHz	58.6167	39.8532
410.000000 MHz	58.6473	39.7861
412.000000 MHz	58.5985	39.6307
414.000000 MHz	58.5741	39.4928
416.000000 MHz	58.5217	39.4232
418.000000 MHz	58.5415	39.2993
420.000000 MHz	58.5142	39.1446
422.000000 MHz	58.4519	39.0184
424.000000 MHz	58.3941	38.9128
426.000000 MHz	58.3643	38.7422
428.000000 MHz	58.3520	38.6599
430.000000 MHz	58.3555	38.5051
432.000000 MHz	58.3456	38.4338
434.000000 MHz	58.2768	38.2658
436.000000 MHz	58.2373	38.1922
438.000000 MHz	58.2096	38.0775
440.000000 MHz	58.1616	38.0071
442.000000 MHz	58.1121	37.8790
444.000000 MHz	58.0971	37.8228
446.000000 MHz	58.0079	37.7338
448.000000 MHz	58.0509	37.6281
450.000000 MHz	57.9667	37.5590
452.000000 MHz	57.9893	37.4015
454.000000 MHz	57.9577	37.3516
456.000000 MHz	57.8697	37.2570
458.000000 MHz	57.8983	37.1294
460.000000 MHz	57.9036	37.0263
462.000000 MHz	57.8518	36.9642
464.000000 MHz	57.8128	36.8719
466.000000 MHz	57.7615	36.7644
468.000000 MHz	57.7538	36.6855

APPENDIX F - SAM PHANTOM CERTIFICATE OF CONFORMITY

Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

Certificate of conformity / First Article Inspection

Item	SAM Twin Phantom V4.0
Type No	QD 000 P40 BA
Series No	TP-1002 and higher
Manufacturer / Origin	Untersee Composites Hauptstr. 69 CH-8559 Fruthwilen Switzerland

Tests

The series production process used allows the limitation to test of first articles. Complete tests were made on the pre-series Type No. QD 000 P40 AA, Serial No. TP-1001 and on the series first article Type No. QD 000 P40 BA, Serial No. TP-1006. Certain parameters have been retested using further series units (called samples).

Test	Requirement	Details	Units tested
Shape	Compliance with the geometry according to the CAD model.	IT'IS CAD File (*)	First article, Samples
Material thickness	Compliant with the requirements according to the standards	2mm +/- 0.2mm in specific areas	First article, Samples
Material parameters	Dielectric parameters for required frequencies	200 MHz – 3 GHz Relative permittivity < 5 Loss tangent < 0.05.	Material sample TP 104-5
Material resistivity	The material has been tested to be compatible with the liquids defined in the standards	Liquid type HSL 1800 and others according to the standard.	Pre-series, First article

Standards

- [1] CENELEC EN 50361
 - [2] IEEE P1528-200x draft 6.5
 - [3] IEC PT 62209 draft 0.9
- (*) The IT'IS CAD file is derived from [2] and is also within the tolerance requirements of the shapes of [1] and [3].

Conformity

Based on the sample tests above, we certify that this item is in compliance with the uncertainty requirements of SAR measurements specified in standard [1] and draft standards [2] and [3].

Date 18.11.2001




Signature / Stamp

**Schmid & Partner
Engineering AG**


Zeughausstrasse 43, CH-8004 Zurich
Tel. +41 1 245 97 00, Fax +41 1 245 97 79

APPENDIX G - SAR TEST SETUP & EUT PHOTOGRAPHS


FACE-HELD SAR TEST SETUP PHOTOGRAPHS
2.5cm Separation Distance

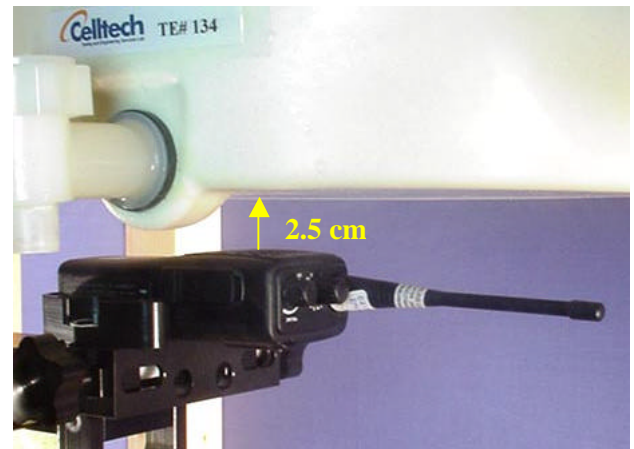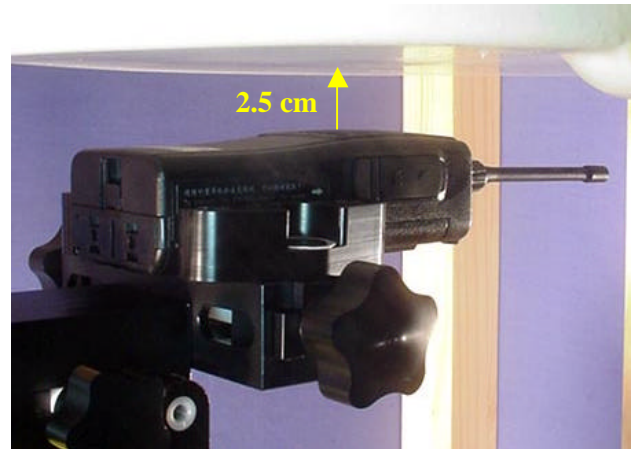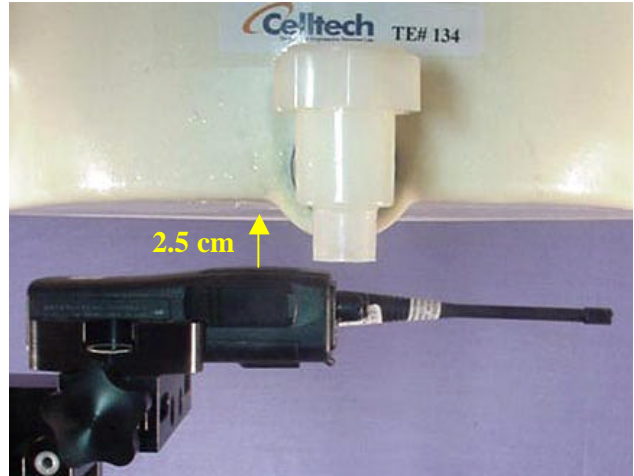

**BODY-WORN SAR TEST SETUP PHOTOGRAPHS
with 1.3cm Belt-Clip Separation Distance**

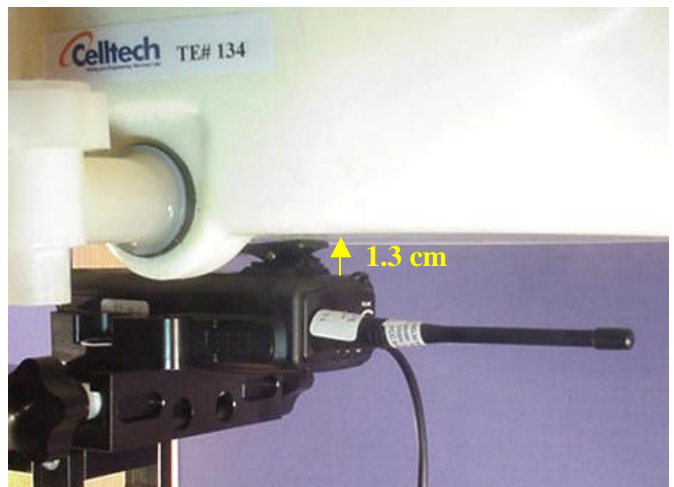


BODY-WORN SAR TEST SETUP PHOTOGRAPHS
with 1.0cm Belt-Holster Separation Distance

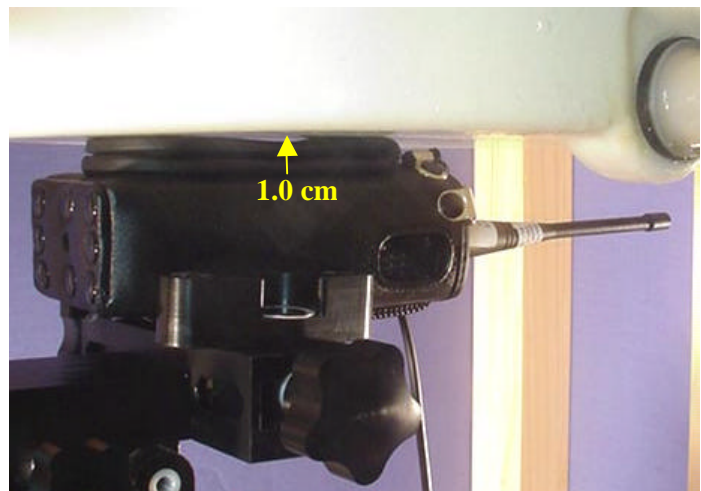

EUT PHOTOGRAPHS



EUT PHOTOGRAPHS

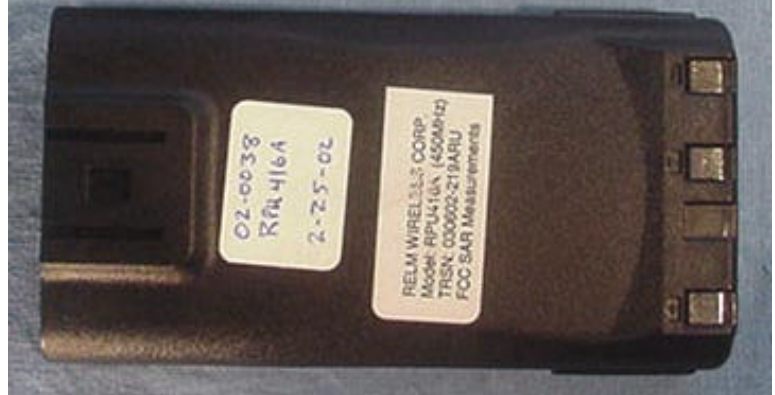

**EUT PHOTOGRAPHS
with Belt-Clip**



**EUT PHOTOGRAPHS
with Belt-Holster**

