



**DECLARATION OF COMPLIANCE SAR ASSESSMENT Part 1 of 2**

**Motorola Solutions Inc.**  
**EME Test Laboratory**  
 8000 West Sunrise Blvd  
 Fort Lauderdale, FL. 33322

**Date of Report:** 6/11/2013  
**Report Revision:** A  
**Report ID:** SR11011 RMU2080 UHF Rev A 130611

**Responsible Engineer:** Kim Uong (Principal Staff EME Engineer)  
**Report Author:** Kim Uong (Principal Staff EME Engineer)  
**Date/s Tested:** 3/6/2013  
**Manufacturer/Location:** Motorola, Penang  
**Sector/Group/Div.:** Radio Product & Accessories (RPA) - Business Light  
**Date submitted for test:** 2/13/2013  
**DUT Description:** RMU2080 UHF BRUS, 8Ch,Non-Display, Fixed Antenna, 2.0Watts, Black  
**Test TX mode(s):** CW (PTT)  
**Max. Power output:** 2.0 W  
**Nominal Power:** 1.0 - 1.9 W  
**Tx Frequency Bands:** 450-470 MHz  
**Signaling type:** FM  
**Model(s) Tested:** PMUE4178A  
**Model(s) Certified:** PMUE4178A  
**Serial Number(s):** 024TPB0158  
**Classification:** Occupational/Controlled  
**FCC ID:** AZ489FT4913; Rule Part 90 (450 – 470 MHz)

\* Refer to section 15 of part 1 for highest SAR summary results.

The test results clearly demonstrate compliance with FCC Occupational/Controlled RF Exposure limits of 8 W/kg averaged over 1 gram per the requirements of 47 CFR 2.1093(d). The 10 grams result is not applicable to FCC filing. The test results clearly demonstrate compliance with ICNIRP (1998) Guidelines for limiting exposure in time-varying electric, magnetic, and electromagnetic fields (up to 300 GHz), Health Physics 74, 494-522 RF Exposure limits of 10 W/kg averaged over 10grams of contiguous tissue.

Based on the information and the testing results provided herein, the undersigned certifies that when used as stated in the operating instructions supplied, said product complies with the national and international reference standards and guidelines listed in section 3.0 of this report. This report shall not be reproduced without written approval from an officially designated representative of the Motorola Solutions Inc EME Laboratory.  
 I attest to the accuracy of the data and assume full responsibility for the completeness of these measurements. This reporting format is consistent with the suggested guidelines of the TIA TSB-150 December 2004. The results and statements contained in this report pertain only to the device(s) evaluated.

**Deanna Zakharia**  
**EMS EME Lab Senior Resource Manager,**  
**Laboratory Director**

**Approval Date:** 6/11/2013

**Certification Date:** 3/21/2013

**Certification No.:** L1130324

**Part 1 of 2**

1.0 Introduction..... 4

2.0 Abbreviations / Definitions..... 4

3.0 Referenced Standards and Guidelines ..... 4

4.0 SAR Limits ..... 5

5.0 SAR Result Scaling Methodology ..... 6

6.0 Description of Device Under Test (DUT) ..... 6

7.0 Optional Accessories and Test Criteria..... 6

    7.1 Antennas ..... 7

    7.2 Batteries ..... 7

    7.3 Body worn Accessories..... 7

    7.4 Audio Accessories ..... 7

8.0 Description of Test System..... 8

    8.1 Descriptions of Robotics/Probes/Readout Electronics ..... 8

    8.2 Description of Phantom(s) ..... 9

    8.3 Description of Simulated Tissue..... 9

9.0 Additional Test Equipment..... 10

10.0 SAR Measurement System Verification..... 10

    10.1 Equivalent Tissue Test Results ..... 11

    10.2 System Check Test Results..... 11

11.0 Environmental Test Conditions ..... 12

12.0 DUT Test Methodology ..... 12

    12.1 Measurements ..... 12

    12.2 DUT Configuration(s)..... 12

    12.3 DUT Positioning Procedures ..... 12

        12.3.1 Body..... 12

        12.3.2 Head..... 13

        12.3.3 Face..... 13

    12.4 DUT Test Channels ..... 13

    12.5 DUT Test Plan ..... 13

13.0 DUT Test Data..... 13

    13.1 Assessments at the Body for 450-470 MHz band..... 13

        13.1.1 Assessments at the Body with Body worn PMLN6455A..... 14

        13.1.2 Assessment of other audio accessories at the body..... 14

    13.2 Assessments at the Face for 450-470 MHz band..... 14

    13.3 Shortened Scan Assessment..... 15

14.0 Simultaneous Transmission Exclusion ..... 15

15.0 Conclusion ..... 16

    APPENDIX A - Measurement Uncertainty ..... 17

    APPENDIX B - Probe Calibration Certificates ..... 20

    APPENDIX C - Dipole Calibration Certificates and Validation..... 34

**Part 2 of 2**

**APPENDICES**

APPENDIX D - Test System Check Scans ..... 2  
 APPENDIX E - DUT Scans (Shortened Scan and Highest SAR configurations)..... 5  
 APPENDIX F - DUT scans - FCC Part 90 ..... 9  
 APPENDIX G - DUT Test Position Photos ..... 11  
 APPENDIX H - DUT, Body worn and audio accessories Photos ..... 12

**Report Revision History**

Date	Revision	Comments
3/20/2013	O	Initial release
6/11/2013	A	Validation data added to Appendix C and updated table of contents

## 1.0 Introduction

This report details the utilization, test setup, test equipment, and test results of the Specific Absorption Rate (SAR) measurements performed at the Motorola Solutions Inc. EME Test Laboratory for model number PMUE4178A.

## 2.0 Abbreviations / Definitions

CNR: Calibration Not Required  
EME: Electromagnetic Energy  
CW: Continuous Wave  
DUT: Device Under Test  
DC: Duty Cycle  
FM: Frequency Modulation/Factorial Mutual  
NA: Not Applicable  
PTT: Push to Talk  
RSM: Remote Speaker Microphone  
SAR: Specific Absorption Rate  
RF: Radio Frequency

Audio accessories: These accessories allow communication while the DUT is worn on the body.

Body worn accessories: These accessories allow the DUT to be worn on the body of the user.

Maximum Power: Defined as the upper limit of the production line final test station.

## 3.0 Referenced Standards and Guidelines

This product is designed to comply with the following applicable national and international standards and guidelines.

- IEC62209-1\*(2005) Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)
- United States Federal Communications Commission, Code of Federal Regulations; Rule Part 47CFR § 2.1093 sub-part J:1999
- Federal Communications Commission, “Evaluating Compliance with FCC Guidelines for Human Exposure to Radio frequency Electromagnetic Fields”, OET Bulletin 65, Supplement C (Edition 01-01), FCC, Washington, D.C.: June 2001.
- IEEE 1528\*(2003), Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques
- American National Standards Institute (ANSI) / Institute of Electrical and Electronics Engineers (IEEE) C95. 1-1992
- Institute of Electrical and Electronics Engineers (IEEE) C95.1-2005

- International Commission on Non-Ionizing Radiation Protection (ICNIRP) 1998
- Ministry of Health (Canada) Safety Code 6 (2009), Limits of Human Exposure to Radio frequency Electromagnetic Fields in the Frequency Range from 3 kHz to 300 GHz
- Australian Communications Authority Radio communications (Electromagnetic Radiation - Human Exposure) Standard (2003)
- ANATEL, Brazil Regulatory Authority, Resolution No. 303 of July 2, 2002 "Regulation of the limitation of exposure to electrical, magnetic, and electromagnetic fields in the radio frequency range between 9 kHz and 300 GHz." and "Attachment to resolution # 303 from July 2, 2002"
- IEC62209-2 Edition 1.0 2010-03, Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices – Human models, instrumentation, and procedures – Part 2: Procedure to determine the specific absorption rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz).  
(\* )The IEC62209-1 and IEEE 1528 are applicable for hand-held devices used in close proximity to the ear only.

#### 4.0 SAR Limits

**TABLE 1**

EXPOSURE LIMITS	SAR (W/kg)	
	(General Population / Uncontrolled Exposure Environment)	(Occupational / Controlled Exposure Environment)
Spatial Average - ANSI - (averaged over the whole body)	0.08	0.4
Spatial Peak - ANSI - (averaged over any 1-g of tissue)	1.6	8.0
Spatial Peak – ICNIRP/ANSI - (hands/wrists/feet/ankles averaged over 10-g)	4.0	20.0
Spatial Peak - ICNIRP - (Head and Trunk 10-g)	2.0	10.0

## 5.0 SAR Result Scaling Methodology

The calculated 1-gram and 10-gram averaged SAR results indicated as “Max Calc. 1g-SAR” and “Max Calc.10g-SAR” in the data tables is determined by scaling the measured SAR to account for power leveling variations and power slump. For this device the “Max Calc. 1g-SAR” and “Max Calc.10g-SAR” are scaled using the following formula:

$$Max\_Calc = SAR\_meas \cdot 10^{\frac{-Drift}{10}} \cdot \frac{P\_max}{P\_int} \cdot DC$$

P\_max = Maximum Power (W)

P\_int = Initial Power (W)

Drift = DASY drift results (dB)

SAR\_meas = Measured 1-g or 10-g Avg. SAR (W/kg)

DC = Transmission mode duty cycle in % where applicable

50% duty cycle is applied for PTT operation

Note: for conservative results, the following are applied:

If P\_int > P\_max, then P\_max/P\_int = 1.

Drift = 1 for positive drift

Additional SAR scaling was applied using the methodologies outlined in FCC KDB450824 using tissue sensitivity values. SAR was scaled for conditions where the tissue permittivity was measured above the nominal target and for tissue conductivity that was measured below the nominal target. Negative or reduced SAR scaling is not permitted.

## 6.0 Description of Device Under Test (DUT)

This device operates using frequency modulation (FM) signaling incorporating traditional simplex two-way radio transmission protocol.

The model represented under this filing utilizes a fixed antenna and is capable of transmitting in the 450- 470MHz band. The nominal output powers are 1.0-1.9W with maximum output powers of 2.0W as defined by upper limit of the production line final test station. The intended operating positions are “at the face” with the DUT at least 1 inch from the mouth, and “at the body” by means of the offered body worn accessories. Body worn audio and PTT operation is accomplished by means of optional remote accessories that are connected to the radio.

## 7.0 Optional Accessories and Test Criteria

This device is offered with optional accessories. All accessories were individually evaluated during the test plan creation to determine if testing was required per the guidelines outlined in “SAR Test Reduction Considerations for Occupational PTT Radios” FCC KDB 643646 D01 dated 4/4/11 to assess compliance of this device. The following sections identify the test criteria and details for each accessory category. Refer to Exhibit 7B for antenna separation distances.

### 7.1 Antennas

This product has a fixed, non-removable, antenna. The table below lists its descriptions.

**TABLE 2**

Antenna Model	Description	Selected for test	Tested
Fixed	¼ wave Helical 450-470MHz	Yes	Yes

### 7.2 Batteries

There is only one battery offered for this product. The table below lists the battery, and battery description.

**TABLE 3**

Battery Model	Description	Selected for test	Tested	Comments
PMNN4434AR	RM /XT/RVA Standard Battery	Yes	Yes	

### 7.3 Body worn Accessories

There is only one body worn accessory offered for this product. The table below lists the body worn accessory, and body worn accessory description.

**TABLE 4**

Body worn Model	Description	Selected for test	Tested	Comments
PMLN6455A	RMX Series Holster	Yes	Yes	

### 7.4 Audio Accessories

All audio accessories were considered. The table below lists the offered audio accessories and their descriptions. Exhibit 7B illustrates photos of the tested audio accessories.

**TABLE 5**

Audio Acc. Models	Description	Selected for test	Tested	Comments
HCSN4000D	(56517) Earpiece w/ PTT Mic	Yes	No	
HCSN4001C	(56518) Earpiece w/Boom Mic	Yes	No	
HKLN4477B	Earpiece Surveillance Mic	Yes	No	
HMN9025D	(53866) Earbud w/PTT Mic	Yes	No	
HMN9026D	(53862) Remote Spk Mic	Yes	Yes	
HMN9030A	Remote Speaker Mic	Yes	No	
HMN9038A	(53865) Headset W/swivel Boom Mic	Yes	No	
HMN9039E	(53863) Earpiece w/Boom Mic	Yes	No	
NTN9159F	(53815) Lightweight Headset	Yes	No	
RLN5714B	Earpiece w/Inline Mic	Yes	No	
RLN6423A	(52730) Swivel Earpiece	Yes	No	
RMN5114A	Light Weight Temple Transducer Headset	Yes	No	

## 8.0 Description of Test System



### 8.1 Descriptions of Robotics/Probes/Readout Electronics

**TABLE 6**

Dosimetric System type	System version	DAE type	Probe Type
Schmid & Partner Engineering AG SPEAG DASY 5	52.8.2.969	DAE4	ES3DV3 (E-Field)

The DASY5™ system is operated per the instructions in the DASY5™ Users Manual. The complete manual is available directly from SPEAG™. All measurement equipment used to assess EME SAR compliance was calibrated according to ISO/IEC 17025 A2LA guidelines. Section 9.0 presents additional test equipment information. Appendices B and C present the applicable calibration certificates. The E-field probe first scans a coarse grid over a large area inside the phantom in order to locate the interpolated maximum SAR distribution. After the coarse scan measurement, the probe is automatically moved to a position at the interpolated maximum. The subsequent scan can directly use this position as reference for the cube evaluations.

8.2 Description of Phantom(s)

TABLE 7

Phantom type	Phantom ID (s)	Material Parameters	Phantom Dimensions LxWxD (mm)	Material Thickness (mm)	Support Structure Material	Loss Tangent (wood)
Dual Flat	NA	300MHz -6GHz; Er = 4+/- 1, Loss Tangent = ≤0.05	600x400x190	2mm +/- 0.2mm	Wood	< 0.05
SAM	NA					
Elliptical	OVAL1011 OVAL1020					

8.3 Description of Simulated Tissue

The sugar based simulate tissue is produced by placing the correct measured amount of De-ionized water into a large container. Each of the dried ingredients are weighed and added to the water carefully to avoid clumping. If the solution has a high sugar concentration the water is pre-heated to aid in dissolving the ingredients. For Diacetin and similar type simulates, sugar and HEC ingredients are not needed. The solution is mixed thoroughly, covered, and allowed to sit overnight prior to use.

The simulated tissue mixture was mixed based on the Simulated Tissue Composition indicated in table 8 below for 450MHz. During the daily testing of this product, the applicable mixture was used to measure the Di-electric parameters at each of the tested frequencies to verify that the Di-electric parameters were within the tolerance of the tissue specifications.

Simulated Tissue Composition (by mass)

TABLE 8

Reference Standards	% of listed ingredients	450MHz	
		Head	Body
FCC Supplement C (Edition 01-01) to OET Bulletin 65 (Edition 91-01)	Sugar	56.0	46.5
IEEE 1528-2003	Diacetin	NA	NA
IEC62209-1 (2005)	De ionized –Water	39.1	50.53
CENELEC – EN62209-1 (2006)	Salt	3.8	1.87
	HEC	1.0	1.0
	Bact.	0.1	0.1

Reference section 10.1 for target parameters

## 9.0 Additional Test Equipment

The table below lists additional test equipment used during the SAR assessment.

**TABLE 9**

Equipment Type	Model Number	Serial Number	Calibration Date	Calibration Due Date
DAE	DAE4	729	4/20/2012	4/20/2013
SAR Probe	EX3DV3	3163	4/25/2012	4/25/2013
Power Meter (Agilent)	E4419B	MY45103725	3/1/2013	3/1/2014
E-Series Avg. Power Sensor (Agilent)	E9301B	MY50280001	8/3/2012	8/3/2013
E-Series Avg. Power Sensor (Agilent)	E9301B	MY50290001	8/3/2012	8/3/2013
Bi-Directional Coupler (NARDA)	3020A	40296	2/9/2012	2/9/2014
Signal Generator (Agilent)	E4428C	MY47381119	6/24/2011	6/24/2013
AMP (Amplifier Research)	10WD1000	28782	CNR	CNR
Dickson Temperature Recorder	TM325	12121144	5/18/2012	5/18/2013
Omega Digital Thermometer with J Type TC Probe	HH202A	18801	5/23/2012	5/23/2013
(DAK) Dielectric Probe Station				
Agilent PNA-L Network Analyzer	N5230A	MY45001092	6/4/2012	6/4/2013
Speag Dipole	D450V3	1075	8/22/2011	8/22/2013

## 10.0 SAR Measurement System Verification

The system performance check was conducted daily and within 24 hours prior to testing. DASY output files of the probe/dipole calibration certificates and system performance test results are included in appendices B, C, D respectively.

### 10.1 Equivalent Tissue Test Results

Simulated tissue prepared for SAR measurements is measured daily and within 24 hours prior to actual SAR testing to verify that the tissue is within +/- 5% of target parameters at the center of the transmit band. This measurement is done using the applicable equipment indicated in section 9.0. The table below summarizes the measured tissue parameters used for the SAR assessment.

**TABLE 10**

Frequency (MHz)	Tissue Type	Conductivity Target (S/m)	Dielectric Constant Target	Conductivity Meas. (S/m)	Dielectric Constant Meas.	Tested Date
450	FCC Body	0.94 (0.89-0.99)	56.7 (53.9-59.5)	0.94	56.5	3/6/2013
450	IEEE /IEC Head	0.87 (0.83-0.91)	43.5 (41.3-45.7)	0.84	43.5	3/6/2013

### 10.2 System Check Test Results

System performance checks were conducted each day during the SAR assessment. The results are normalized to 1W. APPENDIX D includes DASY plots for each day during the SAR assessment. The table below summarizes the daily system check results used for the SAR assessment.

**TABLE 11**

Probe Serial #	Tissue Type	Dipole Kit / Serial #	Reference SAR @ 1W (W/kg)	System Check Results Measured (W/kg)	System Check Test Results when normalized to 1W (W/kg)	Tested Date
3163	450 MHz FCC Body	D450V3 SN 1075	4.50 +/- 10%	1.12	4.48	3/6/2013
3163	450 MHz IEEE/IEC Head	D450V3 SN 1075	4.69 +/- 10%	1.12	4.48	3/6/2013

## 11.0 Environmental Test Conditions

The EME Laboratory's ambient environment is well controlled resulting in very stable simulated tissue temperature and therefore stable dielectric properties. Simulated tissue temperature is measured prior to each scan to insure it is within  $\pm 2^{\circ}\text{C}$  of the temperature at which the dielectric properties were determined. The liquid depth within the phantom used for measurements was at least 15cm. Additional precautions are routinely taken to ensure the stability of the simulated tissue such as covering the phantoms when scans are not actively in process in order to minimize evaporation. The lab environment is continuously monitored. The table below presents the range and average environmental conditions during the SAR tests reported herein:

**TABLE 12**

	Target	Measured
Ambient Temperature	18 – 25 °C	Range: 20.7 – 21.3°C Avg. 21.1 °C
Relative Humidity	30 – 70 %	Range: 41.0 -52.7 % Avg. 49.3%
Tissue Temperature	NA	Range: 20.2-20.3°C Avg. 20.3°C

Relative humidity target range is a recommended target

The EME Lab RF environment uses a Spectrum Analyzer to monitor for extraneous large signal RF contaminants that could possibly affect the test results. If such unwanted signals are discovered the SAR scans are repeated.

## 12.0 DUT Test Methodology

### 12.1 Measurements

SAR measurements were performed using the DASY system described in section 8.0 using zoom scans. Elliptical flat phantoms filled with applicable simulated tissue were used for body and face testing.

### 12.2 DUT Configuration(s)

The DUT is a portable device operational at the body and face as described in section 6.0 while using the applicable accessories listed in section 7.0. All accessories listed in section 7.0 of this report were considered when implementing the guidelines specified in KDB 643646 D01.

### 12.3 DUT Positioning Procedures

The positioning of the device for each body location is described below and illustrated in APPENDIX G.

#### 12.3.1 Body

The DUT was positioned in normal use configuration against the phantom with the offered body worn accessory as well as with and without the offered audio accessories as applicable.

**12.3.2 Head**

Not applicable.

**12.3.3 Face**

The DUT was positioned with its’ front side separated 2.5cm from the phantom.

**12.4 DUT Test Channels**

The number of test channels was determined by using the following IEEE 1528 equation. The use of this equation produces the same or more test channels compared to the FCC KDB 447498 number of test channels formula.

$$N_c = 2 * roundup[10 * (f_{high} - f_{low}) / f_c] + 1$$

Where

N<sub>c</sub> = Number of channels

F<sub>high</sub> = Upper channel

F<sub>low</sub> = Lower channel

F<sub>c</sub> = Center channel

**12.5 DUT Test Plan**

The guidelines and requirements outlined in “SAR Test Reduction Considerations for Occupational PTT Radios” FCC KDB 643646 D01 dated 4/4/11 for head (face) and body were used to assess compliance of this device. All modes of operation identified in section 6.0 were considered during the development of the test plan. All tests were performed in 100% CW mode and then 50% duty cycle was applied to the final results to account for PTT operation.

**13.0 DUT Test Data**

**13.1 Assessments at the Body for 450-470 MHz band**

The battery PMNN4434AR was selected as the default battery. The conducted power measurement for all test channels within Part 90 frequency range using the default battery PMNN4434AR is indicated in Table 13. The channel with the highest conducted power will be identified as the default channel per KDB 643646 D01 SAR Test for PTT Radios v01r01. SAR plots of the highest results per table (bolded) are presented in APPENDICES E-F.

**TABLE 13**

<b>Test Freq (MHz)</b>	<b>Power (W)</b>
450.2	1.97
460.0	1.95
469.8	1.95

**13.1.1 Assessments at the Body with Body worn PMLN6455A**

Assessment of the offered antenna with the default battery, body worn PMLN6455A, and default audio accessory HMN9026D per KDB 643646 D01 SAR Test for PTT Radios v01r01 – Body SAR Test Considerations for Body worn Accessories. Refer to Table 13 for highest output power channel.

**TABLE 14**

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (mW/g)	Meas. 10g-SAR (mW/g)	Max Calc. 1g-SAR (mW/g)	Max Calc. 10g-SAR (mW/g)	Run#
Fixed Antenna	PMNN4434AR	PMLN6455A	HMN9026D	450.2	1.97	-0.42	2.01	1.50	<b>1.12</b>	0.84	ErC-Ab-130306-02
				460.0							
				469.8							

**13.1.2 Assessment of other audio accessories at the body**

Assessment per “KDB 643646 D01 Body SAR Test Consideration for Audio Accessories without Built-in Antenna; Sec 1, A. when overall < 4.0 W/kg, SAR tested for that audio accessory is not necessary.” This was applicable to all remaining accessories.

**13.2 Assessments at the Face for 450-470 MHz band**

The highest capacity battery PMNN4434AR was selected as the default battery. The conducted power measurement for all test channels within Part 90 frequency range using the default battery PMNN4434AR is indicated in the Table 15. The channel with the highest conducted power was used as the default channel per KDB 643646 D01 SAR Test for PTT Radios v01r01. SAR plots of the highest results per table (bolded) are presented in APPENDICES E-F.

**TABLE 15**

Test Freq (MHz)	Power (W)
450.2	1.97
460.0	1.95
469.8	1.95

Assessment of the offered antenna with the default battery PMNN4434AR, front of DUT facing phantom, and additional offered battery per KDB 643646 D01 SAR Test for PTT Radios v01r01 – Head SAR Test Considerations. Refer to Table 15 for highest output power channel.

**TABLE 16**

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (mW/g)	Meas. 10g-SAR (mW/g)	Max Calc. 1g-SAR (mW/g)	Max Calc. 10g-SAR (mW/g)	Run#
Fixed Antenna	PMNN4434AR	PMLN6455A	HMN9026D	450.2	1.97	-0.46	1.96	1.45	1.11	0.82	ErC-Face-130306-06
				460.0							
				469.8							

### 13.3 Shortened Scan Assessment

A “shortened” scan using the highest SAR configuration overall from above was performed to validate the SAR drift of the full DASY5™ coarse and zoom scans. Note that the shortened scan represents the zoom scan performance result; this is obtained by first running a coarse scan to find the peak area and then, using a newly charged battery, a zoom scan only was performed. The results of the shortened cube scan presented in APPENDIX E demonstrate that the scaling methodology used to determine the calculated SAR results presented herein are valid. The SAR result from the table below is provided in APPENDIX E.

**TABLE 17**

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (mW/g)	Meas. 10g-SAR (mW/g)	Max Calc. 1g-SAR (mW/g)	Max Calc. 10g-SAR (mW/g)	Run#
Fixed Antenna	PMNN4434AR	PMLN6455A	HMN9026D	450.2	1.97	-0.26	2.16	1.61	1.16	0.87	ErC-Ab-130306-04

### 14.0 Simultaneous Transmission Exclusion

Not applicable.

## 15.0 Conclusion

Based on the test guidelines from KDB 643646, the highest Operational Maximum Calculated 1-gram and 10-gram average SAR values found for this filing:

**TABLE 18**

Designator	Frequency band (MHz)	Max Calc at Body (mW/g)		Max Calc at Face (mW/g)	
		1g-SAR	10g-SAR	1g-SAR	10g-SAR
Overall	450-470	1.16	0.87	1.11	0.82
FCC	450-470	1.16	0.87	1.11	0.82

All results are scaled to the maximum output power

The test results clearly demonstrate compliance with FCC Occupational/Controlled RF Exposure limits of 8 W/kg averaged over 1 gram per the requirements of 47 CFR 2.1093(d). The 10 grams result is not applicable to FCC filing.

## APPENDIX A - Measurement Uncertainty

The Measurement Uncertainty tables indicated in this APPENDIX are applicable to the DUT test frequencies 450MHz  $\pm$  100MHz and for Dipole test frequency at 450MHz. Therefore, the highest tolerance for the probe calibration uncertainty is indicated.

**Uncertainty Budget for Device Under Test, for 450 MHz ±100MHz.**

<i>a</i>	<i>b</i>	<i>c</i>	<i>d</i>	<i>e = f(d,k)</i>	<i>f</i>	<i>g</i>	<i>h = c x f / e</i>	<i>i = c x g / e</i>	<i>k</i>
Uncertainty Component	IEEE 1528 section	Tol. (± %)	Prob Dist	Div.	<i>c<sub>i</sub></i> (1 g)	<i>c<sub>i</sub></i> (10 g)	1 g <i>u<sub>i</sub></i> (±%)	10 g <i>u<sub>i</sub></i> (±%)	<i>v<sub>i</sub></i>
<b>Measurement System</b>									
Probe Calibration	E.2.1	6.7	N	1.00	1	1	6.7	6.7	∞
Axial Isotropy	E.2.2	4.7	R	1.73	0.707	0.707	1.9	1.9	∞
Hemispherical Isotropy	E.2.2	9.6	R	1.73	0.707	0.707	3.9	3.9	∞
Boundary Effect	E.2.3	1.0	R	1.73	1	1	0.6	0.6	∞
Linearity	E.2.4	4.7	R	1.73	1	1	2.7	2.7	∞
System Detection Limits	E.2.5	1.0	R	1.73	1	1	0.6	0.6	∞
Readout Electronics	E.2.6	0.3	N	1.00	1	1	0.3	0.3	∞
Response Time	E.2.7	1.1	R	1.73	1	1	0.6	0.6	∞
Integration Time	E.2.8	1.1	R	1.73	1	1	0.6	0.6	∞
RF Ambient Conditions - Noise	E.6.1	3.0	R	1.73	1	1	1.7	1.7	∞
RF Ambient Conditions - Reflections	E.6.1	0.0	R	1.73	1	1	0.0	0.0	∞
Probe Positioner Mech. Tolerance	E.6.2	0.4	R	1.73	1	1	0.2	0.2	∞
Probe Positioning w.r.t Phantom	E.6.3	1.4	R	1.73	1	1	0.8	0.8	∞
Max. SAR Evaluation (ext., int., avg.)	E.5	3.4	R	1.73	1	1	2.0	2.0	∞
<b>Test sample Related</b>									
Test Sample Positioning	E.4.2	3.2	N	1.00	1	1	3.2	3.2	29
Device Holder Uncertainty	E.4.1	4.0	N	1.00	1	1	4.0	4.0	8
SAR drift	6.6.2	5.0	R	1.73	1	1	2.9	2.9	∞
<b>Phantom and Tissue Parameters</b>									
Phantom Uncertainty	E.3.1	4.0	R	1.73	1	1	2.3	2.3	∞
Liquid Conductivity (target)	E.3.2	5.0	R	1.73	0.64	0.43	1.8	1.2	∞
Liquid Conductivity (measurement)	E.3.3	3.3	N	1.00	0.64	0.43	2.1	1.4	∞
Liquid Permittivity (target)	E.3.2	5.0	R	1.73	0.6	0.49	1.7	1.4	∞
Liquid Permittivity (measurement)	E.3.3	1.9	N	1.00	0.6	0.49	1.1	0.9	∞
<b>Combined Standard Uncertainty</b>			RSS				12	11	482
<b>Expanded Uncertainty</b> (95% CONFIDENCE LEVEL)			<i>k</i> =2				23	23	

**FCD-0558 Uncertainty Budget Rev.8**

**Uncertainty Budget for System Verification (dipole & flat phantom) for 450 MHz**

## Notes:

- a) Column headings a-k are given for reference.
- b) Tol. - tolerance in influence quantity.
- c) Prob. Dist. – Probability distribution
- d) N, R - normal, rectangular probability distributions
- e) Div. - divisor used to translate tolerance into normally distributed standard uncertainty
- f)  $c_i$  - sensitivity coefficient that should be applied to convert the variability of the uncertainty component into a variability of SAR.
- g)  $u_i$  – SAR uncertainty
- h)  $\nu_i$  - degrees of freedom for standard uncertainty and effective degrees of freedom for the expanded uncertainty

## APPENDIX B - Probe Calibration Certificates

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**S** Service suisse d'étalonnage  
**C** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Motorola EME**

Certificate No: **ES3-3163\_Apr12**

**CALIBRATION CERTIFICATE**

Object **ES3DV3 - SN:3163**

Calibration procedure(s) **QA CAL-01.v8, QA CAL-12.v7, QA CAL-14.v3, QA CAL-23.v4,  
QA CAL-25.v4  
Calibration procedure for dosimetric E-field probes**

Calibration date: **April 25, 2012**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	29-Mar-12 (No. 217-01508)	Apr-13
Power sensor E4412A	MY41498087	29-Mar-12 (No. 217-01508)	Apr-13
Reference 3 dB Attenuator	SN: S5054 (3c)	27-Mar-12 (No. 217-01531)	Apr-13
Reference 20 dB Attenuator	SN: S5086 (20b)	27-Mar-12 (No. 217-01529)	Apr-13
Reference 30 dB Attenuator	SN: S5129 (30b)	27-Mar-12 (No. 217-01532)	Apr-13
Reference Probe ES3DV2	SN: 3013	29-Dec-11 (No. ES3-3013_Dec11)	Dec-12
DAE4	SN: 660	10-Jan-12 (No. DAE4-660_Jan12)	Jan-13
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-11)	In house check: Apr-13
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-11)	In house check: Oct-12

	Name	Function	Signature
Calibrated by:	Jeton Kastrati	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	

Issued: April 25, 2012

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S  
C  
S** Schweizerischer Kalibrierdienst  
Service suisse d'étalonnage  
Servizio svizzero di taratura  
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

### Glossary:

TSL	tissue simulating liquid
NORM <sub>x,y,z</sub>	sensitivity in free space
ConvF	sensitivity in TSL / NORM <sub>x,y,z</sub>
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C	modulation dependent linearization parameters
Polarization $\varphi$	$\varphi$ rotation around probe axis
Polarization $\vartheta$	$\vartheta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

### Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>**: Assessed for E-field polarization  $\vartheta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not affect the  $E^2$ -field uncertainty inside TSL (see below ConvF).
- NORM(f)<sub>x,y,z</sub> = NORM<sub>x,y,z</sub> \* frequency\_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>x,y,z</sub>**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; VR<sub>x,y,z</sub>; A, B, C** are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

ES3DV3 – SN:3163

April 25, 2012

# Probe ES3DV3

## SN:3163

Manufactured: October 8, 2007  
Calibrated: April 25, 2012

Calibrated for DASY/EASY Systems  
(Note: non-compatible with DASY2 system!)

ES3DV3- SN:3163

April 25, 2012

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3163

### Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) <sup>A</sup>	1.31	1.13	1.04	$\pm 10.1 \%$
DCP (mV) <sup>B</sup>	101.8	101.0	102.5	

### Modulation Calibration Parameters

UID	Communication System Name	PAR		A dB	B dB	C dB	VR mV	Unc <sup>E</sup> (k=2)
0	CW	0.00	X	0.00	0.00	1.00	160.8	$\pm 3.0 \%$
			Y	0.00	0.00	1.00	149.8	
			Z	0.00	0.00	1.00	149.1	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3163

### Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>c</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
300	45.3	0.87	7.37	7.37	7.37	0.24	1.02	± 13.4 %
450	43.5	0.87	6.71	6.71	6.71	0.16	1.81	± 13.4 %
750	41.9	0.89	6.30	6.30	6.30	0.39	1.61	± 12.0 %
900	41.5	0.97	6.00	6.00	6.00	0.26	2.12	± 12.0 %
1810	40.0	1.40	5.28	5.28	5.28	0.51	1.65	± 12.0 %
1950	40.0	1.40	4.98	4.98	4.98	0.43	1.58	± 12.0 %
2300	39.5	1.67	4.75	4.75	4.75	0.62	1.42	± 12.0 %
2450	39.2	1.80	4.44	4.44	4.44	0.80	1.22	± 12.0 %
2600	39.0	1.96	4.27	4.27	4.27	0.80	1.24	± 12.0 %
3500	37.9	2.91	3.91	3.91	3.91	1.00	1.32	± 13.1 %
3700	37.7	3.12	3.73	3.73	3.73	1.00	1.25	± 13.1 %

<sup>c</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3163


### Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
300	58.2	0.92	6.78	6.78	6.78	0.22	1.78	± 13.4 %
450	56.7	0.94	6.97	6.97	6.97	0.08	1.00	± 13.4 %
750	55.5	0.96	6.16	6.16	6.16	0.25	2.12	± 12.0 %
900	55.0	1.05	6.02	6.02	6.02	0.34	1.77	± 12.0 %
1810	53.3	1.52	4.71	4.71	4.71	0.58	1.60	± 12.0 %
1950	53.3	1.52	4.64	4.64	4.64	0.47	1.88	± 12.0 %
2300	52.9	1.81	4.25	4.25	4.25	0.80	1.29	± 12.0 %
2450	52.7	1.95	4.05	4.05	4.05	0.70	1.19	± 12.0 %
2600	52.5	2.16	3.88	3.88	3.88	0.69	1.01	± 12.0 %
3500	51.3	3.31	3.36	3.36	3.36	0.85	1.58	± 13.1 %
3700	51.0	3.55	3.23	3.23	3.23	0.58	2.05	± 13.1 %

<sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

### Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)


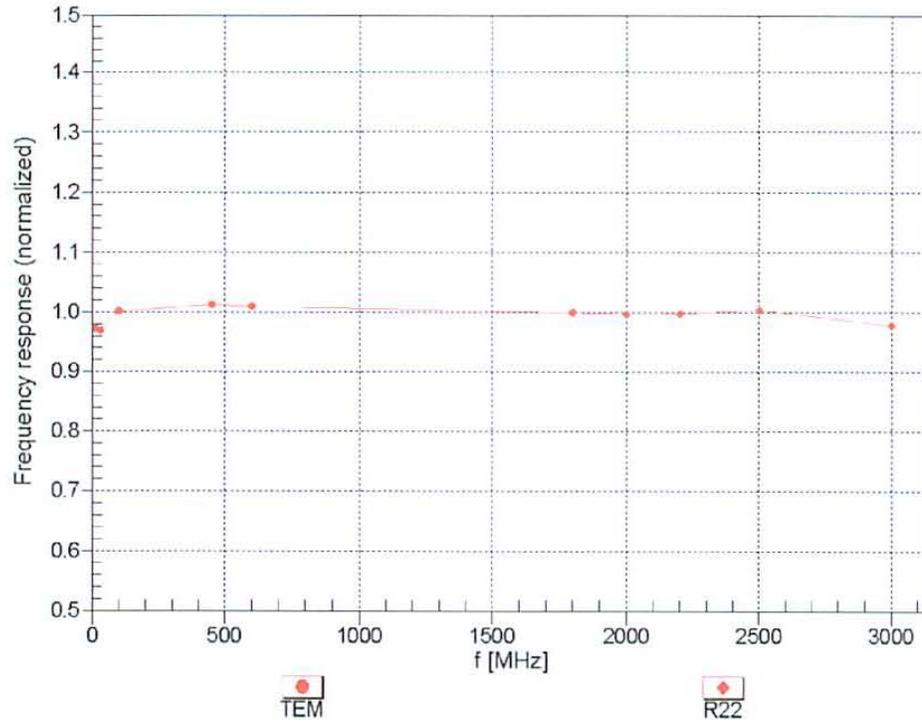


Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  (k=2)

### Receiving Pattern ( $\phi$ ), $\vartheta = 0^\circ$



f=600 MHz,TEM

f=1800 MHz,R22

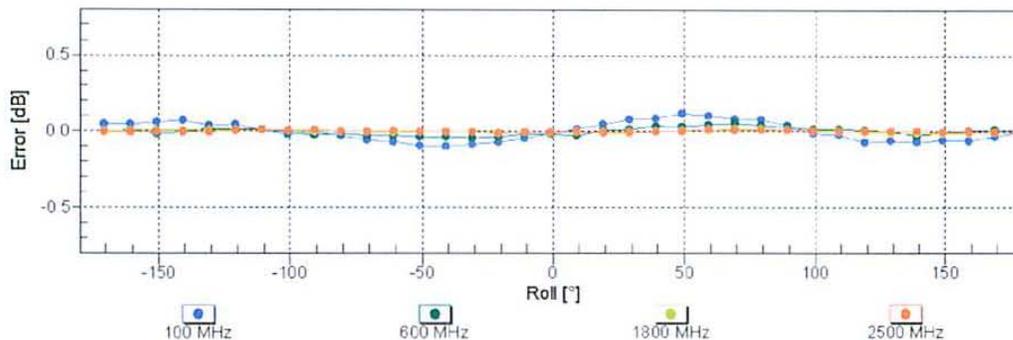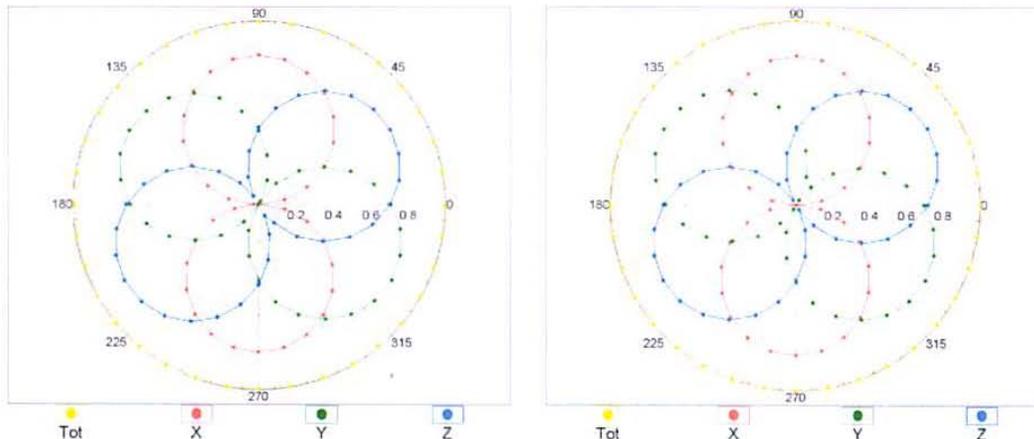


Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  (k=2)

### Dynamic Range $f(SAR_{head})$ (TEM cell , $f = 900$ MHz)

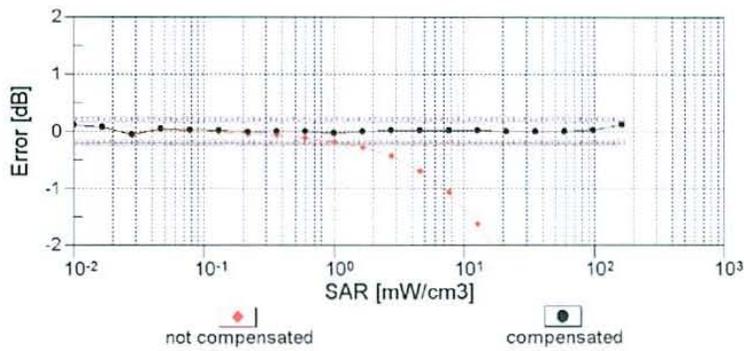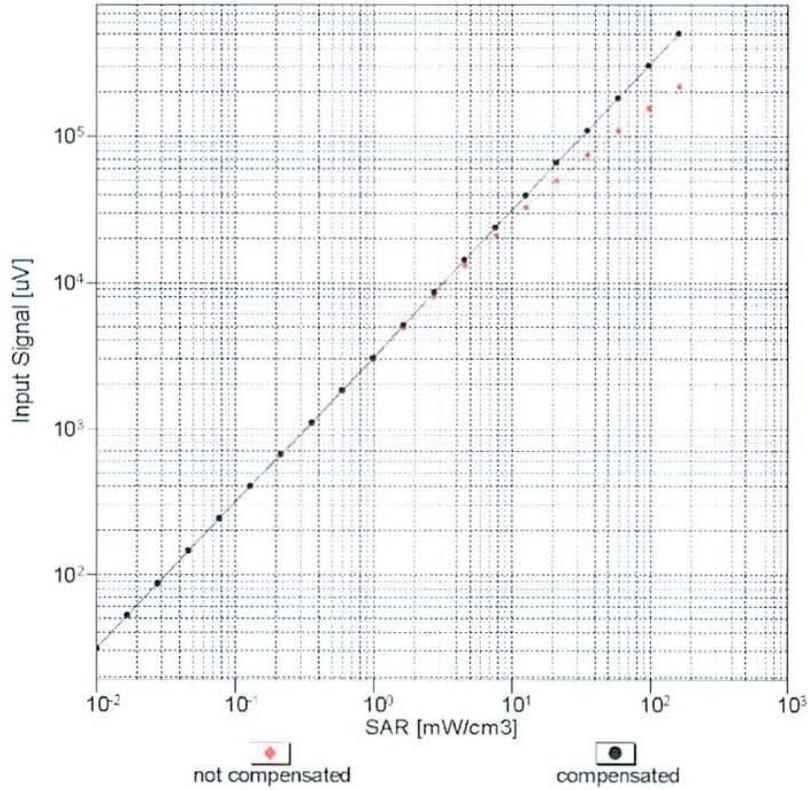


Uncertainty of Linearity Assessment:  $\pm 0.6\%$  ( $k=2$ )

### Conversion Factor Assessment

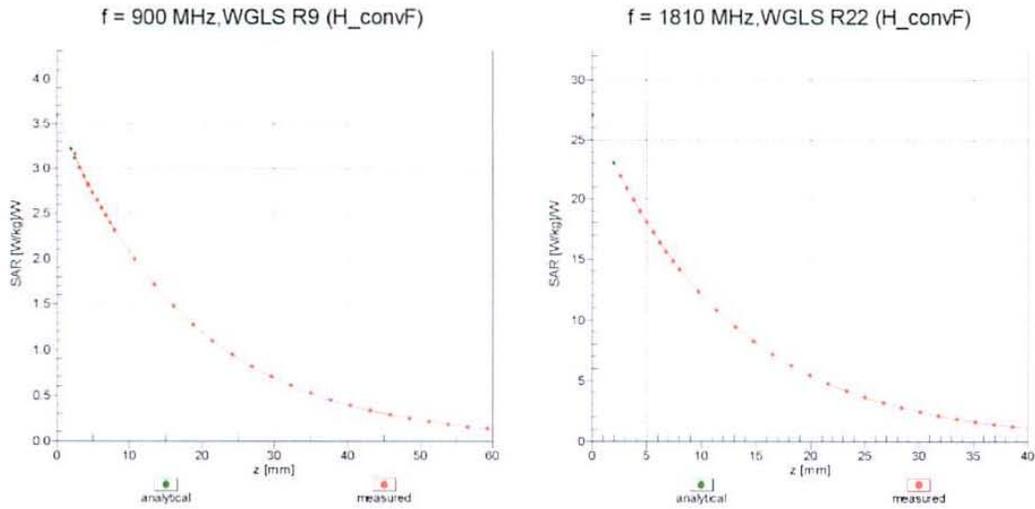

### Deviation from Isotropy in Liquid Error ( $\phi, \vartheta$ ), f = 900 MHz

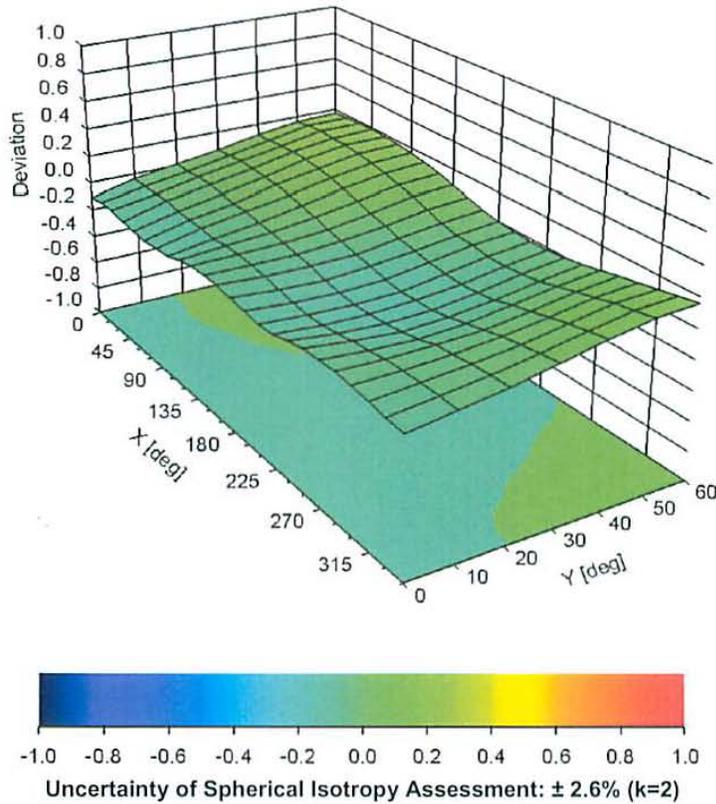

**DASY/EASY - Parameters of Probe: ES3DV3 - SN:3163****Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	-170.9
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	4 mm
Probe Tip to Sensor X Calibration Point	2 mm
Probe Tip to Sensor Y Calibration Point	2 mm
Probe Tip to Sensor Z Calibration Point	2 mm
Recommended Measurement Distance from Surface	3 mm

Schmid & Partner Engineering AG

**s p e a g**

Zeughausstrasse 43, 8004 Zurich, Switzerland  
 Phone +41 44 245 9700, Fax +41 44 245 9779  
 info@speag.com, http://www.speag.com

## Additional Conversion Factors for Dosimetric E-Field Probe

Type:	<b>ES3DV3</b>
Serial Number:	<b>3163</b>
Place of Assessment:	<b>Zurich</b>
Date of Assessment:	<b>April 26, 2012</b>
Probe Calibration Date:	<b>April 25, 2012</b>

Schmid & Partner Engineering AG hereby certifies that conversion factor(s) of this probe have been evaluated on the date indicated above. The assessment was performed using the FDTD numerical code SEMCAD of Schmid & Partner Engineering AG. Since the evaluation is coupled with measured conversion factors, it has to be recalculated yearly, i.e., following the re-calibration schedule of the probe. The uncertainty of the numerical assessment is based on the extrapolation from measured value at 450, 900 MHz or 1810 MHz.

Assessed by:



Schmid & Partner Engineering AG

**s p e a g**

Zeughausstrasse 43, 8004 Zurich, Switzerland  
 Phone +41 44 245 9700, Fax +41 44 245 9779  
 info@speag.com, http://www.speag.com

**Dosimetric E-Field Probe ES3DV3 SN:3163**

Conversion factor ( $\pm$  standard deviation)

150  $\pm$  50 MHz      *ConvF*      8.2  $\pm$  10%

$\epsilon_r = 52.3 \pm 5\%$   
 $\sigma = 0.76 \pm 5\%$  mho/m  
 (head tissue)

150  $\pm$  50 MHz      *ConvF*      7.9  $\pm$  10%

$\epsilon_r = 61.9 \pm 5\%$   
 $\sigma = 0.80 \pm 5\%$  mho/m  
 (body tissue)

**Important Note:**

**For numerically assessed probe conversion factors, parameters Alpha and Delta in the DASY software must have the following entries: Alpha = 0 and Delta = 1.**

**Please see also DASY Manual.**

## APPENDIX C - Dipole Calibration Certificates and Validation

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Motorola EME**

Certificate No: **D450V3-1075\_Aug11/2**

**CALIBRATION CERTIFICATE (Replacement of No:D450V3-1075\_Aug11)**

Object **D450V3 - SN: 1075**

Calibration procedure(s) **QA CAL-15.v6  
Calibration procedure for dipole validation kits below 700 MHz**

Calibration date: **August 22, 2011**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	31-Mar-11 (No. 217-01372)	Apr-12
Power sensor E4412A	MY41498087	31-Mar-11 (No. 217-01372)	Apr-12
Reference 3 dB Attenuator	SN: S5054 (3c)	29-Mar-11 (No. 217-01369)	Apr-12
Reference 20 dB Attenuator	SN: S5086 (20b)	29-Mar-11 (No. 217-01367)	Apr-12
Type-N mismatch combination	SN: 5047.3 / 06327	29-Mar-11 (No. 217-01168)	Apr-12
Reference Probe ET3DV6	SN: 1507	29-Apr-11 (No. ET3-1507_Apr11)	Apr-12
DAE4	SN: 654	3-May-11 (No. DAE4-654_May11)	May-12
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-09)	In house check: Oct-11
RF generator R&S SMT-06	100005	4-Aug-99 (in house check Oct-09)	In house check: Oct-11
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-10)	In house check: Oct-11

	Name	Function	Signature
Calibrated by:	Jeton Kastrati	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	

Issued: March 5, 2012

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

**Glossary:**

TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORM x,y,z  
N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

**Additional Documentation:**

- d) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

<b>DASY Version</b>	DASY5	V52.6.2
<b>Extrapolation</b>	Advanced Extrapolation	
<b>Phantom</b>	ELI4 Flat Phantom	Shell thickness: 2 ± 0.2 mm
<b>Distance Dipole Center - TSL</b>	15 mm	with Spacer
<b>Zoom Scan Resolution</b>	dx, dy, dz = 5 mm	
<b>Frequency</b>	450 MHz ± 1 MHz	

**Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
<b>Nominal Head TSL parameters</b>	22.0 °C	43.5	0.87 mho/m
<b>Measured Head TSL parameters</b>	(22.0 ± 0.2) °C	44.5 ± 6 %	0.86 mho/m ± 6 %
<b>Head TSL temperature change during test</b>	< 0.5 °C	----	----

**SAR result with Head TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	398 mW input power	1.84 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	<b>4.69 mW / g ± 18.1 % (k=2)</b>

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	398 mW input power	1.23 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	<b>3.12 mW / g ± 17.6 % (k=2)</b>

**Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
<b>Nominal Body TSL parameters</b>	22.0 °C	56.7	0.94 mho/m
<b>Measured Body TSL parameters</b>	(22.0 ± 0.2) °C	55.5 ± 6 %	0.94 mho/m ± 6 %
<b>Body TSL temperature change during test</b>	< 0.5 °C	----	----

**SAR result with Body TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	398 mW input power	1.80 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	<b>4.50 mW / g ± 18.1 % (k=2)</b>

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	398 mW input power	1.20 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	<b>3.01 mW / g ± 17.6 % (k=2)</b>

**Appendix**

**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	59.4 Ω - 2.2 jΩ
Return Loss	- 21.1 dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	56.6 Ω - 5.8 jΩ
Return Loss	- 21.7 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.355 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	June 24, 2010

**DASY5 Validation Report for Head TSL**

Date: 22.08.2011

Test Laboratory: SPEAG

**DUT: Dipole 450 MHz; Type: D450V3; Serial: D450V3 - SN: 1075**

Communication System: CW; Frequency: 450 MHz

Medium parameters used:  $f = 450$  MHz;  $\sigma = 0.86$  mho/m;  $\epsilon_r = 44.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ET3DV6 - SN1507; ConvF(6.59, 6.59, 6.59); Calibrated: 29.04.2011
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 03.05.2011
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1003
- DASY52 52.6.2(482); SEMCAD X 14.4.5(3634)

**Dipole Calibration for Head Tissue/d=15mm, Pin=398mW/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 49.673 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 2.798 W/kg


**SAR(1 g) = 1.84 mW/g; SAR(10 g) = 1.23 mW/g**

Maximum value of SAR (measured) = 1.967 mW/g

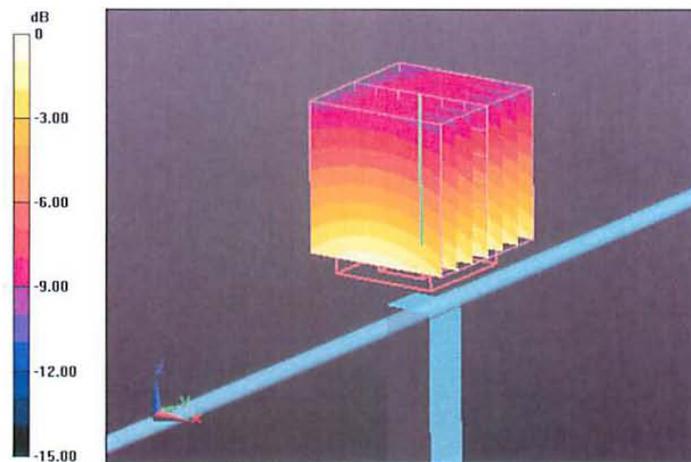

0 dB = 1.970mW/g

### Impedance Measurement Plot for Head TSL

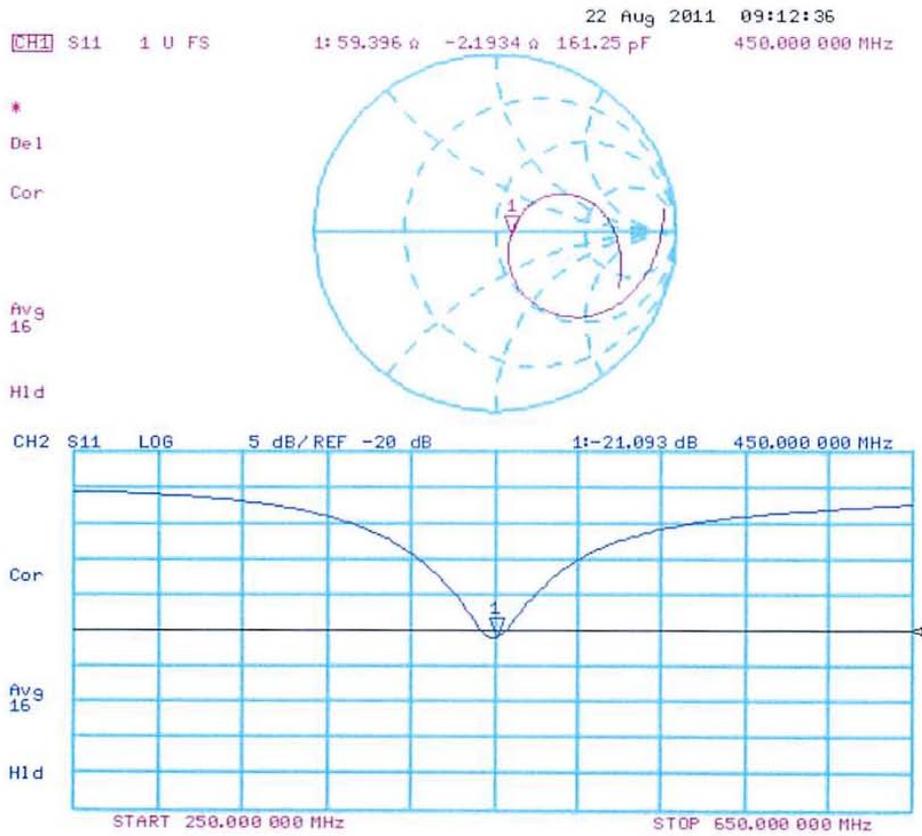

**DASY5 Validation Report for Body TSL**

Date: 22.08.2011

Test Laboratory: SPEAG

**DUT: Dipole 450 MHz; Type: D450V3; Serial: D450V3 - SN: 1075**

Communication System: CW; Frequency: 450 MHz

Medium parameters used:  $f = 450 \text{ MHz}$ ;  $\sigma = 0.94 \text{ mho/m}$ ;  $\epsilon_r = 55.5$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ET3DV6 - SN1507; ConvF(7.05, 7.05, 7.05); Calibrated: 29.04.2011
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 03.05.2011
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1003
- DASY52 52.6.2(482); SEMCAD X 14.4.5(3634)

**Dipole Calibration for Body Tissue/d=15mm, Pin=398mW/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 46.440 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 2.825 W/kg


**SAR(1 g) = 1.8 mW/g; SAR(10 g) = 1.2 mW/g**

Maximum value of SAR (measured) = 1.924 mW/g

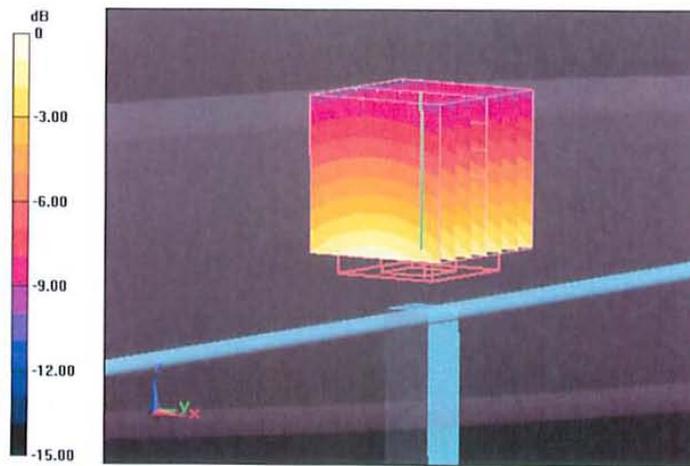

0 dB = 1.920mW/g

### Impedance Measurement Plot for Body TSL

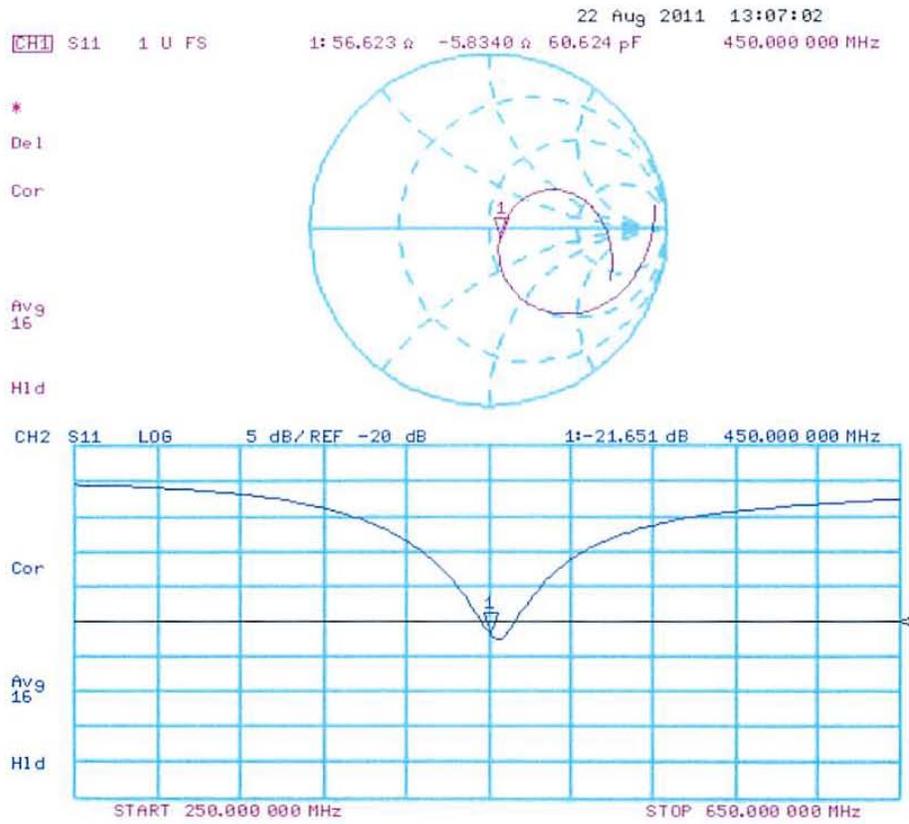

System Validation - Head

Date:	<u>09/04/12</u>	Frequency (MHz):	<u>450</u>
Lab Location:	<u>FL08</u>	Mixture Type:	<u>IEEE Head</u>
DAE Serial #:	<u>363</u>	Ambient Temp.(°C):	<u>21.6</u>

Tissue Characteristics		Phantom Type/SN:	<u>OVAL1108</u>
Permittivity:	<u>44.5</u>	Distance (mm):	<u>15</u>
Conductivity:	<u>0.86</u>		
Tissue Temp.(°C):	<u>21.1</u>		

Reference Source:	<u>Dipole</u>	Power to Dipole:	<u>250</u> mW
Reference SN:	<u>1075</u>		

IEEE Target 1g-SAR Value (mW/g, normalized to 1.0 W):

<b>4.58</b>
-------------

Difference from Target

2.18% (1g-SAR)
----------------

Result:

Average 1g-SAR Value (mW/g):	<b>4.68</b>
---------------------------------	-------------

<b>Passes K=2</b>
-------------------

Percent Difference From Target (MUST be within k=2 Uncertainty):

Probe SN #s	1g-SAR (Cube)	Diff from Avg	Robot
3163	4.68	0.0%	R3
Average <b>4.6800</b>		New Measured SAR Value	

(normalized to 1.0 W)

Test performed by: C. Miller