



DECLARATION OF COMPLIANCE SAR ASSESSMENT Part 1 of 2

Motorola Solutions Inc.
EME Test Laboratory
 Motorola Solutions Malaysia Sdn Bhd (Innoplex)
 Plot 2A, Medan Bayan Lepas,
 Mukim 12 SWD 11900 Bayan Lepas Penang, Malaysia.

Date of Report: 08/24/2018
Report Revision: B

Responsible Engineer: Ch'ng Jian Sheng (EME Engineer)
Report Author: Ch'ng Jian Sheng (EME Engineer)
Date/s Tested: 07/24/2018 – 07/27/2018, 08/03/2018 - 08/05/2018
Manufacturer: Motorola Solutions Inc
DUT Description: Handheld Portable T503 Consumer Radio 462-467 MHz Orange & T600 Consumer Radio 462-467 MHz Impact Green
Test TX mode(s): CW (PTT)
Max. Power output: 2.00W (462.5500 – 462.7250 MHz), 0.50W (467.5625 – 467.7125 MHz)
Nominal Power: 1.80W (462.5500 – 462.7250 MHz), 0.40W (467.5625 – 467.7125 MHz)
Tx Frequency Bands: 462.5500 – 462.7250 MHz, 467.5625 - 467.7125 MHz
Signaling type: FM
Model(s) Tested: T6B22201GWRAAW (PMUE4915B), T5B22201EWRAAW (PMUE5289B)
Model(s) Certified: T6B22201GWRAAW (PMUE4915B), T5B22201EWRAAW (PMUE5289B), T6B22201GWCAAG (PMUE4915B)
Serial Number(s): 1754RV0003, 1754RV0009
Classification: General Population/Uncontrolled Environment
FCC ID: AZ489FT4950
IC: 109U-89FT4950
ISED Test Site registration: 109AK
FCC Test Firm Registration Number: 823256

The test results clearly demonstrate compliance with General Population / Uncontrolled RF Exposure limits of 1.6 W/kg averaged over 1 gram per the requirements of FCC 47 CFR § 2.1093 and ISED RSS-102 (Issue 5).

Based on the information and the testing results provided herein, the undersigned certifies that when used as stated in the operating instructions supplied, said product complies with the national and international reference standards and guidelines listed in section 4.0 of this report. This report shall not be reproduced without written approval from an officially designated representative of the Motorola Solutions Inc EME Laboratory. I attest to the accuracy of the data and assume full responsibility for the completeness of these measurements. This reporting format is consistent with the suggested guidelines of the TIA TSB-150 December 2004. The results and statements contained in this report pertain only to the device(s) evaluated.

Tiong Nguk Ing
Deputy Technical Manager (Approved Signatory)
Approval Date: 8/24/2018

CONTENTS**Part 1 of 2**

1.0	Introduction.....	4
2.0	FCC SAR Summary.....	4
3.0	Abbreviations / Definitions.....	4
4.0	Referenced Standards and Guidelines	5
5.0	SAR Limits	6
6.0	Description of Device Under Test (DUT)	6
7.0	Optional Accessories and Test Criteria.....	7
7.1	Antennas	7
7.2	Batteries	7
7.3	Body worn Accessories.....	7
7.4	Audio Accessories	8
8.0	Description of Test System	9
8.1	Descriptions of Robotics/Probes/Readout Electronics	9
8.2	Description of Phantom(s).....	10
8.3	Description of Simulated Tissue.....	10
9.0	Additional Test Equipment.....	11
10.0	SAR Measurement System Validation and Verification	12
10.1	System Validation.....	12
10.2	System Verification	12
10.3	Equivalent Tissue Test Results	13
11.0	Environmental Test Conditions	14
12.0	DUT Test Setup and Methodology	14
12.1	Measurements	14
12.2	DUT Configuration(s).....	15
12.3	DUT Positioning Procedures	15
12.3.1	Body.....	15
12.3.2	Head.....	15
12.3.3	Face.....	15
12.4	DUT Test Channels	16
12.5	SAR Result Scaling Methodology	16
12.6	DUT Test Plan	16
13.0	DUT Test Data.....	17
13.1	Assessment at the Body for 462.5500 – 462.7250MHz band.....	17
13.2	Assessment at the Face for 462.5500 – 462.7250MHz band.....	19
13.3	Assessment at the Body for 467.5625 – 467.7125MHz band.....	20
13.4	Assessment at the Face for 467.5625 – 467.7125MHz band.....	22
13.5	Shortened Scan Assessment.....	23
14.0	Results Summary	23
15.0	Variability Assessment	24
16.0	System Uncertainty	24

APPENDICES

A	Measurement Uncertainty Budget	25
B	Probe Calibration Certificates	28
C	Dipole Calibration Certificates	63
D	SAR Summary Results Table for FCC review	73

Part 2 of 2**APPENDICES**

E	System Verification Check Scans	2
F	DUT Scans	9
G	Shorten Scan of Highest SAR Configuration	19
H	DUT Test Position Photos	21
I	DUT, Body worn and audio accessories Photos	22

Report Revision History

Date	Revision	Comments
08/06/2018	A	Initial release
08/24/2018	B	Update models number

1.0 Introduction

This report details the utilization, test setup, test equipment, and test results of the Specific Absorption Rate (SAR) measurements performed at the Motorola Solutions Inc. EME Test Laboratory for handheld portable model number T6B22201GWRAAW (PMUE4915B) and T5B22201EWRAAW (PMUE5289B). These devices are classified as General Population/Uncontrolled.

2.0 FCC SAR Summary

Table 1

Equipment Class	Frequency band (MHz)	Max Calc at Body (W/kg)	Max Calc at Face (W/kg)
		1g-SAR	1g-SAR
FRF	462.5500 – 462.7250	1.04	0.94
	467.5625 - 467.7125	0.54	0.50

3.0 Abbreviations / Definitions

CNR: Calibration Not Required
 CW: Continuous Wave
 DUT: Device Under Test
 FRF: Part 95 Family Radio Face Held Transmitter
 EME: Electromagnetic Energy
 FM: Frequency Modulation
 NA: Not Applicable
 PTT: Push to Talk
 SAR: Specific Absorption Rate
 NiMH: Nickel Metal Hydride

Audio accessories: These accessories allow communication while the DUT is worn on the body.

Body worn accessories: These accessories allow the DUT to be worn on the body of the user.

Maximum Power: Defined as the upper limit of the production line final test station.

4.0 Referenced Standards and Guidelines

This product is designed to comply with the following applicable national and international standards and guidelines.

- IEC62209-1 (2016) Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)
- Federal Communications Commission, “Evaluating Compliance with FCC Guidelines for Human Exposure to Radio frequency Electromagnetic Fields”, OET Bulletin 65, FCC, Washington, D.C.: 1997.
- IEEE 1528 (2013), Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques
- American National Standards Institute (ANSI) / Institute of Electrical and Electronics Engineers (IEEE) C95. 1-1992
- Institute of Electrical and Electronics Engineers (IEEE) C95.1-2005
- International Commission on Non-Ionizing Radiation Protection (ICNIRP) 1998
- Ministry of Health (Canada) Safety Code 6 (2015), Limits of Human Exposure to Radio frequency Electromagnetic Fields in the Frequency Range from 3 kHz to 300 GHz
- RSS-102 (Issue 5) – Radio Frequency (RF) Exposure Compliance of Radiocommunication Apparatus (All Frequency Bands)
- Australian Communications Authority Radio communications (Electromagnetic Radiation - Human Exposure) Standard (2014)
- ANATEL, Brazil Regulatory Authority, Resolution No. 303 of July 2, 2002 "Regulation of the limitation of exposure to electrical, magnetic, and electromagnetic fields in the radio frequency range between 9 kHz and 300 GHz." and “Attachment to resolution # 303 from July 2, 2002”
- IEC62209-2 Edition 1.0 2010-03, Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices – Human models, instrumentation, and procedures – Part 2: Procedure to determine the specific absorption rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz).
- FCC KDB – 643646 D01 SAR Test for PTT Radios v01r03
- FCC KDB – 865664 D01 SAR Measurement 100 MHz to 6 GHz v01r04
- FCC KDB – 865664 D02 RF Exposure Reporting v01r02
- FCC KDB – 447498 D01 General RF Exposure Guidance v06

5.0 SAR Limits

Table 2

EXPOSURE LIMITS	SAR (W/kg)	
	(General Population / Uncontrolled Exposure Environment)	(Occupational / Controlled Exposure Environment)
Spatial Average - ANSI - (averaged over the whole body)	0.08	0.4
Spatial Peak - ANSI - (averaged over any 1-g of tissue)	1.6	8.0
Spatial Peak – ICNIRP/ANSI - (hands/wrists/feet/ankles averaged over 10-g)	4.0	20.0
Spatial Peak - ICNIRP - (Head and Trunk 10-g)	2.0	10.0

6.0 Description of Device Under Test (DUT)

These devices operate in a half duplex system. A half duplex system only allows the user to transmit or receive. These devices cannot transmit and receive simultaneously. The user must stop transmitting in order to receive a signal or listen for a response, regardless of PTT button or use of voice activated audio accessories. This type of operation, along with the RF safety booklet, which instructs the user to transmit no more than 50% of the time, justifies the use of 50% duty factor for this device.

Table 3 below summarizes the bands, maximum duty cycles and maximum output powers. Maximum output powers are defined as upper limit of the production line final test station.

Table 3

Band (MHz)	Duty Cycle (%)	Max Power (W)
467.5625 – 467.7125	*50	0.50
462.5500 – 462.7250	*50	2.00

Note - * includes 50% PTT operation

The intended operating positions are “at the face” with the DUT at least 2.5cm from the mouth, and “at the body” by means of the offered body worn accessories. Body worn audio and PTT operation is accomplished by means of optional remote accessories that are connected to the radio.

7.0 Optional Accessories and Test Criteria

This device is offered with optional accessories. All accessories were individually evaluated during the test plan creation to determine if testing was required per the guidelines outlined in 4.0 to assess compliance of the device.

7.1 Antennas

There is one fixed antenna offered for this product. The table below lists its descriptions.

Table 4

Antenna No.	Antenna Models	Description	Selected for test	Tested
1	EAN.144F.823RA1	FIXED, 100-500 MHz, ¼ wave, -0.5dBi	Yes	Yes

7.2 Batteries

There are three batteries offered for this product. The table below lists their descriptions.

Table 5

Battery No.	Battery Models	Description	Selected for test	Tested	Comments
1	AA Alkaline	3xAA Alkaline individual batteries	Yes	Yes	
2	KEBT-1300	1300mAh 3xAA NiMH Rechargeable Battery Pack	Yes	Yes	
3	PMNN4477A	800mAh 3xAA NiMH Rechargeable Battery Pack	Yes	Yes	

7.3 Body worn Accessories

All body worn accessories were considered. The Table below lists the body worn accessories, and body worn accessory descriptions.

Table 6

Body worn No.	Body worn Models	Description	Selected for test	Tested	Comments
1	PMLN7240A	T400 Series Whistle Belt Clip	Yes	Yes	
2	PMLN7706AR	Carry Pouch	Yes	Yes	
3	PMLN7220A	T400 Series Belt Clip	Yes	Yes	

7.4 Audio Accessories

All audio accessories were considered. The Table below lists the offered audio accessories and their descriptions. Exhibit 7B illustrates photos of the tested audio accessories.

Table 7

Audio No.	Audio Acc. Models	Description	Selected for test	Tested	Comments
1	53725C	Headset w/Swivel Boom Microphone	Yes	Yes	Default audio for testing; with VOX feature
2	53727B	Earbud w/Push-to-Talk Microphone	Yes	Yes	
3	56320B	Earpiece w/Boom Microphone	Yes	Yes	
4	GU6443A (1518)	Surveillance Headset	Yes	Yes	
5	PMLN7705AR	Throat mic with PTT-VOX switch	Yes	Yes	
6	53724C	Remote Speaker Microphone	Yes	Yes	

8.0 Description of Test System



8.1 Descriptions of Robotics/Probes/Readout Electronics

Table 8

Dosimetric System type	System version	DAE type	Probe Type
Schmid & Partner Engineering AG SPEAG DASY 5	52.8.2.969	DAE4	ES3DV3 & EX3DV4 (E-Field)

The DASYSTM system is operated per the instructions in the DASYSTM Users Manual. The complete manual is available directly from SPEAGTM. All measurement equipment used to assess SAR compliance was calibrated according to ISO/IEC 17025 A2LA guidelines. Section 9.0 presents additional test equipment information. Appendices B and C present the applicable calibration certificates. The E-field probe first scans a coarse grid over a large area inside the phantom in order to locate the interpolated maximum SAR distribution. After the coarse scan measurement, the probe is automatically moved to a position at the interpolated maximum. The subsequent scan can directly use this position as reference for the cube evaluations.

8.2 Description of Phantom(s)

Table 9

Phantom Type	Phantom(s) Used	Material Parameters	Phantom Dimensions LxWxD (mm)	Material Thickness (mm)	Support Structure Material	Loss Tangent (wood)
Triple Flat	NA	200MHz -6GHz; Er = 3-5, Loss Tangent = ≤ 0.05	280x175x175	2mm +/- 0.2mm	Wood	< 0.05
SAM	NA	300MHz -6GHz; Er = < 5, Loss Tangent = ≤ 0.05	Human Model			
Oval Flat	✓	300MHz -6GHz; Er = 4+/- 1, Loss Tangent = ≤ 0.05	600x400x190			

8.3 Description of Simulated Tissue

The sugar based simulate tissue is produced by placing the correct measured amount of De-ionized water into a large container. Each of the dried ingredients are weighed and added to the water carefully to avoid clumping. If the solution has a high sugar concentration the water is pre-heated to aid in dissolving the ingredients.

The simulated tissue mixture was mixed based on the Simulated Tissue Composition indicated in Table 10. During the daily testing of this product, the applicable mixture was used to measure the Di-electric parameters at each of the tested frequencies to verify that the Di-electric parameters were within the tolerance of the tissue specifications.

Simulated Tissue Composition (percent by mass)

Table 10

Ingredients	450MHz	
	Head	Body
Sugar	56.0	46.5
Diacetin	0	0
De ionized – Water	39.10	50.53
Salt	3.80	1.87
HEC	1.0	1.0
Bact.	0.1	0.1

9.0 Additional Test Equipment

The Table below lists additional test equipment used during the SAR assessment.

Table 11

Equipment Type	Model Number	Serial Number	Calibration Date	Calibration Due Date
SPEAG PROBE	ES3DV3	3122	04/18/2018	04/18/2019
SPEAG PROBE	EX3DV4	7486	03/20/2018	03/20/2019
SPEAG DAE	DAE4	850	03/07/2018	03/07/2019
SPEAG DAE	DAE4	1488	03/09/2018	03/09/2019
AMPLIFIER	10W1000C	312859	CNR	CNR
BI-DIRECTIONAL COUPLER	3020A	40295	09/04/2017	09/04/2018
POWER SENSOR	E8481B	MY41091170	04/23/2018	04/23/2019
POWER SENSOR	E9301B	MY55210006	11/12/2017	11/12/2018
POWER SENSOR	E9301B	MY55210003	09/29/2017	09/29/2018
POWER METER	E4418B	MY45100532	11/01/2017	11/01/2018
POWER METER	E4418B	MY45107917	05/22/2017	05/22/2019
POWER METER	E4416A	MY50001037	05/22/2017	05/22/2019
VECTOR SIGNAL GENERATOR	E4438C	MY42081753	03/27/2018	03/27/2019
THERMOMETER	HH806AU	080307	11/30/2017	11/30/2018
THERMOMETER	HH202A	35881	12/13/2017	12/13/2018
TEMPERATURE PROBE	80PK-22	06032017	03/07/2018	03/07/2019
TEMPERATURE PROBE	80PK-22	05032017	03/07/2018	03/07/2019
TEMPERATURE & HUMIDITY LOGGER*	TM320	06153216	08/11/2017	08/11/2018
NETWORK ANALYZER	E5071B	MY42403218	08/24/2017	08/24/2018
DIELECTRIC ASSESSMENT KIT	DAK-12	1069	01/09/2018	01/09/2019
SPEAG DIPOLE	D450V3	1054	10/25/2017	10/25/2019

Note: *Equipment used for SAR assessment before calibration due date

10.0 SAR Measurement System Validation and Verification

DASY output files of the probe/dipole calibration certificates and system verification test results are included in appendices B, C & D respectively.

10.1 System Validation

The SAR measurement system was validated according to procedures in KDB 865664. The validation status summary Table is below.

Table 12

Dates	Probe Calibration Point		Probe SN	Measured Tissue Parameters		Validation		
				σ	ϵ_r	Sensitivity	Linearity	Isotropy
CW								
04/29/2018	Body	450	3122	0.88	55.5	Pass	Pass	Pass
04/29/2018	Head	450		0.87	42.3	Pass	Pass	Pass
04/17/2018	Body	450	7486	0.94	58.4	Pass	Pass	Pass
04/17/2018	Head	450		0.91	42.6	Pass	Pass	Pass

10.2 System Verification

System verification checks were conducted each day during the SAR assessment. The results are normalized to 1W. Appendix D includes DASY plots for each day during the SAR assessment. The Table below summarizes the daily system check results used for the SAR assessment.

Table 13

Probe Serial #	Tissue Type	Dipole Kit / Serial #	Ref SAR @ 1W (W/kg)	System Check Results Measured (W/kg)	System Check Test Results when normalized to 1W (W/kg)	Tested Date
3122	FCC Body	SPEAG D450V3 / 1054	4.57 +/- 10%	1.16	4.64	07/24/2018#
				1.15	4.60	07/25/2018#
	IEEE/IEC Head		4.48 +/- 10%	1.17	4.68	07/26/2018
				1.15	4.60	07/27/2018
7486	FCC Body		4.57 +/- 10%	1.15	4.60	08/02/2018#
				1.18	4.72	08/03/2018#

Note: # System verification covered next test day (within 24 hours)

10.3 Equivalent Tissue Test Results

Simulated tissue prepared for SAR measurements is measured daily and within 24 hours prior to actual SAR testing to verify that the tissue is within +/- 5% of target parameters at the center of the transmit band. This measurement is done using the applicable equipment indicated in section 9.0. The Table below summarizes the measured tissue parameters used for the SAR assessment.

Table 14

Frequency (MHz)	Tissue Type	Conductivity Target (S/m)	Dielectric Constant Target	Conductivity Meas. (S/m)	Dielectric Constant Meas.	Tested Date
450	FCC Body	0.94 (0.89-0.99)	56.70 (53.90-59.50)	0.93	54.7	07/24/2018#
				0.90	54.2	07/25/2018#
				0.95	55.3	08/02/2018#
				0.95	55.2	08/03/2018#
	IEEE/IEC Head	0.87 (0.83-0.91)	43.5 (41.30-45.70)	0.90	42.1	07/26/2018
				0.89	41.9	07/27/2018
463	FCC Body	0.94 (0.89-0.99)	56.60 (53.80-59.50)	0.94	54.6	07/24/2018#
				0.97	55.2	08/02/2018#
				0.96	55.1	08/03/2018#
	IEEE/IEC Head	0.87 (0.83-0.91)	43.4 (41.30-45.60)	0.91	41.8	07/26/2018
				0.90	41.6	07/27/2018
468	FCC Body	0.94 (0.89-0.99)	56.60 (53.80-59.50)	0.94	54.5	07/24/2018#
				0.92	54.0	07/25/2018#
				0.96	55.0	08/03/2018
	IEEE/IEC Head	0.87 (0.83-0.91)	43.4 (41.20-45.60)	0.91	41.7	07/26/2018

Note: # tissue date covered for next test day (within 24 hours)

11.0 Environmental Test Conditions

The EME Laboratory's ambient environment is well controlled resulting in very stable simulated tissue temperature and therefore stable dielectric properties. Simulated tissue temperature is measured prior to each scan to insure it is within $\pm 2^{\circ}\text{C}$ of the temperature at which the dielectric properties were determined. The liquid depth within the phantom used for measurements was at least 15cm. Additional precautions are routinely taken to ensure the stability of the simulated tissue such as covering the phantoms when scans are not actively in process in order to minimize evaporation. The lab environment is continuously monitored. The Table below presents the range and average environmental conditions during the SAR tests reported herein:

Table 15

	Target	Measured
Ambient Temperature	18 - 25 °C	Range: 20.4 - 23.3°C Avg. 22.0 °C
Tissue Temperature	18 - 25 °C	Range: 19.9 - 22.6°C Avg. 21.3°C

Relative humidity target range is a recommended target

The EME Lab RF environment uses a Spectrum Analyzer to monitor for extraneous large signal RF contaminants that could possibly affect the test results. If such unwanted signals are discovered the SAR scans are repeated.

12.0 DUT Test Setup and Methodology

12.1 Measurements

SAR measurements were performed using the DASY system described in section 8.0 using zoom scans. Oval flat phantoms filled with applicable simulated tissue were used for body and face testing.

The Table below includes the step sizes and resolution of area and zoom scans per KDB 865664 requirements.

Table 16

Description		≤ 3 GHz	> 3 GHz
Maximum distance from closest measurement point (geometric center of probe sensors) to phantom surface		5 ± 1 mm	$\frac{1}{2} \cdot \delta \cdot \ln(2) \pm 0.5$ mm
Maximum probe angle from probe axis to phantom surface normal at the measurement location		$30^\circ \pm 1^\circ$	$20^\circ \pm 1^\circ$
Maximum area scan spatial resolution: Δx_{Area} , Δy_{Area}		≤ 2 GHz: ≤ 15 mm 2 – 3 GHz: ≤ 12 mm	3 – 4 GHz: ≤ 12 mm 4 – 6 GHz: ≤ 10 mm
		When the x or y dimension of the test device, in the measurement plane orientation, is smaller than the above, the measurement resolution must be \leq the corresponding x or y dimension of the test device with at least one measurement point on the test device.	
Maximum zoom scan spatial resolution: Δx_{Zoom} , Δy_{Zoom}		≤ 2 GHz: ≤ 8 mm 2 – 3 GHz: ≤ 5 mm*	3 – 4 GHz: ≤ 5 mm* 4 – 6 GHz: ≤ 4 mm*
Maximum zoom scan spatial resolution, normal to phantom surface	uniform grid: $\Delta z_{Zoom}(n)$	≤ 5 mm	3 – 4 GHz: ≤ 4 mm 4 – 5 GHz: ≤ 3 mm 5 – 6 GHz: ≤ 2 mm
Note: δ is the penetration depth of a plane-wave at normal incidence to the tissue medium; see draft standard IEEE P1528-2011 for details. * When zoom scan is required and the reported SAR from the area scan based 1-g SAR estimation procedures of KDB 447498 is ≤ 1.4 W/kg, ≤ 8 mm, ≤ 7 mm and ≤ 5 mm zoom scan resolution may be applied, respectively, for 2 GHz to 3 GHz, 3 GHz to 4 GHz and 4 GHz to 6 GHz.			

12.2 DUT Configuration(s)

The DUT is a portable device operational at the body and face as described in section 6.0 while using the applicable accessories listed in section 7.0. All accessories listed in section 7.0 of this report were considered.

12.3 DUT Positioning Procedures

The positioning of the device for each body location is described below and illustrated in Appendix H.

12.3.1 Body

The DUT was positioned in normal use configuration against the phantom with the offered body worn accessory as well as with the offered audio accessories as applicable.

12.3.2 Head

Not applicable.

12.3.3 Face

The DUT was positioned with its front side separated 2.5cm from the phantom.

12.4 DUT Test Channels

The number of test channels was determined by using the following IEEE 1528 equation. The use of this equation produces the same or more test channels compared to the FCC KDB 447498 number of test channels formula.

$$N_c = 2 * \text{roundup}[10 * (f_{\text{high}} - f_{\text{low}}) / f_c] + 1$$

Where

N_c = Number of channels

F_{high} = Upper channel

F_{low} = Lower channel

F_c = Center channel

12.5 SAR Result Scaling Methodology

The calculated 1-gram averaged SAR results indicated as “Max Calc. 1g-SAR” in the data Tables is determined by scaling the measured SAR to account for power leveling variations and drift. Appendix F includes a shortened scan to justify SAR scaling for drift. For this device the “Max Calc. 1g-SAR” is scaled using the following formula:

$$\text{Max_Calc} = \text{SAR_meas} \cdot 10^{\frac{-\text{Drift}}{10}} \cdot \frac{P_{\text{max}}}{P_{\text{int}}} \cdot \text{DC}$$

P_{max} = Maximum Power (W)

P_{int} = Initial Power (W)

Drift = DASY drift results (dB)

SAR_meas = Measured 1-g (W/kg)

DC = Transmission mode duty cycle in % where applicable

50% duty cycle is applied for PTT operation

Note: for conservative results, the following are applied:

If $P_{\text{int}} > P_{\text{max}}$, then $P_{\text{max}}/P_{\text{int}} = 1$.

Drift = 1 for positive drift

Additional SAR scaling was applied using the methodologies outlined in FCC KDB 865664 using tissue sensitivity values. SAR was scaled for conditions where the tissue permittivity was measured above the nominal target and for tissue conductivity that was measured below the nominal target. Negative or reduced SAR scaling is not permitted.

12.6 DUT Test Plan

The guidelines and requirements outlined in section 4.0 were used to assess compliance of this device. All modes of operation identified in section 6.0 were considered during the development of the test plan. All tests were performed in CW mode and 50% duty cycle was applied to PTT configurations in the final results.

13.0 DUT Test Data

13.1 Assessment at the Body for 462.5500 – 462.7250MHz band

Conducted power measurements for channel within FCC allocated frequency range 462.5500 - 462.7250 MHz was measured and listed in Table 17.

Table 17

Test Freq. (MHz)	Power (W)		
	AA Alkaline	KEBT-1300	PMNN4477A
462.6375	1.62	1.45	1.42

Assessment at the Body with Body worn PMLN7240A

DUT assessment with the fixed antenna, batteries and above mentioned body worn accessory. SAR plots of the highest results per Table 18 (bolded) are presented in Appendix F.

Table 18

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
EAN.144F.823RA1	AA Alkaline	PMLN7240A	53725C	462.6375	1.62	-0.84	1.25	0.94	FAZ-AB-180725-01#
EAN.144F.823RA1	KEBT-1300	PMLN7240A	53725C	462.6375	1.45	-0.35	1.05	0.78	FAZ-AB-180725-02#
EAN.144F.823RA1	PMNN4477A	PMLN7240A	53725C	462.6375	1.42	-0.72	1.12	0.93	FAZ-AB-180725-03#

Assessment at the Body with Body worn PMLN7706AR

DUT assessment with fixed antenna, batteries and above mentioned body worn accessory. SAR plots of the highest results per Table 19 (bolded) are presented in Appendix F.

Table 19

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
EAN.144F.823RA1	AA Alkaline	PMLN7706AR	53725C	462.6375	1.62	-0.75	1.14	0.84	FAZ-AB-180725-04#
EAN.144F.823RA1	KEBT-1300	PMLN7706AR	53725C	462.6375	1.45	-0.34	1.21	0.90	FAZ-AB-180725-05#
EAN.144F.823RA1	PMNN4477A	PMLN7706AR	53725C	462.6375	1.42	-0.61	0.90	0.73	FAZ-AB-180725-06#

Assessment at the Body with Body worn PMLN7220A

Table 20 below shows the DUT assessment with offered antenna, batteries and above mentioned body worn accessory. SAR plots of the highest results per Table 20 (bolded) are presented in Appendix F.

Table 20

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
EAN.144F.823RA1	AA Alkaline	PMLN7220A	53725C	462.6375	1.62	-0.83	1.29	0.96	FD-AB-180803-01#
EAN.144F.823RA1	KEBT-1300	PMLN7220A	53725C	462.6375	1.45	-0.52	1.26	0.98	FD-AB-180803-02#
EAN.144F.823RA1	PMNN4477A	PMLN7220A	53725C	462.6375	1.42	-0.58	1.21	0.97	FD-AB-180803-03#

Assessment at the Body with other audio accessories

Assessment per “KDB 643646 Body SAR Test consideration for Audio Accessories without Built-in Antenna” (adapting SAR thresholds to general population limits). SAR plots of the highest results per Table 20 (bolded) are presented in Appendix F.

Table 21

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
EAN.144F.823RA1	KEBT-1300	PMLN7220A	56320B	462.6375	1.45	-0.44	1.21	0.92	FD-AB-180803-06
EAN.144F.823RA1	KEBT-1300	PMLN7220A	GU6443A (1518)	462.6375	1.45	-0.63	1.31	1.04	FD-AB-180803-07
EAN.144F.823RA1	KEBT-1300	PMLN7220A	PMLN7705AR	462.6375	1.45	-0.36	1.15	0.86	FD-AB-180803-08
EAN.144F.823RA1	KEBT-1300	PMLN7220A	53727B	462.6375	1.45	-0.32	1.28	0.95	FD-AB-180803-09
EAN.144F.823RA1	KEBT-1300	PMLN7220A	53724C	462.6375	1.45	-0.55	1.20	0.94	FD-AB-180803-10

13.2 Assessment at the Face for 462.5500 – 462.7250MHz band

Conducted power measurements for channel within FCC allocated frequency range 462.5500 - 462.7250 MHz was measured and listed in Table 22.

Table 22

Test Freq. (MHz)	Power (W)		
	AA Alkaline	KEBT-1300	PMNN4477A
462.6375	1.62	1.45	1.42

Assessment of fix antenna with offered batteries with front of DUT positioned 2.5cm facing phantom was performed. SAR plots of the highest results per Table 23 (bolded) are presented in Appendix F.

Table 23

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
EAN.144F.823RA1	AA Alkaline	None, Radio @ Front	None	462.6375	1.62	-0.88	1.18	0.89	ZZ-FACE-180726-06
EAN.144F.823RA1	KEBT-1300	None, Radio @ Front	None	462.6375	1.43	-0.32	1.25	0.94	ZZ-FACE-180727-09
EAN.144F.823RA1	PMNN4477A	None, Radio @ Front	None	462.6375	1.42	-0.38	1.16	0.89	ZZ-FACE-180726-08

13.3 Assessment at the Body for 467.5625 – 467.7125MHz band

Conducted power measurements for channel within FCC allocated frequency range 467.5625-467.7125 MHz was measured and listed in Table 24.

Table 24

Test Freq. (MHz)	Power (W)		
	AA Alkaline	KEBT-1300	PMNN4477A
467.6375	0.43	0.33	0.33

Assessment at the Body with Body worn PMLN7240A

DUT assessment with the fixed antenna, batteries and above mentioned body worn accessory. SAR plots of the highest results per Table 25 (bolded) are presented in Appendix F.

Table 25

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
EAN.144F.823RA1	AA Alkaline	PMLN7240A	53725C	467.6375	0.43	-0.68	0.69	0.48	ZZ-AB-180725-07#
EAN.144F.823RA1	KEBT-1300	PMLN7240A	53725C	467.6375	0.33	-0.42	0.55	0.47	ZZ-AB-180725-09#
EAN.144F.823RA1	PMNN4477A	PMLN7240A	53725C	467.6375	0.33	-0.60	0.53	0.47	ZZ-AB-180725-10#

Assessment at the Body with Body worn PMLN7706AR

DUT assessment with fixed antenna, batteries and above mentioned body worn accessory. SAR plots of the highest results per Table 26 (bolded) are presented in Appendix F.

Table 26

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
EAN.144F.823RA1	AA Alkaline	PMLN7706AR	53725C	467.6375	0.43	-0.69	0.60	0.41	LOH-AB-180726-01#
EAN.144F.823RA1	KEBT-1300	PMLN7706AR	53725C	467.6375	0.33	-0.56	0.50	0.44	LOH-AB-180726-02#
EAN.144F.823RA1	PMNN4477A	PMLN7706AR	53725C	467.6375	0.33	-0.27	0.36	0.29	LOH-AB-180726-03#

Assessment at the Body with Body worn PMLN7220A

DUT assessment with fixed antenna, default battery and above mentioned body worn accessory. SAR plots of the highest results per Table 27 (bolded) are presented in Appendix F.

Table 27

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
EAN.144F.823RA1	AA Alkaline	PMLN7220A	53725C	467.6375	0.43	-0.67	0.65	0.45	AN-AB-180803-11
EAN.144F.823RA1	KEBT-1300	PMLN7220A	53725C	467.6375	0.34	-0.39	0.66	0.54	AM-AB-180805-06
EAN.144F.823RA1	PMNN4477A	PMLN7220A	53725C	467.6375	0.33	-0.32	0.48	0.39	AN-AB-180803-13

Assessment at the Body with other audio accessories

By adapting SAR thresholds to general population limits per “KDB 643646 Body SAR Test Consideration for Audio Accessories without Built-In Antenna”, SAR testing with other audio accessories was deemed not necessary as previous results in Tables 25, 26 & 27 shows highest result of < 0.8 W/kg, which is more than 3dB from the specification limit.

13.4 Assessment at the Face for 467.5625 – 467.7125MHz band

Conducted power measurements for channel within FCC allocated frequency range 467.5625-467.7125 MHz was measured and listed in Table 28.

Table 28

Test Freq. (MHz)	Power (W)		
	AA Alkaline	KEBT-1300	PMNN4477A
467.6375	0.43	0.33	0.33

Assessment with the fixed antenna and default battery with front of DUT positioned 2.5cm facing phantom. SAR plots of the highest results per Table 29 (bolded) are presented in Appendix F.

Table 29

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
EAN.144F.823RA1	AA Alkaline	None	None	467.6375	0.43	-0.66	0.65	0.44	ZZ-FACE-180726-09
EAN.144F.823RA1	KEBT-1300	None	None	467.6375	0.33	-0.33	0.56	0.35	ZZ-FACE-180726-10
EAN.144F.823RA1	PMNN4477A	None	None	467.6375	0.33	-0.62	0.57	0.50	ZZ-FACE-180726-11

13.5 Shortened Scan Assessment

A “shortened” scan using the highest SAR configuration overall from above was performed to validate the SAR drift of the full DASY5™ coarse and zoom scans. Note that the shortened scan represents the zoom scan performance result; this is obtained by first running a coarse scan to find the peak area and then, using a newly charged battery, a zoom scan was performed. The results of the shortened cube scan presented in Appendix G demonstrate that the scaling methodology used to determine the calculated SAR results presented herein are valid. The SAR result from the Table below is provided in Appendix F.

Table 30

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
EAN.144F.823RA1	KEBT-1300	PMLN7220A	GU6443A (1518)	462.6375	1.45	-0.44	1.35	1.03	AN-AB-180804-01#

14.0 Results Summary

Based on the test guidelines from section 4.0 and satisfying frequencies within FCC bands and ISED Canada Frequency Bands, the highest Operational Maximum Calculated 1-gram average SAR values found for this filing:

Table 31

Technologies	Frequency band (MHz)	Max Calc at Body (W/kg)	Max Calc at Face (W/kg)
		1g-SAR	1g-SAR
FCC US & ISED Canada			
FM	462.5500 – 462.7250	1.04	0.94
FM	467.5625 – 467.7125	0.54	0.50

All results are scaled to the maximum output power.

15.0 Variability Assessment

Per the guidelines in KDB 865664, SAR variability assessment is not required because measured SAR with PTT duty factor of 50% is below 0.8W/kg (General Population).

16.0 System Uncertainty

A system uncertainty analysis is not required for this report per KDB 865664 because the highest report SAR value for General Population exposure is less than 1.5W/kg.

Per the guidelines of ISO17025 a reported system uncertainty is required and therefore measurement uncertainty budget is included in Appendix A.

Appendix A

Measurement Uncertainty Budget

Table A.1: Uncertainty Budget for Device Under Test for 450 MHz

<i>a</i>	<i>b</i>	<i>c</i>	<i>d</i>	<i>e = f(d,k)</i>	<i>f</i>	<i>g</i>	<i>h = c x f / e</i>	<i>i = c x g / e</i>	<i>k</i>
Uncertainty Component	IEEE 1528 section	Tol. (± %)	Prob Dist	Div.	ci (1 g)	ci (10 g)	1 g u _i (±%)	10 g u _i (±%)	v _i
Measurement System									
Probe Calibration	E.2.1	6.7	N	1.00	1	1	6.7	6.7	∞
Axial Isotropy	E.2.2	4.7	R	1.73	0.707	0.707	1.9	1.9	∞
Hemispherical Isotropy	E.2.2	9.6	R	1.73	0.707	0.707	3.9	3.9	∞
Boundary Effect	E.2.3	1.0	R	1.73	1	1	0.6	0.6	∞
Linearity	E.2.4	4.7	R	1.73	1	1	2.7	2.7	∞
System Detection Limits	E.2.5	1.0	R	1.73	1	1	0.6	0.6	∞
Readout Electronics	E.2.6	0.3	N	1.00	1	1	0.3	0.3	∞
Response Time	E.2.7	1.1	R	1.73	1	1	0.6	0.6	∞
Integration Time	E.2.8	1.1	R	1.73	1	1	0.6	0.6	∞
RF Ambient Conditions - Noise	E.6.1	3.0	R	1.73	1	1	1.7	1.7	∞
RF Ambient Conditions - Reflections	E.6.1	0.0	R	1.73	1	1	0.0	0.0	∞
Probe Positioner Mech. Tolerance	E.6.2	0.4	R	1.73	1	1	0.2	0.2	∞
Probe Positioning w.r.t Phantom	E.6.3	1.4	R	1.73	1	1	0.8	0.8	∞
Max. SAR Evaluation (ext., int., avg.)	E.5	3.4	R	1.73	1	1	2.0	2.0	∞
Test sample Related									
Test Sample Positioning	E.4.2	3.2	N	1.00	1	1	3.2	3.2	29
Device Holder Uncertainty	E.4.1	4.0	N	1.00	1	1	4.0	4.0	8
SAR drift	6.6.2	5.0	R	1.73	1	1	2.9	2.9	∞
Phantom and Tissue Parameters									
Phantom Uncertainty	E.3.1	4.0	R	1.73	1	1	2.3	2.3	∞
Liquid Conductivity (target)	E.3.2	5.0	R	1.73	0.64	0.43	1.8	1.2	∞
Liquid Conductivity (measurement)	E.3.3	3.3	N	1.00	0.64	0.43	2.1	1.4	∞
Liquid Permittivity (target)	E.3.2	5.0	R	1.73	0.6	0.49	1.7	1.4	∞
Liquid Permittivity (measurement)	E.3.3	1.9	N	1.00	0.6	0.49	1.1	0.9	∞
Combined Standard Uncertainty			RSS				11	11	477
Expanded Uncertainty (95% CONFIDENCE LEVEL)			k=2				23	22	

Notes for uncertainty budget Tables:

a) Column headings *a-k* are given for reference.

b) Tol. - Tolerance in influence quantity.

c) Prob. Dist. – Probability distribution

d) N, R - normal, rectangular probability distributions

e) Div. - divisor used to translate tolerance into normally distributed standard uncertainty

f) *ci* - sensitivity coefficient that should be applied to convert the variability of the uncertainty component into a variability of SAR.g) *ui* – SAR uncertainty

h) ν_i - degrees of freedom for standard uncertainty and effective degrees of freedom for the expanded uncertainty

Table A.2: Uncertainty Budget for System Validation (dipole & flat phantom) for 450 MHz

<i>a</i>	<i>b</i>	<i>c</i>	<i>d</i>	<i>e = f(d,k)</i>	<i>f</i>	<i>g</i>	<i>h = c x f / e</i>	<i>i = c x g / e</i>	<i>k</i>
Uncertainty Component	IEEE 1528 section	Tol. (± %)	Prob Dist	Div.	<i>c_i</i> (1 g)	<i>c_i</i> (10 g)	1 g <i>U_i</i> (±%)	10 g <i>U_i</i> (±%)	ν_i
Measurement System									
Probe Calibration	E.2.1	6.7	N	1.00	1	1	6.7	6.7	∞
Axial Isotropy	E.2.2	4.7	R	1.73	1	1	2.7	2.7	∞
Spherical Isotropy	E.2.2	9.6	R	1.73	0	0	0.0	0.0	∞
Boundary Effect	E.2.3	1.0	R	1.73	1	1	0.6	0.6	∞
Linearity	E.2.4	4.7	R	1.73	1	1	2.7	2.7	∞
System Detection Limits	E.2.5	1.0	R	1.73	1	1	0.6	0.6	∞
Readout Electronics	E.2.6	0.3	N	1.00	1	1	0.3	0.3	∞
Response Time	E.2.7	1.1	R	1.73	1	1	0.6	0.6	∞
Integration Time	E.2.8	0.0	R	1.73	1	1	0.0	0.0	∞
RF Ambient Conditions - Noise	E.6.1	3.0	R	1.73	1	1	1.7	1.7	∞
RF Ambient Conditions - Reflections	E.6.1	0.0	R	1.73	1	1	0.0	0.0	∞
Probe Positioner Mechanical Tolerance	E.6.2	0.4	R	1.73	1	1	0.2	0.2	∞
Probe Positioning w.r.t. Phantom	E.6.3	1.4	R	1.73	1	1	0.8	0.8	∞
Max. SAR Evaluation (ext., int., avg.)	E.5	3.4	R	1.73	1	1	2.0	2.0	∞
Dipole									
Dipole Axis to Liquid Distance	8, E.4.2	2.0	R	1.73	1	1	1.2	1.2	∞
Input Power and SAR Drift Measurement	8, 6.6.2	5.0	R	1.73	1	1	2.9	2.9	∞
Phantom and Tissue Parameters									
Phantom Uncertainty	E.3.1	4.0	R	1.73	1	1	2.3	2.3	∞
Liquid Conductivity (target)	E.3.2	5.0	R	1.73	0.64	0.43	1.8	1.2	∞
Liquid Conductivity (measurement)	E.3.3	3.3	R	1.73	0.64	0.43	1.2	0.8	∞
Liquid Permittivity (target)	E.3.2	5.0	R	1.73	0.6	0.49	1.7	1.4	∞
Liquid Permittivity (measurement)	E.3.3	1.9	R	1.73	0.6	0.49	0.6	0.5	∞
Combined Standard Uncertainty			RSS				10	9	99999
Expanded Uncertainty (95% CONFIDENCE LEVEL)			<i>k</i> =2				19	18	

Notes for uncertainty budget Tables:

a) Column headings *a-k* are given for reference.

b) Tol. - Tolerance in influence quantity.

c) Prob. Dist. – Probability distribution

d) N, R - normal, rectangular probability distributions

e) Div. - divisor used to translate tolerance into normally distributed standard uncertainty

f) *c_i* - sensitivity coefficient that should be applied to convert the variability of the uncertainty component into a variability of SAR.

g) *u_i* – SAR uncertainty

h) ν_i - degrees of freedom for standard uncertainty and effective degrees of freedom for the expanded uncertainty

Appendix B

Probe Calibration Certificates

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Motorola Solutions MY**

Certificate No: **EX3-7486_Mar18/2**

CALIBRATION CERTIFICATE (Replacement of No:EX3-7486_Mar18)

Object **EX3DV4 - SN:7486**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v4, QA CAL-23.v5,
QA CAL-25.v6
Calibration procedure for dosimetric E-field probes**

Calibration date: **March 20, 2018**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^{\circ}\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-17 (No. 217-02521/02522)	Apr-18
Power sensor NRP-Z91	SN: 103244	04-Apr-17 (No. 217-02521)	Apr-18
Power sensor NRP-Z91	SN: 103245	04-Apr-17 (No. 217-02525)	Apr-18
Reference 20 dB Attenuator	SN: S5277 (20x)	07-Apr-17 (No. 217-02528)	Apr-18
Reference Probe ES3DV2	SN: 3013	30-Dec-17 (No. ES3-3013_Dec17)	Dec-18
DAE4	SN: 660	21-Dec-17 (No. DAE4-660_Dec17)	Dec-18
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (in house check Jun-16)	In house check: Jun-18
Power sensor E4412A	SN: MY41498087	06-Apr-16 (in house check Jun-16)	In house check: Jun-18
Power sensor E4412A	SN: 000110210	06-Apr-16 (in house check Jun-16)	In house check: Jun-18
RF generator HP 8648C	SN: US3842U01700	04-Aug-99 (in house check Jun-16)	In house check: Jun-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-17)	In house check: Oct-18

Calibrated by:	Name	Function	Signature
	Jeton Kastrati	Laboratory Technician	
Approved by:	Name	Function	Signature
	Katja Pokovic	Technical Manager	

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Issued: April 13, 2018

Certificate No: EX3-7486_Mar18/2

Page 1 of 16

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization ϕ	ϕ rotation around probe axis
Polarization ϑ	ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}**: Assessed for E-field polarization $\vartheta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)_{x,y,z} = NORM_{x,y,z} * frequency_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP_{x,y,z}**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A_{x,y,z}; B_{x,y,z}; C_{x,y,z}; D_{x,y,z}; VR_{x,y,z}; A, B, C, D** are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM_x (no uncertainty required).

EX3DV4 – SN:7486

March 20, 2018

Probe EX3DV4

SN:7486

Manufactured: March 20, 2017
Calibrated: March 20, 2018

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

Certificate No: EX3-7486_Mar18/2

Page 3 of 16

EX3DV4- SN:7486

March 20, 2018

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7486

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ($\mu\text{V}/(\text{V}/\text{m})^2$) ^A	0.37	0.47	0.49	$\pm 10.1\%$
DCP (mV) ^B	101.3	90.8	100.1	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Unc ^E (k=2)
0	CW	X	0.0	0.0	1.0	0.00	134.1	$\pm 3.0\%$
		Y	0.0	0.0	1.0		129.8	
		Z	0.0	0.0	1.0		135.9	

Note: For details on UID parameters see Appendix.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X,Y,Z do not affect the E^2 -field uncertainty inside TSL (see Pages 5 and 6).

^B Numerical linearization parameter: uncertainty not required.

^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4-- SN:7486

March 20, 2018

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7486

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^f	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ^g	Depth ^g (mm)	Unc (k=2)
150	52.3	0.76	13.66	13.66	13.66	0.00	1.00	± 13.3 %
300	45.3	0.87	12.30	12.30	12.30	0.08	1.20	± 13.3 %
450	43.5	0.87	11.43	11.43	11.43	0.14	1.30	± 13.3 %
750	41.9	0.89	10.72	10.72	10.72	0.34	0.99	± 12.0 %
835	41.5	0.90	10.29	10.29	10.29	0.44	0.80	± 12.0 %
900	41.5	0.97	10.11	10.11	10.11	0.24	1.21	± 12.0 %
1450	40.5	1.20	9.06	9.06	9.06	0.36	0.80	± 12.0 %
1810	40.0	1.40	8.66	8.66	8.66	0.40	0.80	± 12.0 %
1900	40.0	1.40	8.32	8.32	8.32	0.28	0.85	± 12.0 %
2100	39.8	1.49	8.67	8.67	8.67	0.33	0.85	± 12.0 %
2300	39.5	1.67	8.06	8.06	8.06	0.30	0.80	± 12.0 %
2450	39.2	1.80	7.72	7.72	7.72	0.36	0.87	± 12.0 %
2600	39.0	1.96	7.42	7.42	7.42	0.36	0.84	± 12.0 %
4950	36.3	4.40	5.98	5.98	5.98	0.35	1.80	± 13.1 %
5250	35.9	4.71	5.61	5.61	5.61	0.40	1.80	± 13.1 %
5500	35.6	4.96	5.15	5.15	5.15	0.40	1.80	± 13.1 %
5600	35.5	5.07	4.93	4.93	4.93	0.40	1.80	± 13.1 %
5750	35.4	5.22	5.13	5.13	5.13	0.40	1.80	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^f At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^g Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:7486

March 20, 2018

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7486

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^f	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ^g	Depth ^g (mm)	Unc (k=2)
150	61.9	0.80	13.10	13.10	13.10	0.00	1.00	± 13.3 %
300	58.2	0.92	12.07	12.07	12.07	0.05	1.20	± 13.3 %
450	56.7	0.94	11.68	11.68	11.68	0.09	1.30	± 13.3 %
750	55.5	0.96	10.35	10.35	10.35	0.55	0.80	± 12.0 %
835	55.2	0.97	9.98	9.98	9.98	0.59	0.80	± 12.0 %
900	55.0	1.05	9.94	9.94	9.94	0.41	0.91	± 12.0 %
1450	54.0	1.30	8.98	8.98	8.98	0.34	0.80	± 12.0 %
1810	53.3	1.52	8.42	8.42	8.42	0.39	0.80	± 12.0 %
1900	53.3	1.52	8.30	8.30	8.30	0.38	0.85	± 12.0 %
2100	53.2	1.62	8.60	8.60	8.60	0.34	0.89	± 12.0 %
2300	52.9	1.81	7.85	7.85	7.85	0.41	0.80	± 12.0 %
2450	52.7	1.95	7.77	7.77	7.77	0.38	0.80	± 12.0 %
2600	52.5	2.16	7.49	7.49	7.49	0.36	0.80	± 12.0 %
4950	49.4	5.01	5.16	5.16	5.16	0.45	1.90	± 13.1 %
5250	48.9	5.36	4.77	4.77	4.77	0.50	1.90	± 13.1 %
5500	48.6	5.65	4.27	4.27	4.27	0.50	1.90	± 13.1 %
5600	48.5	5.77	4.11	4.11	4.11	0.50	1.90	± 13.1 %
5750	48.3	5.94	4.27	4.27	4.27	0.50	1.90	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^f At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.


^g Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:7486

March 20, 2018

Frequency Response of E-Field



(TEM-Cell:ifi110 EXX, Waveguide: R22)

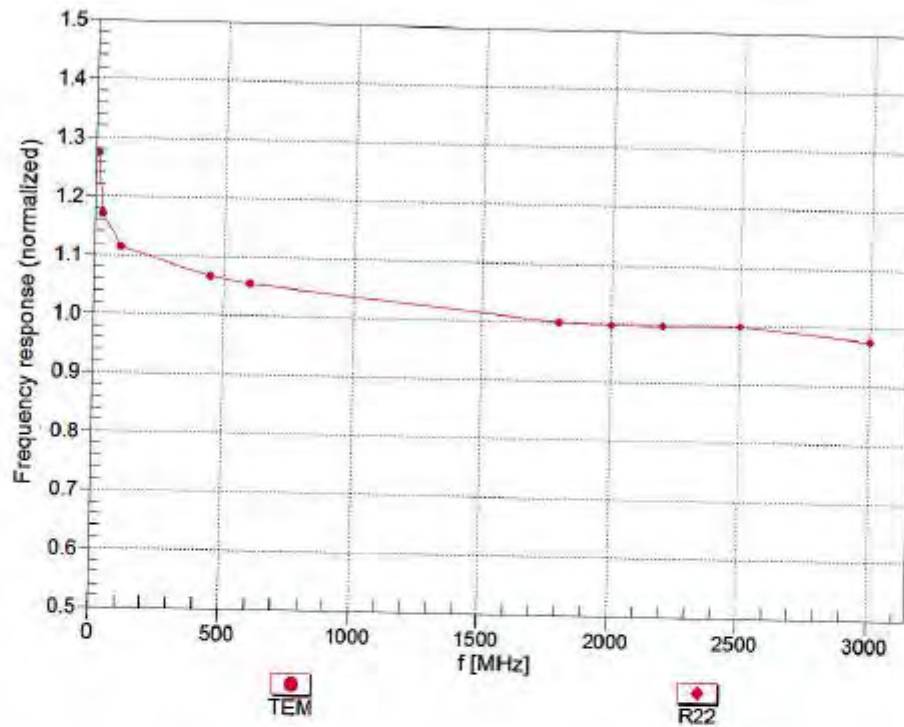

Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ ($k=2$)

EX3DV4- SN:7486



March 20, 2018

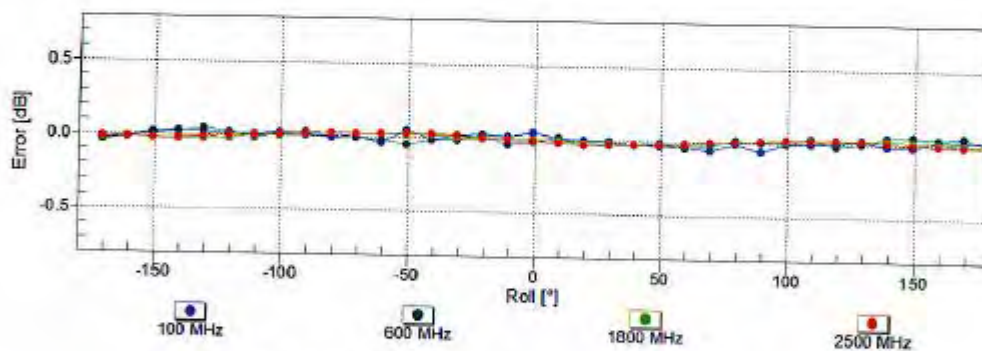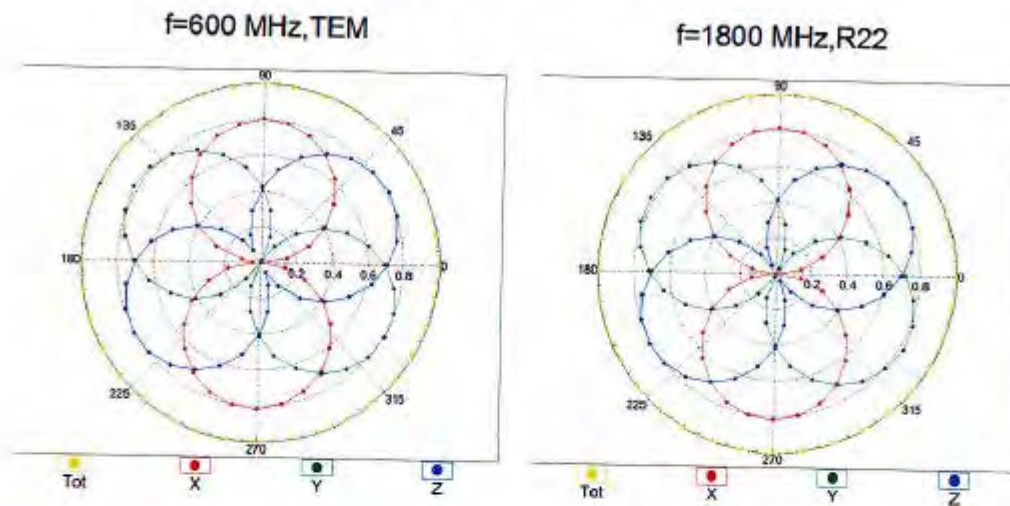Receiving Pattern (ϕ), $\vartheta = 0^\circ$ **Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)**

EX3DV4- SN:7486

March 20, 2018

Dynamic Range f(SAR_{head})
(TEM cell , f_{eval}= 1900 MHz)

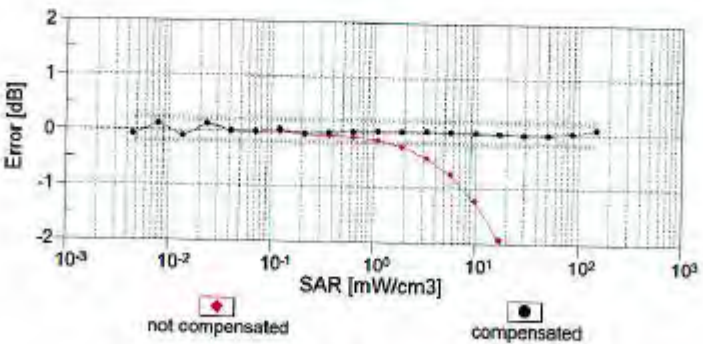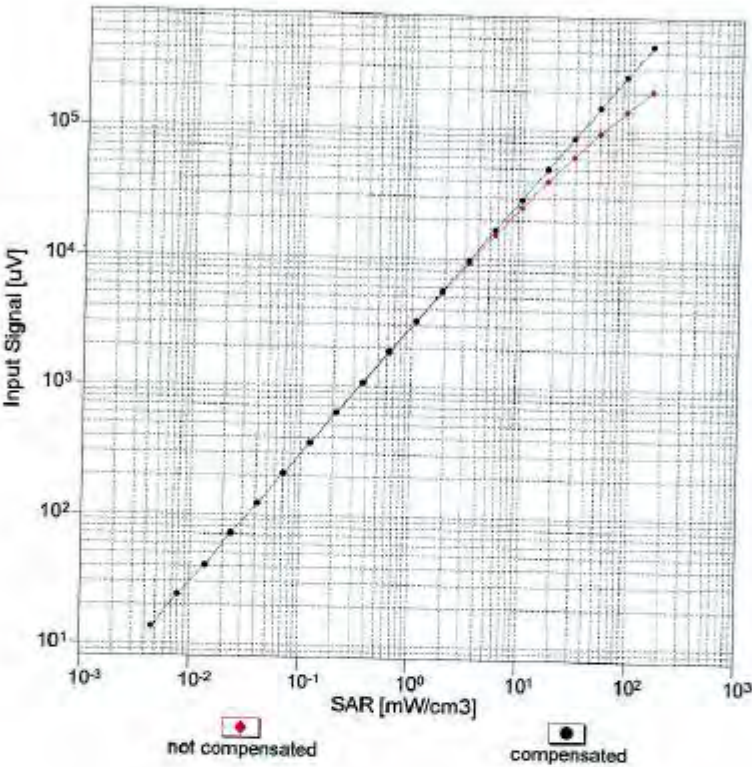


Uncertainty of Linearity Assessment: ± 0.6% (k=2)


EX3DV4- SN:7486

March 20, 2018

Conversion Factor Assessment

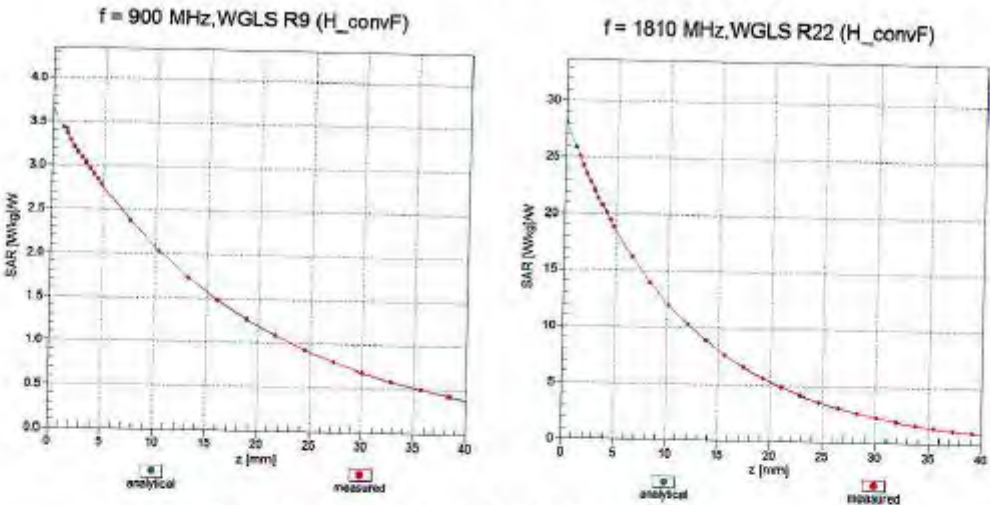

Deviation from Isotropy in Liquid
Error (ϕ, θ), $f = 900 \text{ MHz}$

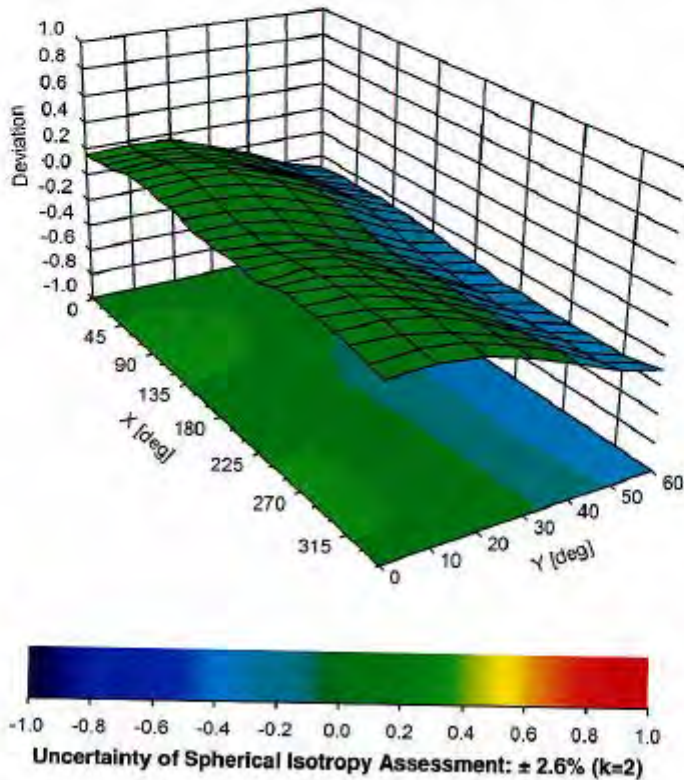

EX3DV4-- SN:7486

March 20, 2018

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7486**Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	19.1
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

EX3DV4- SN:7486

March 20, 2018

Appendix: Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu V}$	C	D dB	VR mV	Unc ^E (k=2)
0	CW	X	0.0	0.0	1.0	0.00	134.1	$\pm 3.0\%$
		Y	0.0	0.0	1.0		129.8	
		Z	0.0	0.0	1.0		135.9	
10021-DAC	GSM-FDD (TDMA, GMSK)	X	1.23	59.7	9.5	9.39	79.8	$\pm 1.9\%$
		Y	1.64	64.6	12.9		66.6	
		Z	1.58	63.0	11.5		93.7	
10023-DAC	GPRS-FDD (TDMA, GMSK, TN 0)	X	1.31	60.4	9.9	9.57	77.2	$\pm 1.9\%$
		Y	1.71	65.2	13.1		64.2	
		Z	1.56	62.3	11.3		90.7	
10024-DAC	GPRS-FDD (TDMA, GMSK, TN 0-1)	X	1.32	63.4	10.1	6.56	147.2	$\pm 2.2\%$
		Y	3.32	76.5	16.6		132.6	
		Z	1.43	64.4	11.2		144.8	
10025-DAC	EDGE-FDD (TDMA, 8PSK, TN 0)	X	4.76	70.7	24.3	12.62	56.7	$\pm 1.7\%$
		Y	4.37	68.2	23.8		47.2	
		Z	5.41	74.8	27.1		66.8	
10026-DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1)	X	4.29	70.7	22.6	9.55	116.8	$\pm 1.7\%$
		Y	3.95	68.2	21.8		96.1	
		Z	4.86	73.8	24.5		138.6	
10027-DAC	GPRS-FDD (TDMA, GMSK, TN 0-1-2)	X	0.96	62.2	8.9	4.80	135.3	$\pm 1.9\%$
		Y	1.12	65.3	11.3		141.0	
		Z	1.05	62.3	8.7		139.1	
10028-DAC	GPRS-FDD (TDMA, GMSK, TN 0-1-2-3)	X	0.53	58.4	6.0	3.55	131.7	$\pm 1.7\%$
		Y	0.86	63.5	9.5		144.8	
		Z	38.88	97.7	19.9		135.9	
10029-DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1-2)	X	4.31	72.6	22.6	7.78	146.7	$\pm 1.7\%$
		Y	4.25	72.0	23.1		136.1	
		Z	4.88	75.6	24.5		136.8	
10039-CAB	CDMA2000 (1xRTT, RC1)	X	4.48	66.3	18.5	4.57	141.8	$\pm 0.9\%$
		Y	4.50	65.6	18.5		138.4	
		Z	4.67	67.2	19.2		145.8	
10056-CAA	UMTS-TDD (TD-SCDMA, 1.28 Mcps)	X	3.77	67.7	22.6	11.01	82.1	$\pm 1.4\%$
		Y	3.60	66.5	22.7		68.6	
		Z	4.07	69.7	24.1		97.1	
10058-DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1-2-3)	X	4.28	73.6	22.5	6.52	149.5	$\pm 1.7\%$
		Y	3.98	71.2	21.9		142.7	
		Z	4.54	74.9	23.5		134.9	
10081-CAB	CDMA2000 (1xRTT, RC3)	X	3.87	66.3	18.4	3.97	138.9	$\pm 0.7\%$
		Y	3.84	65.5	18.4		135.4	
		Z	3.99	67.0	19.0		142.5	
10090-DAC	GPRS-FDD (TDMA, GMSK, TN 0-4)	X	1.19	61.8	8.9	6.56	145.6	$\pm 1.9\%$
		Y	1.75	67.1	11.8		131.7	
		Z	1.37	63.4	10.2		143.5	

EX3DV4- SN:7486

March 20, 2018

10099-DAC	EDGE-FDD (TDMA, 8PSK, TN 0-4)	X	4.71	73.7	24.3	9.55	114.9	±2.7 %
		Y	4.59	72.7	24.5		96.4	
		Z	5.27	76.6	26.1		136.9	
10117-CAC	IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)	X	9.85	68.2	20.8	8.07	145.6	±3.0 %
		Y	9.82	67.8	20.9		141.9	
		Z	9.64	67.7	20.7		124.8	
10196-CAC	IEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)	X	9.44	68.1	20.8	8.10	137.7	±3.0 %
		Y	9.52	67.8	21.0		135.6	
		Z	9.63	68.5	21.3		142.3	
10290-AAB	CDMA2000, RC1, SO55, Full Rate	X	4.09	66.9	18.5	3.91	142.6	±0.7 %
		Y	4.05	66.1	18.5		139.2	
		Z	4.31	68.0	19.3		145.0	
10291-AAB	CDMA2000, RC3, SO55, Full Rate	X	3.58	67.0	18.5	3.46	138.6	±0.7 %
		Y	3.52	66.1	18.5		135.6	
		Z	3.76	68.0	19.3		142.5	
10292-AAB	CDMA2000, RC3, SO32, Full Rate	X	3.55	67.1	18.5	3.39	138.8	±0.7 %
		Y	3.45	66.0	18.3		135.3	
		Z	3.72	68.2	19.3		142.1	
10293-AAB	CDMA2000, RC3, SO3, Full Rate	X	3.59	66.8	18.4	3.50	139.1	±0.7 %
		Y	3.53	65.9	18.3		135.3	
		Z	3.75	67.9	19.2		142.1	
10295-AAB	CDMA2000, RC1, SO3, 1/8th Rate 25 fr.	X	4.79	64.7	22.2	12.49	67.0	±0.9 %
		Y	4.55	62.7	21.6		55.7	
		Z	5.09	66.2	23.5		79.2	
10403-AAB	CDMA2000 (1xEV-DO, Rev. 0)	X	4.94	70.5	19.4	3.76	143.1	±0.5 %
		Y	4.58	67.9	18.5		142.3	
		Z	5.28	71.7	20.3		147.5	
10404-AAB	CDMA2000 (1xEV-DO, Rev. A)	X	4.98	71.0	19.7	3.77	142.4	±0.7 %
		Y	4.65	68.7	19.0		140.8	
		Z	5.22	71.9	20.4		146.7	
10406-AAB	CDMA2000, RC3, SO32, SCH0, Full Rate	X	6.06	70.3	20.2	5.22	144.0	±0.9 %
		Y	6.09	69.1	20.0		144.9	
		Z	6.35	71.1	20.9		126.5	
10415-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	X	2.84	68.7	18.4	1.54	147.1	±0.7 %
		Y	2.69	67.9	18.5		142.7	
		Z	3.42	72.6	20.5		127.9	
10416-AAA	IEEE 802.11g WiFi 2.4 GHz (ERP-OFDM, 6 Mbps, 99pc duty cycle)	X	9.55	68.1	21.0	8.23	138.3	±3.0 %
		Y	9.63	67.9	21.1		135.2	
		Z	9.74	68.6	21.4		143.3	
10417-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps, 99pc duty cycle)	X	9.55	68.1	21.0	8.23	138.6	±3.0 %
		Y	9.57	67.7	21.0		135.1	
		Z	9.75	68.7	21.5		142.9	

Certificate No: EX3-7486_Mar18/2

Page 13 of 16

EX3DV4- SN:7486

March 20, 2018

10418-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 99pc duty cycle, Long preamble)	X	9.42	68.1	20.9	8.14	137.4	±2.7 %
		Y	9.48	67.8	21.1		133.4	
		Z	9.60	68.6	21.4		142.1	
10458-AAA	CDMA2000 (1xEV-DO, Rev. B, 2 carriers)	X	8.00	69.1	20.4	6.55	146.0	±1.4 %
		Y	8.03	68.3	20.3		145.6	
		Z	7.90	68.7	20.4		126.9	
10459-AAA	CDMA2000 (1xEV-DO, Rev. B, 3 carriers)	X	10.44	70.1	21.8	8.25	142.9	±3.0 %
		Y	10.66	69.7	21.9		145.3	
		Z	10.16	69.1	21.5		125.4	
10515-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 99pc duty cycle)	X	2.80	68.5	18.3	1.58	146.7	±0.7 %
		Y	2.68	67.7	18.4		142.1	
		Z	3.39	72.6	20.6		127.7	
10518-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps, 99pc duty cycle)	X	9.54	68.2	21.0	8.23	137.2	±2.7 %
		Y	9.60	67.9	21.1		134.4	
		Z	9.73	68.7	21.4		142.6	
10525-AAB	IEEE 802.11ac WiFi (20MHz, MCS0, 99pc duty cycle)	X	9.75	68.3	21.1	8.36	139.0	±3.0 %
		Y	9.84	68.1	21.3		136.8	
		Z	9.97	68.9	21.6		144.9	
10526-AAB	IEEE 802.11ac WiFi (20MHz, MCS1, 99pc duty cycle)	X	9.83	68.4	21.2	8.42	139.8	±3.0 %
		Y	9.87	68.1	21.3		136.8	
		Z	10.02	68.9	21.7		145.1	
10534-AAB	IEEE 802.11ac WiFi (40MHz, MCS0, 99pc duty cycle)	X	10.28	68.7	21.3	8.45	147.5	±3.3 %
		Y	10.29	68.4	21.4		142.9	
		Z	10.10	68.2	21.2		126.2	
10535-AAB	IEEE 802.11ac WiFi (40MHz, MCS1, 99pc duty cycle)	X	10.28	68.7	21.3	8.45	147.1	±3.3 %
		Y	10.31	68.5	21.5		143.9	
		Z	10.06	68.1	21.1		126.4	
10544-AAB	IEEE 802.11ac WiFi (80MHz, MCS0, 99pc duty cycle)	X	10.17	67.8	20.6	8.47	126.6	±3.0 %
		Y	10.49	68.4	21.3		147.4	
		Z	10.41	68.4	21.2		131.6	
10545-AAB	IEEE 802.11ac WiFi (80MHz, MCS1, 99pc duty cycle)	X	10.26	68.0	20.8	8.55	126.9	±3.0 %
		Y	10.58	68.5	21.4		147.6	
		Z	10.47	68.5	21.2		131.4	
10564-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 9 Mbps, 99pc duty cycle)	X	9.59	68.3	21.1	8.25	138.4	±3.0 %
		Y	9.65	68.0	21.2		135.3	
		Z	9.77	68.7	21.5		143.3	
10571-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 90pc duty cycle)	X	2.92	68.6	18.6	1.99	142.6	±0.9 %
		Y	2.91	68.8	19.2		138.5	
		Z	3.22	71.0	20.0		146.2	
10572-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 90pc duty cycle)	X	2.98	69.3	18.9	1.99	142.2	±0.7 %
		Y	2.73	67.6	18.5		137.3	
		Z	3.32	71.8	20.4		146.3	

EX3DV4- SN:7486

March 20, 2018

10575-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 90pc duty cycle)	X	9.66	68.2	21.3	8.59	135.0	±3.0 %
		Y	9.71	67.9	21.3		131.3	
		Z	9.86	68.7	21.7		140.0	
10576-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 9 Mbps, 90pc duty cycle)	X	9.65	68.2	21.3	8.60	134.6	±3.0 %
		Y	9.72	68.0	21.4		130.7	
		Z	9.86	68.7	21.7		140.0	
10583-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps, 90pc duty cycle)	X	9.65	68.2	21.2	8.59	135.2	±3.0 %
		Y	9.73	68.0	21.4		131.7	
		Z	9.86	68.8	21.8		140.4	
10584-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps, 90pc duty cycle)	X	9.68	68.3	21.3	8.60	134.7	±3.0 %
		Y	9.70	67.9	21.4		131.0	
		Z	9.87	68.8	21.8		139.9	
10591-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS0, 90pc duty cycle)	X	9.78	68.2	21.3	8.63	136.5	±3.3 %
		Y	9.77	67.8	21.3		132.6	
		Z	9.98	68.8	21.7		141.9	
10592-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS1, 90pc duty cycle)	X	9.93	68.4	21.5	8.79	137.0	±3.3 %
		Y	9.95	68.0	21.5		132.6	
		Z	10.14	68.9	21.9		142.4	
10599-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS0, 90pc duty cycle)	X	10.39	68.7	21.6	8.79	144.8	±3.3 %
		Y	10.30	68.2	21.6		138.5	
		Z	10.20	68.2	21.4		124.8	
10600-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS1, 90pc duty cycle)	X	10.45	68.8	21.6	8.88	144.7	±3.5 %
		Y	10.43	68.4	21.7		139.6	
		Z	10.26	68.3	21.5		124.7	
10607-AAB	IEEE 802.11ac WiFi (20MHz, MCS0, 90pc duty cycle)	X	9.79	68.2	21.3	8.64	136.8	±3.0 %
		Y	9.85	67.9	21.4		133.4	
		Z	10.02	68.9	21.8		142.3	
10608-AAB	IEEE 802.11ac WiFi (20MHz, MCS1, 90pc duty cycle)	X	9.93	68.4	21.5	8.77	136.9	±3.3 %
		Y	9.99	68.1	21.6		132.2	
		Z	10.15	69.0	22.0		142.6	
10616-AAB	IEEE 802.11ac WiFi (40MHz, MCS0, 90pc duty cycle)	X	10.42	68.8	21.6	8.82	144.9	±3.3 %
		Y	10.38	68.3	21.6		139.5	
		Z	10.24	68.3	21.5		124.8	
10617-AAB	IEEE 802.11ac WiFi (40MHz, MCS1, 90pc duty cycle)	X	10.39	68.7	21.5	8.81	144.8	±3.5 %
		Y	10.40	68.4	21.7		139.7	
		Z	10.20	68.2	21.4		124.6	
10626-AAB	IEEE 802.11ac WiFi (80MHz, MCS0, 90pc duty cycle)	X	10.30	67.8	20.9	8.83	124.0	±3.0 %
		Y	10.61	68.4	21.5		143.7	
		Z	10.54	68.5	21.4		129.7	
10627-AAB	IEEE 802.11ac WiFi (80MHz, MCS1, 90pc duty cycle)	X	10.35	67.9	21.0	8.88	124.1	±3.0 %
		Y	10.68	68.6	21.7		144.0	
		Z	10.58	68.5	21.5		129.5	

Certificate No: EX3-7486_Mar18/2

Page 15 of 16

EX3DV4- SN:7486

March 20, 2018

10648- AAA	CDMA2000 (1x Advanced)	X	3.62	67.2	18.6	3.45	139.5	±0.7 %
		Y	3.49	66.1	18.5		135.6	
		Z	3.75	68.1	19.4		143.0	

⁵ Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Motorola Solutions MY**

Certificate No: **ES3-3122_Apr18**

CALIBRATION CERTIFICATE

Object **ES3DV3 - SN:3122**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v4, QA CAL-23.v5,
QA CAL-25.v6
Calibration procedure for dosimetric E-field probes**

Calibration date: **April 18, 2018**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-18 (No. 217-02672/02673)	Apr-19
Power sensor NRP-Z91	SN: 103244	04-Apr-18 (No. 217-02672)	Apr-19
Power sensor NRP-Z91	SN: 103245	04-Apr-18 (No. 217-02673)	Apr-19
Reference 20 dB Attenuator	SN: S5277 (20x)	04-Apr-18 (No. 217-02682)	Apr-19
Reference Probe ES3DV2	SN: 3013	30-Dec-17 (No. ES3-3013_Dec17)	Dec-18
DAE4	SN: 660	21-Dec-17 (No. DAE4-660_Dec17)	Dec-18
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (in house check Jun-16)	In house check: Jun-18
Power sensor E4412A	SN: MY41488087	06-Apr-16 (in house check Jun-16)	In house check: Jun-18
Power sensor E4412A	SN: 000110210	06-Apr-16 (in house check Jun-16)	In house check: Jun-18
RF generator HP 8548C	SN: U83842U01700	04-Aug-99 (in house check Jun-16)	In house check: Jun-18
Network Analyzer HP 8753E	SN: US37390685	18-Oct-01 (in house check Oct-17)	In house check: Oct-18

Calibrated by:	Name Claudio Leubler	Function Laboratory Technician	Signature
Approved by:	Name Katja Pokovic	Function Technical Manager	Signature

Issued: April 19, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Calibration Laboratory of
Schmid & Partner
Engineering AG
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
 Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization θ	θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}**: Assessed for E-field polarization $\theta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)_{x,y,z} = NORM_{x,y,z} * frequency_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP_{x,y,z}**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A_{x,y,z}; B_{x,y,z}; C_{x,y,z}; D_{x,y,z}; VR_{x,y,z}**: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM_x (no uncertainty required).

ES3DV3 – SN:3122

April 18, 2018

Probe ES3DV3

SN:3122

Manufactured: July 11, 2006
Calibrated: April 18, 2018

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

ES3DV3- SN:3122

April 18, 2018

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3122

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ($\mu\text{V}/(\text{V/m})^2$) ^A	1.30	1.19	1.39	± 10.1 %
DCP (mV) ^B	101.7	102.8	102.3	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Unc ^E (k=2)
0	CW	X	0.0	0.0	1.0	0.00	212.2	±3.5 %
		Y	0.0	0.0	1.0		209.0	
		Z	0.0	0.0	1.0		170.3	

Note: For details on UID parameters see Appendix.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).

^B Numerical linearization parameter; uncertainty not required.

^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

ES3DV3- SN:3122

April 18, 2018

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3122

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^f	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ^g	Depth ^g (mm)	Unc (k=2)
150	52.3	0.76	7.20	7.20	7.20	0.08	1.20	± 13.3 %
300	45.3	0.87	7.01	7.01	7.01	0.13	1.20	± 13.3 %
450	43.5	0.87	6.80	6.80	6.80	0.23	1.30	± 13.3 %
750	41.9	0.89	6.61	6.61	6.61	0.80	1.17	± 12.0 %
835	41.5	0.90	6.31	6.31	6.31	0.61	1.31	± 12.0 %
900	41.5	0.97	6.18	6.18	6.18	0.66	1.28	± 12.0 %
1450	40.5	1.20	5.64	5.64	5.64	0.80	1.12	± 12.0 %
1810	40.0	1.40	5.24	5.24	5.24	0.39	1.66	± 12.0 %
1900	40.0	1.40	5.21	5.21	5.21	0.44	1.51	± 12.0 %
2100	39.8	1.49	5.28	5.28	5.28	0.80	1.20	± 12.0 %
2300	39.5	1.67	4.86	4.86	4.86	0.80	1.21	± 12.0 %
2450	39.2	1.80	4.64	4.64	4.64	0.69	1.32	± 12.0 %
2600	39.0	1.96	4.46	4.46	4.46	0.80	1.33	± 12.0 %
3500	37.9	2.91	4.38	4.38	4.38	0.80	1.25	± 13.1 %
3700	37.7	3.12	4.08	4.08	4.08	0.70	1.25	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^f At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^g Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

ES3DV3- SN:3122

April 18, 2018

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3122

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^f	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ^g	Depth ^g (mm)	Unc (k=2)
150	61.9	0.80	6.82	6.82	6.82	0.08	1.20	± 13.3 %
300	58.2	0.92	6.79	6.79	6.79	0.10	1.20	± 13.3 %
450	56.7	0.94	6.95	6.95	6.95	0.10	1.30	± 13.3 %
750	55.5	0.96	6.39	6.39	6.39	0.54	1.37	± 12.0 %
835	55.2	0.97	6.28	6.28	6.28	0.80	1.14	± 12.0 %
900	55.0	1.05	6.22	6.22	6.22	0.58	1.33	± 12.0 %
1450	54.0	1.30	5.39	5.39	5.39	0.80	1.12	± 12.0 %
1810	53.3	1.52	5.02	5.02	5.02	0.51	1.53	± 12.0 %
1900	53.3	1.52	4.81	4.81	4.81	0.67	1.36	± 12.0 %
2100	53.2	1.62	5.09	5.09	5.09	0.57	1.53	± 12.0 %
2300	52.9	1.81	4.58	4.58	4.58	0.80	1.24	± 12.0 %
2450	52.7	1.95	4.52	4.52	4.52	0.80	1.18	± 12.0 %
2600	52.5	2.16	4.26	4.26	4.26	0.79	1.20	± 12.0 %
3500	51.3	3.31	3.86	3.86	3.86	0.70	1.30	± 13.1 %
3700	51.0	3.55	3.85	3.85	3.85	0.70	1.30	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), also it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^f At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.


^g Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

ES3DV3-SN:3122

April 18, 2018

Frequency Response of E-Field

(TEM-Cell: ifi110 EXX, Waveguide: R22)

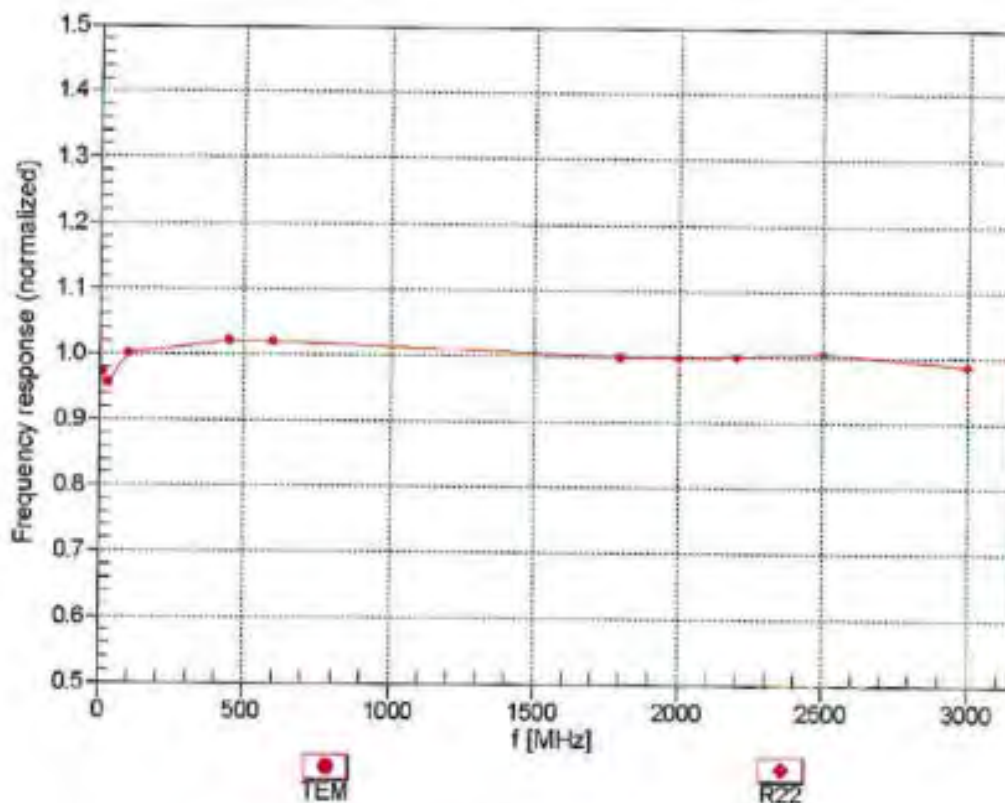


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ ($k=2$)

ES3DV3- SN:3122



April 18, 2018

Receiving Pattern (ϕ), $\theta = 0^\circ$

f=600 MHz, TEM

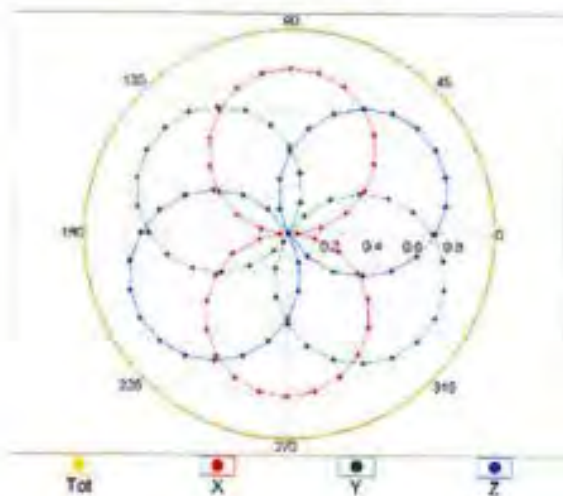



f=1800 MHz, R22

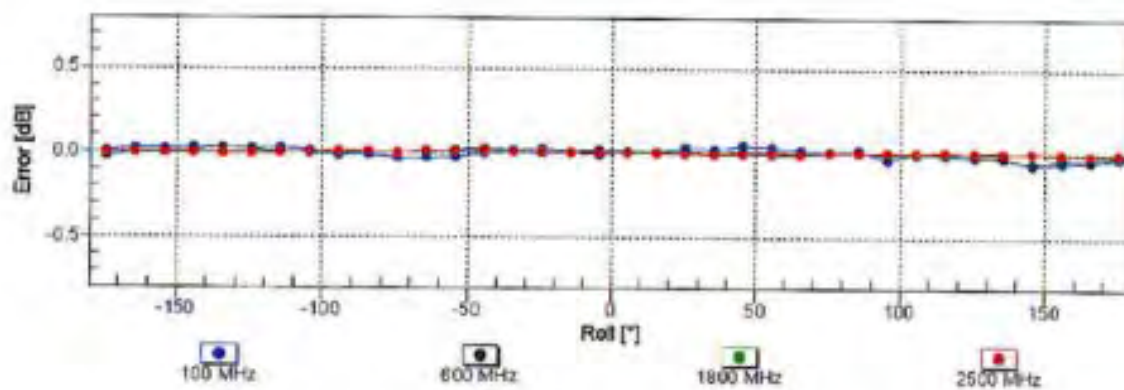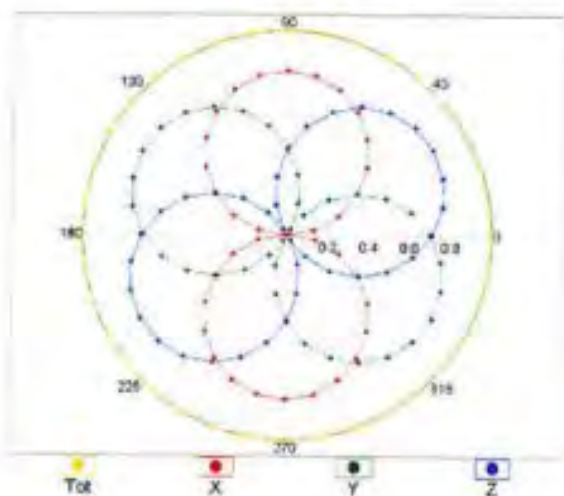Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ (k=2)

ES3DV3- SN:3122

April 18, 2018

Dynamic Range f(SAR_{head})
(TEM cell , f_{eval}= 1900 MHz)

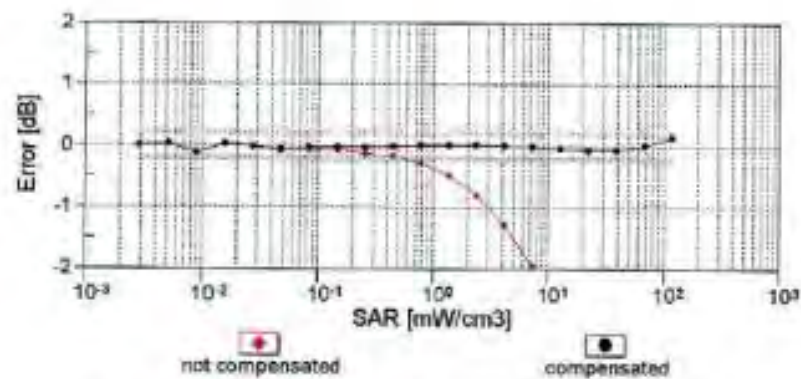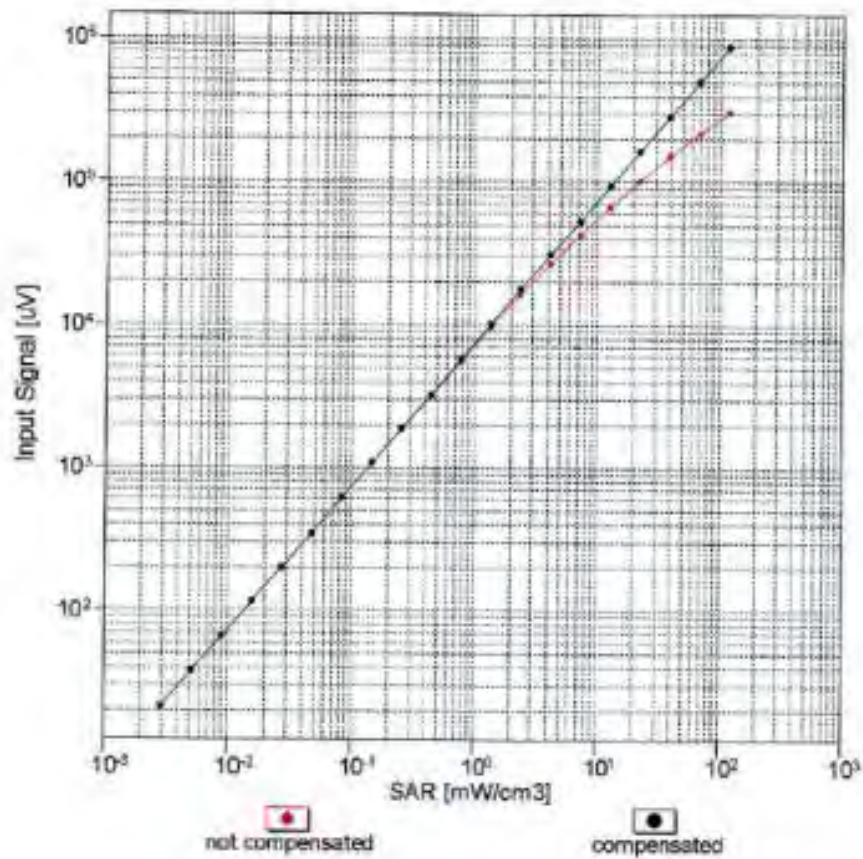


Uncertainty of Linearity Assessment: ± 0.6% (k=2)


ES3DV3- SN:3122

April 18, 2018

Conversion Factor Assessment

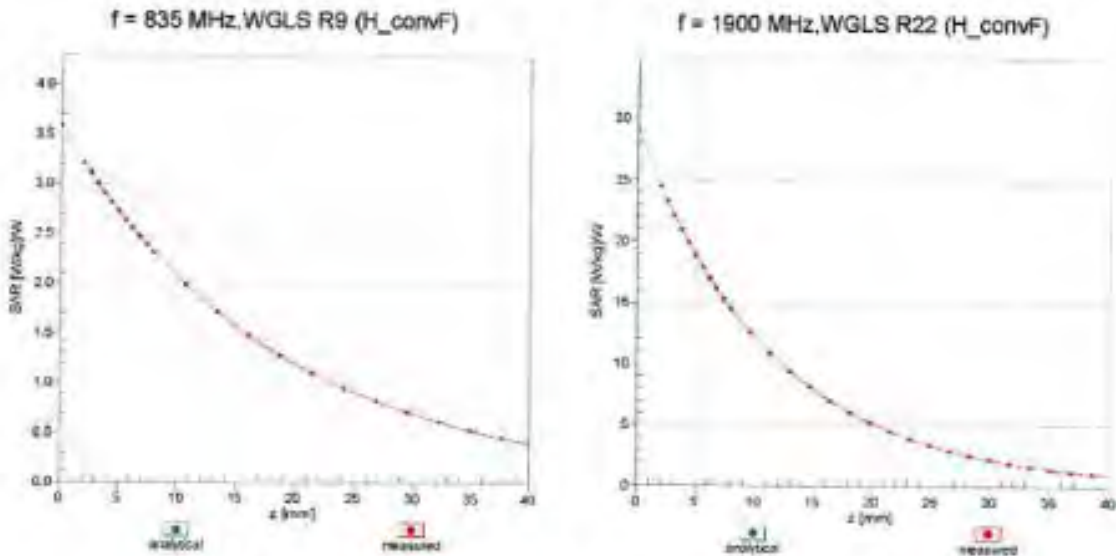

Deviation from Isotropy in Liquid
Error (ϕ, θ), $f = 900 \text{ MHz}$

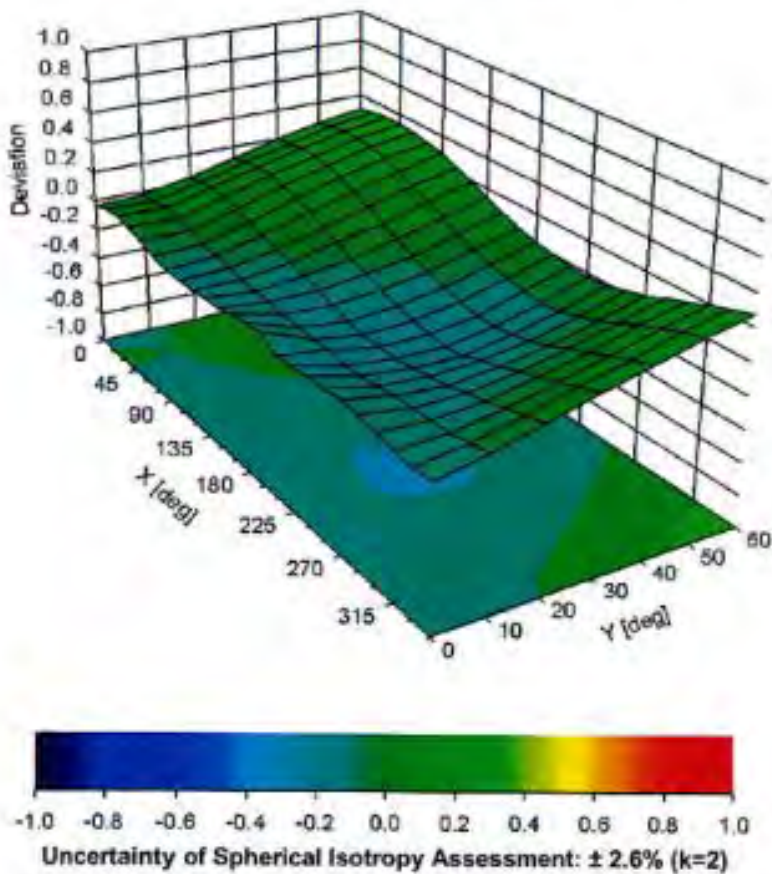

ES3DV3- SN:3122

April 18, 2018

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3122**Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	25.7
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	4 mm
Probe Tip to Sensor X Calibration Point	2 mm
Probe Tip to Sensor Y Calibration Point	2 mm
Probe Tip to Sensor Z Calibration Point	2 mm
Recommended Measurement Distance from Surface	3 mm

ES3DV3- SN:3122

April 18, 2018

Appendix: Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu V}$	C	D dB	VR mV	Unc ^F (k=2)
0	CW	X	0.0	0.0	1.0	0.00	212.2	±3.5 %
		Y	0.0	0.0	1.0		209.0	
		Z	0.0	0.0	1.0		170.3	
10011-CAB	UMTS-FDD (WCDMA)	X	2.98	64.8	17.0	2.91	126.1	±0.7 %
		Y	3.13	65.9	17.9		124.0	
		Z	3.15	66.2	18.0		136.1	
10097-CAB	UMTS-FDD (HSDPA)	X	4.38	65.4	17.7	3.98	134.3	±0.7 %
		Y	4.50	66.1	18.2		132.7	
		Z	4.48	66.2	18.3		145.2	
10098-CAB	UMTS-FDD (HSUPA, Subtest 2)	X	4.34	65.2	17.5	3.98	134.1	±0.7 %
		Y	4.49	66.0	18.2		132.3	
		Z	4.50	66.3	18.3		145.2	
10100-CAD	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	X	6.27	67.0	19.3	5.67	140.9	±1.2 %
		Y	6.41	67.6	19.8		139.9	
		Z	5.90	65.7	18.8		108.7	
10101-CAD	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM)	X	6.87	65.7	18.9	6.42	106.2	±1.4 %
		Y	7.57	68.1	20.4		149.7	
		Z	7.03	66.4	19.4		115.6	
10108-CAE	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X	6.22	66.8	19.4	5.80	138.9	±1.2 %
		Y	6.37	67.5	19.9		137.7	
		Z	5.89	65.6	18.8		107.6	
10109-CAE	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM)	X	7.24	67.4	19.9	6.43	148.0	±1.4 %
		Y	7.38	68.0	20.4		146.2	
		Z	6.83	66.2	19.3		113.4	
10110-CAE	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, QPSK)	X	5.97	66.4	19.2	5.75	136.1	±1.2 %
		Y	6.07	66.9	19.6		135.0	
		Z	6.07	67.0	19.7		147.6	
10111-CAE	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM)	X	7.04	67.2	19.8	6.44	145.2	±1.2 %
		Y	7.15	67.8	20.3		143.0	
		Z	6.63	66.0	19.3		110.9	
10117-CAC	IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)	X	9.95	68.4	21.0	8.07	128.7	±1.9 %
		Y	10.18	69.0	21.5		127.3	
		Z	10.18	69.1	21.5		141.1	
10140-CAD	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	X	7.06	65.9	19.1	6.49	107.8	±1.2 %
		Y	7.20	66.4	19.5		105.6	
		Z	7.24	66.6	19.5		117.5	
10142-CAD	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, QPSK)	X	5.88	66.4	19.2	5.73	134.9	±1.2 %
		Y	5.92	66.7	19.5		132.9	
		Z	5.90	66.8	19.6		145.1	
10143-CAD	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM)	X	6.86	67.2	19.8	6.35	142.8	±1.2 %
		Y	6.92	67.6	20.2		140.2	
		Z	6.39	65.8	19.2		108.6	

ES3DV3- SN:3122

April 16, 2018

10145-CAE	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK)	X	5.65	66.0	19.0	5.76	131.7	±0.9 %
		Y	5.68	66.4	19.4		129.3	
		Z	5.69	66.7	19.5		140.8	
10146-CAE	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	X	6.63	67.1	19.8	6.41	137.8	±1.2 %
		Y	6.66	67.6	20.2		134.4	
		Z	6.66	67.7	20.3		146.5	
10149-CAD	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM)	X	7.25	67.4	20.0	6.42	147.7	±1.4 %
		Y	7.35	67.9	20.4		145.9	
		Z	6.83	66.2	19.3		113.4	
10154-CAE	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	X	5.99	66.5	19.3	5.75	136.2	±1.2 %
		Y	6.07	66.9	19.6		134.5	
		Z	6.07	67.0	19.7		147.4	
10155-CAE	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM)	X	7.06	67.3	19.9	6.43	145.5	±1.4 %
		Y	7.14	67.7	20.3		142.7	
		Z	6.59	65.9	19.2		110.4	
10156-CAE	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, QPSK)	X	5.81	66.1	19.1	5.79	133.7	±1.2 %
		Y	5.87	66.5	19.5		131.2	
		Z	5.86	66.7	19.6		143.6	
10157-CAE	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM)	X	6.87	67.2	19.9	6.49	140.8	±1.2 %
		Y	6.94	67.7	20.4		138.5	
		Z	6.41	65.9	19.3		107.2	
10160-CAD	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, QPSK)	X	6.37	66.8	19.4	5.82	141.1	±1.2 %
		Y	6.51	67.4	19.9		139.7	
		Z	6.01	65.7	18.9		108.6	
10161-CAD	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM)	X	7.33	67.5	20.0	6.43	149.2	±1.4 %
		Y	7.44	68.0	20.4		147.2	
		Z	6.88	66.2	19.3		114.2	
10166-CAE	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK)	X	5.07	65.8	18.8	5.46	126.4	±0.9 %
		Y	5.09	66.0	19.1		124.0	
		Z	5.12	66.3	19.3		136.0	
10167-CAE	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM)	X	6.07	66.9	19.6	6.21	130.6	±1.2 %
		Y	6.12	67.4	20.1		127.4	
		Z	6.13	67.7	20.2		139.8	
10169-CAD	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	X	4.95	65.8	19.0	5.73	120.9	±0.9 %
		Y	5.02	66.5	19.6		118.9	
		Z	5.03	66.6	19.6		130.3	
10170-CAD	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM)	X	5.79	67.1	20.0	6.52	121.6	±1.2 %
		Y	5.87	67.7	20.5		118.9	
		Z	5.88	67.9	20.5		130.8	
10175-CAE	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	X	4.94	65.8	18.9	5.72	121.0	±0.9 %
		Y	5.03	66.5	19.5		118.8	
		Z	5.04	66.7	19.6		130.1	
10176-CAE	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM)	X	5.81	67.2	20.0	6.52	121.6	±1.2 %
		Y	5.88	67.8	20.6		118.6	
		Z	5.90	68.0	20.6		130.7	

Certificate No: ES3-3122, Apr18

Page 13 of 18

ES3DV3- SN:3122

April 18, 2018

10177-CAG	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, QPSK)	X	4.97	65.9	19.0	5.73	121.3	±0.9 %
		Y	5.02	66.4	19.5		118.7	
		Z	5.04	66.7	19.6		130.4	
10178-CAE	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM)	X	5.82	67.2	20.0	6.52	121.9	±1.2 %
		Y	5.84	67.6	20.4		118.9	
		Z	5.91	68.0	20.6		131.0	
10181-CAD	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	X	4.94	65.7	18.9	5.72	121.0	±0.9 %
		Y	5.02	66.4	19.5		118.7	
		Z	5.06	66.8	19.7		130.4	
10182-CAD	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM)	X	5.80	67.1	19.9	6.52	121.6	±1.2 %
		Y	5.86	67.7	20.5		118.8	
		Z	5.91	68.0	20.6		130.8	
10184-CAD	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, QPSK)	X	4.96	65.9	19.0	5.73	121.0	±0.9 %
		Y	5.03	66.5	19.6		118.7	
		Z	5.03	66.6	19.6		130.0	
10185-CAD	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM)	X	5.80	67.1	20.0	6.51	121.5	±1.2 %
		Y	5.88	67.8	20.5		118.7	
		Z	5.92	68.1	20.7		130.9	
10187-CAE	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK)	X	4.95	65.8	18.9	5.73	120.9	±0.9 %
		Y	5.03	66.4	19.5		119.0	
		Z	5.02	66.5	19.5		130.1	
10188-CAE	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM)	X	5.81	67.1	20.0	6.52	121.6	±1.2 %
		Y	5.87	67.7	20.5		118.9	
		Z	5.91	68.0	20.6		131.0	
10196-CAC	IEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)	X	9.69	68.1	20.9	6.10	124.2	±1.9 %
		Y	9.87	68.7	21.5		122.8	
		Z	9.86	68.9	21.5		136.4	
10225-CAB	UMTS-FDD (HSPA+)	X	6.58	65.3	18.5	5.97	107.4	±1.2 %
		Y	6.57	65.5	18.7		104.1	
		Z	6.70	66.1	19.0		116.2	
10274-CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.10)	X	5.90	66.4	18.6	4.87	146.3	±0.9 %
		Y	6.00	66.9	19.0		144.2	
		Z	5.62	65.8	18.3		112.0	
10275-CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.4)	X	4.25	65.6	18.0	3.96	130.0	±0.7 %
		Y	4.34	66.2	18.5		128.8	
		Z	4.37	66.5	18.6		140.4	
10297-AAC	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	X	6.29	67.1	19.6	5.81	138.4	±1.2 %
		Y	6.38	67.4	19.9		137.2	
		Z	5.90	65.7	18.9		106.8	
10298-AAC	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, QPSK)	X	5.72	66.2	19.1	5.72	132.5	±1.2 %
		Y	5.78	66.7	19.6		130.4	
		Z	5.74	66.7	19.6		142.0	
10299-AAC	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM)	X	6.73	67.1	19.8	6.39	139.4	±1.2 %
		Y	6.79	67.7	20.3		136.6	
		Z	6.79	67.9	20.4		149.1	

ES3DV3--SN.3122

April 18, 2018

10311-AAC	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	X	6.77	67.4	19.8	8.06	143.5	±1.2 %
		Y	6.94	68.0	20.3		142.6	
		Z	6.39	66.2	19.2		110.2	
10415-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	X	2.33	65.6	17.0	1.54	129.1	±0.5 %
		Y	2.47	66.6	17.8		127.4	
		Z	2.44	66.8	17.9		139.9	
10416-AAA	IEEE 802.11g WiFi 2.4 GHz (ERP-OFDM, 6 Mbps, 99pc duty cycle)	X	9.79	68.3	21.2	8.23	125.1	±1.9 %
		Y	10.02	69.0	21.7		122.7	
		Z	9.95	68.9	21.6		136.4	
10418-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 99pc duty cycle, Long preamble)	X	9.68	68.3	21.1	8.14	124.1	±1.7 %
		Y	9.88	68.9	21.6		121.6	
		Z	9.84	68.9	21.5		135.2	
10430-AAB	LTE-FDD (OFDMA, 5 MHz, E-TM 3.1)	X	9.17	67.9	21.0	8.26	114.8	±1.7 %
		Y	9.27	68.5	21.6		111.7	
		Z	9.24	68.6	21.6		123.3	
10431-AAB	LTE-FDD (OFDMA, 10 MHz, E-TM 3.1)	X	9.64	68.2	21.2	8.38	120.8	±1.9 %
		Y	9.80	68.8	21.7		118.2	
		Z	9.78	68.9	21.7		131.0	
10432-AAB	LTE-FDD (OFDMA, 15 MHz, E-TM 3.1)	X	9.81	68.3	21.2	8.34	123.7	±1.9 %
		Y	10.05	69.1	21.9		121.5	
		Z	9.98	69.0	21.7		135.3	
10433-AAB	LTE-FDD (OFDMA, 20 MHz, E-TM 3.1)	X	9.99	68.5	21.3	8.34	126.5	±1.9 %
		Y	10.26	69.3	21.9		124.6	
		Z	10.17	69.2	21.8		137.9	
10435-AAC	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	7.10	71.6	23.1	7.82	112.9	±1.9 %
		Y	7.32	72.6	23.9		111.3	
		Z	7.64	73.9	24.5		123.1	
10457-AAA	UMTS-FDD (DC-HSDPA)	X	7.93	66.1	19.2	6.62	119.3	±1.4 %
		Y	8.08	66.6	19.6		118.1	
		Z	8.09	66.7	19.6		130.5	
10460-AAA	UMTS-FDD (WCDMA, AMR)	X	2.62	65.9	17.6	2.39	123.9	±0.5 %
		Y	2.76	66.9	18.4		122.0	
		Z	2.79	67.5	18.7		134.0	
10461-AAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	7.13	71.6	23.1	7.82	113.1	±1.9 %
		Y	7.43	73.0	24.1		111.8	
		Z	7.64	73.8	24.4		122.7	
10462-AAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.65	72.3	23.7	8.30	112.2	±2.2 %
		Y	7.95	73.7	24.7		111.2	
		Z	8.26	74.9	25.2		122.1	
10464-AAA	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	7.11	71.6	23.1	7.82	112.9	±1.9 %
		Y	7.35	72.7	23.9		111.4	
		Z	7.58	73.6	24.3		122.6	

ES3DV3- SN:3122

April 18, 2018

10465-AAA	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.68	72.4	23.8	8.32	111.9	±1.9 %
		Y	7.92	73.6	24.6		111.2	
		Z	8.26	74.8	25.1		122.0	
10467-AAC	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	7.15	71.7	23.2	7.82	112.9	±1.9 %
		Y	7.43	73.0	24.1		111.0	
		Z	7.66	73.9	24.5		122.9	
10468-AAC	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.68	72.4	23.8	8.32	112.4	±1.9 %
		Y	7.93	73.6	24.7		110.9	
		Z	8.22	74.7	25.1		121.8	
10470-AAC	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	7.09	71.5	23.1	7.82	112.7	±1.9 %
		Y	7.34	72.7	23.9		111.2	
		Z	7.62	73.7	24.4		122.5	
10471-AAC	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.67	72.4	23.8	8.32	112.3	±2.2 %
		Y	7.88	73.4	24.5		110.9	
		Z	8.24	74.7	25.1		122.2	
10473-AAC	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	7.12	71.6	23.2	7.82	112.9	±1.9 %
		Y	7.37	72.8	24.0		111.2	
		Z	7.60	73.7	24.4		122.6	
10474-AAC	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.73	72.6	23.9	8.32	112.4	±1.9 %
		Y	7.87	73.4	24.6		111.0	
		Z	8.21	74.6	25.0		121.8	
10477-AAC	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.64	72.3	23.7	8.32	111.8	±2.2 %
		Y	7.90	73.5	24.6		111.1	
		Z	8.18	74.6	25.0		121.9	
10479-AAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	7.45	71.3	22.9	7.74	120.3	±2.2 %
		Y	7.66	72.3	23.7		118.0	
		Z	7.88	73.2	24.1		129.9	
10480-AAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	8.25	72.2	23.6	8.18	123.2	±2.2 %
		Y	8.45	73.3	24.4		120.5	
		Z	8.67	74.1	24.7		133.0	
10482-AAA	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	8.03	71.7	23.1	7.71	127.5	±2.2 %
		Y	8.19	72.5	23.7		125.5	
		Z	8.42	73.5	24.2		138.2	
10483-AAA	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	9.13	72.6	23.9	8.39	134.8	±2.7 %
		Y	9.37	73.7	24.7		132.1	
		Z	9.59	74.6	25.1		146.2	
10485-AAC	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	8.00	71.7	22.9	7.59	129.1	±2.2 %
		Y	8.29	72.8	23.8		127.4	
		Z	8.44	73.5	24.1		140.5	
10486-AAC	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	9.23	72.6	23.9	8.38	137.5	±2.7 %
		Y	9.54	73.8	24.8		135.8	
		Z	9.69	74.4	25.0		149.2	
10488-AAC	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	8.43	72.1	23.2	7.70	133.5	±2.5 %
		Y	8.75	73.3	24.1		131.7	
		Z	8.90	73.8	24.3		146.1	

ES3DV3- SN:3122

April 18, 2018

10489-AAC	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	9.50	72.7	23.9	8.31	143.4	±2.7 %
		Y	9.76	73.6	24.6		141.5	
		Z	8.33	69.4	22.2		106.1	
10491-AAC	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	8.89	72.5	23.4	7.74	138.5	±2.5 %
		Y	9.25	73.7	24.2		138.1	
		Z	7.77	69.3	21.8		103.9	
10492-AAC	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	8.48	68.5	21.6	8.41	101.7	±2.2 %
		Y	10.41	74.3	25.0		148.8	
		Z	8.85	69.9	22.5		111.1	
10494-AAC	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	8.83	72.6	23.4	7.74	137.3	±2.5 %
		Y	9.23	73.8	24.3		136.5	
		Z	7.73	69.3	21.8		102.7	
10495-AAC	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	9.90	73.0	24.1	8.37	148.8	±3.0 %
		Y	10.25	74.1	24.9		147.7	
		Z	8.73	69.8	22.4		110.1	
10497-AAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	7.88	71.5	22.9	7.67	126.6	±2.2 %
		Y	8.14	72.7	23.8		124.7	
		Z	8.32	73.5	24.1		137.7	
10498-AAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	8.98	72.6	23.9	8.40	132.5	±2.7 %
		Y	9.18	73.5	24.6		129.6	
		Z	9.41	74.4	25.0		143.5	
10500-AAA	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	8.22	71.9	23.1	7.67	131.3	±2.2 %
		Y	8.51	73.0	24.0		129.2	
		Z	8.66	73.7	24.2		142.6	
10501-AAA	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	9.44	72.7	24.0	8.44	140.1	±2.7 %
		Y	9.70	73.7	24.8		137.6	
		Z	8.19	69.2	22.2		103.6	
10503-AAC	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	8.41	72.0	23.2	7.72	133.4	±2.5 %
		Y	8.78	73.3	24.1		132.4	
		Z	8.93	73.9	24.3		146.1	
10504-AAC	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	9.47	72.6	23.8	8.31	143.3	±2.7 %
		Y	9.78	73.7	24.7		141.4	
		Z	8.34	69.4	22.2		106.3	
10506-AAC	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	8.81	72.5	23.4	7.74	137.6	±2.2 %
		Y	9.27	74.0	24.4		136.6	
		Z	7.75	69.4	21.9		102.8	
10507-AAC	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	9.64	72.8	24.0	8.36	148.2	±2.7 %
		Y	10.25	74.1	24.9		147.3	
		Z	8.73	69.7	22.3		110.1	
10509-AAC	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	9.51	73.2	23.8	7.99	144.0	±2.5 %
		Y	10.02	74.6	24.8		143.6	
		Z	8.39	69.9	22.2		107.5	

ES3DV3- SN:3122

April 18, 2018

10510-AAC	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	8.90	69.0	21.8	8.49	104.8	±1.9 %
		Y	9.29	70.1	22.6		104.4	
		Z	9.32	70.3	22.7		115.7	
10512-AAC	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	9.20	73.1	23.6	7.74	141.4	±2.2 %
		Y	9.71	74.6	24.5		140.9	
		Z	8.12	70.0	22.1		105.9	
10513-AAC	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	8.75	68.9	21.8	8.42	103.2	±1.9 %
		Y	9.18	70.2	22.7		102.7	
		Z	9.18	70.3	22.7		114.3	
10515-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 99pc duty cycle)	X	2.40	66.0	17.2	1.58	129.3	±0.5 %
		Y	2.48	66.6	17.8		128.1	
		Z	2.48	67.0	18.0		140.0	
10564-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 9 Mbps, 99pc duty cycle)	X	9.86	68.4	21.2	8.25	124.9	±1.9 %
		Y	10.07	69.1	21.7		122.7	
		Z	10.05	69.1	21.7		136.5	
10571-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 90pc duty cycle)	X	3.14	68.9	18.5	1.99	129.3	±0.7 %
		Y	3.26	69.5	19.1		127.8	
		Z	3.46	71.1	19.7		140.3	
10572-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 90pc duty cycle)	X	3.02	68.2	18.2	1.99	128.8	±0.5 %
		Y	3.29	69.8	19.2		127.7	
		Z	3.48	71.2	19.7		139.7	
10575-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 90pc duty cycle)	X	10.24	69.0	21.7	8.59	125.8	±2.2 %
		Y	10.50	69.8	22.3		123.8	
		Z	10.46	69.7	22.3		137.2	
10576-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 9 Mbps, 90pc duty cycle)	X	10.24	69.0	21.7	8.60	125.5	±2.2 %
		Y	10.55	69.9	22.4		123.8	
		Z	10.47	69.8	22.3		136.8	
10591-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS0, 90pc duty cycle)	X	10.36	69.0	21.8	8.63	127.3	±3.0 %
		Y	10.67	69.9	22.5		125.9	
		Z	10.57	69.8	22.3		138.9	
10592-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS1, 90pc duty cycle)	X	10.54	69.3	22.0	8.79	127.5	±3.3 %
		Y	10.87	70.2	22.7		126.3	
		Z	10.80	70.1	22.6		140.1	
10599-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS0, 90pc duty cycle)	X	10.88	69.6	22.1	8.79	132.3	±2.2 %
		Y	11.27	70.6	22.8		131.4	
		Z	11.17	70.4	22.7		145.6	
10600-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS1, 90pc duty cycle)	X	10.98	69.7	22.2	8.88	132.5	±3.5 %
		Y	11.36	70.7	22.9		131.7	
		Z	11.27	70.6	22.8		146.1	

⁶ Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Appendix C

Dipole Calibration Certificates

Calibration Laboratory of
Schmid & Partner
Engineering AG
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Motorola Solutions MY**

Certificate No: **D450V3-1054_Oct17**

CALIBRATION CERTIFICATE

Object **D450V3 - SN:1054**

Calibration procedure(s) **QA CAL-15.v8**
Calibration procedure for dipole validation kits below 700 MHz

Calibration date: **October 25, 2017**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^{\circ}\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-17 (No. 217-02521/02522)	Apr-18
Power sensor NRP-Z91	SN: 103244	04-Apr-17 (No. 217-02521)	Apr-18
Power sensor NRP-Z91	SN: 103245	04-Apr-17 (No. 217-02522)	Apr-18
Reference 20 dB Attenuator	SN: 5277 (20x)	07-Apr-17 (No. 217-02528)	Apr-18
Type-N mismatch combination	SN: 5047.2 / 06327	07-Apr-17 (No. 217-02529)	Apr-18
Reference Probe EX3DV4	SN: 3877	31-Dec-16 (No. EX3-3877_Dec16)	Dec-17
DAE4	SN: 654	24-Jul-17 (No. DAE4-654_Jul17)	Jul-18
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (No. 217-02265/02284)	In house check: Jun-18
Power sensor E4412A	SN: MY41498087	06-Apr-16 (No. 217-02265)	In house check: Jun-18
Power sensor E4412A	SN: 000110210	06-Apr-16 (No. 217-02264)	In house check: Jun-18
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-16)	In house check: Jun-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-17)	In house check: Oct-18

	Name	Function	Signature
Calibrated by:	Jeton Kastrati	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	

Issued: October 25, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D450V3-1054_Oct17

Page 1 of 8

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.0
Extrapolation	Advanced Extrapolation	
Phantom	ELI4 Flat Phantom	Shell thickness: 2 ± 0.2 mm
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	450 MHz \pm 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	43.5	0.87 mho/m
Measured Head TSL parameters	(22.0 \pm 0.2) °C	43.5 \pm 6 %	0.87 mho/m \pm 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	1.12 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	4.48 W/kg \pm 18.1 % (k=2)

SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	0.750 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	3.00 W/kg \pm 17.6 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	56.7	0.94 mho/m
Measured Body TSL parameters	(22.0 \pm 0.2) °C	55.2 \pm 6 %	0.93 mho/m \pm 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	1.14 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	4.57 W/kg \pm 18.1 % (k=2)

SAR averaged over 10 cm³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	0.759 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	3.05 W/kg \pm 17.6 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	57.9 Ω - 4.1 j Ω
Return Loss	- 21.6 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	54.4 Ω - 8.9 j Ω
Return Loss	- 20.4 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.349 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	December 16, 2005

DASY5 Validation Report for Head TSL

Date: 25.10.2017

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 450 MHz D450V3; Type: D450V3; Serial: D450V3 - SN:1054

Communication System: UID 0 - CW; Frequency: 450 MHz

Medium parameters used: $f = 450$ MHz; $\sigma = 0.87$ S/m; $\epsilon_r = 43.5$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(10.5, 10.5, 10.5); Calibrated: 31.12.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 24.07.2017
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

Dipole Calibration for Head Tissue/d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 43.28 V/m; Power Drift = -0.06 dB


Peak SAR (extrapolated) = 1.74 W/kg

SAR(1 g) = 1.12 W/kg; SAR(10 g) = 0.750 W/kg

Maximum value of SAR (measured) = 1.52 W/kg

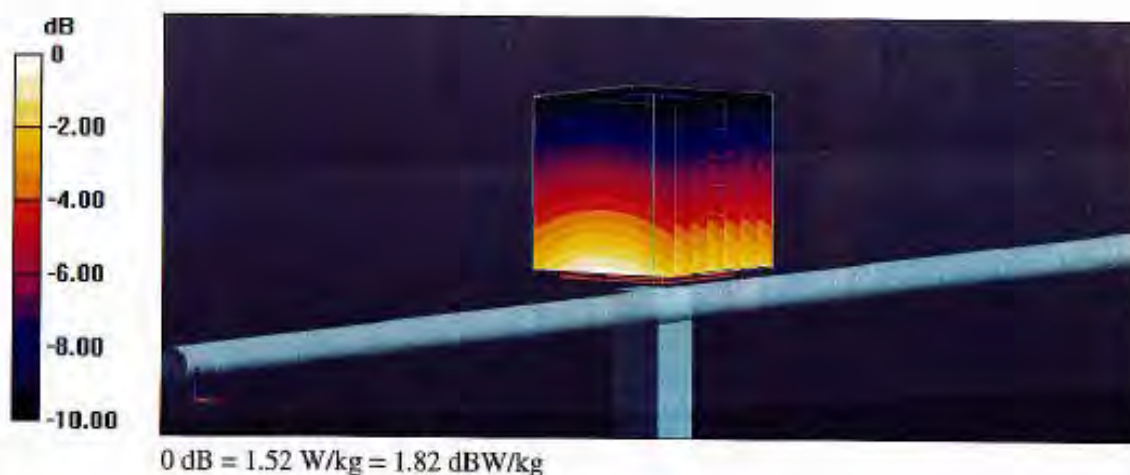

Impedance Measurement Plot for Head TSL

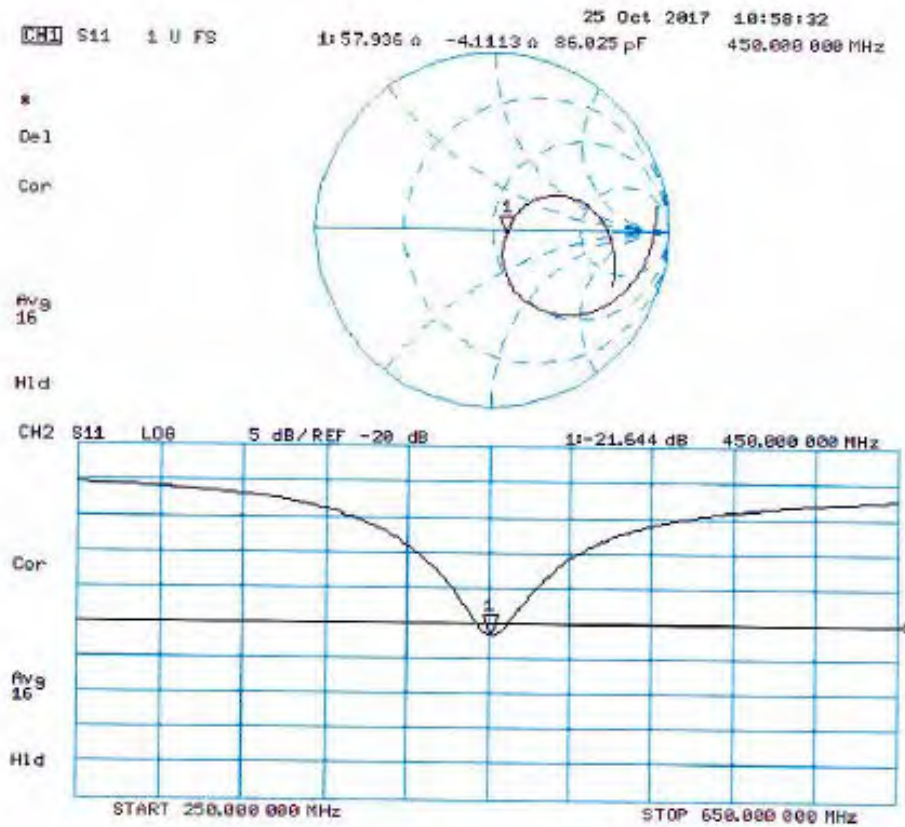

DASY5 Validation Report for Body TSL

Date: 25.10.2017

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 450 MHz D450V3; Type: D450V3; Serial: D450V3 - SN:1054

Communication System: UID 0 - CW; Frequency: 450 MHz

Medium parameters used: $f = 450$ MHz; $\sigma = 0.93$ S/m; $\epsilon_r = 55.2$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(10.7, 10.7, 10.7); Calibrated: 31.12.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 24.07.2017
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

Dipole Calibration for Body Tissue/d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm


Reference Value = 42.19 V/m; Power Drift = -0.05dB

Peak SAR (extrapolated) = 1.76 W/kg

SAR(1 g) = 1.14 W/kg; SAR(10 g) = 0.759 W/kg

Maximum value of SAR (measured) = 1.53 W/kg

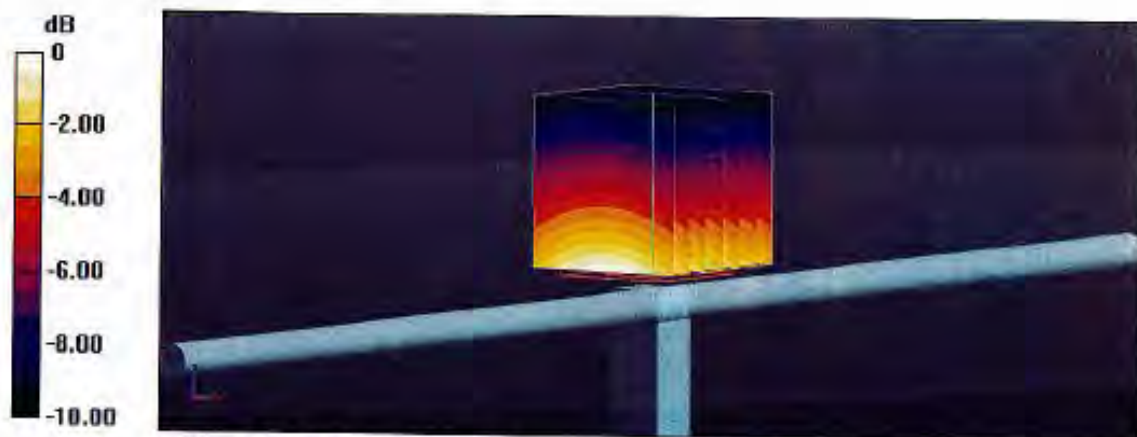

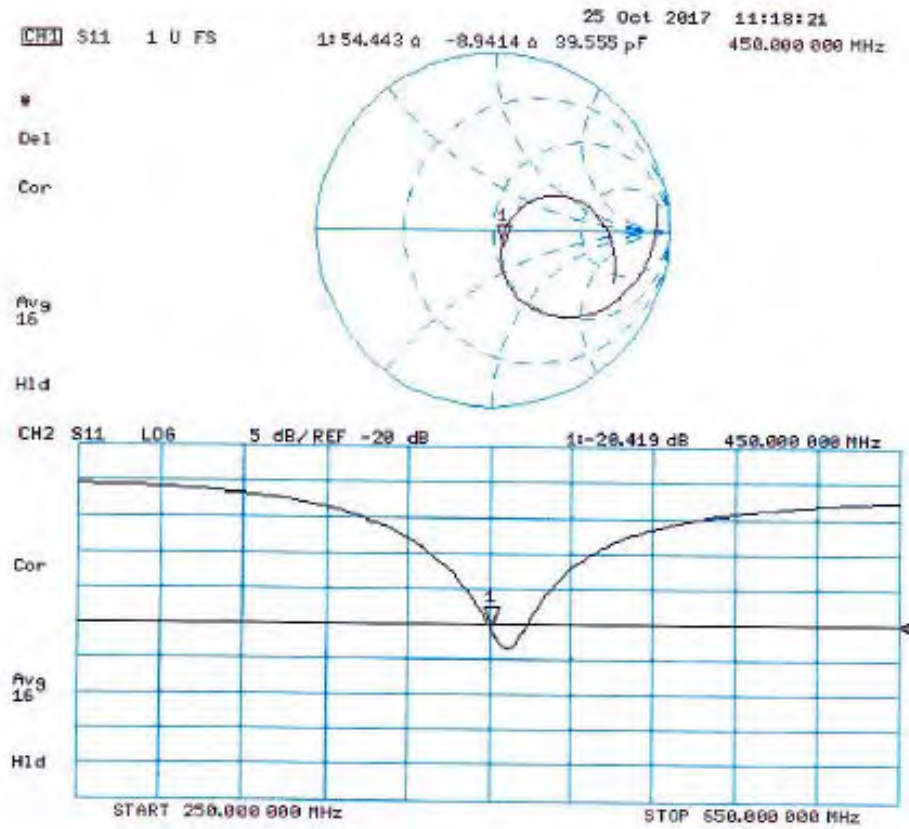Impedance Measurement Plot for Body TSL

Dipole Data

As stated in KDB 865664, only dipoles used for longer calibration intervals required to provide supporting information and measurement to qualify for extended calibration interval.

Dipole D450V3 (serial number 1054) do not exceed annual calibration date, therefore further justification and validation for impedance and return loss are not required.

Appendix D

SAR Summary Results Table for FCC review

Table D.1 462.5500 – 462.7250 MHz SAR Summary Result

Table #	Body / Head / Face	Antenna No.	Battery No.	Body Worn No.	Audio No.	Front / Back	Freq.
							462.6375
18	Body	1	1	1	1	Back	0.94
18	Body	1	2	1	1	Back	0.78
18	Body	1	3	1	1	Back	0.93
19	Body	1	1	2	1	Back	0.84
19	Body	1	2	2	1	Back	0.90
19	Body	1	3	2	1	Back	0.73
20	Body	1	1	3	1	Back	0.96
20	Body	1	2	3	1	Back	0.98
20	Body	1	3	3	1	Back	0.97
21	Body	1	2	3	2	Back	0.92
21	Body	1	2	3	3	Back	1.04
21	Body	1	2	3	4	Back	0.86
21	Body	1	2	3	5	Back	0.95
21	Body	1	2	3	6	Back	0.94
23	Face	1	1	None	None	Front	0.89
23	Face	1	2	None	None	Front	0.94
23	Face	1	3	None	None	Front	0.89

Table D.2 467.5625-467.7125 MHz SAR Summary Result

Table #	Body / Head / Face	Antenna No.	Battery No.	Body Worn No.	Audio No.	Front / Back	Freq.
							467.6375
25	Body	1	1	1	1	Back	0.48
25	Body	1	2	1	1	Back	0.47
25	Body	1	3	1	1	Back	0.47
26	Body	1	1	2	1	Back	0.41
26	Body	1	2	2	1	Back	0.44
26	Body	1	3	2	1	Back	0.29
27	Body	1	1	3	1	Back	0.45
27	Body	1	2	3	1	Back	0.54
27	Body	1	3	3	1	Back	0.39
29	Face	1	1	None	None	Front	0.44
29	Face	1	2	None	None	Front	0.35
29	Face	1	3	None	None	Front	0.50