



MOTOROLA SOLUTIONS

MS ISO/IEC 17025
TESTING
SAMM No. 0826

CERTIFICATE 2518.05

DECLARATION OF COMPLIANCE SAR ASSESSMENT Part 1 of 2

Motorola Solutions Inc.
EME Test Laboratory
 Motorola Solutions Malaysia Sdn Bhd
 Plot 2A, Medan Bayan Lepas,
 Mukim 12 SWD 11900 Bayan Lepas Penang, Malaysia.

Date of Report: 07/27/2020
Report Revision: D

Responsible Engineer: Ch'ng Jian Sheng (EME Engineer)
Report Author: Lee Kin Kting (Senior Technician)
Date/s Tested: 5/22/2020 - 5/26/2020, 06/03/2020, 06/17/2020, 06/19/2020
Manufacturer: Motorola Solutions Inc.
DUT Description: Tanapa T270 FRS Consumer Radio 462-467MHz Blue
Test TX mode(s): CW (PTT)
Max. Power output: 1.20W (462.5500 MHz - 462.7250 MHz),
 0.60W (467.5625 MHz - 467.7125 MHz)
Nominal Power: 1.00W (462.5500 MHz - 462.7250 MHz),
 0.53W (467.5625 MHz - 467.7125 MHz)
Tx Frequency Bands: 462.5500 MHz - 462.7250 MHz , 467.5625 MHz - 467.7125 MHz
Signaling type: FM
Model(s) Tested: T27X (PMUE5688A)
Model(s) Certified: T27X (PMUE5695A)
Serial Number(s): 16510WK0601, 16510WK0602
Classification: General Population/Uncontrolled Environment
Applicant name: Motorola Solutions Inc.
Applicant address: 8000 West Sunrise Boulevard, Fort Lauderdale, Florida 33322
FCC ID: AZ489FT4961
IC: 109U-89FT4961
ISED Test Site registration: 24843
FCC Test Firm Registration Number: 823256

The test results clearly demonstrate compliance with FCC General Population / Uncontrolled RF Exposure limits of 1.6 W/kg averaged over 1 gram per the requirements of FCC 47 CFR § 2.1093 and RSS-102 (Issue 5).

Based on the information and the testing results provided herein, the undersigned certifies that when used as stated in the operating instructions supplied, said product complies with the national and international reference standards and guidelines listed in section 4.0 of this report (no deviation from standard methods). This report shall not be reproduced without written approval from an officially designated representative of the Motorola Solutions Inc EME Laboratory.

I attest to the accuracy of the data and assume full responsibility for the completeness of these measurements. This reporting format is consistent with the suggested guidelines of the TIA TSB-150 December 2004. The results and statements contained in this report pertain only to the device(s) evaluated.

Tiong Nguk Ing

Deputy Technical Manager (Approved Signatory)

Approval Date: 07/27/2020

Part 1 of 2

1.0	Introduction.....	4
2.0	FCC SAR Summary.....	4
3.0	Abbreviations / Definitions.....	4
4.0	Referenced Standards and Guidelines	5
5.0	SAR Limits	6
6.0	Description of Device Under Test (DUT)	6
7.0	Optional Accessories and Test Criteria	7
7.1	Antenna.....	7
7.2	Batteries	7
7.3	Body worn Accessories	7
7.4	Audio Accessories	8
8.0	Description of Test System.....	9
8.1	Descriptions of Robotics/Probes/Readout Electronics	9
8.2	Description of Phantom(s)	10
8.3	Description of Simulated Tissue.....	10
9.0	Additional Test Equipment.....	11
10.0	SAR Measurement System Validation and Verification	12
10.1	System Validation.....	12
10.2	System Verification	12
10.3	Equivalent Tissue Test Results	13
11.0	Environmental Test Conditions	14
12.0	DUT Test Setup and Methodology.....	14
12.1	Measurements	14
12.2	DUT Configuration(s)	15
12.3	DUT Positioning Procedures	15
12.3.1	Body.....	15
12.3.2	Head.....	15
12.3.3	Face.....	15
12.4	DUT Test Channels	16
12.5	SAR Result Scaling Methodology.....	16
12.6	DUT Test Plan	16
13.0	DUT Test Data.....	17
13.1	Assessment at the Body for 462.5500 MHz – 462.7250 MHz band	17
13.2	Assessment at the Face for 462.5500 MHz – 462.7250 MHz band	19
13.3	Assessment at the Body for 467.5625 MHz - 467.7125 MHz band.....	20
13.4	Assessment at the Face for 467.5625 MHz - 467.7125 MHz band.....	22
13.5	Shortened Scan Assessment	22
14.0	Results Summary	23
15.0	Variability Assessment	23
16.0	System Uncertainty.....	23

APPENDICES

A	Measurement Uncertainty Budget	24
B	Probe Calibration Certificates.....	27
C	Dipole Calibration Certificates	45

Part 2 of 2**APPENDICES**

D	System Verification Check Scans.....	2
E	DUT Scans	4
F	Shorten Scan of Highest SAR Configuration	7
G	DUT Test Position Photos	10
H	DUT, Body worn and audio accessories Photos.....	11

Report Revision History

Date	Revision	Comments
06/10/2020	A	Initial release
07/01/2020	B	Updates Antenna Gain
07/16/2020	C	Updates Radio Model, removed T210 series
07/27/2020	D	Updates antenna description to include VHF weather frequency range.

1.0 Introduction

This report details the utilization, test setup, test equipment, and test results of the Specific Absorption Rate (SAR) measurements performed at the Motorola Solutions Inc. EME Test Laboratory for handheld portable model number T27X (PMUE5688A). This device is classified as General Population/Uncontrolled.

2.0 FCC SAR Summary

Table 1

Equipment Class	Frequency band (MHz)	Max Calc at Body (W/kg)	Max Calc at Face (W/kg)
		1g-SAR	1g-SAR
FRF	462.5500 - 462.7250	1.21	0.79
	467.5625 - 467.7125	0.45	0.49

3.0 Abbreviations / Definitions

CNR: Calibration Not Required

CW: Continuous Wave

DUT: Device Under Test

FRF: Part 95 Family Radio Face Held Transmitter

EME: Electromagnetic Energy

FM: Frequency Modulation

NA: Not Applicable

PTT: Push to Talk

SAR: Specific Absorption Rate

Body worn accessories: These accessories allow the DUT to be worn on the body of the user.

Maximum Power: Defined as the upper limit of the production line final test station.

4.0 Referenced Standards and Guidelines

This product is designed to comply with the following applicable national and international standards and guidelines.

- IEC62209-1 (2016) Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)
- Federal Communications Commission, "Evaluating Compliance with FCC Guidelines for Human Exposure to Radio frequency Electromagnetic Fields", OET Bulletin 65, FCC, Washington, D.C.: 1997.
- IEEE 1528 (2013), Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques
- American National Standards Institute (ANSI) / Institute of Electrical and Electronics Engineers (IEEE) C95. 1-1992
- Institute of Electrical and Electronics Engineers (IEEE) C95.1-2005
- International Commission on Non-Ionizing Radiation Protection (ICNIRP) 1998
- Ministry of Health (Canada) Safety Code 6 (2015), Limits of Human Exposure to Radio frequency Electromagnetic Fields in the Frequency Range from 3 kHz to 300 GHz
- RSS-102 (Issue 5) – Radio Frequency (RF) Exposure Compliance of Radio communication Apparatus (All Frequency Bands)
- Australian Communications Authority Radio communications (Electromagnetic Radiation - Human Exposure) Standard (2014)
- ANATEL, Brazil Regulatory Authority, Resolution No. 303 of July 2, 2002 "Regulation of the limitation of exposure to electrical, magnetic, and electromagnetic fields in the radio frequency range between 9 kHz and 300 GHz." and "Attachment to resolution # 303 from July 2, 2002"
- IEC62209-2 Edition 1.0 2010-03, Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices – Human models, instrumentation, and procedures – Part 2: Procedure to determine the specific absorption rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz).
- FCC KDB – 643646 D01 SAR Test for PTT Radios v01r03
- FCC KDB – 865664 D01 SAR Measurement 100 MHz to 6 GHz v01r04
- FCC KDB – 865664 D02 RF Exposure Reporting v01r02
- FCC KDB – 447498 D01 General RF Exposure Guidance v06

5.0 SAR Limits

Table 2

EXPOSURE LIMITS	SAR (W/kg)	
	(General Population / Uncontrolled Exposure Environment)	(Occupational / Controlled Exposure Environment)
Spatial Average - ANSI - (averaged over the whole body)	0.08	0.4
Spatial Peak - ANSI - (averaged over any 1-g of tissue)	1.6	8.0
Spatial Peak – ICNIRP/ANSI - (hands/wrists/feet/ankles averaged over 10-g)	4.0	20.0
Spatial Peak - ICNIRP - (Head and Trunk 10-g)	2.0	10.0

6.0 Description of Device Under Test (DUT)

This device operates in a half duplex system. A half duplex system only allows the user to transmit or receive. This device cannot transmit and receive simultaneously. The user must stop transmitting in order to receive a signal or listen for a response, regardless of PTT button or use of voice activated audio accessories. This type of operation, along with the RF safety booklet, which instructs the user to transmit no more than 50% of the time, justifies the use of 50% duty factor for this device.

Table 3 below summarizes the bands, maximum duty cycles and maximum output powers. Maximum output powers are defined as upper limit of the production line final test station.

Table 3

Band (MHz)	Duty Cycle (%)	Max Power (W)
467.5625 - 467.7125	*50	0.60
462.5500 - 462.7250		1.20

Note - * includes 50% PTT operation

The intended operating positions are “at the face” with the DUT at least 1 inch (2.5cm) from the mouth. Body worn audio and PTT operation is accomplished by means of optional remote accessories that are connected to the radio.

7.0 Optional Accessories and Test Criteria

This device is offered with optional accessories. All accessories were individually evaluated during the test plan creation to determine if testing was required per the guidelines outlined in 4.0 to assess compliance of the device.

7.1 Antenna

There is one fixed antenna offered for this product. The table below lists its descriptions.

Table 4

Antenna No.	Antenna Models	Description	Selected for test	Tested
1	Fixed Antenna	Fixed, 160-170 MHz/ 460-470MHz ,1/2 wave, 1.45 dBi	Yes	Yes

7.2 Batteries

There is one battery offered for this product. The table below lists its descriptions.

Table 5

Battery No.	Battery Models	Description	Selected for test	Tested	Comments
1	1532	1300mAh 3xAA NiMH Rechargeable Battery Pack	Yes	Yes	
2	AA Alkaline	3xAA Alkaline individual batteries	Yes	Yes	
3	PMNN4477A	800 mAh 3xAA NiMH Rechargeable Battery Pack	Yes	Yes	

7.3 Body worn Accessories

All body worn accessories were considered. The Table below lists the body worn accessories, and body worn accessory descriptions.

Table 6

Body worn No.	Body worn Models	Description	Selected for test	Tested	Comments
1	1564028V01 (PMLN7438A)	TLKR- T3 T40 T50 T60 XTB Belt Clip	Yes	Yes	
2	42015005001	Carry Lanyard	Yes	Yes	
3	PMLN7706A (PMLN7706AR)	Carry Pouch	Yes	Yes	

7.4 Audio Accessories

All audio accessories were considered. The Table below lists the offered audio accessories and their descriptions. Exhibit 7B illustrates photos of the tested audio accessories.

Table 7

Audio No.	Audio Models	Description	Selected for test	Tested	Comments
1	GU7140A (1884)	Wired PTT button + Headset with Boom Microphone Bundle	Yes	Yes	Default Audio
2	NTN8868C (53725C)	Headset w/Swivel Boom Microphone	Yes	Yes	
3	NTN8870D (53727B)	Ear bud W/Push-to-Talk Microphone	Yes	Yes	
4	PMLN7251A	Ear bud with PTT Microphone	Yes	Yes	
5	NTN8867A (53724C)	Single Pin Remote Speaker Microphone	Yes	Yes	
6	IXTN4022A	Single Pin Surveillance Earpiece	Yes	Yes	
7	PMLN7705A (PMLN7705AR)	Single Pin Throat Mic With PTT/VOX	Yes	Yes	
8	NTN9396B (56320B)	Earpiece w/Boom Microphone	Yes	No	By similarity to NTN8868C (53725C)
9	IXTN4011A (IXTN4011AR)	Single Pin Earpiece With BOOM MIC/VOX	Yes	No	By similarity to NTN8870D (53727B)
10	GU6443A(1518)	Surveillance Headset (1518)	Yes	No	By similarity to IXTN4022A

8.0 Description of Test System



8.1 Descriptions of Robotics/Probes/Readout Electronics

Table 8

Dosimetric System type	System version	DAE type	Probe Type
Schmid & Partner Engineering AG SPEAG DASY 5	52.10.2.1495	DAE4	EX3DV4 (E-Field)

The DASY5™ system is operated per the instructions in the DASY5™ Users Manual. The complete manual is available directly from SPEAG™. All measurement equipment used to assess SAR compliance was calibrated according to ISO/IEC 17025 A2LA guidelines. Section 9.0 presents additional test equipment information. Appendices B and C present the applicable calibration certificates. The E-field probe first scans a coarse grid over a large area inside the phantom in order to locate the interpolated maximum SAR distribution. After the coarse scan measurement, the probe is automatically moved to a position at the interpolated maximum. The subsequent scan can directly use this position as reference for the cube evaluations.

8.2 Description of Phantom(s)

Table 9

Phantom Type	Phantom(s) Used	Material Parameters	Phantom Dimensions LxWxD (mm)	Material Thickness (mm)	Support Structure Material	Loss Tangent (wood)
Triple Flat	NA	200MHz -6GHz; Er = 3-5, Loss Tangent = ≤ 0.05	280x175x175	2mm +/- 0.2mm	Wood	< 0.05
SAM	NA	300MHz -6GHz; Er = < 5, Loss Tangent = ≤ 0.05	Human Model			
Oval Flat	✓	300MHz -6GHz; Er = 4+/- 1, Loss Tangent = ≤ 0.05	600x400x190			

8.3 Description of Simulated Tissue

The sugar based simulate tissue is produced by placing the correct measured amount of De-ionized water into a large container. Each of the dried ingredients are weighed and added to the water carefully to avoid clumping. If the solution has a high sugar concentration the water is pre-heated to aid in dissolving the ingredients.

The simulated tissue mixture was mixed based on the Simulated Tissue Composition indicated in Table 10. During the daily testing of this product, the applicable mixture was used to measure the Di-electric parameters at each of the tested frequencies to verify that the Di-electric parameters were within the tolerance of the tissue specifications.

Simulated Tissue Composition (percent by mass)

Table 10

Ingredients	450MHz
Sugar	56.0
Diacetin	0
De ionized -Water	39.10
Salt	3.80
HEC	1.0
Bact.	0.1

9.0 Additional Test Equipment

The Table below lists additional test equipment used during the SAR assessment.

Table 11

Equipment Type	Model Number	Serial Number	Calibration Date	Calibration Due Date
Speag Probe	EX3DV4	7534	07/25/2019	07/25/2020
Speag DAE	DAE4	374	07/17/2019	07/17/2020
Speag Probe	EX3DV4	7511	10/24/2019	10/24/2020
Speag DAE	DAE4	729	10/16/2019	10/16/2020
Amplifier Power	10W1000C	312859	CNR	CNR
Amplifier Power	50W 1000A	14715	CNR	CNR
Power Meter	E4416A	MY50001037	08/30/2019	08/30/2021
Power Meter	E4418B	MY45107917	07/01/2019	07/01/2021
Power Sensor	E9301B	MY50280001	04/22/2020	04/22/2021
Power Sensor	E9301B	MY55210006	04/22/2020	04/22/2021
Power Meter	E4419B	MY45103725	6/10/2019	6/10/2021
Power Meter	E4418B	MY45100911	8/30/2019	8/30/2021
Power Meter	E4418B	MY45100739	12/09/2019	12/09/2020
Power Sensor	8481B	MY41091243	12/17/2019	12/17/2020
Power Sensor	E4412A	US38488023	4/23/2020	4/23/2021
Power Sensor	8481B	3318A10982	2/5/2020	2/5/2021
Bi-Directional Coupler	3020A	41931	07/11/2019	07/11/2020
Bi-Directional Coupler	3020A	40295	9/12/2019	9/12/2020
Vector Signal Generator	E4438C	MY47272101	10/29/2019	10/29/2021
Vector Signal Generator	E4438C	MY42081753	9/5/2019	9/5/2021
Temperature & Humidity Logger	DSB	16326820	11/25/2019	11/25/2020
Temperature Probe	80PK-22	5032017	12/24/2019	12/24/2020
Temperature Probe	PR-10-3-100-1/4-6-E	WNWR020579	7/6/2019	7/6/2020
Thermometer	HH202A	35881	12/24/2019	12/24/2020
Dielectric Assessment Kit	DAK-3.5	1120	07/11/2019	07/11/2020
Network Analyzer	E5071B	MY42403218	09/13/2019	09/13/2020
Speag Dipole	450V3	1054	03/11/2019	03/11/2021
Speag Dipole	450V3	1053	10/19/2018	10/19/2020

10.0 SAR Measurement System Validation and Verification

DASY output files of the probe/dipole calibration certificates and system verification test results are included in appendices B, C & D respectively.

10.1 System Validation

The SAR measurement system was validated according to procedures in KDB 865664. The validation status summary Table is below.

Table 12

Dates	Probe Calibration Point	Probe SN	Measured Tissue Parameters		Validation		
			σ	ϵ_r	Sensitivity	Linearity	Isotropy
CW							
09/13/2019	Head	450	7534	0.91	44.8	Pass	Pass
11/26/2019	Head	450	7511	0.89	42.3	Pass	Pass

10.2 System Verification

System verification checks were conducted each day during the SAR assessment. The results are normalized to 1W. Appendix D includes DASY plots for each day during the SAR assessment. The Table below summarizes the daily system check results used for the SAR assessment.

Table 13

Probe Serial #	Tissue Type	Dipole Kit / Serial #	Ref SAR @ 1W (W/kg)	System Check Results Measured (W/kg)	System Check Test Results when normalized to 1W (W/kg)	Tested Date
7534	IEEE/IEC	SPEAG D450V3 / 1054	4.57 +/- 10%	1.10	4.40	05/22/2020#
				1.13	4.52	05/24/2020#
				1.12	4.48	05/25/2020#
				1.15	4.60	05/26/2020
		7511	4.57 +/- 10%	1.08	4.32	06/03/2020
		1.10	4.40	06/17/2020		
		1.14	4.56	06/19/2020		

Note: # System verification covered next test day (within 24 hours)

10.3 Equivalent Tissue Test Results

Simulated tissue prepared for SAR measurements is measured daily and within 24 hours prior to actual SAR testing to verify that the tissue is within +/- 5% of target parameters at the center of the transmit band. This measurement is done using the applicable equipment indicated in section 9.0. The Table below summarizes the measured tissue parameters used for the SAR assessment.

Table 14

Frequency (MHz)	Tissue Type	Conductivity Target (S/m)	Dielectric Constant Target	Conductivity Meas. (S/m)	Dielectric Constant Meas.	Tested Date
450	IEEE/IEC	0.87 (0.83-0.91)	43.5 (41.3-45.7)	0.90	42.9	05/22/2020#
				0.85	41.9	05/24/2020#
				0.85	42.2	05/25/2020#
				0.84	41.7	05/26/2020
				0.89	42.0	06/03/2020
				0.89	43.1	06/17/2020
				0.87	42.2	06/19/2020
463		0.87 (0.83-0.91)	43.4 (41.3-45.6)	0.91	42.6	05/22/2020#
				0.86	41.6	05/24/2020
				0.85	41.4	05/26/2020
				0.88	42.2	06/19/2020
468		0.87 (0.83-0.91)	43.4 (41.2-45.6)	0.87	41.8	05/25/2020#
				0.90	41.7	06/03/2020
				0.91	42.7	06/17/2020

Note: # tissue date covered for next test day (within 24 hours)

11.0 Environmental Test Conditions

The EME Laboratory's ambient environment is well controlled resulting in very stable simulated tissue temperature and therefore stable dielectric properties. Simulated tissue temperature is measured prior to each scan to insure it is within +/- 2°C of the temperature at which the dielectric properties were determined. The liquid depth within the phantom used for measurements was at least 15cm. Additional precautions are routinely taken to ensure the stability of the simulated tissue such as covering the phantoms when scans are not actively in process in order to minimize evaporation. The lab environment is continuously monitored. The Table below presents the range and average environmental conditions during the SAR tests reported herein:

Table 15

	Target	Measured
Ambient Temperature	18 – 25 °C	Range: 21.7 – 23.5°C Avg. 22.6 °C
Tissue Temperature	18 – 25 °C	Range: 20.5-22.8°C Avg. 21.3°C

Relative humidity target range is a recommended target

The EME Lab RF environment uses a Spectrum Analyzer to monitor for extraneous large signal RF contaminants that could possibly affect the test results. If such unwanted signals are discovered the SAR scans are repeated.

12.0 DUT Test Setup and Methodology

12.1 Measurements

SAR measurements were performed using the DASY system described in section 8.0 using zoom scans. Oval flat phantoms filled with applicable simulated tissue were used for face testing.

The Table below includes the step sizes and resolution of area and zoom scans per KDB 865664 requirements.

Table 16

Description	$\leq 3 \text{ GHz}$	$> 3 \text{ GHz}$
Maximum distance from closest measurement point (geometric center of probe sensors) to phantom surface	$5 \pm 1 \text{ mm}$	$\frac{1}{2} \cdot \delta \cdot \ln(2) \pm 0.5 \text{ mm}$
Maximum probe angle from probe axis to phantom surface normal at the measurement location	$30^\circ \pm 1^\circ$	$20^\circ \pm 1^\circ$
	$\leq 2 \text{ GHz}: \leq 15 \text{ mm}$ $2 - 3 \text{ GHz}: \leq 12 \text{ mm}$	$3 - 4 \text{ GHz}: \leq 12 \text{ mm}$ $4 - 6 \text{ GHz}: \leq 10 \text{ mm}$
Maximum area scan spatial resolution: $\Delta x_{\text{Area}}, \Delta y_{\text{Area}}$	When the x or y dimension of the test device, in the measurement plane orientation, is smaller than the above, the measurement resolution must be \leq the corresponding x or y dimension of the test device with at least one measurement point on the test device.	
Maximum zoom scan spatial resolution: $\Delta x_{\text{Zoom}}, \Delta y_{\text{Zoom}}$	$\leq 2 \text{ GHz}: \leq 8 \text{ mm}$ $2 - 3 \text{ GHz}: \leq 5 \text{ mm}^*$	$3 - 4 \text{ GHz}: \leq 5 \text{ mm}^*$ $4 - 6 \text{ GHz}: \leq 4 \text{ mm}^*$
Maximum zoom scan spatial resolution, normal to phantom surface	$\leq 5 \text{ mm}$	$3 - 4 \text{ GHz}: \leq 4 \text{ mm}$ $4 - 5 \text{ GHz}: \leq 3 \text{ mm}$ $5 - 6 \text{ GHz}: \leq 2 \text{ mm}$
Note: δ is the penetration depth of a plane-wave at normal incidence to the tissue medium; see draft standard IEEE P1528-2011 for details.		
* When zoom scan is required and the reported SAR from the area scan based 1-g SAR estimation procedures of KDB 447498 is $\leq 1.4 \text{ W/kg}$, $\leq 8 \text{ mm}$, $\leq 7 \text{ mm}$ and $\leq 5 \text{ mm}$ zoom scan resolution may be applied, respectively, for 2 GHz to 3 GHz, 3 GHz to 4 GHz and 4 GHz to 6 GHz.		

12.2 DUT Configuration(s)

The DUT is a portable device operational at the face as described in section 6.0 while using the applicable accessories listed in section 7.0. All accessories listed in section 7.0 of this report were considered when implementing the guidelines specified in KDB 643646.

12.3 DUT Positioning Procedures

The positioning of the device for each body location is described below and illustrated in Appendix G.

12.3.1 Body

The DUT was positioned in normal use configuration against the phantom with the offered body worn accessory as well as with the offered audio accessories as applicable.

12.3.2 Head

Not applicable.

12.3.3 Face

The DUT was positioned with its' front side separated 2.5cm from the phantom.

12.4 DUT Test Channels

The number of test channels was determined by using the following IEEE 1528 equation. The use of this equation produces the same or more test channels compared to the FCC KDB 447498 number of test channels formula.

$$N_c = 2 * \text{roundup}[10 * (f_{\text{high}} - f_{\text{low}}) / f_c] + 1$$

Where

N_c = Number of channels

F_{high} = Upper channel

F_{low} = Lower channel

F_c = Center channel

12.5 SAR Result Scaling Methodology

The calculated 1-gram averaged SAR results indicated as “Max Calc. 1g-SAR” in the data Tables is determined by scaling the measured SAR to account for power leveling variations and drift. Appendix F includes a shortened scan to justify SAR scaling for drift. For this device the “Max Calc. 1g-SAR” is scaled using the following formula:

$$\text{Max_Calc} = \text{SAR_meas} \cdot 10^{\frac{-\text{Drift}}{10}} \cdot \frac{P_{\text{max}}}{P_{\text{int}}} \cdot DC$$

P_{max} = Maximum Power (W)

P_{int} = Initial Power (W)

Drift = DASY drift results (dB)

SAR_meas = Measured 1-g or 10-g Avg. SAR (W/kg)

DC = Transmission mode duty cycle in % where applicable

50% duty cycle is applied for PTT operation

Note: for conservative results, the following are applied:

If $P_{\text{int}} > P_{\text{max}}$, then $P_{\text{max}}/P_{\text{int}} = 1$.

Drift = 1 for positive drift

Additional SAR scaling was applied using the methodologies outlined in FCC KDB 865664 using tissue sensitivity values. SAR was scaled for conditions where the tissue permittivity was measured above the nominal target and for tissue conductivity that was measured below the nominal target. Negative or reduced SAR scaling is not permitted.

12.6 DUT Test Plan

The guidelines and requirements outlined in section 4.0 were used to assess compliance of this device. All modes of operation identified in section 6.0 were considered during the development of the test plan. All tests were performed in CW modes and 50% duty cycle was applied to PTT configurations in the final results.

13.0 DUT Test Data

13.1 Assessment at the Body for 462.5500 MHz – 462.7250 MHz band

Conducted power measurements for channel within FCC allocated frequency range 462.5500 - 462.7250 MHz was measured and listed in Table 17.

Table 17

Test Freq: 462.625 (MHz)	
Battery	Power (W)
PMNN4477A	1.12
AA Alkaline	1.18
1532	1.09

Assessments at the Body with belt clip 1564028V01

DUT assessment with the fixed antenna, batteries and above mentioned body worn accessory. SAR plots of the highest results per Table 18 (bolded) are presented in Appendix E.

Table 18

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
Fixed antenna	PMNN4477A	1564028V01	GU7140A (1884)	462.625	1.12	-0.73	1.72	1.09	BL-AB-200522-11
	AA Alkaline				1.18	-0.65	1.55	0.92	BL-AB-200522-12
	1532				1.09	-0.32	1.82	1.08	BL-AB-200522-13

Assessments at the Body Carry Lanyard 42015005001

DUT assessment with the fixed antenna, batteries and above mentioned body worn accessory. SAR plots of the highest results per Table 19 (bolded) are presented in Appendix E.

Table 19

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
Fixed antenna	PMNN4477A	42015005001	GU7140A (1884)	462.625	1.12	-0.51	1.90	1.14	BL-AB-200522-14
	AA Alkaline				1.18	-0.88	1.50	0.93	NZ-AB-200619-13
	1532				1.09	-0.67	1.88	1.21	BL-AB-200523-02#

Assessments at the Body Carry Pouch PMLN7706A

DUT assessment with the fixed antenna, batteries and above mentioned body worn accessory. SAR plots of the highest results per Table 20 (bolded) are presented in Appendix E.

Table 20

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
Fixed antenna	PMNN4477A	PMLN7706A	GU7140A (1884)	462.625	1.12	-0.50	1.09	0.66	BL-AB-200523-03#
	AA Alkaline				1.18	-0.79	1.14	0.70	BL-AB-200523-04#
	1532				1.09	-0.02	1.13	0.62	BL-AB-200523-05#

Assessment at the Body with other audio accessories

Assessment of additional audio accessories with the highest SAR results from table 18, 19 & 20. SAR plots of the highest results per Table 21 (bolded) are presented in Appendix E.

Table 21

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
Fixed antenna	1532	42015005001	NTN8868C (53725C)	462.625	1.09	-0.37	1.59	0.95	BL-AB-200524-02
			NTN8870D (53727B)			-0.54	1.51	0.94	BL-AB-200524-03
			PMLN7251A			-0.63	1.46	0.93	BL-AB-200524-04
			NTN8867A (53724C)			-0.53	1.63	1.01	BL-AB-200524-05
			IXTN4022A			-0.56	1.79	1.12	BL-AB-200524-06
			PMLN7705A (PMLN7705AR)			-0.81	1.75	1.16	BL-AB-200524-07

13.2 Assessment at the Face for 462.5500 MHz – 462.7250 MHz band

Conducted power measurements for channel within FCC allocated frequency range 462.5500 – 462.7250MHz was measured and listed in Table 22.

Table 22

Test Freq: 462.625 (MHz)	
Battery	Power (W)
PMNN4477A	1.12
AA Alkaline	1.18
1532	1.09

DUT assessment with fixed antenna and offered battery with front of DUT positioned 2.5cm facing Phantom per KDB 643646. SAR plot of the highest result per Table 23 (Bolded) are presented in Appendix E.

Table 23

Antenna	Battery	Carry Accessory	Cable Accessory	Test Fred (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
Fixed antenna	PMNN4477A	None	None	462.625	1.12	-0.91	1.13	0.75	BL-FACE-200524-08
	AA Alkaline				1.18	-0.73	1.26	0.76	BL-FACE-200524-09
	1532				1.09	-0.51	1.28	0.79	BL-FACE-200524-11

13.3 Assessment at the Body for 467.5625 MHz - 467.7125 MHz band

Conducted power measurements for channel within FCC allocated frequency range 467.5625 - 467.7125MHz was measured and listed in Table 24.

Table 24

Test Freq: 467.6375 (MHz)	
Battery	Power (W)
PMNN4477A	0.57
AA Alkaline	0.59
1532	0.53

Assessments at the Body with belt clip 1564028V01

DUT assessment with the fixed antenna, batteries and above mentioned body worn accessory. SAR plots of the highest results per Table 25 (bolded) are presented in Appendix E.

Table 25

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
Fixed antenna	PMNN4477A	1564028V01	GU7140A (1884)	467.6375	0.57	-0.63	0.68	0.42	BL-AB-200525-01#
	AA Alkaline				0.59	-0.59	0.51	0.30	BL-AB-200525-02#
	1532				0.53	-0.36	0.72	0.45	ZZ(MA)-AB-200617-12

Assessments at the Body Carry Lanyard 42015005001

DUT assessment with the fixed antenna, batteries and above mentioned body worn accessory. SAR plots of the highest results per Table 26 (bolded) are presented in Appendix E.

Table 26

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
Fixed antenna	PMNN4477A	42015005001	GU7140 A (1884)	467.6375	0.57	-0.43	0.59	0.34	BL-AB-200525-05
	AA Alkaline				0.59	-0.54	0.64	0.37	BL-AB-200525-06
	1532				0.53	-0.37	0.61	0.38	BL-AB-200525-07

Assessments at the Body Carry Pouch PMLN7706A

DUT assessment with the fixed antenna, batteries and above mentioned body worn accessory. SAR plots of the highest results per Table 27 (bolded) are presented in Appendix E.

Table 27

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
Fixed antenna	PMNN4477A	PMLN7706A	GU7140A (1884)	467.6375	0.57	-0.42	0.56	0.33	BL-AB-200525-08
	AA Alkaline				0.59	-0.56	0.48	0.28	BL-AB-200525-09
	1532				0.53	-0.47	0.56	0.35	BL-AB-200525-10

Assessment at the Body with other audio accessories

By adapting SAR thresholds to general population limits per “KDB 643646 Body SAR Test Consideration for Audio Accessories without Built-In Antenna”, SAR testing with other audio accessories not necessary as previous results in Tables 25, 26 and 27 shows highest result of < 0.8 W/kg, which is more than 3dB from the specification limit.

13.4 Assessment at the Face for 467.5625 MHz - 467.7125 MHz band

Conducted power measurements for channel within FCC allocated frequency range 467.5625 - 467.7125MHz was measured and listed in Table 28.

Table 28

Test Freq: 467.6375 (MHz)	
Battery	Power (W)
PMNN4477A	0.57
AA Alkaline	0.59
1532	0.53

DUT assessment with fixed antenna and offered battery with front of DUT positioned 2.5cm facing Phantom per KDB 643646. SAR plot of the result per Table 29 are presented in Appendix E.

Table 29

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
Fixed antenna	PMNN4477A	None	None	467.6375	0.57	-0.48	0.72	0.43	BL-FACE-200525-12
	AA Alkaline				0.59	-0.55	0.60	0.34	BL-FACE-200526-01#
	1532				0.53	-0.44	0.78	0.49	BL-FACE-200526-03#

13.5 Shortened Scan Assessment

A “shortened” scan using the highest SAR configuration overall from above was performed to validate the SAR drift of the full DASY5™ coarse and zoom scans. Note that the shortened scan represents the zoom scan performance result; this is obtained by first running a coarse scan to find the peak area and then, using a newly charged battery, a zoom scan was performed. The results of the shortened cube scan presented in Appendix F demonstrate that the scaling methodology used to determine the calculated SAR results presented herein are valid. The SAR result from the Table below is provided in Appendix F.

Table 30

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
Fixed	1532	42015005001	GU7140A (1884)	462.6250	1.09	-0.44	1.89	1.15	BL-AB-200526-06

14.0 Results Summary

Based on the test guidelines from section 4.0 and satisfying frequencies within FCC and ISED frequency band, the highest Operational Maximum Calculated 1-gram average SAR values found for this filing:

Table 22

Technologies	Frequency band (MHz)	Max Calc at Body (W/kg)	Max Calc at Face (W/kg)
		1g-SAR	1g-SAR
FM	462.5500 – 462.7250	1.21	0.79
FM	467.5625 – 467.7125	0.45	0.49

All results are scaled to the maximum output power.

The test results clearly demonstrate compliance with FCC General Population/ Uncontrolled RF Exposure limits of 1.6 W/kg averaged over 1 gram per the requirements of FCC 47 CFR § 2.1093 and RSS-102 (Issue 5).

15.0 Variability Assessment

Per the guidelines in KDB 865664 SAR variability assessment is required because SAR results are below 0.8W/kg (General population).

Run#	Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq. (MHz)	Adj Calc. 1g-SAR (W/kg)	Ratio	Comments
BL-AB-200523-02#	Fixed	1532	42015005001	GU7140A (1884)	462.6250	1.10	1.05	No additional repeated scans is required due to the Ratio (SAR_{high}/SAR_{low}) < 1.20
BL-AB-200526-06						1.05		

16.0 System Uncertainty

A system uncertainty analysis is not required for this report per KDB 865664 because the highest report SAR value for General Population is less than 1.5 W/kg.

Per the guidelines of ISO 17025 a reported system uncertainty is required and therefore measurement uncertainty budget is included in Appendix A.

Appendix A

Measurement Uncertainty Budget

Table A.1: Uncertainty Budget for Device Under Test for 450 MHz

<i>a</i>	<i>b</i>	<i>c</i>	<i>d</i>	<i>e = f(d,k)</i>	<i>f</i>	<i>g</i>	<i>h = c x f / e</i>	<i>i = c x g / e</i>	<i>k</i>
Uncertainty Component	IEEE 1528 section	Tol. ($\pm \%$)	Prob Dist	Div.	ci (1 g)	ci (10 g)	1 g u_i ($\pm \%$)	10 g u_i ($\pm \%$)	v_i
Measurement System									
Probe Calibration	E.2.1	6.7	N	1.00	1	1	6.7	6.7	∞
Axial Isotropy	E.2.2	4.7	R	1.73	0.707	0.707	1.9	1.9	∞
Hemispherical Isotropy	E.2.2	9.6	R	1.73	0.707	0.707	3.9	3.9	∞
Boundary Effect	E.2.3	1.0	R	1.73	1	1	0.6	0.6	∞
Linearity	E.2.4	4.7	R	1.73	1	1	2.7	2.7	∞
System Detection Limits	E.2.5	1.0	R	1.73	1	1	0.6	0.6	∞
Readout Electronics	E.2.6	0.3	N	1.00	1	1	0.3	0.3	∞
Response Time	E.2.7	1.1	R	1.73	1	1	0.6	0.6	∞
Integration Time	E.2.8	1.1	R	1.73	1	1	0.6	0.6	∞
RF Ambient Conditions - Noise	E.6.1	3.0	R	1.73	1	1	1.7	1.7	∞
RF Ambient Conditions - Reflections	E.6.1	0.0	R	1.73	1	1	0.0	0.0	∞
Probe Positioner Mech. Tolerance	E.6.2	0.4	R	1.73	1	1	0.2	0.2	∞
Probe Positioning w.r.t Phantom	E.6.3	1.4	R	1.73	1	1	0.8	0.8	∞
Max. SAR Evaluation (ext., int., avg.)	E.5	3.4	R	1.73	1	1	2.0	2.0	∞
Test sample Related									
Test Sample Positioning	E.4.2	3.2	N	1.00	1	1	3.2	3.2	29
Device Holder Uncertainty	E.4.1	4.0	N	1.00	1	1	4.0	4.0	8
SAR drift	6.6.2	5.0	R	1.73	1	1	2.9	2.9	∞
Phantom and Tissue Parameters									
Phantom Uncertainty	E.3.1	4.0	R	1.73	1	1	2.3	2.3	∞
Liquid Conductivity (target)	E.3.2	5.0	R	1.73	0.64	0.43	1.8	1.2	∞
Liquid Conductivity (measurement)	E.3.3	3.3	N	1.00	0.64	0.43	2.1	1.4	∞
Liquid Permittivity (target)	E.3.2	5.0	R	1.73	0.6	0.49	1.7	1.4	∞
Liquid Permittivity (measurement)	E.3.3	1.9	N	1.00	0.6	0.49	1.1	0.9	∞
Combined Standard Uncertainty									
Expanded Uncertainty (95% CONFIDENCE LEVEL)				RSS			11	11	477
				<i>k=2</i>			23	22	

Notes for uncertainty budget Tables:

- a) Column headings *a-k* are given for reference.
- b) Tol. - tolerance in influence quantity.
- c) Prob. Dist. – Probability distribution
- d) N, R - normal, rectangular probability distributions
- e) Div. - divisor used to translate tolerance into normally distributed standard uncertainty
- f) *ci* - sensitivity coefficient that should be applied to convert the variability of the uncertainty component into a variability of SAR.
- g) *ui* – SAR uncertainty
- h) *vi* - degrees of freedom for standard uncertainty and effective degrees of freedom for the expanded uncertainty

Table A.2: Uncertainty Budget for System Validation (dipole & flat phantom) for 450 MHz

<i>a</i>	<i>b</i>	<i>c</i>	<i>d</i>	<i>e = f(d,k)</i>	<i>f</i>	<i>g</i>	<i>h = c x f / e</i>	<i>i = c x g / e</i>	<i>k</i>
Uncertainty Component	IEEE 1528 section	Tol. ($\pm \%$)	Prob Dist	Div.	<i>c_i</i> (1 g)	<i>c_i</i> (10 g)	1 g U _i ($\pm \%$)	10 g U _i ($\pm \%$)	<i>v_i</i>
Measurement System									
Probe Calibration	E.2.1	6.7	N	1.00	1	1	6.7	6.7	∞
Axial Isotropy	E.2.2	4.7	R	1.73	1	1	2.7	2.7	∞
Spherical Isotropy	E.2.2	9.6	R	1.73	0	0	0.0	0.0	∞
Boundary Effect	E.2.3	1.0	R	1.73	1	1	0.6	0.6	∞
Linearity	E.2.4	4.7	R	1.73	1	1	2.7	2.7	∞
System Detection Limits	E.2.5	1.0	R	1.73	1	1	0.6	0.6	∞
Readout Electronics	E.2.6	0.3	N	1.00	1	1	0.3	0.3	∞
Response Time	E.2.7	1.1	R	1.73	1	1	0.6	0.6	∞
Integration Time	E.2.8	0.0	R	1.73	1	1	0.0	0.0	∞
RF Ambient Conditions - Noise	E.6.1	3.0	R	1.73	1	1	1.7	1.7	∞
RF Ambient Conditions - Reflections	E.6.1	0.0	R	1.73	1	1	0.0	0.0	∞
Probe Positioner Mechanical Tolerance	E.6.2	0.4	R	1.73	1	1	0.2	0.2	∞
Probe Positioning w.r.t. Phantom	E.6.3	1.4	R	1.73	1	1	0.8	0.8	∞
Max. SAR Evaluation (ext., int., avg.)	E.5	3.4	R	1.73	1	1	2.0	2.0	∞
Dipole									
Dipole Axis to Liquid Distance	8, E.4.2	2.0	R	1.73	1	1	1.2	1.2	∞
Input Power and SAR Drift Measurement	8, 6.6.2	5.0	R	1.73	1	1	2.9	2.9	∞
Phantom and Tissue Parameters									
Phantom Uncertainty	E.3.1	4.0	R	1.73	1	1	2.3	2.3	∞
Liquid Conductivity (target)	E.3.2	5.0	R	1.73	0.64	0.43	1.8	1.2	∞
Liquid Conductivity (measurement)	E.3.3	3.3	R	1.73	0.64	0.43	1.2	0.8	∞
Liquid Permittivity (target)	E.3.2	5.0	R	1.73	0.6	0.49	1.7	1.4	∞
Liquid Permittivity (measurement)	E.3.3	1.9	R	1.73	0.6	0.49	0.6	0.5	∞
Combined Standard Uncertainty									
Expanded Uncertainty (95% CONFIDENCE LEVEL)									
				RSS			10	9	99999
				<i>k=2</i>			19	18	

Notes for uncertainty budget Tables:

- a) Column headings *a-k* are given for reference.
- b) Tol. - tolerance in influence quantity.
- c) Prob. Dist. – Probability distribution
- d) N, R - normal, rectangular probability distributions
- e) Div. - divisor used to translate tolerance into normally distributed standard uncertainty
- f) *c_i* - sensitivity coefficient that should be applied to convert the variability of the uncertainty component into a variability of SAR.
- g) *ui* – SAR uncertainty
- h) *vi* - degrees of freedom for standard uncertainty and effective degrees of freedom for the expanded uncertainty

Appendix B

Probe Calibration Certificates

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Motorola Solutions MY**

Certificate No: **EX3-7534_Jul19**

CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:7534**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v5, QA CAL-23.v5,
QA CAL-25.v7**
Calibration procedure for dosimetric E-field probes

Calibration date: **July 25, 2019**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	03-Apr-19 (No. 217-02892/02893)	Apr-20
Power sensor NRP-Z91	SN: 103244	03-Apr-19 (No. 217-02892)	Apr-20
Power sensor NRP-Z91	SN: 103245	03-Apr-19 (No. 217-02893)	Apr-20
Reference 20 dB Attenuator	SN: S5277 (20x)	04-Apr-19 (No. 217-02894)	Apr-20
DAE4	SN: 660	19-Dec-18 (No. DAE4-660_Dec18)	Dec-19
Reference Probe ES3DV2	SN: 3013	31-Dec-16 (No. ES3-3013_Dec18)	Dec-19
<hr/>			
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	05-Apr-16 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: MY41498067	05-Apr-16 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: 000110210	05-Apr-16 (in house check Jun-18)	In house check: Jun-20
RF generator HP 8641C	SN: US3642U01700	04-Aug-99 (in house check Jun-18)	In house check: Jun-20
Network Analyzer E8358A	SN: US41060477	31-Mar-14 (in house check Oct-18)	In house check: Oct-19

Calibrated by:	Name Manu Seitz	Function Laboratory Technician	Signature
Approved by:	Katja Pokovic	Technical Manager	

Issued: July 25, 2019

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization β	β rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\beta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, ", "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- $NORM_{x,y,z}$: Assessed for E-field polarization $\beta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). $NORM_{x,y,z}$ are only intermediate values, i.e., the uncertainties of $NORM_{x,y,z}$ does not affect the E^2 -field uncertainty inside TSL (see below ConvF).
- $NORM(f)x,y,z = NORM_{x,y,z} * frequency_response$ (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- $DCPx,y,z$: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR : PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- $A_{x,y,z}$; $B_{x,y,z}$; $C_{x,y,z}$; $D_{x,y,z}$; $VR_{x,y,z}$; A , B , C , D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- $ConvF$ and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to $NORM_{x,y,z} * ConvF$ whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the $NORM_x$ (no uncertainty required).

EX3DV4 - SN:7534

July 25, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7534**Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ($\mu\text{V}/(\text{V/m})^2$) ^a	0.48	0.40	0.50	$\pm 10.1 \%$
DCP (mV) ^b	95.7	98.1	103.0	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Unc ^c (k=2)
0	CW	X	0.0	0.0	1.0	0.00	114.8	$\pm 2.5 \%$
		Y	0.0	0.0	1.0		141.6	
		Z	0.0	0.0	1.0		127.4	

Note: For details on UID parameters see Appendix

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^a The uncertainties of Norm X,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).^b Numerical linearization parameter: uncertainty not required.^c Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4- SN:7534

July 25, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7534**Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	85.3
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

EX3DV4- SN:7534

July 25, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7534**Calibration Parameter Determined in Head Tissue Simulating Media**

f (MHz) ^c	Relative Permittivity ^f	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ^g	Depth ^h (mm)	Unc (k=2)
150	52.3	0.76	13.79	13.79	13.79	0.00	1.00	± 13.3 %
300	45.3	0.87	12.60	12.60	12.60	0.08	1.20	± 13.3 %
450	43.5	0.87	11.59	11.59	11.59	0.12	1.30	± 13.3 %
750	41.9	0.89	10.17	10.17	10.17	0.35	1.04	± 12.0 %
835	41.5	0.90	9.90	9.90	9.90	0.49	0.83	± 12.0 %
900	41.5	0.97	9.84	9.84	9.84	0.49	0.80	± 12.0 %
1450	40.5	1.20	8.73	8.73	8.73	0.37	0.80	± 12.0 %
1810	40.0	1.40	8.13	8.13	8.13	0.34	0.88	± 12.0 %
1900	40.0	1.40	8.05	8.05	8.05	0.33	0.88	± 12.0 %
2100	39.8	1.49	8.04	8.04	8.04	0.33	0.85	± 12.0 %
2300	39.5	1.67	7.83	7.83	7.83	0.31	0.90	± 12.0 %
2450	39.2	1.80	7.58	7.58	7.58	0.36	0.90	± 12.0 %
2600	39.0	1.96	7.29	7.29	7.29	0.34	0.90	± 12.0 %
3500	37.9	2.91	6.61	6.61	6.61	0.30	1.30	± 13.1 %
3700	37.7	3.12	6.48	6.48	6.48	0.30	1.30	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 6 MHz is 4-9 MHz, and ConvF assessed at 13 MHz is 9-19 MHz. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^f At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^g AlphaDepth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4 - SN:7534

July 25, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7534**Calibration Parameter Determined in Body Tissue Simulating Media**

f (MHz) ^c	Relative Permittivity ^f	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ^g	Depth ^h (mm)	Unc (k=2)
150	61.9	0.80	13.36	13.36	13.36	0.00	1.00	± 13.3 %
300	58.2	0.92	12.35	12.35	12.35	0.03	1.20	± 13.3 %
450	56.7	0.94	11.87	11.87	11.87	0.06	1.30	± 13.3 %
750	55.5	0.96	10.23	10.23	10.23	0.42	0.89	± 12.0 %
835	55.2	0.97	10.04	10.04	10.04	0.47	0.80	± 12.0 %
900	55.0	1.05	9.80	9.80	9.80	0.49	0.80	± 12.0 %
1450	54.0	1.30	8.59	8.59	8.59	0.33	0.80	± 12.0 %
1810	53.3	1.52	8.16	8.16	8.16	0.42	0.88	± 12.0 %
1900	53.3	1.52	7.95	7.95	7.95	0.36	0.88	± 12.0 %
2100	53.2	1.62	7.93	7.93	7.93	0.36	0.85	± 12.0 %
2300	52.9	1.81	7.88	7.88	7.88	0.34	0.90	± 12.0 %
2450	52.7	1.95	7.68	7.68	7.68	0.33	0.90	± 12.0 %
2600	52.5	2.16	7.59	7.59	7.59	0.23	0.90	± 12.0 %
3500	51.3	3.31	6.37	6.37	6.37	0.40	1.30	± 13.1 %
3700	51.0	3.55	6.13	6.13	6.13	0.40	1.30	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 6 MHz is 4-9 MHz, and ConvF assessed at 13 MHz is 9-19 MHz. Above 5 GHz frequency validity can be extended to ± 110 MHz.

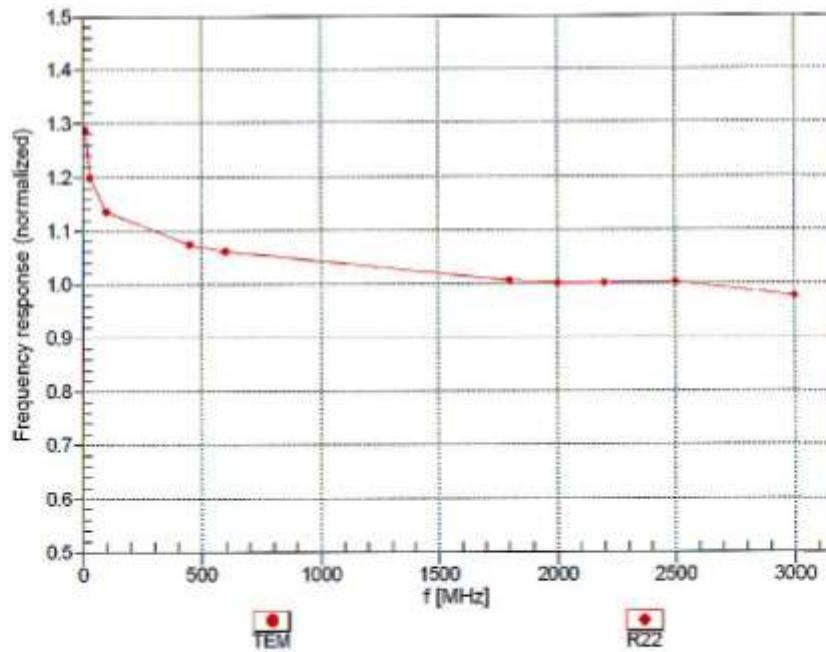
^f At frequencies below 3 GHz, the validity of tissue parameters (c and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (c and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^g Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:7534

July 25, 2019

Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

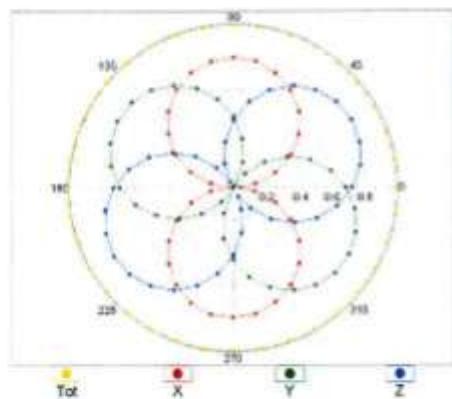
Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ ($k=2$)

EX3DV4- SN:7534

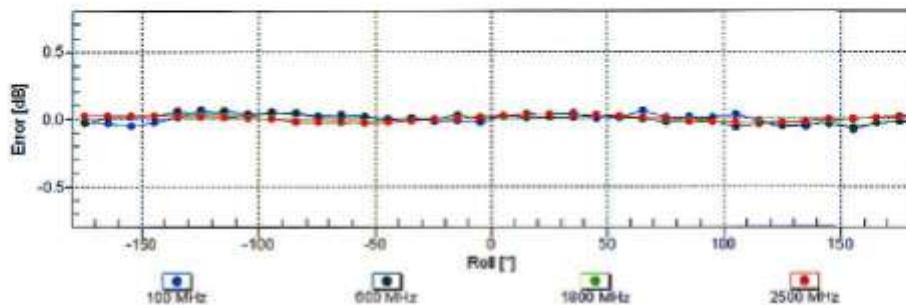
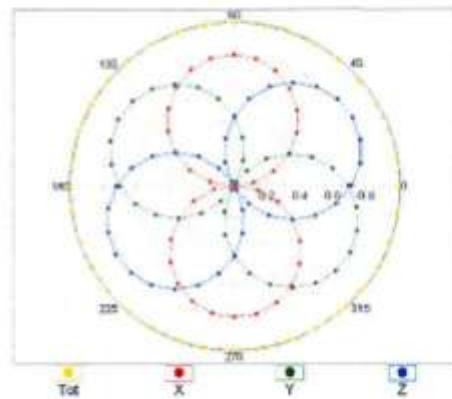
July 25, 2019

Receiving Pattern (ϕ), $\theta = 0^\circ$

f=600 MHz, TEM



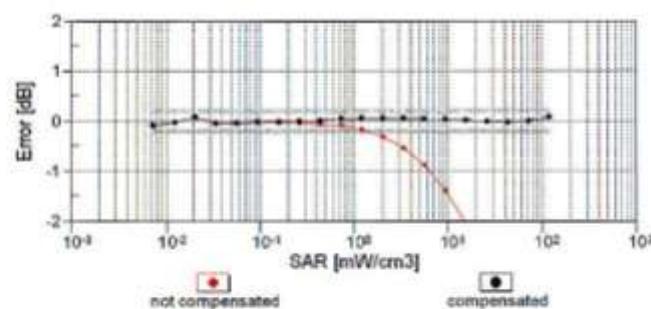
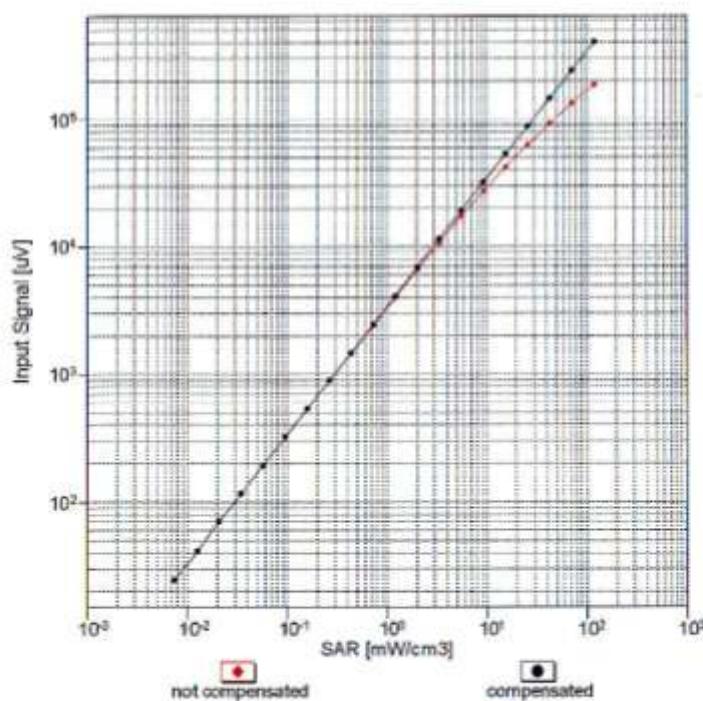
f=1800 MHz, R22

Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ (k=2)

EX3DV4- SN:7534

July 25, 2019

Dynamic Range f(SAR_{head})
(TEM cell , f_{eval}= 1900 MHz)

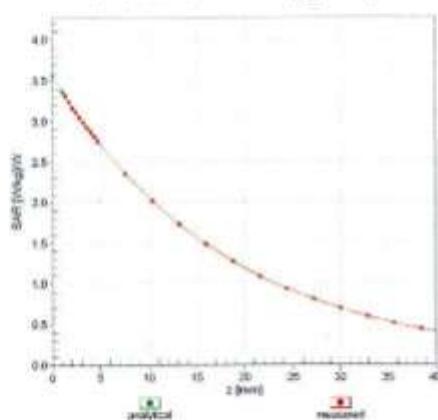
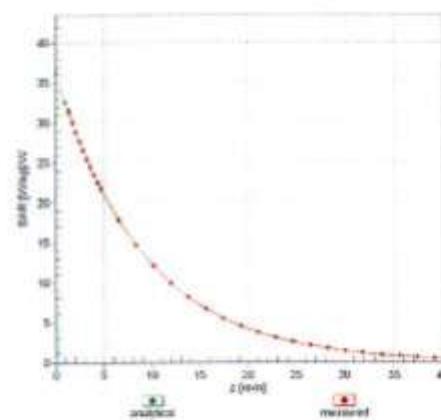


Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)


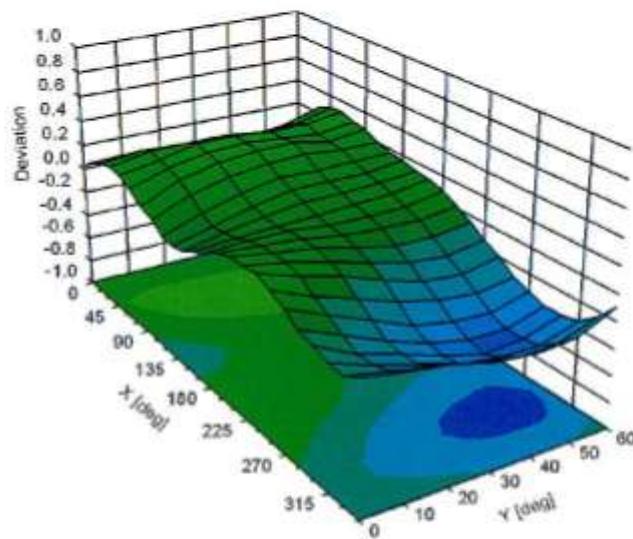
EX3DV4-SN:7534

July 25, 2019

Conversion Factor Assessment

 $f = 900 \text{ MHz}, \text{WG}LS R9 (H_convF)$  $f = 2450 \text{ MHz}, \text{WG}LS R22 (H_convF)$ 

Deviation from Isotropy in Liquid

Error (ϕ, θ), $f = 900 \text{ MHz}$ 

EX3DV4- SN:7534

July 25, 2019

Appendix: Modulation Calibration Parameters

UID	Communication System Name	A dB	B dB/ μ V	C	D dB	VR mV	Unc ^E (k=2)
0	CW	X 0.0	0.0	1.0	0.00	114.8	$\pm 2.5\%$
		Y 0.0	0.0	1.0		141.6	
		Z 0.0	0.0	1.0		127.4	
10011-CAB	UMTS-FDD (WCDMA)	X 3.14	64.9	17.0	2.91	123.6	$\pm 0.7\%$
		Y 2.93	64.5	17.1		110.4	
		Z 3.59	69.6	20.1		137.7	
10097-CAB	UMTS-FDD (HSDPA)	X 4.49	65.6	17.8	3.98	130.9	$\pm 0.9\%$
		Y 4.14	64.7	17.5		115.6	
		Z 4.74	68.2	19.6		146.7	
10098-CAB	UMTS-FDD (HSUPA, Subtest 2)	X 4.54	65.8	18.0	3.98	131.5	$\pm 0.9\%$
		Y 4.19	65.0	17.6		116.2	
		Z 4.73	68.1	19.5		146.4	
10100-CAE	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	X 6.37	66.8	19.2	5.67	138.6	$\pm 1.4\%$
		Y 5.80	65.1	18.3		120.5	
		Z 5.96	66.1	19.2		109.1	
10101-CAE	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM)	X 7.51	67.4	19.9	6.42	147.7	$\pm 1.7\%$
		Y 6.92	65.9	19.0		128.1	
		Z 7.01	66.6	19.6		115.7	
10108-CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X 6.24	66.4	19.2	5.80	135.8	$\pm 1.2\%$
		Y 5.70	64.9	18.4		118.3	
		Z 5.83	65.8	19.1		107.3	
10109-CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM)	X 7.25	67.2	19.9	6.43	143.2	$\pm 1.7\%$
		Y 6.64	65.6	18.9		123.8	
		Z 6.76	66.4	19.6		112.2	
10110-CAG	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, QPSK)	X 5.94	66.0	19.0	5.75	132.1	$\pm 1.2\%$
		Y 5.42	64.6	18.2		115.7	
		Z 5.97	67.3	20.0		146.9	
10111-CAG	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM)	X 6.96	67.0	19.8	6.44	138.0	$\pm 1.4\%$
		Y 6.39	65.5	18.9		119.4	
		Z 6.50	66.4	19.6		108.4	
10117-CAC	IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)	X 9.93	68.0	20.8	8.07	125.4	$\pm 2.2\%$
		Y 9.20	66.5	19.9		105.4	
		Z 10.03	68.9	21.5		140.9	
10140-CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	X 7.71	67.7	20.1	6.49	149.5	$\pm 1.7\%$
		Y 7.05	66.0	19.1		129.0	
		Z 7.17	66.8	19.8		116.6	
10142-CAE	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, QPSK)	X 5.75	65.9	19.0	5.73	129.0	$\pm 1.2\%$
		Y 5.24	64.4	18.1		112.8	
		Z 5.77	67.2	19.9		143.4	
10143-CAE	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM)	X 6.69	67.0	19.7	6.35	134.2	$\pm 1.4\%$
		Y 6.08	65.4	18.8		115.5	
		Z 6.71	68.2	20.6		148.6	

EX3DV4- SN:7534

July 25, 2019

10145-CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK)	X	5.53	66.1	19.1	5.76	124.5	$\pm 1.2\%$
		Y	5.03	64.6	18.2		108.8	
		Z	5.56	67.5	20.1		137.7	
10146-CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	X	6.37	67.1	19.8	6.41	127.2	$\pm 1.4\%$
		Y	5.77	65.6	18.9		108.8	
		Z	6.41	68.6	20.8		140.5	
10149-CAE	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM)	X	7.24	67.2	19.9	6.42	143.4	$\pm 1.4\%$
		Y	6.65	65.6	18.9		124.0	
		Z	6.73	66.3	19.6		111.7	
10154-CAG	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	X	5.93	66.0	19.0	5.75	131.8	$\pm 1.2\%$
		Y	5.44	64.6	18.2		115.4	
		Z	5.97	67.2	19.9		147.1	
10155-CAG	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM)	X	6.97	67.1	19.8	6.43	138.0	$\pm 1.7\%$
		Y	6.38	65.5	18.9		118.9	
		Z	6.46	66.3	19.6		108.1	
10156-CAG	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, QPSK)	X	5.69	65.8	18.9	5.79	127.9	$\pm 1.2\%$
		Y	5.23	64.5	18.2		111.8	
		Z	5.73	67.2	20.0		141.7	
10157-CAG	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM)	X	6.68	67.0	19.8	6.49	131.7	$\pm 1.4\%$
		Y	6.09	65.5	18.9		113.7	
		Z	6.72	66.3	20.8		146.2	
10160-CAE	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, QPSK)	X	6.37	66.6	19.3	5.82	137.1	$\pm 1.4\%$
		Y	5.80	64.9	18.4		119.2	
		Z	5.93	65.9	19.1		107.4	
10161-CAE	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM)	X	7.27	67.3	19.9	6.43	143.5	$\pm 1.4\%$
		Y	6.68	65.8	19.0		123.6	
		Z	6.78	66.5	19.7		112.0	
10166-CAF	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK)	X	4.92	65.6	18.7	5.46	119.3	$\pm 0.9\%$
		Y	4.74	65.5	18.7		144.1	
		Z	4.98	67.4	20.0		132.3	
10167-CAF	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM)	X	5.77	67.0	19.7	6.21	120.3	$\pm 1.2\%$
		Y	5.56	66.9	19.7		144.3	
		Z	5.80	68.5	20.8		132.4	
10169-CAE	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	X	4.74	65.6	18.9	5.73	113.7	$\pm 1.2\%$
		Y	4.59	65.5	18.9		138.0	
		Z	4.74	67.0	20.1		125.7	
10170-CAE	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM)	X	5.35	66.3	19.7	6.52	111.5	$\pm 1.2\%$
		Y	5.17	66.2	19.6		135.2	
		Z	5.35	67.8	20.8		123.4	
10175-CAG	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	X	4.73	65.5	18.9	5.72	113.4	$\pm 0.9\%$
		Y	4.56	65.4	18.8		137.6	
		Z	4.74	67.0	20.1		125.7	
10176-CAG	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM)	X	5.34	66.3	19.7	6.52	111.6	$\pm 1.2\%$
		Y	5.16	66.1	19.6		135.1	
		Z	5.34	67.7	20.8		123.8	

Certificate No: EX3-7534_Jul19

Page 12 of 17

EX3DV4- SN:7534

July 25, 2019

10177-CAI	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, QPSK)	X	4.75	65.6	19.0	5.73	113.3	$\pm 0.9\%$
		Y	4.58	65.4	18.9		137.6	
		Z	4.77	67.2	20.2		125.9	
10178-CAG	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM)	X	5.35	66.3	19.7	6.52	111.6	$\pm 1.2\%$
		Y	5.17	66.2	19.6		135.2	
		Z	5.33	67.7	20.7		123.7	
10181-CAE	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	X	4.73	65.5	18.9	5.72	113.5	$\pm 1.2\%$
		Y	4.61	65.6	19.0		137.6	
		Z	4.75	67.1	20.1		125.4	
10182-CAE	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM)	X	5.35	66.4	19.7	6.52	111.8	$\pm 1.2\%$
		Y	5.16	66.2	19.6		135.1	
		Z	5.37	67.9	20.9		123.6	
10184-CAE	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, QPSK)	X	4.72	65.4	18.8	5.73	113.4	$\pm 1.2\%$
		Y	4.60	65.6	19.0		138.0	
		Z	4.76	67.1	20.1		125.7	
10185-CAE	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM)	X	5.32	66.3	19.6	6.51	111.7	$\pm 1.2\%$
		Y	5.19	66.4	19.7		135.4	
		Z	5.36	67.8	20.8		123.8	
10187-CAF	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK)	X	4.73	65.5	18.9	5.73	113.3	$\pm 0.9\%$
		Y	4.60	65.6	18.9		137.8	
		Z	4.76	67.1	20.1		125.8	
10188-CAF	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM)	X	5.34	66.3	19.6	6.52	111.7	$\pm 1.2\%$
		Y	5.16	66.1	19.5		135.5	
		Z	5.38	67.8	20.8		123.8	
10196-CAC	IEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)	X	9.51	67.7	20.8	8.10	118.9	$\pm 2.2\%$
		Y	9.41	67.9	20.8		145.9	
		Z	9.59	68.7	21.4		133.1	
10225-CAB	UMTS-FDD (HSPA+)	X	7.07	67.3	19.6	5.97	145.5	$\pm 1.4\%$
		Y	6.45	65.9	18.7		124.9	
		Z	6.56	66.7	19.4		113.3	
10274-CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.10)	X	5.94	66.7	18.7	4.87	140.9	$\pm 1.2\%$
		Y	5.41	65.5	18.0		122.0	
		Z	5.63	66.8	19.0		109.8	
10275-CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.4)	X	4.31	65.5	17.8	3.96	127.3	$\pm 0.7\%$
		Y	3.94	64.4	17.4		111.9	
		Z	4.44	67.5	19.3		141.2	
10297-AAD	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	X	6.26	66.5	19.2	5.81	135.5	$\pm 1.4\%$
		Y	5.87	64.7	18.2		116.9	
		Z	6.28	67.6	20.1		150.0	
10298-AAD	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, QPSK)	X	5.54	65.8	18.9	5.72	126.1	$\pm 1.2\%$
		Y	5.04	64.4	18.1		109.6	
		Z	5.56	67.2	19.9		138.9	
10299-AAD	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM)	X	6.48	67.2	19.8	6.39	129.9	$\pm 1.4\%$
		Y	5.88	65.7	19.0		110.4	
		Z	6.53	68.6	20.8		143.0	

Certificate No: EX3-7534_Jul19

Page 13 of 17

EX3DV4- SN:7534

July 25, 2019

10311-AAD	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	X	6.79	66.9	19.5	6.06	140.5	$\pm 1.4\%$
		Y	6.24	65.4	18.7		122.4	
		Z	6.33	66.2	19.3		110.2	
10415-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	X	2.56	65.8	16.8	1.54	127.6	$\pm 0.5\%$
		Y	2.32	65.0	16.6		113.0	
		Z	3.18	72.3	20.8		141.3	
10418-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 99pc duty cycle, Long preamble)	X	9.46	67.7	20.8	8.14	118.5	$\pm 2.5\%$
		Y	9.37	67.9	20.8		143.7	
		Z	9.53	68.5	21.4		131.7	
10435-AAF	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.60	66.3	21.8	7.82	132.6	$\pm 1.7\%$
		Y	4.90	65.6	20.2		114.4	
		Z	5.54	69.6	22.8		143.8	
10457-AAA	UMTS-FDD (DC-HSDPA)	X	7.92	65.9	19.1	6.62	115.8	$\pm 1.4\%$
		Y	7.95	66.5	19.3		142.3	
		Z	8.00	66.9	19.8		128.8	
10460-AAA	UMTS-FDD (WCDMA, AMR)	X	2.76	65.6	17.2	2.39	121.7	$\pm 0.5\%$
		Y	2.62	65.7	17.5		148.3	
		Z	3.27	71.2	20.7		134.2	
10461-AAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.60	66.3	21.7	7.82	132.4	$\pm 1.9\%$
		Y	4.89	65.5	20.1		114.5	
		Z	5.54	69.6	22.8		144.3	
10462-AAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.02	69.1	22.3	8.30	129.7	$\pm 1.7\%$
		Y	5.54	67.8	21.6		147.7	
		Z	5.96	70.5	23.4		141.0	
10464-AAB	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.58	66.2	21.7	7.82	131.9	$\pm 1.7\%$
		Y	4.90	65.6	20.2		115.3	
		Z	5.57	69.8	22.9		143.8	
10465-AAB	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.02	69.1	22.3	8.32	129.4	$\pm 1.7\%$
		Y	5.55	67.8	21.6		147.7	
		Z	5.99	70.5	23.4		141.2	
10467-AAE	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.57	66.2	21.6	7.82	131.7	$\pm 1.7\%$
		Y	4.92	65.7	20.2		115.6	
		Z	5.54	69.6	22.8		143.4	
10468-AAE	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.03	69.1	22.4	8.32	129.6	$\pm 1.7\%$
		Y	5.55	67.8	21.6		147.8	
		Z	5.99	70.6	23.5		141.2	
10470-AAE	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.57	66.2	21.6	7.82	132.2	$\pm 1.7\%$
		Y	4.90	65.6	20.2		115.1	
		Z	5.52	69.5	22.7		143.8	
10471-AAE	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.03	69.1	22.3	8.32	130.0	$\pm 1.9\%$
		Y	5.54	67.7	21.6		147.7	
		Z	5.99	70.5	23.5		141.0	

EX3DV4- SN:7534

July 25, 2019

10473-AAE	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.56	68.2	21.7	7.82	131.5	$\pm 1.7\%$
		Y	4.88	65.5	20.1		115.4	
		Z	5.55	69.5	22.8		143.9	
10474-AAE	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.03	69.2	22.4	8.32	129.7	$\pm 1.9\%$
		Y	5.56	67.8	21.6		147.9	
		Z	6.02	70.7	23.5		141.6	
10477-AAF	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.02	69.1	22.3	8.32	130.1	$\pm 1.7\%$
		Y	5.56	67.8	21.7		148.4	
		Z	5.99	70.5	23.5		141.8	
10479-AAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.86	67.8	21.3	7.74	138.5	$\pm 1.7\%$
		Y	5.21	65.6	20.1		121.3	
		Z	5.51	67.6	21.5		111.1	
10480-AAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.54	69.2	22.2	8.18	140.8	$\pm 1.7\%$
		Y	5.70	66.5	20.6		120.5	
		Z	6.13	68.9	22.2		111.5	
10482-AAB	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.26	67.8	21.3	7.71	146.1	$\pm 1.7\%$
		Y	5.53	65.3	19.8		126.5	
		Z	5.90	67.5	21.3		117.2	
10483-AAB	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.87	67.5	21.2	8.39	109.9	$\pm 1.7\%$
		Y	6.44	66.6	20.7		129.7	
		Z	6.88	68.8	22.2		120.2	
10485-AAE	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.26	67.7	21.2	7.59	149.1	$\pm 1.7\%$
		Y	5.54	65.3	19.8		128.9	
		Z	5.91	67.4	21.3		119.3	
10486-AAE	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.00	67.3	21.2	8.38	112.9	$\pm 1.9\%$
		Y	6.56	66.4	20.6		133.1	
		Z	7.00	68.5	22.0		123.8	
10488-AAE	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.27	66.3	20.3	7.70	113.1	$\pm 1.7\%$
		Y	5.90	65.4	19.9		133.5	
		Z	6.25	67.3	21.2		123.4	
10489-AAE	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.28	67.3	21.1	8.31	118.7	$\pm 1.9\%$
		Y	6.82	66.2	20.5		139.4	
		Z	7.24	68.2	21.8		130.2	
10491-AAE	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.66	66.7	20.5	7.74	117.4	$\pm 1.7\%$
		Y	6.23	65.7	20.0		138.2	
		Z	6.67	67.8	21.4		128.6	
10492-AAE	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.74	67.6	21.3	8.41	124.1	$\pm 2.2\%$
		Y	7.25	66.5	20.7		144.6	
		Z	7.72	68.5	22.0		136.0	
10494-AAF	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.65	66.8	20.6	7.74	117.0	$\pm 1.7\%$
		Y	6.19	65.6	20.0		137.3	
		Z	6.67	67.9	21.5		128.3	
10495-AAF	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.66	67.4	21.2	8.37	124.2	$\pm 2.2\%$
		Y	7.15	66.2	20.5		144.7	
		Z	7.66	68.4	22.0		136.0	

Certificate No: EX3-7534_Jul19

Page 15 of 17

EX3DV4- SN:7534

July 25, 2019

10497-AAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.18	67.9	21.2	7.67	145.5	$\pm 1.7\%$
		Y	5.45	65.5	19.9		125.5	
		Z	5.82	67.6	21.3		116.2	
10498-AAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.18	69.3	22.2	8.40	149.4	$\pm 1.9\%$
		Y	6.32	66.7	20.7		126.7	
		Z	6.76	68.8	22.2		118.6	
10500-AAB	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.08	66.2	20.3	7.67	110.6	$\pm 1.7\%$
		Y	5.70	65.3	19.8		130.2	
		Z	6.06	67.3	21.2		120.7	
10501-AAB	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.18	67.4	21.2	8.44	115.2	$\pm 1.9\%$
		Y	6.74	66.5	20.7		134.8	
		Z	7.16	68.4	22.0		125.5	
10503-AAE	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.30	66.3	20.4	7.72	113.1	$\pm 1.7\%$
		Y	5.89	65.3	19.8		133.2	
		Z	6.29	67.4	21.3		124.1	
10504-AAE	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.27	67.2	21.1	8.31	118.8	$\pm 1.9\%$
		Y	6.83	66.3	20.5		139.5	
		Z	7.27	68.2	21.9		129.9	
10506-AAE	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.63	66.7	20.5	7.74	116.8	$\pm 1.7\%$
		Y	6.17	65.6	19.9		137.5	
		Z	6.66	67.9	21.5		128.5	
10507-AAE	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.66	67.5	21.2	8.36	124.2	$\pm 1.9\%$
		Y	7.18	66.4	20.6		145.1	
		Z	7.66	68.4	22.0		136.1	
10509-AAE	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	7.26	67.3	20.9	7.99	122.4	$\pm 1.9\%$
		Y	6.73	66.1	20.3		142.7	
		Z	7.30	68.4	21.8		134.5	
10510-AAE	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	8.19	67.9	21.5	8.49	130.0	$\pm 2.2\%$
		Y	7.33	65.5	20.0		111.1	
		Z	8.17	68.8	22.2		143.1	
10512-AAF	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.96	67.3	20.8	7.74	120.4	$\pm 1.9\%$
		Y	6.44	65.9	20.1		141.5	
		Z	7.01	68.4	21.6		132.9	
10513-AAF	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	8.03	67.7	21.4	8.42	129.6	$\pm 2.2\%$
		Y	7.47	66.4	20.6		149.7	
		Z	8.03	68.6	22.1		142.1	
10515-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 90pc duty cycle)	X	2.56	65.8	16.8	1.58	127.2	$\pm 0.5\%$
		Y	2.33	65.4	16.9		113.2	
		Z	3.31	73.3	21.3		139.9	
10571-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 90pc duty cycle)	X	2.72	66.3	17.3	1.99	124.0	$\pm 0.7\%$
		Y	2.48	65.6	17.1		108.9	
		Z	3.56	74.0	21.8		137.0	

EX3DV4- SN:7534

July 25, 2019

10572- AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 90pc duty cycle)	X	2.65	65.9	17.0	1.99	123.7	$\pm 0.5\%$
		Y	2.37	65.1	16.9		149.6	
		Z	3.37	73.1	21.3		136.5	
10575- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 90pc duty cycle)	X	9.66	67.7	21.0	8.59	116.3	$\pm 2.5\%$
		Y	9.59	68.0	21.2		140.9	
		Z	9.79	68.8	21.8		129.6	
10591- AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS0, 90pc duty cycle)	X	9.84	67.9	21.2	8.63	118.1	$\pm 2.5\%$
		Y	9.69	68.0	21.2		142.7	
		Z	9.93	68.8	21.9		131.7	
10599- AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS0, 90pc duty cycle)	X	10.43	68.4	21.4	8.79	124.7	$\pm 2.7\%$
		Y	10.24	68.4	21.4		150.0	
		Z	10.54	69.3	22.1		138.8	

^a Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**Client **Motorola Solutions MY**Certificate No: **EX3-7511_Oct19****CALIBRATION CERTIFICATE**Object **EX3DV4 - SN:7511**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v5, QA CAL-23.v5,
QA CAL-25.v7
Calibration procedure for dosimetric E-field probes**

Calibration date: **October 24, 2019**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	03-Apr-19 (No. 217-02892/02893)	Apr-20
Power sensor NRP-Z91	SN: 103244	03-Apr-19 (No. 217-02892)	Apr-20
Power sensor NRP-Z91	SN: 103245	03-Apr-19 (No. 217-02893)	Apr-20
Reference 20 dB Attenuator	SN: S5277 (20x)	04-Apr-19 (No. 217-02894)	Apr-20
DAE4	SN: 660	07-Oct-19 (No. DAE4-660_Oct19)	Oct-20
Reference Probe ES3DV2	SN: 3013	31-Dec-18 (No. ES3-3013_Dec18)	Dec-19
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: MY41498087	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: 000110210	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
RF generator HP 8648C	SN: US3642UD1700	04-Aug-99 (in house check Jun-18)	In house check: Jun-20
Network Analyzer E8358A	SN: US41080477	31-Mar-14 (in house check Oct-18)	In house check: Oct-19

Calibrated by:	Name: Jeton Kastrati	Function: Laboratory Technician	Signature:
Approved by:	Name: Katja Pokovic	Function: Technical Manager	Signature:

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Issued: October 24, 2019

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
NORMx,y,z	sensitivity in free space
ConvF	sensitivity in TSL / NORMx,y,z
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization θ	θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, ", "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- *NORMx,y,z*: Assessed for E-field polarization $\theta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). *NORMx,y,z* are only intermediate values, i.e., the uncertainties of *NORMx,y,z* does not affect the E^2 -field uncertainty inside TSL (see below *ConvF*).
- *NORM(f)x,y,z = NORMx,y,z * frequency_response* (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of *ConvF*.
- *DCPx,y,z*: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- *PAR*: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- *Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z; A, B, C, D* are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- *ConvF and Boundary Effect Parameters*: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to *NORMx,y,z * ConvF* whereby the uncertainty corresponds to that given for *ConvF*. A frequency dependent *ConvF* is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- *Spherical isotropy (3D deviation from isotropy)*: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- *Sensor Offset*: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- *Connector Angle*: The angle is assessed using the information gained by determining the *NORMx* (no uncertainty required).

EX3DV4 - SN:7511

October 24, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7511**Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ($\mu\text{V}/(\text{V}/\text{m})^2$) ^A	0.46	0.37	0.44	$\pm 10.1 \%$
DCP (mV) ^B	99.0	96.6	99.9	

Calibration Results for Modulation Response

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Max dev.	Unc ^C (k=2)
0	CW	X	0.0	0.0	1.0	0.00	118.4	$\pm 3.8 \%$	$\pm 4.7 \%$
		Y	0.0	0.0	1.0		133.1		
		Z	0.0	0.0	1.0		117.4		

Note: For details on UID parameters see Appendix

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).^B Numerical linearization parameter: uncertainty not required.^C Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4-SN:7511

October 24, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7511**Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	0.8
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

EX3DV4-SN:7511

October 24, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7511**Calibration Parameter Determined in Head Tissue Simulating Media**

f (MHz) ^c	Relative Permittivity ^e	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ^g	Depth ^d (mm)	Unc (k=2)
150	52.3	0.76	12.15	12.15	12.15	0.00	1.00	± 13.3 %
300	45.3	0.87	10.87	10.87	10.87	0.08	1.20	± 13.3 %
450	43.5	0.87	10.30	10.30	10.30	0.10	1.30	± 13.3 %
750	41.9	0.89	9.57	9.57	9.57	0.46	0.80	± 12.0 %
835	41.5	0.90	9.28	9.28	9.28	0.33	1.01	± 12.0 %
900	41.5	0.97	9.06	9.06	9.06	0.49	0.81	± 12.0 %
1450	40.5	1.20	8.17	8.17	8.17	0.10	0.80	± 12.0 %
1810	40.0	1.40	7.94	7.94	7.94	0.28	0.80	± 12.0 %
1900	40.0	1.40	7.69	7.69	7.69	0.34	0.80	± 12.0 %
2100	39.8	1.49	7.73	7.73	7.73	0.33	0.80	± 12.0 %
2300	39.5	1.67	7.35	7.35	7.35	0.36	0.90	± 12.0 %
2450	39.2	1.80	7.06	7.06	7.06	0.33	0.90	± 12.0 %
2600	39.0	1.96	6.81	6.81	6.81	0.39	0.90	± 12.0 %
3500	37.9	2.91	6.66	6.66	6.66	0.35	1.30	± 13.1 %
3700	37.7	3.12	6.56	6.56	6.56	0.35	1.30	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 6 MHz is 4-9 MHz, and ConvF assessed at 13 MHz is 9-19 MHz. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^e All frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^d Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4-SN:7511

October 24, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7511**Calibration Parameter Determined in Body Tissue Simulating Media**

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^H (mm)	Unc (k=2)
150	61.9	0.80	11.72	11.72	11.72	0.00	1.00	± 13.3 %
300	58.2	0.92	11.12	11.12	11.12	0.04	1.20	± 13.3 %
450	56.7	0.94	10.59	10.59	10.59	0.08	1.30	± 13.3 %
750	55.5	0.96	9.52	9.52	9.52	0.49	0.80	± 12.0 %
835	55.2	0.97	9.26	9.26	9.26	0.40	0.80	± 12.0 %
900	55.0	1.05	9.14	9.14	9.14	0.42	0.84	± 12.0 %
1450	54.0	1.30	7.97	7.97	7.97	0.30	0.80	± 12.0 %
1810	53.3	1.52	7.64	7.64	7.64	0.34	0.80	± 12.0 %
1900	53.3	1.52	7.37	7.37	7.37	0.44	0.80	± 12.0 %
2100	53.2	1.62	7.46	7.46	7.46	0.31	0.86	± 12.0 %
2300	52.9	1.81	7.21	7.21	7.21	0.35	0.90	± 12.0 %
2450	52.7	1.95	6.97	6.97	6.97	0.36	0.90	± 12.0 %
2600	52.5	2.16	6.88	6.88	6.88	0.32	0.90	± 12.0 %
3500	51.3	3.31	6.11	6.11	6.11	0.40	1.35	± 13.1 %
3700	51.0	3.55	6.02	6.02	6.02	0.40	1.35	± 13.1 %

^C Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 6 MHz is 4-9 MHz, and ConvF assessed at 13 MHz is 9-19 MHz. Above 5 GHz frequency validity can be extended to ± 110 MHz.

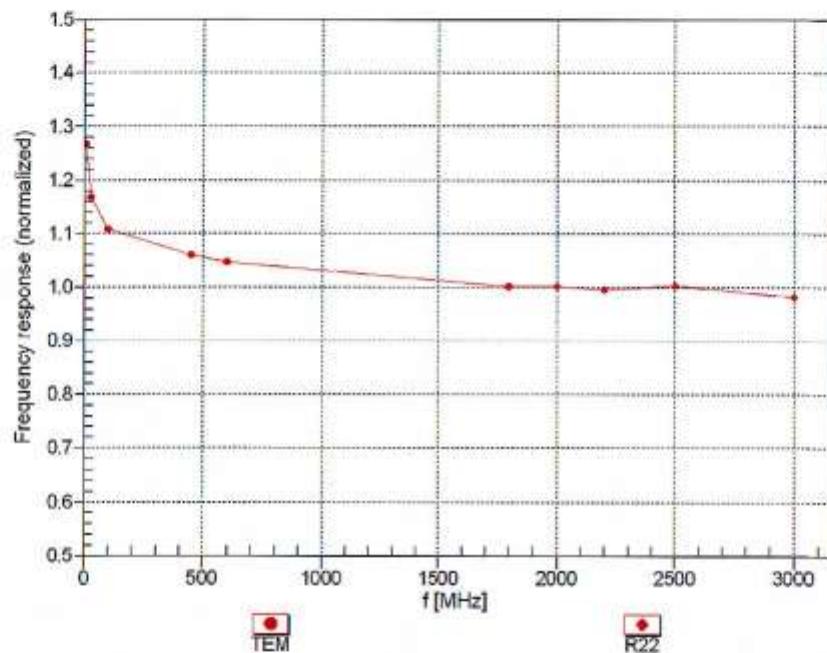
^F At frequencies below 3 GHz, the validity of tissue parameters (c and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (c and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:7511

October 24, 2019

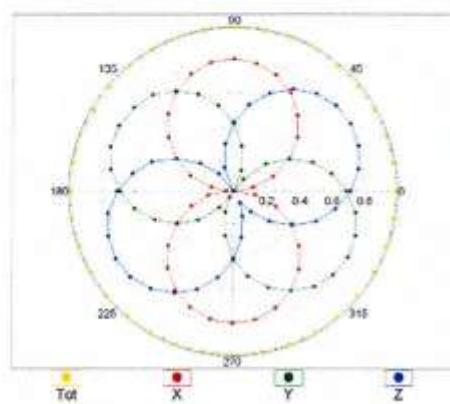
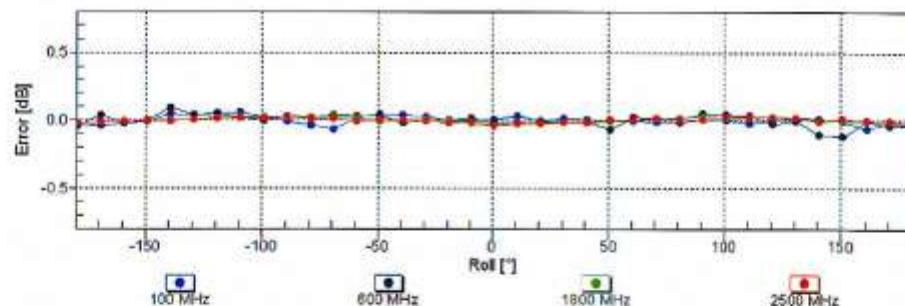
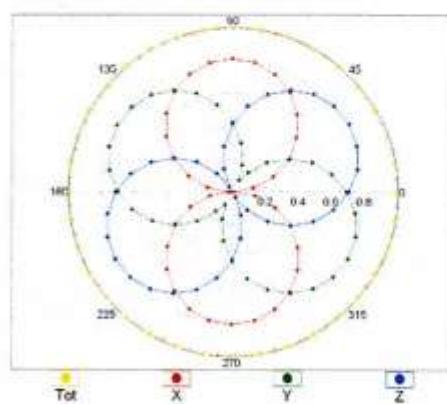
Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)



Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ ($k=2$)

EX3DV4- SN:7511

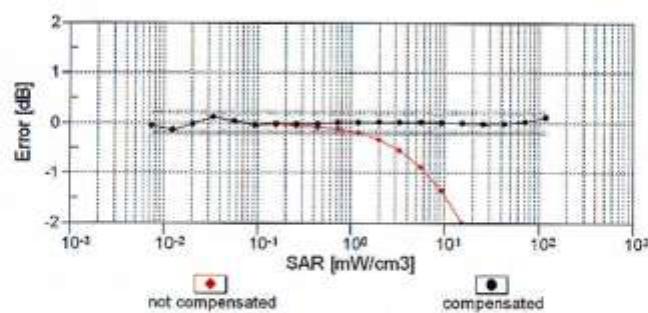
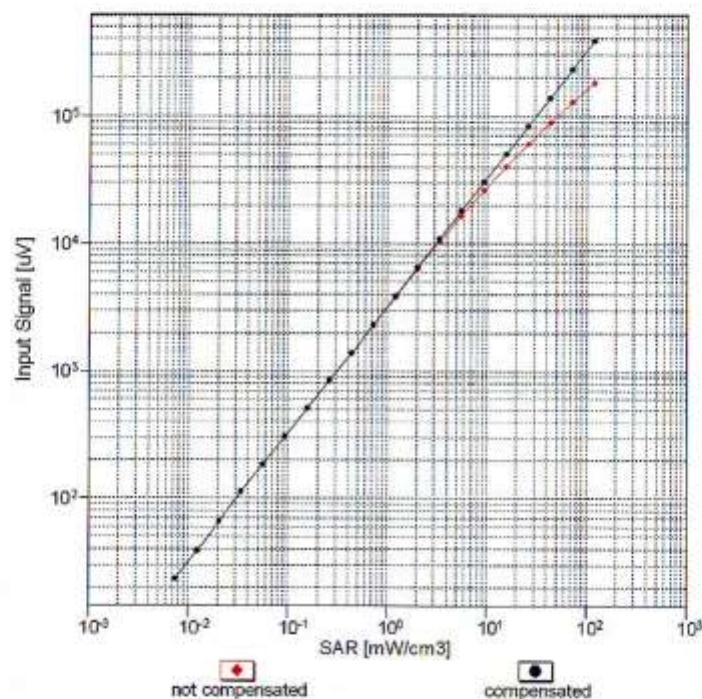
October 24, 2019

Receiving Pattern (ϕ), $\theta = 0^\circ$ $f=600 \text{ MHz, TEM}$  $f=1800 \text{ MHz, R22}$ **Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)**

EX3DV4- SN:7511

October 24, 2019

Dynamic Range f(SAR_{head})
(TEM cell , f_{eval}= 1900 MHz)

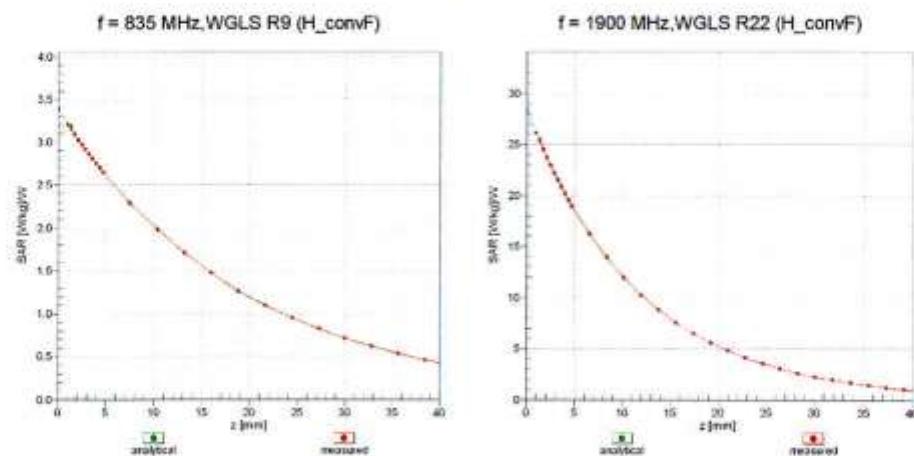


Uncertainty of Linearity Assessment: $\pm 0.6\% (k=2)$

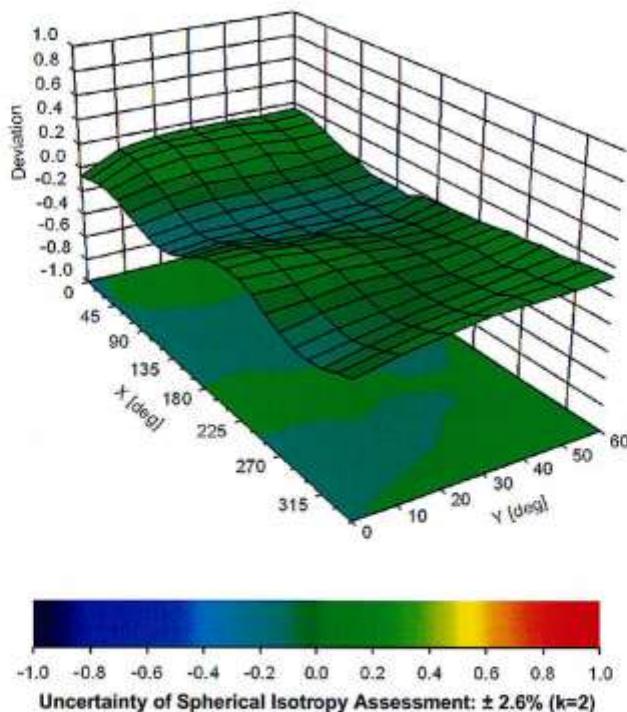
EX3DV4- SN:7511

October 24, 2019

Conversion Factor Assessment



Deviation from Isotropy in Liquid

Error (ϕ, θ), $f = 900 \text{ MHz}$ 

EX3DV4– SN:7511

October 24, 2019

Appendix: Modulation Calibration Parameters

UID	Communication System Name	A dB	B dB/ μ V	C	D dB	VR mV	Max dev.	Unc (k=2)
0	CW	X 0.0	0.0	1.0	0.00	118.4	$\pm 3.8\%$	$\pm 4.7\%$
		Y 0.0	0.0	1.0		133.1		
		Z 0.0	0.0	1.0		117.4		
10100-CAE	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	X 6.43	67.6	19.8	5.67	141.8	$\pm 1.4\%$	$\pm 4.7\%$
		Y 6.81	70.2	22.1		112.8		
		Z 6.38	67.4	19.7		140.0		
10108-CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X 6.29	67.3	19.8	5.80	138.5	$\pm 2.2\%$	$\pm 4.7\%$
		Y 7.56	73.7	24.5		110.1		
		Z 6.28	67.3	19.8		136.5		
10110-CAG	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, QPSK)	X 5.97	67.0	19.8	5.75	134.4	$\pm 2.5\%$	$\pm 4.7\%$
		Y 6.87	72.6	24.2		149.0		
		Z 5.93	66.8	19.6		132.2		
10154-CAG	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	X 5.97	67.0	19.8	5.75	134.3	$\pm 2.5\%$	$\pm 4.7\%$
		Y 6.95	73.0	24.5		149.0		
		Z 5.95	66.9	19.6		132.6		
10156-CAG	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, QPSK)	X 5.77	67.1	19.8	5.79	129.9	$\pm 2.5\%$	$\pm 4.7\%$
		Y 6.92	74.0	25.2		144.8		
		Z 5.72	66.8	19.7		128.0		
10160-CAE	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, QPSK)	X 6.41	67.5	20.0	5.82	140.2	$\pm 2.5\%$	$\pm 4.7\%$
		Y 8.27	76.0	25.8		111.2		
		Z 6.37	67.4	19.9		137.5		
10169-CAE	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	X 4.81	67.0	20.0	5.73	116.5	$\pm 2.7\%$	$\pm 4.7\%$
		Y 7.29	81.0	29.2		129.3		
		Z 4.77	66.7	19.8		114.7		
10175-CAG	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	X 4.80	66.9	20.0	5.72	116.1	$\pm 2.5\%$	$\pm 4.7\%$
		Y 6.87	79.0	28.1		129.3		
		Z 4.80	66.9	19.9		114.1		
10177-CAI	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, QPSK)	X 4.82	67.1	20.1	5.73	115.5	$\pm 2.5\%$	$\pm 4.7\%$
		Y 6.68	78.1	27.6		129.4		
		Z 4.78	66.8	19.9		113.9		
10181-CAE	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	X 4.88	67.4	20.3	5.72	116.3	$\pm 2.5\%$	$\pm 4.7\%$
		Y 6.81	78.7	27.9		129.1		
		Z 4.80	66.8	19.9		114.1		
10297-AAD	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	X 6.37	67.7	20.2	5.81	136.2	$\pm 2.5\%$	$\pm 4.7\%$
		Y 7.95	75.1	25.4		110.4		
		Z 6.32	67.5	20.0		136.2		
10311-AAD	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	X 6.90	68.1	20.4	6.06	144.1	$\pm 2.5\%$	$\pm 4.7\%$
		Y 8.57	75.6	25.7		113.8		
		Z 6.90	68.0	20.4		140.7		

EX3DV4- SN:7511

October 24, 2019

10415-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	X	3.27	71.5	20.0	1.54	130.5	$\pm 3.0\%$	$\pm 4.7\%$
		Y	7.44	100.0	36.1		146.5		
		Z	3.30	71.7	20.1		128.2		
10435-AAF	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.67	70.0	23.2	7.82	134.0	$\pm 2.2\%$	$\pm 4.7\%$
		Y	6.40	76.6	28.9		142.3		
		Z	5.66	69.8	23.0		132.2		
10467-AAF	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.67	70.0	23.2	7.82	133.7	$\pm 1.4\%$	$\pm 4.7\%$
		Y	5.81	72.6	26.0		142.6		
		Z	5.65	69.7	22.9		131.7		
10470-AAF	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.64	69.8	23.0	7.82	133.5	$\pm 1.4\%$	$\pm 4.7\%$
		Y	5.73	71.9	25.4		142.7		
		Z	5.69	69.9	23.0		131.9		
10473-AAE	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.67	70.1	23.2	7.82	133.5	$\pm 1.2\%$	$\pm 4.7\%$
		Y	5.65	71.4	25.1		142.7		
		Z	5.67	69.8	23.0		131.5		
10485-AAF	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.02	67.8	21.6	7.59	110.4	$\pm 1.2\%$	$\pm 4.7\%$
		Y	6.00	69.0	23.2		121.1		
		Z	6.30	68.9	22.1		149.7		
10488-AAF	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.35	67.6	21.5	7.70	114.9	$\pm 1.2\%$	$\pm 4.7\%$
		Y	6.26	68.5	22.9		124.7		
		Z	6.37	67.6	21.4		113.3		
10491-AAE	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.74	68.0	21.6	7.74	119.3	$\pm 1.2\%$	$\pm 4.7\%$
		Y	6.58	68.6	22.9		129.0		
		Z	6.73	67.8	21.5		117.8		
10494-AAF	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.75	68.1	21.7	7.74	119.1	$\pm 1.2\%$	$\pm 4.7\%$
		Y	6.56	68.6	23.0		128.9		
		Z	6.74	67.9	21.6		117.6		
10503-AAF	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.37	67.7	21.5	7.72	114.8	$\pm 1.4\%$	$\pm 4.7\%$
		Y	6.34	68.9	23.2		124.8		
		Z	6.36	67.4	21.3		113.4		
10506-AAF	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.72	68.0	21.7	7.74	118.9	$\pm 1.4\%$	$\pm 4.7\%$
		Y	6.56	68.6	23.0		128.6		
		Z	6.73	67.9	21.6		117.8		
10509-AAE	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	7.35	68.6	22.0	7.99	124.0	$\pm 1.4\%$	$\pm 4.7\%$
		Y	7.06	68.7	23.0		133.6		
		Z	7.37	68.5	22.0		122.9		

EX3DV4– SN:7511

October 24, 2019

10512-AAF	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	7.09	68.6	21.9	7.74	122.9	±1.4 %	± 4.7 %
		Y	6.83	69.0	23.0		131.8		
		Z	7.10	68.5	21.8		121.3		
10571-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 90pc duty cycle)	X	3.42	71.9	20.4	1.99	127.1	±1.9 %	± 4.7 %
		Y	9.13	99.3	33.8		140.7		
		Z	3.61	72.9	21.0		124.4		

^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Appendix C

Dipole Calibration Certificates

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**Client **Motorola Solutions MY**Certificate No: **D450V3-1054_Mar19**

CALIBRATION CERTIFICATE

Object **D450V3 - SN:1054**

Calibration procedure(s) **QA CAL-15.v9**
Calibration Procedure for SAR Validation Sources below 700 MHz

Calibration date: **March 11, 2019**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-18 (No. 217-02672/02673)	Apr-19
Power sensor NRP-Z91	SN: 103244	04-Apr-18 (No. 217-02672)	Apr-19
Power sensor NRP-Z91	SN: 103245	04-Apr-18 (No. 217-02673)	Apr-19
Reference 20 dB Attenuator	SN: 5277 (20x)	04-Apr-18 (No. 217-02682)	Apr-19
Type-N mismatch combination	SN: 5047.2 / 06327	04-Apr-18 (No. 217-02683)	Apr-19
Reference Probe EX3DV4	SN: 3877	31-Dec-18 (No. EX3-3877..Dec18)	Dec-19
DAE4	SN: 654	05-Jul-18 (No. DAE4-654..Jul18)	Jul-19
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: MY41498087	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: 000110210	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-18)	In house check: Jun-20
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-18)	In house check: Oct-19

Calibrated by:	Name	Function	Signature
	Claudio Leubler	Laboratory Technician	

Approved by:	Name	Function	Signature
	Katja Pokovic	Technical Manager	

Issued: March 11, 2019

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.2
Extrapolation	Advanced Extrapolation	
Phantom	ELI4 Flat Phantom	Shell thickness: 2 ± 0.2 mm
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	$dx, dy, dz = 5$ mm	
Frequency	450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	43.5	0.87 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	44.1 ± 6 %	0.87 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	1.14 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	4.57 W/kg ± 18.1 % (k=2)

SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	0.763 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	3.06 W/kg ± 17.6 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	56.7	0.94 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	55.7 ± 6 %	0.93 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

SAR result with Body TSL

SAR averaged over 1 cm³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	1.13 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	4.54 W/kg ± 18.1 % (k=2)

SAR averaged over 10 cm³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	0.762 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	3.06 W/kg ± 17.6 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	60.2 Ω - 0.4 $j\Omega$
Return Loss	- 20.7 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	57.7 Ω - 3.6 $j\Omega$
Return Loss	- 22.1 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.346 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

DASY5 Validation Report for Head TSL

Date: 11.03.2019

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 450 MHz; Type: D450V3; Serial: D450V3 - SN:1054

Communication System: UID 0 - CW; Frequency: 450 MHz

Medium parameters used: $f = 450 \text{ MHz}$; $\sigma = 0.87 \text{ S/m}$; $\epsilon_r = 44.1$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(10.5, 10.5, 10.5) @ 450 MHz; Calibrated: 31.12.2018
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 05.07.2018
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52 52.10.2(1495); SEMCAD X 14.6.12(7450)

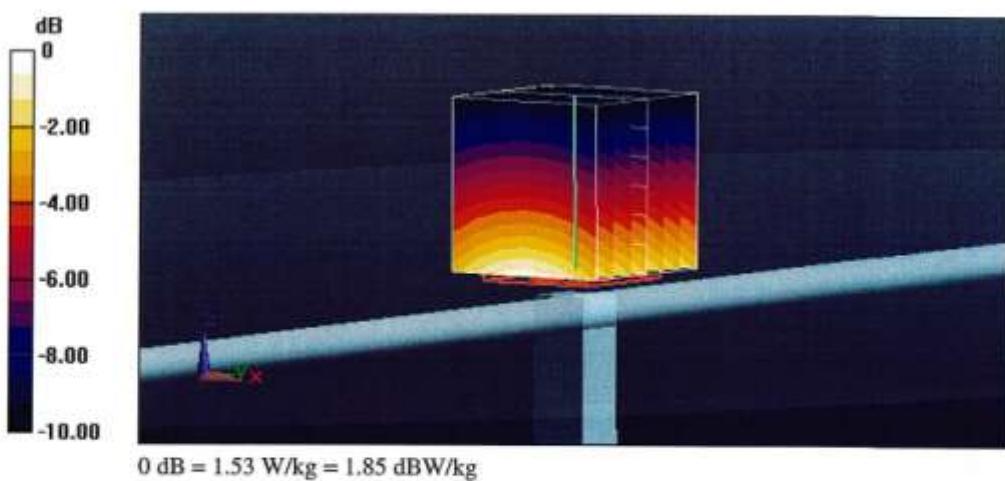
Dipole Calibration for Head Tissue/d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0:Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

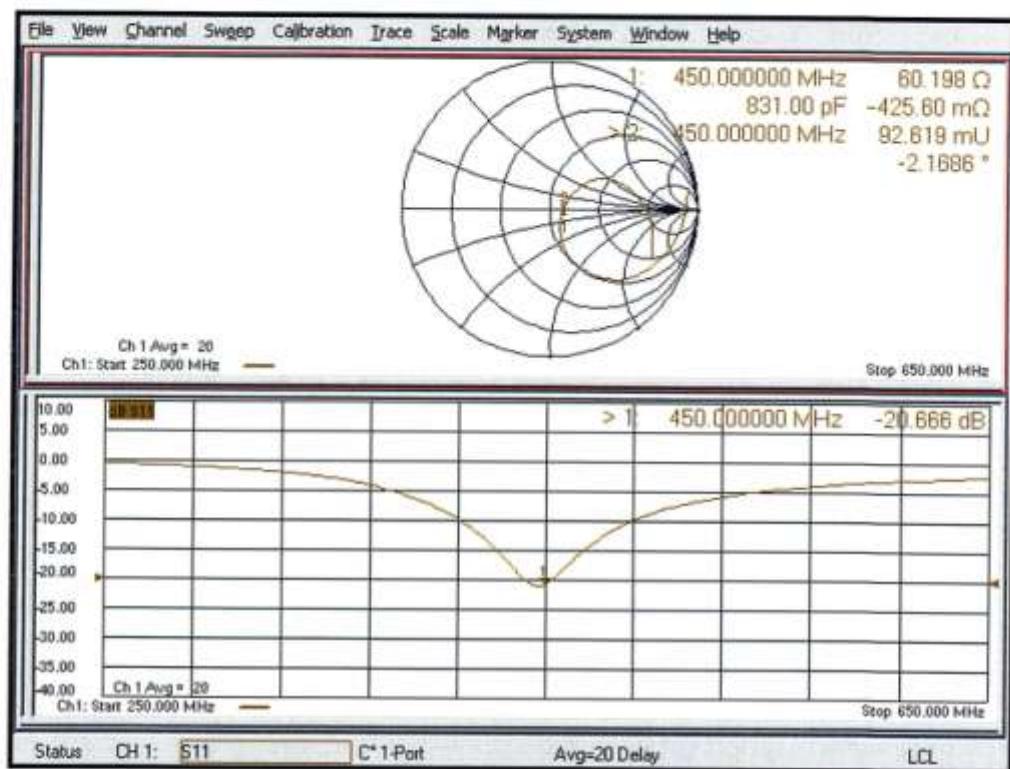
Reference Value = 38.90 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 1.75 W/kg

SAR(1 g) = 1.14 W/kg; SAR(10 g) = 0.763 W/kg

Maximum value of SAR (measured) = 1.53 W/kg



Impedance Measurement Plot for Head TSL

DASY5 Validation Report for Body TSL

Date: 11.03.2019

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 450 MHz; Type: D450V3; Serial: D450V3 - SN:1054

Communication System: UID 0 - CW; Frequency: 450 MHz

Medium parameters used: $f = 450 \text{ MHz}$; $\sigma = 0.93 \text{ S/m}$; $\epsilon_r = 55.7$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(10.7, 10.7, 10.7) @ 450 MHz; Calibrated: 31.12.2018
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 05.07.2018
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52 52.10.2(1495); SEMCAD X 14.6.12(7450)

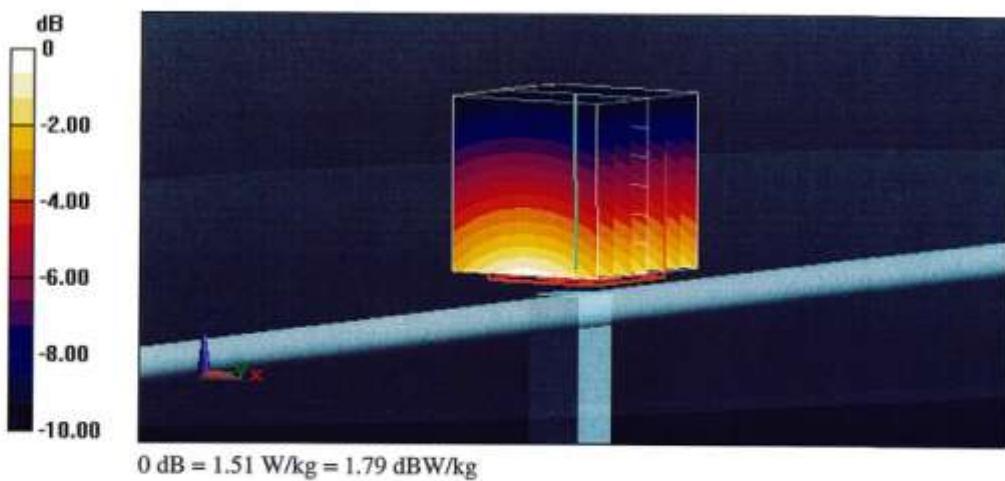
Dipole Calibration for Body Tissue/d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0:Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

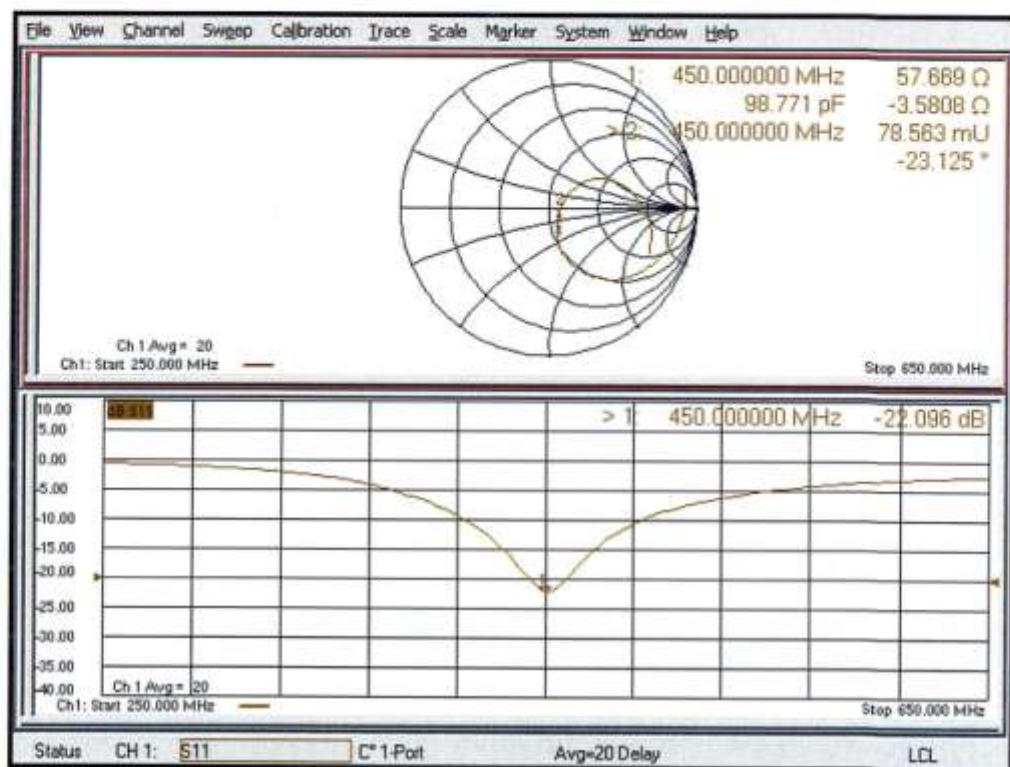
Reference Value = 41.61 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 1.73 W/kg

SAR(1 g) = 1.13 W/kg; SAR(10 g) = 0.762 W/kg

Maximum value of SAR (measured) = 1.51 W/kg



Impedance Measurement Plot for Body TSL

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client Motorola Solutions MY

Certificate No: D450V3-1053_Oct18

CALIBRATION CERTIFICATE

Object D450V3 - SN:1053

Calibration procedure(s) QA CAL-15.v8
Calibration procedure for dipole validation kits below 700 MHz

Calibration date: October 19, 2018

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-18 (No. 217-02672/02673)	Apr-19
Power sensor NRP-Z91	SN: 103244	04-Apr-18 (No. 217-02672)	Apr-19
Power sensor NRP-Z91	SN: 103245	04-Apr-18 (No. 217-02673)	Apr-19
Reference 20 dB Attenuator	SN: 5277 (20x)	04-Apr-18 (No. 217-02682)	Apr-19
Type-N mismatch combination	SN: 5047.2 / 06327	04-Apr-18 (No. 217-02683)	Apr-19
Reference Probe EX3DV4	SN: 3877	30-Dec-17 (No. EX3-3877_Dec17)	Dec-18
DAE4	SN: 654	05-Jul-18 (No. DAE4-654_Jul18)	Jul-19

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	12-Jun-18 (No. 217-02285/02284)	In house check: Jun-20
Power sensor E4412A	SN: MY41498087	12-Jun-18 (No. 217-02285)	In house check: Jun-20
Power sensor E4412A	SN: 000110210	12-Jun-18 (No. 217-02284)	In house check: Jun-20
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-18)	In house check: Jun-20
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-18)	In house check: Oct-19

Calibrated by:	Name	Function	Signature
	Claudio Leubler	Laboratory Technician	

Approved by:	Name	Function	Signature
	Katja Pokovic	Technical Manager	

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Issued: October 19, 2018

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.2
Extrapolation	Advanced Extrapolation	
Phantom	ELI4 Flat Phantom	Shell thickness: 2 ± 0.2 mm
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	$dx, dy, dz = 5$ mm	
Frequency	450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	43.5	0.87 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	44.1 ± 6 %	0.87 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	1.14 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	4.57 W/kg ± 18.1 % (k=2)

SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	0.762 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	3.05 W/kg ± 17.6 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	56.7	0.94 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	55.5 ± 6 %	0.92 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	1.12 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	4.53 W/kg ± 18.1 % (k=2)

SAR averaged over 10 cm³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	0.753 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	3.05 W/kg ± 17.6 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	$57.6 \Omega - 4.4 j\Omega$
Return Loss	- 21.7 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	$55.1 \Omega - 7.0 j\Omega$
Return Loss	- 21.7 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.351 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	December 16, 2005

DASY5 Validation Report for Head TSL

Date: 19.10.2018

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 450 MHz; Type: D450V3; Serial: D450V3 - SN:1053

Communication System: UID 0 - CW; Frequency: 450 MHz

Medium parameters used: $f = 450 \text{ MHz}$; $\sigma = 0.87 \text{ S/m}$; $\epsilon_r = 44.1$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(10.5, 10.5, 10.5) @ 450 MHz; Calibrated: 30.12.2017
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 05.07.2018
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52 52.10.2(1495); SEMCAD X 14.6.12(7450)

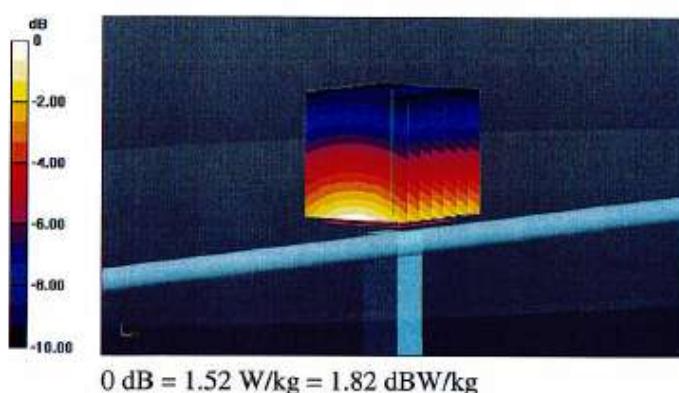
Dipole Calibration for Head Tissue/d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0:Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Reference Value = 38.89 V/m; Power Drift = -0.00 dB

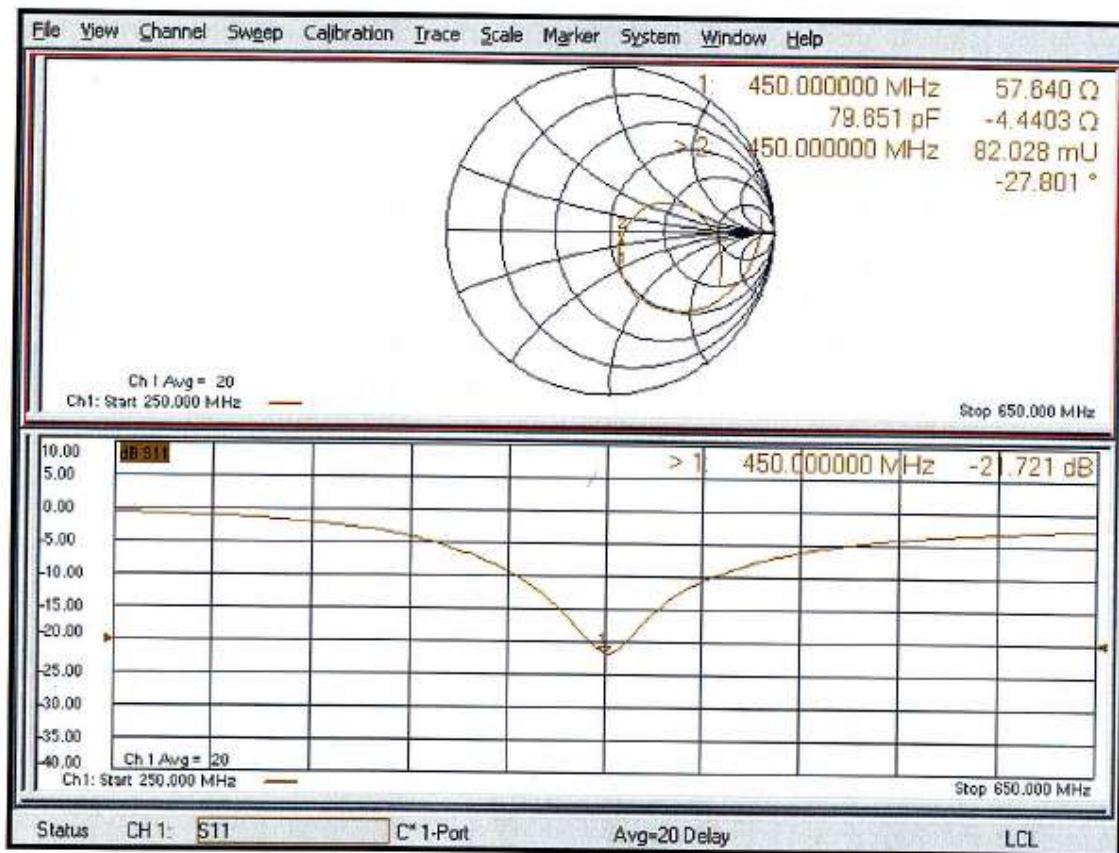
Peak SAR (extrapolated) = 1.74 W/kg

SAR(1 g) = 1.14 W/kg; SAR(10 g) = 0.762 W/kg

Maximum value of SAR (measured) = 1.52 W/kg



$$0 \text{ dB} = 1.52 \text{ W/kg} = 1.82 \text{ dBW/kg}$$

Impedance Measurement Plot for Head TSL

DASY5 Validation Report for Body TSL

Date: 19.10.2018

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 450 MHz; Type: D450V3; Serial: D450V3 - SN:1053

Communication System: UID 0 - CW; Frequency: 450 MHz

Medium parameters used: $f = 450 \text{ MHz}$; $\sigma = 0.92 \text{ S/m}$; $\epsilon_r = 55.5$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(10.8, 10.8, 10.8) @ 450 MHz; Calibrated: 30.12.2017
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 05.07.2018
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52 52.10.2(1495); SEMCAD X 14.6.12(7450)

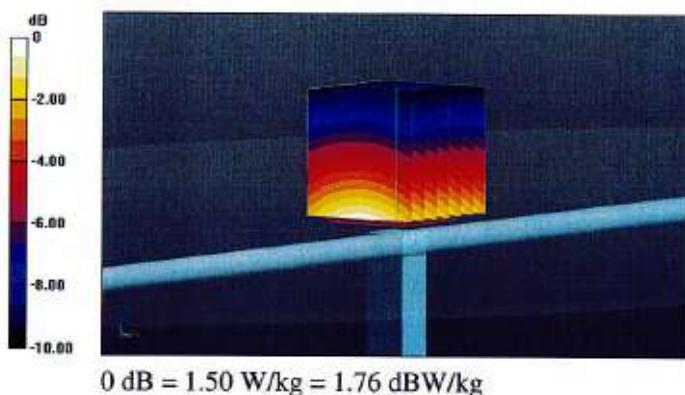
Dipole Calibration for Body Tissue/d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0:Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

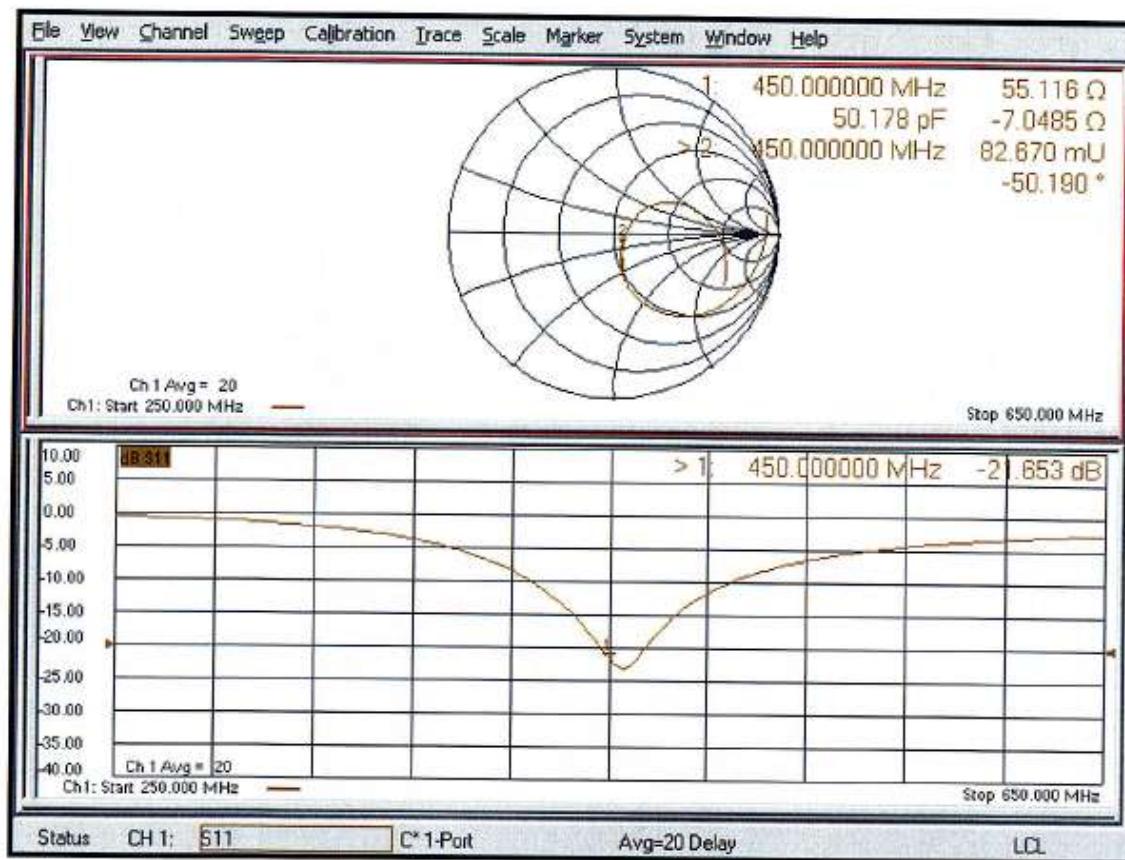
Reference Value = 41.78 V/m; Power Drift = -0.04 dB

Peak SAR (extrapolated) = 1.72 W/kg

SAR(1 g) = 1.12 W/kg; SAR(10 g) = 0.753 W/kg

Maximum value of SAR (measured) = 1.50 W/kg



Impedance Measurement Plot for Body TSL

Dipole Data

As stated in KDB 865664, only dipoles used for longer calibration intervals required to provide supporting information and measurement to qualify for extended calibration interval.

Dipole 450-1054	Head		
	Impedance		Return Loss
Date Measured	real Ω	imag $j\Omega$	dB
04/08/2019	59.46	-4.57	-20.36
04/13/2020	57.08	-6.58	-20.38

Dipole 450-1053	Head		
	Impedance		Return Loss
Date Measured	real Ω	imag $j\Omega$	dB
11/08/2018	53.78	-7.39	-21.97
11/10/2019	53.95	-6.72	-22.49