



## DECLARATION OF COMPLIANCE SAR ASSESSMENT PCII REPORT Part 2 of 2

<b>Motorola Solutions Inc.</b> <b>EME Test Laboratory</b> Motorola Solutions Malaysia Sdn Bhd Plot 2A, Medan Bayan Lepas, Mukim 12 SWD 11900 Bayan Lepas Penang, Malaysia.	<b>Date of Report:</b> 10/25/2022 <b>Report Revision:</b> B
----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------	----------------------------------------------------------------

**Responsible Engineer:** Saw Sun Hock (Senior EME Engineer)  
**Report Author:** Lee Kin Kting (EME Technician)  
**Date/s Tested:** 7/19/2022-7/20/2022, 07/26/2022, 08/30/2022, 09/04/2022  
**Manufacturer:** Motorola Solutions Inc.  
**DUT Description:** Handheld Portable – Curve 1W 900 MHZ 10CH (BRUS/BRCAN)  
**Test TX mode(s):** ISM & WLAN  
**Max. Power output:** Refer Table 3  
**Tx Frequency Bands:** Refer Table 3  
**Signaling type:** FSK, DSSS, OFDM  
**Model(s) Tested:** DLR110NBHLAA(HVIN: DLR110NB1)(PMUF1982A)  
**Model(s) Certified:** DLR110NBHLAA(HVIN: DLR110NB1)(PMUF1982A)  
 DLR110NBHLAB(HVIN: DLR110NB2)(PMUF1982A)  
**Firmware Version (FVIN):** R01.01.00  
**Serial Number(s):** 55017YL0119  
**Classification:** General Population/Uncontrolled  
**Applicant Name:** Motorola Solutions Inc.  
**Applicant Address:** 8000 West Sunrise Boulevard, Fort Lauderdale, Florida 33322  
**FCC ID:** AZ489FT7146; ISM 902-928MHz, WLAN 2.4GHz and 5GHz  
**IC:** 109U-89FT7146; ISM 902-928MHz, WLAN 2.4GHz and 5GHz  
  
**ISED Test Site registration:** 24843  
**FCC Test Firm Registration Number:** 823256

The test results clearly demonstrate compliance with FCC General Population/Uncontrolled RF Exposure limits of 1.6 W/kg averaged over 1 gram per the requirements of FCC 47 CFR § 2.1093 and RSS-102 (Issue 5).

Based on the information and the testing results provided herein, the undersigned certifies that when used as stated in the operating instructions supplied, said product complies with the national and international reference standards and guidelines listed in section 4.0 of this report (no deviation from standard methods). This report shall not be reproduced without written approval from an officially designated representative of the Motorola Solutions Inc EME Laboratory.

I attest to the accuracy of the data and assume full responsibility for the completeness of these measurements. This reporting format is consistent with the suggested guidelines of the TIA TSB-150 December 2004. The results and statements contained in this report pertain only to the device(s) evaluated.

**Tey Pei Loo (Approved Signatory)**  
**Approval Date: 10/25/2022**

## **Appendix C**

### **Dipole Calibration Certificates**

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
**Zeughausstrasse 43, 8004 Zurich, Switzerland**



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**Client **Motorola Solutions MY**Certificate No: **D835V2-4d029\_Aug21**

## CALIBRATION CERTIFICATE

Object **D835V2 - SN:4d029**

Calibration procedure(s) **QA CAL-05.v11**  
Calibration Procedure for SAR Validation Sources between 0.7-3 GHz

Calibration date: **August 27, 2021**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	09-Apr-21 (No. 217-03291/03292)	Apr-22
Power sensor NRP-Z91	SN: 103244	09-Apr-21 (No. 217-03291)	Apr-22
Power sensor NRP-Z91	SN: 103245	09-Apr-21 (No. 217-03292)	Apr-22
Reference 20 dB Attenuator	SN: BH9394 (20k)	09-Apr-21 (No. 217-03343)	Apr-22
Type-N mismatch combination	SN: 310982 / 06327	09-Apr-21 (No. 217-03344)	Apr-22
Reference Probe EX3DV4	SN: 7349	28-Dec-20 (No. EX3-7349_Dec20)	Dec-21
DAE4	SN: 601	02-Nov-20 (No. DAE4-601_Nov20)	Nov-21
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oct-20)	In house check: Oct-22
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-20)	In house check: Oct-22
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-20)	In house check: Oct-22
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-20)	In house check: Oct-22
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-20)	In house check: Oct-21

Calibrated by:	Name	Function	Signature
	Jeffrey Katzman	Laboratory Technician	

Approved by:	Name	Function	Signature
	Katja Pokovic	Technical Manager	

Issued: August 27, 2021

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
**Zeughausstrasse 43, 8004 Zurich, Switzerland**



**S** Schweizerischer Kaliibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

#### Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

#### Calibration is Performed According to the Following Standards:

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Additional Documentation:

- DASY System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:* The source is mounted in a touch configuration below the center marking of the flat phantom.
- Return Loss:* This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- SAR measured:* SAR measured at the stated antenna input power.
- SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

<b>DASY Version</b>	DASY52	V52.10.4
<b>Extrapolation</b>	Advanced Extrapolation	
<b>Phantom</b>	Modular Flat Phantom	
<b>Distance Dipole Center - TSL</b>	15 mm	with Spacer
<b>Zoom Scan Resolution</b>	dx, dy, dz = 5 mm	
<b>Frequency</b>	835 MHz ± 1 MHz	

**Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
<b>Nominal Head TSL parameters</b>	22.0 °C	41.5	0.90 mho/m
<b>Measured Head TSL parameters</b>	(22.0 ± 0.2) °C	41.6 ± 6 %	0.92 mho/m ± 6 %
<b>Head TSL temperature change during test</b>	< 0.5 °C	----	----

**SAR result with Head TSL**

<b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>	Condition	
SAR measured	250 mW input power	2.50 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	9.84 W/kg ± 17.0 % (k=2)
<b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b>	condition	
SAR measured	250 mW input power	1.61 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	6.36 W/kg ± 16.5 % (k=2)

**Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
<b>Nominal Body TSL parameters</b>	22.0 °C	55.2	0.97 mho/m
<b>Measured Body TSL parameters</b>	(22.0 ± 0.2) °C	54.9 ± 6 %	0.99 mho/m ± 6 %
<b>Body TSL temperature change during test</b>	< 0.5 °C	----	----

**SAR result with Body TSL**

<b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Body TSL</b>	Condition	
SAR measured	250 mW input power	2.50 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	9.83 W/kg ± 17.0 % (k=2)
<b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Body TSL</b>	condition	
SAR measured	250 mW input power	1.66 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	6.62 W/kg ± 16.5 % (k=2)

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with Head TSL**

Impedance, transformed to feed point	51.0 $\Omega$ - 2.5 $j\Omega$
Return Loss	- 31.6 dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	50.0 $\Omega$ - 5.7 $j\Omega$
Return Loss	- 24.9 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.387 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
-----------------	-------

**DASY5 Validation Report for Head TSL**

Date: 27.08.2021

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:4d029**

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used:  $f = 835 \text{ MHz}$ ;  $\sigma = 0.92 \text{ S/m}$ ;  $\epsilon_r = 41.6$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(9.69, 9.69, 9.69) @ 835 MHz; Calibrated: 28.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 02.11.2020
- Phantom: Flat Phantom 4.9 (front); Type: QD 00L P49 AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:**Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$ 

Reference Value = 64.05 V/m; Power Drift = -0.00 dB


Peak SAR (extrapolated) = 3.80 W/kg


**SAR(1 g) = 2.5 W/kg; SAR(10 g) = 1.61 W/kg**

Smallest distance from peaks to all points 3 dB below = 16 mm

Ratio of SAR at M2 to SAR at M1 = 65.6%

Maximum value of SAR (measured) = 3.36 W/kg

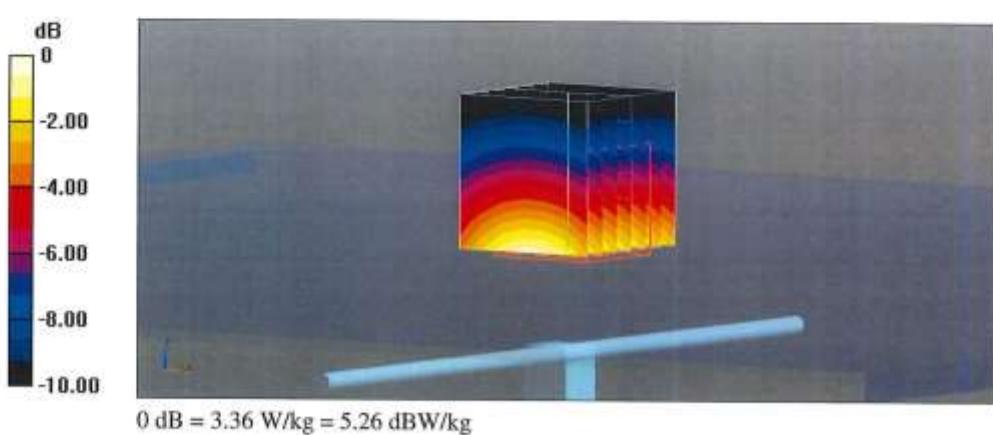

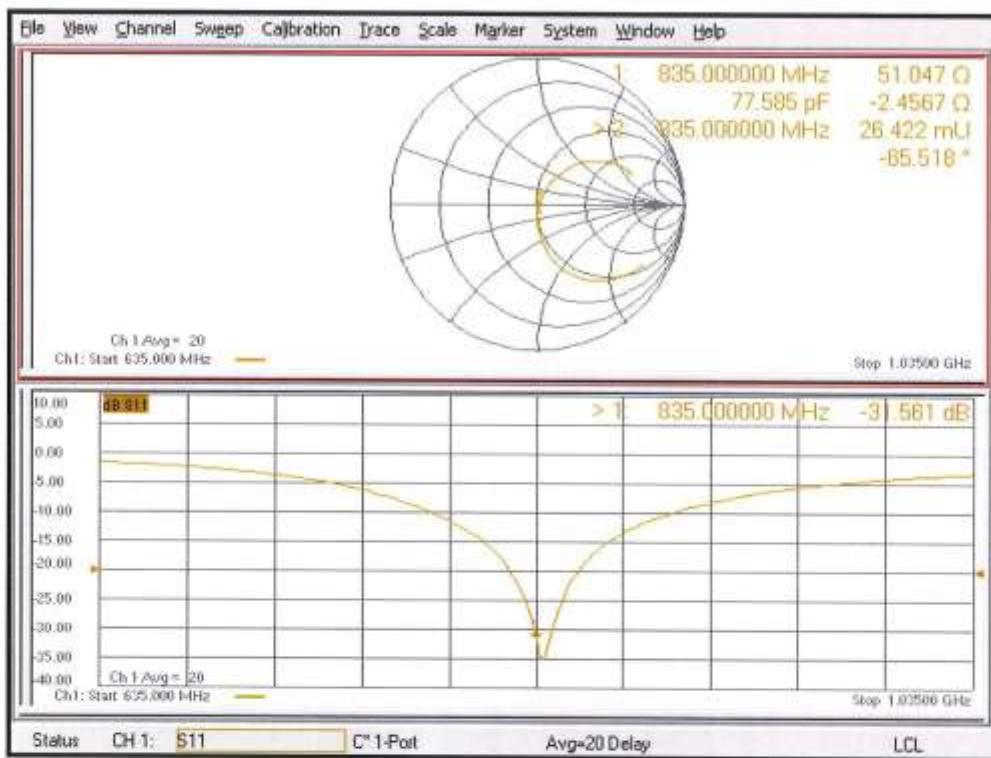**Impedance Measurement Plot for Head TSL**

**DASY5 Validation Report for Body TSL**

Date: 27.08.2021

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:4d029**

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used:  $f = 835 \text{ MHz}$ ;  $\sigma = 0.99 \text{ S/m}$ ;  $\epsilon_r = 54.9$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(9.85, 9.85, 9.85) @ 835 MHz; Calibrated: 28.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 02.11.2020
- Phantom: Flat Phantom 4.9 (Back); Type: QD 00R P49 AA; Serial: 1005
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:**Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$ 

Reference Value = 59.18 V/m; Power Drift = -0.06 dB


Peak SAR (extrapolated) = 3.57 W/kg


**SAR(1 g) = 2.50 W/kg; SAR(10 g) = 1.68 W/kg**

Smallest distance from peaks to all points 3 dB below = 17 mm

Ratio of SAR at M2 to SAR at M1 = 70.1%

Maximum value of SAR (measured) = 3.24 W/kg

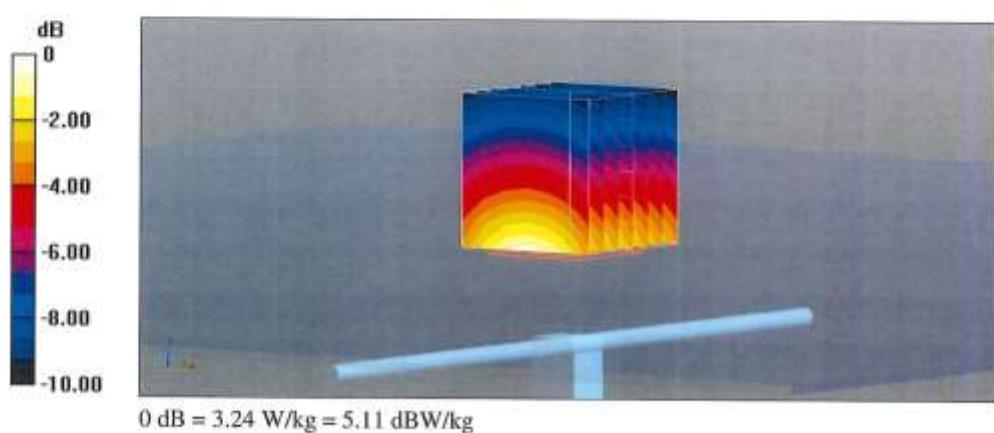

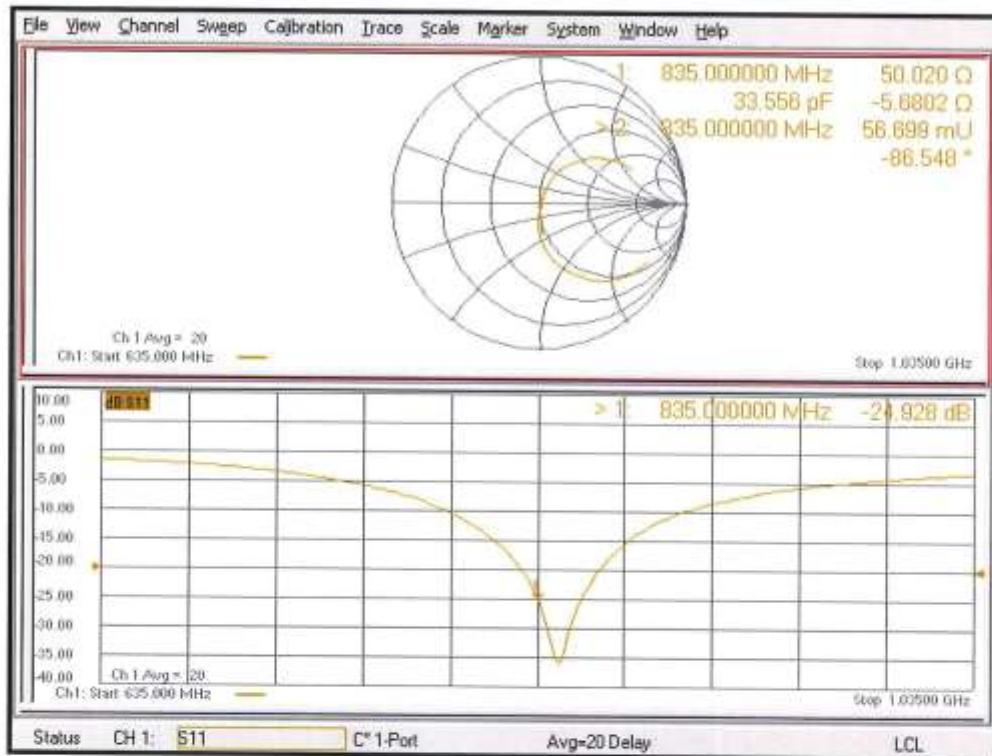**Impedance Measurement Plot for Body TSL**

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
**Zeughausstrasse 43, 8004 Zurich, Switzerland**



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**C** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client **Motorola Solutions MY**

Certificate No: D900V2-1d026\_Feb20

## CALIBRATION CERTIFICATE

Object **D900V2 - SN:1d026**

Calibration procedure(s) **QA CAL-05.v11**  
 Calibration Procedure for SAR Validation Sources between 0.7-3 GHz

Calibration date: **February 24, 2020**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	03-Apr-19 (No. 217-02892/02893)	Apr-20
Power sensor NRP-Z91	SN: 103244	03-Apr-19 (No. 217-02892)	Apr-20
Power sensor NRP-Z91	SN: 103245	03-Apr-19 (No. 217-02893)	Apr-20
Reference 20 dB Attenuator	SN: 5058 (20k)	04-Apr-19 (No. 217-02894)	Apr-20
Type-N mismatch combination	SN: 5047.2 / 06327	04-Apr-19 (No. 217-02895)	Apr-20
Reference Probe EX3DV4	SN: 7349	31-Dec-19 (No. EX3-7349_Dec19)	Dec-20
DAE4	SN: 601	27-Dec-19 (No. DAE4-601_Dec19)	Dec-20
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Feb-19)	In house check: Oct-20
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-18)	In house check: Oct-20
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-18)	In house check: Oct-20
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-18)	In house check: Oct-20
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-19)	In house check: Oct-20

Calibrated by: Name **Michael Weber** Function **Laboratory Technician**

Signature

Approved by: Name **Katja Pokovic** Function **Technical Manager**

Issued: February 24, 2020

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
**Zeughausstrasse 43, 8004 Zurich, Switzerland**



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

#### Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Additional Documentation:

- e) DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

<b>DASY Version</b>	DASY5	V52.10.4
<b>Extrapolation</b>	Advanced Extrapolation	
<b>Phantom</b>	Modular Flat Phantom	
<b>Distance Dipole Center - TSL</b>	15 mm	with Spacer
<b>Zoom Scan Resolution</b>	dx, dy, dz = 5 mm	
<b>Frequency</b>	900 MHz ± 1 MHz	

**Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
<b>Nominal Head TSL parameters</b>	22.0 °C	41.5	0.97 mho/m
<b>Measured Head TSL parameters</b>	(22.0 ± 0.2) °C	42.6 ± 6 %	0.93 mho/m ± 6 %
<b>Head TSL temperature change during test</b>	< 0.5 °C	---	---

**SAR result with Head TSL**

<b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>	Condition	
SAR measured	250 mW input power	2.70 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	11.2 W/kg ± 17.0 % (k=2)
<b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b>	condition	
SAR measured	250 mW input power	1.74 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	7.16 W/kg ± 16.5 % (k=2)

**Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
<b>Nominal Body TSL parameters</b>	22.0 °C	55.0	1.05 mho/m
<b>Measured Body TSL parameters</b>	(22.0 ± 0.2) °C	55.1 ± 6 %	1.02 mho/m ± 6 %
<b>Body TSL temperature change during test</b>	< 0.5 °C	---	---

**SAR result with Body TSL**

<b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Body TSL</b>	Condition	
SAR measured	250 mW input power	2.68 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	11.0 W/kg ± 17.0 % (k=2)
<b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Body TSL</b>	condition	
SAR measured	250 mW input power	1.75 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	7.12 W/kg ± 16.5 % (k=2)

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with Head TSL**

Impedance, transformed to feed point	50.7 $\Omega$ - 0.1 $j\Omega$
Return Loss	- 43.4 dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	47.0 $\Omega$ - 2.1 $j\Omega$
Return Loss	- 28.4 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.402 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
-----------------	-------

**DASY5 Validation Report for Head TSL**

Date: 21.02.2020

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 900 MHz; Type: D900V2; Serial: D900V2 - SN:1d026**

Communication System: UID 0 - CW; Frequency: 900 MHz

Medium parameters used:  $f = 900 \text{ MHz}$ ;  $\sigma = 0.93 \text{ S/m}$ ;  $\epsilon_r = 42.6$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(9.79, 9.79, 9.79) @ 900 MHz; Calibrated: 31.12.2019
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 27.12.2019
- Phantom: Flat Phantom 4.9 (front); Type: QD 00L P49 AA; Serial: 1001
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

**Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:**Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$ 

Reference Value = 65.78 V/m; Power Drift = 0.02 dB


Peak SAR (extrapolated) = 4.08 W/kg


**SAR(1 g) = 2.7 W/kg; SAR(10 g) = 1.74 W/kg**

Smallest distance from peaks to all points 3 dB below = 16 mm

Ratio of SAR at M2 to SAR at M1 = 66.2%

Maximum value of SAR (measured) = 3.60 W/kg

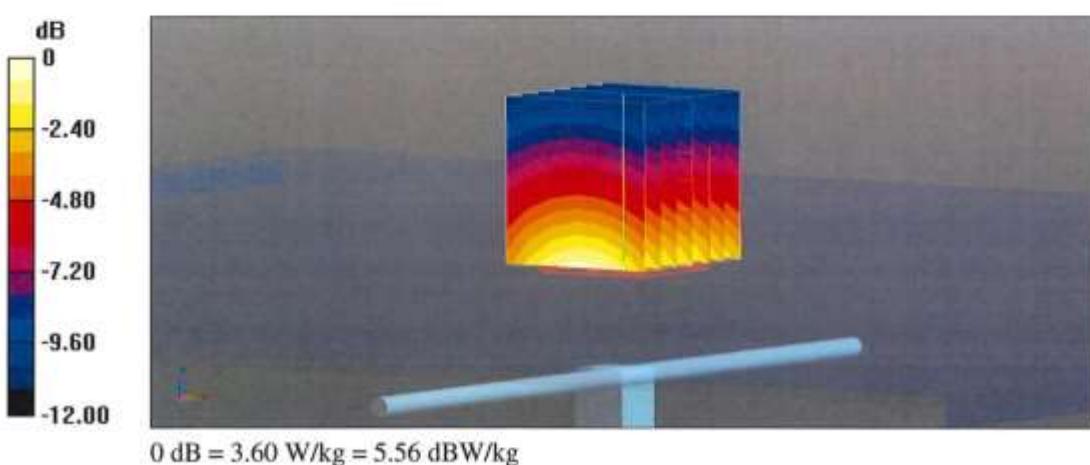

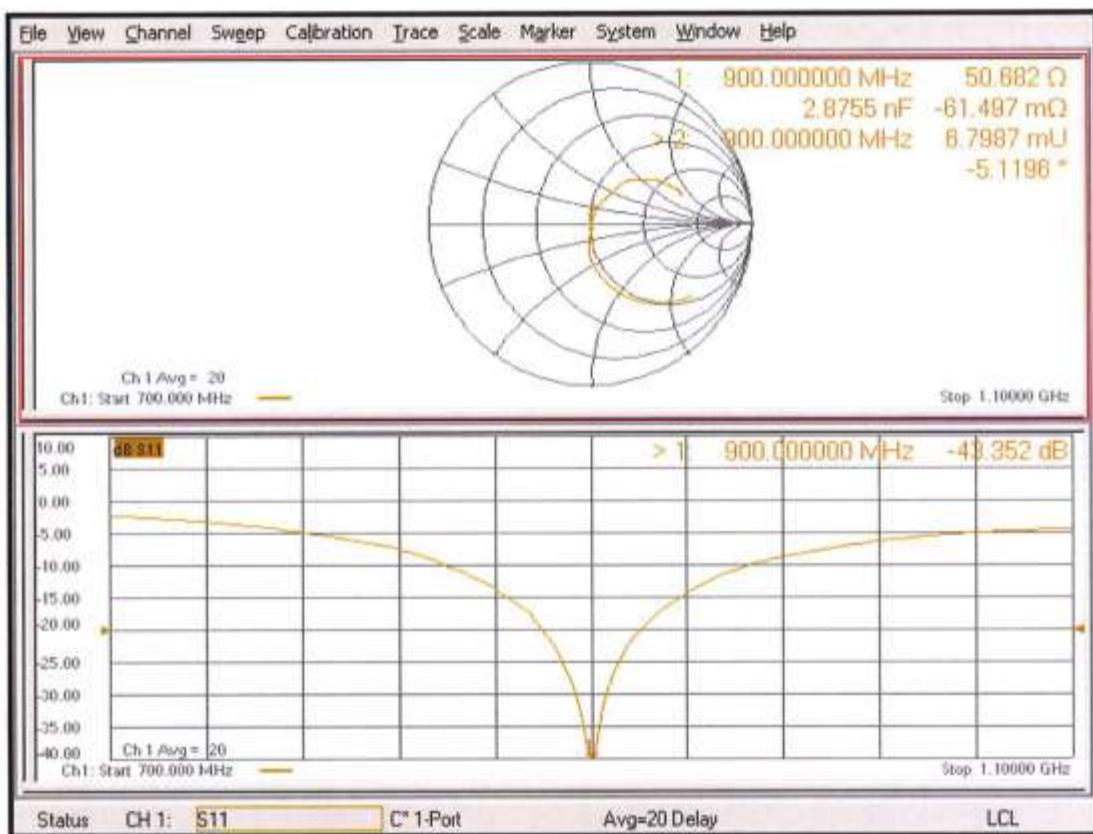**Impedance Measurement Plot for Head TSL**

**DASY5 Validation Report for Body TSL**

Date: 24.02.2020

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 900 MHz; Type: D900V2; Serial: D900V2 - SN:1d026**

Communication System: UID 0 - CW; Frequency: 900 MHz

Medium parameters used:  $f = 900 \text{ MHz}$ ;  $\sigma = 1.02 \text{ S/m}$ ;  $\epsilon_r = 55.1$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(10.05, 10.05, 10.05) @ 900 MHz; Calibrated: 31.12.2019
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 27.12.2019
- Phantom: Flat Phantom 4.9 (Back); Type: QD 00R P49 AA; Serial: 1005
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

**Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:**Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$ 

Reference Value = 60.45 V/m; Power Drift = 0.03 dB


Peak SAR (extrapolated) = 3.94 W/kg


**SAR(1 g) = 2.68 W/kg; SAR(10 g) = 1.75 W/kg**

Smallest distance from peaks to all points 3 dB below = 14.9 mm

Ratio of SAR at M2 to SAR at M1 = 67.8%

Maximum value of SAR (measured) = 3.55 W/kg

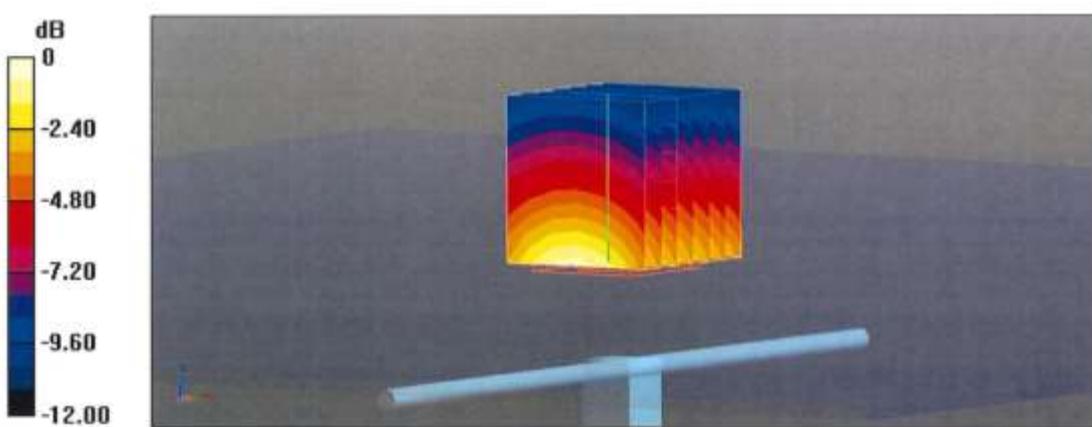

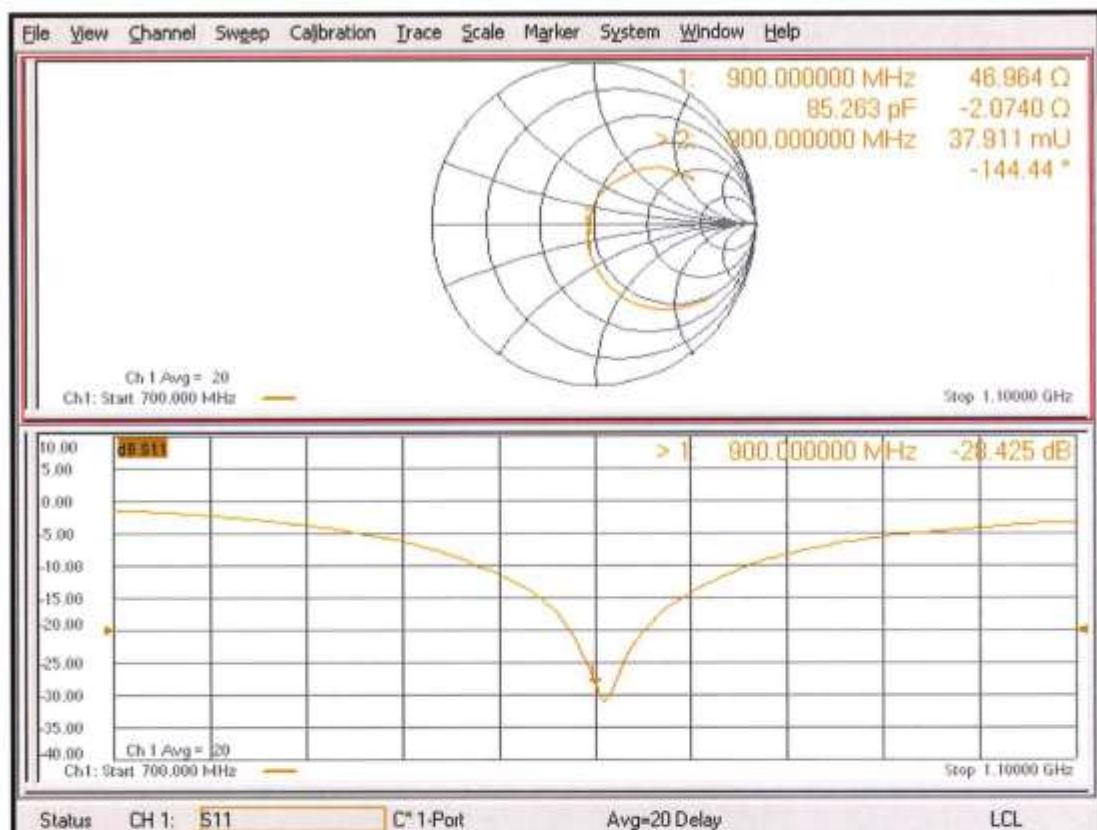**Impedance Measurement Plot for Body TSL**

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
**Zeughausstrasse 43, 8004 Zurich, Switzerland**



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**C** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**Client **Motorola Solutions MY**Certificate No: **D2450V2-781\_Oct21**

## CALIBRATION CERTIFICATE

Object **D2450V2 - SN:781**

Calibration procedure(s) **QA CAL-05.v11**  
Calibration Procedure for SAR Validation Sources between 0.7-3 GHz

Calibration date: **October 13, 2021**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	09-Apr-21 (No. 217-03291/03292)	Apr-22
Power sensor NRP-Z91	SN: 103244	09-Apr-21 (No. 217-03291)	Apr-22
Power sensor NRP-Z91	SN: 103245	09-Apr-21 (No. 217-03292)	Apr-22
Reference 20 dB Attenuator	SN: BH9394 (20k)	09-Apr-21 (No. 217-03343)	Apr-22
Type-N mismatch combination	SN: 310982 / 08327	09-Apr-21 (No. 217-03344)	Apr-22
Reference Probe EX3DV4	SN: 7349	28-Dec-20 (No. EX3-7349_Dec20)	Dec-21
DAE4	SN: 601	02-Nov-20 (No. DAE4-601_Nov20)	Nov-21
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oct-20)	In house check: Oct-22
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-20)	In house check: Oct-22
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-20)	In house check: Oct-22
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-20)	In house check: Oct-22
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-20)	In house check: Oct-22

Calibrated by:	Name: Jeton Kastrati	Function: Laboratory Technician	Signature:
----------------	----------------------	---------------------------------	------------

Approved by:	Katja Pokovic	Technical Manager	Signature:
--------------	---------------	-------------------	------------

Issued: October 14, 2021

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
**Zeughausstrasse 43, 8004 Zurich, Switzerland**



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

#### Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

#### Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Additional Documentation:

- c) DASY System Handbook

#### Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The source is mounted in a touch configuration below the center marking of the flat phantom.
- *Return Loss:* This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

<b>DASY Version</b>	DASY52	V52.10.4
<b>Extrapolation</b>	Advanced Extrapolation	
<b>Phantom</b>	Modular Flat Phantom	
<b>Distance Dipole Center - TSL</b>	10 mm	with Spacer
<b>Zoom Scan Resolution</b>	dx, dy, dz = 5 mm	
<b>Frequency</b>	2450 MHz ± 1 MHz	

**Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
<b>Nominal Head TSL parameters</b>	22.0 °C	39.2	1.80 mho/m
<b>Measured Head TSL parameters</b>	(22.0 ± 0.2) °C	37.6 ± 6 %	1.89 mho/m ± 6 %
<b>Head TSL temperature change during test</b>	< 0.5 °C	---	---

**SAR result with Head TSL**

<b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>	Condition	
SAR measured	250 mW input power	13.6 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	52.7 W/kg ± 17.0 % (k=2)
<b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b>	condition	
SAR measured	250 mW Input power	6.26 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.6 W/kg ± 16.5 % (k=2)

**Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
<b>Nominal Body TSL parameters</b>	22.0 °C	52.7	1.95 mho/m
<b>Measured Body TSL parameters</b>	(22.0 ± 0.2) °C	52.2 ± 6 %	2.05 mho/m ± 6 %
<b>Body TSL temperature change during test</b>	< 0.5 °C	---	---

**SAR result with Body TSL**

<b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Body TSL</b>	Condition	
SAR measured	250 mW input power	13.1 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	51.1 W/kg ± 17.0 % (k=2)
<b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Body TSL</b>	condition	
SAR measured	250 mW input power	6.18 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	24.4 W/kg ± 16.5 % (k=2)

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with Head TSL**

Impedance, transformed to feed point	$52.8 \Omega + 3.4 j\Omega$
Return Loss	- 27.4 dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	$49.3 \Omega + 6.4 j\Omega$
Return Loss	- 23.7 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.152 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
-----------------	-------

**DASY5 Validation Report for Head TSL**

Date: 13.10.2021

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:781**

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used:  $f = 2450 \text{ MHz}$ ;  $\sigma = 1.89 \text{ S/m}$ ;  $\epsilon_r = 37.6$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.96, 7.96, 7.96) @ 2450 MHz; Calibrated: 28.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 02.11.2020
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$ 

Reference Value = 118.0 V/m; Power Drift = 0.01 dB


Peak SAR (extrapolated) = 27.0 W/kg


**SAR(1 g) = 13.6 W/kg; SAR(10 g) = 6.26 W/kg**

Smallest distance from peaks to all points 3 dB below = 9 mm

Ratio of SAR at M2 to SAR at M1 = 50.4%

Maximum value of SAR (measured) = 22.3 W/kg

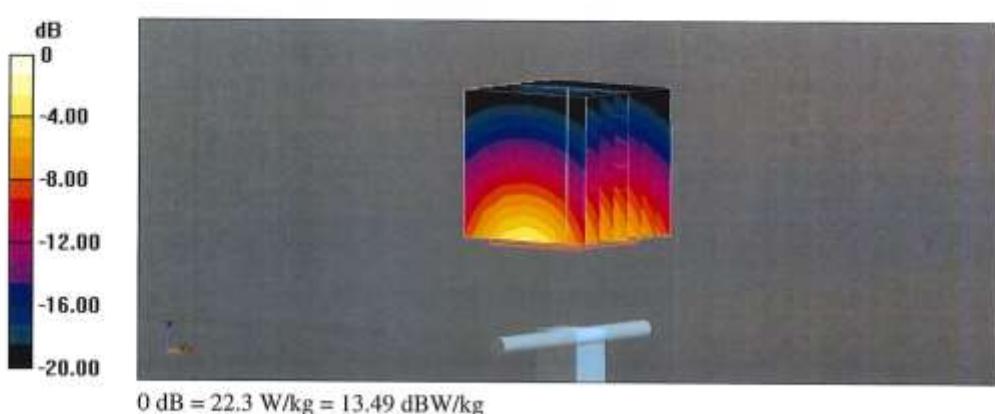

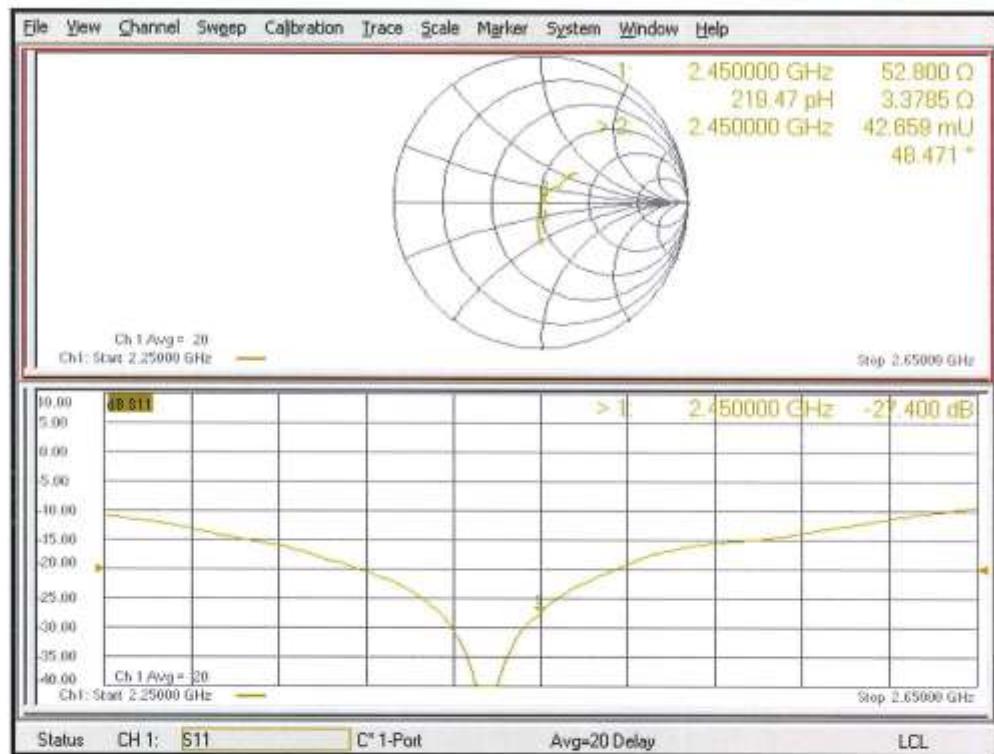**Impedance Measurement Plot for Head TSL**

**DASY5 Validation Report for Body TSL**

Date: 13.10.2021

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:781**

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used:  $f = 2450 \text{ MHz}$ ;  $\sigma = 2.05 \text{ S/m}$ ;  $\epsilon_r = 52.2$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.12, 8.12, 8.12) @ 2450 MHz; Calibrated: 28.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 02.11.2020
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$ 

Reference Value = 109.7 V/m; Power Drift = -0.05 dB


Peak SAR (extrapolated) = 24.1 W/kg


SAR(1 g) = 13.1 W/kg; SAR(10 g) = 6.18 W/kg

Smallest distance from peaks to all points 3 dB below = 8.9 mm

Ratio of SAR at M2 to SAR at M1 = 54.8%

Maximum value of SAR (measured) = 20.6 W/kg

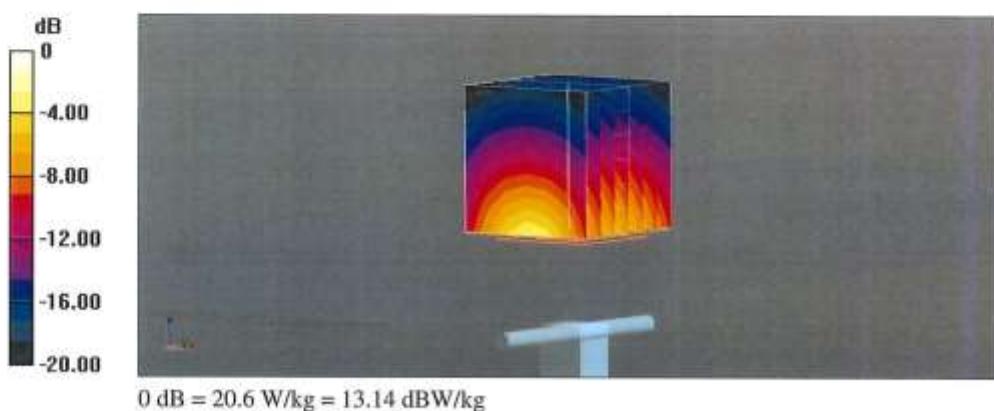

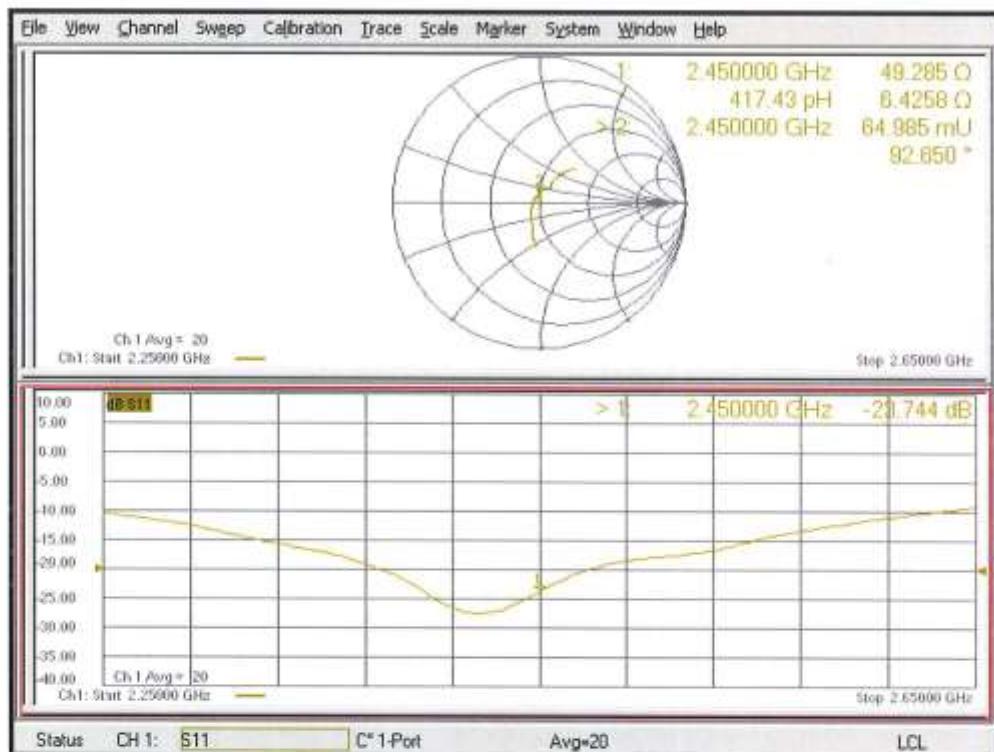**Impedance Measurement Plot for Body TSL**

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
**Zeughausstrasse 43, 8004 Zurich, Switzerland**



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**Client **Motorola Solutions MY**Certificate No: **D5GHzV2-1026\_Sep21**

## CALIBRATION CERTIFICATE

Object **D5GHzV2 - SN:1026**

Calibration procedure(s) **QA CAL-22.v6**  
Calibration Procedure for SAR Validation Sources between 3-10 GHz

Calibration date: **September 24, 2021**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	09-Apr-21 (No. 217-03291/03292)	Apr-22
Power sensor NRP-Z91	SN: 103244	09-Apr-21 (No. 217-03291)	Apr-22
Power sensor NRP-Z91	SN: 103245	09-Apr-21 (No. 217-03292)	Apr-22
Reference 20 dB Attenuator	SN: BH9394 (20k)	09-Apr-21 (No. 217-03343)	Apr-22
Type-N mismatch combination	SN: 310982 / 06327	09-Apr-21 (No. 217-03344)	Apr-22
Reference Probe EX3DV4	SN: 3503	30-Dec-20 (No. EX3-3503_Dec20)	Dec-21
DAE4	SN: 601	02-Nov-20 (No. DAE4-601_Nov20)	Nov-21

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oct-20)	In house check: Oct-22
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-20)	In house check: Oct-22
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-20)	In house check: Oct-22
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-20)	In house check: Oct-22
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-20)	In house check: Oct-21

Calibrated by:	Name	Function	Signature
	Jeton Kastrati	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	

Issued: September 24, 2021

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
**Zeughausstrasse 43, 8004 Zurich, Switzerland**



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**Swiss Calibration Service**

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

#### Glossary:

<b>TSL</b>	tissue simulating liquid
<b>ConvF</b>	sensitivity in TSL / NORM x,y,z
<b>N/A</b>	not applicable or not measured

#### Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Additional Documentation:

- c) DASY System Handbook

#### Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The source is mounted in a touch configuration below the center marking of the flat phantom.
- *Return Loss:* This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	V52.10.4
<b>Extrapolation</b>	Advanced Extrapolation	
<b>Phantom</b>	Modular Flat Phantom V5.0	
<b>Distance Dipole Center - TSL</b>	10 mm	with Spacer
<b>Zoom Scan Resolution</b>	$dx, dy = 4.0 \text{ mm}, dz = 1.4 \text{ mm}$	Graded Ratio = 1.4 (Z direction)
<b>Frequency</b>	5250 MHz $\pm 1 \text{ MHz}$ 5500 MHz $\pm 1 \text{ MHz}$ 5600 MHz $\pm 1 \text{ MHz}$ 5750 MHz $\pm 1 \text{ MHz}$	

**Head TSL parameters at 5250 MHz**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
<b>Nominal Head TSL parameters</b>	22.0 °C	35.9	4.71 mho/m
<b>Measured Head TSL parameters</b>	(22.0 $\pm 0.2$ ) °C	34.7 $\pm 6$ %	4.52 mho/m $\pm 6$ %
Head TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Head TSL at 5250 MHz**

<b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>	Condition	
SAR measured	100 mW input power	8.12 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	80.6 W/kg $\pm 19.9$ % (k=2)

<b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b>	condition	
SAR measured	100 mW input power	2.32 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.0 W/kg $\pm 19.5$ % (k=2)

**Head TSL parameters at 5500 MHz**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
<b>Nominal Head TSL parameters</b>	22.0 °C	35.6	4.96 mho/m
<b>Measured Head TSL parameters</b>	(22.0 $\pm 0.2$ ) °C	34.4 $\pm 6$ %	4.76 mho/m $\pm 6$ %
Head TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Head TSL at 5500 MHz**

<b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>	Condition	
SAR measured	100 mW input power	8.78 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	87.0 W/kg $\pm 19.9$ % (k=2)

<b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b>	condition	
SAR measured	100 mW input power	2.45 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.2 W/kg $\pm 19.5$ % (k=2)

**Head TSL parameters at 5600 MHz**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.2 ± 6 %	4.86 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	—	---

**SAR result with Head TSL at 5600 MHz**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.47 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	83.9 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.39 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.6 W/kg ± 19.5 % (k=2)

**Head TSL parameters at 5750 MHz**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.4	5.22 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.0 ± 6 %	5.01 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	—	---

**SAR result with Head TSL at 5750 MHz**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.06 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	79.7 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.27 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.4 W/kg ± 19.5 % (k=2)

**Body TSL parameters at 5250 MHz**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.9	5.36 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	48.8 ± 6 %	5.50 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Body TSL at 5250 MHz**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.50 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	75.0 W/kg ± 19.9 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.08 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	20.8 W/kg ± 19.5 % (k=2)

**Body TSL parameters at 5500 MHz**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.6	5.65 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	48.4 ± 6 %	5.85 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

**SAR result with Body TSL at 5500 MHz**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.95 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	79.6 W/kg ± 19.9 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.19 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	21.9 W/kg ± 19.5 % (k=2)

**Body TSL parameters at 5600 MHz**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.5	5.77 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	48.2 ± 6 %	5.99 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Body TSL at 5600 MHz**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.94 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	79.5 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	Condition	
SAR measured	100 mW input power	2.20 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	22.0 W/kg ± 19.5 % (k=2)

**Body TSL parameters at 5750 MHz**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.3	5.94 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	48.0 ± 6 %	6.20 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Body TSL at 5750 MHz**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.64 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	76.5 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	Condition	
SAR measured	100 mW input power	2.13 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	21.3 W/kg ± 19.5 % (k=2)

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with Head TSL at 5250 MHz**

Impedance, transformed to feed point	52.9 $\Omega$ - 4.4 $j\Omega$
Return Loss	- 25.9 dB

**Antenna Parameters with Head TSL at 5500 MHz**

Impedance, transformed to feed point	46.4 $\Omega$ + 0.5 $j\Omega$
Return Loss	- 28.6 dB

**Antenna Parameters with Head TSL at 5600 MHz**

Impedance, transformed to feed point	52.4 $\Omega$ + 0.6 $j\Omega$
Return Loss	- 32.2 dB

**Antenna Parameters with Head TSL at 5750 MHz**

Impedance, transformed to feed point	57.5 $\Omega$ + 6.5 $j\Omega$
Return Loss	- 20.7 dB

**Antenna Parameters with Body TSL at 5250 MHz**

Impedance, transformed to feed point	$50.8 \Omega - 2.6 j\Omega$
Return Loss	- 31.5 dB

**Antenna Parameters with Body TSL at 5500 MHz**

Impedance, transformed to feed point	$46.3 \Omega + 2.5 j\Omega$
Return Loss	- 26.8 dB

**Antenna Parameters with Body TSL at 5600 MHz**

Impedance, transformed to feed point	$53.4 \Omega + 1.4 j\Omega$
Return Loss	- 29.0 dB

**Antenna Parameters with Body TSL at 5750 MHz**

Impedance, transformed to feed point	$58.1 \Omega + 6.1 j\Omega$
Return Loss	- 20.6 dB

Electrical Delay (one direction)	1.193 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
-----------------	-------

**DASY5 Validation Report for Head TSL**

Date: 23.09.2021

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole D5GHzV2; Type: D5GHzV2; Serial: D5GHzV2 - SN:1026**

Communication System: UID 0 - CW; Frequency: 5250 MHz, Frequency: 5500 MHz, Frequency: 5600 MHz, Frequency: 5750 MHz

Medium parameters used:  $f = 5250 \text{ MHz}$ ;  $\sigma = 4.52 \text{ S/m}$ ;  $\epsilon_r = 34.7$ ;  $\rho = 1000 \text{ kg/m}^3$ ,Medium parameters used:  $f = 5500 \text{ MHz}$ ;  $\sigma = 4.76 \text{ S/m}$ ;  $\epsilon_r = 34.4$ ;  $\rho = 1000 \text{ kg/m}^3$ ,Medium parameters used:  $f = 5600 \text{ MHz}$ ;  $\sigma = 4.86 \text{ S/m}$ ;  $\epsilon_r = 34.2$ ;  $\rho = 1000 \text{ kg/m}^3$ ,Medium parameters used:  $f = 5750 \text{ MHz}$ ;  $\sigma = 5.01 \text{ S/m}$ ;  $\epsilon_r = 34$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(5.5, 5.5, 5.5) @ 5250 MHz, ConvF(5.25, 5.25, 5.25) @ 5500 MHz, ConvF(5.1, 5.1, 5.1) @ 5600 MHz, ConvF(5.08, 5.08, 5.08) @ 5750 MHz; Calibrated: 30.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 02.11.2020
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5250 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 79.51 V/m; Power Drift = -0.00 dB

Peak SAR (extrapolated) = 27.5 W/kg

**SAR(1 g) = 8.12 W/kg; SAR(10 g) = 2.32 W/kg**

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 71.3%

Maximum value of SAR (measured) = 18.1 W/kg

**Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 78.89 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 33.5 W/kg

**SAR(1 g) = 8.78 W/kg; SAR(10 g) = 2.45 W/kg**


Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 67.3%


Maximum value of SAR (measured) = 20.6 W/kg

**Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm  
Reference Value = 80.35 V/m; Power Drift = 0.00 dB  
Peak SAR (extrapolated) = 31.0 W/kg  
**SAR(1 g) = 8.47 W/kg; SAR(10 g) = 2.39 W/kg**  
Smallest distance from peaks to all points 3 dB below = 7.4 mm  
Ratio of SAR at M2 to SAR at M1 = 68.5%  
Maximum value of SAR (measured) = 19.5 W/kg

**Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5750 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm  
Reference Value = 76.68 V/m; Power Drift = 0.02 dB  
Peak SAR (extrapolated) = 31.2 W/kg  
**SAR(1 g) = 8.06 W/kg; SAR(10 g) = 2.27 W/kg**  
Smallest distance from peaks to all points 3 dB below = 7.4 mm  
Ratio of SAR at M2 to SAR at M1 = 66.7%  
Maximum value of SAR (measured) = 19.2 W/kg

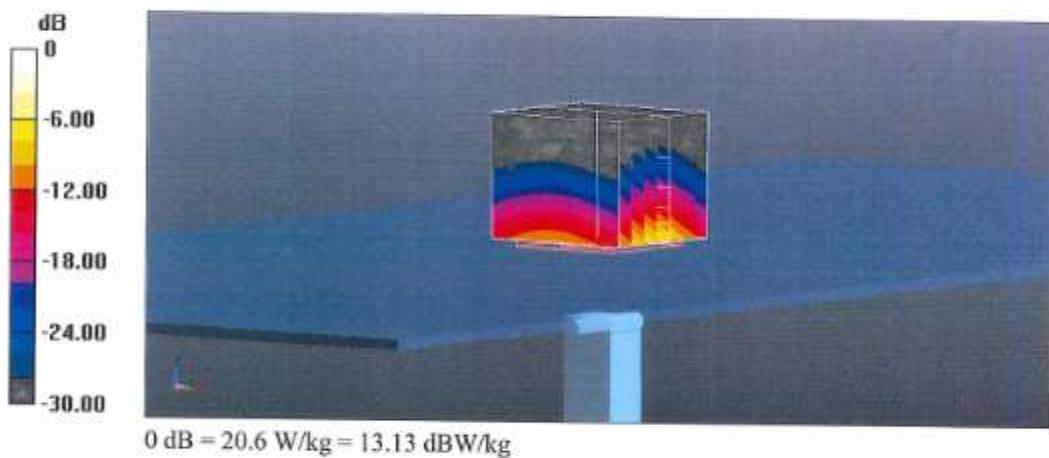

## Impedance Measurement Plot for Head TSL

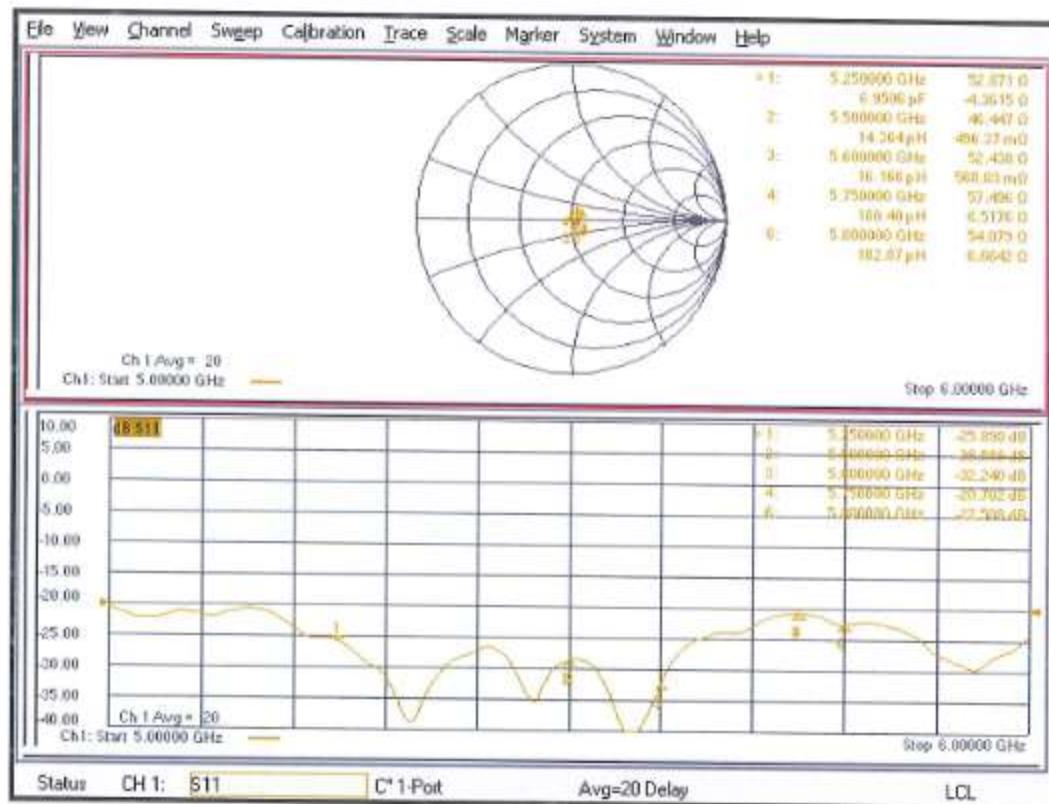

**DASY5 Validation Report for Body TSL**

Date: 24.09.2021

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole D5GHzV2; Type: D5GHzV2; Serial: D5GHzV2 - SN:1026**

Communication System: UID 0 - CW; Frequency: 5250 MHz, Frequency: 5500 MHz, Frequency: 5600 MHz, Frequency: 5750 MHz

Medium parameters used:  $f = 5250 \text{ MHz}$ ;  $\sigma = 5.5 \text{ S/m}$ ;  $\epsilon_r = 48.8$ ;  $\rho = 1000 \text{ kg/m}^3$ ,Medium parameters used:  $f = 5500 \text{ MHz}$ ;  $\sigma = 5.85 \text{ S/m}$ ;  $\epsilon_r = 48.4$ ;  $\rho = 1000 \text{ kg/m}^3$ ,Medium parameters used:  $f = 5600 \text{ MHz}$ ;  $\sigma = 5.99 \text{ S/m}$ ;  $\epsilon_r = 48.2$ ;  $\rho = 1000 \text{ kg/m}^3$ ,Medium parameters used:  $f = 5750 \text{ MHz}$ ;  $\sigma = 6.2 \text{ S/m}$ ;  $\epsilon_r = 48$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(5.26, 5.26, 5.26) @ 5250 MHz, ConvF(4.84, 4.84, 4.84) @ 5500 MHz, ConvF(4.79, 4.79, 4.79) @ 5600 MHz, ConvF(4.66, 4.66, 4.66) @ 5750 MHz; Calibrated: 30.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 02.11.2020
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5250 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:**

Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 67.65 V/m; Power Drift = -0.09 dB

Peak SAR (extrapolated) = 27.2 W/kg

**SAR(1 g) = 7.50 W/kg; SAR(10 g) = 2.08 W/kg**

Smallest distance from peaks to all points 3 dB below = 6.8 mm

Ratio of SAR at M2 to SAR at M1 = 68.6%

Maximum value of SAR (measured) = 17.2 W/kg

**Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:**

Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 67.54 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 31.1 W/kg

**SAR(1 g) = 7.95 W/kg; SAR(10 g) = 2.19 W/kg**


Smallest distance from peaks to all points 3 dB below = 6.8 mm


Ratio of SAR at M2 to SAR at M1 = 66.3%

Maximum value of SAR (measured) = 18.8 W/kg

**Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm  
Reference Value = 66.91 V/m; Power Drift = -0.08 dB  
Peak SAR (extrapolated) = 32.0 W/kg  
**SAR(1 g) = 7.94 W/kg; SAR(10 g) = 2.20 W/kg**  
Smallest distance from peaks to all points 3 dB below = 6.9 mm  
Ratio of SAR at M2 to SAR at M1 = 65.2%  
Maximum value of SAR (measured) = 18.3 W/kg

**Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5750 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm  
Reference Value = 65.07 V/m; Power Drift = -0.09 dB  
Peak SAR (extrapolated) = 32.2 W/kg  
**SAR(1 g) = 7.64 W/kg; SAR(10 g) = 2.13 W/kg**  
Smallest distance from peaks to all points 3 dB below = 6.8 mm  
Ratio of SAR at M2 to SAR at M1 = 63.8%  
Maximum value of SAR (measured) = 18.5 W/kg

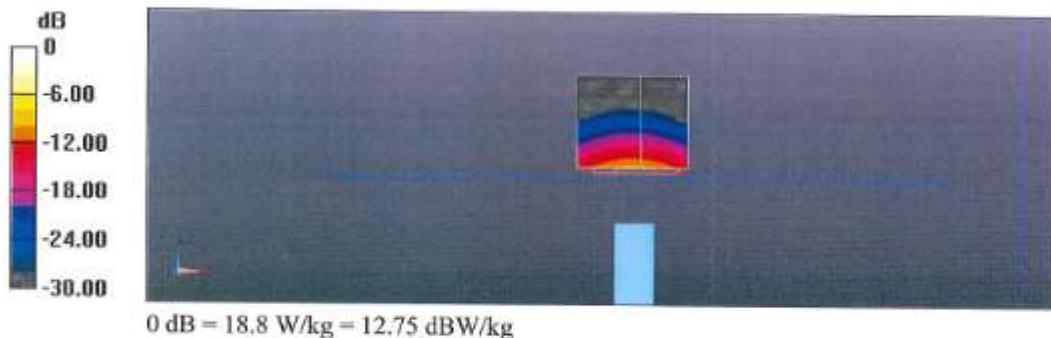

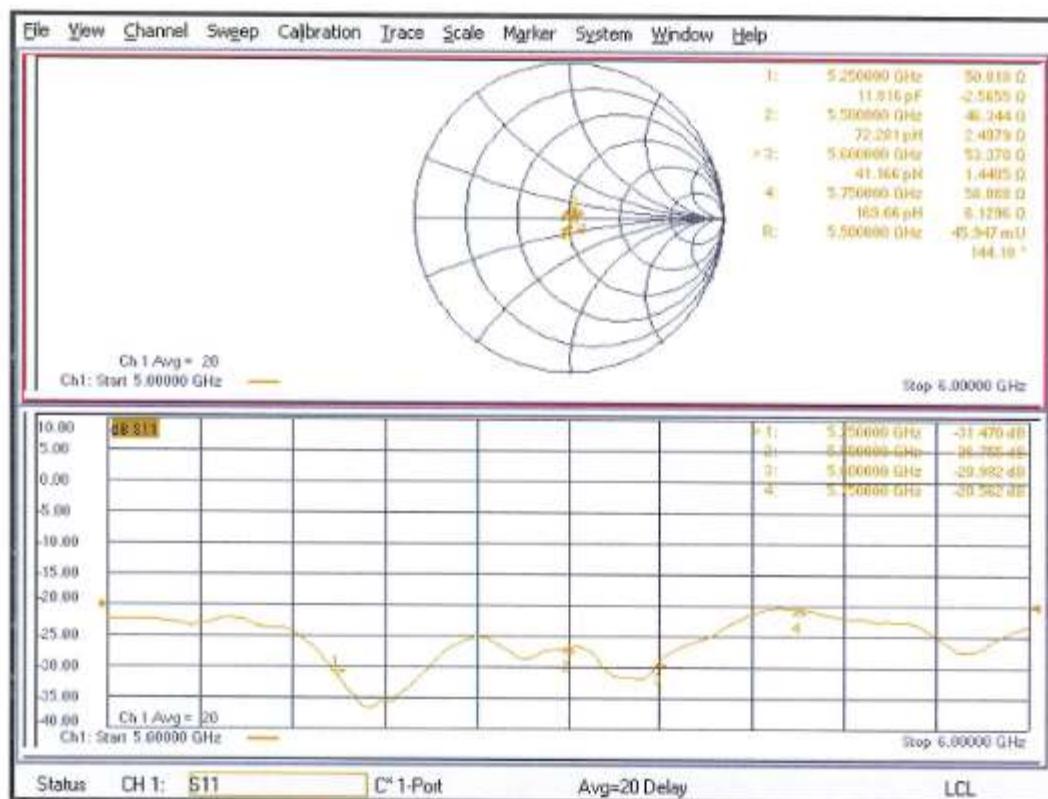**Impedance Measurement Plot for Body TSL**

## Dipole Data

The table below includes dipole impedance and return loss measurement data measured by Motorola Solutions' EME lab. The results meet the requirements stated in KDB 865664.

Dipole D835V2 (S/N:4d029), D2450V2(S/N: 781) and D5GHzV2 (S/N: 1026) has yet to exceed the annual calibration date, hence no further justification is required.

Dipole 900 (S/N: 1d026) has exceeded the annual calibration date thus the dipole impedance and return loss measurement data measured by Motorola Solutions' EME lab for Dipole 900 (S/N: 1d026) are provided in the table below. The results meet the requirements stated in KDB 865664.

<b>Dipole D900V2- 1d026</b>	<b>Head</b>		
	<b>Impedance</b>		<b>Return Loss</b>
<b>Date Measured</b>	<b>real <math>\Omega</math></b>	<b>imag <math>j\Omega</math></b>	<b>dB</b>
04/20/2020	51.18	-1.90	-34.28
05/07/2021	50.34	-2.92	-34.66
02/05/2022	46.56	-0.03	-33.33

## **Appendix D**

### **System Verification Check Scans**

## Motorola Solutions, Inc. EME Laboratory

Date/Time: 7/19/2022 8:50:07 PM

Robot#: DASY5-PG-2 | Run#: MFR-SYSP-900H-220719-24  
 Dipole Model# D900V2  
 Phantom#: ELI4 1028  
 Tissue Temp: 20.6 (C)  
 Serial#: 1d026  
 Test Freq: 900.0000 (MHz)  
 Start Power: 250 (mW)  
 Rotation (1D): 0.043 dB  
 Adjusted SAR (1W): 11.36 mW/g (1g)

**Comments:**

Communication System Band: Dipole 900, Communication System UID: 0, Duty Cycle: 1:1,  
 Medium parameters used:  $f = 900$  MHz;  $\sigma = 0.98$  S/m;  $\epsilon_r = 40.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
 Probe: EX3DV4 - SN7364, Calibrated: 2/28/2022, Frequency: 900 MHz, ConvF(9.81, 9.81, 9.81) @ 900 MHz  
 Electronics: DAE4 Sn1294, Calibrated: 2/22/2022

### **Below 2 GHz-Rev.3/System Performance Check/Dipole Area Scan 2 (41x141x1):**


Interpolated grid: dx=1.500 mm, dy=1.500 mm  
 Reference Value = 66.04 V/m; Power Drift = 0.03 dB  
**Fast SAR:** SAR(1 g) = 2.94 W/kg; SAR(10 g) = 1.91 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 3.88 W/kg

### **Below 2 GHz-Rev.3/System Performance Check/0-Degree Cube (5x5x7)/Cube 0:**

Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm  
 Reference Value = 66.04 V/m; Power Drift = 0.03 dB  
 Peak SAR (extrapolated) = 4.45 W/kg  
**SAR(1 g) = 2.84 W/kg; SAR(10 g) = 1.83 W/kg (SAR corrected for target medium)**  
 Smallest distance from peaks to all points 3 dB below = 19.2 mm  
 Ratio of SAR at M2 to SAR at M1 = 64.4%  
 Maximum value of SAR (measured) = 3.92 W/kg

### **Below 2 GHz-Rev.3/System Performance Check/Z-Axis Retraction (1x1x17):** Measurement

grid: dx=20mm, dy=20mm, dz=10mm  
 Maximum value of SAR (measured) = 3.94 W/kg

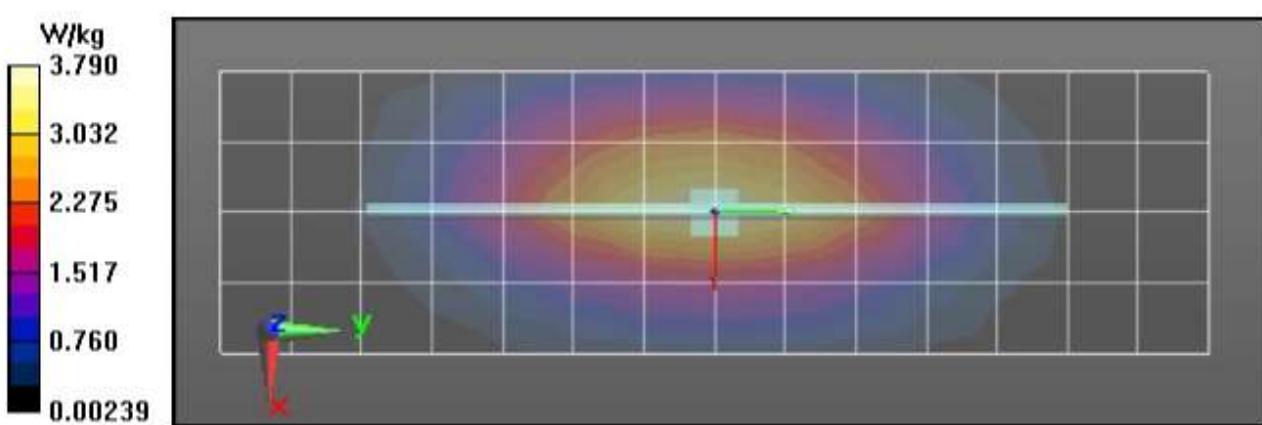

**Motorola Solutions, Inc. EME Laboratory**

Date/Time: 7/26/2022 9:10:28 AM

Robot#: DASY5-PG-03 | Run#: DAN-SYSP-835H-220726-01

Dipole Model# D835V2

Phantom#: ELI4 1028

Tissue Temp: 22.5(C)

Serial#: 4D029

Test Freq: 835.0000(MHz)

Start Power: 250(mW)

Rotation (1D): 0.038dB

Adjusted SAR (1W): 9.60mW/g (1g)

## Comments:

Communication System Band: Dipole 835, Communication System UID: 0, Duty Cycle: 1:1,

Medium parameters used:  $f = 835 \text{ MHz}$ ;  $\sigma = 0.92 \text{ S/m}$ ;  $\epsilon_r = 41.7$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Probe: EX3DV4 - SN7519, Calibrated: 2/28/2022, Frequency: 835 MHz, ConvF(9.8, 9.8, 9.8) @ 835 MHz

Electronics: DAE4 Sn684, Calibrated: 2/22/2022

**Below 2 GHz-Rev.3/System Performance Check/Dipole Area Scan 2 (41x121x1):**

Interpolated grid: dx=1.500 mm, dy=1.500 mm

Reference Value = 62.61 V/m; Power Drift = -0.12 dB

**Fast SAR: SAR(1 g) = 2.49 W/kg; SAR(10 g) = 1.62 W/kg** (SAR corrected for target medium)

Maximum value of SAR (interpolated) = 3.25 W/kg

**Below 2 GHz-Rev.3/System Performance Check/0-Degree Cube (5x5x7)/Cube 0:**

Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm

Reference Value = 62.61 V/m; Power Drift = -0.12 dB

Peak SAR (extrapolated) = 3.68 W/kg

**SAR(1 g) = 2.4 W/kg; SAR(10 g) = 1.56 W/kg** (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 21.2 mm


Ratio of SAR at M2 to SAR at M1 = 65.3%

Maximum value of SAR (measured) = 3.25 W/kg

**Below 2 GHz-Rev.3/System Performance Check/Z-Axis Retraction (1x1x17):** Measurement

grid: dx=20mm, dy=20mm, dz=10mm

Maximum value of SAR (measured) = 3.25 W/kg

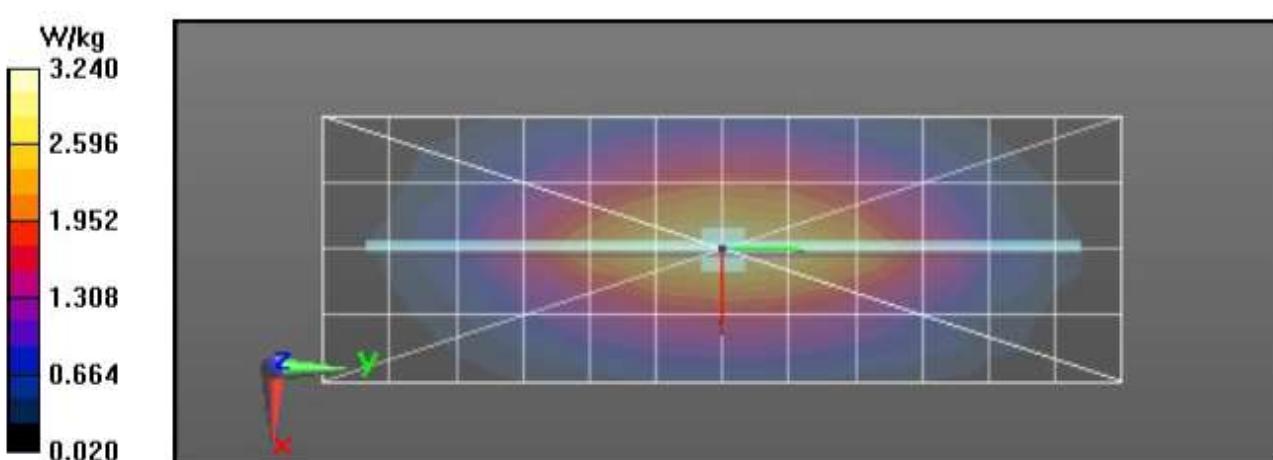

### Motorola Solutions, Inc. EME Laboratory

Date/Time: 8/30/2022 8:00:52 AM

Robot#: DASY5-PG-03 | Run#: BAD-SYSP-835H-220830-01  
 Dipole Model# D835V2  
 Phantom#: ELI4 1050  
 Tissue Temp: 22.0 (C)  
 Serial#: 4D029  
 Test Freq: 835.0000 (MHz)  
 Start Power: 250 (mW)  
 Rotation (ID): 0.068 dB  
 Adjusted SAR (1W): 10.16 mW/g (1g)

Comments:

Communication System Band: Dipole 835, Communication System UID: 0, Duty Cycle: 1:1,  
 Medium parameters used:  $f = 835$  MHz;  $\sigma = 0.92$  S/m;  $\epsilon_r = 40.5$ ;  $\rho = 1000$  kg/m $^3$   
 Probe: EX3DV4 - SN7519, Calibrated: 2/28/2022, Frequency: 835 MHz, ConvF(9.8, 9.8, 9.8) @ 835 MHz  
 Electronics: DAE4 Sn684, Calibrated: 2/22/2022


#### **Below 2 GHz-Rev.3/System Performance Check/Dipole Area Scan 2 (41x131x1):**

Interpolated grid: dx=1.500 mm, dy=1.500 mm  
 Reference Value = 62.61 V/m; Power Drift = 0.14 dB  
**Fast SAR:** SAR(1 g) = 2.64 W/kg; SAR(10 g) = 1.72 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 3.47 W/kg

#### **Below 2 GHz-Rev.3/System Performance Check/0-Degree Cube (5x5x7)/Cube 0:**

Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm  
 Reference Value = 62.61 V/m; Power Drift = 0.14 dB  
 Peak SAR (extrapolated) = 3.98 W/kg  
**SAR(1 g) = 2.54 W/kg; SAR(10 g) = 1.65 W/kg** (SAR corrected for target medium)  
 Smallest distance from peaks to all points 3 dB below = 18.3 mm  
 Ratio of SAR at M2 to SAR at M1 = 64.4%  
 Maximum value of SAR (measured) = 3.49 W/kg

**Below 2 GHz-Rev.3/System Performance Check/Z-Axis Retraction (1x1x17):** Measurement grid: dx=20mm, dy=20mm, dz=10mm  
 Maximum value of SAR (measured) = 3.44 W/kg

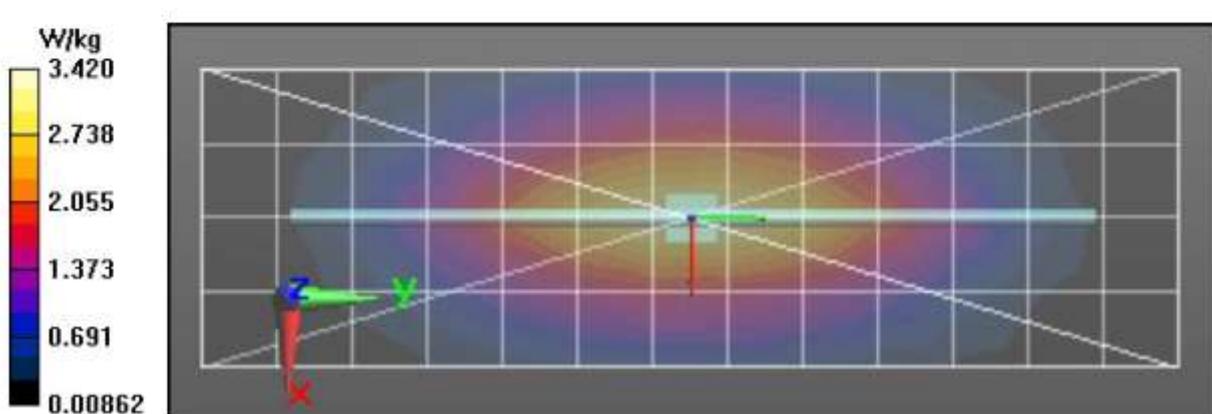

**Motorola Solutions, Inc. EME Laboratory**

Date/Time: 9/4/2022 8:12:50 PM

Robot#: DASY5-PG-3 | Run#: BAD-SYSP-900H-220904-14  
 Dipole Model# D900V2  
 Phantom#: ELI4 1050  
 Tissue Temp: 21.0 (C)  
 Serial#: 1D025  
 Test Freq: 900.0000 (MHz)  
 Start Power: 250 (mW)  
 Rotation (1D): 0.046 dB  
 Adjusted SAR (1W): 11.28 mW/g (1g)

**Comments:**


Communication System Band: Dipole 900, Communication System UID: 0, Duty Cycle: 1:1,  
 Medium parameters used:  $f = 900$  MHz;  $\sigma = 0.93$  S/m;  $\epsilon_r = 42.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
 Probe: EX3DV4 - SN7519, Calibrated: 2/28/2022, Frequency: 900 MHz, ConvF(9.57, 9.57, 9.57) @ 900 MHz  
 Electronics: DAE4 Sn684, Calibrated: 2/22/2022

**Below 2 GHz-Rev.3/System Performance Check/Dipole Area Scan 2 (41x121x1):**

Interpolated grid: dx=1.500 mm, dy=1.500 mm  
 Reference Value = 65.73 V/m; Power Drift = 0.02 dB  
**Fast SAR: SAR(1 g) = 2.89 W/kg; SAR(10 g) = 1.84 W/kg** (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 3.63 W/kg

**Below 2 GHz-Rev.3/System Performance Check/0-Degree Cube (5x5x7)/Cube 0:**

Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm  
 Reference Value = 65.73 V/m; Power Drift = 0.02 dB  
 Peak SAR (extrapolated) = 4.10 W/kg  
**SAR(1 g) = 2.82 W/kg; SAR(10 g) = 1.82 W/kg** (SAR corrected for target medium)  
 Smallest distance from peaks to all points 3 dB below = 18.3 mm  
 Ratio of SAR at M2 to SAR at M1 = 66%  
 Maximum value of SAR (measured) = 3.64 W/kg

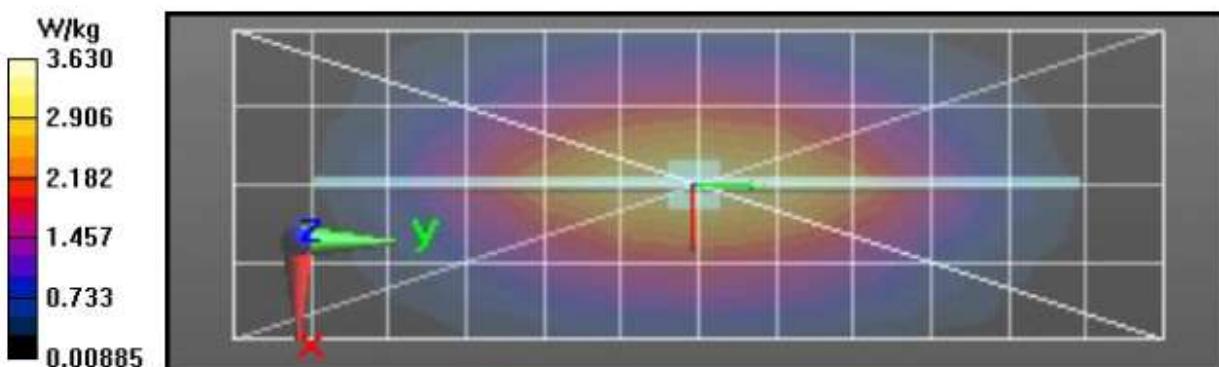**Below 2 GHz-Rev.3/System Performance Check/Z-Axis Retraction (1x1x17):** Measurement  
grid: dx=20mm, dy=20mm, dz=10mm  
Maximum value of SAR (measured) = 3.63 W/kg



**Motorola Solutions, Inc. EME Laboratory**  
**Date/Time: 7/20/2022 11:21:17 AM**

Robot#: DASY5-PG-2 | Run#: SAN-SYSP-5750H-220720-06  
Dipole Model# D5GHzV2  
Phantom#: ELI4 1108  
Tissue Temp: 21.8 (C)  
Serial#: 1026  
Test Freq: 5750.0000 (MHz)  
Start Power: 100 (mW)  
Rotation (1D): 0.057 dB  
Adjusted SAR (1W): 76.70 mW/g (1g)


## Comments:

Communication System Band: Dipole 5000, Communication System UID: 0, Duty Cycle: 1:1,  
Medium parameters used:  $f = 5750$  MHz;  $\sigma = 5.04$  S/m;  $\epsilon_r = 32.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Probe: EX3DV4 - SN7364, Calibrated: 2/28/2022, Frequency: 5750 MHz, ConvF(4.79, 4.79, 4.79) @ 5750 MHz  
Electronics: DAE4 Sn1294, Calibrated: 2/22/2022

**4-6 GHz-Rev.5/System Performance Check/Dipole Area Scan 2 (61x61x1):** Interpolated grid:  
dx=0.9000 mm, dy=0.9000 mm  
Reference Value = 70.95 V/m; Power Drift = -0.03 dB  
**Fast SAR:** SAR(1 g) = 7.32 W/kg; SAR(10 g) = 2.01 W/kg (SAR corrected for target medium)  
Maximum value of SAR (interpolated) = 20.5 W/kg

**4-6 GHz-Rev.5/System Performance Check/0-Degree Cube (8x8x12)/Cube 0:** Measurement grid:  
dx=4mm, dy=4mm, dz=2mm  
Reference Value = 70.95 V/m; Power Drift = -0.03 dB  
Peak SAR (extrapolated) = 35.2 W/kg  
**SAR(1 g) = 7.67 W/kg; SAR(10 g) = 2.17 W/kg (SAR corrected for target medium)**  
Smallest distance from peaks to all points 3 dB below = 7.5 mm  
Ratio of SAR at M2 to SAR at M1 = 51%  
Maximum value of SAR (measured) = 18.8 W/kg

**4-6 GHz-Rev.5/System Performance Check/Z-Axis Retraction (1x1x17):** Measurement grid:  
dx=20mm, dy=20mm, dz=10mm  
Maximum value of SAR (measured) = 20.9 W/kg

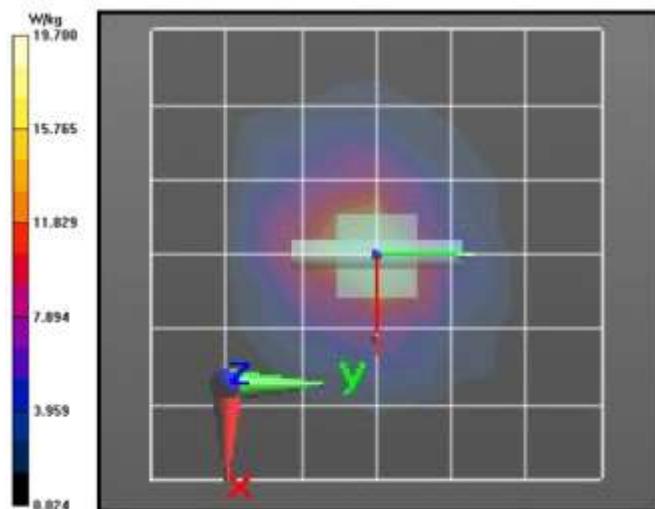

## Appendix E DUT Scans



**Table 18 - Assessment at Face for 902-928MHz band**

**Motorola Solutions, Inc. EME Laboratory**  
Date/Time: 9/4/2022 8:50:17 PM

Robot#: DASY5-PG-2 | Run#: BAD-FACE-220904-15  
 Model#: PMUF1982A  
 Phantom#: ELI4 1050  
 Tissue Temp: 21.0 (C)  
 Serial#: 55017YL0119  
 Antenna: Fixed antenna  
 Test Freq: 915.0000 (MHz)  
 Battery: PMNN4578A  
 Carry Acc: @ front  
 Audio Acc: N/A  
 Start Power: 0.913 (W)

## Comments:

Communication System Band: Biz Lite DLRx1100, Communication System UID: 0, Duty Cycle: 1:1,

Medium parameters used:  $f = 915$  MHz;  $\sigma = 0.93$  S/m;  $\epsilon_r = 42.7$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Probe: EX3DV4 - SN7519, Calibrated: 2/28/2022, Frequency: 915 MHz, ConvF(9.57, 9.57, 9.57) @ 915 MHz  
 Electronics: DAE4 Sn684, Calibrated: 2/22/2022

**Below 2 GHz-Rev.3/Face Scan/1-Area Scan (61x131x1):** Interpolated grid: dx=1.500 mm, dy=1.500 mm

Reference Value = 48.53 V/m; Power Drift = -0.52 dB

**Fast SAR:** SAR(1 g) = 1.76 W/kg; SAR(10 g) = 1.21 W/kg (SAR corrected for target medium)

Maximum value of SAR (interpolated) = 2.15 W/kg

**Below 2 GHz-Rev.3/Face Scan/3-Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm

Reference Value = 48.53 V/m; Power Drift = -0.58 dB

Peak SAR (extrapolated) = 2.32 W/kg

SAR(1 g) = 1.76 W/kg; SAR(10 g) = 1.27 W/kg (SAR corrected for target medium)


Smallest distance from peaks to all points 3 dB below: Larger than measurement grid

Ratio of SAR at M2 to SAR at M1 = 72.7%

Maximum value of SAR (measured) = 2.10 W/kg

**Below 2 GHz-Rev.3/Face Scan/4-Z-Axis Scan (1x1x17):** Measurement grid: dx=20mm, dy=20mm, dz=10mm

Maximum value of SAR (measured) = 2.08 W/kg

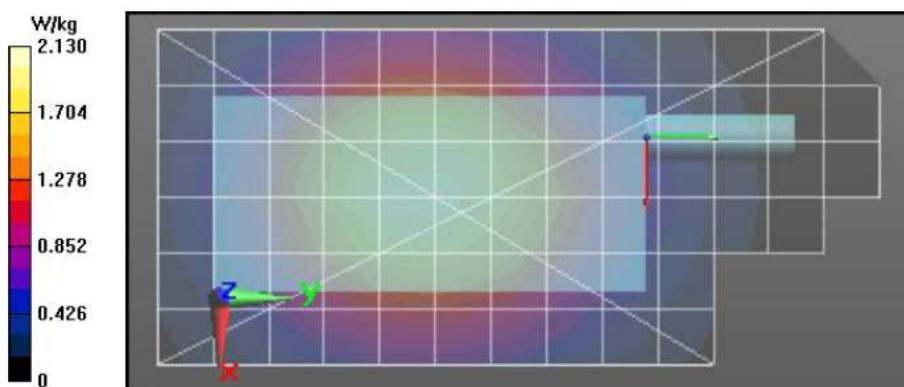

### Table 20 - Assessment at Body for 2.4GHz (802.11b)

#### Motorola Solutions, Inc. EME Laboratory

Date/Time: 7/20/2022 2:58:10 PM

Robot#: DASY5-PG-2 | Run#: SAN-AB-220720-08  
 Model#: PMUF1982A  
 Phantom#: ELI4 1108  
 Tissue Temp: 21.3 (C)  
 Serial#: 55017YL0119  
 Antenna: 2.4 GHz Wifi Antenna  
 Test Freq: 2462.0000 (MHz)  
 Battery: PMNN4578A  
 Carry Acc: PMLN8293A  
 Audio Acc: None  
 Start Power: 0.0168 (W)

Comments: Full Scan

Communication System Band: WLAN 2.4GHz (2412.0 - 2484.0 MHz), Communication System UID: 10415 - AAA, Duty Cycle: 1:1.4243,

Medium parameters used:  $f = 2462$  MHz;  $\sigma = 1.88$  S/m;  $\epsilon_r = 35.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Probe: EX3DV4 - SN7364, Calibrated: 2/28/2022, Frequency: 2462 MHz, ConvF(7.5, 7.5, 7.5) @ 2462 MHz

Electronics: DAE4 Sn1294, Calibrated: 2/22/2022

#### **2-3 GHz-Rev.3/Ab Scan/1-Area Scan (81x161x1):** Interpolated grid: dx=1.200 mm, dy=1.200 mm

Reference Value = 4.157 V/m; Power Drift = -0.34 dB

**Fast SAR:** SAR(1 g) = 0.028 W/kg; SAR(10 g) = 0.015 W/kg (SAR corrected for target medium)

Maximum value of SAR (interpolated) = 0.0440 W/kg

#### **2-3 GHz-Rev.3/Ab Scan/3-Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm,

dz=5mm

Reference Value = 4.157 V/m; Power Drift = -0.41 dB

Peak SAR (extrapolated) = 0.0540 W/kg

**SAR(1 g) = 0.027 W/kg; SAR(10 g) = 0.012 W/kg** (SAR corrected for target medium)


Smallest distance from peaks to all points 3 dB below: Larger than measurement grid

Ratio of SAR at M2 to SAR at M1 = 45.6%

Maximum value of SAR (measured) = 0.0428 W/kg

#### **2-3 GHz-Rev.3/Ab Scan/4-Z-Axis Scan (1x1x17):** Measurement grid: dx=20mm, dy=20mm, dz=10mm

Maximum value of SAR (measured) = 0.0431 W/kg

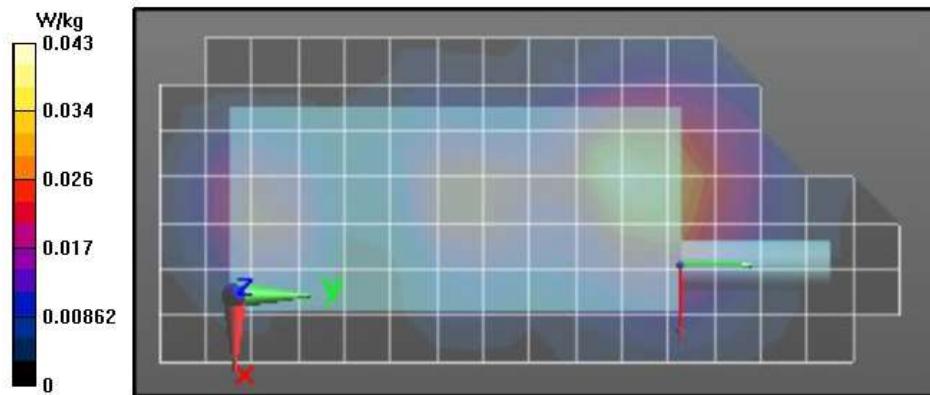**Table 22 - Assessment at Body for 5GHz (802.11a)****Motorola Solutions, Inc. EME Laboratory**

Date/Time: 7/20/2022 6:23:06 PM

Robot#: DASY5-PG-2 | Run#: SAN-AB-220720-11  
 Model#: PMUF1982A  
 Phantom#: ELI4 1108  
 Tissue Temp: 20.8 (C)  
 Serial#: 55017YL0119  
 Antenna: 5.0 GHz Wifi Antenna  
 Test Freq: 5785.0000 (MHz)  
 Battery: PMNN4578A  
 Carry Acc: PMLN8293A  
 Audio Acc: None  
 Start Power: 0.0136 (W)

Comments: Full Scan

Communication System Band: WLAN 5GHz (4915.0 - 5825.0 MHz), Communication System UID: 10417 - AAC, Duty Cycle: 1:6.64967,

Medium parameters used:  $f = 5785$  MHz;  $\sigma = 5.08$  S/m;  $\epsilon_r = 32.1$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Probe: EX3DV4 - SN7364, Calibrated: 2/28/2022, Frequency: 5785 MHz, ConvF(4.79, 4.79, 4.79) @ 5785 MHz

Electronics: DAE4 Sn1294, Calibrated: 2/22/2022

**4-6 GHz-Rev.5/Shortened Ab Scan/1-Area Scan (111x221x1):** Interpolated grid: dx=0.9000 mm, dy=0.9000 mm

Reference Value = 3.313 V/m; Power Drift = -0.84 dB

**Fast SAR:** SAR(1 g) = 0.090 W/kg; SAR(10 g) = 0.029 W/kg (SAR corrected for target medium)

Maximum value of SAR (interpolated) = 0.230 W/kg

**4-6 GHz-Rev.5/Shortened Ab Scan/2-Zoom Scan (9x9x12)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=2mm

Reference Value = 6.226 V/m; Power Drift = -0.16 dB

Peak SAR (extrapolated) = 0.512 W/kg

**SAR(1 g) = 0.055 W/kg; SAR(10 g) = 0.017 W/kg** (SAR corrected for target medium)


Smallest distance from peaks to all points 3 dB below = 8 mm

Ratio of SAR at M2 to SAR at M1 = 45.7%

Maximum value of SAR (measured) = 0.170 W/kg

**4-6 GHz-Rev.5/Shortened Ab Scan/3-Z-Axis Scan (1x1x17):** Measurement grid: dx=20mm, dy=20mm, dz=10mm

Maximum value of SAR (measured) = 0.122 W/kg

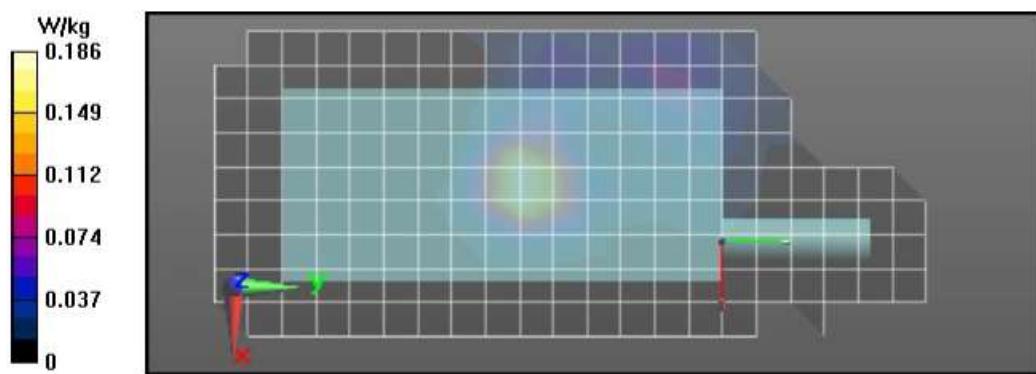

## APPENDIX F

### Shortened Scan of Highest SAR configuration

**Table 23 - Shortened Scan**

**Motorola Solutions, Inc. EME Laboratory**

Date/Time: 7/26/2022 6:02:33 PM

Robot#: DASY5-PG-2 | Run#: DAN-AB-220726-11  
 Model#: PMUF1982A  
 Phantom#: ELI4 1028  
 Tissue Temp: 21.8(C)  
 Serial#: 55017YL0119  
 Antenna: Fixed antenna  
 Test Freq: 927.9875 (MHz)  
 Battery: PMNN4578A  
 Carry Acc: PMLN8392A  
 Audio Acc: PMLN8311A  
 Start Power: 0.920(W)

## Comments:

Communication System Band: Biz Lite DLRX, Communication System UID: 0, Duty Cycle: 1:1,  
 Medium parameters used:  $f = 928$  MHz;  $\sigma = 1.01$  S/m;  $\epsilon_r = 40.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
 Probe: EX3DV4 - SN7519, Calibrated: 2/28/2022, Frequency: 927.988 MHz, ConvF(9.57, 9.57, 9.57) @ 927.988 MHz  
 Electronics: DAE4 Sn684, Calibrated: 2/22/2022

**Below 2 GHz-Rev.3/Ab Scan/1-Area Scan (61x131x1):** Interpolated grid: dx=1.500 mm, dy=1.500 mm  
 Reference Value = 54.72 V/m; Power Drift = 0.03 dB

**Fast SAR:** SAR(1 g) = 2.56 W/kg; SAR(10 g) = 1.75 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 3.28 W/kg

**Below 2 GHz-Rev.3/Ab Scan/2-Volume 2D Scan (41x41x1):** Interpolated grid: dx=0.7500 mm,  
 dy=0.7500 mm, dz=1.000 mm


Reference Value = 54.72 V/m; Power Drift = 0.00 dB  
**Fast SAR:** SAR(1 g) = 2.61 W/kg; SAR(10 g) = 1.81 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 3.29 W/kg

**Below 2 GHz-Rev.3/Ab Scan/3-Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=7.5mm,  
 dy=7.5mm, dz=5mm

Reference Value = 59.19 V/m; Power Drift = -0.19 dB  
 Peak SAR (extrapolated) = 3.49 W/kg  
**SAR(1 g) = 2.48 W/kg; SAR(10 g) = 1.73 W/kg** (SAR corrected for target medium)  
 Smallest distance from peaks to all points 3 dB below: Larger than measurement grid  
 Ratio of SAR at M2 to SAR at M1 = 70.9%  
 Maximum value of SAR (measured) = 3.14 W/kg

**Below 2 GHz-Rev.3/Ab Scan/4-Z-Axis Scan (1x1x17):** Measurement grid: dx=20mm, dy=20mm,  
 dz=10mm

Maximum value of SAR (measured) = 3.22 W/kg

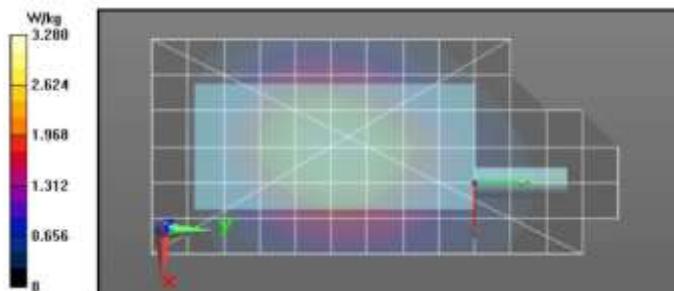

Shortened scan reflects highest SAR producing configuration and is compared to the full scan.

Scan Description	Referenced Table	Test Time (min.)	SAR 1g (W/kg)
Shorten scan (zoom)	25	7	1.41
Full scan (area & zoom)	18	15	1.42

## APPENDIX G


### DUT Test Position Photos

**ISM highest SAR Test Position per body location**

DUT with antenna Fixed Antenna with offered battery PMNN4578A and body worn kit PMLN8392A against the phantom with an audio accessory PMLN8311A attached.

**ISM highest SAR Test Position per Face location**

DUT with antenna Fixed Antenna with offered battery PMNN4578A separated 2.5cm from the phantom without an audio accessory attached.

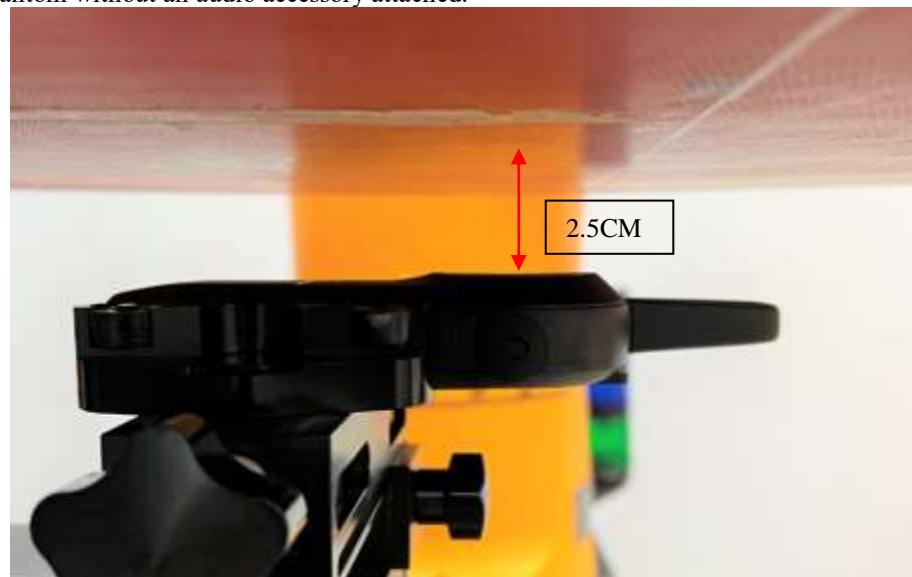

**APPENDIX H**  
**DUT, Body worn and audio accessories Photos**

**Please Refer Original Filing Report**