

**APPENDIX 2: SAR Measurement data**

**Appendix 2-1: Worst Scaled (Reported) SAR Plot**

**Plot 1a-1: 2.4GHz band, SAR(10g), Antenna 1; Back & touch / 11b (1Mbps) / 2412 MHz**

**EUT: Built-in Wireless Module with BT/Flat Panel Detector; Type: WM01B/WM501B; Serial: f4:a9:97:ff:d0:bc/21MED-0036**

**Mode: 11b(1Mbps, DBPSK/DSSS)** (UID: 0, Wi-fi\_2.4GHz (0), Frame Length in ms: 0, PAR: 0, PMF: 1); **Frequency: 2412 MHz; Crest Factor: 1.0**

**Medium: HSL5GHz(v6); Medium parameters used (\*interpolated): f = 2412 MHz;  $\sigma = 1.825$  S/m;  $\epsilon_r = 40.34$ ;  $\rho = 1000$  kg/m<sup>3</sup>**  
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section  
-DASY52 52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(7.35, 7.35, 7.35) @ 2412 MHz; Calibrated: 2021/04/21  
-Sensor-Surface: 2mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 2mm (Mechanical Surface Detection), z = 1.0, 31.0, 161.0

**touch,rear,h24a/24h9,2412,ant1,Rear&d0,b(1m)/**

**Area:108x96,12 (10x9x1):** Measurement grid: dx=12mm, dy=12mm; Maximum value of SAR (measured) = 0.480 W/kg


**Area:108x96,12 (91x81x1):** Interpolated grid: dx=1.200 mm, dy=1.200 mm; Maximum value of SAR (interpolated) = 0.565 W/kg

**Z;160,5 (1x1x33):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 0.696 W/kg

**Zoom:30^3,5 (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm;

Reference Value = 19.83 V/m; Power Drift = 0.00 dB; Maximum value of SAR (measured) = 0.698 W/kg; Peak SAR (extrapolated) = 0.961 W/kg

**SAR(1 g) = 0.436 W/kg; SAR(10 g) = 0.192 W/kg** (\*Smallest distance from peaks to all points 3 dB below = 6.7 mm; Ratio of SAR at M2 to SAR at M1 = 47.1%)

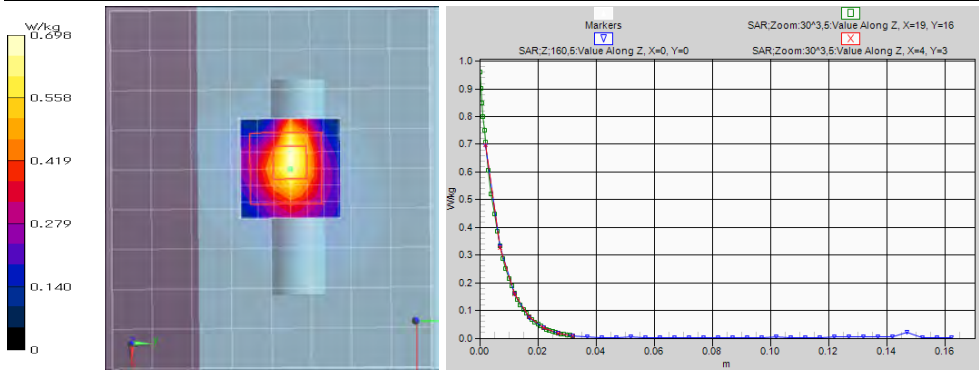

Remarks: \* Date tested: 2021/5/17; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,

\* liquid depth: 150 mm; Position: distance of EUT to phantom: 0 mm (2 mm to liquid); ambient: (23~25) deg.C. / (50~70) %RH,

\* liquid temperature: 22.8(start)/22.8(end)/22.5(in check) deg.C.; \* White cubic: zoom scan area, Red cubic: big=SAR(10g) / small=SAR(1g)

**Plot 1b-1: 2.4GHz band, SAR(1g), Antenna 1; Side(antenna 1) & touch / 11b (1Mbps) / 2412 MHz**

**EUT: Built-in Wireless Module with BT/Flat Panel Detector; Type: WM01B/WM501B; Serial: f4:a9:97:ff:d0:bc/21MED-0036**

**Mode: 11b(1Mbps, DBPSK/DSSS)** (UID: 0, Wi-fi\_2.4GHz (0), Frame Length in ms: 0, PAR: 0, PMF: 1); **Frequency: 2412 MHz; Crest Factor: 1.0**

**Medium: HSL5GHz(v6); Medium parameters used (\*interpolated): f = 2412 MHz;  $\sigma = 1.825$  S/m;  $\epsilon_r = 40.34$ ;  $\rho = 1000$  kg/m<sup>3</sup>**

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section  
-DASY52 52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(7.35, 7.35, 7.35) @ 2412 MHz; Calibrated: 2021/04/21  
-Sensor-Surface: 2mm (Mechanical Surface Detection), z = 1.0, 31.0, 161.0

**touch,side1a/o24h35,2412,ant1,side(1)&d0,b(1m)/**

**Area:100x60,10 (11x7x1):** Measurement grid: dx=10mm, dy=10mm; Maximum value of SAR (measured) = 0.137 W/kg


**Area:100x60,10 (101x61x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm; Maximum value of SAR (interpolated) = 0.170 W/kg

**Z;160,5 (1x1x33):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 0.145 W/kg

**Zoom:30^3,5 (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm;

Reference Value = 9.116 V/m; Power Drift = -0.02 dB; Maximum value of SAR (measured) = 0.144 W/kg; Peak SAR (extrapolated) = 0.222 W/kg

**SAR(1 g) = 0.095 W/kg; SAR(10 g) = 0.040 W/kg** (\*Smallest distance from peaks to all points 3 dB below = 7 mm; Ratio of SAR at M2 to SAR at M1 = 45.5%)

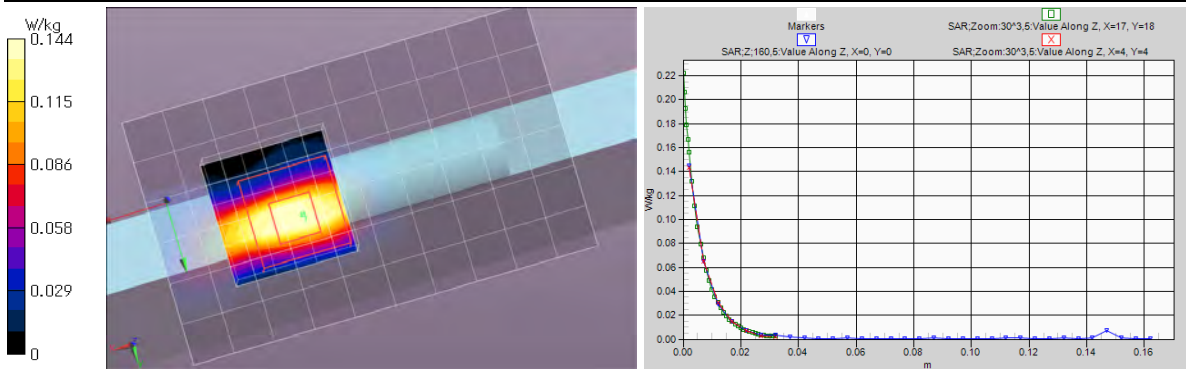

Remarks: \* Date tested: 2021/5/17; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,

\* liquid depth: 150 mm; Position: distance of EUT to phantom: 0 mm (2 mm to liquid); ambient: (23~25) deg.C. / (50~70) %RH,

\* liquid temperature: 22.8(start)/22.8(end)/22.5(in check) deg.C.; \* White cubic: zoom scan area, Red cubic: big=SAR(10g) / small=SAR(1g)

**APPENDIX 2: SAR Measurement data / Appendix 2-1: Worst Scaled (Reported) SAR Plot (cont'd)**

**Plot 2a-1: 5.3GHz band, SAR(10g), Antenna 1; Back & touch / 11n(40HT) (MCS0) / 5310 MHz**

**EUT: Built-in Wireless Module with BT/Flat Panel Detector; Type: WM01B/WM501B; Serial: f4:a9:97:ff:d0:bc/21MED-0036**

**Mode: n40(MCS0, BPSK/OFDM)** (UID: 0, Wi-fi\_5GHz (0), Frame Length in ms: 0; PAR: 0; PMF: 1); **Frequency: 5310 MHz; Crest Factor: 1.0**

**Medium: HSL5GHz(v6); Medium parameters used: f = 5310 MHz;  $\sigma = 4.672$  S/m;  $\epsilon_r = 35.98$ ;  $\rho = 1000$  kg/m<sup>3</sup>**

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section

-DASY52 52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(5.14, 5.14, 5.14) @ 5310 MHz; Calibrated: 2021/04/21

-Sensor-Surface: 1.4mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 1.4mm (Mechanical Surface Detection), z = 1.0, 25.0, 156.0

**touch,rear,h5c/5h17.53.3,ant1,Rear&d0,n40(m0),5310/**

**Area:100x90,stp10 (11x10x1):** Measurement grid: dx=10mm, dy=10mm; Maximum value of SAR (measured) = 1.93 W/kg


**Area:100x90,stp10 (101x91x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm; Maximum value of SAR (interpolated) = 2.02 W/kg

**Z;155.5 (1x1x32):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 1.93 W/kg

**Zoom:28x28x24,xy4-z1.4(ratio) (9x9x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm;

Reference Value = 22.86 V/m; Power Drift = -0.01 dB; Maximum value of SAR (measured) = 1.92 W/kg; Peak SAR (extrapolated) = 3.22 W/kg

**SAR(1 g) = 0.770 W/kg; SAR(10 g) = 0.225 W/kg** (\*. Smallest distance from peaks to all points 3 dB below = 5.4 mm; Ratio of SAR at M2 to SAR at M1 = 65.4%)

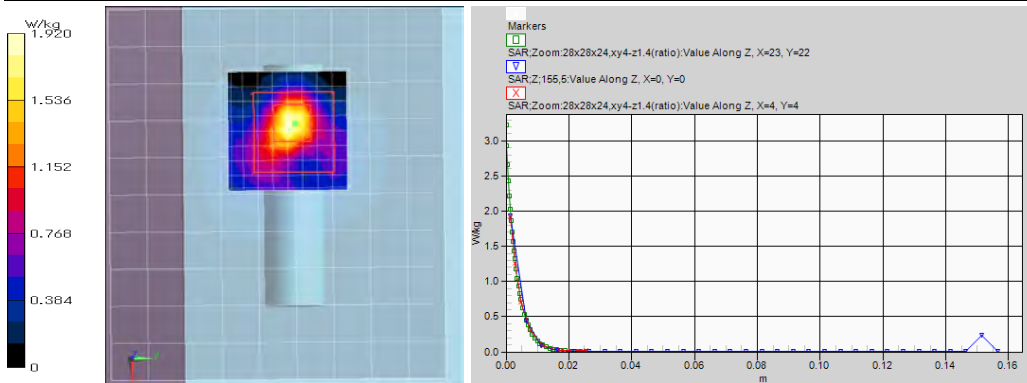

Remarks: \* Date tested: 2021/5/13; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,  
 \* liquid depth: 152 mm; Position: distance of EUT to phantom: 0 mm (2 mm to liquid); ambient: (23~25) deg.C. / (50~70) %RH,  
 \* liquid temperature: 22.3(start)/22.1(end)/22.5(in check) deg.C.; \*.White cubic: zoom scan area, Red cubic: big=SAR(10g) /small=SAR(1g)

**Plot 2b-1: 5.3GHz band, SAR(1g), Antenna 1; Side(antenna 1) & touch / 11n(40HT) (MCS0) / 5310 MHz**

**EUT: Built-in Wireless Module with BT/Flat Panel Detector; Type: WM01B/WM501B; Serial: f4:a9:97:ff:d0:bc/21MED-0036**

**Mode: n40(MCS0, BPSK/OFDM)** (UID: 0, Wi-fi\_5GHz (0), Frame Length in ms: 0; PAR: 0; PMF: 1); **Frequency: 5310 MHz; Crest Factor: 1.0**

**Medium: HSL5GHz(v6); Medium parameters used: f = 5310 MHz;  $\sigma = 4.617$  S/m;  $\epsilon_r = 35.64$ ;  $\rho = 1000$  kg/m<sup>3</sup>**

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section

-DASY52 52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(5.14, 5.14, 5.14) @ 5310 MHz; Calibrated: 2021/04/21

-Sensor-Surface: 2mm (Mechanical Surface Detection), Sensor-Surface: 1.4mm (Mechanical Surface Detection), z = 1.0, 25.0, 156.0

**touch,side1b/o5h71.53.16,ant1,side(1)&d0,n40(m0),5310/**

**Area:230x60,10 (24x7x1):** Measurement grid: dx=10mm, dy=10mm; Maximum value of SAR (measured) = 0.499 W/kg


**Area:230x60,10 (231x61x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm; Maximum value of SAR (interpolated) = 0.562 W/kg

**Z;155.5 (1x1x32):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 0.603 W/kg

**Zoom:28x28x24,xy4-z1.4(ratio) (9x9x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm;

Reference Value = 12.99 V/m; Power Drift = -0.03 dB; Maximum value of SAR (measured) = 0.610 W/kg; Peak SAR (extrapolated) = 1.02 W/kg

**SAR(1 g) = 0.268 W/kg; SAR(10 g) = 0.084 W/kg** (\*. Smallest distance from peaks to all points 3 dB below = 6.4 mm; Ratio of SAR at M2 to SAR at M1 = 66.1%)

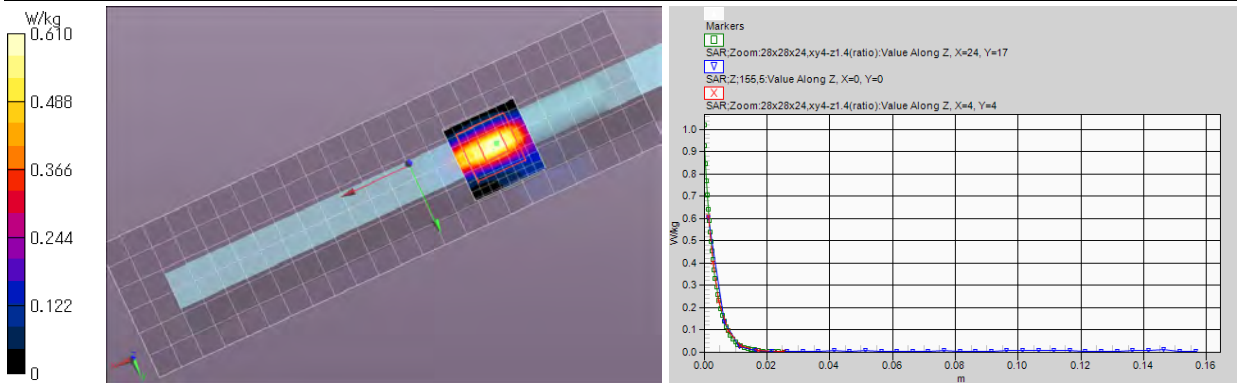

Remarks: \* Date tested: 2021/5/19; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,  
 \* liquid depth: 150 mm; Position: distance of EUT to phantom: 0 mm (2 mm to liquid); ambient: (23~25) deg.C. / (50~70) %RH,  
 \* liquid temperature: 22.7(start)/22.6(end)/22.5(in check) deg.C.; \*.White cubic: zoom scan area, Red cubic: big=SAR(10g) /small=SAR(1g)

**APPENDIX 2: SAR Measurement data / Appendix 2-1: Worst Scaled (Reported) SAR Plot (cont'd)**

**Plot 2c-1: 5.2GHz band, SAR(10g), Antenna 1; Back & touch / 11n(40HT) (MCS0) / 5230 MHz**

**EUT: Built-in Wireless Module with BT/Flat Panel Detector; Type: WM01B/WM501B; Serial: f4:a9:97:ff:d0:bc/21MED-0036**

**Mode: n40(MCS0, BPSK/OFDM)** (UID: 0, Wi-fi\_5GHz (0), Frame Length in ms: 0; PAR: 0; PMF: 1); **Frequency: 5230 MHz; Crest Factor: 1.0**

**Medium: HSL5GHz(v6); Medium parameters used: f = 5230 MHz;  $\sigma = 4.588$  S/m;  $\epsilon_r = 36.13$ ;  $\rho = 1000$  kg/m<sup>3</sup>**

Measurement Standard: DASYS5 (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section

-DASY52 52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(5.14, 5.14, 5.14) @ 5230 MHz; Calibrated: 2021/04/21

-Sensor-Surface: 1.4mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 1.4mm (Mechanical Surface Detection), z = 1.0, 25.0, 156.0

**touch,rear,h5c/5h20.52.4,ant1,Rear&d0,n40(m0),5230/**

**Area:100x90,stp10 (11x10x1):** Measurement grid: dx=10mm, dy=10mm; Maximum value of SAR (measured) = 1.50 W/kg


**Area:100x90,stp10 (101x91x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm; Maximum value of SAR (interpolated) = 1.59 W/kg

**Z;155.5 (1x1x32):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 2.04 W/kg

**Zoom:28x28x24,xy4-z1.4(ratio) (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm;

Reference Value = 22.33 V/m; Power Drift = -0.02 dB; Maximum value of SAR (measured) = 2.06 W/kg; Peak SAR (extrapolated) = 3.22 W/kg

**SAR(1 g) = 0.788 W/kg; SAR(10 g) = 0.227 W/kg** (\*Smallest distance from peaks to all points 3 dB below = 5.8 mm; Ratio of SAR at M2 to SAR at M1 = 65.8%)

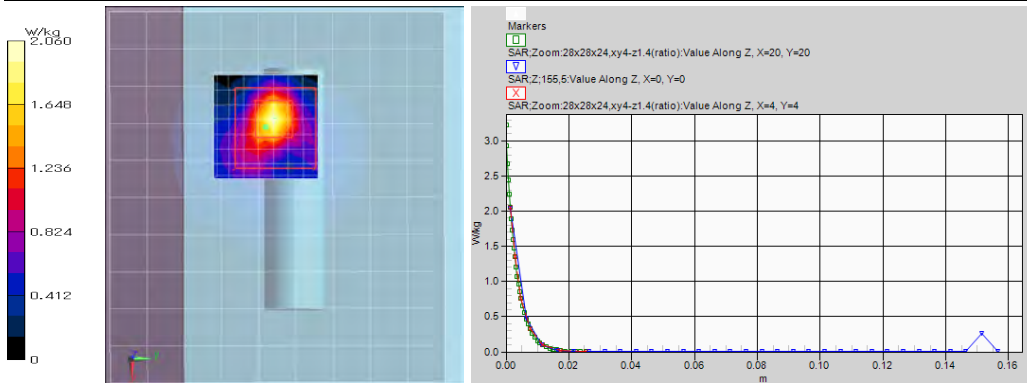

Remarks: \* Date tested: 2021/5/13; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,  
 \* liquid depth: 152 mm; Position: distance of EUT to phantom: 0 mm (2 mm to liquid); ambient: (23~25) deg.C. / (50~70) %RH,  
 \* liquid temperature: 22.3(start)/22.3(end)/22.5(in check) deg.C.; \*White cubic: zoom scan area, Red cubic: big=SAR(10g) /small=SAR(1g)

**Plot 2d-1: 5.2GHz band, SAR(1g), Antenna 2; Bottom (antenna 2) & touch / 11n(40HT) (MCS0) / 5190 MHz**

**EUT: Built-in Wireless Module with BT/Flat Panel Detector; Type: WM01B/WM501B; Serial: f4:a9:97:ff:d0:bc/21MED-0036**

**Mode: n40(MCS0, BPSK/OFDM)** (UID: 0, Wi-fi\_5GHz (0), Frame Length in ms: 0; PAR: 0; PMF: 1); **Frequency: 5190 MHz; Crest Factor: 1.0**

**Medium: HSL5GHz(v6); Medium parameters used: f = 5190 MHz;  $\sigma = 4.491$  S/m;  $\epsilon_r = 35.83$ ;  $\rho = 1000$  kg/m<sup>3</sup>**

Measurement Standard: DASYS5 (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section

-DASY52 52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(5.14, 5.14, 5.14) @ 5190 MHz; Calibrated: 2021/04/21

-Sensor-Surface: 2mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 1.4mm (Mechanical Surface Detection), z = 1.0, 25.0, 156.0

**touch,side0a/05h63.52.11,ant0,side(0)&d0,n40(m0),5190/**

**Area:60x140,10 (7x15x1):** Measurement grid: dx=10mm, dy=10mm; Maximum value of SAR (measured) = 0.410 W/kg


**Area:60x140,10 (61x141x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm; Maximum value of SAR (interpolated) = 0.430 W/kg

**Z;155.5 (1x1x32):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 0.489 W/kg

**Zoom:28x28x24,xy4-z1.4(ratio) (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm;

Reference Value = 11.77 V/m; Power Drift = -0.02 dB; Maximum value of SAR (measured) = 0.487 W/kg; Peak SAR (extrapolated) = 0.795 W/kg

**SAR(1 g) = 0.220 W/kg; SAR(10 g) = 0.066 W/kg** (\*Smallest distance from peaks to all points 3 dB below = 5.6 mm; Ratio of SAR at M2 to SAR at M1 = 68.1%)

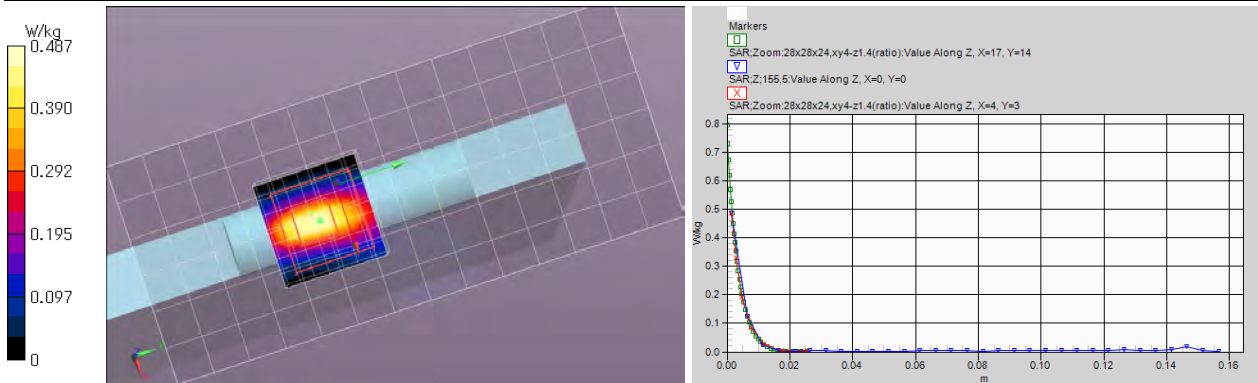

Remarks: \* Date tested: 2021/5/19; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,  
 \* liquid depth: 150 mm; Position: distance of EUT to phantom: 0 mm (2 mm to liquid); ambient: (23~25) deg.C. / (50~70) %RH,  
 \* liquid temperature: 22.8(start)/22.8(end)/22.5(in check) deg.C.; \*White cubic: zoom scan area, Red cubic: big=SAR(10g) /small=SAR(1g)

**APPENDIX 2: SAR Measurement data / Appendix 2-1: Worst Scaled (Reported) SAR Plot (cont'd)**

**Plot 3a-1: 5.6GHz band, SAR(10g), Antenna 1; Back & touch / 11n(40HT) (MCS0) / 5550 MHz**

**EUT: Built-in Wireless Module with BT/Flat Panel Detector; Type: WM01B/WM501B; Serial: f4:a9:97:ff:d0:bc/21MED-0036**

**Mode: n40(MCS0, BPSK/OFDM)** (UID: 0, Wi-fi\_5GHz (0), Frame Length in ms: 0, PAR: 0, PMF: 1); **Frequency: 5550 MHz; Crest Factor: 1.0**

**Medium: HSL5GHz(v6); Medium parameters used: f = 5550 MHz;  $\sigma = 4.944$  S/m;  $\epsilon_r = 35.53$ ;  $\rho = 1000$  kg/m<sup>3</sup>**

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section

-DASY52 52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(4.56, 4.56, 4.56) @ 5550 MHz; Calibrated: 2021/04/21

-Sensor-Surface: 1.4mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 1.4mm (Mechanical Surface Detection), z = 1.0, 25.0, 156.0

**touch,rear,h5b/5h12.56.6,ant1,Rear&d0,n40(m0),5550/**

**Area:100x90,stp10 (11x10x1):** Measurement grid: dx=10mm, dy=10mm; Maximum value of SAR (measured) = 1.66 W/kg


**Area:100x90,stp10 (101x91x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm; Maximum value of SAR (interpolated) = 1.78 W/kg

**Z;155.5 (1x1x32):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 1.79 W/kg

**Zoom:28x28x24,xy4-z1.4(ratio) (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm;

Reference Value = 21.13 V/m; Power Drift = -0.04 dB; Maximum value of SAR (measured) = 1.80 W/kg; Peak SAR (extrapolated) = 3.10 W/kg

**SAR(1 g) = 0.686 W/kg; SAR(10 g) = 0.203 W/kg** (\*. Smallest distance from peaks to all points 3 dB below = 5.8 mm; Ratio of SAR at M2 to SAR at M1 = 63.3%)

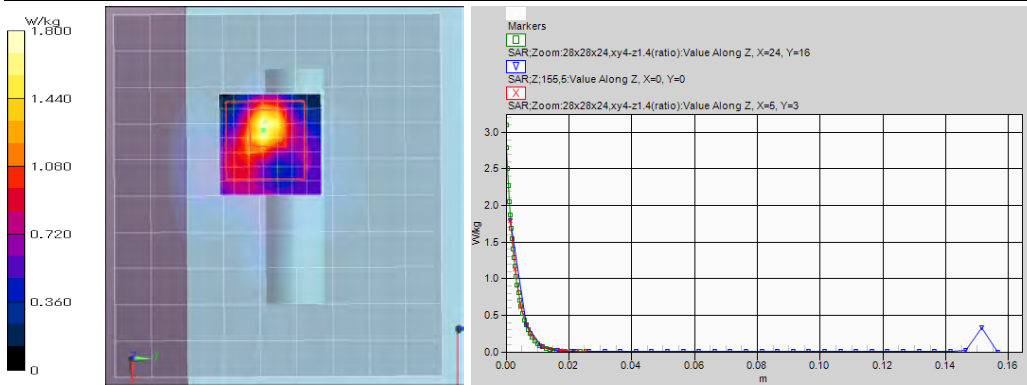

Remarks: \* Date tested: 2021/5/12; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,  
 \* liquid depth: 152 mm; Position: distance of EUT to phantom: 0 mm (2 mm to liquid); ambient: (23~25) deg.C. / (50~70) %RH,  
 \* liquid temperature: 22.3(start)/22.3(end)/22.5(in check) deg.C.; \*.White cubic: zoom scan area, Red cubic: big=SAR(10g) /small=SAR(1g)

**Plot 3b-1: 5.6GHz band, SAR(1g), Antenna 1; Side (antenna 1) & touch / 11n(40HT) (MCS0) / 5550 MHz**

**EUT: Built-in Wireless Module with BT/Flat Panel Detector; Type: WM01B/WM501B; Serial: f4:a9:97:ff:d0:bc/21MED-0036**

**Mode: n40(MCS0, BPSK/OFDM)** (UID: 0, Wi-fi\_5GHz (0), Frame Length in ms: 0, PAR: 0, PMF: 1); **Frequency: 5550 MHz; Crest Factor: 1.0**

**Medium: HSL5GHz(v6); Medium parameters used: f = 5550 MHz;  $\sigma = 4.885$  S/m;  $\epsilon_r = 35.25$ ;  $\rho = 1000$  kg/m<sup>3</sup>**

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section

-DASY52 52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(4.56, 4.56, 4.56) @ 5550 MHz; Calibrated: 2021/04/21

-Sensor-Surface: 2mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 1.4mm (Mechanical Surface Detection), z = 1.0, 25.0, 156.0

**touch,side1b/o5h74.56.26,ant1,side(1)&d0,n40(m0),5550/**

**Area:100x60,10 (11x7x1):** Measurement grid: dx=10mm, dy=10mm; Maximum value of SAR (measured) = 0.577 W/kg


**Area:100x60,10 (101x61x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm; Maximum value of SAR (interpolated) = 0.721 W/kg

**Z;155.5 (1x1x32):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 0.775 W/kg

**Zoom:28x28x24,xy4-z1.4(ratio) (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm;

Reference Value = 13.96 V/m; Power Drift = -0.01 dB; Maximum value of SAR (measured) = 0.760 W/kg; Peak SAR (extrapolated) = 1.29 W/kg

**SAR(1 g) = 0.334 W/kg; SAR(10 g) = 0.102 W/kg** (\*. Smallest distance from peaks to all points 3 dB below = 5.7 mm; Ratio of SAR at M2 to SAR at M1 = 64.5%)

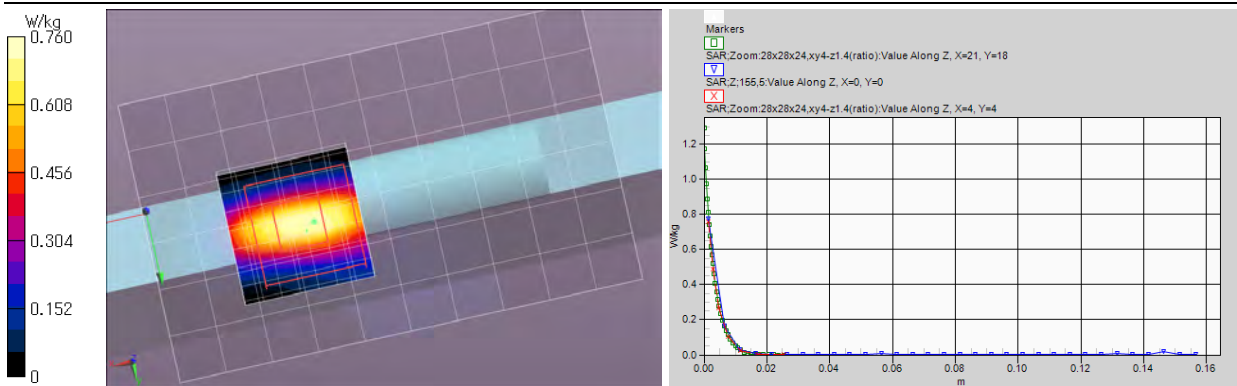

Remarks: \* Date tested: 2021/5/18; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,  
 \* liquid depth: 150 mm; Position: distance of EUT to phantom: 0 mm (2 mm to liquid); ambient: (23~25) deg.C. / (50~70) %RH,  
 \* liquid temperature: 22.6(start)/22.6(end)/22.5(in check) deg.C.; \*.White cubic: zoom scan area, Red cubic: big=SAR(10g) /small=SAR(1g)

**APPENDIX 2: SAR Measurement data / Appendix 2-1: Worst Scaled (Reported) SAR Plot (cont'd)**

**Plot 4a-1: 5.8GHz band, SAR(10g), Antenna 1; Back & touch / 11n(40HT) (MCS0) / 5795 MHz**

**EUT: Built-in Wireless Module with BT/Flat Panel Detector; Type: WM01B/WM501B; Serial: f4:a9:97:ff:d0:bc/21MED-0036**

**Mode: n40(MCS0, BPSK/OFDM)** (UID: 0, Wi-fi\_5GHz (0), Frame Length in ms: 0, PAR: 0, PMF: 1); **Frequency: 5795 MHz; Crest Factor: 1.0**

**Medium: HSL5GHz(v6); Medium parameters used (\*interpolated): f = 5795 MHz;  $\sigma = 5.237$  S/m;  $\epsilon_r = 35.13$ ;  $\rho = 1000$  kg/m<sup>3</sup>**

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section

-DASY52.52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(4.6, 4.6, 4.6) @ 5795 MHz; Calibrated: 2021/04/21

-Sensor-Surface: 1.4mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 1.4mm (Mechanical Surface Detection), z = 1.0, 25.0, 156.0

**touch,rear,h5c/5h16.58.4,ant1,Rear&d0,n40(m0),5795/**

**Area:100x90,stp10 (11x10x1):** Measurement grid: dx=10mm, dy=10mm; Maximum value of SAR (measured) = 1.48 W/kg


**Area:100x90,stp10 (101x91x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm; Maximum value of SAR (interpolated) = 1.50 W/kg

**Z;155.5 (1x1x32):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 1.51 W/kg

**Zoom:28x28x24,xy4-z1.4(ratio) (9x9x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm;

Reference Value = 18.11 V/m; Power Drift = -0.10 dB; Maximum value of SAR (measured) = 1.49 W/kg; Peak SAR (extrapolated) = 2.67 W/kg

**SAR(1 g) = 0.534 W/kg; SAR(10 g) = 0.171 W/kg** (\*.Smallest distance from peaks to all points 3 dB below = 6.1 mm; Ratio of SAR at M2 to SAR at M1 = 59.5%)

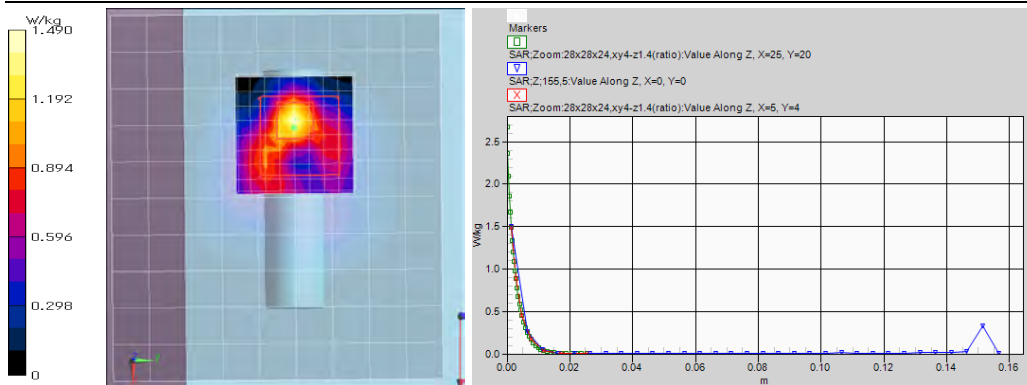

Remarks: \* Date tested: 2021/5/14; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,  
 \* liquid depth: 152 mm; Position: distance of EUT to phantom: 0 mm (2 mm to liquid); ambient: (23~25) deg.C. / (50~70) %RH,  
 \* liquid temperature: 22.3(start)/22.3(end)/22.5(in check) deg.C.; \*.White cubic: zoom scan area, Red cubic: big=SAR(10g) /small=SAR(1g)

**Plot 4b-1: 5.8GHz band, SAR(1g), Antenna 1; Side (antenna 1) & touch / 11n(40HT) (MCS0) / 5795 MHz**

**EUT: Built-in Wireless Module with BT/Flat Panel Detector; Type: WM01B/WM501B; Serial: f4:a9:97:ff:d0:bc/21MED-0036**

**Mode: n40(MCS0, BPSK/OFDM)** (UID: 0, Wi-fi\_5GHz (0), Frame Length in ms: 0, PAR: 0, PMF: 1); **Frequency: 5795 MHz; Crest Factor: 1.0**

**Medium: HSL5GHz(v6); Medium parameters used (\*interpolated): f = 5795 MHz;  $\sigma = 5.173$  S/m;  $\epsilon_r = 34.84$ ;  $\rho = 1000$  kg/m<sup>3</sup>**

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section

-DASY52.52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(4.6, 4.6, 4.6) @ 5795 MHz; Calibrated: 2021/04/21

-Sensor-Surface: 2mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 1.4mm (Mechanical Surface Detection), z = 1.0, 25.0, 156.0

**touch,side1b/o5h78.58.16,ant1,side(1)&d0,n40(m0),5795/**

**Area:100x60,10 (11x7x1):** Measurement grid: dx=10mm, dy=10mm; Maximum value of SAR (measured) = 0.352 W/kg


**Area:100x60,10 (101x61x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm; Maximum value of SAR (interpolated) = 0.565 W/kg

**Z;155.5 (1x1x32):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 0.584 W/kg

**Zoom:28x28x24,xy4-z1.4(ratio) (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm;

Reference Value = 11.85 V/m; Power Drift = -0.00 dB; Maximum value of SAR (measured) = 0.600 W/kg; Peak SAR (extrapolated) = 1.07 W/kg

**SAR(1 g) = 0.242 W/kg; SAR(10 g) = 0.075 W/kg** (\*.Smallest distance from peaks to all points 3 dB below = 6.4 mm; Ratio of SAR at M2 to SAR at M1 = 61.3%)

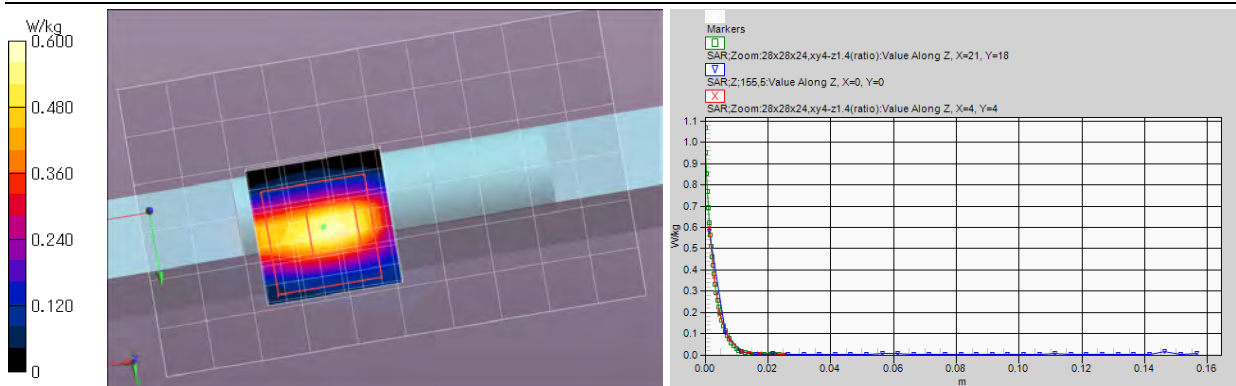

Remarks: \* Date tested: 2021/5/20; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,  
 \* liquid depth: 150 mm; Position: distance of EUT to phantom: 0 mm (2 mm to liquid); ambient: (23~25) deg.C. / (50~70) %RH,  
 \* liquid temperature: 22.7(start)/22.7(end)/22.5(in check) deg.C.; \*.White cubic: zoom scan area, Red cubic: big=SAR(10g) /small=SAR(1g)

**UL Japan, Inc.**

**Shonan EMC Lab.**

1-22-3 Megumigaoka, Hiratsuka-shi, Kanagawa-ken, 259-1220 JAPAN

Telephone: +81 463 50 6400 / Facsimile: +81 463 50 6401

**Appendix 2: SAR measurement data (cont'd)**

**Appendix 2-2: Other SAR Plots**

**Plot 1a-2: 2.4GHz band, SAR(10g), Antenna 2; Back & touch / 11b (1Mbps) / 2462 MHz**

**EUT: Built-in Wireless Module with BT/Flat Panel Detector; Type: WM01B/WM501B; Serial: f4:a9:97:ff:d0:bc/21MED-0036**  
**Mode: 11b(1Mbps, DBPSK/DSSS)** (UID: 0, Wi-fi\_2.4GHz (0), Frame Length in ms: 0, PAR: 0, PMF: 1); **Frequency: 2462 MHz; Crest Factor: 1.0**  
**Medium: HSL5GHz(v6); Medium parameters used (\*interpolated): f = 2462 MHz;  $\sigma = 1.865$  S/m;  $\epsilon_r = 40.26$ ;  $\rho = 1000$  kg/m<sup>3</sup>**  
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section  
 -DASY52.52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(7.35, 7.35, 7.35) @ 2462 MHz; Calibrated: 2021/04/21  
 -Sensor-Surface: 2mm (Mechanical Surface Detection), z = 1.0, 31.0, 161.0


**touch, rear, h24a/24h1; 2462, ant0, Rear&d0, b(1m)**

**Area: 156x216, 12 (19x14x1):** Measurement grid: dx=12mm, dy=12mm; Maximum value of SAR (measured) = 0.515 W/kg  
**Area: 156x216, 12 (181x131x1):** Interpolated grid: dx=1.200 mm, dy=1.200 mm; Maximum value of SAR (interpolated) = 0.600 W/kg  
**Z: 160, 5 (1x1x33):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 0.487 W/kg

**Zoom: 30^3, 5 (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm;

Reference Value = 16.53 V/m; Power Drift = 0.06 dB; Maximum value of SAR (measured) = 0.491 W/kg; Peak SAR (extrapolated) = 0.711 W/kg

**SAR(1g) = 0.315 W/kg; SAR(10g) = 0.143 W/kg** (\*Smallest distance from peaks to all points 3 dB below = 5.4 mm; Ratio of SAR at M2 to SAR at M1 = 50%)

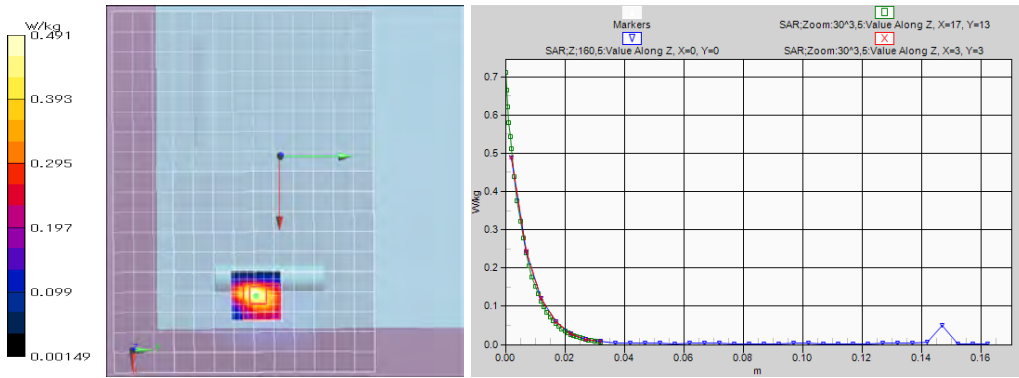

Remarks: \* Date tested: 2021/5/17; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,  
 \* liquid depth: 150 mm; Position: distance of EUT to phantom: 0 mm (2 mm to liquid); ambient: (23~25) deg.C. / (50~70) %RH,  
 \* liquid temperature: 22.6(start)/22.7(end)/22.5(in check) deg.C.; \*White cubic: zoom scan area, Red cubic: big=SAR(10g) /small=SAR(1g)

**Plot 1b-2: 2.4GHz band, SAR(1g), Antenna 2; Bottom (antenna 2) & touch / 11b (1Mbps) / 2437 MHz**

**EUT: Built-in Wireless Module with BT/Flat Panel Detector; Type: WM01B/WM501B; Serial: f4:a9:97:ff:d0:bc/21MED-0036**  
**Mode: 11b(1Mbps, DBPSK/DSSS)** (UID: 0, Wi-fi\_2.4GHz (0), Frame Length in ms: 0, PAR: 0, PMF: 1); **Frequency: 2437 MHz; Crest Factor: 1.0**  
**Medium: HSL5GHz(v6); Medium parameters used (\*interpolated): f = 2437 MHz;  $\sigma = 1.845$  S/m;  $\epsilon_r = 40.30$ ;  $\rho = 1000$  kg/m<sup>3</sup>**  
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section  
 -DASY52.52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(7.35, 7.35, 7.35) @ 2437 MHz; Calibrated: 2021/04/21  
 -Sensor-Surface: 2mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 2mm (Mechanical Surface Detection), z = 1.0, 31.0, 161.0


**touch, side0a/24h26; 2437, ant0, side(0)&d0, b(1m)**

**Area: 60x140, 10 (7x15x1):** Measurement grid: dx=10mm, dy=10mm; Maximum value of SAR (measured) = 0.127 W/kg  
**Area: 60x140, 10 (61x141x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm; Maximum value of SAR (interpolated) = 0.143 W/kg  
**Z: 160, 5 (1x1x33):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 0.135 W/kg

**Zoom: 30^3, 5 (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm;

Reference Value = 8.740 V/m; Power Drift = -0.02 dB; Maximum value of SAR (measured) = 0.134 W/kg; Peak SAR (extrapolated) = 0.182 W/kg

**SAR(1g) = 0.088 W/kg; SAR(10g) = 0.040 W/kg** (\*Smallest distance from peaks to all points 3 dB below = 7 mm; Ratio of SAR at M2 to SAR at M1 = 50.2%)

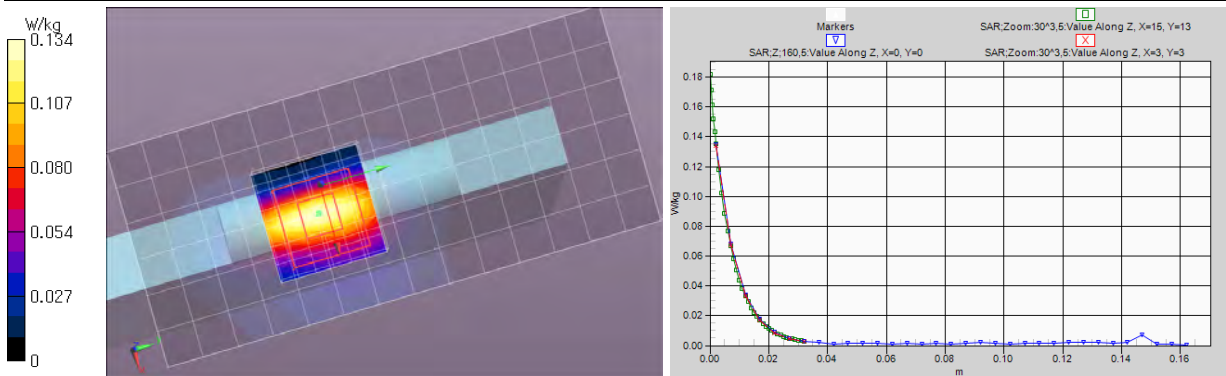

Remarks: \* Date tested: 2021/5/17; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,  
 \* liquid depth: 150 mm; Position: distance of EUT to phantom: 0 mm (2 mm to liquid); ambient: (23~25) deg.C. / (50~70) %RH,  
 \* liquid temperature: 22.6(start)/22.6(end)/22.5(in check) deg.C.; \*White cubic: zoom scan area, Red cubic: big=SAR(10g) /small=SAR(1g)

**Appendix 2: SAR measurement data / Appendix 2-2: Other SAR Plots (cont'd)**

**Plot 2a-2: 5.3GHz band, SAR(10g), Antenna 2; Back & touch / 11n(40HT) (MCS0) / 5310 MHz**

**EUT: Built-in Wireless Module with BT/Flat Panel Detector; Type: WM01B/WM501B; Serial: f4:a9:97:ff:d0:bc/21MED-0036**

**Mode: n40(MCS0, BPSK/OFDM)** (UID: 0, Wi-fi\_5GHz (0), Frame Length in ms: 0; PAR: 0; PMF: 1); **Frequency: 5310 MHz; Crest Factor: 1.0**

**Medium: HSL5GHz(v6); Medium parameters used: f = 5310 MHz;  $\sigma = 4.672$  S/m;  $\epsilon_r = 35.98$ ;  $\rho = 1000$  kg/m<sup>3</sup>**

Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section

-DASY52.52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(5.14, 5.14, 5.14) @ 5310 MHz; Calibrated: 2021/04/21

-Sensor-Surface: 1.4mm (Mechanical Surface Detection), z = 1.0, 25.0

**touch, rear, h5a/5h1.53.1, ant0, Rear&d0, n40(m0), 5310/**


**Area: 200x140, stp10 2 (21x15x1):** Measurement grid: dx=10mm, dy=10mm; Maximum value of SAR (measured) = 0.891 W/kg

**Area: 200x140, stp10 2 (201x141x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm; Maximum value of SAR (interpolated) = 1.06 W/kg

**Zoom: 28x28x24, xy4-z1.4(ratio) (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm;

Reference Value = 20.11 V/m; Power Drift = -0.08 dB; Maximum value of SAR (measured) = 1.39 W/kg; Peak SAR (extrapolated) = 2.55 W/kg

**SAR(1 g) = 0.574 W/kg; SAR(10 g) = 0.154 W/kg** (\*. Smallest distance from peaks to all points 3 dB below = 5.1 mm; Ratio of SAR at M2 to SAR at M1 = 64.8%)

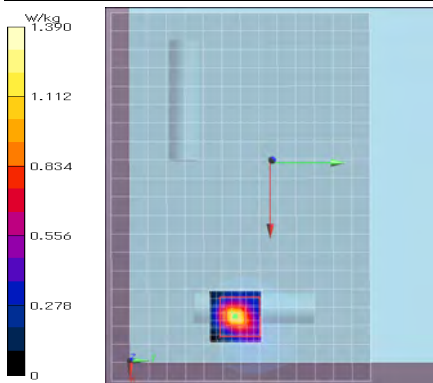

Remarks: \*. Date tested: 2021/5/13; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,

\*. liquid depth: 152 mm; Position: distance of EUT to phantom: 0 mm (2 mm to liquid); ambient: (23~25) deg.C. / (50~70) %RH,

\*. liquid temperature: 22.4(start)/22.4(end)/22.5(in check) deg.C.; \*. White cubic: zoom scan area, Red cubic: big=SAR(10g)/small=SAR(1g)

**Plot 2b-2: 5.3GHz band, SAR(1g), Antenna 2; Bottom (antenna 2) & touch / 11n(40HT) (MCS0) / 5310 MHz**

**EUT: Built-in Wireless Module with BT/Flat Panel Detector; Type: WM01B/WM501B; Serial: f4:a9:97:ff:d0:bc/21MED-0036**

**Mode: n40(MCS0, BPSK/OFDM)** (UID: 0, Wi-fi\_5GHz (0), Frame Length in ms: 0; PAR: 0; PMF: 1); **Frequency: 5310 MHz; Crest Factor: 1.0**

**Medium: HSL5GHz(v6); Medium parameters used: f = 5310 MHz;  $\sigma = 4.617$  S/m;  $\epsilon_r = 35.64$ ;  $\rho = 1000$  kg/m<sup>3</sup>**

Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section

-DASY52.52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(5.14, 5.14, 5.14) @ 5310 MHz; Calibrated: 2021/04/21

-Sensor-Surface: 2mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 1.4mm (Mechanical Surface Detection), z = 1.0, 25.0, 156.0

**touch, side0a/05h55.53.14, ant0, side(0)&d0, n40(m0), 5310/**

**Area: 60x140, 10 (7x15x1):** Measurement grid: dx=10mm, dy=10mm; Maximum value of SAR (measured) = 0.447 W/kg


**Area: 60x140, 10 (61x141x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm; Maximum value of SAR (interpolated) = 0.512 W/kg

**Z: 155, 5 (1x1x32):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 0.577 W/kg

**Zoom: 28x28x24, xy4-z1.4(ratio) (9x9x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm;

Reference Value = 12.45 V/m; Power Drift = -0.05 dB; Maximum value of SAR (measured) = 0.577 W/kg; Peak SAR (extrapolated) = 0.931 W/kg

**SAR(1 g) = 0.256 W/kg; SAR(10 g) = 0.077 W/kg** (\*. Smallest distance from peaks to all points 3 dB below = 6.1 mm; Ratio of SAR at M2 to SAR at M1 = 67.5%)

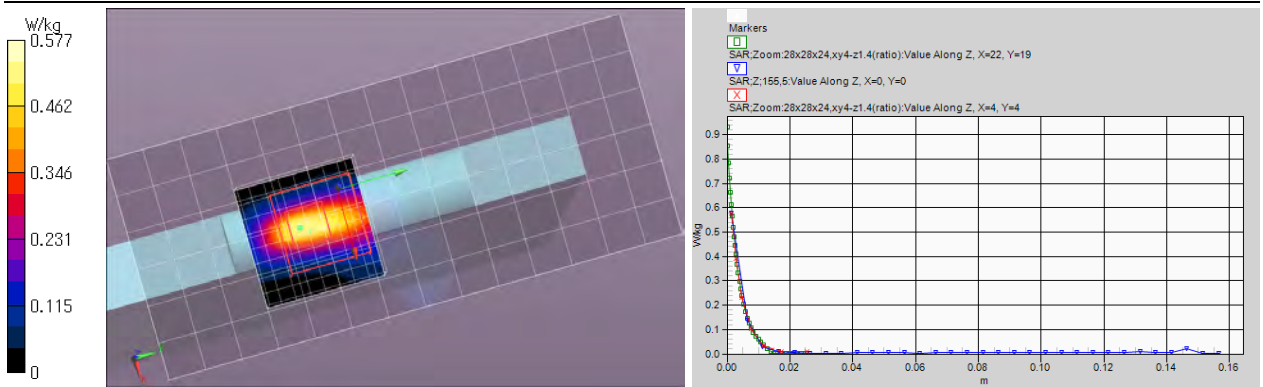

Remarks: \*. Date tested: 2021/5/19; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,

\*. liquid depth: 150 mm; Position: distance of EUT to phantom: 0 mm (2 mm to liquid); ambient: (23~25) deg.C. / (50~70) %RH,

\*. liquid temperature: 22.6(start)/22.6(end)/22.5(in check) deg.C.; \*. White cubic: zoom scan area, Red cubic: big=SAR(10g)/small=SAR(1g)

**Appendix 2: SAR measurement data / Appendix 2-2: Other SAR Plots (cont'd)**

**Plot 2c-2: 5.2GHz band, SAR(10g), Antenna 2; Back & touch / 11n(40HT) (MCS0) / 5190 MHz**

**EUT: Built-in Wireless Module with BT/Flat Panel Detector; Type: WM01B/WM501B; Serial: f4:a9:97:ff:d0:bc/21MED-0036**

**Mode: n40(MCS0, BPSK/OFDM) (UID: 0, Wi-fi\_5GHz (0), Frame Length in ms: 0; PAR: 0; PMF: 1); Frequency: 5190 MHz; Crest Factor: 1.0**

**Medium: HSL5GHz(v6); Medium parameters used: f = 5190 MHz;  $\sigma = 4.54$  S/m;  $\epsilon_r = 36.17$ ;  $\rho = 1000$  kg/m<sup>3</sup>**

Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section

-DASY52.52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(5.14, 5.14, 5.14) @ 5190 MHz; Calibrated: 2021/04/21

-Sensor-Surface: 1.4mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 1.4mm (Mechanical Surface Detection), z = 1.0, 25.0

**touch,rear,h5a/5h9.52.1.ant0,Rear&d0,n40(m0),5190/**


**Area:90x140,stp10 (10x15x1):** Measurement grid: dx=10mm, dy=10mm; Maximum value of SAR (measured) = 1.19 W/kg

**Area:90x140,stp10 (91x141x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm; Maximum value of SAR (interpolated) = 1.23 W/kg

**Zoom:28x28x24,xy4-z1.4(ratio) (9x9x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm;

Reference Value = 19.14 V/m; Power Drift = 0.03 dB; Maximum value of SAR (measured) = 1.40 W/kg; Peak SAR (extrapolated) = 2.33 W/kg

**SAR(1 g) = 0.549 W/kg; SAR(10 g) = 0.155 W/kg** (\*.Smallest distance from peaks to all points 3 dB below = 5.4 mm; Ratio of SAR at M2 to SAR at M1 = 65.5%)

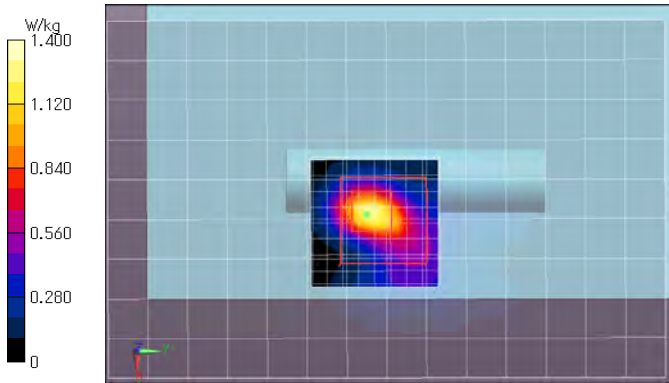

Remarks: \*. Date tested: 2021/5/13; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,

\*. liquid depth: 152 mm; Position: distance of EUT to phantom: 0 mm (2 mm to liquid); ambient: (23~25) deg.C. / (50~70) %RH,

\*. liquid temperature: 22.4(start)/22.4(end)/22.5(in check) deg.C.; \*.White cubic: zoom scan area, Red cubic: big=SAR(10g )/small=SAR(1g)

**Plot 2d-2: 5.2GHz band, SAR(1g), Antenna 1; Side (antenna 1) & touch / 11n(40HT) (MCS0) / 5230 MHz**

**EUT: Built-in Wireless Module with BT/Flat Panel Detector; Type: WM01B/WM501B; Serial: f4:a9:97:ff:d0:bc/21MED-0036**

**Mode: n40(MCS0, BPSK/OFDM) (UID: 0, Wi-fi\_5GHz (0), Frame Length in ms: 0; PAR: 0; PMF: 1); Frequency: 5230 MHz; Crest Factor: 1.0**

**Medium: HSL5GHz(v6); Medium parameters used: f = 5230 MHz;  $\sigma = 4.534$  S/m;  $\epsilon_r = 35.78$ ;  $\rho = 1000$  kg/m<sup>3</sup>**

Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section

-DASY52.52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(5.14, 5.14, 5.14) @ 5230 MHz; Calibrated: 2021/04/21

-Sensor-Surface: 2mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 1.4mm (Mechanical Surface Detection), z = 1.0, 25.0, 156.0

**touch,side1b/o5h80.52.14.ant1,side(1)&d0,n40(m0),5230/**

**Area:100x60,10 (11x7x1):** Measurement grid: dx=10mm, dy=10mm; Maximum value of SAR (measured) = 0.318 W/kg


**Area:100x60,10 (101x61x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm; Maximum value of SAR (interpolated) = 0.443 W/kg

**Z:155,5 (1x1x32):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 0.466 W/kg

**Zoom:28x28x24,xy4-z1.4(ratio) (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm;

Reference Value = 11.26 V/m; Power Drift = -0.02 dB; Maximum value of SAR (measured) = 0.466 W/kg; Peak SAR (extrapolated) = 0.740 W/kg

**SAR(1 g) = 0.207 W/kg; SAR(10 g) = 0.066 W/kg** (\*.Smallest distance from peaks to all points 3 dB below = 6.4 mm; Ratio of SAR at M2 to SAR at M1 = 66.9%)

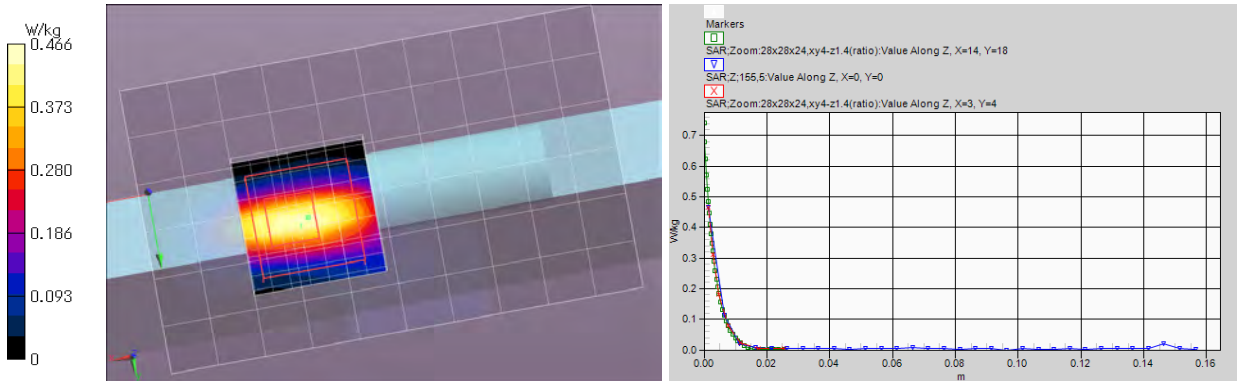

Remarks: \*. Date tested: 2021/5/19; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,

\*. liquid depth: 150 mm; Position: distance of EUT to phantom: 0 mm (2 mm to liquid); ambient: (23~25) deg.C. / (50~70) %RH,

\*. liquid temperature: 22.7(start)/22.8(end)/22.5(in check) deg.C.; \*.White cubic: zoom scan area, Red cubic: big=SAR(10g )/small=SAR(1g)



**Appendix 2: SAR measurement data / Appendix 2-2: Other SAR Plots (cont'd)**

**Plot 3a-2: 5.6GHz band, SAR(10g), Antenna 2; Back & touch / 11n(40HT) (MCS0) / 5670 MHz**

**EUT: Built-in Wireless Module with BT/Flat Panel Detector; Type: WM01B/WM501B; Serial: f4:a9:97:ff:d0:bc/21MED-0036**

**Mode: n40(MCS0, BPSK/OFDM)** (UID: 0, Wi-fi\_5GHz (0), Frame Length in ms: 0, PAR: 0, PMF: 1); **Frequency: 5670 MHz; Crest Factor: 1.0**

**Medium: HSL5GHz(v6); Medium parameters used: f = 5670 MHz;  $\sigma = 5.079$  S/m;  $\epsilon_r = 35.35$ ;  $\rho = 1000$  kg/m<sup>3</sup>**

Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section

-DASY52.52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(4.56, 4.56, 4.56) @ 5670 MHz; Calibrated: 2021/04/21

-Sensor-Surface: 1.4mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 1.4mm (Mechanical Surface Detection), z = 1.0, 25.0, 156.0

**touch, rear, h5a/5h3.56.1, ant0, Rear&d0, n40(m0), 5670/**

**Area: 90x140, stp10 (10x15x1):** Measurement grid: dx=10mm, dy=10mm; Maximum value of SAR (measured) = 1.11 W/kg


**Area: 90x140, stp10 (91x141x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm; Maximum value of SAR (interpolated) = 1.38 W/kg

**Z; 155.5 (1x1x32):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 1.74 W/kg

**Zoom: 28x28x24, xy4-z1.4(ratio) (9x9x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm;

Reference Value = 21.45 V/m; Power Drift = -0.09 dB; Maximum value of SAR (measured) = 1.73 W/kg; Peak SAR (extrapolated) = 3.27 W/kg

**SAR(1 g) = 0.674 W/kg; SAR(10 g) = 0.190 W/kg** (\*. Smallest distance from peaks to all points 3 dB below = 5.6 mm; Ratio of SAR at M2 to SAR at M1 = 62.7%)

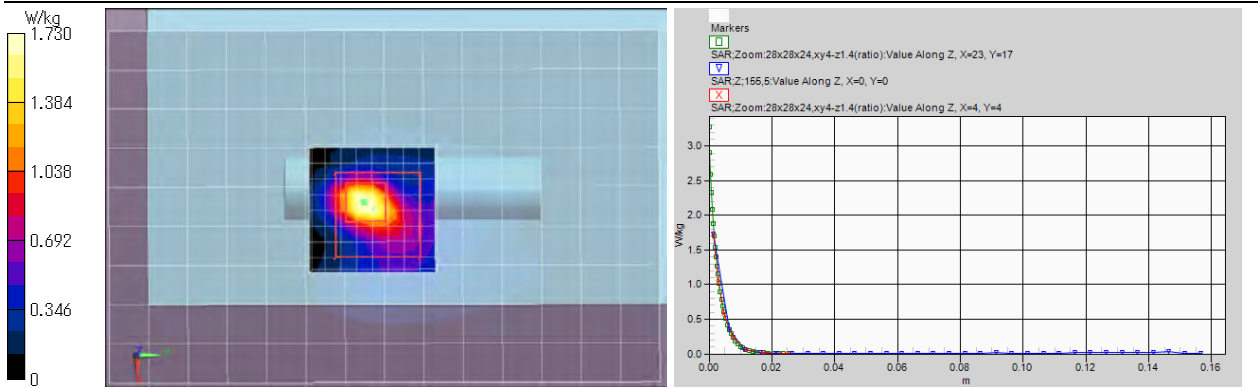

Remarks: \* Date tested: 2021/5/12; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,  
 \* liquid depth: 152 mm; Position: distance of EUT to phantom: 0 mm (2 mm to liquid); ambient: (23~25) deg.C. / (50~70) %RH,  
 \* liquid temperature: 22.4(start)/22.3(end)/22.5(in check) deg.C.; \*. White cubic: zoom scan area, Red cubic: big=SAR(10g)/small=SAR(1g)

**Plot 3b-2: 5.6GHz band, SAR(1g), Antenna 2; Bottom (antenna 2) & touch / 11n(40HT) (MCS0) / 5550 MHz**

**EUT: Built-in Wireless Module with BT/Flat Panel Detector; Type: WM01B/WM501B; Serial: f4:a9:97:ff:d0:bc/21MED-0036**

**Mode: n40(MCS0, BPSK/OFDM)** (UID: 0, Wi-fi\_5GHz (0), Frame Length in ms: 0, PAR: 0, PMF: 1); **Frequency: 5550 MHz; Crest Factor: 1.0**

**Medium: HSL5GHz(v6); Medium parameters used: f = 5550 MHz;  $\sigma = 4.885$  S/m;  $\epsilon_r = 35.25$ ;  $\rho = 1000$  kg/m<sup>3</sup>**

Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section

-DASY52.52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(4.56, 4.56, 4.56) @ 5550 MHz; Calibrated: 2021/04/21

-Sensor-Surface: 2mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 1.4mm (Mechanical Surface Detection), z = 1.0, 25.0, 156.0

**touch, side0a/05h5.56.22, ant0, side(0)&d0, n40(m0), 5550/**

**Area: 60x140, 10 (7x15x1):** Measurement grid: dx=10mm, dy=10mm; Maximum value of SAR (measured) = 0.521 W/kg


**Area: 60x140, 10 (61x141x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm; Maximum value of SAR (interpolated) = 0.583 W/kg

**Z; 155.5 (1x1x32):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 0.655 W/kg

**Zoom: 28x28x24, xy4-z1.4(ratio) (9x9x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm;

Reference Value = 12.75 V/m; Power Drift = -0.02 dB; Maximum value of SAR (measured) = 0.647 W/kg; Peak SAR (extrapolated) = 1.02 W/kg

**SAR(1 g) = 0.271 W/kg; SAR(10 g) = 0.083 W/kg** (\*. Smallest distance from peaks to all points 3 dB below = 6.4 mm; Ratio of SAR at M2 to SAR at M1 = 65.9%)

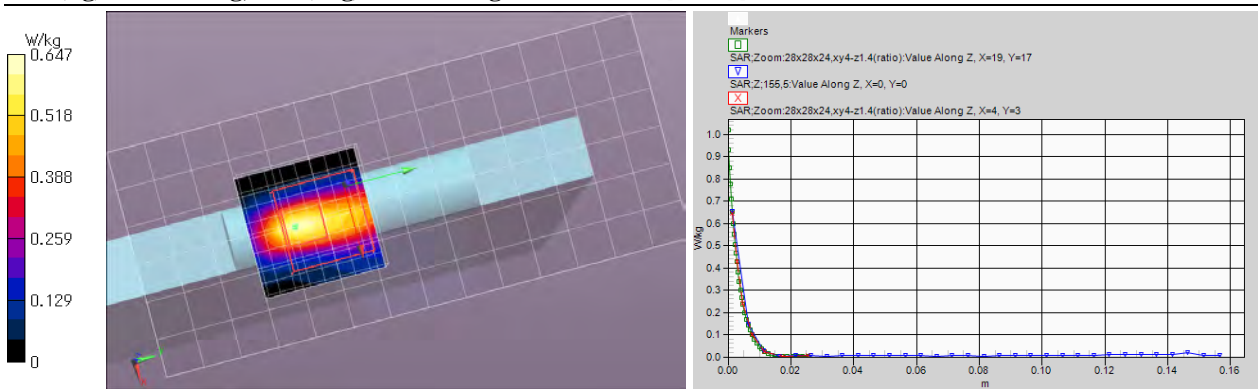

Remarks: \* Date tested: 2021/5/18; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,  
 \* liquid depth: 150 mm; Position: distance of EUT to phantom: 0 mm (2 mm to liquid); ambient: (23~25) deg.C. / (50~70) %RH,  
 \* liquid temperature: 22.6(start)/22.7(end)/22.5(in check) deg.C.; \*. White cubic: zoom scan area, Red cubic: big=SAR(10g)/small=SAR(1g)

**Appendix 2: SAR measurement data / Appendix 2-2: Other SAR Plots (cont'd)**

**Plot 4a-2: 5.8GHz band, SAR(10g), Antenna 2; Back & touch / 11n(40HT) (MCS0) / 5755 MHz**

**EUT: Built-in Wireless Module with BT/Flat Panel Detector; Type: WM01B/WM501B; Serial: f4:a9:97:ff:d0:bc/21MED-0036**

**Mode: n40(MCS0, BPSK/OFDM)** (UID: 0, Wi-fi\_5GHz (0), Frame Length in ms: 0, PAR: 0, PMF: 1); **Frequency: 5755 MHz; Crest Factor: 1.0**

**Medium: HSL5GHz(v6); Medium parameters used (\*interpolated): f = 5755 MHz;  $\sigma = 5.182$  S/m;  $\epsilon_r = 35.21$ ;  $\rho = 1000$  kg/m<sup>3</sup>**

Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section

-DASY52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(4.6, 4.6, 4.6) @ 5755 MHz; Calibrated: 2021/04/21

-Sensor-Surface: 1.4mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 1.4mm (Mechanical Surface Detection), z = 1.0, 25.0, 156.0

**touch,rear,h5a/5h7.58.1,ant0,Rear&d0,n40(m0),5755/**

**Area:90x140,stp10 (10x15x1):** Measurement grid: dx=10mm, dy=10mm; Maximum value of SAR (measured) = 0.889 W/kg


**Area:90x140,stp10 (91x141x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm; Maximum value of SAR (interpolated) = 1.10 W/kg

**Z;155.5 (1x1x32):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 1.46 W/kg

**Zoom:28x28x24,xy4-z1.4(ratio) (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm;

Reference Value = 19.02 V/m; Power Drift = -0.09 dB; Maximum value of SAR (measured) = 1.46 W/kg; Peak SAR (extrapolated) = 2.75 W/kg

**SAR(1 g) = 0.557 W/kg; SAR(10 g) = 0.154 W/kg** (\*. Smallest distance from peaks to all points 3 dB below = 4.7 mm; Ratio of SAR at M2 to SAR at M1 = 61.8%)

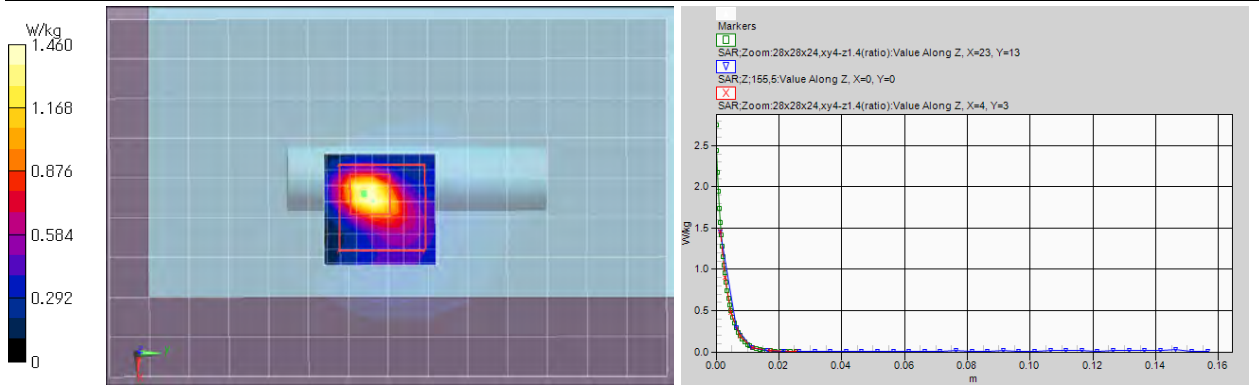

Remarks: \* Date tested: 2021/5/14; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,  
 \* liquid depth: 152 mm; Position: distance of EUT to phantom: 0 mm (2 mm to liquid); ambient: (23~25) deg.C. / (50~70) %RH,  
 \* liquid temperature: 22.4(start)/22.4(end)/22.5(in check) deg.C.; \*.White cubic: zoom scan area, Red cubic: big=SAR(10g)/small=SAR(1g)

**Plot 4b-2: 5.8GHz band, SAR(1g), Antenna 2; Bottom (antenna 2) & touch / 11n(40HT) (MCS0) / 5795 MHz**

**EUT: Built-in Wireless Module with BT/Flat Panel Detector; Type: WM01B/WM501B; Serial: f4:a9:97:ff:d0:bc/21MED-0036**

**Mode: n40(MCS0, BPSK/OFDM)** (UID: 0, Wi-fi\_5GHz (0), Frame Length in ms: 0, PAR: 0, PMF: 1); **Frequency: 5795 MHz; Crest Factor: 1.0**

**Medium: HSL5GHz(v6); Medium parameters used (\*interpolated): f = 5795 MHz;  $\sigma = 5.173$  S/m;  $\epsilon_r = 34.84$ ;  $\rho = 1000$  kg/m<sup>3</sup>**

Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section

-DASY52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(4.6, 4.6, 4.6) @ 5795 MHz; Calibrated: 2021/04/21

-Sensor-Surface: 2mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 1.4mm (Mechanical Surface Detection), z = 1.0, 25.0, 156.0

**touch,side0a/o5h61.58.13,ant0,side(0)&d0,n40(m0),5795/**

**Area:60x140,10 (7x15x1):** Measurement grid: dx=10mm, dy=10mm; Maximum value of SAR (measured) = 0.390 W/kg


**Area:60x140,10 (61x141x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm; Maximum value of SAR (interpolated) = 0.442 W/kg

**Z;155.5 (1x1x32):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 0.475 W/kg

**Zoom:28x28x24,xy4-z1.4(ratio) (9x9x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm;

Reference Value = 10.56 V/m; Power Drift = -0.00 dB; Maximum value of SAR (measured) = 0.480 W/kg; Peak SAR (extrapolated) = 0.852 W/kg

**SAR(1 g) = 0.193 W/kg; SAR(10 g) = 0.062 W/kg** (\*. Smallest distance from peaks to all points 3 dB below = 6.4 mm; Ratio of SAR at M2 to SAR at M1 = 60.9%)

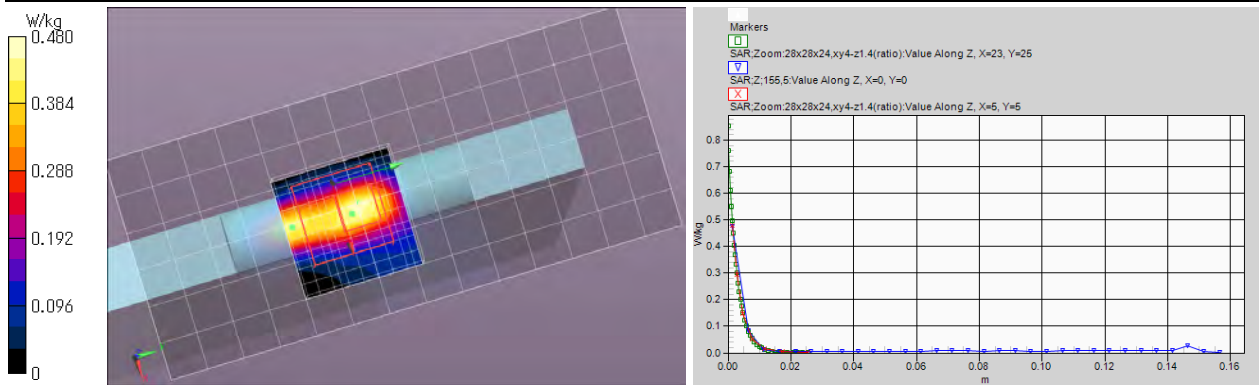

Remarks: \* Date tested: 2021/5/20; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,  
 \* liquid depth: 150 mm; Position: distance of EUT to phantom: 0 mm (2 mm to liquid); ambient: (23~25) deg.C. / (50~70) %RH,  
 \* liquid temperature: 22.8(start)/22.8(end)/22.5(in check) deg.C.; \*.White cubic: zoom scan area, Red cubic: big=SAR(10g)/small=SAR(1g)

**APPENDIX 3: Test instruments****Appendix 3-1: Equipment used**

Test Name	Local ID	LIMS ID	Description	Manufacturer	Model	Serial	Calibration	
							Last Date	Interval (Months)
AT	KSA-08	145089	Spectrum Analyzer	Keysight Technologies Inc	E4446A	MY46180525	2020/11/24	12
AT	SAT10-SARP1	160520	Attenuator	Weinschel - API Technologies Corp	4M-10	-	2020/12/11	12
AT	SPM-13	169910	Power Meter	Keysight Technologies Inc	8990B	MY51000448	2021/01/25	12
AT	SPSS-06	169911	Power sensor	Keysight Technologies Inc	N1923A	MY57270004	2021/01/25	12
AT,SAR	SOS-26	191844	Humidity Indicator	CUSTOM. Inc	CTH-201	-	2020/09/30	12
SAR	COTS-SSAR-02	144885	DASY52 software	Schmid&Partner Engineering AG	DASY5 PRO	Ver.52.10.3.1513	-	-
SAR	COTS-SSEP-02	144886	Dielectric assessment software	Schmid&Partner Engineering AG	DAK	Ver.DAK1.10.317.11	-	-
SAR	KAT10-P1	144882	Attenuator	Weinschel - API Technologies Corp	24-10-34	BY5927	2020/12/11	12
SAR	KCPL-07	146100	Directional Coupler	Pulsar Microwave Corp.	CCS30-B26	621	-	-
SAR	KDAE-01	144944	Data Acquisition Electronics	Schmid&Partner Engineering AG	DAE4	626	2020/11/17	12
SAR	KIU-08	145059	Power sensor	Rohde & Schwarz	NRV-Z4	100372	2020/09/15	12
SAR	KIU-09	145099	Power sensor	Rohde & Schwarz	NRV-Z4	100371	2020/09/15	12
SAR	KOS-14	144986	Thermo-Hygrometer data logger	SATO KEIRYOKI	SK-L200THIIα/SK-LTHIIα-2	015246/08169	2020/10/01	12
SAR	KPA-12	145359	RF Power Amplifier	Milmega	AS2560-50	1018582	-	-
SAR	KPFL-01	145560	Flat Phantom	Schmid&Partner Engineering AG	Oval flat phantom ELI 4.0	1059	2020/08/19	12
SAR	KPM-05	144988	Power meter	Keysight Technologies Inc	E4417A	GB41290718	2021/04/09	12
SAR	KPM-06	144989	Power Meter	Rohde & Schwarz	NRVD	101599	2020/09/15	12
SAR	KPSS-01	144990	Power sensor	Keysight Technologies Inc	E9327A	US40440544	2021/04/09	12
SAR	KRU-04	145086	Ruler(300mm)	SHINWA	13134	-	2021/02/10	12
SAR	KSDA-01	145090	Dipole Antenna	Schmid&Partner Engineering AG	D2450V2	822	2020/11/10	12
SAR	KSDA-02	145091	Dipole Antenna	Schmid&Partner Engineering AG	D5GHzV2	1070	2021/04/20	12
SAR	KSG-08	145109	Signal Generator	Rohde & Schwarz	SMT06	100763	2020/09/14	12
SAR	SALC-01	146112	Primepure Ethanol	Kanto Chemical Co., Inc.	14032-79	-	-	-
SAR	SAT20-SARP1	160521	Attenuator	Weinschel - API Technologies Corp	4M-20	-	2020/12/11	12
SAR	SAT6-SAR1	145160	Attenuator	Huber+Suhner	6806.17.A	766429-1	2020/12/11	12
SAR	SCC-SAR2	145405	Coaxial Cable	Huber+Suhner	SF104A/11PC3542/11N451/4M	MY699/4A	2020/12/11	12
SAR	SEPP-02	145500	Dielectric probe	Schmid&Partner Engineering AG	DAK3.5	1129	2021/04/14	12
SAR	SOS-SAR2	201967	Digital thermomoter	HANNA	Checktemp-4	A01440226111	2020/10/02	12
SAR	SOS-SAR3	201968	Digital thermomoter	HANNA	Checktemp-4	A01310946111	2020/10/02	12
SAR	SPB-02	146235	Dosimetric E-Field Probe	Schmid&Partner Engineering AG	EX3DV4	3907	2021/04/21	12
SAR	SSAR-02	146177	SAR measurement system	Schmid&Partner Engineering AG	DASY5	1324	-	-
SAR	SSLHV6-01	207714	Head Tissue Simulating Liquid	Schmid&Partner Engineering AG	HBBL600-10000V6	SL AAH U16 BC	-	-
SAR	SSNA-01	146258	Network Analyzer	Keysight Technologies Inc	8753ES	US39171777	2020/11/09	12
SAR	SSRBT-02	145621	SAR robot	Schmid&Partner Engineering AG	TX60 Lspeag	F12/5L2QA1/A/01	2020/09/03	12
SAR	SWTR-03	146185	DI water	MonotaRo	34557433	-	-	-

\*. AT (antenna terminal conducted power measurement) was measured May 10~11, 2021. (Refer to Section 5 in this report.)

\*. Local ID: SALC-01, the parameters of primepure Ethanol (as reference liquid) used for the simulated tissue parameter confirmation was defined the NPL Report MAT23 (<http://www.npl.co.uk/content/conpublication/4295>)

The expiration date of calibration is the end of the expired month.

As for some calibrations performed after the tested dates, those test equipment have been controlled by means of an unbroken chain of calibrations.


All equipment is calibrated with valid calibrations. Each measurement data is traceable to the national or international standards.

\*. Hyphens for Last Calibration Date and Cal Int (month) are instruments that Calibration is not required (e.g. software), or instruments checked in advance before use.

[Test Item] SAR: Specific Absorption Rate, AT: Antenna terminal conducted power

**Appendix 3-2: Configuration and peripherals**

These measurements were performed with the automated near-field scanning system DASY5 from Schmid & Partner Engineering AG (SPEAG). The system is based on a high precision robot, which positions the probes with a positional repeatability of better than  $\pm 0.02$  mm. Special E- and H-field probes have been developed for measurements close to material discontinuity, the sensors of which are directly loaded with a Schottky diode and connected via highly resistive lines to the data acquisition unit. The SAR measurements were conducted with the dosimetry probes EX3DV4 (manufactured by SPEAG), designed in the classical triangular configuration and optimized for dosimetric evaluation.

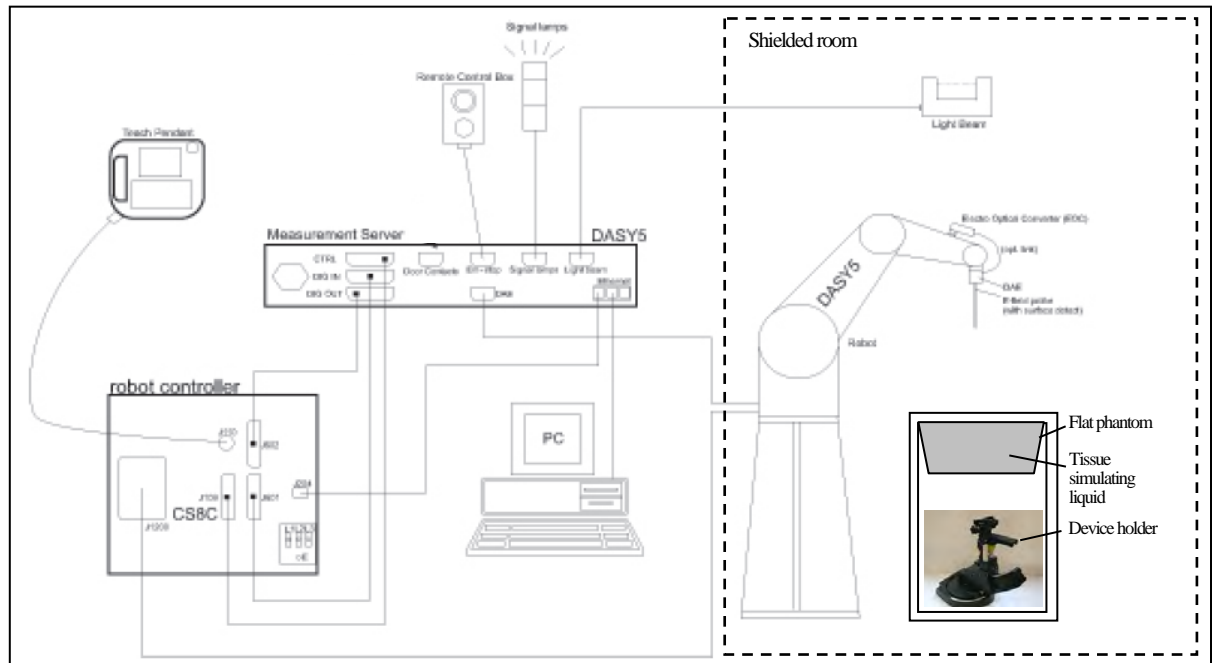

The DASY5 system for performing compliance tests consist of the following items:

1	A standard high precision 6-axis robot (Stäubli TX/RX family) with controller, teach pendant and software. An arm extension for accommodating the data acquisition electronics (DAE).
2	An isotropic field probe optimized and calibrated for the targeted measurement.
3	A data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
4	The Electro-optical converter (EOC) performs the conversion from optical to electrical signals for the digital communication to the DAE. To use optical surface detection, a special version of the EOC is required. The EOC signal is transmitted to the measurement server.
5	The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
6	The Light Beam used is for probe alignment. This improves the (absolute) accuracy of the probe positioning.
7	A computer running Win7 professional operating system and the DASY5 software.
8	R Remote control and teach pendant as well as additional circuitry for robot safety such as warning lamps, etc.
9	The phantom.
10	The device holder for EUT. (low-loss dielectric palette) (*. when it was used.)
11	Tissue simulating liquid mixed according to the given recipes.
12	Validation dipole kits allowing to validate the proper functioning of the system.

**Appendix 3-3: Test system specification**

**TX60 Lsepag robot/CS8Csepag-TX60 robot controller**

- Number of Axes : 6
- Repeatability : ±0.02 mm
- Manufacture : Stäubli Unimation Corp.

**DASY5 Measurement server**

- Features : The DASY5 measurement server is based on a PC/104 CPU board with a 400MHz intel ULV Celeron, 128MB chip-disk and 128MB RAM. The necessary circuits for communication with the DAE4 electronics box, as well as the 16 bit AD converter system for optical detection and digital I/O interface are contained on the DASY5 I/O board, which is directly connected to the PC/104 bus of the CPU board.
- Calibration : No calibration required.
- Manufacture : Schmid & Partner Engineering AG

**Data Acquisition Electronic (DAE)**

- Features : Signal amplifier, multiplexer, A/D converter and control logic.  
Serial optical link for communication with DASY5 embedded system (fully remote controlled). 2 step probe touch detector for mechanical surface detection and emergency robot stop (not in -R version)
- Measurement Range : 1 μV to > 200 mV (16bit resolution and 2 range settings: 4 mV, 400 mV)
- Input Offset voltage : < 1 μV (with auto zero)
- Input Resistance : 200 MΩ
- Battery Power : > 10 hrs. of operation (with two 9 V battery)
- Manufacture : Schmid & Partner Engineering AG

**Electro-Optical Converter (EOC61)**

- Manufacture : Schmid & Partner Engineering AG

**Light Beam Switch (LBS/80)**

- Manufacture : Schmid & Partner Engineering AG

**SAR measurement software**

- Item : Dosimetric Assessment System DASY5
- Software version : Refer to Appendix 3-1 (Equipment used)
- Manufacture : Schmid & Partner Engineering AG

**E-Field Probe**


- Model : EX3DV4 (serial number: 3907)
- Construction : Symmetrical design with triangular core.  
Built-in shielding against static charges.  
PEEK enclosure material (resistant to organic solvents, e.g., DGBE).
- Frequency : 10MHz to 6GHz, Linearity: ±0.2 dB (30MHz to 6GHz)
- Conversion Factors (CF) : Head: (2.45, 5.25, 5.6, 5.8) GHz  
Body: (2.45, 5.25, 5.6, 5.75) GHz
- Directivity : ±0.3 dB in HSL (rotation around probe axis)  
±0.5 dB in tissue material (rotation normal to probe axis)
- Dynamic Range : 10μW/g to > 100 mW/g; Linearity: ±0.2 dB (noise: typically < 1 μW/g)
- Dimension : Overall length: 330 mm (Tip: 20 mm)  
Tip diameter: 2.5 mm (Body: 12 mm)  
Typical distance from probe tip to dipole centers: 1mm
- Application : High precision dosimetric measurement in any exposure scenario (e.g., very strong gradient fields). Only probe which enables compliance testing for frequencies up to 6GHz with precision of better 30%.
- Manufacture : Schmid & Partner Engineering AG

**Phantom**

- Model Number : **ELI 4.0 oval flat phantom**
- Shell Material : Fiberglass
- Shell Thickness : Bottom plate: 2 ±0.2 mm
- Dimensions : Bottom elliptical: 600×400 mm, Depth: 190 mm (Volume: Approx. 30 liters)
- Manufacture : Schmid & Partner Engineering AG

**Device Holder**

- Urethane foam
- KSDH-01: In combination with the ELI4, the Mounting Device enables the rotation of the mounted transmitter device in spherical coordinates. Transmitter devices can be easily and accurately positioned. The low-loss dielectric urethane foam was used for the mounting section of device holder.
  - Material : Polyoxymethylene (POM)
  - Manufacture : Schmid & Partner Engineering AG
- SSDH-02: A simple but effective and easy-to-use extension for the Mounting Device; facilitates testing of larger devices (e.g., laptops, cameras, etc.) according to IEC 62209-2.
  - Material : Polyoxymethylene (POM), PET-G, Foam
  - Manufacture : Schmid & Partner Engineering AG

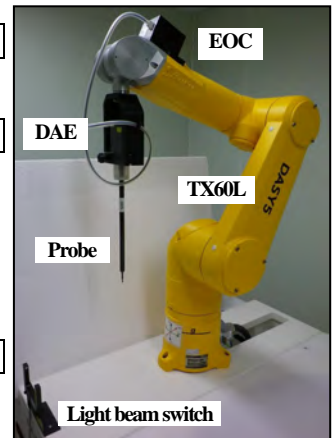

**Data storage and evaluation (postprocessing)**

The DASY5 software stores the measured voltage acquired by the Data Acquisition Electronics (DAE) as raw data together with all the necessary software parameters for the data evaluation (probe calibration data, liquid parameters and communication system parameters) in measurement files with the extension “.da5x”. The postprocessing software evaluates the data every time the data is visualized or exported.

The fields and SAR are calculated from the measured voltage (probe voltage acquired by the DAE) and the following parameters:

Probe parameters:	- Sensitivity	$norm_i, ai0, ai1, ai2$
	- Conversion Factor	$convFi$
	- Diode Compression Point	$dcp_i$
	- Probe Modulation Response Factors	$ai, bi, ci, d$
Device parameters:	- Frequency	$f$
	- Crest factor	$cf$
Media parameters:	- Conductivity	$\sigma$
	- Relative Permittivity	$\rho$

This parameters are stored in the DASY5 V52 measurement file.

These parameters must be correctly set in the DASY5 V52 software setup. They are available as configuration file and can be imported into the measurement file. The values displayed in the multimeter window are assessed using the parameters of the actual system setup. In the scan visualization and export modes, the parameters stored in the measurement file are used.

The measured voltage is not proportional to the exciting. It must be first linearized.

Approximated Probe Response Linearization using Crest Factor;

This linearization method is enabled when a custom defined communication system is measured. The compensation applied is a function of the measured voltage, the detector diode compression point and the crest factor of the measured signal.

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

with $V_i$	= linearized voltage of channel i in $\mu V$	(i = x,y,z)
$U_i$	= measured voltage of channel i in $\mu V$	(i = x,y,z)
$cf$	= crest factor of exciting field	(DASY parameter)
$dcp_i$	= diode compression point of channel i in $\mu V$	(Probe parameter, i= x,y,z)

The resulting linearized voltage is only approximated because the probe is not calibrated to this specific signal.

Field and SAR Calculation

The primary field data for each channel are calculated using the linearized voltage:

$$E - \text{fieldprobes} : E_i = \sqrt{\frac{V_i}{Norm_i \cdot ConvF}}$$

with $V_i$	= linearized voltage of channel i in $\mu V$	(i = x,y,z)
$Norm_i$	= sensor sensitivity of channel i in $\mu V/(V/m)^2$ for E-field Probes	(i = x,y,z)
$ConvF$	= sensitivity enhancement in solution	
$E_i$	= electric field strength of channel i in V/m	(i = x,y,z)

The RMS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$

The primary field data are used to calculate the derived field units.

$$SAR = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1'000}$$

with SAR	= local specific absorption rate in mW/g
$E_{tot}$	= total field strength in V/m
$\sigma$	= conductivity in [mho/m] or [Siemens/m]
$\rho$	= equivalent tissue density in g/cm <sup>3</sup>

**Appendix 3-4: Simulated tissue composition and parameter confirmation**

<b>Liquid type</b>	<b>Head</b>	<b>Control No.</b>	SSLHV6-01	<b>Model No./Product No.</b>	HBBL600-10000V6/SLAAH U16 BC
<b>Ingredient: Mixture [%]</b>	Water: >77, Ethanediol: <5.2, Sodium petroleum sulfonate: <2.9, Hexylene Glycol: <2.9, alkoxyated alcohol (>C <sub>16</sub> ): <2.0				
<b>Tolerance specification</b>	± 10%				
<b>Temperature gradients [% / deg.C]</b>	permittivity: -0.19 / conductivity: -0.57 (at 2.6 GHz), permittivity: +0.31 / conductivity: -1.43 (at 5.5 GHz) (*1)				
<b>Manufacture</b>	Schmid & Partner Engineering AG	Note: *1. speag_920.SLAAxyy-E_1.12.15CL (Maintenance of tissue simulating liquid)			

\*. The dielectric parameters were checked prior to assessment using the DAK3.5 dielectric probe kit.

Date measured	Frequency [MHz]	Liquid type	Ambient/		Liquid temp. [deg.C]	Liquid depth of phantom [mm]	Liquid parameters (*a)										ASAR (*b)	
			[deg.C]	[%RH]			Permittivity (ε <sub>r</sub> ) [-]				Δend, >48hrs	Conductivity [S/m]				Δend, >48hrs	1g [%]	10g [%]
							Target	Meas.	Δε <sub>r</sub> [%]	Limit		Target	Meas.	Δσ [%]	Limit			
May 12, 2021	5600	Head	23	45~55	22.5	152	35.53	35.46	-0.2	10%	-	5.065	5.005	-1.2	10%	-	0.1	0.1
May 13, 2021	5250	Head	23	45~55	22.5	152	35.93	36.03	0.3	10%	-	4.706	4.613	-2.0	10%	-	0.0	0.0
May 14, 2021	5800	Head	23	45~55	22.5	152	35.3	35.12	-0.5	10%	-	5.27	5.247	-0.4	10%	-	0.1	0.1
May 17, 2021	2450	Head	24	50~60	22.5	150	39.2	40.29	2.8	10%	-	1.80	1.853	3.0	10%	-	0.8	0.3
May 18, 2021	5600	Head	24	50~60	22.5	150	35.53	35.15	-1.1	10%	-	5.065	4.944	-2.4	10%	-	0.3	0.4
May 19, 2021	5250	Head	24	50~60	22.5	150	35.93	35.77	-0.4	10%	-	4.706	4.557	-3.2	10%	-	0.2	0.4
May 20, 2021	5800	Head	24	50~60	22.5	150	35.3	34.86	-1.3	10%	-	5.27	5.177	-1.8	10%	-	0.3	0.4

\*. Calculating formula: Δend(>48 hrs) (%) = {(dielectric properties, end of test series) / (dielectric properties, beginning of test series) - 1} × 100

\*a. The target values of (2000, 2450, 3000 and 5800) MHz are parameters defined in Appendix A of KDB 865664 D01. For other frequencies, the target nominal dielectric values shall be obtained by linear interpolation between the higher and lower tabulated figures.

f (MHz)	Standard						Interpolated & Extrapolated												
	Head Tissue		Body Tissue		f (MHz)	Head Tissue		Body Tissue		f (MHz)	Head Tissue		Body Tissue						
	ε <sub>r</sub>	σ [S/m]	ε <sub>r</sub>	σ [S/m]		ε <sub>r</sub>	σ [S/m]	ε <sub>r</sub>	σ [S/m]		ε <sub>r</sub>	σ [S/m]	ε <sub>r</sub>	σ [S/m]					
(1800-2000)	40.0	1.40	53.3	1.52	3000	38.5	2.40	52.0	2.73	5250	35.93	4.706	48.95	5.358	5750	35.36	5.219	48.27	5.942
2450	39.2	1.80	52.7	1.95	5800	35.3	5.27	48.2	6.00	5600	35.53	5.065	48.47	5.766					

\*b. The coefficients are parameters defined in IEEE Std. 1528-2013.

$$ASAR(1g) = C_{\epsilon} \times \Delta\epsilon_r + C_{\sigma} \times \Delta\sigma, C_{\epsilon} = 7.854E-4 \times f^3 + 9.402E-3 \times f^2 - 2.742E-2 \times f + 0.2026 / C_{\sigma} = 9.804E-3 \times f^3 - 8.661E-2 \times f^2 + 2.981E-2 \times f + 0.7829$$

$$ASAR(10g) = C_{\epsilon} \times \Delta\epsilon_r + C_{\sigma} \times \Delta\sigma, C_{\epsilon} = 3.456 \times 10^{-3} \times f^3 - 3.531 \times 10^{-2} \times f^2 + 7.675 \times 10^{-2} \times f + 0.1860 / C_{\sigma} = 4.479 \times 10^{-3} \times f^3 - 1.586 \times 10^{-2} \times f^2 - 0.1972 \times f + 0.7717$$

**Appendix 3-5: Daily check results**

\*. Prior to the SAR assessment of EUT, the Daily check was performed to test whether the SAR system was operating within its target of ±10%. The Daily check results are in the table below.

Date	Frequency [MHz]	ASAR		Daily check results (*. Meas.: Measured, Cal.: Calibration value, STD: Standard value)																		
		Liquid Type	1g [%]	10g [%]	SAR (1g) [W/kg] (*d)										SAR (10g) [W/kg] (*d)							
					Meas. (*c)	ASAR-correct	1W scaled	Target Cal. (*e)	STD (*f)	Deviation [%]	Limit [%]	Pass ?	Meas. (*c)	ASAR-correct	1W scaled	Target Cal. (*e)	STD (*f)	Deviation [%]	Limit [%]	Pass ?		
May 12, 2021	5600	Head	0.1	0.1	8.12	8.11	81.1	82.4	n/a	-1.6	-	10	Pass	2.3	2.3	23	23.4	n/a	-1.7	-	10	Pass
May 13, 2021	5250	Head	0.0	0.0	7.55	7.55	75.5	78.8	n/a	-4.2	-	10	Pass	2.17	2.17	21.7	22.6	n/a	-4.0	-	10	Pass
May 14, 2021	5800	Head	0.1	0.1	7.86	7.85	78.5	80.1	78	-2.0	0.6	10	Pass	2.22	2.22	22.2	22.5	21.9	-1.3	1.4	10	Pass
May 17, 2021	2450	Head	0.8	0.3	12.7	12.6	50.4	53.6	52.4	-6.0	-3.8	10	Pass	5.93	5.91	23.64	24.9	24	-5.1	-1.5	10	Pass
May 18, 2021	5600	Head	0.3	0.4	8.4	8.37	83.7	82.4	n/a	1.6	-	10	Pass	2.38	2.37	23.7	23.4	n/a	1.3	-	10	Pass
May 19, 2021	5250	Head	0.2	0.4	7.76	7.74	77.4	78.8	n/a	-1.8	-	10	Pass	2.23	2.22	22.2	22.6	n/a	-1.8	-	10	Pass
May 20, 2021	5800	Head	0.3	0.4	7.87	7.85	78.5	80.1	78	-2.0	0.6	10	Pass	2.23	2.22	22.2	22.5	21.9	-1.3	1.4	10	Pass


\*. Calculating formula: ASAR corrected SAR (1g, 10g) (W/kg) = (Measured SAR(1g, 10g) (W/kg)) × (100 - (ASAR(%)) / 100

\*c. The "Meas. (Measured)" SAR value is obtained at 250 mW for 2450MHz, 100 mW for (5250, 5600, 5800) MHz

\*d. The measured SAR value of Daily check was compensated for tissue dielectric deviations (ASAR) and scaled to 1W of output power in order to compare with the manufacture's calibration target value which was normalized.


\*e. The target value is a parameter defined in the calibration data sheet of D2450V2 (sn:822) and D5GHZV2 (sn:1070) dipole calibrated by Schmid & Partner Engineering AG (Certification No. D2450V2-822\_Nov20 and D5GHZV2-1070\_Apr21, the data sheet was filed in this report).

\*f. The target value (normalized to 1W) is defined in IEEE Std.1528.

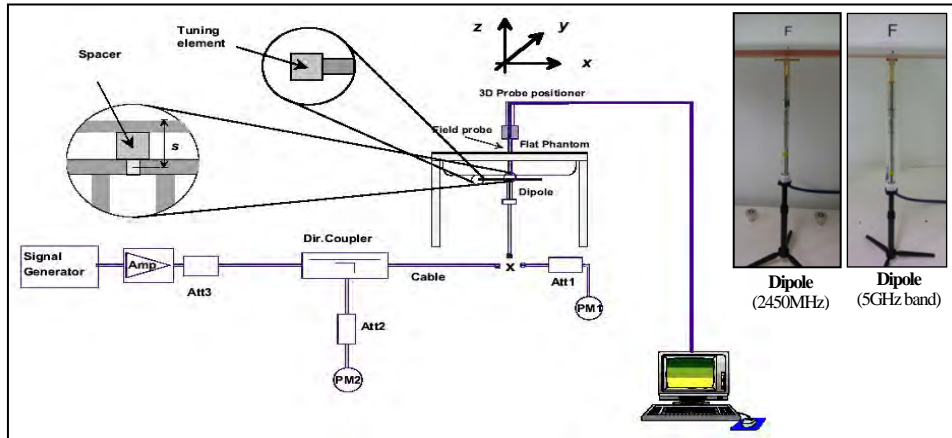

Test setup for the system performance check

**Appendix 3-6: Daily check measurement data**

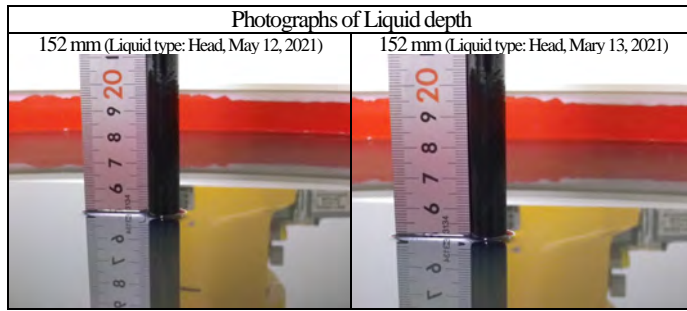


**EUT: Dipole(5GHz)(1070); Type: D5GHzV2; Serial: 1070; Forward conducted power: 100mW**  
**Communication System: CW (0) (\*.UID: 0, Frame Length in ms: 0; Communication System PAR: 0; PMF: 1); Frequency: 5600 MHz; Crest Factor: 1.0**  
**Medium: HSL5GHz(v6); Medium parameters used: f = 5600 MHz;  $\sigma = 5.005$  S/m;  $\epsilon_r = 35.47$ ;  $\rho = 1000$  kg/m<sup>3</sup>**  
 Measurement Standard: DASYS5 (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section  
 -DASY52.52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(4.56, 4.56, 4.56) @ 5600 MHz; Calibrated: 2021/04/21  
 -Sensor-Surface: 1.4mm (Mechanical Surface Detection), z = 1.0, 25.0, 156.0

**Area:60x60,10 (7x7x1):** Measurement grid: dx=10mm, dy=10mm; Maximum value of SAR (measured) = 21.0 W/kg  
**Area:60x60,10 (61x61x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm; Maximum value of SAR (interpolated) = 21.0 W/kg  
**Z;155,5 (1x1x32):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 19.6 W/kg

**Zoom:28x28x24,4,1.4(ratio) (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm;  
 Reference Value = 71.46 V/m; Power Drift = 0.02 dB; Maximum value of SAR (measured) = 19.7 W/kg; Peak SAR (extrapolated) = 34.7 W/kg  
**SAR(1g) = 8.12 W/kg; SAR(10g) = 2.3 W/kg** (\*. Smallest distance from peaks to all points 3 dB below = 7.5 mm; Ratio of SAR at M2 to SAR at M1 = 63.2%)

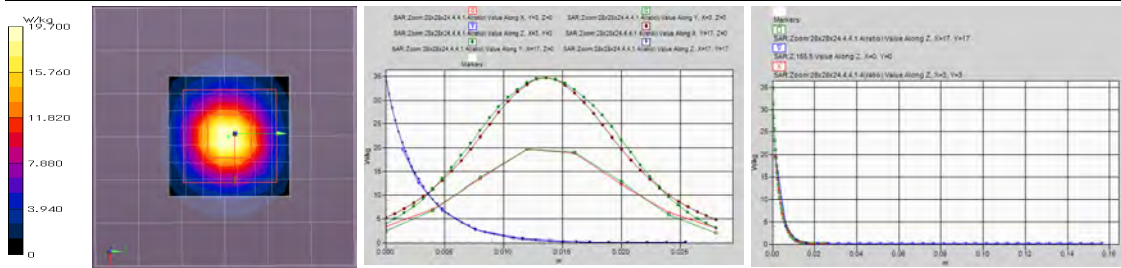


Remarks: \*. Date tested: 2021/5/12; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,  
 \*. liquid depth: 152 mm; Position: distance of dipole to phantom: 8mm (10mm to liquid); ambient: 23 deg.C. / (50-60) %RH,  
 \*. liquid temperature: 22.4(start)/22.4(end)/22.5(in check) deg.C.; \*. White cubic: zoom scan area, Red cubic: big=SAR(10g) /small=SAR(1g)

**EUT: Dipole(5GHz)(1070); Type: D5GHzV2; Serial: 1070; Forward conducted power: 100mW**  
**Communication System: CW (0) (\*.UID: 0, Frame Length in ms: 0; Communication System PAR: 0; PMF: 1); Frequency: 5250 MHz; Crest Factor: 1.0**  
**Medium: HSL5GHz(v6); Medium parameters used: f = 5250 MHz;  $\sigma = 4.613$  S/m;  $\epsilon_r = 36.03$ ;  $\rho = 1000$  kg/m<sup>3</sup>**  
 Measurement Standard: DASYS5 (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section  
 -DASY52.52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(5.14, 5.14, 5.14) @ 5250 MHz; Calibrated: 2021/04/21  
 -Sensor-Surface: 1.4mm (Mechanical Surface Detection), z = 1.0, 25.0, 156.0

**Area:60x60,10 (7x7x1):** Measurement grid: dx=10mm, dy=10mm; Maximum value of SAR (measured) = 18.6 W/kg  
**Area:60x60,10 (61x61x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm; Maximum value of SAR (interpolated) = 18.7 W/kg  
**Z;155,5 (1x1x32):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 17.2 W/kg


**Zoom:28x28x24,4,1.4(ratio) (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm;  
 Reference Value = 70.17 V/m; Power Drift = 0.04 dB; Maximum value of SAR (measured) = 17.3 W/kg; Peak SAR (extrapolated) = 29.4 W/kg  
**SAR(1g) = 7.55 W/kg; SAR(10g) = 2.17 W/kg** (\*. Smallest distance from peaks to all points 3 dB below = 7.4 mm; Ratio of SAR at M2 to SAR at M1 = 66%)

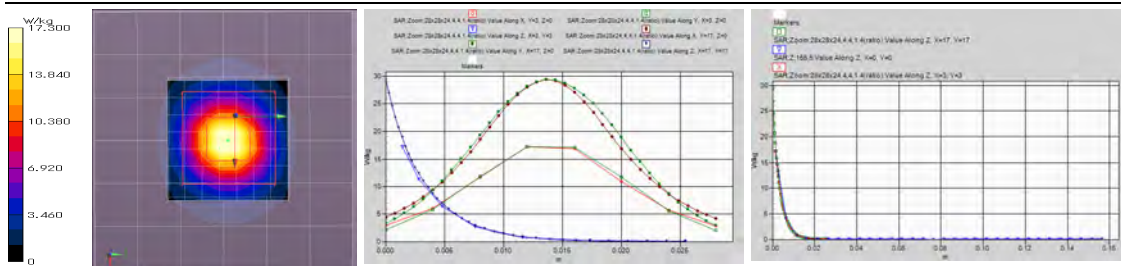

Remarks: \*. Date tested: 2021/5/13; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,  
 \*. liquid depth: 152 mm; Position: distance of dipole to phantom: 8mm (10mm to liquid); ambient: 23 deg.C. / (50-60) %RH,  
 \*. liquid temperature: 22.4(start)/22.4(end)/22.5(in check) deg.C.; \*. White cubic: zoom scan area, Red cubic: big=SAR(10g) /small=SAR(1g)



**Appendix 3-6: Daily check measurement data (cont'd)**

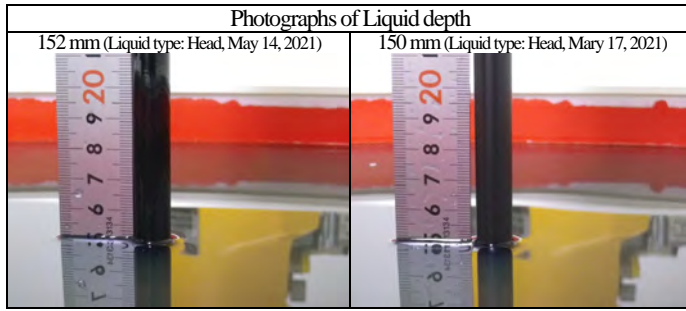


**EUT: Dipole(5GHz)(1070); Type: D5GHzV2; Serial: 1070; Forward conducted power: 100mW**  
**Communication System: CW (0) (\*UID: 0, Frame Length in ms: 0; Communication System PAR: 0; PMF: 1); Frequency: 5800 MHz; Crest Factor: 1.0**  
**Medium: HSL5GHz(v6); Medium parameters used: f = 5800 MHz;  $\sigma = 5.247$  S/m;  $\epsilon_r = 35.12$ ;  $\rho = 1000$  kg/m<sup>3</sup>**  
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section  
 -DASY52.52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(4.6, 4.6, 4.6) @ 5800 MHz; Calibrated: 2021/04/21  
 -Sensor-Surface: 1.4mm (Mechanical Surface Detection), z = 1.0, 25.0, 156.0

**Area:60x60,10 (7x7x1):** Measurement grid: dx=10mm, dy=10mm; Maximum value of SAR (measured) = 20.4 W/kg  
**Area:60x60,10 (61x61x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm; Maximum value of SAR (interpolated) = 20.5 W/kg  
**Z;155,5 (1x1x32):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 19.0 W/kg

**Zoom:28x28x24,4,1.4(ratio) (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm;  
 Reference Value = 68.90 V/m; Power Drift = 0.04 dB; Maximum value of SAR (measured) = 19.0 W/kg; Peak SAR (extrapolated) = 35.3 W/kg  
**SAR(1 g) = 7.86 W/kg; SAR(10 g) = 2.22 W/kg** (\*. Smallest distance from peaks to all points 3 dB below = 7.5 mm; Ratio of SAR at M2 to SAR at M1 = 61.6%)

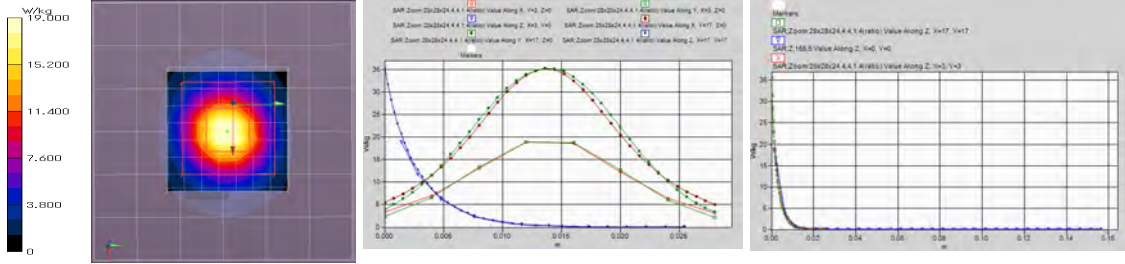


Remarks: \*. Date tested: 2021/5/14; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,  
 \*. liquid depth: 152 mm; Position: distance of dipole to phantom: 8mm (10mm to liquid); ambient: 23 deg.C. / (50~60) %RH,  
 \*. liquid temperature: 22.4(start)/22.4(end)/22.5(in check) deg.C.; \*. White cubic: zoom scan area, Red cubic: big=SAR(10g)/small=SAR(1g)

**EUT: D2450V2 - SN822; Type: D2450V2; Serial: SN822; Forward conducted power: 250mW**  
**Communication System: CW (0) (\*UID: 0, Frame Length in ms: 0; Communication System PAR: 0; PMF: 1); Frequency: 2450 MHz; Crest Factor: 1.0**  
**Medium: HSL5GHz(v6); Medium parameters used: f = 2450 MHz;  $\sigma = 1.853$  S/m;  $\epsilon_r = 40.29$ ;  $\rho = 1000$  kg/m<sup>3</sup>**  
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section  
 -DASY52.52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(7.35, 7.35, 7.35) @ 2450 MHz; Calibrated: 2021/04/21  
 -Sensor-Surface: 2mm (Mechanical Surface Detection), z = 1.0, 31.0, 161.0


**Area:60x60,15 (5x5x1):** Measurement grid: dx=15mm, dy=15mm; Maximum value of SAR (measured) = 19.3 W/kg  
**Area:60x60,15 (41x41x1):** Interpolated grid: dx=1.500 mm, dy=1.500 mm; Maximum value of SAR (interpolated) = 19.3 W/kg  
**Z;160,5 (1x1x33):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 19.4 W/kg

**Zoom:30x30x30,5 (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm;  
 Reference Value = 104.0 V/m; Power Drift = 0.07 dB; Maximum value of SAR (measured) = 19.4 W/kg; Peak SAR (extrapolated) = 25.9 W/kg  
**SAR(1 g) = 12.7 W/kg; SAR(10 g) = 5.93 W/kg** (\*. Smallest distance from peaks to all points 3 dB below = 9.2 mm; Ratio of SAR at M2 to SAR at M1 = 49.5%)

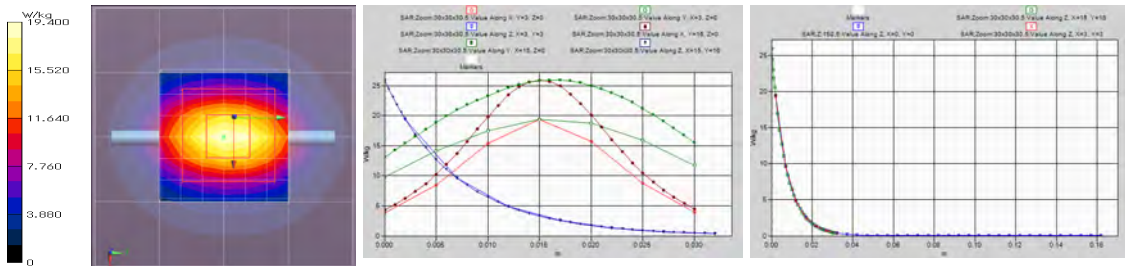

Remarks: \*. Date tested: 2021/5/17; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,  
 \*. liquid depth: 150 mm; Position: distance of dipole to phantom: 8mm (10mm to liquid); ambient: 23 deg.C. / (60~70) %RH,  
 \*. liquid temperature: 22.5(start)/22.6(end)/22.5(in check) deg.C.; \*. White cubic: zoom scan area, Red cubic: big=SAR(10g)/small=SAR(1g)

**Appendix 3-6: Daily check measurement data (cont'd)**

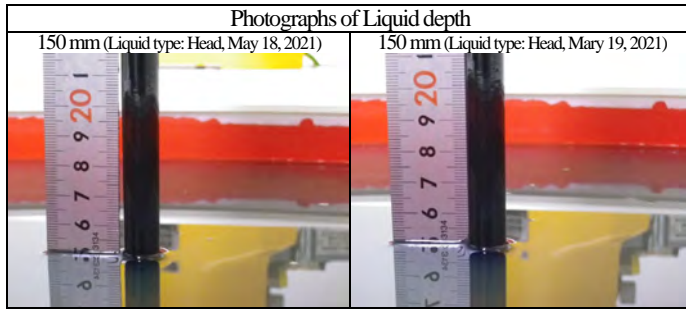

**EUT: Dipole(5GHz)(1070); Type: D5GHzV2; Serial: 1070; Forward conducted power: 100mW**

**Communication System: CW (0) (\*UID: 0, Frame Length in ms: 0; Communication System PAR: 0; PMF: 1); Frequency: 5600 MHz; Crest Factor: 1.0**

**Medium: HSL5GHz(v6); Medium parameters used: f = 5600 MHz;  $\sigma = 4.944$  S/m;  $\epsilon_r = 35.15$ ;  $\rho = 1000$  kg/m<sup>3</sup>**

Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section

-DASY52.52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(4.56, 4.56, 4.56) @ 5600 MHz; Calibrated: 2021/04/21

-Sensor-Surface: 1.4mm (Mechanical Surface Detection), z = 1.0, 25.0, 156.0

**Area:60x60,10 (7x7x1):** Measurement grid: dx=10mm, dy=10mm; Maximum value of SAR (measured) = 21.3 W/kg


**Area:60x60,10 (61x61x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm; Maximum value of SAR (interpolated) = 21.4 W/kg

**Z;155,5 (1x1x32):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 20.4 W/kg

**Zoom:28x28x24,4,4,1.4(ratio) (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm;

Reference Value = 72.36 V/m; Power Drift = 0.09 dB; Maximum value of SAR (measured) = 20.1 W/kg; Peak SAR (extrapolated) = 35.7 W/kg

**SAR(1 g) = 8.4 W/kg; SAR(10 g) = 2.38 W/kg** (\* Smallest distance from peaks to all points 3 dB below = 7.2 mm; Ratio of SAR at M2 to SAR at M1 = 63.6%)

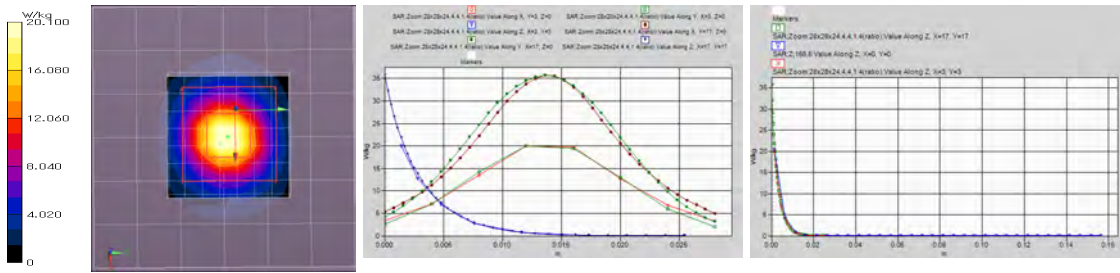

Remarks: \* Date tested: 2021/5/18; Tested by: Hiroshi Naka; Tested place: No.7 shielded room.  
 \* liquid depth: 150 mm; Position: distance of dipole to phantom: 8mm (10mm to liquid); ambient: 23 deg.C. / (60~70) %RH,  
 \* liquid temperature: 22.6(start)/22.6(end)/22.5(in check) deg.C.; \* White cubic: zoom scan area, Red cubic: big-SAR(10g) / small-SAR(1g)

**EUT: Dipole(5GHz)(1070); Type: D5GHzV2; Serial: 1070; Forward conducted power: 100mW**

**Communication System: CW (0) (\*UID: 0, Frame Length in ms: 0; Communication System PAR: 0; PMF: 1); Frequency: 5250 MHz; Crest Factor: 1.0**

**Medium: HSL5GHz(v6); Medium parameters used: f = 5250 MHz;  $\sigma = 4.557$  S/m;  $\epsilon_r = 35.77$ ;  $\rho = 1000$  kg/m<sup>3</sup>**

Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section

-DASY52.52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(5.14, 5.14, 5.14) @ 5250 MHz; Calibrated: 2021/04/21

-Sensor-Surface: 1.4mm (Mechanical Surface Detection), z = 1.0, 25.0, 156.0

**Area:60x60,10 (7x7x1):** Measurement grid: dx=10mm, dy=10mm; Maximum value of SAR (measured) = 19.1 W/kg


**Area:60x60,10 (61x61x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm; Maximum value of SAR (interpolated) = 19.1 W/kg

**Z;155,5 (1x1x32):** Measurement grid: dx=20mm, dy=20mm, dz=5mm; Maximum value of SAR (measured) = 18.2 W/kg

**Zoom:28x28x24,4,4,1.4(ratio) (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm;


Reference Value = 70.93 V/m; Power Drift = 0.10 dB; Maximum value of SAR (measured) = 18.1 W/kg; Peak SAR (extrapolated) = 30.3 W/kg

**SAR(1 g) = 7.76 W/kg; SAR(10 g) = 2.23 W/kg** (\* Smallest distance from peaks to all points 3 dB below = 7.2 mm; Ratio of SAR at M2 to SAR at M1 = 66.2%)

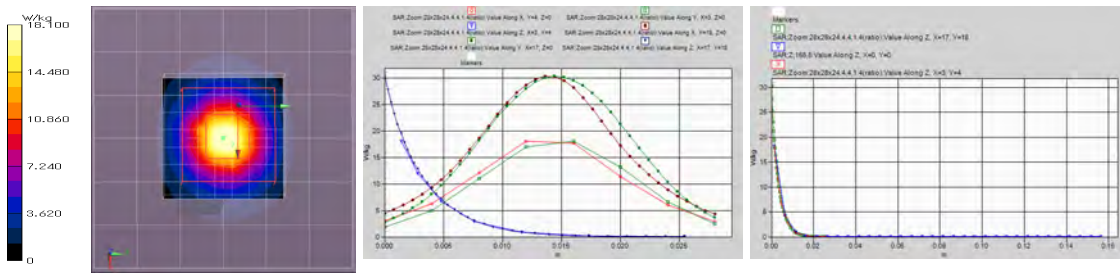

Remarks: \* Date tested: 2021/5/19; Tested by: Hiroshi Naka; Tested place: No.7 shielded room.  
 \* liquid depth: 150 mm; Position: distance of dipole to phantom: 8mm (10mm to liquid); ambient: 23 deg.C. / (60~70) %RH,  
 \* liquid temperature: 22.6(start)/22.6(end)/22.5(in check) deg.C.; \* White cubic: zoom scan area, Red cubic: big-SAR(10g) / small-SAR(1g)

**Appendix 3-6: Daily check measurement data (cont'd)**

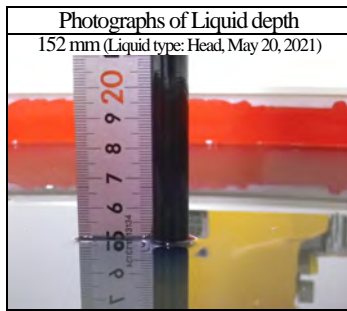

**EUT: Dipole(5GHz)(1070); Type: D5GHzV2; Serial: 1070; Forward conducted power: 100mW**

**Communication System: CW (0) (\*UID: 0, Frame Length in ms: 0; Communication System PAR: 0; PMF: 1); Frequency: 5800 MHz; Crest Factor: 1.0**

**Medium: HSL5GHz(v6); Medium parameters used:  $f = 5800$  MHz;  $\sigma = 5.177$  S/m;  $\epsilon_r = 34.86$ ;  $\rho = 1000$  kg/m<sup>3</sup>**

Measurement Standard: DASYS5 (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** -Electronics: DAE4 Sn626; Calibrated: 2020/11/17 / -Phantom: ELI v4.0; Type: QDOVA001BA; Serial: 1059; Phantom section: Flat Section

-DASY52.52.10.3(1513); SEMCAD X 14.6.13(7474) / -Probe: EX3DV4 - SN3907; ConvF(4.6, 4.6, 4.6) @ 5800 MHz; Calibrated: 2021/04/21

-Sensor-Surface: 1.4mm (Mechanical Surface Detection),  $z = 1.0, 25.0, 156.0$

**Area:60x60,10 (7x7x1):** Measurement grid:  $dx=10$ mm,  $dy=10$ mm; Maximum value of SAR (measured) = 20.4 W/kg


**Area:60x60,10 (61x61x1):** Interpolated grid:  $dx=1.000$  mm,  $dy=1.000$  mm; Maximum value of SAR (interpolated) = 20.5 W/kg

**Z;155,5 (1x1x32):** Measurement grid:  $dx=20$ mm,  $dy=20$ mm,  $dz=5$ mm; Maximum value of SAR (measured) = 18.7 W/kg

**Zoom:28x28x24,4,4,1.4(ratio) (8x8x7)/Cube 0:** Measurement grid:  $dx=4$ mm,  $dy=4$ mm,  $dz=1.4$ mm;

Reference Value = 68.93 V/m; Power Drift = 0.06 dB; Maximum value of SAR (measured) = 18.9 W/kg; Peak SAR (extrapolated) = 35.1 W/kg

**SAR(1g) = 7.87 W/kg; SAR(10g) = 2.23 W/kg** (\*. Smallest distance from peaks to all points 3 dB below = 7.2 mm; Ratio of SAR at M2 to SAR at M1 = 61.8%)

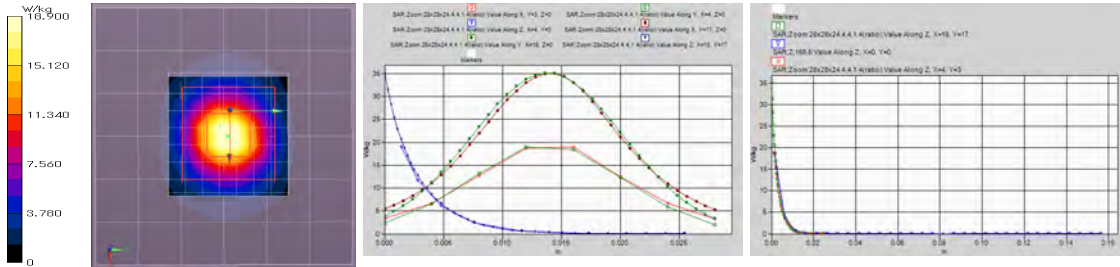

Remarks: \* Date tested: 2021/5/20; Tested by: Hiroshi Naka; Tested place: No.7 shielded room,  
 \* liquid depth: 150 mm; Position: distance of dipole to phantom: 8mm (10mm to liquid); ambient: 23 deg.C. / (60~70) %RH,  
 \* liquid temperature: 22.6(start)/22.6(end)/22.5(in check) deg.C.; \*.White cubic: zoom scan area, Red cubic: big=SAR(10g )/small=SAR(1g)

**Appendix 3-7: Uncertainty Assessment (SAR measurement/Daily check)**

\*. Although this standard determines only the limit value of uncertainty, there is no applicable rule of uncertainty in this. Therefore, the following results are derived depending on whether or not laboratory uncertainty is applied.

Uncertainty of SAR measurement (2.4GHz~6GHz) (*.v6h,e&σ: 10%, DAK3.5, Tx: ≈100% duty cycle) (v09r02)							1g SAR	10g SAR	
Combined measurement uncertainty of the measurement system (k=1)							± 13.2 %	± 13.1 %	
Expanded uncertainty (k=2)							± 26.4 %	± 26.2 %	
	Error Description (2.4-6GHz)	Uncertainty Value	Probability distribution	Divisor	ci (1g)	ci (10g)	ui (1g)	ui (10g)	Vi, veff
<b>A</b>	<b>Measurement System (DASY5)</b>						(std. uncertainty)	(std. uncertainty)	
1	Probe Calibration Error	±7.0 %	Normal	1	1	1	±7.0 %	±7.0 %	∞
2	Axial isotropy Error	±4.7 %	Rectangular	√3	0.71	0.71	±1.9 %	±1.9 %	∞
3	Hemispherical isotropy Error	±9.6 %	Rectangular	√3	0.71	0.71	±3.9 %	±3.9 %	∞
4	Linearity Error	±4.7 %	Rectangular	√3	1	1	±2.7 %	±2.7 %	∞
5	Probe modulation response (v09)	±5.5 %	Rectangular	√3	1	1	±3.2 %	±3.2 %	∞
6	Sensitivity Error (detection limit)	±1.0 %	Rectangular	√3	1	1	±0.6 %	±0.6 %	∞
7	Boundary effects Error	±4.3 %	Rectangular	√3	1	1	±2.5 %	±2.5 %	∞
8	Readout Electronics Error(DAE)	±0.3 %	Rectangular	√3	1	1	±0.3 %	±0.3 %	∞
9	Response Time Error	±0.8 %	Normal	1	1	1	±0.5 %	±0.5 %	∞
10	Integration Time Error (≈100% duty cycle)	±0 %	Rectangular	√3	1	1	0 %	0 %	∞
11	RF ambient conditions-noise (v09)	±1.0 %	Rectangular	√3	1	1	±0.6 %	±0.6 %	∞
12	RF ambient conditions-reflections	±3.0 %	Rectangular	√3	1	1	±1.7 %	±1.7 %	∞
13	Probe positioner mechanical tolerance	±3.3 %	Rectangular	√3	1	1	±1.9 %	±1.9 %	∞
14	Probe Positioning with respect to phantom shell	±6.7 %	Rectangular	√3	1	1	±3.9 %	±3.9 %	∞
15	Max. SAR evaluation (Post-processing)	±4.0 %	Rectangular	√3	1	1	±2.3 %	±2.3 %	∞
<b>B</b>	<b>Test Sample Related</b>								
16	Device Holder or Positioner Tolerance (v09)	±3.2 %	Normal	1	1	1	±3.2 %	±3.2 %	5
17	Test Sample Positioning Error (v09)	±2.1 %	Normal	1	1	1	±2.1 %	±2.1 %	10
18	Power scaling	±0 %	Rectangular	√3	1	1	±0 %	±0 %	∞
19	Drift of output power (measured, <0.2dB)	±5.0 %	Rectangular	√3	1	1	±2.9 %	±2.9 %	∞
<b>C</b>	<b>Phantom and Setup</b>								
20	Phantom uncertainty (shape, thickness tolerances)	±7.5 %	Rectangular	√3	1	1	±4.3 %	±4.3 %	∞
21	Algorithm for correcting SAR (e',σ: 10%)	±1.9 %	Normal	1	1	0.84	±1.9 %	±1.6 %	∞
22	Measurement Liquid Conductivity Error (DAK3.5)	±3.0 %	Normal	1	0.78	0.71	±2.3 %	±2.1 %	7
23	Measurement Liquid Permittivity Error (DAK3.5)	±3.1 %	Normal	1	0.23	0.26	±0.7 %	±0.8 %	7
24	Liquid Conductivity-temp.uncertainty (≤2deg.C.v6h)	±3.0 %	Rectangular	√3	0.78	0.71	±1.4 %	±1.2 %	∞
25	Liquid Permittivity-temp.uncertainty (≤2deg.C.v6h)	±1.0 %	Rectangular	√3	0.23	0.26	±0.1 %	±0.2 %	∞
	<b>Combined Standard Uncertainty (v09r02)</b>						± 13.2 %	± 13.1 %	945
	<b>Expanded Uncertainty (k=2) (v09r02)</b>						± 26.4 %	± 26.2 %	

\*. This measurement uncertainty budget is suggested by IEEE Std.1528(2013) and determined by Schmid & Partner Engineering AG (DASY5 Uncertainty Budget). Per KDB 865664 D01 (v01r04) SAR Measurement 100 MHz to 6 GHz, Section 2.8.1., when the highest measured SAR(1g) within a frequency band is < 1.5W/kg, the extensive SAR measurement uncertainty analysis described in IEEE Std.1528 (2013) is not required in SAR reports submitted for equipment approval.

Uncertainty of daily check (2.4~6GHz) (*.v6h,e&σ tolerance: 10%, DAK3.5, CW) (v09r02)							1g SAR	10g SAR	
Combined measurement uncertainty of the measurement system (k=1)							± 10.8 %	± 10.7 %	
Expanded uncertainty (k=2)							± 21.6 %	± 21.4 %	
	Error Description (2.4-6GHz)	Uncertainty Value	Probability distribution	Divisor	ci (1g)	ci (10g)	ui (1g)	ui (10g)	Vi, veff
<b>A</b>	<b>Measurement System (DASY5)</b>						(std. uncertainty)	(std. uncertainty)	
1	Probe Calibration Error	±7.0 %	Normal	1	1	1	±7.0 %	±7.0 %	∞
2	Axial isotropy error	±4.7 %	Rectangular	√3	0.71	0.71	±1.9 %	±1.9 %	∞
3	Hemispherical isotropy error	±9.6 %	Rectangular	√3	0	0	0 %	0 %	∞
4	Probe linearity	±4.7 %	Rectangular	√3	1	1	±2.7 %	±2.7 %	∞
5	Probe modulation response (CW)	±0.0 %	Rectangular	√3	1	1	0 %	0 %	∞
6	System detection limit	±1.0 %	Rectangular	√3	1	1	±0.6 %	±0.6 %	∞
7	Boundary effects	±4.3 %	Rectangular	√3	1	1	±2.5 %	±2.5 %	∞
8	System readout electronics (DAE)	±0.3 %	Normal	1	1	1	±0.3 %	±0.3 %	∞
9	Response Time Error (<5ms/100ms wait)	±0.0 %	Rectangular	√3	1	1	0 %	0 %	∞
10	Integration Time Error (CW)	±0.0 %	Rectangular	√3	1	1	0 %	0 %	∞
11	RF ambient conditions-noise	±3.0 %	Rectangular	√3	1	1	±1.7 %	±1.7 %	∞
12	RF ambient conditions-reflections	±3.0 %	Rectangular	√3	1	1	±1.7 %	±1.7 %	∞
13	Probe positioner mechanical tolerance	±3.3 %	Rectangular	√3	1	1	±1.9 %	±1.9 %	∞
14	Probe positioning with respect to phantom shell	±6.7 %	Rectangular	√3	1	1	±3.9 %	±3.9 %	∞
15	Max. SAR evaluation (Post-processing)	±4.0 %	Rectangular	√3	1	1	±2.3 %	±2.3 %	∞
<b>B</b>	<b>Test Sample Related</b>								
16	Deviation of the experimental source	±1.9 %	Normal	1	1	1	±1.9 %	±1.9 %	∞
17	Dipole to liquid distance (10mm±0.2mm,<2deg.)	±2.0 %	Rectangular	√3	1	1	±1.2 %	±1.2 %	∞
18	Drift of output power (measured, <0.1dB)	±2.3 %	Rectangular	√3	1	1	±1.3 %	±1.3 %	∞
<b>C</b>	<b>Phantom and Setup</b>								
19	Phantom uncertainty	±2.0 %	Rectangular	√3	1	1	±1.2 %	±1.2 %	∞
20	Algorithm for correcting SAR (e',σ: 10%)	±1.9 %	Normal	1	1	0.84	±1.9 %	±1.6 %	∞
21	Liquid conductivity (meas.) (DAK3.5)	±3.0 %	Normal	1	0.78	0.71	±2.3 %	±2.1 %	∞
22	Liquid permittivity (meas.) (DAK3.5)	±3.1 %	Normal	1	0.23	0.26	±0.7 %	±0.8 %	∞
23	Liquid Conductivity-temp.uncertainty (≤2deg.C.v6h)	±3.0 %	Rectangular	√3	0.78	0.71	±1.4 %	±1.2 %	∞
24	Liquid Permittivity-temp.uncertainty (≤2deg.C.v6h)	±1.0 %	Rectangular	√3	0.23	0.26	±0.1 %	±0.2 %	∞
	<b>Combined Standard Uncertainty (v09r02)</b>						± 10.8 %	± 10.7 %	
	<b>Expanded Uncertainty (k=2) (v09r02)</b>						± 21.6 %	± 21.4 %	

\*. This measurement uncertainty budget is suggested by IEEE Std. 1528(2013) and determined by Schmid & Partner Engineering AG (DASY5 Uncertainty Budget).

\*. Table of uncertainties are listed for ISO/IEC 17025.

**Appendix 3-8: Calibration certificate: E-Field Probe (EX3DV4)**

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **UL Japan (RCC)**

Certificate No: **EX3-3907\_Apr21**

**CALIBRATION CERTIFICATE**

Object **EX3DV4 - SN:3907**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-14.v6, QA CAL-23.v5, QA CAL-25.v7  
Calibration procedure for dosimetric E-field probes**

Calibration date: **April 21, 2021**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	09-Apr-21 (No. 217-03291/03292)	Apr-22
Power sensor NRP-Z91	SN: 103244	09-Apr-21 (No. 217-03291)	Apr-22
Power sensor NRP-Z91	SN: 103245	09-Apr-21 (No. 217-03292)	Apr-22
Reference 20 dB Attenuator	SN: CC2552 (20x)	09-Apr-21 (No. 217-03343)	Apr-22
DAE4	SN: 660	23-Dec-20 (No. DAE4-660_Dec20)	Dec-21
Reference Probe ES3DV2	SN: 3013	30-Dec-20 (No. ES3-3013_Dec20)	Dec-21
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (in house check Jun-20)	In house check: Jun-22
Power sensor E4412A	SN: MY41498087	06-Apr-16 (in house check Jun-20)	In house check: Jun-22
Power sensor E4412A	SN: 000110210	06-Apr-16 (in house check Jun-20)	In house check: Jun-22
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-20)	In house check: Jun-22
Network Analyzer E8358A	SN: US41080477	31-Mar-14 (in house check Oct-20)	In house check: Oct-21

Calibrated by:	Name <b>Jeffrey Katzman</b>	Function <b>Laboratory Technician</b>	Signature 
Approved by:	Name <b>Katja Pokovic</b>	Function <b>Technical Manager</b>	Signature 

Issued: April 24, 2021

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Appendix 3-8: Calibration certificate: E-Field Probe (EX3DV4) (cont'd)**

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 0108**

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

**Glossary:**

TSL	tissue simulating liquid
NORM <sub>x,y,z</sub>	sensitivity in free space
ConvF	sensitivity in TSL / NORM <sub>x,y,z</sub>
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization $\varphi$	$\varphi$ rotation around probe axis
Polarization $\vartheta$	$\vartheta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

**Calibration is Performed According to the Following Standards:**

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Methods Applied and Interpretation of Parameters:**

- NORM<sub>x,y,z</sub>**: Assessed for E-field polarization  $\vartheta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not affect the E<sup>2</sup>-field uncertainty inside TSL (see below ConvF).
- NORM(f)<sub>x,y,z</sub> = NORM<sub>x,y,z</sub> \* frequency\_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>x,y,z</sub>**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; D<sub>x,y,z</sub>; VR<sub>x,y,z</sub>**: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM<sub>x</sub> (no uncertainty required).

**Appendix 3-8: Calibration certificate: E-Field Probe (EX3DV4) (cont'd)**

EX3DV4 – SN:3907

April 21, 2021

**DASY/EASY - Parameters of Probe: EX3DV4 - SN:3907****Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) <sup>A</sup>	0.45	0.58	0.54	$\pm 10.1\%$
DCP (mV) <sup>B</sup>	102.7	97.5	99.0	

**Calibration Results for Modulation Response**

UID	Communication System Name		A dB	B dB/ $\mu\text{V}$	C	D dB	VR mV	Max dev.	Unc <sup>C</sup> (k=2)
0	CW	X	0.0	0.0	1.0	0.00	134.6	$\pm 3.5\%$	$\pm 4.7\%$
		Y	0.0	0.0	1.0		129.4		
		Z	0.0	0.0	1.0		129.5		

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of Norm X,Y,Z do not affect the  $E^2$ -field uncertainty inside TSL (see Pages 5 and 6).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>C</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

**Appendix 3-8: Calibration certificate: E-Field Probe (EX3DV4) (cont'd)**

EX3DV4- SN:3907

April 21, 2021

**DASY/EASY - Parameters of Probe: EX3DV4 - SN:3907****Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	-143.3
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

**Note:** Measurement distance from surface can be increased to 3-4 mm for an *Area Scan* job.



**Appendix 3-8: Calibration certificate: E-Field Probe (EX3DV4) (cont'd)**

EX3DV4– SN:3907

April 21, 2021

**DASY/EASY - Parameters of Probe: EX3DV4 - SN:3907****Calibration Parameter Determined in Head Tissue Simulating Media**

f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unc (k=2)
2450	39.2	1.80	7.35	7.35	7.35	0.41	0.90	± 12.0 %
5250	35.9	4.71	5.14	5.14	5.14	0.40	1.80	± 13.1 %
5600	35.5	5.07	4.56	4.56	4.56	0.40	1.80	± 13.1 %
5800	35.3	5.27	4.60	4.60	4.60	0.40	1.80	± 13.1 %

<sup>C</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 6 MHz is 4-9 MHz, and ConvF assessed at 13 MHz is 9-19 MHz. Above 5 GHz frequency validity can be extended to ± 110 MHz.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

**Appendix 3-8: Calibration certificate: E-Field Probe (EX3DV4) (cont'd)**

EX3DV4- SN:3907

April 21, 2021

**DASY/EASY - Parameters of Probe: EX3DV4 - SN:3907****Calibration Parameter Determined in Body Tissue Simulating Media**

f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unc (k=2)
2450	52.7	1.95	7.44	7.44	7.44	0.36	0.95	± 12.0 %
5250	48.9	5.36	4.49	4.49	4.49	0.50	1.90	± 13.1 %
5600	48.5	5.77	3.96	3.96	3.96	0.50	1.90	± 13.1 %
5750	48.3	5.94	4.07	4.07	4.07	0.50	1.90	± 13.1 %

<sup>C</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 6 MHz is 4-9 MHz, and ConvF assessed at 13 MHz is 9-19 MHz. Above 5 GHz frequency validity can be extended to ± 110 MHz.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.


<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

**Appendix 3-8: Calibration certificate: E-Field Probe (EX3DV4) (cont'd)**

EX3DV4- SN:3907

April 21, 2021

**Frequency Response of E-Field**  
(TEM-Cell:ifi110 EXX, Waveguide: R22)

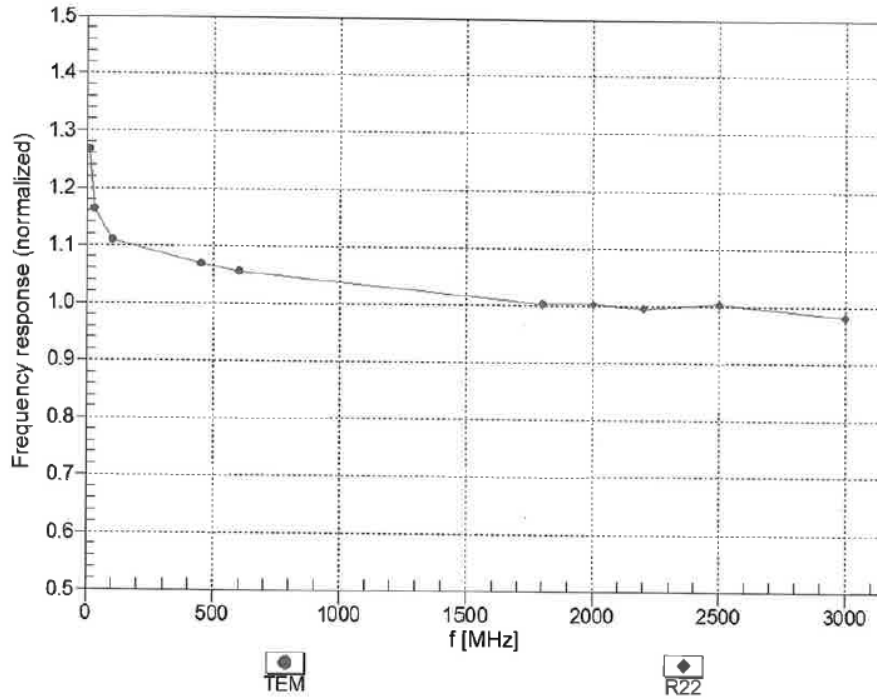



Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  ( $k=2$ )

**Appendix 3-8: Calibration certificate: E-Field Probe (EX3DV4) (cont'd)**

EX3DV4- SN:3907

April 21, 2021

**Receiving Pattern ( $\phi$ ),  $\theta = 0^\circ$**

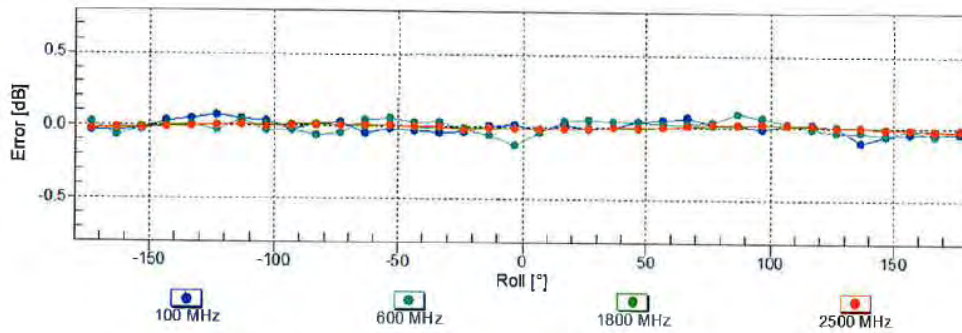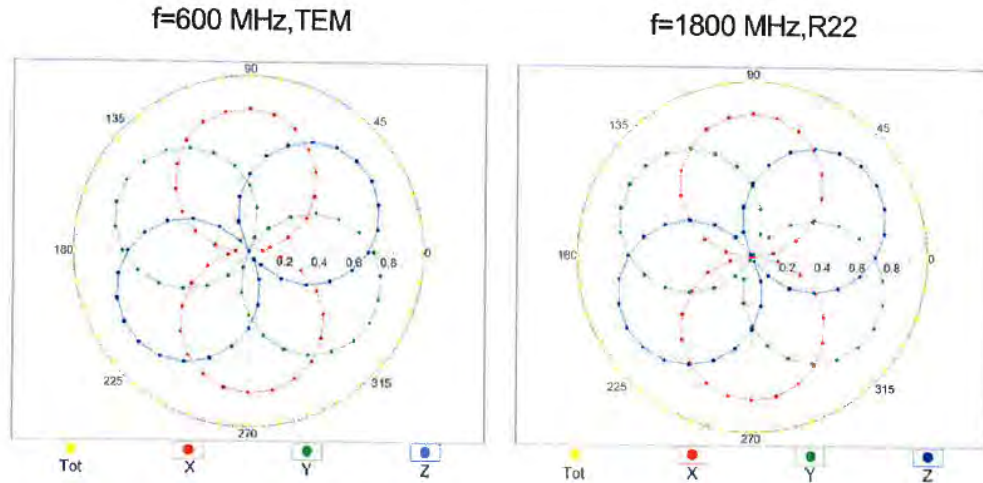



**Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )**

Appendix 3-8: Calibration certificate: E-Field Probe (EX3DV4) (cont'd)

EX3DV4- SN:3907

April 21, 2021

### Dynamic Range f(SAR<sub>head</sub>) (TEM cell , f<sub>eval</sub>= 1900 MHz)

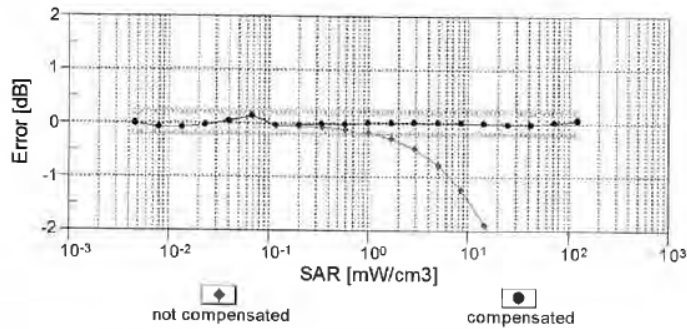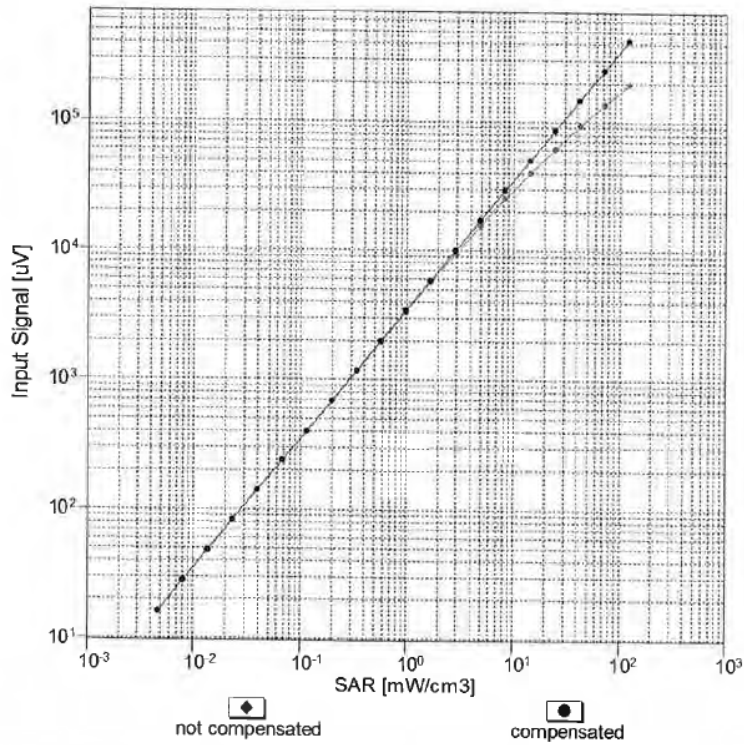


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

**Appendix 3-8: Calibration certificate: E-Field Probe (EX3DV4) (cont'd)**


EX3DV4- SN:3907

April 21, 2021

### Conversion Factor Assessment

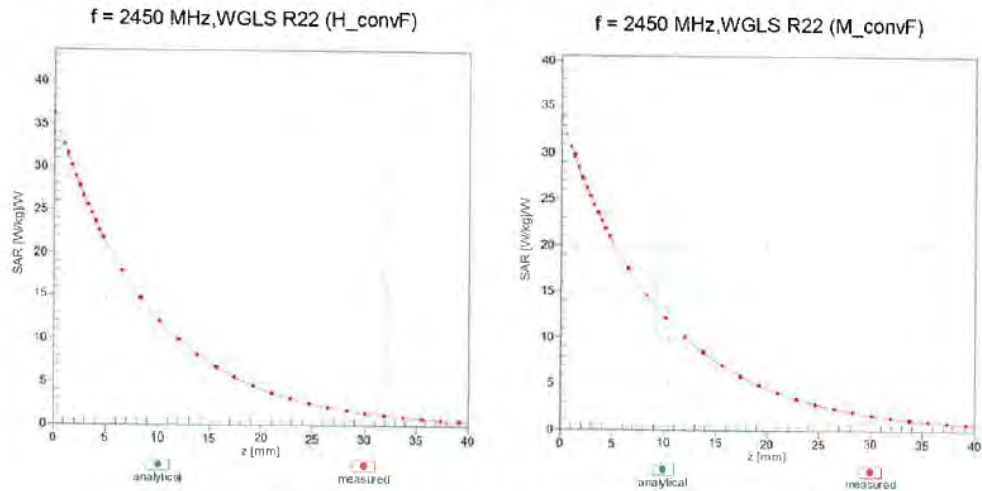

### Deviation from Isotropy in Liquid Error ( $\phi, \theta$ ), f = 900 MHz

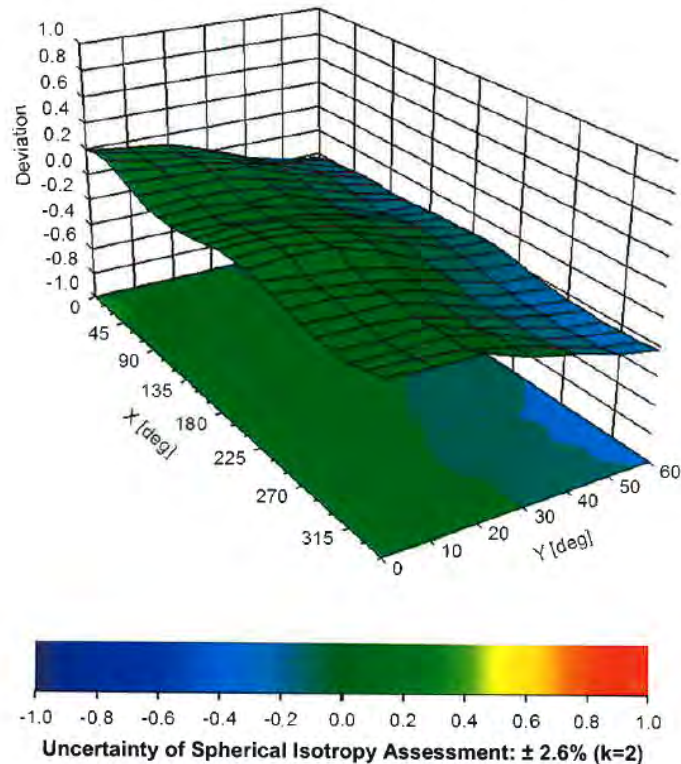

**Appendix 3-9: Calibration certificate: Dipole (D2450V2)**

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schwalzerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **UL Japan (RCC)**

Certificate No: **D2450V2-822\_Nov20**

**CALIBRATION CERTIFICATE**

Object **D2450V2 - SN:822**

Calibration procedure(s) **QA CAL-05.v11  
Calibration Procedure for SAR Validation Sources between 0.7-3 GHz**

Calibration date: **November 10, 2020**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	01-Apr-20 (No. 217-03100/03101)	Apr-21
Power sensor NRP-Z91	SN: 103244	01-Apr-20 (No. 217-03100)	Apr-21
Power sensor NRP-Z91	SN: 103245	01-Apr-20 (No. 217-03101)	Apr-21
Reference 20 dB Attenuator	SN: BH8394 (20k)	31-Mar-20 (No. 217-03106)	Apr-21
Type-N mismatch combination	SN: 310982 / 06327	31-Mar-20 (No. 217-03104)	Apr-21
Reference Probe EX3DV4	SN: 7405	29-Jun-20 (No. EX3-7405_Jun20)	Jun-21
DAE4	SN: 601	02-Nov-20 (No. DAE4-601_Nov20)	Nov-21
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oct-20)	In house check: Oct-22
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-20)	In house check: Oct-22
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-20)	In house check: Oct-22
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-20)	In house check: Oct-22
Network Analyzer Agilent E8358A	SN: US41060477	31-Mar-14 (in house check Oct-20)	In house check: Oct-21

Calibrated by:	Name <b>Michael Weber</b>	Function <b>Laboratory Technician</b>	Signature 
Approved by:	Name <b>Katja Pokovic</b>	Function <b>Technical Manager</b>	Signature 

Issued: November 11, 2020

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Appendix 3-9: Calibration certificate: Dipole (D2450V2) (cont'd)**

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

**Glossary:**

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.



**Appendix 3-9: Calibration certificate: Dipole (D2450V2) (cont'd)****Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz $\pm$ 1 MHz	

**Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	38.1 $\pm$ 6 %	1.86 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

**SAR result with Head TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.7 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>53.6 W/kg <math>\pm</math> 17.0 % (k=2)</b>

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.30 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>24.9 W/kg <math>\pm</math> 16.5 % (k=2)</b>

**Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	51.8 $\pm$ 6 %	2.03 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

**SAR result with Body TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.3 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	<b>52.0 W/kg <math>\pm</math> 17.0 % (k=2)</b>

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	6.16 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	<b>24.3 W/kg <math>\pm</math> 16.5 % (k=2)</b>

**Appendix 3-9: Calibration certificate: Dipole (D2450V2) (cont'd)****Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with Head TSL**

Impedance, transformed to feed point	53.3 $\Omega$ + 5.5 j $\Omega$
Return Loss	- 24.1 dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	50.5 $\Omega$ + 6.7 j $\Omega$
Return Loss	- 23.5 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.160 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
-----------------	-------

**Appendix 3-9: Calibration certificate: Dipole (D2450V2) (cont'd)****DASY5 Validation Report for Head TSL**

Date: 10.11.2020

Test Laboratory: SPEAG, Zurich, Switzerland.

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:822**

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.86$  S/m;  $\epsilon_r = 38.1$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7405; ConvF(7.81, 7.81, 7.81) @ 2450 MHz; Calibrated: 29.06.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 02.11.2020
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

**Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 116.9 V/m; Power Drift = 0.04 dB


Peak SAR (extrapolated) = 28.4 W/kg

**SAR(1 g) = 13.7 W/kg; SAR(10 g) = 6.3 W/kg**

Smallest distance from peaks to all points 3 dB below = 9 mm


Ratio of SAR at M2 to SAR at M1 = 48.4%

Maximum value of SAR (measured) = 23.1 W/kg

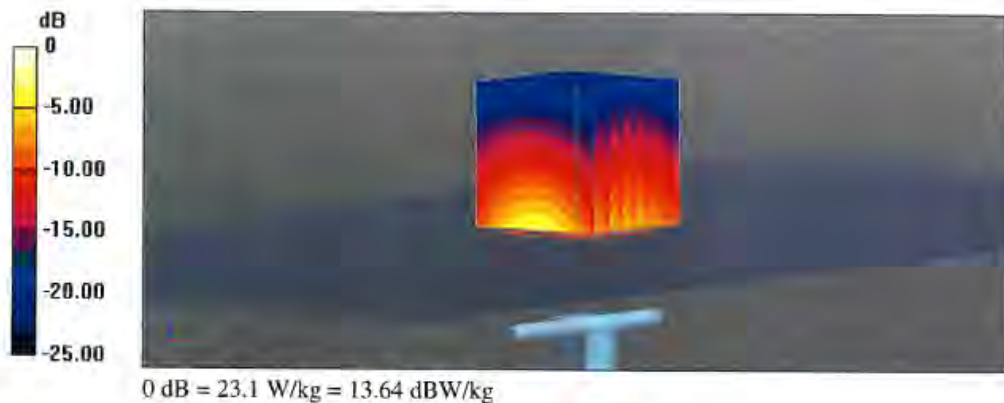

Appendix 3-9: Calibration certificate: Dipole (D2450V2) (cont'd)

Impedance Measurement Plot for Head TSL

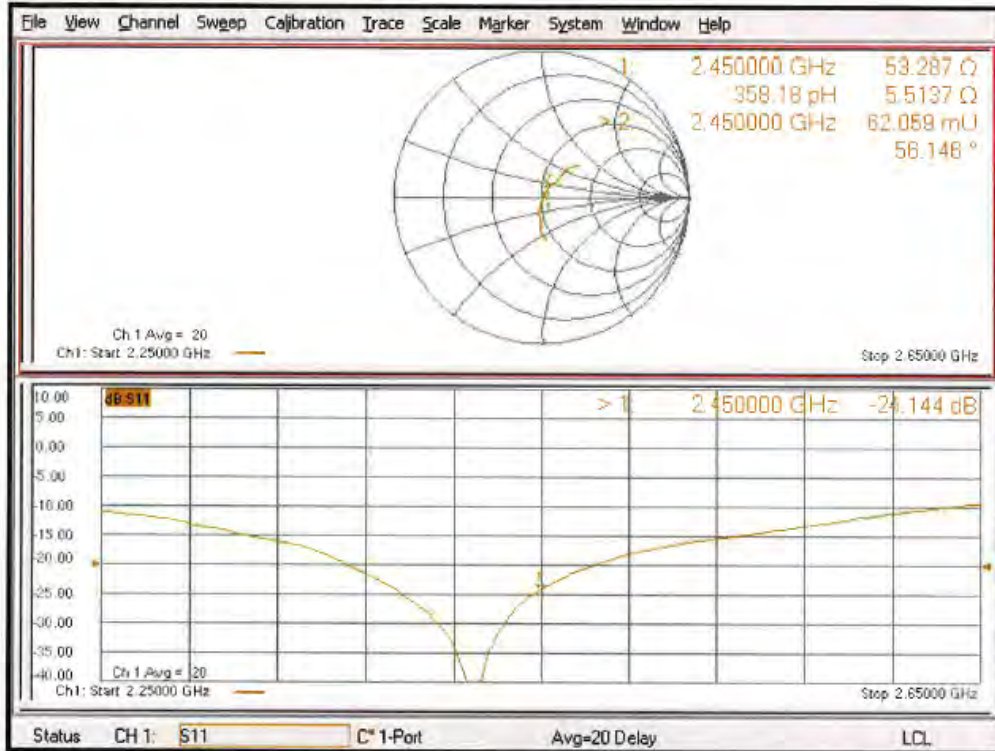

**Appendix 3-9: Calibration certificate: Dipole (D2450V2) (cont'd)****DASY5 Validation Report for Body TSL**

Date: 10.11.2020

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:822**

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 2.03$  S/m;  $\epsilon_r = 51.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7405; ConvF(7.75, 7.75, 7.75) @ 2450 MHz; Calibrated: 29.06.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 02.11.2020
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

**Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 108.1 V/m; Power Drift = -0.07 dB


Peak SAR (extrapolated) = 27.4 W/kg

**SAR(1 g) = 13.3 W/kg; SAR(10 g) = 6.16 W/kg**

Smallest distance from peaks to all points 3 dB below = 8.2 mm


Ratio of SAR at M2 to SAR at M1 = 50%

Maximum value of SAR (measured) = 21.6 W/kg

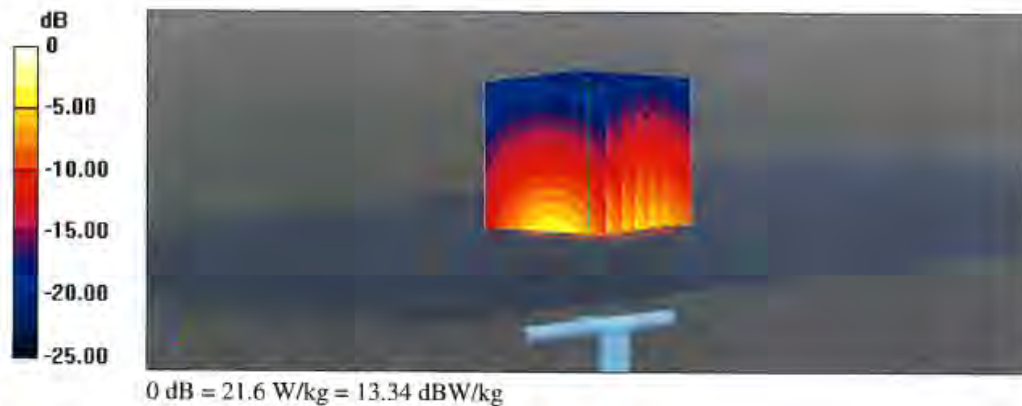

**Appendix 3-9: Calibration certificate: Dipole (D2450V2) (cont'd)**

**Impedance Measurement Plot for Body TSL**

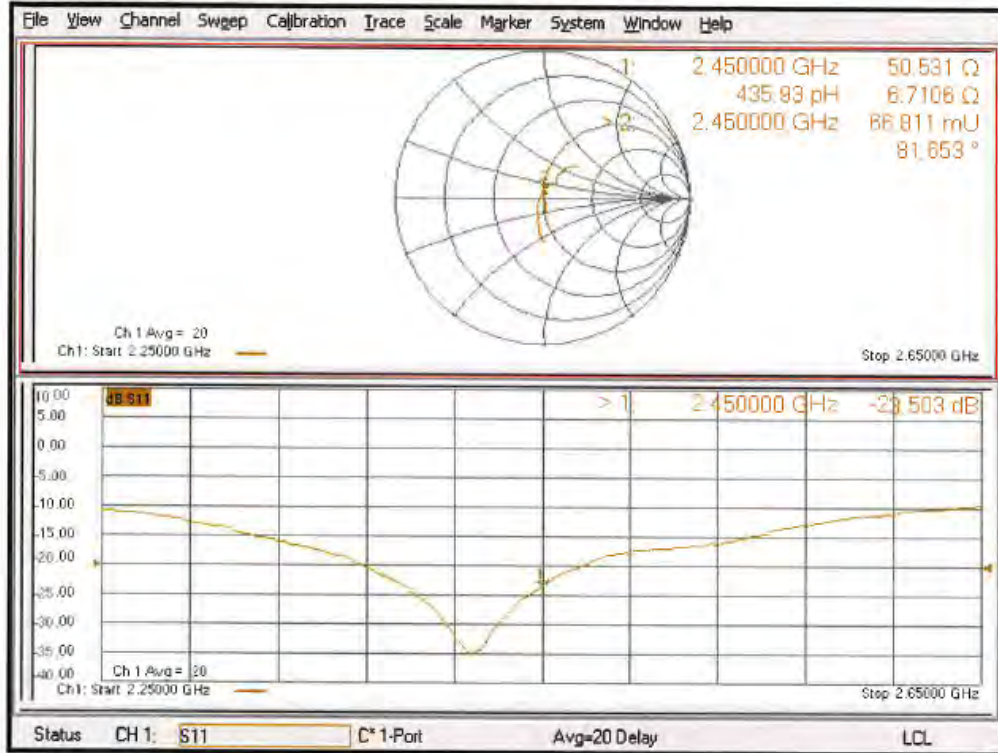

**Appendix 3-10: Calibration certificate: Dipole (D5GHzV2)**

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 0108**

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client **UL Japan (RCC)**

Certificate No: **D5GHzV2-1070\_Apr21**

CALIBRATION CERTIFICATE			
Object	D5GHzV2 - SN:1070		
Calibration procedure(s)	QA CAL-22.v6 Calibration Procedure for SAR Validation Sources between 3-10 GHz		
Calibration date:	April 20, 2021		
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	09-Apr-21 (No. 217-03291/03292)	Apr-22
Power sensor NRP-Z91	SN: 103244	09-Apr-21 (No. 217-03291)	Apr-22
Power sensor NRP-Z91	SN: 103245	09-Apr-21 (No. 217-03292)	Apr-22
Reference 20 dB Attenuator	SN: BH9394 (20k)	09-Apr-21 (No. 217-03343)	Apr-22
Type-N mismatch combination	SN: 310982 / 06327	09-Apr-21 (No. 217-03344)	Apr-22
Reference Probe EX3DV4	SN: 3503	30-Dec-20 (No. EX3-3503_Dec20)	Dec-21
DAE4	SN: 601	02-Nov-20 (No. DAE4-601_Nov20)	Nov-21
Secondary Standards	ID #	Check Date (In house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oct-20)	In house check: Oct-22
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-20)	In house check: Oct-22
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-20)	In house check: Oct-22
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-20)	In house check: Oct-22
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-20)	In house check: Oct-21
Calibrated by:	Name Michael Weber	Function Laboratory Technician	Signature 
Approved by:	Name Katja Pokovic	Function Technical Manager	Signature 
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			Issued: April 20, 2021

**Appendix 3-10: Calibration certificate: Dipole (D5GHzV2) (cont'd)**

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

**Glossary:**

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.



**Appendix 3-10: Calibration certificate: Dipole (D5GHzV2) (cont'd)****Measurement Conditions**

DASY system configuration, as far as not given on page 1.

<b>DASY Version</b>	DASY5	V52.10.4
<b>Extrapolation</b>	Advanced Extrapolation	
<b>Phantom</b>	Modular Flat Phantom V5.0	
<b>Distance Dipole Center - TSL</b>	10 mm	with Spacer
<b>Zoom Scan Resolution</b>	dx, dy = 4.0 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
<b>Frequency</b>	5250 MHz ± 1 MHz 5600 MHz ± 1 MHz 5750 MHz ± 1 MHz 5800 MHz ± 1 MHz	

**Head TSL parameters at 5250 MHz**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
<b>Nominal Head TSL parameters</b>	22.0 °C	35.9	4.71 mho/m
<b>Measured Head TSL parameters</b>	(22.0 ± 0.2) °C	34.9 ± 6 %	4.57 mho/m ± 6 %
<b>Head TSL temperature change during test</b>	< 0.5 °C	----	----

**SAR result with Head TSL at 5250 MHz**

<b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>	Condition	
SAR measured	100 mW input power	7.93 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>78.8 W/kg ± 19.9 % (k=2)</b>

<b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b>	condition	
SAR measured	100 mW input power	2.28 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>22.6 W/kg ± 19.5 % (k=2)</b>

**Appendix 3-10: Calibration certificate: Dipole (D5GHzV2) (cont'd)****Head TSL parameters at 5600 MHz**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.4 ± 6 %	4.93 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

**SAR result with Head TSL at 5600 MHz**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.30 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>82.4 W/kg ± 19.9 % (k=2)</b>

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.36 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>23.4 W/kg ± 19.5 % (k=2)</b>

**Head TSL parameters at 5800 MHz**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.3	5.27 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.1 ± 6 %	5.14 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

**SAR result with Head TSL at 5800 MHz**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.08 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>80.1 W/kg ± 19.9 % (k=2)</b>

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.27 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>22.5 W/kg ± 19.5 % (k=2)</b>

**Appendix 3-10: Calibration certificate: Dipole (D5GHzV2) (cont'd)****Body TSL parameters at 5250 MHz**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.9	5.36 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	48.7 ± 6 %	5.51 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

**SAR result with Body TSL at 5250 MHz**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.50 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	<b>75.0 W/kg ± 19.9 % (k=2)</b>

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.08 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	<b>20.8 W/kg ± 19.5 % (k=2)</b>

**Body TSL parameters at 5600 MHz**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.5	5.77 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	48.1 ± 6 %	6.00 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

**SAR result with Body TSL at 5600 MHz**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.96 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	<b>79.6 W/kg ± 19.9 % (k=2)</b>

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.18 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	<b>21.8 W/kg ± 19.5 % (k=2)</b>

**Appendix 3-10: Calibration certificate: Dipole (D5GHzV2) (cont'd)****Body TSL parameters at 5750 MHz**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.3	5.94 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	47.8 ± 6 %	6.21 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

**SAR result with Body TSL at 5750 MHz**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.53 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	<b>75.3 W/kg ± 19.9 % (k=2)</b>

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.09 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	<b>20.9 W/kg ± 19.5 % (k=2)</b>

**Appendix 3-10: Calibration certificate: Dipole (D5GHzV2) (cont'd)****Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with Head TSL at 5250 MHz**

Impedance, transformed to feed point	51.4 $\Omega$ - 8.8 j $\Omega$
Return Loss	- 21.1 dB

**Antenna Parameters with Head TSL at 5600 MHz**

Impedance, transformed to feed point	54.9 $\Omega$ - 7.8 j $\Omega$
Return Loss	- 21.1 dB

**Antenna Parameters with Head TSL at 5800 MHz**

Impedance, transformed to feed point	51.9 $\Omega$ - 1.6 j $\Omega$
Return Loss	- 32.2 dB

**Antenna Parameters with Body TSL at 5250 MHz**

Impedance, transformed to feed point	53.6 $\Omega$ - 6.9 j $\Omega$
Return Loss	- 22.5 dB

**Antenna Parameters with Body TSL at 5600 MHz**

Impedance, transformed to feed point	58.1 $\Omega$ - 6.6 j $\Omega$
Return Loss	- 20.3 dB

**Antenna Parameters with Body TSL at 5750 MHz**

Impedance, transformed to feed point	58.4 $\Omega$ - 1.5 j $\Omega$
Return Loss	- 22.1 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.202 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
-----------------	-------

**Appendix 3-10: Calibration certificate: Dipole (D5GHzV2) (cont'd)****DASY5 Validation Report for Head TSL**

Date: 20.04.2021

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole D5GHzV2; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1070**

Communication System: UID 0 - CW; Frequency: 5250 MHz, Frequency: 5600 MHz, Frequency: 5800 MHz

Medium parameters used:  $f = 5250$  MHz;  $\sigma = 4.57$  S/m;  $\epsilon_r = 34.9$ ;  $\rho = 1000$  kg/m<sup>3</sup>,Medium parameters used:  $f = 5600$  MHz;  $\sigma = 4.93$  S/m;  $\epsilon_r = 34.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>,Medium parameters used:  $f = 5800$  MHz;  $\sigma = 5.14$  S/m;  $\epsilon_r = 34.1$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(5.5, 5.5, 5.5) @ 5250 MHz, ConvF(5.1, 5.1, 5.1) @ 5600 MHz, ConvF(5.01, 5.01, 5.01) @ 5800 MHz; Calibrated: 30.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 02.11.2020
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

**Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5250 MHz/Zoom Scan,****dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 74.78 V/m; Power Drift = 0.06 dB

Peak SAR (extrapolated) = 27.3 W/kg

**SAR(1 g) = 7.93 W/kg; SAR(10 g) = 2.28 W/kg**

Smallest distance from peaks to all points 3 dB below = 6.8 mm

Ratio of SAR at M2 to SAR at M1 = 69.9%

Maximum value of SAR (measured) = 18.2 W/kg

**Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan,****dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 75.33 V/m; Power Drift = 0.09 dB

Peak SAR (extrapolated) = 30.7 W/kg

**SAR(1 g) = 8.30 W/kg; SAR(10 g) = 2.36 W/kg**

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 68.7%

Maximum value of SAR (measured) = 19.6 W/kg

**Appendix 3-10: Calibration certificate: Dipole (D5GHzV2) (cont'd)**

**Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5800 MHz/Zoom Scan,**

**dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 73.25 V/m; Power Drift = 0.09 dB


Peak SAR (extrapolated) = 31.8 W/kg

**SAR(1 g) = 8.08 W/kg; SAR(10 g) = 2.27 W/kg**

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 66.5%


Maximum value of SAR (measured) = 19.8 W/kg

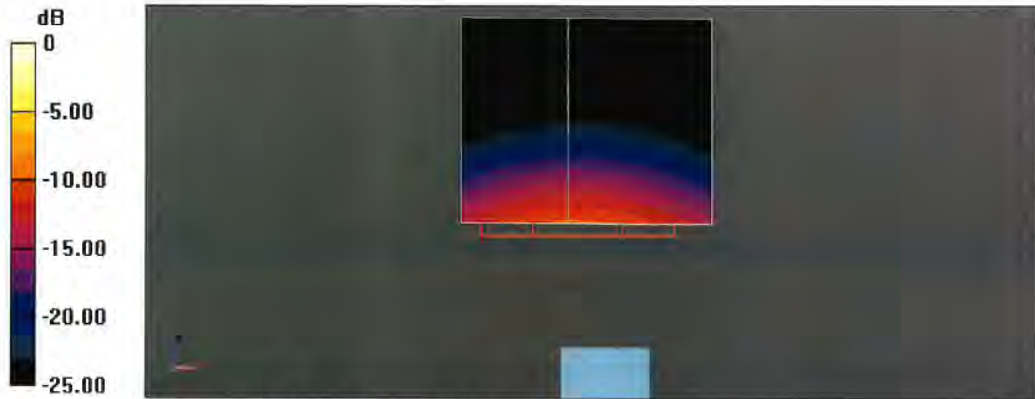

0 dB = 19.8 W/kg = 12.97 dBW/kg

Appendix 3-10: Calibration certificate: Dipole (D5GHzV2) (cont'd)

Impedance Measurement Plot for Head TSL

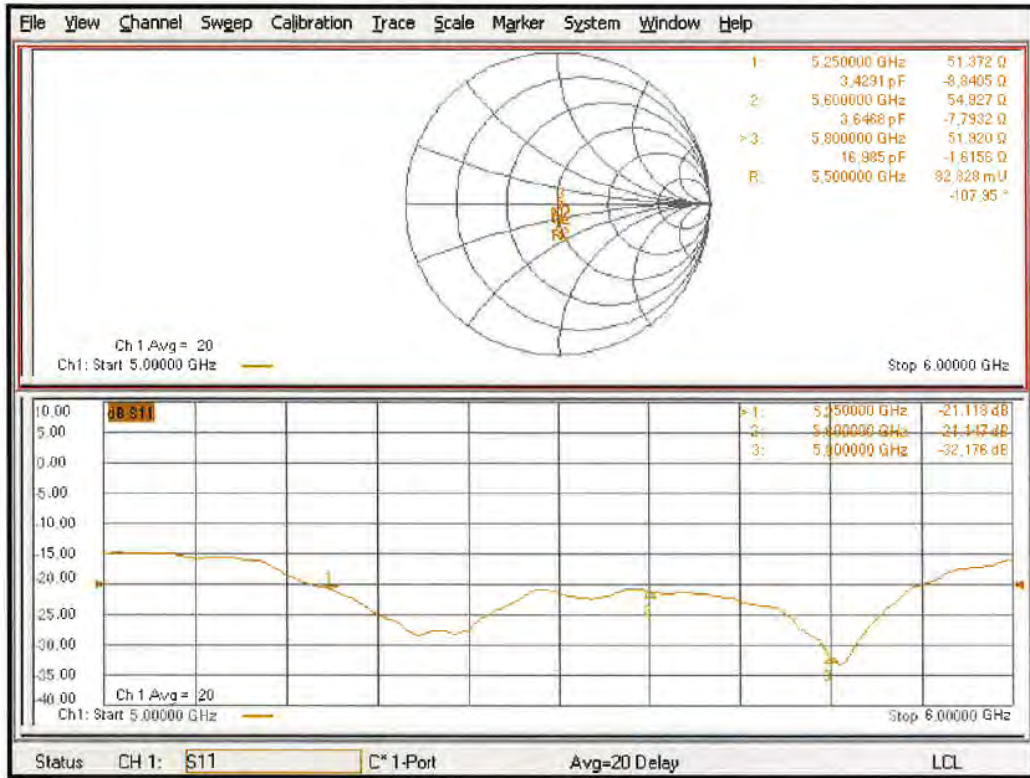



**Appendix 3-10: Calibration certificate: Dipole (D5GHzV2) (cont'd)****DASY5 Validation Report for Body TSL**

Date: 19.04.202

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole D5GHzV2; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1070**

Communication System: UID 0 - CW; Frequency: 5250 MHz, Frequency: 5600 MHz, Frequency: 5750 MHz;

Medium parameters used:  $f = 5250$  MHz;  $\sigma = 5.51$  S/m;  $\epsilon_r = 48.7$ ;  $\rho = 1000$  kg/m<sup>3</sup>,Medium parameters used:  $f = 5600$  MHz;  $\sigma = 6$  S/m;  $\epsilon_r = 48.1$ ;  $\rho = 1000$  kg/m<sup>3</sup>,Medium parameters used:  $f = 5750$  MHz;  $\sigma = 6.21$  S/m;  $\epsilon_r = 47.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(5.26, 5.26, 5.26) @ 5250 MHz, ConvF(4.79, 4.79, 4.79) @ 5600 MHz, ConvF(4.66, 4.66, 4.66) @ 5750 MHz; Calibrated: 30.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 02.11.2020
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

**Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5250 MHz/Zoom Scan,****dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 67.14 V/m; Power Drift = 0.00 dB

Peak SAR (extrapolated) = 28.9 W/kg

**SAR(1 g) = 7.50 W/kg; SAR(10 g) = 2.08 W/kg**

Smallest distance from peaks to all points 3 dB below = 6.9 mm

Ratio of SAR at M2 to SAR at M1 = 66.1%

Maximum value of SAR (measured) = 17.2 W/kg

**Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan,****dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 67.13 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 34.0 W/kg

**SAR(1 g) = 7.96 W/kg; SAR(10 g) = 2.18 W/kg**

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 63.2%

Maximum value of SAR (measured) = 19.0 W/kg

**Appendix 3-10: Calibration certificate: Dipole (D5GHzV2) (cont'd)**

**Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5750 MHz/Zoom Scan,**

**dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 65.86 V/m; Power Drift = -0.04 dB


Peak SAR (extrapolated) = 34.0 W/kg

**SAR(1 g) = 7.53 W/kg; SAR(10 g) = 2.09 W/kg**

Smallest distance from peaks to all points 3 dB below = 6.8 mm

Ratio of SAR at M2 to SAR at M1 = 62.6%

Maximum value of SAR (measured) = 18.6 W/kg

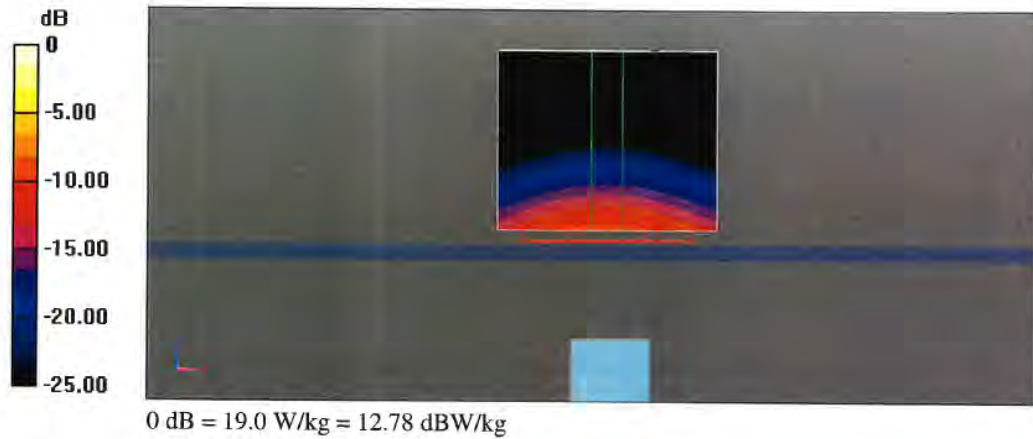

Appendix 3-10: Calibration certificate: Dipole (D5GHzV2) (cont'd)

Impedance Measurement Plot for Body TSL

